

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100382

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 08/29/2020

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.23: 0.078

LOT #: ~~AG92342~~ **AG923401** *JM 09/16/20*

EXPIRATION: 08/22/2021

TANK PRESSURE: 1235 psi

BLANK TEST	0.000	11:39
INTERNAL STANDARD	VERIFIED	11:40
EXTERNAL STANDARD	0.079	11:40
BLANK TEST	0.000	11:41
EXTERNAL STANDARD	0.079	11:41
BLANK TEST	0.000	11:42
EXTERNAL STANDARD	0.078	11:42
BLANK TEST	0.000	11:43
EXTERNAL STANDARD	0.079	11:44
BLANK TEST	0.000	11:44
EXTERNAL STANDARD	0.079	11:45
BLANK TEST	0.000	11:46

Average = 0.0788

Std Dev = 0.0004

Diagnostic Check

VERSIONS

DMT: 3.02

PIC: 3.02

Modem: 2.6

Questions: 2.2

TEMPERATURES

Sample Chamber = 49.2°C

PASSED

Breath Tube = 48.1°C

PASSED

PUMP INFO

Flow Rate = 4.970 L/M

PASSED

DETECTOR INFO

PUMP ON

PASSED

PUMP OFF

PASSED

FILTER INFO

Filter 1

PASSED

Filter 2

PASSED

Filter 3

PASSED

INTERNAL STANDARD

PASSED

I, Brandi M. Barnett, after being first duly sworn, depose and state as follows:

(1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.

(2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.

(3) I am the Scientific Director of the State Breath Alcohol Program.

(4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.

(5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.



(6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Brandi M Barnett 10/16/20

Brandi M. Barnett
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 16 day of Oct. 2020

[Signature]
Notary Public
My Commission Expires With Office

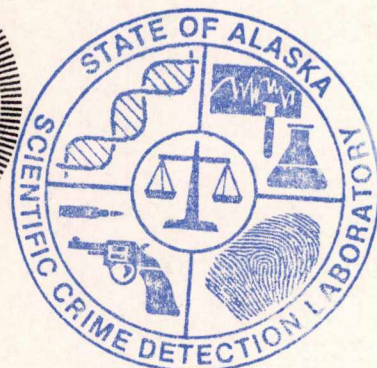

JM 09/16/20