

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument  
State of Alaska

Serial #: 100383

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 10/11/2015

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.09: 0.078  
LOT #: 09214080A2  
EXPIRATION: 05/01/2016  
TANK PRESSURE: 1076 psi

BLANK TEST	0.000	16:28
INTERNAL STANDARD	VERIFIED	16:28
EXTERNAL STANDARD	0.074	16:28
BLANK TEST	0.000	16:29
EXTERNAL STANDARD	0.074	16:29
BLANK TEST	0.000	16:30
EXTERNAL STANDARD	0.074	16:30
BLANK TEST	0.000	16:31
EXTERNAL STANDARD	0.074	16:32
BLANK TEST	0.000	16:32
EXTERNAL STANDARD	0.074	16:33
BLANK TEST	0.000	16:34

Average = 0.0740  
Std Dev = 0.0000

## Diagnostic Check

### VERSIONS

DMT: 3.01  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.8°C PASSED  
Breath Tube = 47.3°C PASSED

### PUMP INFO

Flow Rate = 4.714 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

### FILTER INFO

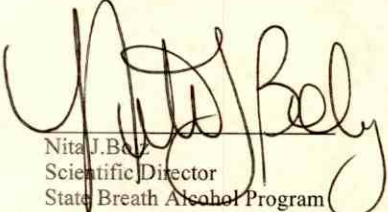
Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

### INTERNAL STANDARD

PASSED


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

11/6/2015

Subscribed and sworn before me this 6<sup>th</sup> day of Nov., 20 15

  
Nikki Roth, Notary Public  
My Commission Expires With Office



C0810/14/15