

Rcd 10/16/19 BMB  
Verified 11/7/19  
COX



Airgas USA LLC (LAB)  
3500 Bernard Street  
St. Louis, Mo. 63103  
Ph: (314) 533-3100  
Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**  
*Exclusive Supplier*  
Intoximeters, Inc.  
2081 Craig Road  
St. Louis, Mo 63146

**Test Date:** 23-Apr-2019

**Lot # AG911203 Model 108cacc**

<u>Exp. Date</u>	<u>Cyl. Type</u>	<u>Component</u>	<u>Certified Concentration</u>
22-Apr-2021	108	Ethanol Nitrogen	0.200 ± 2% BrAC (521 ppm) Balance

**Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:**

<u>RGM Serial No.</u>	<u>Concentration</u>	<u>RGM Serial No.</u>	<u>Concentration</u>
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

<u>CRM Serial No.</u>	<u>Concentration</u>	<u>CRM Serial No.</u>	<u>Concentration</u>
CC434668	800.0 ppm	0056649	390.1 ppm
CC234503	253.0 ppm	0056662	150.2 ppm

**Analytical Method:** NDIR

Digitally signed by Quality Control  
Date: 2019.04.24 14:32:15 -05:00  
Reason: Dry gas standard certification of analysis  
Location: Airgas USA LLC (Lab)

Approved for Release:

Rod Marsala

**ISO 17025:2005 A2LA accredited. Certificate Number 3082.06**  
**ISO 17034:2016 A2LA accredited. Certificate Number 3082.07**

**SUPERVISOR TEST**

Alaska Department of Public Safety  
 DATAMASTER dmt: 100405

Date: 11/07/2019  
 Time: 14:03:48

SUPERVISOR NAME:  
 COLLEEN S OBRYANT  
 OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.200  
 TARGET AT 29.52: 0.197  
 TANK PRESSURE: 599 psi

BLANK TEST	0.000	14:05
INTERNAL STANDARD	VERIFIED	14:05
EXTERNAL STANDARD	0.192	14:05
BLANK TEST	0.000	14:06
EXTERNAL STANDARD	0.191	14:06
BLANK TEST	0.000	14:07
EXTERNAL STANDARD	0.191	14:08
BLANK TEST	0.000	14:08
EXTERNAL STANDARD	0.192	14:09
BLANK TEST	0.000	14:10
EXTERNAL STANDARD	0.191	14:10
BLANK TEST	0.000	14:11

Average = 0.1914  
 Std Dev = 0.0005






*Lot AG 911203*

*Exp 4/22/21*

*Tank 005*

*003"/7/19*

*Average - 0.195*

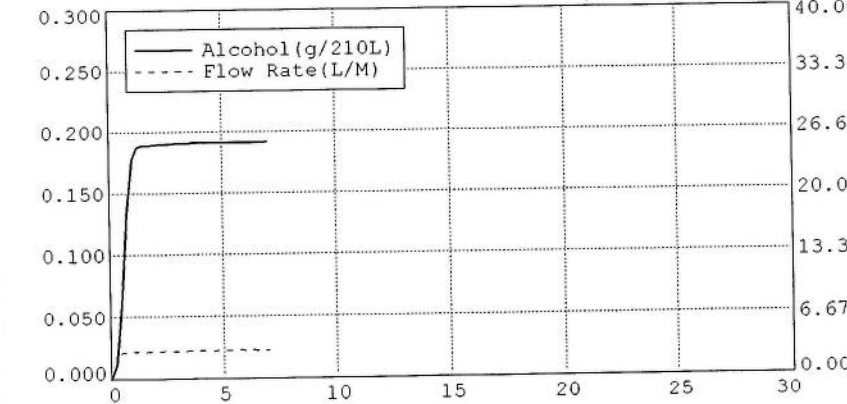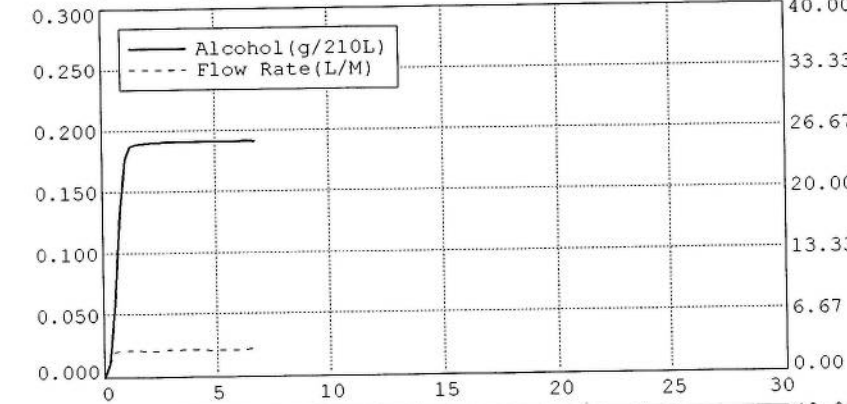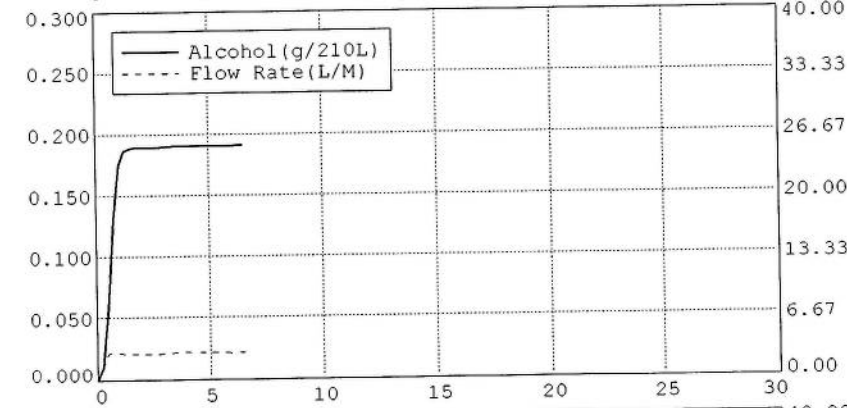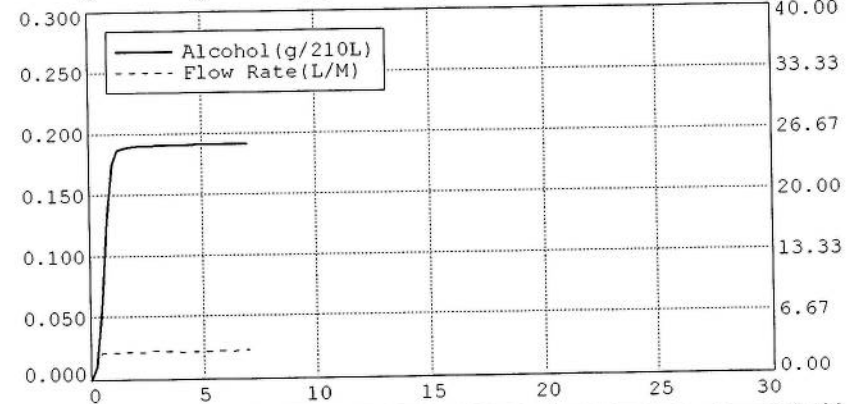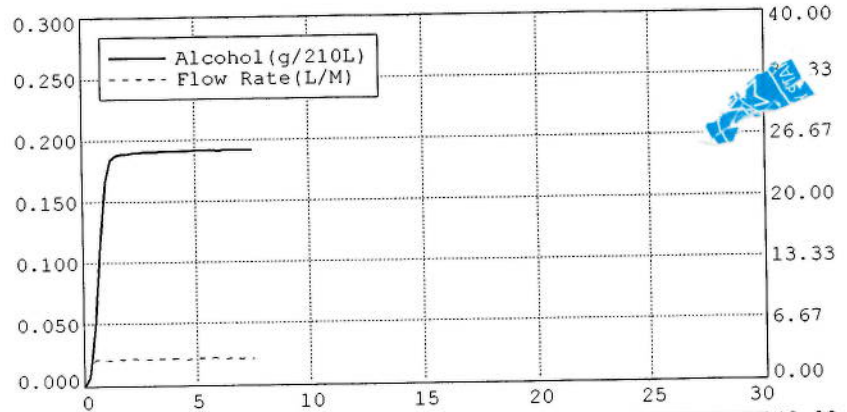

**SUPERVISOR TEST**

Alaska Department of Public Safety  
 DATAMASTER dmt: 100353

Date: 11/07/2019  
 Time: 14:55:14






SUPERVISOR NAME:  
 COLLEEN S OBRYANT  
 OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.200  
 TARGET AT 29.52: 0.197  
 TANK PRESSURE: 627 psi

BLANK TEST	0.000	14:56
INTERNAL STANDARD	VERIFIED 0.198	14:57
EXTERNAL STANDARD	0.198	14:57
BLANK TEST	0.000	14:58
EXTERNAL STANDARD	0.197	14:58
BLANK TEST	0.000	14:59
EXTERNAL STANDARD	0.197	14:59
BLANK TEST	0.000	15:00
EXTERNAL STANDARD	0.198	15:00
BLANK TEST	0.000	15:01
EXTERNAL STANDARD	0.198	15:01
BLANK TEST	0.000	15:02

Average = 0.1976  
 Std Dev = 0.0005

*Lot AB 911203*  
*Exp 4/20/21*  
*Tank 005*  
*COB 11/4/19*

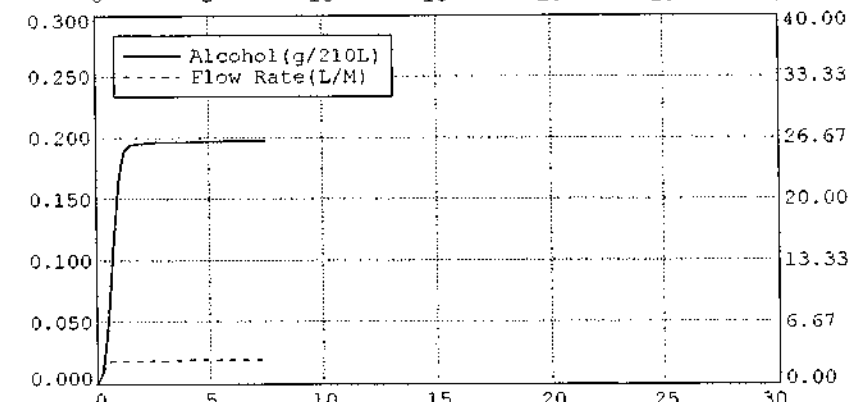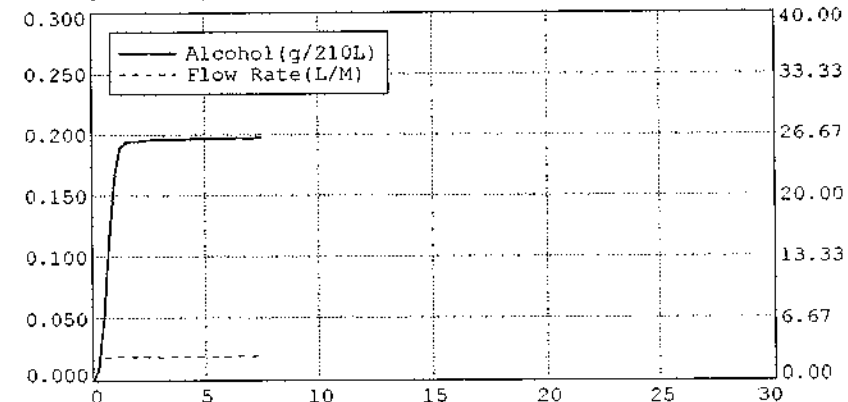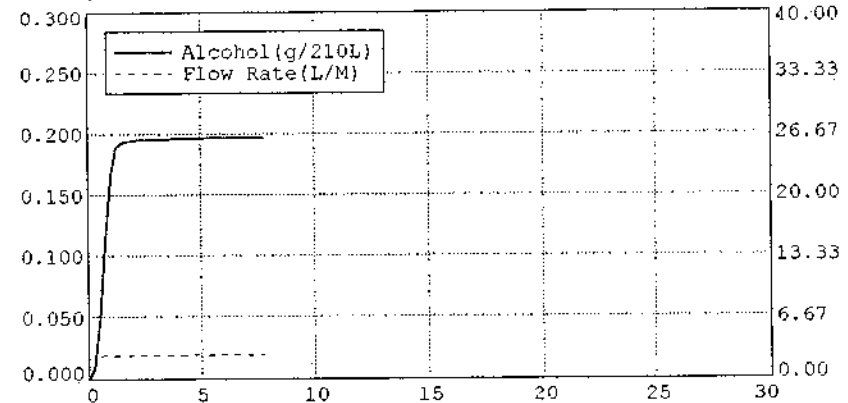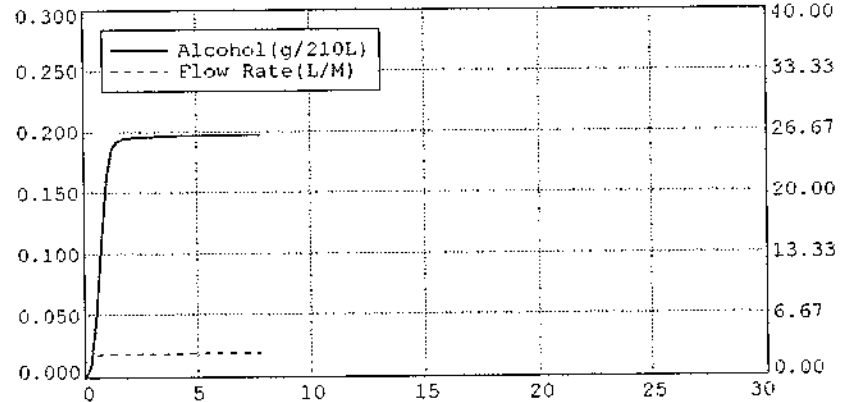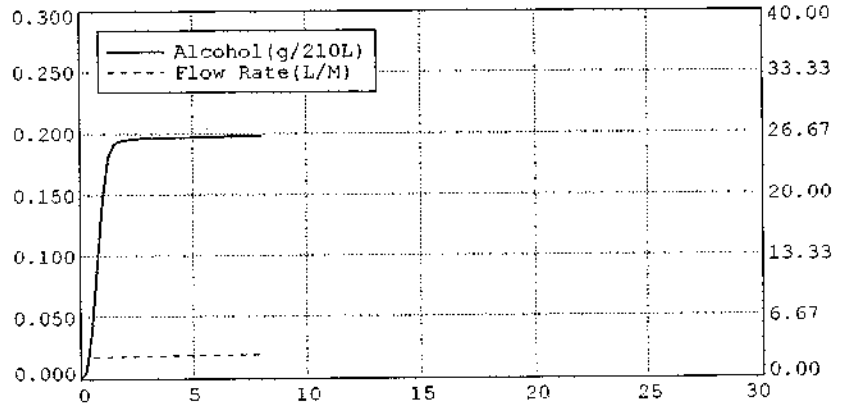

**SUPERVISOR TEST**

Alaska Department of Public Safety  
 DATAMASTER dmt: 100671

Date: 11/07/2019  
 Time: 14:23:47






SUPERVISOR NAME:  
 COLLEEN S OBRYANT  
 OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.200  
 TARGET AT 29.52: 0.197  
 TANK PRESSURE: 587 psi

BLANK TEST	0.000	14:25
INTERNAL STANDARD	VERIFIED	14:25
EXTERNAL STANDARD	0.196	14:25
BLANK TEST	0.000	14:26
EXTERNAL STANDARD	0.196	14:26
BLANK TEST	0.000	14:27
EXTERNAL STANDARD	0.196	14:28
BLANK TEST	0.000	14:28
EXTERNAL STANDARD	0.196	14:29
BLANK TEST	0.000	14:30
EXTERNAL STANDARD	0.195	14:30
BLANK TEST	0.000	14:31

Average = 0.1958  
 Std Dev = 0.0004

*Lot AG911203  
 Exp 4/20/21  
 Tank 005  
 COB 11/7/19*

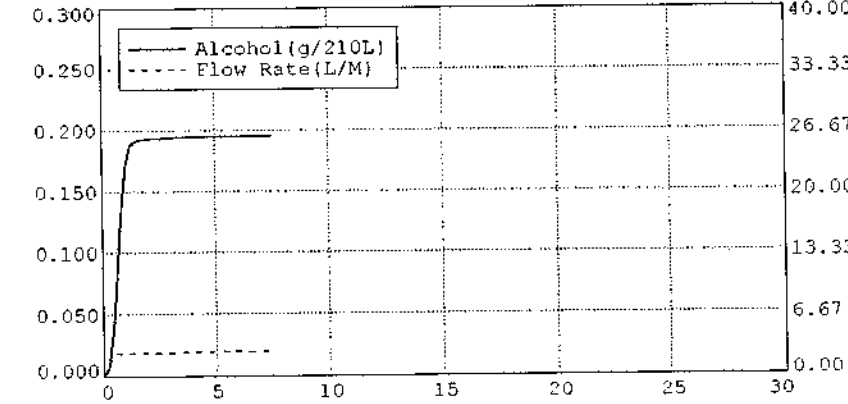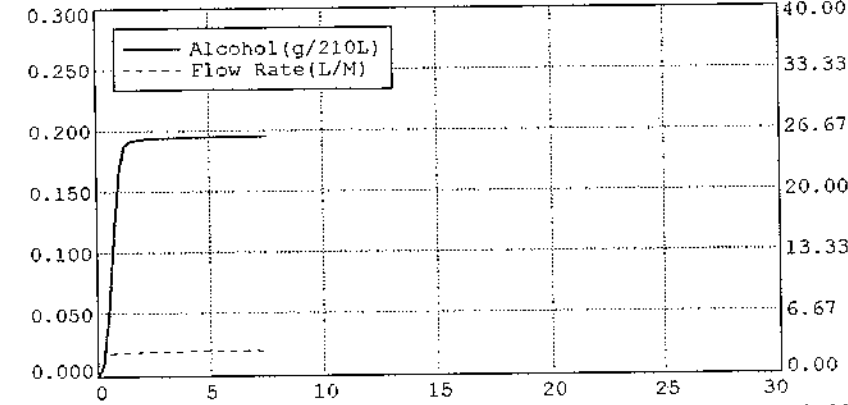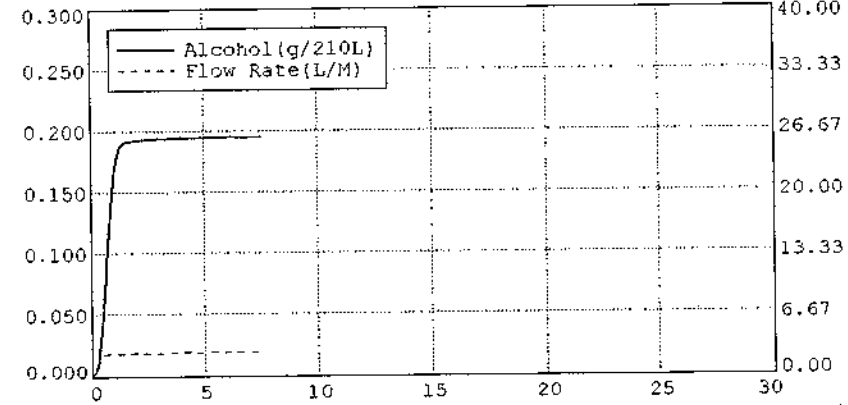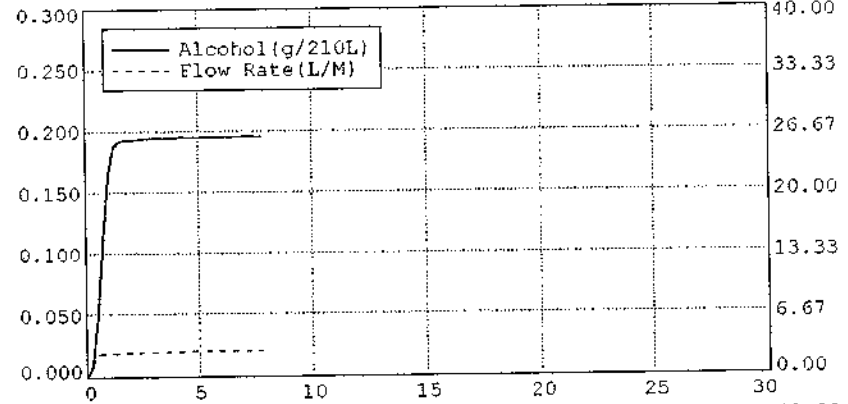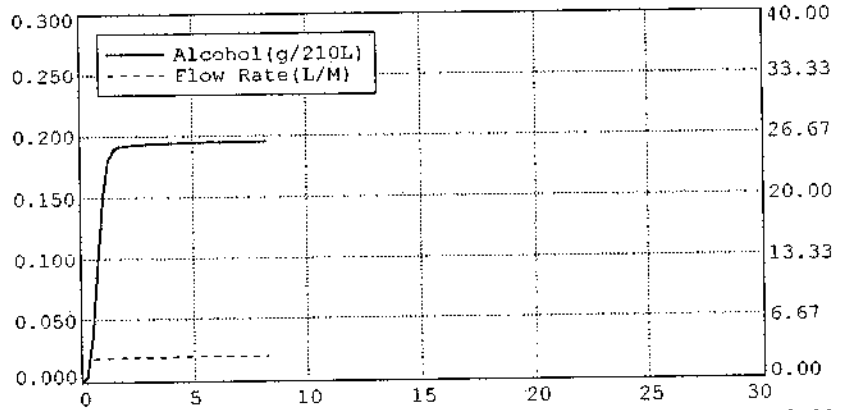

SUPERVISOR TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100405

Date: 11/07/2019  
 Time: 13:55:38

SUPERVISOR NAME:  
 COLLEEN S OBRYANT  
 OPERATOR'S #: 6237






EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.200  
 TARGET AT 29.52: 0.197  
 TANK PRESSURE: 600 psi

BLANK TEST	0.000	13:56
INTERNAL STANDARD	VERIFIED	13:56
EXTERNAL STANDARD	0.192	13:57
BLANK TEST	0.000	13:57
EXTERNAL STANDARD	0.192	13:58
BLANK TEST	0.000	13:59
EXTERNAL STANDARD	0.191	13:59
BLANK TEST	0.000	14:00
EXTERNAL STANDARD	0.191	14:00
BLANK TEST	0.000	14:01
EXTERNAL STANDARD	0.192	14:01
BLANK TEST	0.000	14:02

Average = 0.1916  
 Std Dev = 0.0005

*Lot AG911203*  
*Exp 4/22/21*  
*Tank 006*  
*COB 11/7/19*

*Average - 0.195*

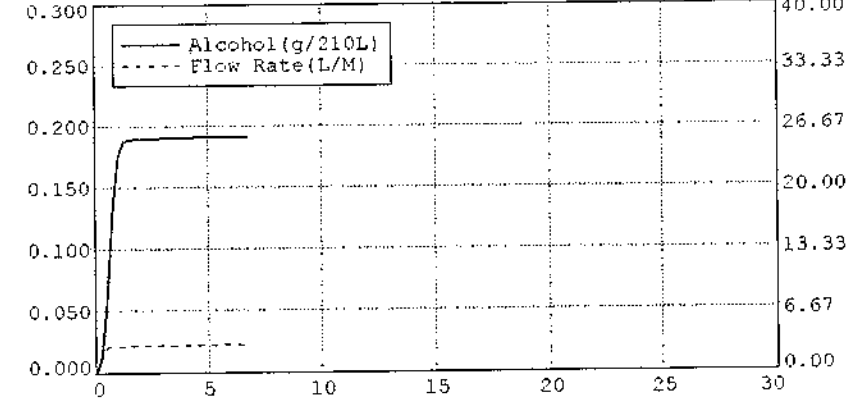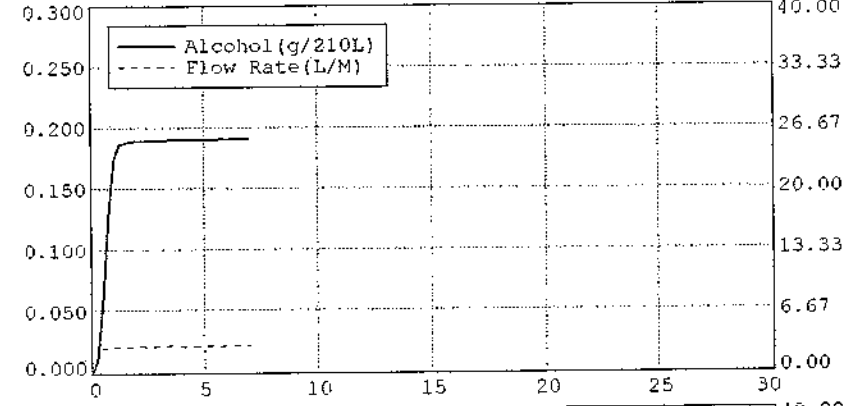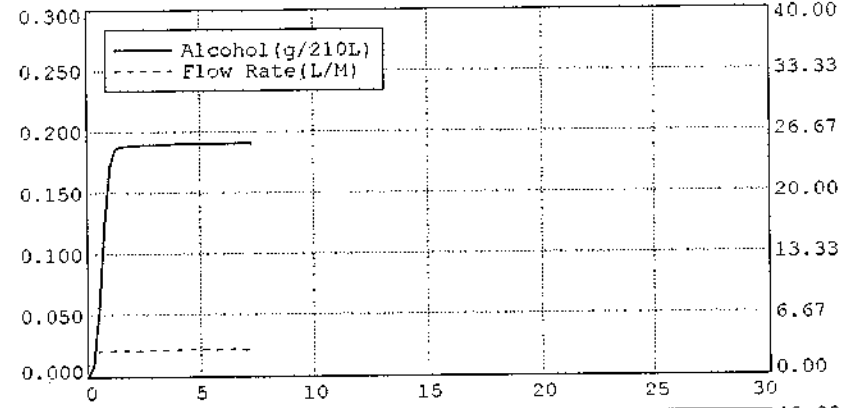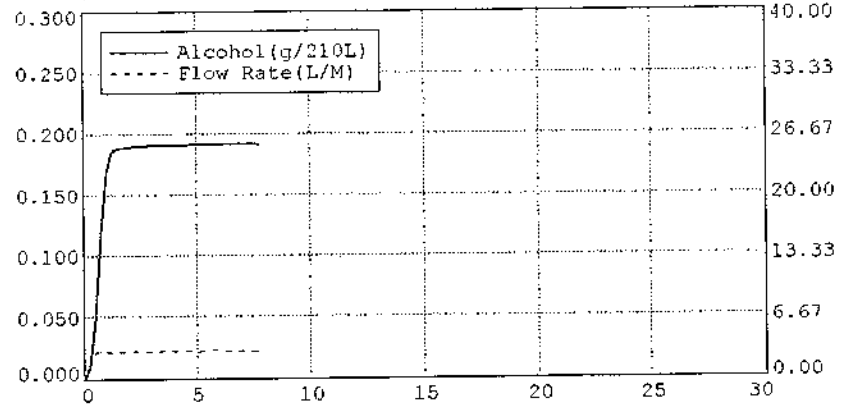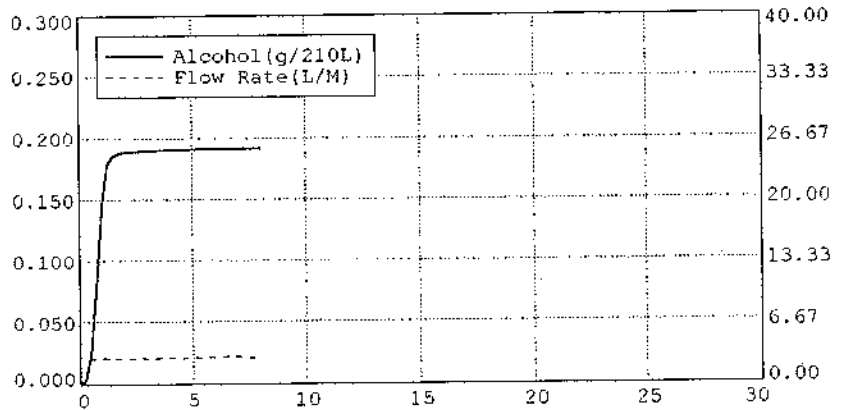

SUPERVISOR TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100353

Date: 11/07/2019  
 Time: 14:46:15

SUPERVISOR NAME:  
 COLLEEN S OBRYANT  
 OPERATOR'S #: 6237






EXTERNAL STANDARD INFORMATION

NOMINAL: 0.200  
 TARGET AT 29.51: 0.197  
 TANK PRESSURE: 628 psi

BLANK TEST	0.000	14:47
INTERNAL STANDARD	VERIFIED	14:47
EXTERNAL STANDARD	0.197	14:48
BLANK TEST	0.000	14:49
EXTERNAL STANDARD	0.197	14:49
BLANK TEST	0.000	14:50
EXTERNAL STANDARD	0.197	14:50
BLANK TEST	0.000	14:51
EXTERNAL STANDARD	0.197	14:51
BLANK TEST	0.000	14:52
EXTERNAL STANDARD	0.198	14:52
BLANK TEST	0.000	14:53

Average = 0.1972  
 Std Dev = 0.0004

*Lot AG 9/1/03*  
*Exp 4/22/21*  
*Tank 006*  
*003 11/7/19*

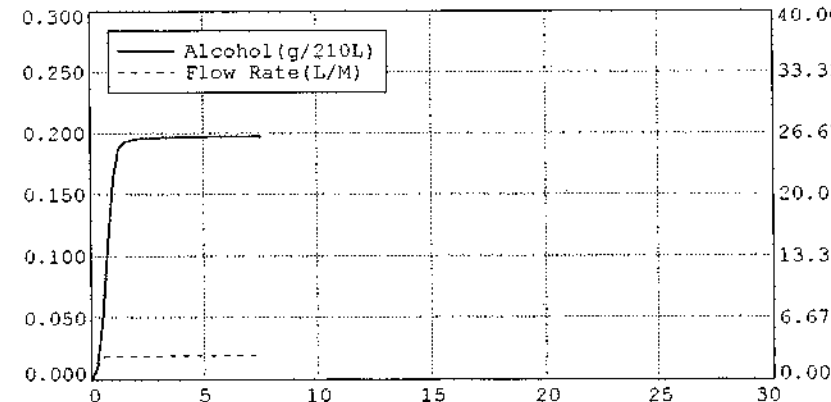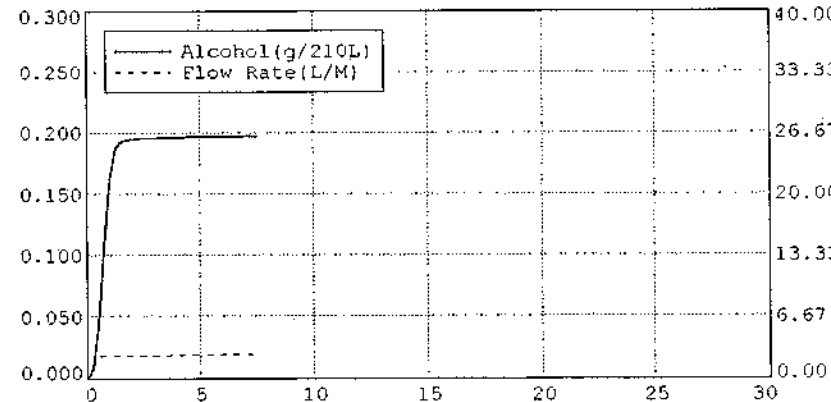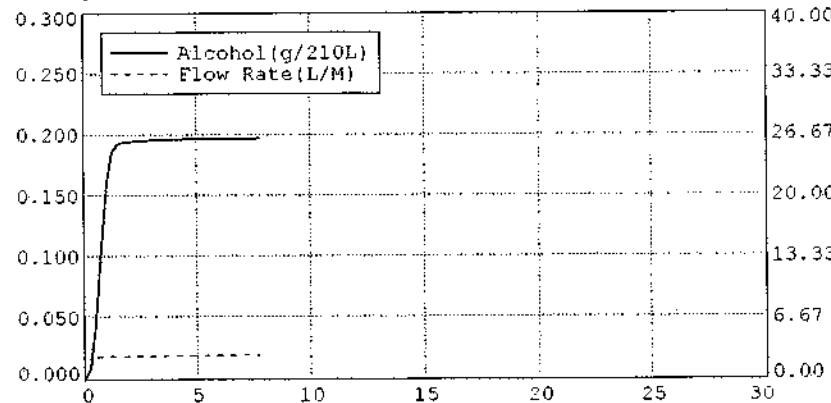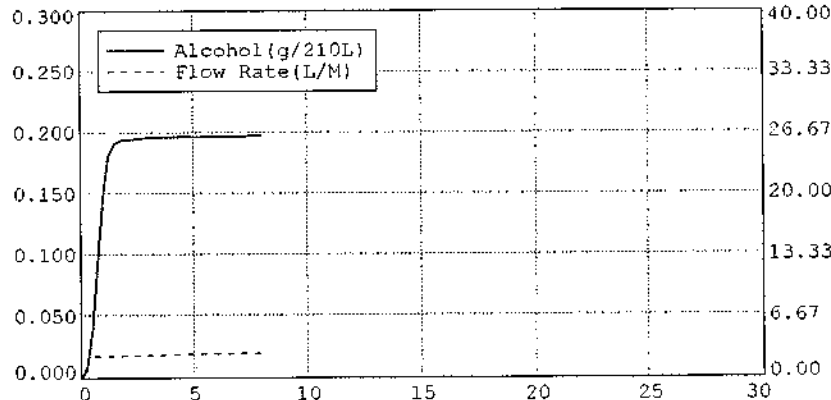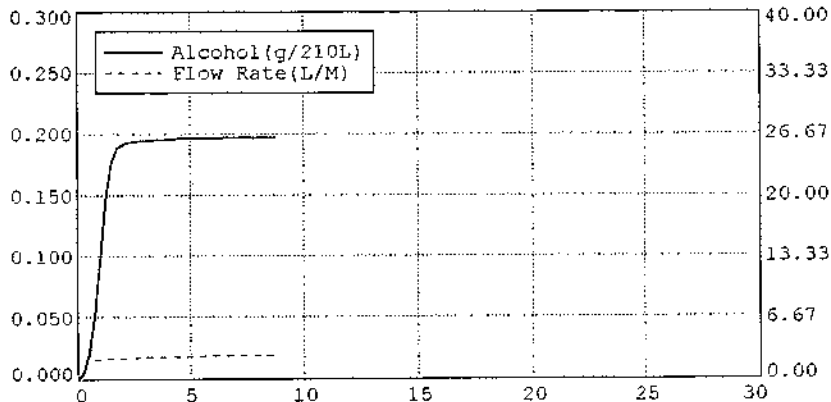

SUPERVISOR TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100671

Date: 11/07/2019  
 Time: 14:14:11

SUPERVISOR NAME:  
 COLLEEN S OBRYANT  
 OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.200  
 TARGET AT 29.52: 0.197  
 TANK PRESSURE: 589 psi

BLANK TEST	0.000	14:15
INTERNAL STANDARD	VERIFIED	14:15
EXTERNAL STANDARD	0.196	14:15
BLANK TEST	0.000	14:16
EXTERNAL STANDARD	0.195	14:16
BLANK TEST	0.000	14:17
EXTERNAL STANDARD	0.196	14:17
BLANK TEST	0.000	14:18
EXTERNAL STANDARD	0.196	14:19
BLANK TEST	0.000	14:19
EXTERNAL STANDARD	0.195	14:20
BLANK TEST	0.000	14:21






Average = 0.1956  
 Std Dev = 0.0005

*Lot AG911203*

*Exp 4/22/1*

*Tank 006*

*003 11/4/19*

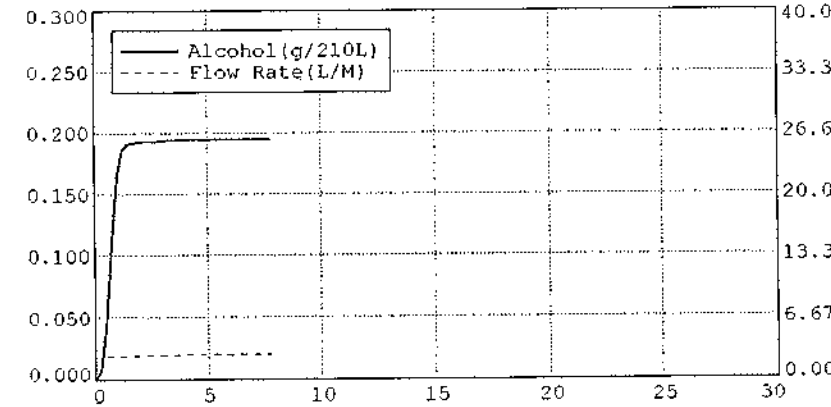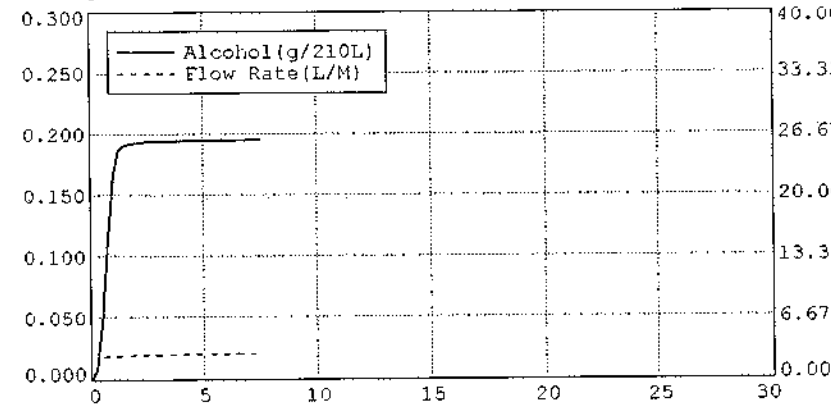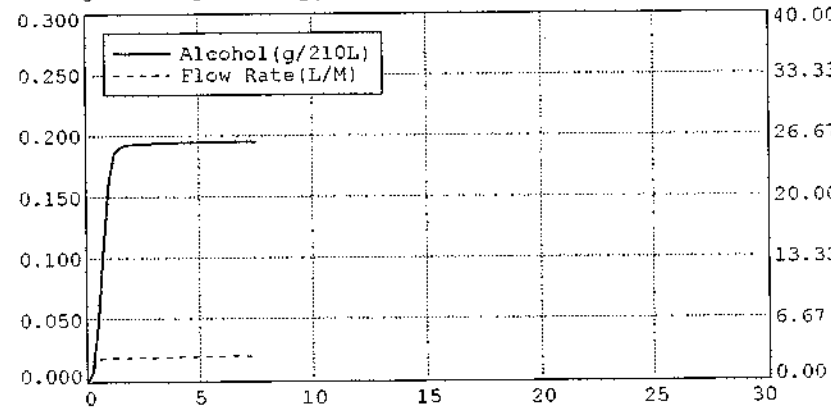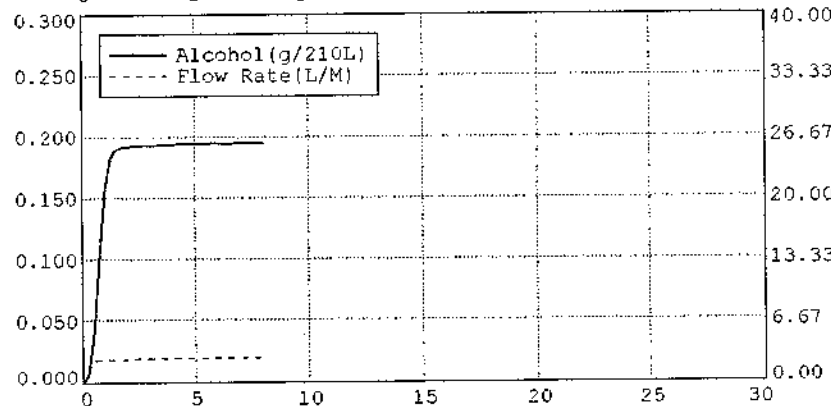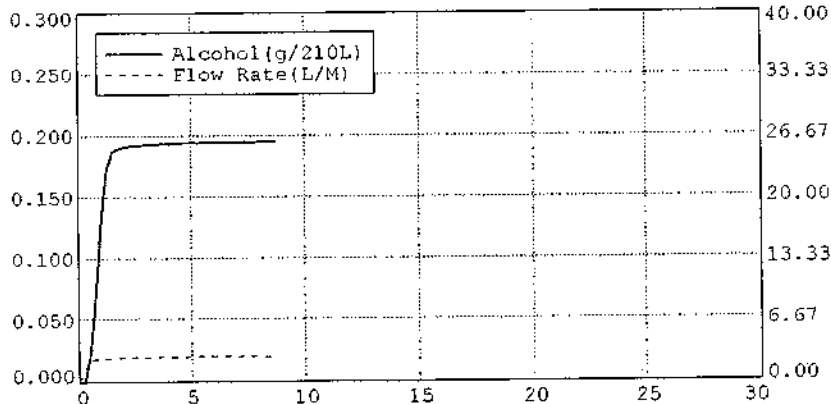

DIAGNOSTIC RECORD

Alaska Department of Public Safety  
DATAMASTER dmt: 100353

Date: 11/07/2019  
Time: 11:57:43

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.1°C PASSED  
Breath Tube = 48.1°C PASSED

PUMP INFO  
Flow Rate = 5.018 L/M PASSED

DETECTOR INFO  
PUMP ON PASSED  
PUMP OFF PASSED

FILTER INFO  
Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED

*In-house QA*

*• 100353*

*• 100405*

*• 100671*

*003 11/7/19*



Technician Screen

-----  
DATAMASTER dmt: 100353  
-----

Date: 11/07/2019

Time: 12:01 PM

Temperatures (°C)

Sample Cell: 48.7°C

Breath Tube: 48.1°C

Current Barometer 29.5 in

Volume (Ltr) 0.00

Settings

Lamp: 2.31 V

Bias: 79 V

Cooler: 1.90 V

Chopper: 536 Hz

Voltages (V)

Flow: 1.06 V

Detector: 0.079 V

LINEARITY CHECK

Alaska Department of Public Safety  
DATAMASTER dmt: 100353


Date: 11/07/2019  
Time: 13:26:42

SUPERVISOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.099	0.0992	0.0004
0.300	0.3032	0.0008

SLOPE = 1.012114  
R<sup>2</sup> = 0.999993

CM

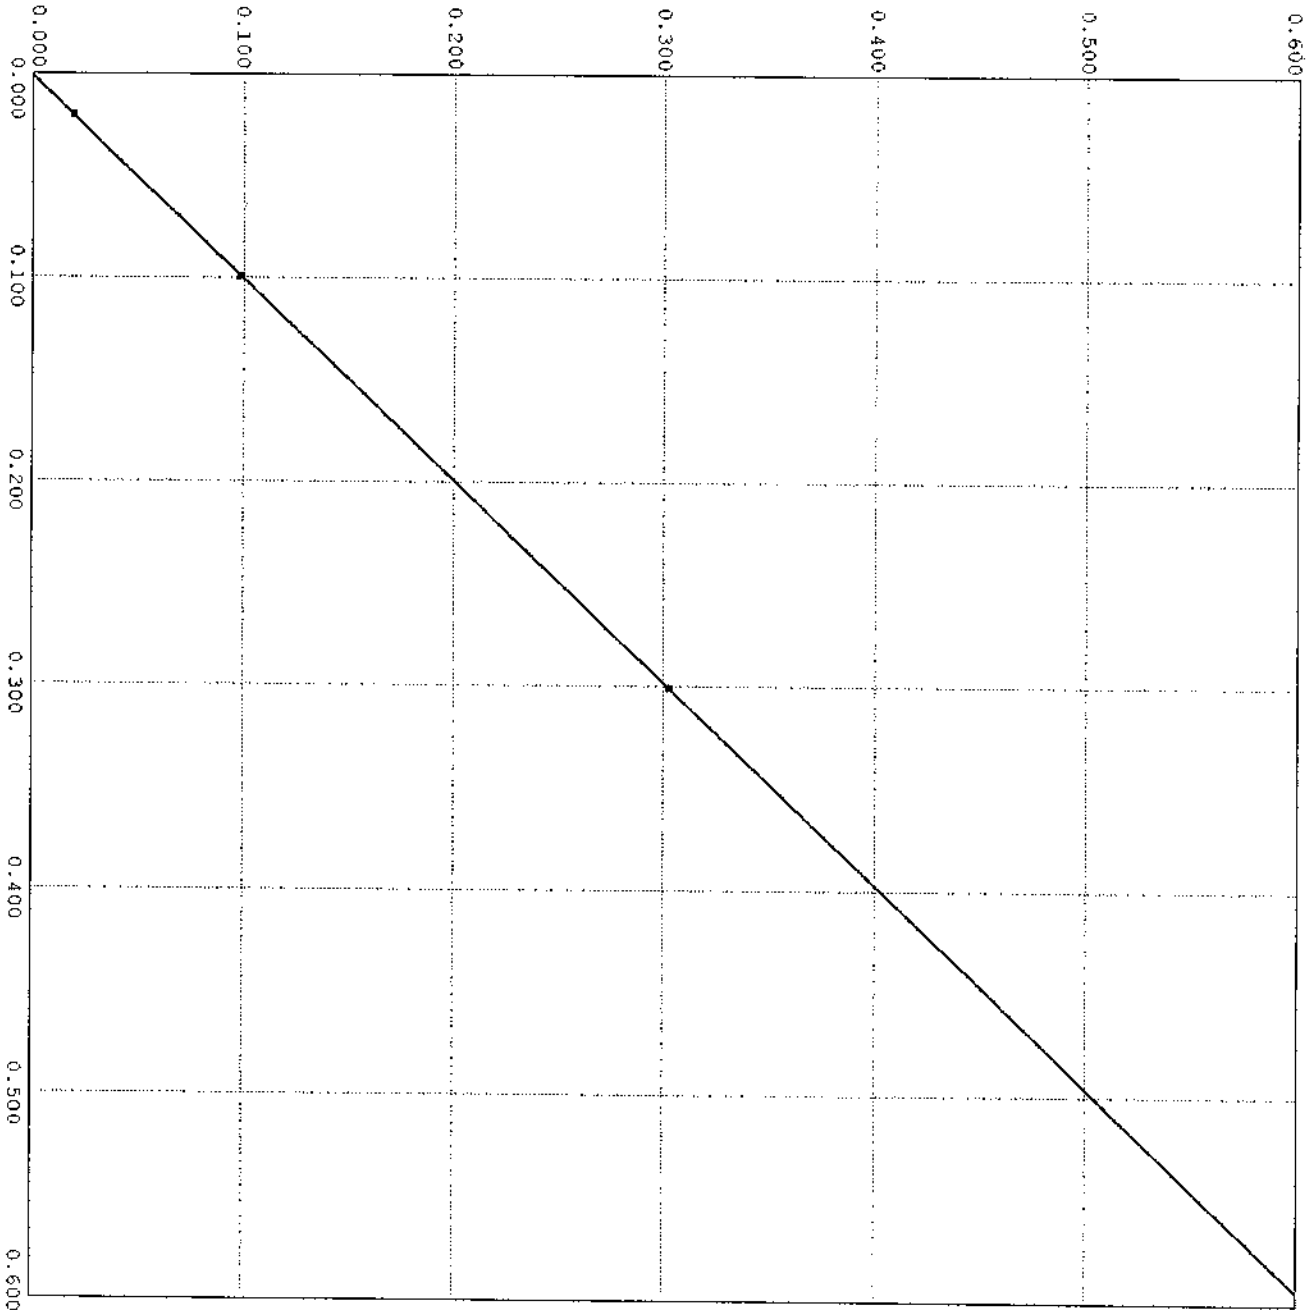

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100353






Date: 11/07/2019  
 Time: 13:26:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.52: 0.020  
 LOT #: AG805804  
 EXPIRATION: 02/27/2020  
 TANK PRESSURE: 423 psi

BLANK TEST	0.000	13:28
INTERNAL STANDARD	VERIFIED	13:28
EXTERNAL STANDARD	0.020	13:28
BLANK TEST	0.000	13:29
EXTERNAL STANDARD	0.020	13:29
BLANK TEST	0.000	13:30
EXTERNAL STANDARD	0.020	13:30
BLANK TEST	0.000	13:31
EXTERNAL STANDARD	0.020	13:31
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.020	13:32
BLANK TEST	0.000	13:33

Average = 0.0200  
 Std Dev = 0.0000

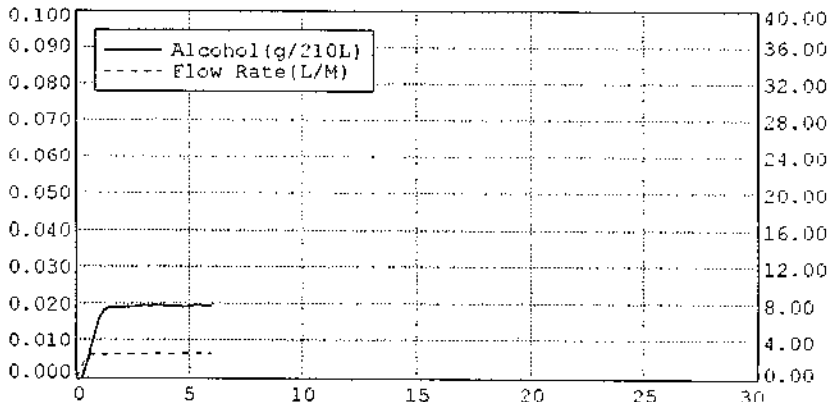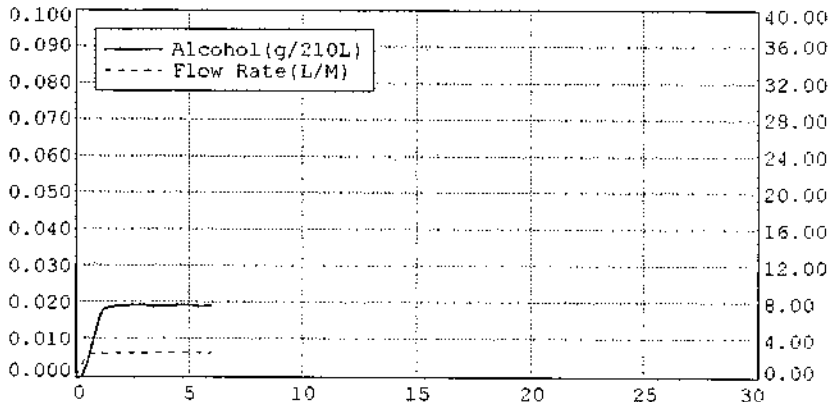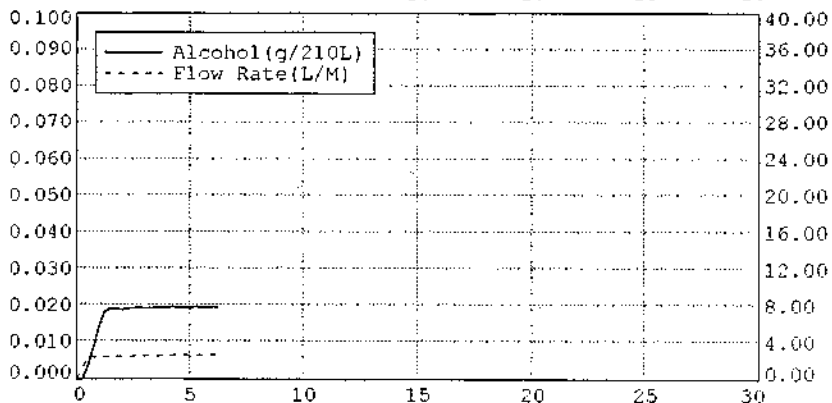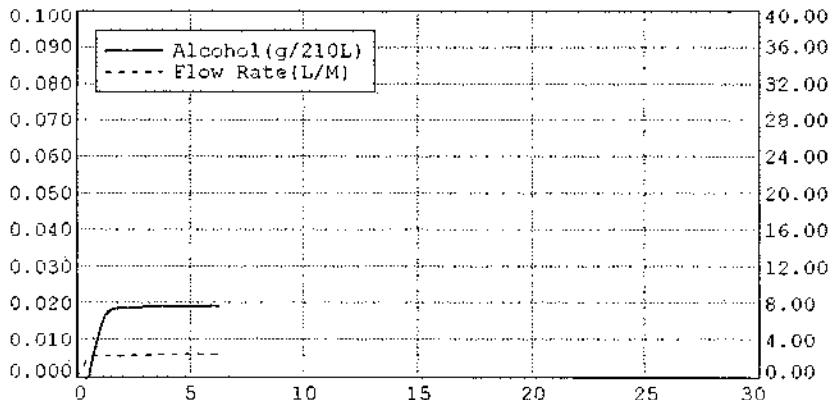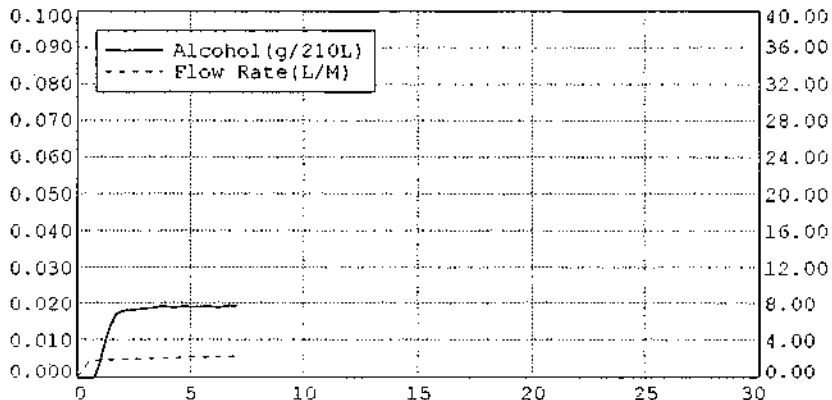

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100353






Date: 11/07/2019  
 Time: 13:35:03

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.51: 0.099  
 LOT #: ~~ACC805903~~ **AG805903**  
 EXPIRATION: 02/28/2020  
 TANK PRESSURE: 857 psi

BLANK TEST	0.000	13:36
INTERNAL STANDARD	VERIFIED	13:36
EXTERNAL STANDARD	0.100	13:36
BLANK TEST	0.000	13:37
EXTERNAL STANDARD	0.099	13:38
BLANK TEST	0.000	13:39
EXTERNAL STANDARD	0.099	13:39
BLANK TEST	0.000	13:40
EXTERNAL STANDARD	0.099	13:40
BLANK TEST	0.000	13:41
EXTERNAL STANDARD	0.099	13:41
BLANK TEST	0.000	13:42

Average = 0.0992  
 Std Dev = 0.0004

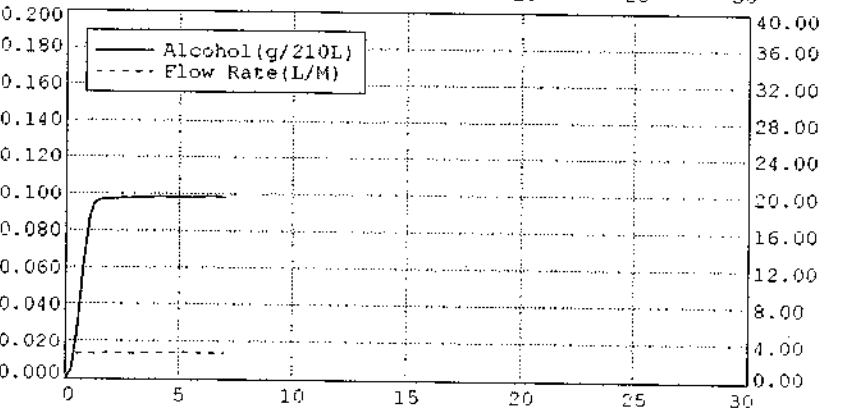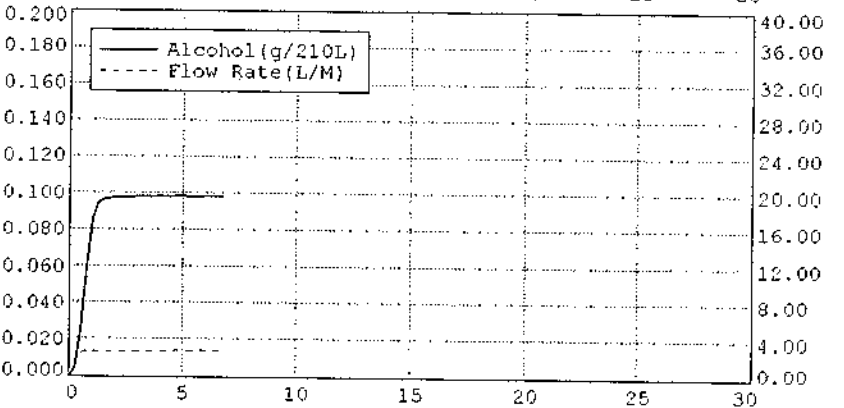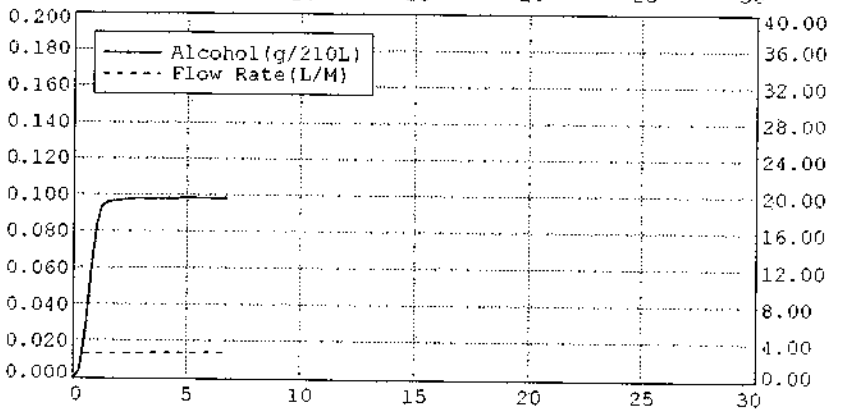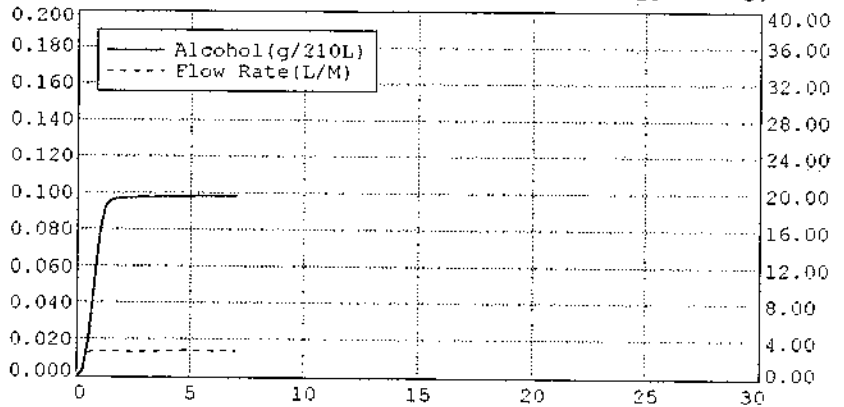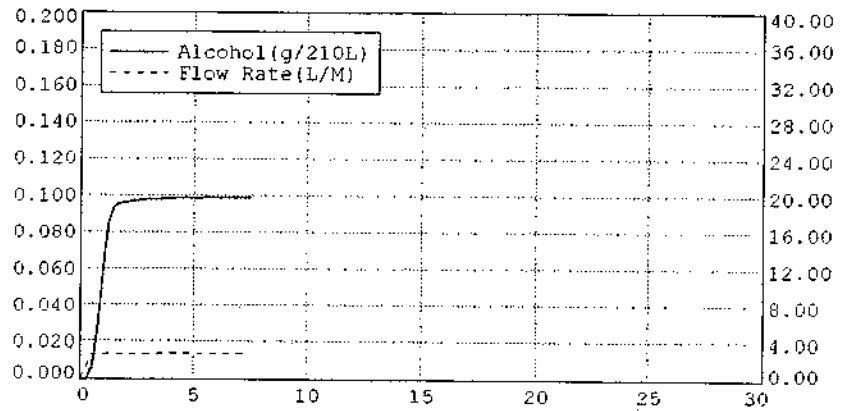

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100353






Date: 11/07/2019  
 Time: 13:47:05

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.300  
 LOT #: 19010  
 EXPIRATION: 01/03/2021

BLANK TEST	0.000	13:48
INTERNAL STANDARD	VERIFIED	13:48
EXTERNAL STANDARD	0.304	13:48
BLANK TEST	0.000	13:49
EXTERNAL STANDARD	0.302	13:50
BLANK TEST	0.000	13:51
EXTERNAL STANDARD	0.303	13:51
BLANK TEST	0.000	13:52
EXTERNAL STANDARD	0.303	13:53
BLANK TEST	0.000	13:54
EXTERNAL STANDARD	0.304	13:54
BLANK TEST	0.000	13:55

Average = 0.3032  
 Std Dev = 0.0008

*Simulator SD1088  
 calibrated 3/5/19  
 COB 11/7/19*

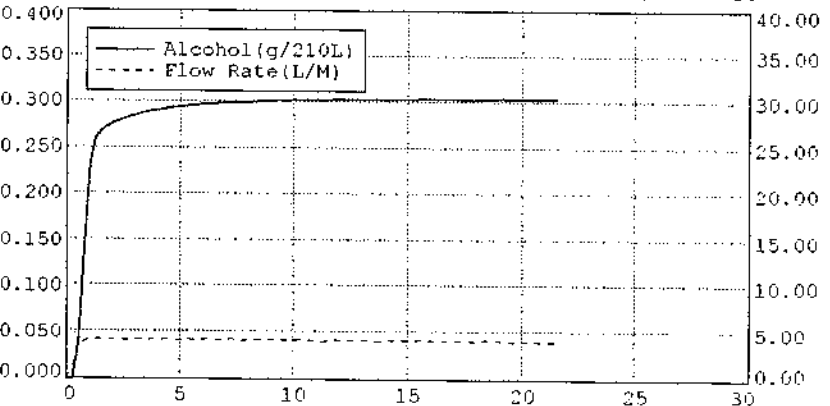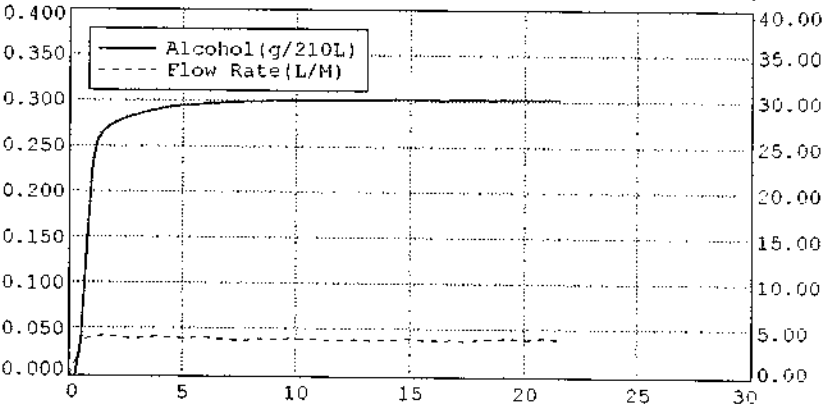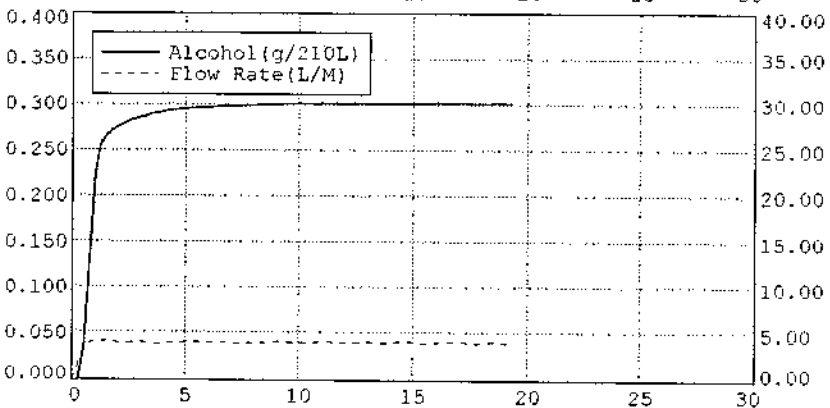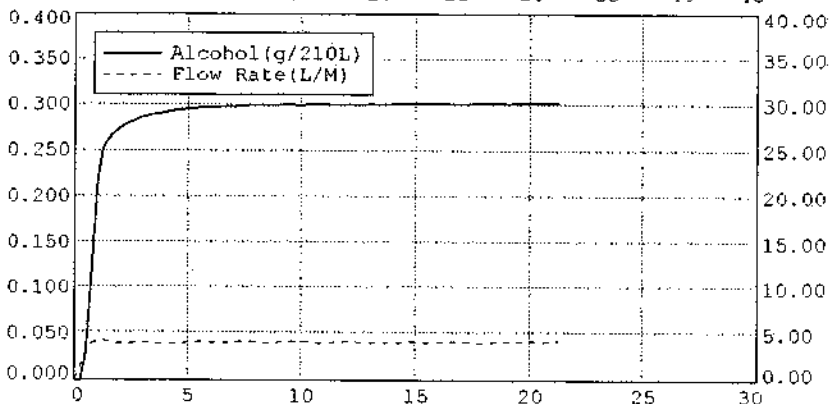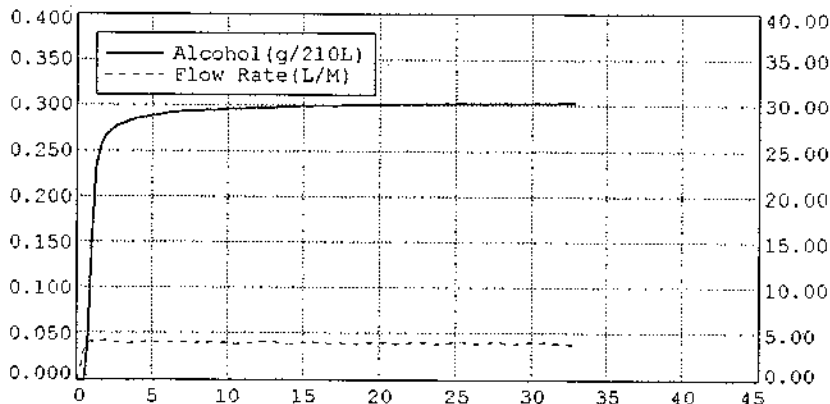

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100405  
-----

Date: 11/07/2019  
Time: 10:48:11

VERSIONS

DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED  
Breath Tube = 45.9°C PASSED

PUMP INFO

Flow Rate = 5.045 L/M PASSED

DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED

Technician Screen

-----  
DATAMASTER dmt: 100405  
-----

Date: 11/07/2019  
Time: 10:52 AM

Temperatures (°C)  
Sample Cell: 48.7°C  
Breath Tube: 45.6°C

Current Barometer 29.5 in  
Volume (Ltr) 0.00

Settings  
Lamp: 1.75 V  
Bias: 81 V  
Cooler: 1.71 V  
Chopper: 527 Hz

Voltages (V)  
Flow: 1.05 V  
Detector: 0.035 V

LINEARITY CHECK

Alaska Department of Public Safety  
DATAMASTER dmt: 100405


Date: 11/07/2019  
Time: 12:18:27

SUPERVISOR NAME:  
COLLEEN S O'BRYEN  
OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0196	0.0005
0.099	0.0962	0.0004
0.300	0.2942	0.0004

SLOPE = 0.981569  
R<sup>2</sup> = 0.999988

C103

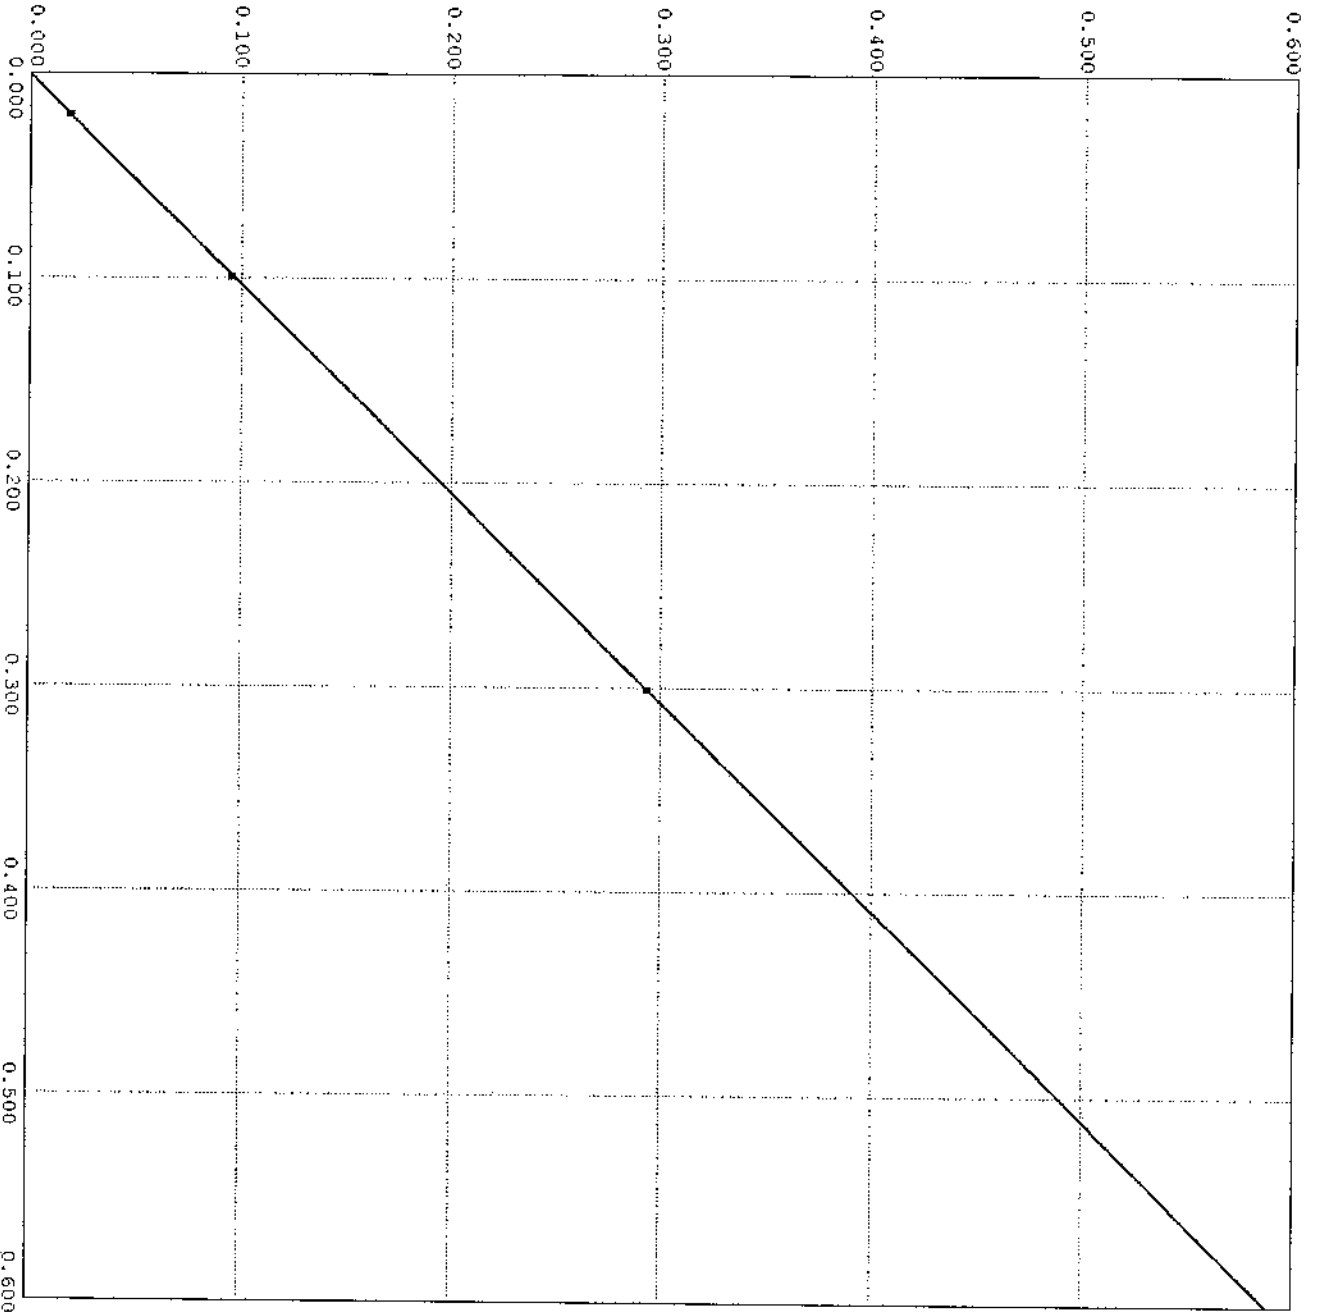



LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100405






Date: 11/07/2019  
 Time: 12:18:28

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.52: 0.020  
 LOT #: AG805804  
 EXPIRATION: 02/27/2020  
 TANK PRESSURE: 402 psi

BLANK TEST	0.000	12:26
INTERNAL STANDARD	VERIFIED	12:26
EXTERNAL STANDARD	0.020	12:27
BLANK TEST	0.000	12:27
EXTERNAL STANDARD	0.020	12:28
BLANK TEST	0.000	12:29
EXTERNAL STANDARD	0.019	12:29
BLANK TEST	0.000	12:30
EXTERNAL STANDARD	0.020	12:30
BLANK TEST	0.000	12:31
EXTERNAL STANDARD	0.019	12:31
BLANK TEST	0.000	12:32

Average = 0.0196  
 Std Dev = 0.0005

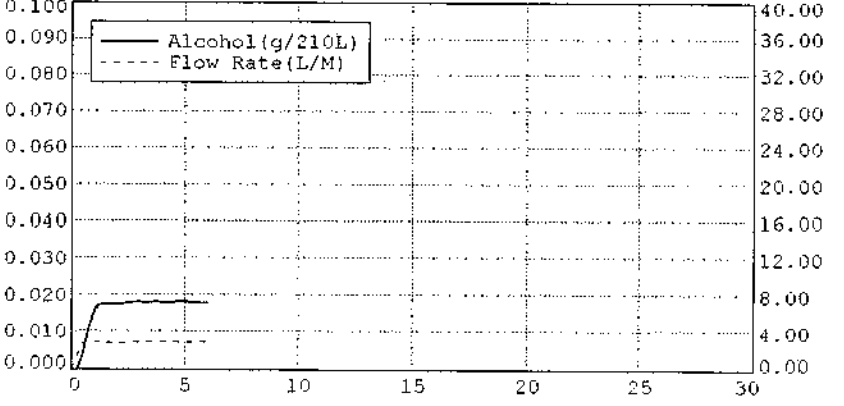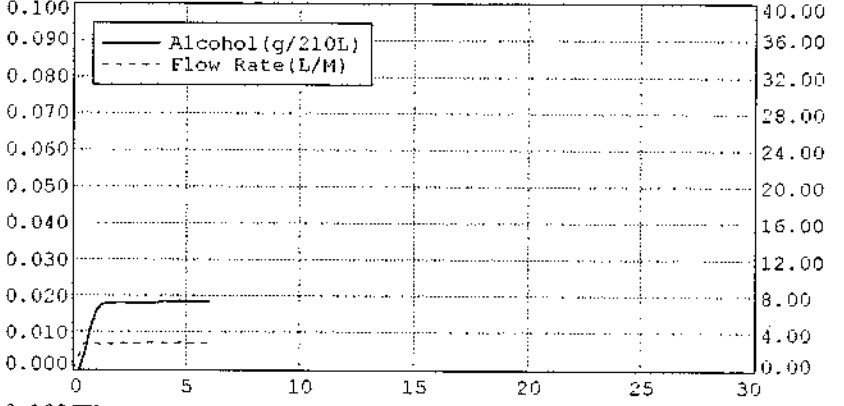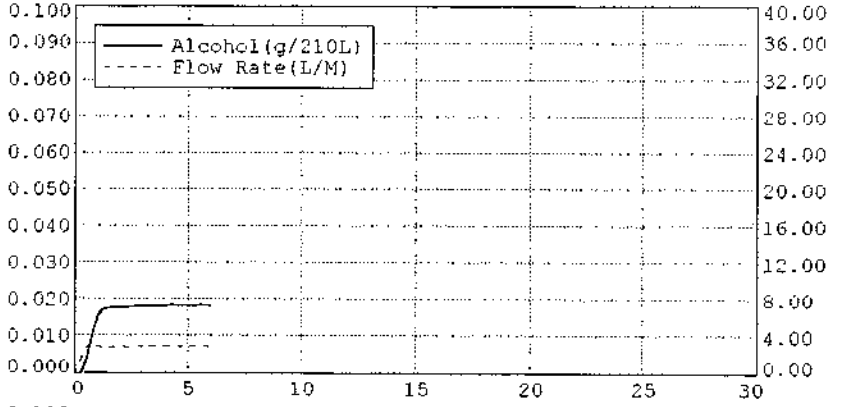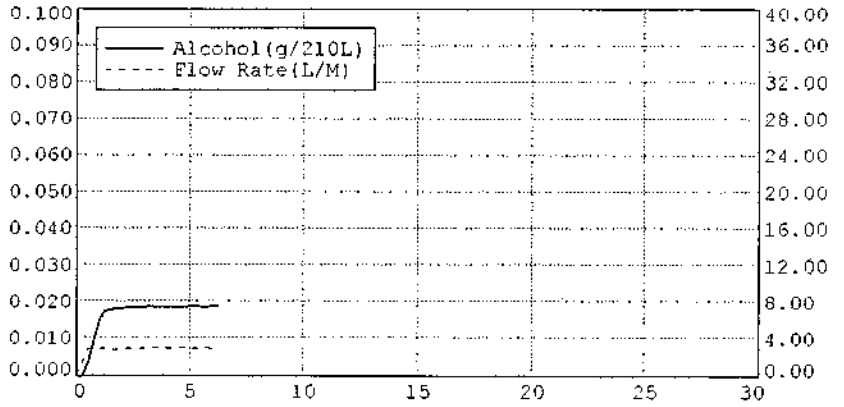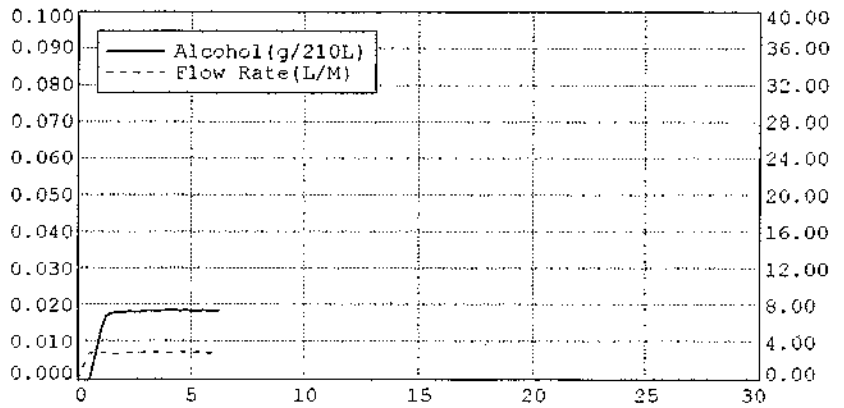

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100405






Date: 11/07/2019  
 Time: 12:36:43

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.52: 0.099  
 LOT #: AG805903  
 EXPIRATION: 02/28/2020  
 TANK PRESSURE: 832 psi

BLANK TEST	0.000	12:37
INTERNAL STANDARD	VERIFIED	12:37
EXTERNAL STANDARD	0.097	12:38
BLANK TEST	0.000	12:39
EXTERNAL STANDARD	0.096	12:39
BLANK TEST	0.000	12:40
EXTERNAL STANDARD	0.096	12:40
BLANK TEST	0.000	12:41
EXTERNAL STANDARD	0.096	12:41
BLANK TEST	0.000	12:42
EXTERNAL STANDARD	0.096	12:42
BLANK TEST	0.000	12:43

Average = 0.0962  
 Std Dev = 0.0004

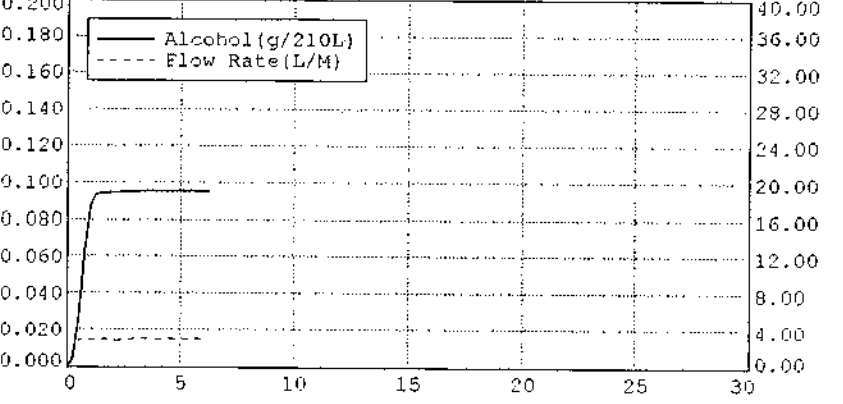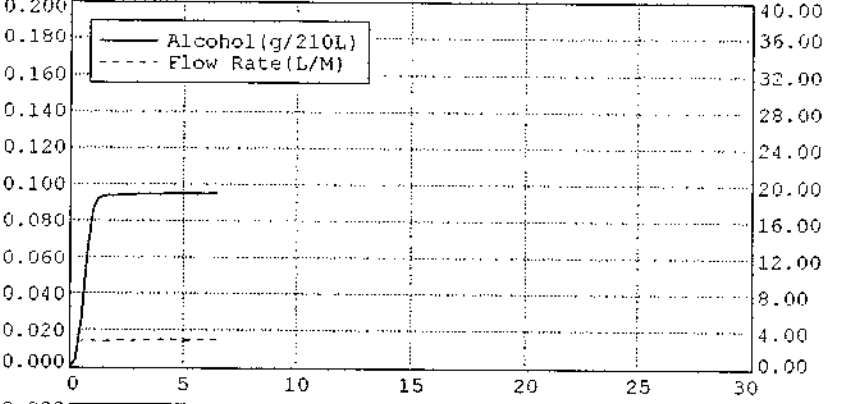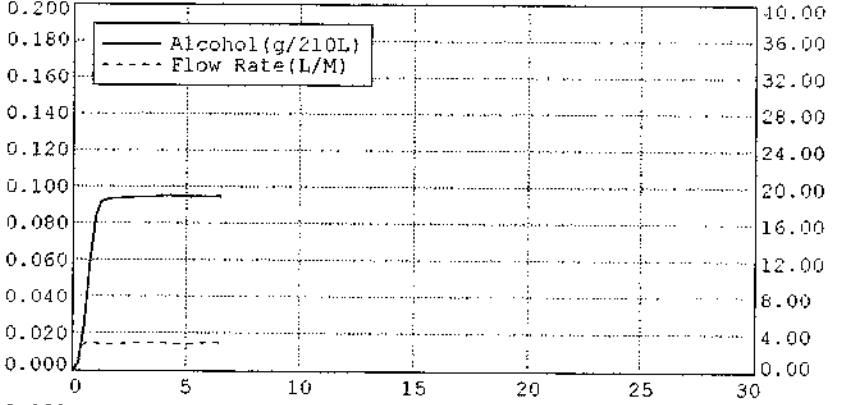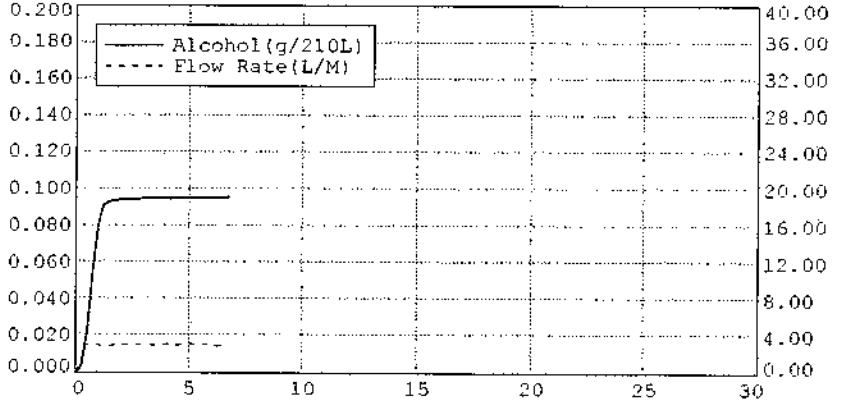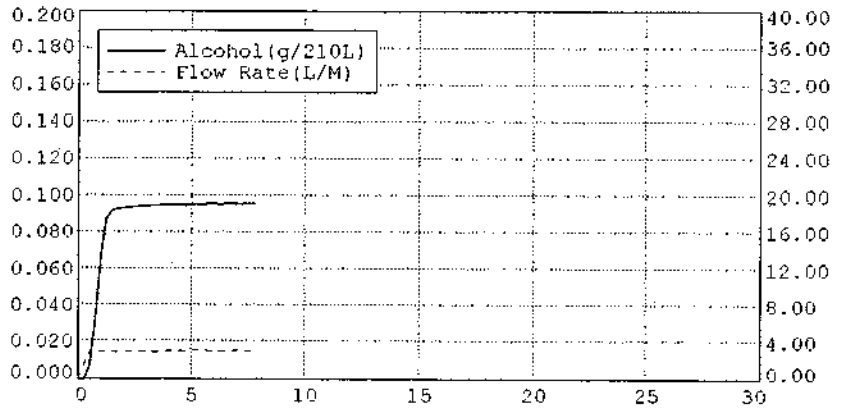

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100405

Date: 11/07/2019  
 Time: 12:45:38






EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 LOT #: 19010  
 EXPIRATION: 01/03/2021

BLANK TEST	0.000	12:47
INTERNAL STANDARD	VERIFIED	12:47
EXTERNAL STANDARD	0.295	12:48
BLANK TEST	0.000	12:49
EXTERNAL STANDARD	0.294	12:49
BLANK TEST	0.000	12:50
EXTERNAL STANDARD	0.294	12:51
BLANK TEST	0.000	12:51
EXTERNAL STANDARD	0.294	12:52
BLANK TEST	0.000	12:53
EXTERNAL STANDARD	0.294	12:53
BLANK TEST	0.000	12:54

Average = 0.2942  
 Std Dev = 0.0004

*Simulator SD1088  
 calibrated 3/5/19  
 COB 11/7/19*

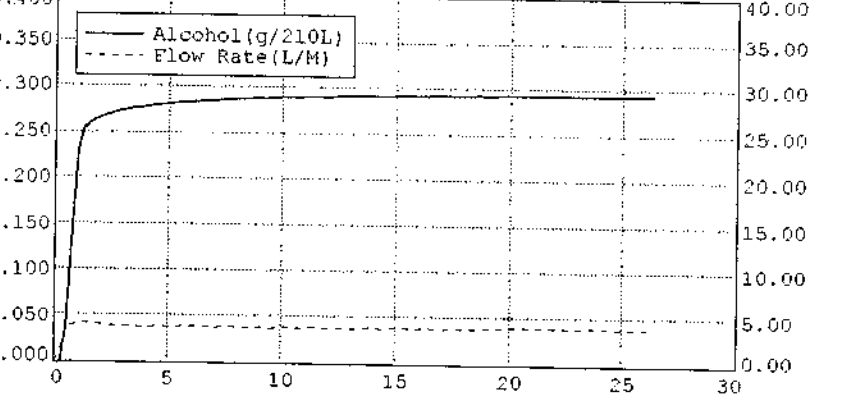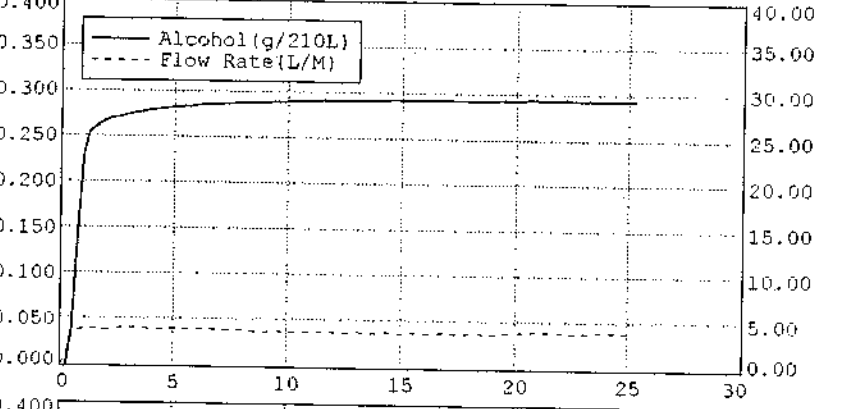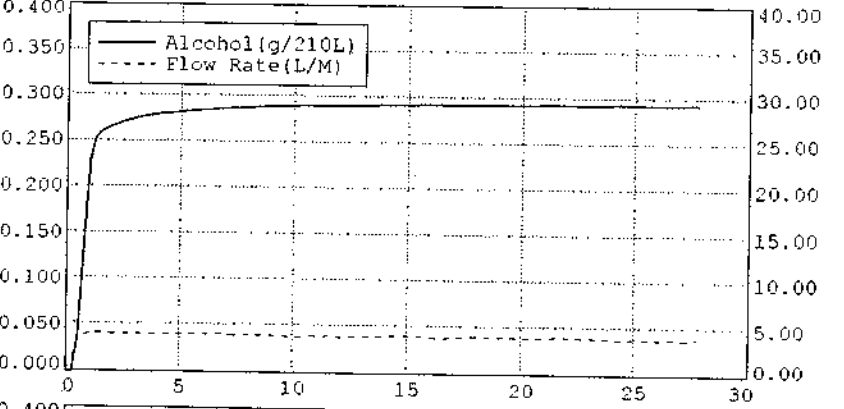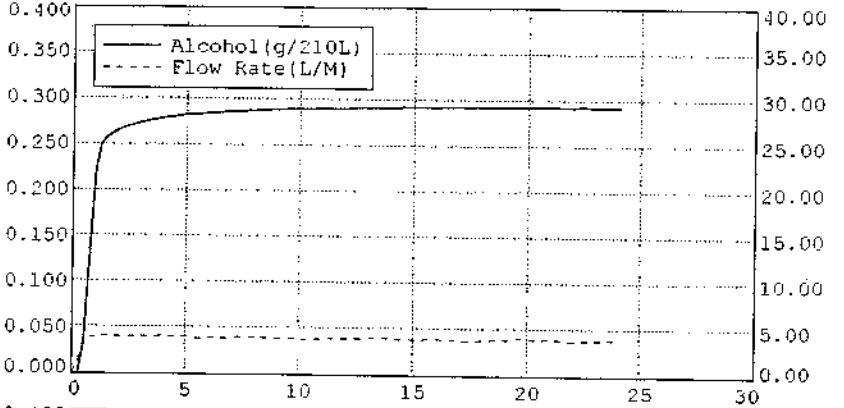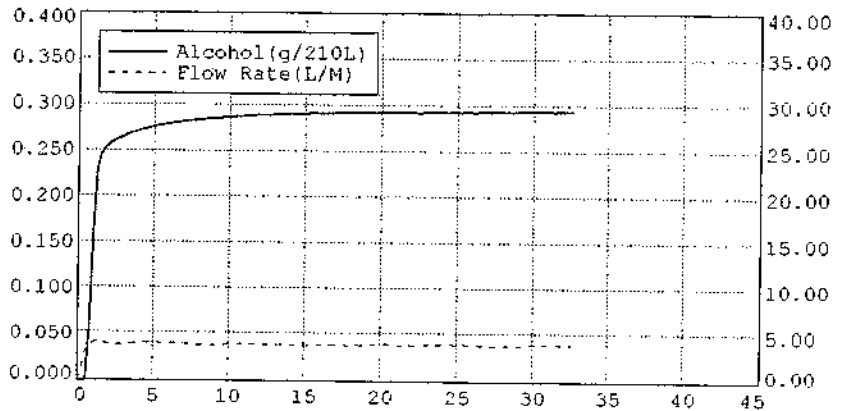

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100671  
-----

Date: 11/07/2019  
Time: 10:57:12

VERSIONS

DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED  
Breath Tube = 46.9°C PASSED

PUMP INFO

Flow Rate = 4.719 L/M PASSED

DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED

Technician Screen

-----  
DATAMASTER dmt: 100671  
-----

Date: 11/07/2019  
Time: 11:01 AM

Temperatures (°C)

Sample Cell: 48.9°C  
Breath Tube: 47.1°C

Current Barometer 29.5 in  
Volume (Ltr) 0.00

Settings

Lamp: 1.69 V  
Bias: 79 V  
Cooler: 1.78 V  
Chopper: 543 Hz

Voltages (V)

Flow: 1.06 V  
Detector: 0.040 V

LINEARITY CHECK

Alaska Department of Public Safety  
DATAMASTER dmt: 100671


Date: 11/07/2019  
Time: 12:35:49

SUPERVISOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.099	0.0982	0.0004
0.300	0.2998	0.0008

SLOPE = 1.000011  
R<sup>2</sup> = 0.999992

MS

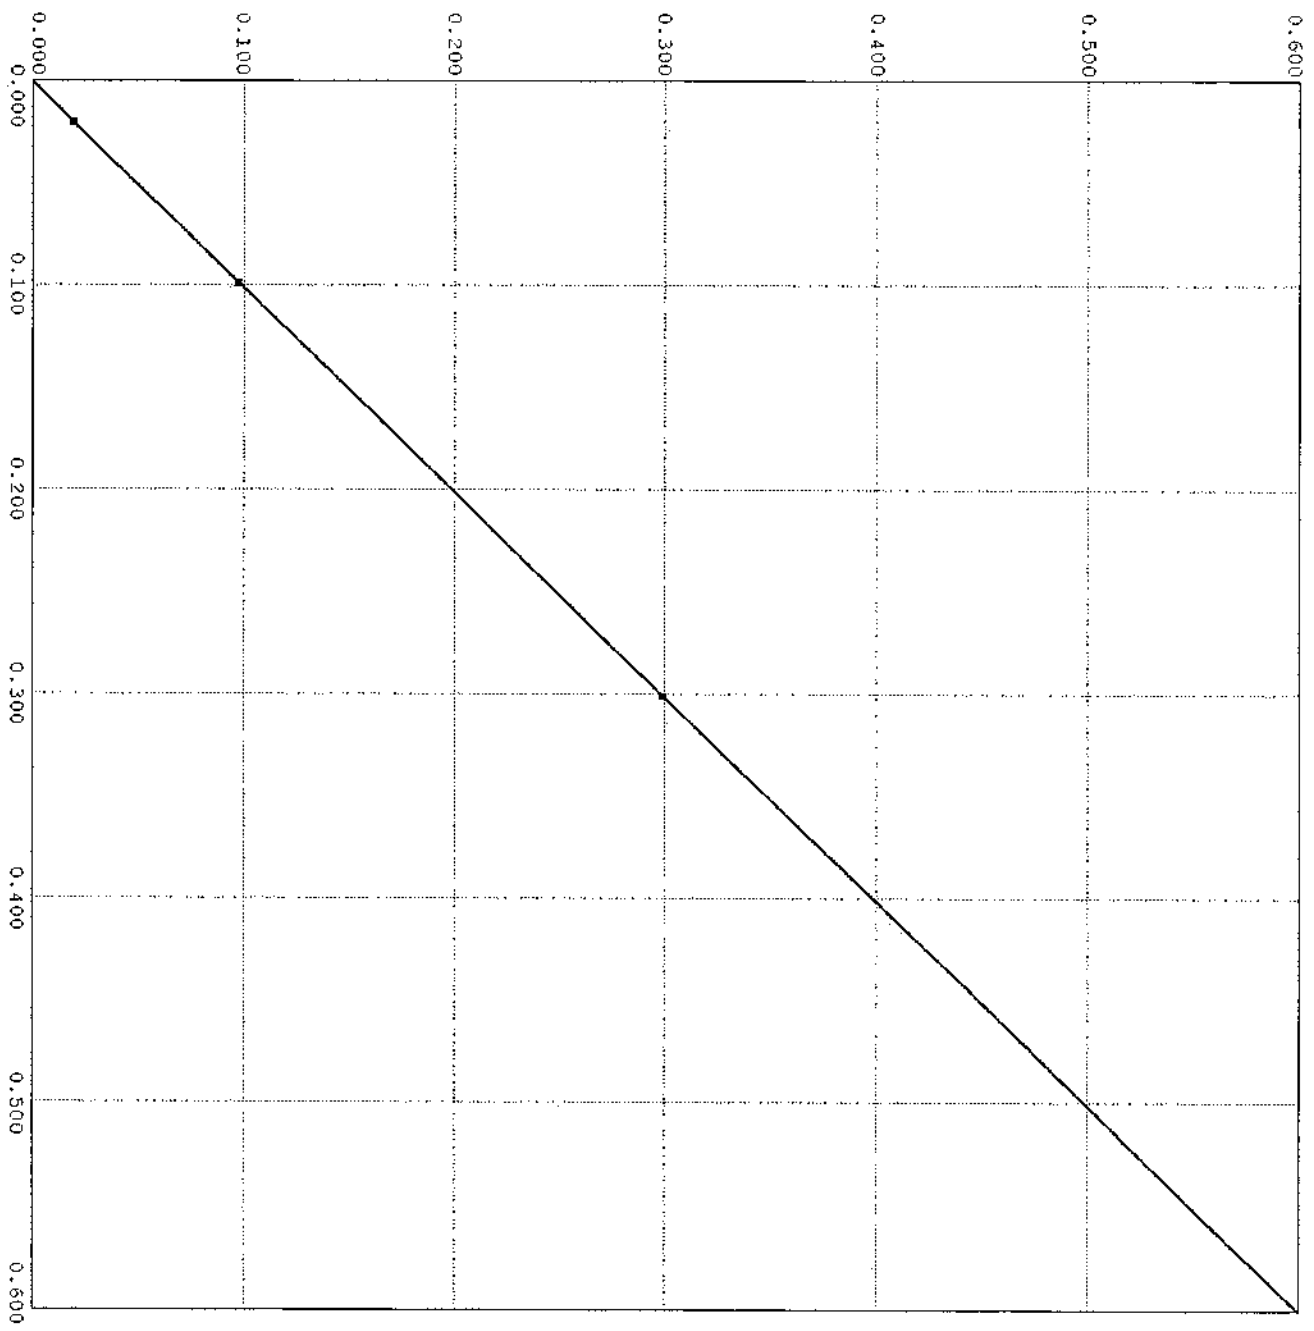

LINEARITY CHECK: Control Test 1






Alaska Department of Public Safety  
 DATAMASTER dmt: 100671

Date: 11/07/2019  
 Time: 12:45:06

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.020  
 TARGET AT 29.52: 0.020  
 LOT #: AG805804  
 EXPIRATION: 02/27/2020  
 TANK PRESSURE: 395 psi

BLANK TEST	0.000	12:46
INTERNAL STANDARD	VERIFIED	12:46
EXTERNAL STANDARD	0.020	12:46
BLANK TEST	0.000	12:47
EXTERNAL STANDARD	0.020	12:47
BLANK TEST	0.000	12:48
EXTERNAL STANDARD	0.020	12:48
BLANK TEST	0.000	12:49
EXTERNAL STANDARD	0.020	12:49
BLANK TEST	0.000	12:50
EXTERNAL STANDARD	0.020	12:50
BLANK TEST	0.000	12:51

Average = 0.0200  
 Std Dev = 0.0000

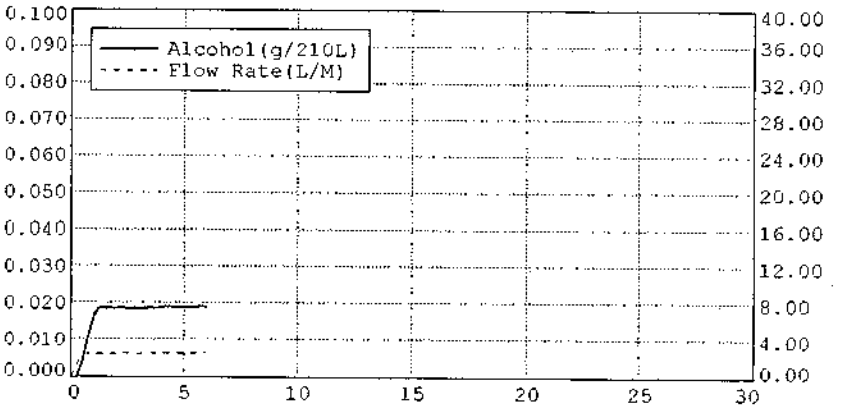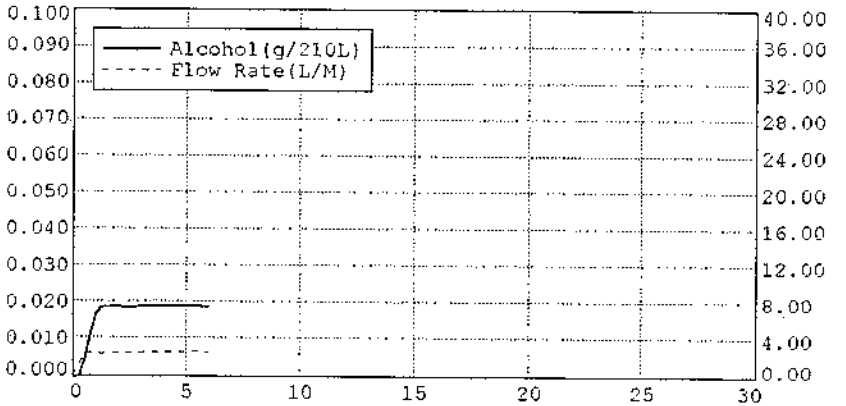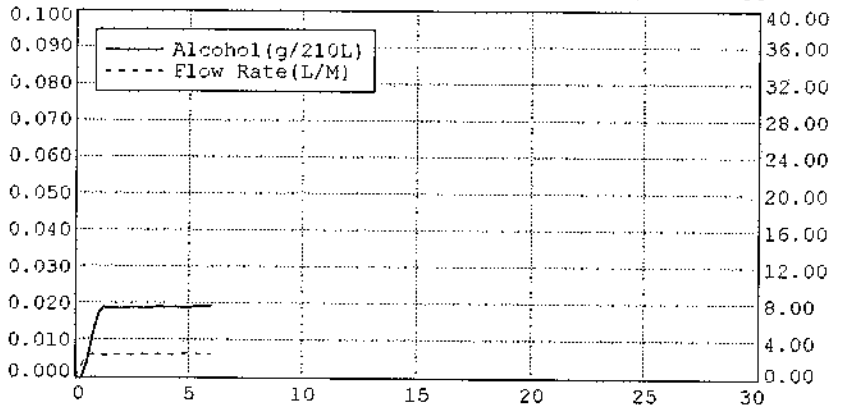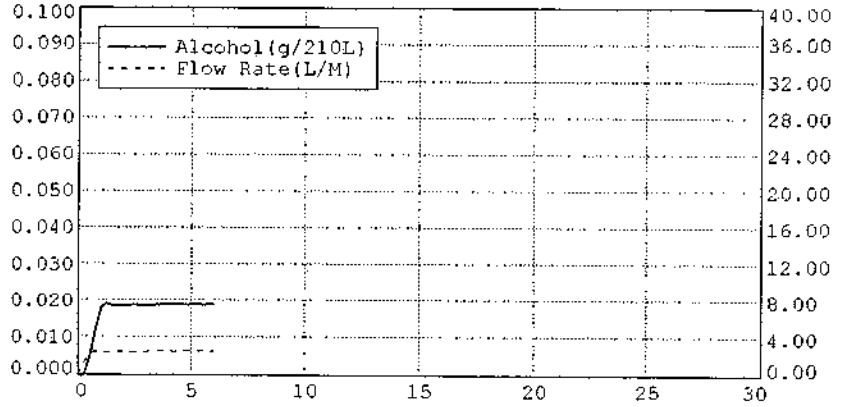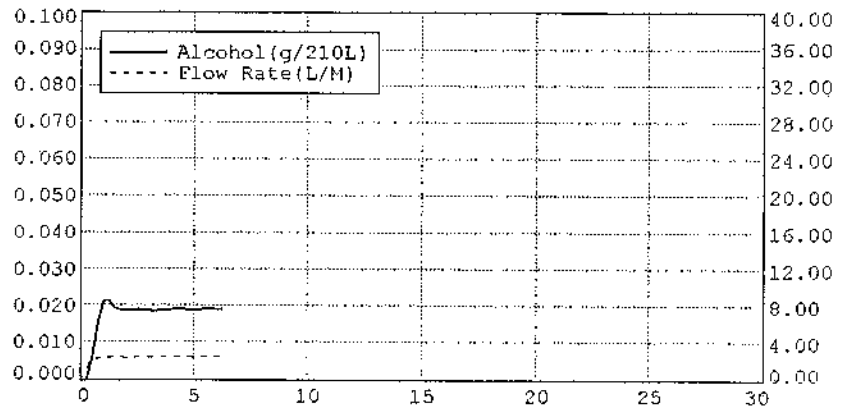

LINEARITY CHECK: Control Test 2






Alaska Department of Public Safety  
 DATAMASTER dmt: 100671

Date: 11/07/2019  
 Time: 12:56:13

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.100  
 TARGET AT 29.52: 0.099  
 LOT #: AG805903  
 EXPIRATION: 02/28/2020  
 TANK PRESSURE: 821 psi

BLANK TEST	0.000	12:57
INTERNAL STANDARD	VERIFIED	12:57
EXTERNAL STANDARD	0.098	12:57
BLANK TEST	0.000	12:58
EXTERNAL STANDARD	0.098	12:58
BLANK TEST	0.000	12:59
EXTERNAL STANDARD	0.098	12:59
BLANK TEST	0.000	13:00
EXTERNAL STANDARD	0.098	13:00
BLANK TEST	0.000	13:01
EXTERNAL STANDARD	0.099	13:02
BLANK TEST	0.000	13:03

Average = 0.0982  
 Std Dev = 0.0004

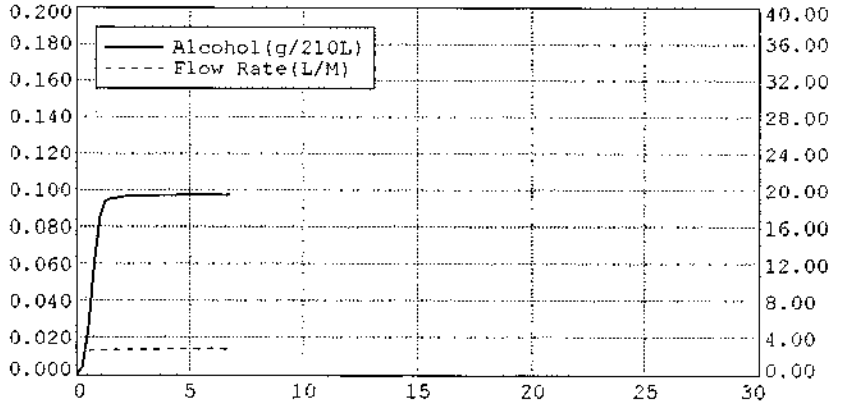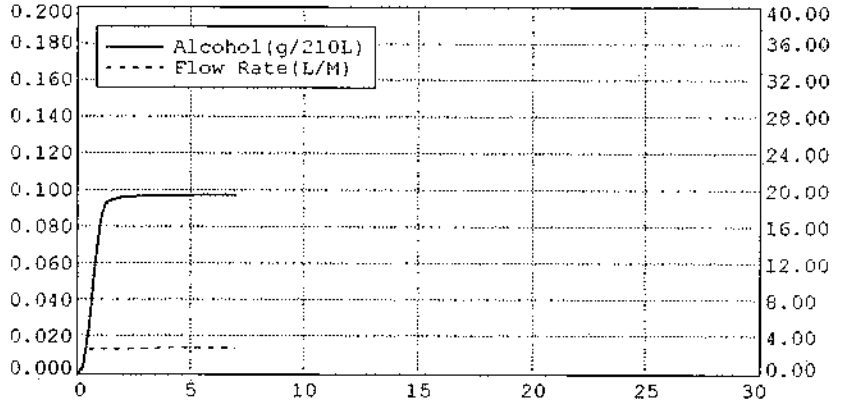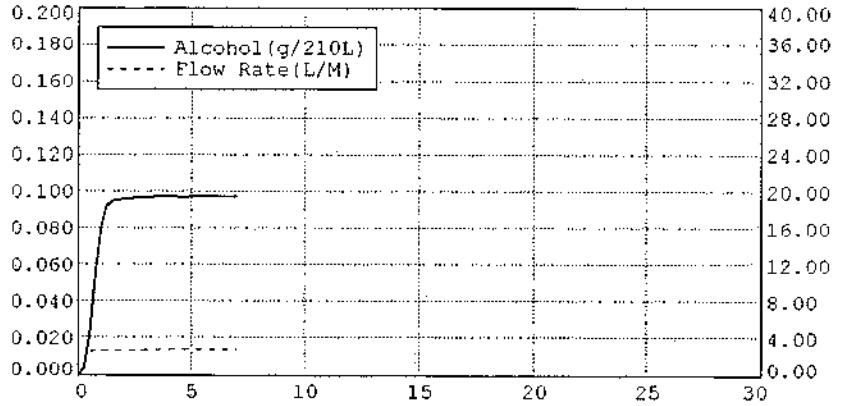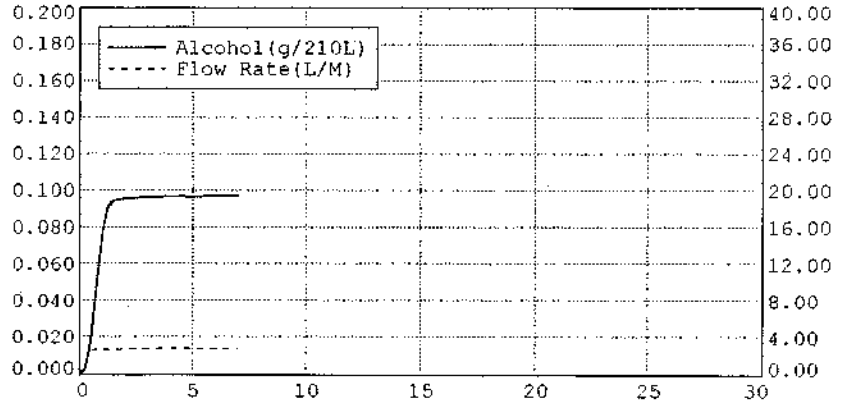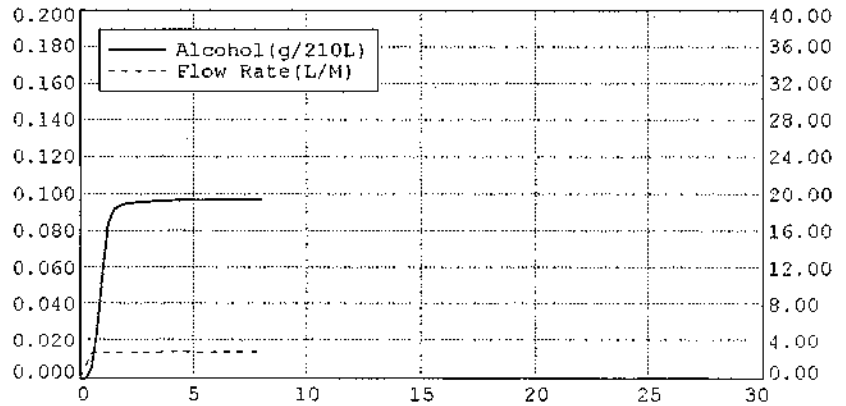



LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100671

Date: 11/07/2019  
 Time: 13:07:46

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.300  
 LOT #: 19010  
 EXPIRATION: 01/03/2021

BLANK TEST	0.000	13:09
INTERNAL STANDARD	VERIFIED	13:09
EXTERNAL STANDARD	0.299	13:10
BLANK TEST	0.000	13:11
EXTERNAL STANDARD	0.300	13:11
BLANK TEST	0.000	13:12
EXTERNAL STANDARD	0.299	13:13
BLANK TEST	0.000	13:14
EXTERNAL STANDARD	0.300	13:14
BLANK TEST	0.000	13:15
EXTERNAL STANDARD	0.301	13:16
BLANK TEST	0.000	13:17

Average = 0.2998  
 Std Dev = 0.0008

*Simulator SD1088  
 Calibrated 3/5/19  
 COB 11/7/19*

