



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100364

Report Issue Date: 02/21/2023
Date Received: 2022-11-14
Condition of Item: Needs Repair

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

Start Date 11/15/2022 - As Found - End Date 11/15/2022 As Found - Evaluation Analyst: Colleen O'Bryant
 As Found Conditions - Barometric Pressure (inHg): 30.37 Barometer Used: Temperature (C): 22.0 Relative Humidity (%): 18

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG100401	0.020	0.021	0.021	0.021	0.021	0.021	0.021
0.080	0.081	AG135004	0.082	0.082	0.083	0.082	0.082	0.082	0.082
0.300	0.305	AG217903	0.310	0.310	0.311	0.311	0.311	0.311	0.311

Start Date 01/03/2023 - As Left - End Date 01/04/2023
 As Left Conditions - Barometric Pressure (inHg): 29.14 Barometer Used: Fisher S/N 221250180 Temperature (C): 23.3 Relative Humidity (%): 16

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.019	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002	
0.040	0.039	AG217904	0.038	0.039	0.039	0.039	0.039	0.039	+/- 0.003	
0.080	0.078	AG113402	0.076	0.076	0.077	0.077	0.077	0.077	+/- 0.003	
0.100	0.097	AG211003	0.097	0.097	0.097	0.097	0.097	0.097	+/- 0.003	
0.150	0.146	AG134205	0.145	0.145	0.145	0.146	0.146	0.145	+/- 0.004	
0.300	0.292	AG217903	0.291	0.291	0.291	0.290	0.291	0.291	+/- 0.008	

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Technically and administratively reviewed by Brandi Barnett on 02/21/2023

Results authorized by Colleen O'Bryant on 02/16/2023
colleen.obryant@alaska.gov

* Data TR'd + entered by COB 1/9/23

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100364 Analyst: Tatiana Malnosko Start Date: 01-03-2023

- Diagnostic Test (attached)
- Adjust voltages, if needed
 - o Lamp (2.60 V Maximum)
 - o Bias
 - o Cooler (2.00 V Maximum)
- Internal Standard value \leq 3.00%
 - o Chopper Frequency
 - o Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.4 L (1.3L to 1.7L)

As Left Conditions: Barometer 221250180 exp. 02-14-2024 TLM 01-03-2023

Barometric Pressure (in Hg): 29.14 Temperature (C): 23.3 Relative Humidity (%) 16%

Linearity Test (attached)

0.020g/210L Mnf: <u>Airgas</u>	Lot: <u>AG217902</u>	Exp: <u>06-28-2024</u>
0.040g/210L Mnf: <u>Airgas</u>	Lot: <u>AG217904</u>	Exp: <u>06-28-2024</u>
0.080g/210L Mnf: <u>Airgas</u>	Lot: <u>AG113402</u>	Exp: <u>05-14-2023</u>
0.100g/210L Mnf: <u>Airgas</u>	Lot: <u>AG211003</u>	Exp: <u>04-20-2024</u>
0.150g/210L Mnf: <u>Airgas</u>	Lot: <u>AG1134205</u>	Exp: <u>12-08-2023</u>
0.300g/210L Mnf: <u>Airgas</u>	Lot: <u>AG217903</u>	Exp: <u>06-28-2024</u>

Functional Tests (attached)

- Incomplete
 - Maximum Attempts Exceeded
 - Interference (Volatiles)
 - Invalid
 - Radio Frequency Interference (RFI)
- Acetone Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11-09-2023
 Simulator S/N: DK5298 Verification Performed?
- Isopropanol Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11-09-2023
 Simulator S/N: SD1198 Verification Performed?
- Neg. Control Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11-09-2023
 Simulator S/N: SD1202 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210A58384 Calibration Due Date: 11-09-2023

- Verify stylus is calibrated
 - Reset Options
 - Clear Memory
 - Verification of Calibration (VOC)
 - Non-Drinking Subject Test
 - Upload
 - Remove Tank Prior to Shutdown
- Calibration End Date: 01-04-2023

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 08:09:33

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 46.5°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 2.18 V PASSED
(1.31 V - 3.05 V)
Cooler Voltage = 1.78 V PASSED
(1.07 V - 2.49 V)
Bias Voltage = 78 V PASSED
(47 V - 109 V)
Chopper Freq = 533 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.1 in

PUMP INFO

Flow Rate = 5.002 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.100 0.52% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 9:17 AM

Temperatures (°C)
Sample Cell: 49.6°C
Breath Tube: 45.2°C

Current Barometer 29.1 in
Volume (Ltr) 1.52

Settings
Lamp: 2.13 V
Bias: 78 V
Cooler: 1.78 V
Chopper: 533 Hz

Voltages (V)
Flow: 1.03 V
Detector: 0.089 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 12/29/2022
Time: 14:35:07

OPERATOR NAME:
COLLEEN S OBRYANT
CERTIFICATE #: 6237

Ca = 0.1000
CAL = 0.976440 0.800 <= CAL < 1.200
b1 = 0.0006 0.0000 <= b1 < 0.0040
b2 = 0.0061 0.0010 <= b2 < 0.0100
b3 = 0.0002 0.0000 <= b3 < 0.0040
Xq = 0.1007 0.0500 <= Xq < 0.2000
a21 = 1.174236 1.050 <= a21 < 1.300
a31 = 0.591726 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 09:18:51

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
MINIMUM TEST VOLUME
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.13: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:19
BLANK TEST	0.000	09:19
INTERNAL STANDARD	VERIFIED	09:20
EXTERNAL STANDARD	0.076	09:20
BLANK TEST	0.000	09:21
SUBJECT SAMPLE (Vol=1.51L)	0.000	09:21
BLANK TEST	0.000	09:22
EXTERNAL STANDARD	0.077	09:23
BLANK TEST	0.000	09:23

TLM

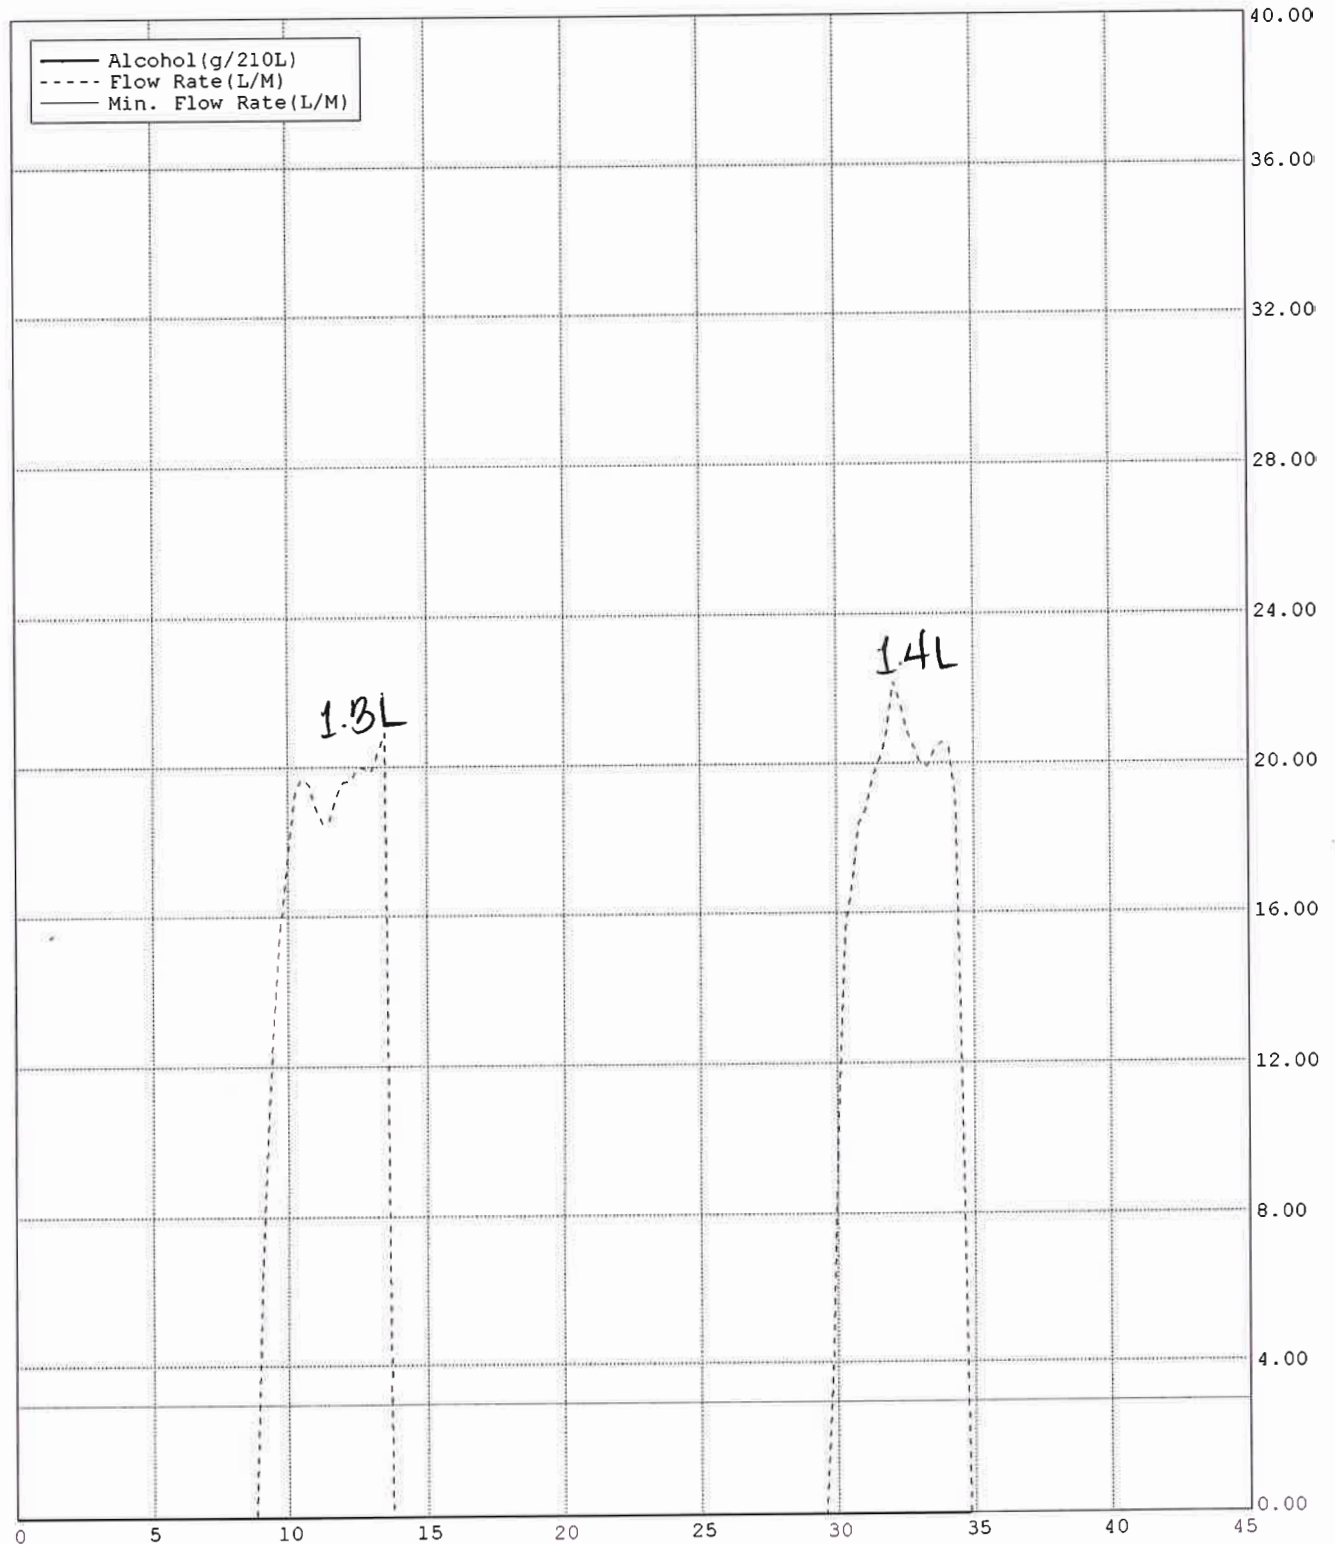

LINEARITY CHECK

Alaska Department of Public Safety
DATAMASTER dmt: 100364


Date: 01/03/2023
Time: 09:25:18

SUPERVISOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

TARGET	AVERAGE	STD. DEV.
0.019	0.0200	0.0000
0.039	0.0388	0.0004
0.078	0.0766	0.0005
0.097	0.0970	0.0000
0.146	0.1454	0.0005
0.292	0.2908	0.0004

SLOPE = 0.994529
R² = 0.999951

TLM

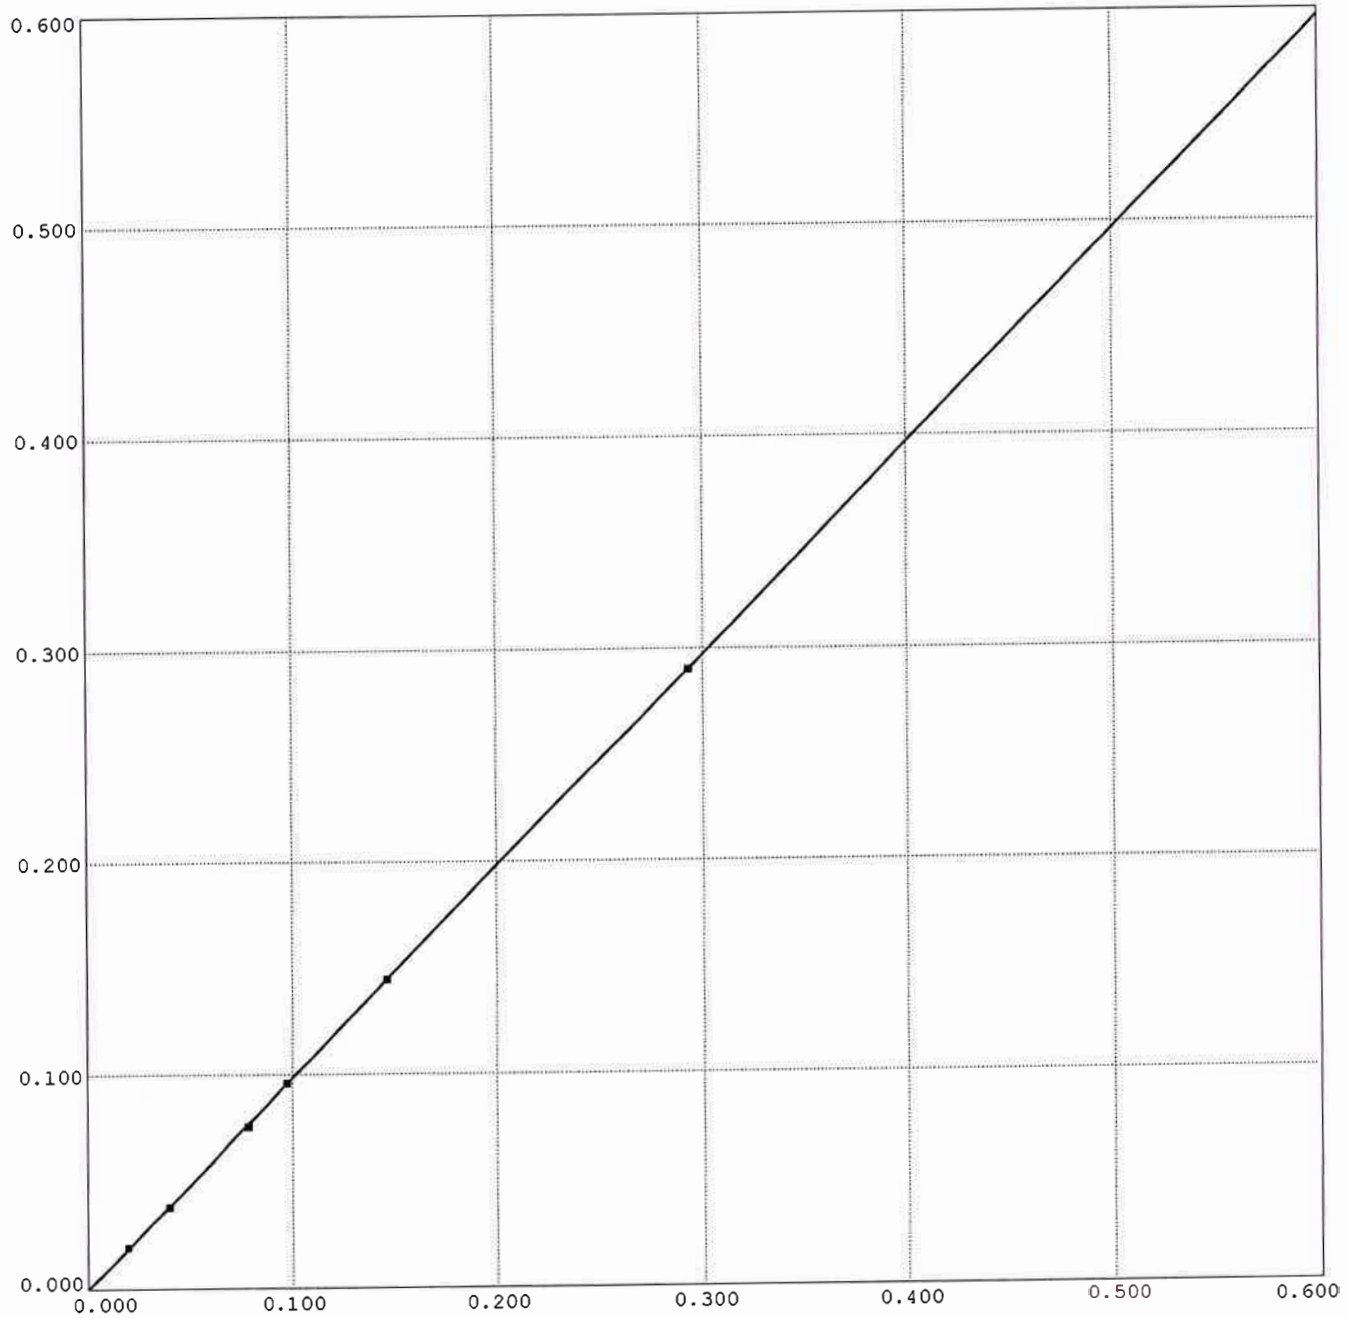

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100364






Date: 01/03/2023
 Time: 09:25:21

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.13: 0.019
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 1010 psi

BLANK TEST	0.000	09:26
INTERNAL STANDARD	VERIFIED	09:26
EXTERNAL STANDARD	0.020	09:27
BLANK TEST	0.000	09:28
EXTERNAL STANDARD	0.020	09:28
BLANK TEST	0.000	09:29
EXTERNAL STANDARD	0.020	09:29
BLANK TEST	0.000	09:30
EXTERNAL STANDARD	0.020	09:30
BLANK TEST	0.000	09:31
EXTERNAL STANDARD	0.020	09:31
BLANK TEST	0.000	09:32

Average = 0.0200
 Std Dev = 0.0000

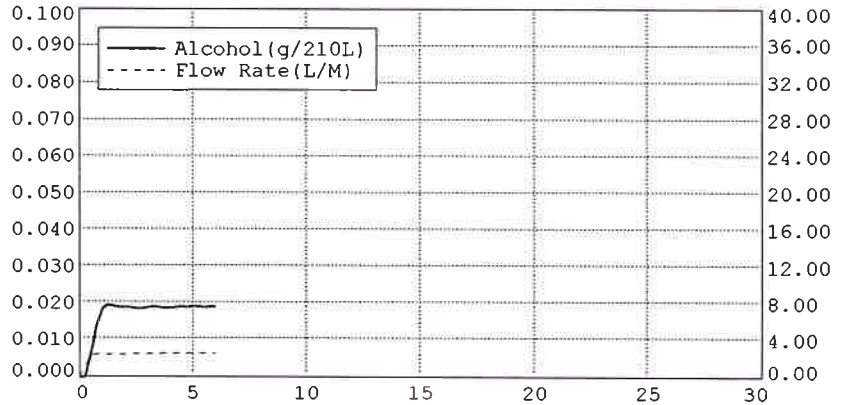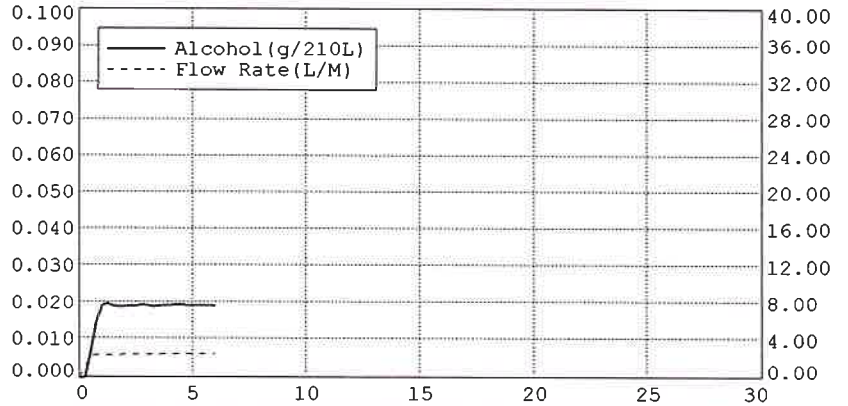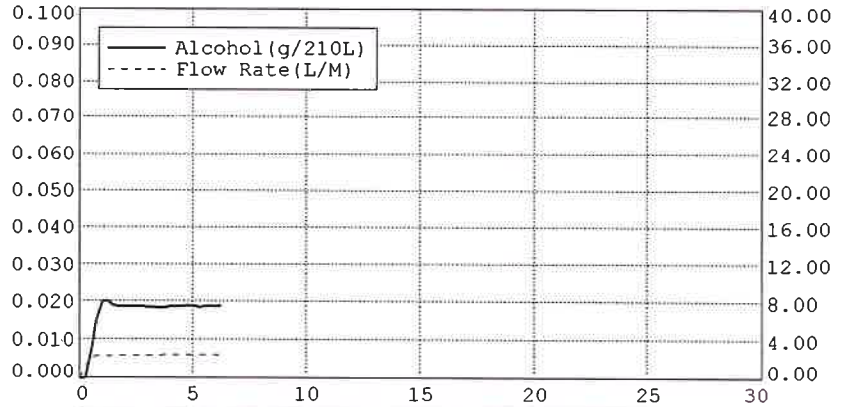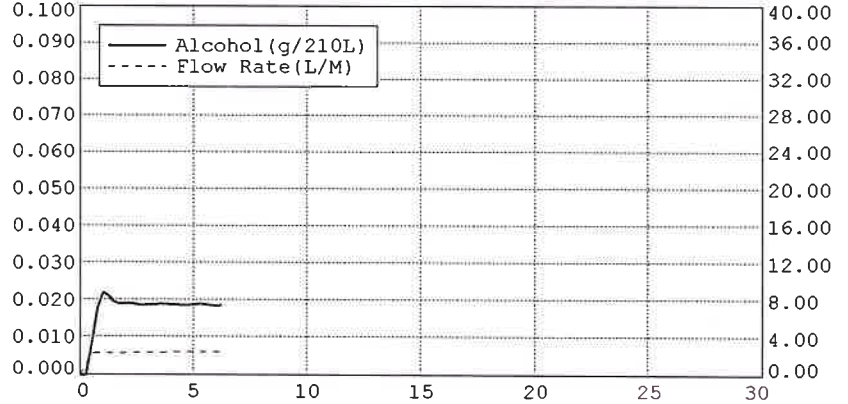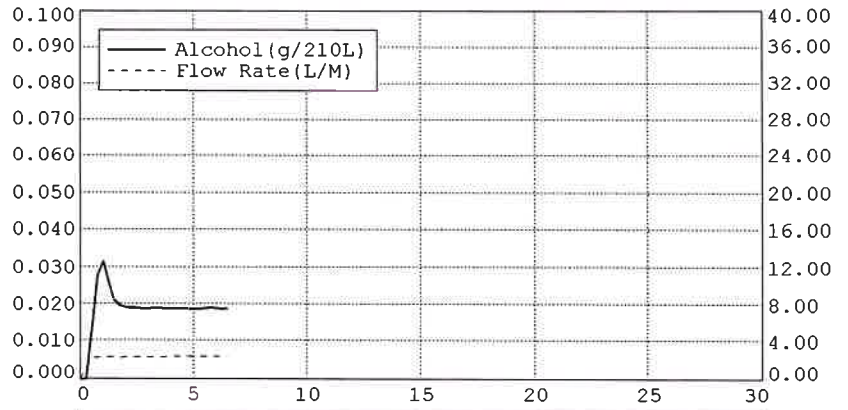

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100364






Date: 01/03/2023
 Time: 09:34:54

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.14: 0.039
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 1086 psi

BLANK TEST	0.000	09:36
INTERNAL STANDARD	VERIFIED	09:36
EXTERNAL STANDARD	0.038	09:36
BLANK TEST	0.000	09:37
EXTERNAL STANDARD	0.039	09:37
BLANK TEST	0.000	09:38
EXTERNAL STANDARD	0.039	09:38
BLANK TEST	0.000	09:39
EXTERNAL STANDARD	0.039	09:39
BLANK TEST	0.000	09:40
EXTERNAL STANDARD	0.039	09:41
BLANK TEST	0.000	09:41

Average = 0.0388
 Std Dev = 0.0004

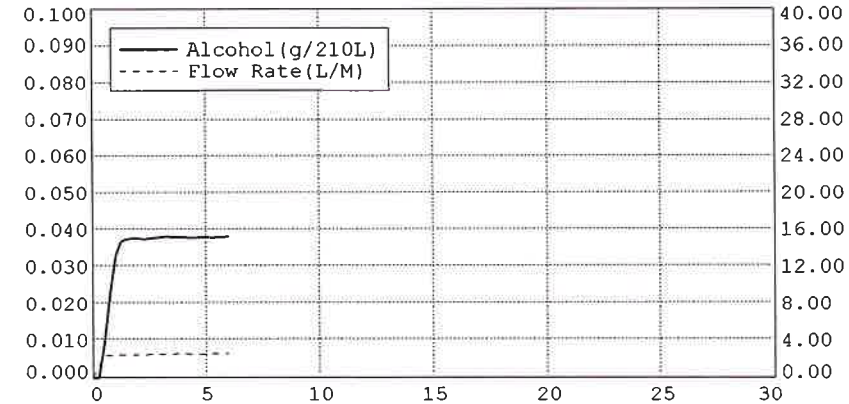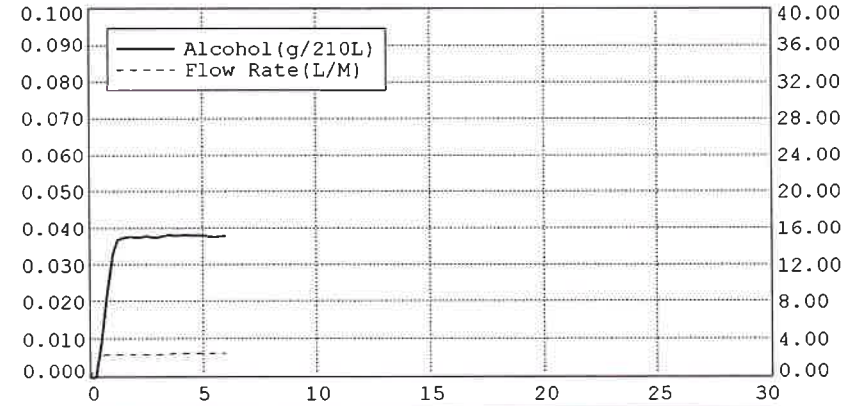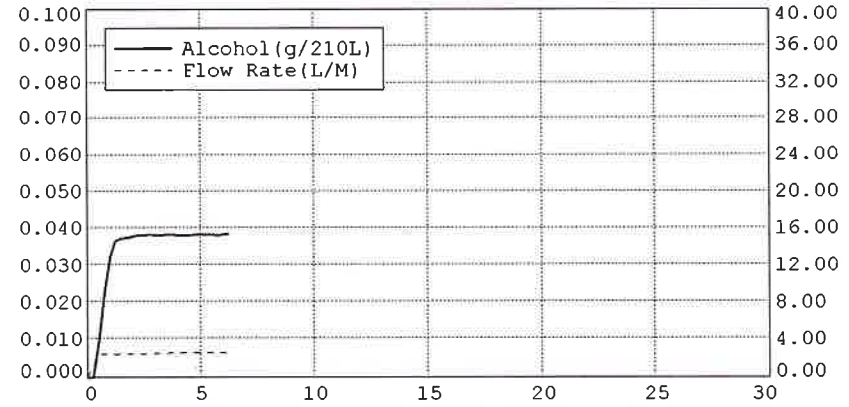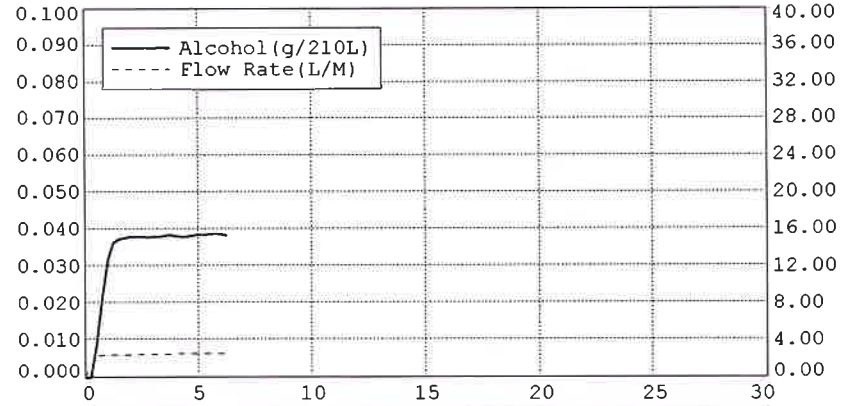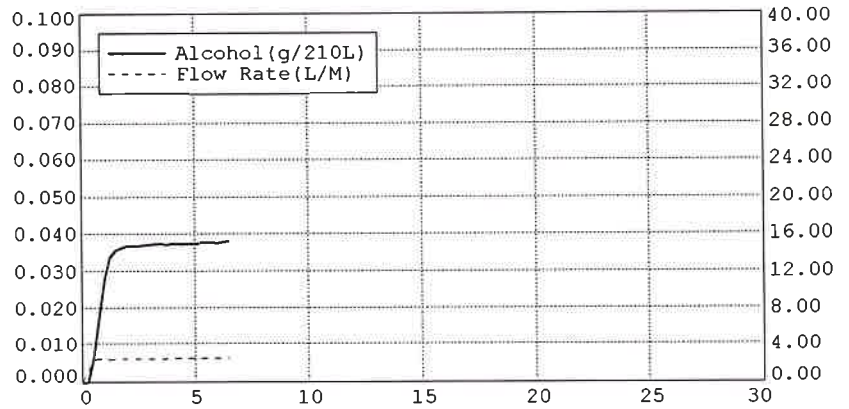

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100364






Date: 01/03/2023
 Time: 09:42:16

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.14: 0.078
 LOT #: AG113402
 EXPIRATION: 05/14/2023
 TANK PRESSURE: 487 psi

BLANK TEST	0.000	09:43
INTERNAL STANDARD	VERIFIED	09:43
EXTERNAL STANDARD	0.076	09:44
BLANK TEST	0.000	09:44
EXTERNAL STANDARD	0.076	09:45
BLANK TEST	0.000	09:46
EXTERNAL STANDARD	0.077	09:46
BLANK TEST	0.000	09:47
EXTERNAL STANDARD	0.077	09:47
BLANK TEST	0.000	09:48
EXTERNAL STANDARD	0.077	09:48
BLANK TEST	0.000	09:49

Average = 0.0766
 Std Dev = 0.0005

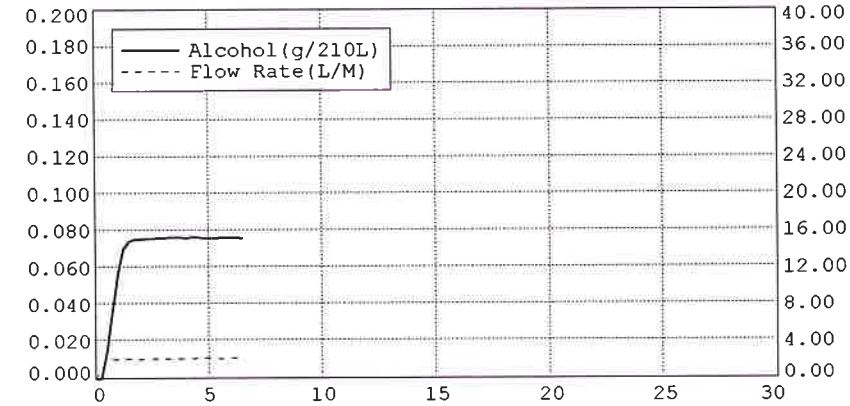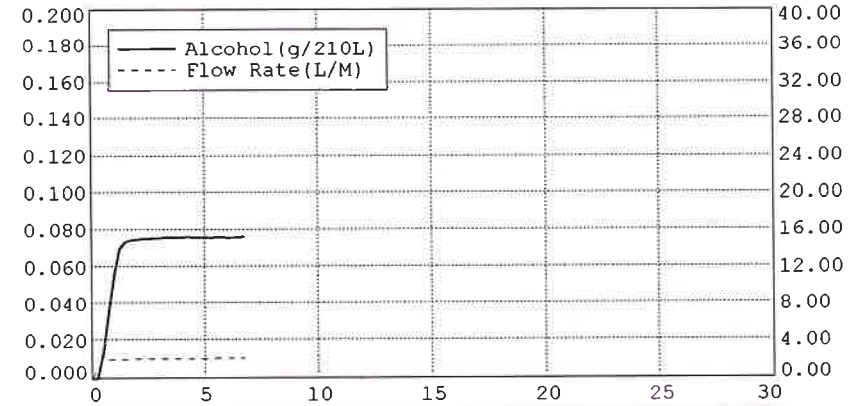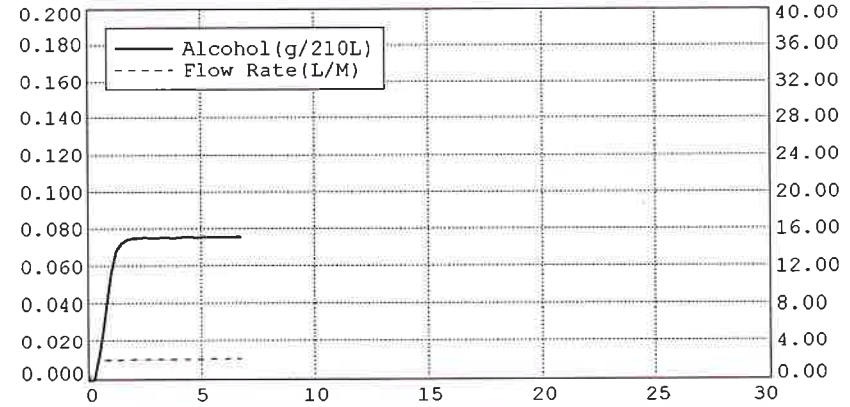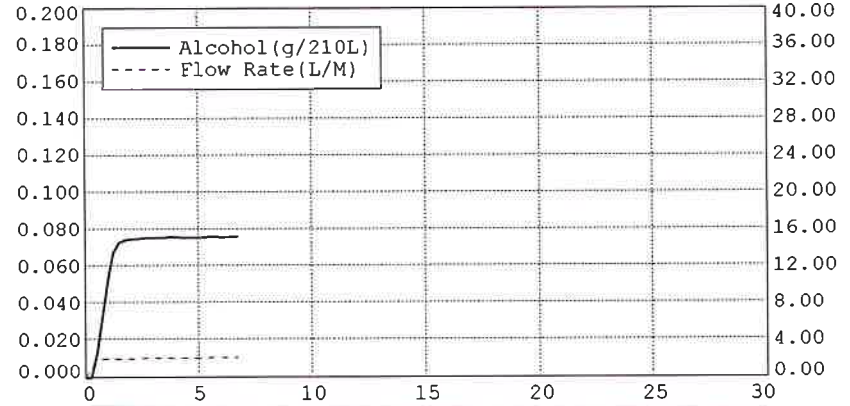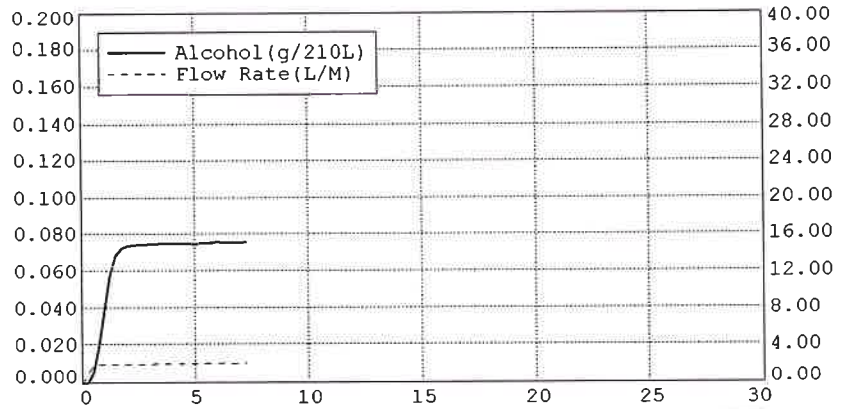

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100364






Date: 01/03/2023
 Time: 09:50:14

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.14: 0.097
 LOT #: AG211003
 EXPIRATION: 04/20/2024
 TANK PRESSURE: 945 psi

BLANK TEST	0.000	09:51
INTERNAL STANDARD	VERIFIED	09:51
EXTERNAL STANDARD	0.097	09:51
BLANK TEST	0.000	09:52
EXTERNAL STANDARD	0.097	09:53
BLANK TEST	0.000	09:53
EXTERNAL STANDARD	0.097	09:54
BLANK TEST	0.000	09:55
EXTERNAL STANDARD	0.097	09:55
BLANK TEST	0.000	09:56
EXTERNAL STANDARD	0.097	09:56
BLANK TEST	0.000	09:57

Average = 0.0970
 Std Dev = 0.0000

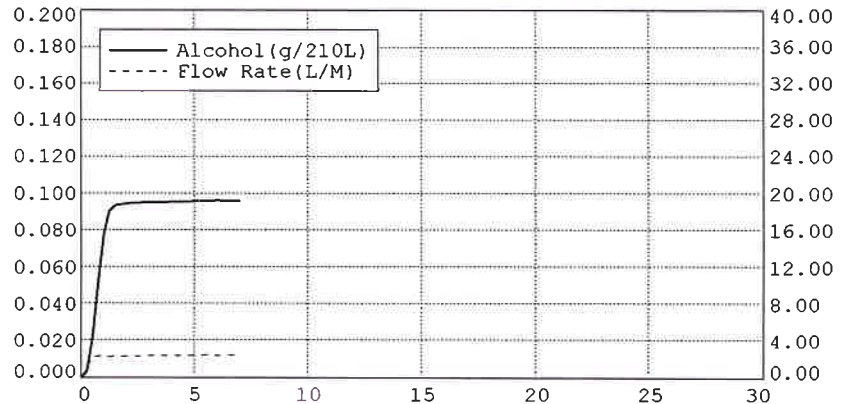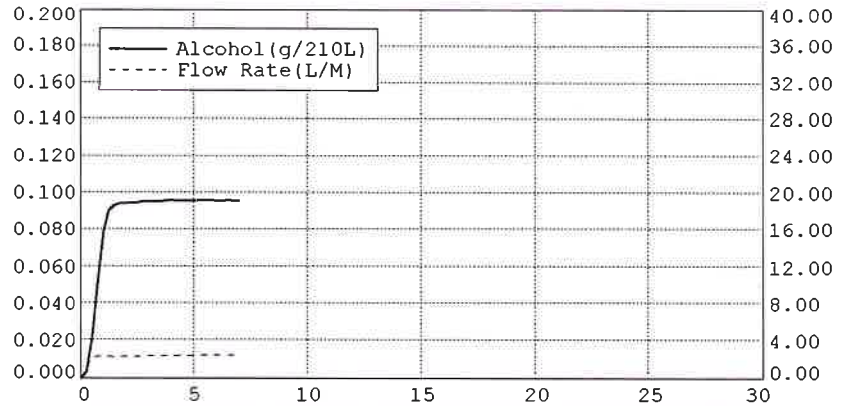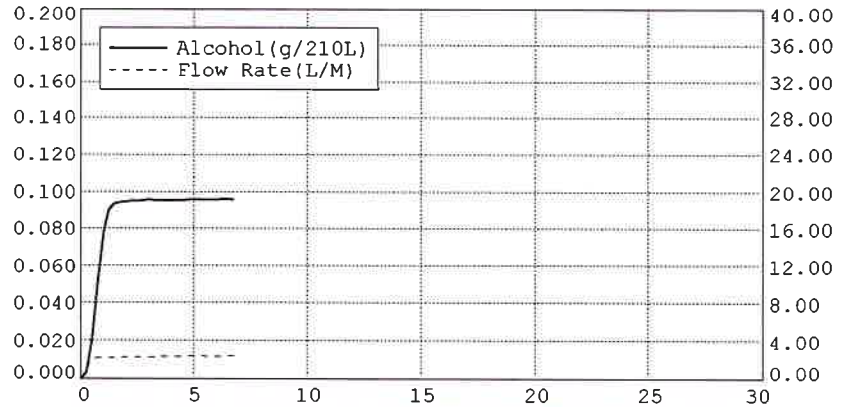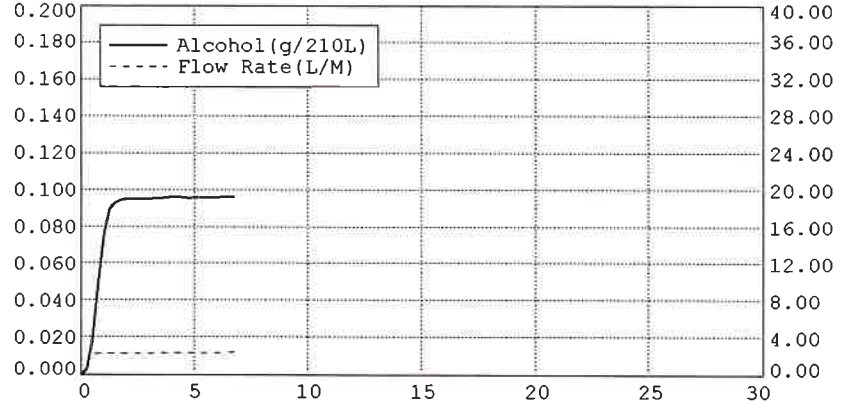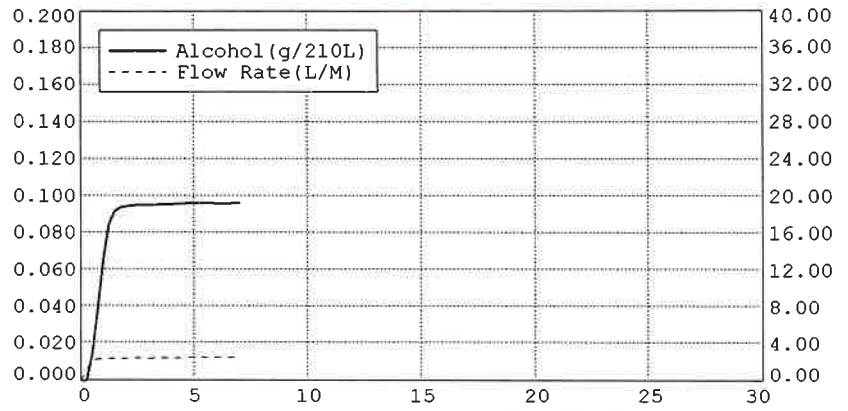

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100364






Date: 01/03/2023
 Time: 09:57:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.14: 0.146
 LOT #: AG134205
 EXPIRATION: 12/08/2023
 TANK PRESSURE: 979 psi

BLANK TEST	0.000	09:59
INTERNAL STANDARD	VERIFIED	09:59
EXTERNAL STANDARD	0.145	09:59
BLANK TEST	0.000	10:00
EXTERNAL STANDARD	0.145	10:00
BLANK TEST	0.000	10:01
EXTERNAL STANDARD	0.145	10:02
BLANK TEST	0.000	10:02
EXTERNAL STANDARD	0.146	10:03
BLANK TEST	0.000	10:04
EXTERNAL STANDARD	0.146	10:04
BLANK TEST	0.000	10:05

Average = 0.1454
 Std Dev = 0.0005

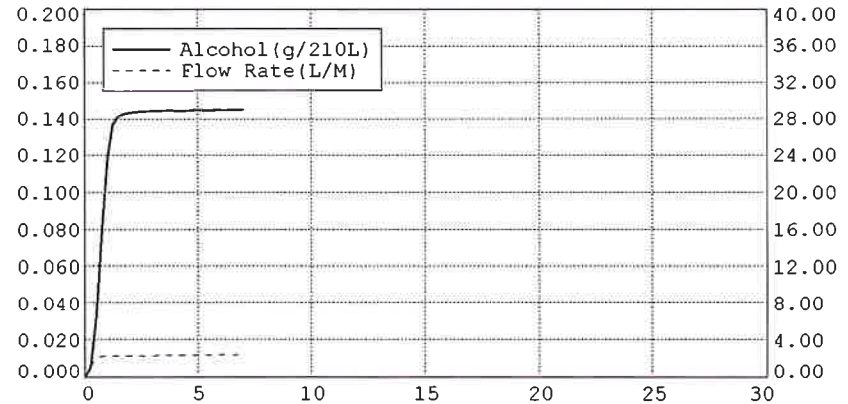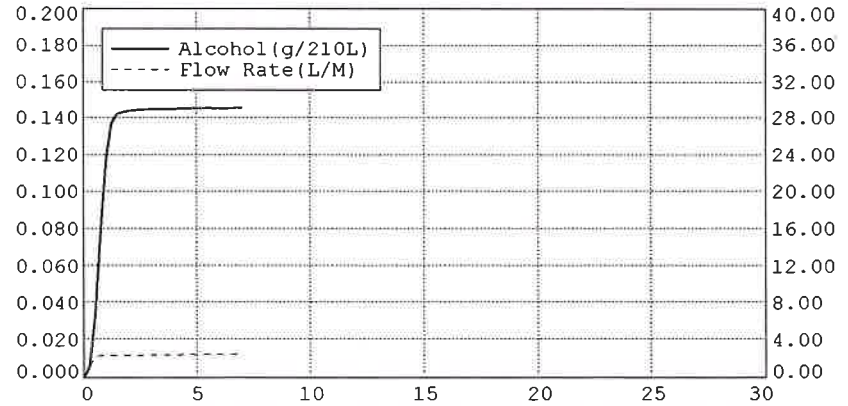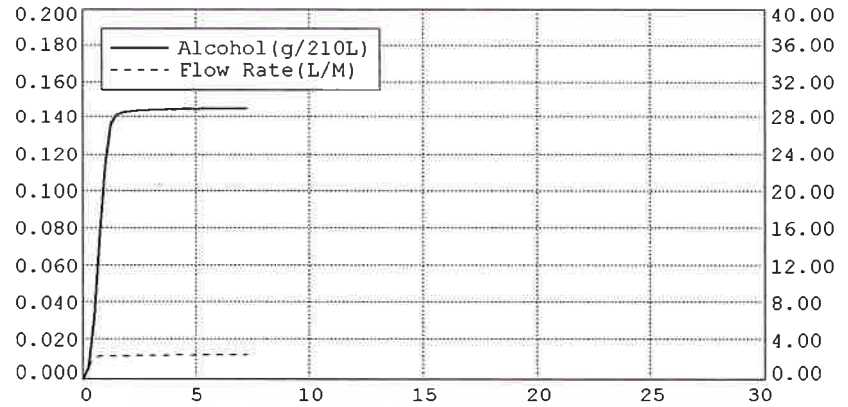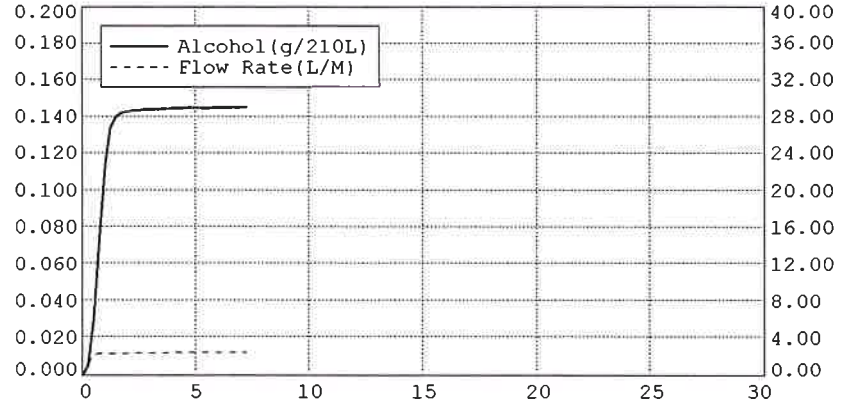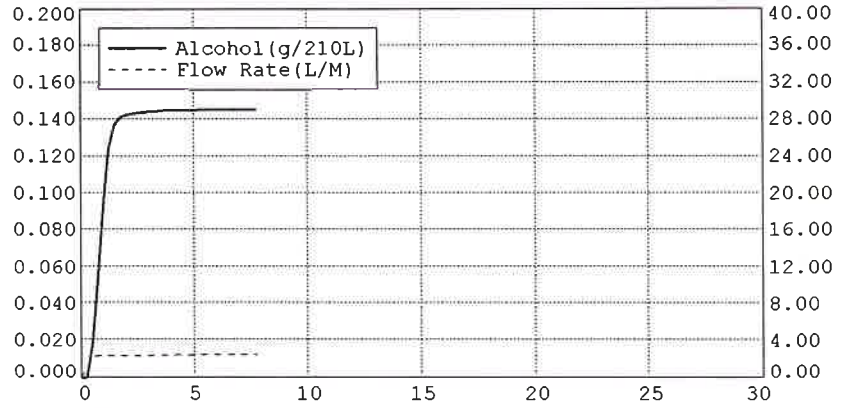

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100364






Date: 01/03/2023
 Time: 10:06:20

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.14: 0.292
 LOT #: AG217903
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 519 psi

BLANK TEST	0.000	10:07
INTERNAL STANDARD	VERIFIED	10:07
EXTERNAL STANDARD	0.291	10:07
BLANK TEST	0.000	10:08
EXTERNAL STANDARD	0.291	10:09
BLANK TEST	0.000	10:09
EXTERNAL STANDARD	0.291	10:10
BLANK TEST	0.000	10:11
EXTERNAL STANDARD	0.290	10:11
BLANK TEST	0.000	10:12
EXTERNAL STANDARD	0.291	10:12
BLANK TEST	0.000	10:13

Average = 0.2908
 Std Dev = 0.0004

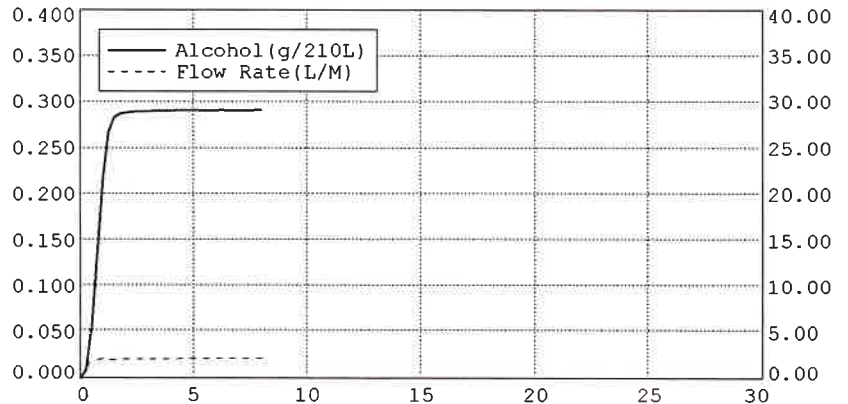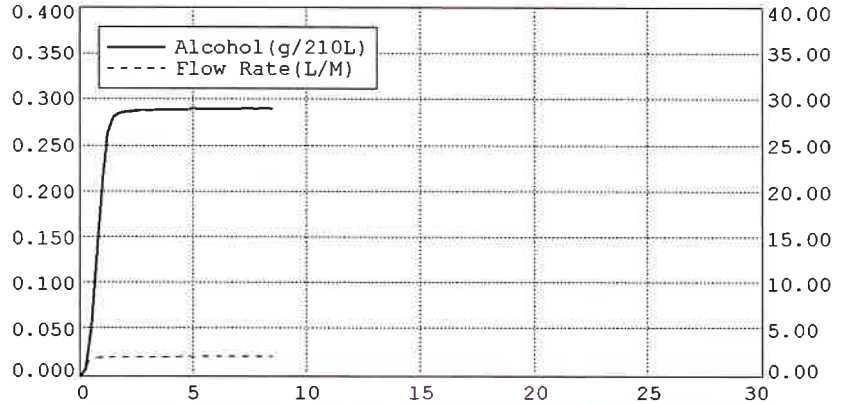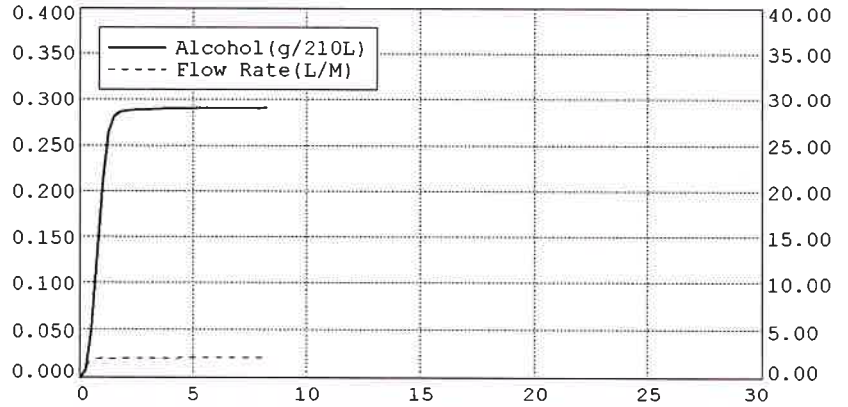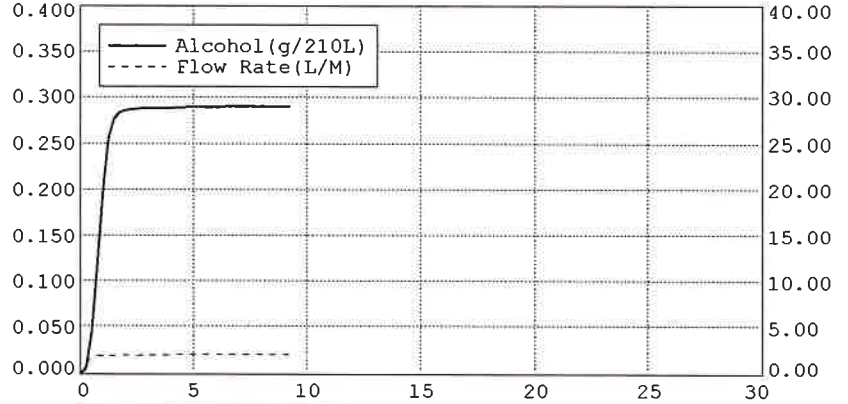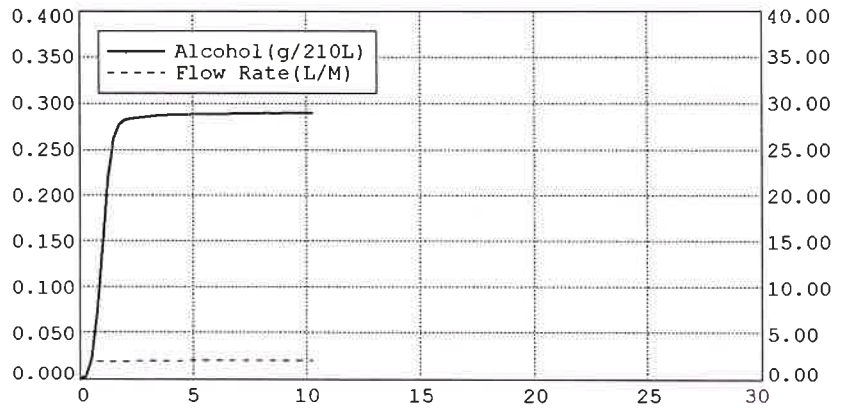

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 14:20:53

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078


DIAGNOSTIC CHECK	PASSED	14:22
BLANK TEST	0.000	14:22
INTERNAL STANDARD	VERIFIED	14:22
EXTERNAL STANDARD	0.076	14:22
BLANK TEST	0.000	14:23
SUBJECT SAMPLE	INCOMPLETE	14:25

External Standard Tank Information
Lot # AG113402
Expiration: 05/14/2023

* Calibration subject test sequences didn't have the external standard tank lot no. and expiration date. This was caught during the Technical Review. Tank information was verified by checking the VOC and Calibration form.

TLM 02/14/2023

TLM

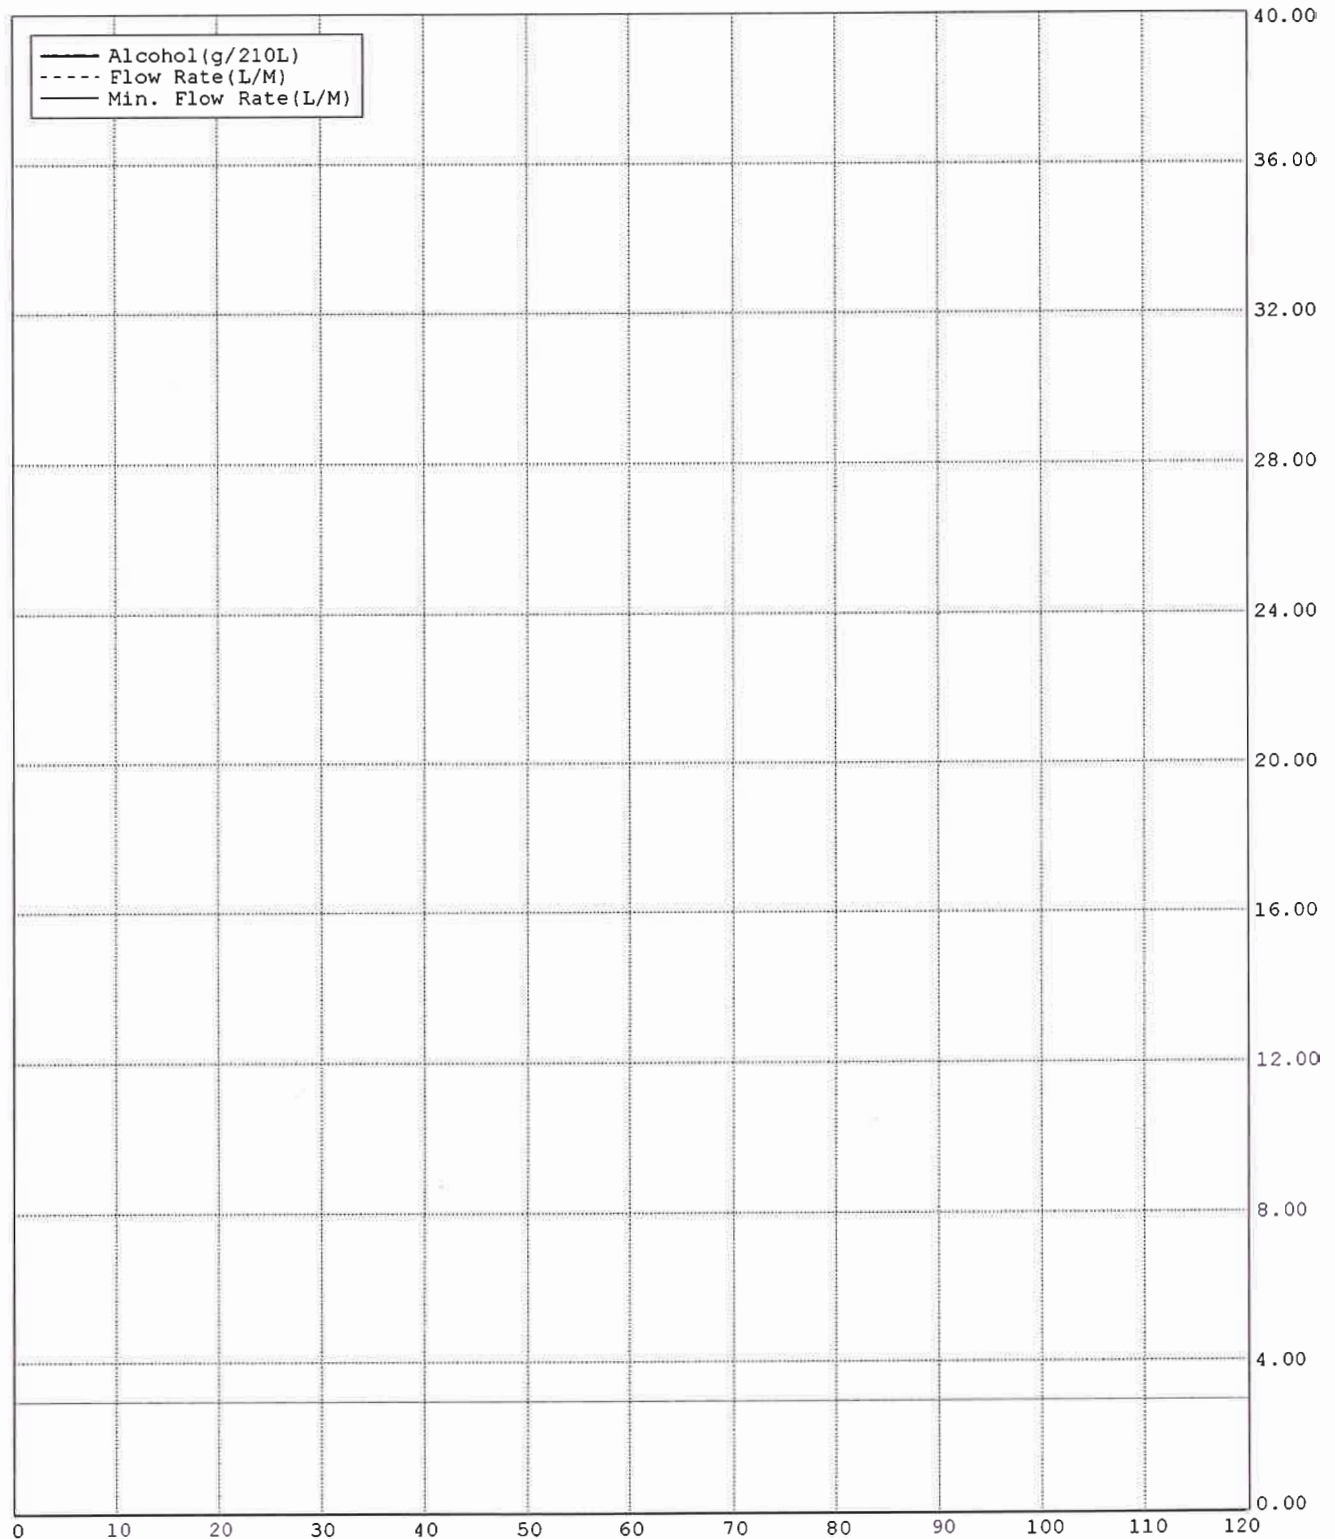

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 14:29:44

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437


DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078

DIAGNOSTIC CHECK	PASSED	14:30
BLANK TEST	0.000	14:30
INTERNAL STANDARD	VERIFIED	14:30
EXTERNAL STANDARD	0.076	14:31
BLANK TEST	0.000	14:32
SUBJECT SAMPLE	XXX	14:32

Maximum Attempts Exceeded

TLM

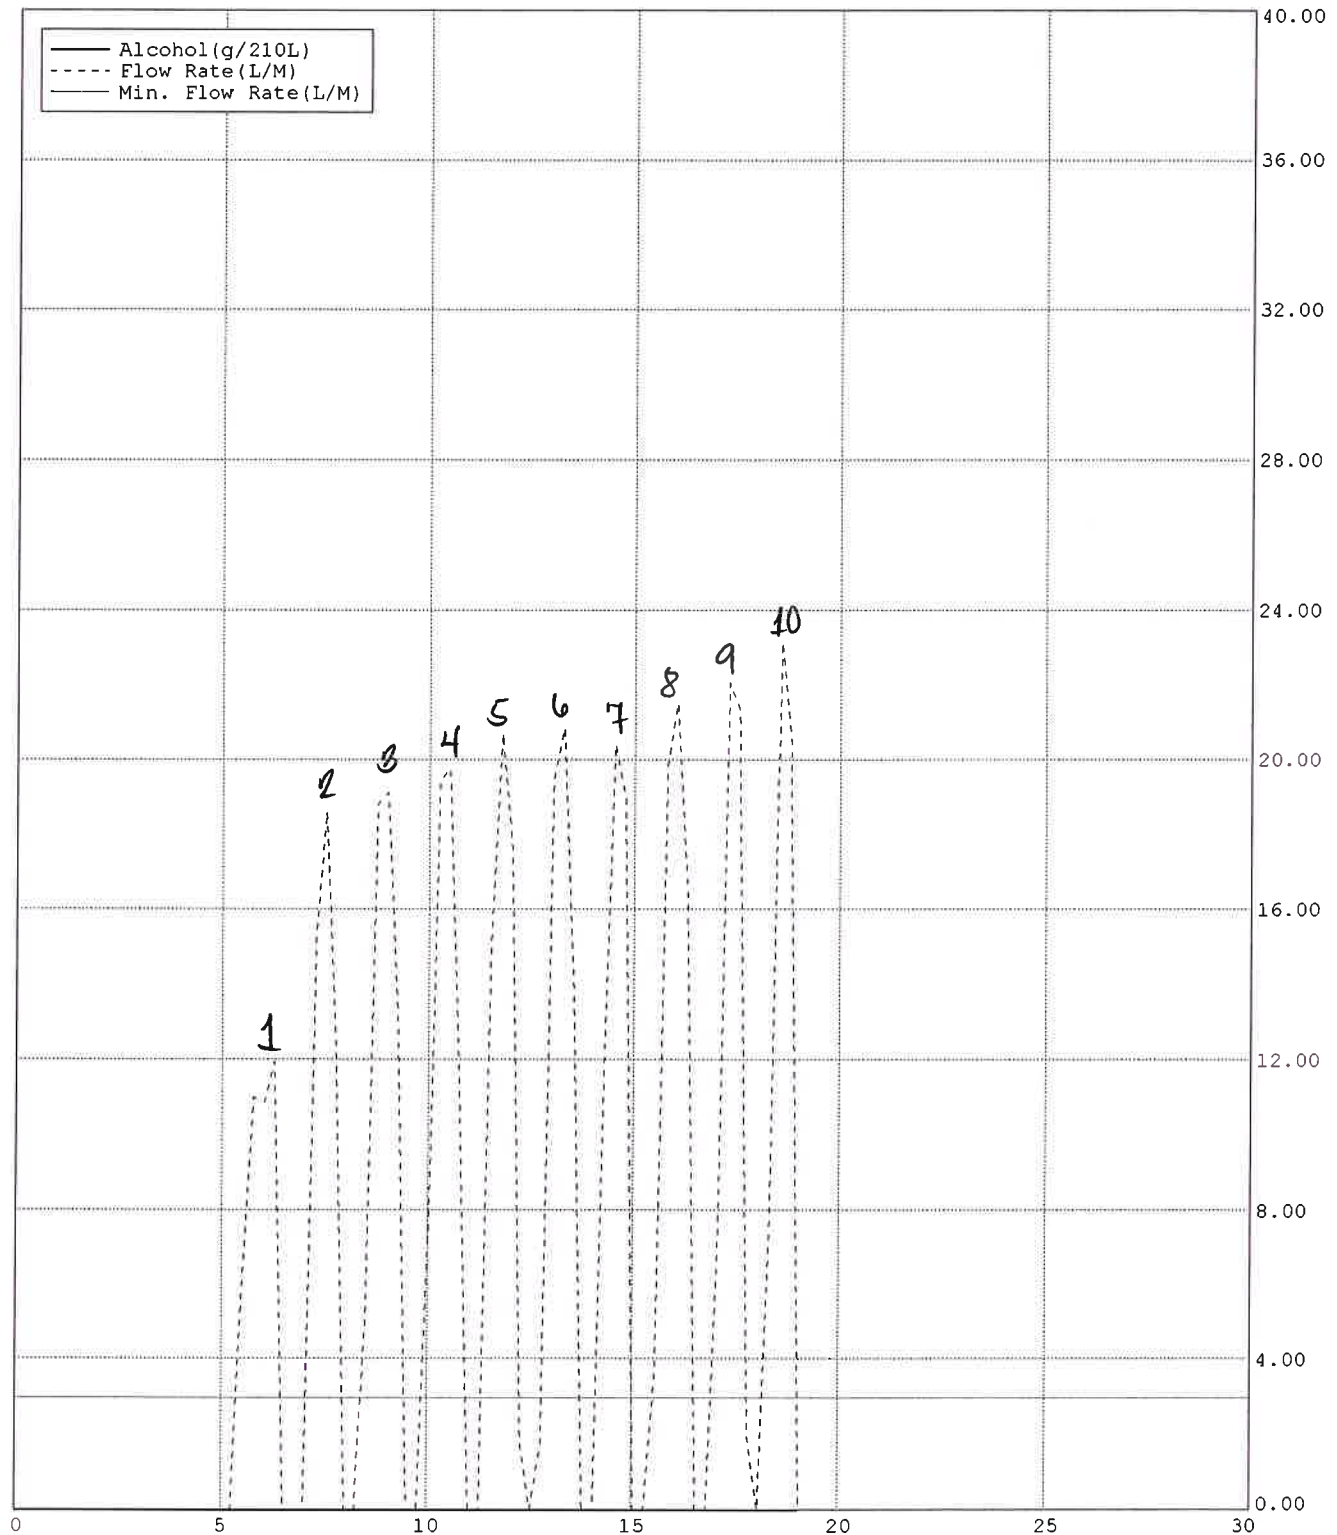

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 14:49:34

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.16: 0.078

DIAGNOSTIC CHECK	PASSED	14:50
BLANK TEST	0.000	14:50
INTERNAL STANDARD	VERIFIED	14:50
EXTERNAL STANDARD	0.076	14:51
BLANK TEST	0.000	14:51
SUBJECT SAMPLE	INVALID	14:52

TLM

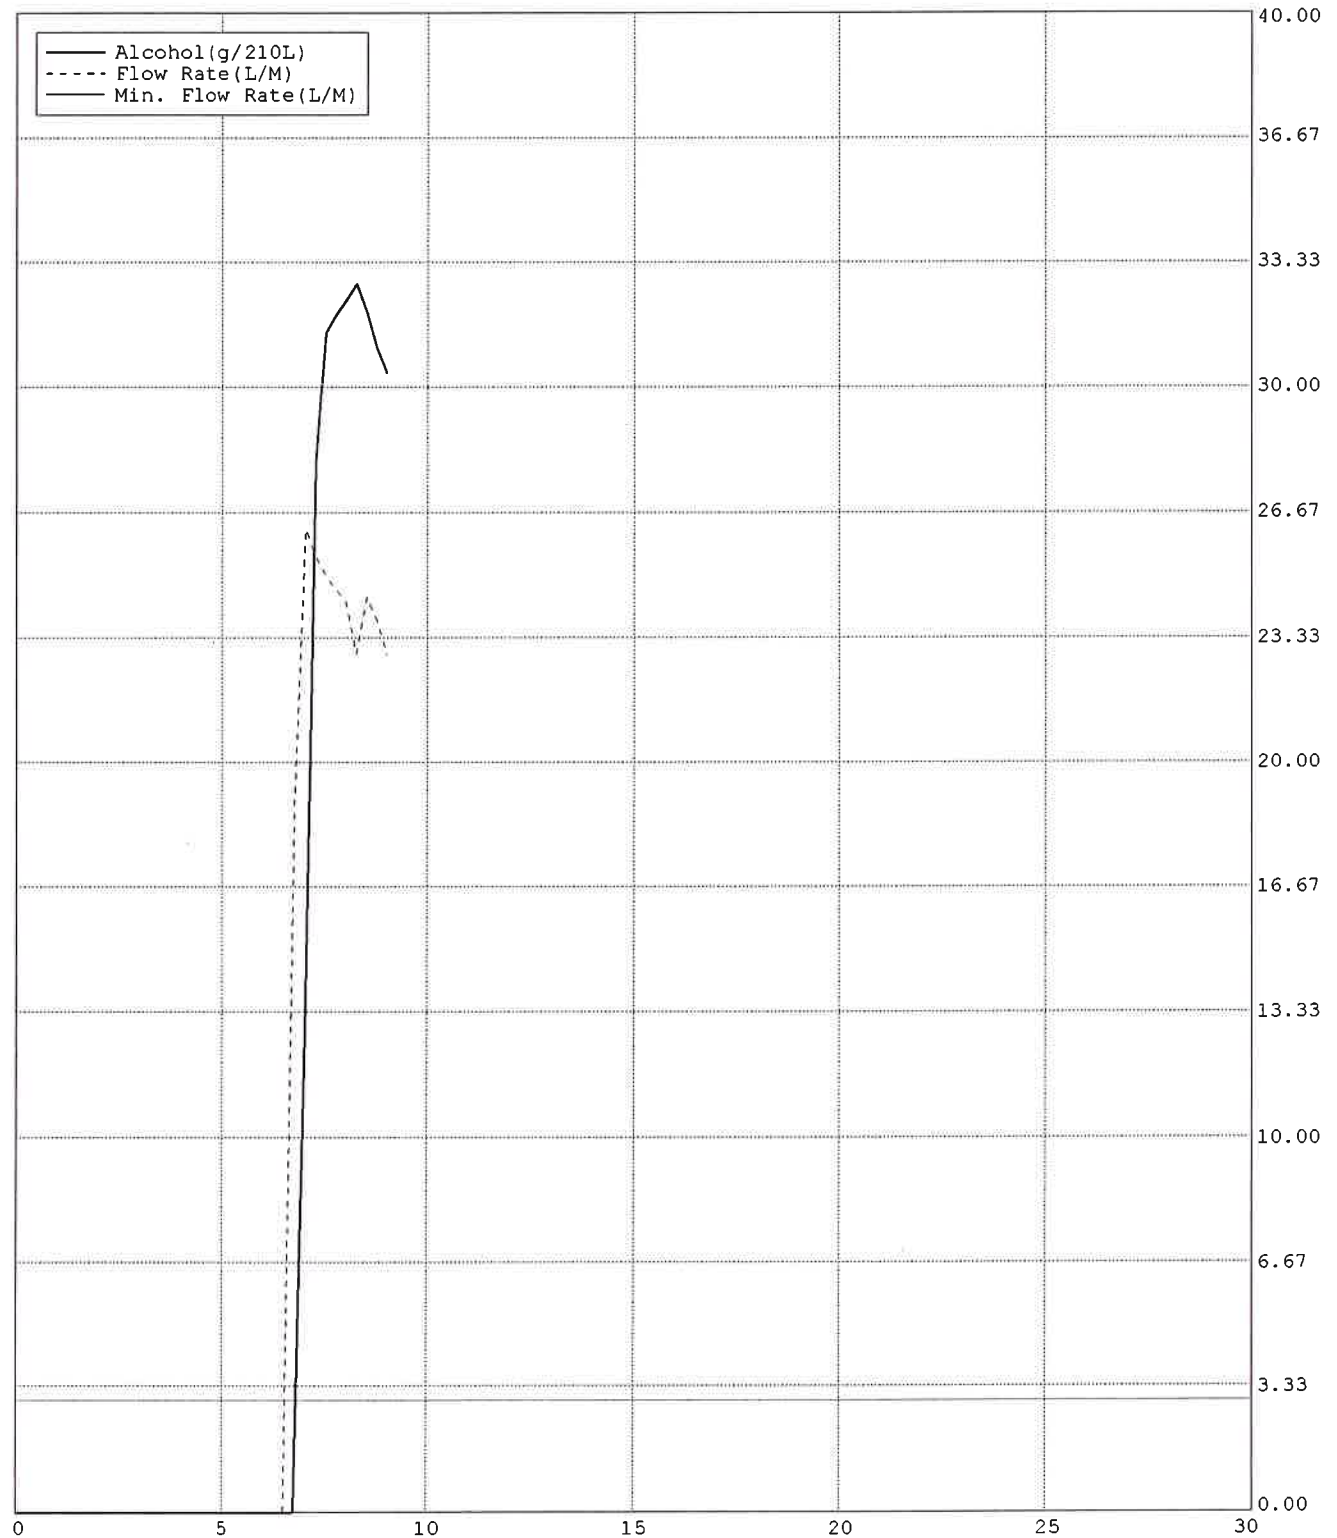

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 15:25:48

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437


DEPT/AGENCY:
RADIO FREQUENCY INTERFERENCE (RFI)
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078

DIAGNOSTIC CHECK	PASSED	15:26
BLANK TEST	0.000	15:26
INTERNAL STANDARD	VERIFIED	15:27
EXTERNAL STANDARD	0.076	15:27
BLANK TEST	0.000	15:28

RFI DETECTED

TLM

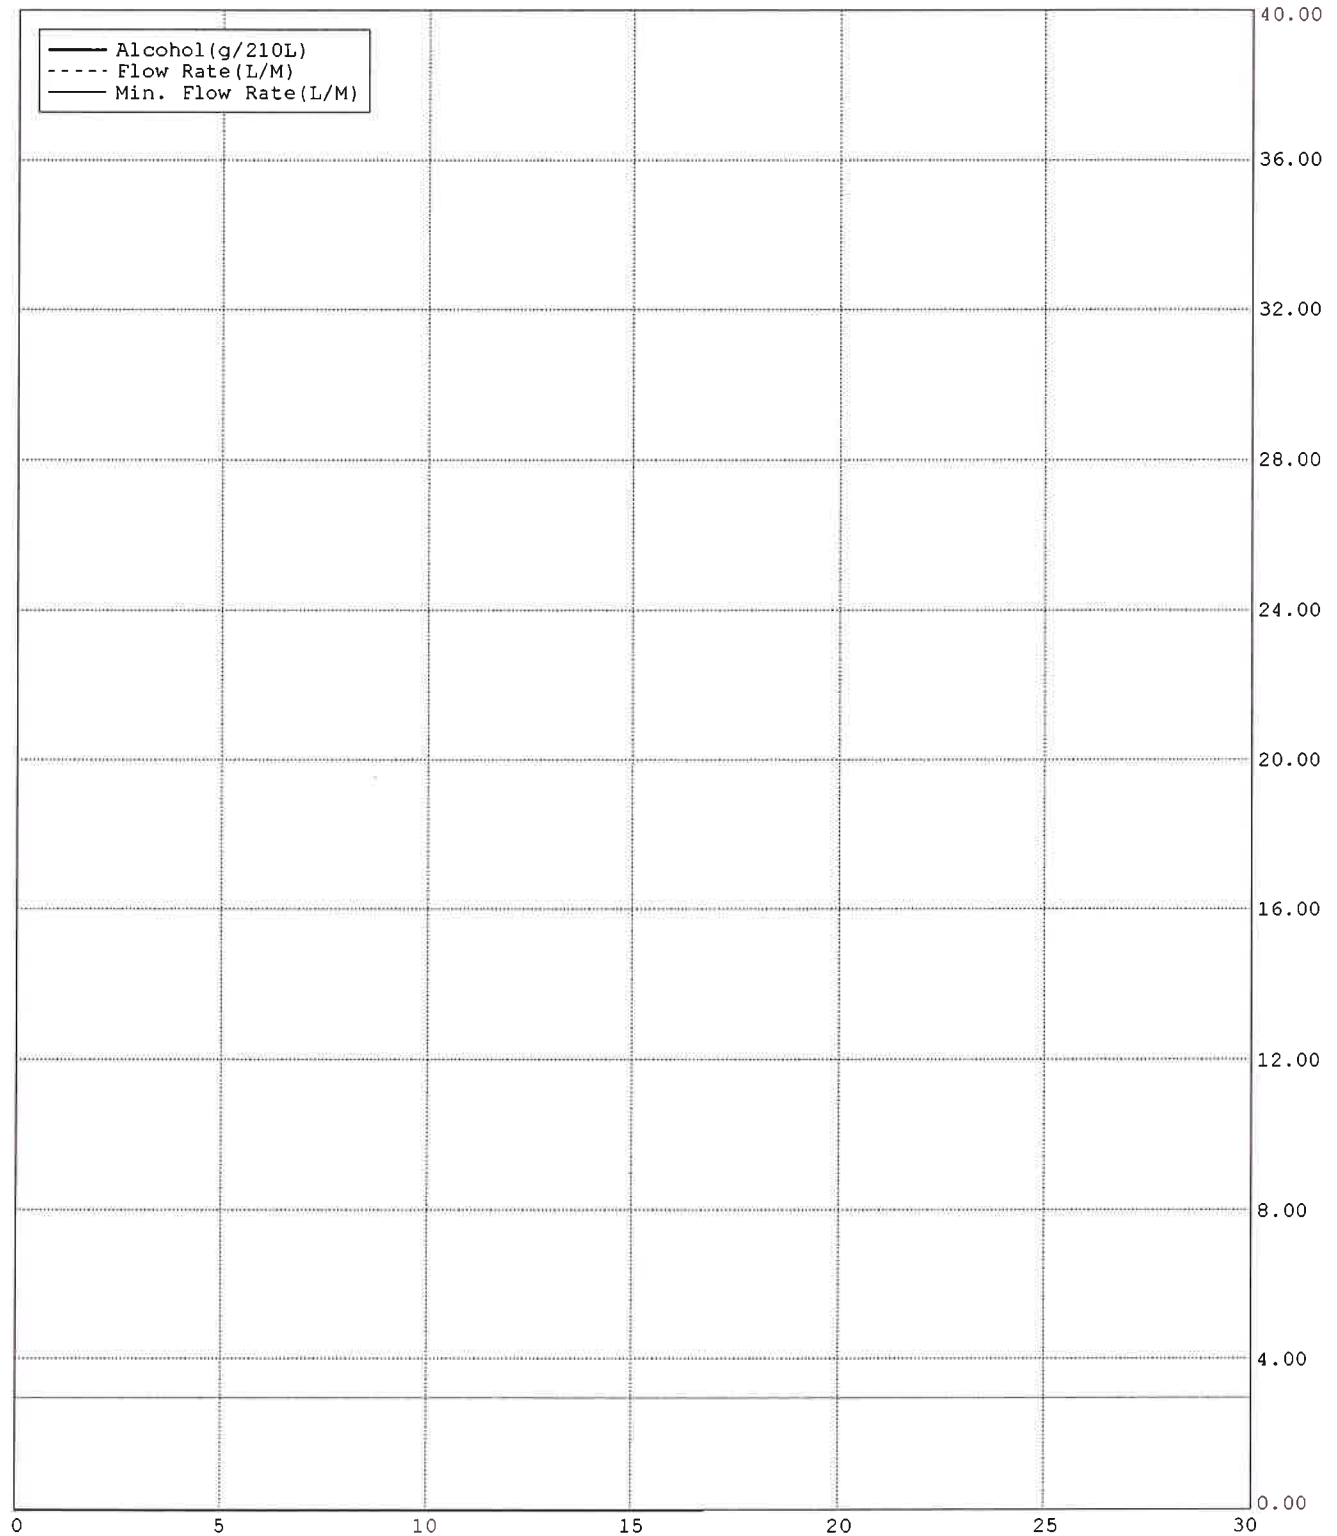

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 15:16:39

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.16: 0.078

DIAGNOSTIC CHECK	PASSED	15:17
BLANK TEST	0.000	15:17
INTERNAL STANDARD	VERIFIED	15:17
Xq = 0.101 (0.44%)		
EXTERNAL STANDARD	0.076	15:18
X[1] = 0.0763 (-0.0014) (0.0024)		
BLANK TEST	0.000	15:19
SUBJECT SAMPLE	XXX	15:19
X[1] = 0.1100 (-0.0173) (0.0019)		

Interference Detected

Filter 2 Average: -0.0014
Filter 3 Average: 0.0024

TLM 01-04-2023

TLM



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 15:10:03

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437


DEPT/AGENCY:
INTERFERENCE - ISOPROPRANOL
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078

DIAGNOSTIC CHECK	PASSED	15:11
BLANK TEST	0.000	15:11
INTERNAL STANDARD	VERIFIED	15:11
Xq = 0.101 (0.00%)		
EXTERNAL STANDARD	0.077	15:11
X[1] = 0.0767 (-0.0007) (0.0030)		
BLANK TEST	0.000	15:12
SUBJECT SAMPLE	XXX	15:12
X[1] = 0.1143 (-0.0230) (-0.0001)		

Interference Detected

TLM

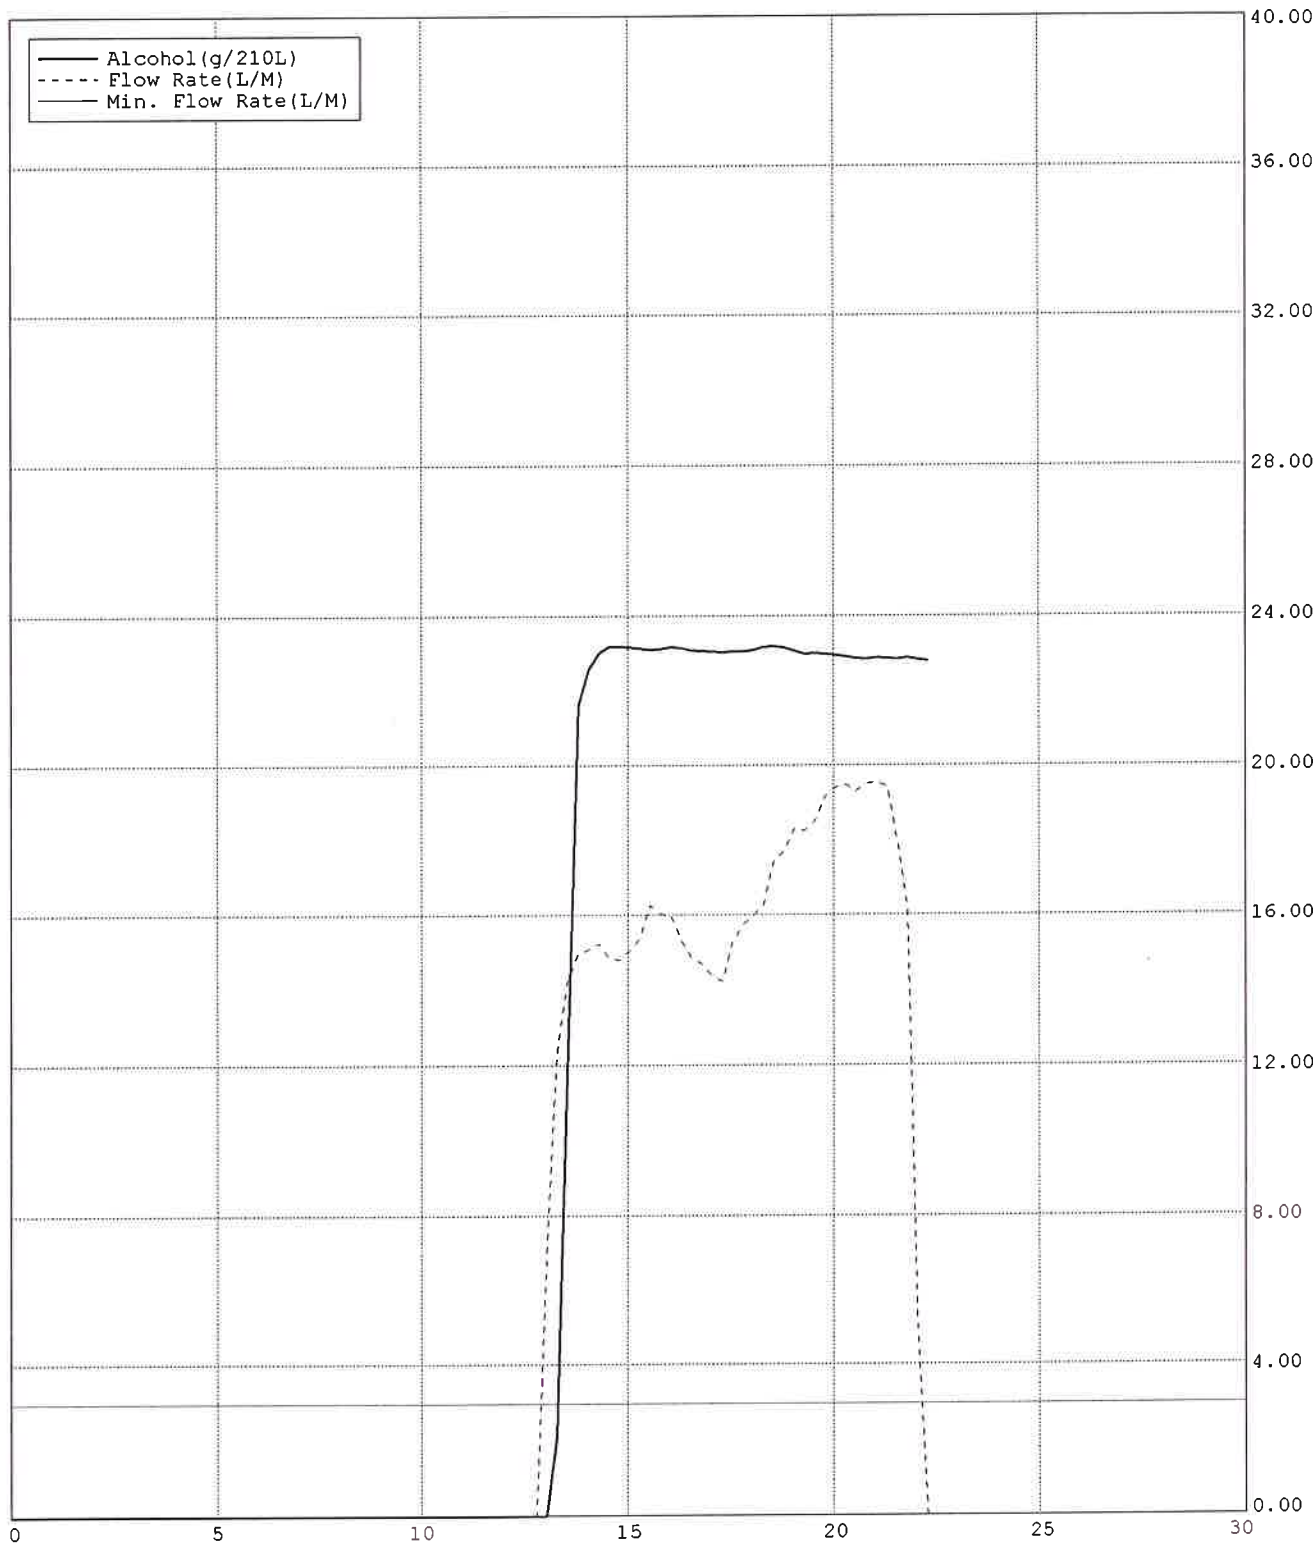

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 15:00:54

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INTERFERENCE - NEGATIVE CONTROL
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.16: 0.078

DIAGNOSTIC CHECK	PASSED	15:01
BLANK TEST	0.000	15:02
INTERNAL STANDARD	VERIFIED	15:02
Xq = 0.100 (0.52%)		
EXTERNAL STANDARD	0.075	15:02
X[1] = 0.0752 (-0.0015) (0.0026)		
BLANK TEST	0.000	15:03
SUBJECT SAMPLE (Vol=2.42L)	0.095	15:03
X[1] = 0.0952 (-0.0008) (0.0004)		
BLANK TEST	0.000	15:04
EXTERNAL STANDARD	0.075	15:05
X[1] = 0.0751 (-0.0020) (0.0017)		
BLANK TEST	0.000	15:06

TLM

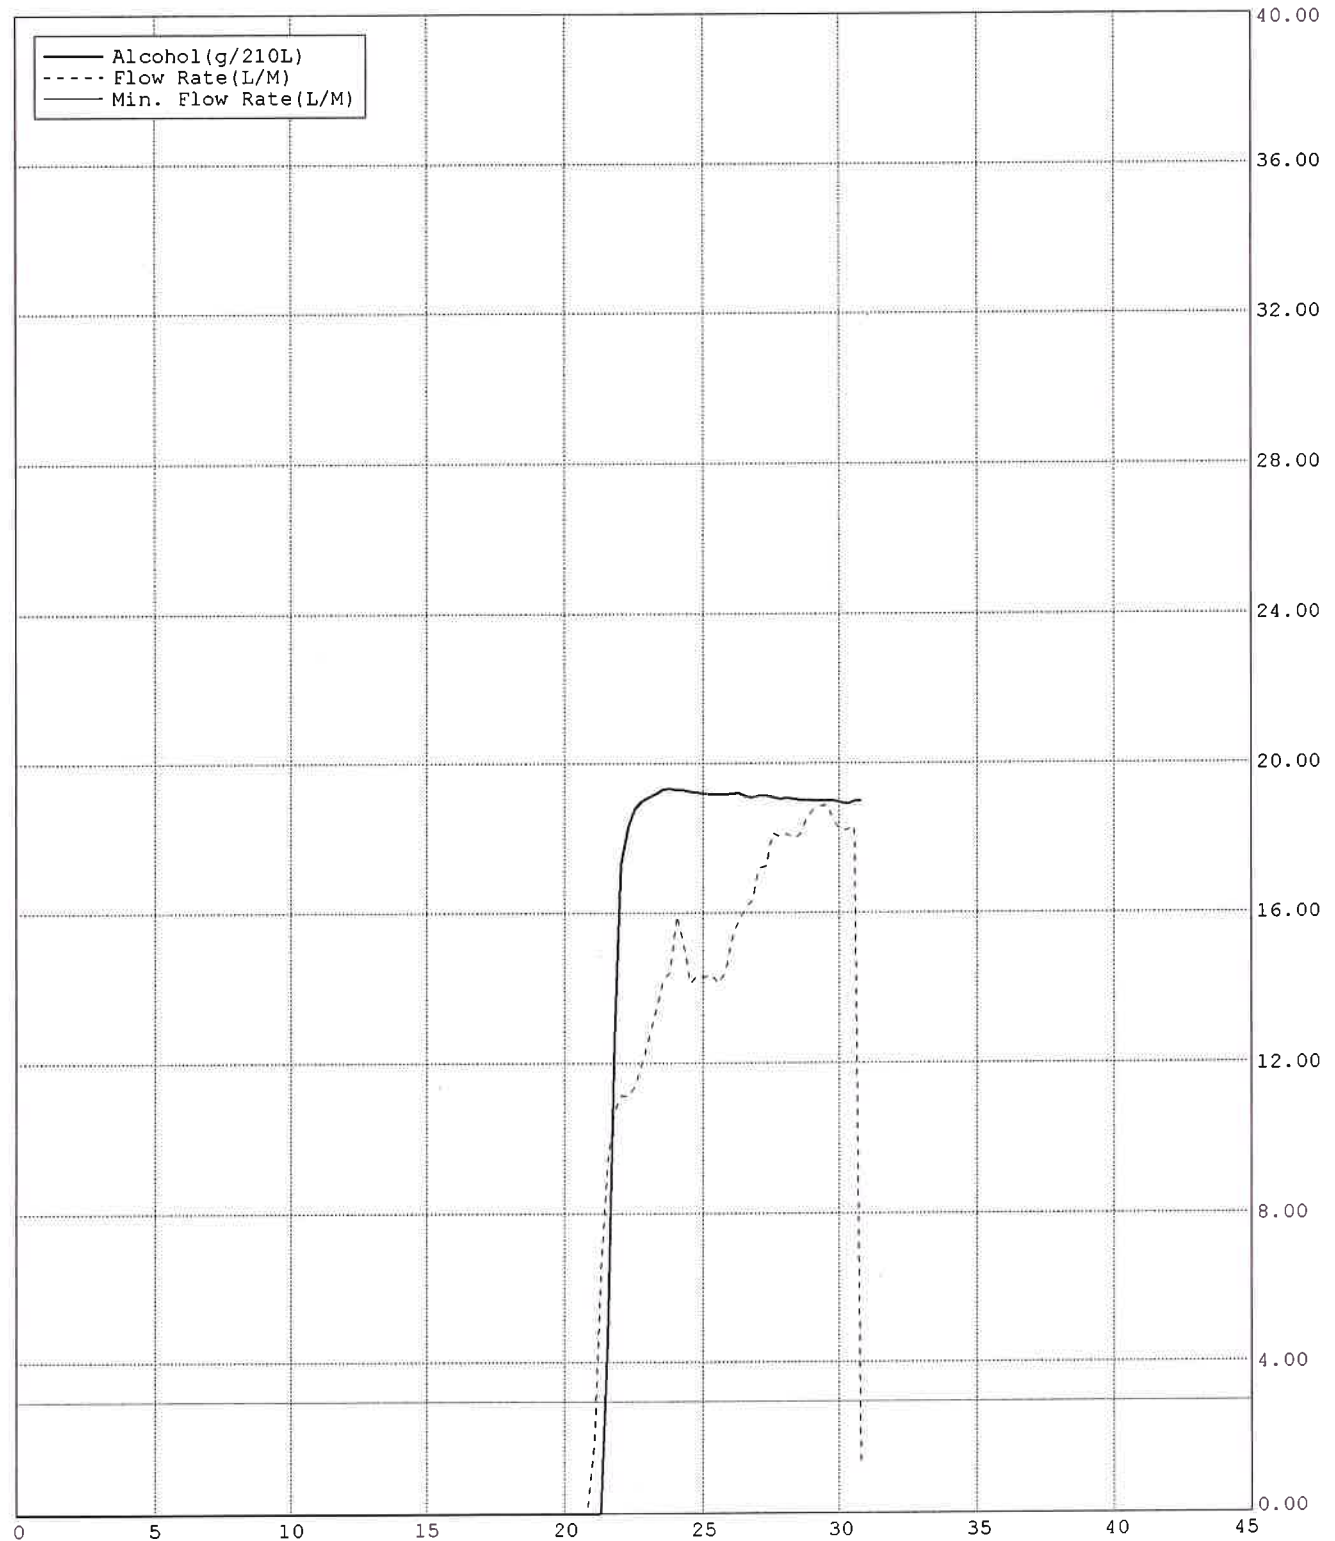

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100364

Date: 01/03/2023
Time: 15:51:37

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
NON DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.16: 0.078

DIAGNOSTIC CHECK	PASSED	15:53
BLANK TEST	0.000	15:53
INTERNAL STANDARD	VERIFIED	15:54
EXTERNAL STANDARD	0.077	15:54
BLANK TEST	0.000	15:55
SUBJECT SAMPLE (Vol=2.19L)	0.000	15:55
BLANK TEST	0.000	15:56
EXTERNAL STANDARD	0.077	15:56
BLANK TEST	0.000	15:57

TLM

