



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**

**Calibration Item:** DataMaster DMT

**Serial Number:** 100388

**Report Issue Date:** 05/16/2023

**Date Received:** 2023-02-27

**Condition of Item:** Good

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual

**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 03/08/2023 - As Found - End Date 03/08/2023 As Found - Evaluation Analyst:** Tatiana Malnoske

As Found Conditions - Barometric Pressure (inHg): 29.98 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.5

Relative Humidity (%): 13%

**As-Found Data**

Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG217902	0.021	0.020	0.020	0.021	0.020	0.020
0.080	0.080	AG135004	0.080	0.080	0.079	0.079	0.079	0.079
0.300	0.301	AG217903	0.297	0.297	0.297	0.297	0.297	0.297

**Start Date 04/05/2023 - As Left - End Date 04/05/2023**

As Left Conditions - Barometric Pressure (inHg): 29.36 Barometer Used: Fisher S/N 221250180 Temperature (C): 21.3 Relative

Humidity (%): 23

**As-Left Data**

Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG217904	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.078	AG135004	0.077	0.077	0.077	0.077	0.077	0.077	+/- 0.003
0.100	0.098	AG211003	0.097	0.097	0.097	0.097	0.097	0.097	+/- 0.003
0.150	0.147	AG134205	0.145	0.145	0.145	0.146	0.145	0.145	+/- 0.004
0.300	0.294	AG217903	0.292	0.292	0.292	0.292	0.292	0.292	+/- 0.008

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Technically and administratively reviewed by Brandi Barnett on 05/16/2023

Results authorized by Colleen O'Bryant on 05/16/2023

[colleen.obryant@alaska.gov](mailto:colleen.obryant@alaska.gov)

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100388 Analyst: C. O'Bryant Start Date: 4/5/23

- Diagnostic Test (attached)  Internal Standard value  $\leq$  3.00%  
 Adjust voltages, if needed

- Lamp (2.60 V Maximum)  Chopper Frequency  
 Bias  Detector Voltage  
 Cooler (2.00 V Maximum) (-0.100V to 0.100V)

- Set RFI Sensitivity  
 Adjust internal barometer reading to match NIST-traceable barometer  
 Adjust volume setting, if needed (1.50 L +/- 0.10 L)  
 Print Technician Screen (attached)  
 Print Calibration Factors (attached)  
 Minimum Volume Test 1.6 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg) 29.36 Temperature (C): 21.3 Relative Humidity (%) 23

Linearity Test (attached)

0.020g/210L Mnf: Airgas Lot: AG217902 Exp: 6/28/24  
0.040g/210L Mnf: Airgas Lot: AG217904 Exp: 6/28/24  
0.080g/210L Mnf: Airgas Lot: AG135004 Exp: 12/16/23  
0.100g/210L Mnf: Airgas Lot: AG211003 Exp: 4/20/24  
0.150g/210L Mnf: Airgas Lot: AG134205 Exp: 12/8/23  
0.300g/210L Mnf: Airgas Lot: AG217903 Exp: 6/28/23

Functional Tests (attached)

- Incomplete  Invalid  
 Maximum Attempts Exceeded  Radio Frequency Interference (RFI)  
 Interference (Volatiles)

Acetone Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: DIRG 4161 Verification Performed?

Isopropanol Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: SD1088 Verification Performed?

Neg. Control Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: SD1177 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/9/23

- Verify stylus is calibrated  Non-Drinking Subject Test  
 Reset Options  Upload  
 Clear Memory  Remove Tank Prior to Shutdown  
 Verification of Calibration (VOC) Calibration End Date: 4/5/23

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100388  
-----

Date: 04/05/2023  
Time: 11:09:46

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 48.1°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.75 V PASSED  
(1.04 V - 2.42 V)  
Cooler Voltage = 1.71 V PASSED  
(1.04 V - 2.42 V)  
Bias Voltage = 79 V PASSED  
(48 V - 112 V)  
Chopper Freq = 538 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.4 in

PUMP INFO

Flow Rate = 4.809 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.001 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED  
Xq = 0.100 0.62% (0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100388  
-----

Date: 04/05/2023  
Time: 11:41 AM

Temperatures (°C)

Sample Cell: 48.8°C  
Breath Tube: 47.6°C

Current Barometer 29.4 in  
Volume (Ltr) 1.48

Settings

Lamp: 1.81 V  
Bias: 81 V  
Cooler: 1.71 V  
Chopper: 537 Hz

Voltages (V)

Flow: 1.06 V  
Detector: 0.050 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100388  
-----

Date: 04/01/2019  
Time: 09:09:29

OPERATOR NAME:  
DEREK WALTON  
CERTIFICATE #: 9508

Ca = 0.1000  
CAL = 0.971164    0.800 <= CAL < 1.200  
b1 = 0.0010    0.0000 <= b1 < 0.0040  
b2 = 0.0060    0.0010 <= b2 < 0.0100  
b3 = 0.0008    0.0000 <= b3 < 0.0040  
Xq = 0.0998    0.0500 <= Xq < 0.2000  
a21 = 1.162721    1.050 <= a21 < 1.300  
a31 = 0.552254    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100388

Date: 04/05/2023

Time: 11:43:16

SUBJECT NAME:

TEST TEST

LICENSE #: VOLUME

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 23-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.37: 0.079

LOT #: AG135004

EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE (Vol=1.58L)

BLANK TEST

EXTERNAL STANDARD

BLANK TEST

PASSED 11:44

0.000 11:44

VERIFIED 11:44

0.077 11:45


0.000 11:46

0.000 11:47

0.000 11:48

0.077 11:48

0.000 11:49

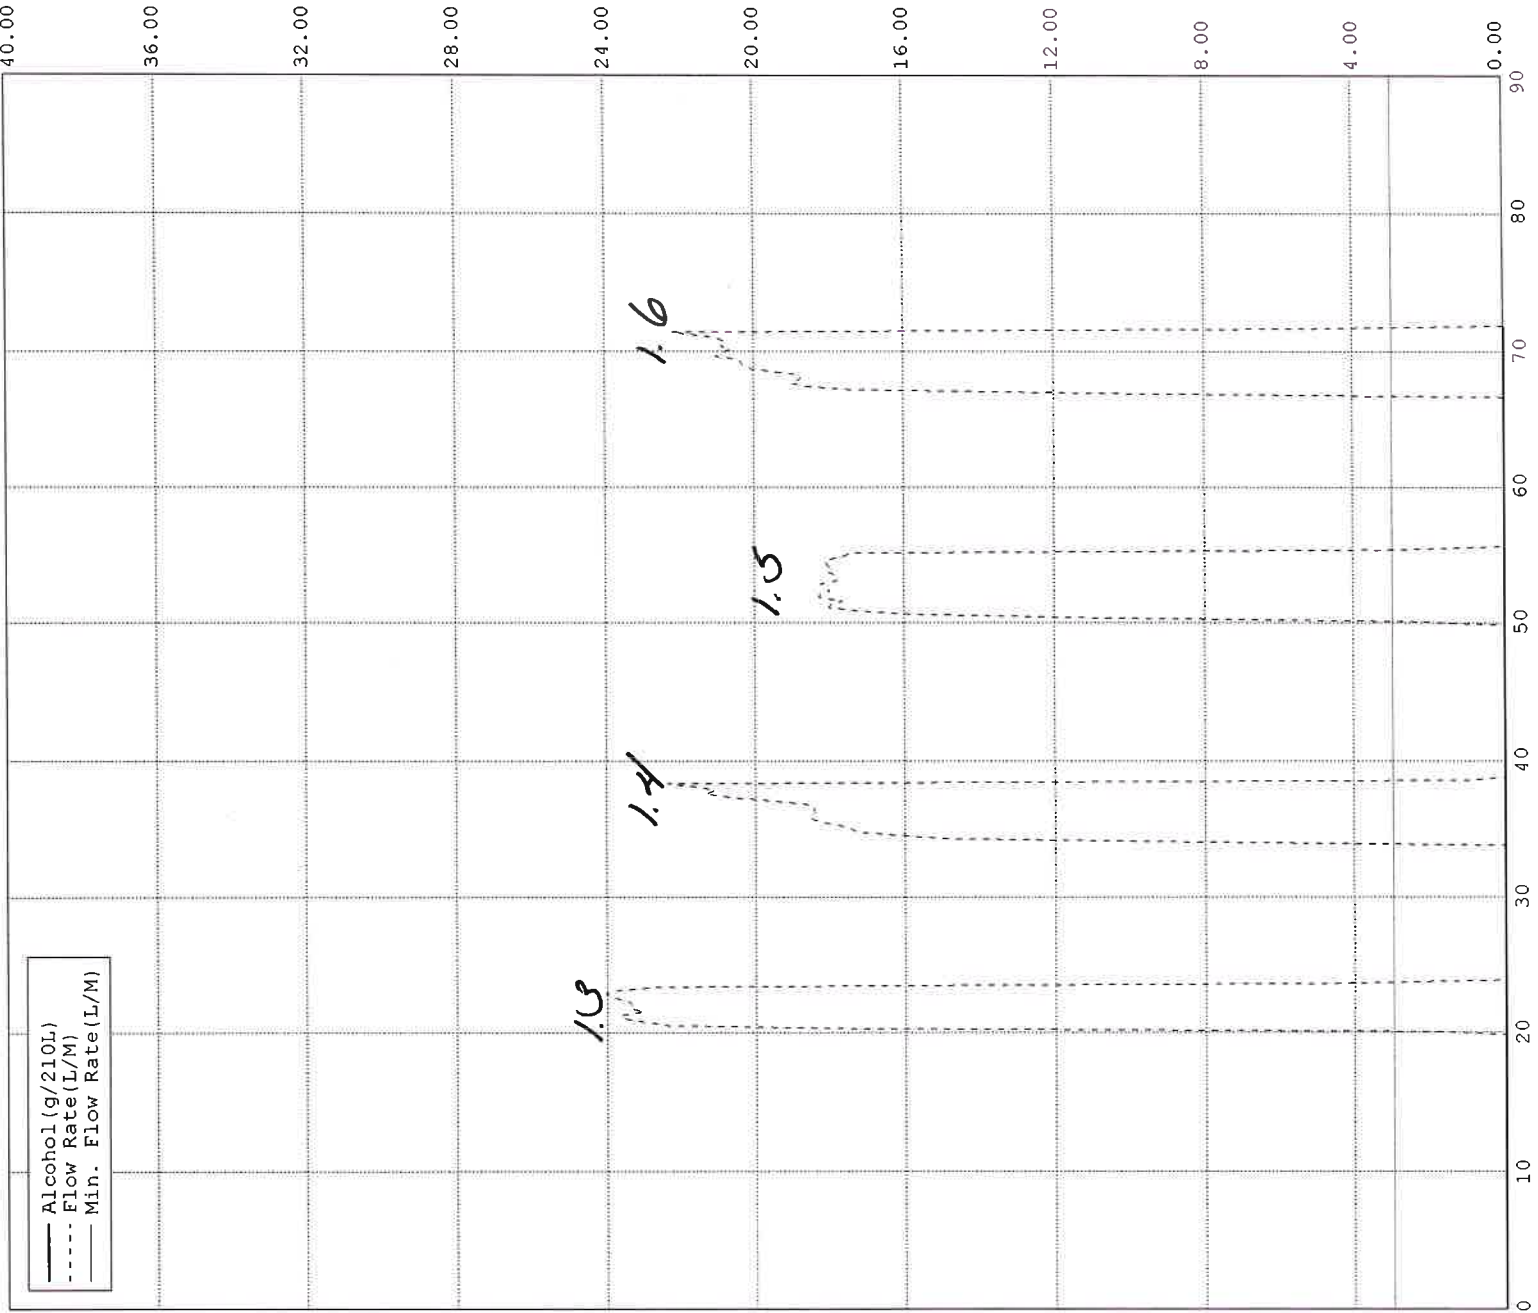

*CMS*

LINEARITY CHECK


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100388  
 -----

Date: 04/05/2023  
 Time: 11:51:04

SUPERVISOR NAME:  
 COLLEEN S OBRyant  
 OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.039	0.0390	0.0000
0.078	0.0770	0.0000
0.098	0.0970	0.0000
0.147	0.1452	0.0004
0.294	0.2920	0.0000

SLOPE = 0.992420  
 R<sup>2</sup> = 0.999984

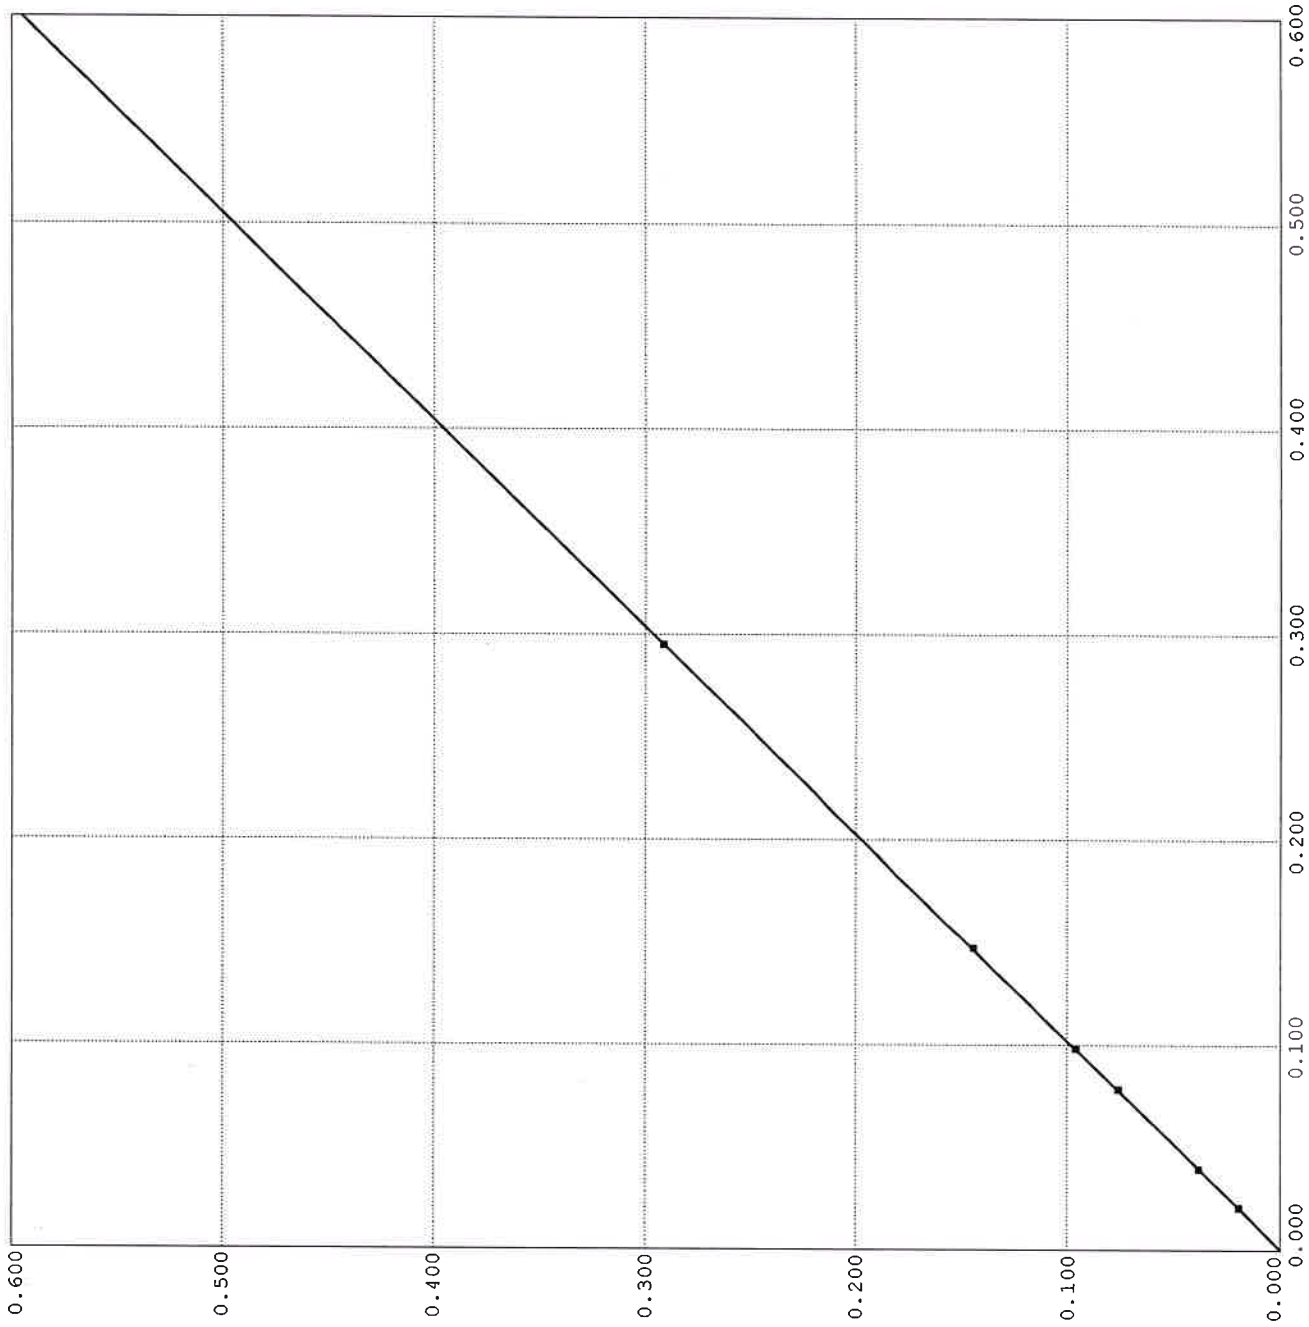



LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100388






Date: 04/05/2023  
Time: 11:51:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.37: 0.020  
LOT #: AG217902  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 1023 psi

BLANK TEST	0.000	11:56
INTERNAL STANDARD	VERIFIED	11:56
EXTERNAL STANDARD	0.020	11:56
BLANK TEST	0.000	11:57
EXTERNAL STANDARD	0.020	11:57
BLANK TEST	0.000	11:58
EXTERNAL STANDARD	0.020	11:58
BLANK TEST	0.000	11:59
EXTERNAL STANDARD	0.020	11:59
BLANK TEST	0.000	12:00
EXTERNAL STANDARD	0.020	12:00
BLANK TEST	0.000	12:01

Average = 0.0200  
Std Dev = 0.0000

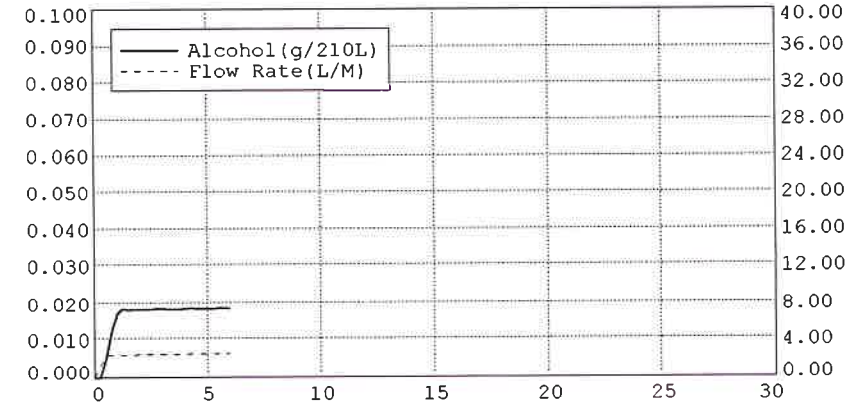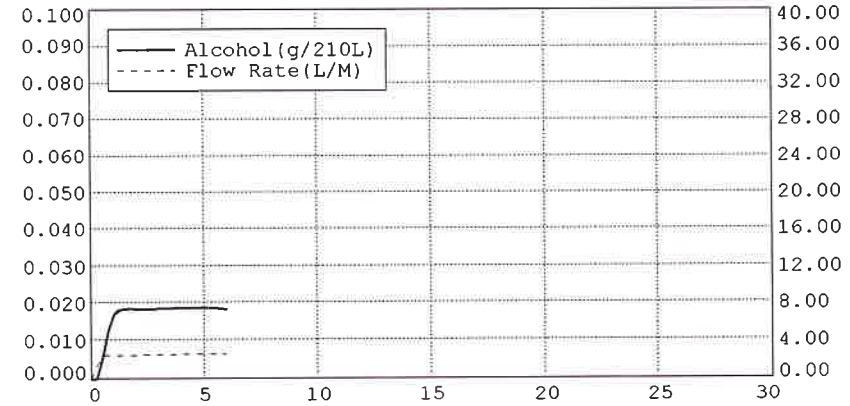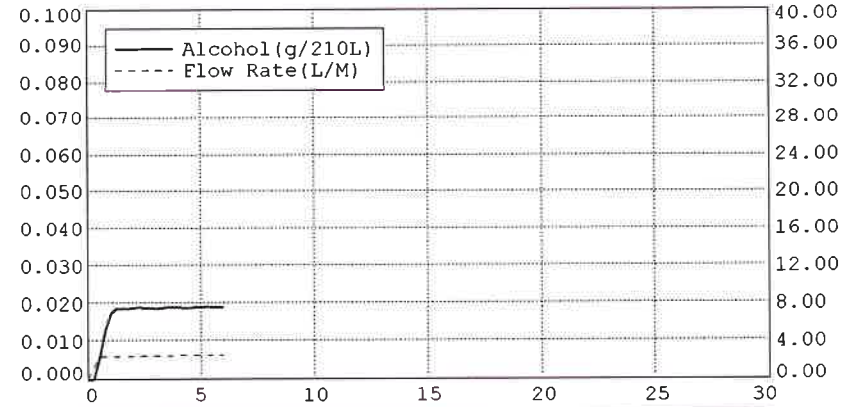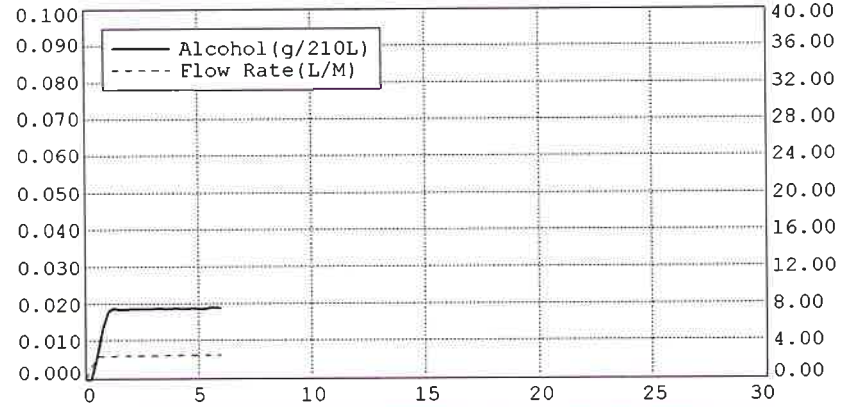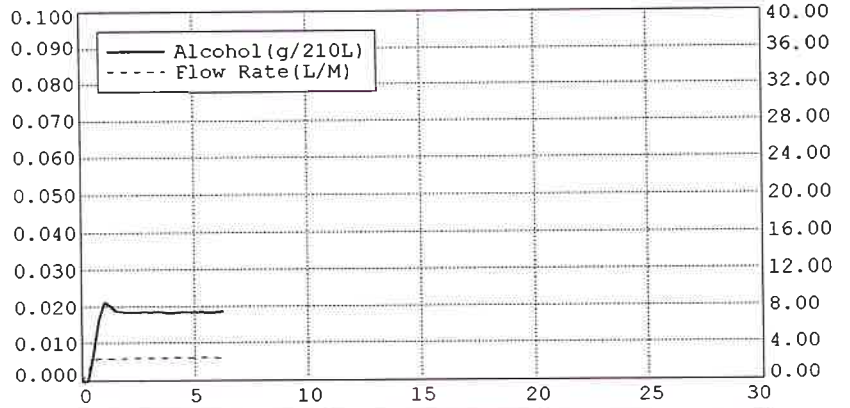



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100388






Date: 04/05/2023  
 Time: 12:33:13

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.35: 0.039  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 1076 psi

BLANK TEST	0.000	12:34
INTERNAL STANDARD	VERIFIED	12:34
EXTERNAL STANDARD	0.039	12:34
BLANK TEST	0.000	12:35
EXTERNAL STANDARD	0.039	12:35
BLANK TEST	0.000	12:36
EXTERNAL STANDARD	0.039	12:36
BLANK TEST	0.000	12:37
EXTERNAL STANDARD	0.039	12:38
BLANK TEST	0.000	12:38
EXTERNAL STANDARD	0.039	12:39
BLANK TEST	0.000	12:40

Average = 0.0390  
 Std Dev = 0.0000

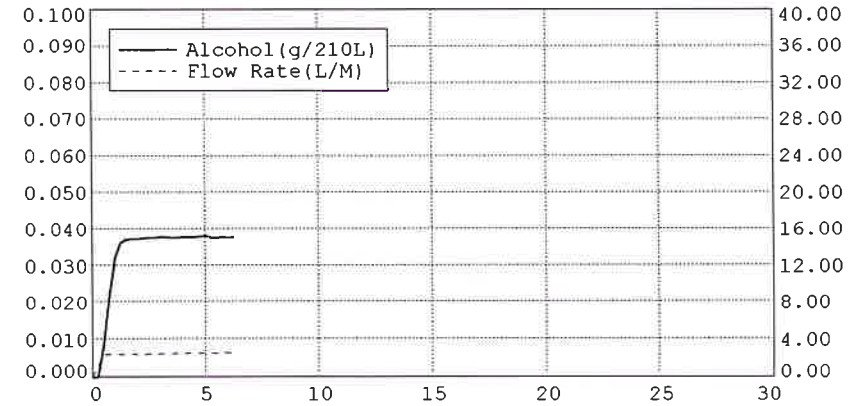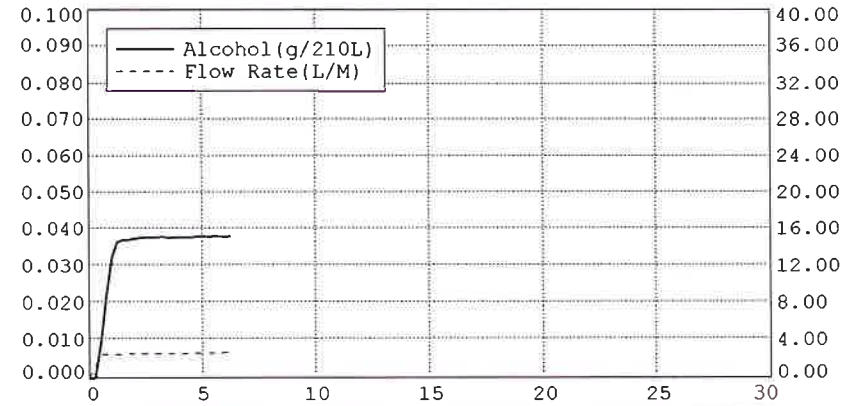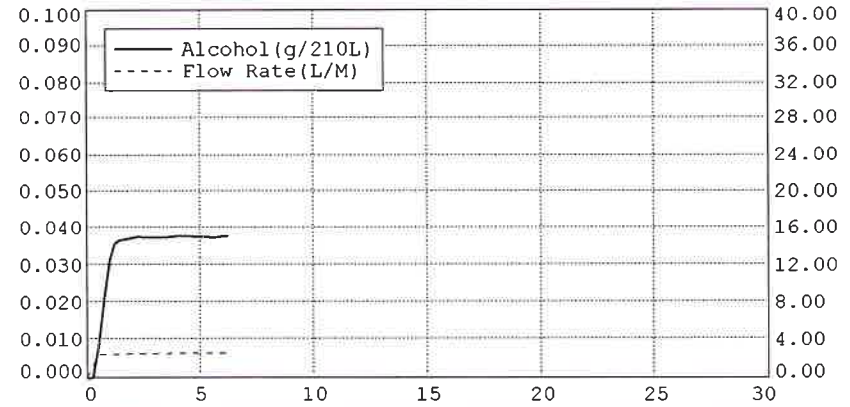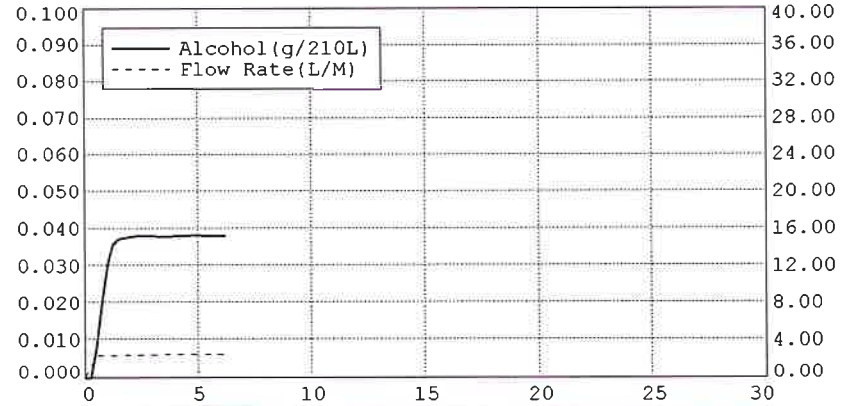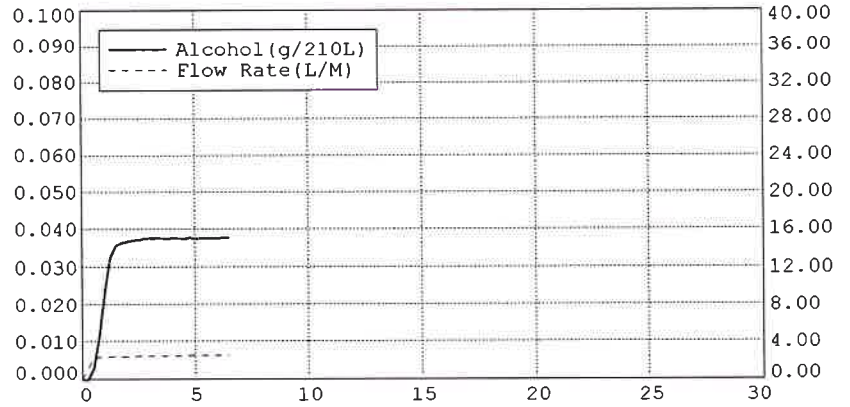

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100388






Date: 04/05/2023  
 Time: 12:42:27

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.35: 0.078  
 LOT #: AG135004  
 EXPIRATION: 12/16/2023  
 TANK PRESSURE: 539 psi

BLANK TEST	0.000	12:43
INTERNAL STANDARD	VERIFIED	12:43
EXTERNAL STANDARD	0.077	12:43
BLANK TEST	0.000	12:44
EXTERNAL STANDARD	0.077	12:44
BLANK TEST	0.000	12:45
EXTERNAL STANDARD	0.077	12:46
BLANK TEST	0.000	12:46
EXTERNAL STANDARD	0.077	12:47
BLANK TEST	0.000	12:48
EXTERNAL STANDARD	0.077	12:48
BLANK TEST	0.000	12:49

Average = 0.0770  
 Std Dev = 0.0000

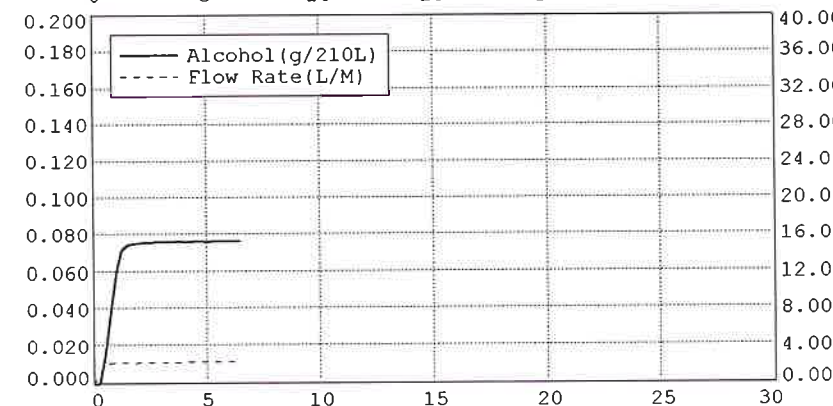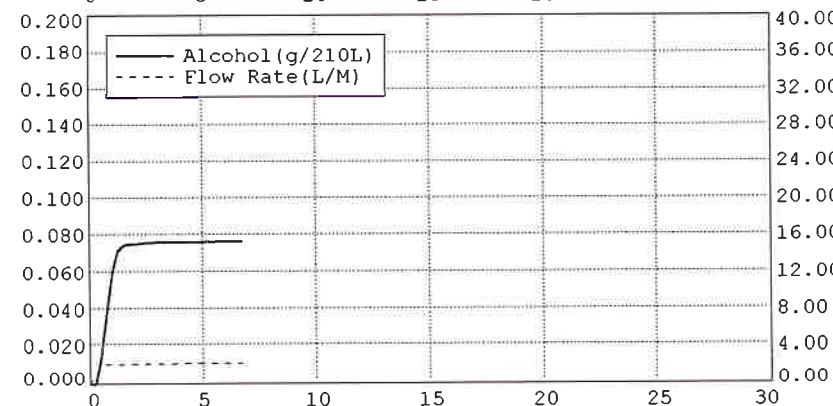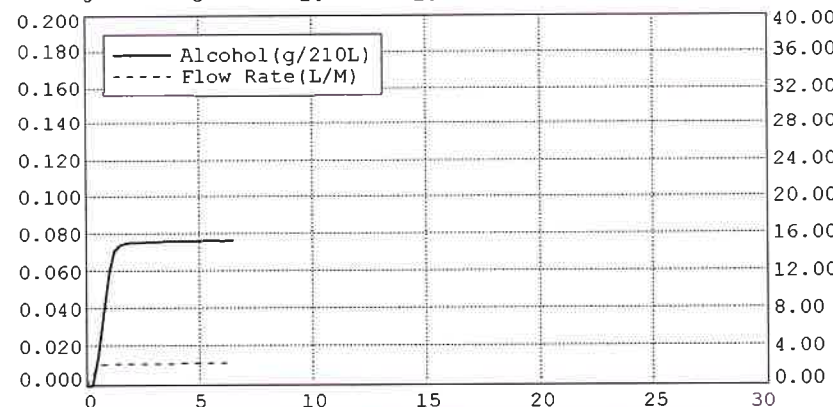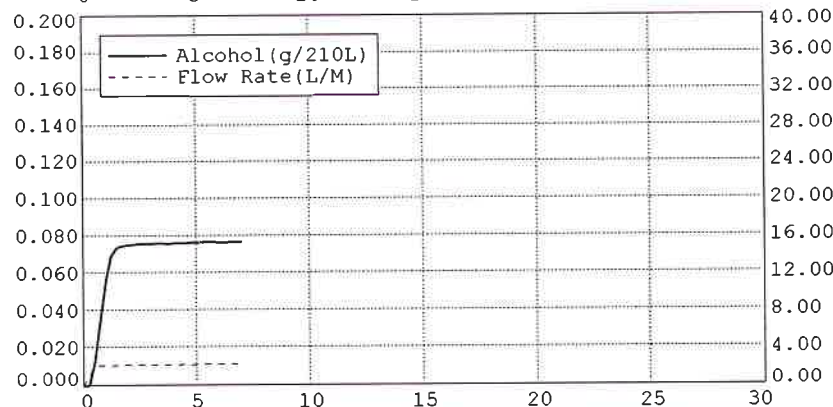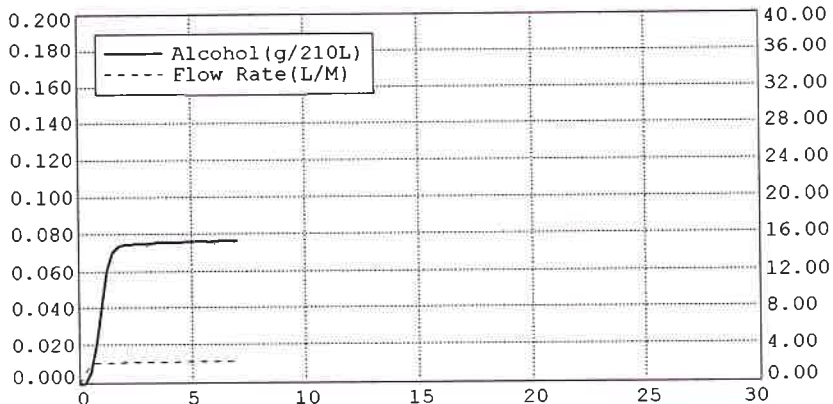

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100388






Date: 04/05/2023  
 Time: 12:51:11

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.35: 0.098  
 LOT #: AG211003  
 EXPIRATION: 04/20/2024  
 TANK PRESSURE: 778 psi

BLANK TEST	0.000	12:52
INTERNAL STANDARD	VERIFIED	12:52
EXTERNAL STANDARD	0.097	12:52
BLANK TEST	0.000	12:53
EXTERNAL STANDARD	0.097	12:53
BLANK TEST	0.000	12:54
EXTERNAL STANDARD	0.097	12:55
BLANK TEST	0.000	12:55
EXTERNAL STANDARD	0.097	12:56
BLANK TEST	0.000	12:57
EXTERNAL STANDARD	0.097	12:57
BLANK TEST	0.000	12:58

Average = 0.0970  
 Std Dev = 0.0000

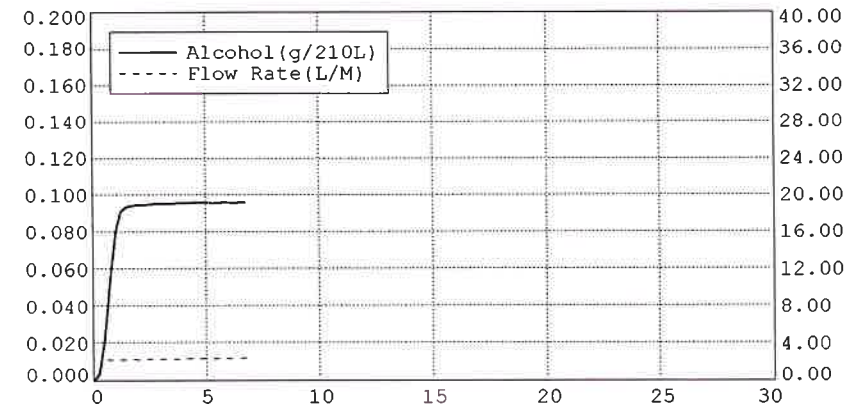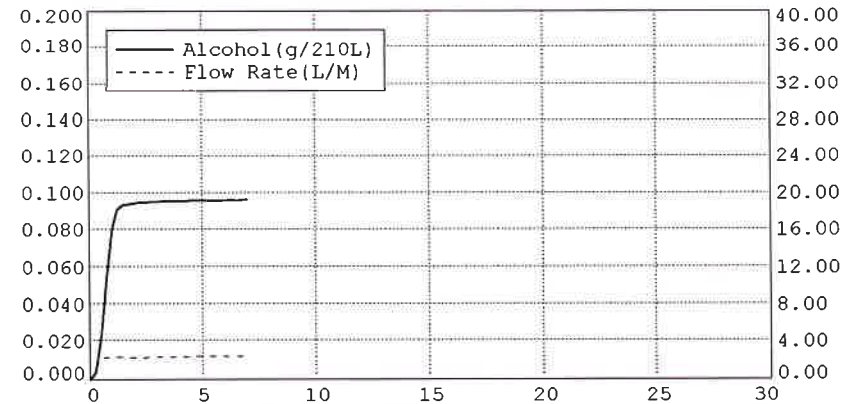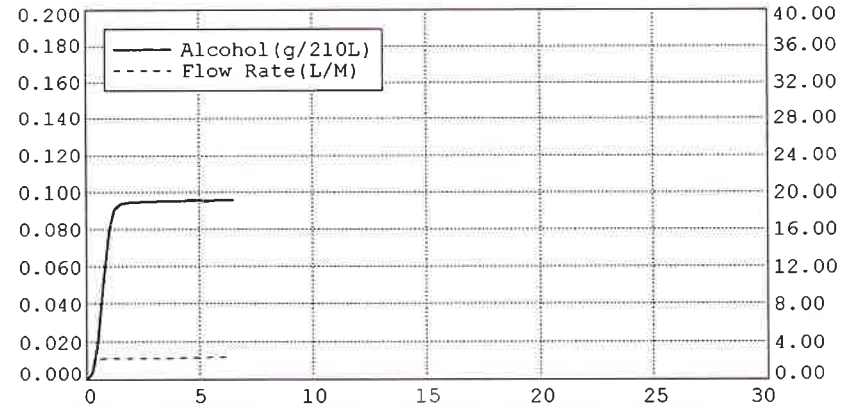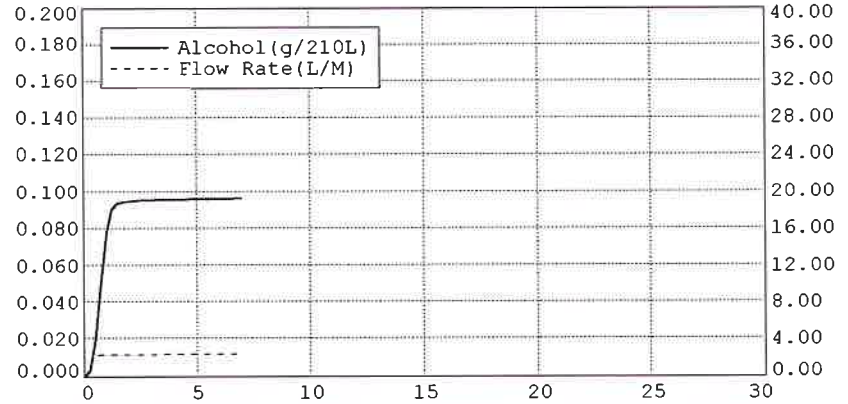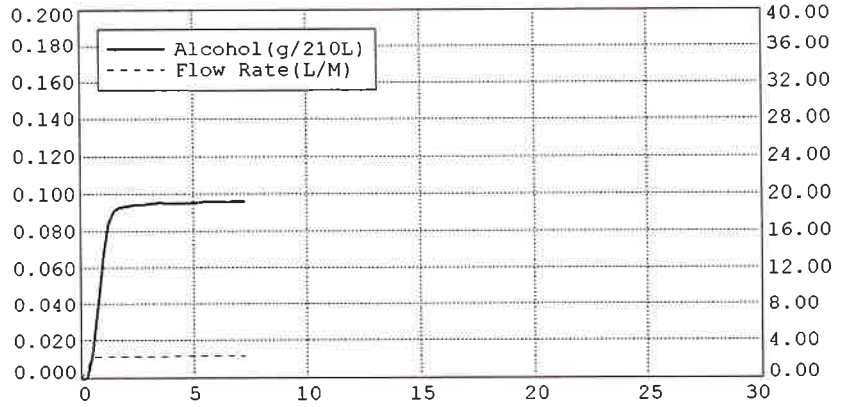



LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100388






Date: 04/05/2023  
 Time: 12:58:26

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.35: 0.147  
 LOT #: AG134205  
 EXPIRATION: 12/08/2023  
 TANK PRESSURE: 1008 psi

BLANK TEST	0.000	12:59
INTERNAL STANDARD	VERIFIED	12:59
EXTERNAL STANDARD	0.145	12:59
BLANK TEST	0.000	13:00
EXTERNAL STANDARD	0.145	13:01
BLANK TEST	0.000	13:02
EXTERNAL STANDARD	0.145	13:02
BLANK TEST	0.000	13:03
EXTERNAL STANDARD	0.146	13:03
BLANK TEST	0.000	13:04
EXTERNAL STANDARD	0.145	13:04
BLANK TEST	0.000	13:05

Average = 0.1452  
 Std Dev = 0.0004

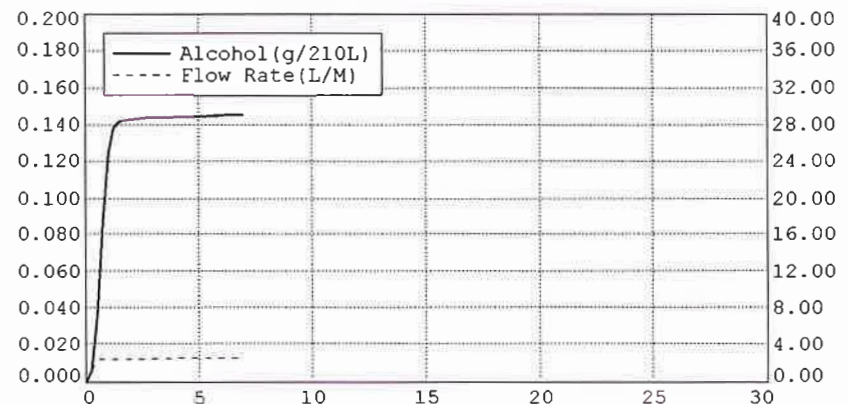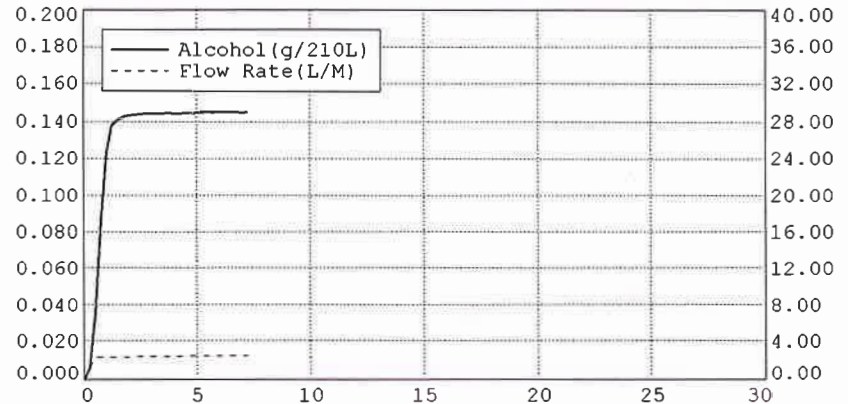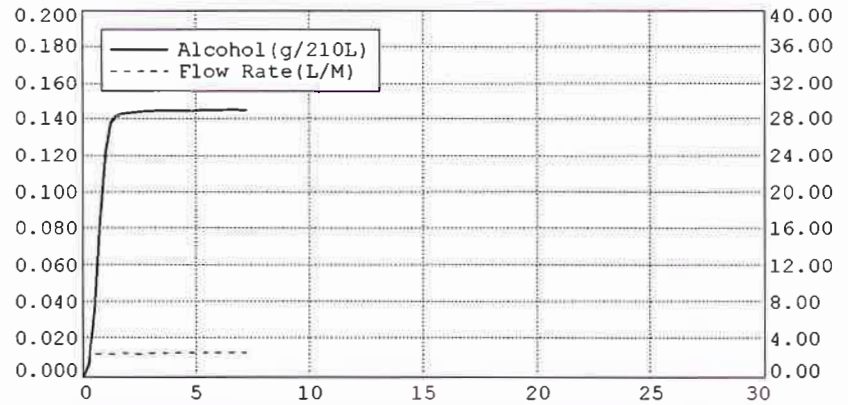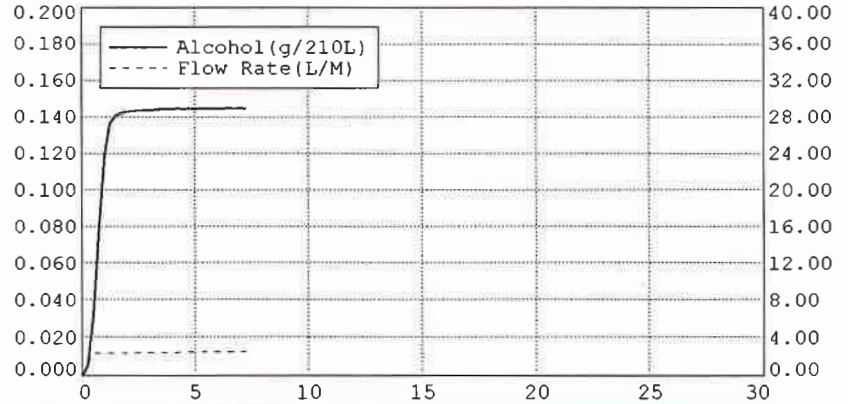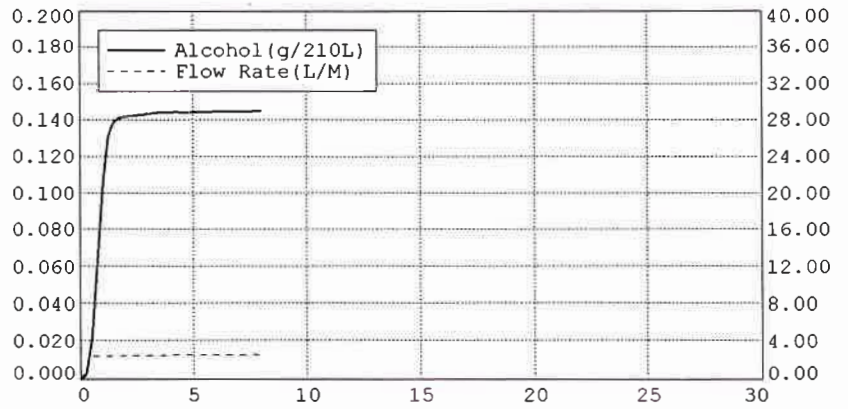

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100388






Date: 04/05/2023  
 Time: 13:06:26

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.34: 0.294  
 LOT #: AG217903  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 358 psi

BLANK TEST	0.000	13:09
INTERNAL STANDARD	VERIFIED	13:09
EXTERNAL STANDARD	0.292	13:09
BLANK TEST	0.000	13:10
EXTERNAL STANDARD	0.292	13:10
BLANK TEST	0.000	13:11
EXTERNAL STANDARD	0.292	13:11
BLANK TEST	0.000	13:12
EXTERNAL STANDARD	0.292	13:13
BLANK TEST	0.000	13:13
EXTERNAL STANDARD	0.292	13:14
BLANK TEST	0.000	13:15

Average = 0.2920  
 Std Dev = 0.0000

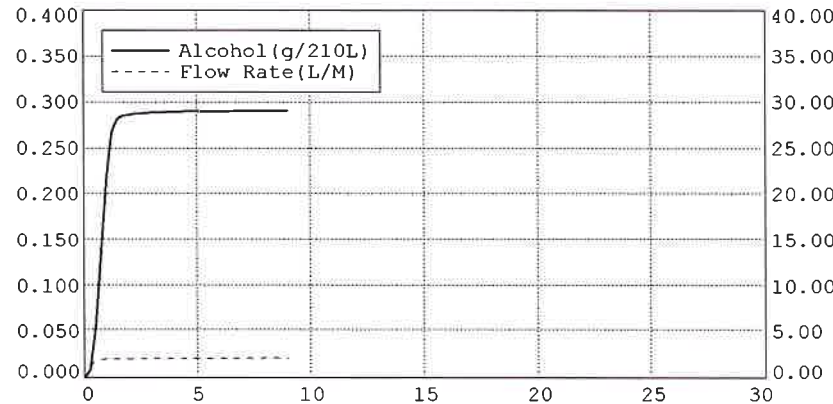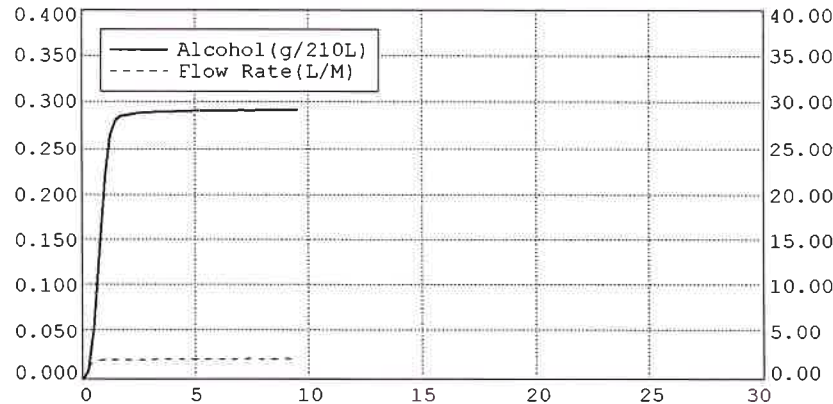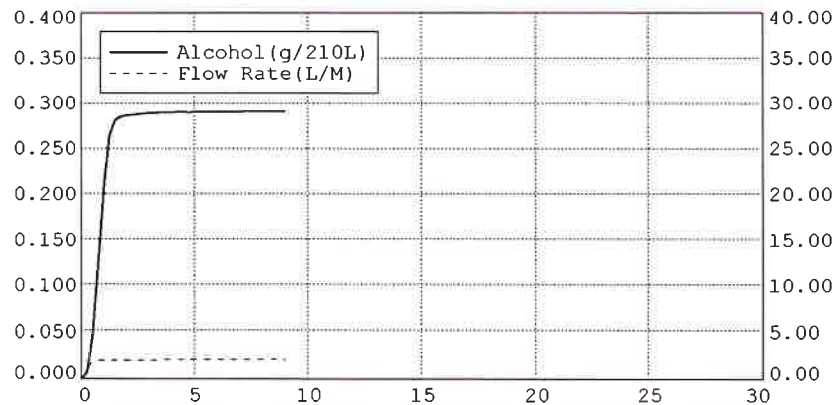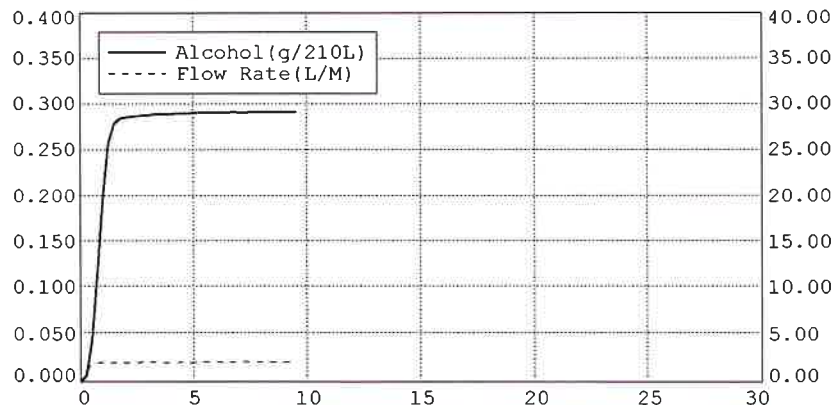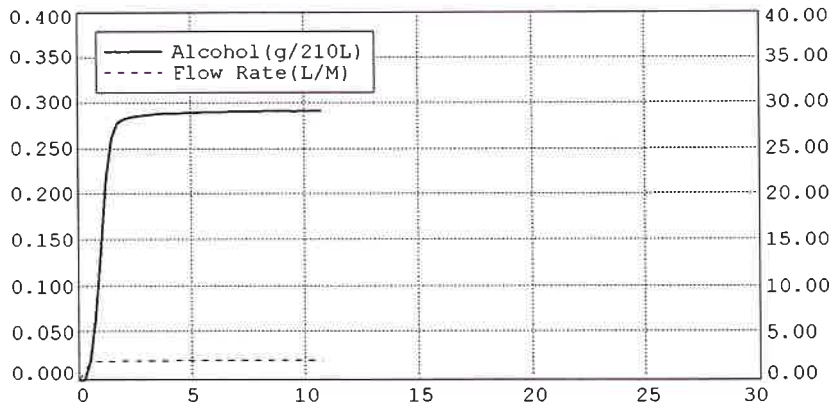

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100388

Date: 04/05/2023  
Time: 13:43:23

SUBJECT NAME:  
TEST TEST  
LICENSE #: INCOMPLETE


OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	13:51
BLANK TEST	0.000	13:51
INTERNAL STANDARD	VERIFIED	13:51
EXTERNAL STANDARD	0.078	13:51
BLANK TEST	0.000	13:52
SUBJECT SAMPLE	INCOMPLETE	13:54

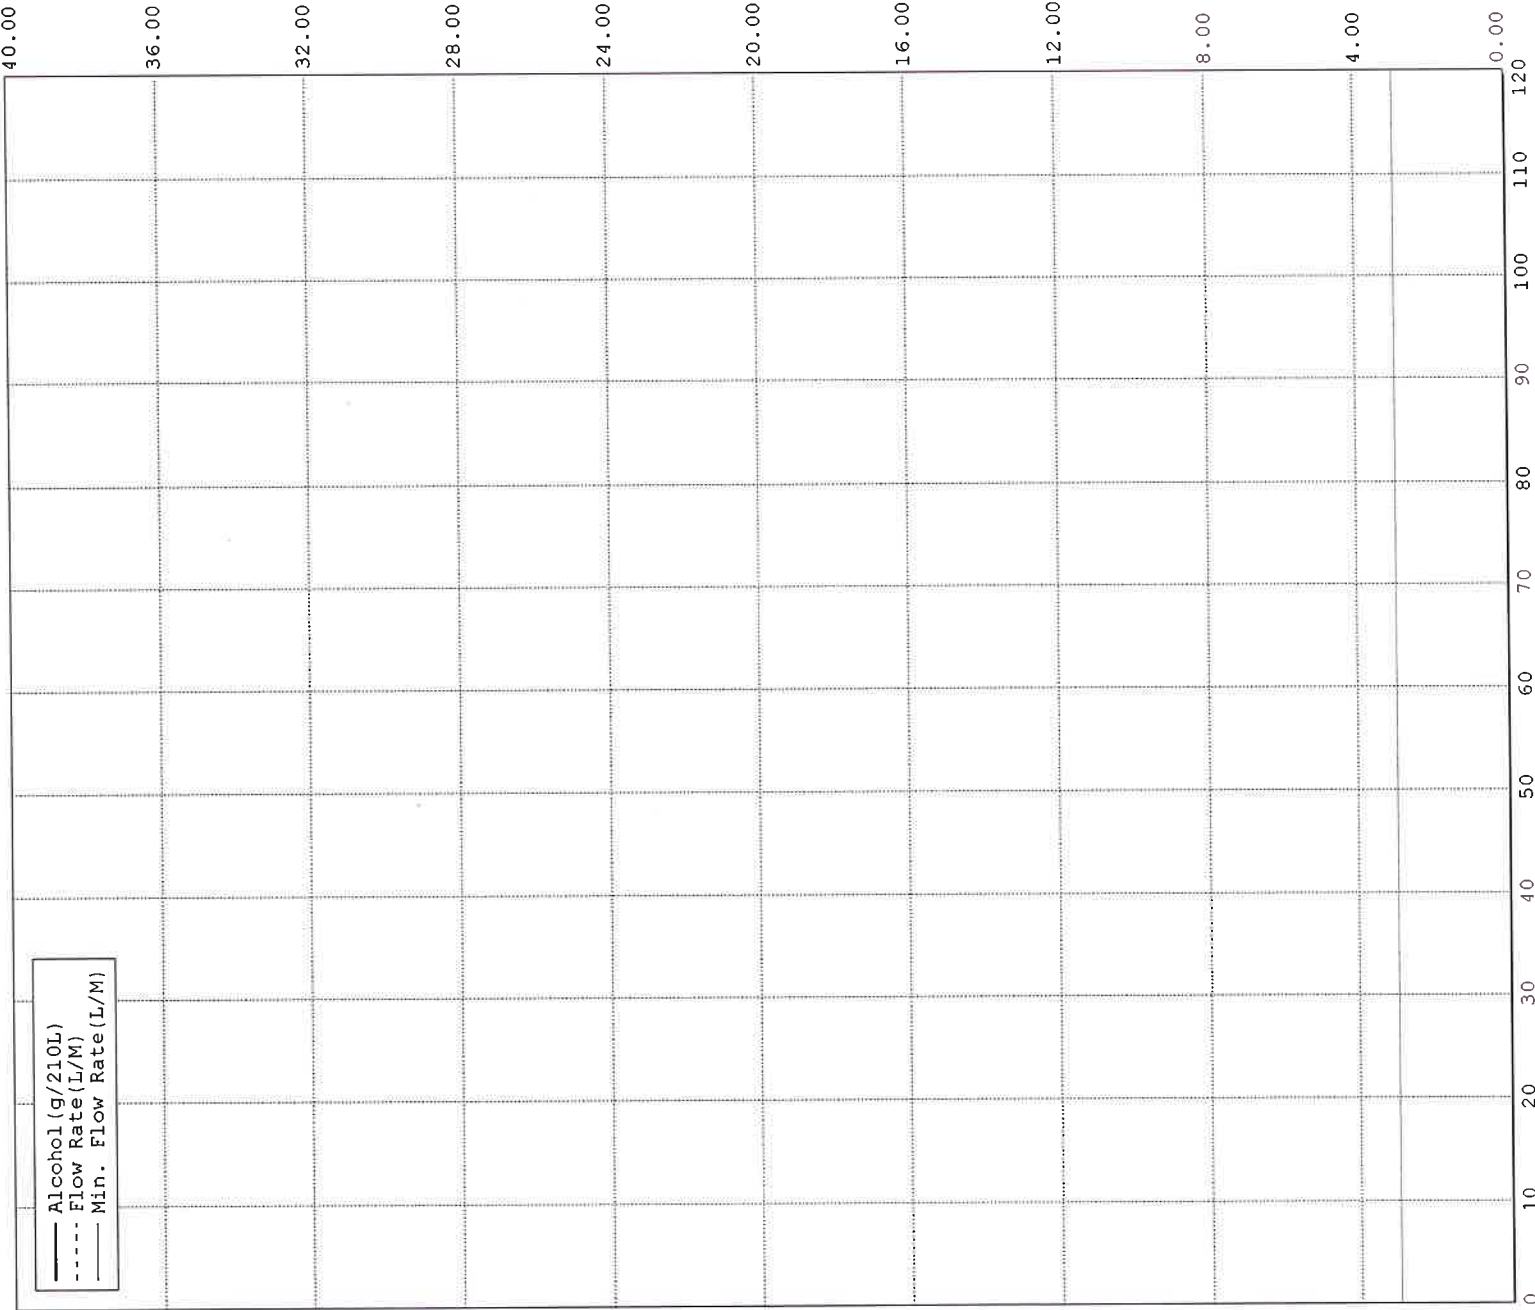



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100388

Date: 04/05/2023  
Time: 13:58:41

SUBJECT NAME:  
TEST TEST  
LICENSE #: MAX ATTEMPTS

OPERATOR NAME:  
COLLEEN S O'BRYANT  
OPERATOR'S #: 6237


DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 13:59  
BLANK TEST 0.000 14:00  
INTERNAL STANDARD VERIFIED 14:00  
EXTERNAL STANDARD 0.078 14:00  
BLANK TEST 0.000 14:01  
SUBJECT SAMPLE XXX 14:02

Maximum Attempts Exceeded

CUS

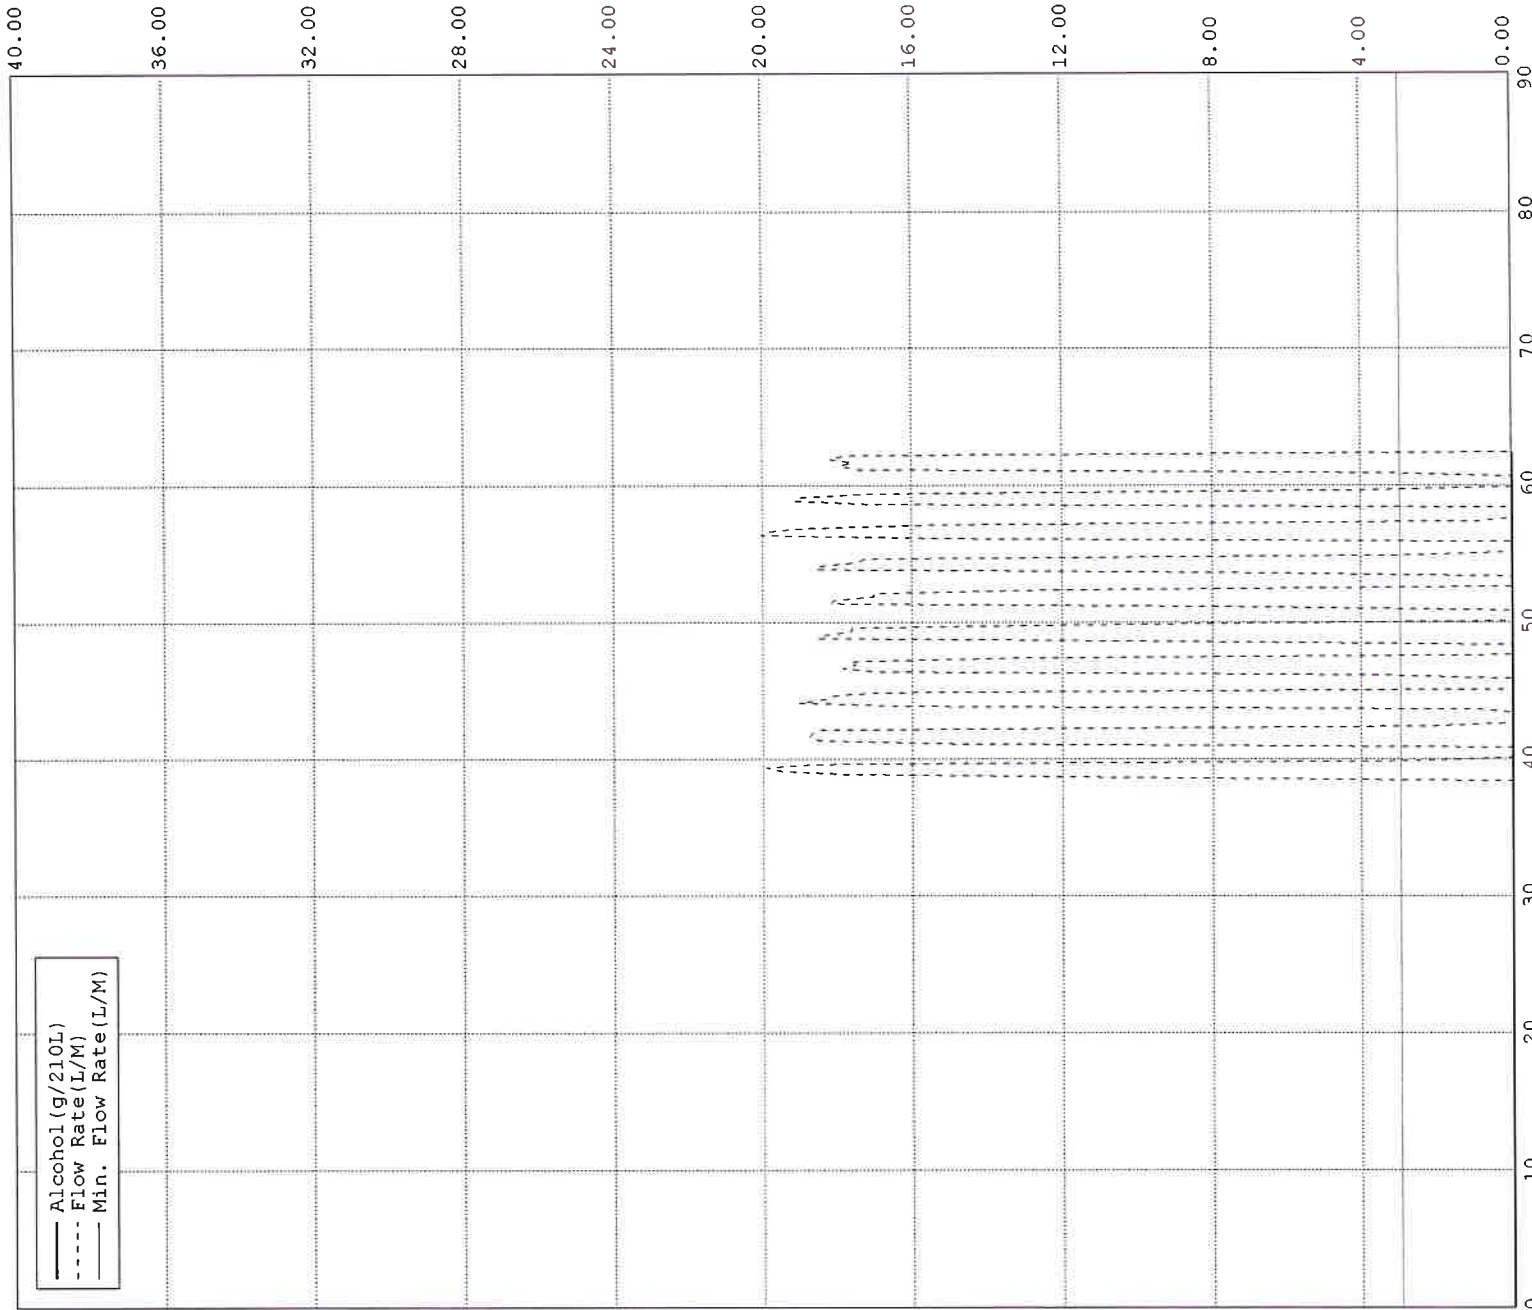

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100388

Date: 04/05/2023  
Time: 14:13:42


SUBJECT NAME:  
TEST TEST  
LICENSE #: INVALID

OPERATOR NAME:  
COLLEEN S O'BRYANT  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.34: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	14:15
BLANK TEST	0.000	14:15
INTERNAL STANDARD	VERIFIED	14:15
EXTERNAL STANDARD	0.078	14:15
BLANK TEST	0.000	14:16
SUBJECT SAMPLE	INVALID	14:17

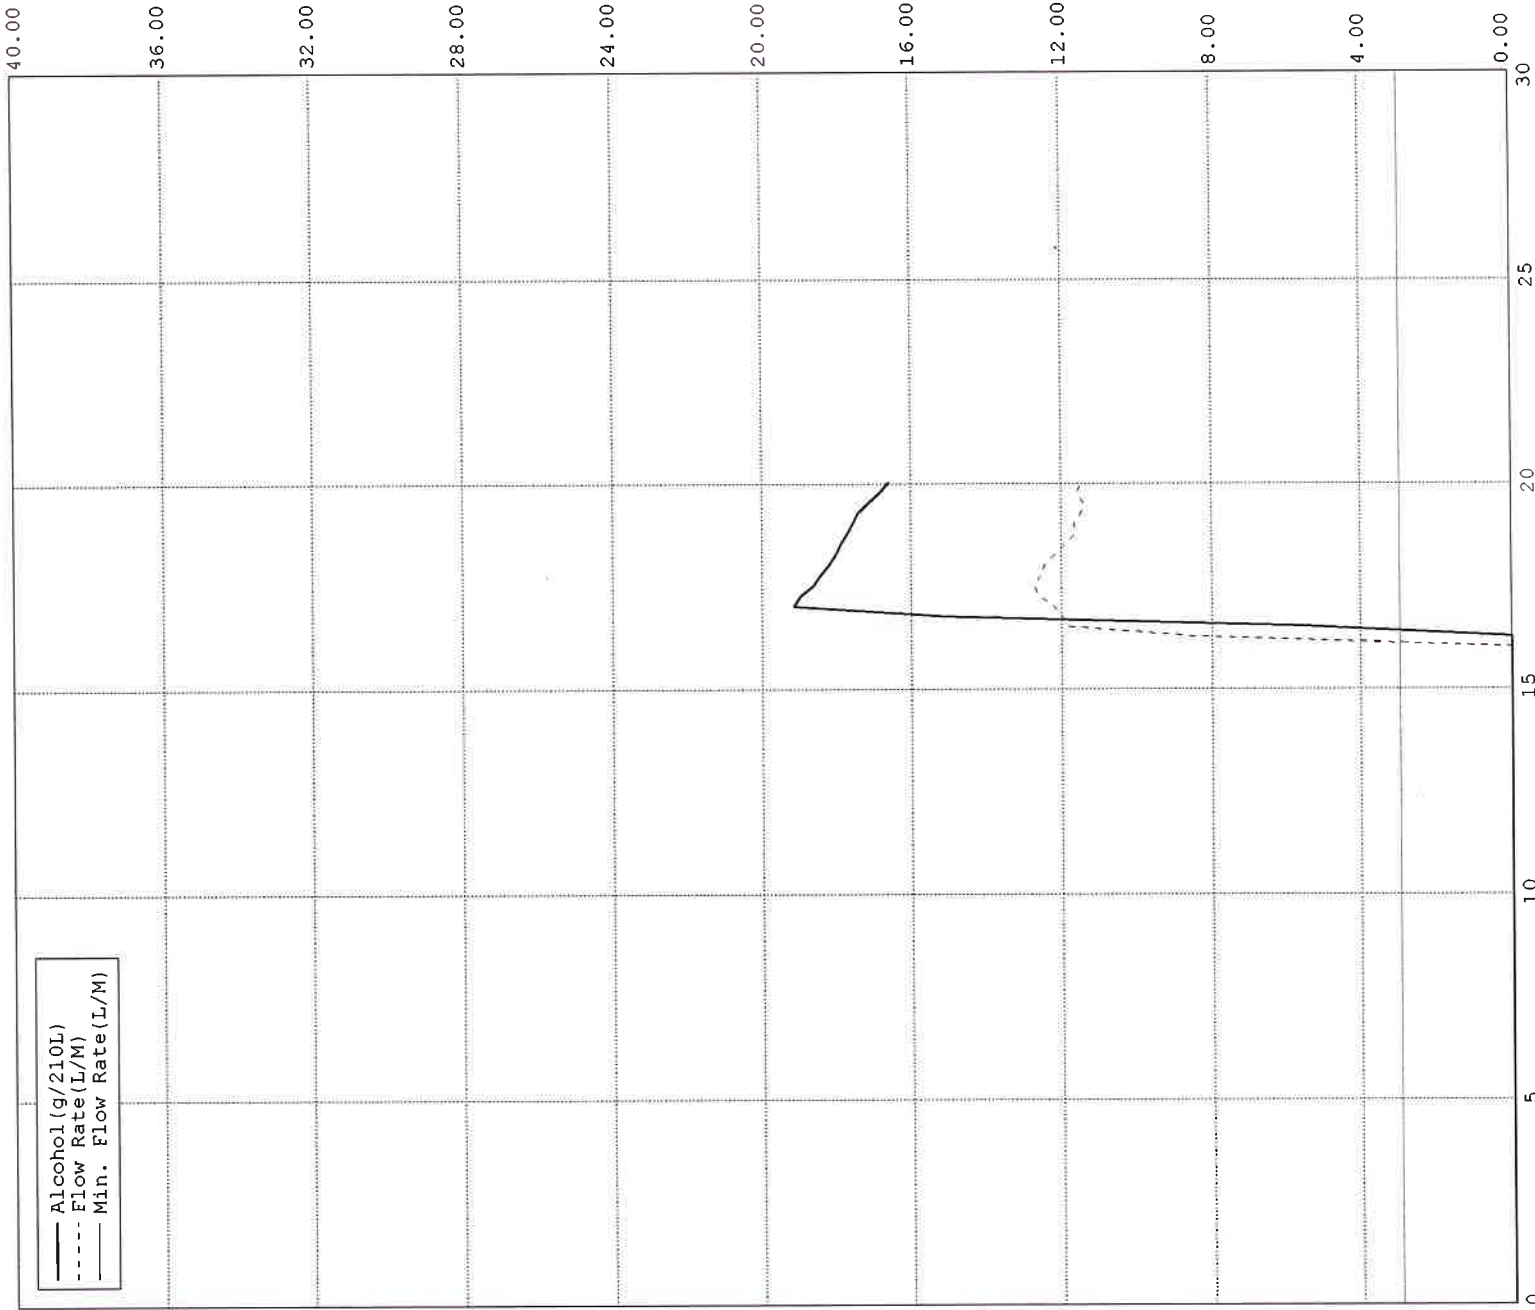

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100388

Date: 04/05/2023  
Time: 14:04:54

SUBJECT NAME:  
TEST TEST  
LICENSE #: RFI

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237


DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 14:05  
BLANK TEST 0.000 14:06  
INTERNAL STANDARD VERIFIED 14:06  
EXTERNAL STANDARD 0.077 14:06  
BLANK TEST 0.000 14:07

RFI DETECTED

ACRS

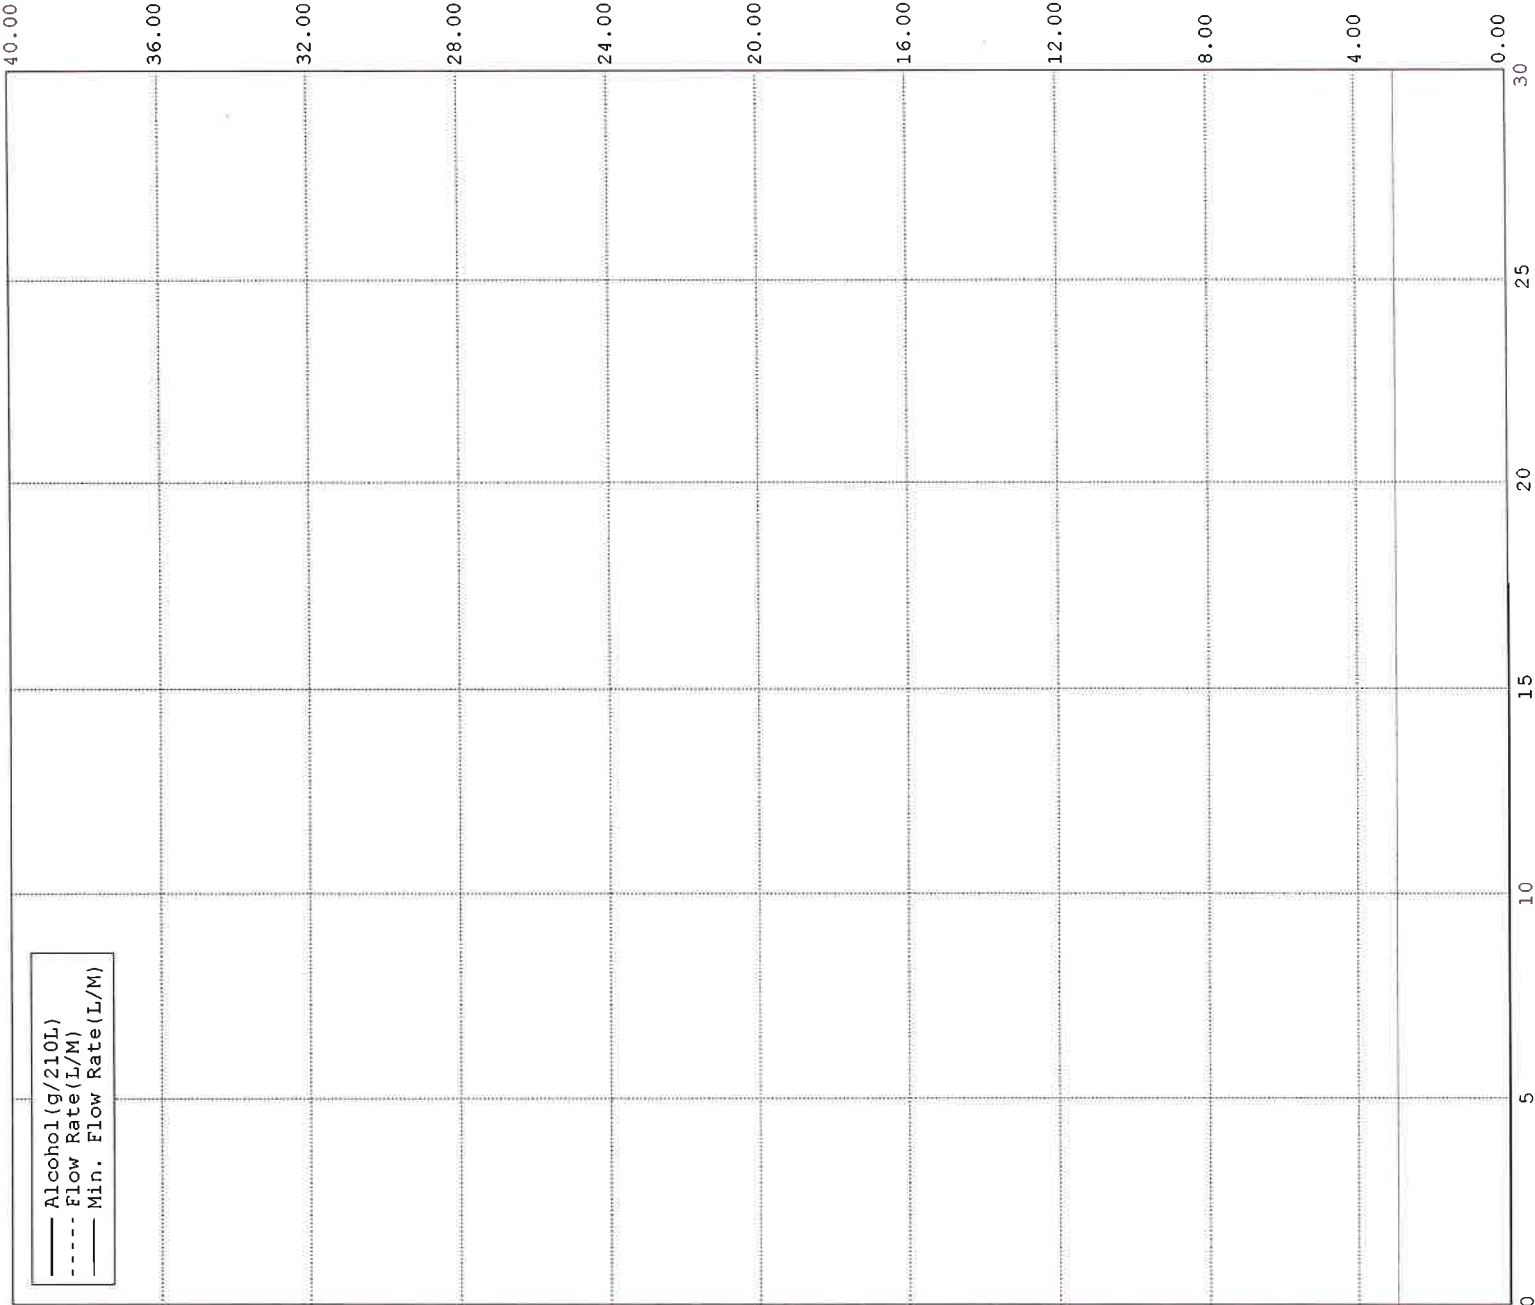

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100388

Date: 04/05/2023  
Time: 13:19:21

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-ACETONE

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237


DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 13:20  
BLANK TEST 0.000 13:20  
INTERNAL STANDARD VERIFIED 13:20  
Xg = 0.101 (1.32%) 0.078 13:20  
EXTERNAL STANDARD X[1] = 0.0784 (-0.0002) (0.0035)  
BLANK TEST 0.000 13:21  
SUBJECT SAMPLE XXX 13:22  
X[1] = 0.1041 (-0.0170) (0.0019)

Interference Detected

*Filter 2 Avg = -0.0003*  
*Filter 3 Avg = 0.0031*

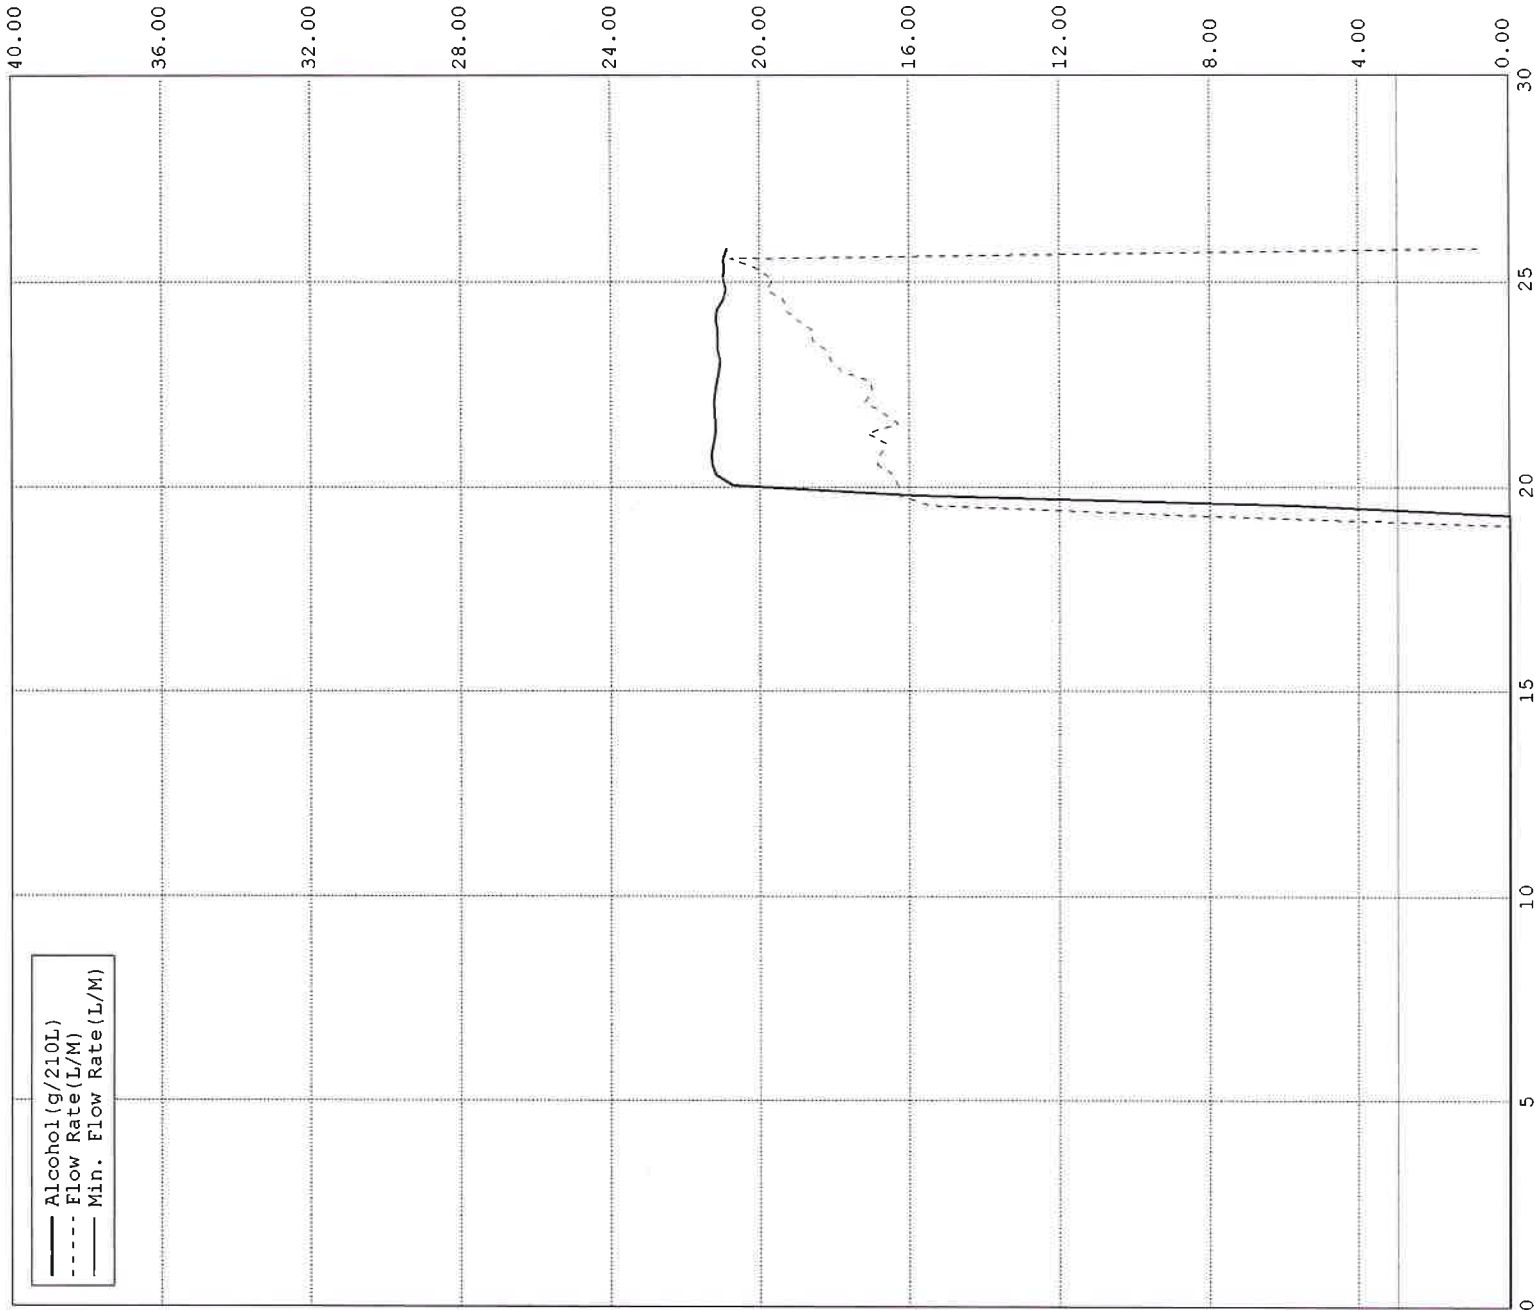

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100388

Date: 04/05/2023  
Time: 13:26:28

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-IPA

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	13:27
BLANK TEST	0.000	13:27
INTERNAL STANDARD	VERIFIED	13:27
Xq = 0.102 (1.93%)		
EXTERNAL STANDARD	0.078	13:27
X[1] = 0.0783 (0.0000) (0.0035)		
BLANK TEST	0.000	13:28
SUBJECT SAMPLE	XXX	13:29
X[1] = 0.1153 (-0.0239) (0.0022)		

Interference Detected

*CAS*

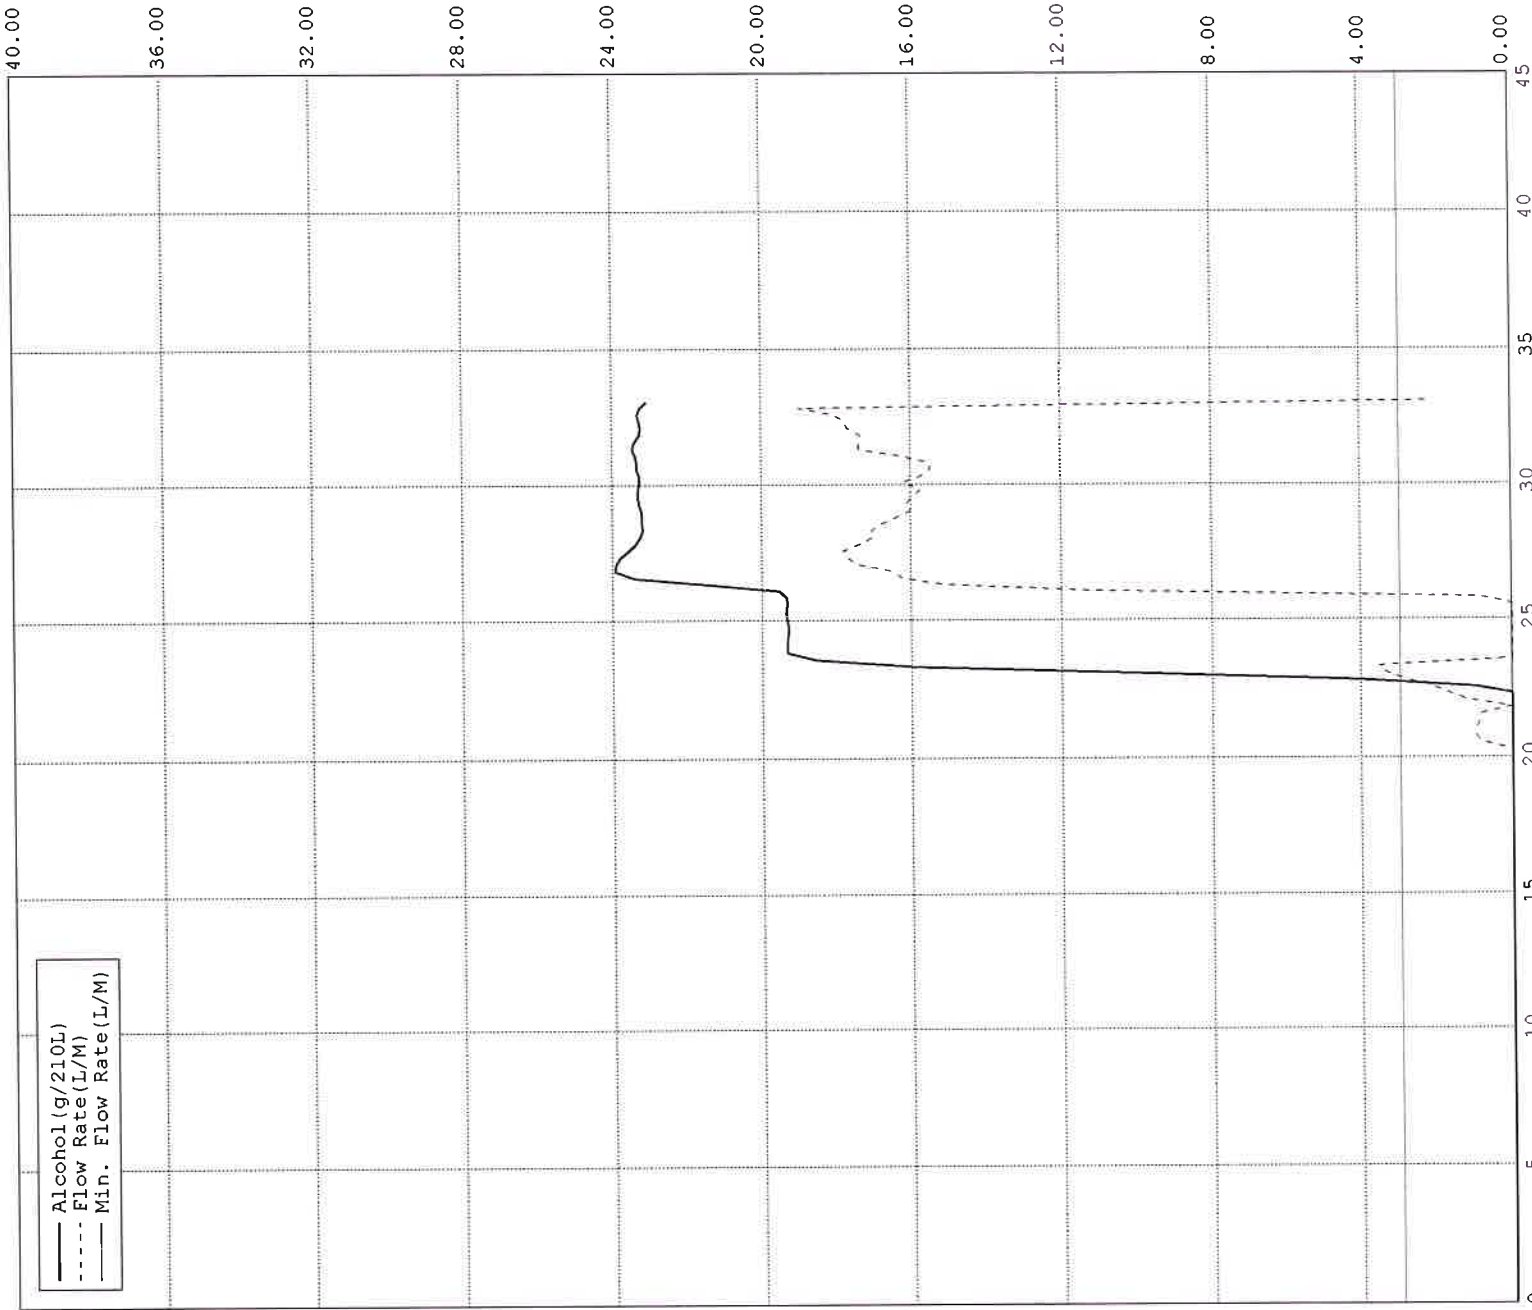



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100388

Date: 04/05/2023  
Time: 13:33:51


SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-NEGATIVE

OPERATOR NAME:  
COLLEEN S OBRYANT  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	13:35
BLANK TEST	0.000	13:35
INTERNAL STANDARD	VERIFIED	13:35
Xq = 0.101 (1.41%)		
EXTERNAL STANDARD	0.078	13:35
X[1] = 0.0776 (-0.0003) (0.0032)		
BLANK TEST	0.000	13:36
SUBJECT SAMPLE (Vol=1.91L)	0.090	13:37
X[1] = 0.0908 (0.0002) (0.0014)		
BLANK TEST	0.000	13:38
EXTERNAL STANDARD	0.077	13:39
X[1] = 0.0770 (-0.0006) (0.0020)		
BLANK TEST	0.000	13:39

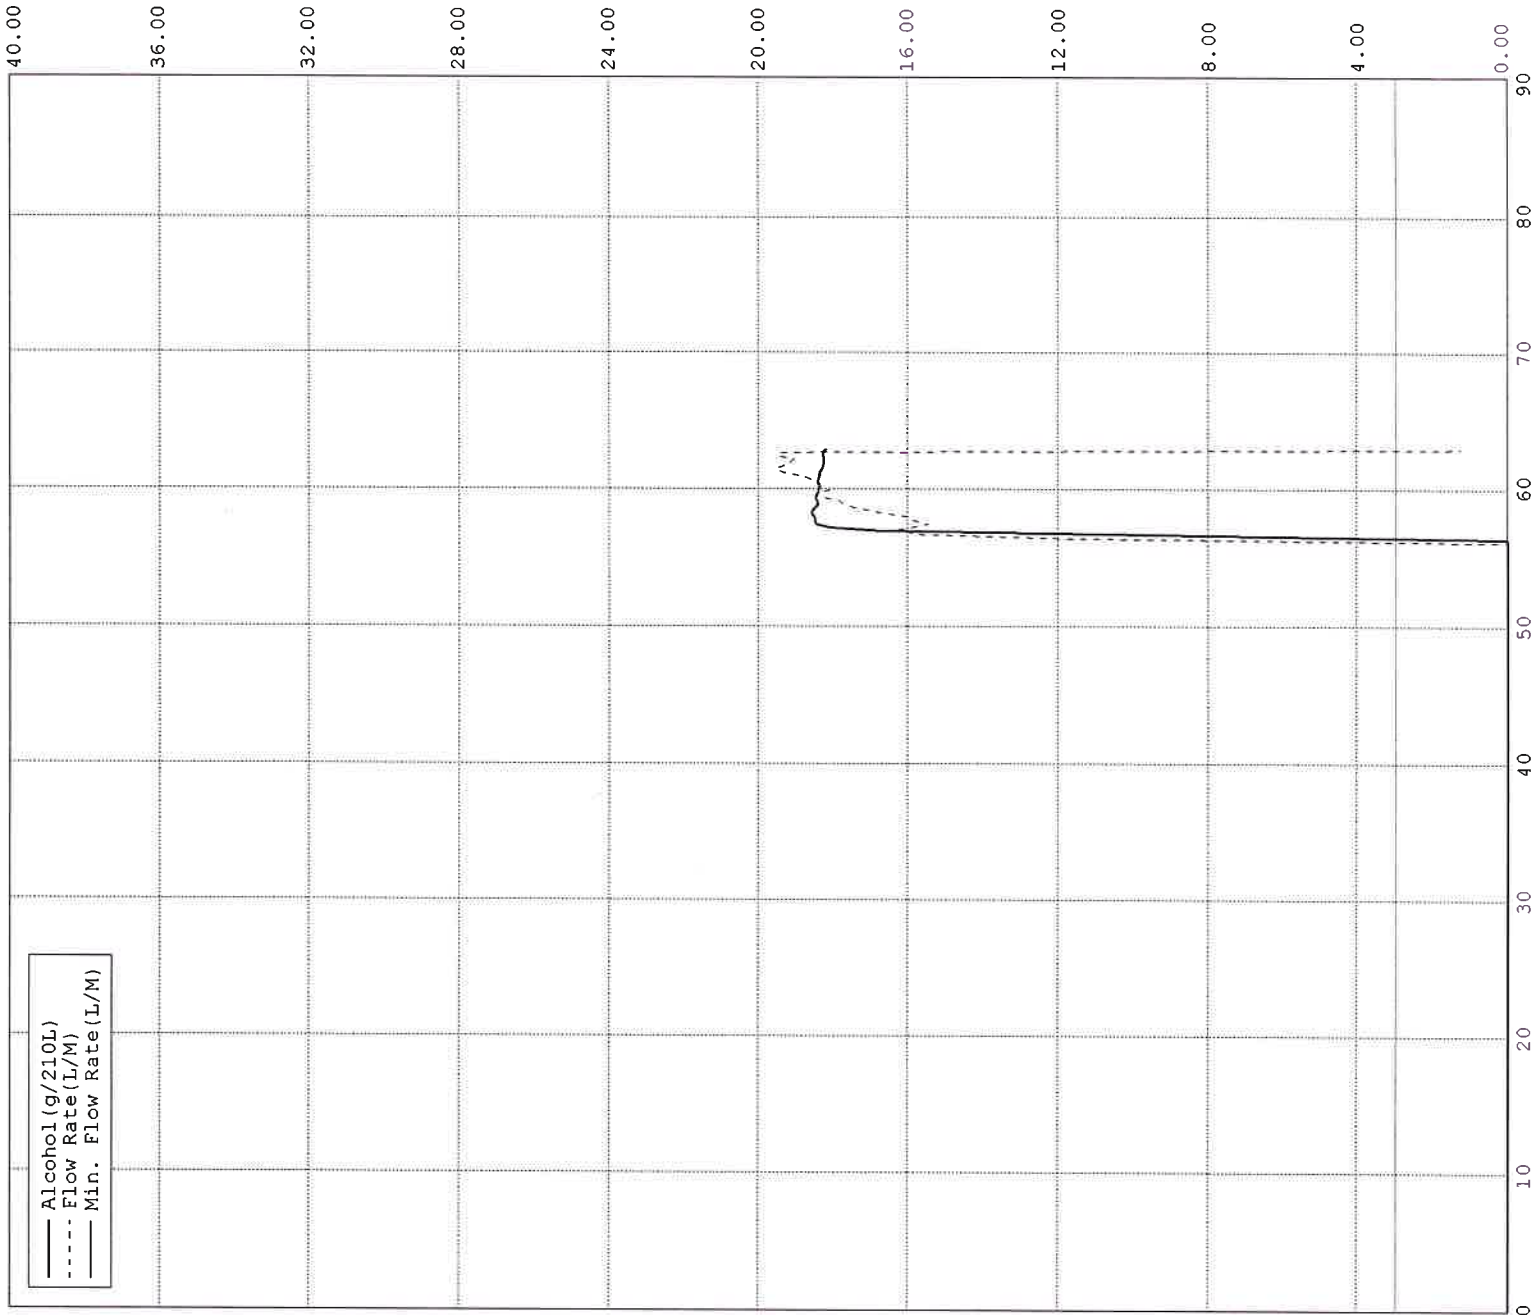



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100388

Date: 04/05/2023  
Time: 16:19:30

SUBJECT NAME:  
TEST TEST  
LICENSE #: NONDRINKING

OPERATOR NAME:  
COLLEEN S OBRyant  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.30: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	16:20
BLANK TEST	0.000	16:20
INTERNAL STANDARD	VERIFIED	16:20
EXTERNAL STANDARD	0.077	16:21
BLANK TEST	0.000	16:21
SUBJECT SAMPLE (Vol=1.94L)	0.000	16:22
BLANK TEST	0.000	16:23
EXTERNAL STANDARD	0.078	16:23
BLANK TEST	0.000	16:24

