




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100414

Report Issue Date: 07/28/2025
Date Received: 2025-07-01
Condition of Item: Damaged

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.019	0.020	0.020	0.020	0.021	0.020
0.080	0.080	AG335202	0.080	0.078	0.079	0.079	0.078	0.079
0.300	0.298	AG427706	0.297	0.296	0.296	0.296	0.296	0.296

As Found - Evaluation Analyst: Carlie Glaister

As Found Conditions - Barometric Pressure (inHg): 29.76 Barometer Used: VWR S/N 240680771 Temperature (C): 21.3 Relative Humidity (%): 41

As-Found Lab Activity Date Range: 07/03/2025 - 07/03/2025

No o-ring present on regulator, added. Solenoid wire is flaking and exposed, resting on mirror block. Recommend replacing and rerouting this wire (touching wire causes pin to move). 5-way valve is stuck - unable to provide breath sample for non-drinking subject test. End of non-drinking subject test has a detector response with no flow. Reset options due to 2 subject tests printing.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.021	0.020	0.020	0.021	0.020	+/- 0.002
0.040	0.040	AG407908	0.039	0.040	0.039	0.040	0.040	0.040	+/- 0.003
0.080	0.080	AG335202	0.079	0.079	0.079	0.079	0.079	0.079	+/- 0.004
0.100	0.100	AG333401	0.100	0.100	0.101	0.101	0.100	0.100	+/- 0.004
0.150	0.150	AG332004	0.147	0.148	0.148	0.148	0.148	0.148	+/- 0.006
0.300	0.300	AG427706	0.300	0.298	0.299	0.298	0.299	0.299	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.97 Barometer Used: VWR S/N 240680771 Temperature (C): 22.5 Relative Humidity (%): 49


As-Left Lab Activity Date Range: 07/21/2025 - 07/24/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Jerrell J. Walton



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Serial Number: 100414

Results authorized by Derek Walton on 07/24/2025

derek.walton@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 07/28/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100414 Analyst or Technician Name: Derek Walton

DataMaster DMT Calibration Start Date: 07/21/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 09/10/26
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.97 Temperature(C) 22.5 Relative Humidity(%) 49%
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) - *Print with View Details*
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20250603KJ Expiration Date: 07/27/25
Simulator S/N: SD1200 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20250603KJ Expiration Date: 09/03/25
Simulator S/N: SD1198 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 23DP41233 Expiration Date: 09/20/25
Simulator S/N: SD1199 Thermometer Verification Performed? ☒

Calibrated External Thermometer S/N: 250159292
Calibration Due Date: 03/14/27

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 07/21/25
Data Interpretation Date (Technician): _____ (if applicable)
Data Interpretation Date (Analyst): 07/23/25 DM

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

 Alaska Department of Public Safety
 DATAMASTER dmt: 100414

Date: 07/21/2025
 Time: 11:19:47

VERSIONS

DMT: 3.02
 PIC: 3.02
 Modem: 2.6
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 45.6°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.88 V	PASSED
(1.13 V - 2.63 V)	
Cooler Voltage = 1.76 V	PASSED
(1.06 V - 2.46 V)	
Bias Voltage = 79 V	PASSED
(47 V - 111 V)	
Chopper Freq = 524 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 30.0 in	

PUMP INFO

Flow Rate = 5.174 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.002 V <= 0.010 V)	
PUMP OFF	PASSED
(0.002 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
Xq = 0.092 0.28% (0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100414

Date: 07/21/2025

Time: 11:29 AM

Temperatures (°C)

Sample Cell: 48.9°C

Breath Tube: 45.3°C

Current Barometer 30.0 in ✓

Volume (Ltr) 1.60 ✓

Settings

Lamp: 1.88 V

Bias: 79 V

Cooler: 1.76 V

Chopper: 527 Hz

Voltages (V)

Flow: 1.04 V

Detector: 0.060 V ✓

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/15/2025
Time: 14:07:37

OPERATOR NAME:
KAIJA SWISHER
CERTIFICATE #: 10746

Ca	=	0.1000		
CAL	=	0.992378	0.800 <=	CAL < 1.200
b1	=	0.0001	0.0000 <=	b1 < 0.0040
b2	=	0.0029	0.0010 <=	b2 < 0.0100
b3	=	0.0004	0.0000 <=	b3 < 0.0040
Xq	=	0.0927	0.0500 <=	Xq < 0.2000
a21	=	1.139712	1.050 <=	a21 < 1.300
a31	=	0.491152	0.300 <=	a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/21/2025
Time: 11:33:06

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

DEPT/AGENCY:
MINIMUM VOLUME
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.98: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:35
BLANK TEST	0.000	11:35
INTERNAL STANDARD	VERIFIED	11:35
EXTERNAL STANDARD	0.079	11:35
BLANK TEST	0.000	11:36
SUBJECT SAMPLE (Vol=1.63L)	0.000	11:37
BLANK TEST	0.000	11:38
EXTERNAL STANDARD	0.079	11:38
BLANK TEST	0.000	11:39

DW

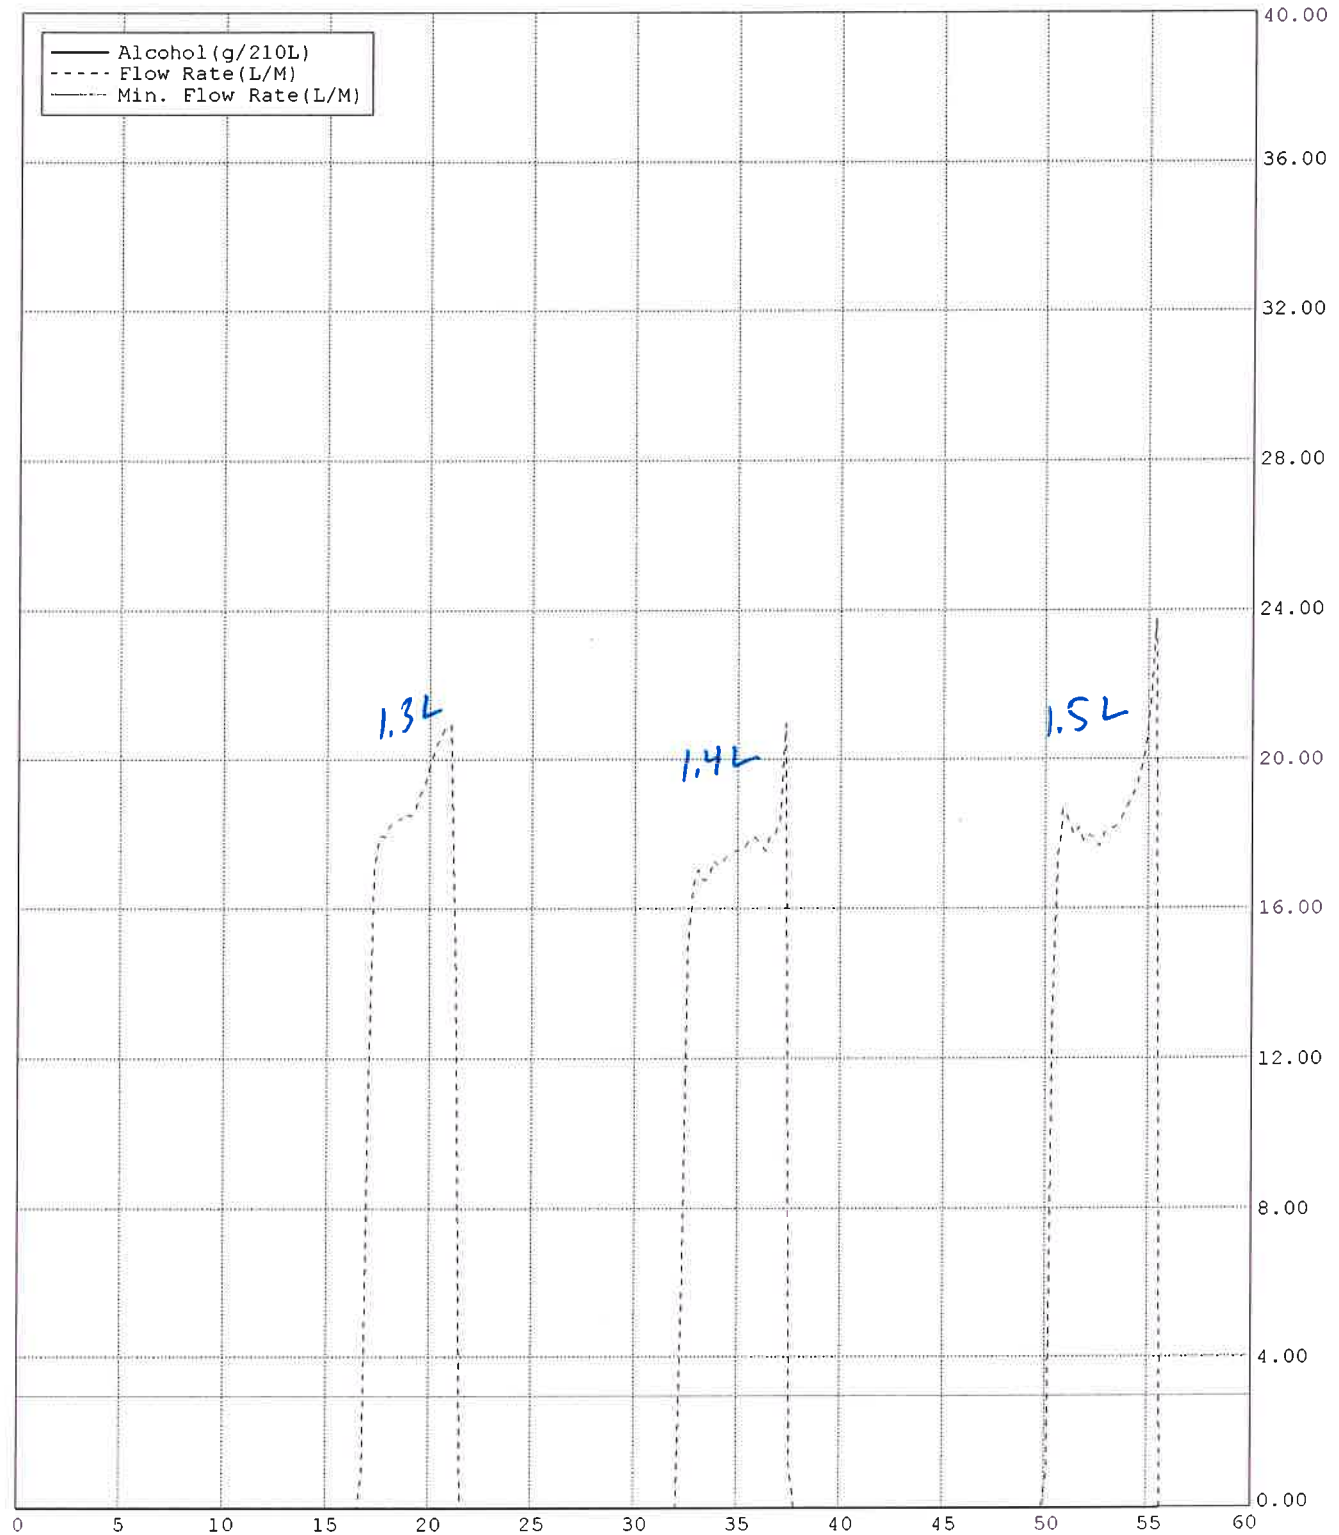

LINEARITY CHECK

Alaska Department of Public Safety
DATAMASTER dmt: 100414


Date: 07/21/2025
Time: 13:12:20

SUPERVISOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

TARGET	AVERAGE	STD. DEV.
0.020	0.0204	0.0005
0.040	0.0396	0.0005
0.080	0.0790	0.0000
0.100	0.1004	0.0005
0.150	0.1478	0.0004
0.300	0.2988	0.0008

SLOPE = 0.994607
 R^2 = 0.999930

DW

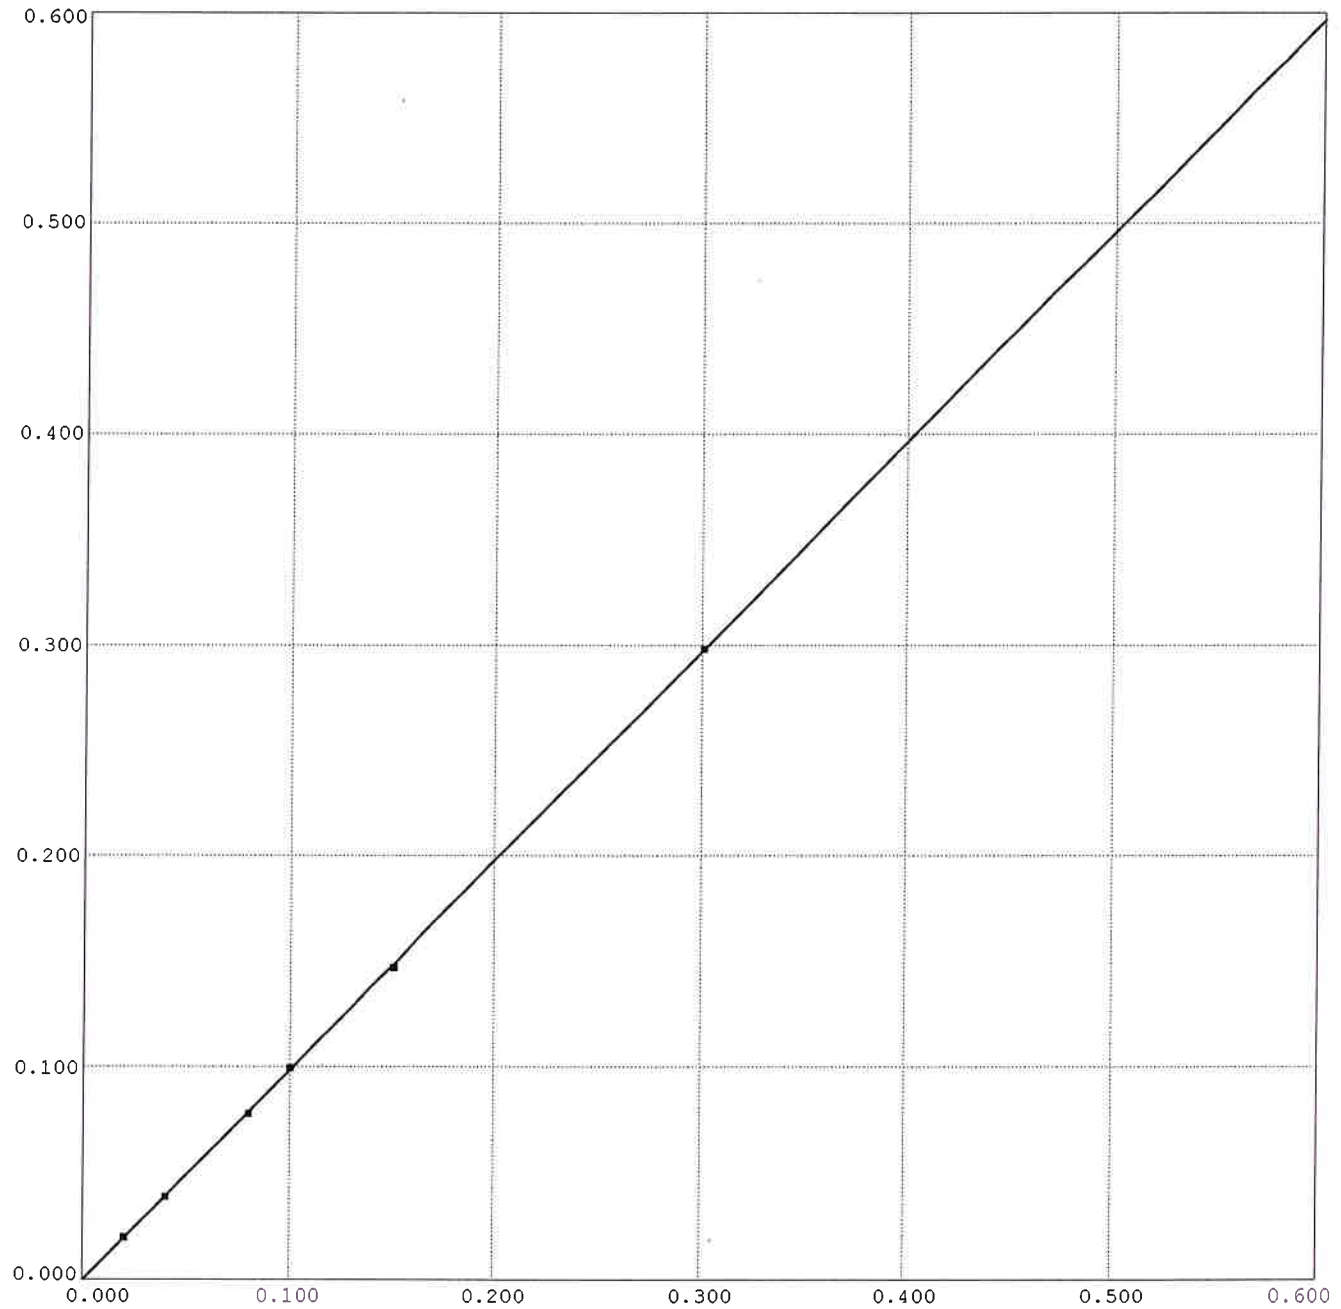

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100414






Date: 07/21/2025
Time: 13:18:16

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.97: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 530 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	13:20
INTERNAL STANDARD	VERIFIED	13:20
EXTERNAL STANDARD	0.020	13:20
BLANK TEST	0.000	13:21
EXTERNAL STANDARD	0.021	13:21
BLANK TEST	0.000	13:22
EXTERNAL STANDARD	0.020	13:22
BLANK TEST	0.000	13:23
EXTERNAL STANDARD	0.020	13:24
BLANK TEST	0.000	13:24
EXTERNAL STANDARD	0.021	13:25
BLANK TEST	0.000	13:26

Average = 0.0204
Std Dev = 0.0005

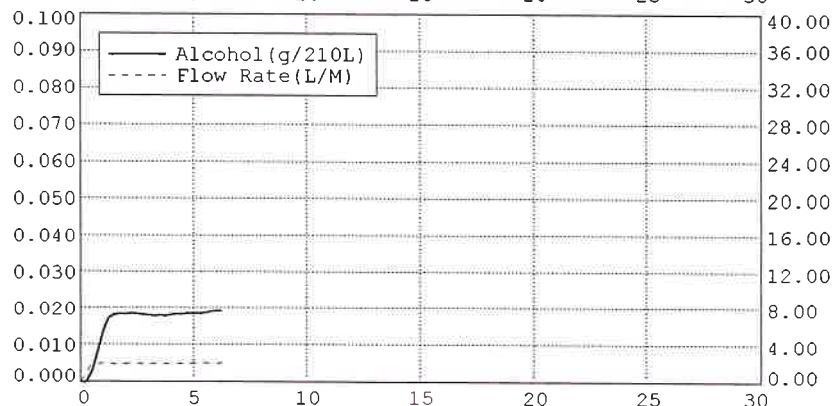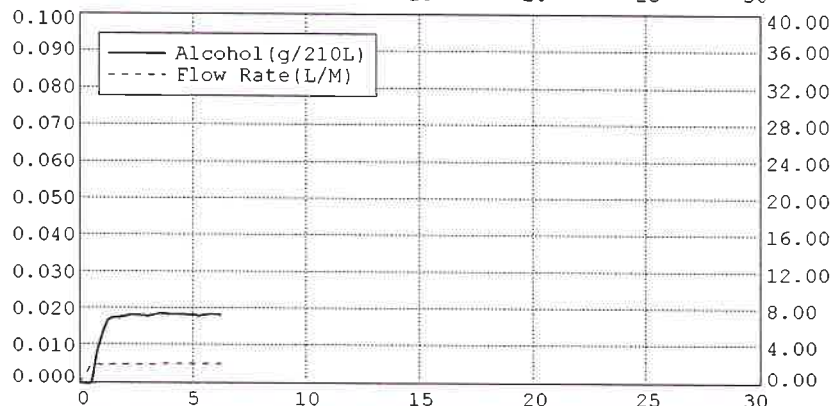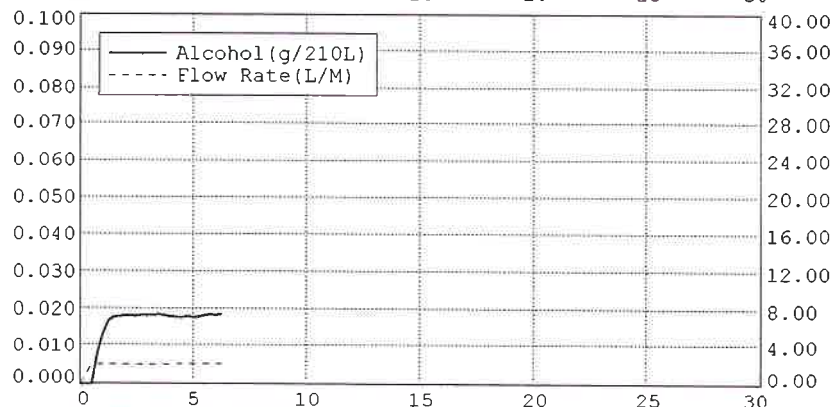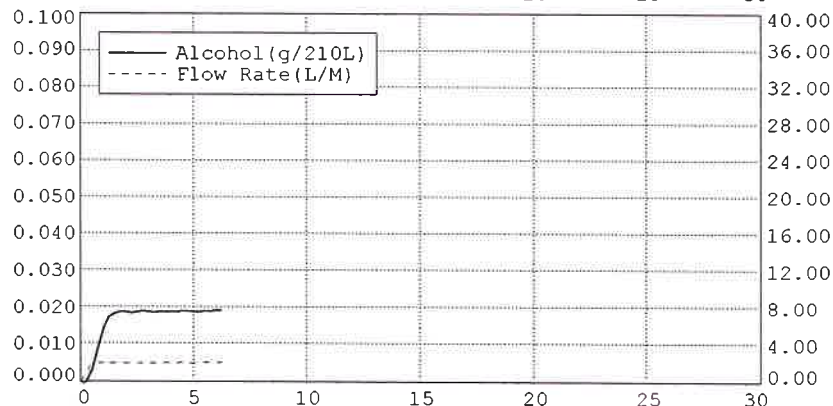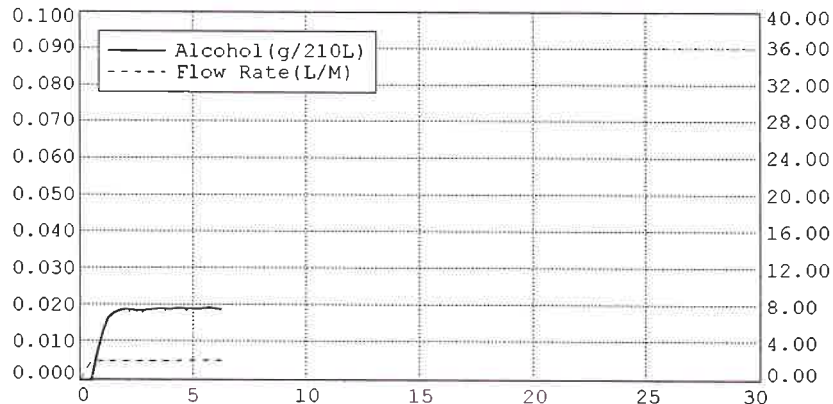

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100414






Date: 07/21/2025
Time: 13:27:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.97: 0.040
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 936 psi

BLANK TEST	0.000	13:29
INTERNAL STANDARD	VERIFIED	13:29
EXTERNAL STANDARD	0.039	13:29
BLANK TEST	0.000	13:30
EXTERNAL STANDARD	0.040	13:30
BLANK TEST	0.000	13:31
EXTERNAL STANDARD	0.039	13:31
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.040	13:32
BLANK TEST	0.000	13:33
EXTERNAL STANDARD	0.040	13:33
BLANK TEST	0.000	13:34

Average = 0.0396
Std Dev = 0.0005

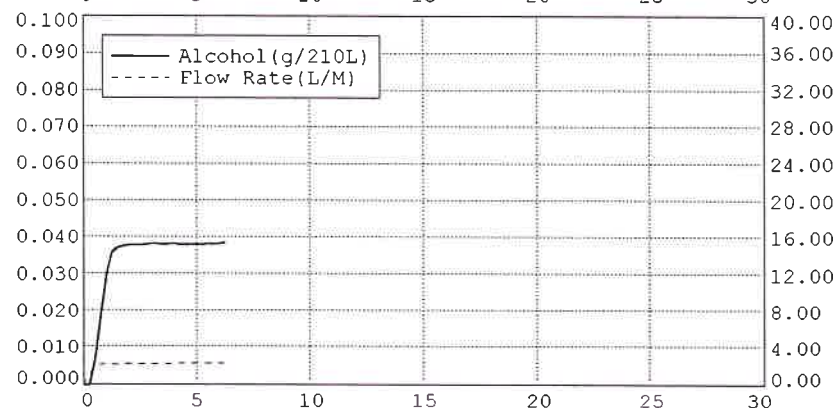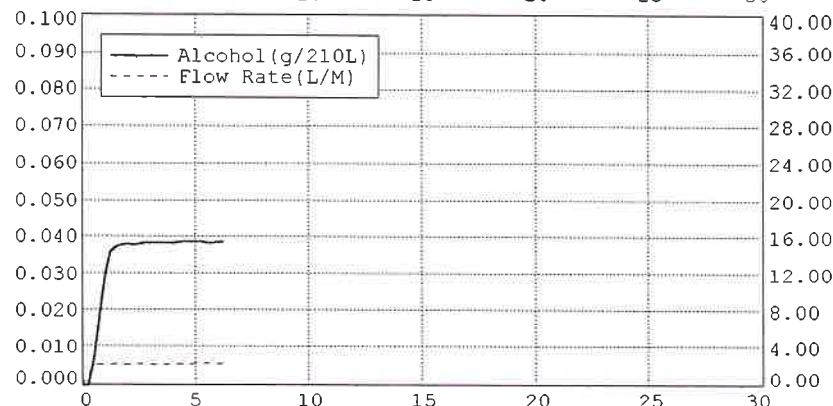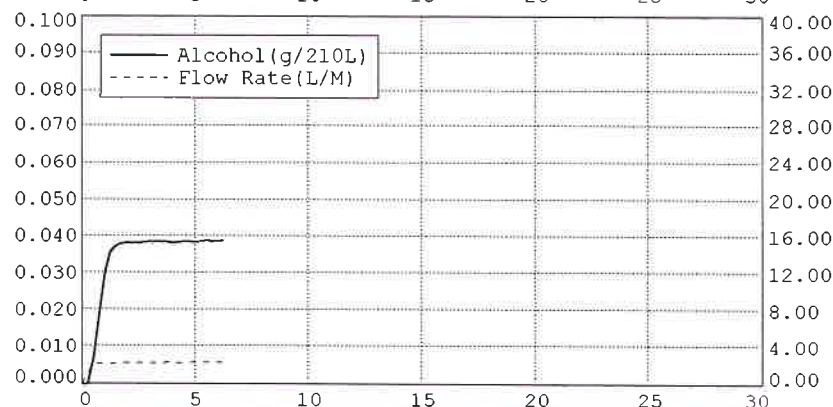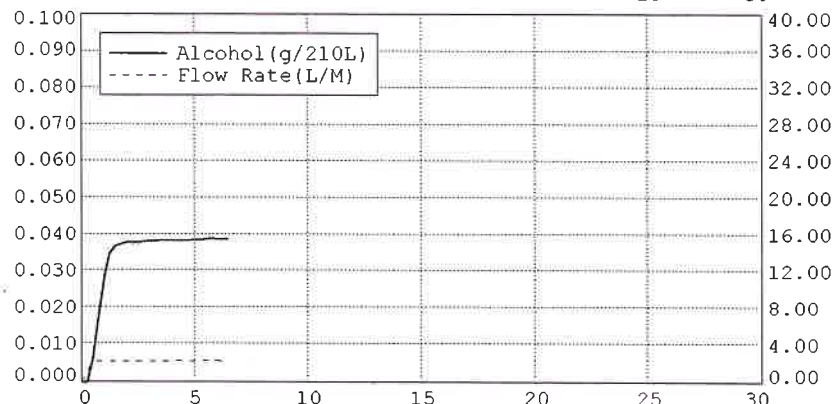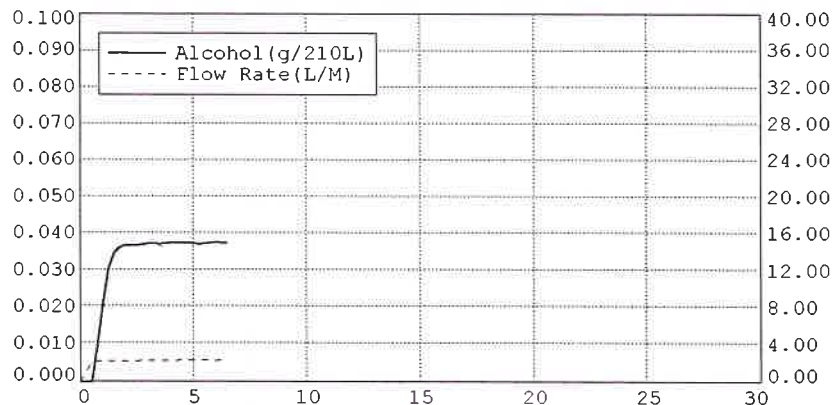

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100414






Date: 07/21/2025
Time: 13:35:41

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.97: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 420 psi

BLANK TEST	0.000	13:37
INTERNAL STANDARD	VERIFIED	13:37
EXTERNAL STANDARD	0.079	13:37
BLANK TEST	0.000	13:38
EXTERNAL STANDARD	0.079	13:39
BLANK TEST	0.000	13:39
EXTERNAL STANDARD	0.079	13:40
BLANK TEST	0.000	13:41
EXTERNAL STANDARD	0.079	13:41
BLANK TEST	0.000	13:42
EXTERNAL STANDARD	0.079	13:42
BLANK TEST	0.000	13:43

Average = 0.0790
Std Dev = 0.0000

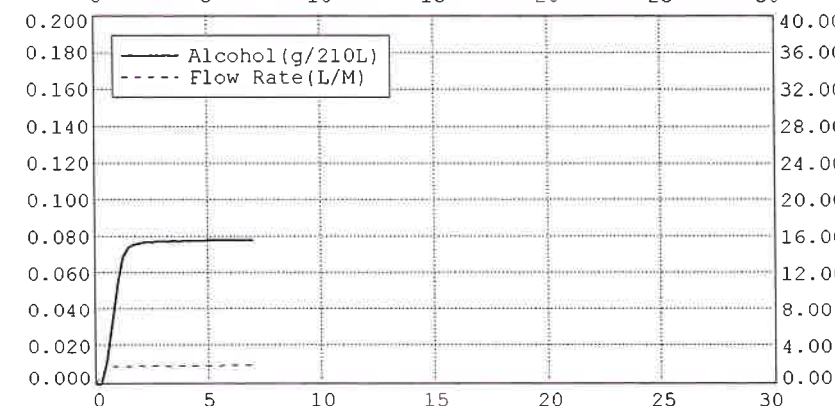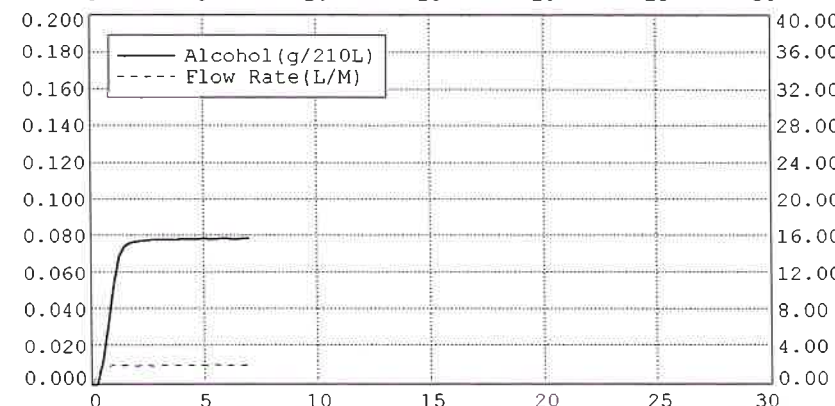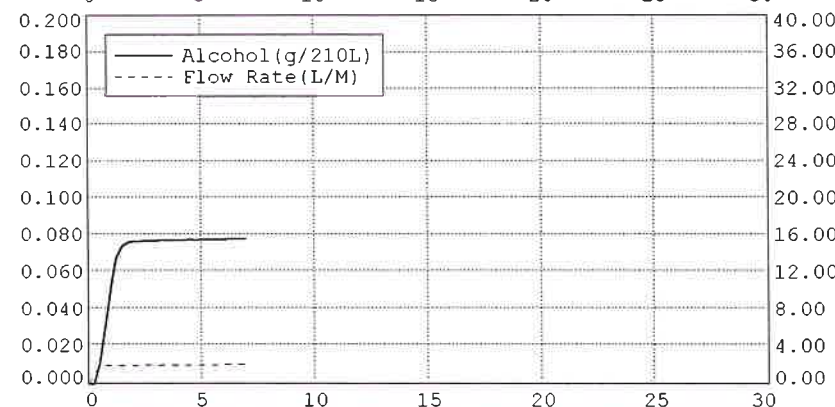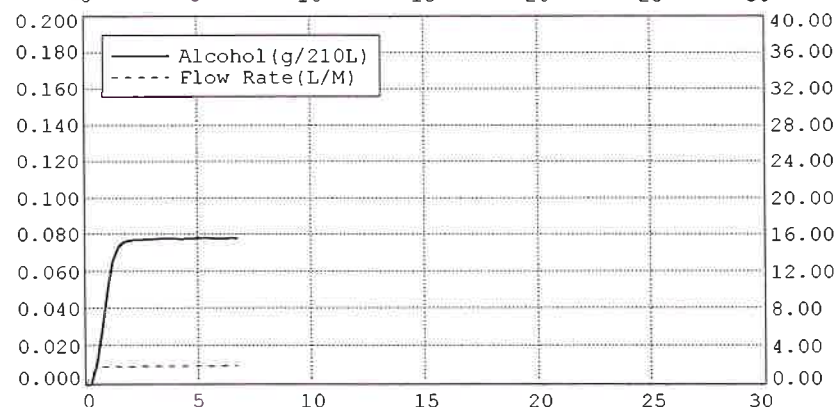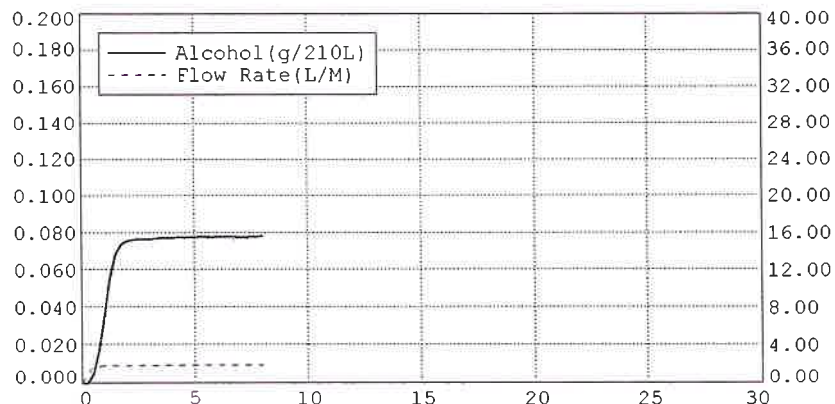

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100414






Date: 07/21/2025
Time: 13:44:26

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.97: 0.100
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 863 psi

BLANK TEST	0.000	13:45
INTERNAL STANDARD	VERIFIED	13:45
EXTERNAL STANDARD	0.100	13:46
BLANK TEST	0.000	13:46
EXTERNAL STANDARD	0.100	13:47
BLANK TEST	0.000	13:48
EXTERNAL STANDARD	0.101	13:48
BLANK TEST	0.000	13:49
EXTERNAL STANDARD	0.101	13:49
BLANK TEST	0.000	13:50
EXTERNAL STANDARD	0.100	13:50
BLANK TEST	0.000	13:51

Average = 0.1004
Std Dev = 0.0005

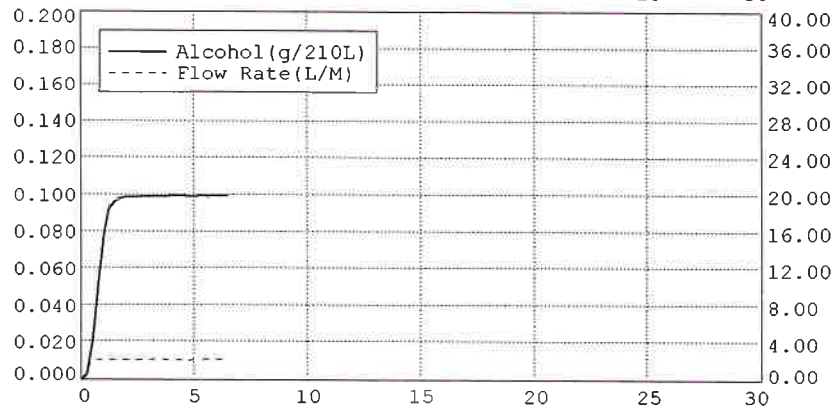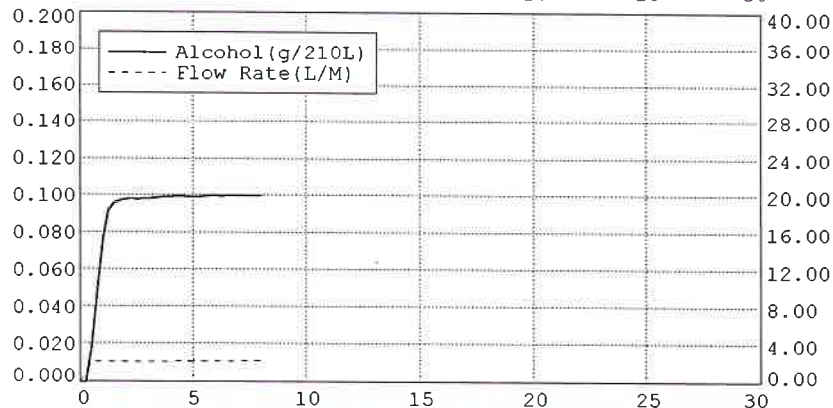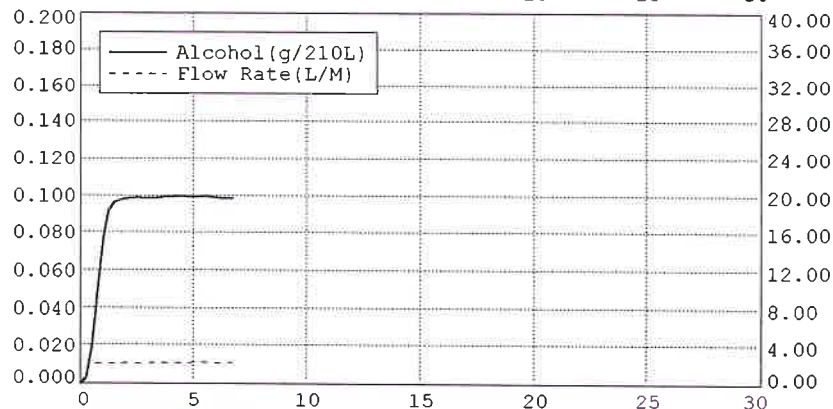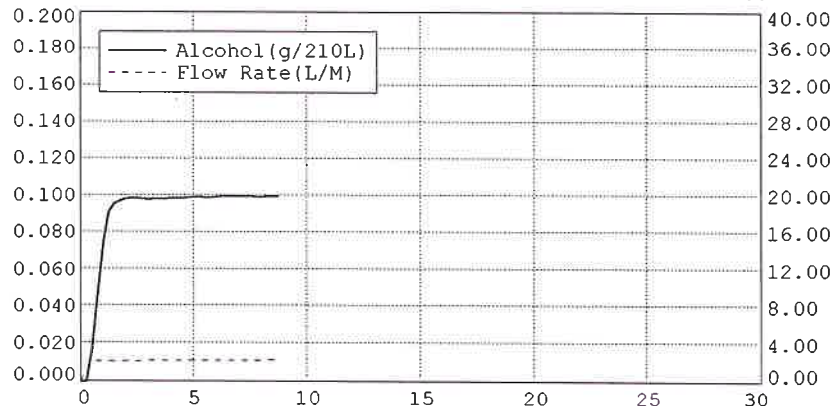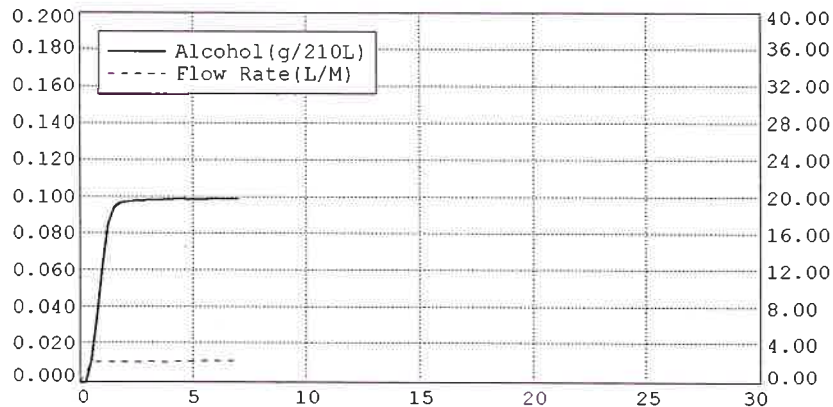

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100414






Date: 07/21/2025
Time: 13:55:13

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.97: 0.150
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 451 psi

BLANK TEST	0.000	13:56
INTERNAL STANDARD	VERIFIED	13:56
EXTERNAL STANDARD	0.147	13:57
BLANK TEST	0.000	13:58
EXTERNAL STANDARD	0.148	13:58
BLANK TEST	0.000	13:59
EXTERNAL STANDARD	0.148	13:59
BLANK TEST	0.000	14:00
EXTERNAL STANDARD	0.148	14:00
BLANK TEST	0.000	14:01
EXTERNAL STANDARD	0.148	14:01
BLANK TEST	0.000	14:02

Average = 0.1478
Std Dev = 0.0004

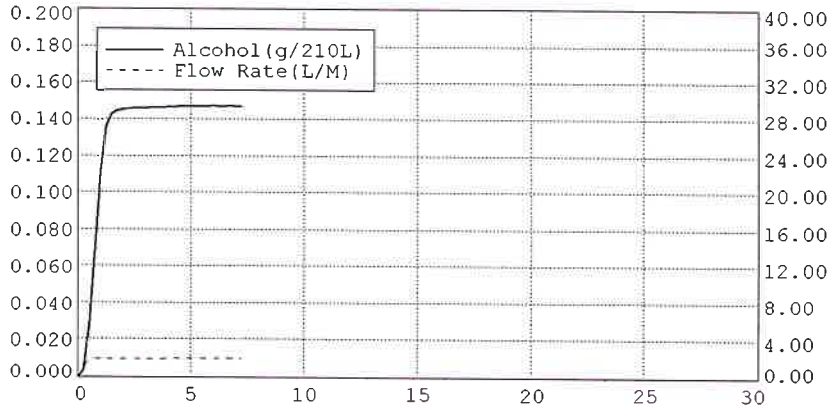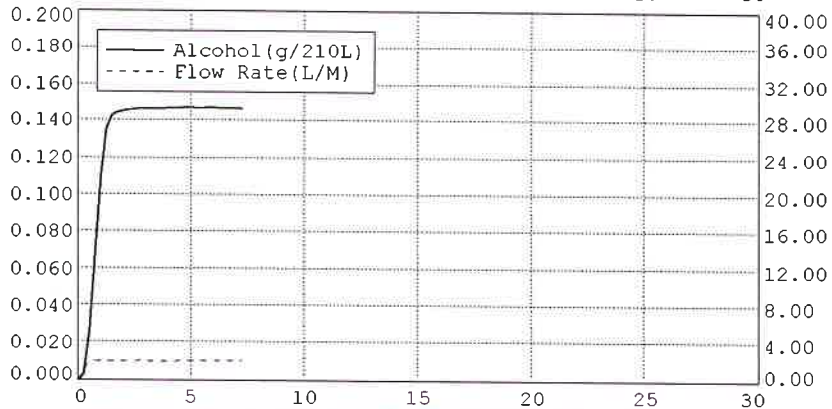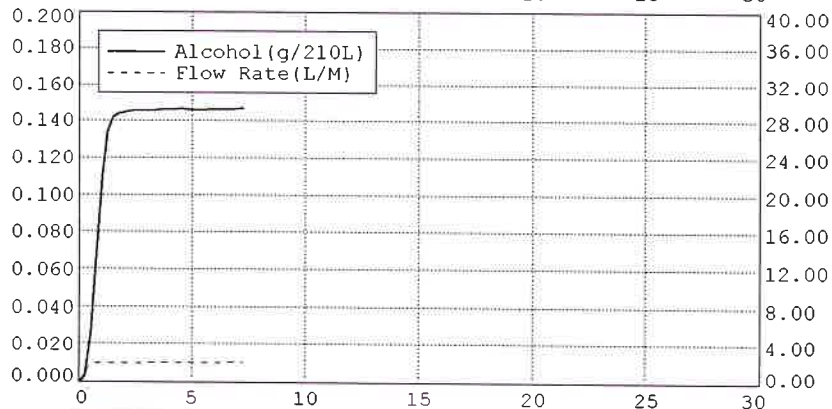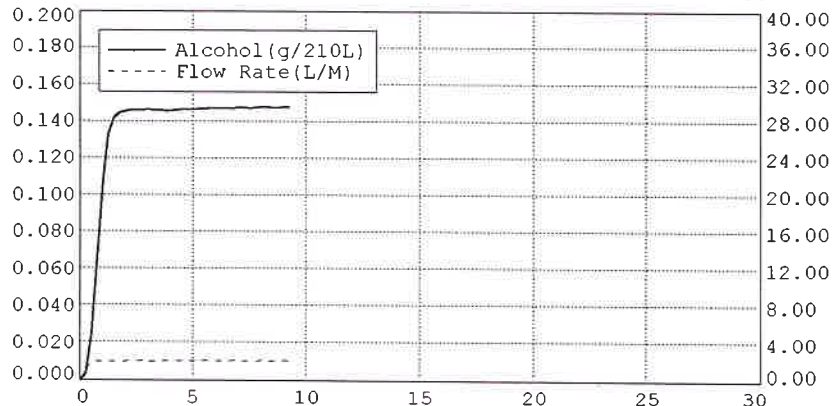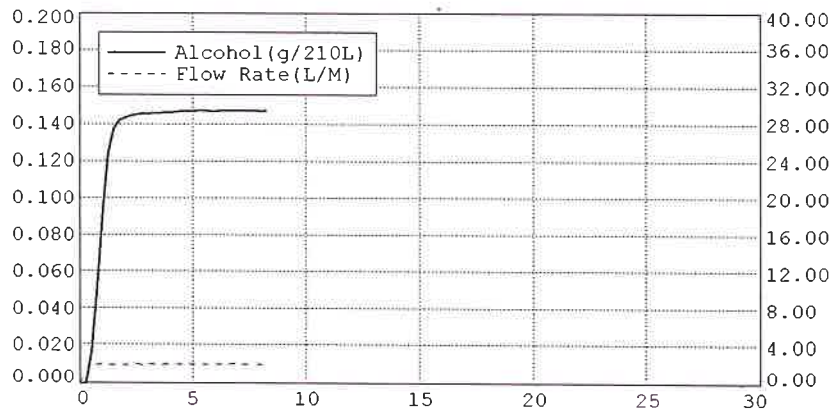

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100414






Date: 07/21/2025
Time: 14:05:15

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.97: 0.300
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 141 psi

BLANK TEST	0.000	14:06
INTERNAL STANDARD	VERIFIED	14:06
EXTERNAL STANDARD	0.300	14:06
BLANK TEST	0.000	14:07
EXTERNAL STANDARD	0.298	14:08
BLANK TEST	0.000	14:08
EXTERNAL STANDARD	0.299	14:09
BLANK TEST	0.000	14:10
EXTERNAL STANDARD	0.298	14:10
BLANK TEST	0.000	14:11
EXTERNAL STANDARD	0.299	14:11
BLANK TEST	0.000	14:12

Average = 0.2988
Std Dev = 0.0008

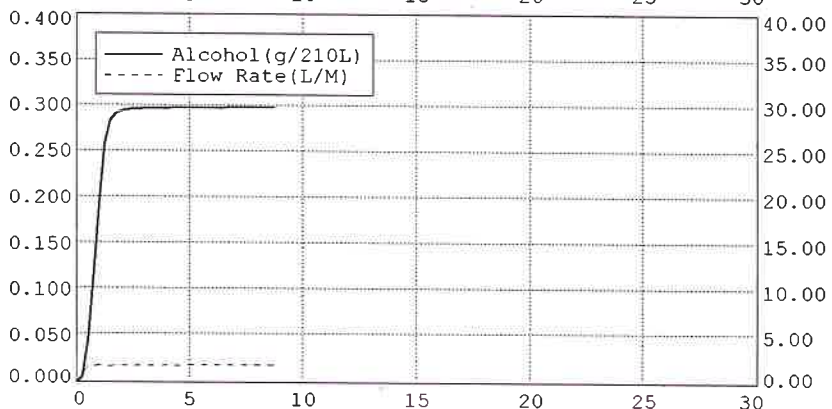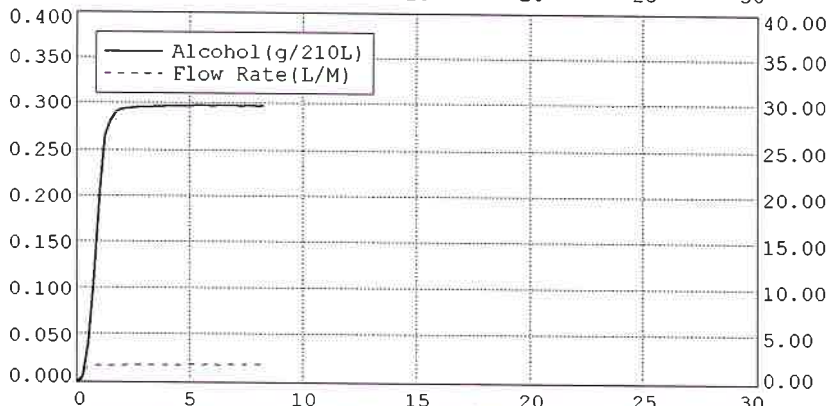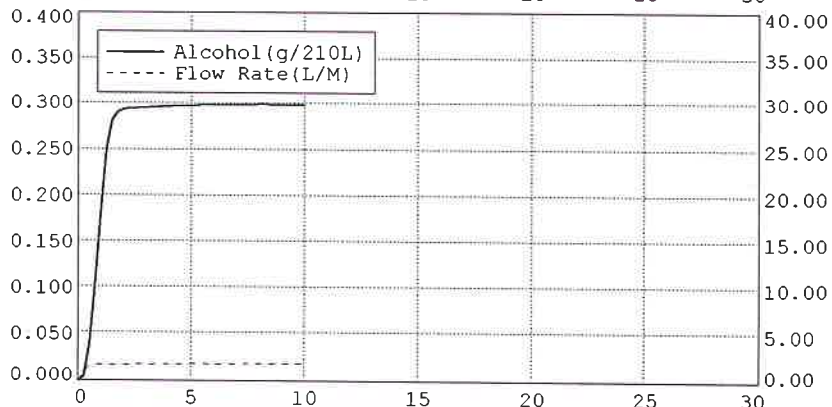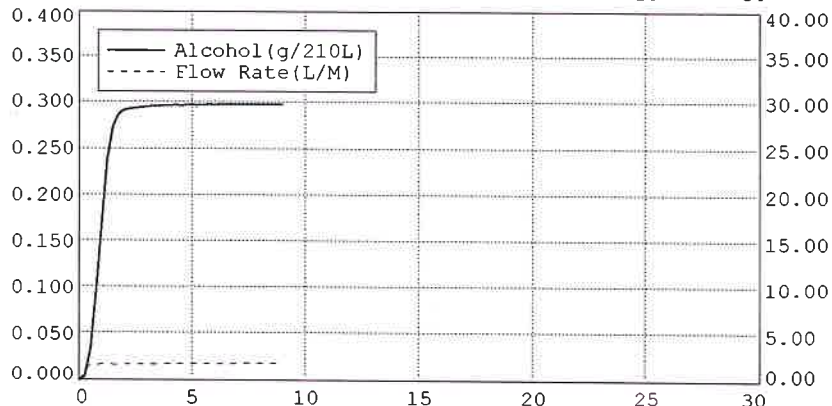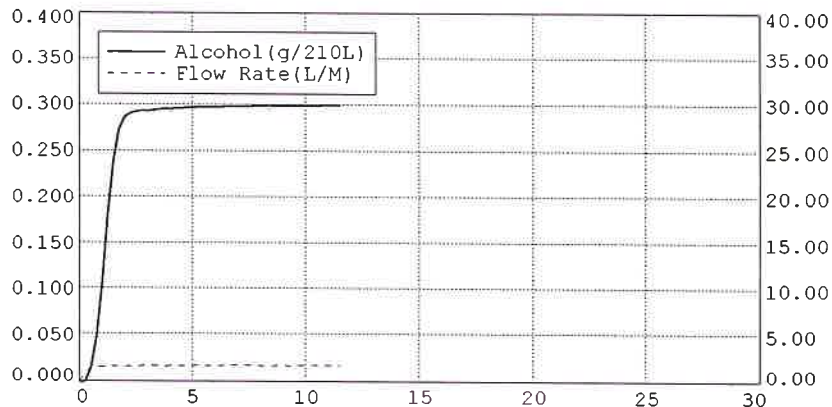

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/21/2025
Time: 14:17:51

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.97: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:18
BLANK TEST	0.000	14:19
INTERNAL STANDARD	VERIFIED	14:19
EXTERNAL STANDARD	INTERFERENCE	14:19

Interference Detected

[Handwritten signature]

Interference Detected status message was not repeated in any other testing for this Calibration. DJW 07/24/2025

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/21/2025
Time: 14:25:17

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.97: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:26
BLANK TEST	0.000	14:26
INTERNAL STANDARD	VERIFIED	14:26
EXTERNAL STANDARD	0.079	14:26
BLANK TEST	0.000	14:27
SUBJECT SAMPLE	INCOMPLETE	14:29

DM

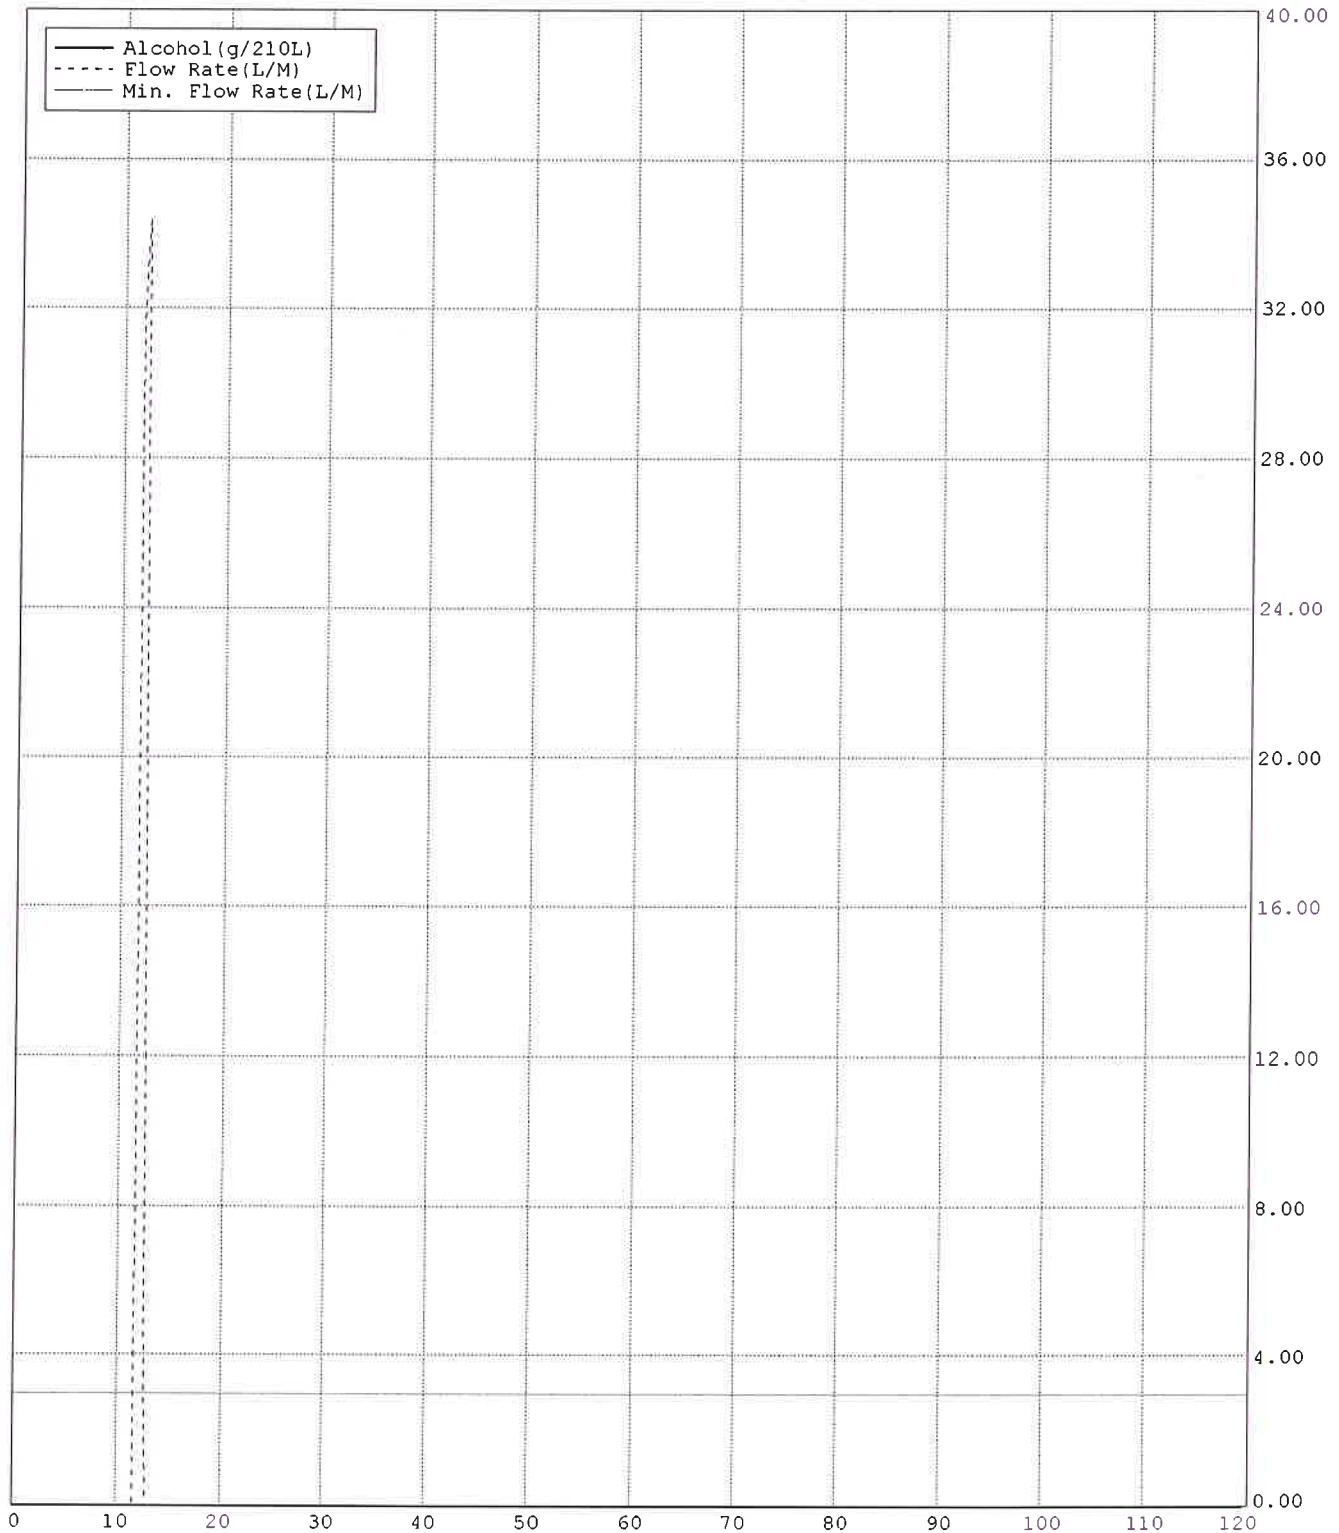

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/21/2025
Time: 14:31:34

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508


DEPT/AGENCY:
MAXIMUM ATTEMPTS
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.97: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:32
BLANK TEST	0.000	14:32
INTERNAL STANDARD	VERIFIED	14:32
EXTERNAL STANDARD	0.079	14:33
BLANK TEST	0.000	14:33
SUBJECT SAMPLE	XXX	14:34

Maximum Attempts Exceeded

[Handwritten signature]

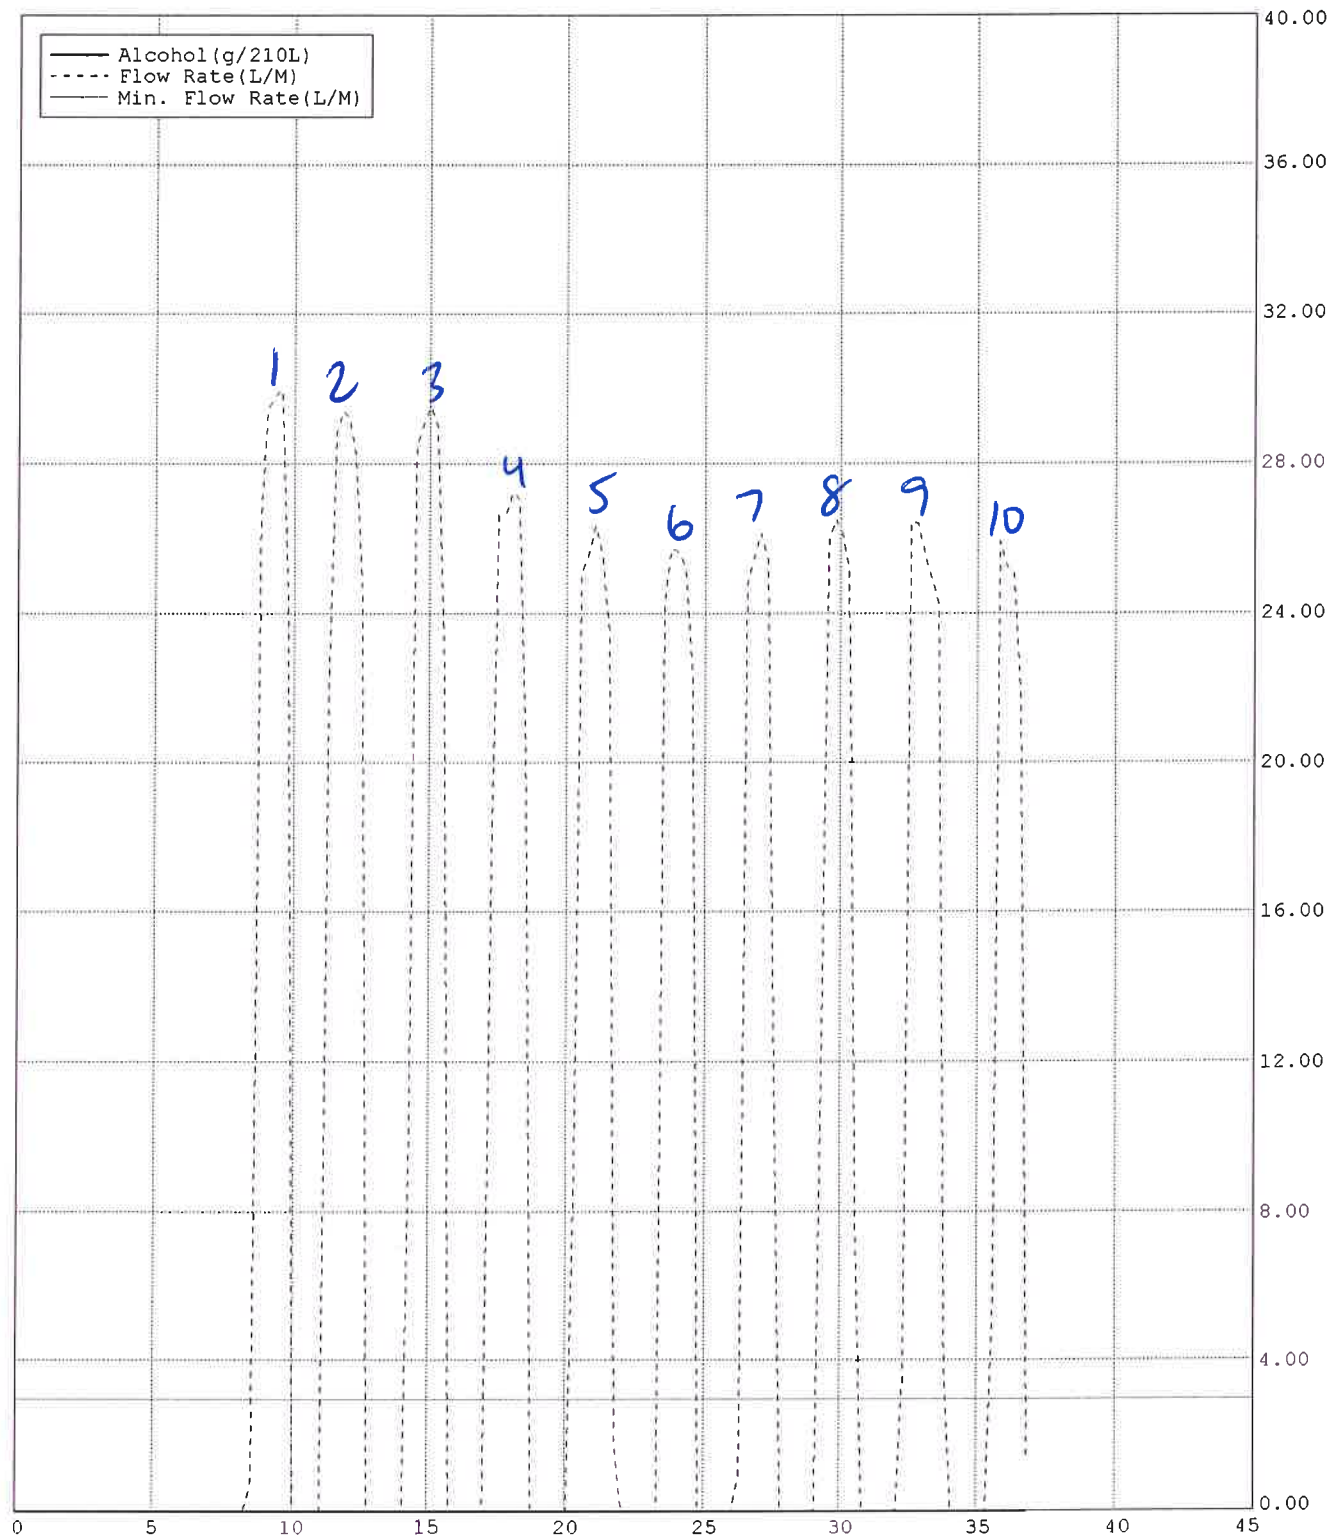

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/21/2025
Time: 14:37:07

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

DEPT/AGENCY:
INVALID
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.96: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:43
BLANK TEST	0.000	14:43
INTERNAL STANDARD	VERIFIED	14:43
EXTERNAL STANDARD	0.080	14:43
BLANK TEST	0.000	14:44
SUBJECT SAMPLE	INVALID	14:45

DWV

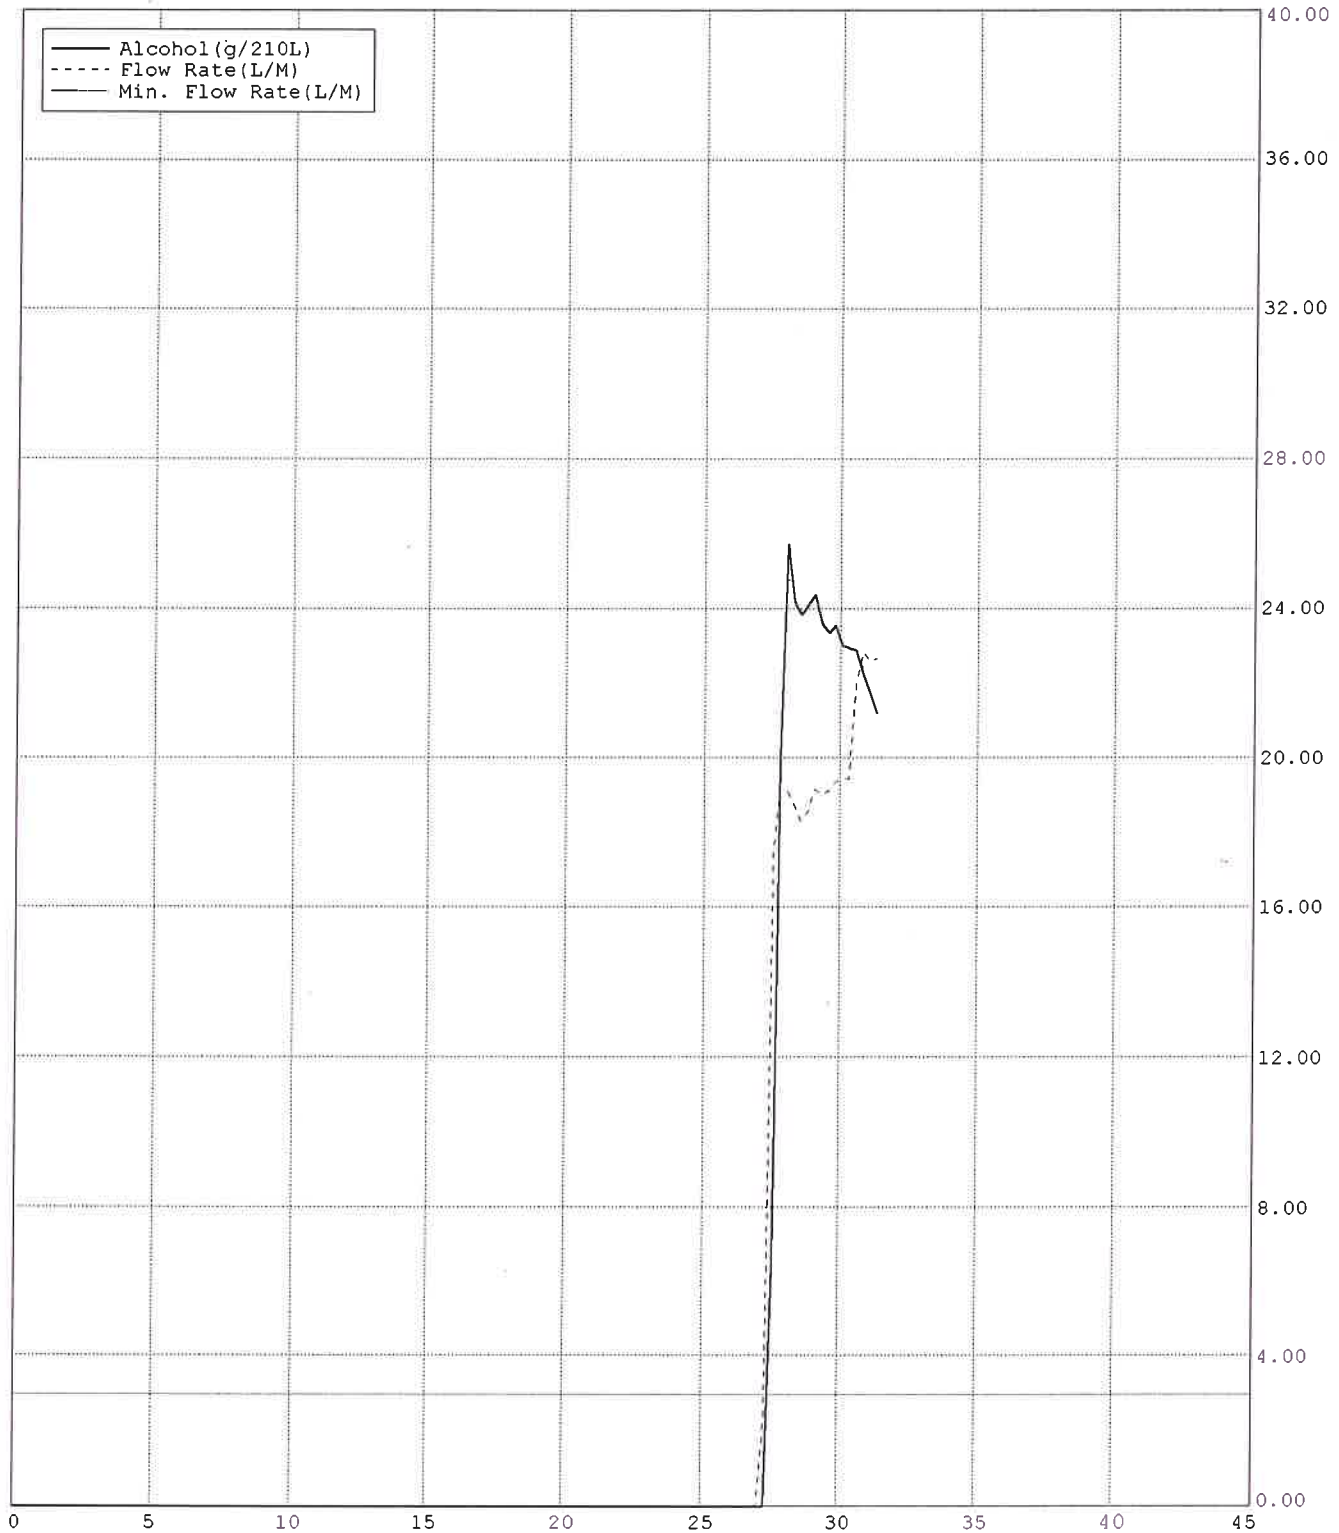

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/21/2025
Time: 14:51:16

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508


DEPT/AGENCY:
RADIO FREQUENCY
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.96: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:52
BLANK TEST	0.000	14:52
INTERNAL STANDARD	VERIFIED	14:53
EXTERNAL STANDARD	0.078	14:53
BLANK TEST	0.000	14:54

RFI DETECTED

WLF

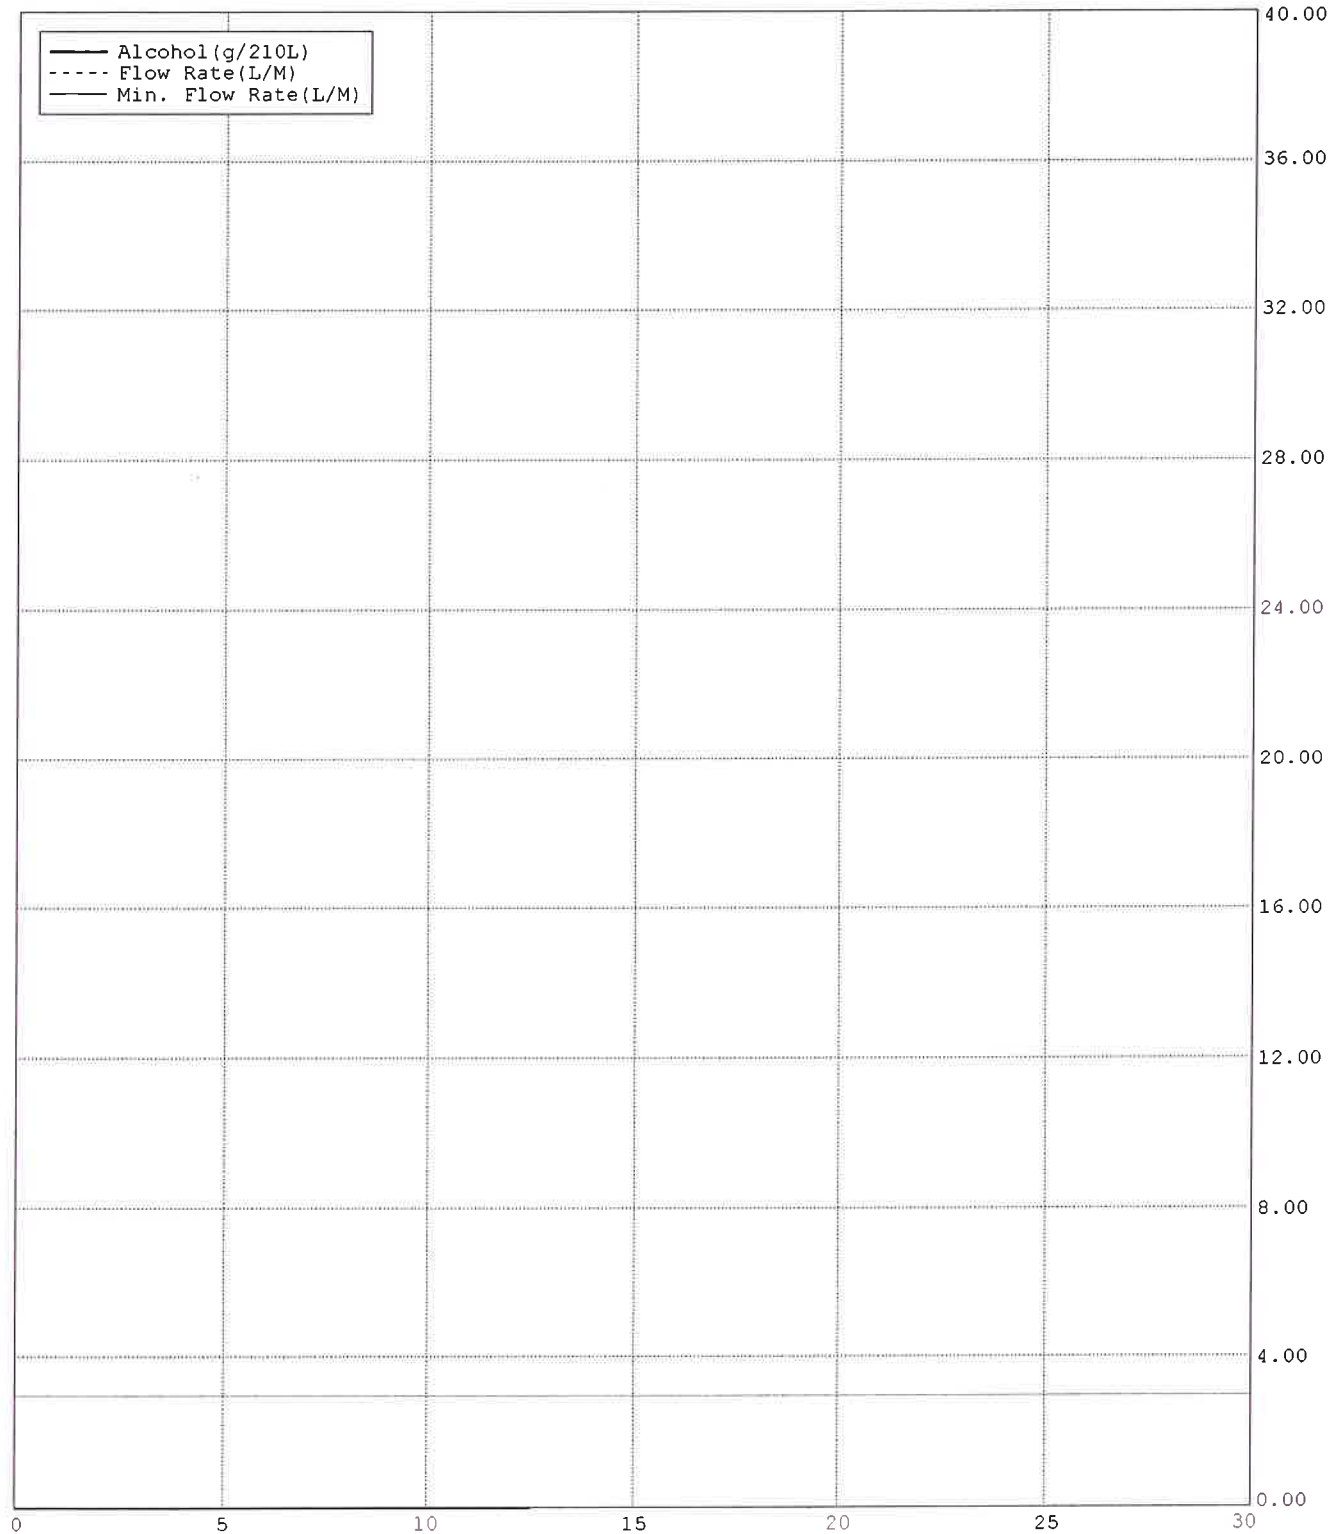

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/21/2025
Time: 15:16:26

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

DEPT/AGENCY:
INTERFERENCE ACETONE
CASE/REPORT: XXXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.96: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	15:17
BLANK TEST	0.000	15:17
INTERNAL STANDARD	VERIFIED	15:17
Xq = 0.090 (3.01%)		
EXTERNAL STANDARD	0.079	15:17
X[1] = 0.0786 (0.0006) (0.0023)		
BLANK TEST	0.000	15:18
SUBJECT SAMPLE	XXX	15:19
X[1] = 0.1080 (-0.0182) (0.0018)		

Interference Detected

Filter 2 average: 0.0011
Filter 3 average: 0.0024
DJW 07/24/2025

[Handwritten signature]

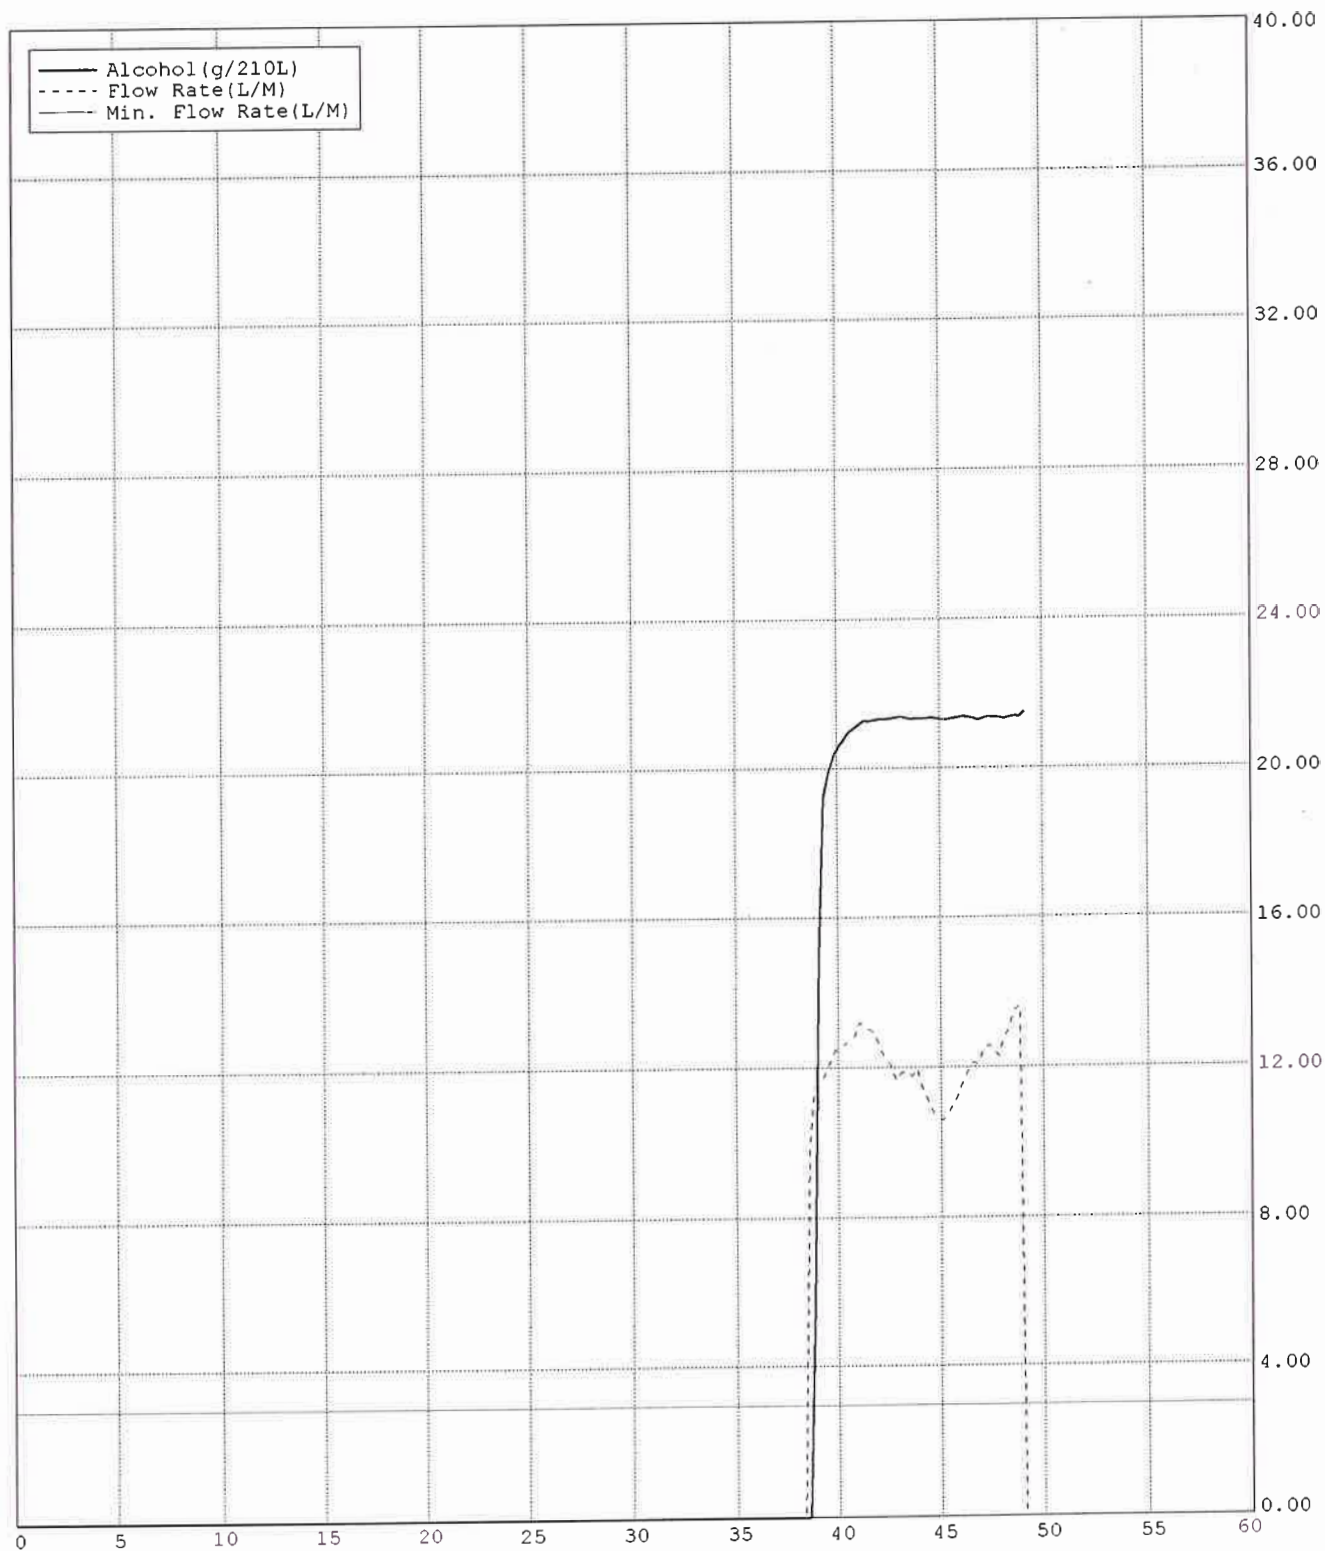

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/21/2025
Time: 15:09:39

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

DEPT/AGENCY:
INTERFERENCE ISOPROPANOL
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.96: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	15:11
BLANK TEST	0.000	15:12
INTERNAL STANDARD	VERIFIED	15:12
Xq = 0.092 (0.85%)		
EXTERNAL STANDARD	0.079	15:12
X[1] = 0.0785 (0.0008) (0.0017)		
BLANK TEST	0.000	15:13
SUBJECT SAMPLE	XXX	15:13
X[1] = 0.1196 (-0.0201) (0.0024)		

Interference Detected

DMW



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/21/2025
Time: 15:22:01

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

DEPT/AGENCY:
INTERFERENCE NEGATIVE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.96: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	15:23
BLANK TEST	0.000	15:23
INTERNAL STANDARD	VERIFIED	15:23
Xq = 0.092 (0.66%)		
EXTERNAL STANDARD	0.079	15:23
X[1] = 0.0787 (0.0010) (0.0024)		
BLANK TEST	0.000	15:24
SUBJECT SAMPLE (Vol=2.18L)	0.090	15:25
X[1] = 0.0909 (0.0013) (0.0015)		
BLANK TEST	0.000	15:26
EXTERNAL STANDARD	0.079	15:26
X[1] = 0.0791 (0.0018) (0.0032)		
BLANK TEST	0.000	15:27

DW

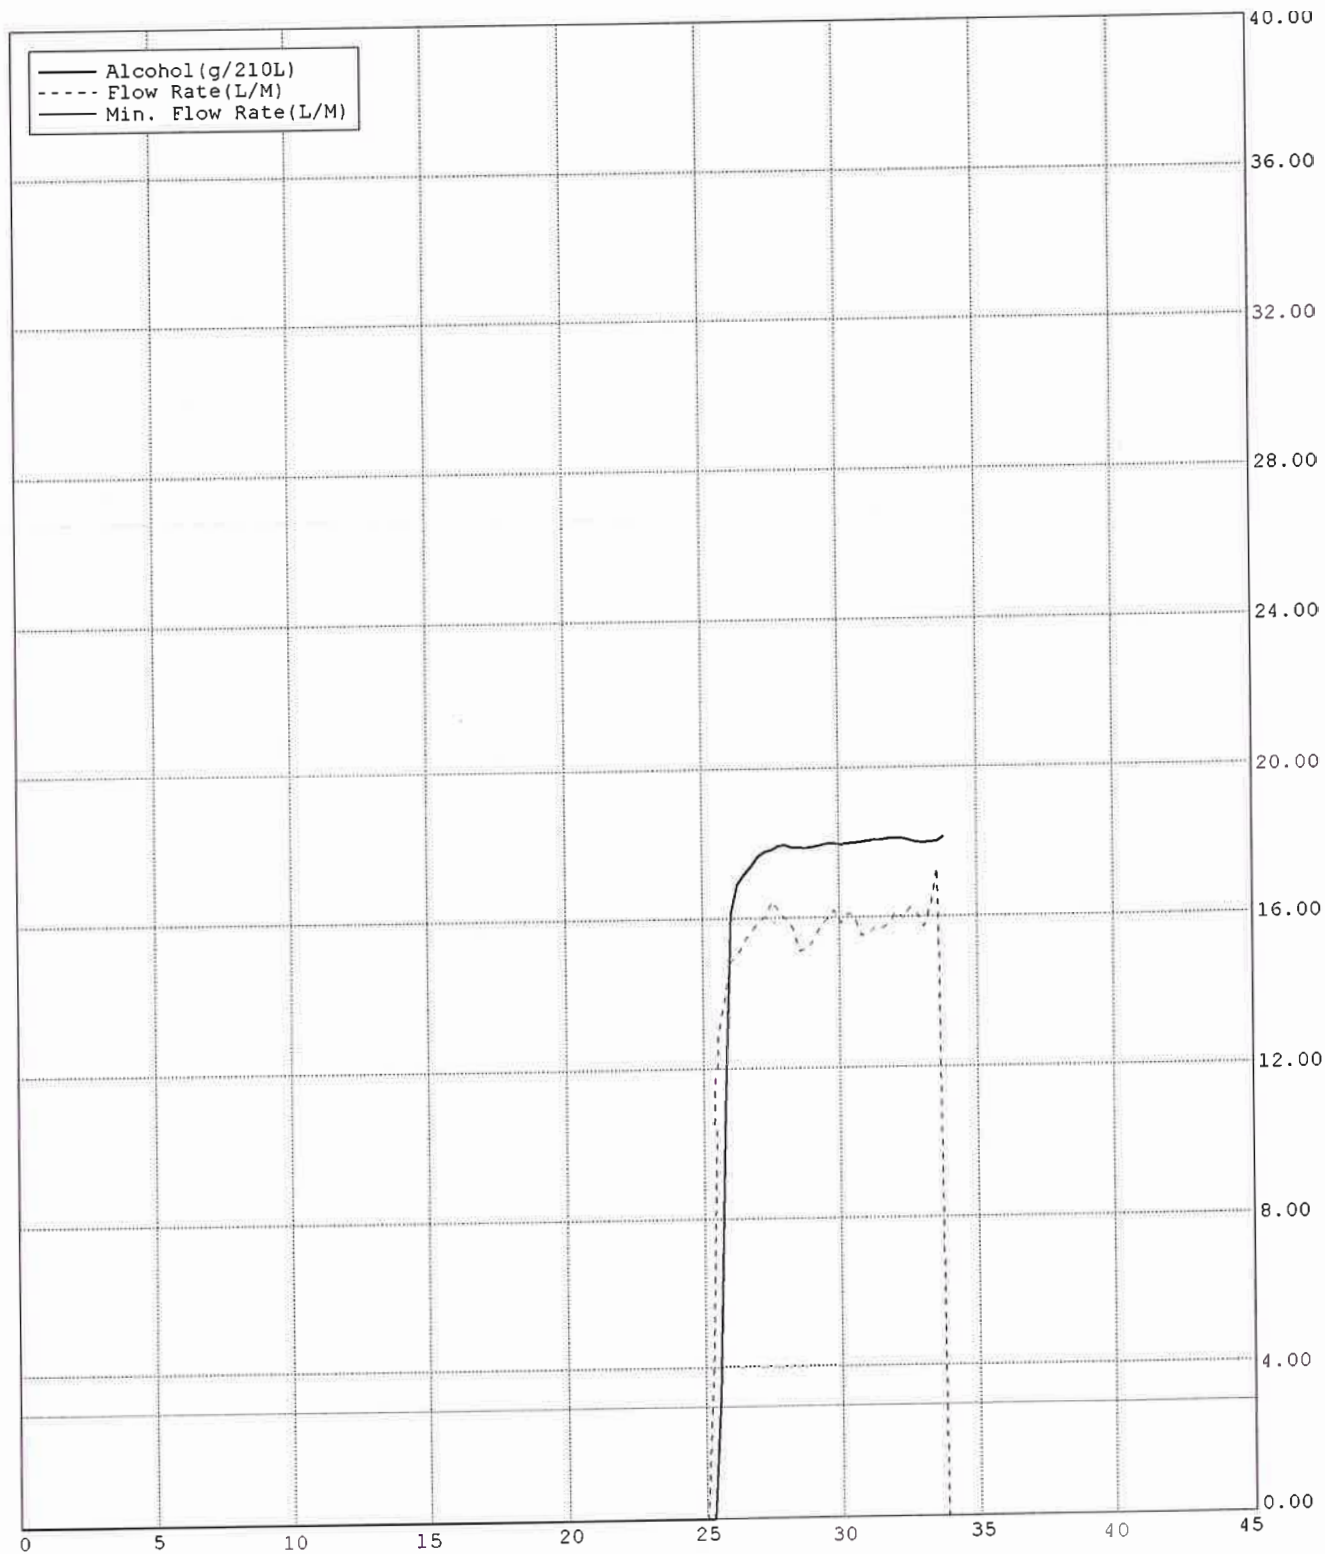

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100414

Date: 07/21/2025
Time: 16:03:19

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

DEPT/AGENCY:
NON-DRINKING SUBJECT
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.95: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	16:05
BLANK TEST	0.000	16:05
INTERNAL STANDARD	VERIFIED	16:05
EXTERNAL STANDARD	0.079	16:05
BLANK TEST	0.000	16:06
SUBJECT SAMPLE (Vol=5.56L)	0.000	16:07
BLANK TEST	0.000	16:08
EXTERNAL STANDARD	0.080	16:08
BLANK TEST	0.000	16:09

DMW

