



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100682

Report Issue Date: 12/07/2023
Date Received: 2023-10-23
Condition of Item: Good

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

Start Date 11/06/2023 - As Found - **End Date 11/06/2023** As Found - Evaluation Analyst: Carlie Glaister
 As Found Conditions - Barometric Pressure (inHg): 29.13 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.3
 Relative Humidity (%): 23

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.019	AG217902	0.018	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.078	AG135004	0.077	0.077	0.078	0.077	0.078	0.077	0.077
0.300	0.291	AG217903	0.297	0.295	0.295	0.296	0.296	0.296	0.296

Cleared memory & reset options before eval. Sheared off screw when attempting to remove.

Start Date 11/30/2023 - As Left - **End Date 12/04/2023**

As Left Conditions - Barometric Pressure (inHg): 28.83 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.3 Relative Humidity (%): 19

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.019	AG217902	0.019	0.019	0.019	0.019	0.019	0.019	+/- 0.002	
0.040	0.039	AG217904	0.038	0.039	0.039	0.039	0.039	0.039	+/- 0.003	
0.080	0.077	AG135004	0.077	0.077	0.077	0.077	0.077	0.077	+/- 0.004	
0.100	0.096	AG211003	0.097	0.097	0.097	0.097	0.097	0.097	+/- 0.004	
0.150	0.145	AG134205	0.146	0.146	0.146	0.146	0.146	0.146	+/- 0.005	
0.300	0.289	AG217903	0.294	0.293	0.293	0.293	0.293	0.293	+/- 0.011	

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Carlie Glaister on 12/04/2023

carlie.glaister@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 12/07/2023

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100682 Analyst: Carlie Haister Start Date: 11/30/23

- Diagnostic Test (attached)
- Adjust voltages, if needed
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
- Internal Standard value \leq 3.00%
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.5 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 28.83 Temperature (C): 22.3 Relative Humidity (%) 19

Linearity Test (attached)

0.020g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217902</u>	Exp: <u>6/28/24</u>
0.040g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217904</u>	Exp: <u>6/28/24</u>
0.080g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-135004</u>	Exp: <u>12/16/23</u>
0.100g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-211003</u>	Exp: <u>4/20/24</u>
0.150g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-134205</u>	Exp: <u>12/8/23</u>
0.300g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217903</u>	Exp: <u>6/28/24</u>

Functional Tests (attached)

- Incomplete
- Maximum Attempts Exceeded
- Interference (Volatiles)
- Invalid
- Radio Frequency Interference (RFI)

Acetone Mnf: Lifelog Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR4176 Verification Performed?

Isopropanol Mnf: Lifelog Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR4177 Verification Performed?

Neg. Control Mnf: Lifelog Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR6267 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 230631104 Calibration Due Date: 9/19/2025

- Verify stylus is calibrated
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Non-Drinking Subject Test
- Upload
- Remove Tank Prior to Shutdown

Calibration End Date: 12/1/23

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 11/30/2023
Time: 10:39:43

VERSIONS

DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 2.40 V PASSED
(1.44 V - 3.36 V)
Cooler Voltage = 1.99 V PASSED
(1.19 V - 2.79 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 530 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 28.8 in

PUMP INFO

Flow Rate = 4.602 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.001 V <= 0.010 V)
PUMP OFF PASSED
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.100 2.31% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100682

Date: 11/30/2023
Time: 11:44 AM

Temperatures (°C)

Sample Cell: 48.9°C
Breath Tube: 47.8°C

Current Barometer 28.8 in
Volume (Ltr) 1.55

Settings

Lamp: 2.40 V
Bias: 80 V
Cooler: 1.91 V
Chopper: 530 Hz

Voltages (V)

Flow: 1.04 V
Detector: -0.013 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 08/24/2023
Time: 08:46:03

OPERATOR NAME:
INTOX I METERS
CERTIFICATE #: INTOXIMETERS

Ca = 0.0800
CAL = 0.984724 0.800 <= CAL < 1.200
b1 = 0.0009 0.0000 <= b1 < 0.0040
b2 = 0.0050 0.0010 <= b2 < 0.0100
b3 = 0.0007 0.0000 <= b3 < 0.0040
Xq = 0.1024 0.0500 <= Xq < 0.2000
a21 = 1.122631 1.050 <= a21 < 1.300
a31 = 0.444709 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 11/30/2023
Time: 12:28:11

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.83: 0.077
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	12:29
BLANK TEST	0.000	12:29
INTERNAL STANDARD	VERIFIED	12:29
EXTERNAL STANDARD	0.077	12:29
BLANK TEST	0.000	12:30
SUBJECT SAMPLE (Vol=1.51L)	0.000	12:31
BLANK TEST	0.000	12:32
EXTERNAL STANDARD	0.077	12:32
BLANK TEST	0.000	12:33

CKG

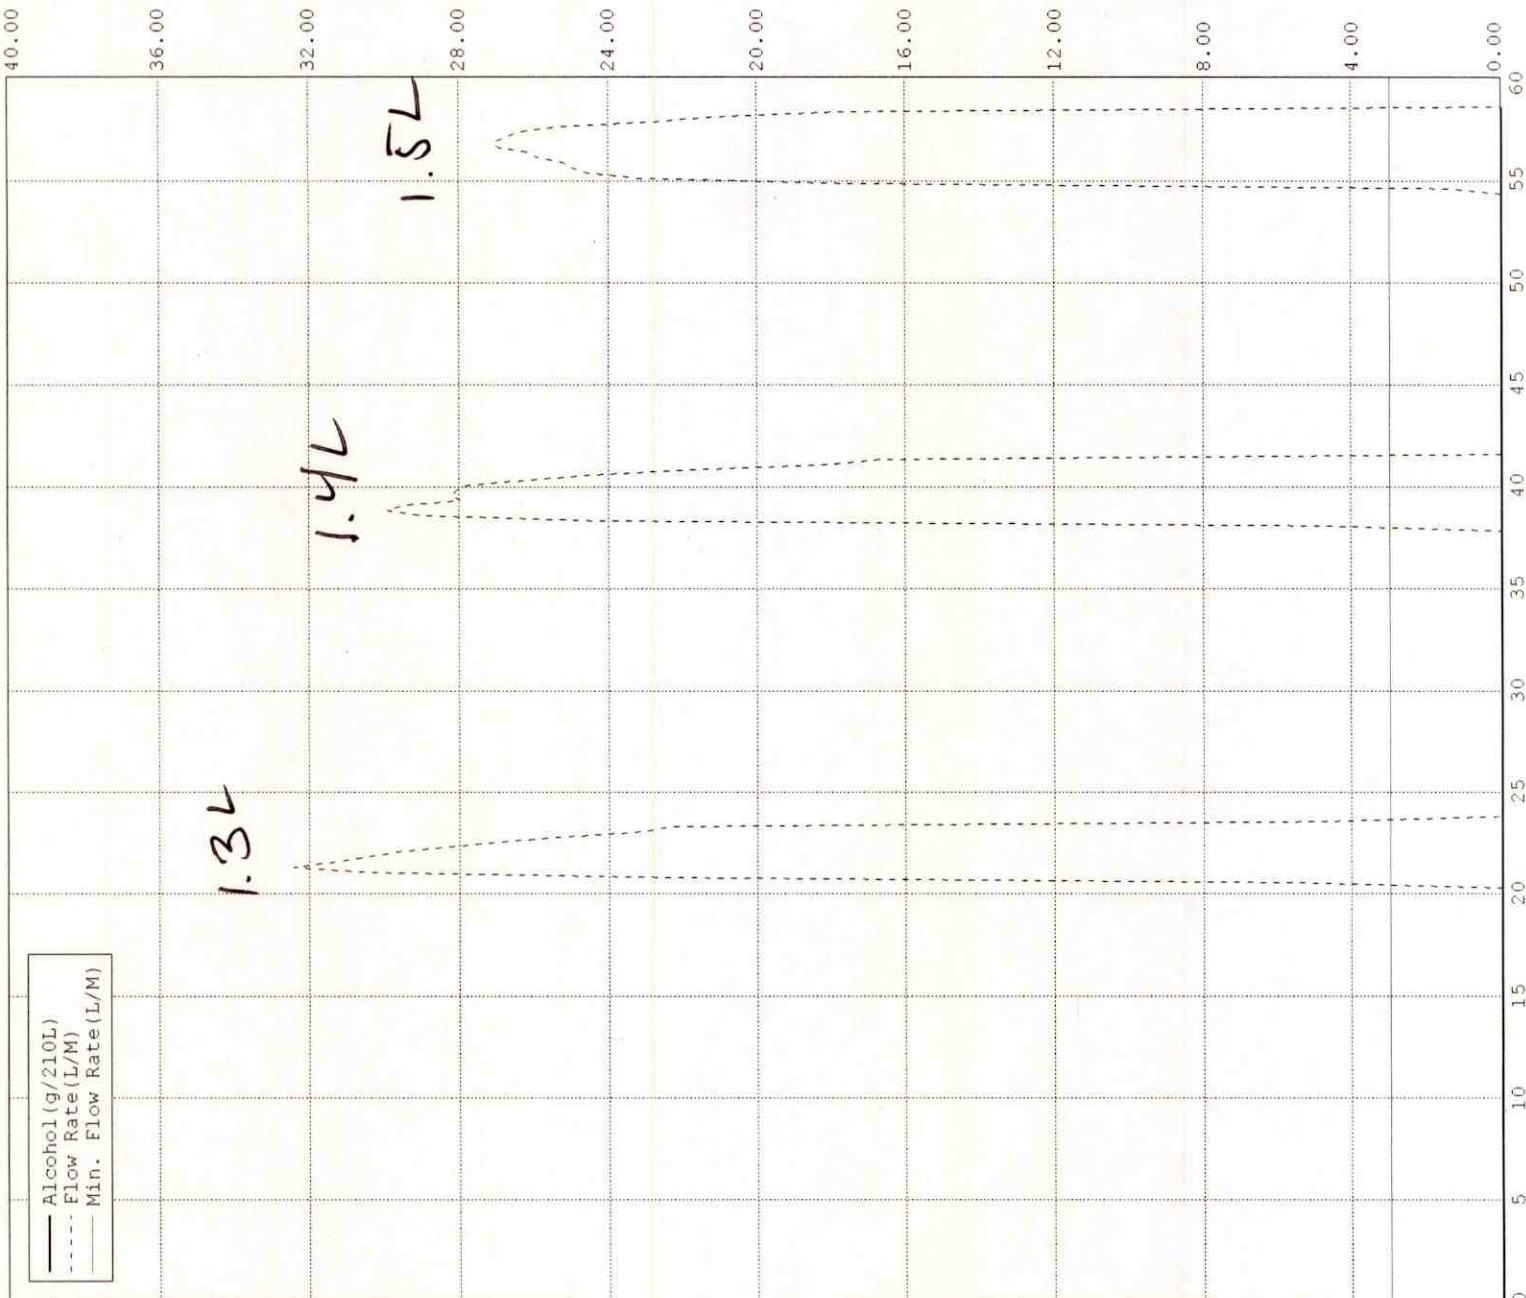

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100682

Date: 11/30/2023
 Time: 13:03:51

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.019	0.0190	0.0000
0.039	0.0388	0.0004
0.077	0.0770	0.0000
0.096	0.0970	0.0000
0.145	0.1460	0.0000
0.289	0.2932	0.0004

SLOPE = 1.016336
 R² = 0.999982

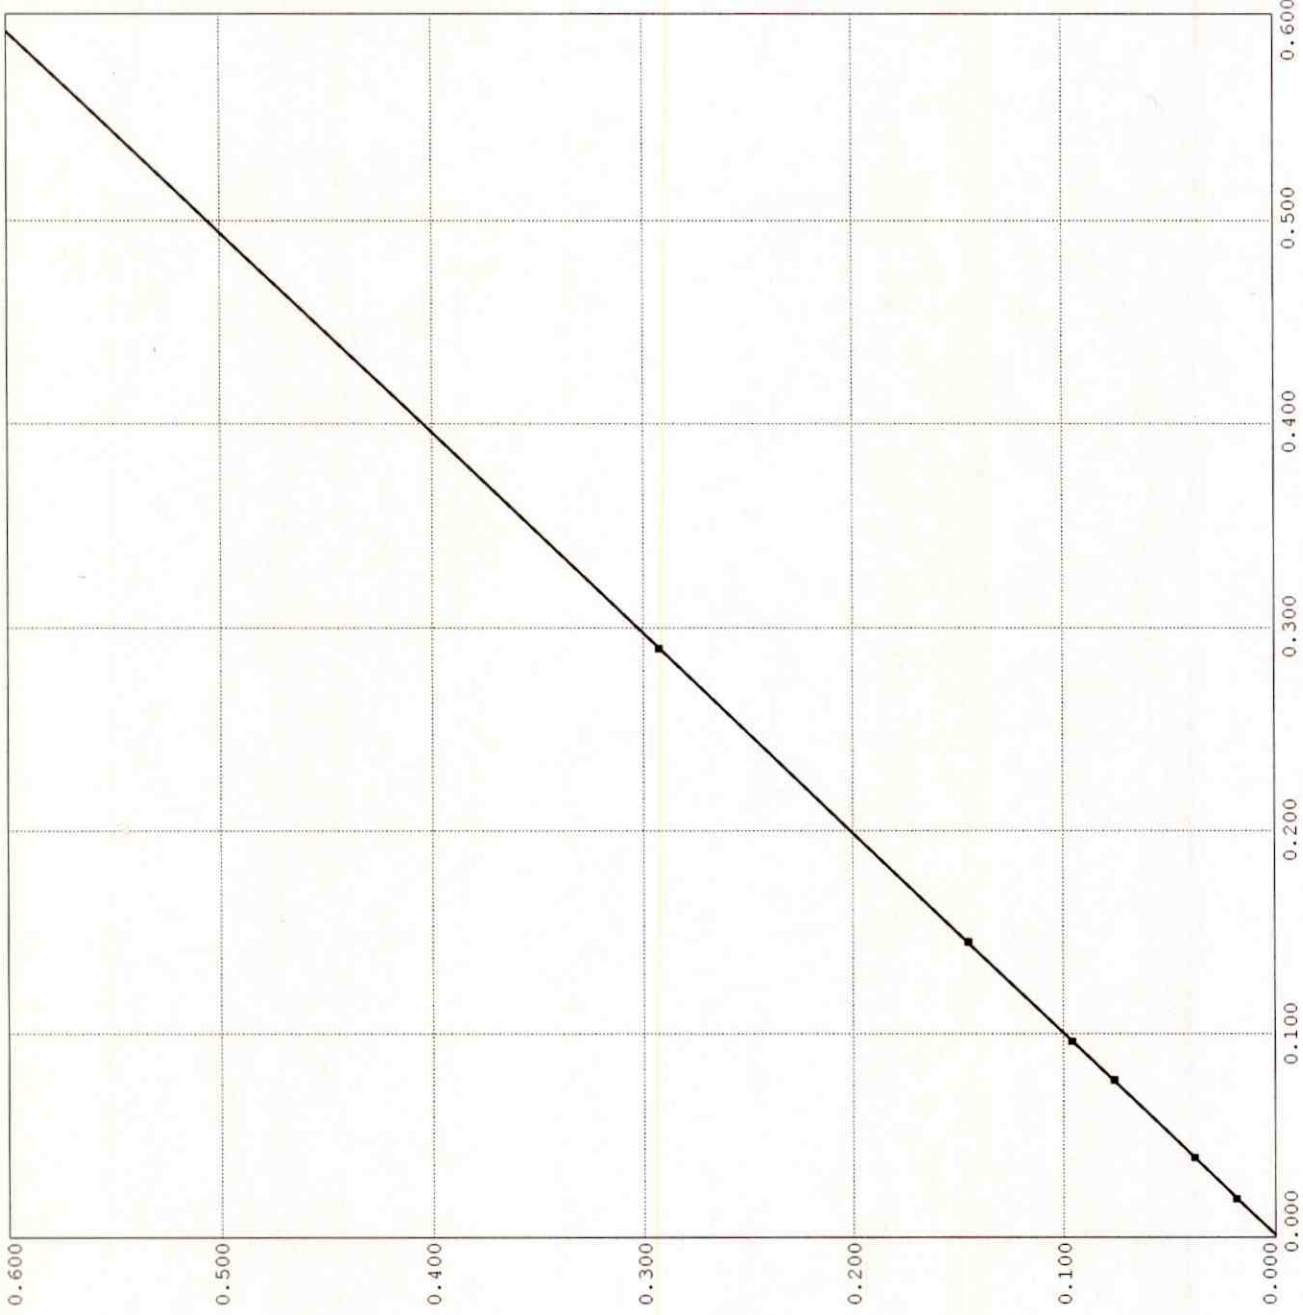

CKG

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100682






Date: 11/30/2023
Time: 13:03:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 28.83: 0.019
LOT #: AG217902
EXPIRATION: 06/28/2024
TANK PRESSURE: 720 psi

BLANK TEST	0.000	13:05
INTERNAL STANDARD	VERIFIED	13:05
EXTERNAL STANDARD	0.019	13:05
BLANK TEST	0.000	13:06
EXTERNAL STANDARD	0.019	13:06
BLANK TEST	0.000	13:07
EXTERNAL STANDARD	0.019	13:07
BLANK TEST	0.000	13:08
EXTERNAL STANDARD	0.019	13:09
BLANK TEST	0.000	13:09
EXTERNAL STANDARD	0.019	13:10
BLANK TEST	0.000	13:10

Average = 0.0190
Std Dev = 0.0000

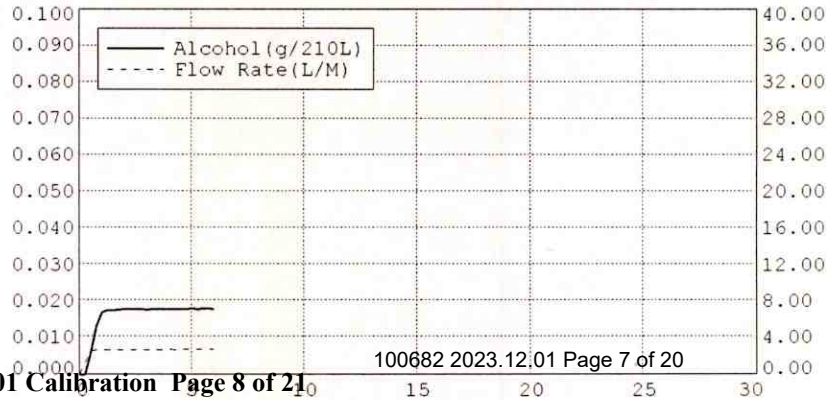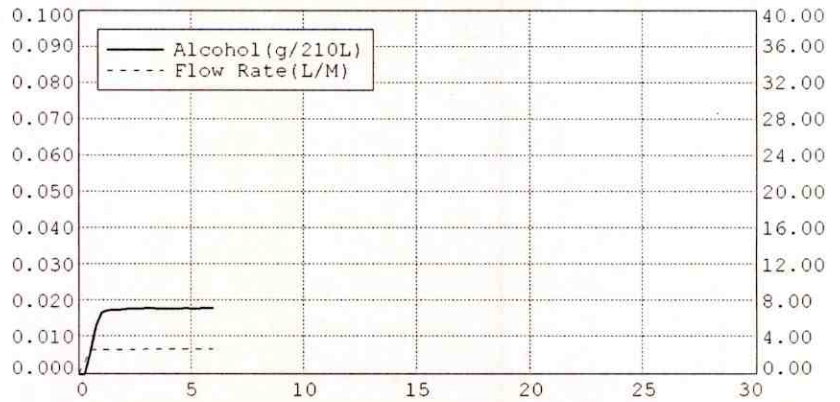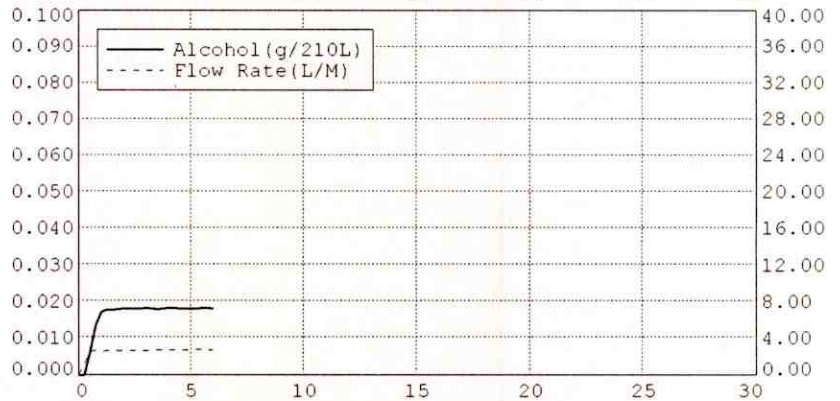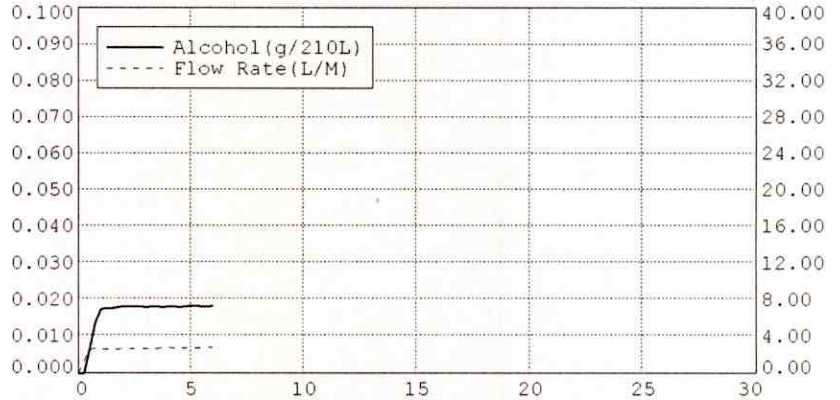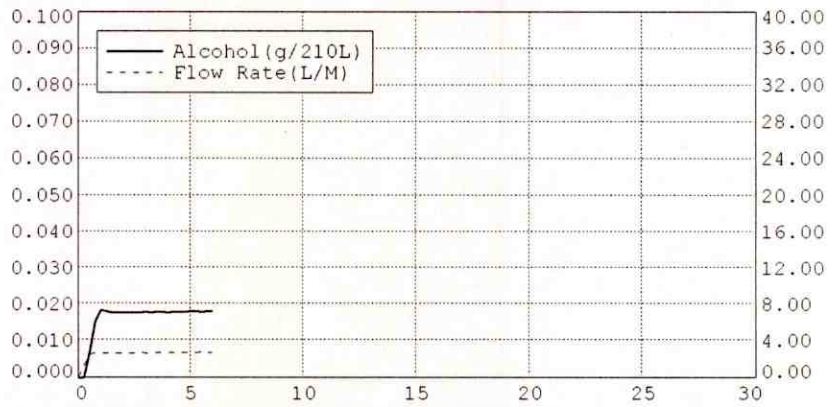

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100682






Date: 11/30/2023
 Time: 13:16:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 28.84: 0.039
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 924 psi

BLANK TEST	0.000	13:18
INTERNAL STANDARD	VERIFIED	13:18
EXTERNAL STANDARD	0.038	13:18
BLANK TEST	0.000	13:19
EXTERNAL STANDARD	0.039	13:19
BLANK TEST	0.000	13:20
EXTERNAL STANDARD	0.039	13:20
BLANK TEST	0.000	13:21
EXTERNAL STANDARD	0.039	13:21
BLANK TEST	0.000	13:22
EXTERNAL STANDARD	0.039	13:22
BLANK TEST	0.000	13:23

Average = 0.0388
 Std Dev = 0.0004

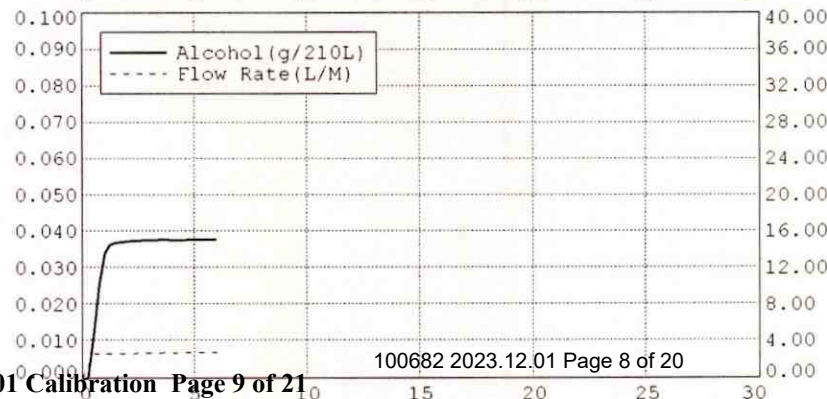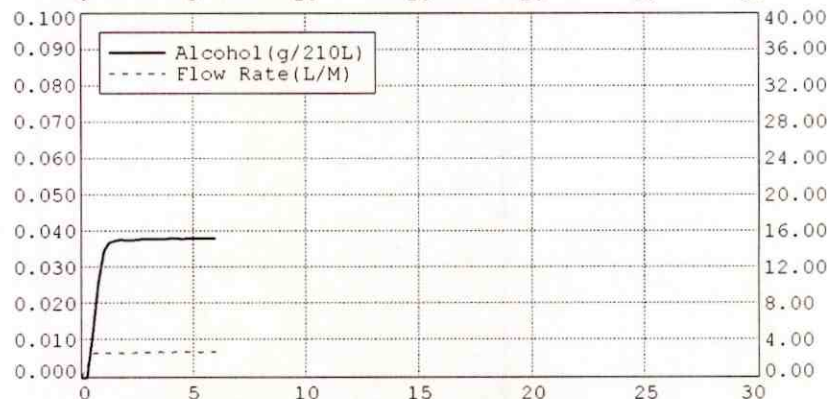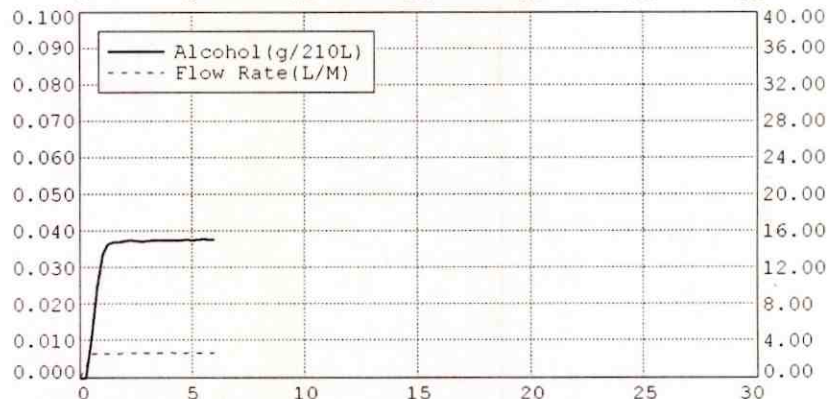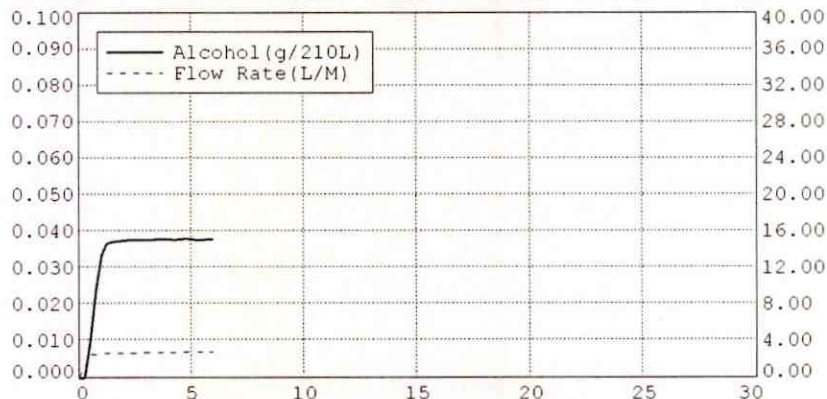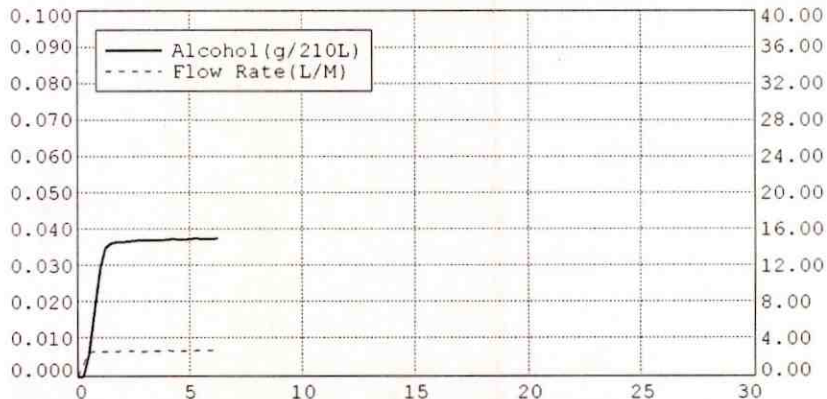

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100682






Date: 11/30/2023
 Time: 13:29:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 28.83: 0.077
 LOT #: AG135004
 EXPIRATION: 12/16/2023
 TANK PRESSURE: 135 psi

BLANK TEST	0.000	13:31
INTERNAL STANDARD	VERIFIED	13:31
EXTERNAL STANDARD	0.077	13:31
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.077	13:32
BLANK TEST	0.000	13:33
EXTERNAL STANDARD	0.077	13:33
BLANK TEST	0.000	13:34
EXTERNAL STANDARD	0.077	13:34
BLANK TEST	0.000	13:35
EXTERNAL STANDARD	0.077	13:35
BLANK TEST	0.000	13:36

Average = 0.0770
 Std Dev = 0.0000

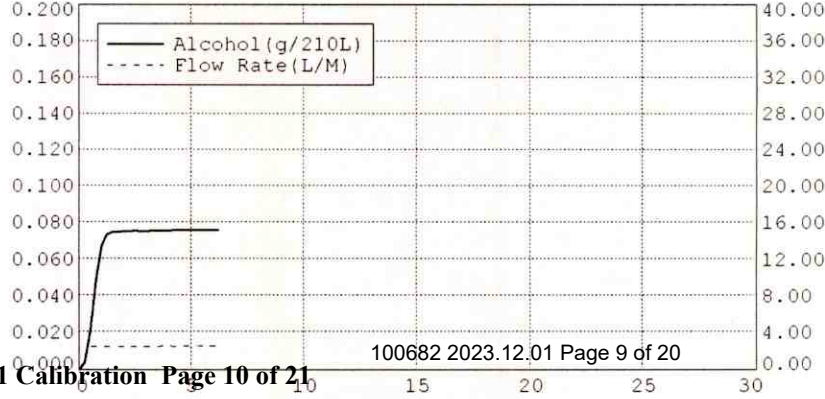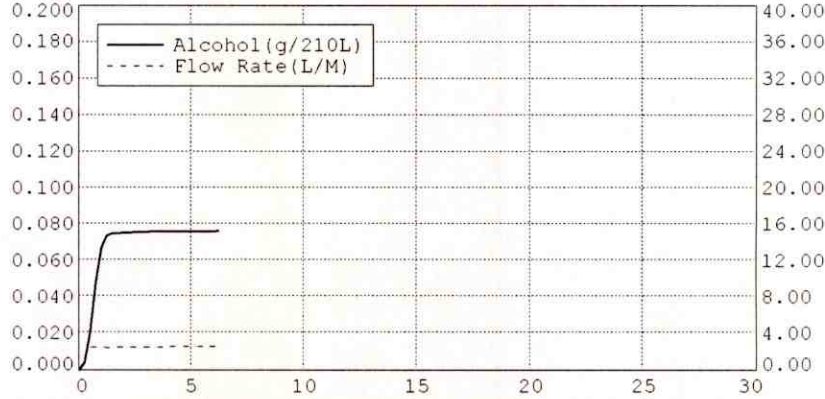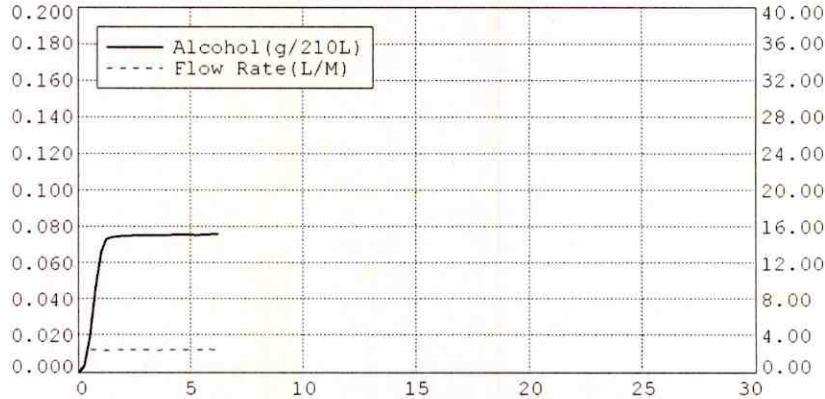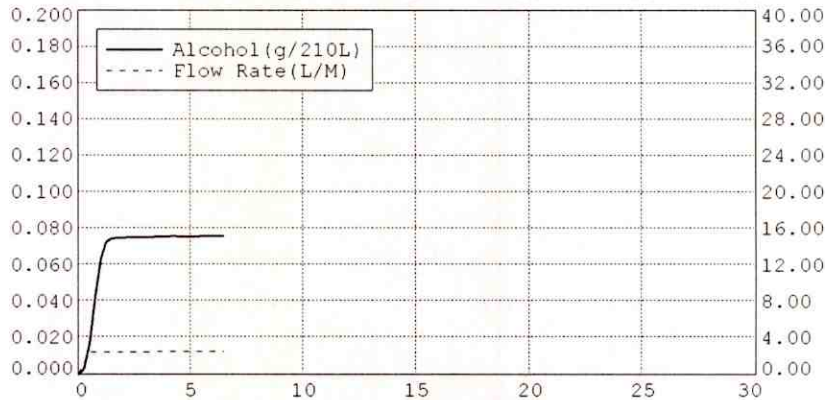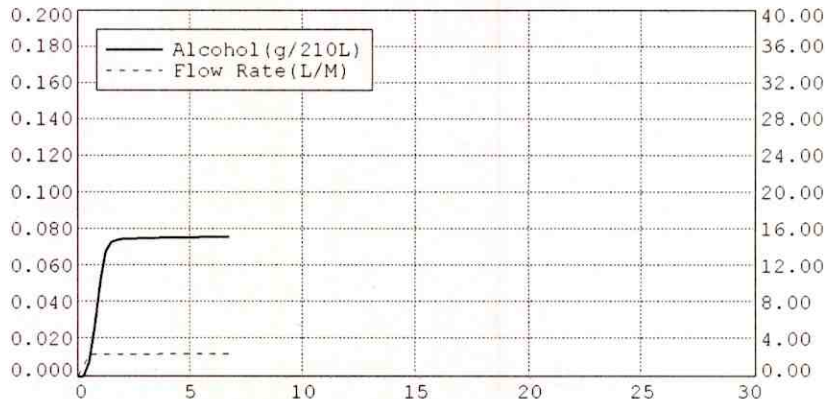

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100682






Date: 11/30/2023
 Time: 15:22:50

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 28.83: 0.096
 LOT #: AG211003
 EXPIRATION: 04/20/2024
 TANK PRESSURE: 724 psi

BLANK TEST	0.000	15:24
INTERNAL STANDARD	VERIFIED	15:24
EXTERNAL STANDARD	0.097	15:24
BLANK TEST	0.000	15:25
EXTERNAL STANDARD	0.097	15:25
BLANK TEST	0.000	15:26
EXTERNAL STANDARD	0.097	15:26
BLANK TEST	0.000	15:27
EXTERNAL STANDARD	0.097	15:27
BLANK TEST	0.000	15:28
EXTERNAL STANDARD	0.097	15:28
BLANK TEST	0.000	15:29

Average = 0.0970
 Std Dev = 0.0000

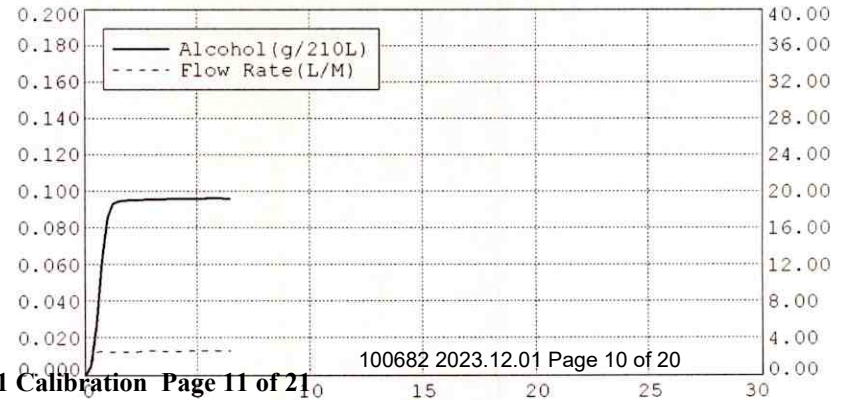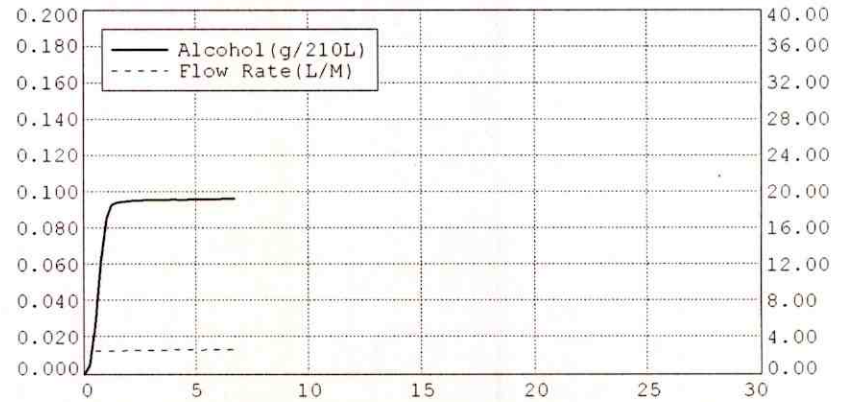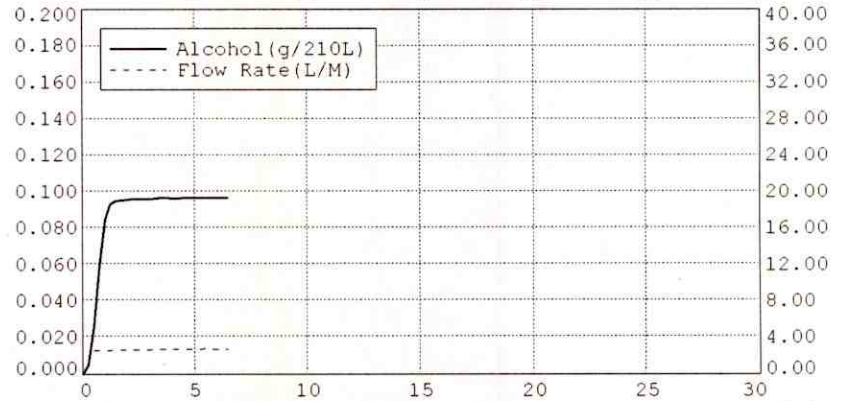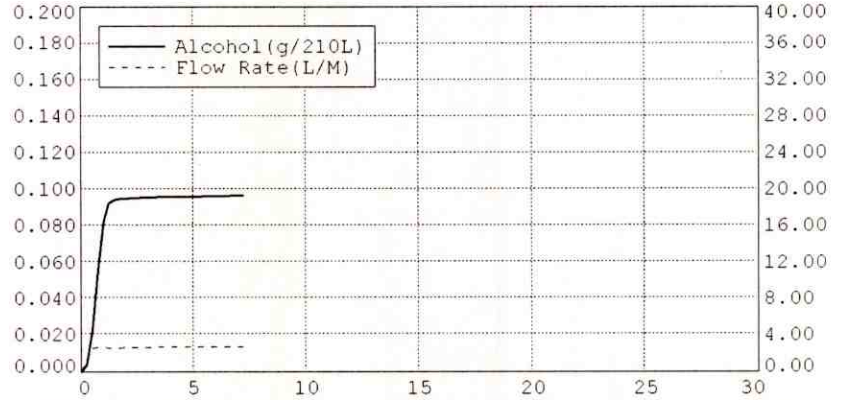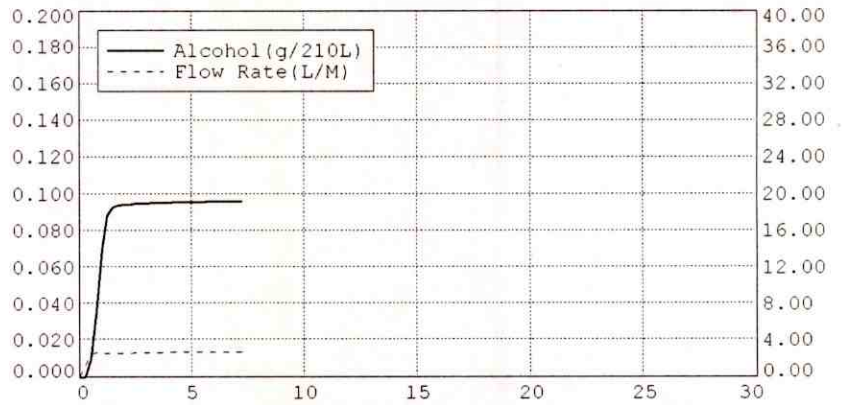

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100682






Date: 11/30/2023
 Time: 15:39:05

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 28.83: 0.145
 LOT #: AG134205
 EXPIRATION: 12/08/2023
 TANK PRESSURE: 631 psi

BLANK TEST	0.000	15:40
INTERNAL STANDARD	VERIFIED	15:40
EXTERNAL STANDARD	0.146	15:41
BLANK TEST	0.000	15:41
EXTERNAL STANDARD	0.146	15:42
BLANK TEST	0.000	15:43
EXTERNAL STANDARD	0.146	15:43
BLANK TEST	0.000	15:44
EXTERNAL STANDARD	0.146	15:44
BLANK TEST	0.000	15:45
EXTERNAL STANDARD	0.146	15:45
BLANK TEST	0.000	15:46

Average = 0.1460
 Std Dev = 0.0000

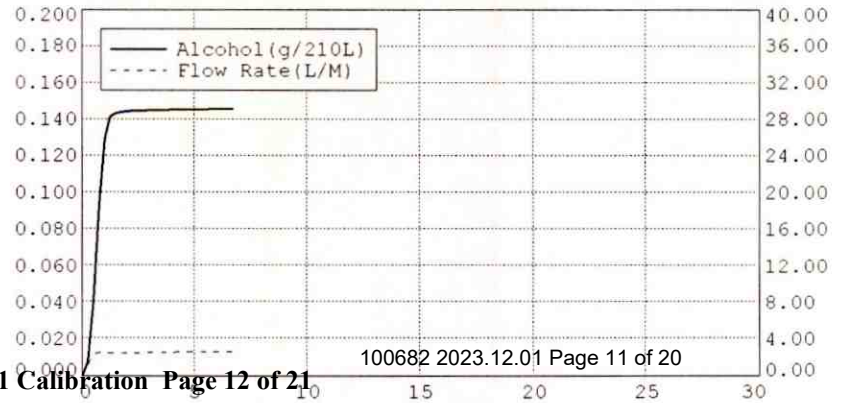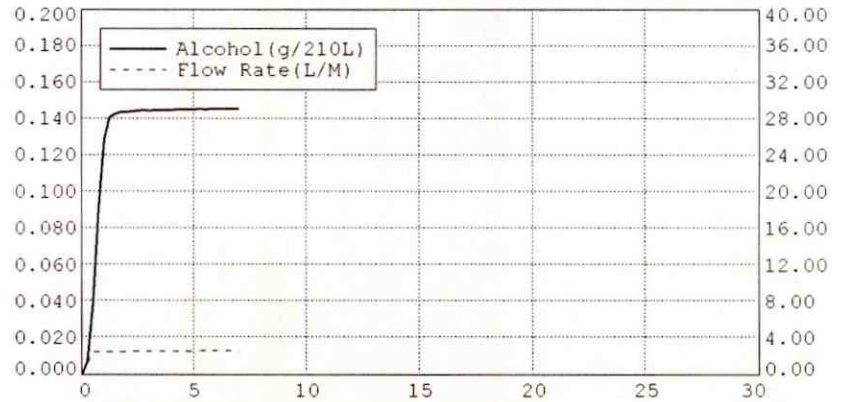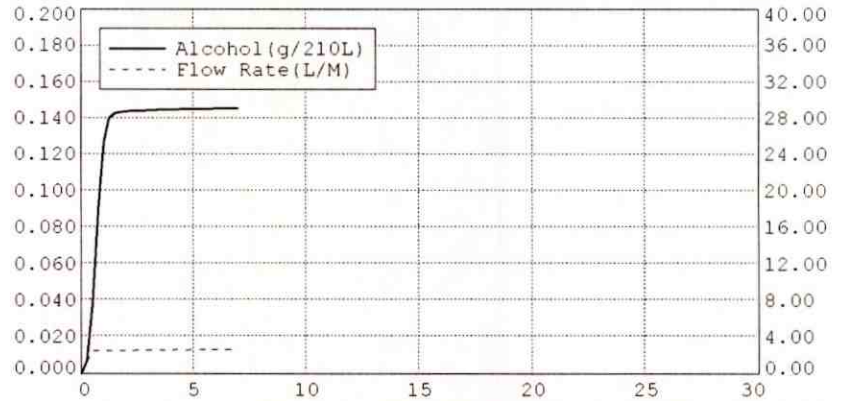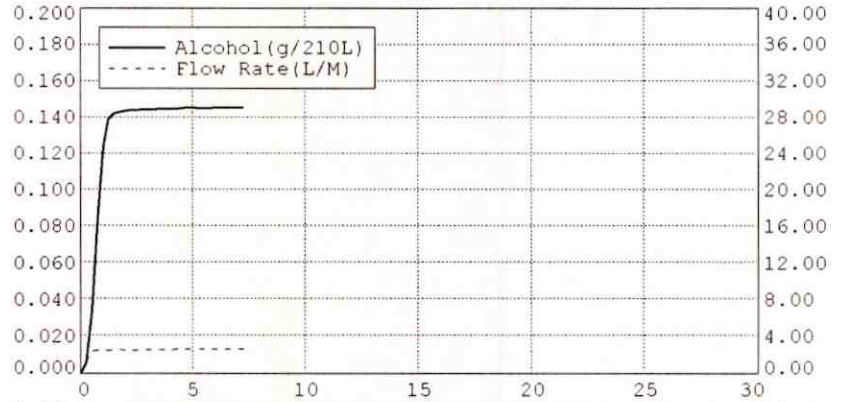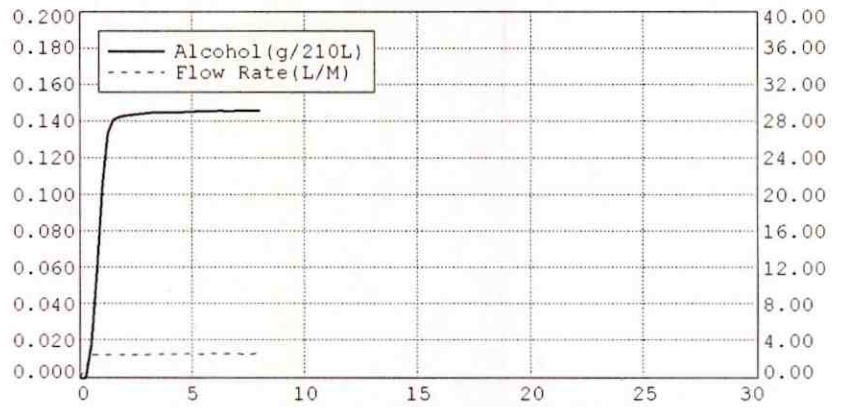

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100682






Date: 11/30/2023
 Time: 15:46:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 28.83: 0.289
 LOT #: AG217903
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 162 psi

BLANK TEST	0.000	15:48
INTERNAL STANDARD	VERIFIED	15:48
EXTERNAL STANDARD	0.294	15:48
BLANK TEST	0.000	15:49
EXTERNAL STANDARD	0.293	15:49
BLANK TEST	0.000	15:50
EXTERNAL STANDARD	0.293	15:51
BLANK TEST	0.000	15:51
EXTERNAL STANDARD	0.293	15:52
BLANK TEST	0.000	15:53
EXTERNAL STANDARD	0.293	15:53
BLANK TEST	0.000	15:54

Average = 0.2932
 Std Dev = 0.0004

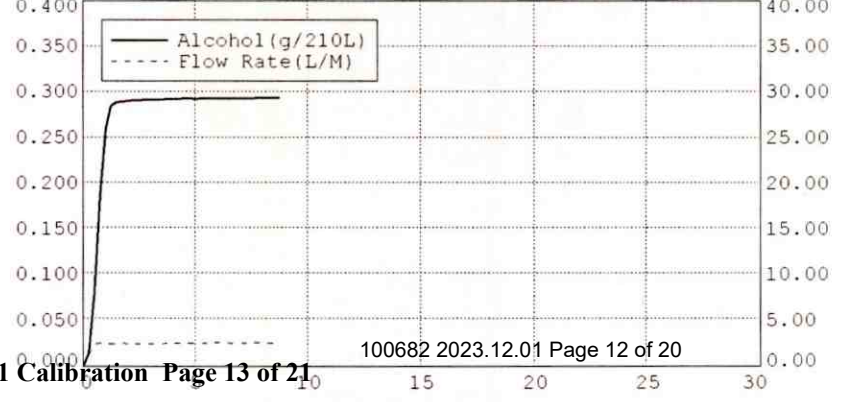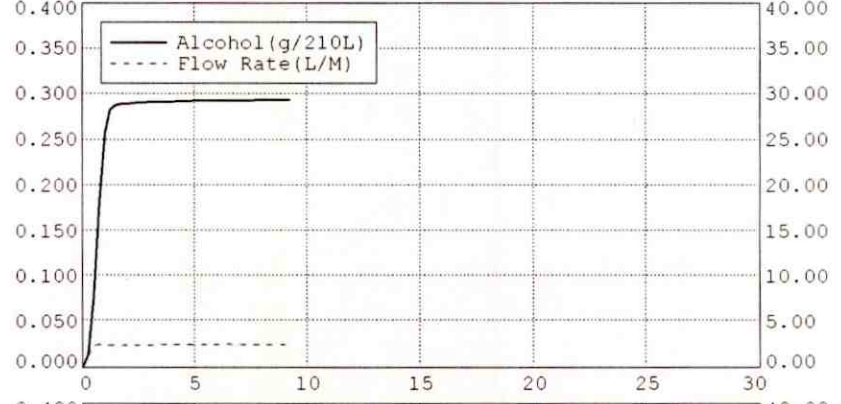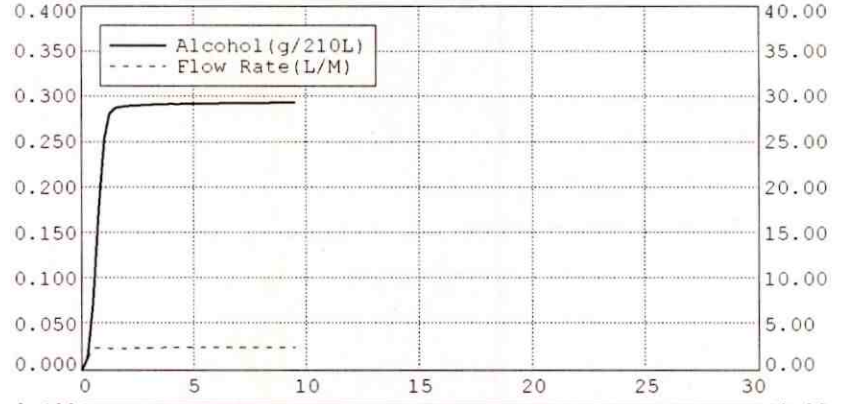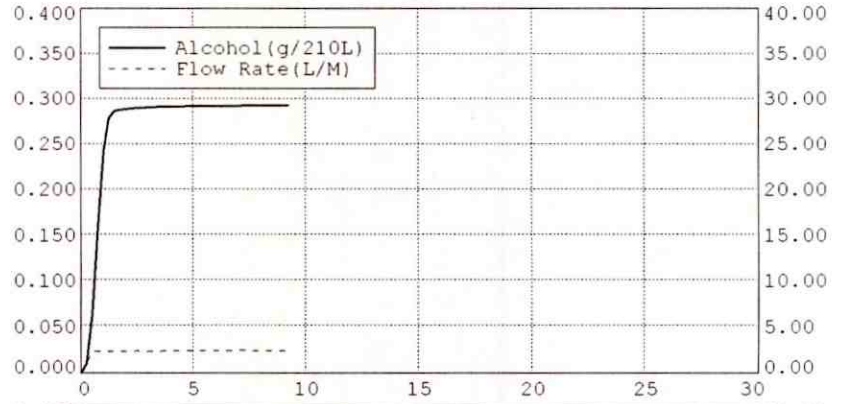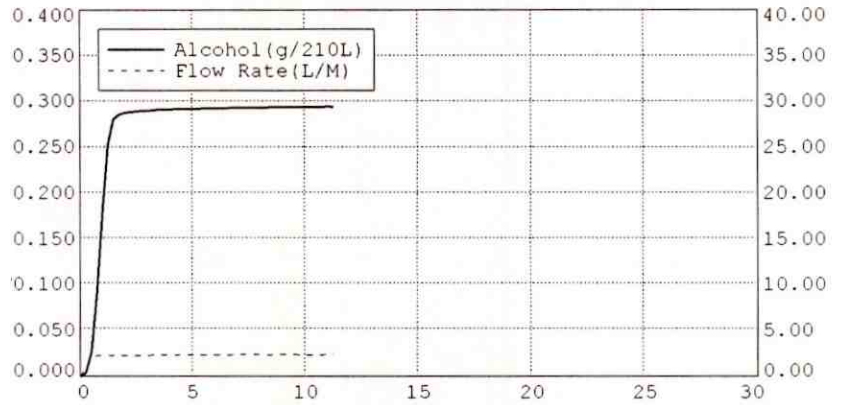

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 11/30/2023
Time: 16:07:23

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.85: 0.077
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 16:08
BLANK TEST 0.000 16:08
INTERNAL STANDARD VERIFIED 16:08
EXTERNAL STANDARD 0.077 16:09
BLANK TEST 0.000 16:09
SUBJECT SAMPLE INCOMPLETE 16:12

CVG



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 12/01/2023
Time: 09:50:51

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.96: 0.077
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 09:52
BLANK TEST 0.000 09:53
INTERNAL STANDARD VERIFIED 09:53
EXTERNAL STANDARD 0.076 09:53
BLANK TEST 0.000 09:54
SUBJECT SAMPLE XXX 09:55

Maximum Attempts Exceeded

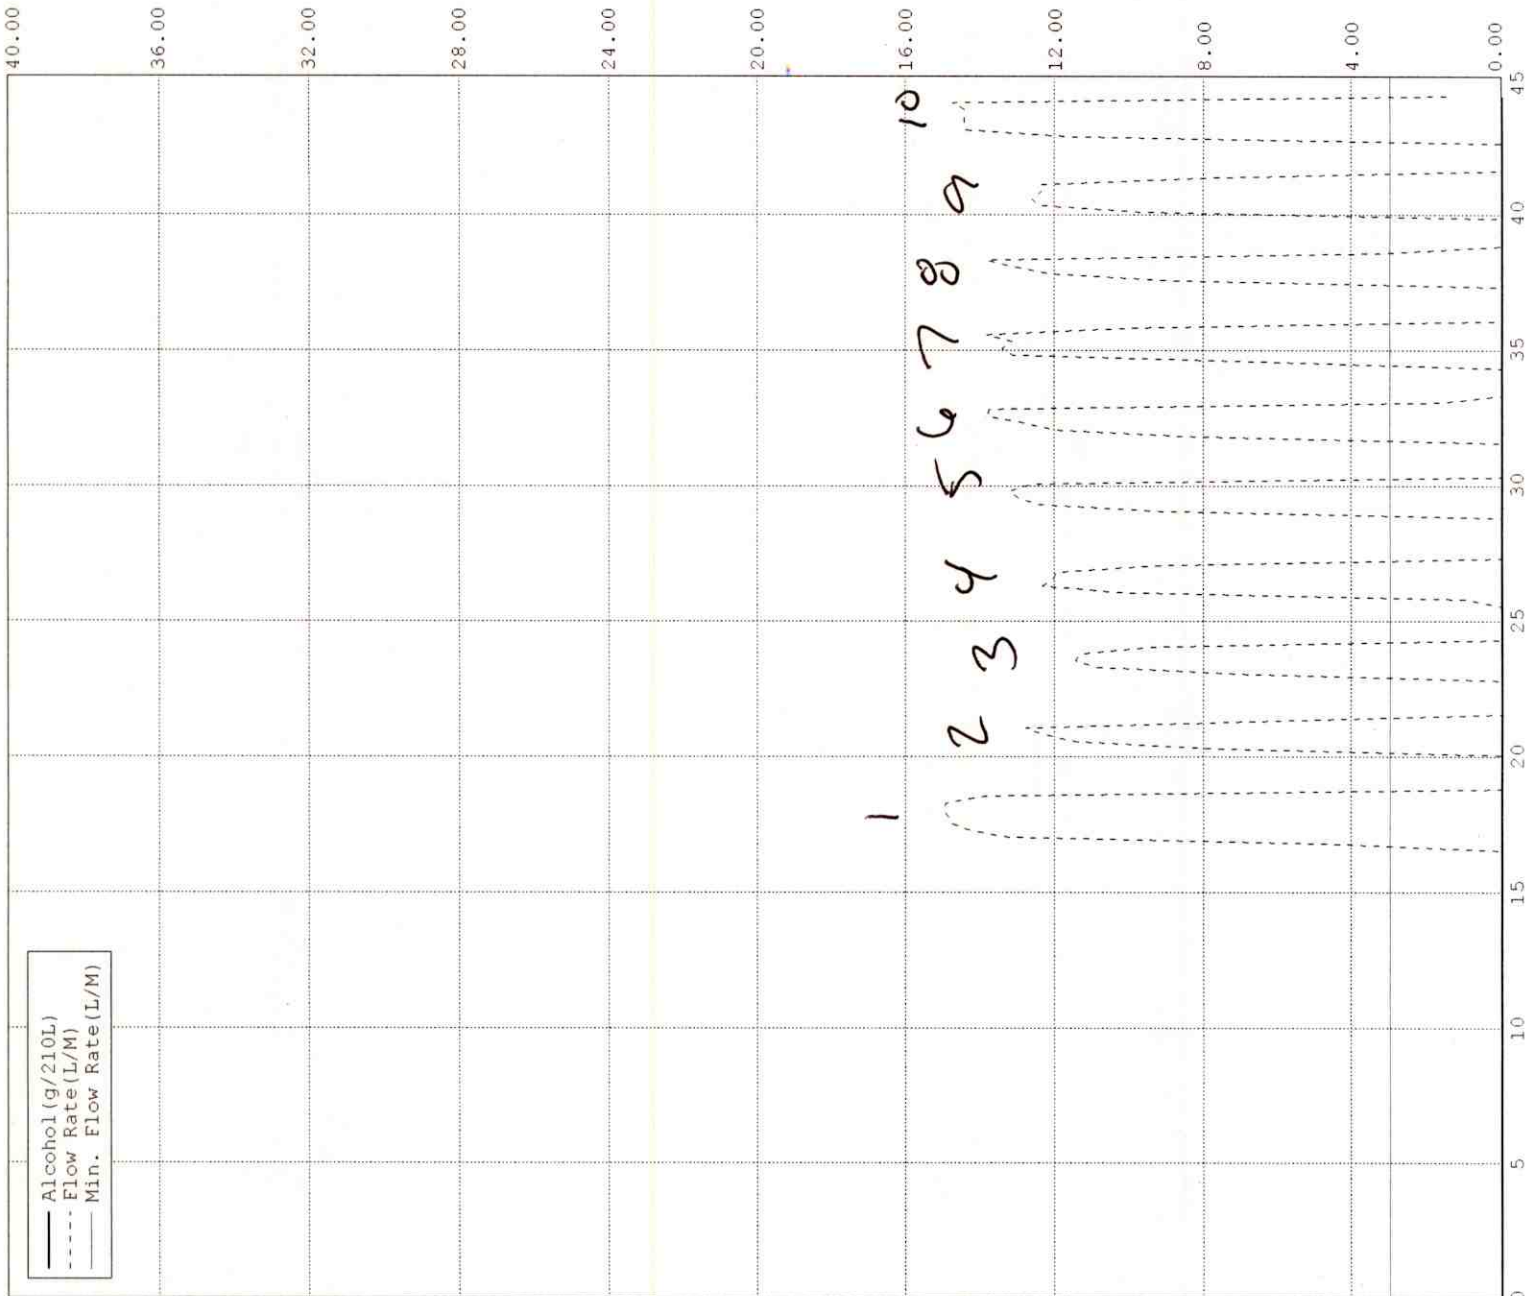

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 12/01/2023
Time: 10:09:15

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INVALID
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.96: 0.077
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 10:13
BLANK TEST 0.000 10:13
INTERNAL STANDARD VERIFIED 10:13
EXTERNAL STANDARD 0.077 10:14
BLANK TEST 0.000 10:14
SUBJECT SAMPLE INVALID 10:16

OK

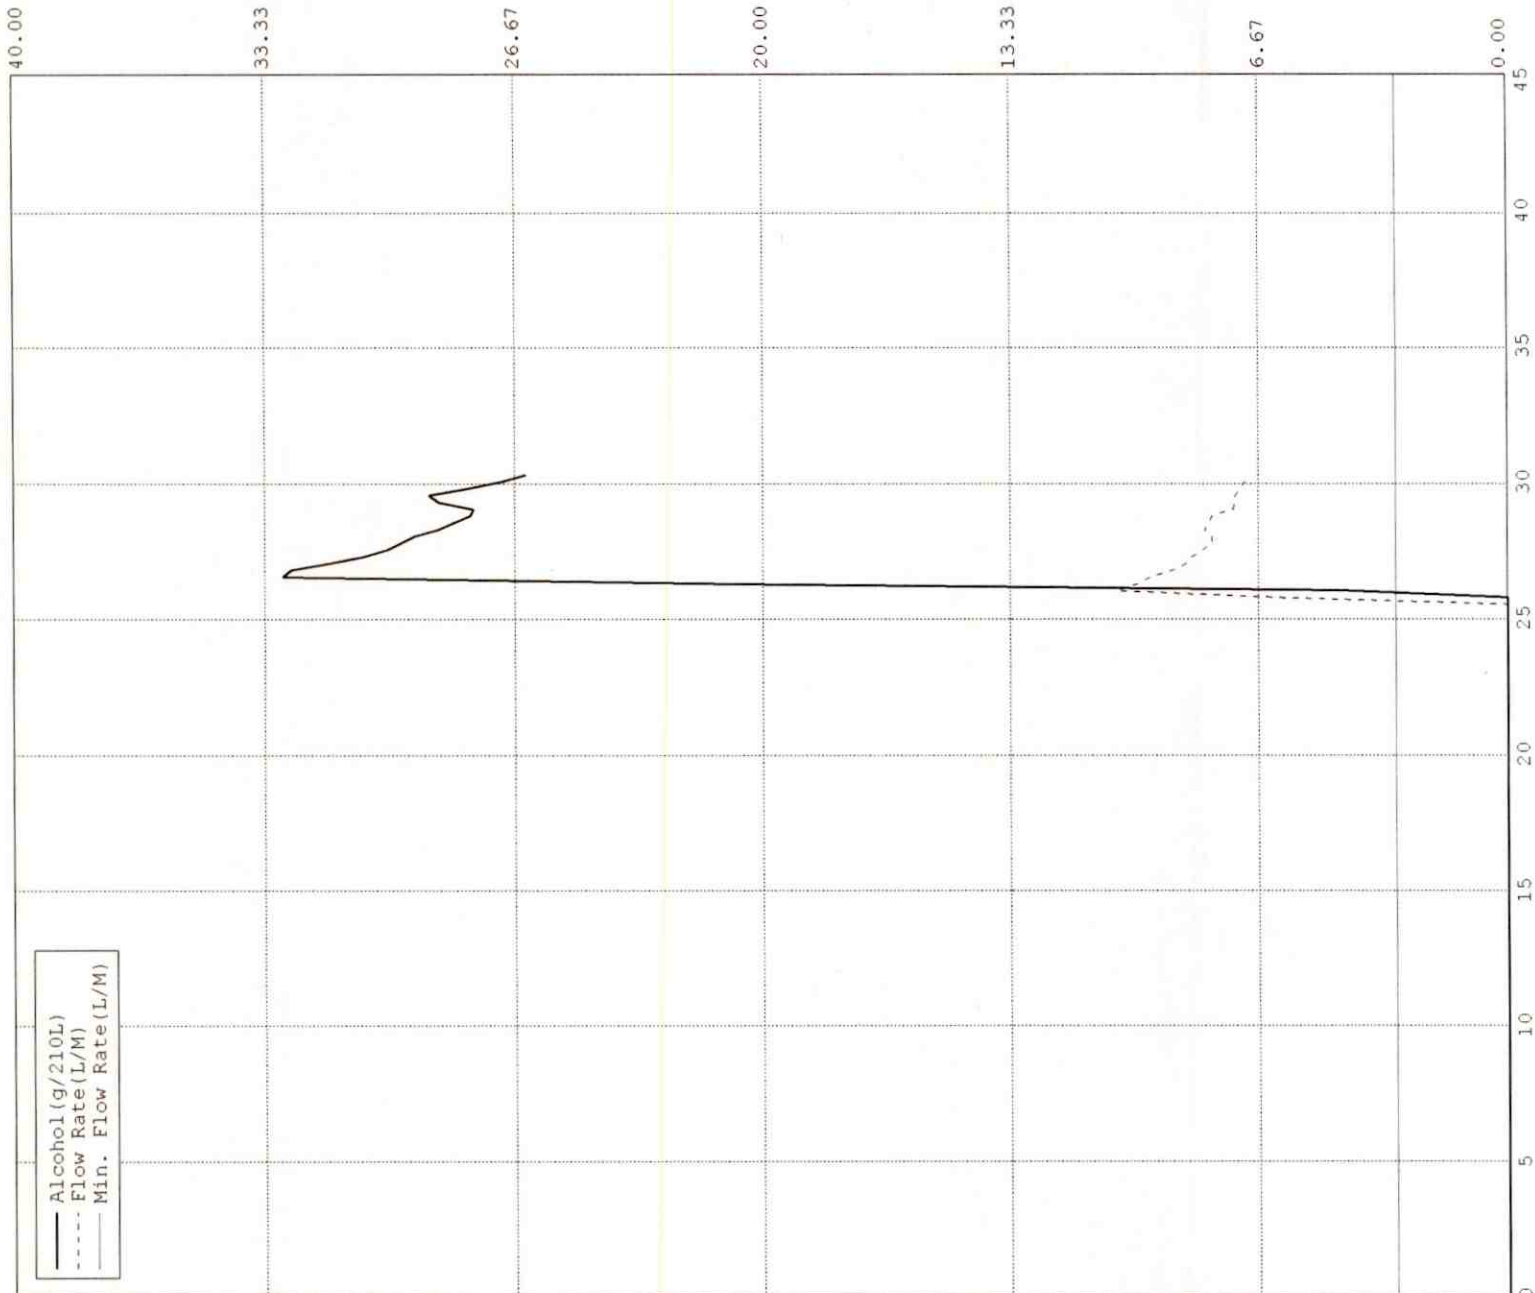

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 12/01/2023
Time: 10:25:33

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:


RFI
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.96: 0.077
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 10:27
BLANK TEST 0.000 10:27
INTERNAL STANDARD VERIFIED 10:27
EXTERNAL STANDARD 0.077 10:27
BLANK TEST 0.000 10:28

RFI DETECTED

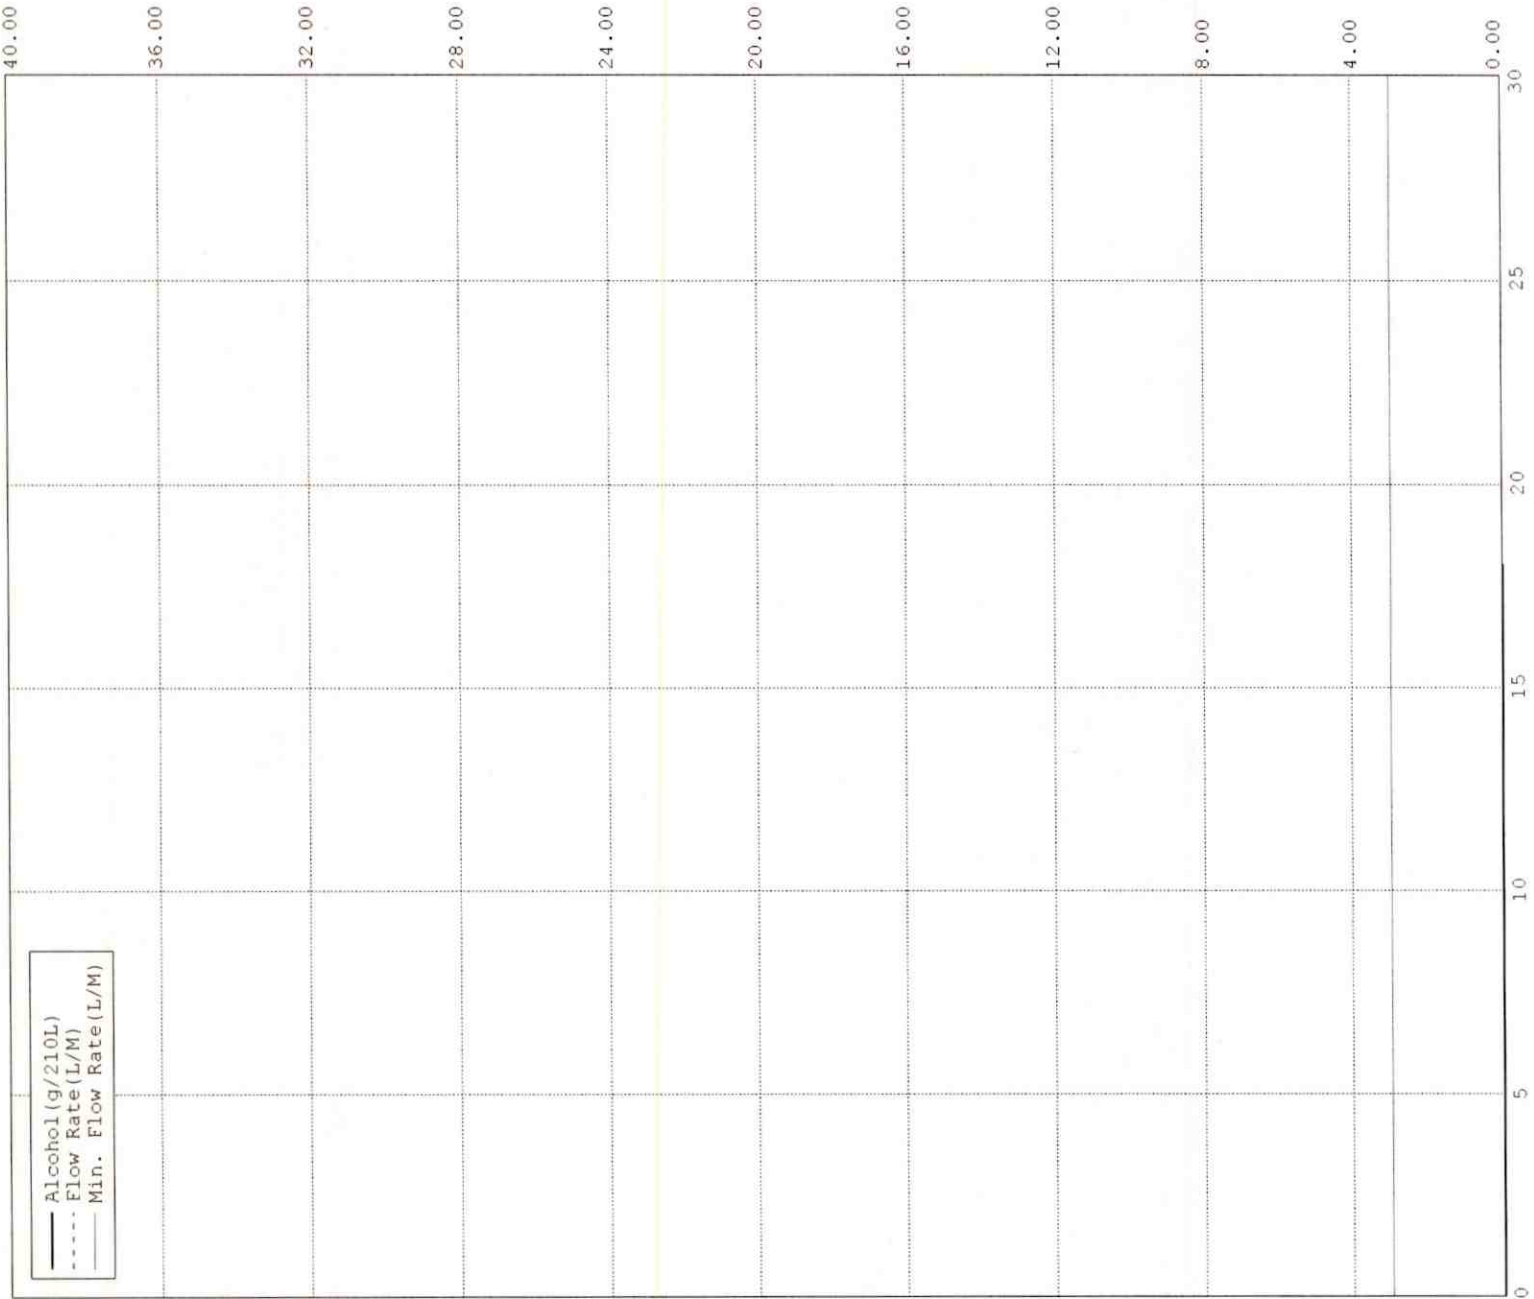

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 12/01/2023
Time: 11:32:15

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INTERFERENCE ACETONE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.97: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 11:33
BLANK TEST 0.000 11:33
INTERNAL STANDARD VERIFIED 11:33
Xg = 0.101 (1.20%)
EXTERNAL STANDARD 0.077 11:33
X[1] = 0.0766 (-0.0008) (0.0026)
BLANK TEST 0.000 11:34
SUBJECT SAMPLE XXX 11:35
X[1] = 0.1113 (-0.0181) (0.0046)

Interference Detected

Filter 2 Average: -0.0012
Filter 3 Average: 0.0022
QWB-12/14/23

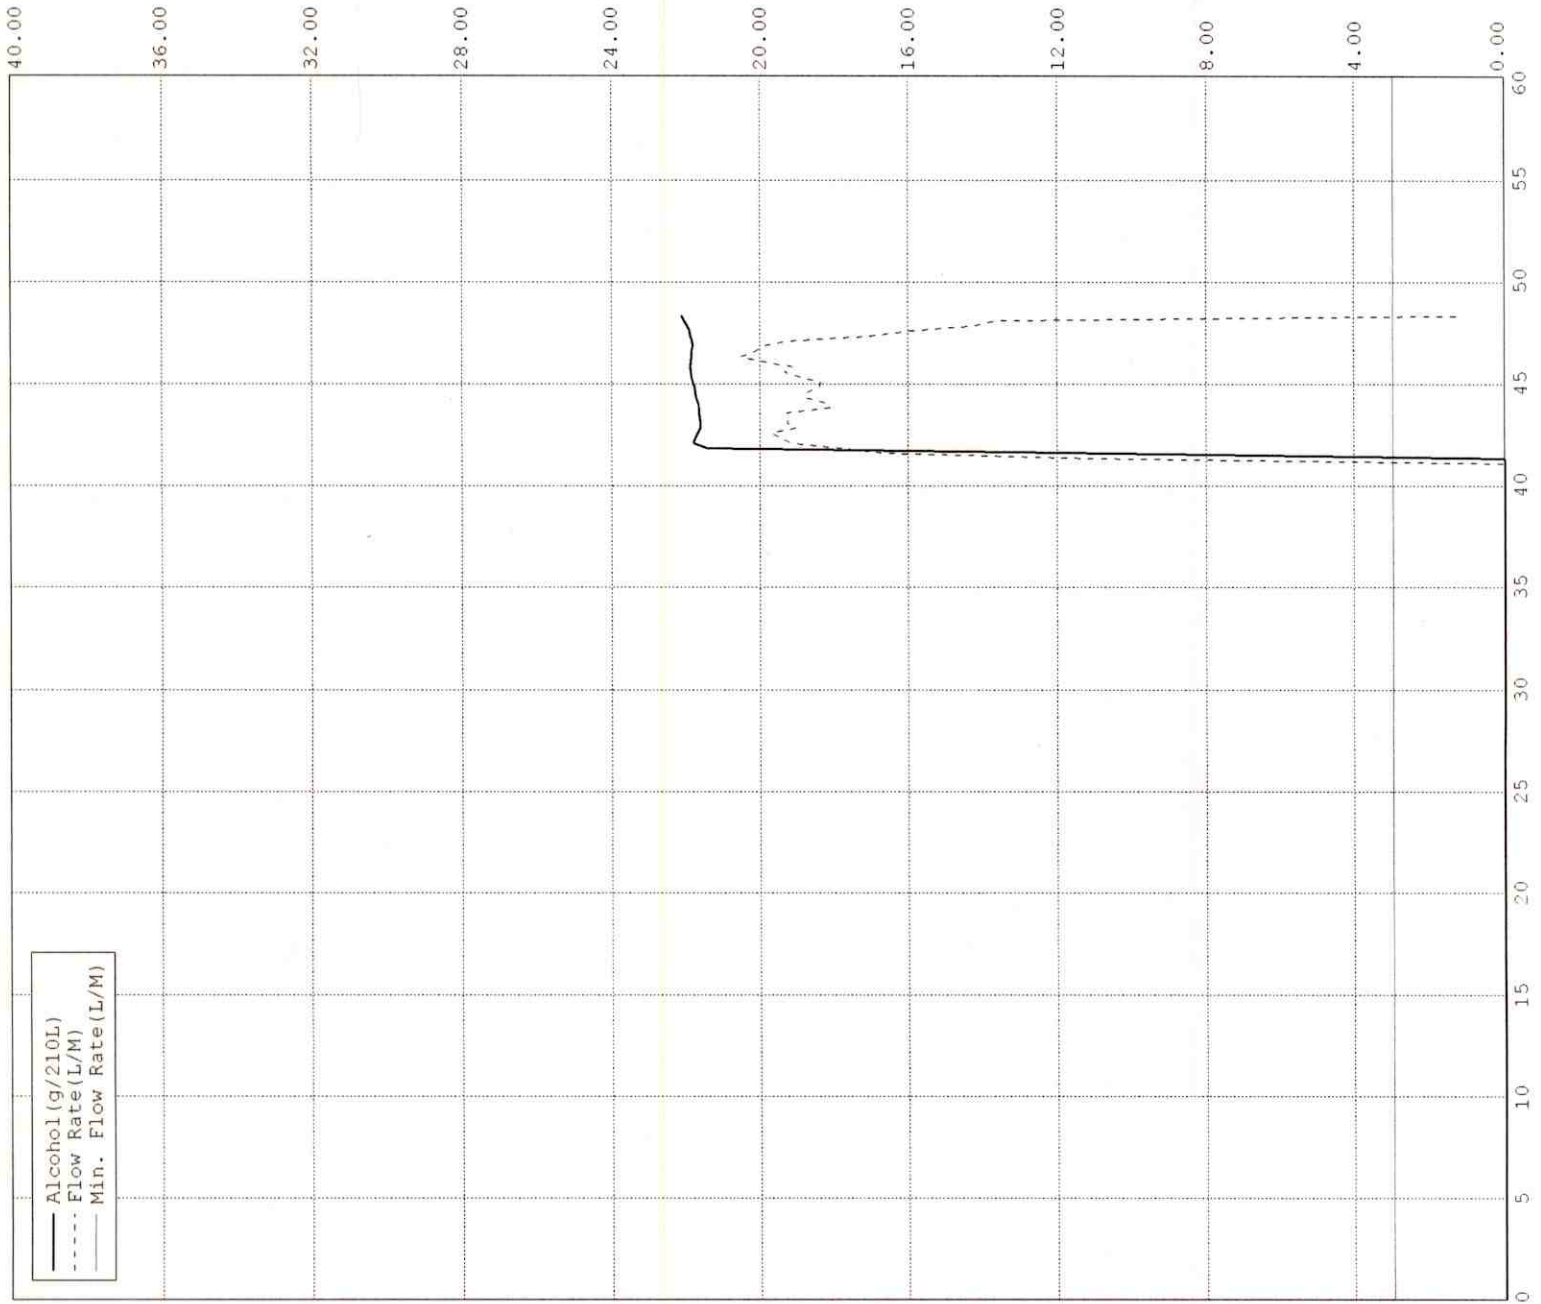

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 12/01/2023
Time: 11:25:46

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INTERFERENCE IPA
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.96: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 11:26
BLANK TEST 0.000 11:26
INTERNAL STANDARD VERIFIED 11:27
Xq = 0.101 (0.94%)
EXTERNAL STANDARD 0.078 11:27
X[1] = 0.0775 (-0.0003) (0.0023)
BLANK TEST 0.000 11:28
SUBJECT SAMPLE XXX 11:28
X[1] = 0.1198 (-0.0256) (0.0033)

Interference Detected

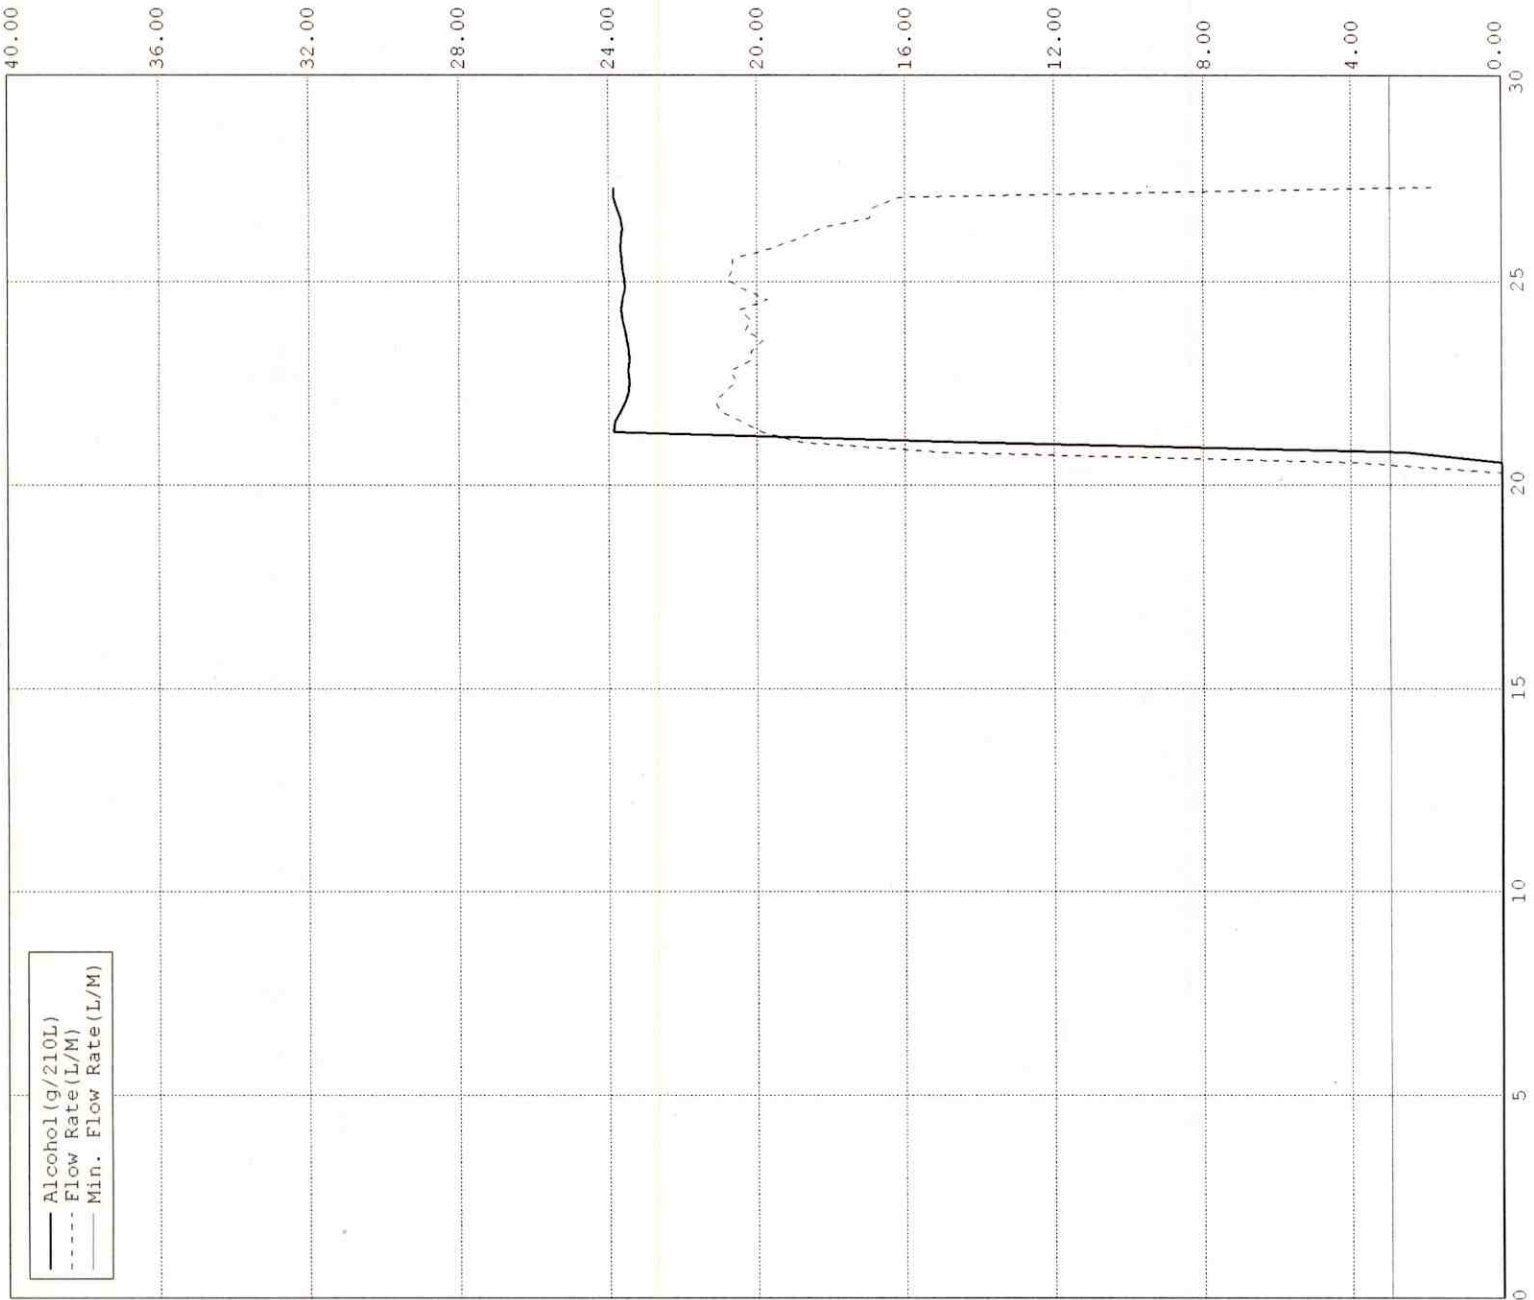

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 12/01/2023
Time: 10:52:17


SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE NEGATIVE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.96: 0.077
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	10:53
BLANK TEST	0.000	10:53
INTERNAL STANDARD	VERIFIED	10:53
Xg = 0.101 (1.11%)		
EXTERNAL STANDARD	0.077	10:54
X[1] = 0.0770 (-0.0012)	(0.0022)	
BLANK TEST	0.000	10:55
SUBJECT SAMPLE (Vol=2.14L)	0.090	10:55
X[1] = 0.0906 (-0.0003)	(0.0009)	
BLANK TEST	0.000	10:56
EXTERNAL STANDARD	0.077	10:56
X[1] = 0.0767 (-0.0026)	(0.0015)	
BLANK TEST	0.000	10:57

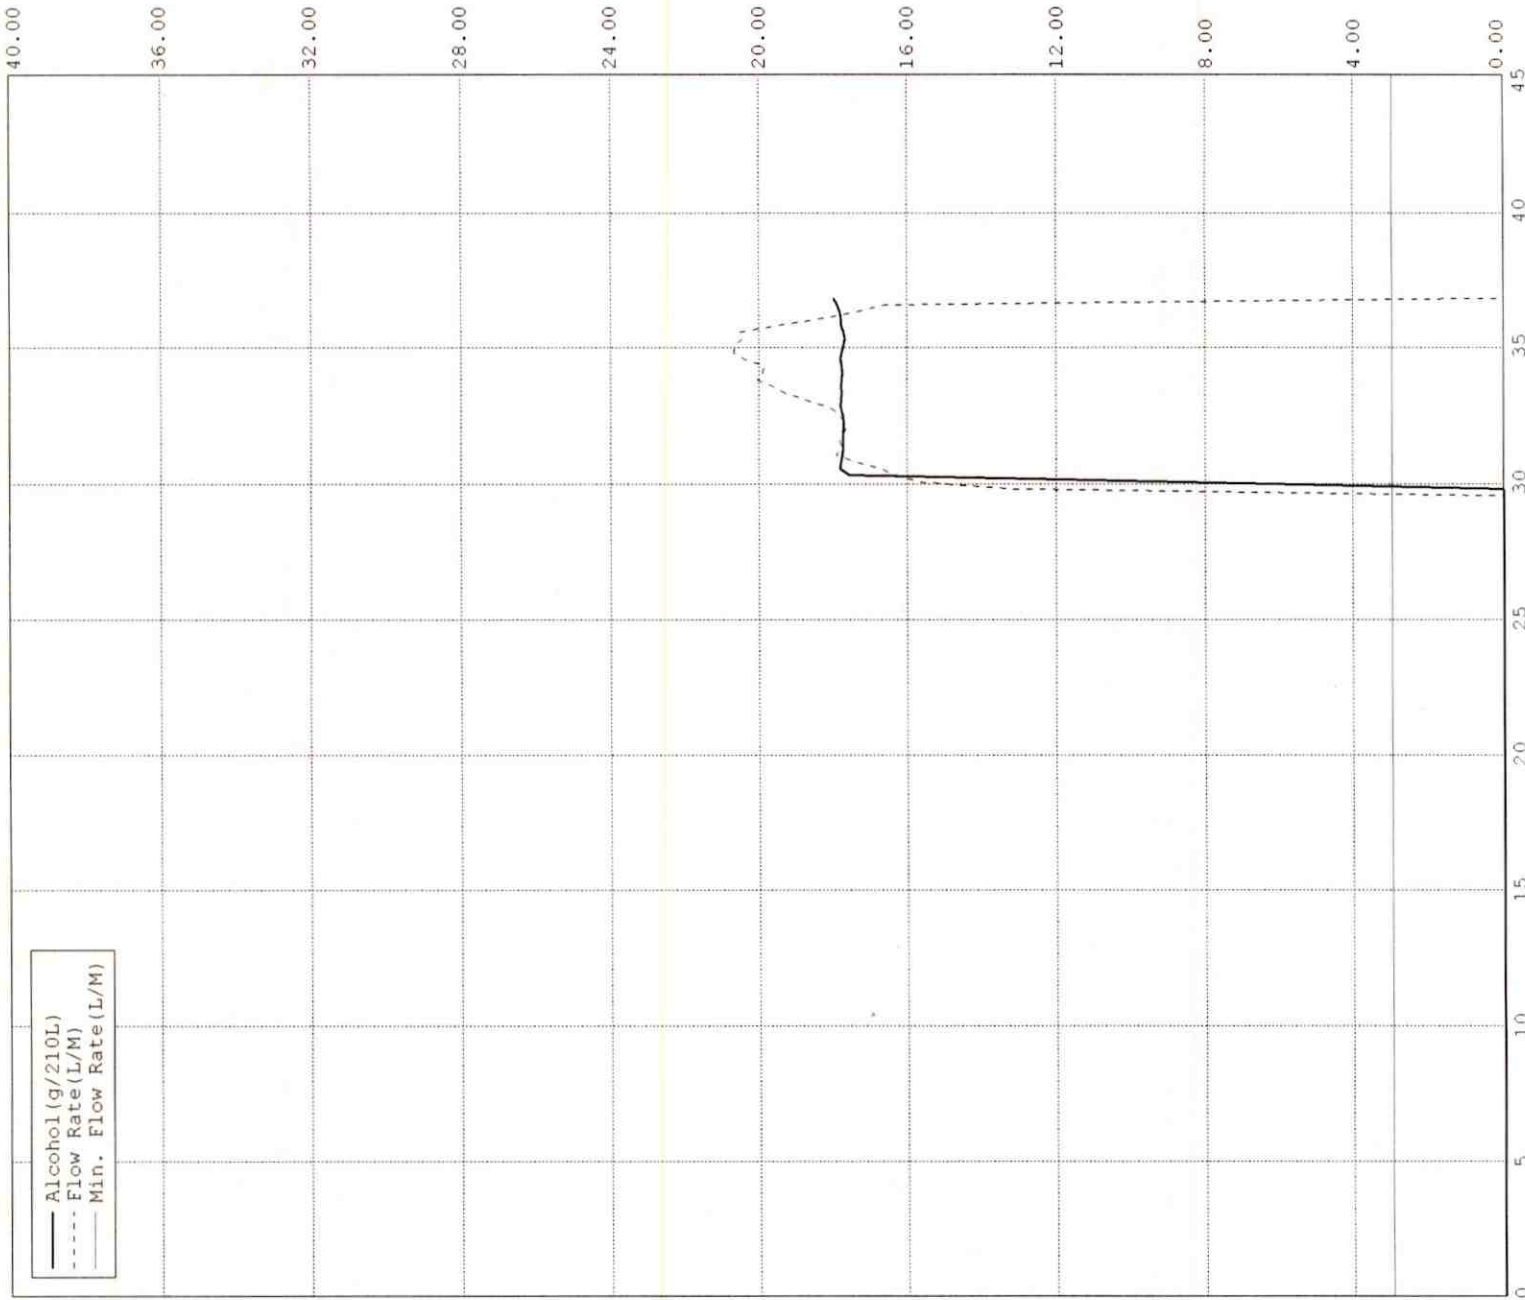

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 12/01/2023
Time: 11:56:46

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.96: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	12:02
BLANK TEST	0.000	12:02
INTERNAL STANDARD	VERIFIED	12:02
EXTERNAL STANDARD	0.078	12:03
BLANK TEST	0.000	12:03
SUBJECT SAMPLE (Vol=1.68L)	0.000	12:04
BLANK TEST	0.000	12:05
EXTERNAL STANDARD	0.078	12:05
BLANK TEST	0.000	12:06

CKG

