

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100359

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 04/11/2013

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.30: 0.081
LOT #: 22612080A1
EXPIRATION: 09/01/2014

| | | |
|-------------------|----------|-------|
| BLANK TEST | 0.000 | 12:02 |
| INTERNAL STANDARD | VERIFIED | 12:02 |
| EXTERNAL STANDARD | 0.079 | 12:02 |
| BLANK TEST | 0.000 | 12:03 |
| EXTERNAL STANDARD | 0.079 | 12:03 |
| BLANK TEST | 0.000 | 12:04 |
| EXTERNAL STANDARD | 0.080 | 12:04 |
| BLANK TEST | 0.000 | 12:05 |
| EXTERNAL STANDARD | 0.080 | 12:05 |
| BLANK TEST | 0.000 | 12:06 |
| EXTERNAL STANDARD | 0.080 | 12:06 |
| BLANK TEST | 0.000 | 12:07 |

Average = 0.0796
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 2.00
PIC: 3.02
Modem: 2.3
Questions: 2.2

TEMPERATURES

| | |
|-------------------------|--------|
| Sample Chamber = 48.8°C | PASSED |
| Breath Tube = 47.6°C | PASSED |

PUMP INFO

Flow Rate = 4.559 L/M PASSED

DETECTOR INFO

| | |
|----------|--------|
| PUMP ON | PASSED |
| PUMP OFF | PASSED |

FILTER INFO

| | |
|----------|--------|
| Filter 1 | PASSED |
| Filter 2 | PASSED |
| Filter 3 | PASSED |

INTERNAL STANDARD PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

5/10/2013

Subscribed and sworn before me this 10th day of May, 2013

Nikki Roth
 Nikki Roth, Notary Public
 My Commission Expires With Office

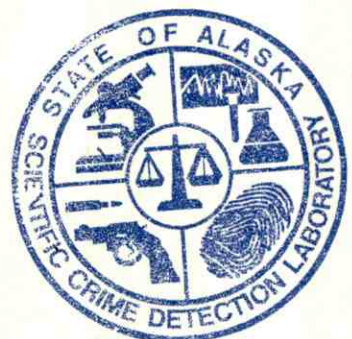

003 4/22/13