

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100379

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 09/21/2017

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.53: 0.079
LOT #: AG608504
EXPIRATION: 03/25/2018
TANK PRESSURE: 248 psi

BLANK TEST	0.000	14:12
INTERNAL STANDARD	VERIFIED	14:12
EXTERNAL STANDARD	0.079	14:12
BLANK TEST	0.000	14:13
EXTERNAL STANDARD	0.080	14:13
BLANK TEST	0.000	14:14
EXTERNAL STANDARD	0.080	14:14
BLANK TEST	0.000	14:15
EXTERNAL STANDARD	0.080	14:15
BLANK TEST	0.000	14:16
EXTERNAL STANDARD	0.079	14:16
BLANK TEST	0.000	14:17

Average = 0.0796
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.1°C PASSED
Breath Tube = 44.7°C PASSED

PUMP INFO

Flow Rate = 4.369 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED


FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED


I, Charles R. Foster, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.



 11/9/17

Charles R. Foster
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 9 day of Nov, 20 17

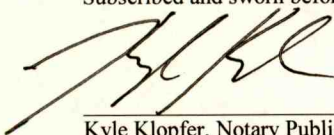

Kyle Klopfer, Notary Public
My Commission Expires With Office

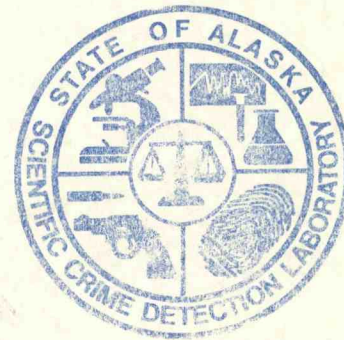

BMB
10/3/17