



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100417

**Report Issue Date:** 10/21/2024  
**Date Received:** 2024-07-29  
**Condition of Item:** No apparent damage

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG408002	0.019	0.019	0.019	0.019	0.019	0.019	0.019
0.080	0.078	AG310901	0.077	0.076	0.077	0.077	0.077	0.077	0.077
0.300	0.294	AG327804	0.294	0.292	0.292	0.293	0.292	0.292	0.293

As Found - Evaluation Analyst: Megan Carlock  
 As Found Conditions - Barometric Pressure (inHg): 29.41 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.9 Relative Humidity (%): 47  
 As-Found Lab Activity Date Range: 07/29/2024 - 07/29/2024

No O-ring present as received; a new O-ring was put on.

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG408002	0.021	0.020	0.020	0.020	0.020	0.020	+/- 0.002	
0.040	0.040	AG407908	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003	
0.080	0.079	AG310901	0.079	0.079	0.079	0.079	0.078	0.079	+/- 0.004	
0.100	0.099	AG333401	0.100	0.100	0.100	0.100	0.100	0.100	+/- 0.004	
0.150	0.149	AG332004	0.148	0.147	0.147	0.148	0.147	0.147	+/- 0.006	
0.300	0.298	AG327804	0.299	0.299	0.299	0.299	0.299	0.299	+/- 0.012	

As Left Conditions - Barometric Pressure (inHg): 29.70 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.4 Relative Humidity (%): 45  
 As-Left Lab Activity Date Range: 09/03/2024 - 09/03/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Carlie Glaister on 09/03/2024

[carlie.glaister@alaska.gov](mailto:carlie.glaister@alaska.gov)

Technically and administratively reviewed by Colleen O'Bryant on 10/21/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100417

Analyst or Technician Name: Carlie Glaister

DataMaster DMT Calibration Start Date: 9/3/2024

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 230307229  
Calibration Due Date: 5/2/2025
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.70 Temperature(C) 21.4 Relative Humidity(%) 45

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

### Interference (Volatiles) - Print with View Details

1. Acetone Reagent Lot Number: 20240731MNC Expiration Date: 10/31/2024  
Simulator S/N: DR4178 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240731MNC Expiration Date: 10/31/2024  
Simulator S/N: DR6267 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 23TP41233 Expiration Date: 9/20/2025  
Simulator S/N: DR4163 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106  
Calibration Due Date: 9/19/2025

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 9/3/2024

Data Interpretation Date (Technician): 9/3/2024 (if applicable)

Data Interpretation Date (Analyst): NA ← CLG 9/3/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100417  
-----

Date: 09/03/2024  
Time: 11:56:29

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 48.1°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.89 V PASSED  
(1.13 V - 2.65 V)  
Cooler Voltage = 1.78 V PASSED  
(1.13 V - 2.65 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 531 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.9 in

PUMP INFO

Flow Rate = 4.660 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED  
Xq = 0.096 1.77% (0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100417  
-----

Date: 09/03/2024  
Time: 12:01 PM

Temperatures (°C)

Sample Cell: 48.9°C  
Breath Tube: 47.8°C

Current Barometer 29.7 in  
Volume (Ltr) 1.49

Settings

Lamp: 1.89 V  
Bias: 80 V  
Cooler: 1.76 V  
Chopper: 530 Hz

Voltages (V)

Flow: 1.03 V  
Detector: -0.036 V


CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100417  
-----

Date: 03/25/2020  
Time: 05:59:25

OPERATOR NAME:  
INTOX I METERS  
CERTIFICATE #: 1


Ca = 0.2000  
CAL = 0.972760    0.800 <= CAL < 1.200  
b1 = 0.0000    0.0000 <= b1 < 0.0040  
b2 = 0.0044    0.0010 <= b2 < 0.0100  
b3 = 0.0000    0.0000 <= b3 < 0.0040  
Xq = 0.0941    0.0500 <= Xq < 0.2000  
a21 = 1.147054    1.050 <= a21 < 1.300  
a31 = 0.516811    0.300 <= a31 < 0.800

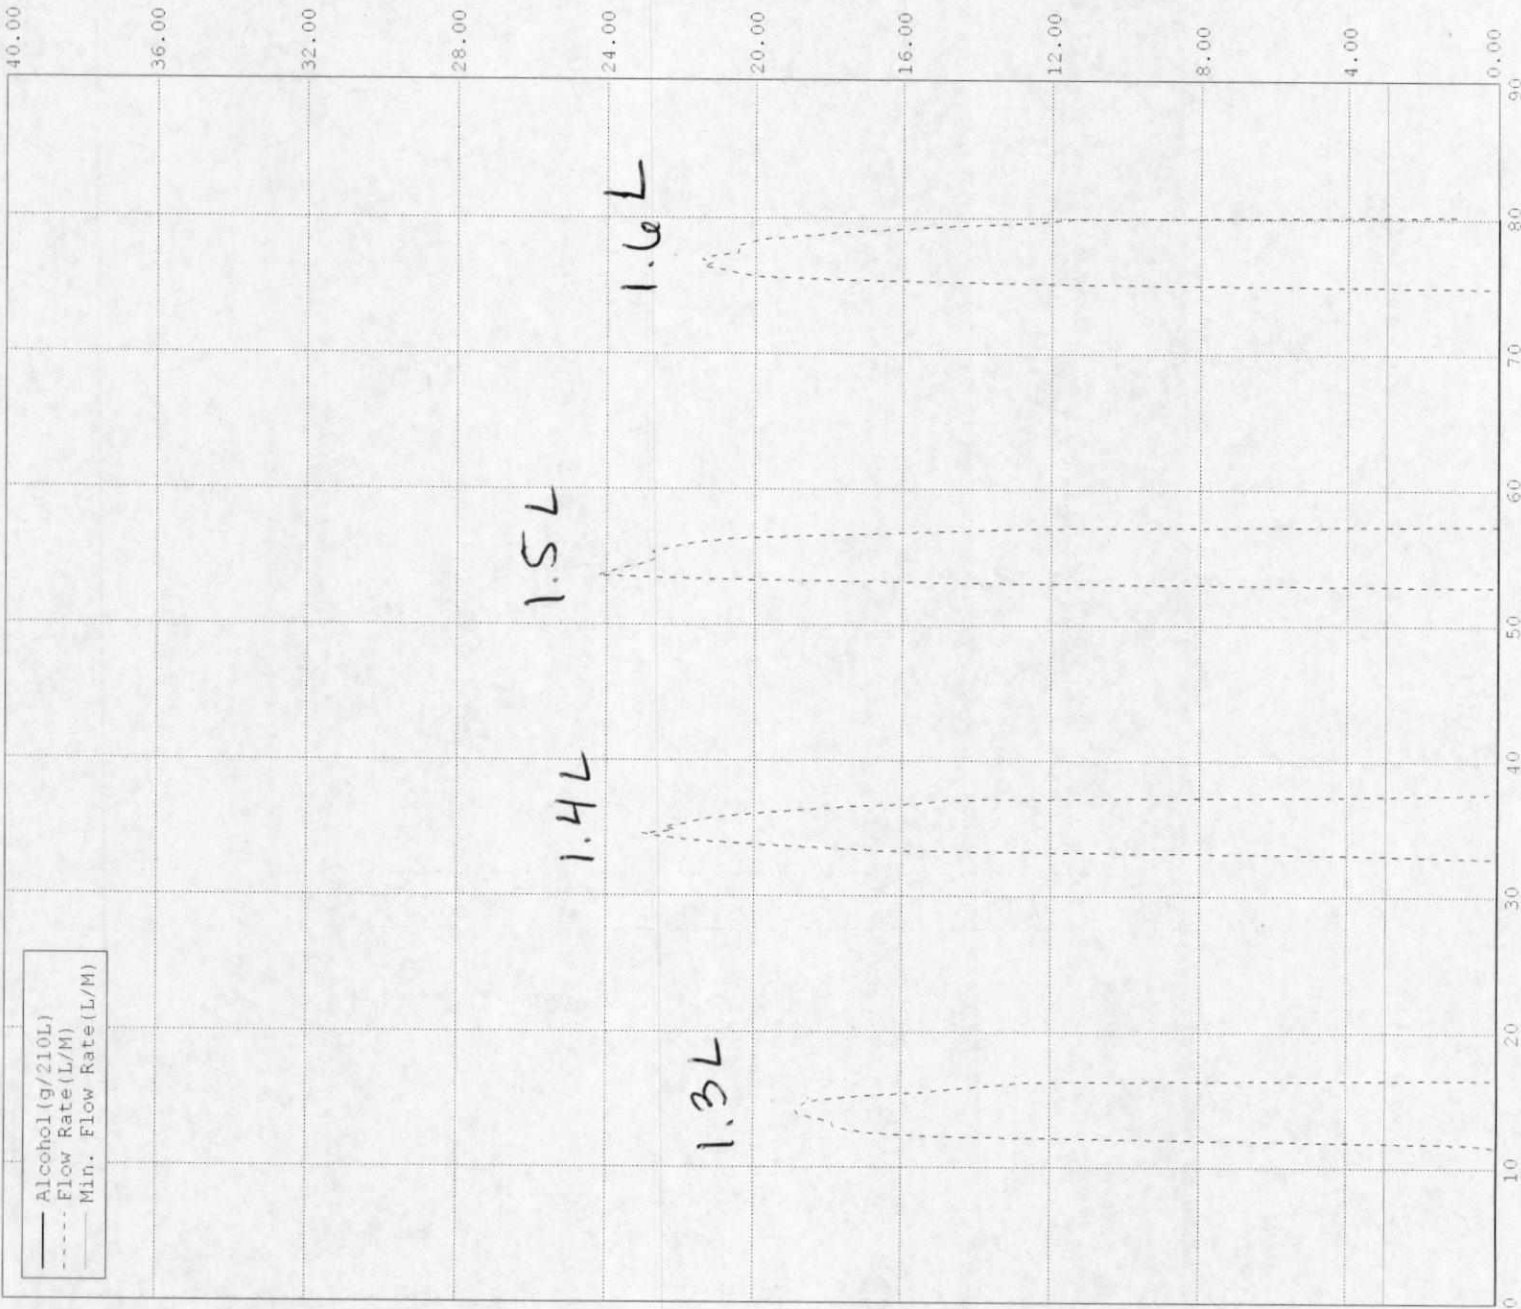

SUBJECT TEST

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100417  
 -----  
 Date: 09/03/2024  
 Time: 12:03:16  
 -----  
 SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX  
 -----  
 OPERATOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436  
 -----  
 DEPT/AGENCY:  
 MINIMUM VOLUME TEST  
 SCALE/REPORT: XXXX  
 TEST TYPE: TEST  
 -----  
 EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.69: 0.079  
 LOT #: AG310901  
 EXPIRATION: 04/19/2025  
 -----  
 DIAGNOSTIC CHECK PASSED 12:04  
 BLANK TEST 0.000 12:04  
 INTERNAL STANDARD VERIFIED 12:04  
 EXTERNAL STANDARD 0.079 12:05  
 BLANK TEST 0.000 12:05  
 SUBJECT SAMPLE (Vol=1.53L) 0.000 12:07  
 BLANK TEST 0.000 12:08  
 EXTERNAL STANDARD 0.080 12:08  
 BLANK TEST 0.000 12:09

CVG

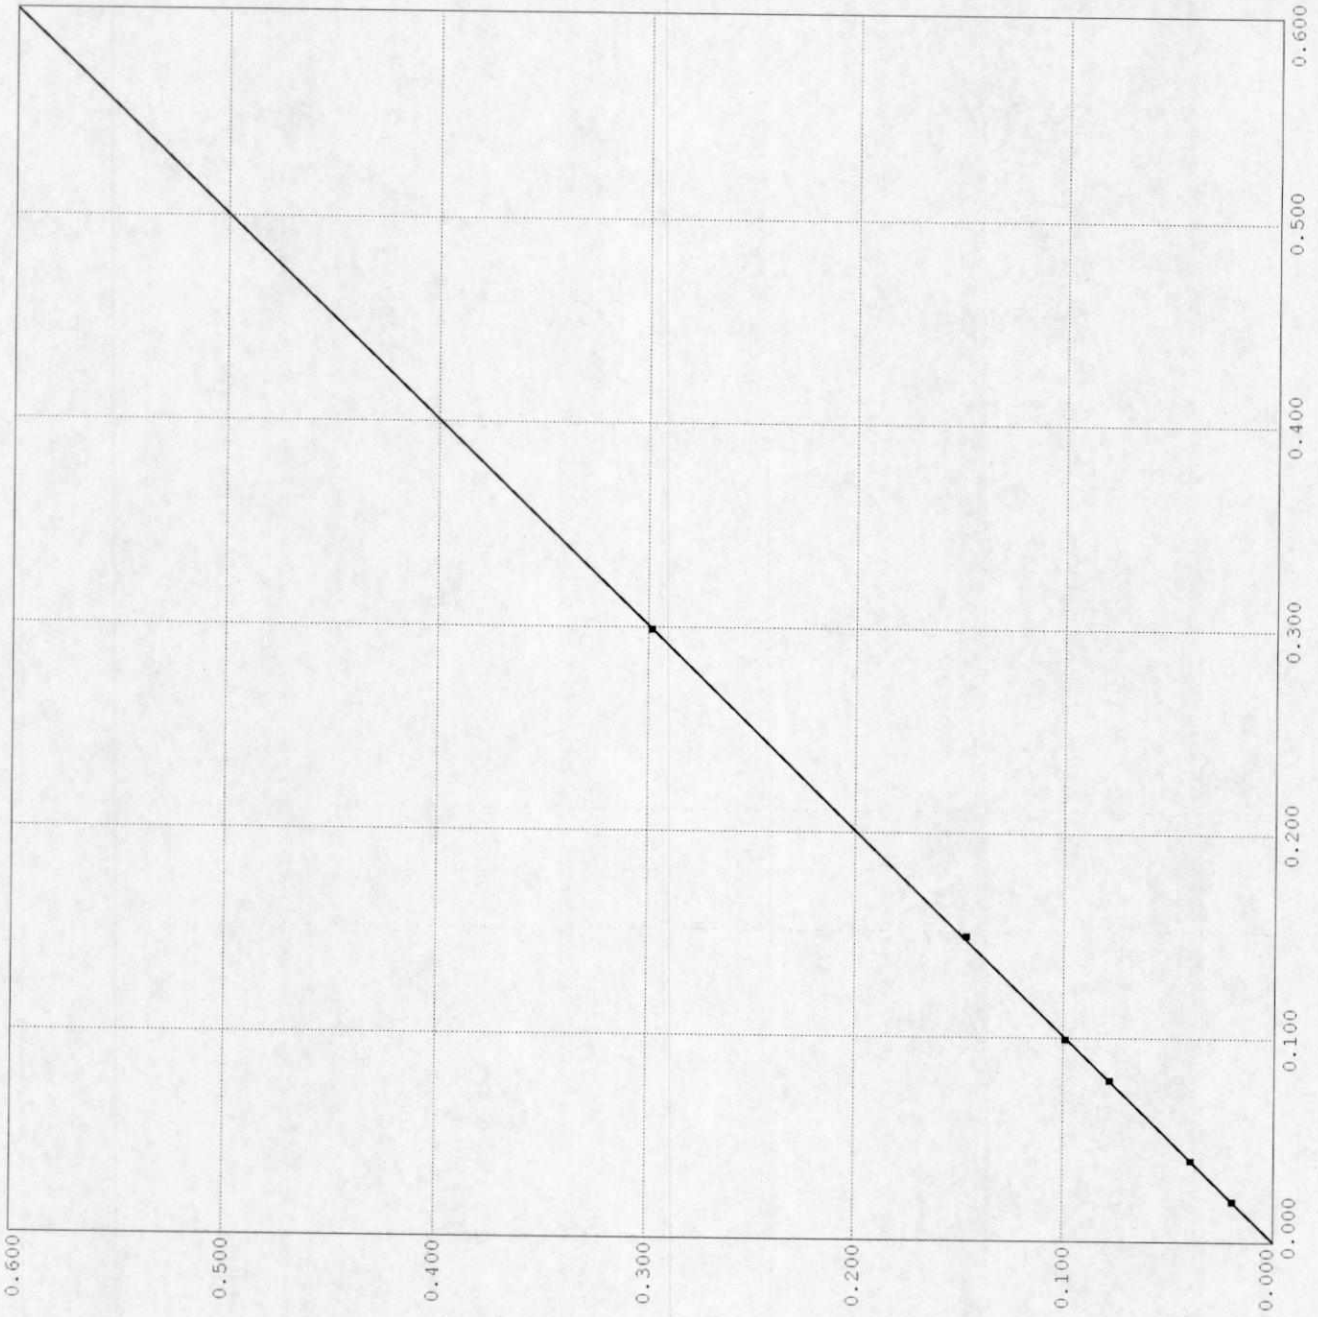

LINEARITY CHECK

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100417  
 -----  
 Date: 09/03/2024  
 Time: 12:18:33  
 -----  
 SUPERVISOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0004
0.040	0.0400	0.0000
0.079	0.0788	0.0004
0.099	0.1000	0.0000
0.149	0.1474	0.0005
0.298	0.2990	0.0000

SLOPE = 1.001989  
 R² = 0.999914

CKG

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100417






Date: 09/03/2024  
 Time: 12:18:35

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.71: 0.020  
 LOT #: AG408002  
 EXPIRATION: 03/20/2026  
 TANK PRESSURE: 433 psi

BLANK TEST	0.000	12:19
INTERNAL STANDARD	VERIFIED	12:20
EXTERNAL STANDARD	0.021	12:20
BLANK TEST	0.000	12:21
EXTERNAL STANDARD	0.020	12:21
BLANK TEST	0.000	12:22
EXTERNAL STANDARD	0.020	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.020	12:23
BLANK TEST	0.000	12:24
EXTERNAL STANDARD	0.020	12:24
BLANK TEST	0.000	12:25

Average = 0.0202  
 Std Dev = 0.0004

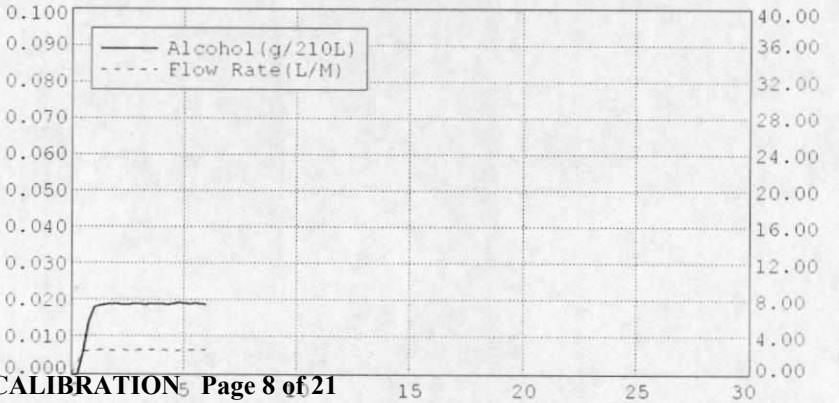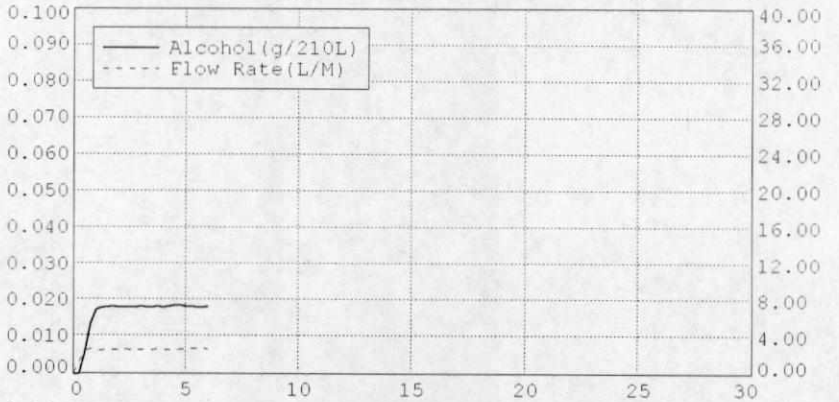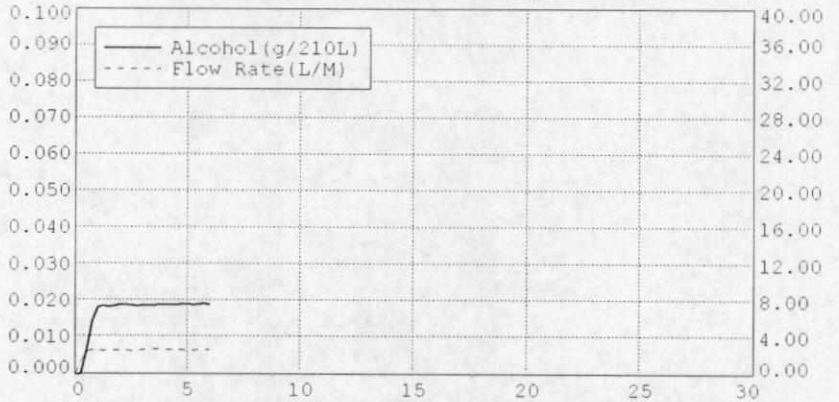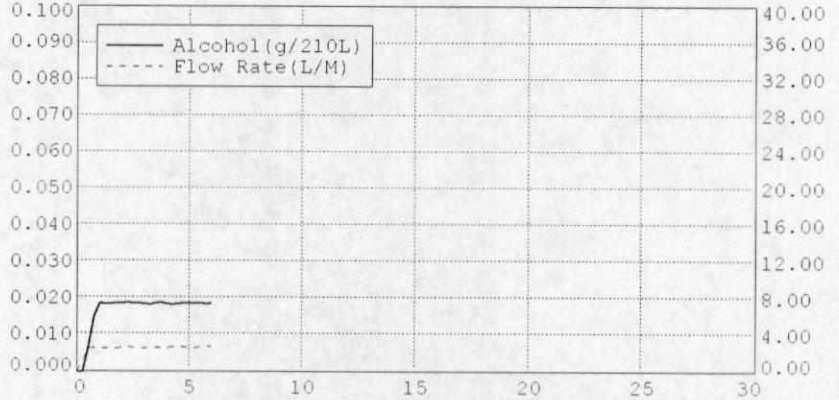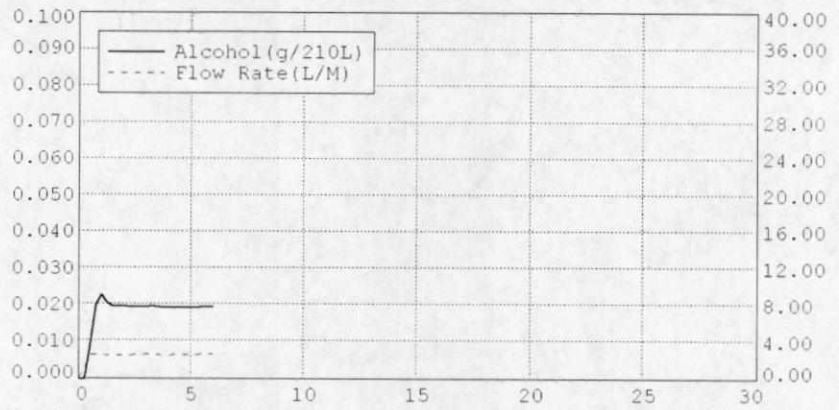



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100417






Date: 09/03/2024  
 Time: 12:26:18

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.70: 0.040  
 LOT #: AG407908  
 EXPIRATION: 03/19/2026  
 TANK PRESSURE: 1039 psi

BLANK TEST	0.000	12:27
INTERNAL STANDARD	VERIFIED	12:27
EXTERNAL STANDARD	0.040	12:28
BLANK TEST	0.000	12:28
EXTERNAL STANDARD	0.040	12:29
BLANK TEST	0.000	12:30
EXTERNAL STANDARD	0.040	12:30
BLANK TEST	0.000	12:31
EXTERNAL STANDARD	0.040	12:31
BLANK TEST	0.000	12:32
EXTERNAL STANDARD	0.040	12:32
BLANK TEST	0.000	12:33

Average = 0.0400  
 Std Dev = 0.0000

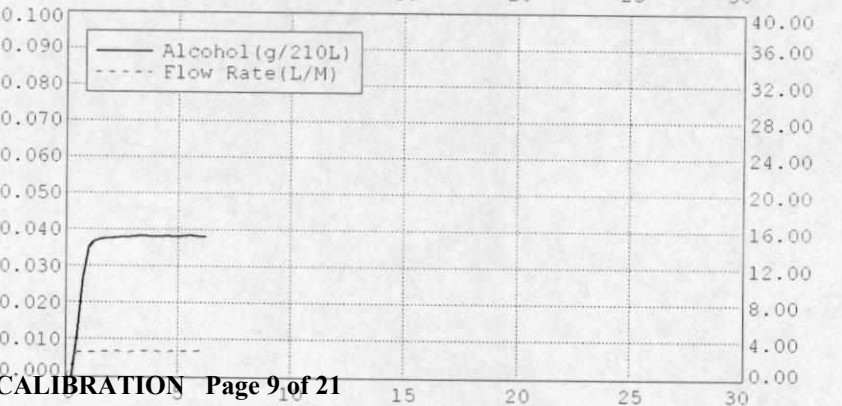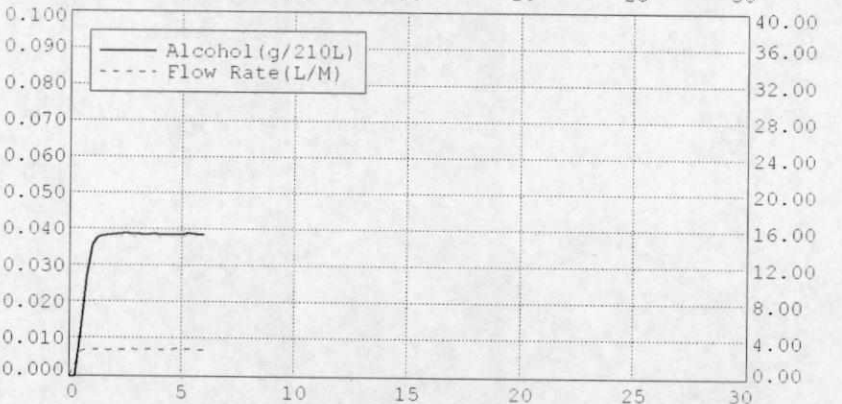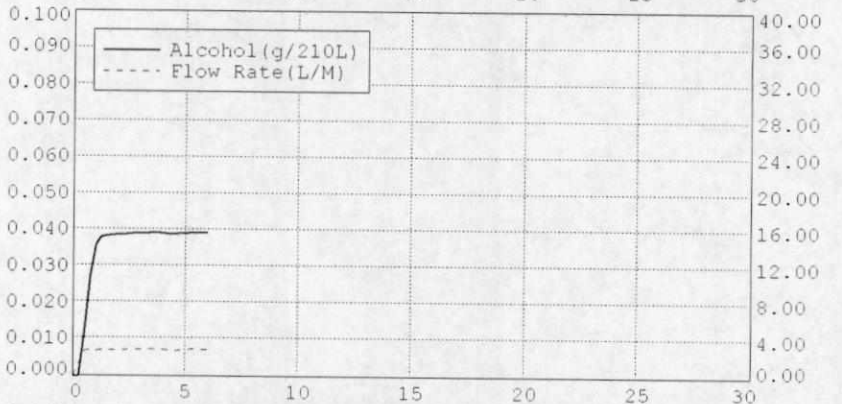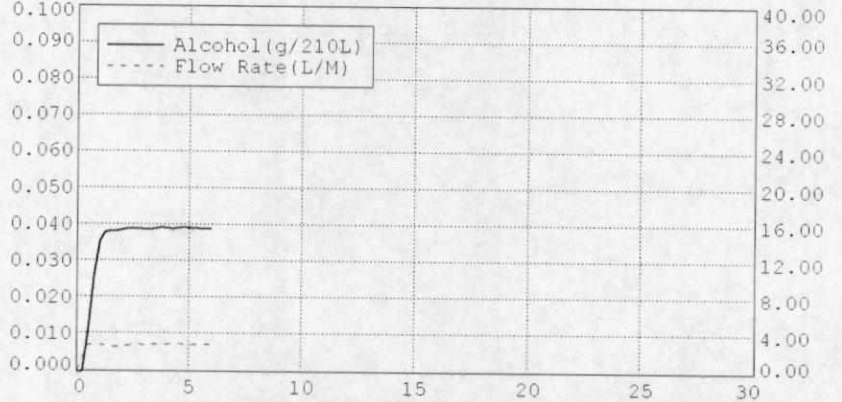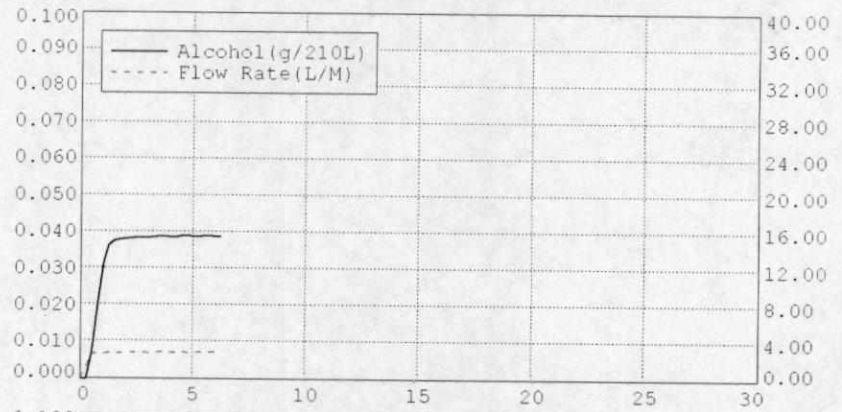

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100417






Date: 09/03/2024  
 Time: 12:34:25

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.70: 0.079  
 LOT #: AG310901  
 EXPIRATION: 04/19/2025  
 TANK PRESSURE: 250 psi

BLANK TEST	0.000	12:35
INTERNAL STANDARD	VERIFIED	12:35
EXTERNAL STANDARD	0.079	12:36
BLANK TEST	0.000	12:36
EXTERNAL STANDARD	0.079	12:37
BLANK TEST	0.000	12:38
EXTERNAL STANDARD	0.079	12:38
BLANK TEST	0.000	12:39
EXTERNAL STANDARD	0.079	12:39
BLANK TEST	0.000	12:40
EXTERNAL STANDARD	0.078	12:40
BLANK TEST	0.000	12:41

Average = 0.0788  
 Std Dev = 0.0004

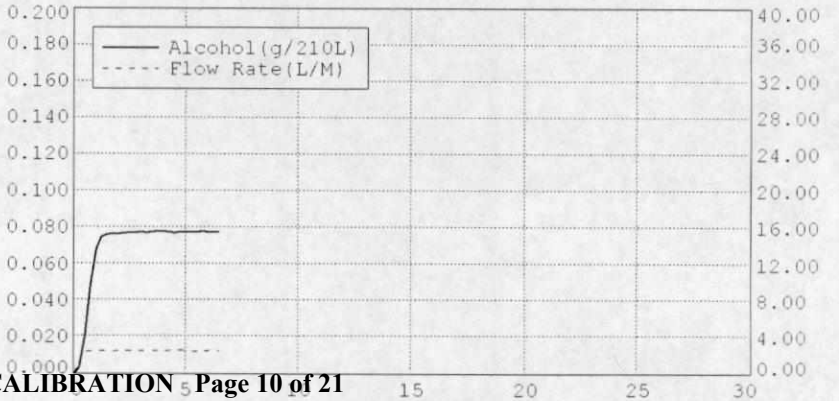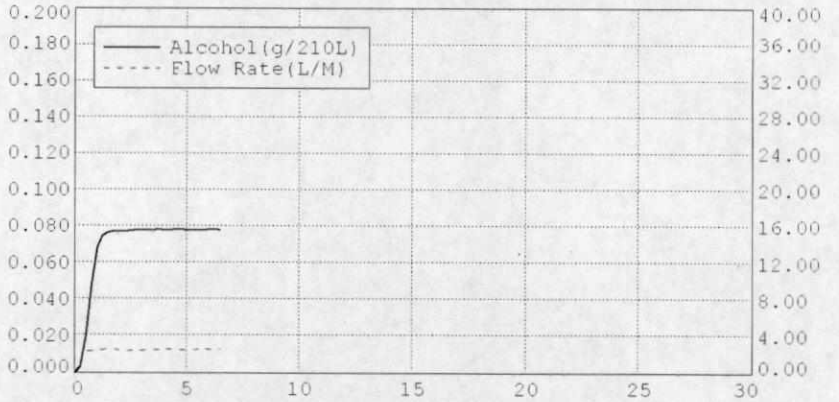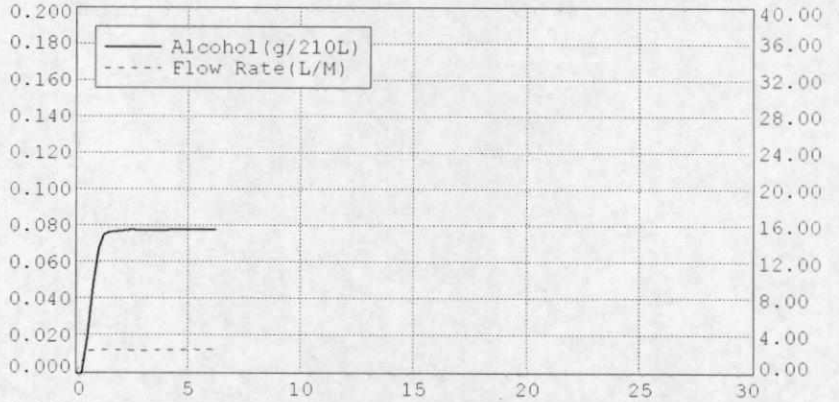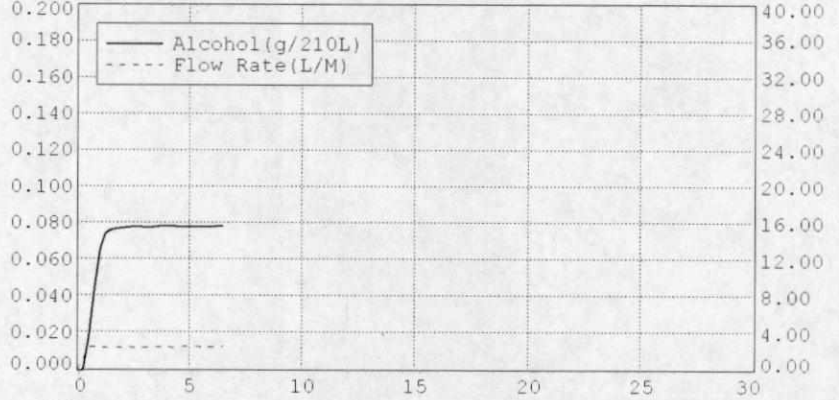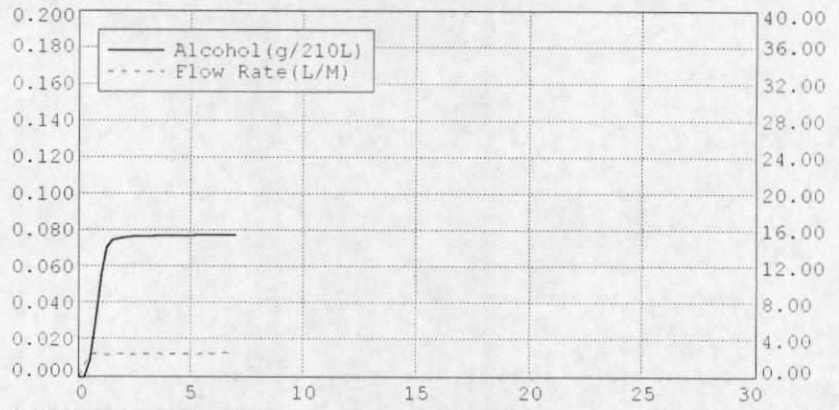

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
DATAMASTER dmt: 100417






Date: 09/03/2024  
Time: 12:42:14

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
TARGET AT 29.69: 0.099  
LOT #: AG333401  
EXPIRATION: 11/30/2025  
TANK PRESSURE: 810 psi

BLANK TEST	0.000	12:43
INTERNAL STANDARD	VERIFIED	12:43
EXTERNAL STANDARD	0.100	12:43
BLANK TEST	0.000	12:44
EXTERNAL STANDARD	0.100	12:44
BLANK TEST	0.000	12:45
EXTERNAL STANDARD	0.100	12:46
BLANK TEST	0.000	12:46
EXTERNAL STANDARD	0.100	12:47
BLANK TEST	0.000	12:48
EXTERNAL STANDARD	0.100	12:48
BLANK TEST	0.000	12:49

Average = 0.1000  
Std Dev = 0.0000

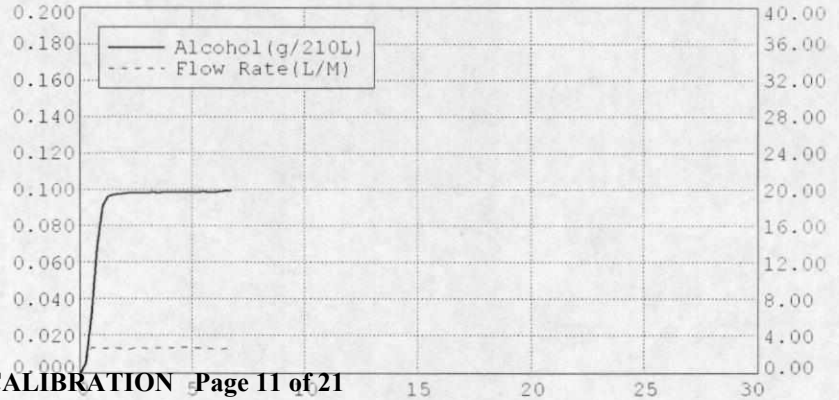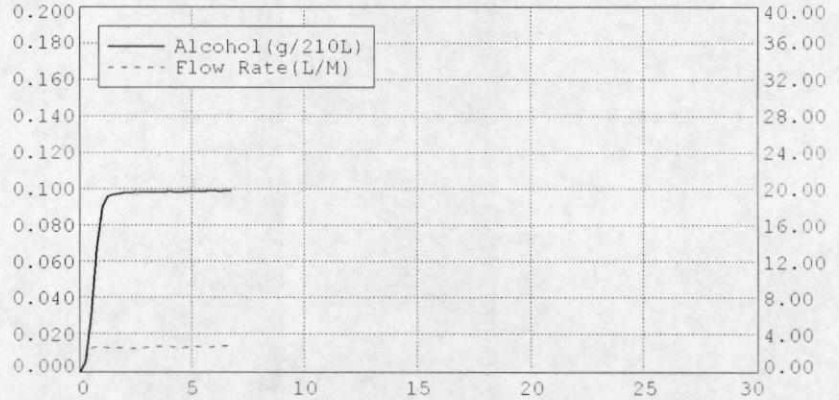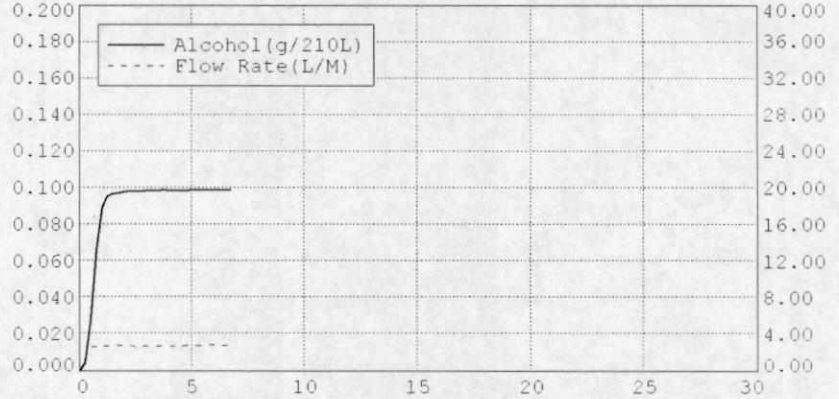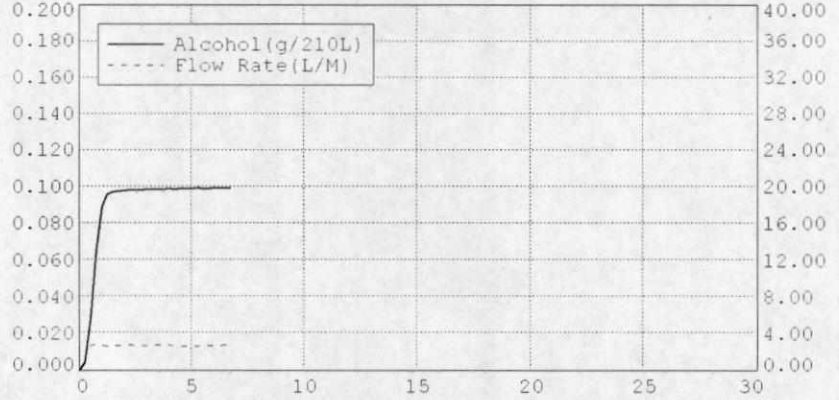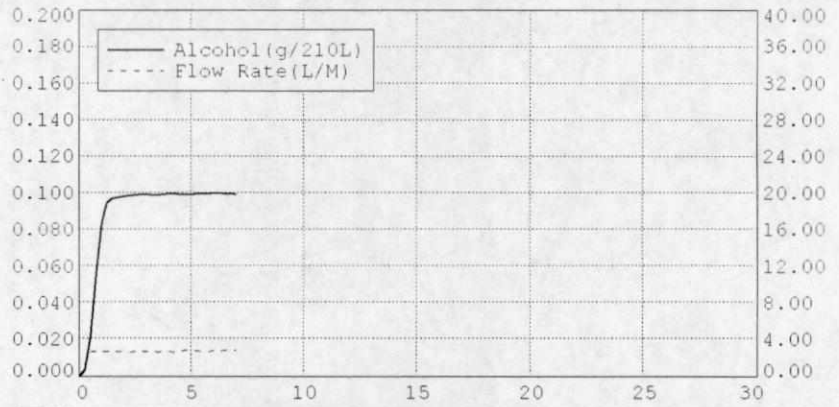

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100417






Date: 09/03/2024  
 Time: 12:50:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.69: 0.149  
 LOT #: AG332004  
 EXPIRATION: 11/16/2025  
 TANK PRESSURE: 434 psi

BLANK TEST	0.000	12:52
INTERNAL STANDARD	VERIFIED	12:52
EXTERNAL STANDARD	0.148	12:52
BLANK TEST	0.000	12:53
EXTERNAL STANDARD	0.147	12:53
BLANK TEST	0.000	12:54
EXTERNAL STANDARD	0.147	12:54
BLANK TEST	0.000	12:55
EXTERNAL STANDARD	0.148	12:55
BLANK TEST	0.000	12:56
EXTERNAL STANDARD	0.147	12:56
BLANK TEST	0.000	12:57

Average = 0.1474  
 Std Dev = 0.0005

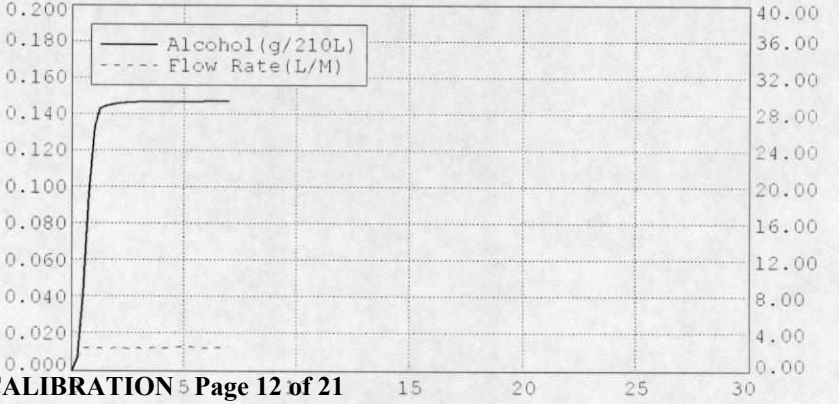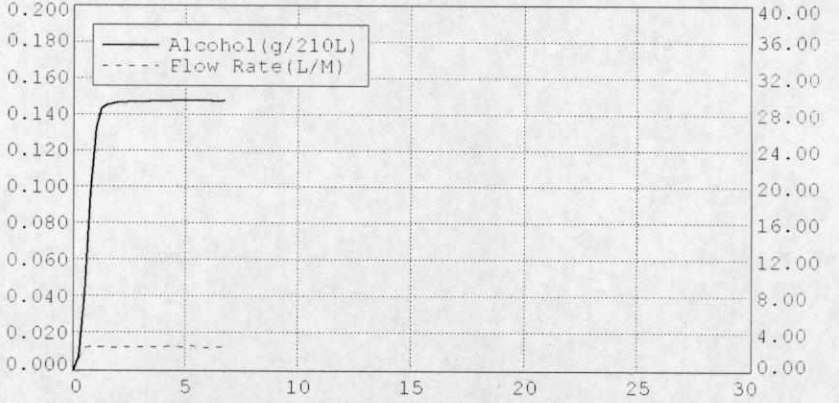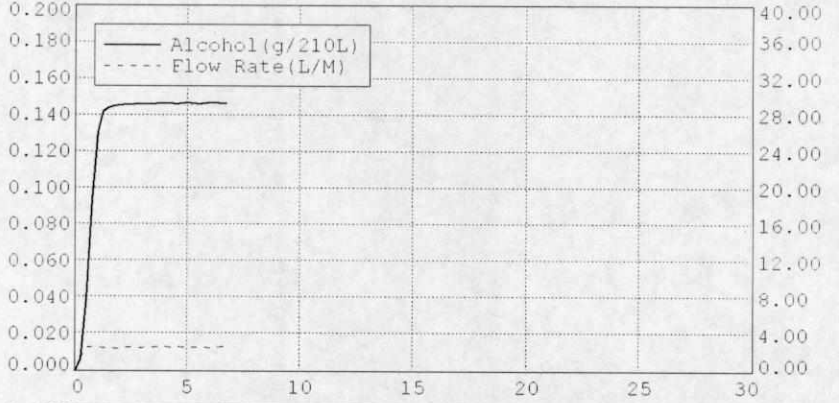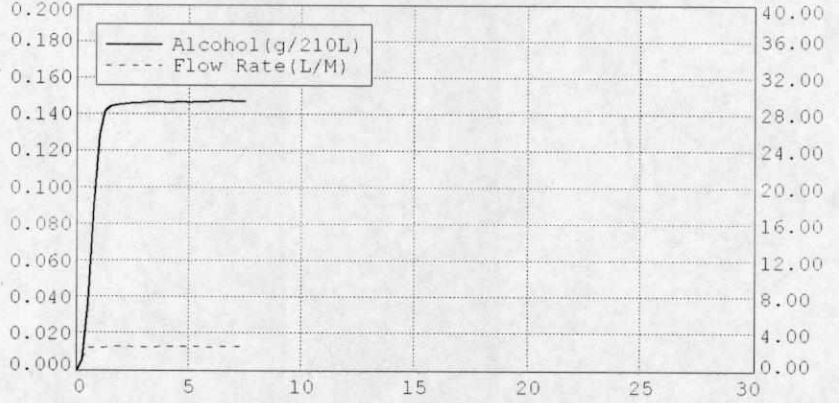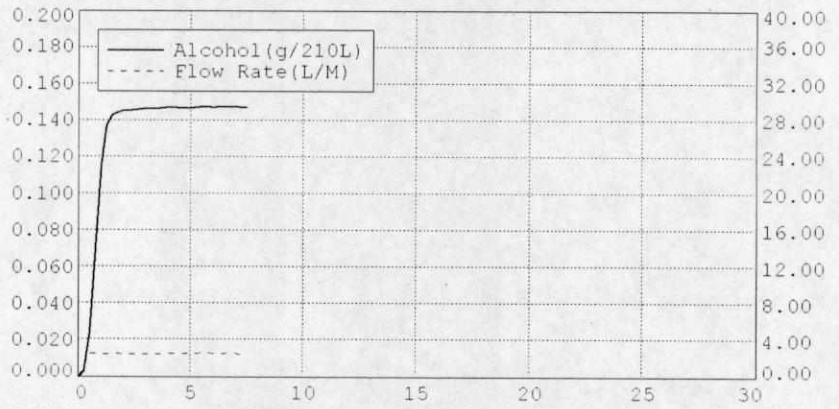

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100417






Date: 09/03/2024  
 Time: 12:58:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.69: 0.298  
 LOT #: AG327804  
 EXPIRATION: 10/05/2025  
 TANK PRESSURE: 154 psi

BLANK TEST	0.000	12:59
INTERNAL STANDARD	VERIFIED	12:59
EXTERNAL STANDARD	0.299	12:59
BLANK TEST	0.000	13:00
EXTERNAL STANDARD	0.299	13:01
BLANK TEST	0.000	13:02
EXTERNAL STANDARD	0.299	13:02
BLANK TEST	0.000	13:03
EXTERNAL STANDARD	0.299	13:03
BLANK TEST	0.000	13:04
EXTERNAL STANDARD	0.299	13:04
BLANK TEST	0.000	13:05

Average = 0.2990  
 Std Dev = 0.0000

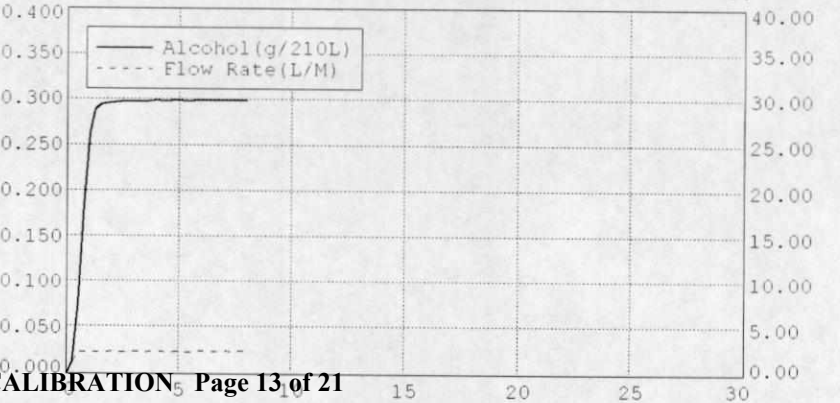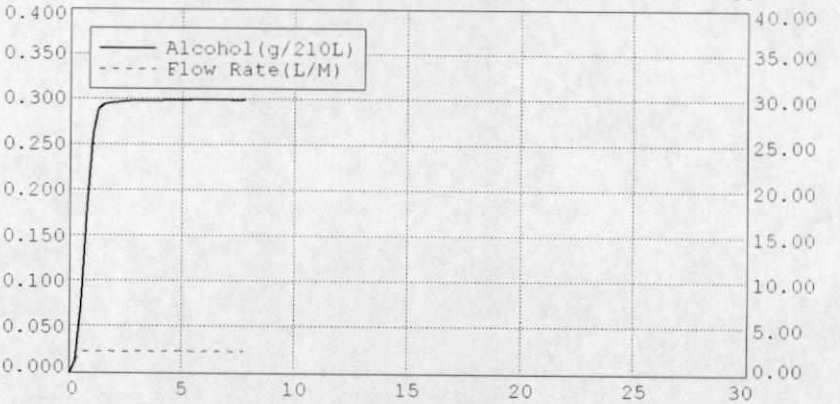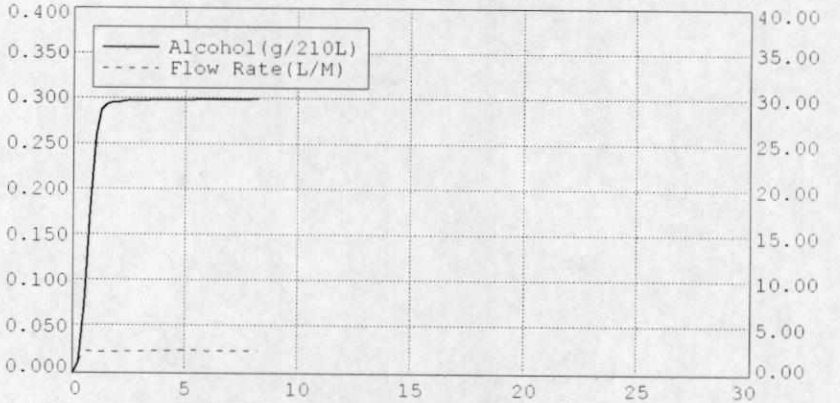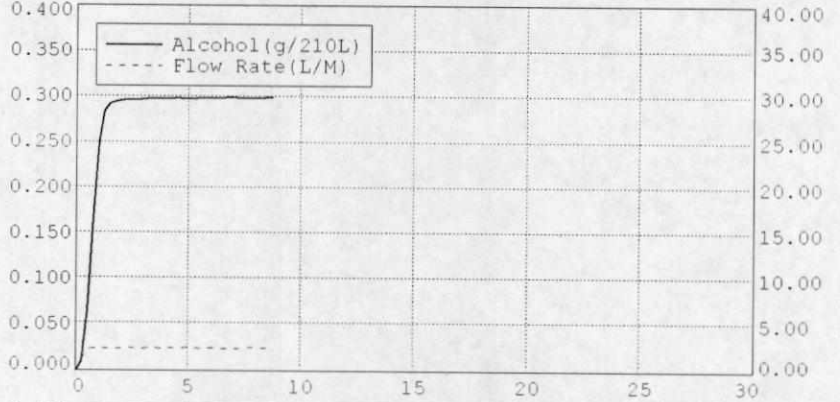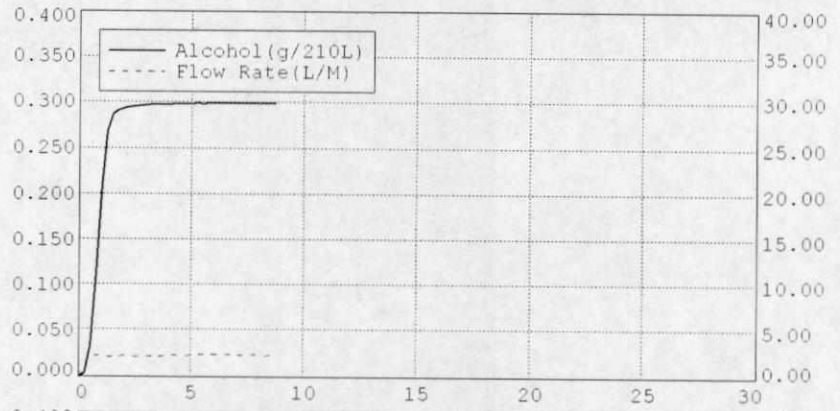

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100417

Date: 09/03/2024  
Time: 13:14:27


SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 13:15  
BLANK TEST 0.000 13:15  
INTERNAL STANDARD VERIFIED 13:15  
EXTERNAL STANDARD 0.080 13:16  
BLANK TEST 0.000 13:17  
SUBJECT SAMPLE INCOMPLETE 13:19

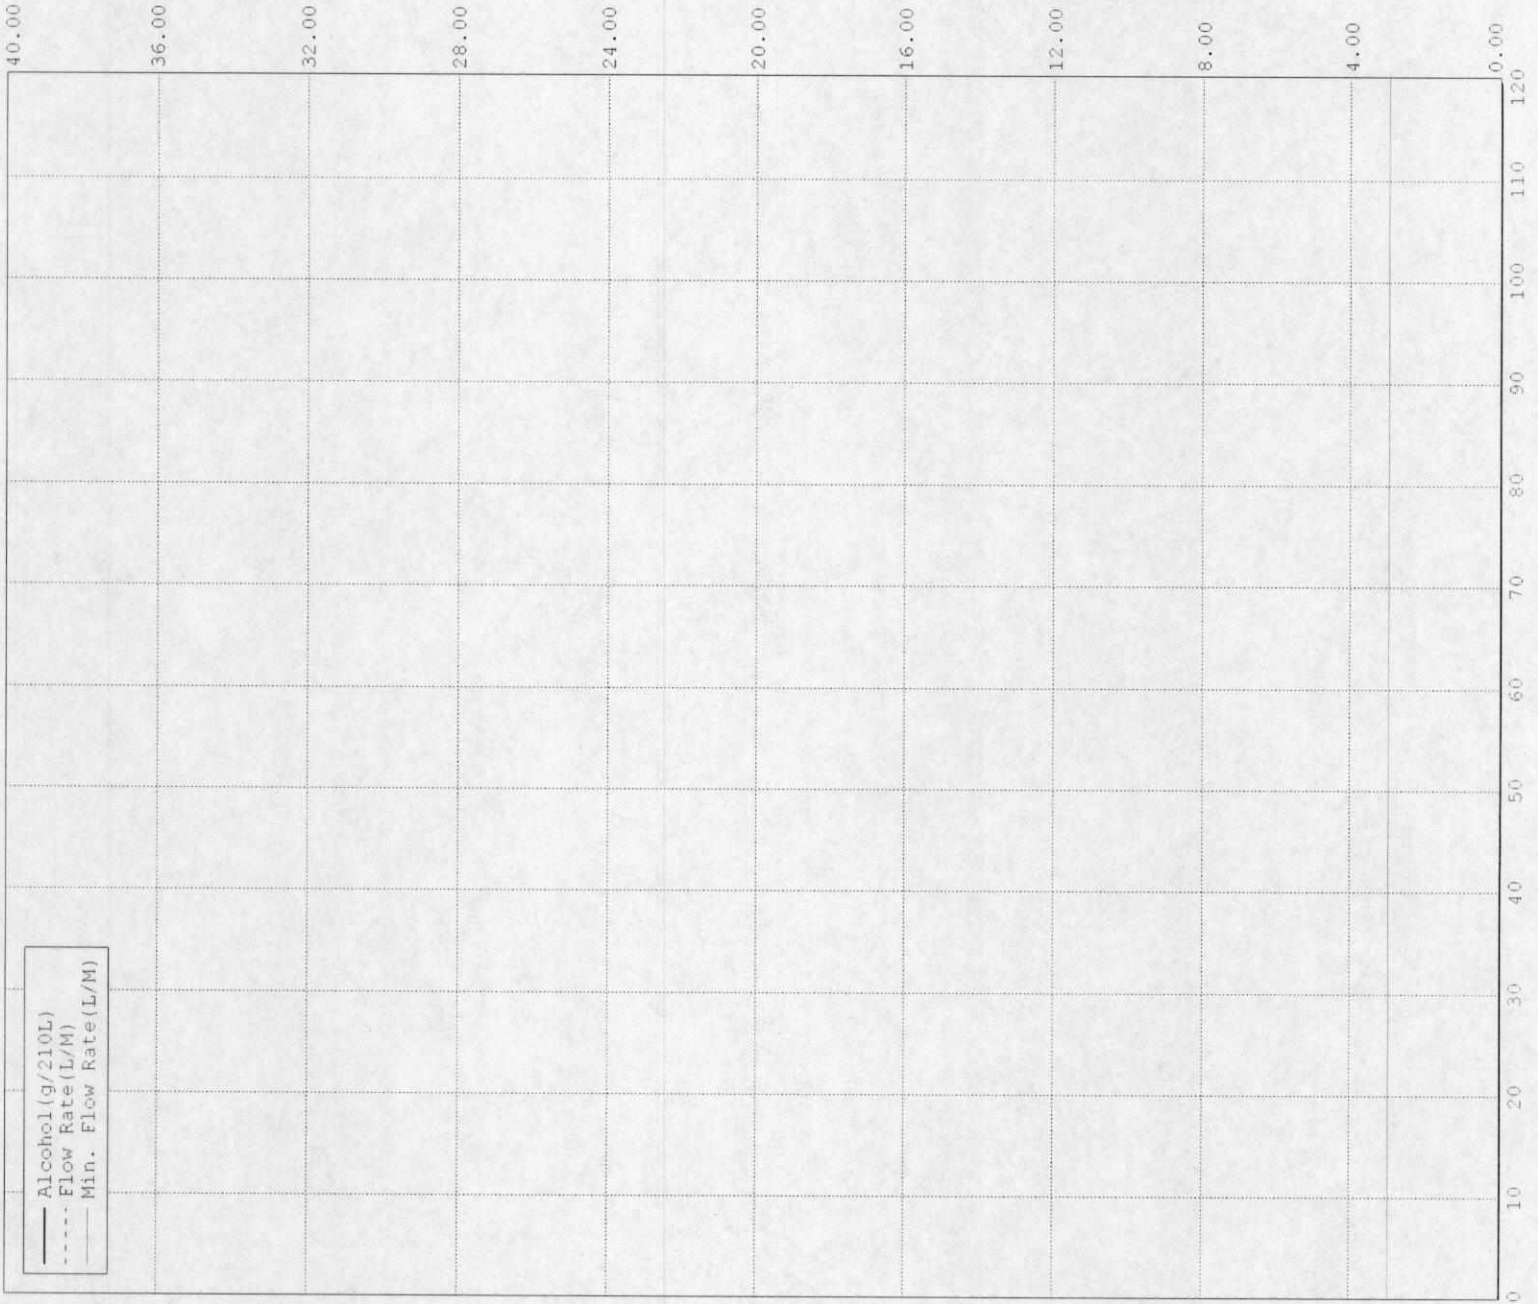

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100417

Date: 09/03/2024  
Time: 13:25:41

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
MAXIMUM ATTEMPTS EXCEEDED  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 13:27  
BLANK TEST 0.000 13:27  
INTERNAL STANDARD VERIFIED 13:27  
EXTERNAL STANDARD 0.080 13:27  
BLANK TEST 0.000 13:28  
SUBJECT SAMPLE XXX 13:29

Maximum Attempts Exceeded

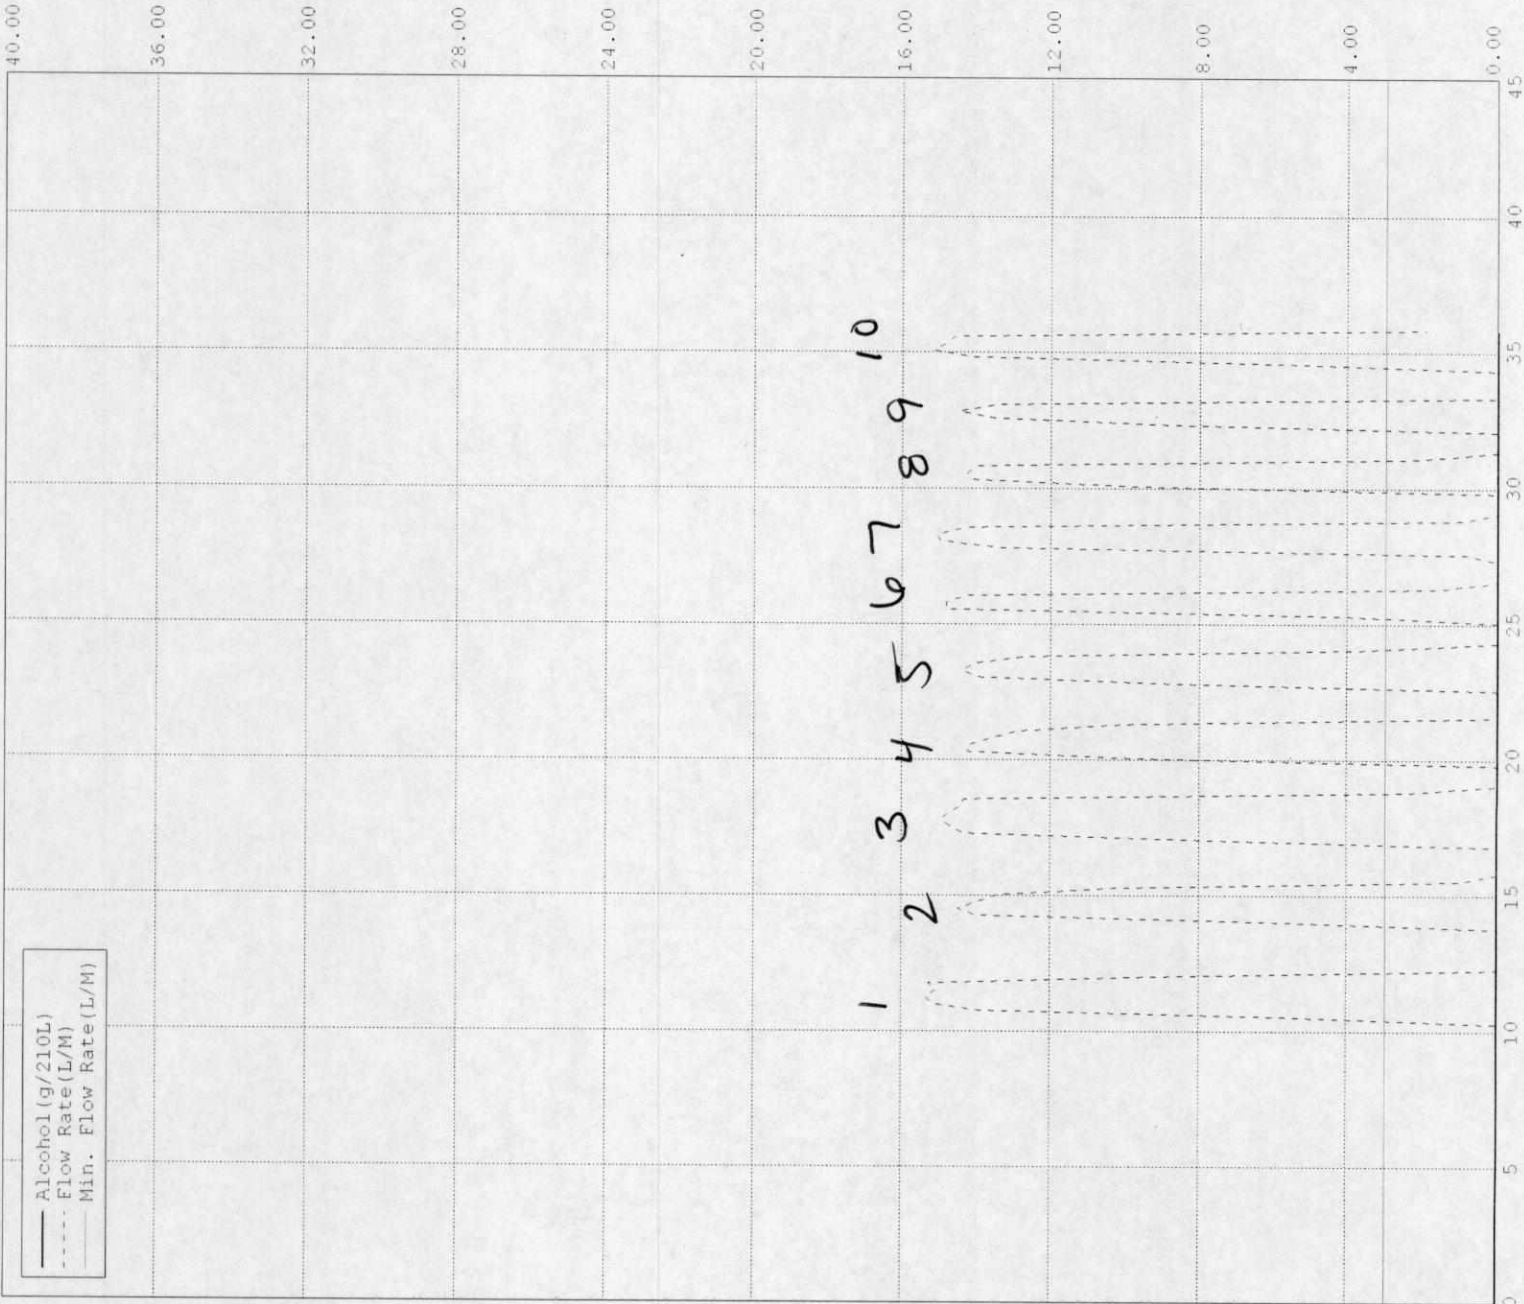

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100417

Date: 09/03/2024  
Time: 13:33:18

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:

INVALID  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	13:34
BLANK TEST	0.000	13:34
INTERNAL STANDARD	VERIFIED	13:35
EXTERNAL STANDARD	0.079	13:35
BLANK TEST	0.000	13:36
SUBJECT SAMPLE	INVALID	13:36

CVG





SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100417

Date: 09/03/2024  
Time: 13:43:34

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
RFI  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 13:44  
BLANK TEST 0.000 13:44  
INTERNAL STANDARD VERIFIED 13:44  
EXTERNAL STANDARD 0.080 13:45  
BLANK TEST 0.000 13:46

RFI DETECTED



SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100417  
-----

Date: 09/03/2024  
Time: 13:57:29

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE - ACETONE  
BASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 13:58  
BLANK TEST 0.000 13:58  
INTERNAL STANDARD VERIFIED 13:58  
Xq = 0.095 (1.39%) 0.079 13:58  
EXTERNAL STANDARD (0.0023)  
X[1] = 0.0791 (-0.0003) 0.000 13:59  
BLANK TEST XXX 14:00  
SUBJECT SAMPLE X[1] = 0.1128 (-0.0216) (0.0001)

Interference Detected

Filter 2 Avg: -0.0003  
Filter 3 Avg: 0.0010  
066-9/13/2024

CKG



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100417

Date: 09/03/2024  
Time: 14:04:01

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE - IPA  
CASE/REPORT: XXXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:05
BLANK TEST	0.000	14:05
INTERNAL STANDARD	VERIFIED	14:05
Xq = 0.096 (1.58%)		
EXTERNAL STANDARD	0.079	14:05
X[1] = 0.0791 (-0.0008)	(-0.0001)	
BLANK TEST	0.000	14:06
SUBJECT SAMPLE	XXX	14:07
X[1] = 0.1239 (-0.0269)	(-0.0002)	

Interference Detected

CKG

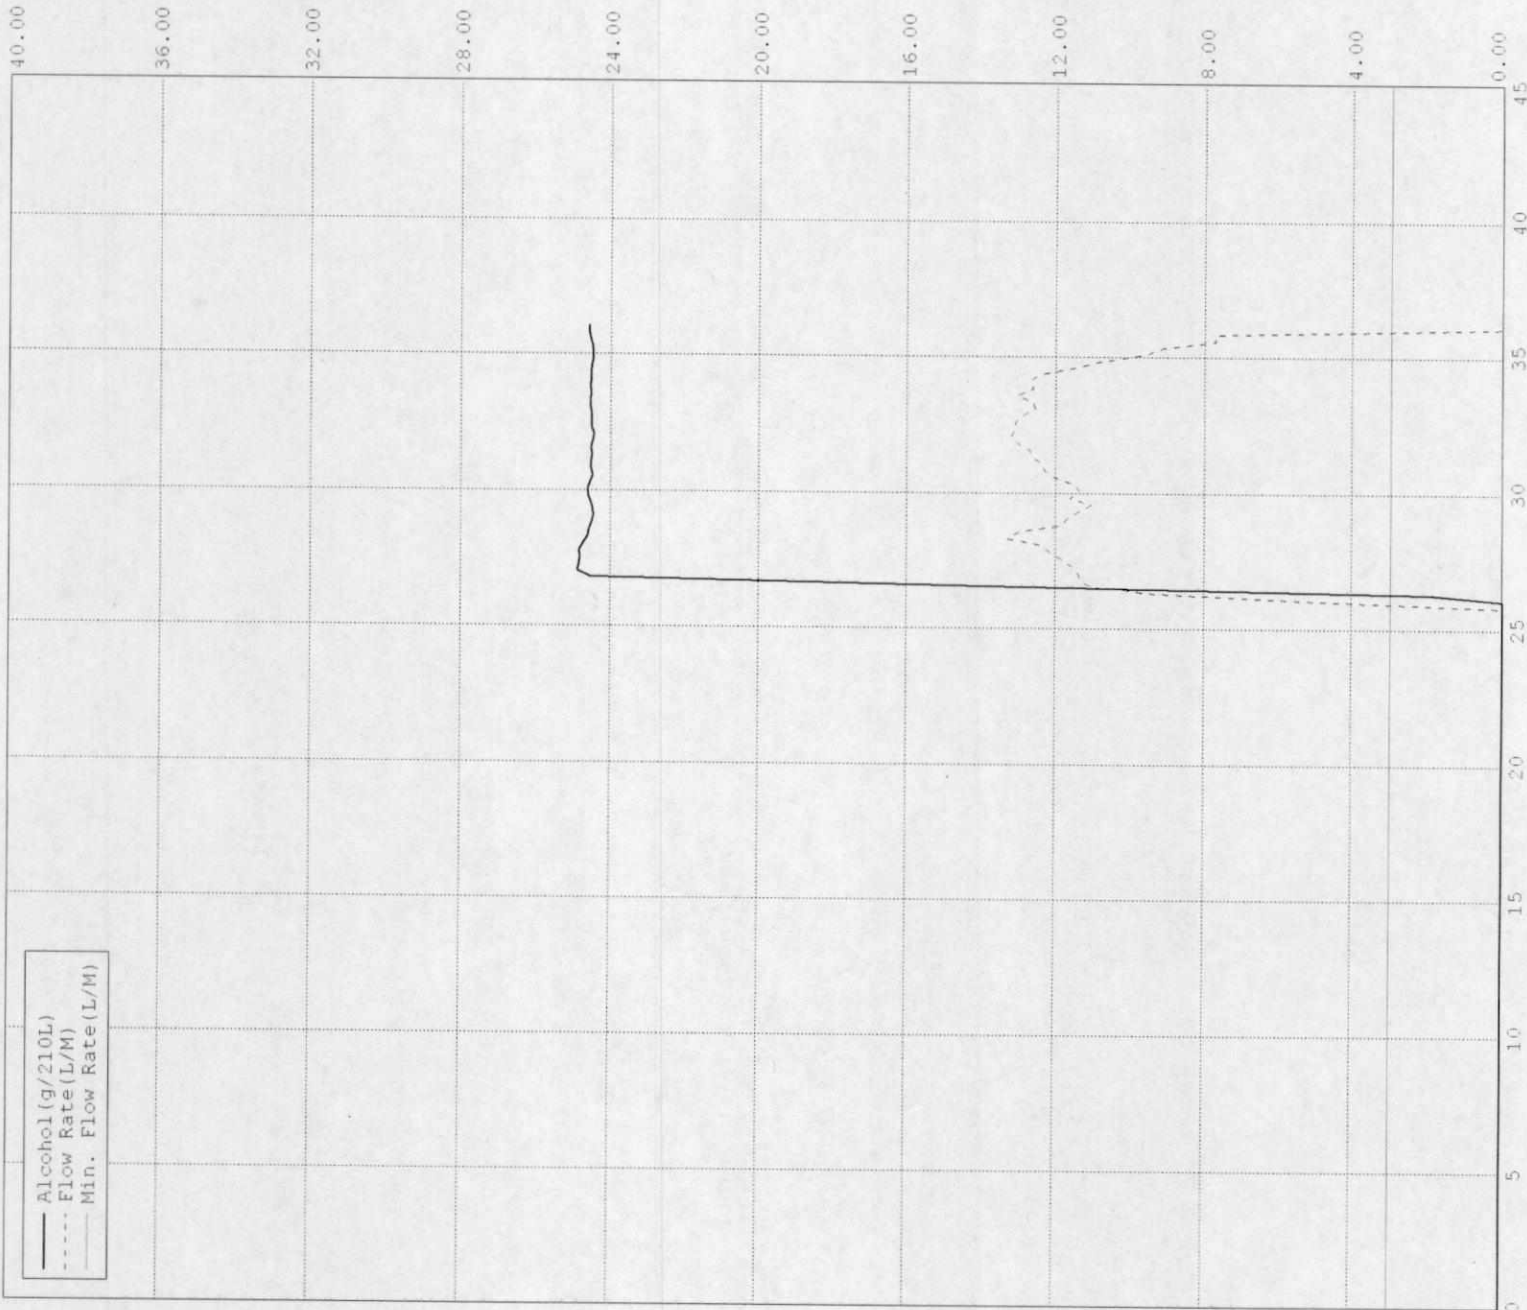

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100417

Date: 09/03/2024  
Time: 14:09:54

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE - NEGATIVE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:11
BLANK TEST	0.000	14:11
INTERNAL STANDARD	VERIFIED	14:11
$X_q = 0.096$ (1.49%)		
EXTERNAL STANDARD	0.079	14:11
$X[1] = 0.0792$ (-0.0001) (0.0014)		
BLANK TEST	0.000	14:12
SUBJECT SAMPLE (Vol=1.80L)	0.097	14:13
$X[1] = 0.0979$ (0.0001) (-0.0009)		
BLANK TEST	0.000	14:14
EXTERNAL STANDARD	0.079	14:14
$X[1] = 0.0788$ (0.0002) (0.0005)		
BLANK TEST	0.000	14:15

*Handwritten signature/initials*

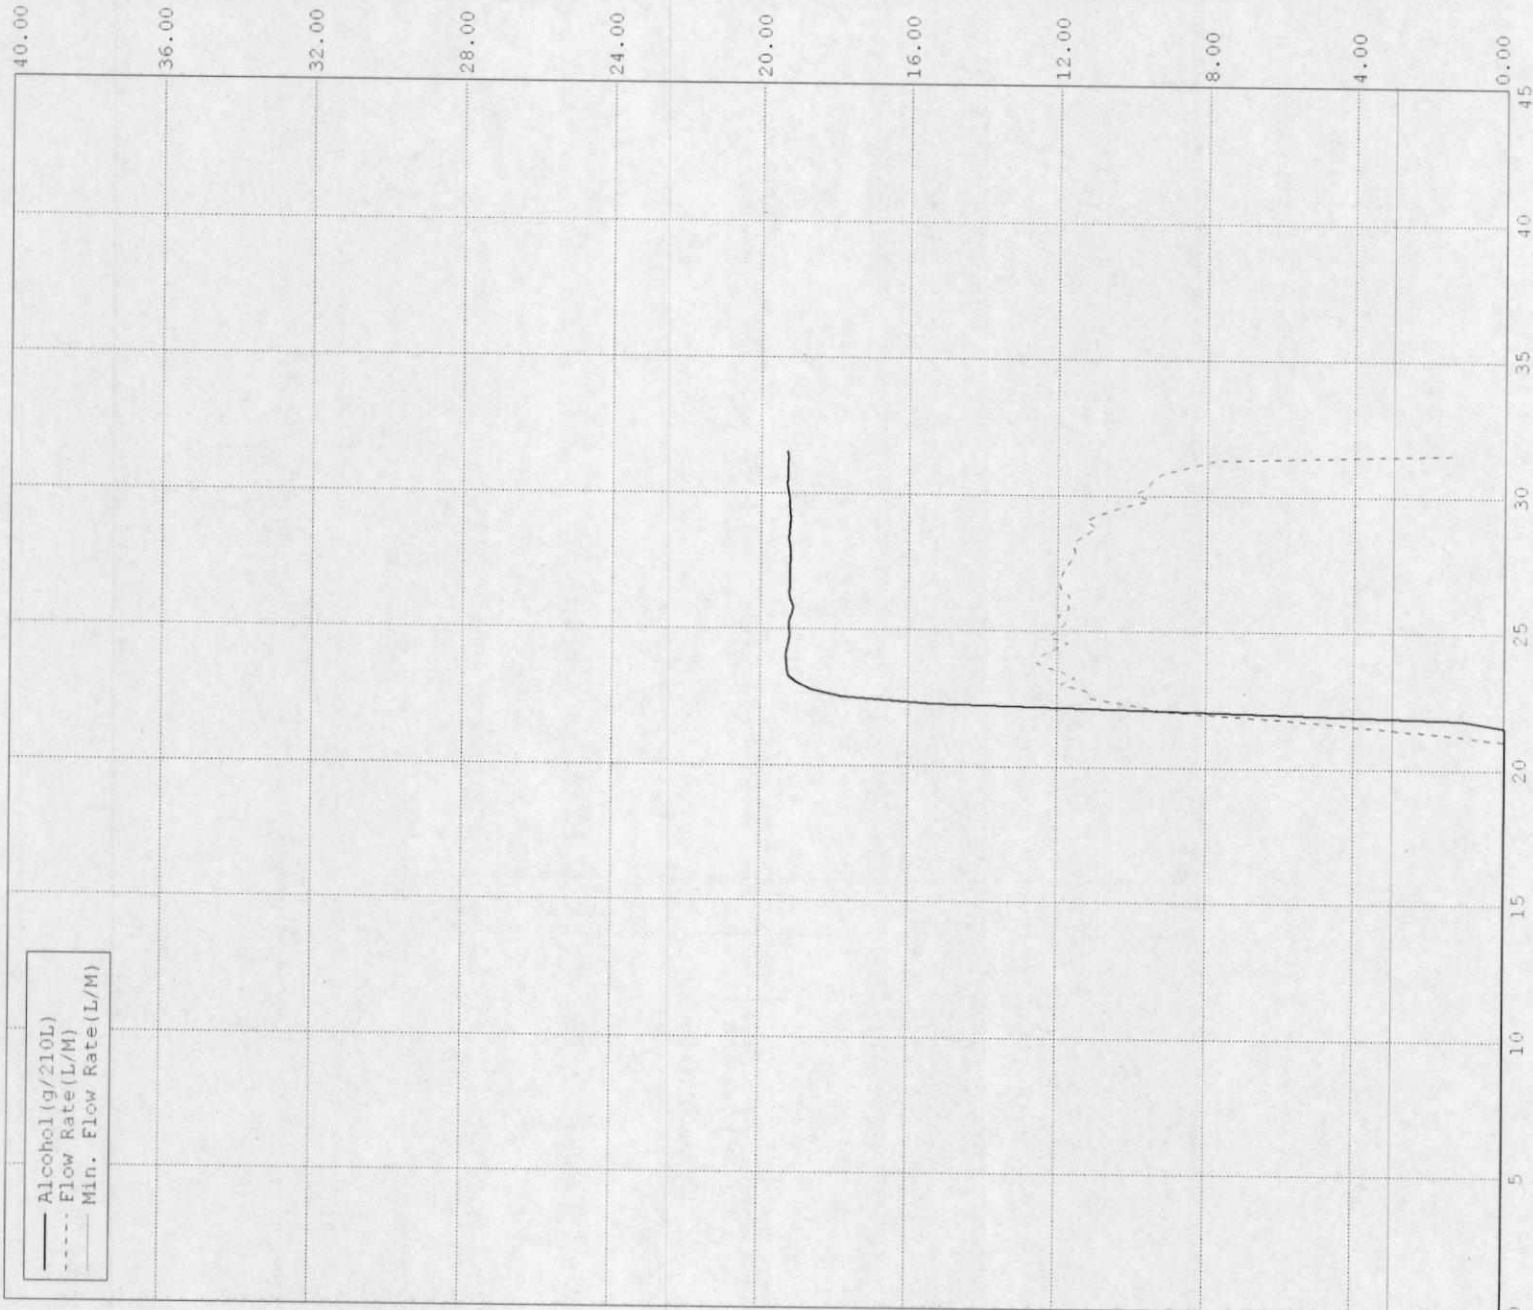

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100417

Date: 09/03/2024  
Time: 14:35:04

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY: NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:36
BLANK TEST	0.000	14:36
INTERNAL STANDARD	VERIFIED	14:36
EXTERNAL STANDARD	0.079	14:36
BLANK TEST	0.000	14:37
SUBJECT SAMPLE (Vol=1.95L)	0.000	14:38
BLANK TEST	0.000	14:39
EXTERNAL STANDARD	0.079	14:39
BLANK TEST	0.000	14:40

CKG

