

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100400

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 02/20/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.74: 0.080
LOT #: 09214080A3
EXPIRATION: 05/01/2016
TANK PRESSURE: 506 psi

BLANK TEST	0.000	10:42
INTERNAL STANDARD	VERIFIED	10:42
EXTERNAL STANDARD	0.078	10:42
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.079	10:43
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.079	10:44
BLANK TEST	0.000	10:45
EXTERNAL STANDARD	0.079	10:46
BLANK TEST	0.000	10:46
EXTERNAL STANDARD	0.079	10:47
BLANK TEST	0.000	10:48

Average = 0.0788
Std Dev = 0.0004

Diagnostic Check

VERSIONS

DMT: 3.00
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
Breath Tube = 48.1°C PASSED

PUMP INFO

Flow Rate = 4.435 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

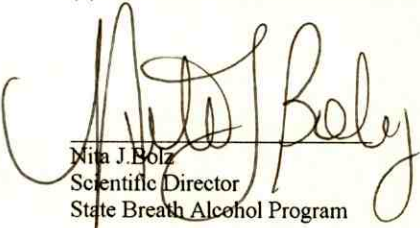
FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

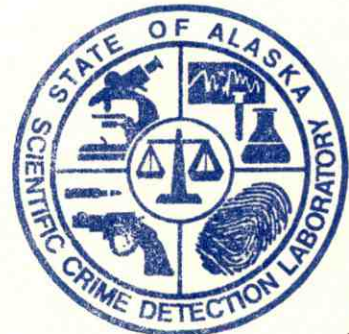
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.



Nita J. Bolz
Scientific Director
State Breath Alcohol Program

3/12/2015

Subscribed and sworn before me this 12th day of Mar, 20 15


Nikki Roth, Notary Public
My Commission Expires With Office




DWB
3/12/15