

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100666

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 12/02/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: 01315080A3
EXPIRATION: 02/05/2017
TANK PRESSURE: 767 psi

BLANK TEST	0.000	15:37
INTERNAL STANDARD	VERIFIED	15:37
EXTERNAL STANDARD	0.079	15:38
BLANK TEST	0.000	15:39
EXTERNAL STANDARD	0.079	15:39
BLANK TEST	0.000	15:40
EXTERNAL STANDARD	0.079	15:40
BLANK TEST	0.000	15:41
EXTERNAL STANDARD	0.079	15:41
BLANK TEST	0.000	15:42
EXTERNAL STANDARD	0.079	15:42
BLANK TEST	0.000	15:43

Average = 0.0790
Std Dev = 0.0000

Diagnostic Check

VERSIONS

DMT: 3.01
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
Breath Tube = 46.2°C PASSED

PUMP INFO

Flow Rate = 4.832 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED


FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:



- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

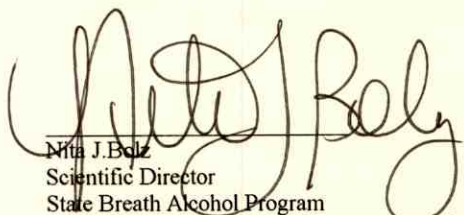
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

12/16/2015

Subscribed and sworn before me this 16th day of Dec. 20 15


Nikki Roth, Notary Public
My Commission Expires With Office

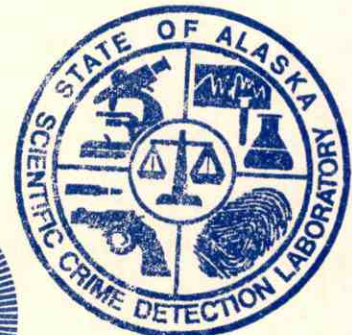

CBS 12/3/15