

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100390

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 12/14/2016

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 30.04: 0.080  
LOT #: 01315080A2  
EXPIRATION: 02/05/2017  
TANK PRESSURE: 855 psi

BLANK TEST	0.000	10:07
INTERNAL STANDARD	VERIFIED	10:07
EXTERNAL STANDARD	0.080	10:07
BLANK TEST	0.000	10:08
EXTERNAL STANDARD	0.081	10:08
BLANK TEST	0.000	10:09
EXTERNAL STANDARD	0.080	10:09
BLANK TEST	0.000	10:10
EXTERNAL STANDARD	0.081	10:10
BLANK TEST	0.000	10:11
EXTERNAL STANDARD	0.080	10:12
BLANK TEST	0.000	10:12

Average = 0.0804  
Std Dev = 0.0005

## Diagnostic Check

### VERSIONS

DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.7°C PASSED  
Breath Tube = 48.1°C PASSED

### PUMP INFO

Flow Rate = 4.846 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED


### FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED


I, Charles R. Foster, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

 12/23/16

Charles R. Foster  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 23<sup>rd</sup> day of Dec 20 16

  
Nikki Roth, Notary Public  
My Commission Expires With Office

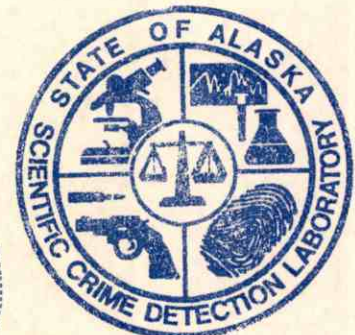

BMB  
12/20/16