



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100348

Report Issue Date: 07/15/2024
Date Received: 2024-06-10
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.019	0.019	0.019	0.019	0.019	0.019	0.019
0.080	0.079	AG335202	0.077	0.077	0.077	0.077	0.077	0.077	0.077
0.300	0.296	AG327804	0.289	0.289	0.290	0.290	0.290	0.290	0.290

As Found - Evaluation Analyst: Kaija Swisher

As Found Conditions - Barometric Pressure (inHg): 29.58 Barometer Used: Fisher S/N 230307229 Temperature (C): 22.5 Relative Humidity (%): 31

As-Found Lab Activity Date Range: 06/10/2024 - 06/14/2024

Replaced O-Ring. Supervised casework with Derek Walton.

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG217902	0.020	0.020	0.019	0.020	0.020	0.020	+/- 0.002	
0.040	0.040	AG217904	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003	
0.080	0.080	AG335202	0.078	0.078	0.079	0.078	0.078	0.078	+/- 0.004	
0.100	0.100	AG333401	0.098	0.098	0.098	0.098	0.098	0.098	+/- 0.004	
0.150	0.150	AG332004	0.145	0.145	0.145	0.145	0.145	0.145	+/- 0.005	
0.300	0.299	AG327804	0.293	0.293	0.294	0.294	0.294	0.294	+/- 0.011	

As Left Conditions - Barometric Pressure (inHg): 29.83 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.3 Relative Humidity (%): 37

As-Left Lab Activity Date Range: 06/13/2024 - 07/12/2024

Supervised casework with Kaija Swisher.

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Derek Walton on 07/12/2024

derek.walton@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 07/15/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100348 Analyst or Technician Name: Kaija Swisher

DataMaster DMT Calibration Start Date: 6/13/24

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

*Supervised calibration with
Derek Watten 06/24/24
Jm*

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: May 2, 2025
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.83 Temperature(C) 20.3 Relative Humidity(%) 37

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

- ✓ 1. Acetone Reagent Lot Number: 20240501KS Expiration Date: 8/1/24
Simulator S/N: SD1088 Thermometer Verification Performed?
- ✓ 2. Isopropanol Reagent Lot Number: 20240501MNC Expiration Date: 8/1/24
Simulator S/N: D24161 Thermometer Verification Performed?
- ✓ 3. Negative (Ethanol Only) Lot Number: 22HP41201 Expiration Date: 8/1/24
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: Sept. 19, 2025

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 6/13/24

Data Interpretation Date (Technician): _____ (if applicable)

Data Interpretation Date (Analyst): 6/13/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 06/13/2024
Time: 07:19:07

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 42.2°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.71 V PASSED
(1.01 V - 2.35 V)
Cooler Voltage = 1.79 V PASSED
(1.04 V - 2.44 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 535 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 30.0 in

PUMP INFO

Flow Rate = 4.495 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.091 1.96% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100348

Date: 06/13/2024
Time: 7:27 AM

Temperatures (°C)

Sample Cell: 48.9°C
Breath Tube: 42.3°C

Current Barometer 29.8 in
Volume (Ltr) 1.45

Settings

Lamp: 1.79 V
Bias: 80 V
Cooler: 1.74 V
Chopper: 535 Hz

Voltages (V)

Flow: 1.03 V
Detector: -0.007 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 09/20/2018
Time: 14:41:22

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca = 0.1000
CAL = 0.951429 0.800 <= CAL < 1.200
b1 = 0.0003 0.0000 <= b1 < 0.0040
b2 = 0.0052 0.0010 <= b2 < 0.0100
b3 = 0.0004 0.0000 <= b3 < 0.0040
Xq = 0.0893 0.0500 <= Xq < 0.2000
a21 = 1.182097 1.050 <= a21 < 1.300
a31 = 0.540738 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100348

Date: 06/13/2024
 Time: 07:29:39

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX


OPERATOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

Lot # AG 335202
 Exp 12/18/25
 KS 6/14/24

DEPT/AGENCY:
 MINIMUM VOLUME TEST
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK	PASSED	07:31
INTERNAL STANDARD	0.000	07:31
EXTERNAL STANDARD	0.078	07:31
INTERNAL STANDARD	0.000	07:32
EXTERNAL STANDARD	0.000	07:32
INTERNAL STANDARD	0.000	07:33
EXTERNAL STANDARD	0.000	07:33
INTERNAL STANDARD	0.078	07:34
EXTERNAL STANDARD	0.000	07:34
INTERNAL STANDARD	0.000	07:35
EXTERNAL STANDARD	0.000	07:35

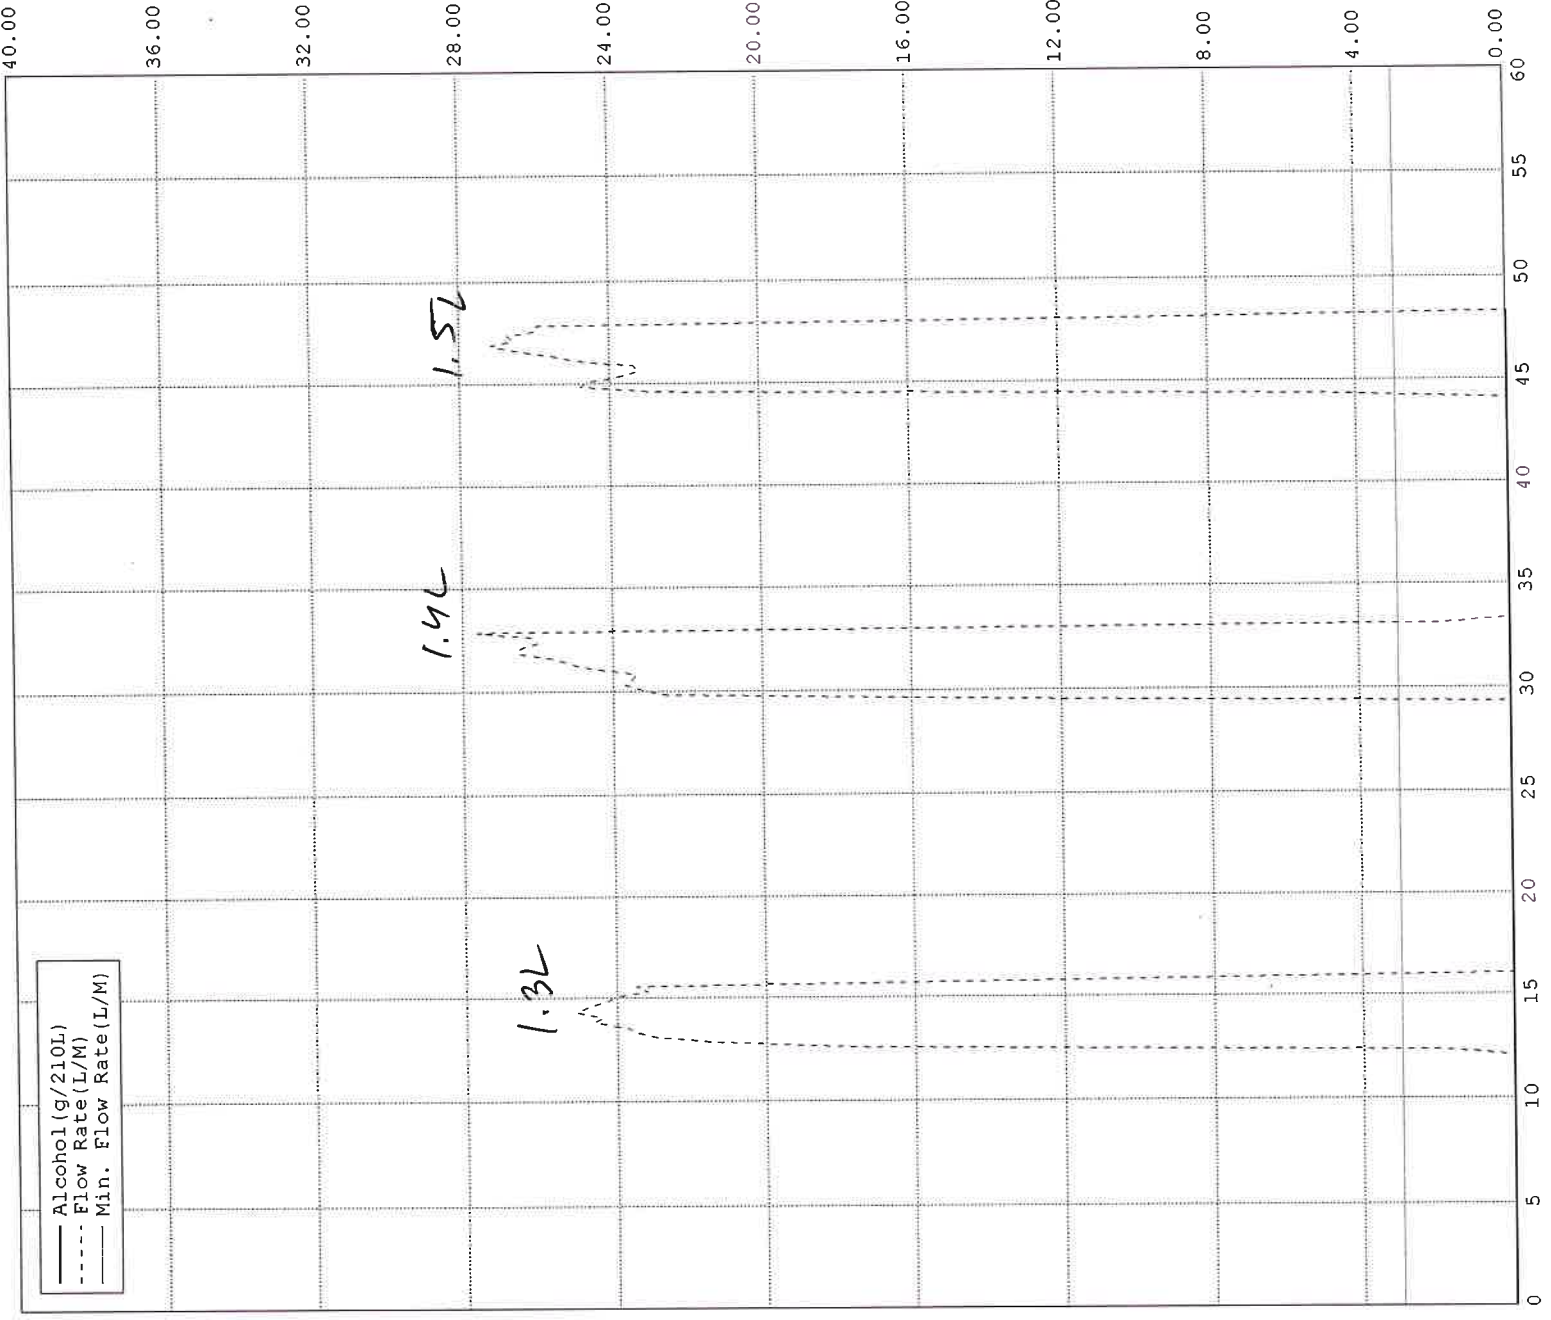

KS

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100348

Date: 06/13/2024
 Time: 07:41:54

SUPERVISOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.020	0.0198	0.0004
0.040	0.0390	0.0000
0.080	0.0782	0.0004
0.100	0.0980	0.0000
0.150	0.1450	0.0000
0.299	0.2936	0.0005

SLOPE = 0.980771
 R² = 0.999919

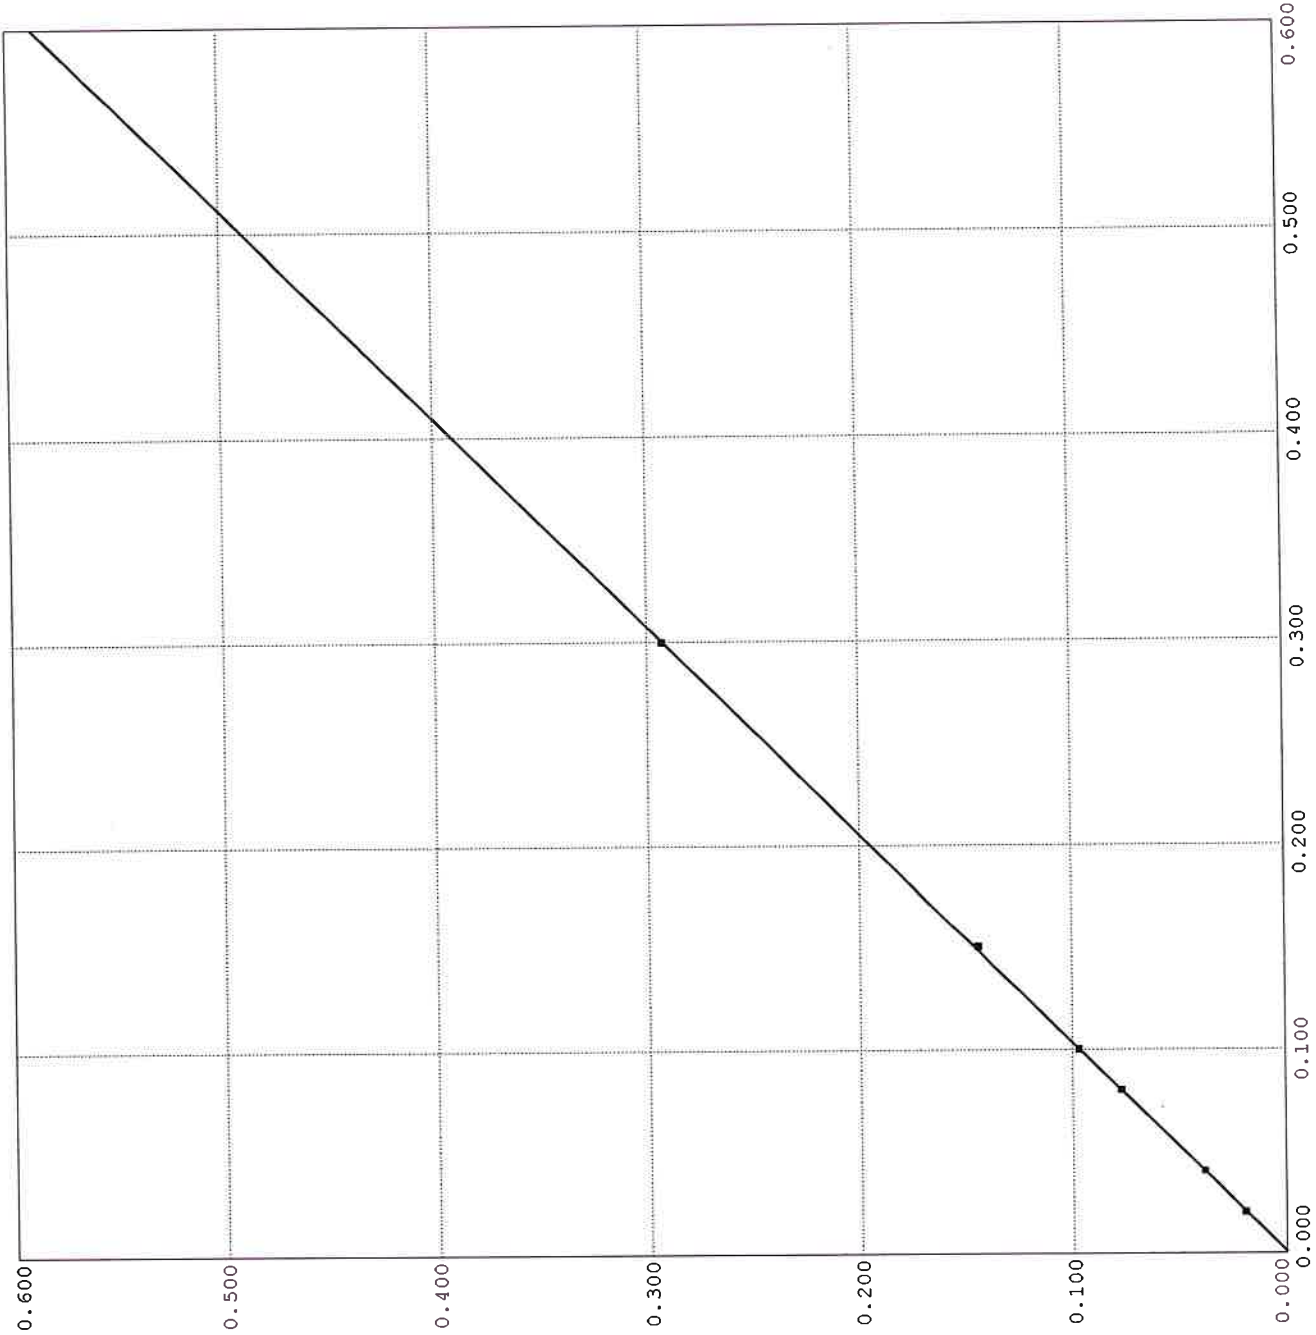

KS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100348






Date: 06/13/2024
Time: 07:41:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.83: 0.020
LOT #: AG217902
EXPIRATION: 06/28/2024
TANK PRESSURE: 687 psi

BLANK TEST	0.000	07:43
INTERNAL STANDARD	VERIFIED	07:43
EXTERNAL STANDARD	0.020	07:43
BLANK TEST	0.000	07:44
EXTERNAL STANDARD	0.020	07:45
BLANK TEST	0.000	07:45
EXTERNAL STANDARD	0.019	07:46
BLANK TEST	0.000	07:47
EXTERNAL STANDARD	0.020	07:47
BLANK TEST	0.000	07:48
EXTERNAL STANDARD	0.020	07:48
BLANK TEST	0.000	07:49

Average = 0.0198
Std Dev = 0.0004

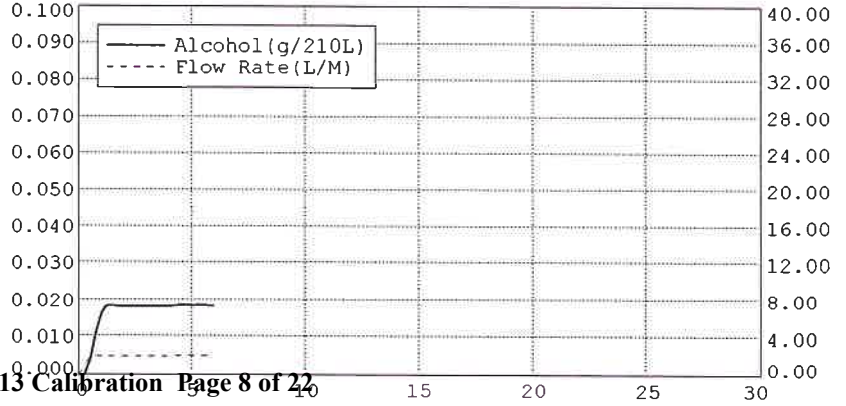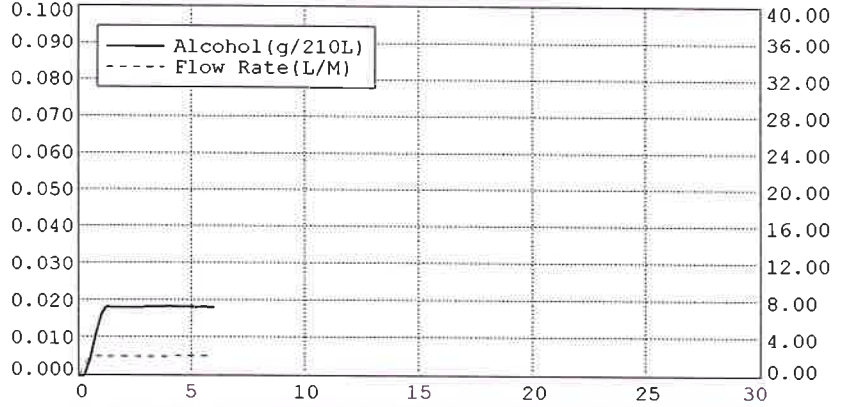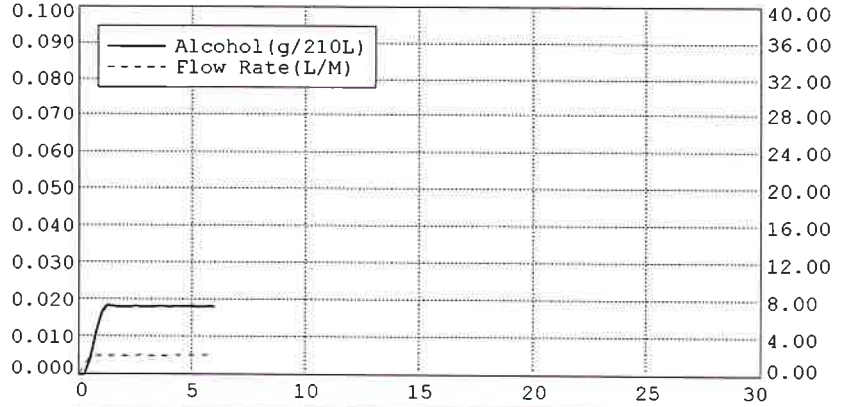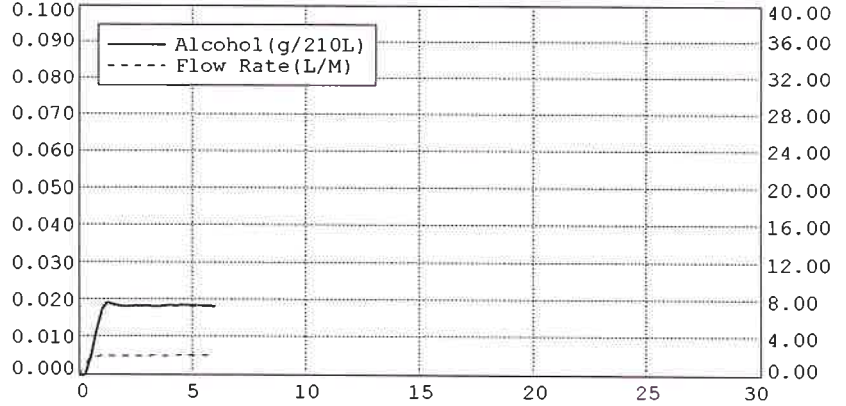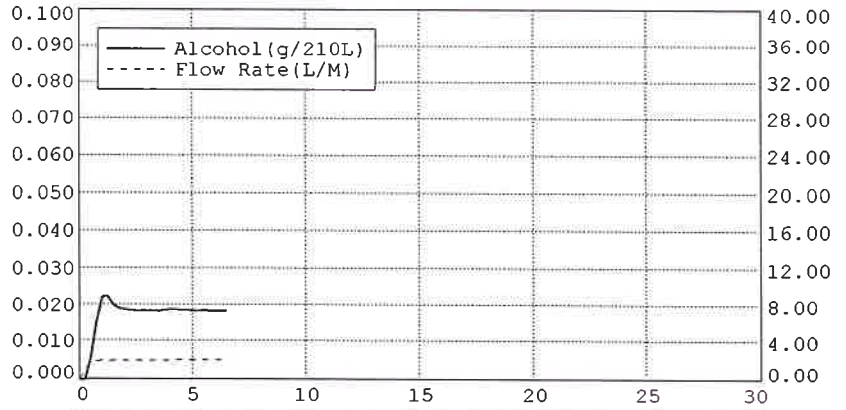

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100348






Date: 06/13/2024
Time: 07:50:09

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.83: 0.040
LOT #: AG217904
EXPIRATION: 06/28/2024
TANK PRESSURE: 616 psi

BLANK TEST	0.000	07:51
INTERNAL STANDARD	VERIFIED	07:51
EXTERNAL STANDARD	0.039	07:51
BLANK TEST	0.000	07:52
EXTERNAL STANDARD	0.039	07:52
BLANK TEST	0.000	07:53
EXTERNAL STANDARD	0.039	07:54
BLANK TEST	0.000	07:54
EXTERNAL STANDARD	0.039	07:55
BLANK TEST	0.000	07:56
EXTERNAL STANDARD	0.039	07:56
BLANK TEST	0.000	07:57

Average = 0.0390
Std Dev = 0.0000

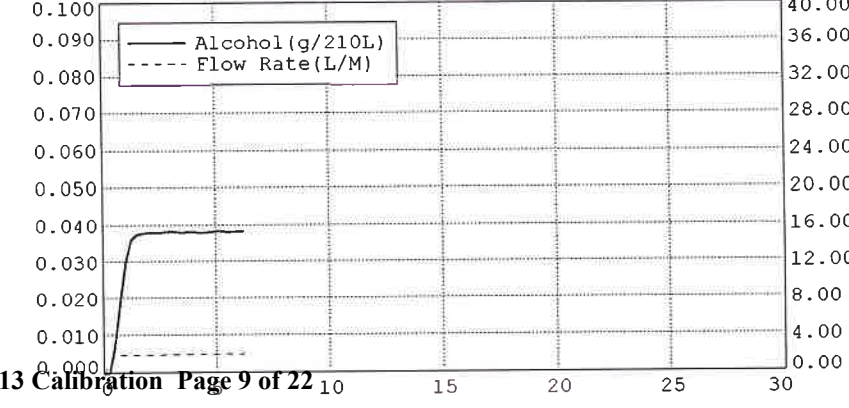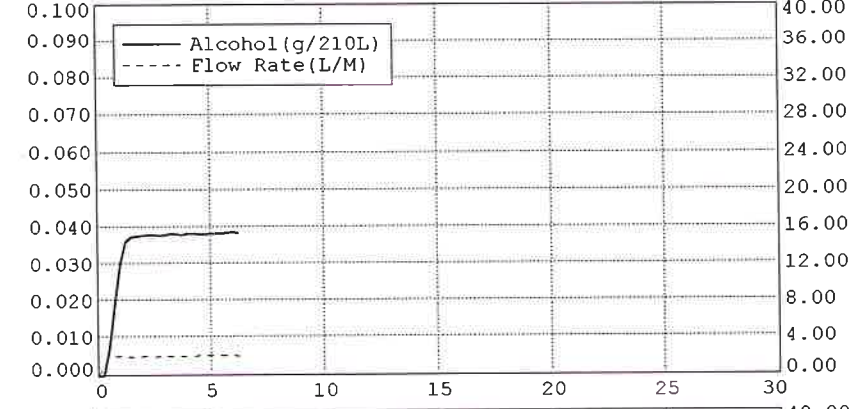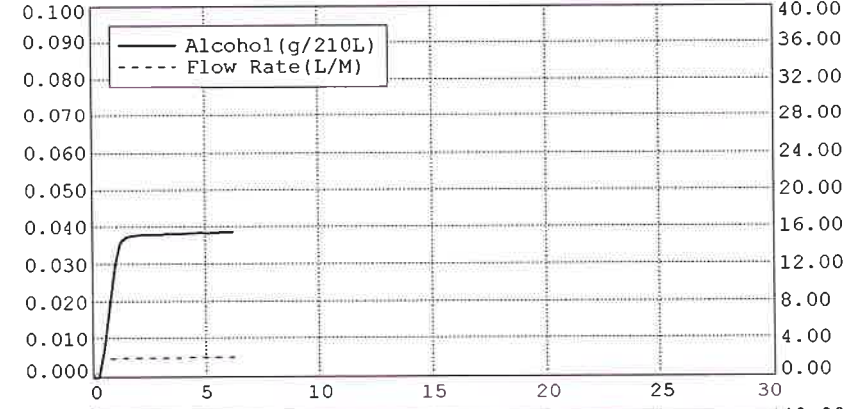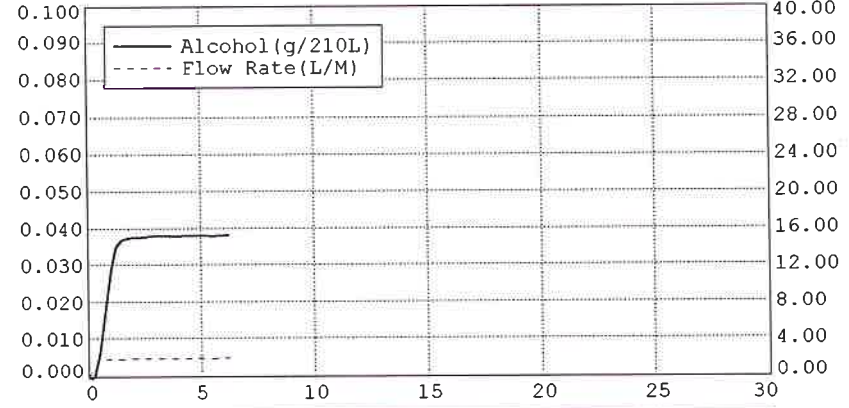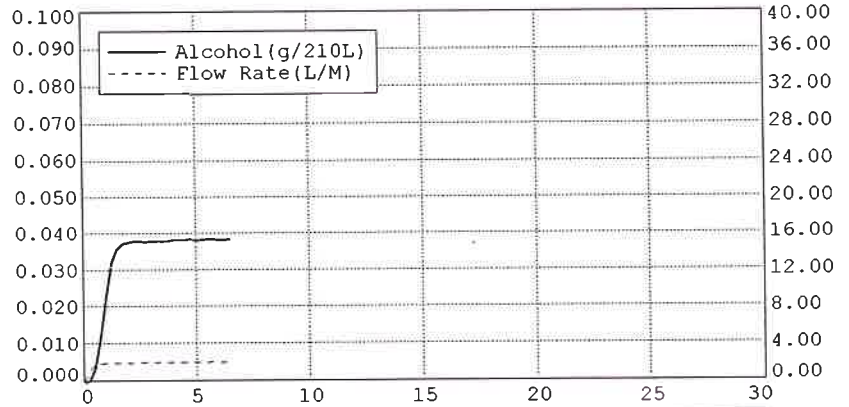

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100348






Date: 06/13/2024
Time: 07:57:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.84: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 657 psi

BLANK TEST	0.000	07:59
INTERNAL STANDARD	VERIFIED	07:59
EXTERNAL STANDARD	0.078	07:59
BLANK TEST	0.000	08:00
EXTERNAL STANDARD	0.078	08:00
BLANK TEST	0.000	08:01
EXTERNAL STANDARD	0.079	08:01
BLANK TEST	0.000	08:02
EXTERNAL STANDARD	0.078	08:02
BLANK TEST	0.000	08:03
EXTERNAL STANDARD	0.078	08:03
BLANK TEST	0.000	08:04

Average = 0.0782
Std Dev = 0.0004

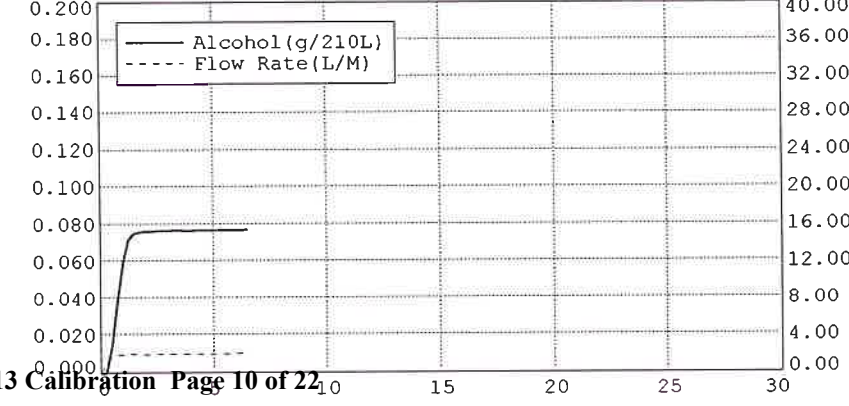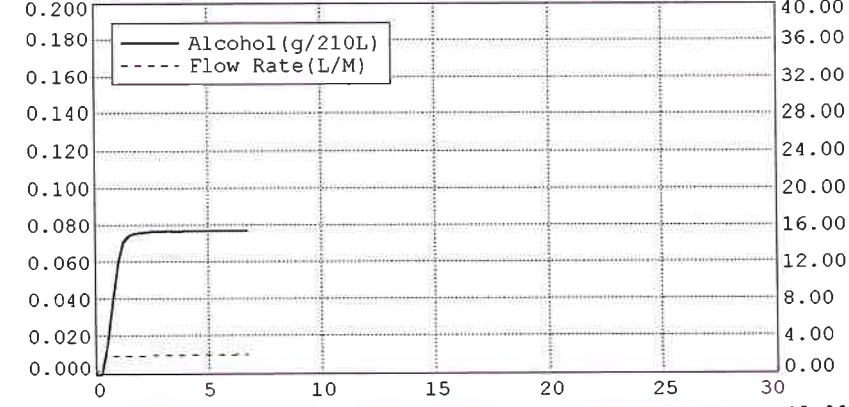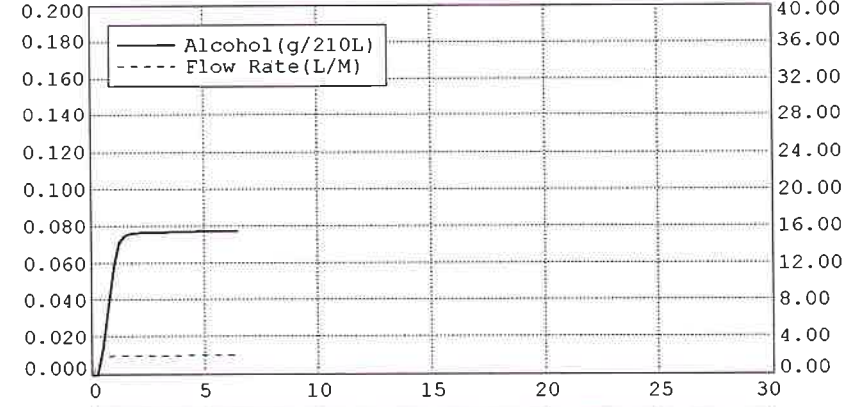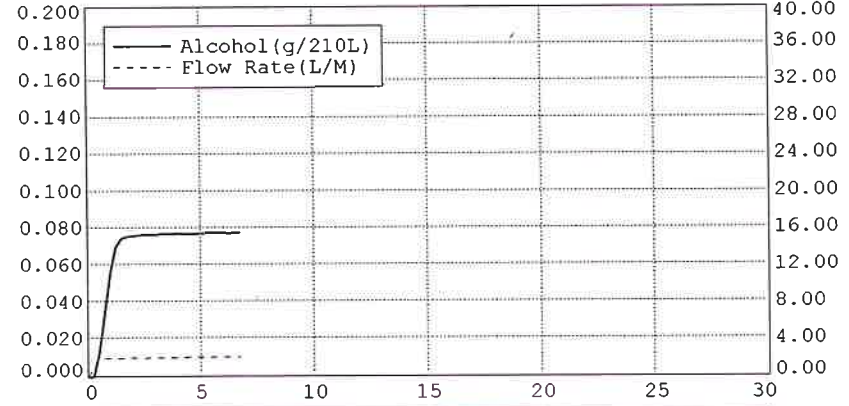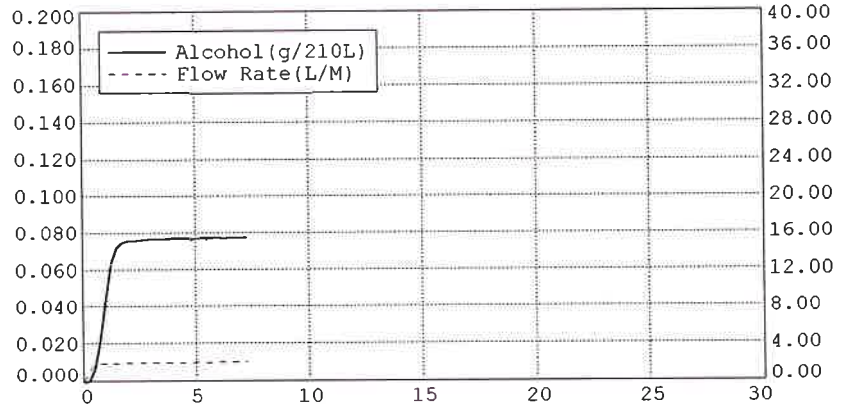

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100348






Date: 06/13/2024
 Time: 08:06:01

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.83: 0.100
 LOT #: AG333401
 EXPIRATION: 11/30/2025
 TANK PRESSURE: 1141 psi

BLANK TEST	0.000	08:07
INTERNAL STANDARD	VERIFIED	08:07
EXTERNAL STANDARD	0.098	08:07
BLANK TEST	0.000	08:08
EXTERNAL STANDARD	0.098	08:08
BLANK TEST	0.000	08:09
EXTERNAL STANDARD	0.098	08:10
BLANK TEST	0.000	08:10
EXTERNAL STANDARD	0.098	08:11
BLANK TEST	0.000	08:12
EXTERNAL STANDARD	0.098	08:12
BLANK TEST	0.000	08:13

Average = 0.0980
 Std Dev = 0.0000

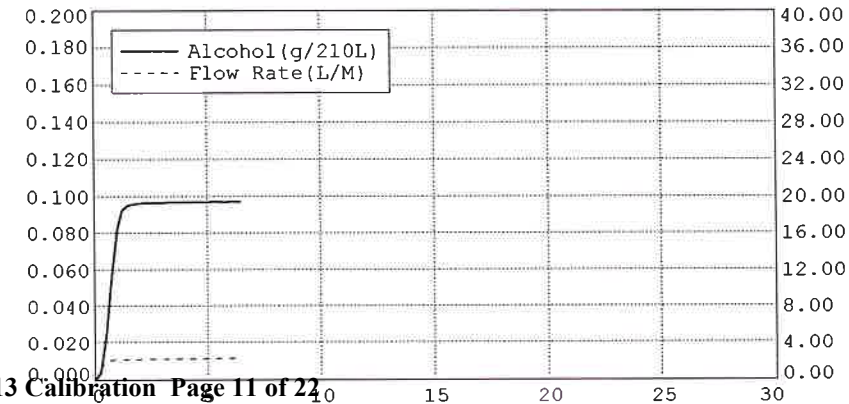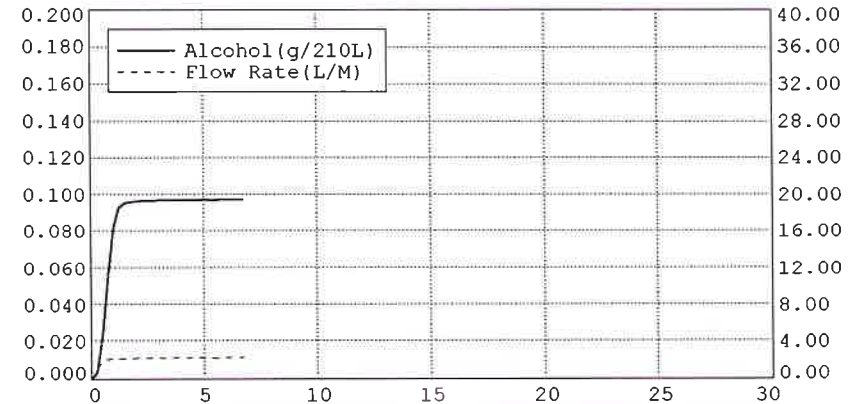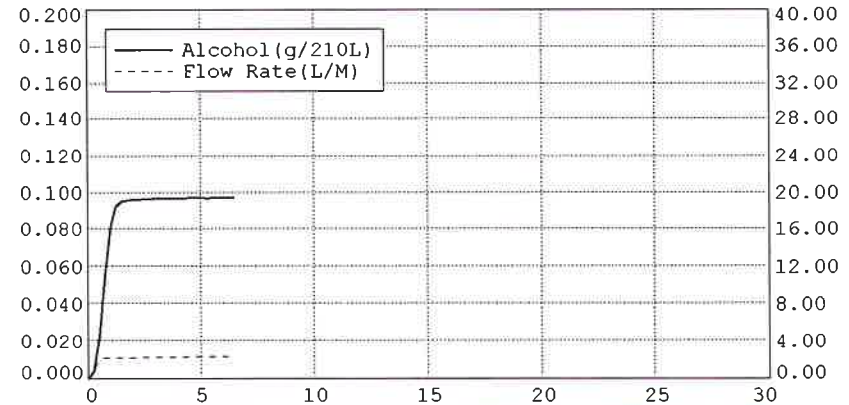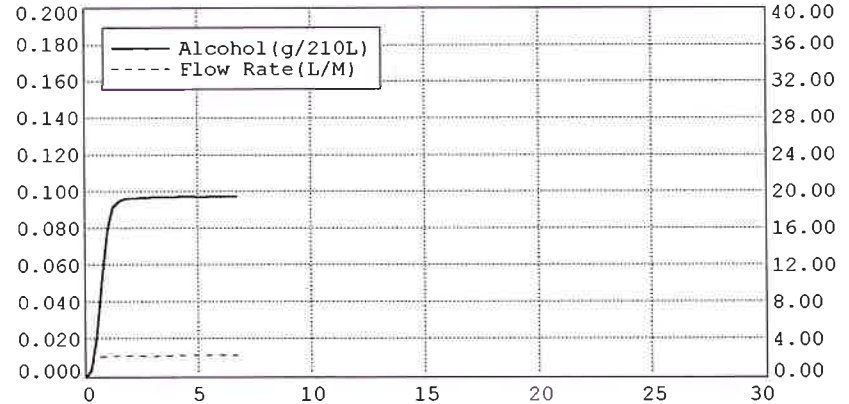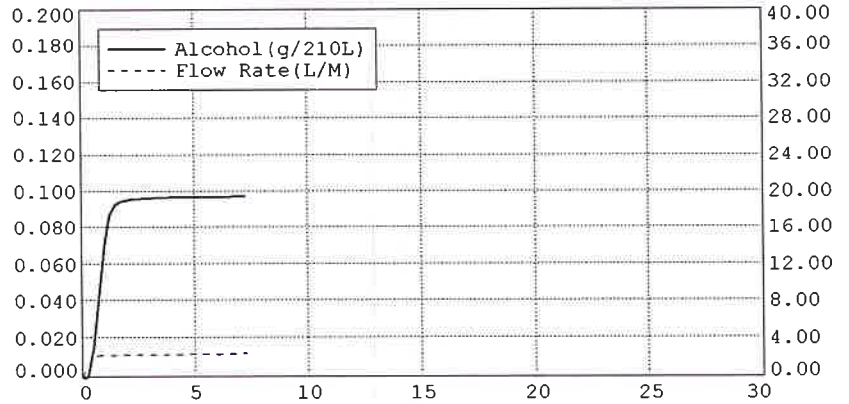

LINEARITY CHECK: Control Test 5






Alaska Department of Public Safety
 DATAMASTER dmt: 100348

Date: 06/13/2024
 Time: 08:15:59

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.150
 TARGET AT 29.82: 0.150
 LOT #: AG332004
 EXPIRATION: 11/16/2025
 TANK PRESSURE: 583 psi

BLANK TEST	0.000	08:17
INTERNAL STANDARD	VERIFIED	08:17
EXTERNAL STANDARD	0.145	08:17
BLANK TEST	0.000	08:18
EXTERNAL STANDARD	0.145	08:19
BLANK TEST	0.000	08:19
EXTERNAL STANDARD	0.145	08:20
BLANK TEST	0.000	08:21
EXTERNAL STANDARD	0.145	08:21
BLANK TEST	0.000	08:22
EXTERNAL STANDARD	0.145	08:22
BLANK TEST	0.000	08:23

Average = 0.1450
 Std Dev = 0.0000

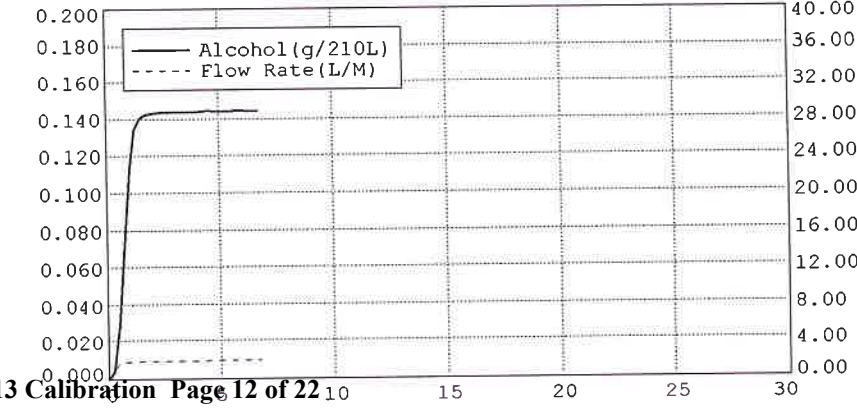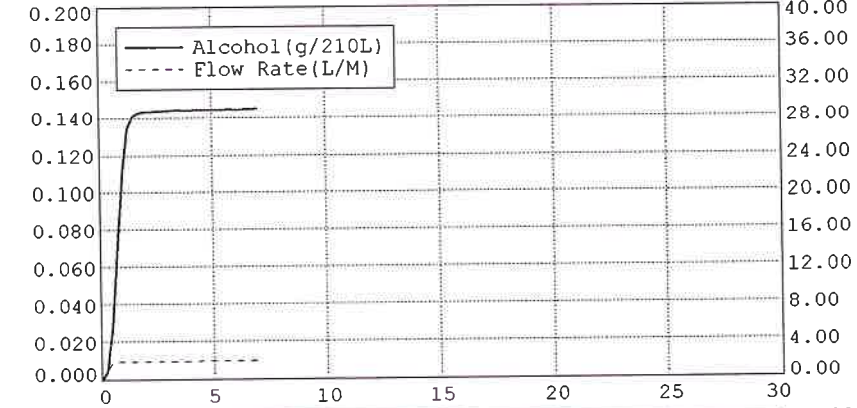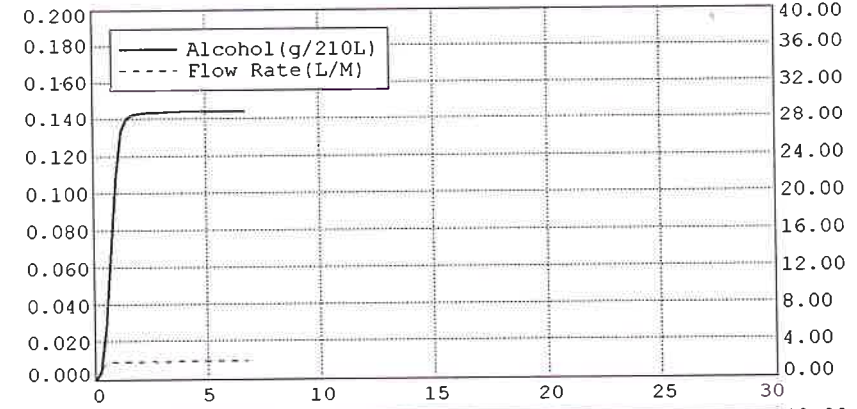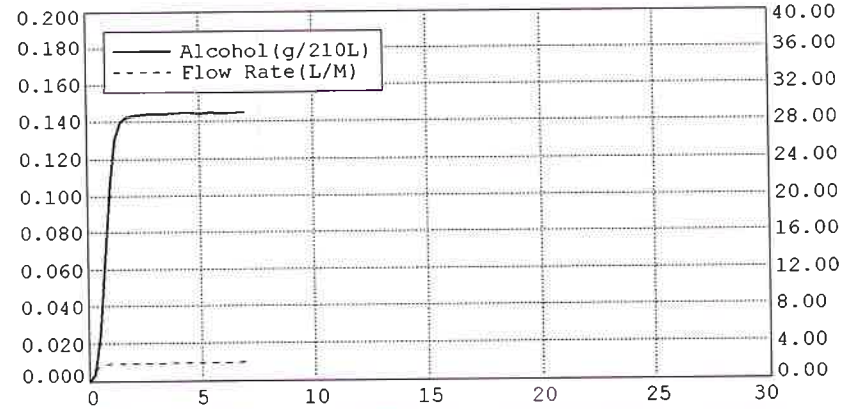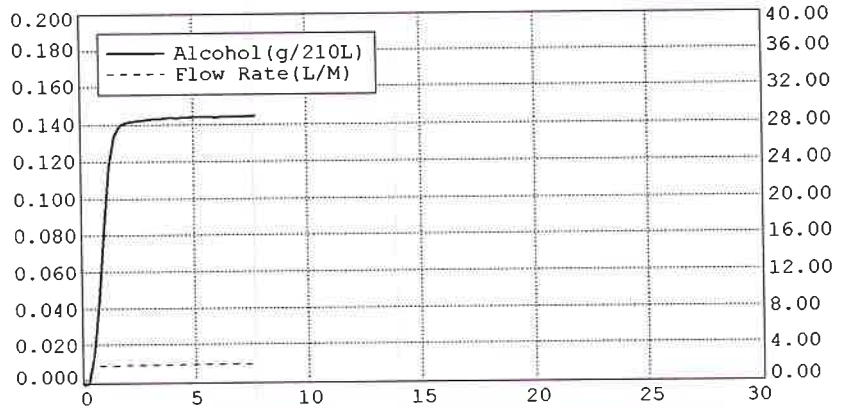

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100348






Date: 06/13/2024
 Time: 08:51:38

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.83: 0.299
 LOT #: AG327804
 EXPIRATION: 10/05/2025
 TANK PRESSURE: 187 psi

BLANK TEST	0.000	08:53
INTERNAL STANDARD	VERIFIED	08:53
EXTERNAL STANDARD	0.293	08:53
BLANK TEST	0.000	08:54
EXTERNAL STANDARD	0.293	08:54
BLANK TEST	0.000	08:55
EXTERNAL STANDARD	0.294	08:55
BLANK TEST	0.000	08:56
EXTERNAL STANDARD	0.294	08:57
BLANK TEST	0.000	08:57
EXTERNAL STANDARD	0.294	08:58
BLANK TEST	0.000	08:59

Average = 0.2936
 Std Dev = 0.0005

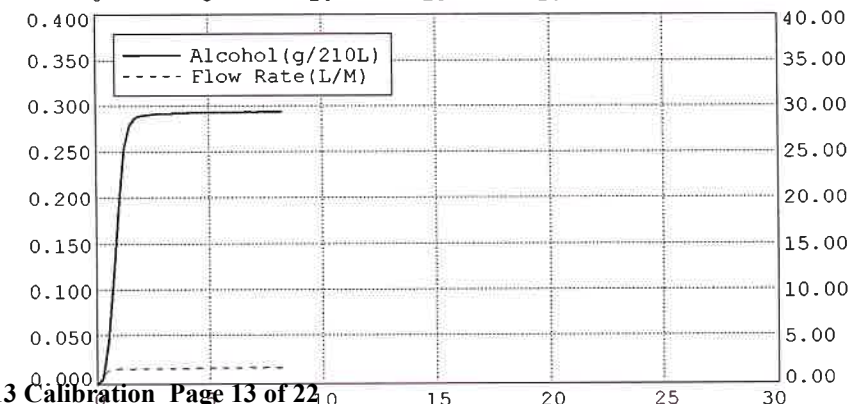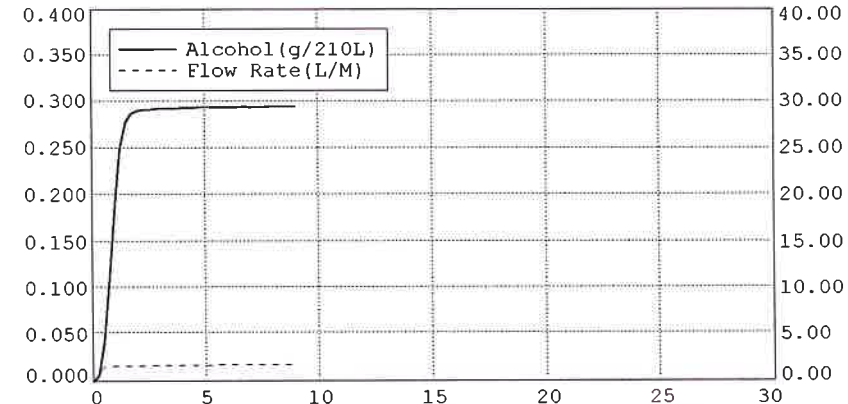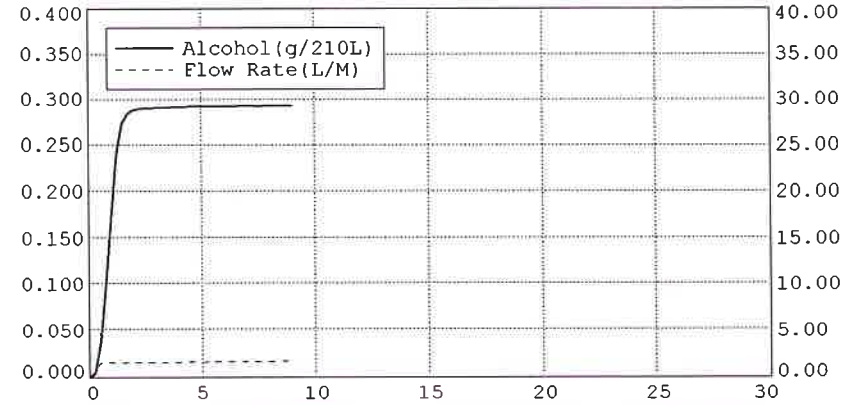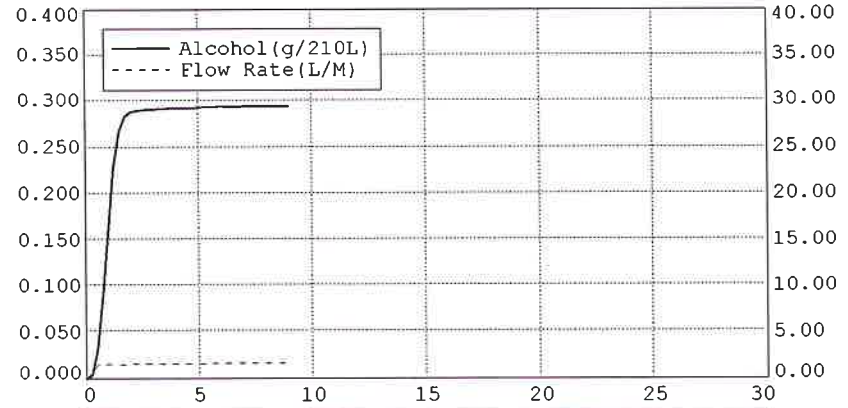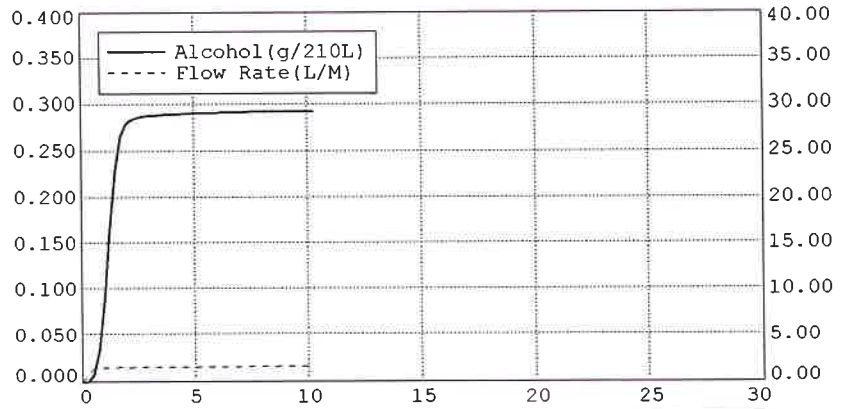

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100348

Date: 06/13/2024
Time: 09:16:17

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INCOMPLETE

CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK	PASSED	09:17
BLANK TEST	0.000	09:17
INTERNAL STANDARD	VERIFIED	09:17
EXTERNAL STANDARD	0.078	09:18
BLANK TEST	0.000	09:19
SUBJECT SAMPLE	INCOMPLETE	09:21

Lot # AG35202
Exp 12/18/25
KS 6/18/24

KS

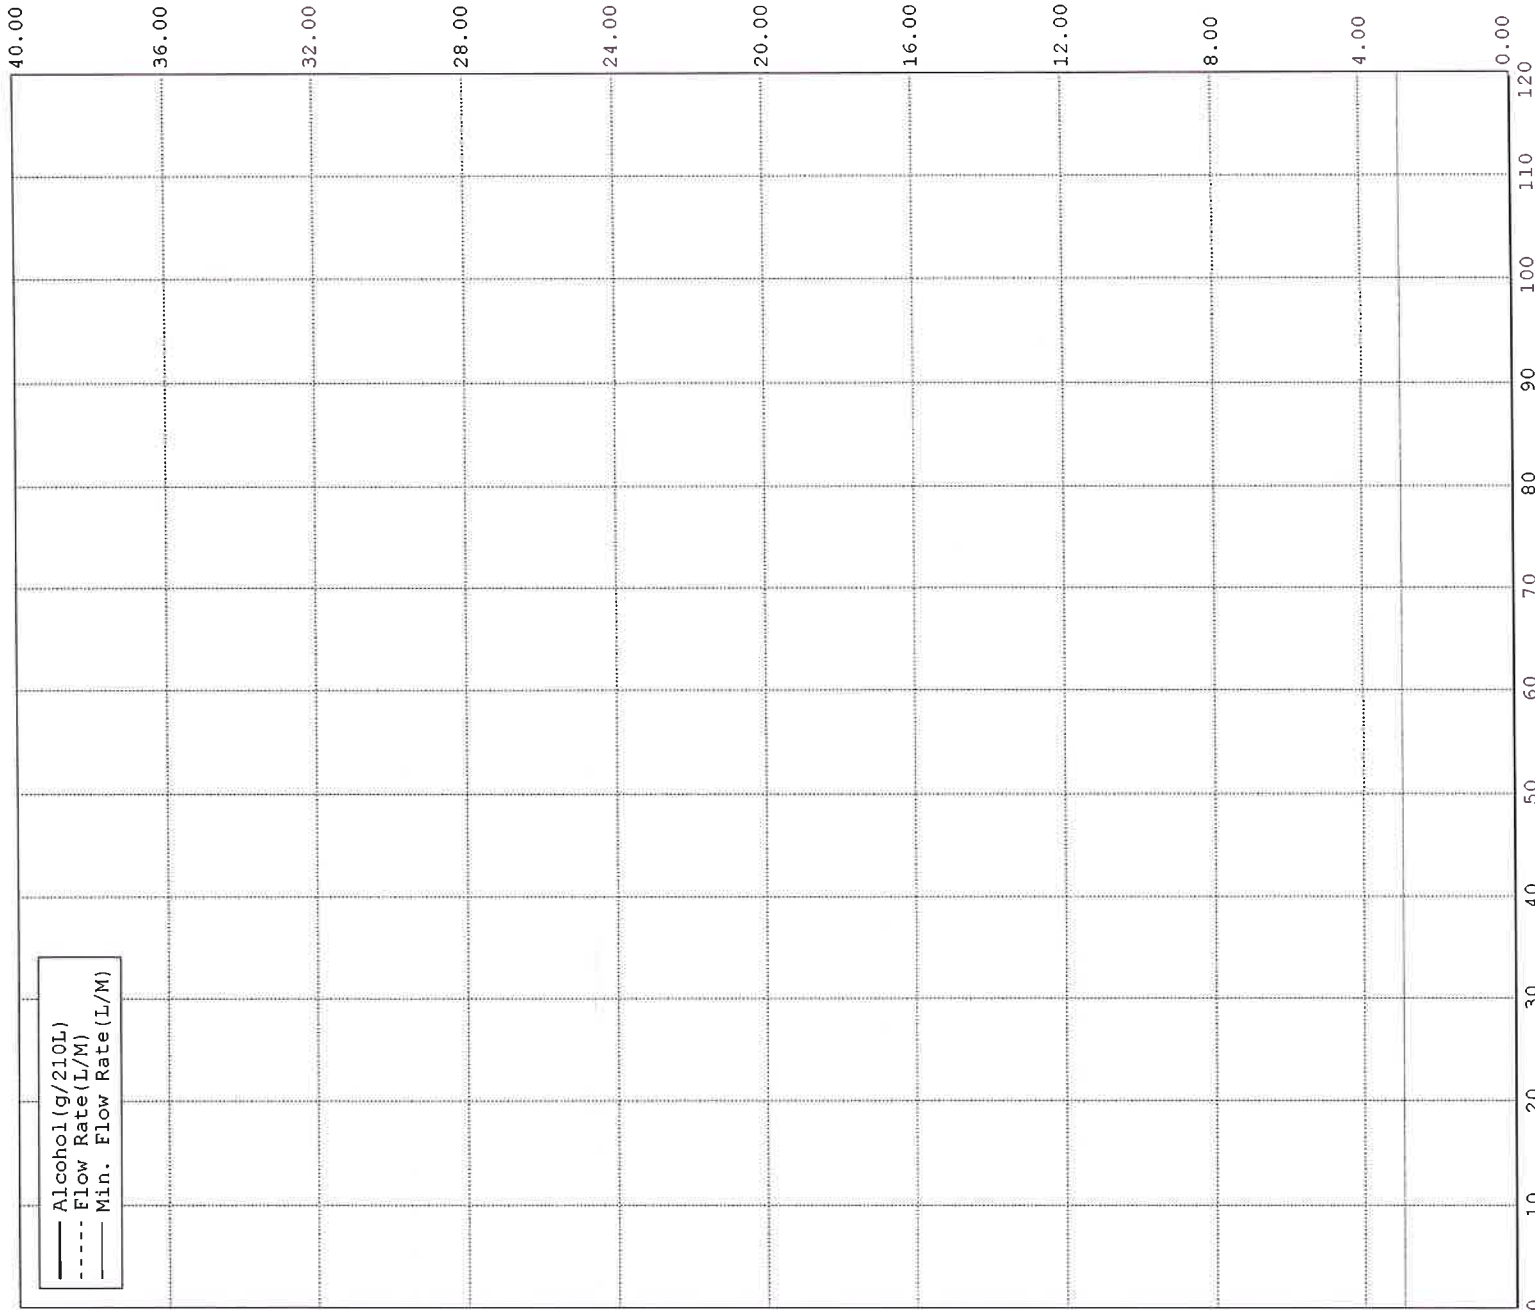

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 06/13/2024
Time: 09:38:48

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME: *lot # A-633502*
KAIJA SWISHER
OPERATOR'S #: 10745 *EXP 12/18/25*
KS 6/18/24

DEPT/AGENCY:
MAX ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.82: 0.080

DIAGNOSTIC CHECK PASSED 09:39
BLANK TEST 0.000 09:39
INTERNAL STANDARD VERIFIED 09:40
EXTERNAL STANDARD 0.078 09:40
BLANK TEST 0.000 09:41
SUBJECT SAMPLE XXX 09:41

Maximum Attempts Exceeded

*Split peaks due to half
breaths KS 6/13/24*

KS

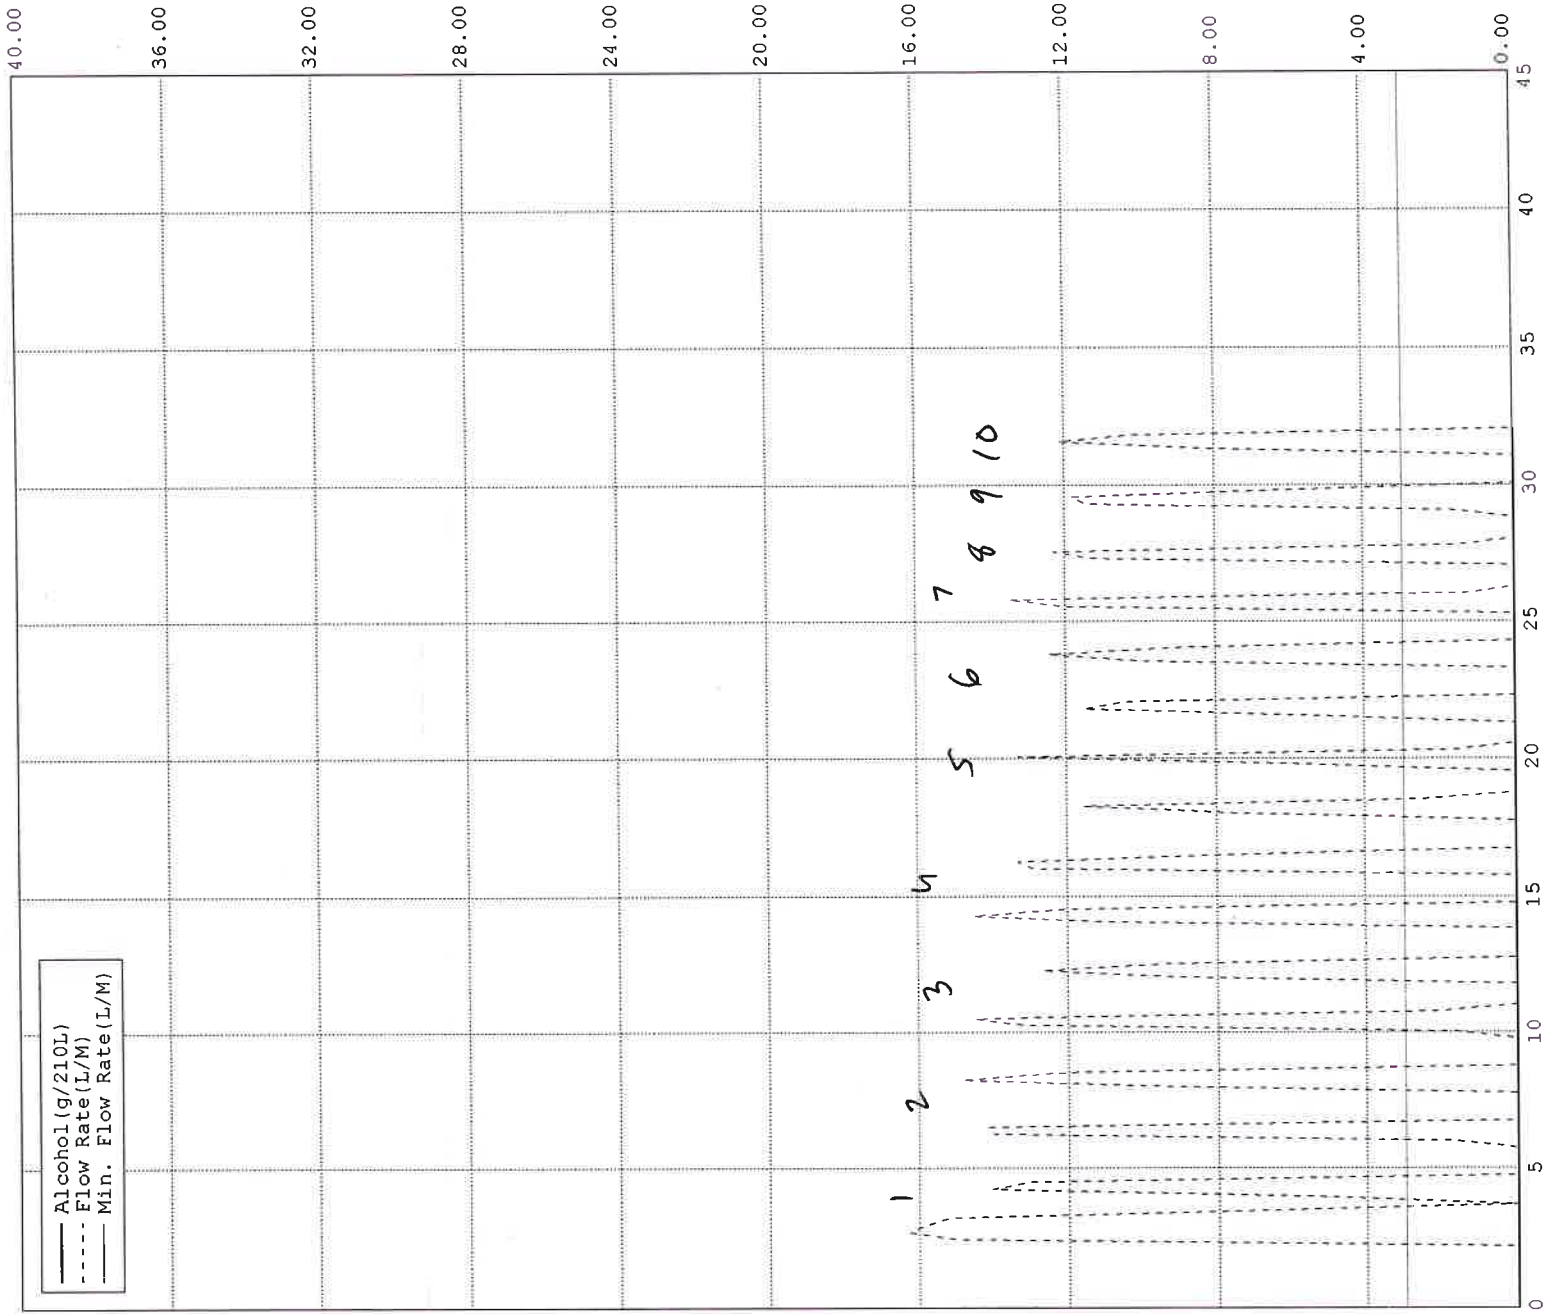

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 07/12/2024
Time: 10:02:21

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.51: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 10:03
BLANK TEST 0.000 10:03
INTERNAL STANDARD VERIFIED 10:03
EXTERNAL STANDARD 0.078 10:03
BLANK TEST 0.000 10:04
SUBJECT SAMPLE XXX 10:05

Maximum Attempts Exceeded

Test repeated to show peak
differentiation. KS 7/12/24.

KS

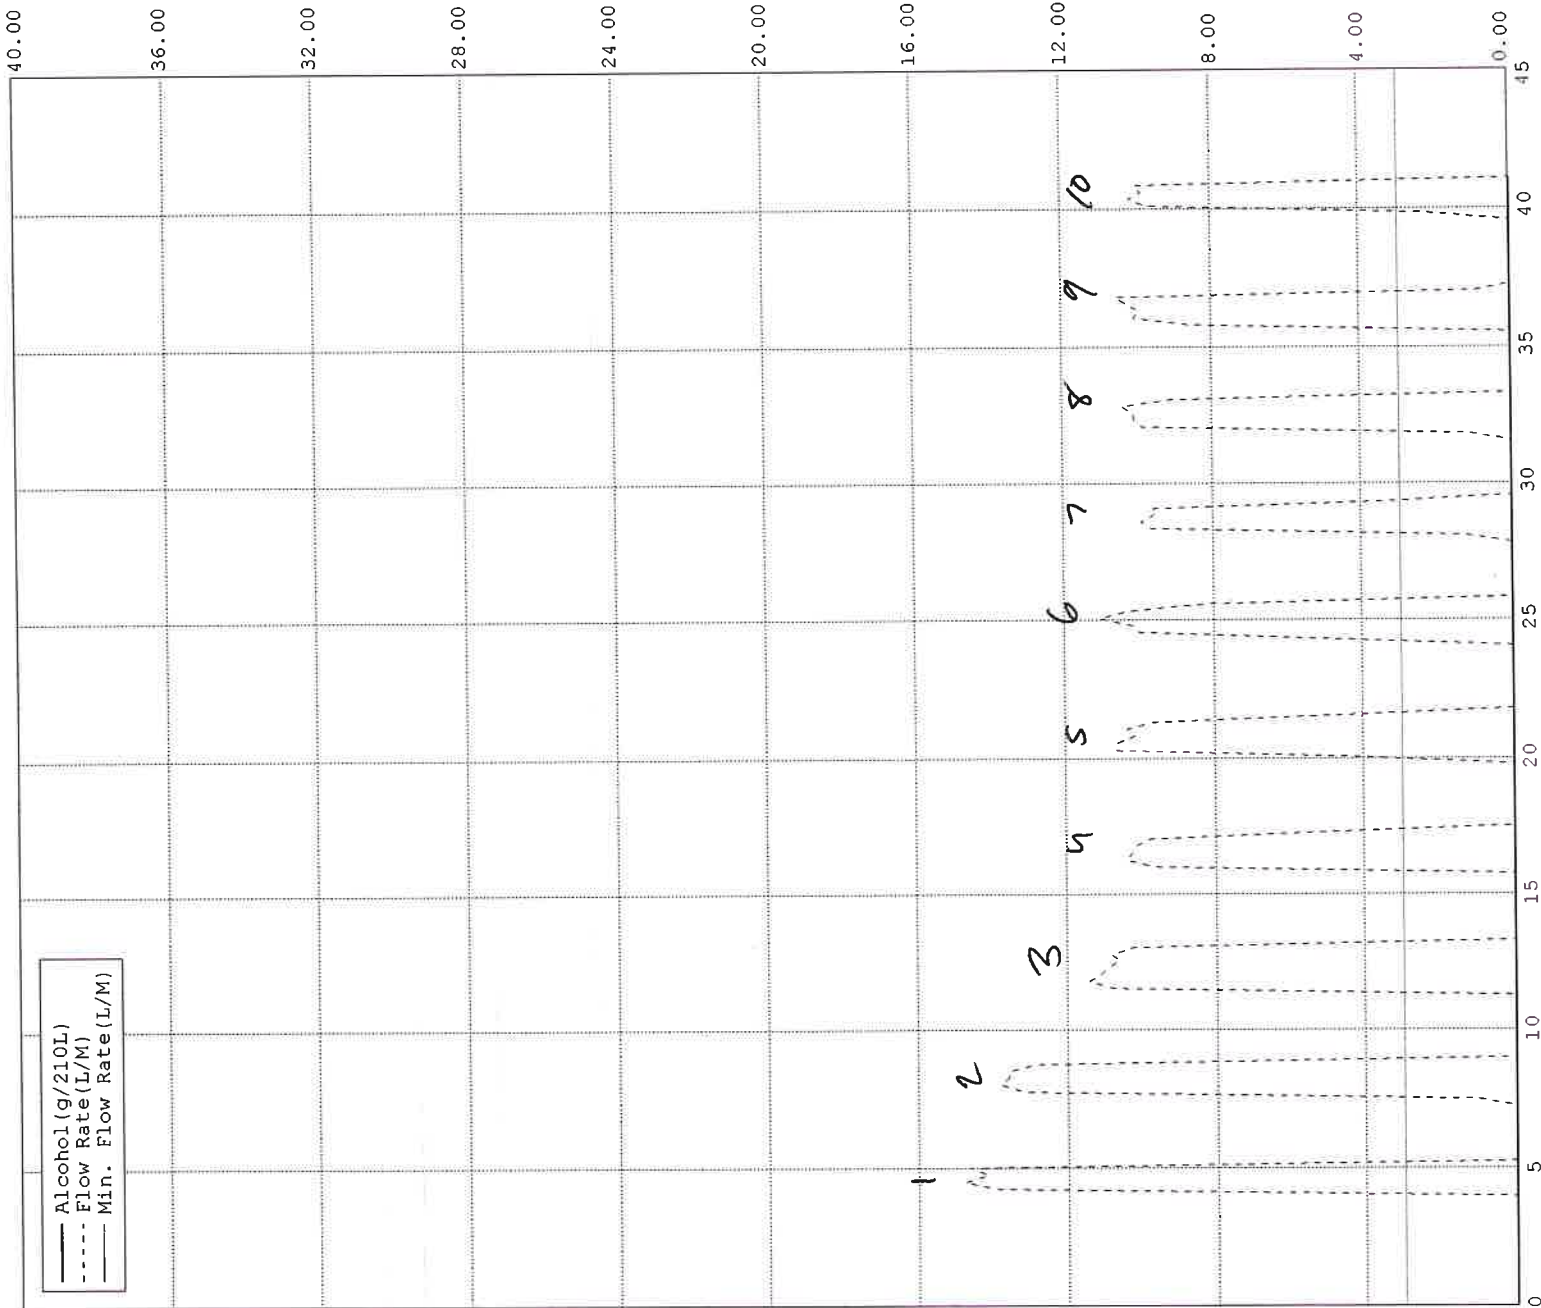

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100348

Date: 06/13/2024

Time: 09:43:23

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10745

DEPT/AGENCY:

INVALID

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK

PASSED 09:47

0.000 09:47

BLANK TEST

VERIFIED 09:47

0.079 09:48

EXTERNAL STANDARD

0.000 09:48


BLANK TEST

INVALID 09:49

SUBJECT SAMPLE

Lot #AG7335202
Exp 12/18/25
KS 6/18/24

KS

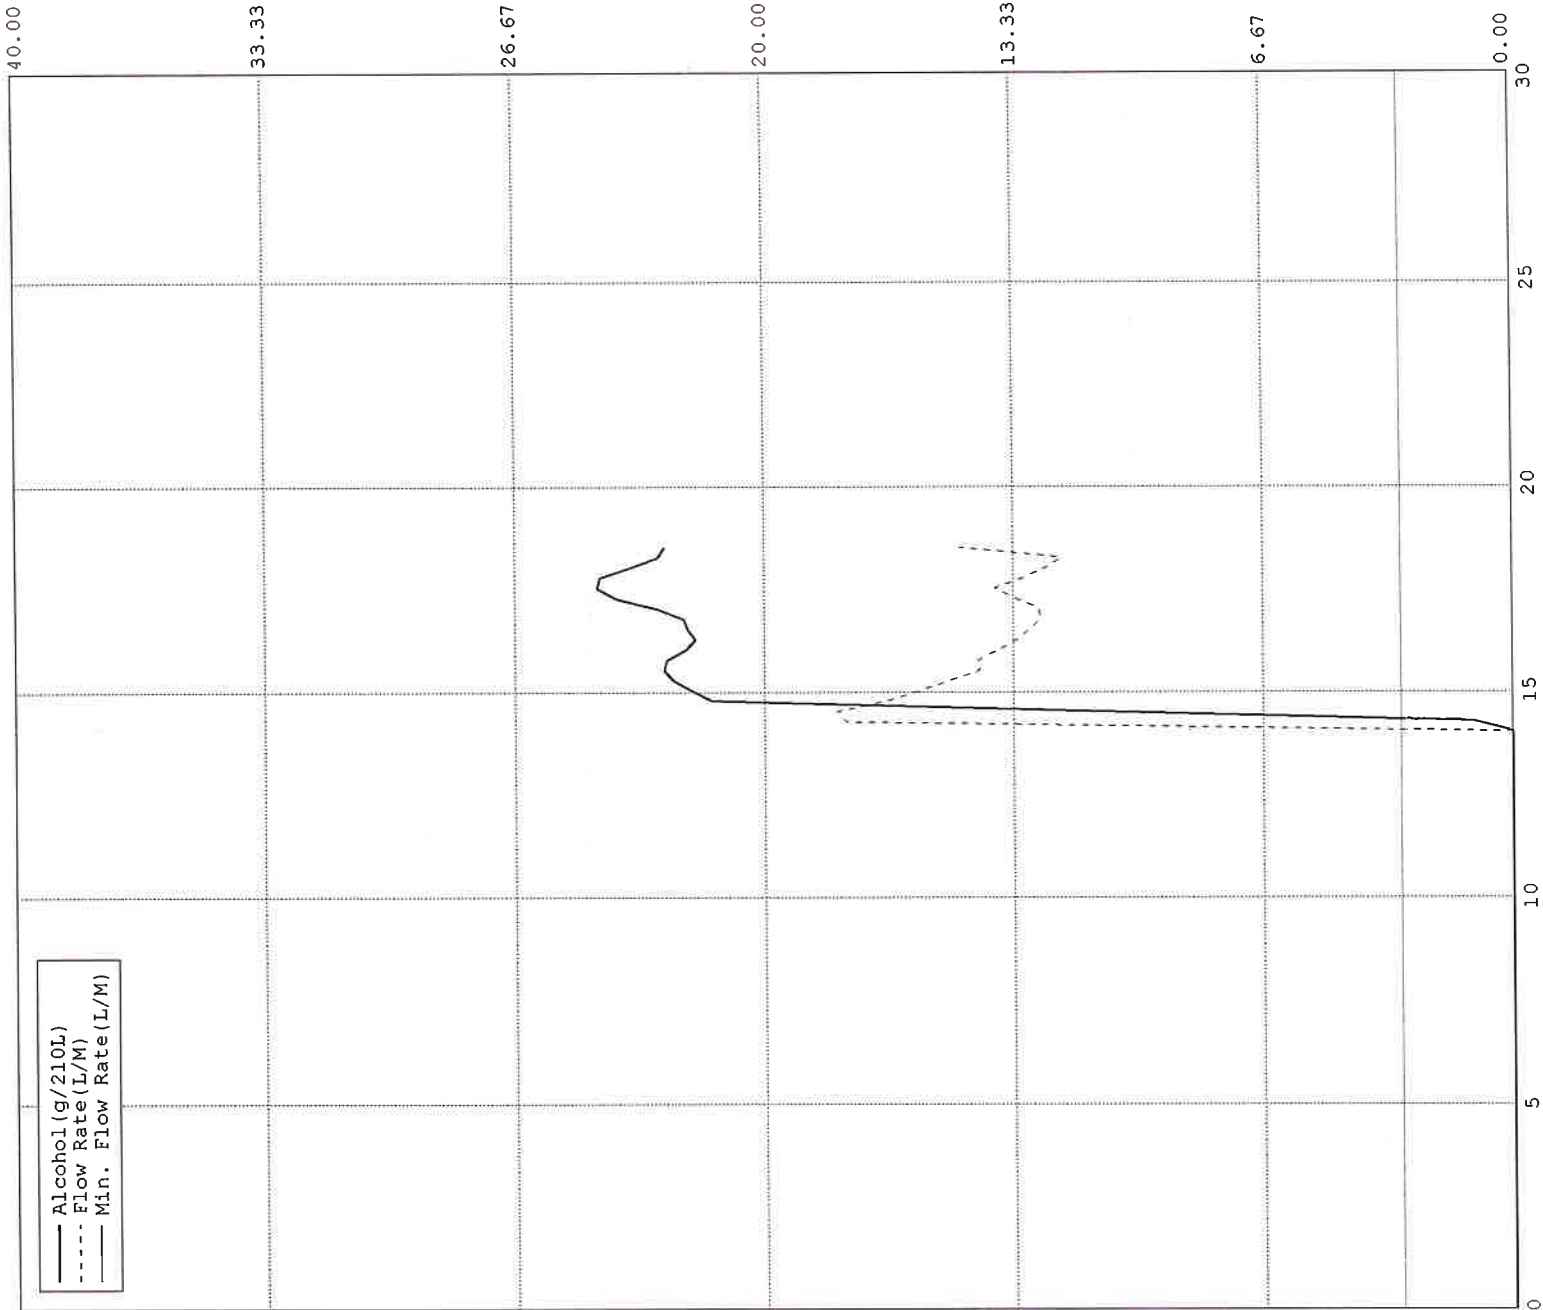

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100348

Date: 06/13/2024

Time: 09:52:24

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10745

DEPT/AGENCY:

RFI

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

RFI DETECTED

Lot # A67335202

Exp 12/18/25

KS 6/18/24

PASSED 09:53

0.000 09:53

VERIFIED 09:53

0.078 09:54

0.000 09:54

KS

40.00

36.00

32.00

28.00

24.00

20.00

16.00

12.00

8.00

4.00

0.00

30

25

20

15

10

5

0

Alcohol (g/210L)
Flow Rate (L/M)
Min. Flow Rate (L/M)

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 06/13/2024
Time: 10:16:48

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME: *lot # AG 35202*
KAIJA SWISHER *Exp 12/14/25*
OPERATOR'S #: 10746 *KS 6/18/24*

DEPT/AGENCY:
ACETONE


CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.82: 0.080

DIAGNOSTIC CHECK	PASSED	10:17
BLANK TEST	0.000	10:18
INTERNAL STANDARD	VERIFIED	10:18
Xq = 0.091 (2.25%)		
EXTERNAL STANDARD	0.078	10:18
X[1] = 0.0782 (-0.0005) (0.0025)		
BLANK TEST	0.000	10:19
SUBJECT SAMPLE	XXX	10:19
X[1] = 0.1035 (-0.0160) (0.0017)		

Interference Detected

KS

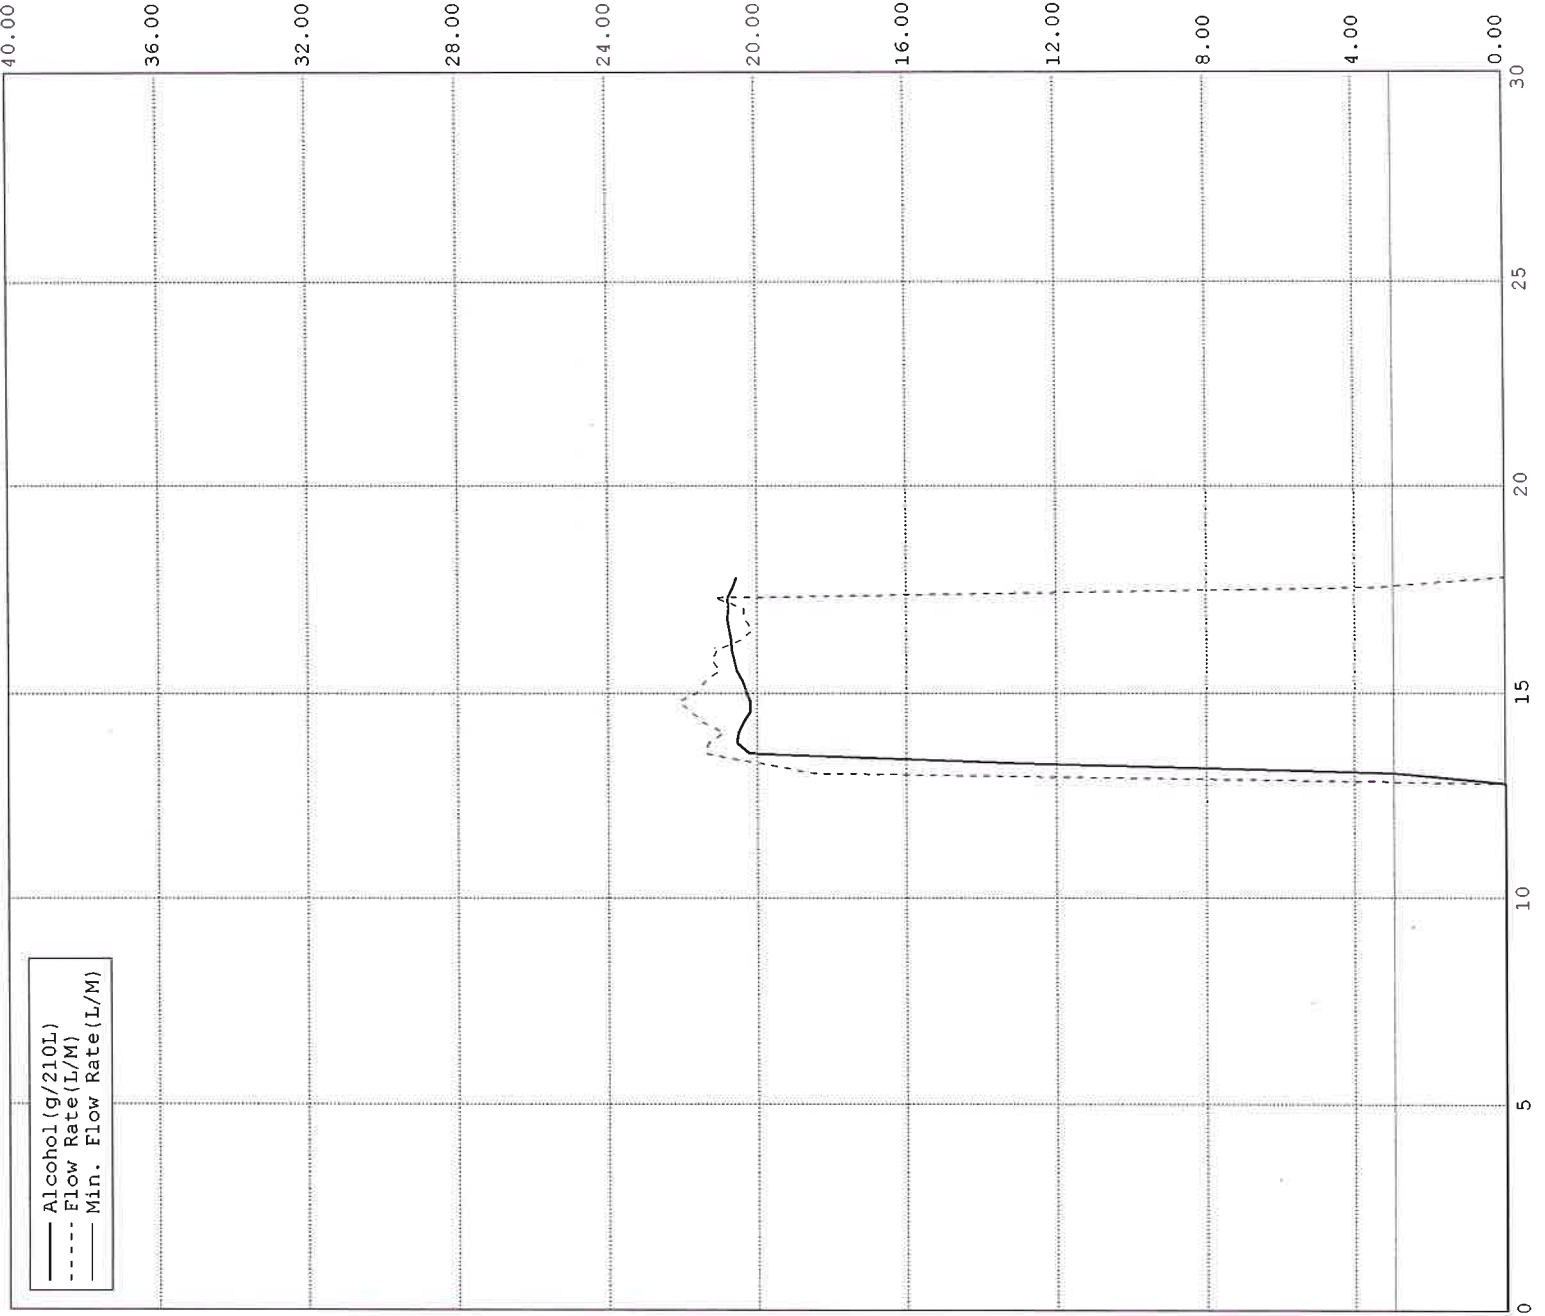

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 06/13/2024
Time: 10:21:33

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:

IPA

CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK	PASSED	10:23
BLANK TEST	0.000	10:23
INTERNAL STANDARD	VERIFIED	10:23
Xq = 0.092 (2.74%)		
EXTERNAL STANDARD	0.078	10:23
X[1] = 0.0783 (-0.0006)	(0.0019)	
BLANK TEST	0.000	10:24
SUBJECT SAMPLE	XXX	10:24
X[1] = 0.1121 (-0.0247)	(0.0008)	

Interference Detected

KS

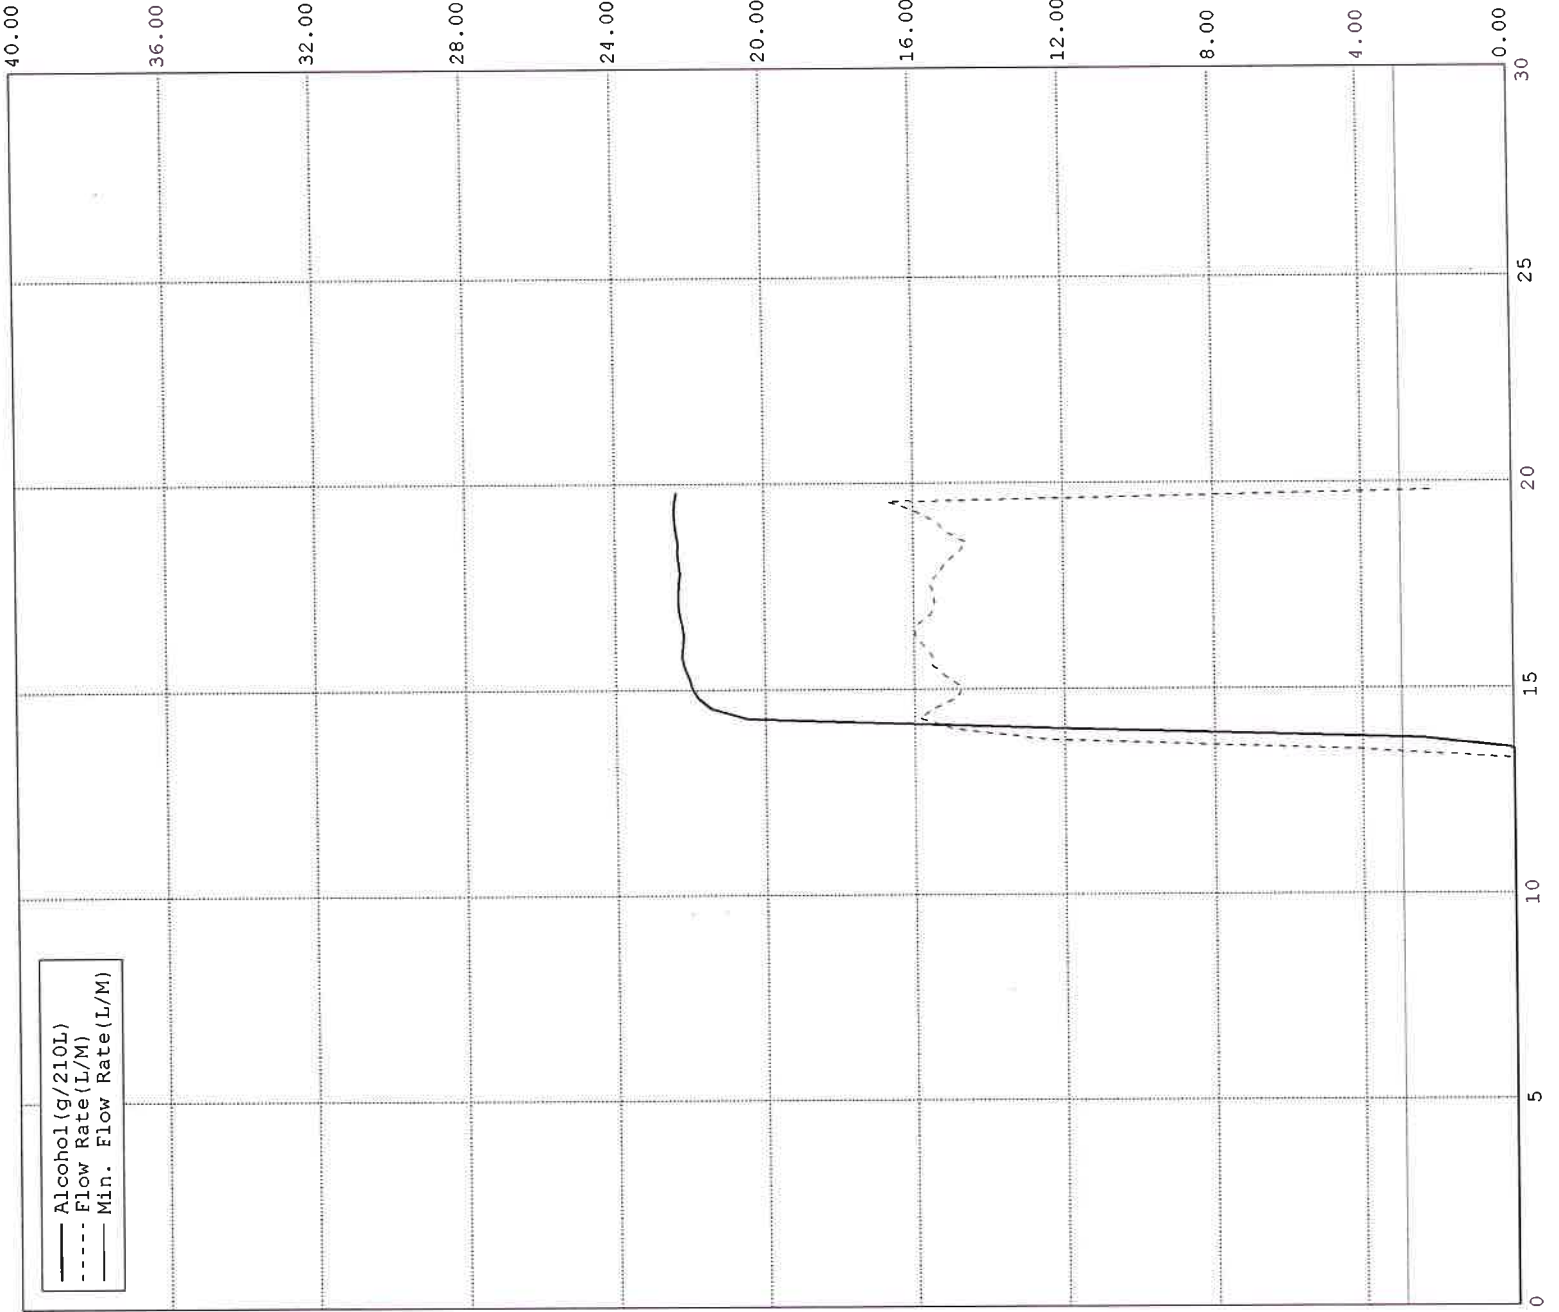

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100348

Date: 06/13/2024
 Time: 10:09:32

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10745

DEPT/AGENCY:
 NEGATIVE

CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.83: 0.080


TEST TYPE	RESULT	TIME
DIAGNOSTIC CHECK	PASSED	10:10
BLANK TEST	0.000	10:10
INTERNAL STANDARD	VERIFIED	10:10
	Xq = 0.091 (1.96%)	10:11
EXTERNAL STANDARD	0.078	10:11
	X[1] = 0.0781 (-0.0008) (0.0028)	10:11
BLANK TEST	0.000	10:12
SUBJECT SAMPLE (Vol=1.72L)	0.089	10:12
	X[1] = 0.0893 (-0.0007) (0.0006)	10:13
BLANK TEST	0.000	10:13
EXTERNAL STANDARD	0.078	10:13
	X[1] = 0.0779 (-0.0004) (0.0016)	10:14
BLANK TEST	0.000	10:14

Filter 2 ave → -0.0006

Filter 3 ave → 0.0022

KS 6/13/24 DM 07/10/24

KS

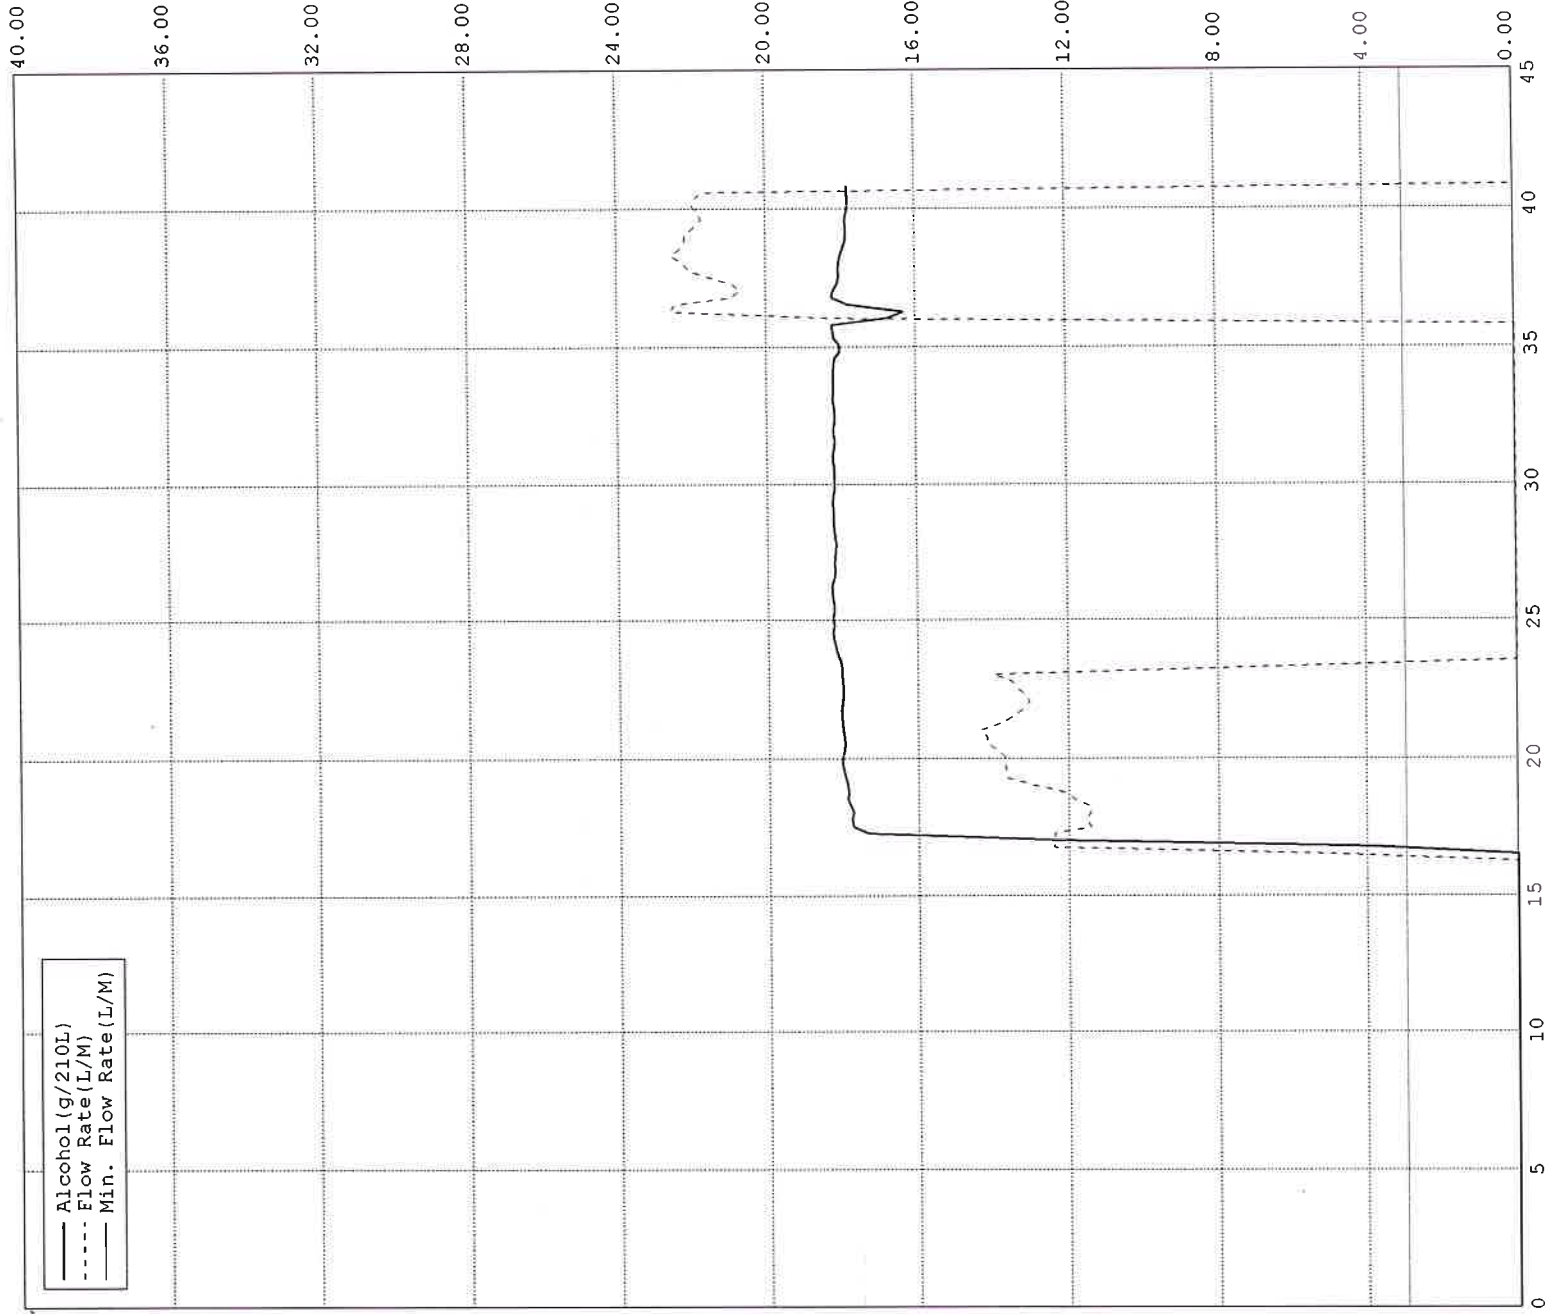

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100348

Date: 06/13/2024
 Time: 10:41:32

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

*Lot # A61335202
 Exp 12/18/25
 KS 6/18/24*

DEPT/AGENCY:
 NON DRINKING SUBJECT TEST
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK	PASSED	10:42
BLANK TEST	0.000	10:42
INTERNAL STANDARD	VERIFIED	10:42
EXTERNAL STANDARD	0.079	10:42
BLANK TEST	0.000	10:43
SUBJECT SAMPLE (Vol=1.74L)	0.000	10:44
BLANK TEST	0.000	10:45
EXTERNAL STANDARD	0.079	10:45
BLANK TEST	0.000	10:46

KS

