

Alaska Scientific Crime Detection Laboratory

DataMaster Acceptance Form

Issued: 01/27/2012
Effective: 01/27/2012

Version: DMAF2012 R0
Status: Active


Instrument # 100677

Date: 3/12/12

Analyst: Brandi Barnett

- Check in instrument in to JusticeTrax Breath Alcohol Database
- Visual Inspection
- Update software + USB fixer
2.00 BMB
- Print calibration factors (attached)
- NPAS calibration paperwork (attached)
- Barcode Instrument
- State of Alaska Property ID# 12FO 368

Verified new controller board + rear vented 3/12/12 BMB

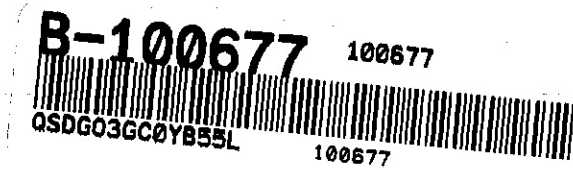


CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100677

Date: 10/26/2011
Time: 08:04:31

Ca	=	0.1000		
CAL	=	1.016524	0.800	<= CAL < 1.200
b1	=	0.0000	0.0000	<= b1 < 0.0040
b2	=	0.0030	0.0010	<= b2 < 0.0100
b3	=	0.0000	0.0000	<= b3 < 0.0040
Xq	=	0.0842	0.0500	<= Xq < 0.2000
a21	=	1.257001	1.050	<= a21 < 1.300
a31	=	0.532617	0.300	<= a31 < 0.800



**National Patent
Analytical Systems, Inc.**

Certificate of Calibration

100677

Instrument Serial Number

10260

Standard Reference Number

The above instrument has been calibrated and is hereby certified for use in determining alcohol breath concentration when used in accordance with the operating guidelines by a properly trained operator.

10-27-11

Date

A handwritten signature in black ink, consisting of several fluid, connected strokes, positioned above a horizontal line.

Technician

Final page for report

\

\\ANCSCLSAN01\JTRAX\CASEDOCS\B-100677\B-100677 ECF-20140

7/10/2014