

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100351

Date: 01/16/2015
Time: 15:56:36

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
BRANDI BARNETT
OPERATOR'S #: 7038

DEPT/AGENCY:
RFI TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.86: 0.077
LOT #: 09214080A2
EXPIRATION: 05/01/2016

DIAGNOSTIC CHECK	PASSED	15:57
BLANK TEST	0.000	15:57
INTERNAL STANDARD	VERIFIED	15:57
EXTERNAL STANDARD	0.076	15:58
BLANK TEST	0.000	15:59

RFI DETECTED

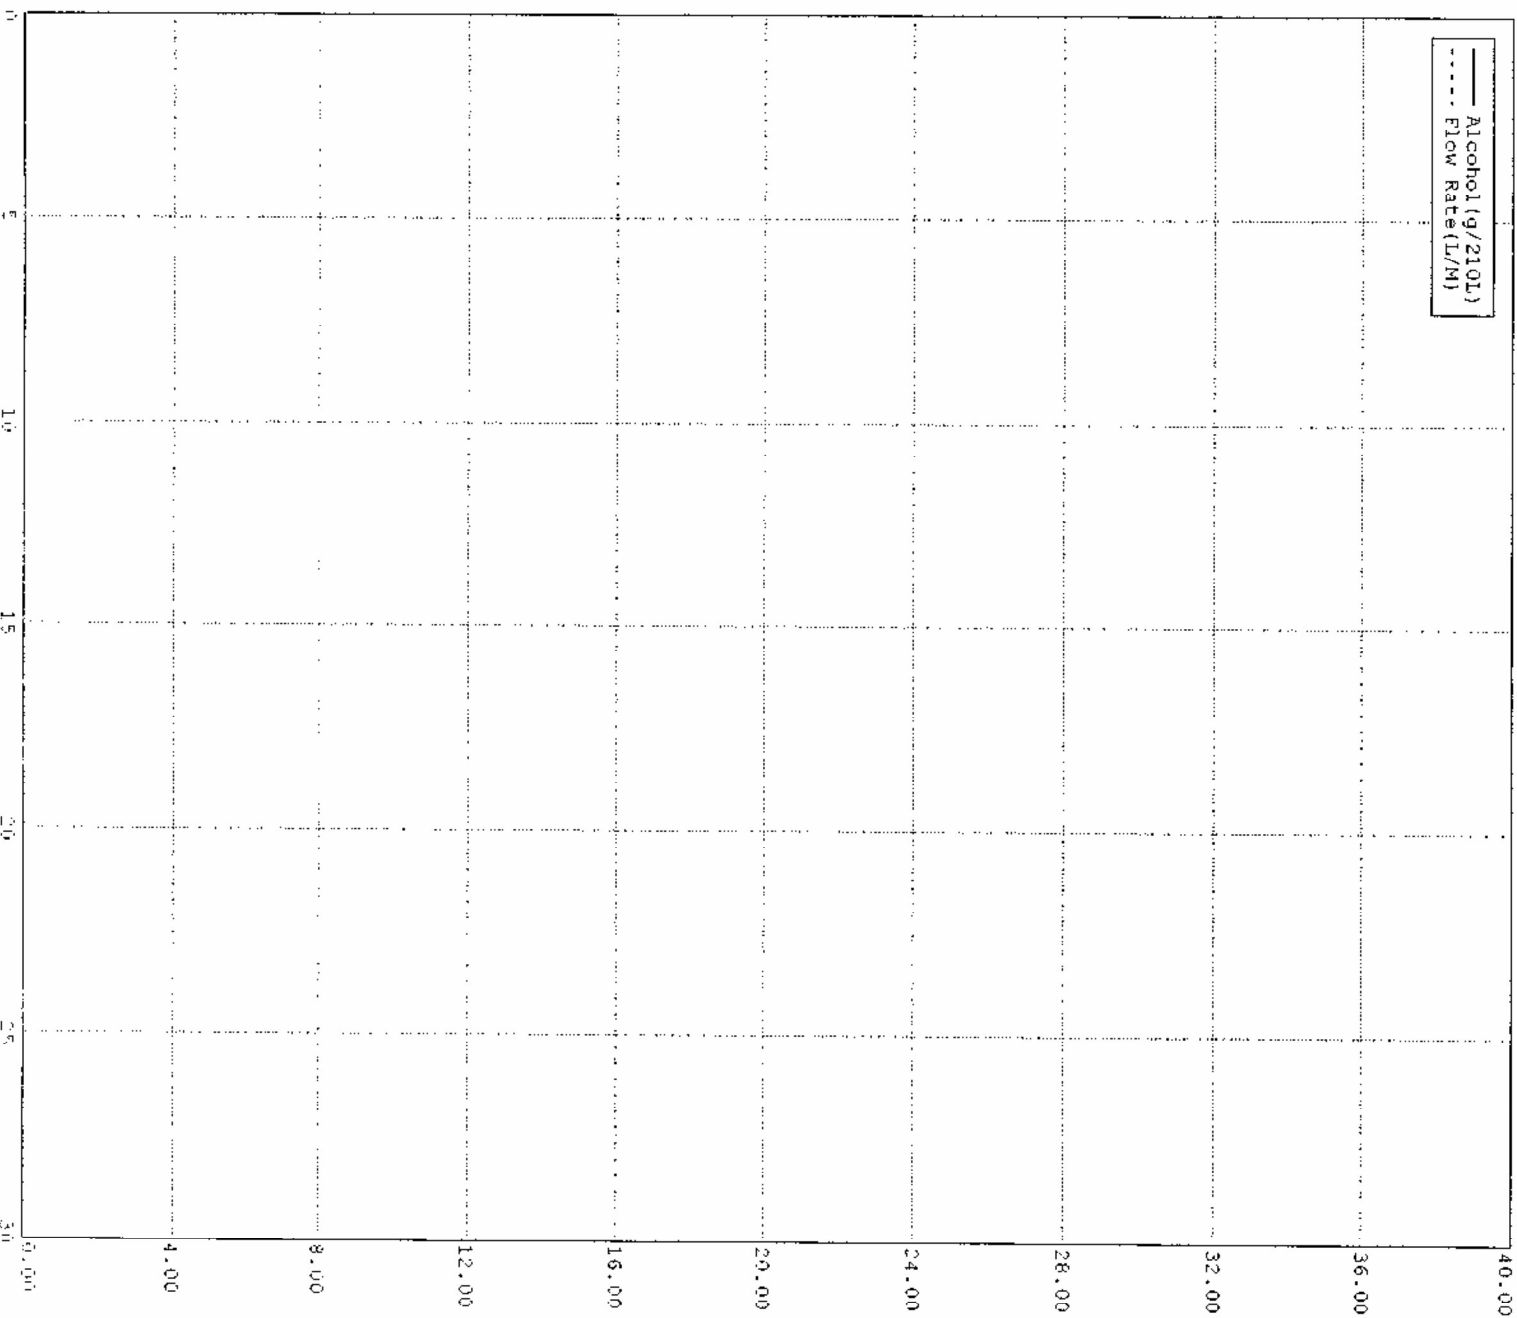

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100351

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 01/16/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 28.86: 0.077
 LOT #: 09214080A2
 EXPIRATION: 05/01/2016

BLANK TEST	0.000	16:02
INTERNAL STANDARD	VERIFIED	16:02
EXTERNAL STANDARD	0.076	16:02
BLANK TEST	0.000	16:03
EXTERNAL STANDARD	0.076	16:04
BLANK TEST	0.000	16:05
EXTERNAL STANDARD	0.076	16:05
BLANK TEST	0.000	16:06
EXTERNAL STANDARD	0.076	16:06
BLANK TEST	0.000	16:07
EXTERNAL STANDARD	0.076	16:07
BLANK TEST	0.000	16:08

Average = 0.0760
 Std Dev = 0.0000

Diagnostic Check

VERSIONS

DMT: 2.00
 PIC: 3.03
 Modem: 2.3
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C	PASSED
Breath Tube = 46.2°C	PASSED

PUMP INFO

Flow Rate = 4.734 L/M	PASSED
-----------------------	--------

DETECTOR INFO

PUMP ON	PASSED
PUMP OFF	PASSED

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
-------------------	--------

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this _____ day of _____, 20 _____