



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100687

**Report Issue Date:** 02/28/2024  
**Date Received:** 2023-11-30  
**Condition of Item:** Needs Repair

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 11/30/2023** - As Found - **End Date 12/01/2023** As Found - Evaluation Analyst: Carlie Glaister  
 As Found Conditions - Barometric Pressure (inHg): 28.84 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.5  
 Relative Humidity (%): 20

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.019	AG217902	0.019	0.019	0.019	0.019	0.019	0.019	0.019
0.080	0.077	AG310901	0.075	0.075	0.076	0.076	0.075	0.075	0.075
0.300	0.289	AG217903	0.287	0.288	0.287	0.288	0.288	0.288	0.288

Replaced o-ring. History of internal standard errors after refurbishment (100687 2021.02.23 Check In). Clean internal standard. Reset options.

**Start Date 02/13/2024** - As Left - **End Date 02/15/2024**

As Left Conditions - Barometric Pressure (inHg): 29.78 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.2 Relative Humidity (%): 14

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG217904	0.039	0.039	0.040	0.039	0.040	0.039	+/- 0.003
0.080	0.080	AG310901	0.077	0.078	0.078	0.078	0.078	0.078	+/- 0.004
0.100	0.099	AG333401	0.100	0.099	0.099	0.099	0.099	0.099	+/- 0.004
0.150	0.149	AG332004	0.145	0.145	0.145	0.145	0.145	0.145	+/- 0.005
0.300	0.298	AG327804	0.296	0.296	0.295	0.295	0.295	0.295	+/- 0.011

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

*C. O. Bryant*



State of Alaska  
Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
Anchorage, Alaska 99507  
David Kanaris, Chief, Forensic Laboratories

---

**Serial Number:** 100687

---

Results authorized by Colleen O'Bryant on 02/27/2024

[colleen.obryant@alaska.gov](mailto:colleen.obryant@alaska.gov)

Technically and administratively reviewed by Carlie Glaister on 02/28/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100687 Analyst or Technician Name: C. O'Bryant

DataMaster DMT Calibration Start Date: 2/13/24

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
  - Barometer/Thermometer/Hygrometer S/N: 221250180
  - Calibration Due Date: 2/14/24
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.78 Temperature(C) 22.2 Relative Humidity(%) 14  
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

- Acetone Reagent Lot Number: 20240214008 Expiration Date: 5/14/24  
Simulator S/N: SD1088 Thermometer Verification Performed?
- Isopropanol Reagent Lot Number: 20240214008 Expiration Date: 5/14/24  
Simulator S/N: DR4161 Thermometer Verification Performed?
- Negative (Ethanol Only) Lot Number: 22HP41201 Expiration Date: 5/14/24  
Simulator S/N: SD1177 Thermometer Verification Performed?  2024.08.24

Calibrated External Thermometer S/N: 230631106  
Calibration Due Date: 9/19/25

COB 2024.02.27

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 2/14/24

Data Interpretation Date (Technician): N/A (if applicable)

Data Interpretation Date (Analyst): 2/15/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety  
DATAMASTER dmt: 100687

Date: 02/14/2023  
Time: 16:43:18

VERSIONS

DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 47.6°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.56 V PASSED  
(0.94 V - 2.18 V)  
Cooler Voltage = 1.56 V PASSED  
(0.94 V - 2.18 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 541 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.7 in

PUMP INFO

Flow Rate = 4.587 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.097 0.54% PASSED  
(0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100687  
-----

Date: 02/15/2023  
Time: 11:14 AM

Temperatures (°C)

Sample Cell: 48.7°C  
Breath Tube: 47.1°C

Current Barometer 29.8 in  
Volume (Ltr) 1.54

Settings

Lamp: 1.56 V  
Bias: 80 V  
Cooler: 1.56 V  
Chopper: 540 Hz

Voltages (V)

Flow: 1.06 V  
Detector: -0.028 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100687  
-----

Date: 01/11/2024  
Time: 11:02:29

OPERATOR NAME:  
CARLIE GLAISTER  
CERTIFICATE #: 10436

Ca = 0.1000  
CAL = 0.993792    0.800 <= CAL < 1.200  
b1 = 0.0006    0.0000 <= b1 < 0.0040  
b2 = 0.0050    0.0010 <= b2 < 0.0100  
b3 = 0.0006    0.0000 <= b3 < 0.0040  
Xq = 0.0975    0.0500 <= Xq < 0.2000  
a21 = 1.155524    1.050 <= a21 < 1.300  
a31 = 0.529186    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100687

Date: 02/15/2023  
Time: 11:15:35


SUBJECT NAME:  
TEST TEST  
LICENSE #: VOLUME TEST

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.79: 0.080  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	TIME
BLANK TEST	0.000	11:17
INTERNAL STANDARD	VERIFIED	11:17
EXTERNAL STANDARD	0.078	11:17
BLANK TEST	0.000	11:18
SUBJECT SAMPLE (Vol=1.53L)	0.000	11:19
BLANK TEST	0.000	11:20
EXTERNAL STANDARD	0.078	11:20
BLANK TEST	0.000	11:21

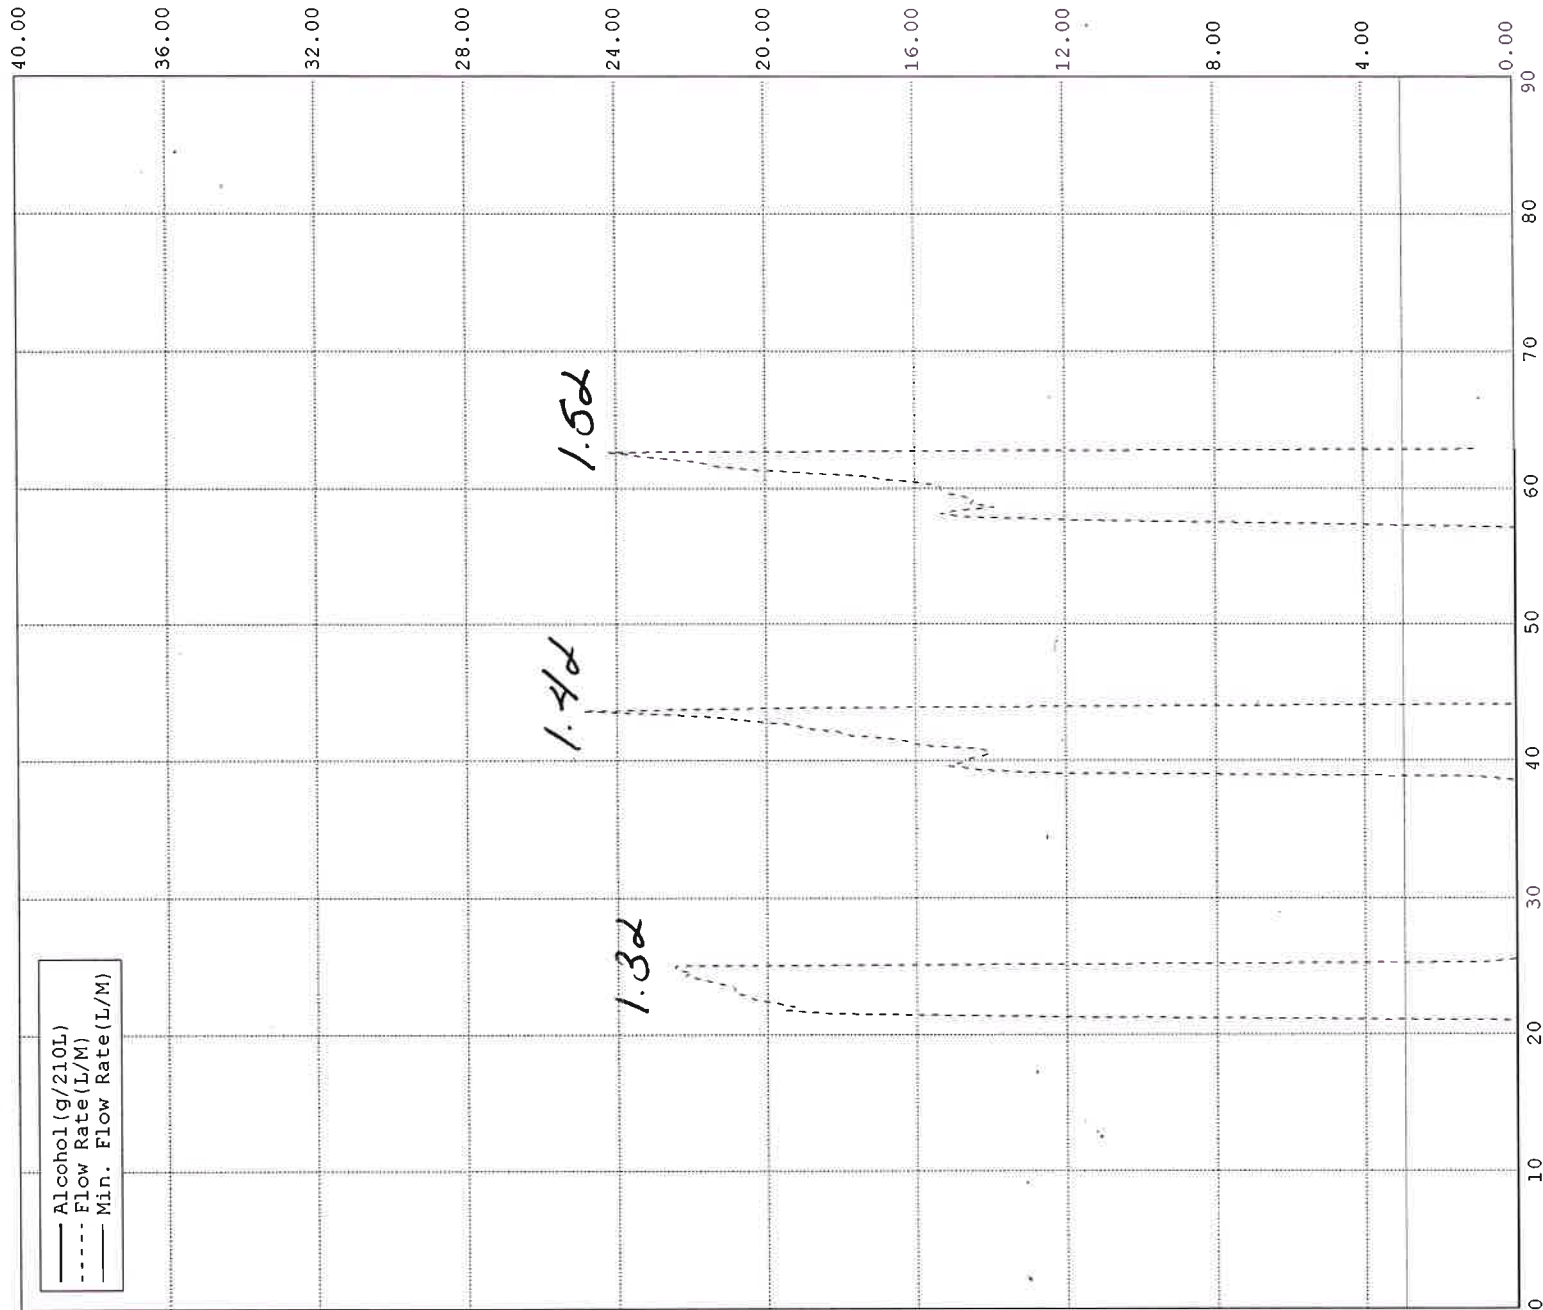

LINEARITY CHECK

Alaska Department of Public Safety  
 DATAMASTER dmt: 100687

Date: 02/15/2023  
 Time: 11:26:04

SUPERVISOR NAME:  
 COLLEEN S O'BRYAN  
 OPERATOR'S #: 6237


TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.040	0.0394	0.0005
0.080	0.0778	0.0004
0.099	0.0992	0.0004
0.149	0.1450	0.0000
0.298	0.2954	0.0005

SLOPE = 0.990169  
 R<sup>2</sup> = 0.999820

100687 2024.02.15 Calibration

Page 8 of 22

*CS*

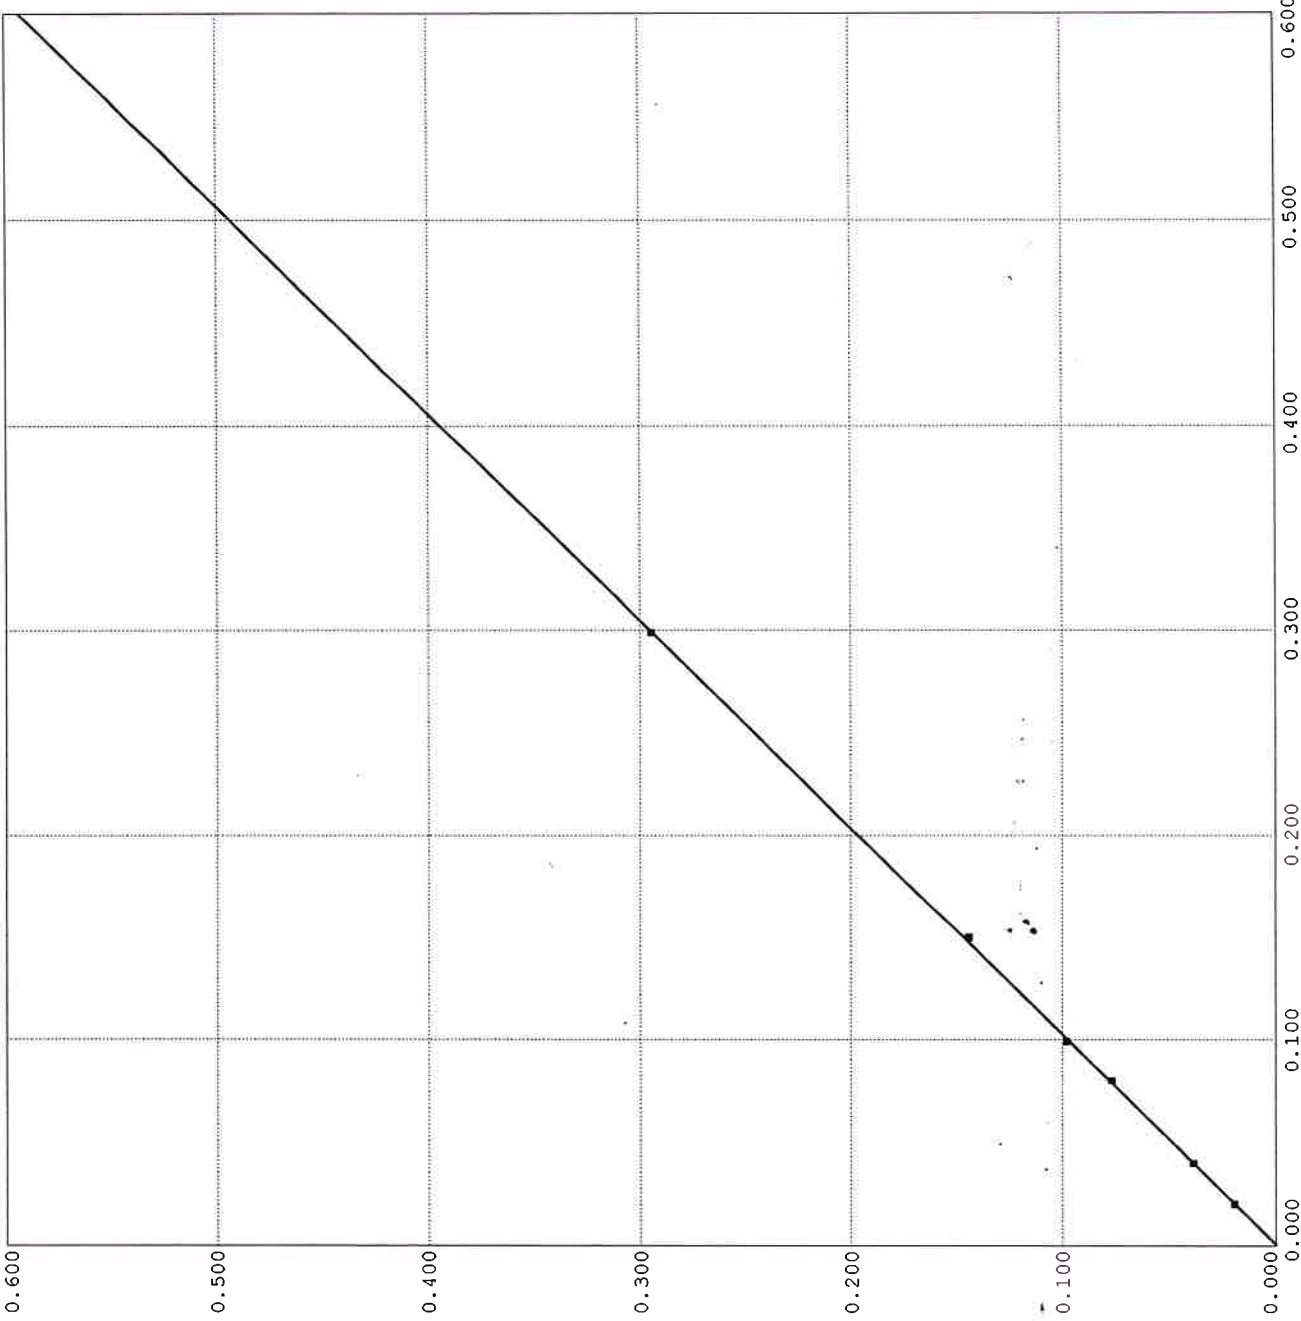



LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100687






Date: 02/15/2023  
Time: 11:26:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.79: 0.020  
LOT #: AG217902  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 329 psi

BLANK TEST	0.000	11:40
INTERNAL STANDARD	VERIFIED	11:40
EXTERNAL STANDARD	0.020	11:40
BLANK TEST	0.000	11:41
EXTERNAL STANDARD	0.020	11:41
BLANK TEST	0.000	11:42
EXTERNAL STANDARD	0.020	11:43
BLANK TEST	0.000	11:43
EXTERNAL STANDARD	0.020	11:44
BLANK TEST	0.000	11:44
EXTERNAL STANDARD	0.020	11:45
BLANK TEST	0.000	11:46

Average = 0.0200  
Std Dev = 0.0000

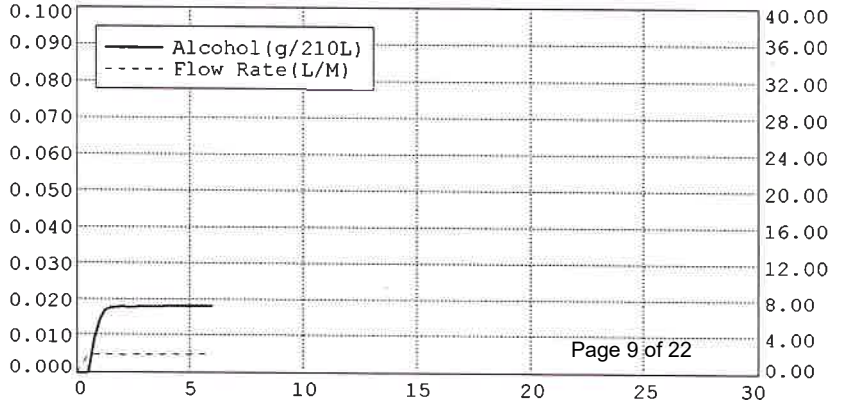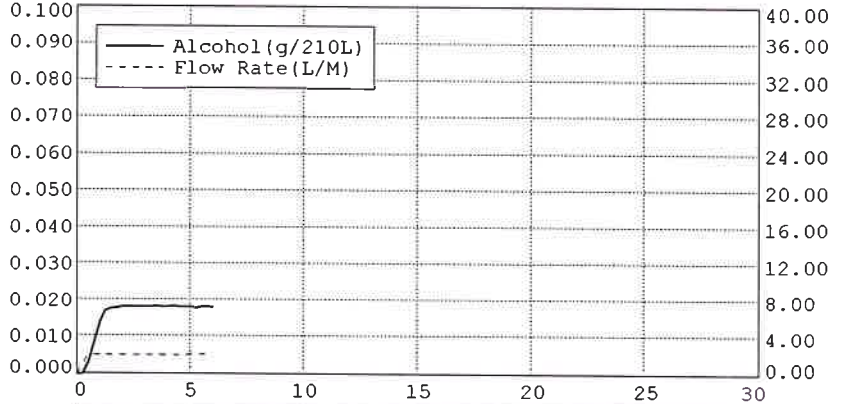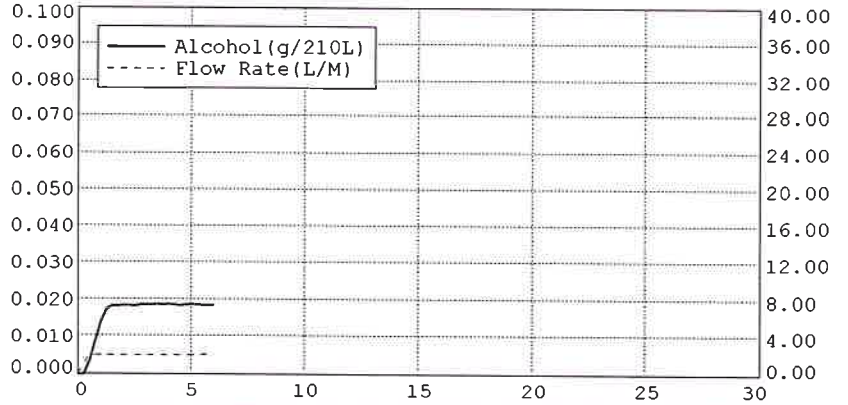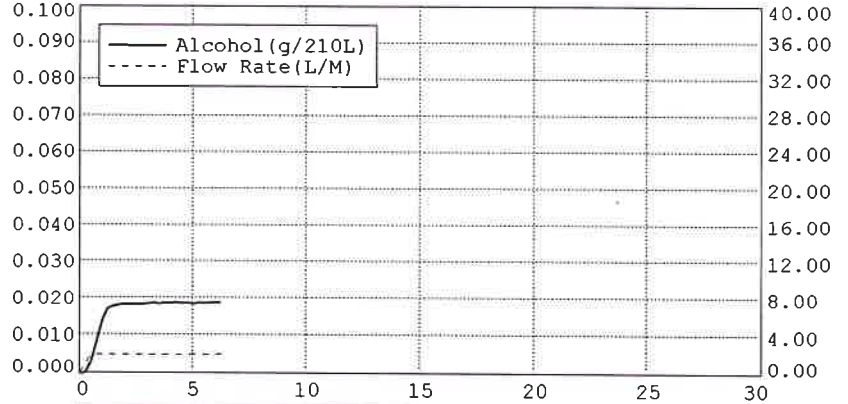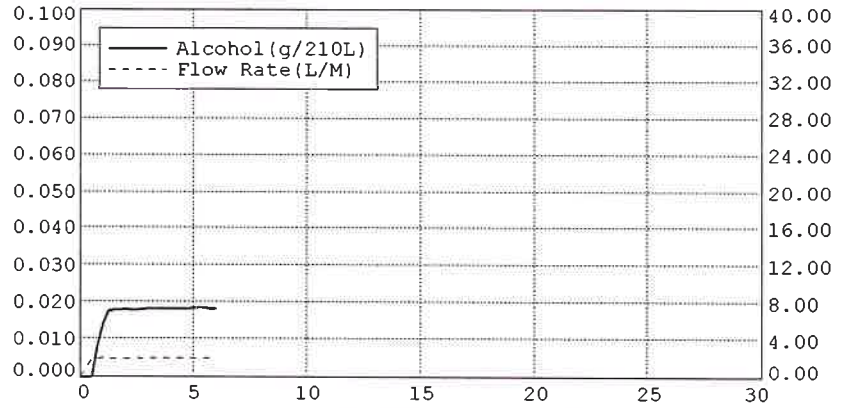

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100687






Date: 02/15/2023  
 Time: 11:51:25

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.78: 0.040  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 693 psi

BLANK TEST	0.000	11:52
INTERNAL STANDARD	VERIFIED	11:52
EXTERNAL STANDARD	0.039	11:52
BLANK TEST	0.000	11:53
EXTERNAL STANDARD	0.039	11:53
BLANK TEST	0.000	11:54
EXTERNAL STANDARD	0.040	11:55
BLANK TEST	0.000	11:55
EXTERNAL STANDARD	0.039	11:56
BLANK TEST	0.000	11:57
EXTERNAL STANDARD	0.040	11:57
BLANK TEST	0.000	11:58

Average = 0.0394  
 Std Dev = 0.0005

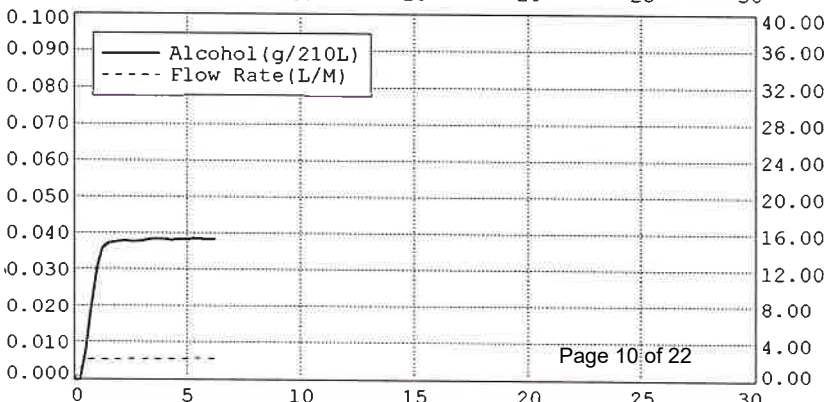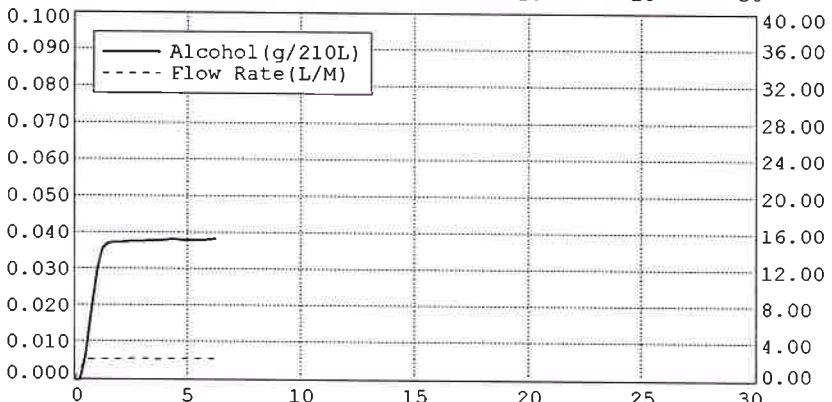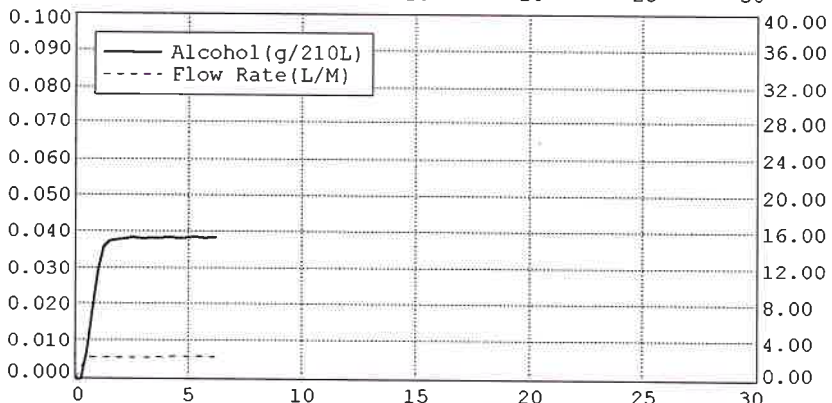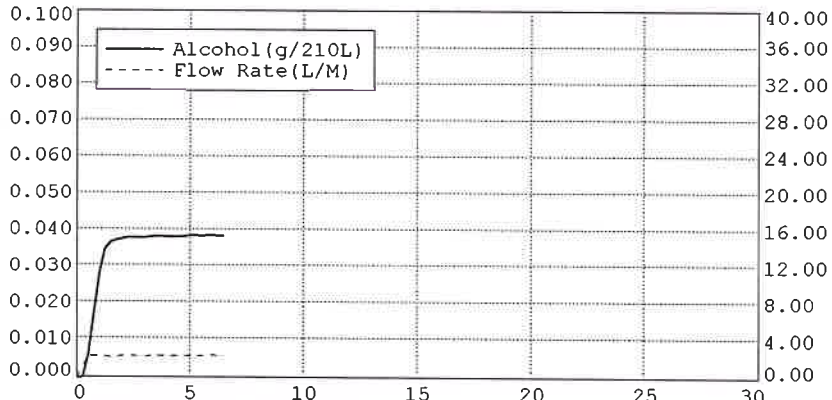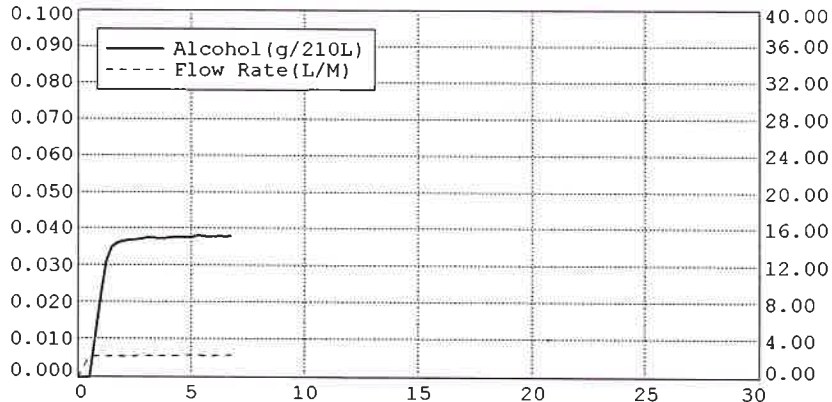

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
DATAMASTER dmt: 100687






Date: 02/15/2023  
Time: 12:01:27

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.79: 0.080  
LOT #: AG310901  
EXPIRATION: 04/19/2025  
TANK PRESSURE: 342 psi

BLANK TEST	0.000	12:02
INTERNAL STANDARD	VERIFIED	12:02
EXTERNAL STANDARD	0.077	12:02
BLANK TEST	0.000	12:03
EXTERNAL STANDARD	0.078	12:04
BLANK TEST	0.000	12:04
EXTERNAL STANDARD	0.078	12:05
BLANK TEST	0.000	12:06
EXTERNAL STANDARD	0.078	12:06
BLANK TEST	0.000	12:07
EXTERNAL STANDARD	0.078	12:07
BLANK TEST	0.000	12:08

Average = 0.0778  
Std Dev = 0.0004

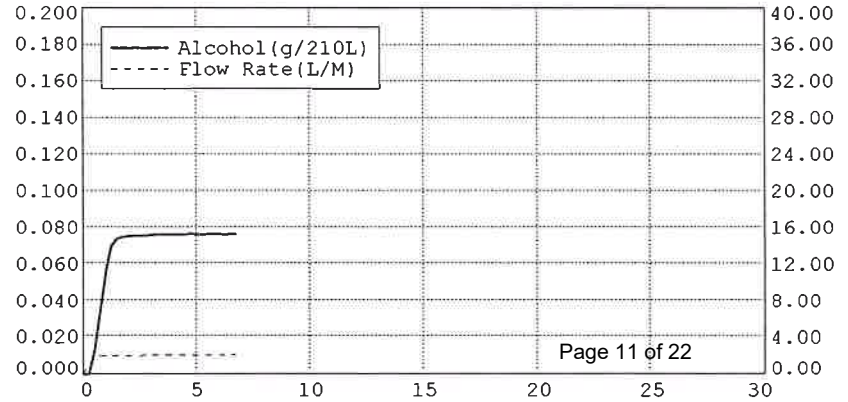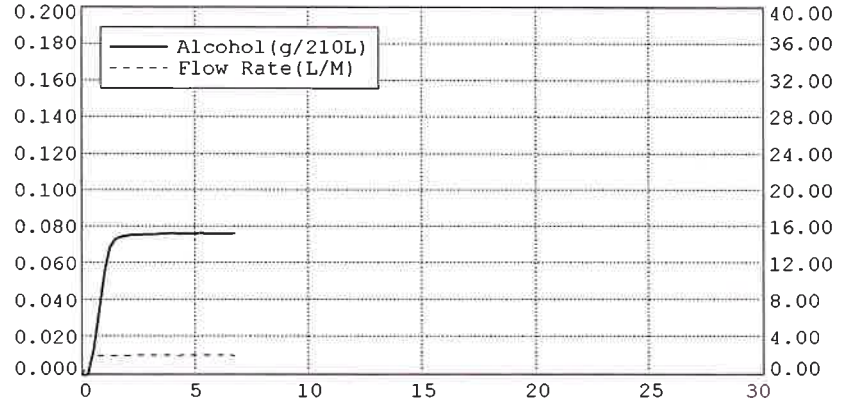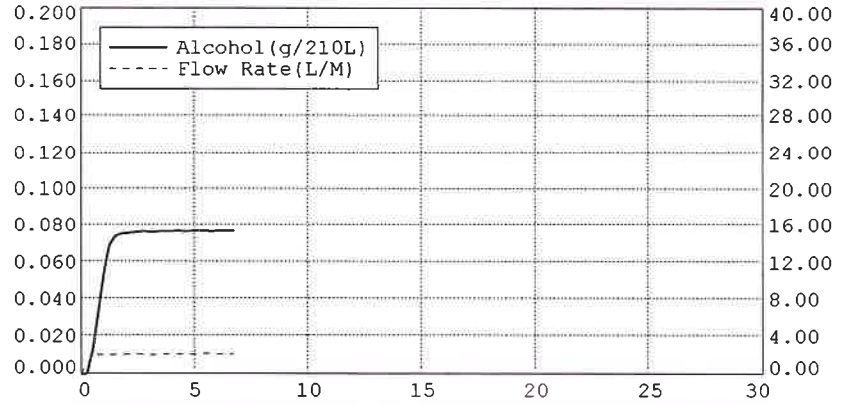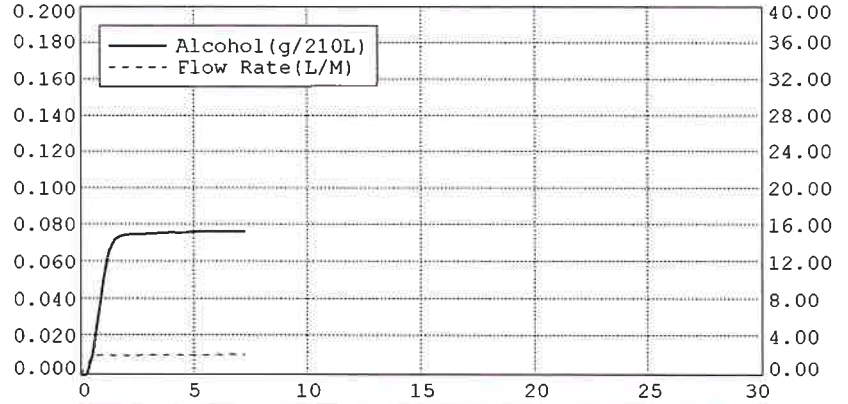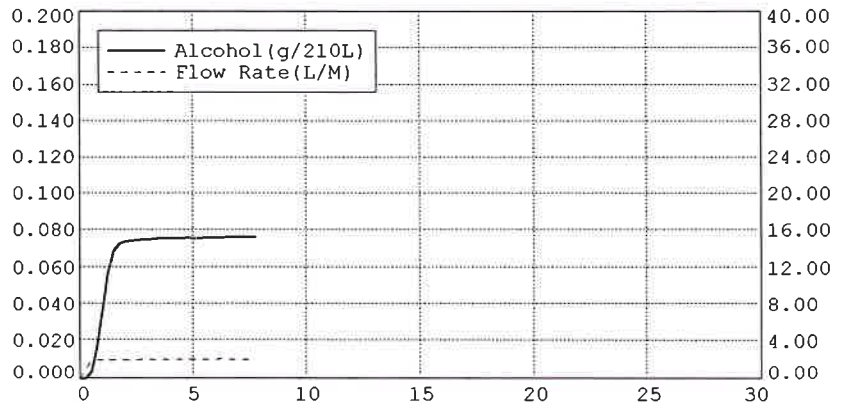

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
DATAMASTER dmt: 100687






Date: 02/15/2023  
Time: 12:08:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
TARGET AT 29.77: 0.099  
LOT #: AG333401  
EXPIRATION: 11/30/2025  
TANK PRESSURE: 1098 psi

BLANK TEST	0.000	12:09
INTERNAL STANDARD	VERIFIED	12:09
EXTERNAL STANDARD	0.100	12:10
BLANK TEST	0.000	12:11
EXTERNAL STANDARD	0.099	12:11
BLANK TEST	0.000	12:12
EXTERNAL STANDARD	0.099	12:12
BLANK TEST	0.000	12:13
EXTERNAL STANDARD	0.099	12:13
BLANK TEST	0.000	12:14
EXTERNAL STANDARD	0.099	12:14
BLANK TEST	0.000	12:15

Average = 0.0992  
Std Dev = 0.0004

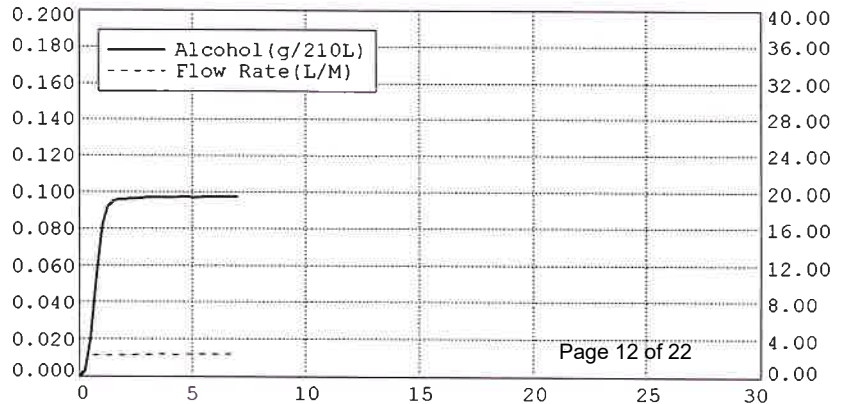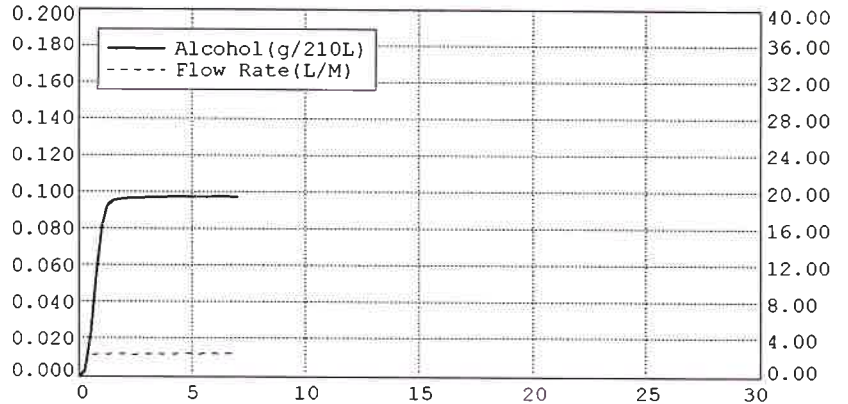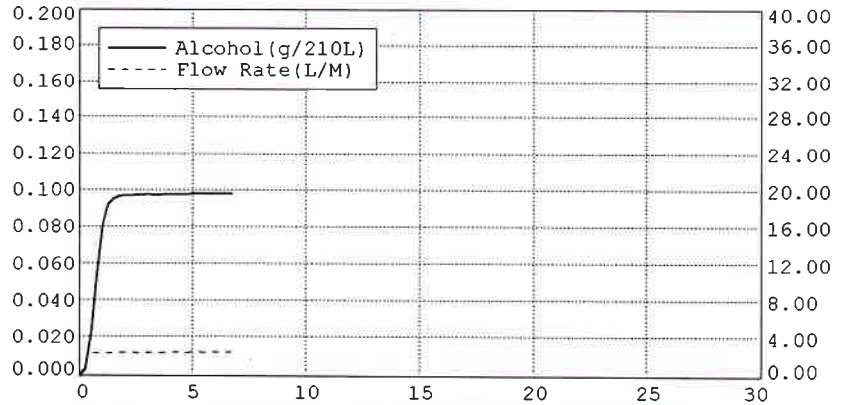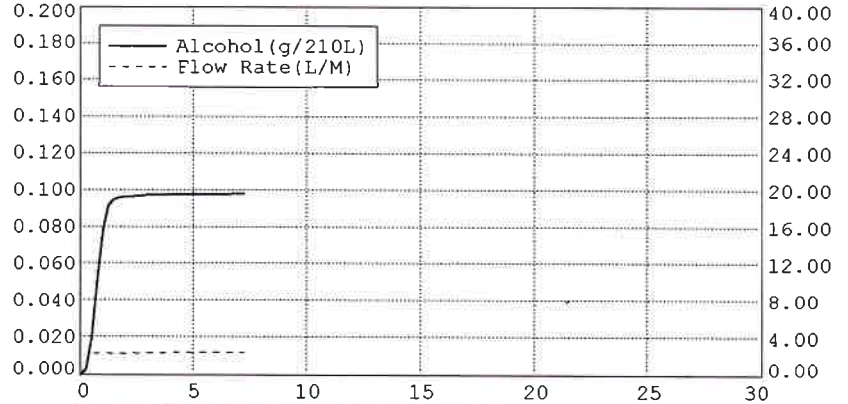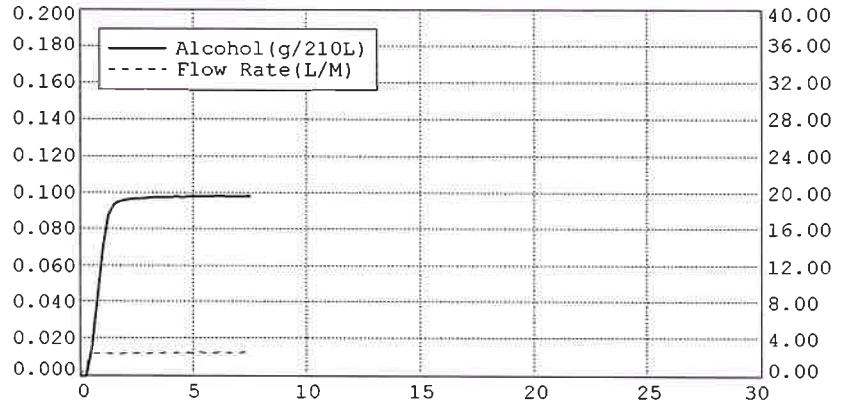

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
DATAMASTER dmt: 100687






Date: 02/15/2023  
Time: 12:16:25

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
TARGET AT 29.76: 0.149  
LOT #: AG332004  
EXPIRATION: 11/16/2025  
TANK PRESSURE: 438 psi

BLANK TEST	0.000	12:17
INTERNAL STANDARD	VERIFIED	12:17
EXTERNAL STANDARD	0.145	12:17
BLANK TEST	0.000	12:18
EXTERNAL STANDARD	0.145	12:19
BLANK TEST	0.000	12:19
EXTERNAL STANDARD	0.145	12:20
BLANK TEST	0.000	12:21
EXTERNAL STANDARD	0.145	12:21
BLANK TEST	0.000	12:22
EXTERNAL STANDARD	0.145	12:22
BLANK TEST	0.000	12:23

Average = 0.1450  
Std Dev = 0.0000

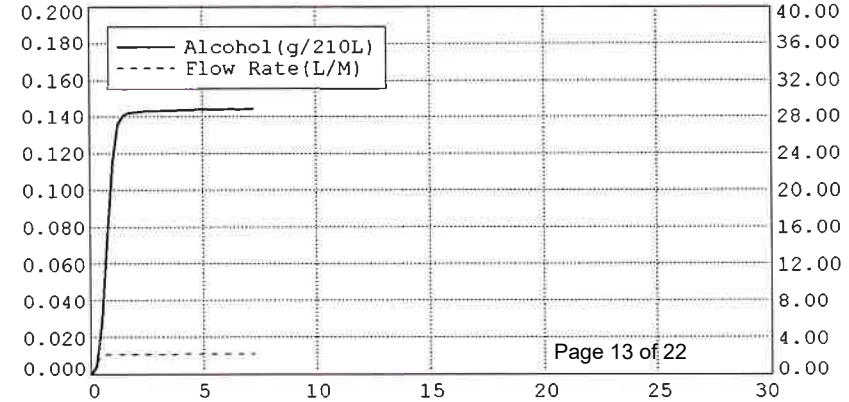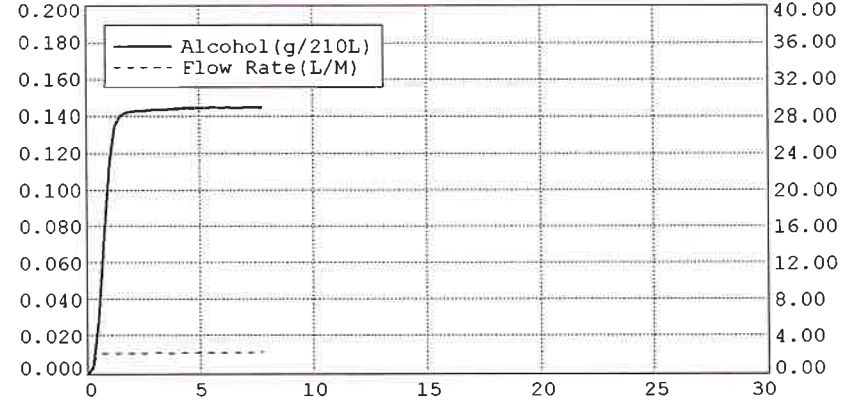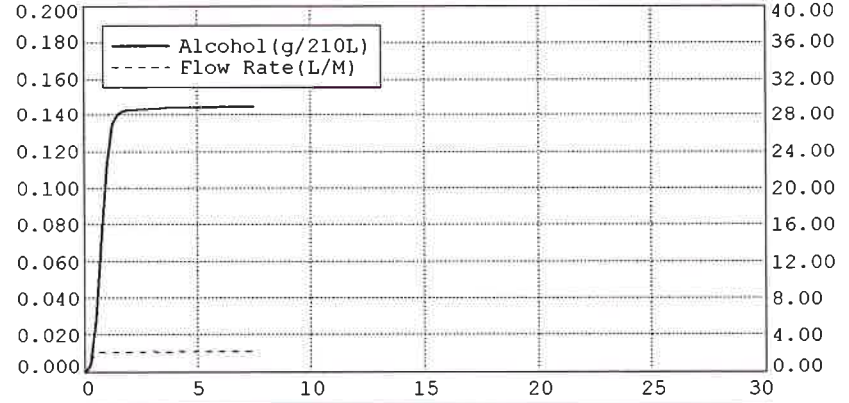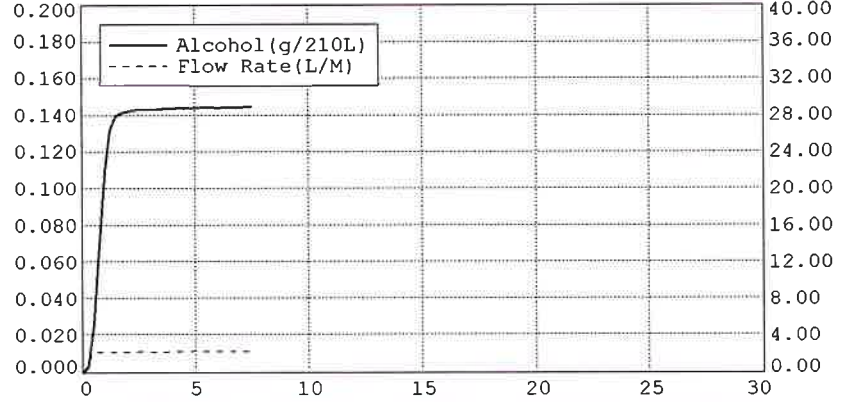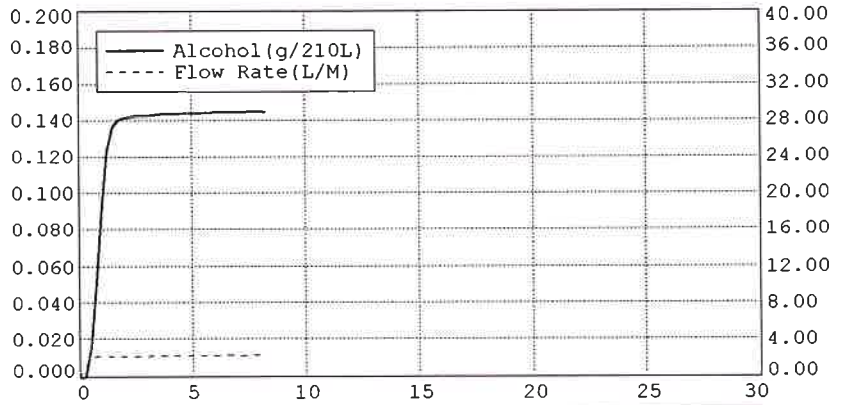

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
DATAMASTER dmt: 100687






Date: 02/15/2023  
Time: 12:23:38

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
TARGET AT 29.76: 0.298  
LOT #: AG327804  
EXPIRATION: 10/05/2025  
TANK PRESSURE: 378 psi

BLANK TEST	0.000	12:24
INTERNAL STANDARD	VERIFIED	12:24
EXTERNAL STANDARD	0.296	12:25
BLANK TEST	0.000	12:26
EXTERNAL STANDARD	0.296	12:26
BLANK TEST	0.000	12:27
EXTERNAL STANDARD	0.295	12:27
BLANK TEST	0.000	12:28
EXTERNAL STANDARD	0.295	12:28
BLANK TEST	0.000	12:29
EXTERNAL STANDARD	0.295	12:29
BLANK TEST	0.000	12:30

Average = 0.2954  
Std Dev = 0.0005

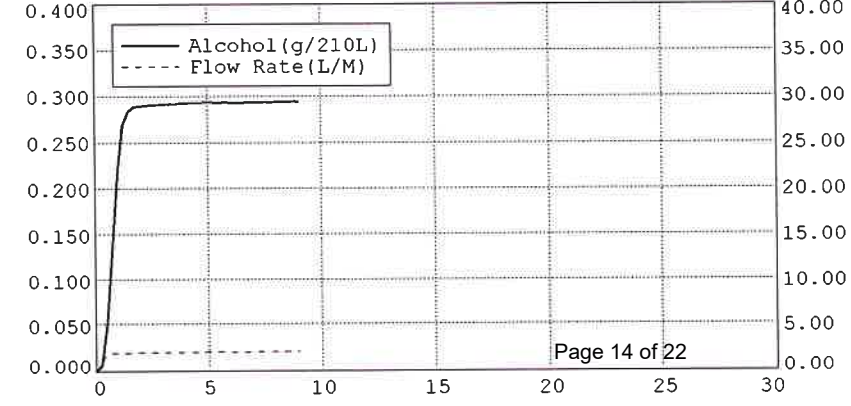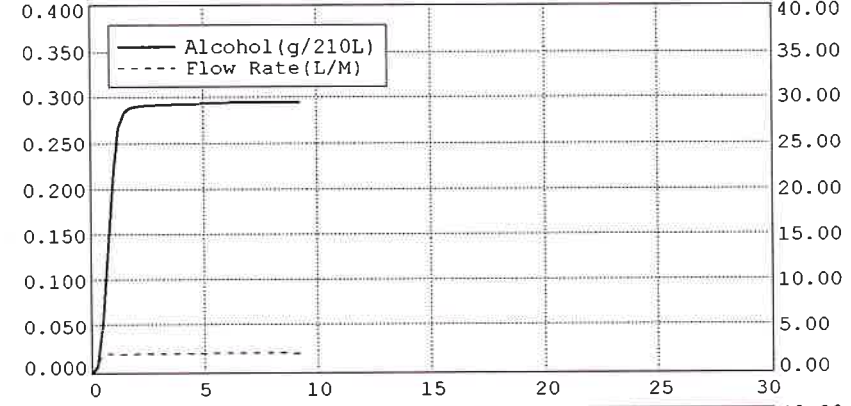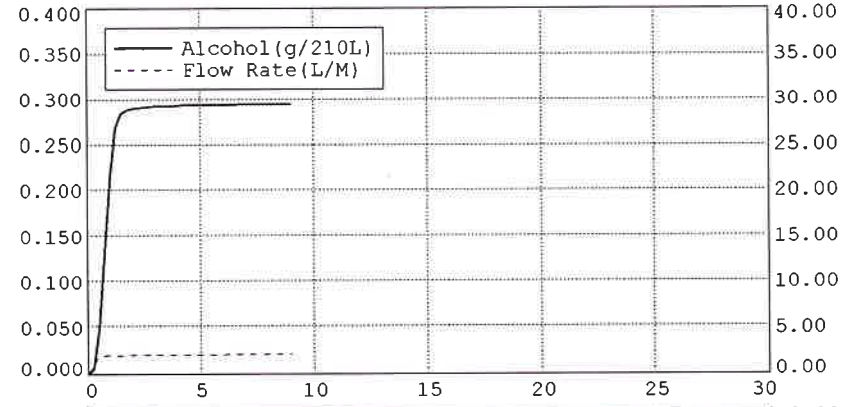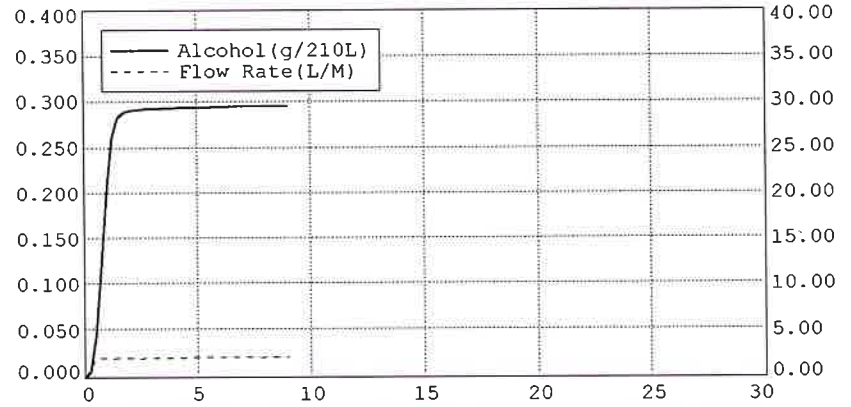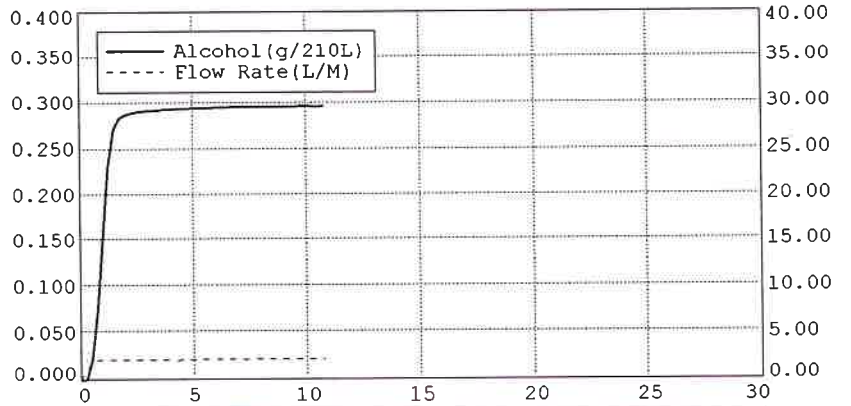

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100687

Date: 02/15/2023  
Time: 14:08:43


SUBJECT NAME:  
TEST TEST  
LICENSE #: INCOMPLETE

OPERATOR NAME:  
COLLEEN S OBRYANT  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.74: 0.080  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:10
BLANK TEST	0.000	14:10
INTERNAL STANDARD	VERIFIED	14:10
EXTERNAL STANDARD	0.078	14:10
BLANK TEST	0.000	14:11
SUBJECT SAMPLE	INCOMPLETE	14:13

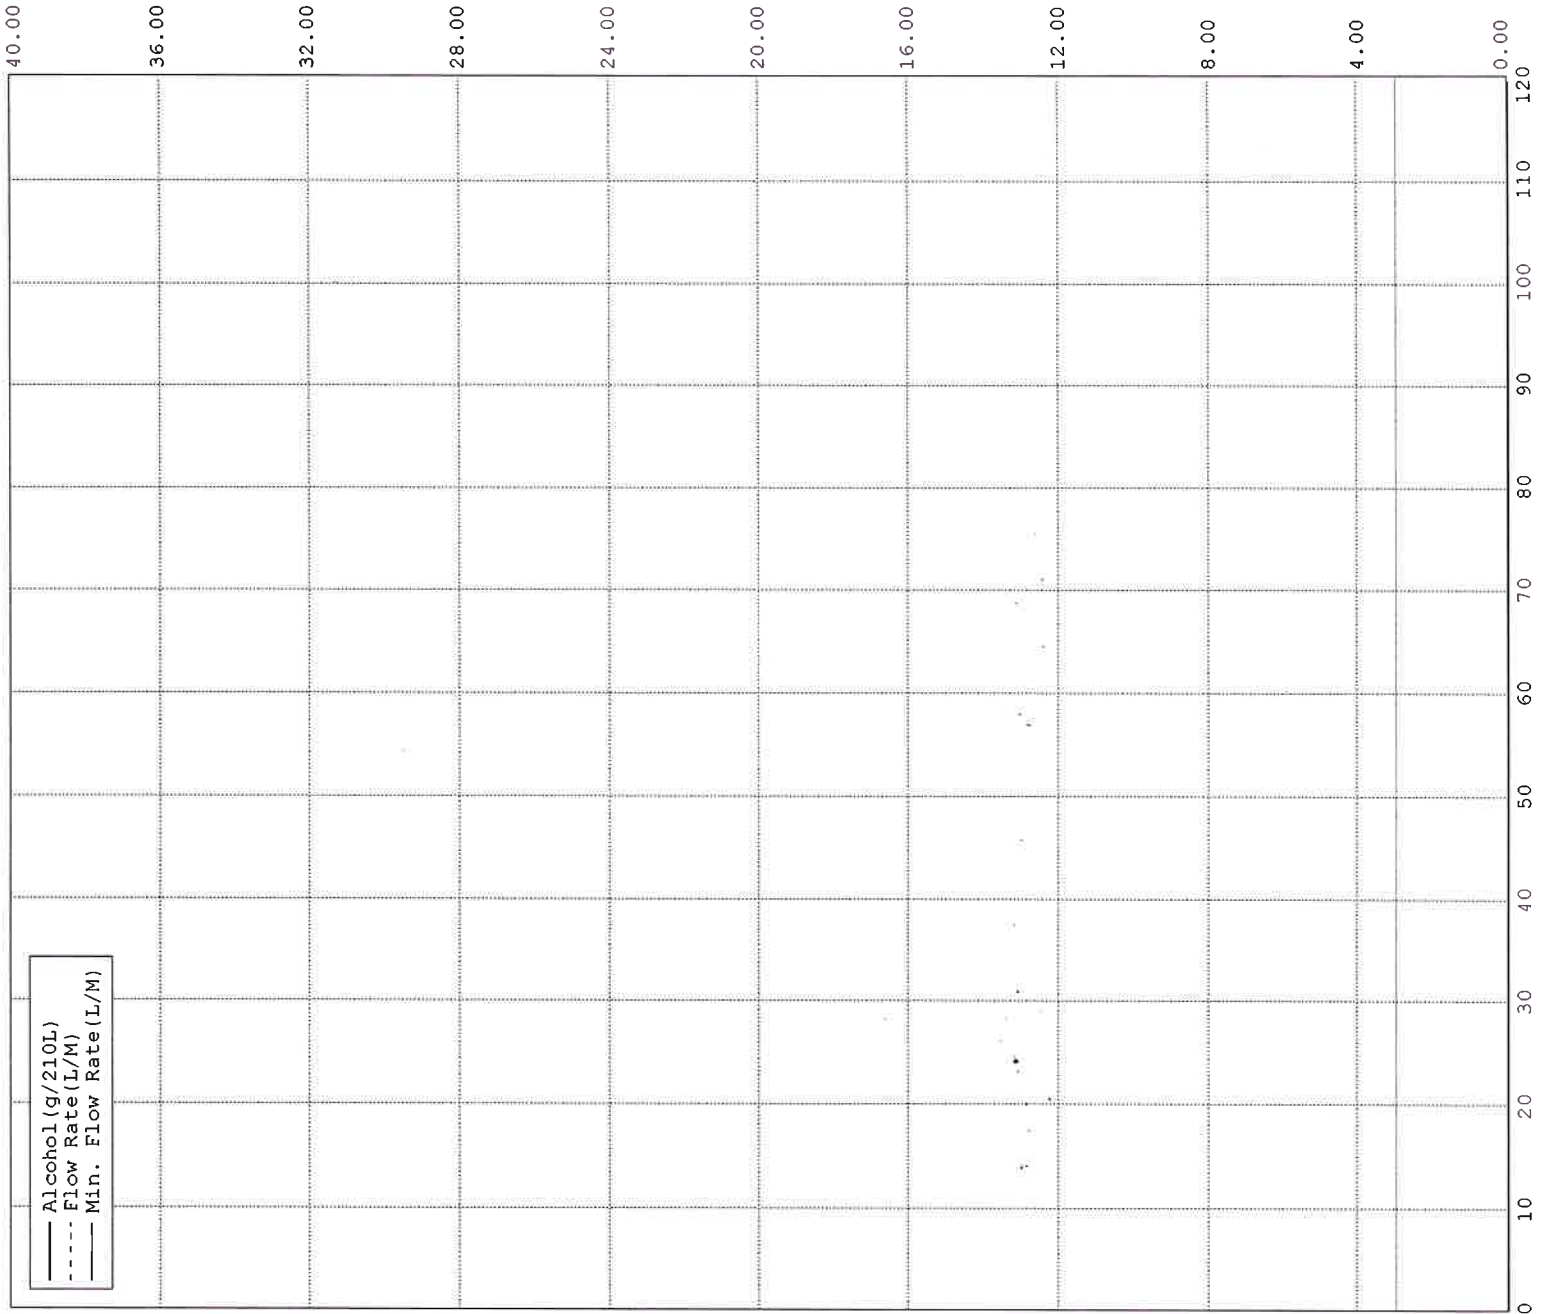

SUBJECT TEST

Alaska Department of Public Safety  
DATA MASTER dmt: 100687

Date: 02/15/2023  
Time: 14:16:49

SUBJECT NAME:  
TEST TEST  
LICENSE #: MAX ATTEMPTS


OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.73: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:17
BLANK TEST	0.000	14:17
INTERNAL STANDARD	VERIFIED	14:18
EXTERNAL STANDARD	0.078	14:18
BLANK TEST	0.000	14:19
SUBJECT SAMPLE	XXX	14:19

Maximum Attempts Exceeded

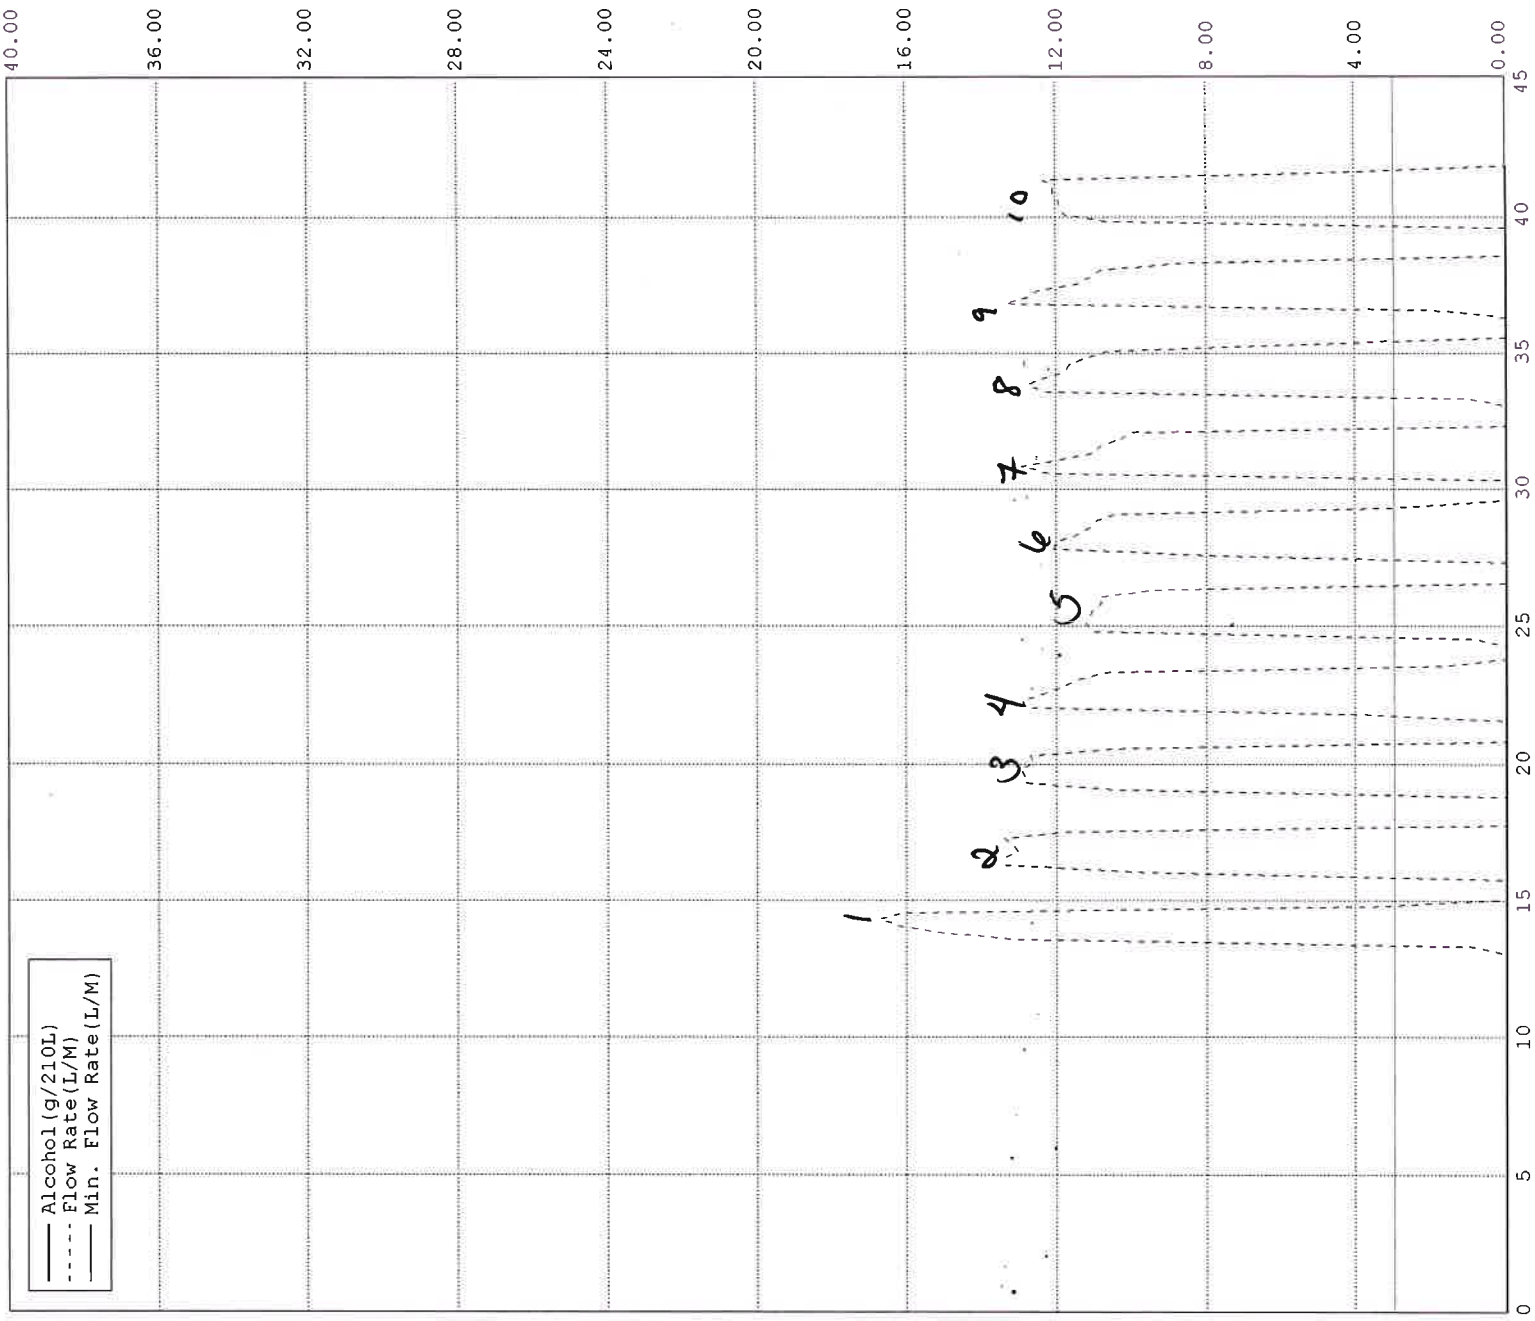



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100687

Date: 02/15/2023  
Time: 14:21:42

SUBJECT NAME:  
TEST TEST  
LICENSE #: INVALID


OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.73: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:22
BLANK TEST	0.000	14:22
INTERNAL STANDARD	VERIFIED	14:23
EXTERNAL STANDARD	0.078	14:23
BLANK TEST	0.000	14:24
SUBJECT SAMPLE	INVALID	14:24

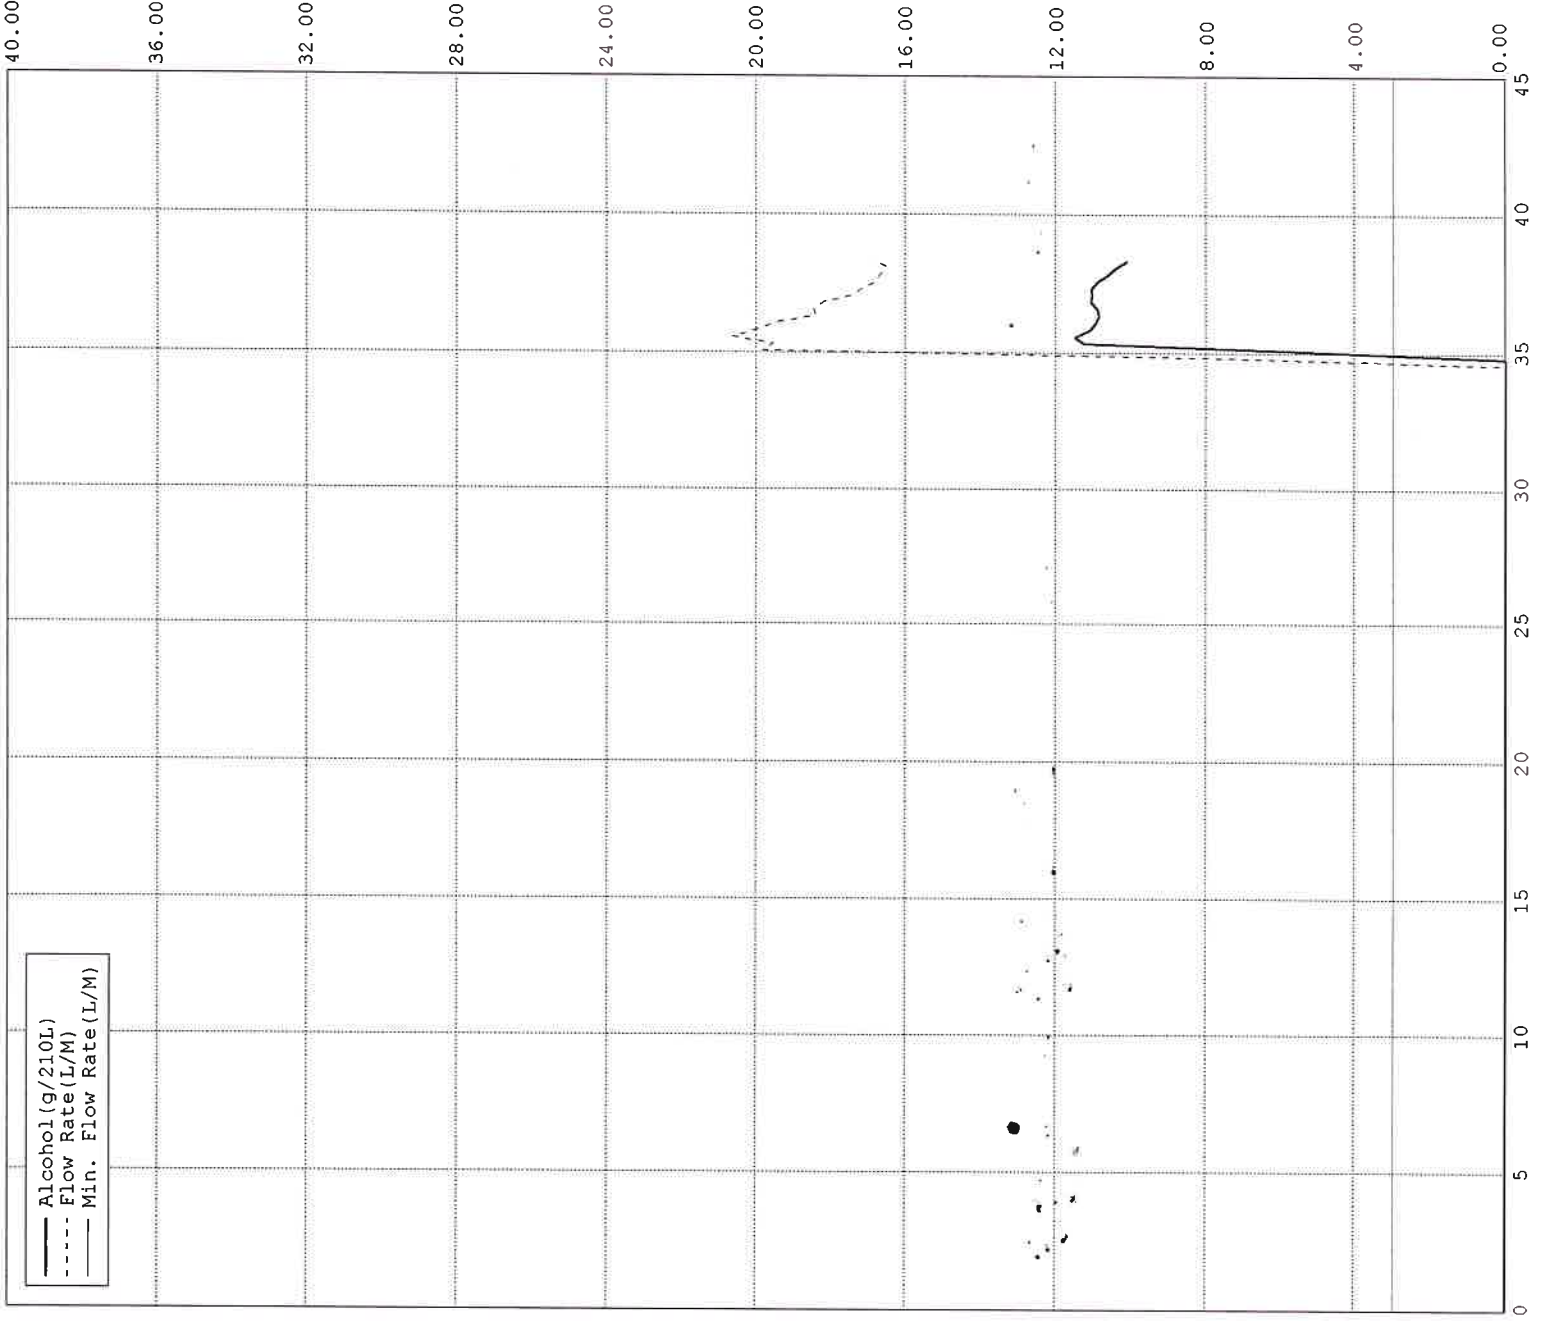

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100687

Date: 02/15/2023  
Time: 14:27:13

SUBJECT NAME:  
TEST TEST  
LICENSE #: RFI


OPERATOR NAME:  
COLLEEN S OBRVANT  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.74: 0.080  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 14:28  
BLANK TEST 0.000 14:28  
INTERNAL STANDARD VERIFIED 14:28  
EXTERNAL STANDARD 0.078 14:28  
BLANK TEST 0.000 14:29

RFI DETECTED

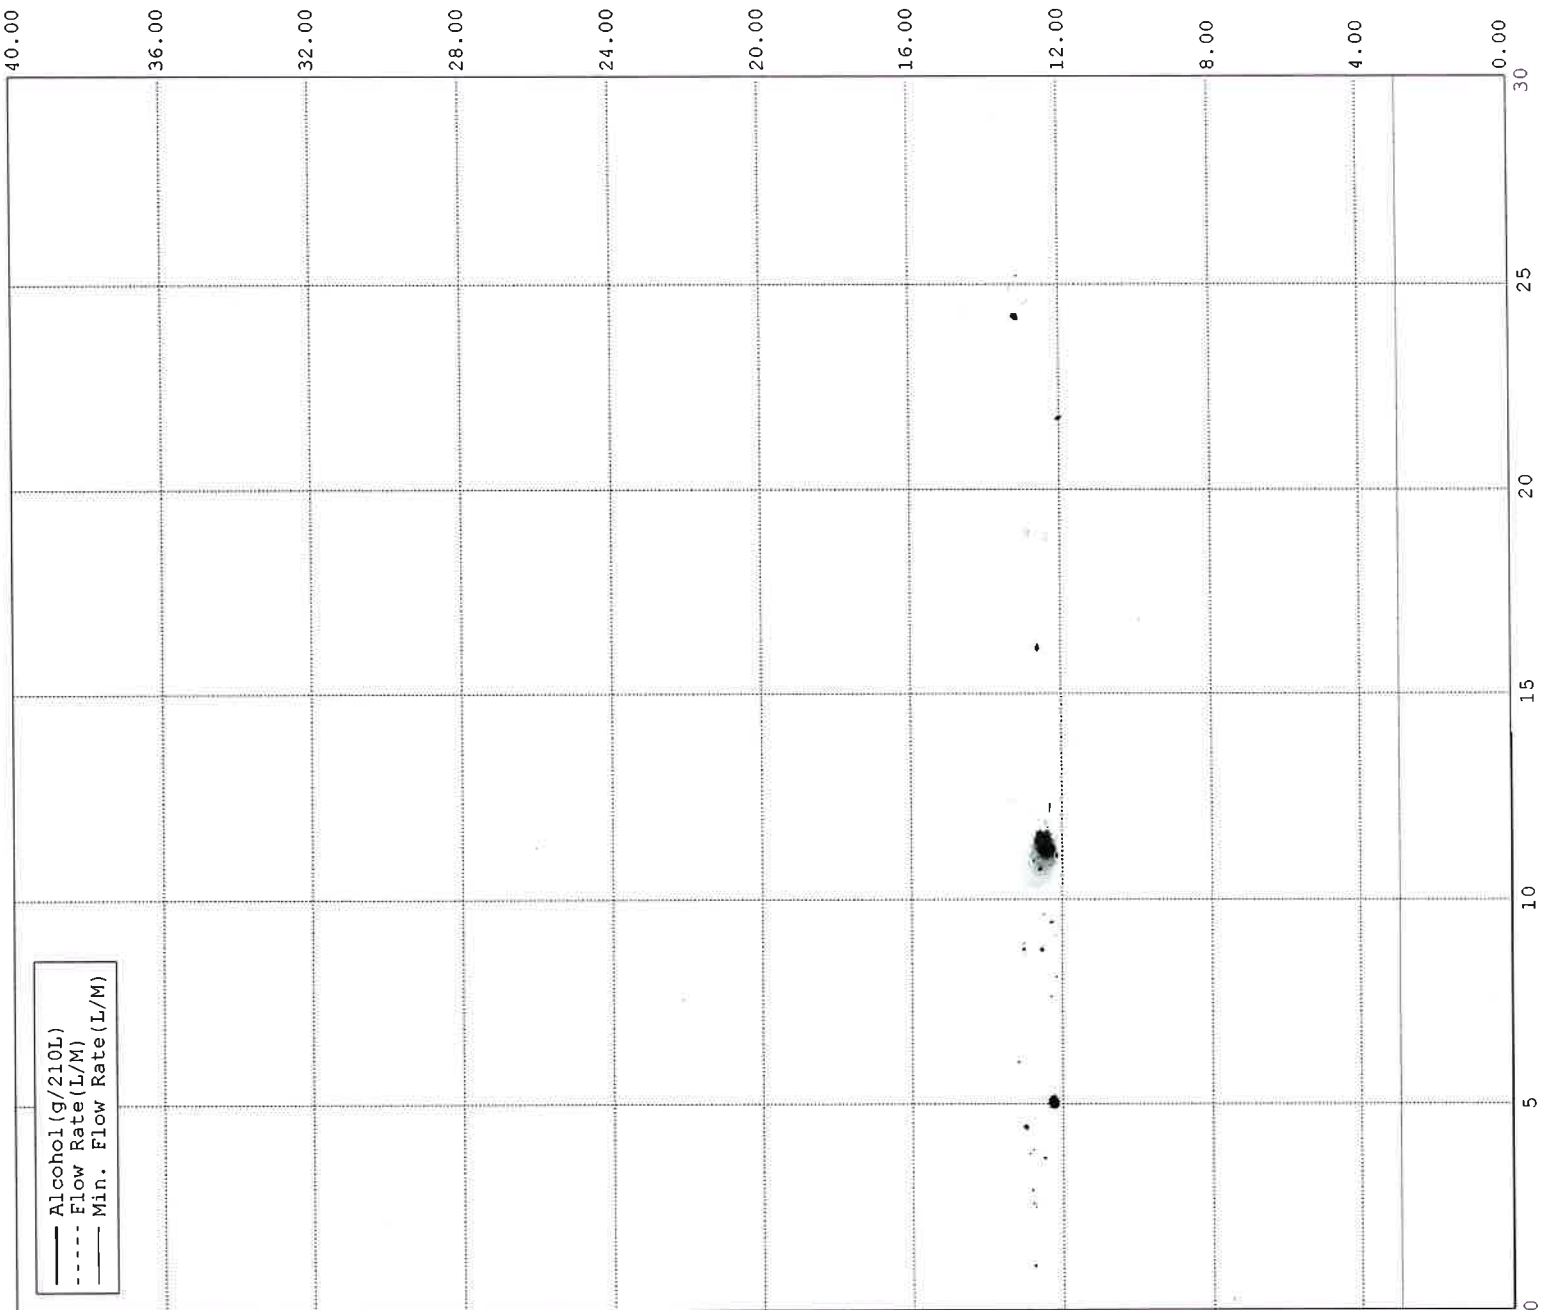

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100687

Date: 02/15/2023  
Time: 14:59:08

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-ACETONE

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080  
TARGET AT 29.73: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 15:02  
BLANK TEST 0.000 15:02  
INTERNAL STANDARD VERIFIED 15:02  
Xq = 0.098 (0.008) 0.078 15:02  
EXTERNAL STANDARD X[1] = 0.0782 (-0.0012) (0.0016)  
BLANK TEST 0.000 15:03  
SUBJECT SAMPLE XXX 15:04  
X[1] = 0.1080 (-0.0216) (-0.0009)

Interference Detected

*Filter Avg = -0.0011*

*Filter 3 Avg = 0.0019*

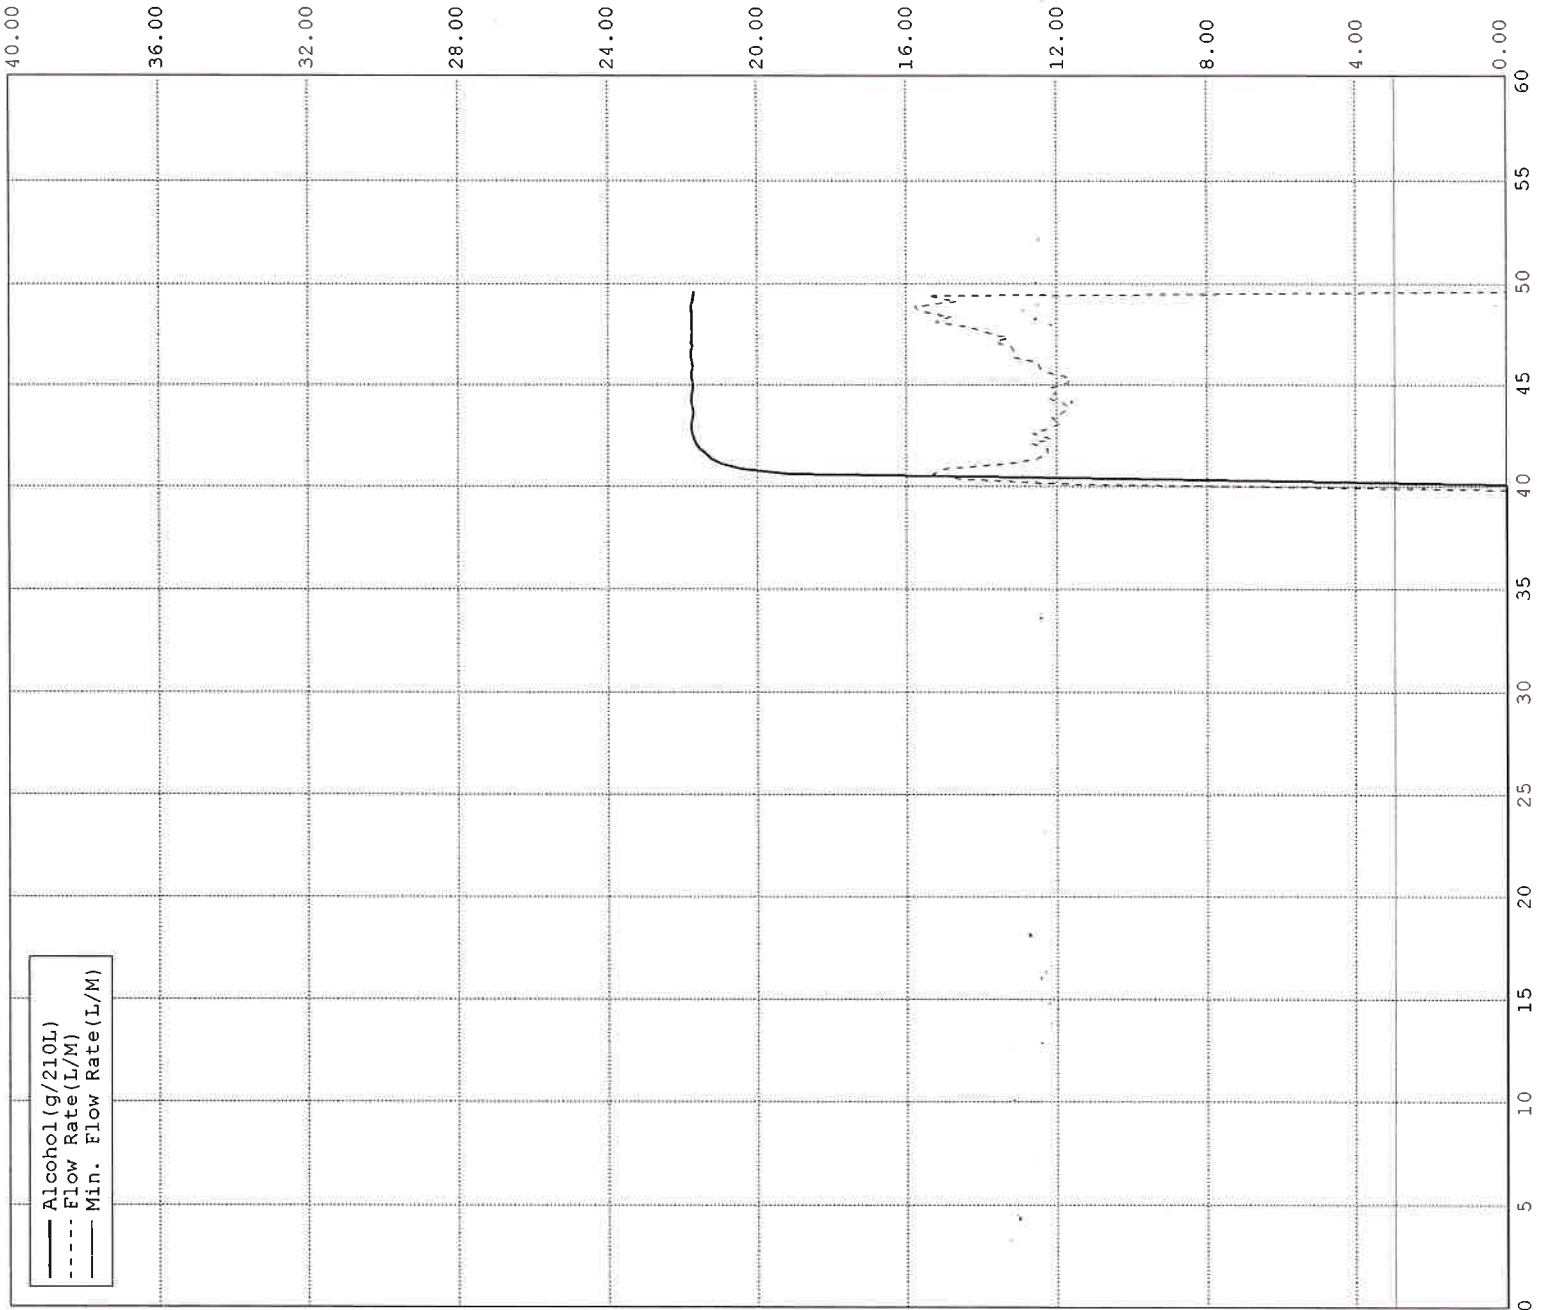

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100687

Date: 02/15/2023  
Time: 15:13:14

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-IPA

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1


CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.72: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	15:14
BLANK TEST	0.000	15:15
INTERNAL STANDARD	VERIFIED	15:15
Xq = 0.098 (0.368)		
EXTERNAL STANDARD	0.078	15:15
X[1] = 0.0780 (-0.0013) (0.0023)		
BLANK TEST	0.000	15:16
SUBJECT SAMPLE	XXX	15:16
X[1] = 0.1205 (-0.0213) (0.0015)		

Interference Detected

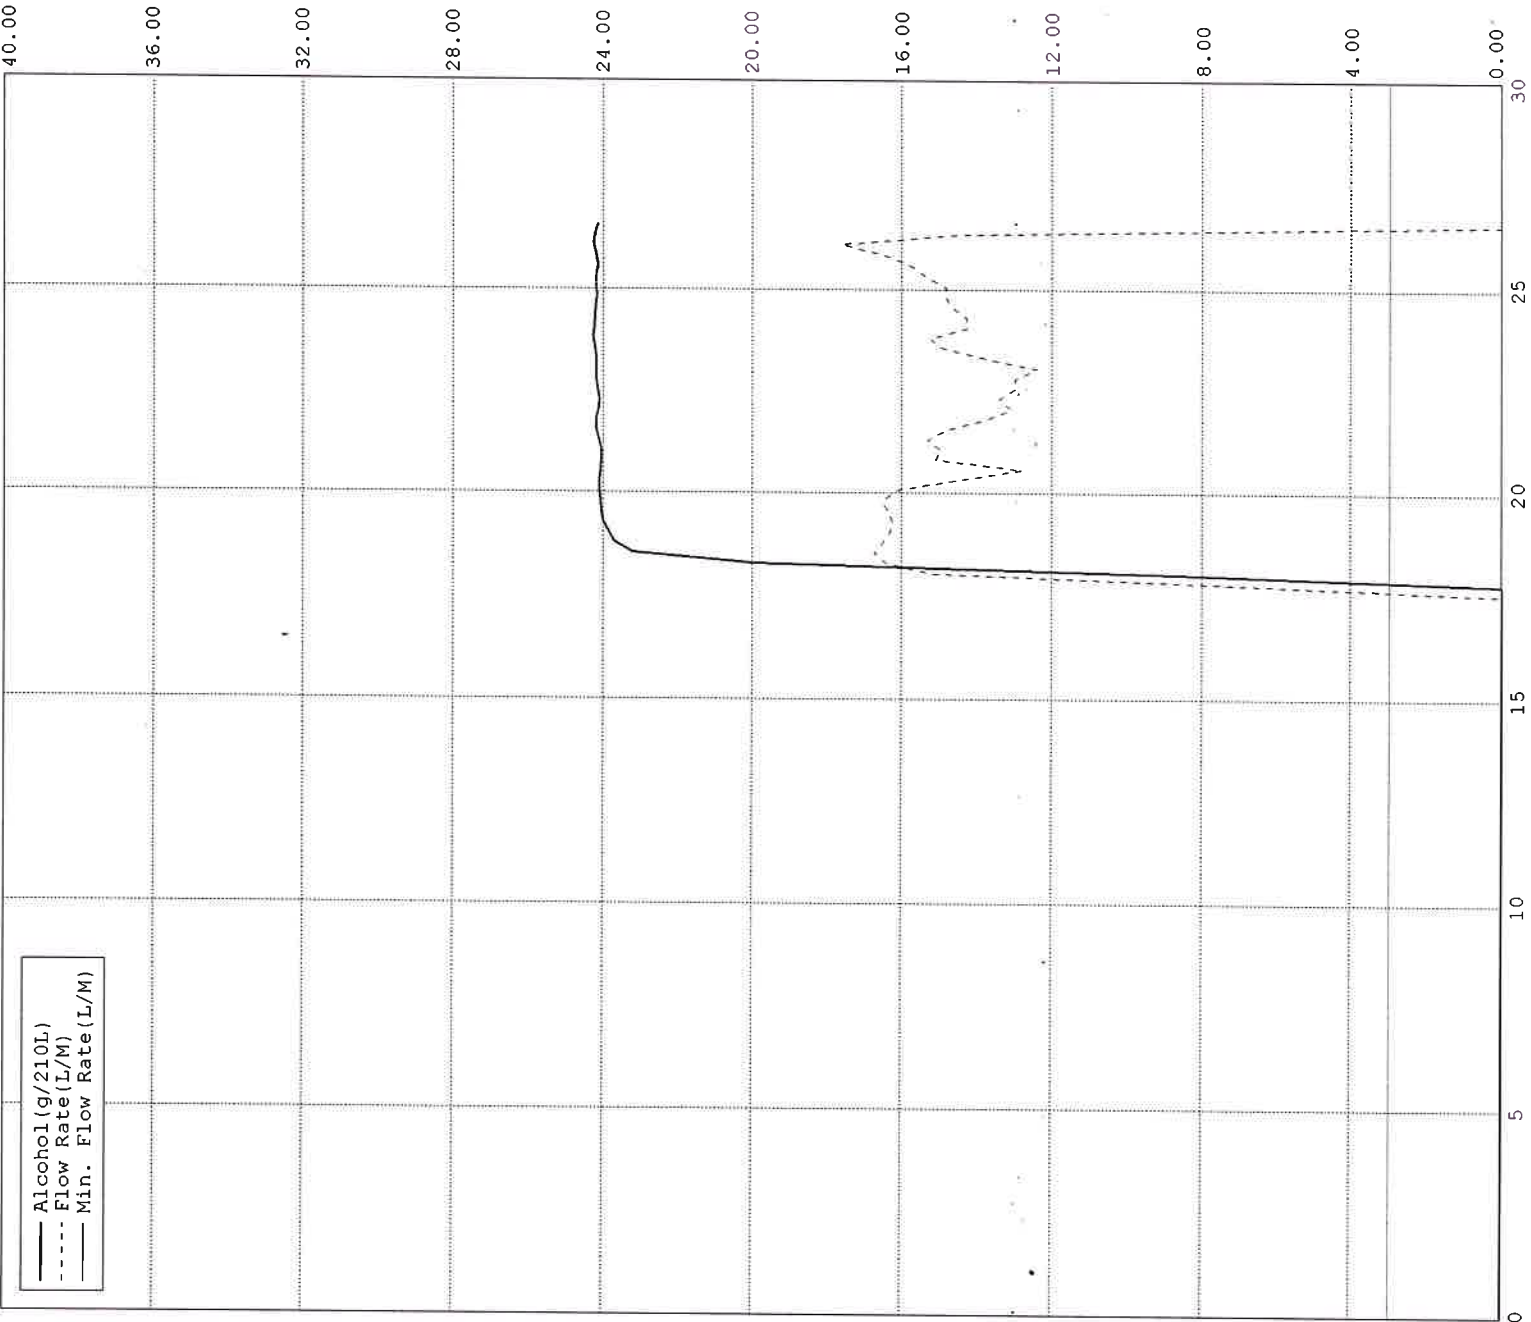

SUBJECT TEST

Alaska Department of Public Safety  
DATA MASTER dmt: 100687

Date: 02/15/2023  
Time: 15:20:31


SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-NEG

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.72: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	15:21
BLANK TEST	0.000	15:21
INTERNAL STANDARD	VERIFIED	15:21
Xq = 0.097 (0.72%)	0.078	15:22
X[1] = 0.0779 (-0.0006)	(0.0020)	
BLANK TEST	0.000	15:22
SUBJECT SAMPLE (Vol=2.01L)	0.096	15:23
X[1] = 0.0961 (-0.0004)	(0.0000)	
BLANK TEST	0.000	15:24
EXTERNAL STANDARD	0.077	15:25
X[1] = 0.0774 (-0.0011)	(0.0017)	
BLANK TEST	0.000	15:25

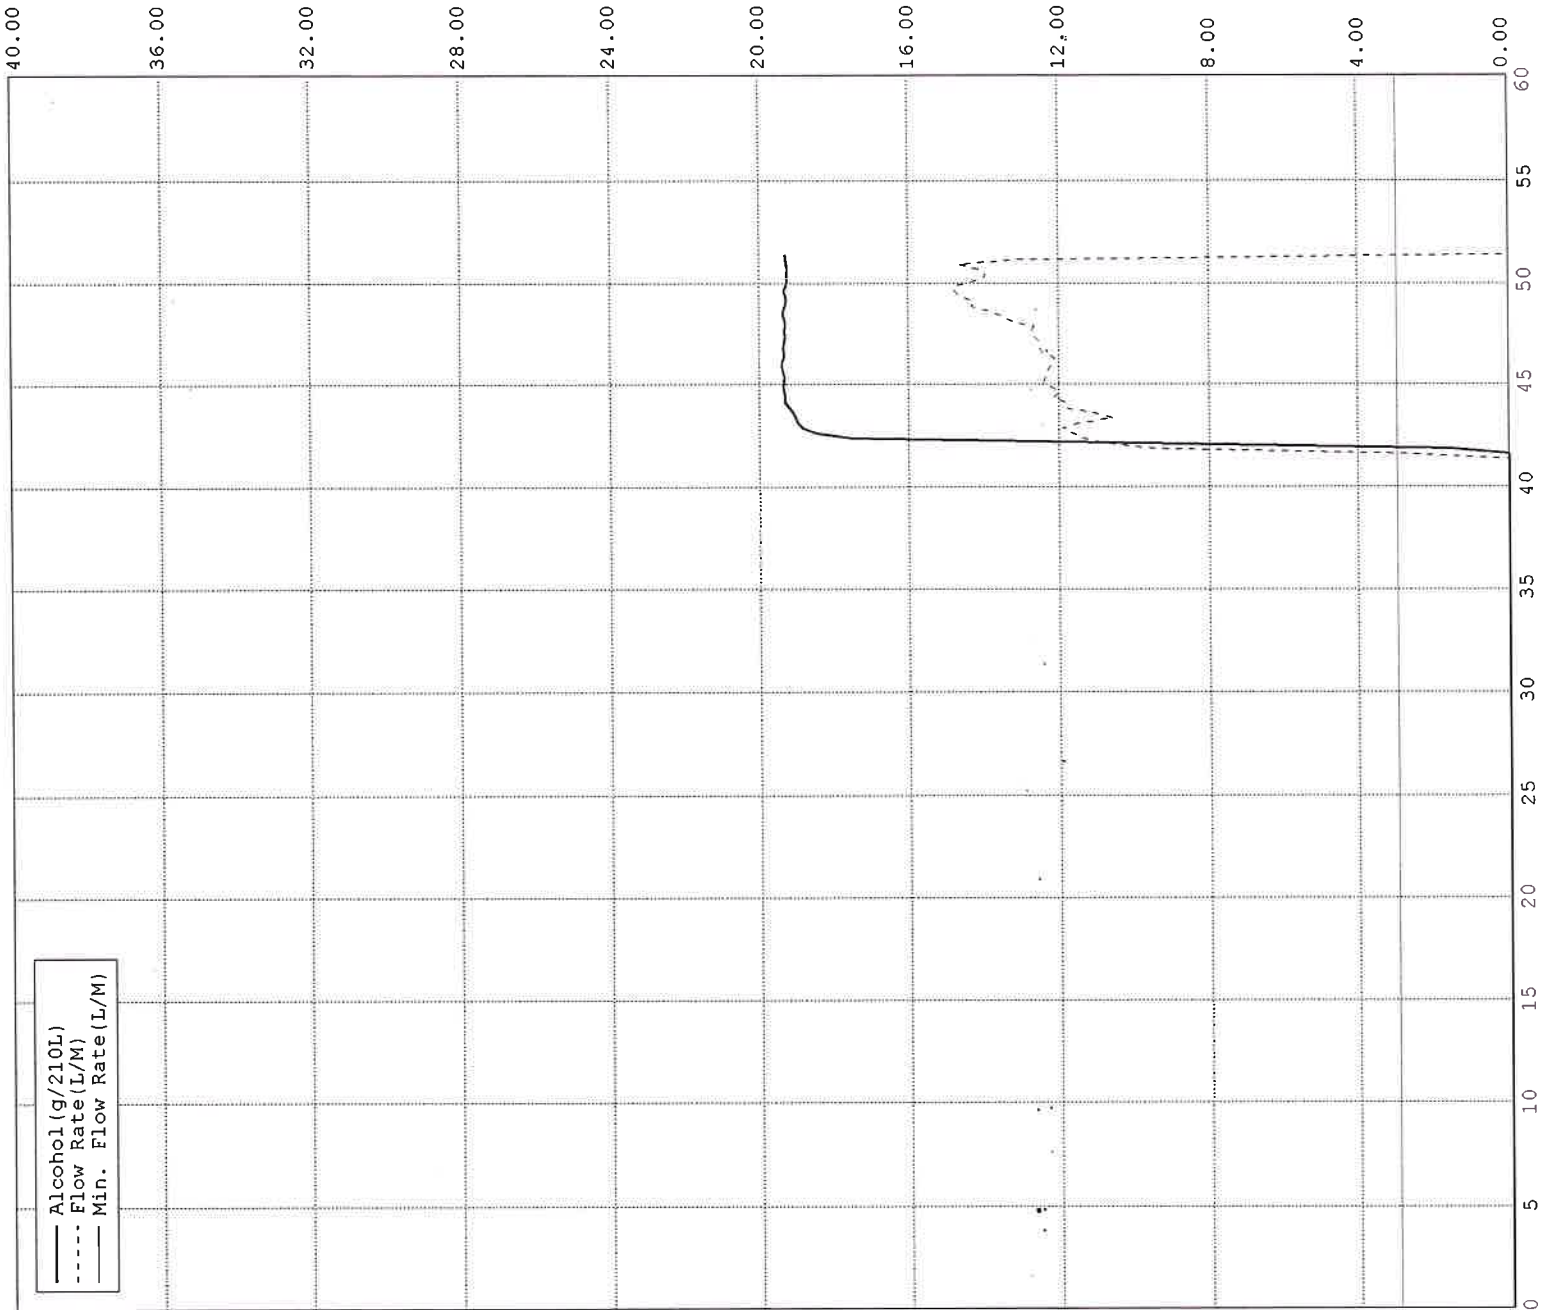

SUBJECT TEST

Alaska Department of Public Safety  
DATA MASTER dmt: 100687

Date: 02/15/2023  
Time: 15:41:20

SUBJECT NAME:  
TEST TEST  
LICENSE #: NONDRINKING

OPERATOR NAME:  
COLLEEN S OBRyant  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.71: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	15:42
BLANK TEST	0.000	15:42
INTERNAL STANDARD	VERIFIED	15:42
EXTERNAL STANDARD	0.078	15:43
BLANK TEST	0.000	15:43
SUBJECT SAMPLE (Vol=2.10L)	0.000	15:44
BLANK TEST	0.000	15:45
EXTERNAL STANDARD	0.078	15:45
BLANK TEST	0.000	15:46

