

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100676

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 11/02/2016

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 27.21: 0.073  
LOT #: AG608504  
EXPIRATION: 03/25/2018  
TANK PRESSURE: 1188 psi

BLANK TEST	0.000	08:16
INTERNAL STANDARD	VERIFIED	08:17
EXTERNAL STANDARD	0.072	08:17
BLANK TEST	0.000	08:18
EXTERNAL STANDARD	0.072	08:18
BLANK TEST	0.000	08:19
EXTERNAL STANDARD	0.072	08:19
BLANK TEST	0.000	08:20
EXTERNAL STANDARD	0.072	08:20
BLANK TEST	0.000	08:21
EXTERNAL STANDARD	0.072	08:21
BLANK TEST	0.000	08:22

Average = 0.0720  
Std Dev = 0.0000

## Diagnostic Check

### VERSIONS

DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 49.1°C PASSED  
Breath Tube = 47.8°C PASSED

### PUMP INFO

Flow Rate = 3.791 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

### FILTER INFO


Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

### INTERNAL STANDARD

PASSED


I, Charles R. Foster, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Charles R. Foster  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 23<sup>rd</sup> day of Dec 20 16

  
Nikki Roth, Notary Public  
My Commission Expires With Office

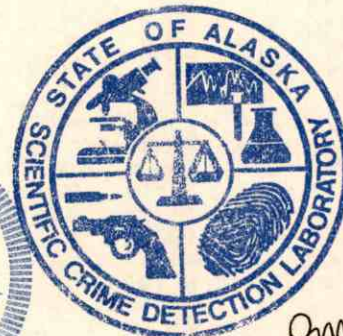

BMB  
12/20/16