



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100356

Report Issue Date: 11/27/2024
Date Received: 2024-09-27
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.019	AG408002	0.020	0.020	0.020	0.020	0.019	0.020
0.080	0.078	AG335202	0.078	0.078	0.078	0.078	0.078	0.078
0.300	0.291	AG427706	0.291	0.291	0.291	0.291	0.291	0.291

As Found - Evaluation Analyst: Megan Carlock
 As Found Conditions - Barometric Pressure (inHg): 29.07 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.4 Relative Humidity (%): 21
 As-Found Lab Activity Date Range: 10/29/2024 - 10/29/2024

Replaced O-ring. The second internal standard reading on the VOC is above 3%.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG408002	0.019	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.039	0.039	0.038	0.039	0.039	0.039	+/- 0.003
0.080	0.077	AG335202	0.077	0.077	0.077	0.077	0.077	0.077	+/- 0.004
0.100	0.096	AG333401	0.096	0.097	0.097	0.097	0.097	0.097	+/- 0.004
0.150	0.145	AG332004	0.142	0.143	0.142	0.143	0.142	0.142	+/- 0.006
0.300	0.289	AG427706	0.287	0.287	0.287	0.287	0.287	0.287	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 28.86 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.8 Relative Humidity (%): 19
 As-Left Lab Activity Date Range: 11/07/2024 - 11/07/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Kaija Swisher on 11/27/2024

kaija.swisher@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 11/27/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 160356 Analyst or Technician Name: Kaya Swisher
DataMaster DMT Calibration Start Date: 11/7/24

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: 5/2/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 28.86 Temperature(C) 21.8 Relative Humidity(%) 19
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20241107KS Expiration Date: 2/7/25
Simulator S/N: DR4161 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20241107KS Expiration Date: 2/7/25
Simulator S/N: DR5298 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 23IP41233 Expiration Date: 2/7/25
Simulator S/N: DR4163 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 9/19/25

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 11/7/24
Data Interpretation Date (Technician): NA (if applicable)
Data Interpretation Date (Analyst): 11/7/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100356

Date: 11/07/2024
Time: 09:27:29

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.1°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 47.3°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.69 V PASSED
(1.01 V - 2.37 V)
Cooler Voltage = 1.56 V PASSED
(0.94 V - 2.18 V)
Bias Voltage = 79 V PASSED
(47 V - 111 V)
Chopper Freq = 521 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 28.9 in

PUMP INFO

Flow Rate = 4.699 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 v <= 0.010 v)
PUMP OFF PASSED
(0.002 v <= 0.010 v)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.103 0.26% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100356

Date: 11/07/2024
Time: 10:01 AM

Temperatures (°C)

Sample Cell: 48.8°C
Breath Tube: 47.3°C

Current Barometer 28.9 in
Volume (Ltr) 1.50

Settings

Lamp: 1.80 V
Bias: 79 V
Cooler: 1.56 V
Chopper: 521 Hz

Voltages (V)

Flow: 1.04 V
Detector: -0.060 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100356

Date: 11/06/2024
Time: 14:21:24

OPERATOR NAME:
KAIJA SWISHER
CERTIFICATE #: 10746

Ca = 0.1000
CAL = 0.982943 0.800 <= CAL < 1.200
b1 = 0.0003 0.0000 <= b1 < 0.0040
b2 = 0.0051 0.0010 <= b2 < 0.0100
b3 = 0.0003 0.0000 <= b3 < 0.0040
Xq = 0.1032 0.0500 <= Xq < 0.2000
a21 = 1.209418 1.050 <= a21 < 1.300
a31 = 0.478348 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100356

Date: 11/07/2024
Time: 10:07:41

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.85: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:12
BLANK TEST	0.000	10:12
INTERNAL STANDARD	VERIFIED	10:12
EXTERNAL STANDARD	0.076	10:12
BLANK TEST	0.000	10:13
SUBJECT SAMPLE (Vol=1.54L)	0.000	10:14
BLANK TEST	0.000	10:15
EXTERNAL STANDARD	0.077	10:15
BLANK TEST	0.000	10:16

KS

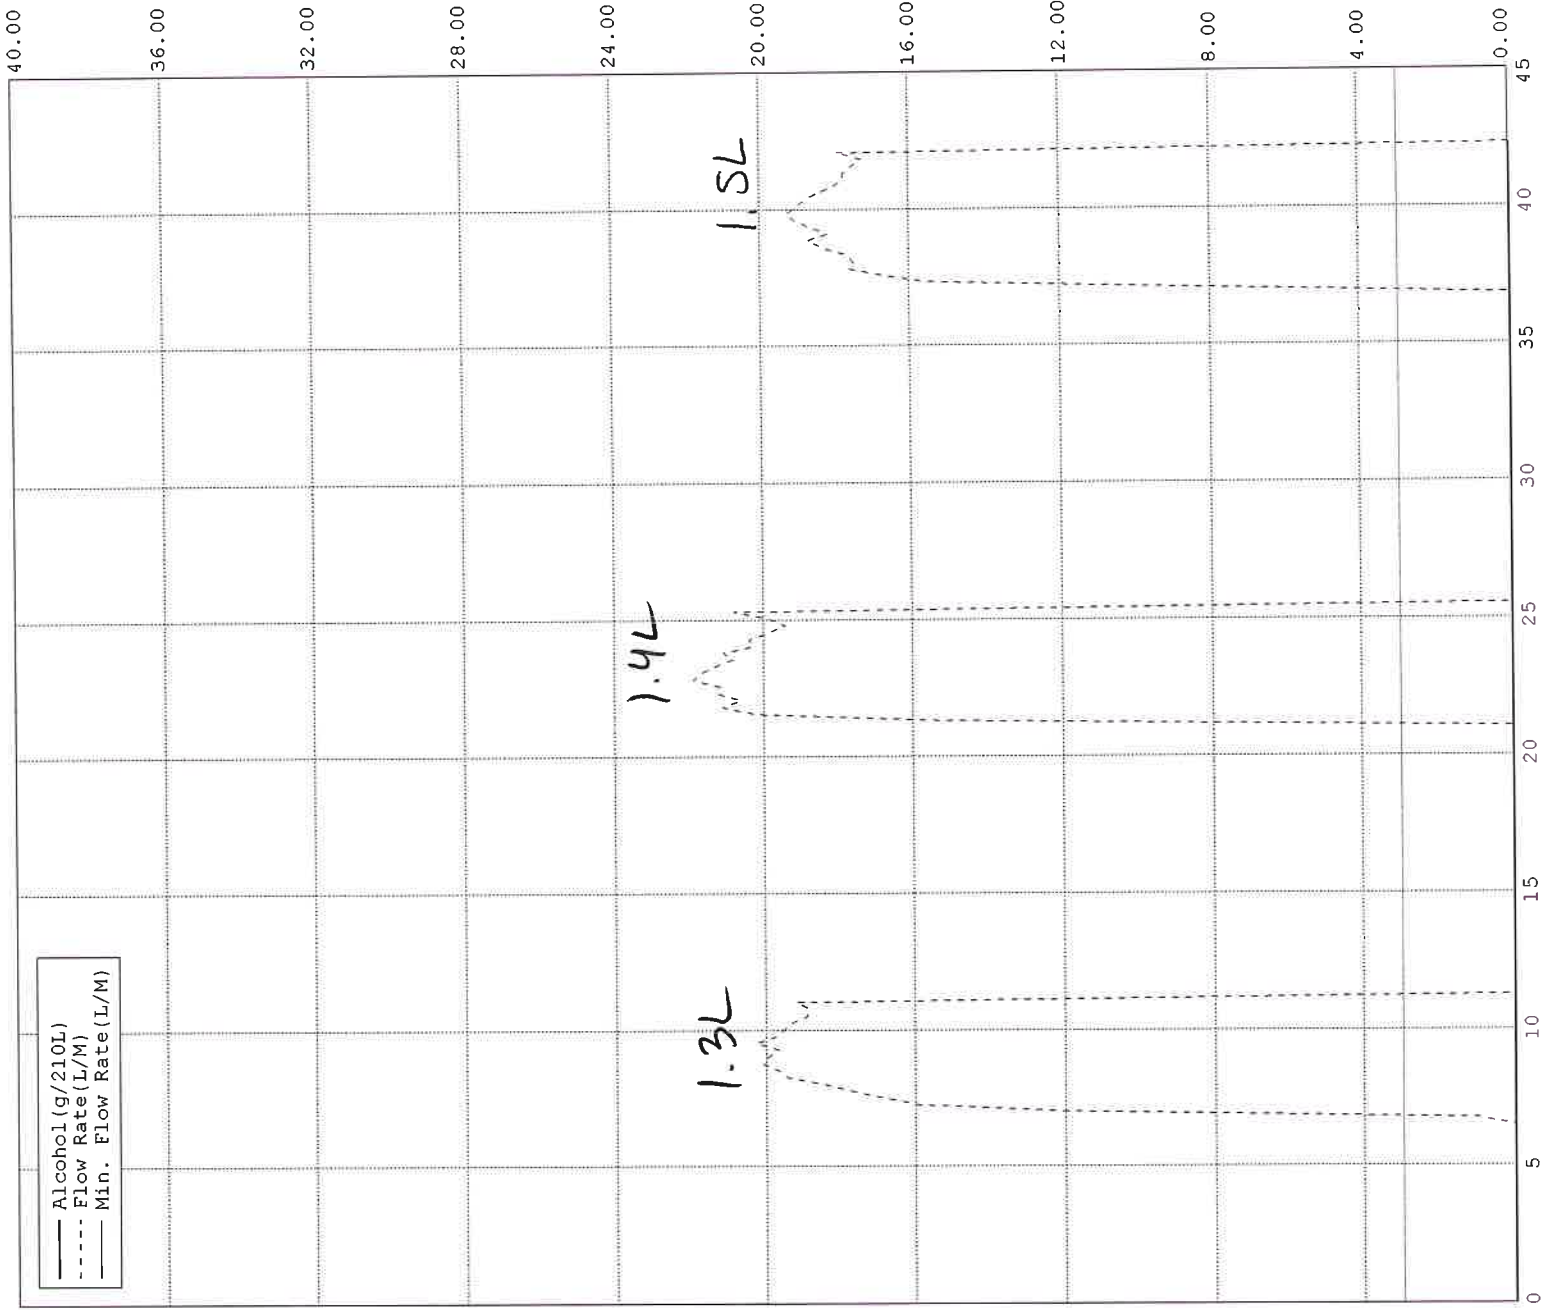

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100356

Date: 11/07/2024
 Time: 10:30:38

SUPERVISOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.019	0.0198	0.0004
0.039	0.0388	0.0004
0.077	0.0770	0.0000
0.096	0.0968	0.0004
0.145	0.1424	0.0005
0.289	0.2870	0.0000

SLOPE = 0.989218
 R² = 0.999897

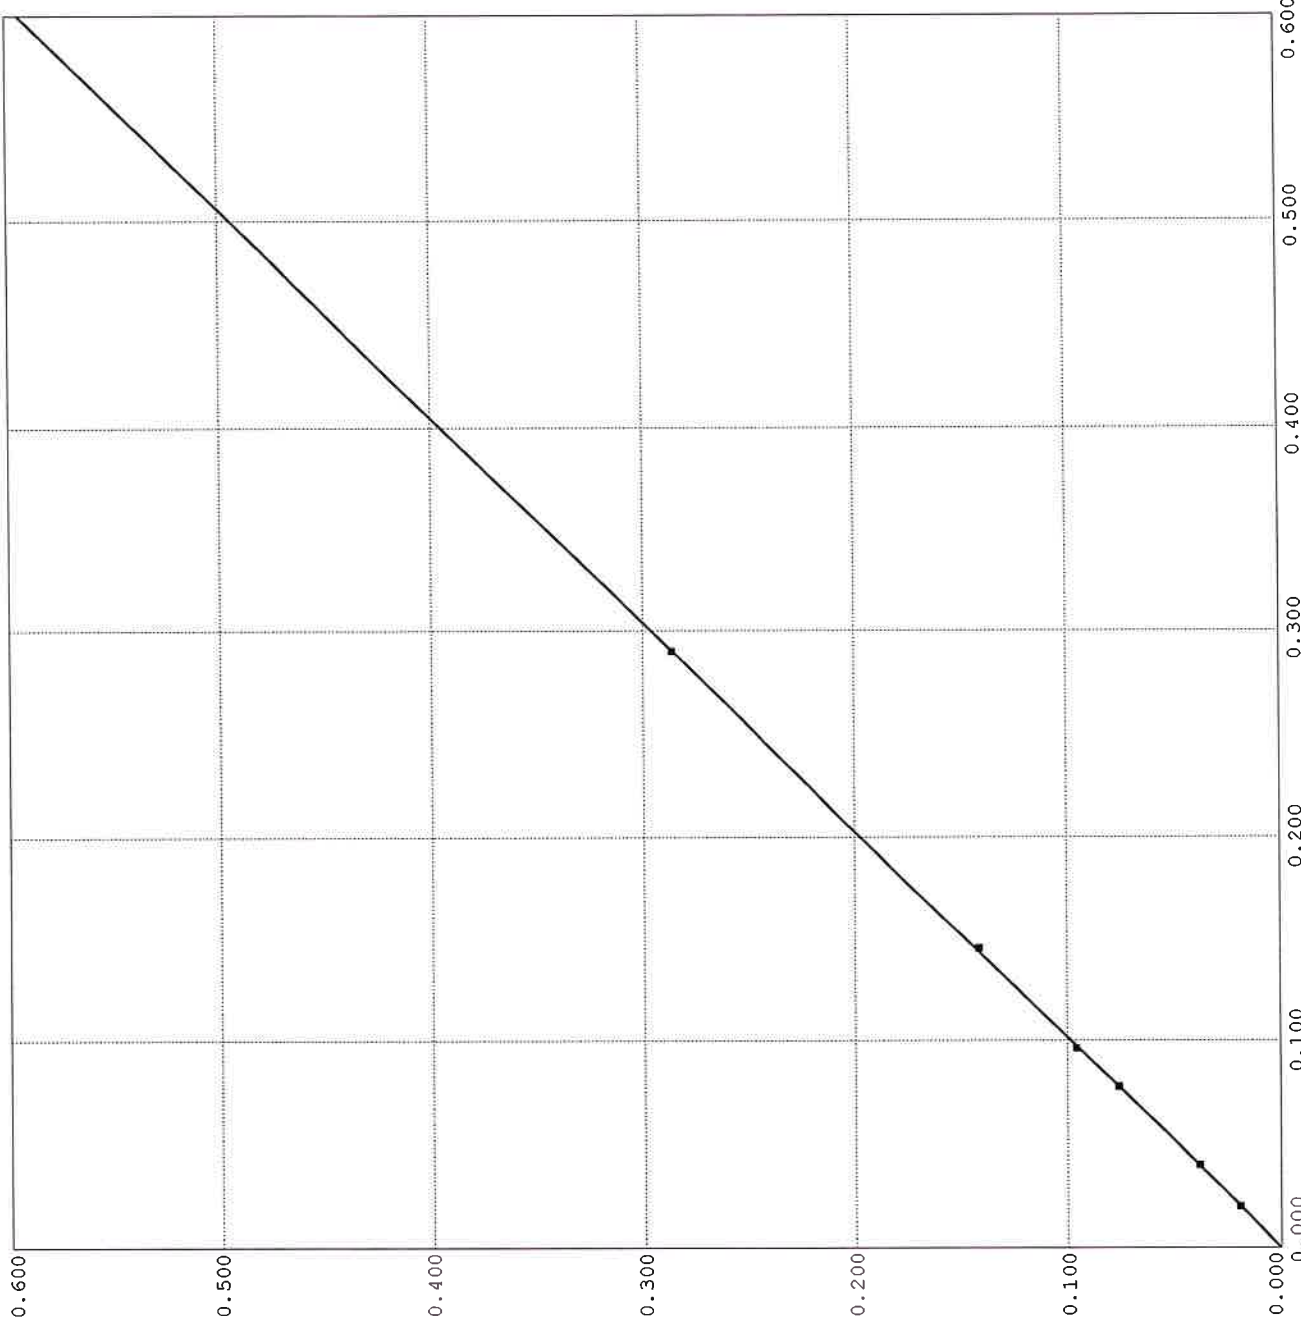

KS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100356






Date: 11/07/2024
Time: 10:30:39

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 28.84: 0.019
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 737 psi

BLANK TEST	0.000	10:31
INTERNAL STANDARD	VERIFIED	10:32
EXTERNAL STANDARD	0.019	10:32
BLANK TEST	0.000	10:33
EXTERNAL STANDARD	0.020	10:33
BLANK TEST	0.000	10:34
EXTERNAL STANDARD	0.020	10:34
BLANK TEST	0.000	10:35
EXTERNAL STANDARD	0.020	10:35
BLANK TEST	0.000	10:36
EXTERNAL STANDARD	0.020	10:36
BLANK TEST	0.000	10:37

Average = 0.0198
Std Dev = 0.0004

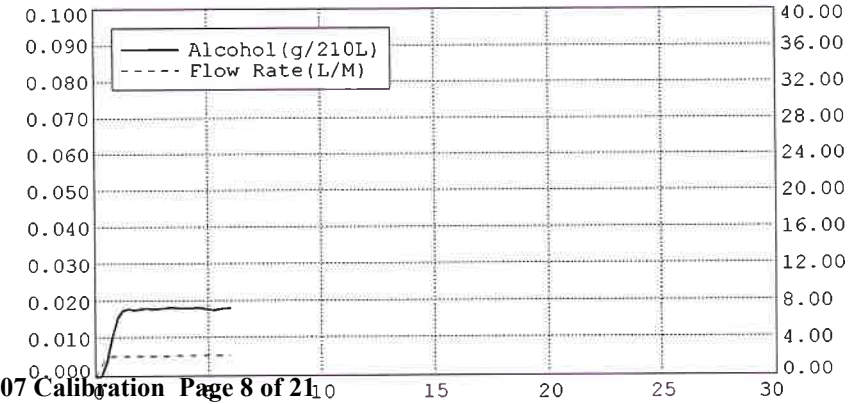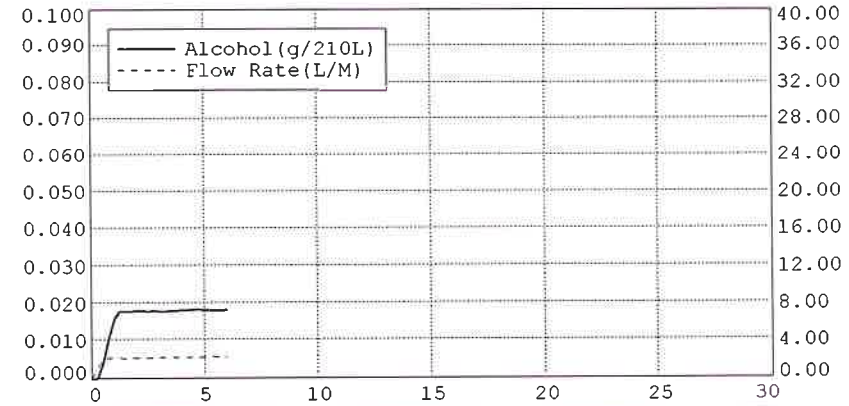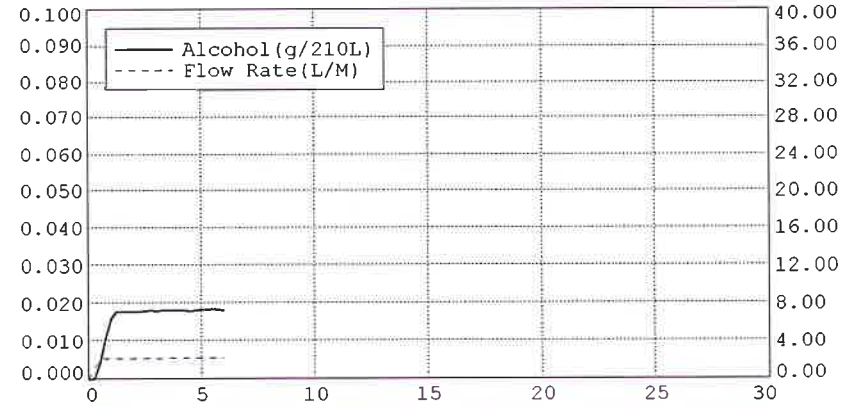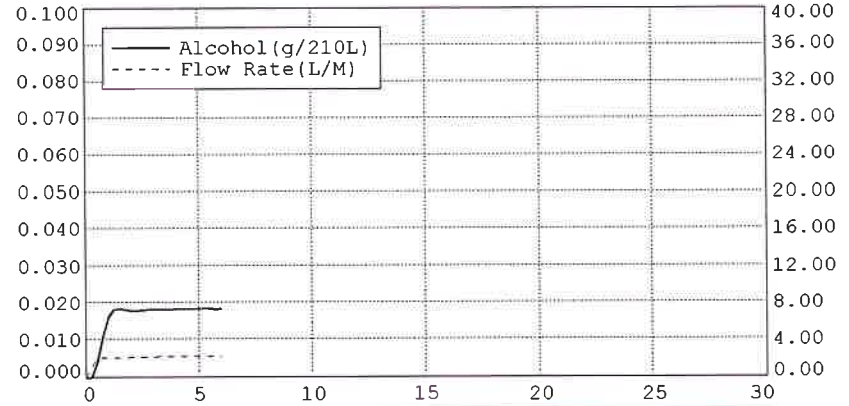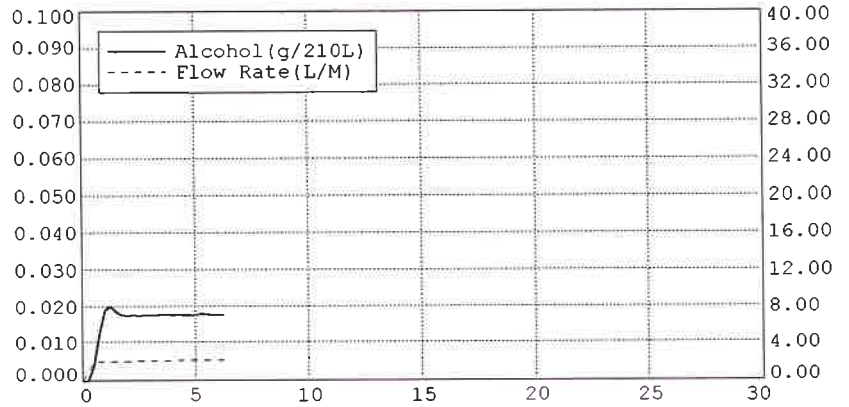

LINEARITY CHECK: Control Test 2






Alaska Department of Public Safety
 DATAMASTER dmt: 100356

Date: 11/07/2024
 Time: 10:38:34

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.040
 TARGET AT 28.85: 0.039
 LOT #: AG407908
 EXPIRATION: 03/19/2026
 TANK PRESSURE: 1012 psi

BLANK TEST	0.000	10:39
INTERNAL STANDARD	VERIFIED	10:39
EXTERNAL STANDARD	0.039	10:40
BLANK TEST	0.000	10:41
EXTERNAL STANDARD	0.039	10:41
BLANK TEST	0.000	10:42
EXTERNAL STANDARD	0.038	10:42
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.039	10:43
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.039	10:44
BLANK TEST	0.000	10:45

Average = 0.0388
 Std Dev = 0.0004

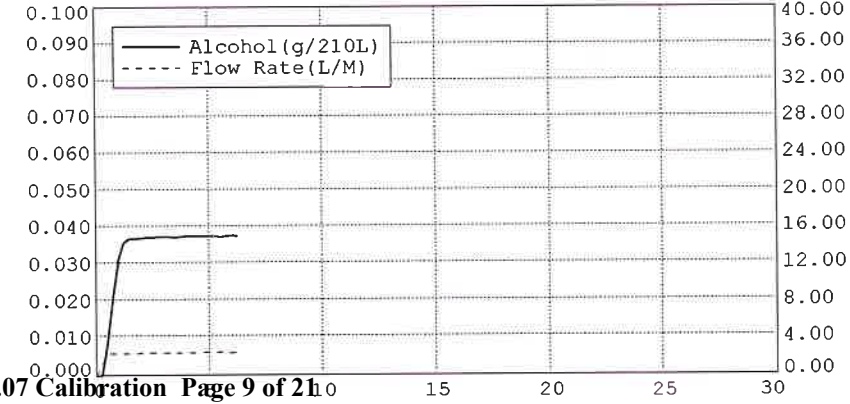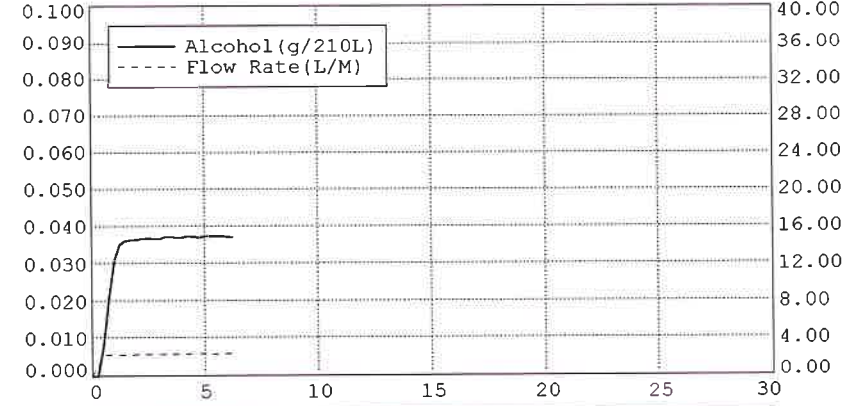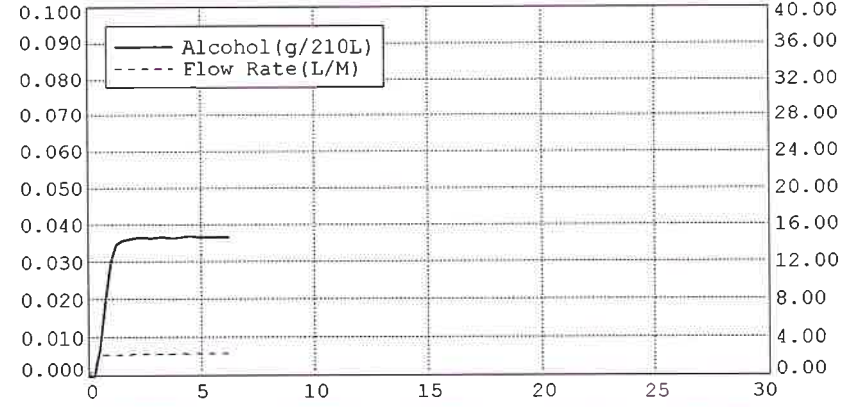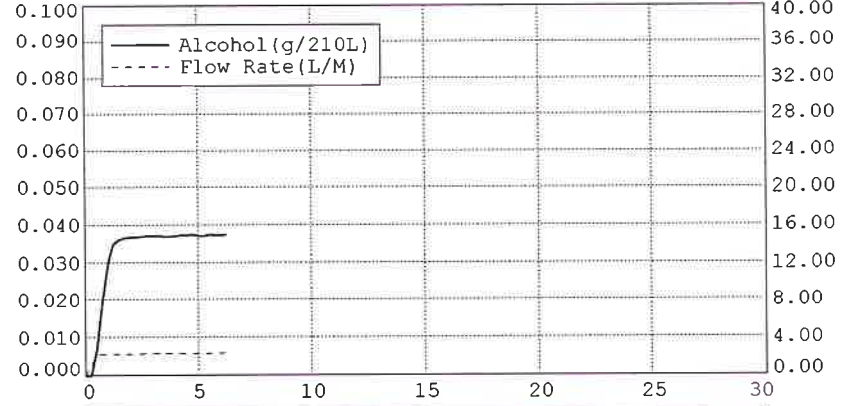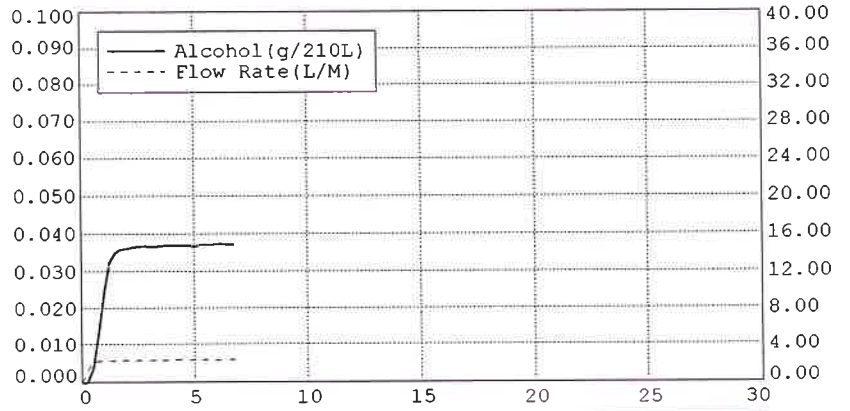

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100356






Date: 11/07/2024
 Time: 10:47:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 28.85: 0.077
 LOT #: AG335202
 EXPIRATION: 12/18/2025
 TANK PRESSURE: 732 psi

BLANK TEST	0.000	10:48
INTERNAL STANDARD	VERIFIED	10:48
EXTERNAL STANDARD	0.077	10:48
BLANK TEST	0.000	10:49
EXTERNAL STANDARD	0.077	10:50
BLANK TEST	0.000	10:50
EXTERNAL STANDARD	0.077	10:51
BLANK TEST	0.000	10:52
EXTERNAL STANDARD	0.077	10:52
BLANK TEST	0.000	10:53
EXTERNAL STANDARD	0.077	10:53
BLANK TEST	0.000	10:54

Average = 0.0770
 Std Dev = 0.0000

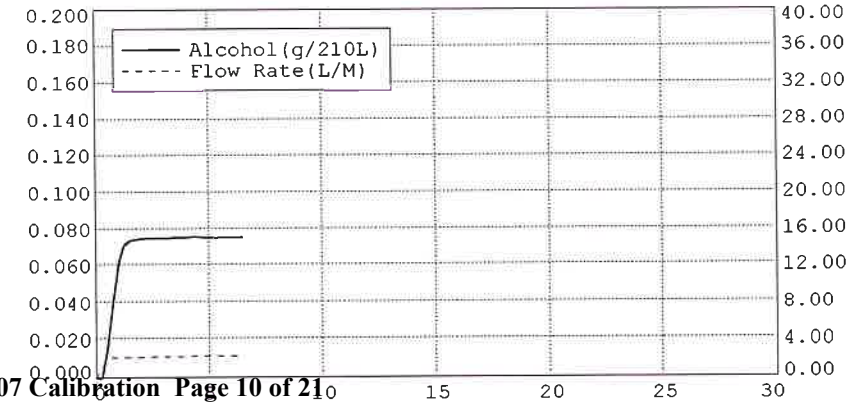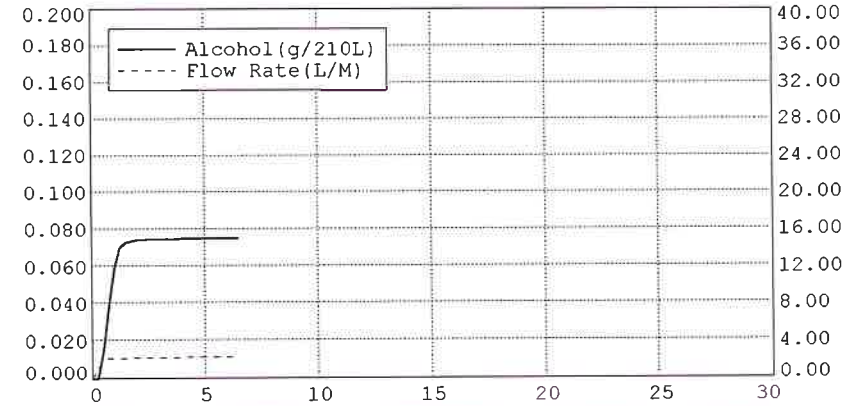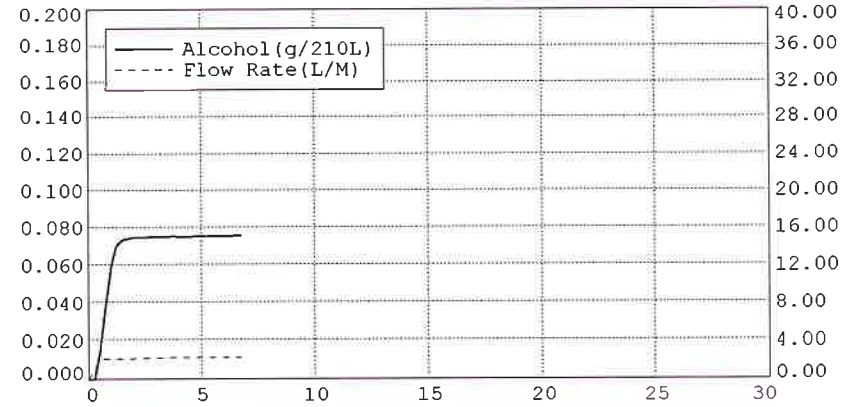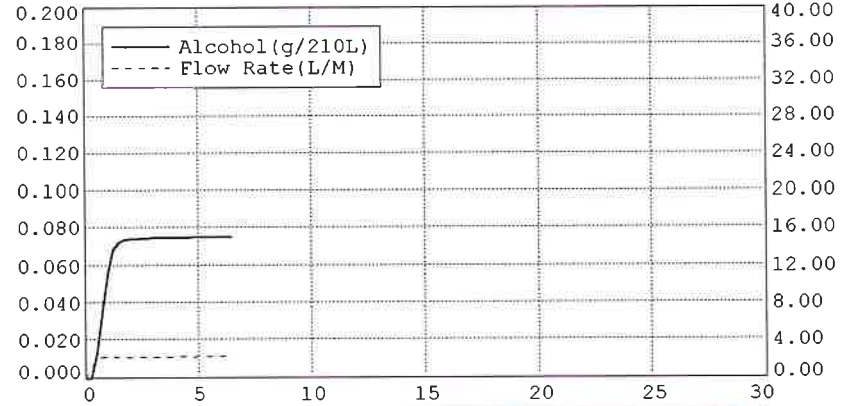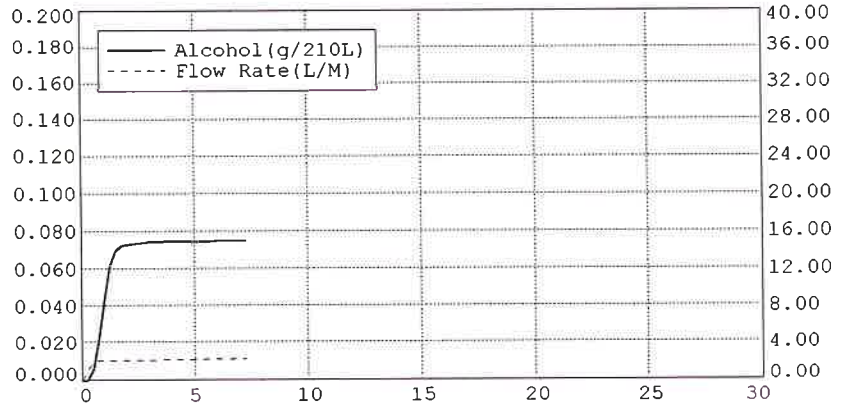

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100356






Date: 11/07/2024
 Time: 10:55:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 28.85: 0.096
 LOT #: AG333401
 EXPIRATION: 11/30/2025
 TANK PRESSURE: 700 psi

BLANK TEST	0.000	10:56
INTERNAL STANDARD	VERIFIED	10:56
EXTERNAL STANDARD	0.096	10:56
BLANK TEST	0.000	10:57
EXTERNAL STANDARD	0.097	10:58
BLANK TEST	0.000	10:58
EXTERNAL STANDARD	0.097	10:59
BLANK TEST	0.000	11:00
EXTERNAL STANDARD	0.097	11:00
BLANK TEST	0.000	11:01
EXTERNAL STANDARD	0.097	11:01
BLANK TEST	0.000	11:02

Average = 0.0968
 Std Dev = 0.0004

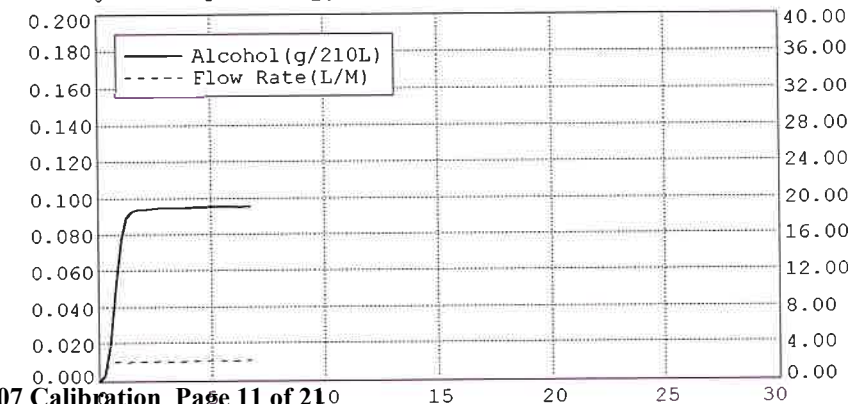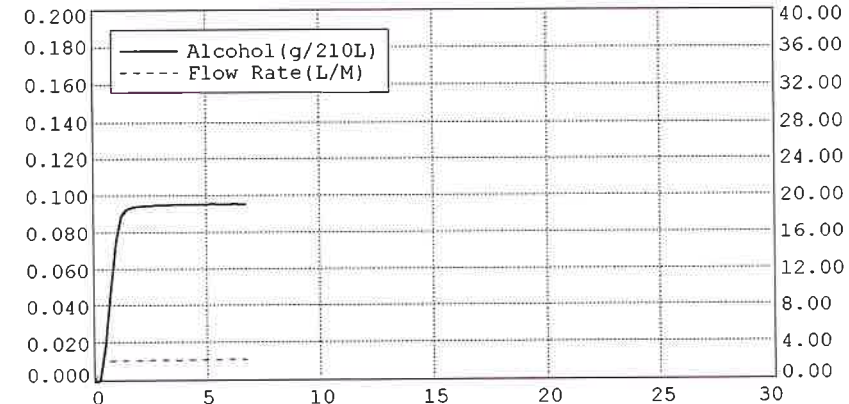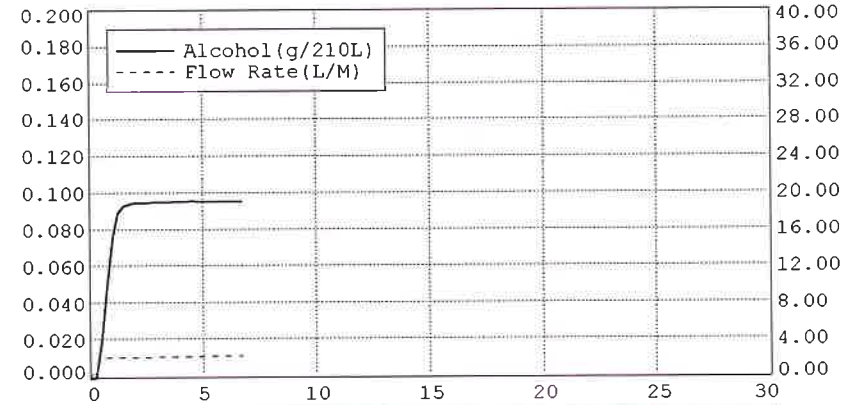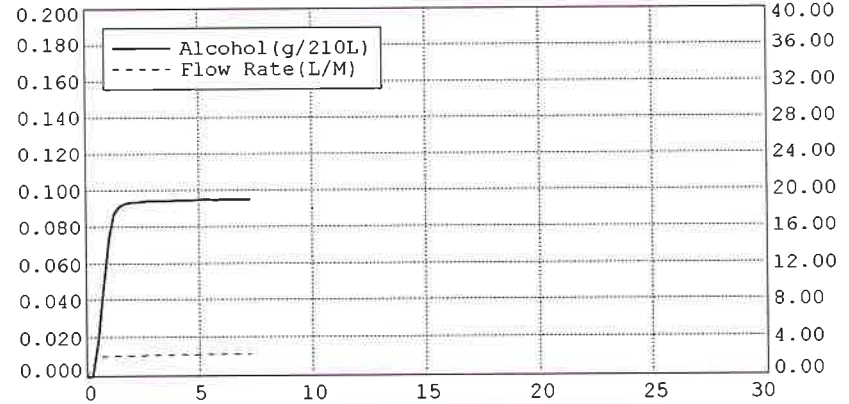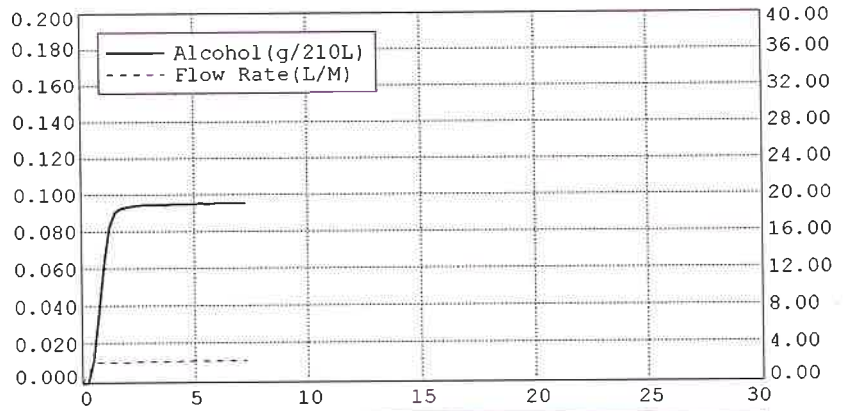

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100356






Date: 11/07/2024
 Time: 11:04:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 28.85: 0.145
 LOT #: AG332004
 EXPIRATION: 11/16/2025
 TANK PRESSURE: 317 psi

BLANK TEST	0.000	11:05
INTERNAL STANDARD	VERIFIED	11:05
EXTERNAL STANDARD	0.142	11:05
BLANK TEST	0.000	11:06
EXTERNAL STANDARD	0.143	11:07
BLANK TEST	0.000	11:07
EXTERNAL STANDARD	0.142	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.143	11:09
BLANK TEST	0.000	11:10
EXTERNAL STANDARD	0.142	11:10
BLANK TEST	0.000	11:11

Average = 0.1424
 Std Dev = 0.0005

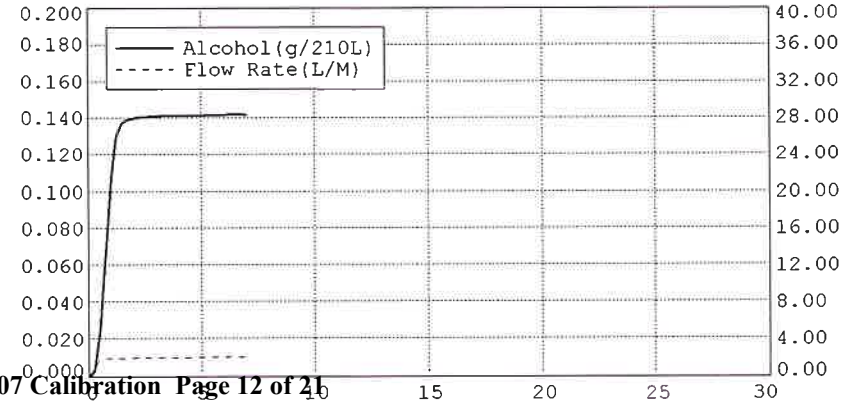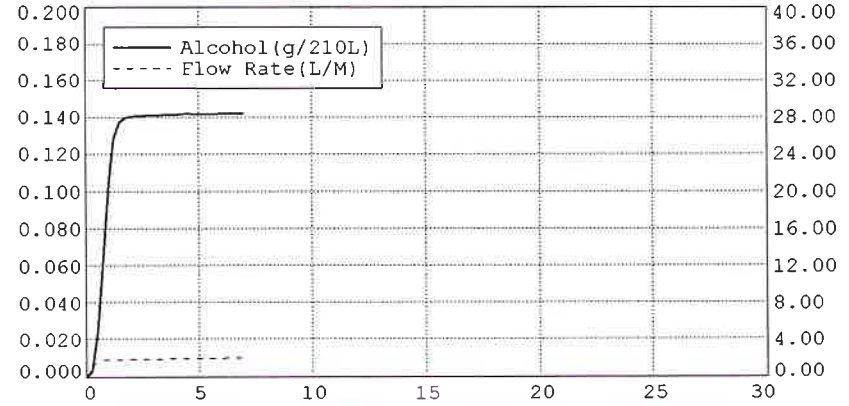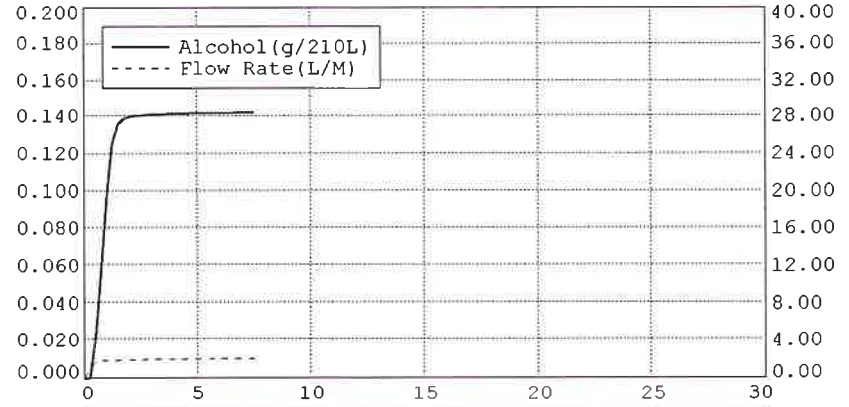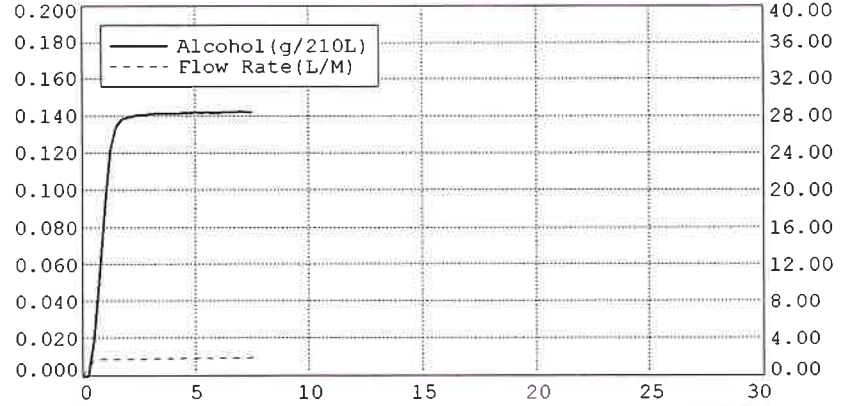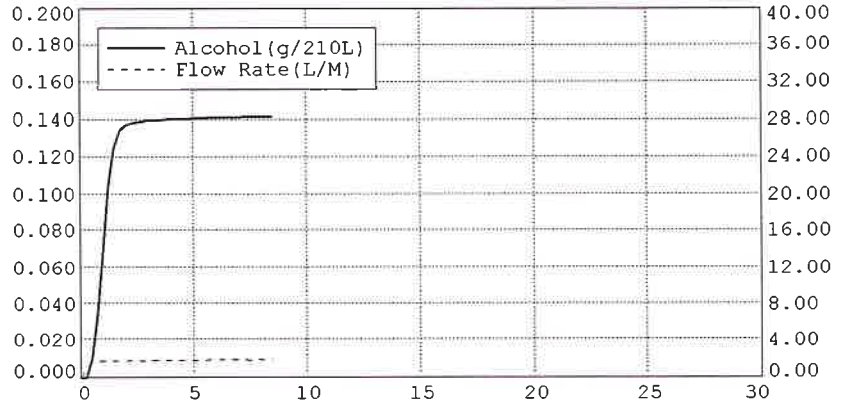

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100356






Date: 11/07/2024
 Time: 11:20:41

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 28.85: 0.289
 LOT #: AG427706
 EXPIRATION: 10/03/2026
 TANK PRESSURE: 314 psi

BLANK TEST	0.000	11:21
INTERNAL STANDARD	VERIFIED	11:22
EXTERNAL STANDARD	0.287	11:22
BLANK TEST	0.000	11:23
EXTERNAL STANDARD	0.287	11:23
BLANK TEST	0.000	11:24
EXTERNAL STANDARD	0.287	11:24
BLANK TEST	0.000	11:25
EXTERNAL STANDARD	0.287	11:25
BLANK TEST	0.000	11:26
EXTERNAL STANDARD	0.287	11:26
BLANK TEST	0.000	11:27

Average = 0.2870
 Std Dev = 0.0000

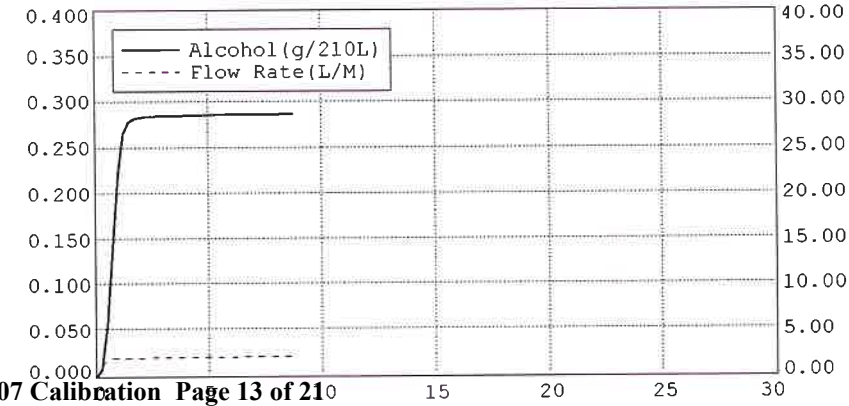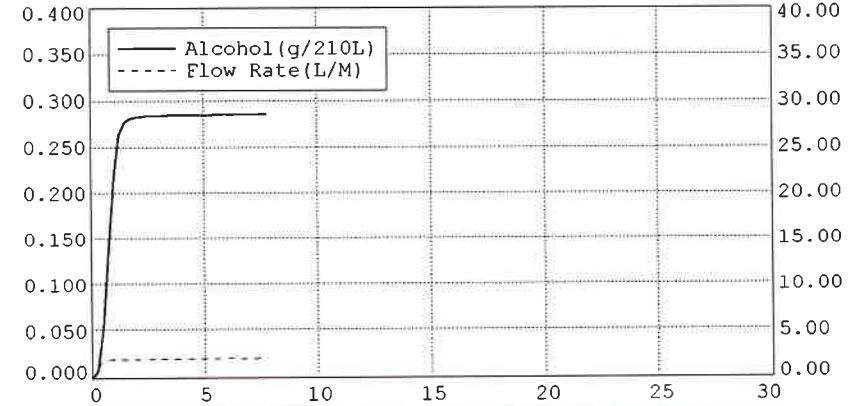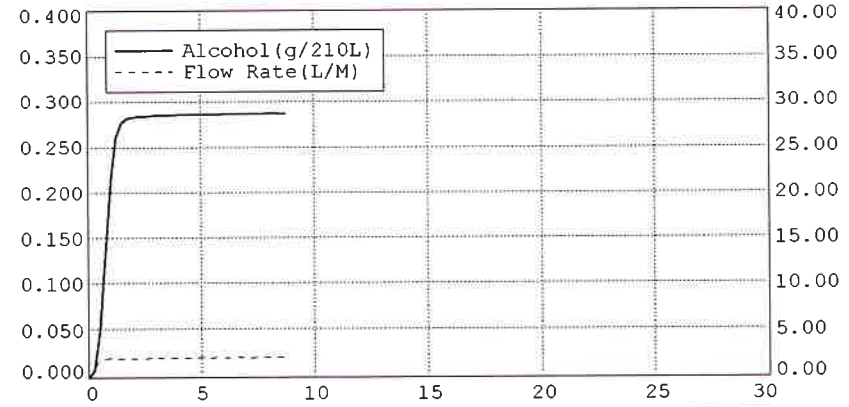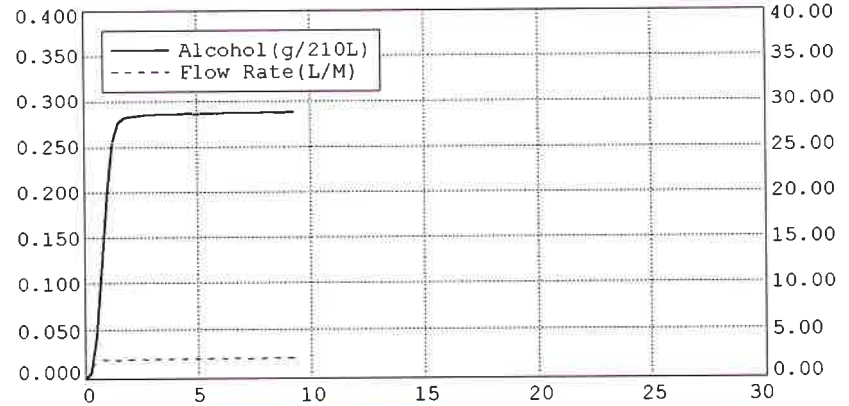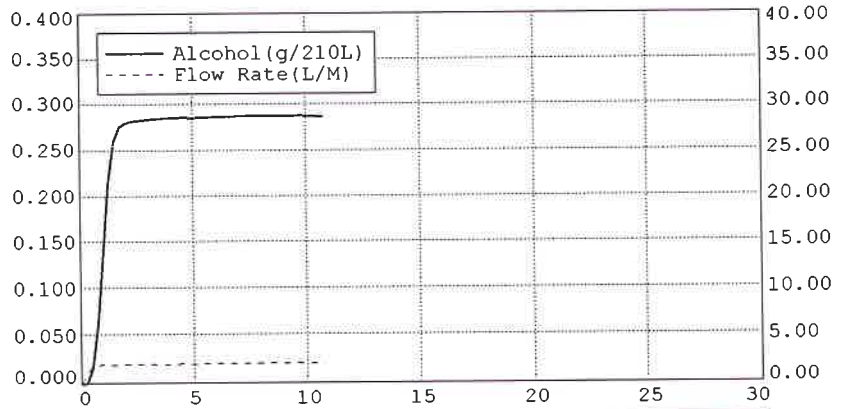

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100356

Date: 11/07/2024
Time: 11:32:41

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.85: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:33
BLANK TEST 0.000 11:33
INTERNAL STANDARD VERIFIED 11:33
EXTERNAL STANDARD 0.077 11:34
BLANK TEST 0.000 11:35
SUBJECT SAMPLE INCOMPLETE 11:37

KS

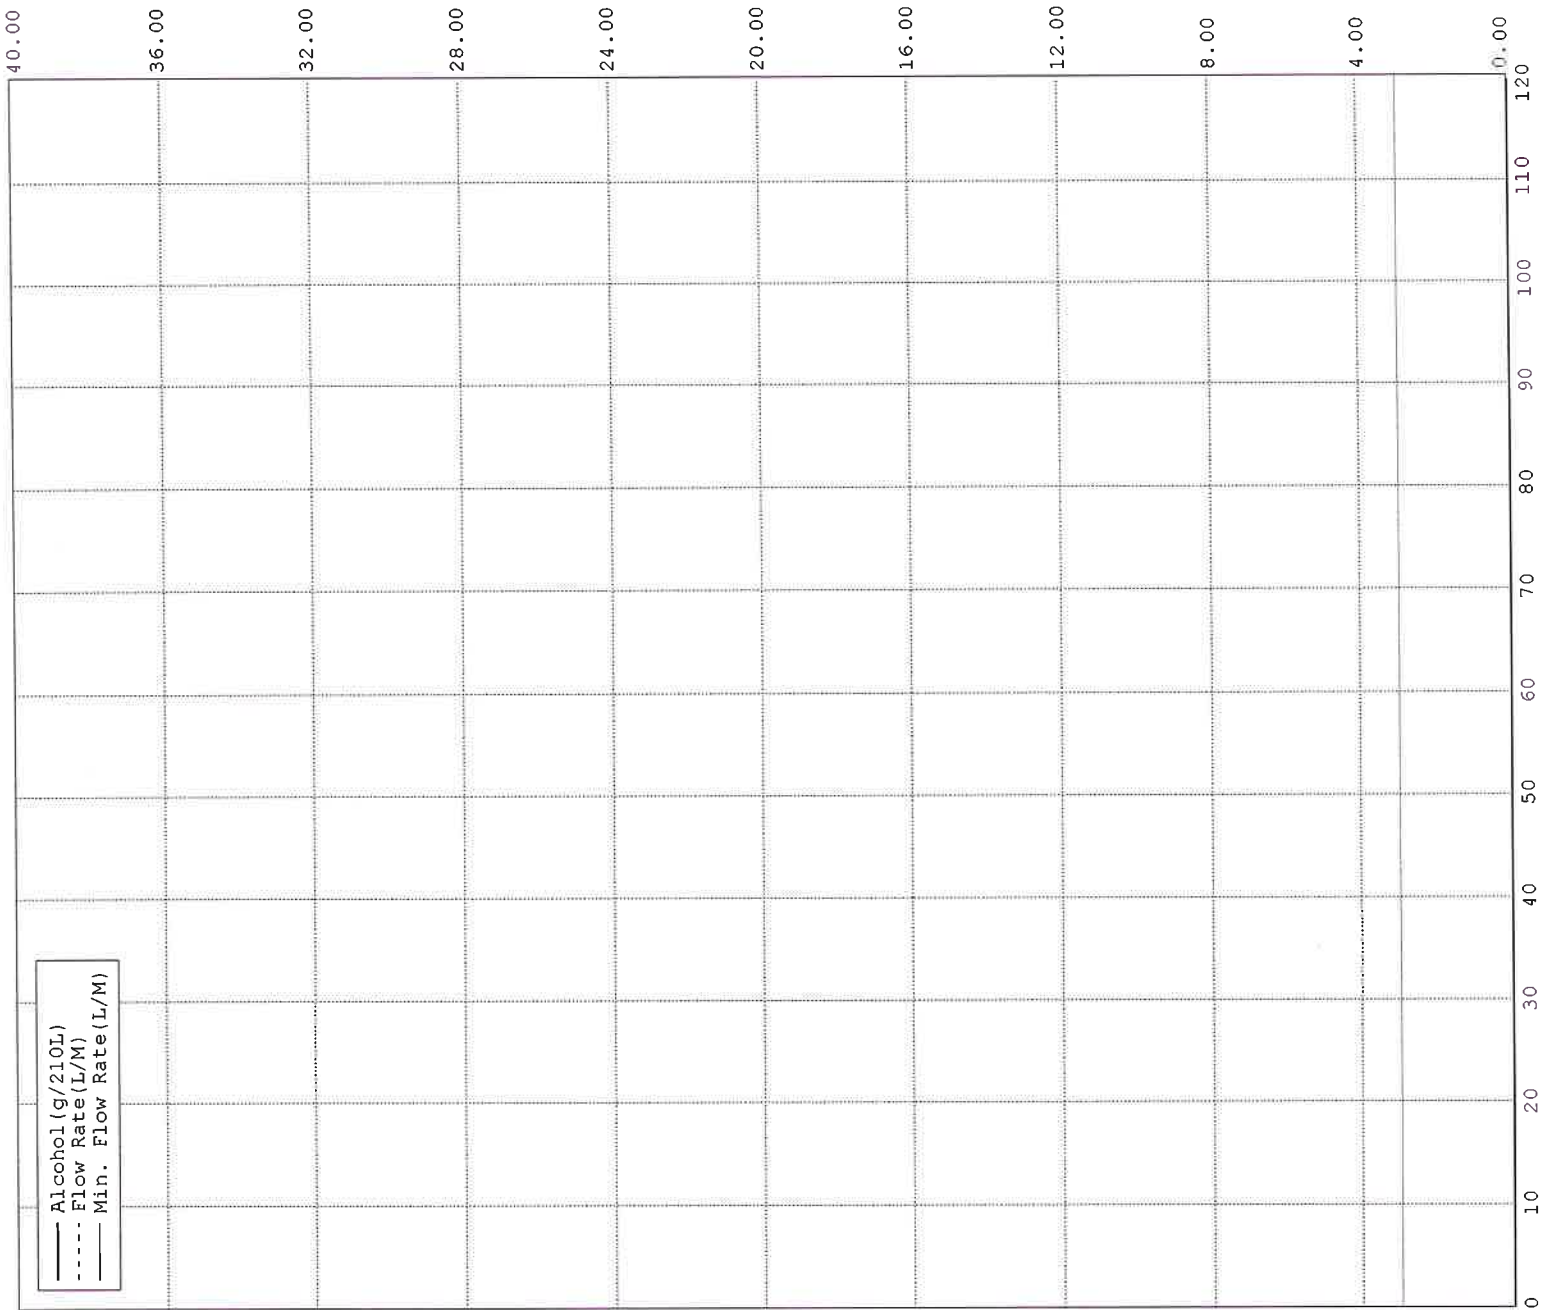

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100356

Date: 11/07/2024
Time: 11:40:42

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAJJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MAX ATTEMPTS
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.85: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:41
BLANK TEST 0.000 11:41
INTERNAL STANDARD VERIFIED 11:41
EXTERNAL STANDARD 0.077 11:42
BLANK TEST 0.000 11:43
SUBJECT SAMPLE XXX 11:43

Maximum Attempts Exceeded

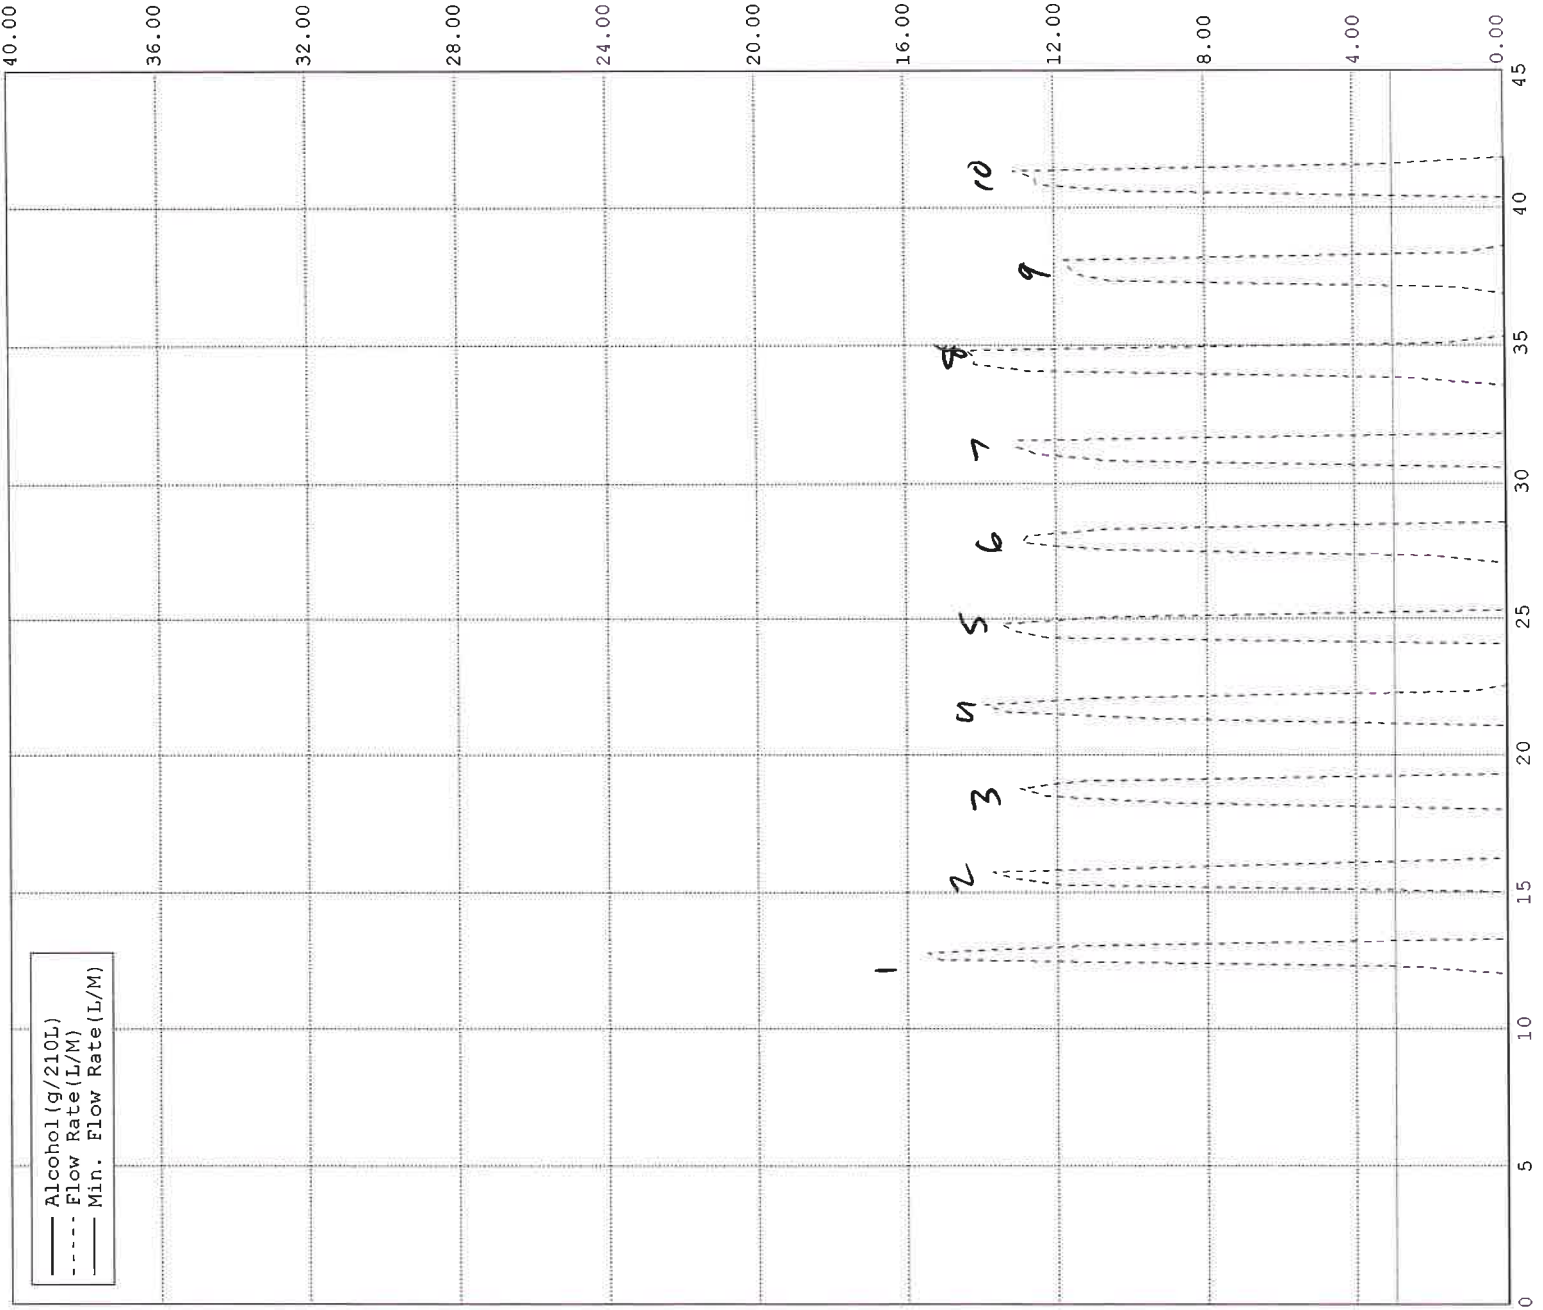

KS

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100356

Date: 11/07/2024
Time: 11:45:16

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.85: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:46
BLANK TEST 0.000 11:46
INTERNAL STANDARD VERIFIED 11:46
EXTERNAL STANDARD 0.077 11:46
BLANK TEST 0.000 11:47
SUBJECT SAMPLE INVALID 11:48

KS

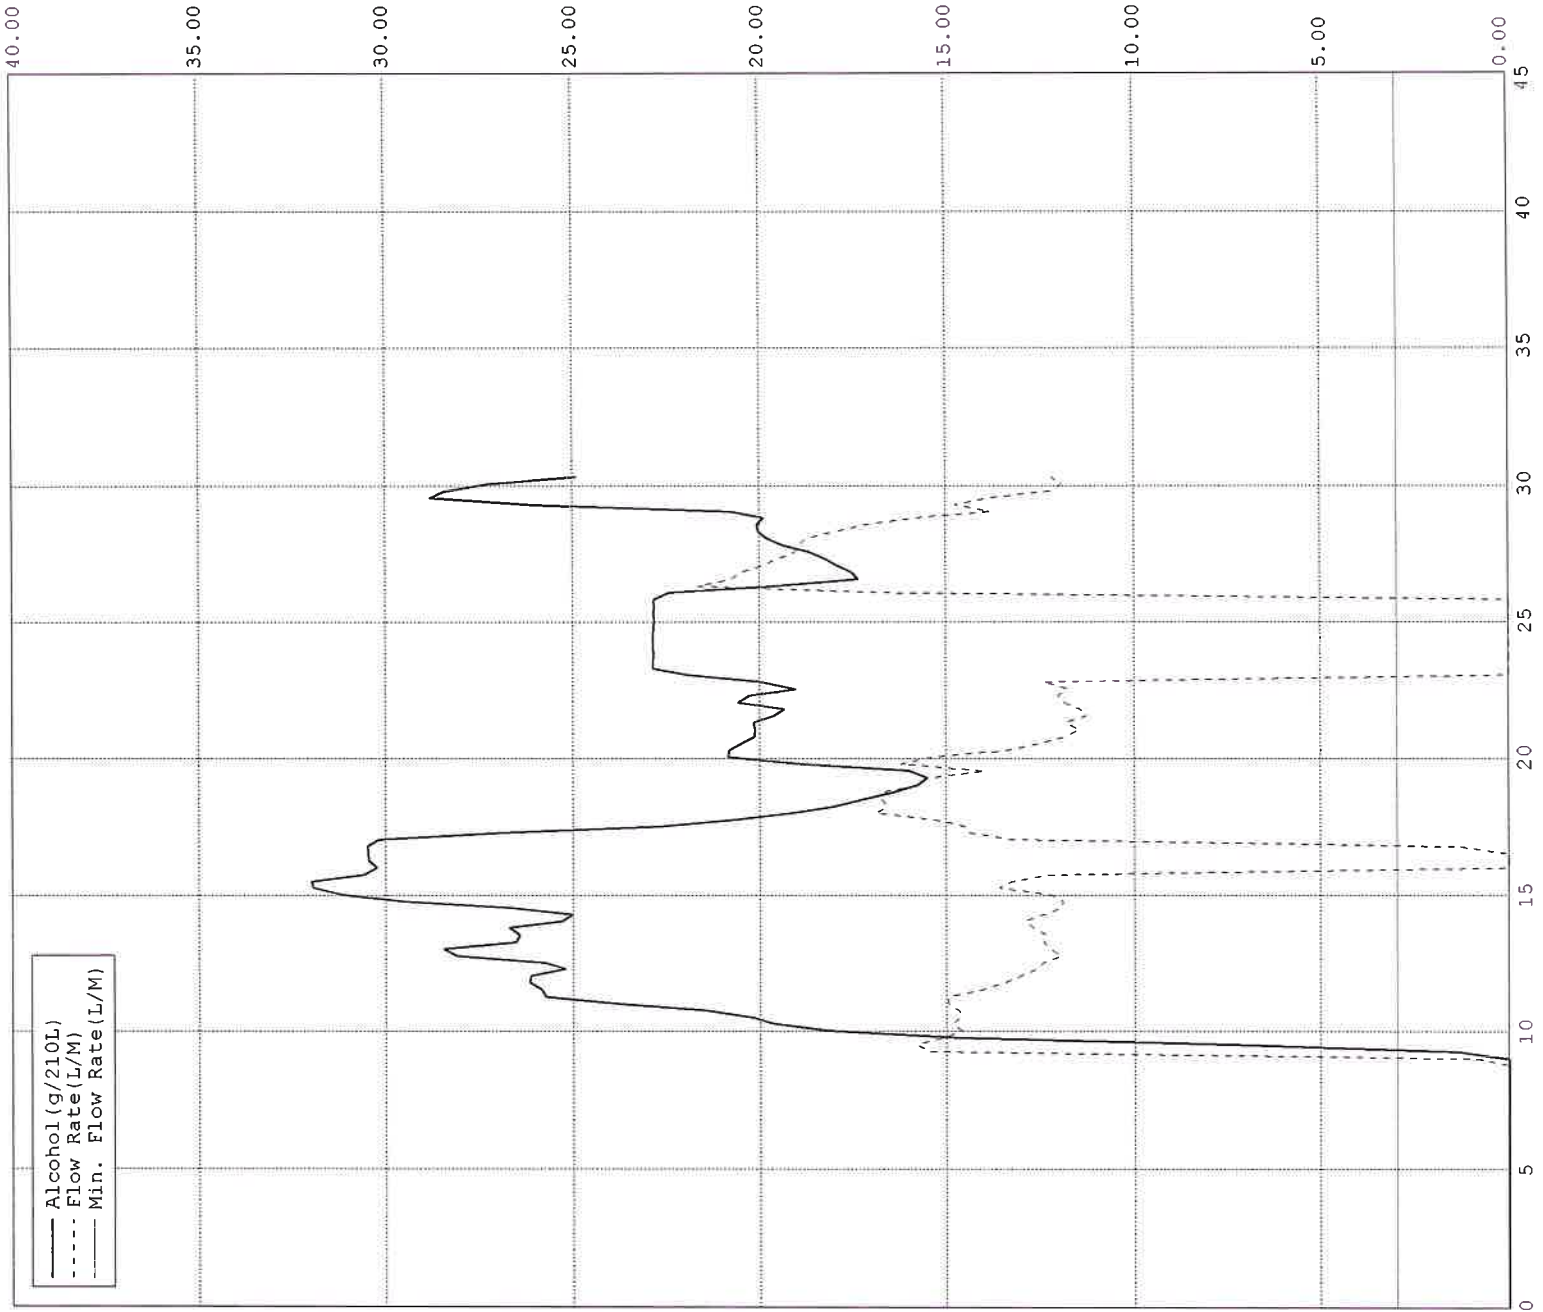

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100356

Date: 11/07/2024
Time: 11:52:30

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
RFI

CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.83: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 11:53
INTERNAL STANDARD VERIFIED 11:53
EXTERNAL STANDARD 0.077 11:53
BLANK TEST 0.000 11:54

RFI DETECTED

KS

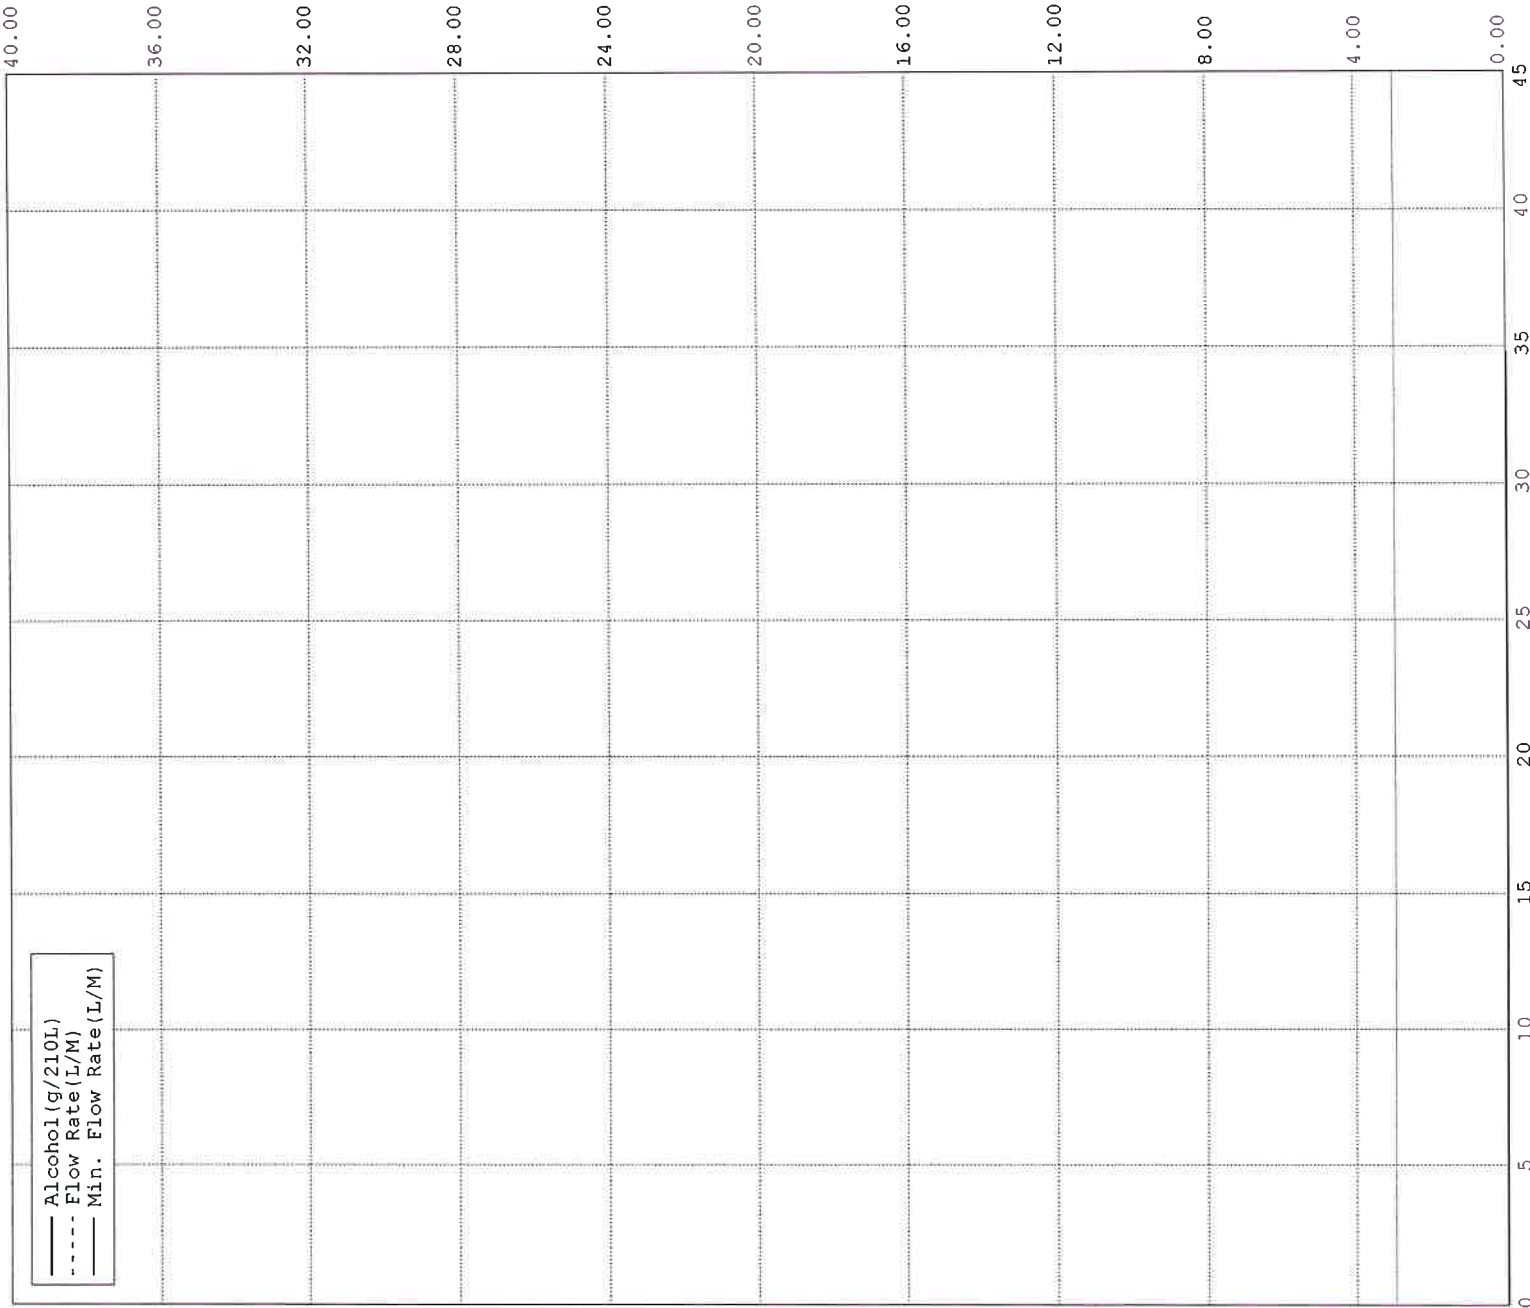

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100356

Date: 11/07/2024
Time: 13:06:53

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.82: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:08
BLANK TEST 0.000 13:08
INTERNAL STANDARD VERIFIED 13:08
Xq = 0.103 (0.00%) 0.077 13:08
EXTERNAL STANDARD X[1] = 0.0767 (0.0000) (0.0017)
BLANK TEST 0.000 13:09
SUBJECT SAMPLE XXX 13:11
X[1] = 0.1113 (-0.0197) (0.0002)

Interference Detected

Filter 2 average is 0.0001
Filter 3 average is 0.0017
KS 11/7/24

KS

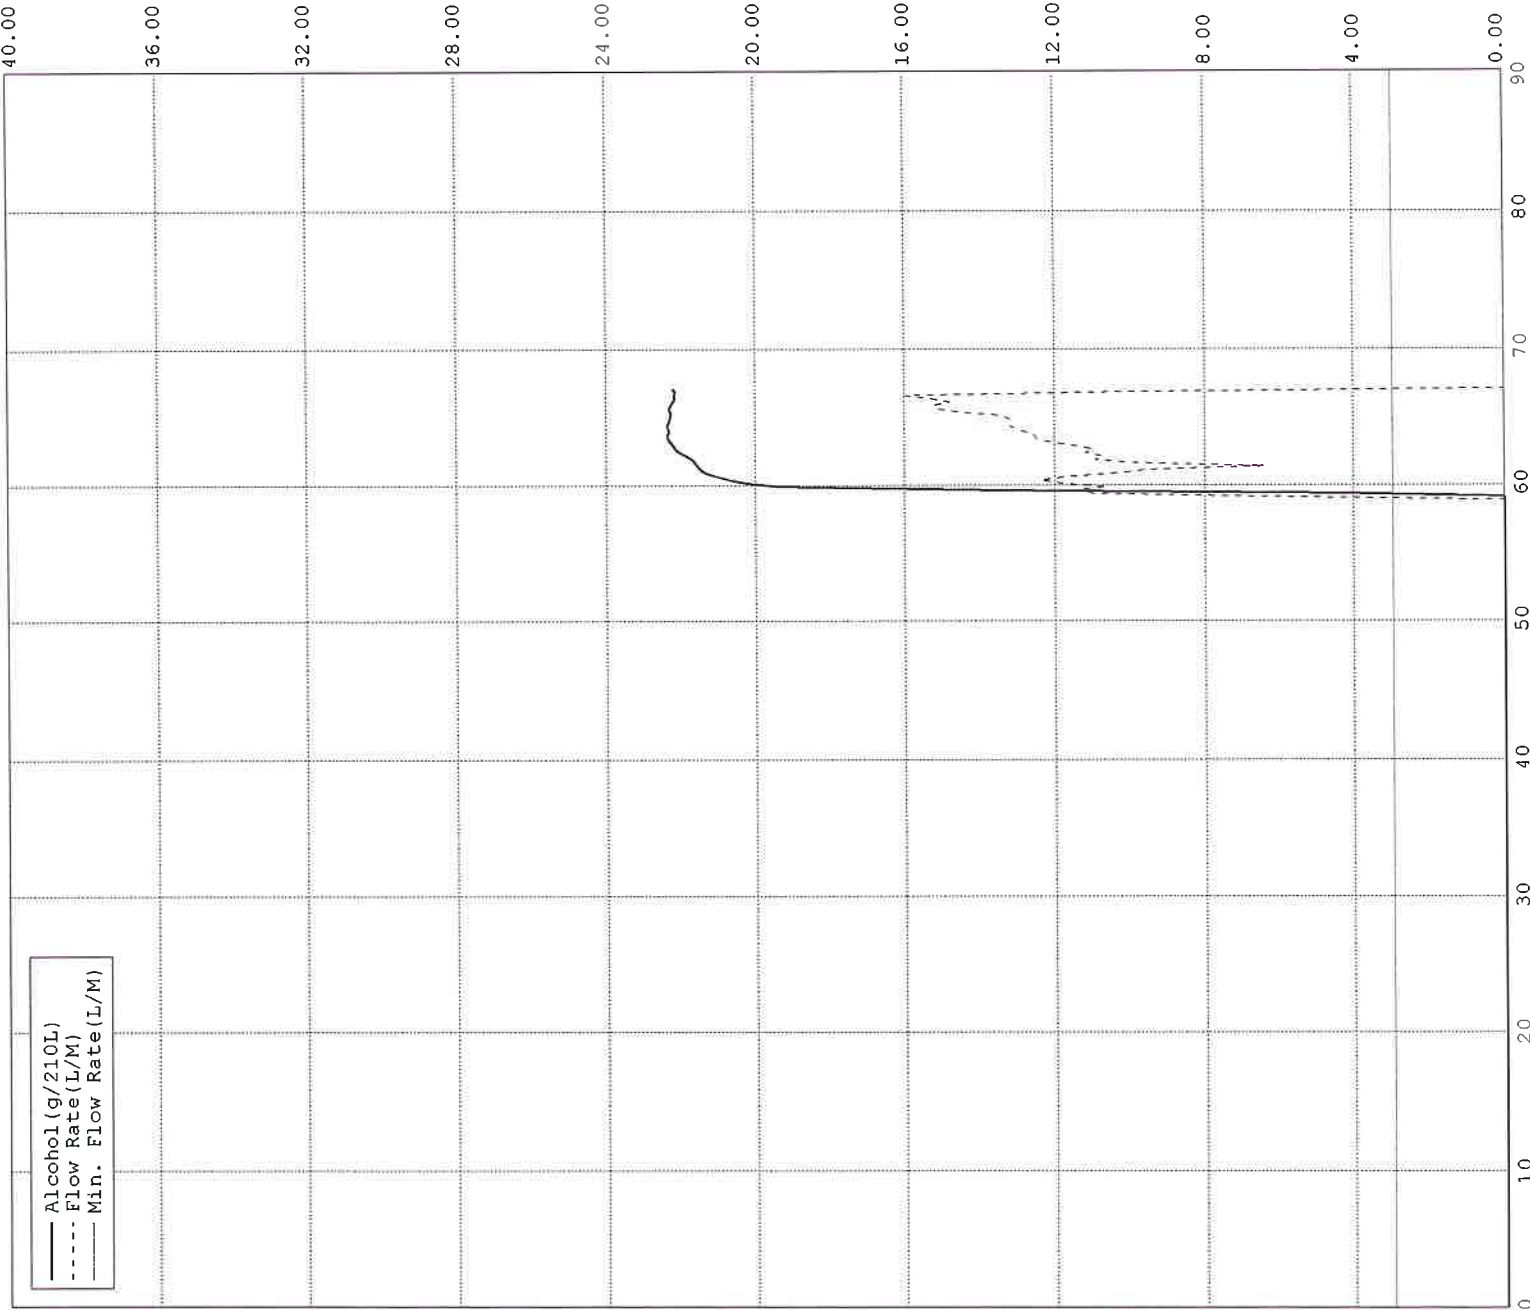

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100356

Date: 11/07/2024
Time: 13:01:34

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.82: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:02
BLANK TEST	0.000	13:02
INTERNAL STANDARD	VERIFIED	13:02
Xq = 0.103 (0.09%)	0.076	13:03
EXTERNAL STANDARD	X[1] = 0.0022	13:03
BLANK TEST	0.000	13:05
SUBJECT SAMPLE	XXX	13:05
X[1] = 0.1210 (-0.0275) (0.0012)		

Interference Detected

KS

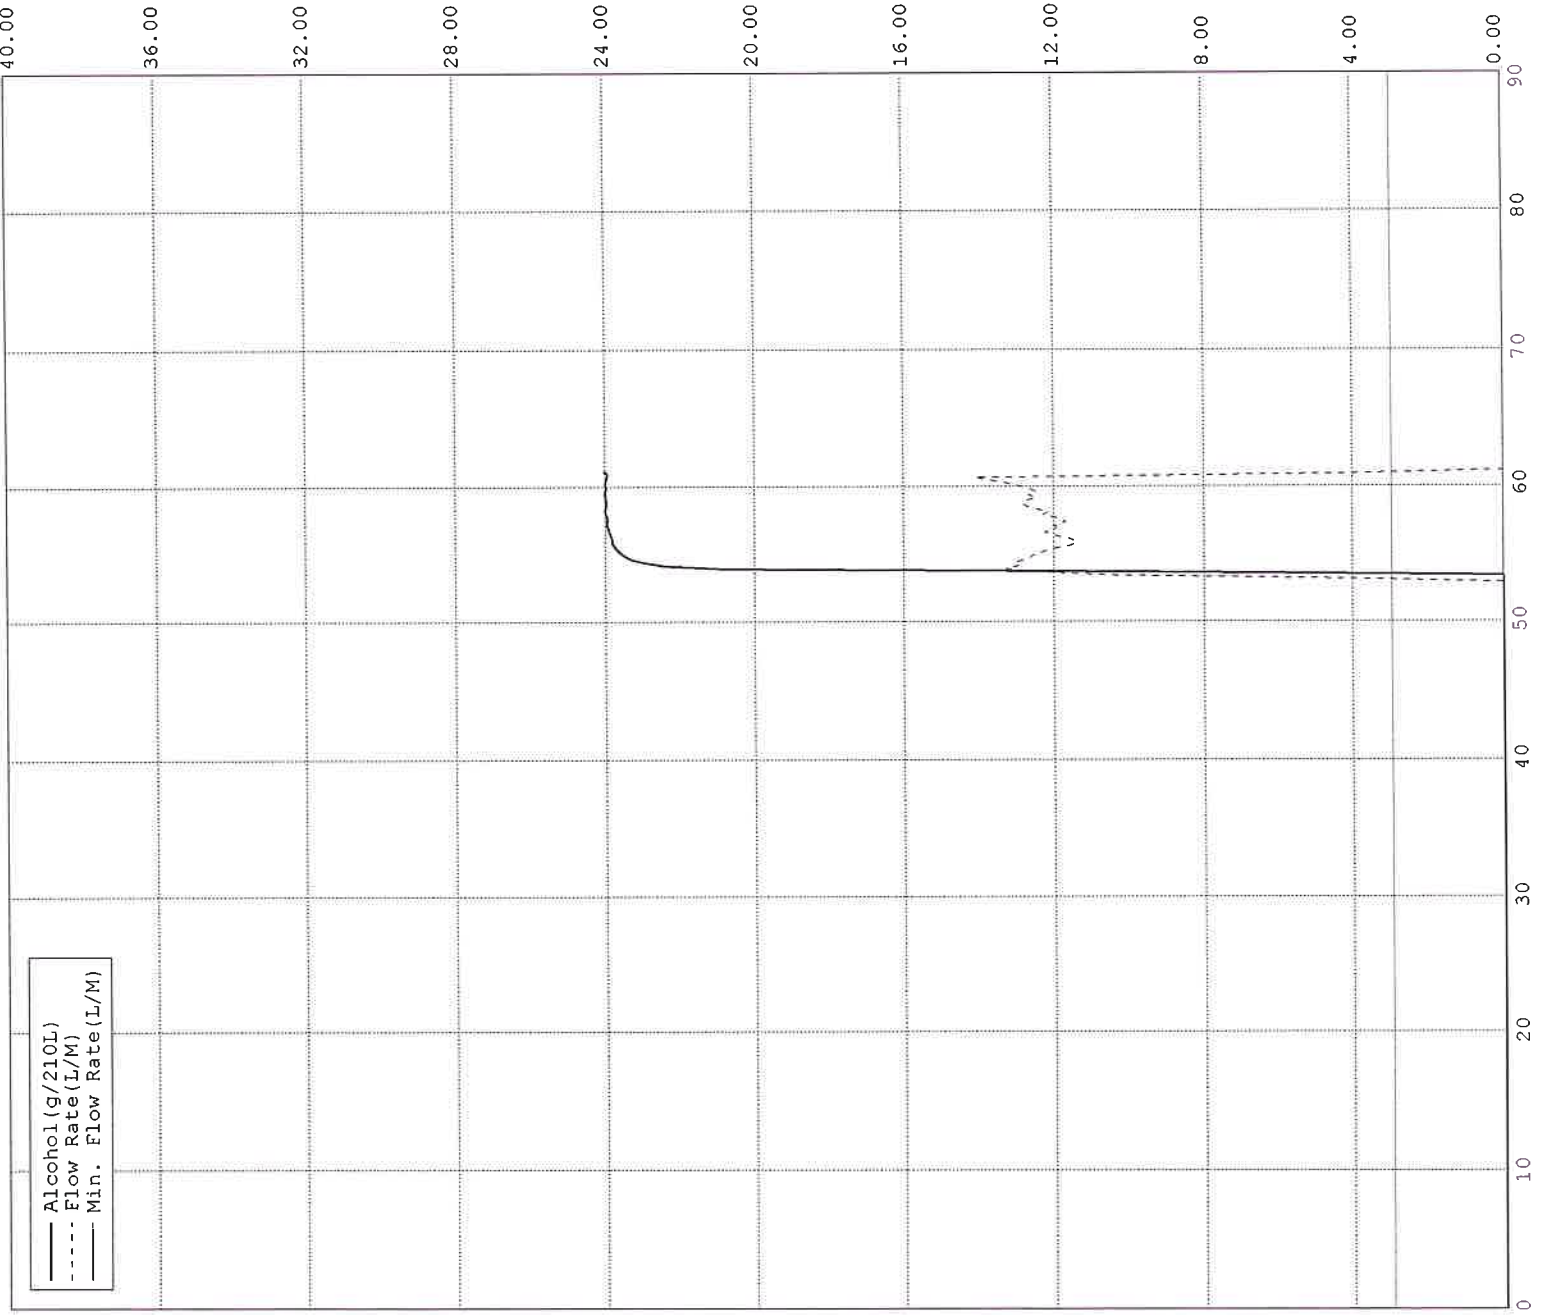

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100356

Date: 11/07/2024
Time: 13:12:57

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.82: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:13
BLANK TEST	0.000	13:14
INTERNAL STANDARD	VERIFIED	13:14
EXTERNAL STANDARD	0.077	13:14
xq = 0.103 (0.26%)		
x[1] = 0.0768 (0.0004)	(0.0016)	
BLANK TEST	0.000	13:15
SUBJECT SAMPLE (Vol=1.63L)	0.095	13:16
x[1] = 0.0952 (0.0004)	(0.0003)	
BLANK TEST	0.000	13:17
EXTERNAL STANDARD	0.076	13:17
x[1] = 0.0761 (0.0001)	(0.0011)	
BLANK TEST	0.000	13:18

FS

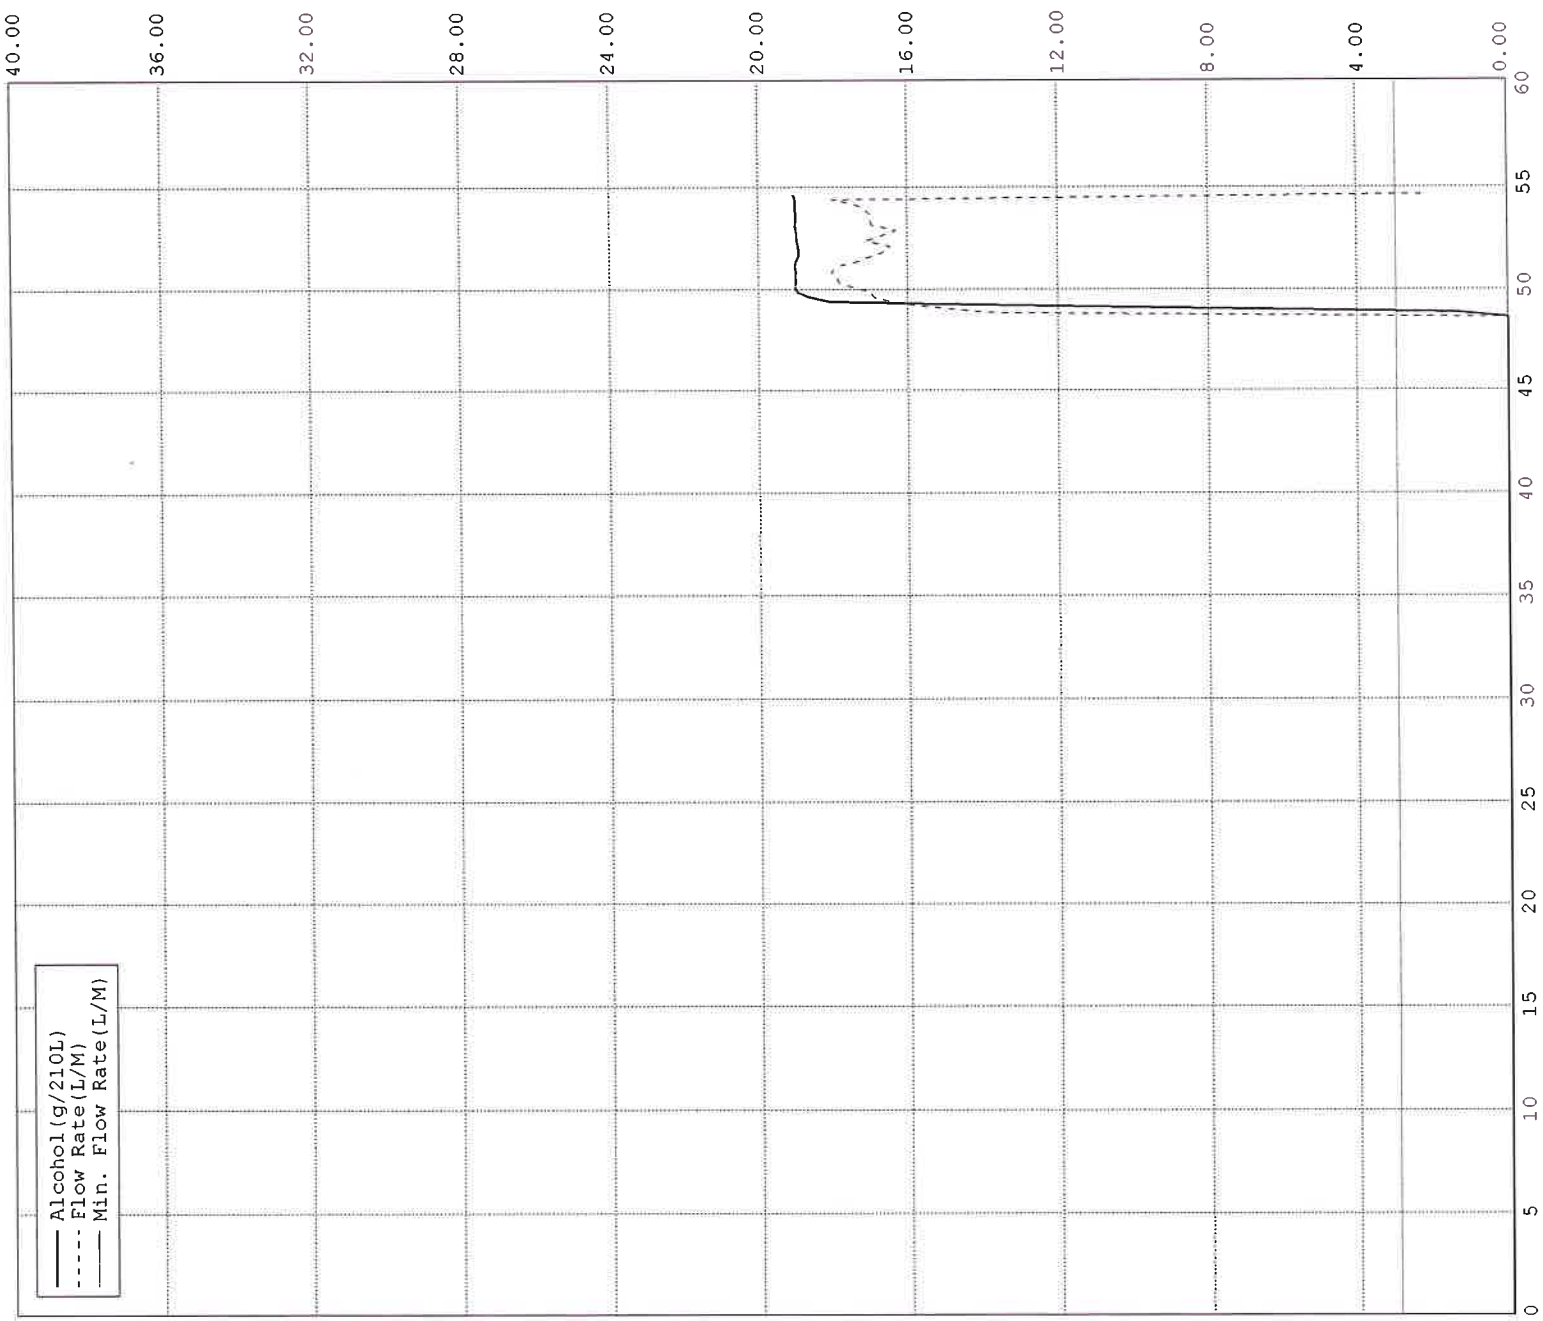

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100356

Date: 11/07/2024
Time: 14:02:11

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.81: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:03
BLANK TEST	0.000	14:03
INTERNAL STANDARD	VERIFIED	14:03
EXTERNAL STANDARD	0.076	14:04
BLANK TEST	0.000	14:05
SUBJECT SAMPLE (Vol=2.05L)	0.000	14:05
BLANK TEST	0.000	14:06
EXTERNAL STANDARD	0.077	14:06
BLANK TEST	0.000	14:07

KS

