



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100699

Report Issue Date: 07/09/2024
Date Received: 2024-05-16
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG217902	0.019	0.020	0.019	0.019	0.019	0.019
0.080	0.080	AG335202	0.080	0.079	0.078	0.078	0.078	0.079
0.300	0.299	AG327804	0.296	0.296	0.298	0.296	0.296	0.296

As Found - Evaluation Analyst: Megan Carlock
 As Found Conditions - Barometric Pressure (inHg): 29.77 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.9 Relative Humidity (%): 22
 As-Found Lab Activity Date Range: 05/16/2024 - 06/13/2024

Replaced O-ring. Supervised casework with Derek Walton. Original As Found start and end date 2024.05.16 were not entered into LIMS. Original technical review date was 2024.05.23. As found dates added and the report was rerolled on 2024.06.13.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.020	0.020	0.021	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG217904	0.040	0.040	0.040	0.039	0.040	0.040	+/- 0.003
0.080	0.080	AG335202	0.079	0.079	0.079	0.079	0.079	0.079	+/- 0.004
0.100	0.099	AG333401	0.100	0.099	0.100	0.099	0.099	0.099	+/- 0.004
0.150	0.149	AG332004	0.148	0.146	0.146	0.146	0.146	0.146	+/- 0.005
0.300	0.298	AG327804	0.298	0.298	0.297	0.297	0.298	0.298	+/- 0.011

As Left Conditions - Barometric Pressure (inHg): 29.77 Barometer Used: Fisher S/N 230307229 Temperature (C): 22.0 Relative Humidity (%): 31
 As-Left Lab Activity Date Range: 05/30/2024 - 06/03/2024

Supervised casework with Megan Carlock.

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Serial Number: 100699

Results authorized by Derek Walton on 06/18/2024

derek.walton@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 07/09/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100699 Analyst or Technician Name: Megan Crouse (Carlock)

DataMaster DMT Calibration Start Date: 5/30/24

*Supervised by Derek Watten
JMW 05/31/24*

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: 5/2/2025
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.4 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.77 Temperature(C) 22.0 Relative Humidity(%) 31
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20240501KS Expiration Date: 8/1/24
Simulator S/N: SD10588 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240501MNC Expiration Date: 8/1/24
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 224P41201 Expiration Date: 8/1/24
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 09/19/2025

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 5/30/24
Data Interpretation Date (Technician): N/A (if applicable)
Data Interpretation Date (Analyst): 5/31/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 05/30/2024
Time: 10:39:26

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 44.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.56 V PASSED
(0.94 V - 2.18 V)
Cooler Voltage = 1.51 V PASSED
(0.94 V - 2.18 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 538 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.9 in

PUMP INFO

Flow Rate = 4.266 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.001 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.077 0.56% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100699

Date: 05/30/2024
Time: 10:53 AM

Temperatures (°C)

Sample Cell: 49.0°C
Breath Tube: 43.4°C

Current Barometer 29.8 in
Volume (Ltr) 1.56

Settings

Lamp: 1.56 V
Bias: 80 V
Cooler: 1.51 V
Chopper: 518 Hz

Voltages (V)

Flow: 1.05 V
Detector: -0.055 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 12/29/2021
Time: 12:00:50

OPERATOR NAME:
CARLIE GLAISTER
CERTIFICATE #: 10436

Ca = 0.1000
CAL = 0.976429 0.800 <= CAL < 1.200
b1 = 0.0001 0.0000 <= b1 < 0.0040
b2 = 0.0059 0.0010 <= b2 < 0.0100
b3 = 0.0016 0.0000 <= b3 < 0.0040
Xq = 0.0772 0.0500 <= Xq < 0.2000
a21 = 1.162257 1.050 <= a21 < 1.300
a31 = 0.412623 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 05/30/2024
Time: 13:49:25

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CROUSE
OPERATOR'S #: 10747


DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.75: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

TEST TYPE	RESULT	TIME
DIAGNOSTIC CHECK	PASSED	13:50
BLANK TEST	0.000	13:50
INTERNAL STANDARD	VERIFIED	13:50
EXTERNAL STANDARD	0.079	13:51
BLANK TEST	0.000	13:51
SUBJECT SAMPLE (Vol=1.52L)	0.000	13:52
BLANK TEST	0.000	13:53
EXTERNAL STANDARD	0.079	13:53
BLANK TEST	0.000	13:54

MNC

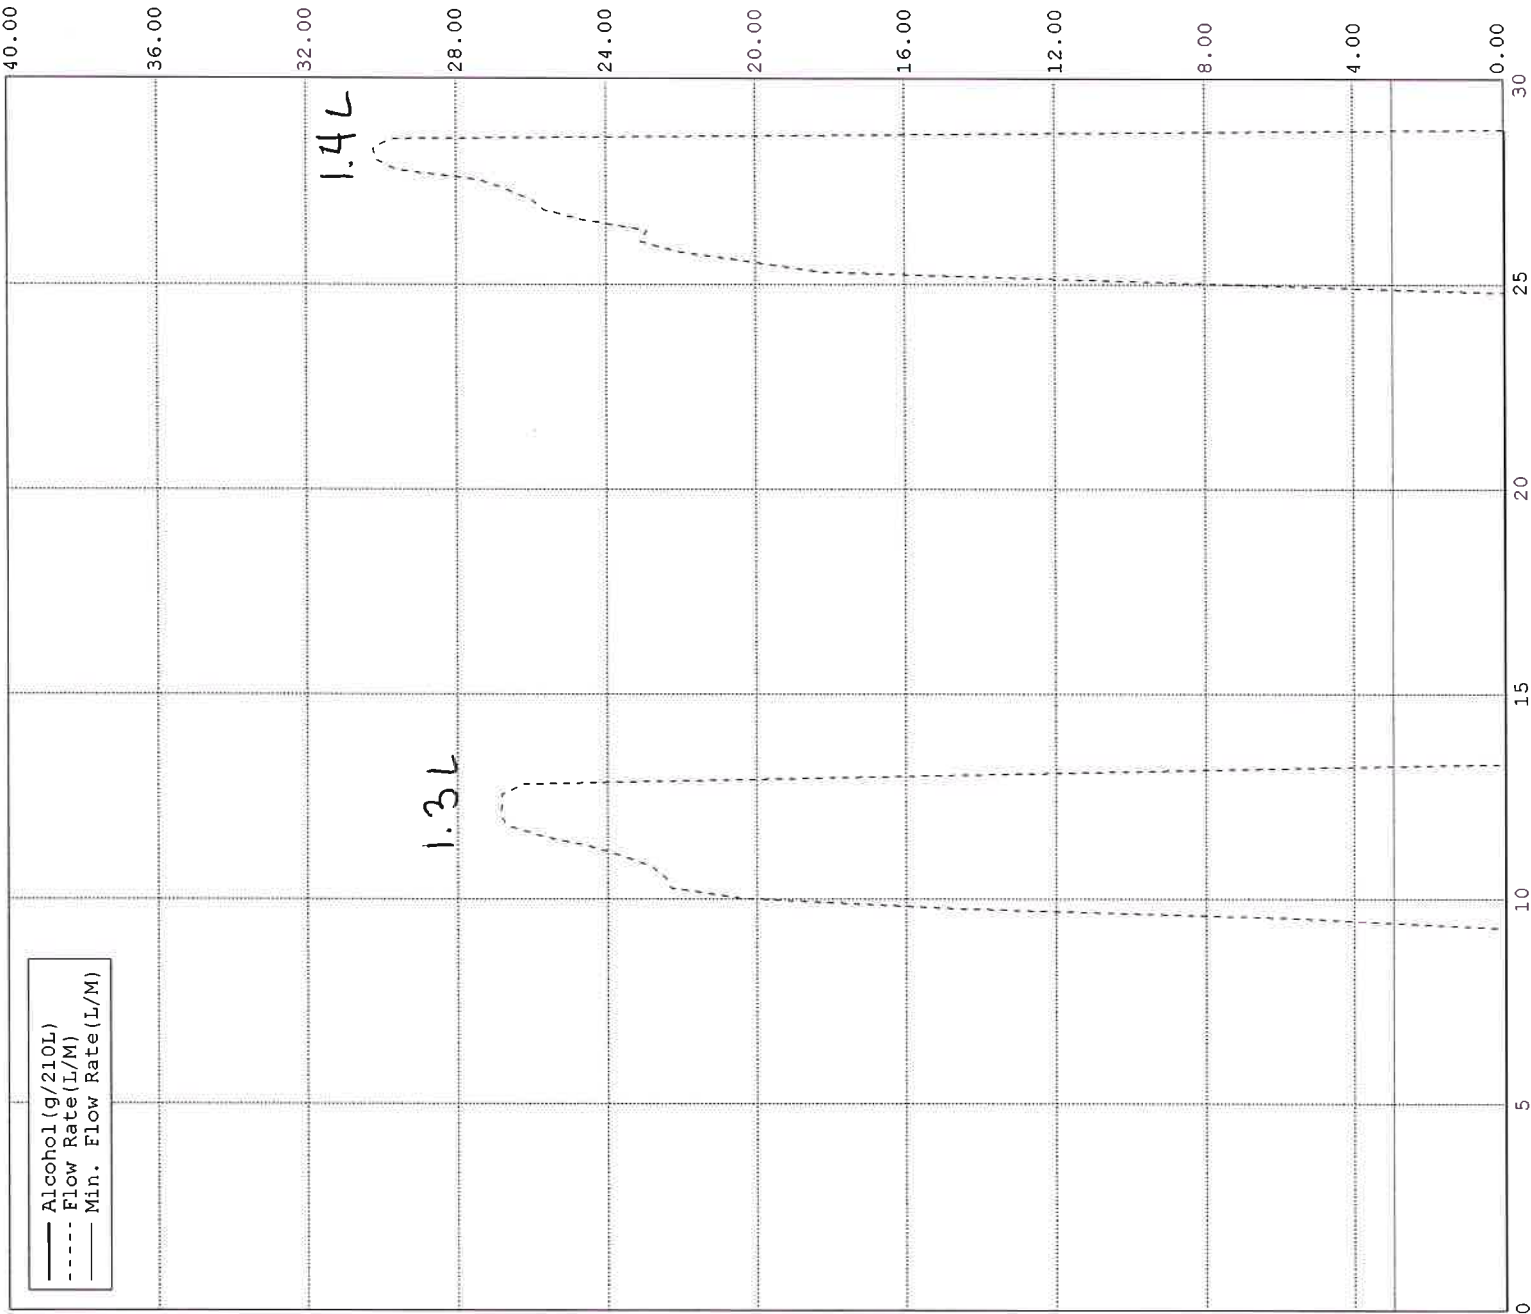

LINEARITY CHECK


Alaska Department of Public Safety
 DATAMASTER dmt: 100699

Date: 05/30/2024
 Time: 12:54:27

SUPERVISOR NAME:
 MEGAN CROUSE
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0004
0.040	0.0398	0.0004
0.080	0.0790	0.0000
0.099	0.0994	0.0005
0.149	0.1464	0.0009
0.298	0.2976	0.0005

SLOPE = 0.997254
 R² = 0.999889

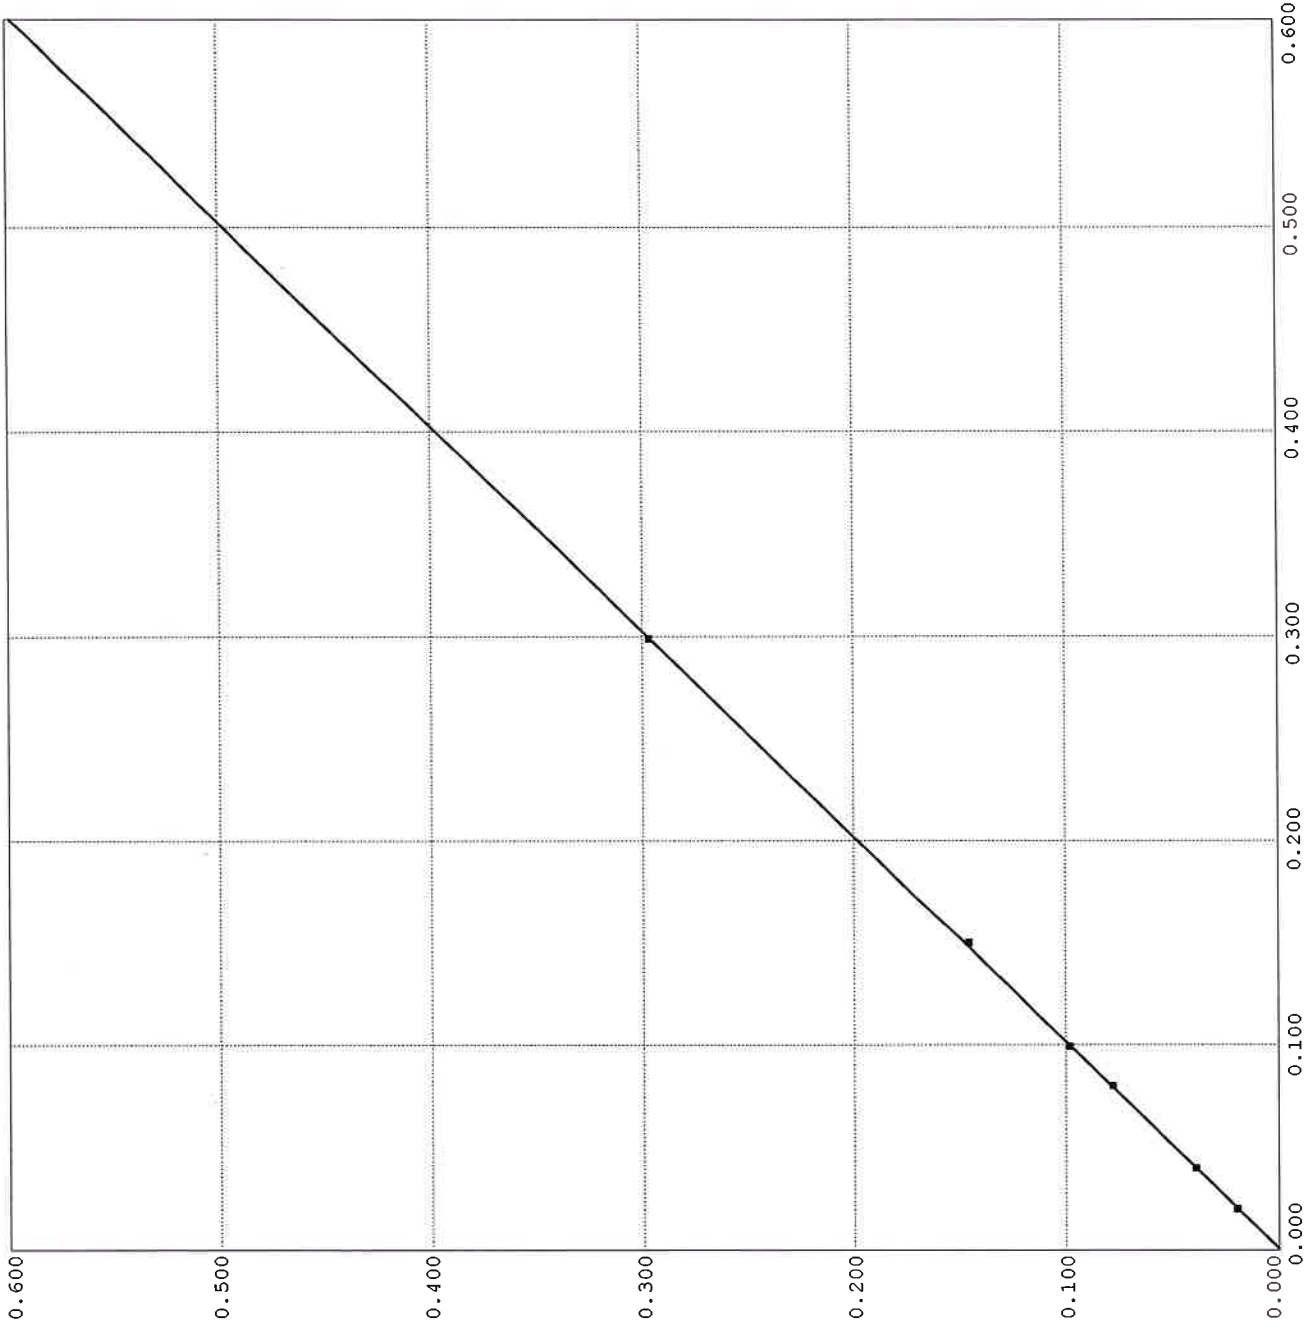

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100699






Date: 05/30/2024
 Time: 12:54:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.75: 0.020
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 308 psi

BLANK TEST	0.000	12:55
INTERNAL STANDARD	VERIFIED	12:56
EXTERNAL STANDARD	0.020	12:56
BLANK TEST	0.000	12:57
EXTERNAL STANDARD	0.020	12:57
BLANK TEST	0.000	12:58
EXTERNAL STANDARD	0.021	12:58
BLANK TEST	0.000	12:59
EXTERNAL STANDARD	0.020	12:59
BLANK TEST	0.000	13:00
EXTERNAL STANDARD	0.020	13:00
BLANK TEST	0.000	13:01

Average = 0.0202
 Std Dev = 0.0004

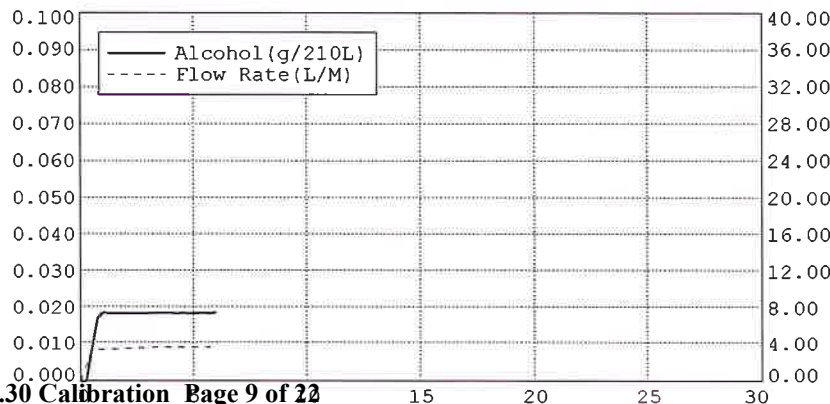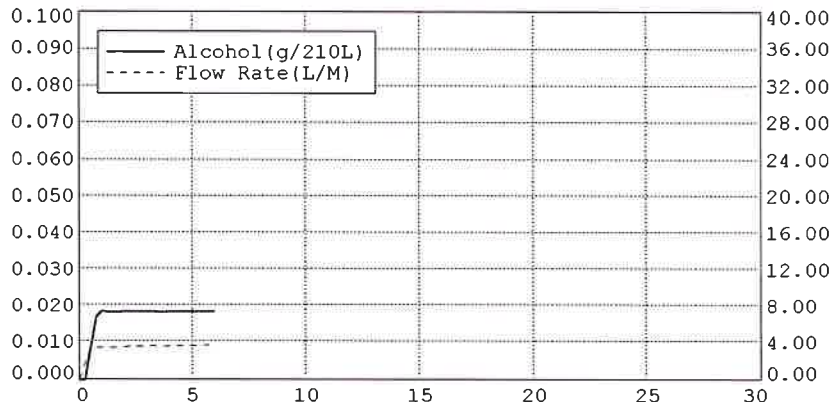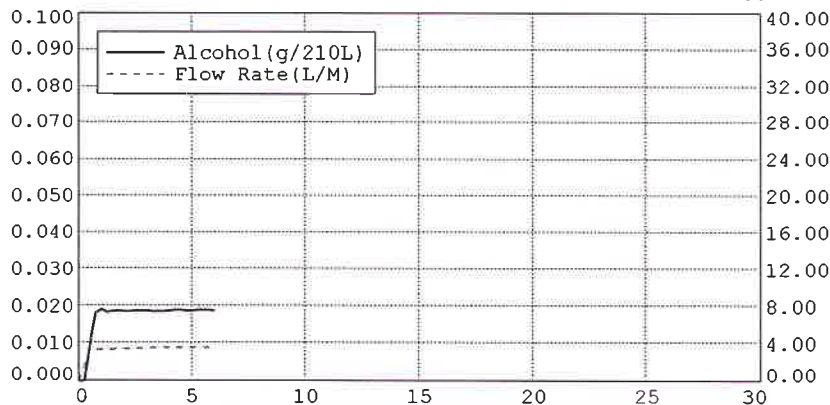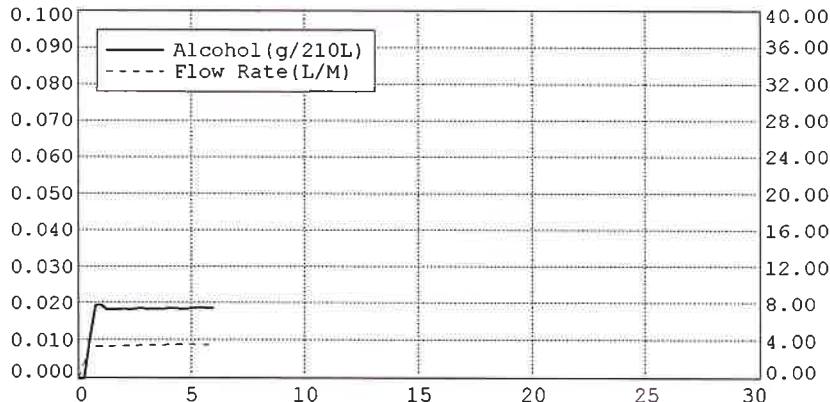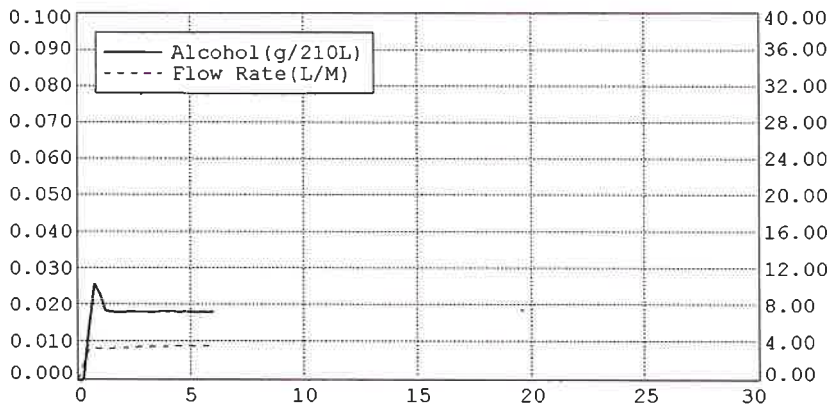

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100699






Date: 05/30/2024
Time: 13:02:57

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.75: 0.040
LOT #: AG217904
EXPIRATION: 06/28/2024
TANK PRESSURE: 686 psi

BLANK TEST	0.000	13:04
INTERNAL STANDARD	VERIFIED	13:04
EXTERNAL STANDARD	0.040	13:04
BLANK TEST	0.000	13:05
EXTERNAL STANDARD	0.040	13:05
BLANK TEST	0.000	13:06
EXTERNAL STANDARD	0.040	13:06
BLANK TEST	0.000	13:07
EXTERNAL STANDARD	0.039	13:07
BLANK TEST	0.000	13:08
EXTERNAL STANDARD	0.040	13:09
BLANK TEST	0.000	13:09

Average = 0.0398
Std Dev = 0.0004

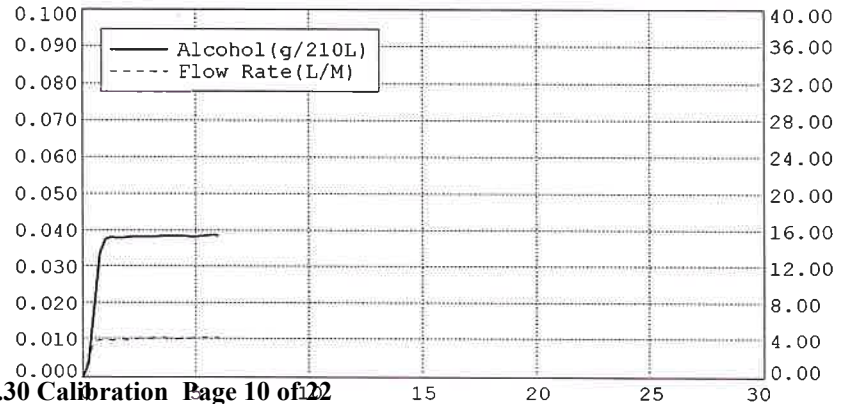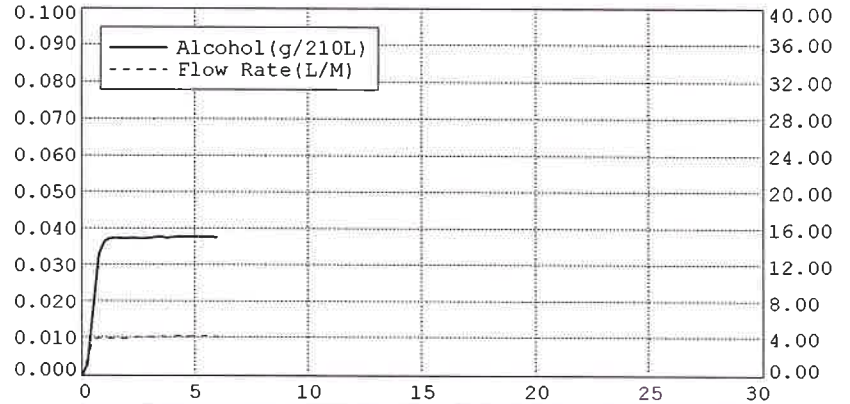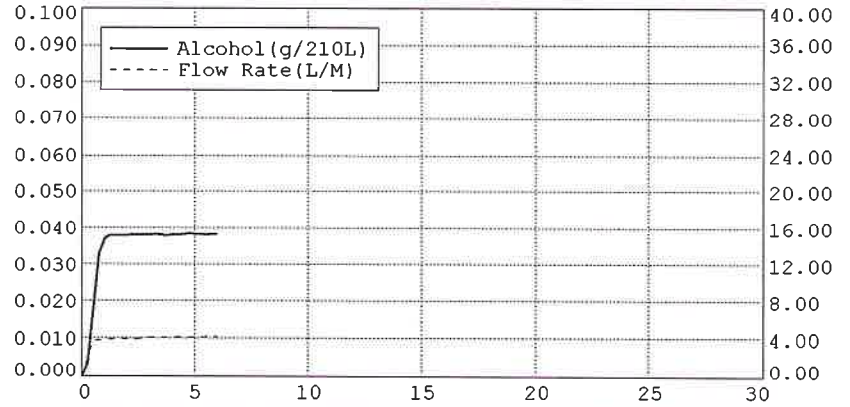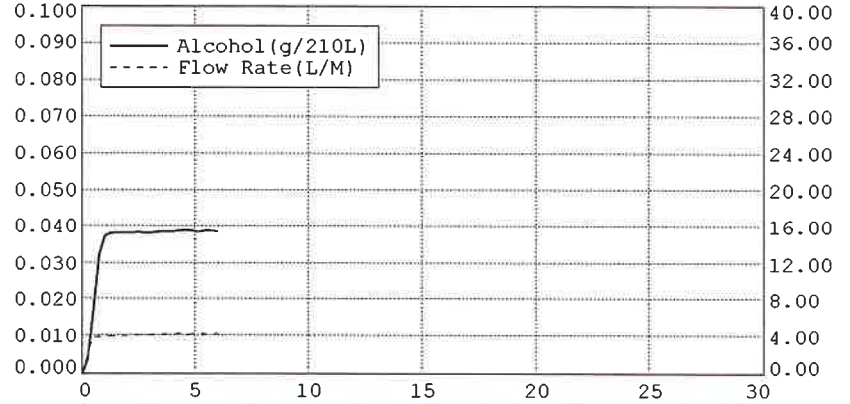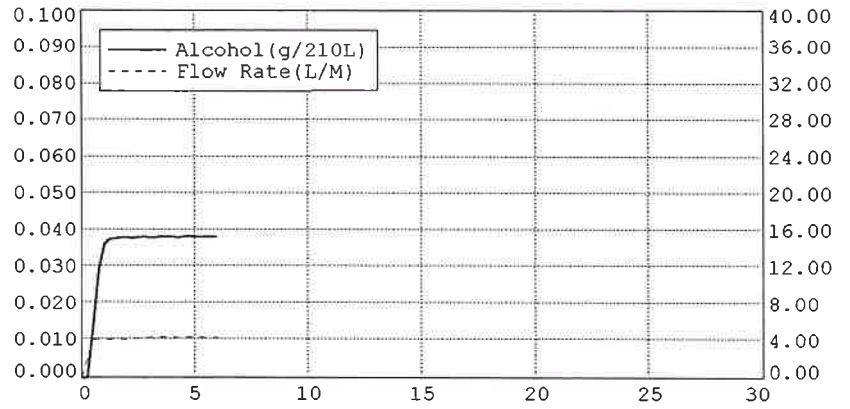

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 05/30/2024
Time: 13:13:34






EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.75: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 0 psi

BLANK TEST	0.000	13:14
INTERNAL STANDARD	VERIFIED	13:14
EXTERNAL STANDARD	0.079	13:14
BLANK TEST	0.000	13:15
EXTERNAL STANDARD	0.079	13:16
BLANK TEST	0.000	13:16
EXTERNAL STANDARD	0.079	13:17
BLANK TEST	0.000	13:18
EXTERNAL STANDARD	0.079	13:18
BLANK TEST	0.000	13:19
EXTERNAL STANDARD	0.079	13:19
BLANK TEST	0.000	13:20

Average = 0.0790
Std Dev = 0.0000

The initial test was started before the tank was fully screwed in all the way resulting in the tank pressure reading 0 psi. Mxc 5/30/24

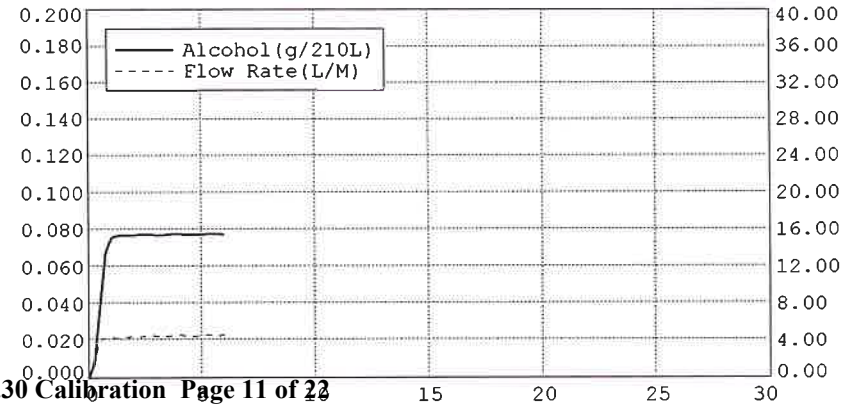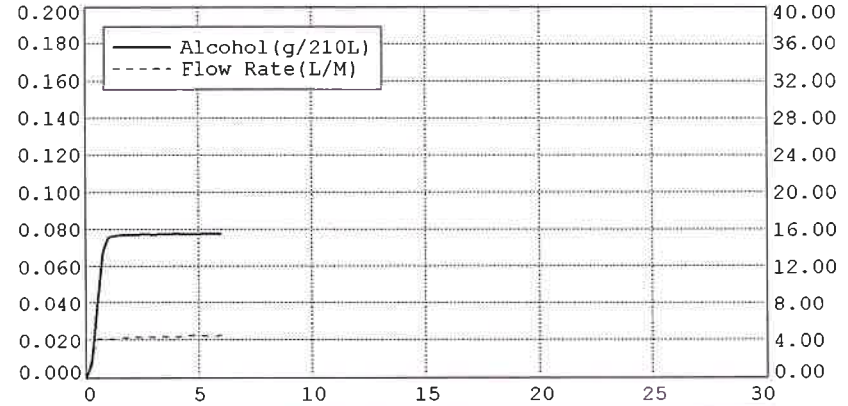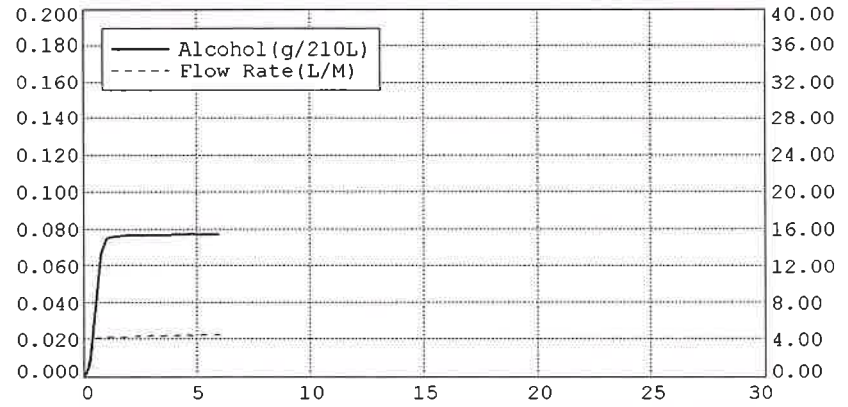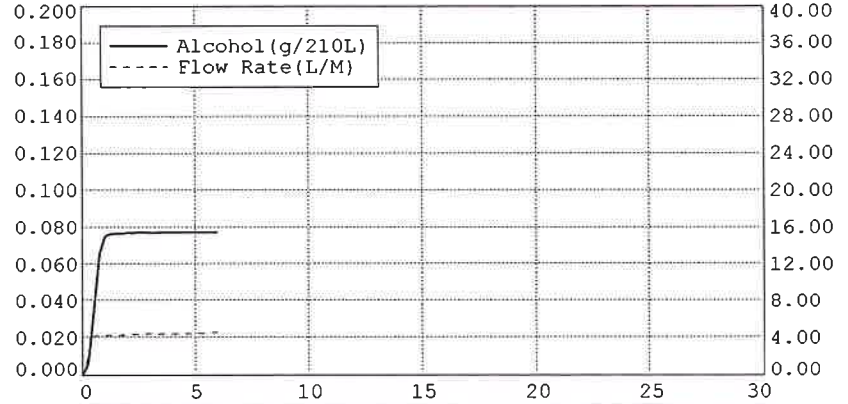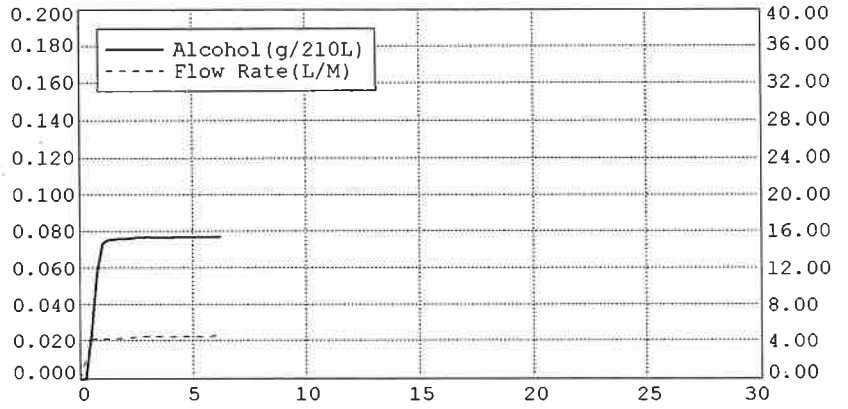

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100699






Date: 05/30/2024
 Time: 13:20:44

EXTERNAL STANDARD INFORMATION

NCMINAL: 0.100
 TARGET AT 29.75: 0.099
 LCT #: AG333401
 EXPIRATION: 11/30/2025
 TANK PRESSURE: 1198 psi

BLANK TEST	0.000	13:22
INTERNAL STANDARD	VERIFIED	13:22
EXTERNAL STANDARD	0.100	13:22
BLANK TEST	0.000	13:23
EXTERNAL STANDARD	0.099	13:23
BLANK TEST	0.000	13:24
EXTERNAL STANDARD	0.100	13:24
BLANK TEST	0.000	13:25
EXTERNAL STANDARD	0.099	13:25
BLANK TEST	0.000	13:26
EXTERNAL STANDARD	0.099	13:26
BLANK TEST	0.000	13:27

Average = 0.0994
 Std Dev = 0.0005

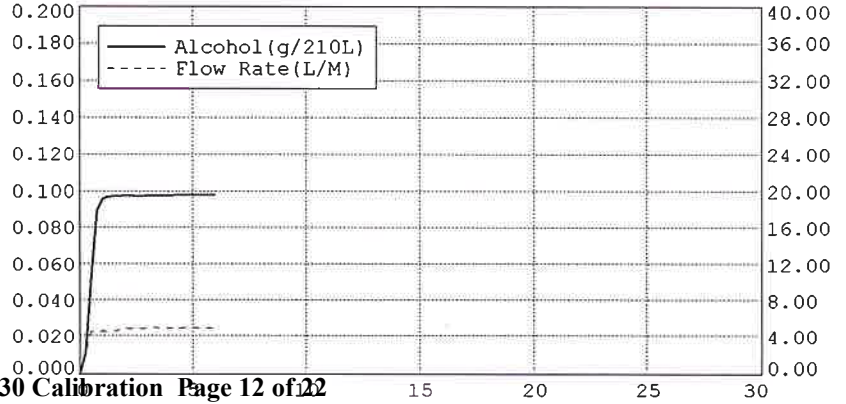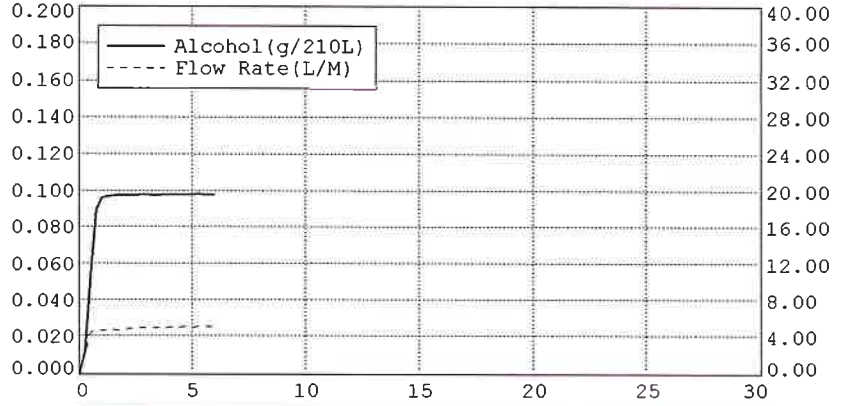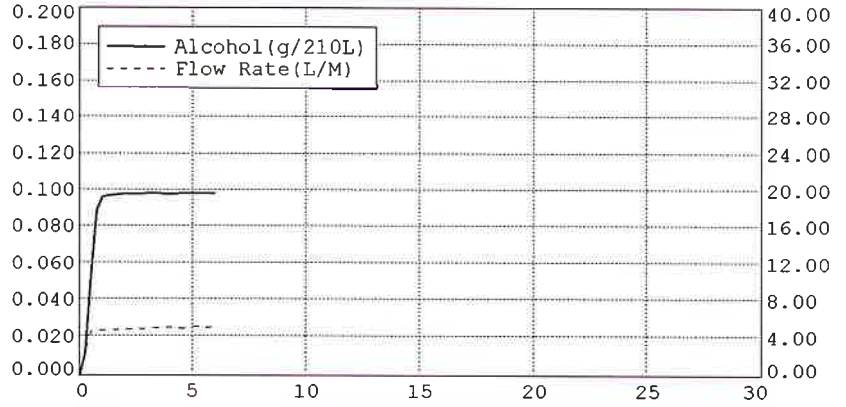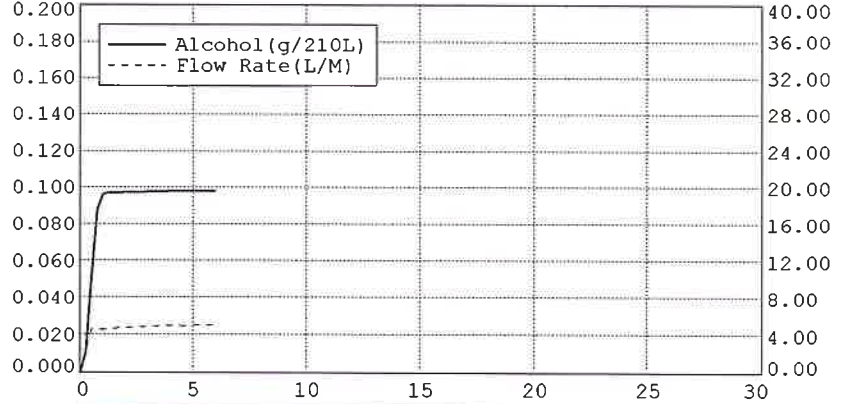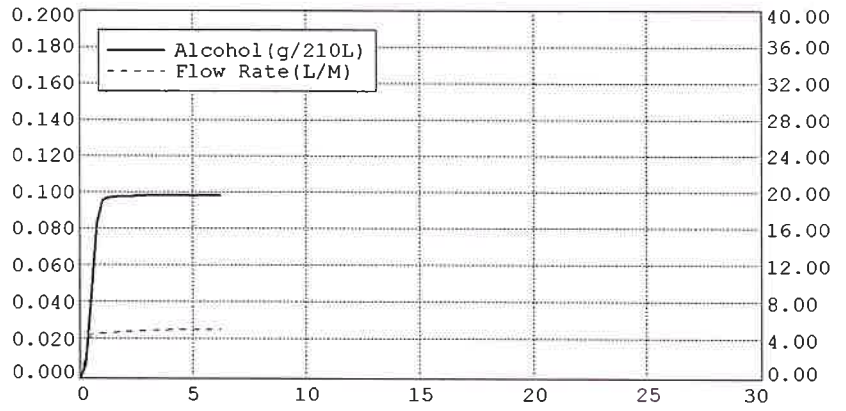

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100699






Date: 05/30/2024
Time: 13:28:13

EXTERNAL STANDARD INFORMATION

NCMINAL: 0.150
TARGET AT 29.75: 0.149
LCT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 547 psi

BLANK TEST	0.000	13:29
INTERNAL STANDARD	VERIFIED	13:29
EXTERNAL STANDARD	0.148	13:30
BLANK TEST	0.000	13:31
EXTERNAL STANDARD	0.146	13:31
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.146	13:32
BLANK TEST	0.000	13:33
EXTERNAL STANDARD	0.146	13:33
BLANK TEST	0.000	13:34
EXTERNAL STANDARD	0.146	13:34
BLANK TEST	0.000	13:35

Average = 0.1464
Std Dev = 0.0009

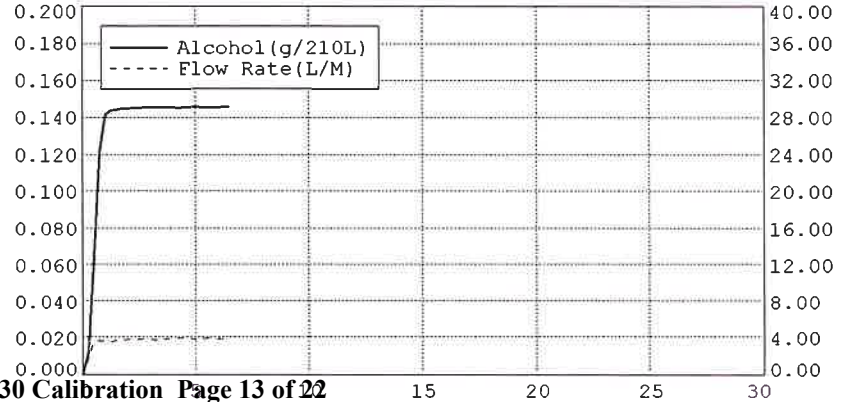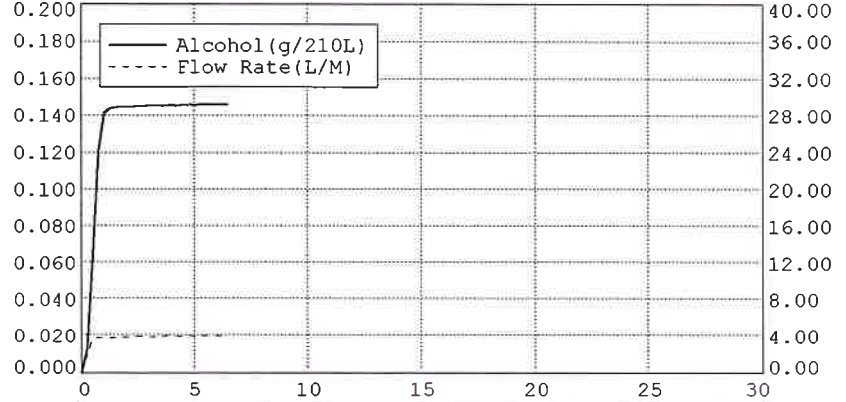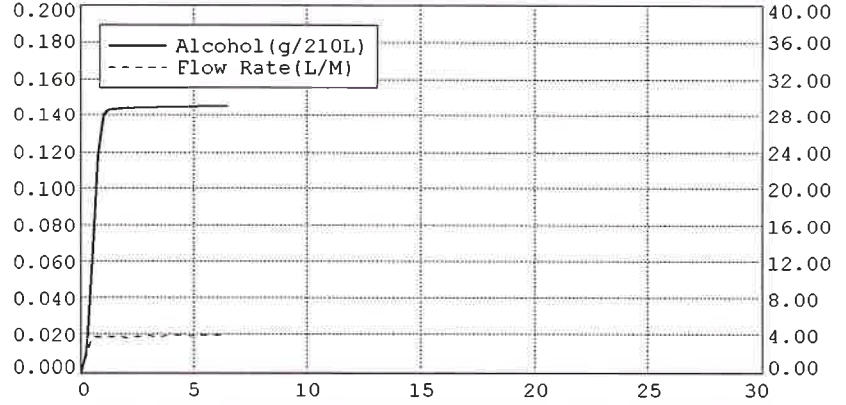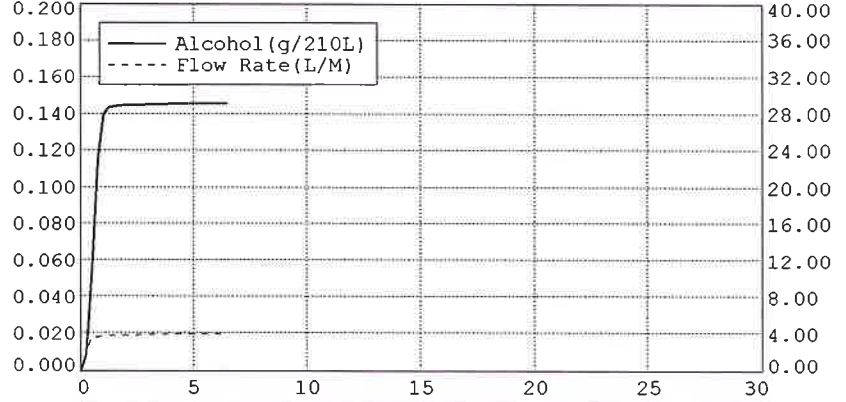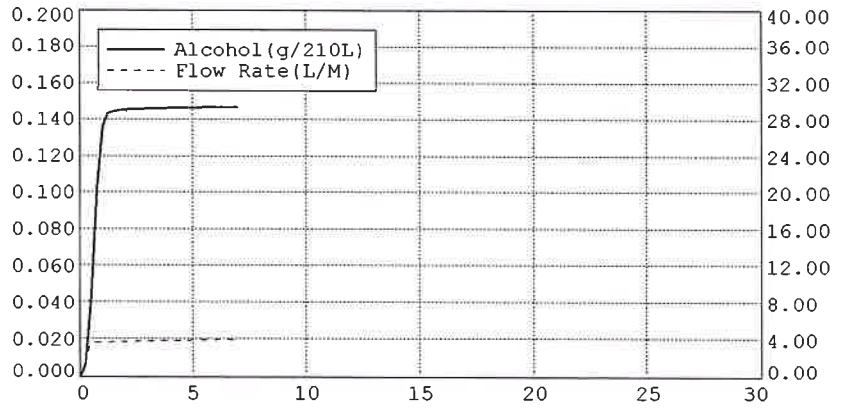

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100699






Date: 05/30/2024
 Time: 13:37:22

EXTERNAL STANDARD INFORMATION

NCMINAL: 0.300
 TARGET AT 29.75: 0.298
 LGT #: AG327804
 EXPIRATION: 10/05/2025
 TANK PRESSURE: 396 psi

BLANK TEST	0.000	13:38
INTERNAL STANDARD	VERIFIED	13:38
EXTERNAL STANDARD	0.298	13:39
BLANK TEST	0.000	13:40
EXTERNAL STANDARD	0.298	13:40
BLANK TEST	0.000	13:41
EXTERNAL STANDARD	0.297	13:41
BLANK TEST	0.000	13:42
EXTERNAL STANDARD	0.297	13:42
BLANK TEST	0.000	13:43
EXTERNAL STANDARD	0.298	13:44
BLANK TEST	0.000	13:45

Average = 0.2976
 S-d Dev = 0.0005

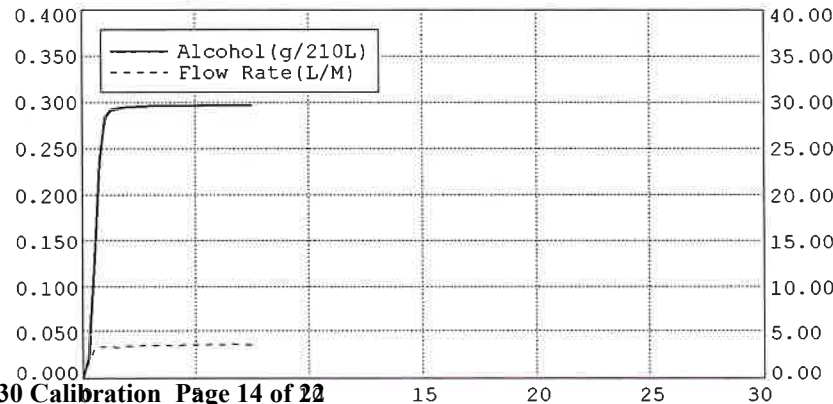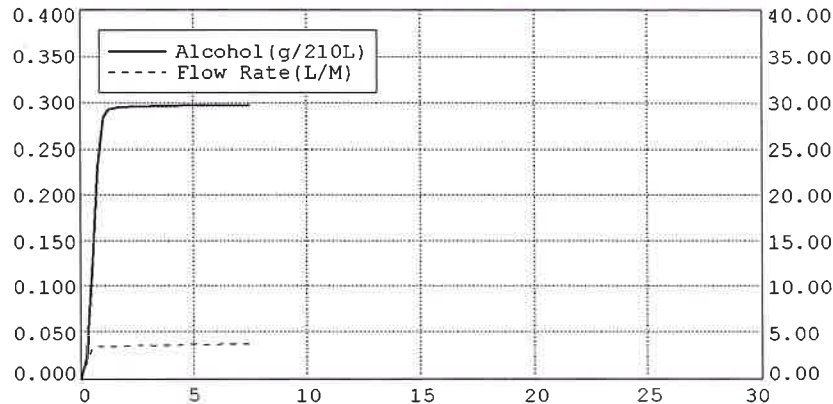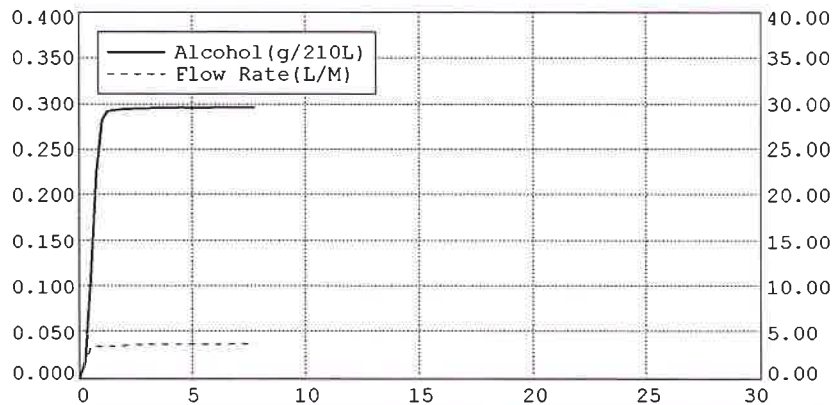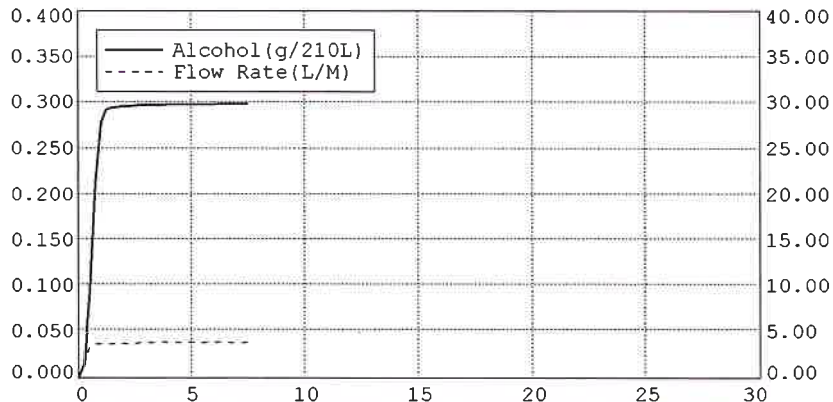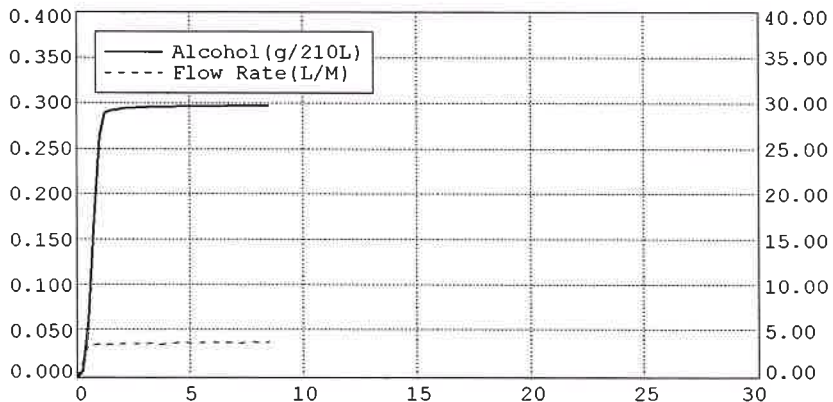

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 05/30/2024
Time: 11:17:26

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CROUSE
OPERATOR'S #: 10747


DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.76: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:18
BLANK TEST 0.000 11:18
INTERNAL STANDARD VERIFIED 11:18
EXTERNAL STANDARD 0.078 11:18
BLANK TEST 0.000 11:19
SUBJECT SAMPLE INCOMPLETE 11:21

MNC

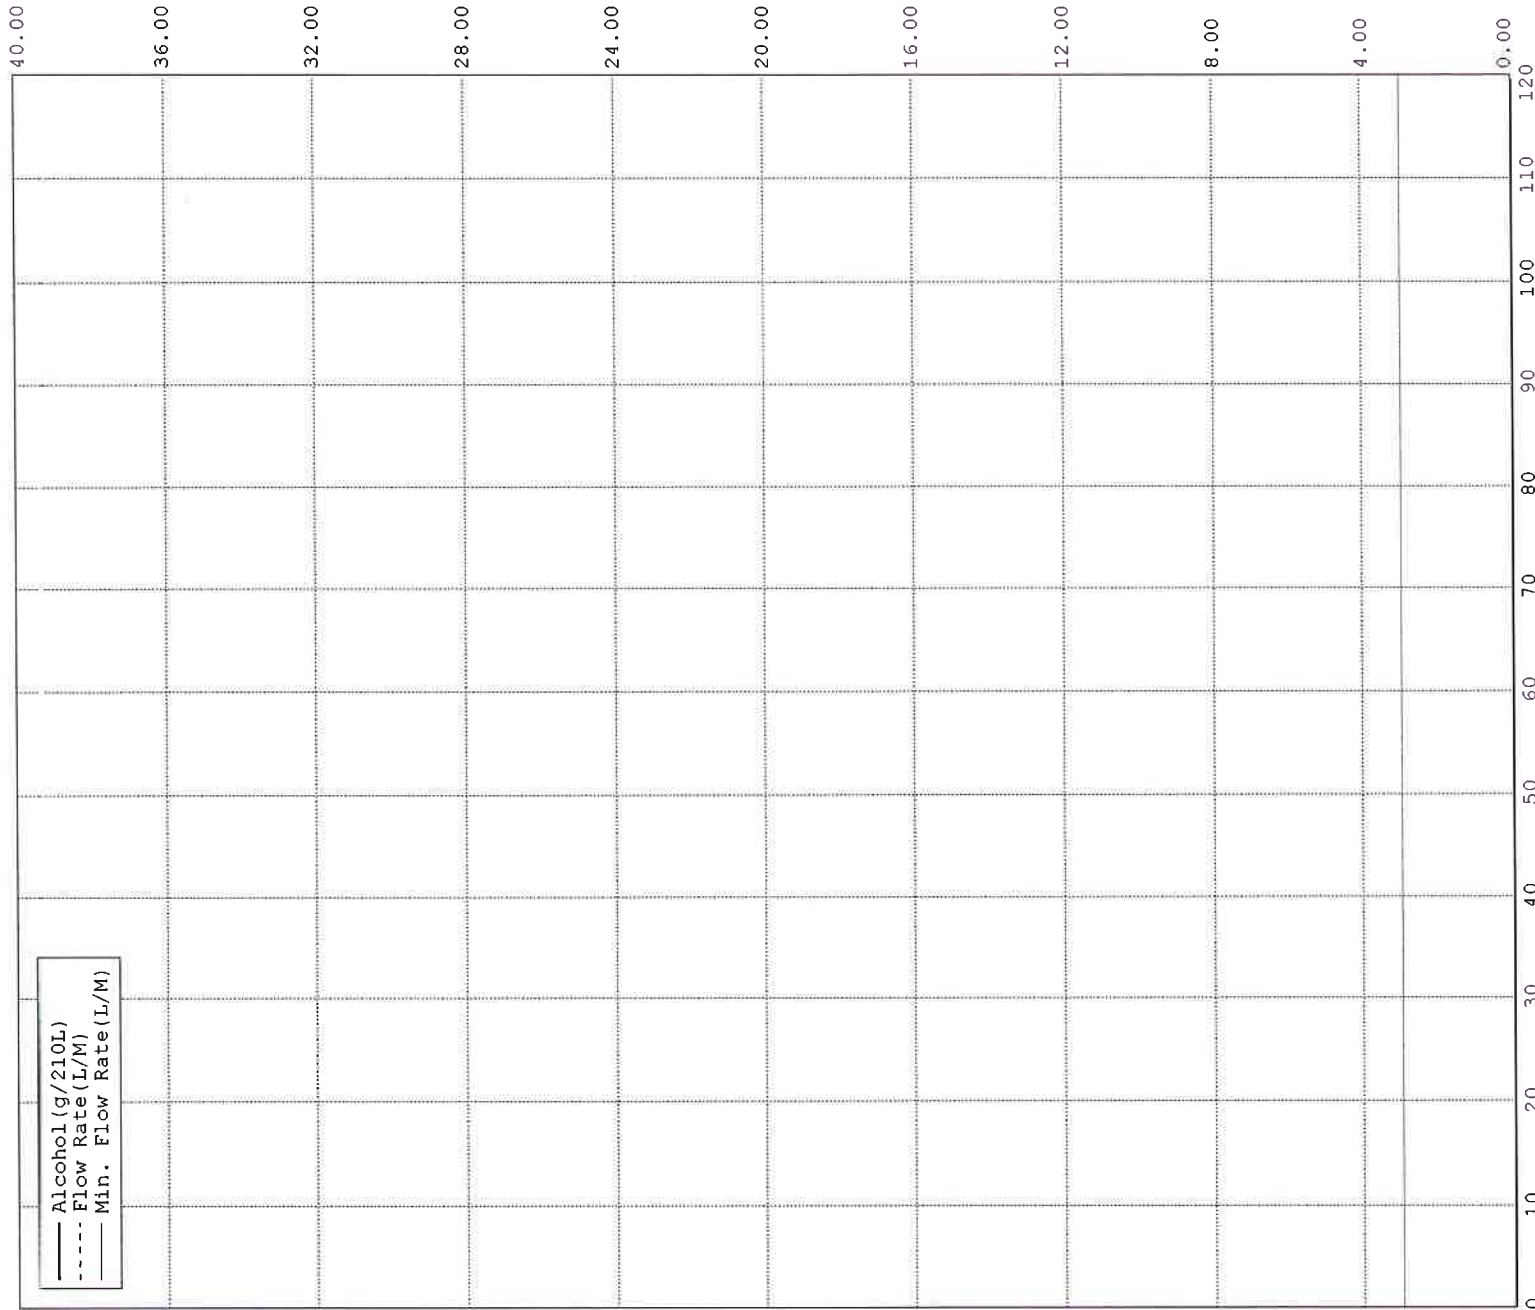

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 05/30/2024
Time: 11:24:55

SUBJECT NAME:
TEST TEST
LICENSE #: XXX
OPERATOR NAME:
MEGAN CROUSE
OPERATOR'S #: 10747


DEPT/AGENCY:
MAXIMUM ATTEMPTS
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.76: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:25
BLANK TEST 0.000 11:26
INTERNAL STANDARD VERIFIED 11:26
EXTERNAL STANDARD 0.081 11:26
BLANK TEST 0.000 11:27
SUBJECT SAMPLE XXX 11:28

Maximum Attempts Exceeded

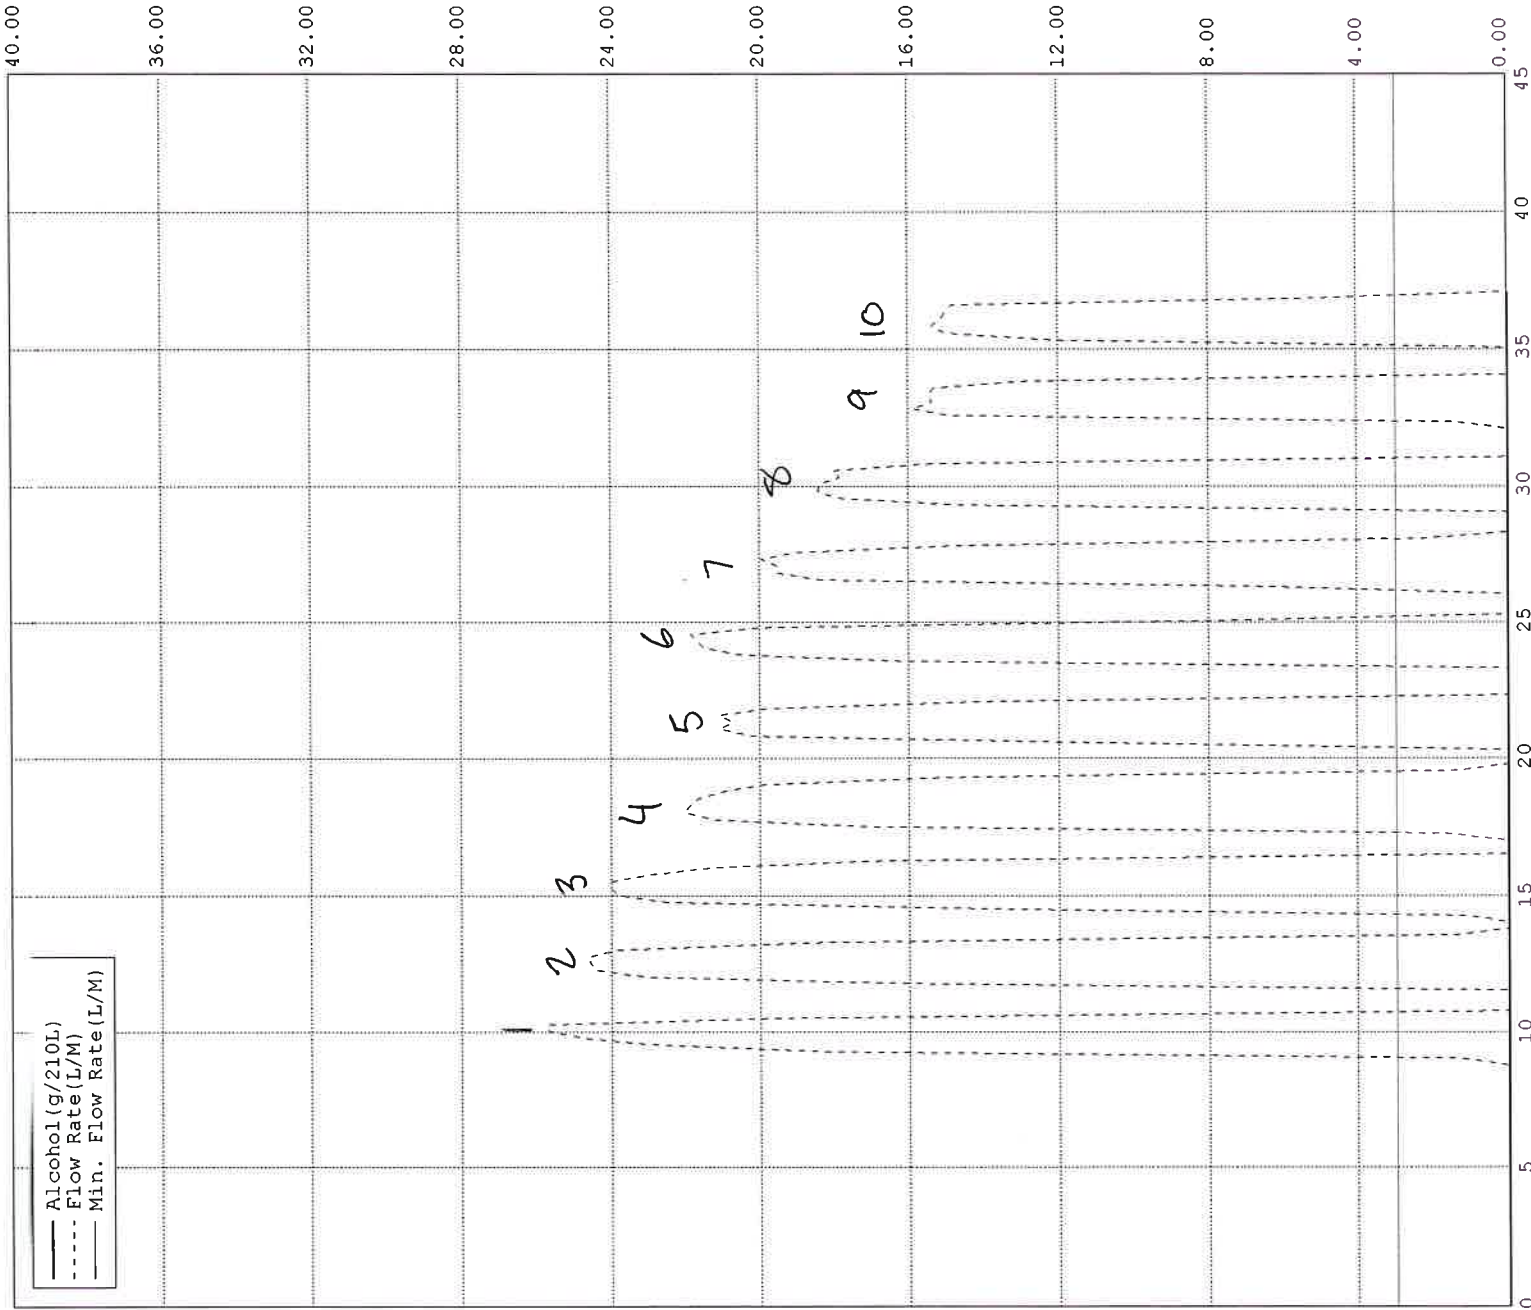

MNC

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 05/30/2024
Time: 11:50:26

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CROUSE
OPERATOR'S #: 10747

DEPT/AGENCY:
INVALID

CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.76: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:51
BLANK TEST 0.000 11:51
INTERNAL STANDARD VERIFIED 11:51
EXTERNAL STANDARD 0.080 11:51
BLANK TEST 0.000 11:52
SUBJECT SAMPLE INVALID 11:53

MJC



SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100699

Date: 05/30/2024

Time: 12:48:03

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CROUSE

OPERATOR'S #: 10747

DEPT/AGENCY:

RFI

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.75: 0.080


LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:49
BLANK TEST	0.000	12:49
INTERNAL STANDARD	VERIFIED	12:49
EXTERNAL STANDARD	0.080	12:49
BLANK TEST	0.000	12:50

RFI DETECTED

MNC

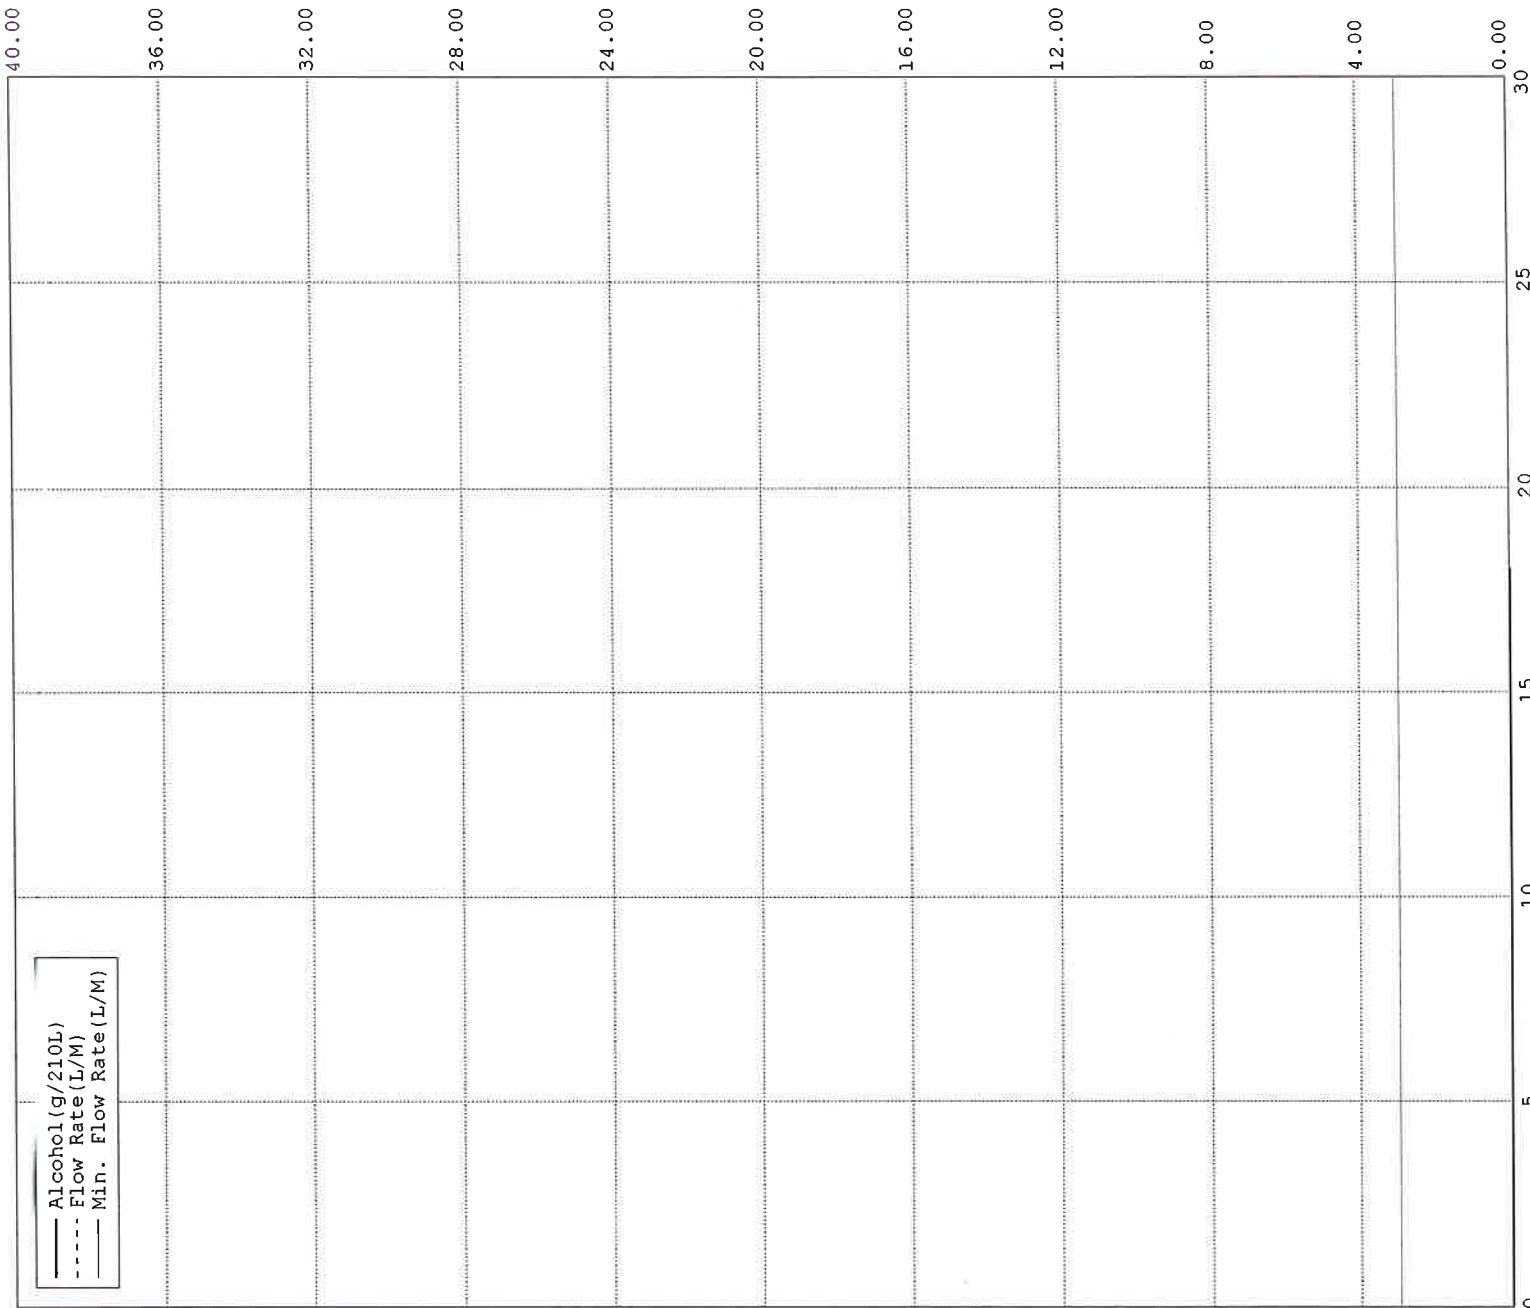

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 05/30/2024
Time: 14:18:10

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CROUSE
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.74: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 14:19
BLANK TEST 0.000 14:19
INTERNAL STANDARD VERIFIED 14:19
Xq = 0.079 (1.91%) 0.079 14:19
X[1] = 0.0788 (-0.0009) (0.0012) 0.000 14:20
BLANK TEST XXX 14:20
SUBJECT SAMPLE X[1] = 0.1123 (-0.0113) (0.0048)

Interference Detected


Filter 2 Average: -0.0010

Filter 3 Average: 0.0018

Verified by JMC

05/31/24

MNC

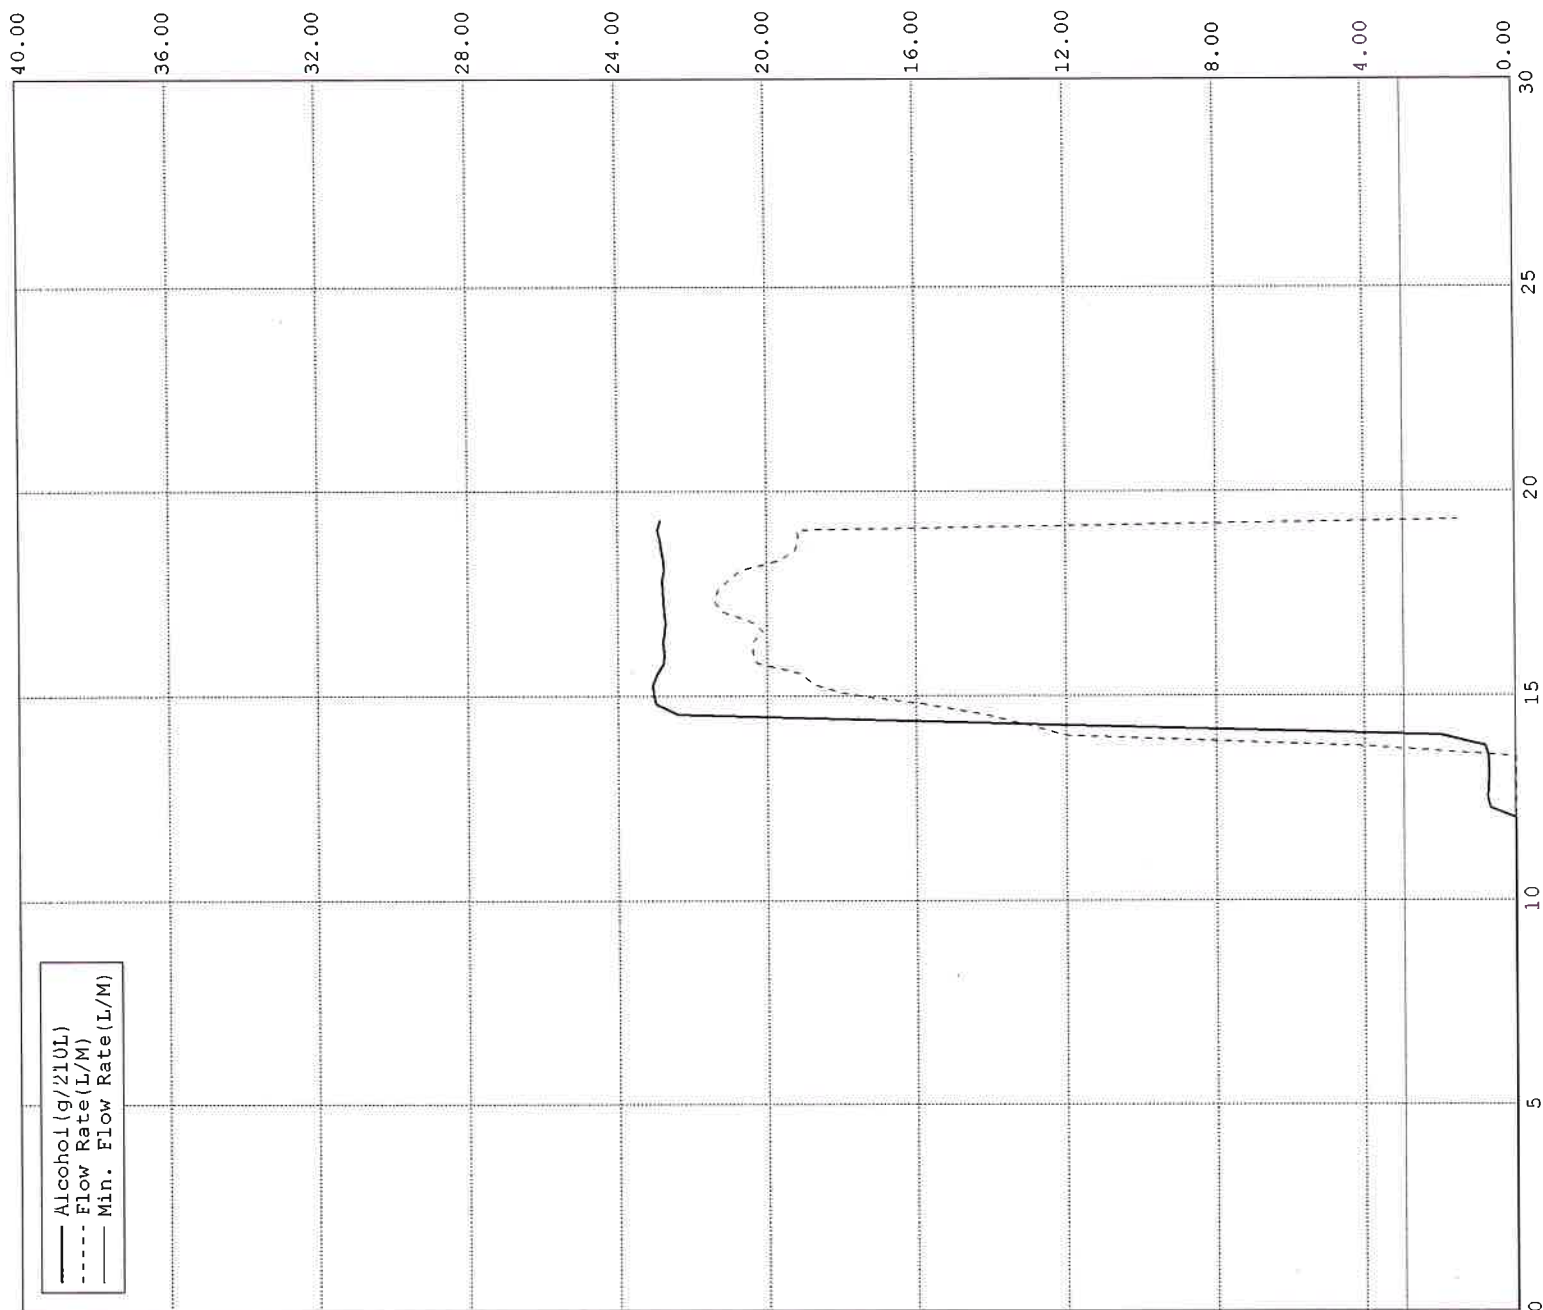

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 05/30/2024
Time: 14:22:58

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CROUSE
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080
TARGET AT 29.74: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 14:24
BLANK TEST 0.000 14:24
INTERNAL STANDARD VERIFIED 14:24
Xq = 0.077 (0.22%) 0.079 14:24
EXTERNAL STANDARD 0.000 (0.0030)
X[1] = 0.0787 (-0.0009) 0.000 14:25
BLANK TEST XXX 14:25
SUBJECT SAMPLE X[1] = 0.1145 (-0.0222) (0.0028)

Interference Detected

MNC

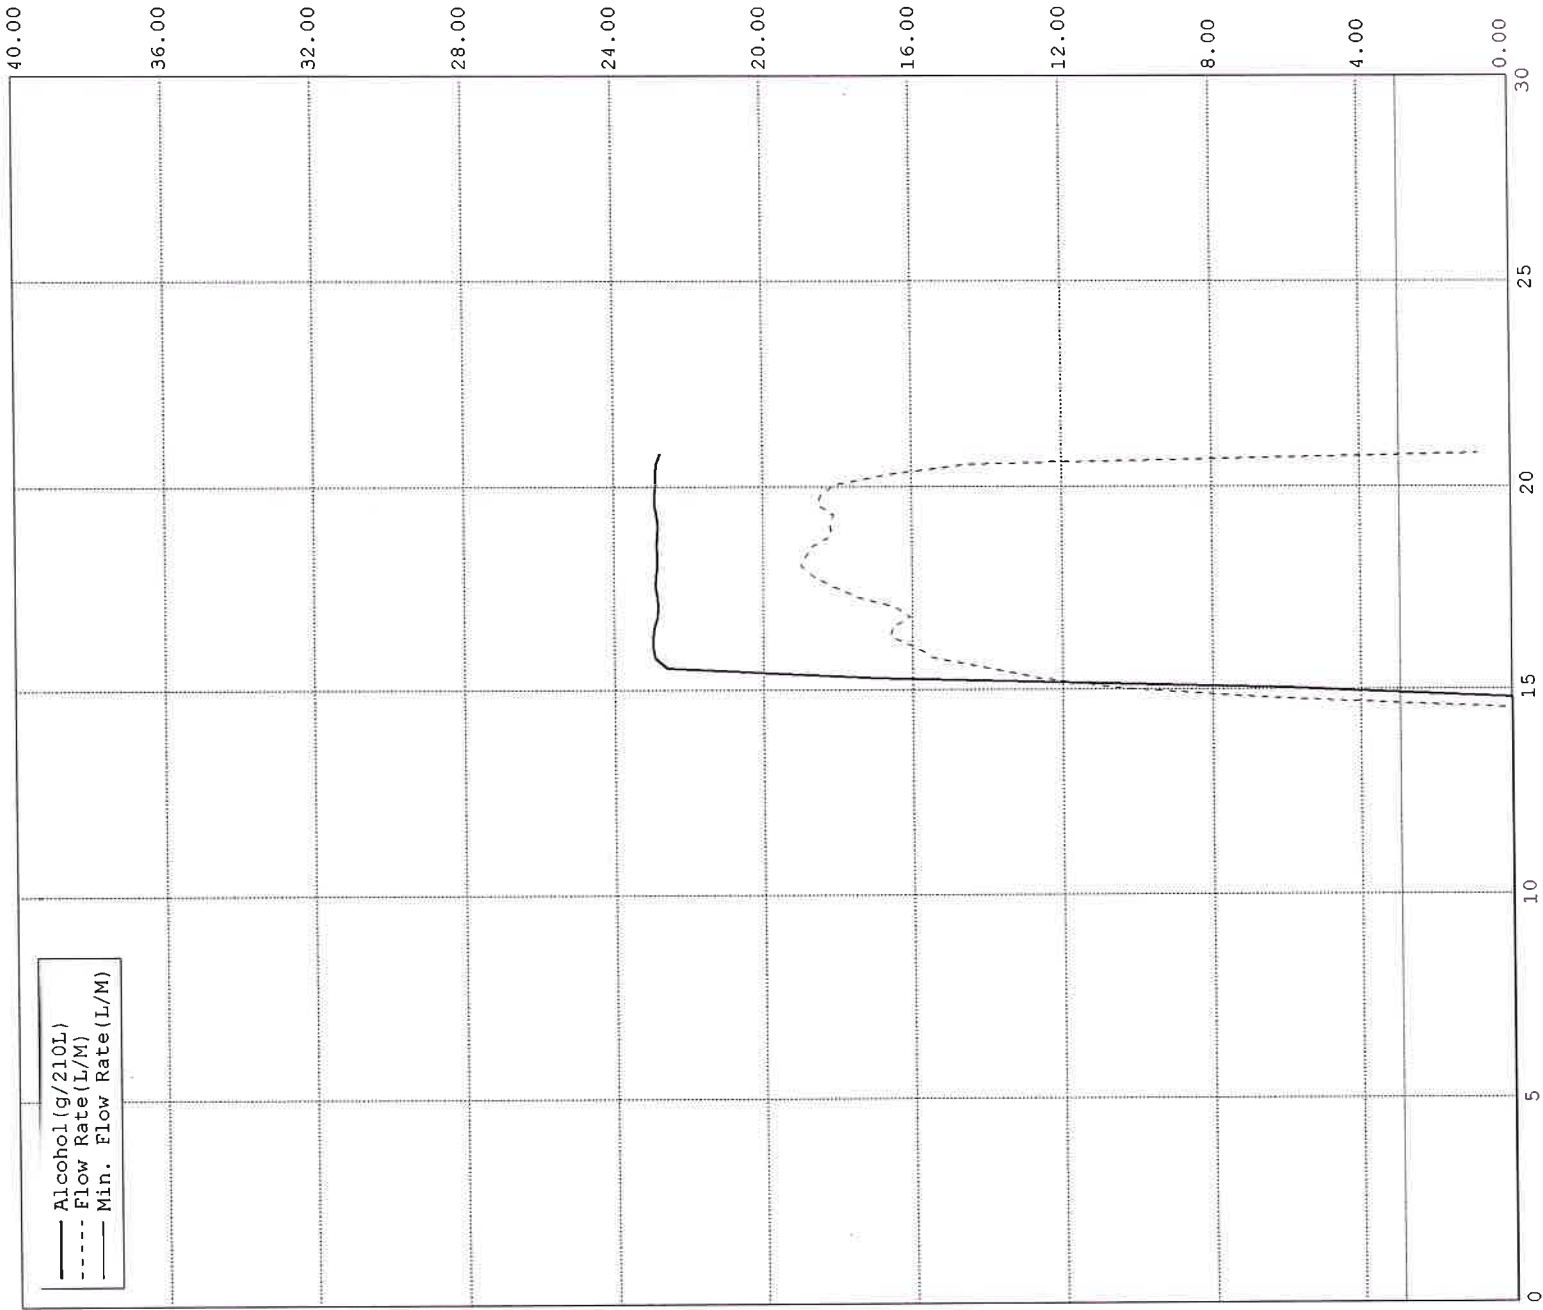

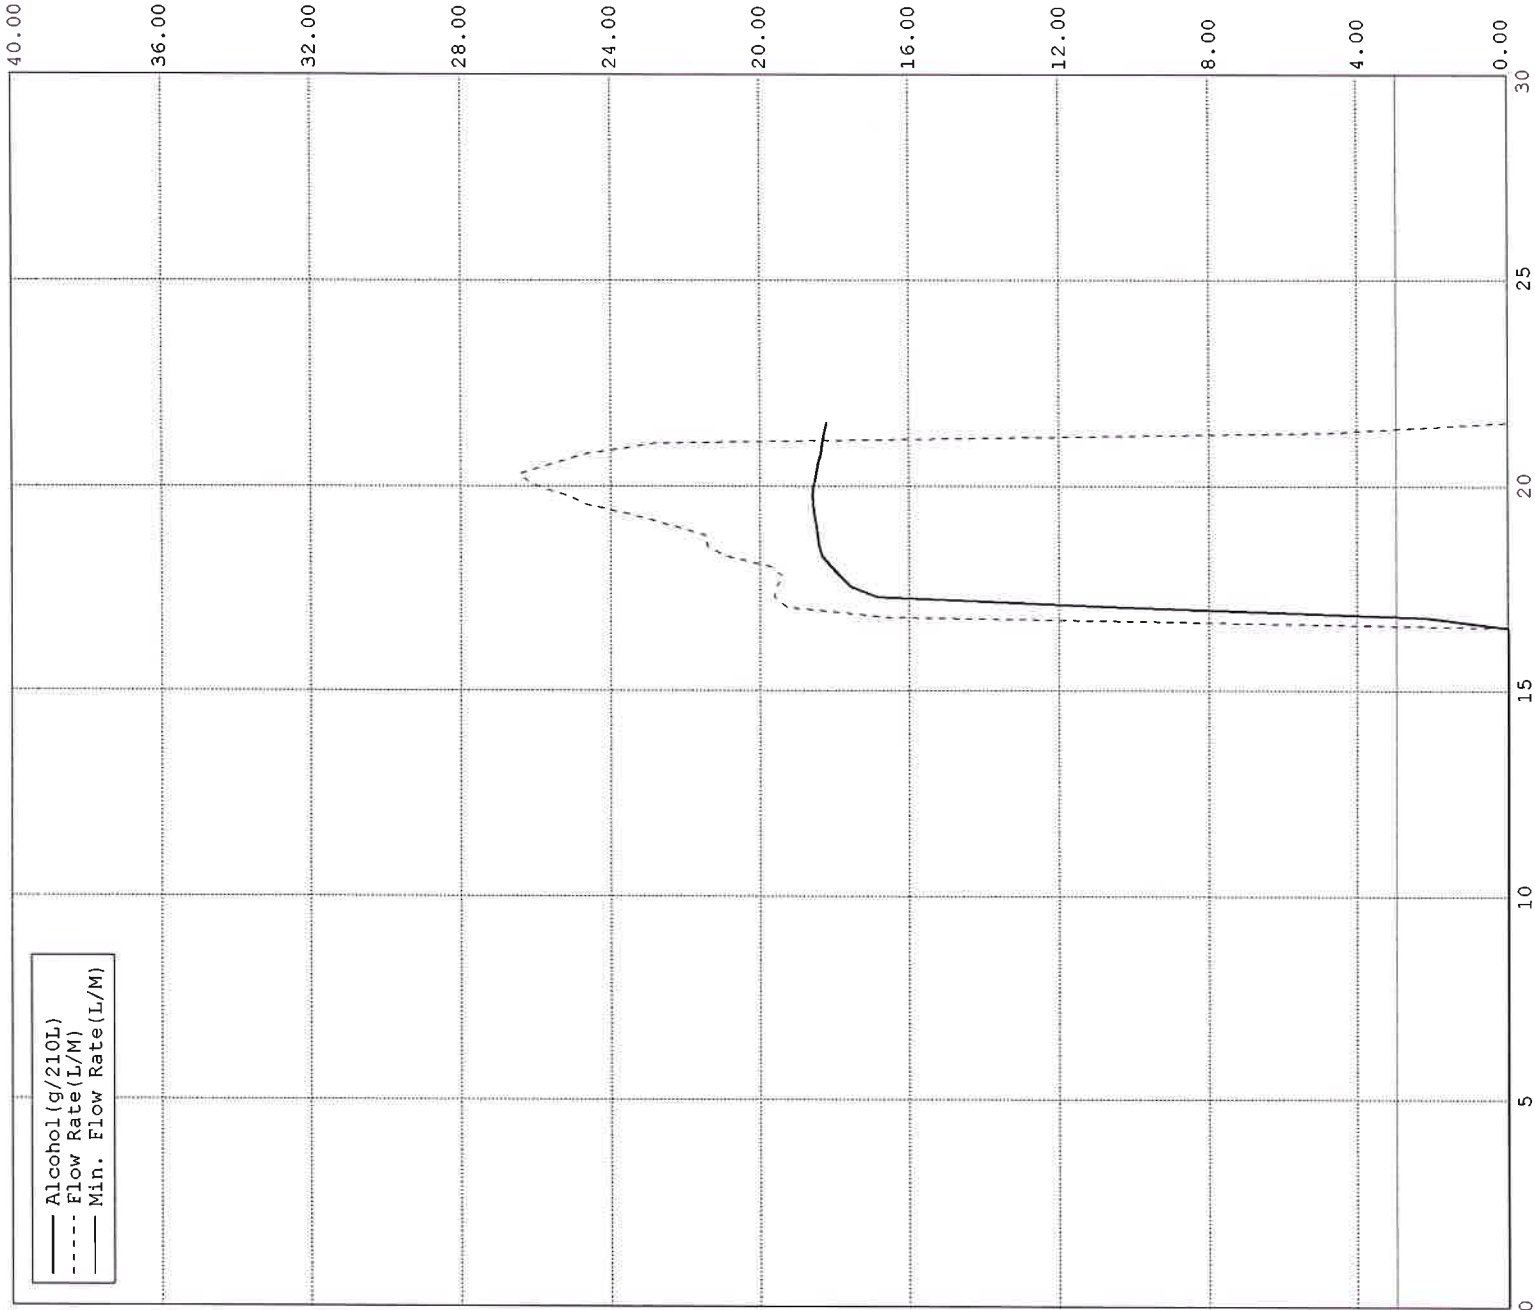

SUBJECT TEST

 Alaska Department of Public Safety
 DATAMASTER dmt: 100699

 Date: 05/30/2024
 Time: 14:28:13

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 MEGAN CROUSE
 OPERATOR'S #: 10747

DEPT/AGENCY:
 INTERFERENCE - NEGATIVE
 CASE/REPORT: XXX
 TEST TYPE: TEST

100699

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.74: 0.080
 LOT #: AG335202
 EXPIRATION: 12/18/2025

2024.05.30 Calibration

DIAGNOSTIC CHECK	PASSED	14:29
BLANK TEST	0.000	14:29
INTERNAL STANDARD	VERIFIED	14:29
Xq = 0.078 (1.12%)		
EXTERNAL STANDARD	0.079	14:29
X[1] = 0.0788 (-0.0005) (0.0019)		
BLANK TEST	0.000	14:30
SUBJECT SAMPLE (Vol=1.69L)	0.091	14:31
X[1] = 0.0916 (0.0016) (0.0017)		
BLANK TEST	0.000	14:32
EXTERNAL STANDARD	0.079	14:32
X[1] = 0.0788 (-0.0017) (0.0009)		
BLANK TEST	0.000	14:33

Page 21 of 22

MNC

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100699

Date: 05/30/2024

Time: 14:46:43

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CROUSE

OPERATOR'S #: 10747

DEPT/AGENCY:

NON-DRINKING SUBJECT TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.74: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:47
BLANK TEST	0.000	14:47
INTERNAL STANDARD	VERIFIED	14:48
EXTERNAL STANDARD	0.079	14:48
BLANK TEST	0.000	14:49
SUBJECT SAMPLE (Vol=2.60L)	0.000	14:49
BLANK TEST	0.000	14:50
EXTERNAL STANDARD	0.080	14:50
BLANK TEST	0.000	14:51

MNC

