

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument
State of Alaska

Serial #: 100365

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 02/20/2016

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.94: 0.077
LOT #: 09214080A2
EXPIRATION: 05/01/2016
TANK PRESSURE: 796 psi

BLANK TEST	0.000	02:24
INTERNAL STANDARD	VERIFIED	02:24
EXTERNAL STANDARD	0.075	02:24
BLANK TEST	0.000	02:25
EXTERNAL STANDARD	0.076	02:25
BLANK TEST	0.000	02:26
EXTERNAL STANDARD	0.076	02:26
BLANK TEST	0.000	02:27
EXTERNAL STANDARD	0.076	02:27
BLANK TEST	0.000	02:28
EXTERNAL STANDARD	0.075	02:29
BLANK TEST	0.000	02:29

Average = 0.0756
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
Breath Tube = 43.9°C PASSED

PUMP INFO

Flow Rate = 4.277 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO


Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

I, Charles R. Foster, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist III at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Acting Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Charles R. Foster
Acting Scientific Director
State Breath Alcohol Program

3/2/16

Subscribed and sworn before me this 2nd day of Mar, 20 16


Nikki Roth, Notary Public
My Commission Expires With Office

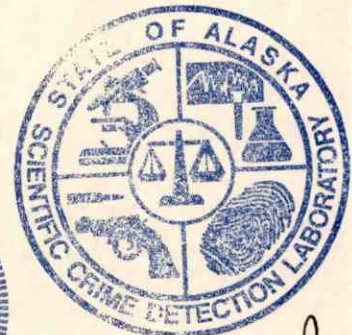

BMB
2/24/16