



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100362

Report Issue Date: 09/04/2024
Date Received: 2024-01-09
Condition of Item: Good

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG217902	0.020	0.020	0.019	0.020	0.020	0.020
0.080	0.079	AG310901	0.077	0.078	0.078	0.077	0.078	0.078
0.300	0.296	AG327804	0.295	0.294	0.294	0.295	0.295	0.295

As Found - Evaluation Analyst: Carlie Glaister
 As Found Conditions - Barometric Pressure (inHg): 29.54 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.7 Relative Humidity (%): 12
 As-Found Lab Activity Date Range: 01/09/2024 - 01/09/2024

Replaced o-ring.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.078	AG335202	0.077	0.077	0.077	0.077	0.078	0.077	+/- 0.004
0.100	0.098	AG333401	0.098	0.098	0.098	0.098	0.098	0.098	+/- 0.004
0.150	0.147	AG332004	0.145	0.144	0.145	0.145	0.145	0.145	+/- 0.006
0.300	0.294	AG327804	0.293	0.293	0.293	0.292	0.292	0.293	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.32 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.3 Relative Humidity (%): 50
 As-Left Lab Activity Date Range: 07/30/2024 - 07/30/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Megan Carlock

Results authorized by Megan Carlock on 09/03/2024

megan.crouse@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 09/04/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100362 Analyst or Technician Name: Megan Carlock

DataMaster DMT Calibration Start Date: 7/30/24

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: 5/2/2025
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.4 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.32 Temperature(C) 21.3 Relative Humidity(%) 50
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20240501KS Expiration Date: 8/1/2024
Simulator S/N: SD1088 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240501MVC Expiration Date: 8/1/2024
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 224P41201 Expiration Date: 8/1/2024 8/24/2024
Simulator S/N: SD1177 Thermometer Verification Performed? MVC 9/3/24

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 9/19/2025

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 7/30/24
Data Interpretation Date (Technician): N/A (if applicable)
Data Interpretation Date (Analyst): 7/30/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100362

Date: 07/30/2024
Time: 11:24:56

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 45.5°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.74 V PASSED
(1.10 V - 2.56 V)
Cooler Voltage = 1.76 V PASSED
(0.97 V - 2.25 V)
Bias Voltage = 78 V PASSED
(47 V - 111 V)
Chopper Freq = 524 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.4 in

PUMP INFO

Flow Rate = 5.300 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.073 0.60% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100362

Date: 07/30/2024
Time: 11:37 AM

Temperatures (°C)
Sample Cell: 48.9°C
Breath Tube: 46.2°C

Current Barometer 29.3 in
Volume (Ltr) 1.55

Settings
Lamp: 1.79 V
Bias: 78 V
Cooler: 1.76 V
Chopper: 524 Hz

Voltages (V)
Flow: 1.03 V
Detector: 0.046 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100362

Date: 03/15/2011
Time: 07:01:28

OPERATOR NAME:
COLLEEN S OBRYANT
CERTIFICATE #: 6237

LOT #: GUTH100
BOTTLE #: 9380
EXPIRATION: 12/17/2011

Ca = 0.1000
CAL = 0.977426 0.800 <= CAL < 1.200
b1 = 0.0004 0.0000 <= b1 < 0.0040
b2 = 0.0058 0.0010 <= b2 < 0.0100
b3 = 0.0000 0.0000 <= b3 < 0.0040
Xq = 0.0727 0.0500 <= Xq < 0.2000
a21 = 1.161401 1.050 <= a21 < 1.300
a31 = 0.532998 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100362

Date: 07/30/2024

Time: 11:39:07

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080

TARGET AT 29.33: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	TIME
BLANK TEST	0.000	11:40
INTERNAL STANDARD	VERIFIED	11:40
EXTERNAL STANDARD	0.077	11:40
BLANK TEST	0.000	11:41
SUBJECT SAMPLE (Vol=1.66L)	0.000	11:42
BLANK TEST	0.000	11:43
EXTERNAL STANDARD	0.078	11:43
BLANK TEST	0.000	11:44

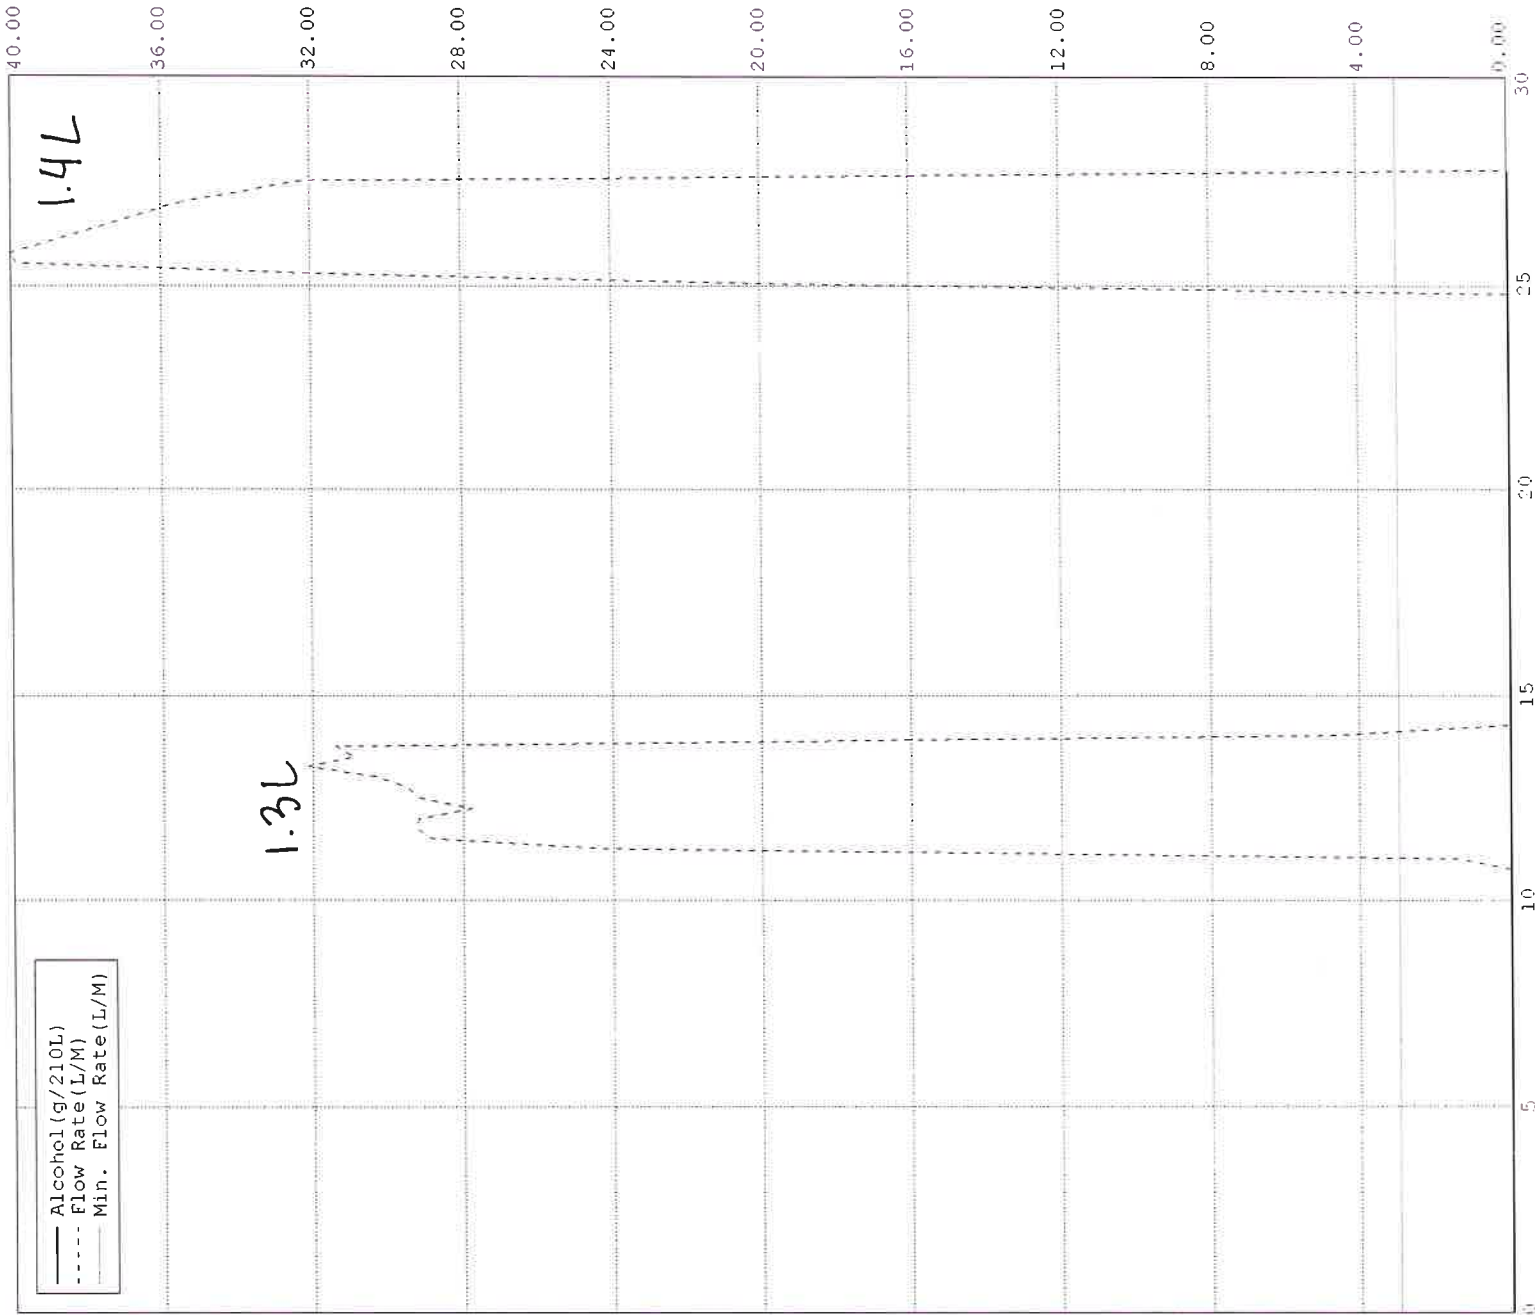

MNC

LINEARITY CHECK

Alaska Department of Public Safety

DATAMASTER dmt: 100362

Date: 07/30/2024

Time: 11:46:49


SUPERVISOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.039	0.0390	0.0000
0.078	0.0772	0.0004
0.098	0.0980	0.0000
0.147	0.1448	0.0004
0.294	0.2926	0.0005

SLOPE = 0.993905
R² = 0.999951

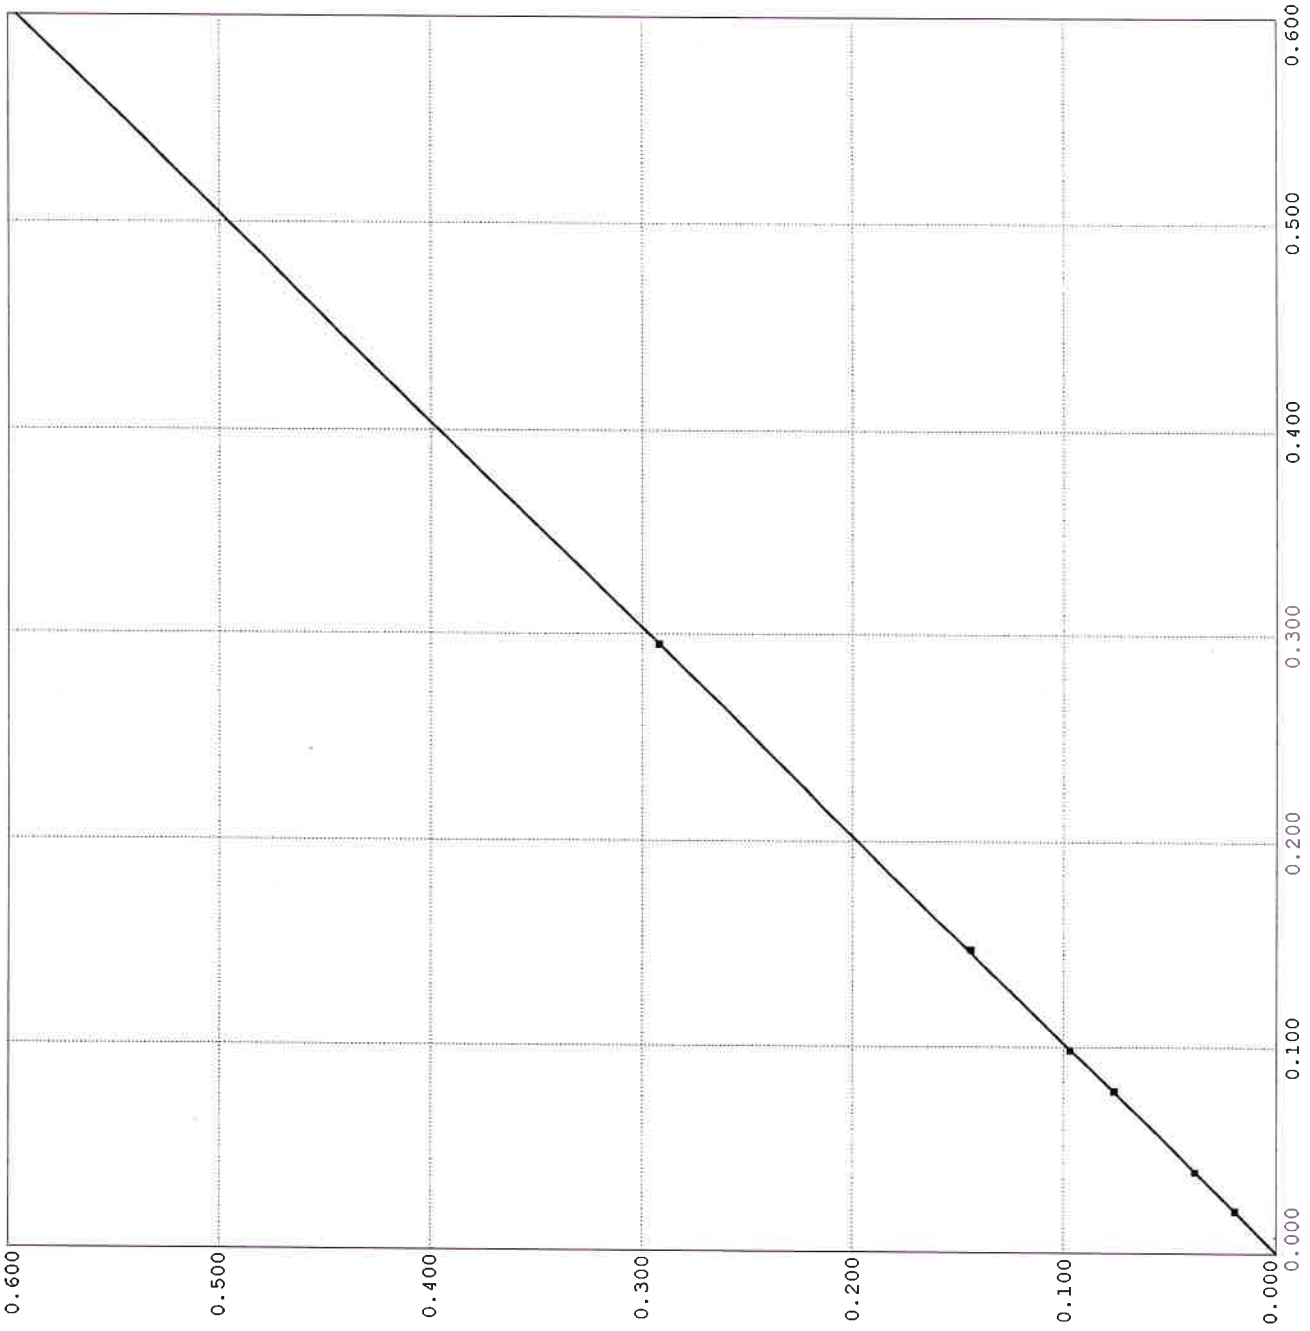

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100362






Date: 07/30/2024
Time: 11:46:51

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.33: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 932 psi

BLANK TEST	0.000	11:48
INTERNAL STANDARD	VERIFIED	11:48
EXTERNAL STANDARD	0.020	11:48
BLANK TEST	0.000	11:49
EXTERNAL STANDARD	0.020	11:49
BLANK TEST	0.000	11:50
EXTERNAL STANDARD	0.020	11:50
BLANK TEST	0.000	11:51
EXTERNAL STANDARD	0.020	11:51
BLANK TEST	0.000	11:52
EXTERNAL STANDARD	0.020	11:52
BLANK TEST	0.000	11:53

Average = 0.0200
Std Dev = 0.0000

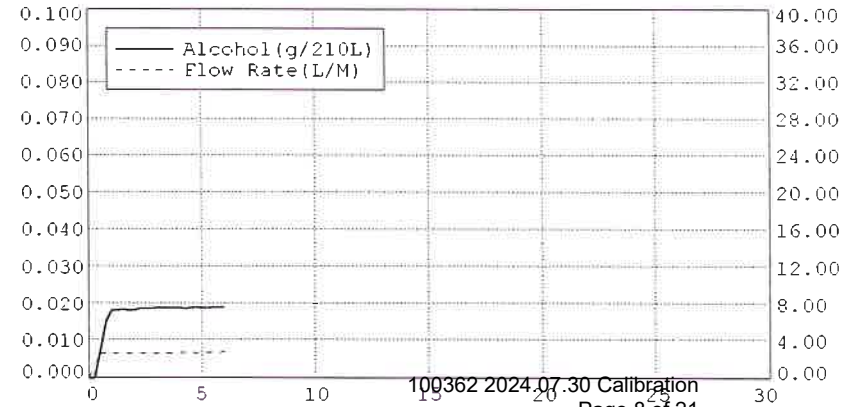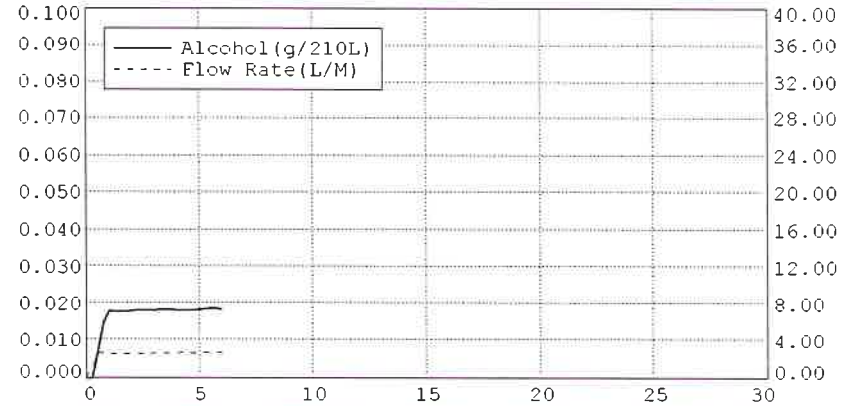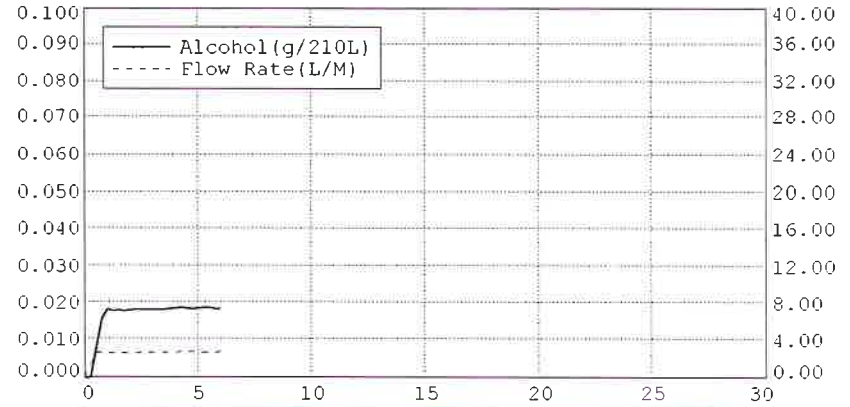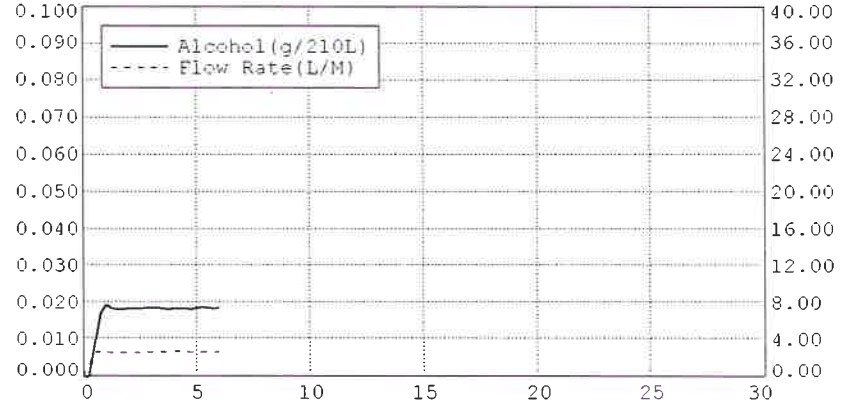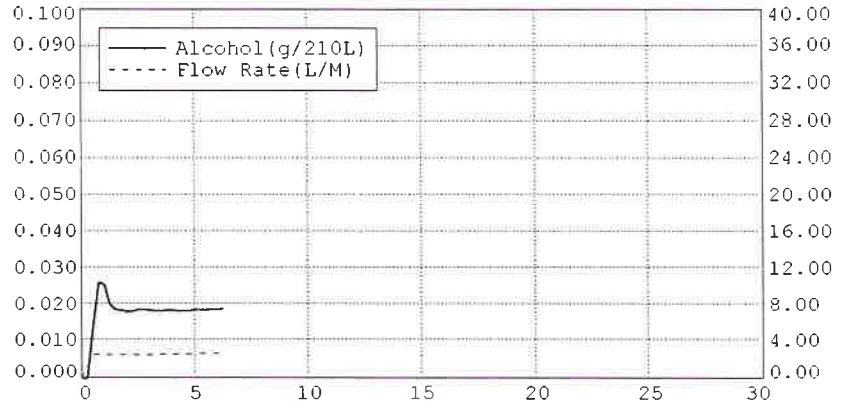

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100362






Date: 07/30/2024
 Time: 11:54:26

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.33: 0.039
 LOT #: AG407908
 EXPIRATION: 03/19/2026
 TANK PRESSURE: 1114 psi

BLANK TEST	0.000	11:55
INTERNAL STANDARD	VERIFIED	11:55
EXTERNAL STANDARD	0.039	11:56
BLANK TEST	0.000	11:57
EXTERNAL STANDARD	0.039	11:57
BLANK TEST	0.000	11:58
EXTERNAL STANDARD	0.039	11:58
BLANK TEST	0.000	11:59
EXTERNAL STANDARD	0.039	11:59
BLANK TEST	0.000	12:00
EXTERNAL STANDARD	0.039	12:00
BLANK TEST	0.000	12:01

Average = 0.0390
 Std Dev = 0.0000

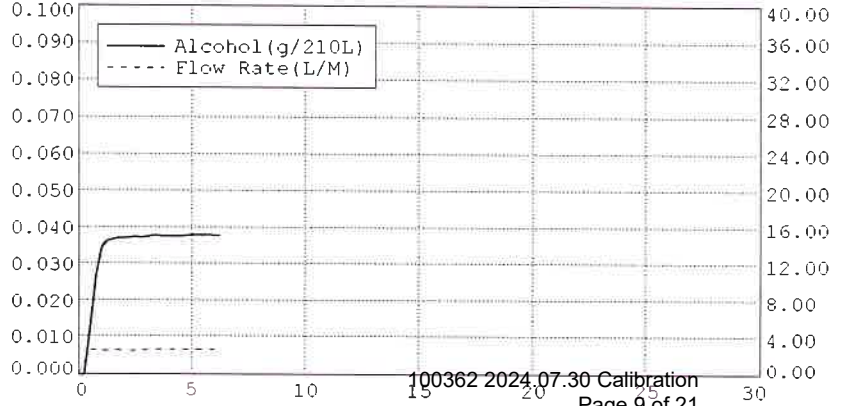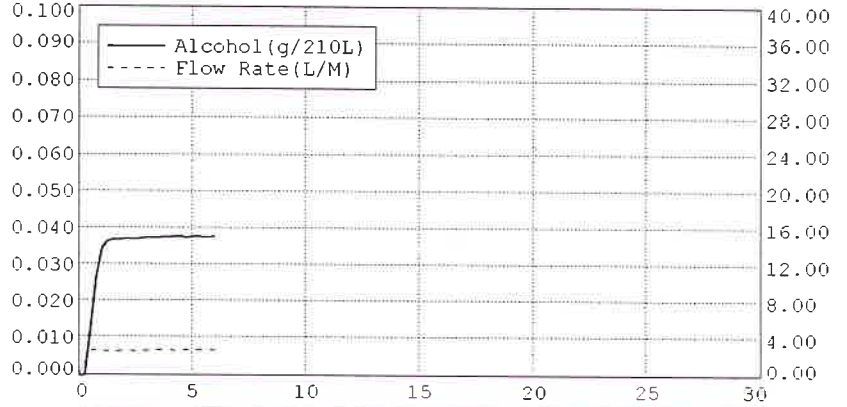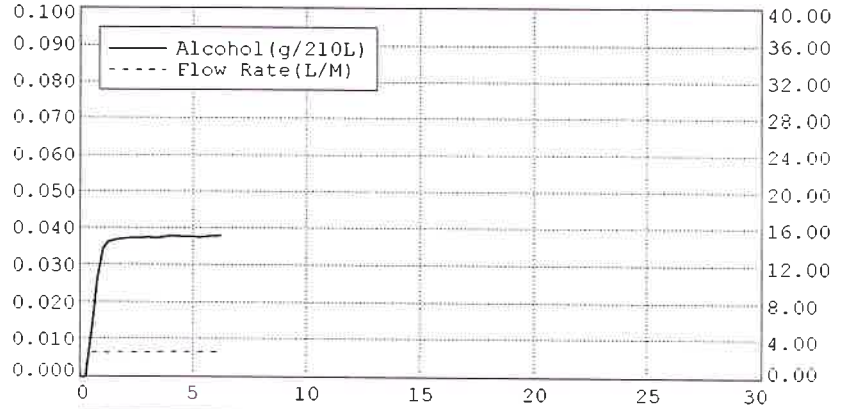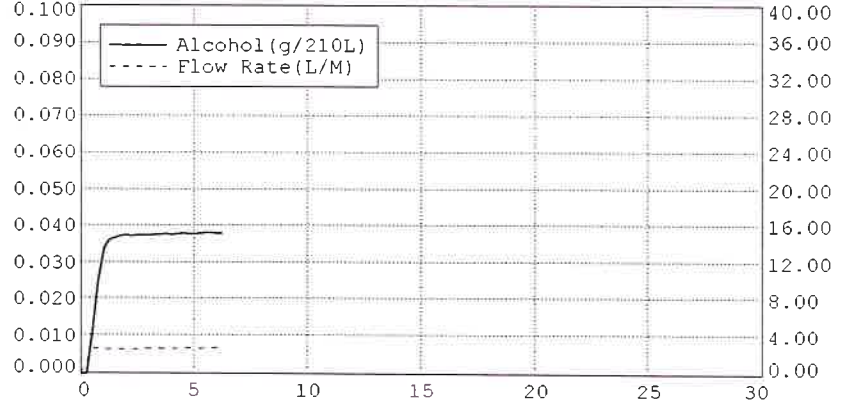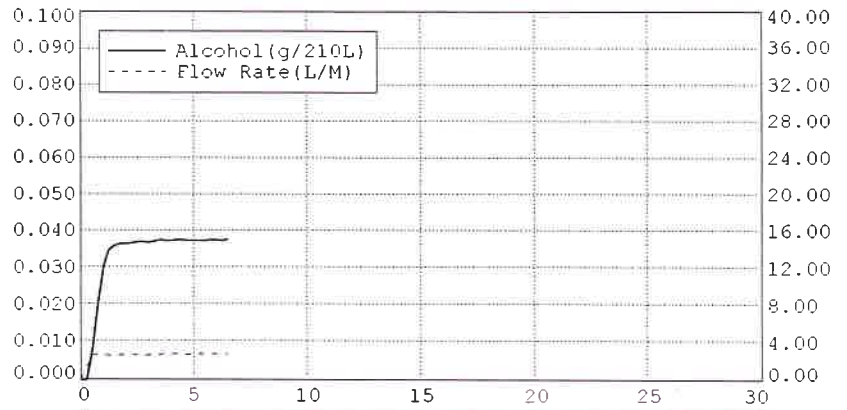

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100362






Date: 07/30/2024
Time: 12:33:07

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.34: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 870 psi

BLANK TEST	0.000	12:34
INTERNAL STANDARD	VERIFIED	12:34
EXTERNAL STANDARD	0.077	12:34
BLANK TEST	0.000	12:35
EXTERNAL STANDARD	0.077	12:35
BLANK TEST	0.000	12:36
EXTERNAL STANDARD	0.077	12:36
BLANK TEST	0.000	12:37
EXTERNAL STANDARD	0.077	12:37
BLANK TEST	0.000	12:38
EXTERNAL STANDARD	0.078	12:38
BLANK TEST	0.000	12:39

Average = 0.0772
Std Dev = 0.0004

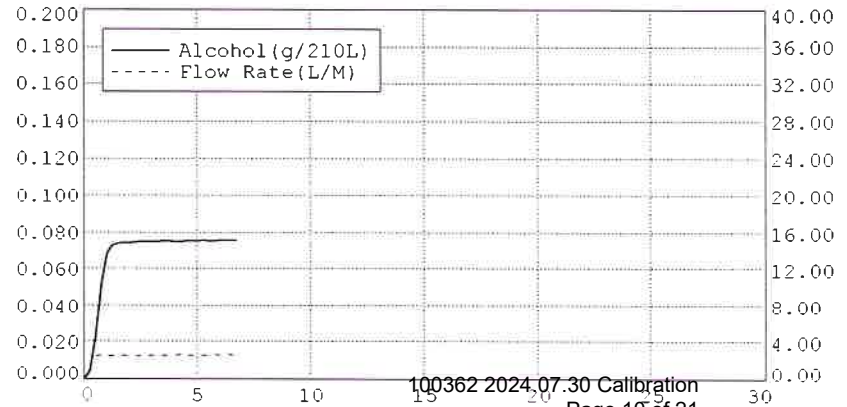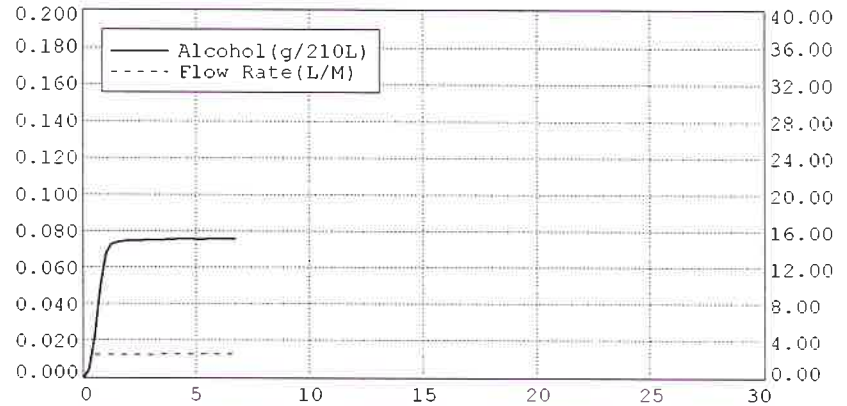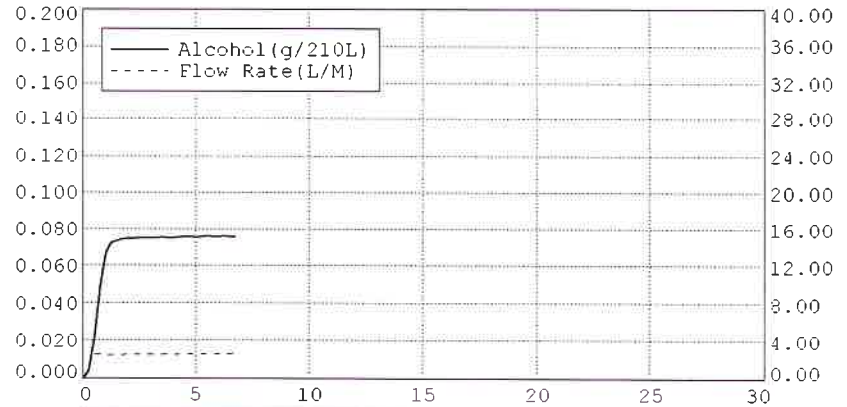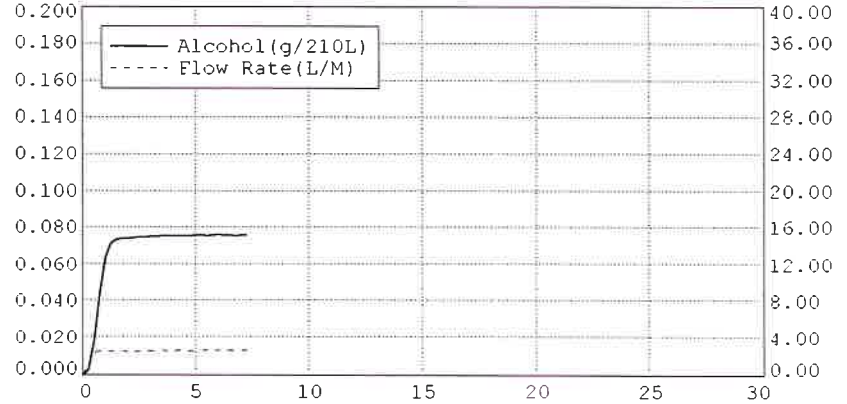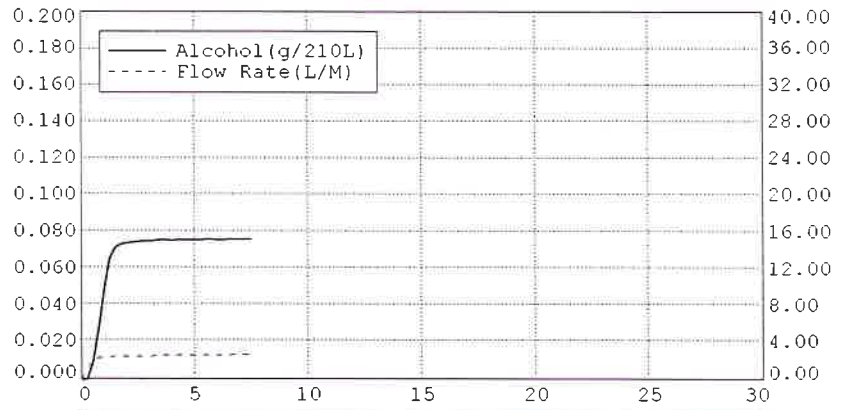

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100362






Date: 07/30/2024
Time: 12:47:20

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.33: 0.098
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 829 psi

BLANK TEST	0.000	12:48
INTERNAL STANDARD	VERIFIED	12:48
EXTERNAL STANDARD	0.098	12:49
BLANK TEST	0.000	12:50
EXTERNAL STANDARD	0.098	12:50
BLANK TEST	0.000	12:51
EXTERNAL STANDARD	0.098	12:51
BLANK TEST	0.000	12:52
EXTERNAL STANDARD	0.098	12:52
BLANK TEST	0.000	12:53
EXTERNAL STANDARD	0.098	12:53
BLANK TEST	0.000	12:54

Average = 0.0980
Std Dev = 0.0000

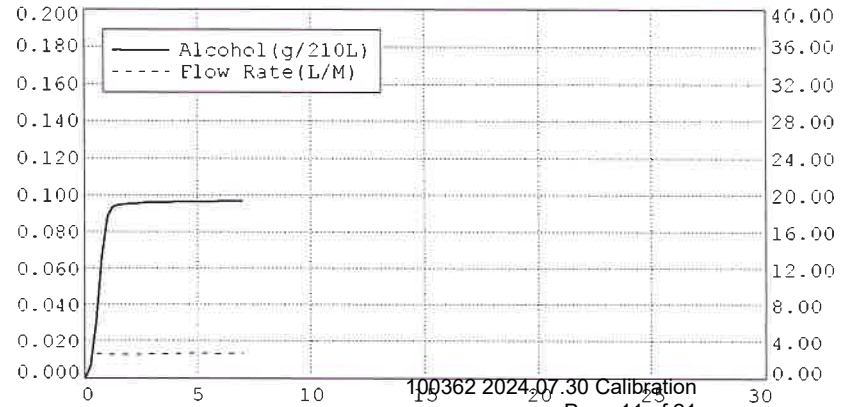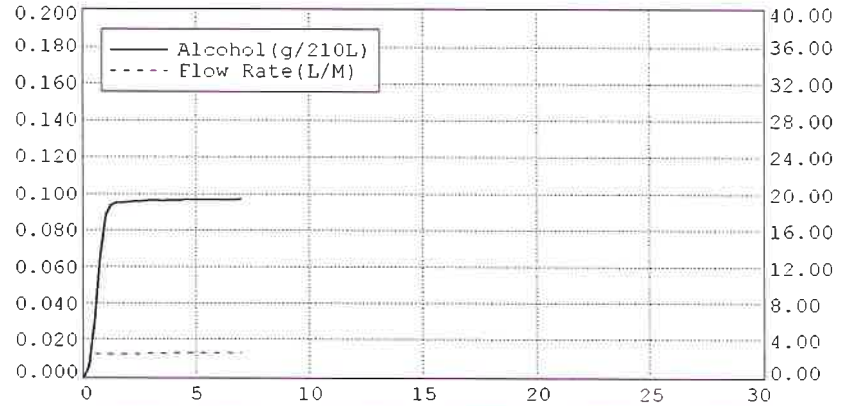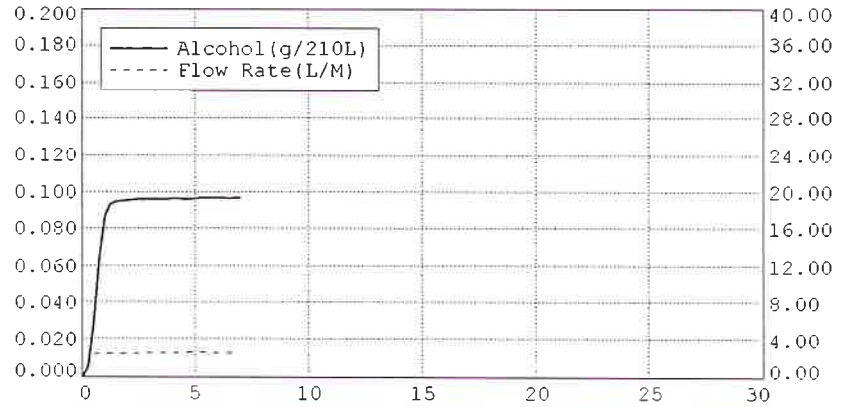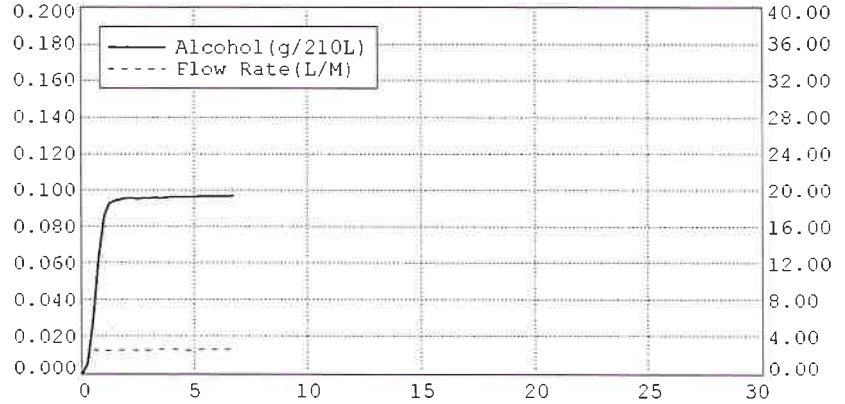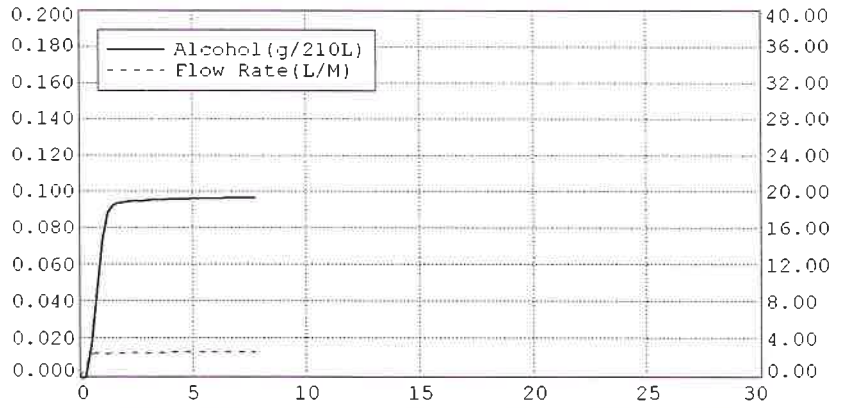

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100362






Date: 07/30/2024
 Time: 12:54:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.35: 0.147
 LOT #: AG332004
 EXPIRATION: 11/16/2025
 TANK PRESSURE: 447 psi

BLANK TEST	0.000	12:56
INTERNAL STANDARD	VERIFIED	12:56
EXTERNAL STANDARD	0.145	12:56
BLANK TEST	0.000	12:57
EXTERNAL STANDARD	0.144	12:57
BLANK TEST	0.000	12:58
EXTERNAL STANDARD	0.145	12:58
BLANK TEST	0.000	12:59
EXTERNAL STANDARD	0.145	12:59
BLANK TEST	0.000	13:00
EXTERNAL STANDARD	0.145	13:01
BLANK TEST	0.000	13:01

Average = 0.1448
 Std Dev = 0.0004

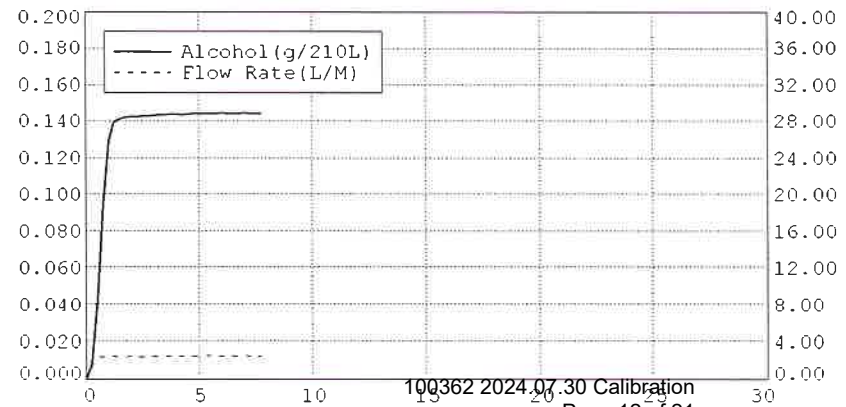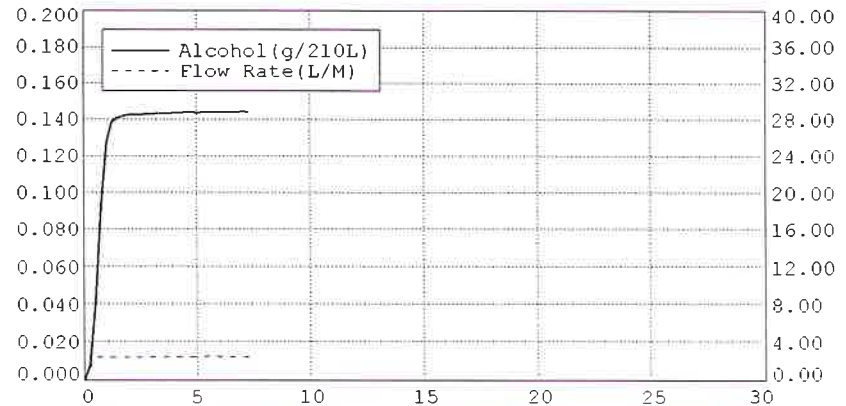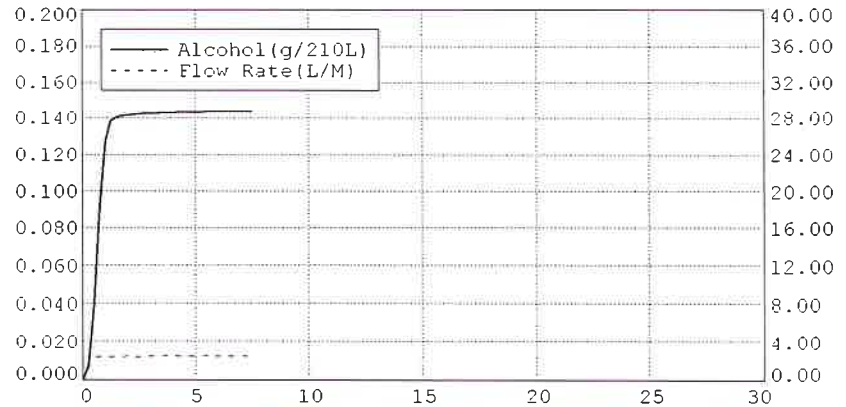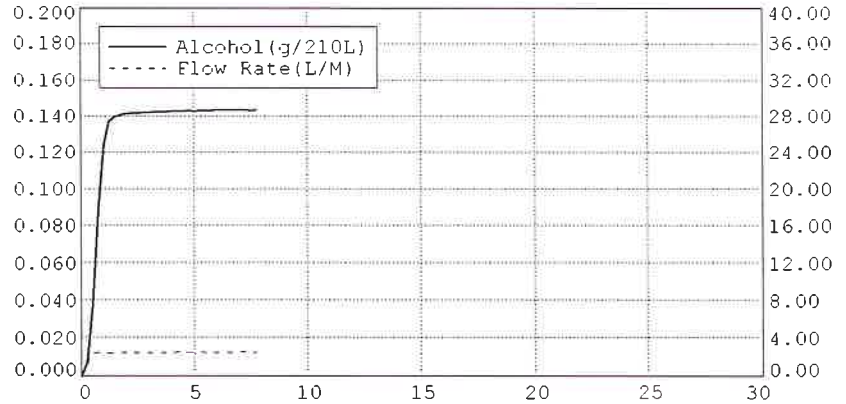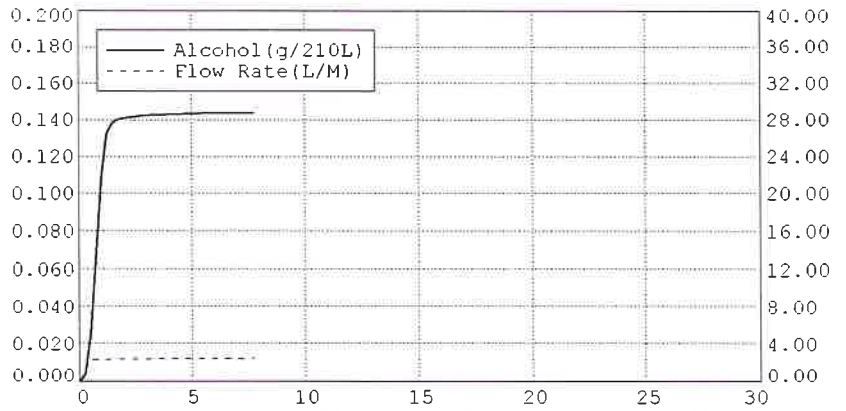

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100362






Date: 07/30/2024
Time: 13:02:35

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.35: 0.294
LOT #: AG327804
EXPIRATION: 10/05/2025
TANK PRESSURE: 246 psi

BLANK TEST	0.000	13:03
INTERNAL STANDARD	VERIFIED	13:04
EXTERNAL STANDARD	0.293	13:04
BLANK TEST	0.000	13:05
EXTERNAL STANDARD	0.293	13:05
BLANK TEST	0.000	13:06
EXTERNAL STANDARD	0.293	13:06
BLANK TEST	0.000	13:07
EXTERNAL STANDARD	0.292	13:07
BLANK TEST	0.000	13:08
EXTERNAL STANDARD	0.292	13:09
BLANK TEST	0.000	13:09

Average = 0.2926
Std Dev = 0.0005

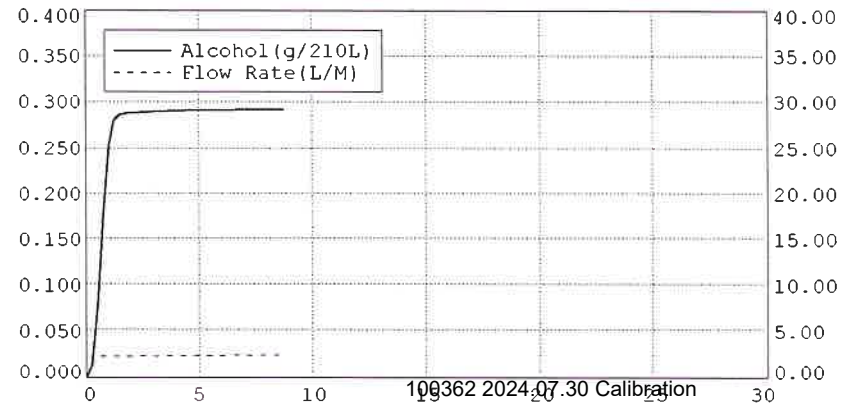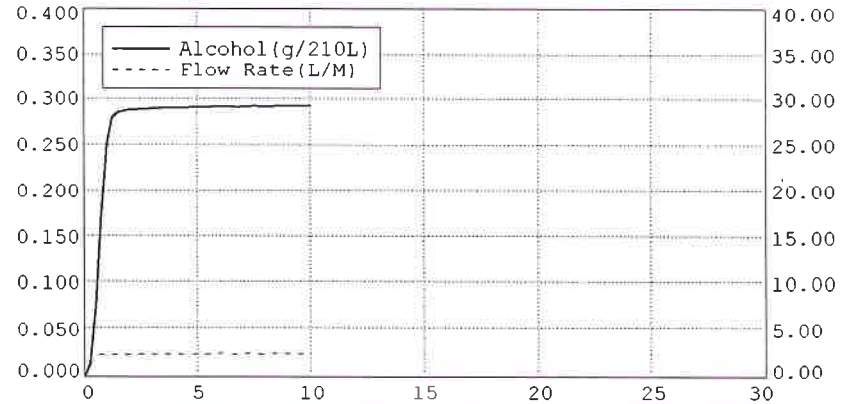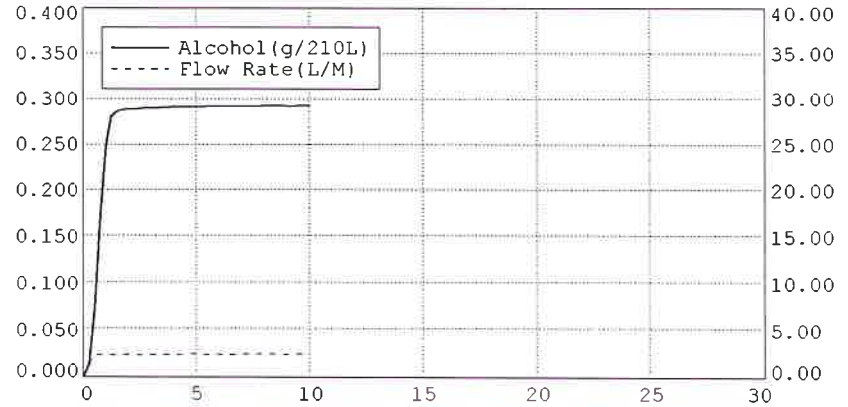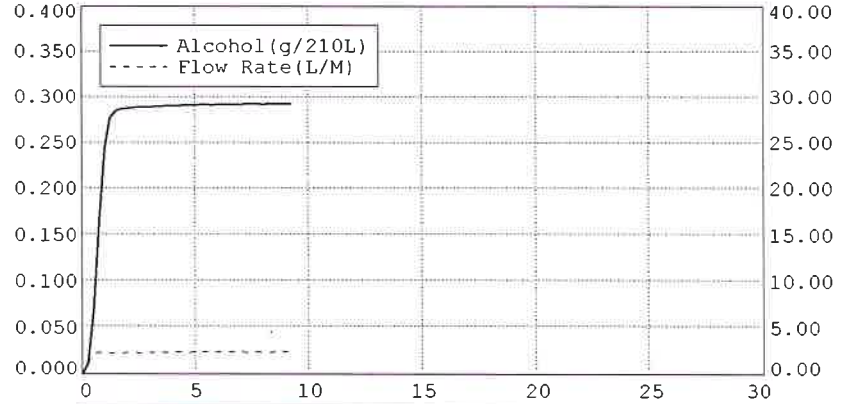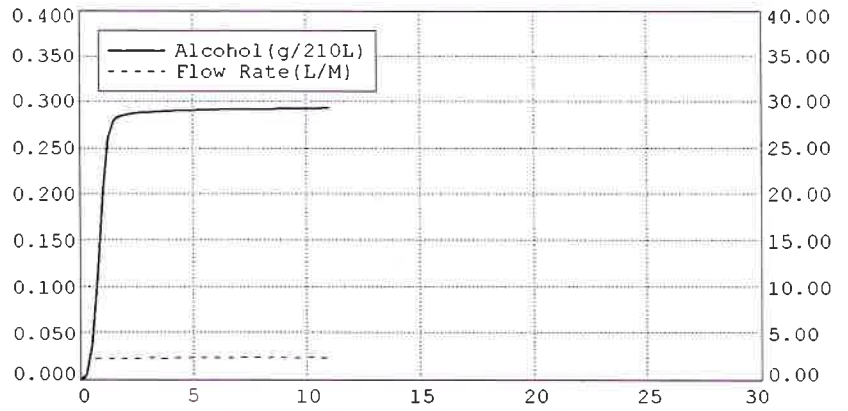

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100362

Date: 07/30/2024
Time: 13:15:34

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.35: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:16
BLANK TEST 0.000 13:16
INTERNAL STANDARD VERIFIED 13:16
EXTERNAL STANDARD 0.078 13:17
BLANK TEST 0.000 13:17
SUBJECT SAMPLE INCOMPLETE 13:20

MNC

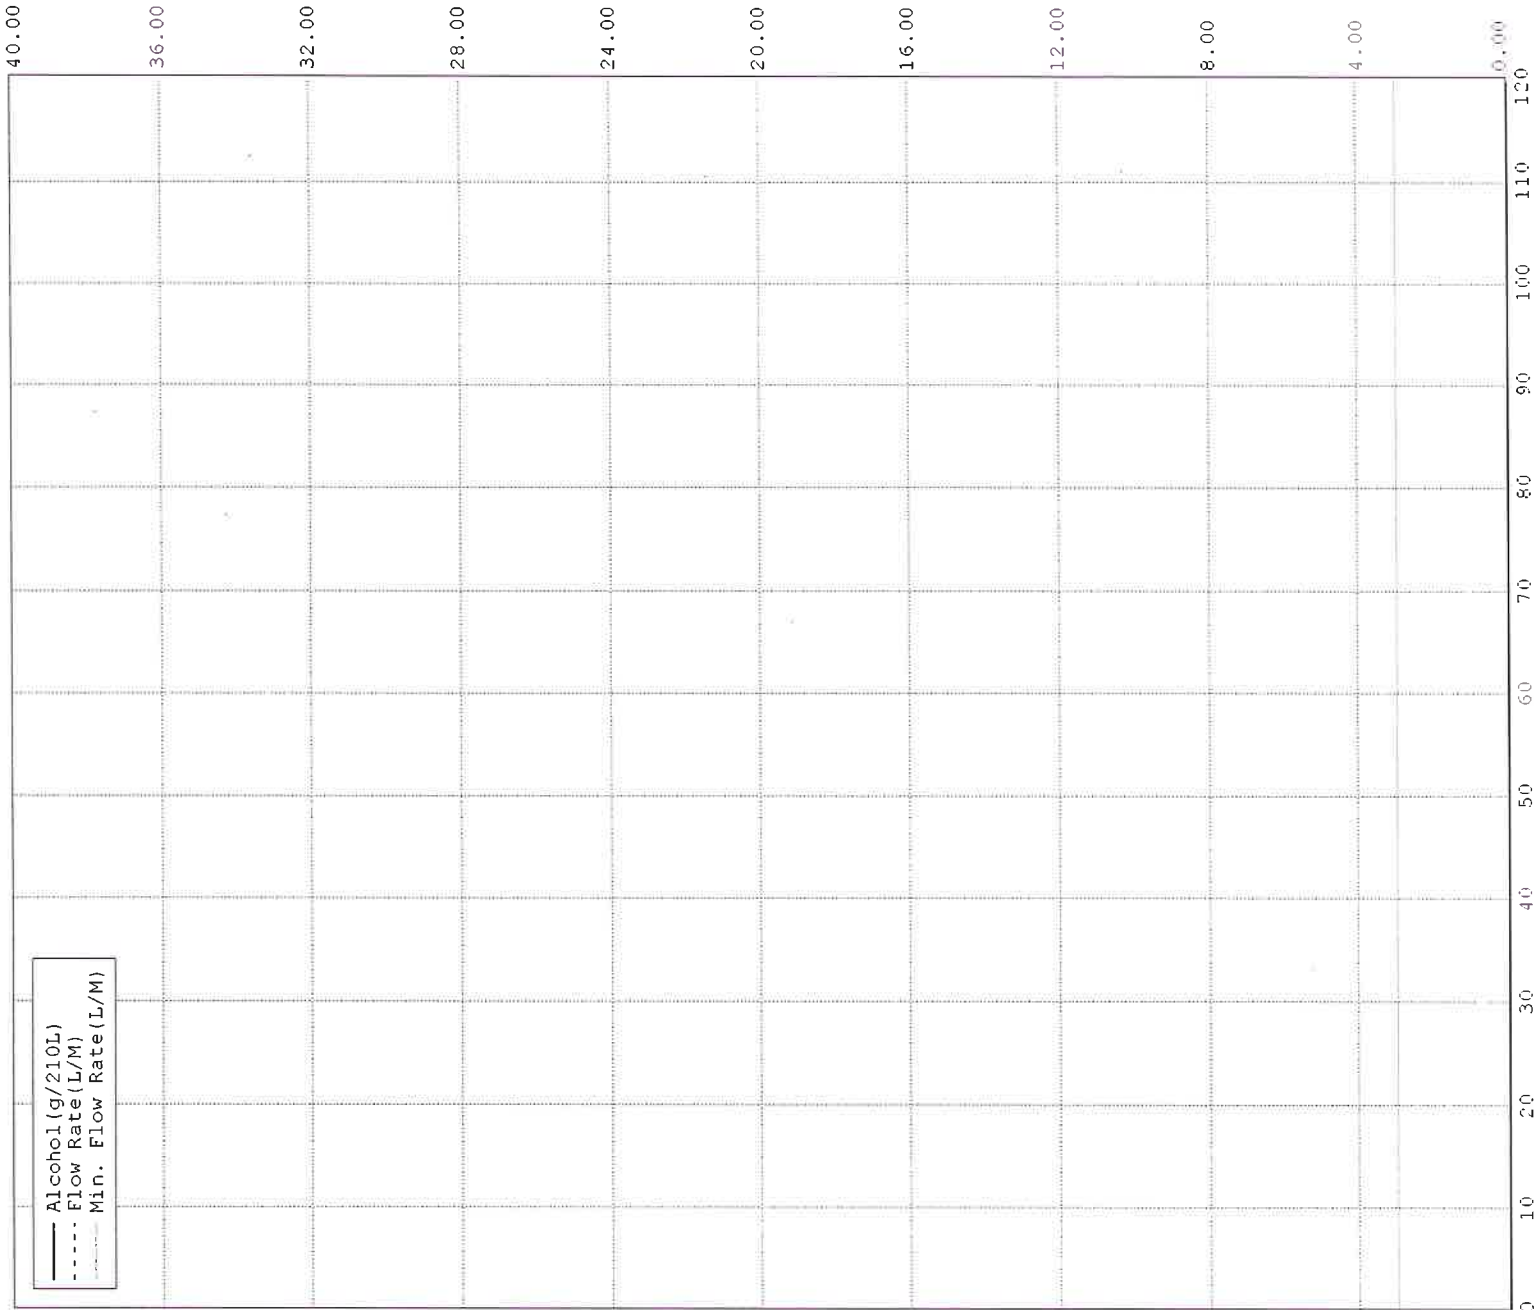

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100362

Date: 07/30/2024
Time: 13:28:03

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.35: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:29
BLANK TEST 0.000 13:29
INTERNAL STANDARD VERIFIED 13:29
EXTERNAL STANDARD 0.077 13:29
BLANK TEST 0.000 13:30
SUBJECT SAMPLE XXX 13:30

Maximum Attempts Exceeded

MNC

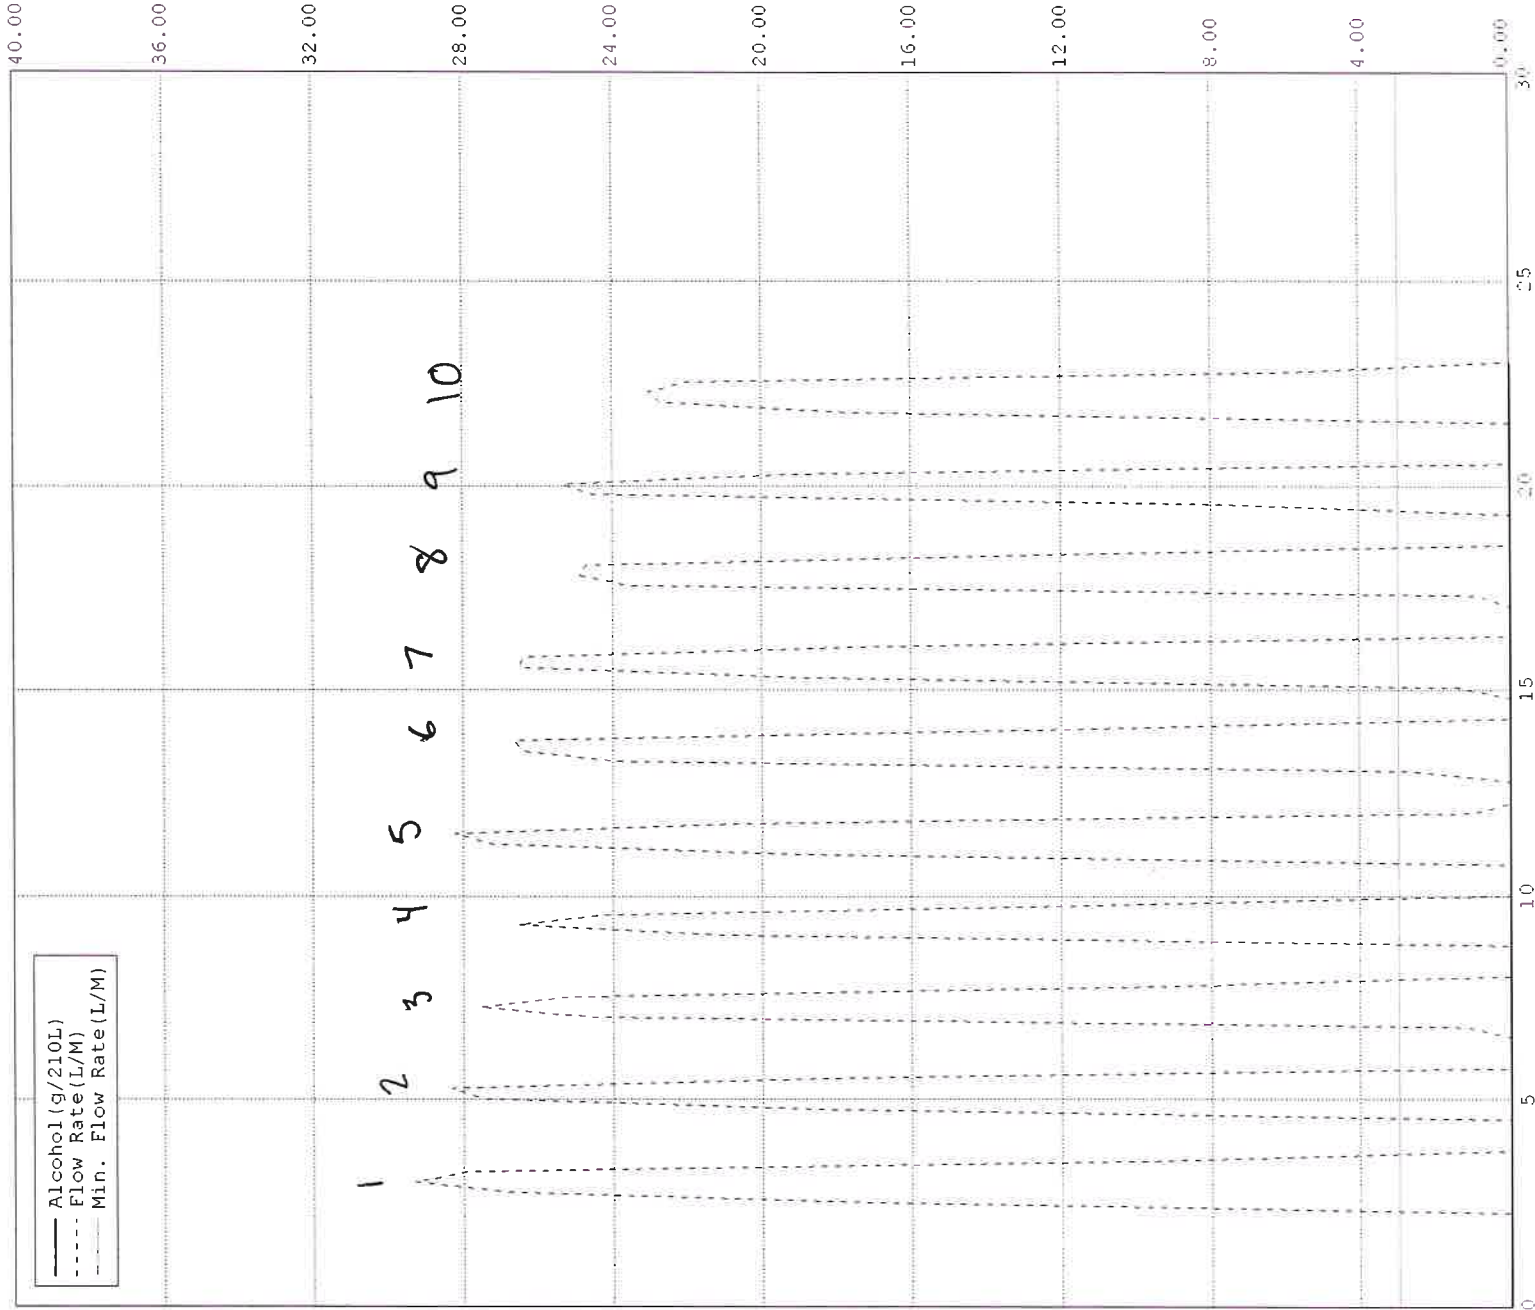

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100362

Date: 07/30/2024
Time: 13:32:25

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.35: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:33
BLANK TEST	0.000	13:33
INTERNAL STANDARD	VERIFIED	13:33
EXTERNAL STANDARD	0.077	13:33
BLANK TEST	0.000	13:34
SUBJECT SAMPLE	INVALID	13:35

MNC

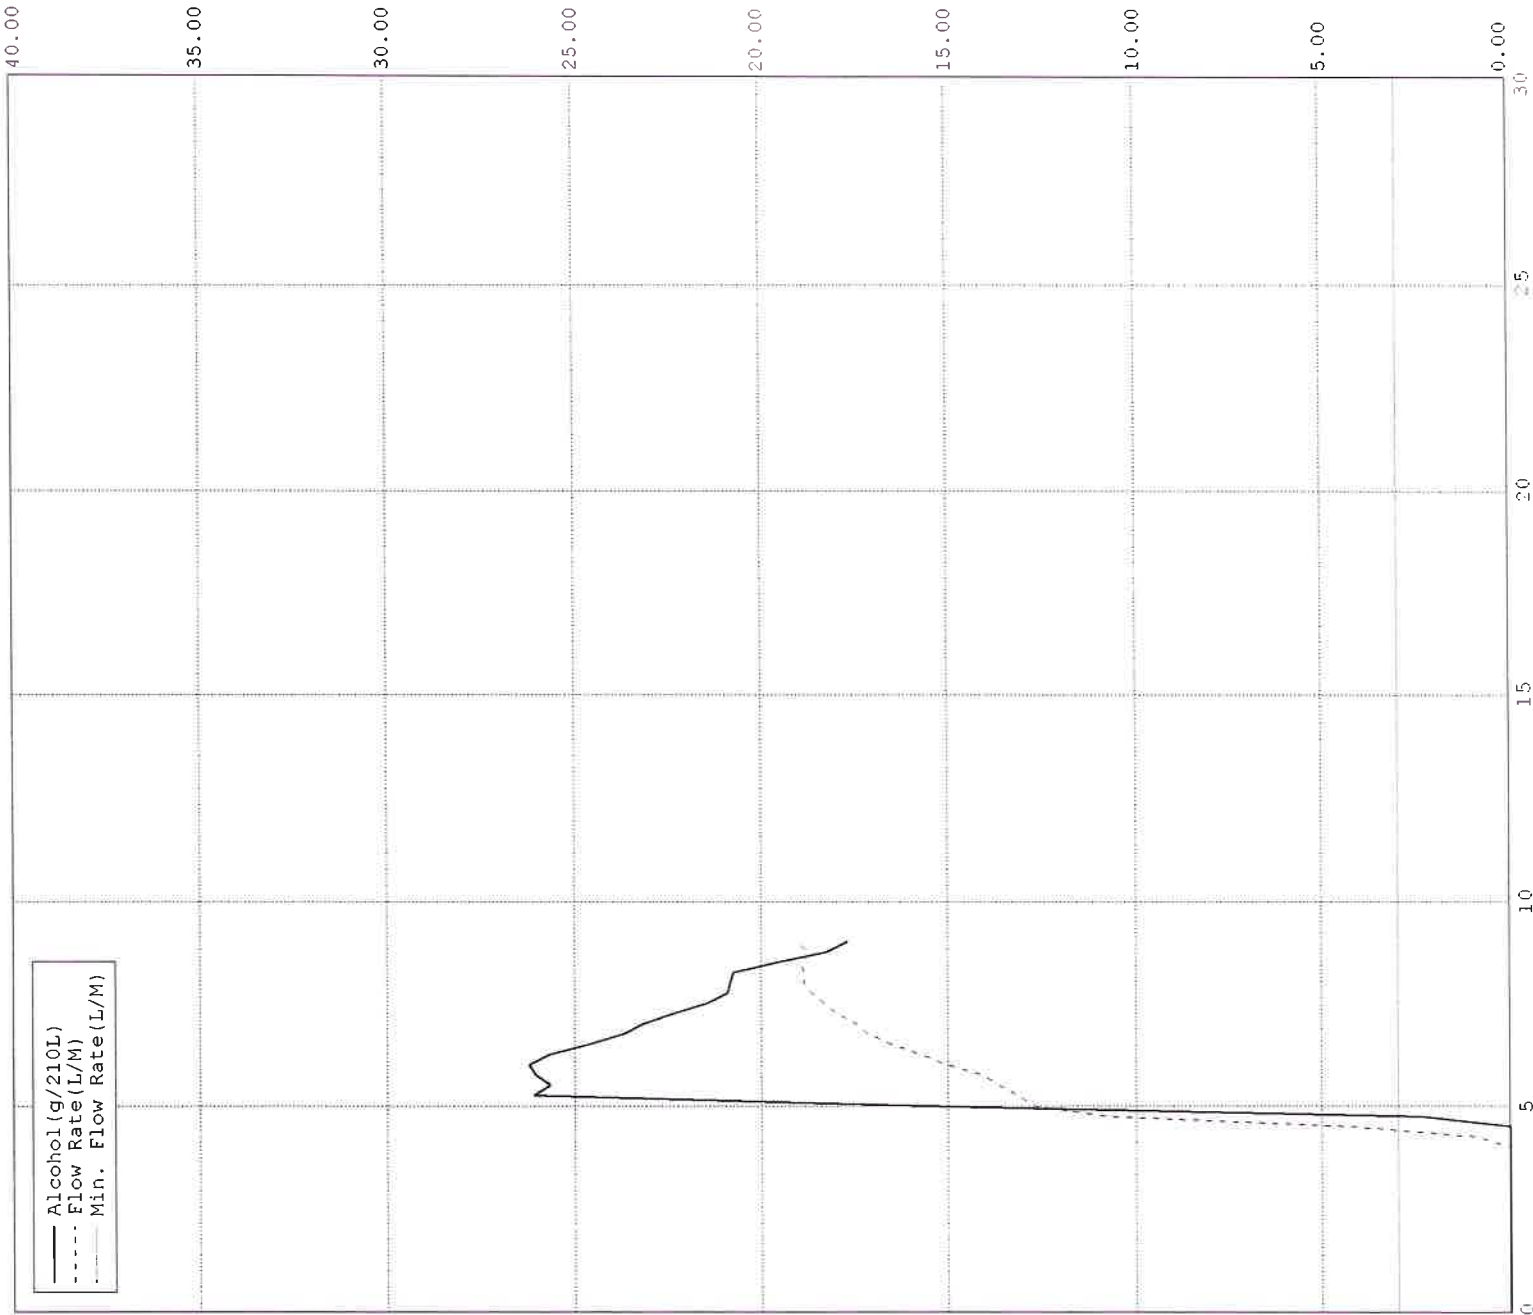

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100362

Date: 07/30/2024
Time: 13:21:24

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.35: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:22
BLANK TEST 0.000 13:22
INTERNAL STANDARD VERIFIED 13:22
EXTERNAL STANDARD 0.078 13:22
BLANK TEST 0.000 13:23

RFI DETECTED

MNC

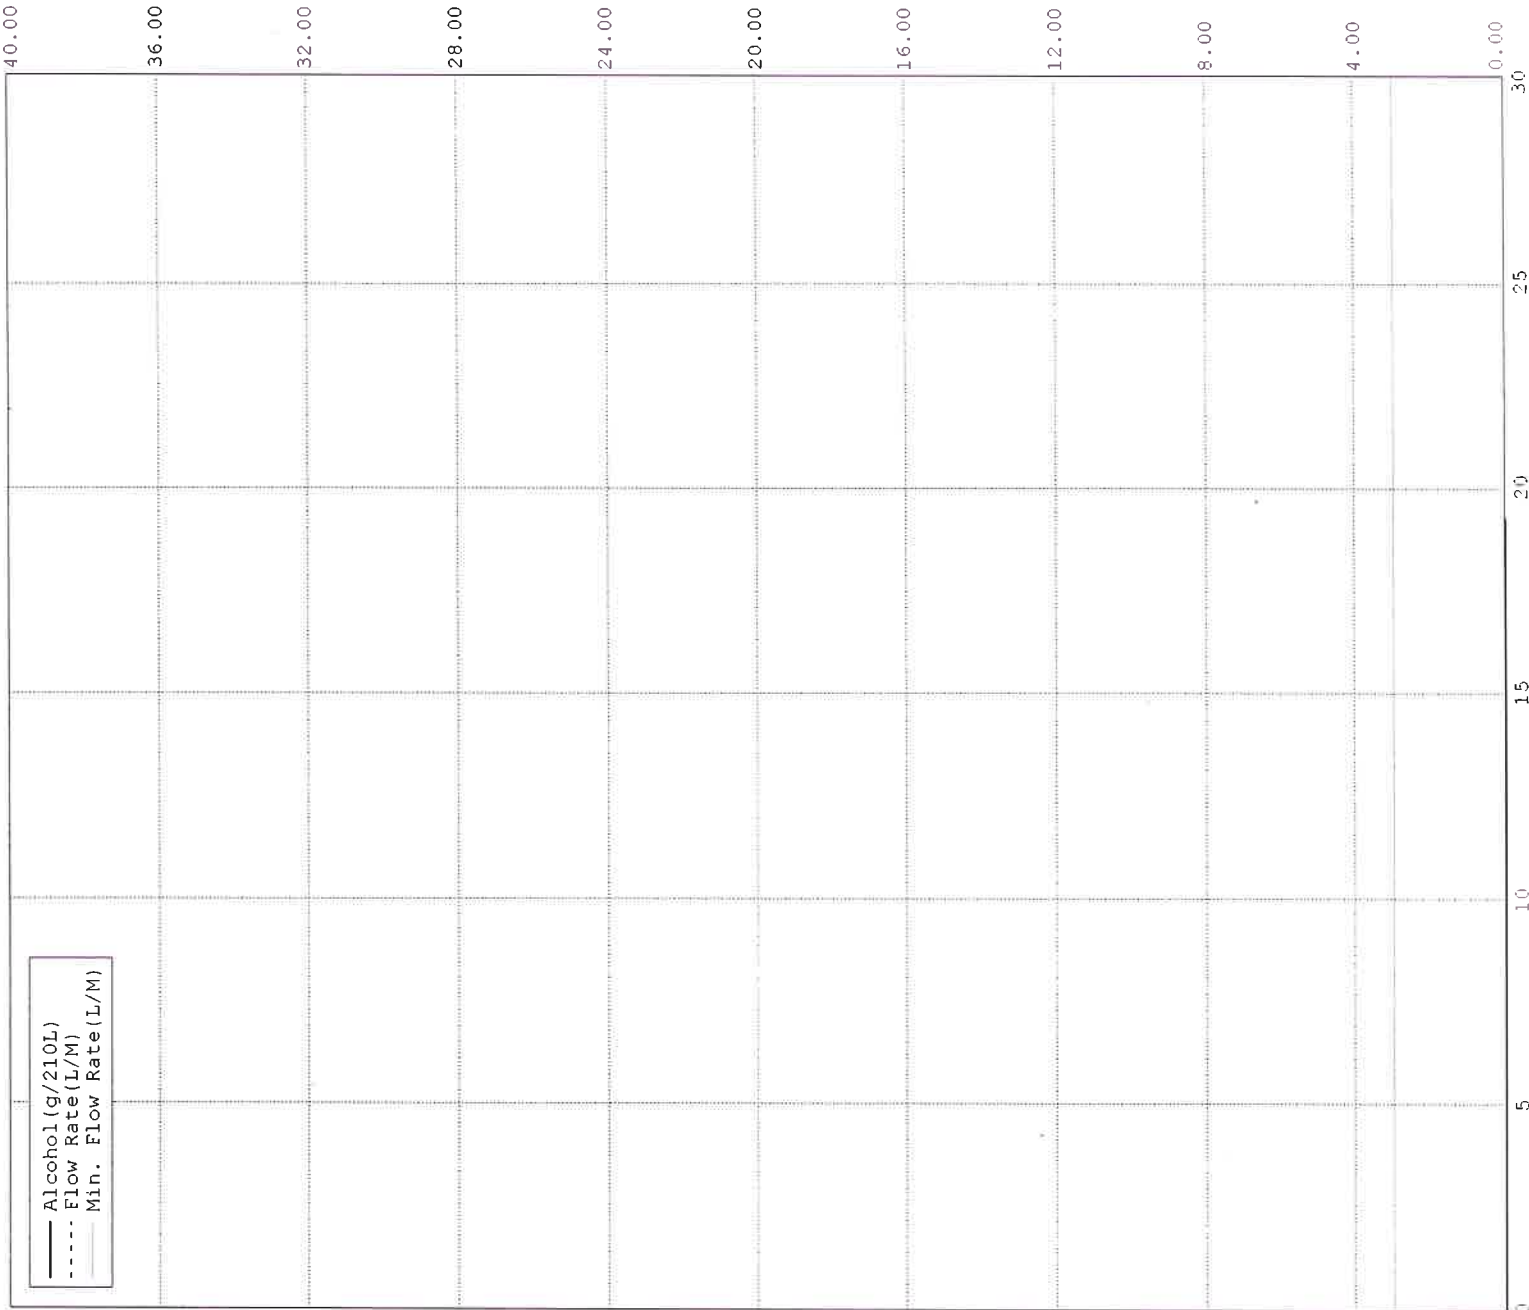

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100362

Date: 07/30/2024
Time: 13:50:53

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.35: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:52
BLANK TEST	0.000	13:52
INTERNAL STANDARD	VERIFIED	13:52
X _q = 0.073 (0.488)		
EXTERNAL STANDARD	0.077	13:52
X[1] = 0.0769 (-0.0015) (0.0024)		
BLANK TEST	0.000	13:53
SUBJECT SAMPLE	XXX	13:53
X[1] = 0.0999 (-0.0154) (0.0021)		

Interference Detected


Filter 2 Average: -0.0006

Filter 3 Average: ~~0.0027~~ 0.0029

MNC 9/3/24

MNC 7/30/24

MNC

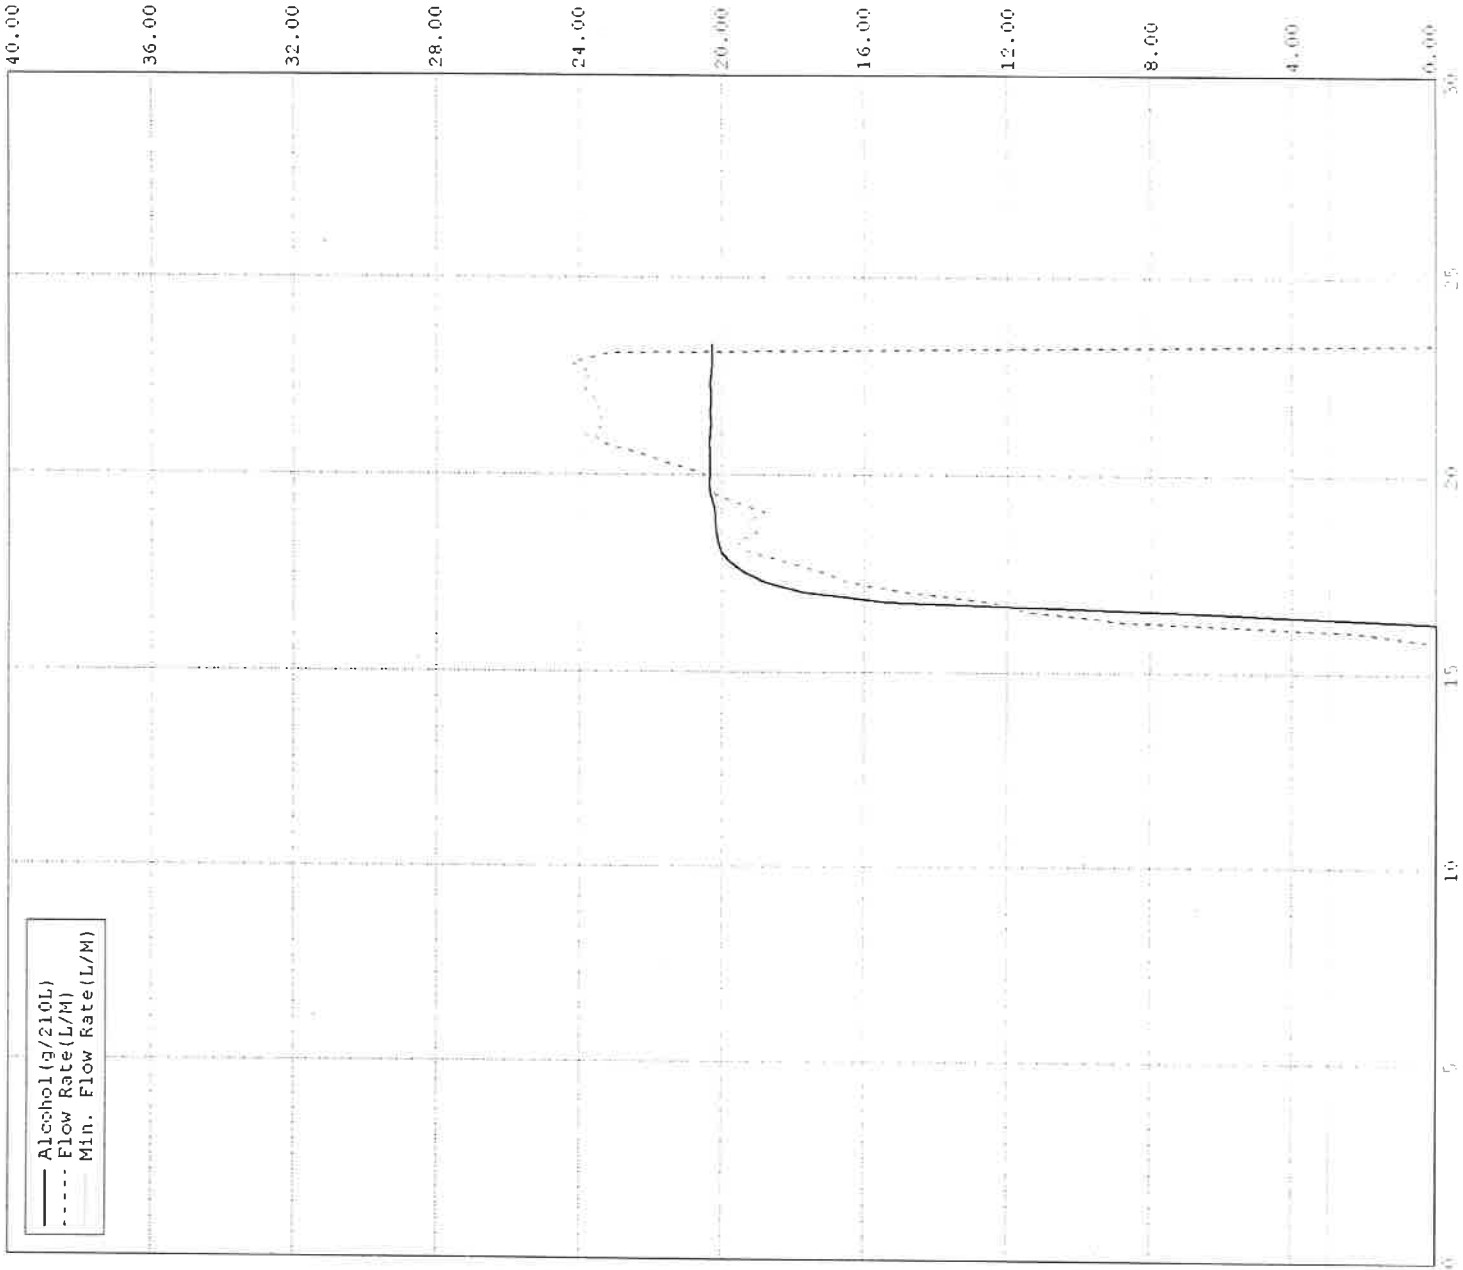

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100362

Date: 07/30/2024
Time: 13:46:01

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.35: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:47
BLANK TEST	0.000	13:47
INTERNAL STANDARD	VERIFIED	13:47
$X_q = 0.074$ (1.43%)		
EXTERNAL STANDARD	0.078	13:47
$X[1] = 0.0779$ (-0.0001) (0.0030)		
BLANK TEST	0.000	13:48
SUBJECT SAMPLE	XXX	13:49
$X[1] = 0.1083$ (-0.0216) (0.0021)		

Interference Detected

MJC

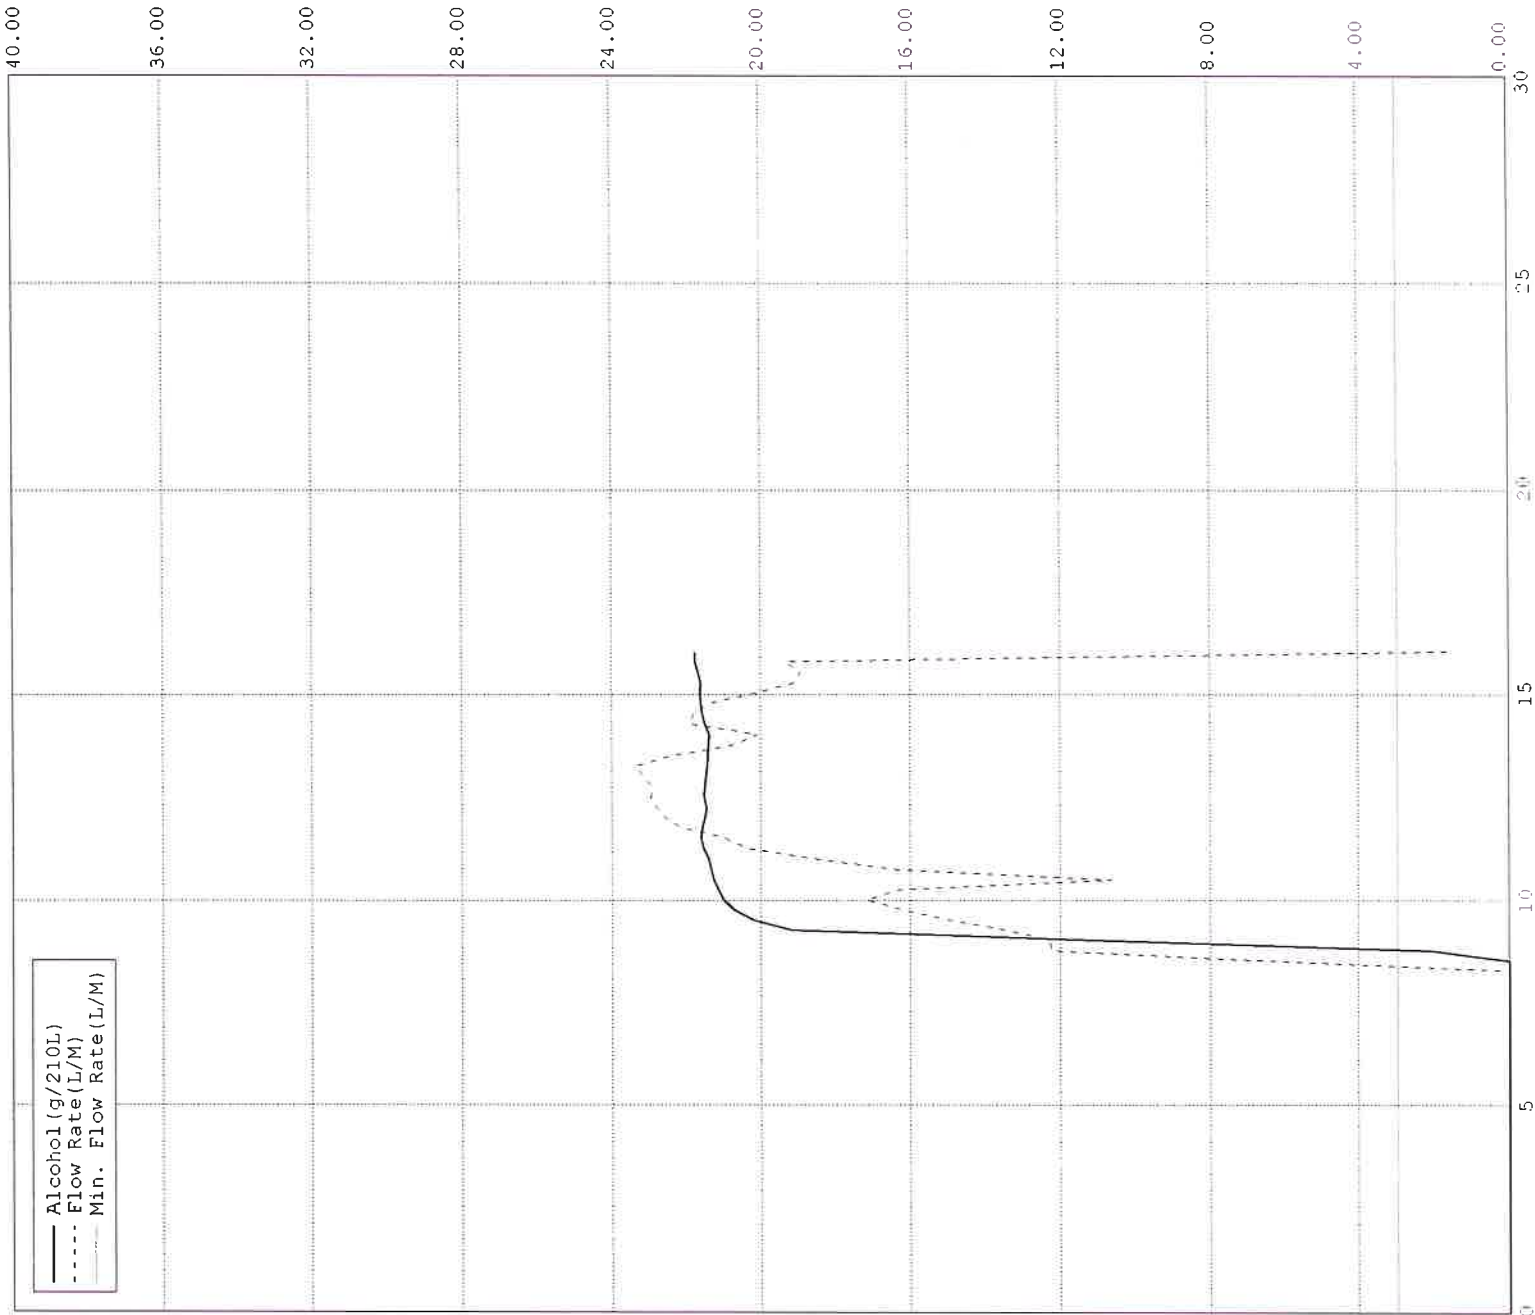

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100362

Date: 07/30/2024

Time: 13:38:06

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INTERFERENCE - NEGATIVE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.35: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

PASSED 13:40

BLANK TEST 0.000 13:40

INTERNAL STANDARD

VERIFIED 13:40

Xq = 0.074 (1.31%)

EXTERNAL STANDARD 0.078 13:40

X[1] = 0.0778 (-0.0002) (0.0034)

BLANK TEST 0.000 13:41

SUBJECT SAMPLE (Vol=2.24L) 0.088 13:42

X[1] = 0.0881 (0.0004) (0.0012)


BLANK TEST 0.000 13:43

EXTERNAL STANDARD 0.077 13:43

X[1] = 0.0774 (-0.0005) (0.0027)

BLANK TEST 0.000 13:44

MNC

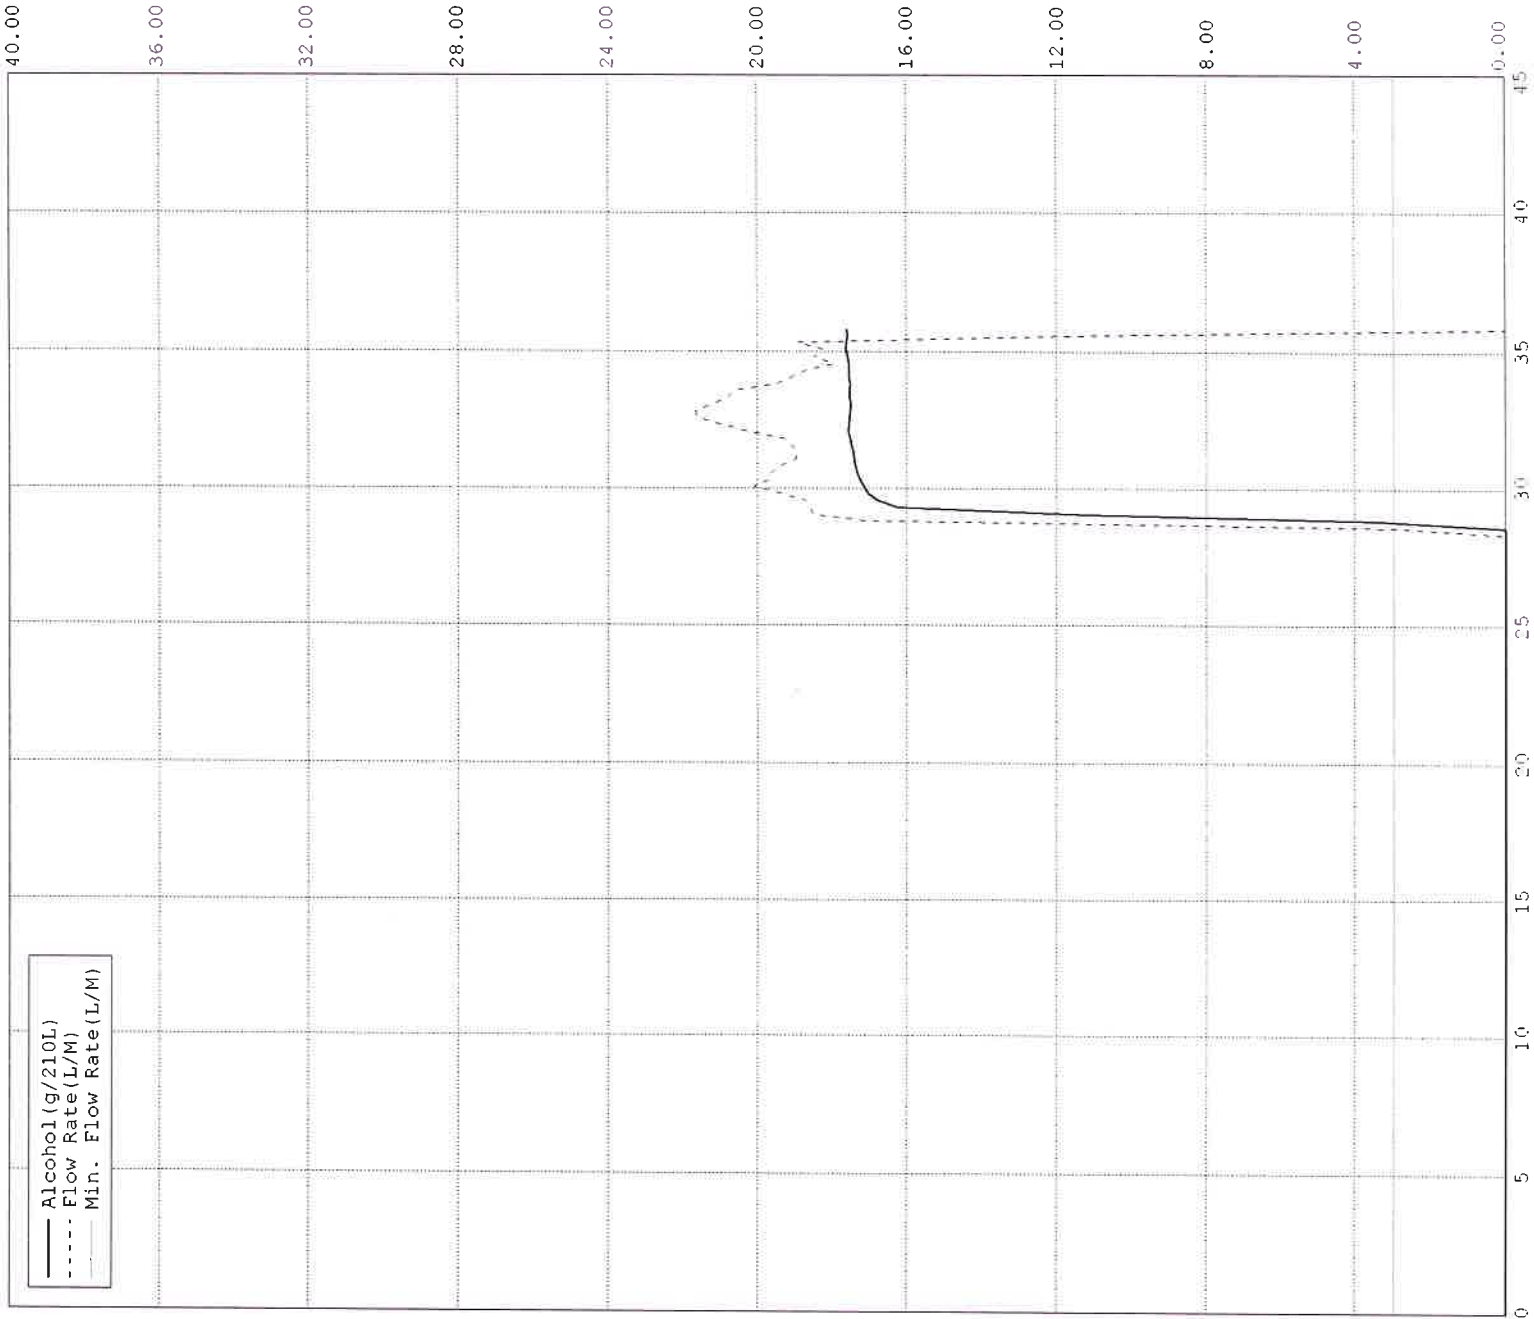

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100362

Date: 07/30/2024
Time: 14:09:00

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.35: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:10
BLANK TEST	0.000	14:10
INTERNAL STANDARD	VERIFIED	14:10
EXTERNAL STANDARD	0.078	14:10
BLANK TEST	0.000	14:11
SUBJECT SAMPLE (Vol=3.18L)	0.000	14:11
BLANK TEST	0.000	14:12
EXTERNAL STANDARD	0.078	14:12
BLANK TEST	0.000	14:13

MNC

