



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100390

**Report Issue Date:** 11/16/2023  
**Date Received:** 2023-02-27  
**Condition of Item:** Needs Repair

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 03/08/2023** - As Found - **End Date 03/08/2023** As Found - Evaluation Analyst: Tatiana Malnoske  
 As Found Conditions - Barometric Pressure (inHg): 29.98 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.5  
 Relative Humidity (%): 13%

As-Found Data				
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)	Mean (g/210L)
0.020				
0.080				
0.300				

Appears to be damage on the threading on the regulator due to issues with screwing in tanks. I was unable to perform linearity testing due to this, I tried 4 different 0.020 tanks and none would screw in.

**Start Date 11/03/2023** - As Left - **End Date 11/06/2023**

As Left Conditions - Barometric Pressure (inHg): 29.33 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.0 Relative Humidity (%): 24

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG217904	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.078	AG310901	0.080	0.080	0.080	0.080	0.079	0.080	+/- 0.004
0.100	0.098	AG211003	0.100	0.100	0.100	0.099	0.099	0.100	+/- 0.004
0.150	0.147	AG134205	0.150	0.149	0.150	0.150	0.149	0.150	+/- 0.005
0.300	0.294	AG217903	0.301	0.300	0.301	0.300	0.300	0.300	+/- 0.011

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**



State of Alaska  
Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
Anchorage, Alaska 99507  
David Kanaris, Chief, Forensic Laboratories

---

**Serial Number:** 100390

---

Results authorized by Derek Walton on 11/16/2023

[derek.walton@alaska.gov](mailto:derek.walton@alaska.gov)

Technically and administratively reviewed by Colleen O'Bryant on 11/16/2023

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100390 Analyst: Derek Walton Start Date: 11/03/23

- Diagnostic Test (attached)
- Adjust voltages, if needed
  - o Lamp (2.60 V Maximum)
  - o Bias
  - o Cooler (2.00 V Maximum)
- Internal Standard value  $\leq$  3.00%
  - o Chopper Frequency
  - o Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.6 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.33 Temperature (C): 22.0 Relative Humidity (%) 24

Linearity Test (attached)

0.020g/210L Mnf: Airgas Lot: AG217902 Exp: 06/28/24  
0.040g/210L Mnf: Airgas Lot: AG217904 Exp: 06/28/24  
0.080g/210L Mnf: Airgas Lot: AG310901 Exp: 04/19/25  
0.100g/210L Mnf: Airgas Lot: AG211003 Exp: 09/20/24  
0.150g/210L Mnf: Airgas Lot: AG134205 Exp: 12/08/23  
0.300g/210L Mnf: Airgas Lot: AG217903 Exp: 06/28/24

Functional Tests (attached)

- Incomplete
  - Maximum Attempts Exceeded
  - Interference (Volatiles)
  - Invalid
  - Radio Frequency Interference (RFI)
- Acetone Mnf: Lifeloc Lot: 22HP41201 Level: 0.100 Exp: 08/24/24  
Simulator S/N: DR4176 Verification Performed?
- Isopropanol Mnf: Lifeloc Lot: 22HP41201 Level: 0.100 Exp: 08/24/24  
Simulator S/N: DR4177 Verification Performed?
- Neg. Control Mnf: Lifeloc Lot: 22HP41201 Level: 0.100 Exp: 08/24/24  
Simulator S/N: DR6267 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/09/23

- Verify stylus is calibrated
  - Reset Options
  - Clear Memory
  - Verification of Calibration (VOC)
  - Non-Drinking Subject Test
  - Upload
  - Remove Tank Prior to Shutdown
- Calibration End Date: 11/03/23

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100390  
-----

Date: 11/03/2023  
Time: 08:02:07

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 46.0°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.65 V PASSED  
(0.99 V - 2.31 V)  
Cooler Voltage = 1.54 V PASSED  
(0.96 V - 2.24 V)  
Bias Voltage = 79 V PASSED  
(48 V - 112 V)  
Chopper Freq = 538 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.3 in

PUMP INFO

Flow Rate = 4.918 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 v <= 0.010 v)  
PUMP OFF PASSED  
(0.002 v <= 0.010 v)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD ✓ PASSED  
Xq = 0.096 0.73% (0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100390  
-----

Date: 11/03/2023  
Time: 8:11 AM

Temperatures (°C)

Sample Cell: 48.8°C  
Breath Tube: 45.6°C

Current Barometer 29.3 in  
Volume (Ltr) 1.50

Settings

Lamp: 1.71 V  
Bias: 79 V  
Cooler: 1.60 V  
Chopper: 526 Hz

Voltages (V)

Flow: 1.06 V  
Detector: -0.087 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100390  
-----

Date: 03/10/2011  
Time: 07:44:47

Ca = 0.1000  
CAL = 0.993918    0.800 <= CAL < 1.200  
b1 = 0.0005    0.0000 <= b1 < 0.0040  
b2 = 0.0038    0.0010 <= b2 < 0.0100  
b3 = 0.0003    0.0000 <= b3 < 0.0040  
Xq = 0.0958    0.0500 <= Xq < 0.2000  
a21 = 1.168537    1.050 <= a21 < 1.300  
a31 = 0.503509    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100390

Date: 11/03/2023  
Time: 08:16:04

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
MINIMUM VOLUME  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.34: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	08:17
BLANK TEST	0.000	08:17
INTERNAL STANDARD	VERIFIED	08:17
EXTERNAL STANDARD	0.079	08:17
BLANK TEST	0.000	08:18
SUBJECT SAMPLE (Vol=1.55L)	0.000	08:19
BLANK TEST	0.000	08:20
EXTERNAL STANDARD	0.079	08:20
BLANK TEST	0.000	08:21

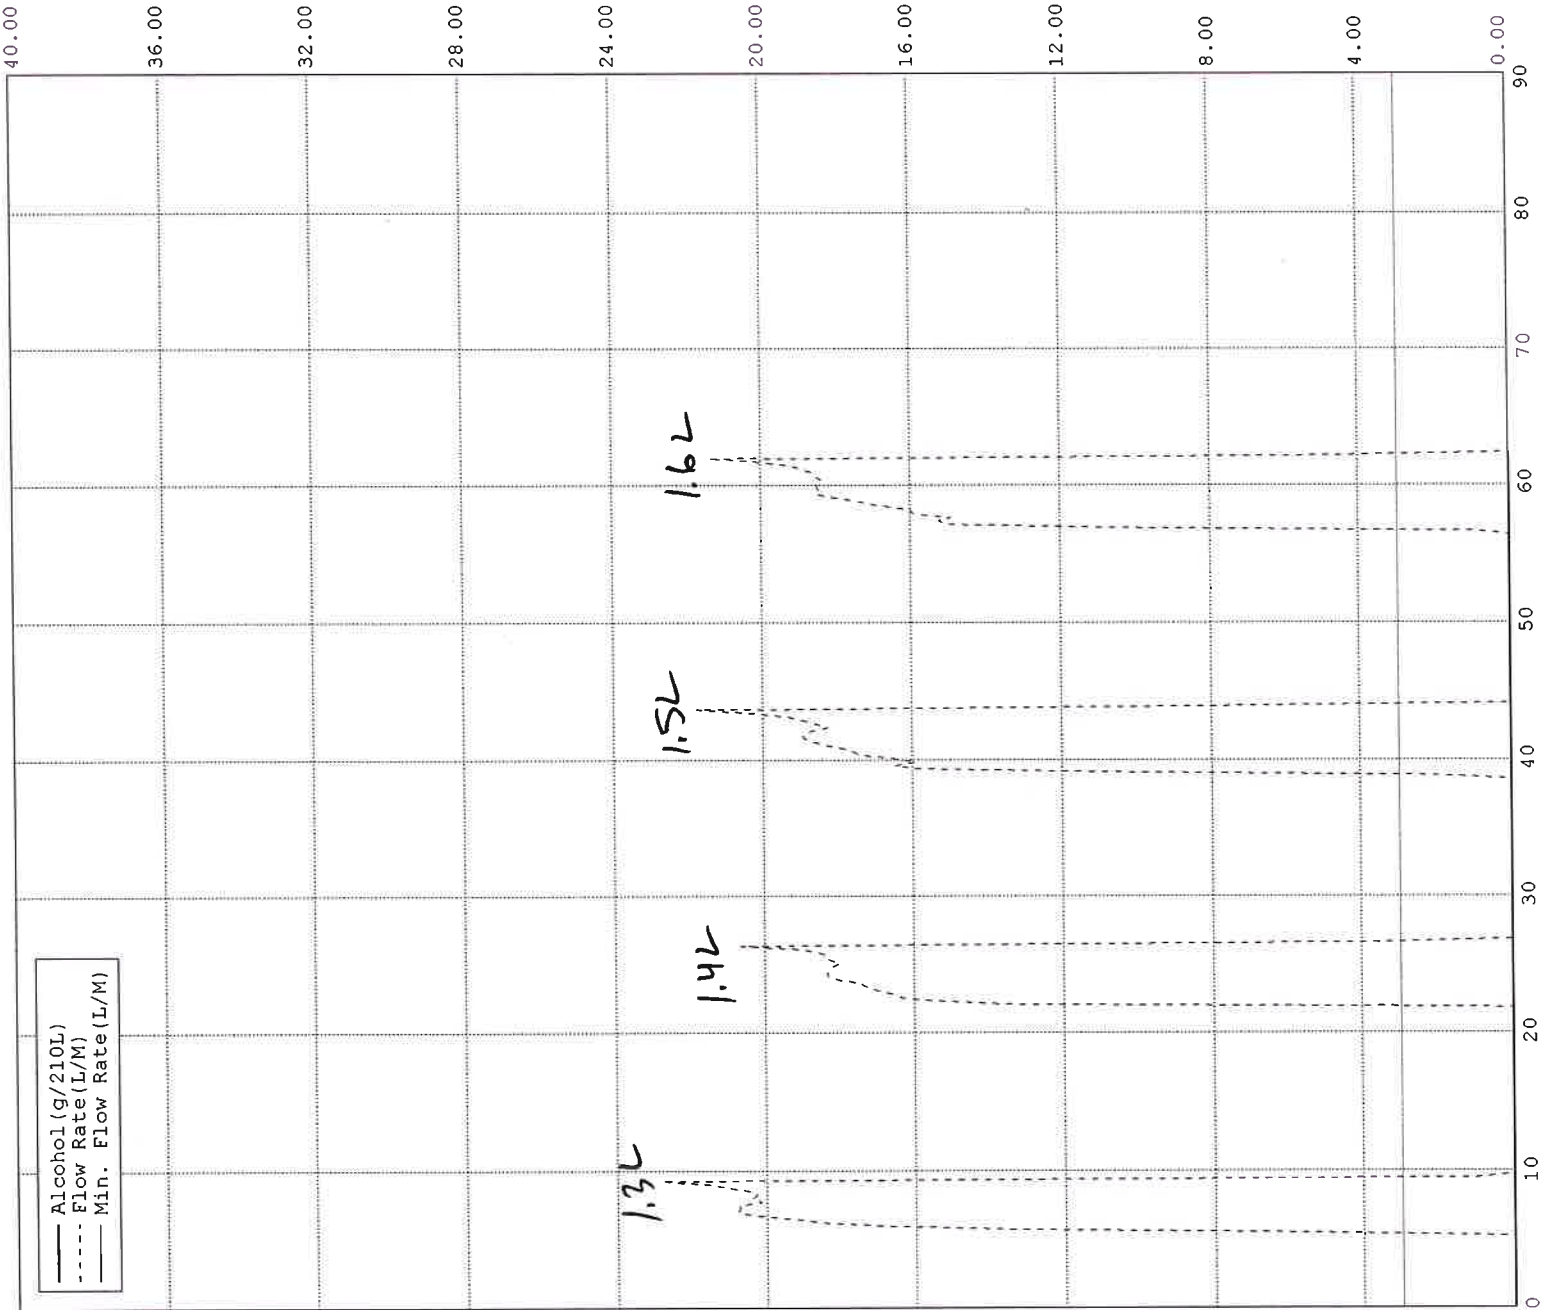

LINEARITY CHECK

Alaska Department of Public Safety  
 DATAMASTER dmt: 100390


Date: 11/03/2023  
 Time: 08:25:48

SUPERVISOR NAME:  
 DEREK WALTON  
 OPERATOR'S #: 9508

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.039	0.0400	0.0000
0.078	0.0798	0.0004
0.098	0.0996	0.0005
0.147	0.1496	0.0005
0.294	0.3004	0.0005

SLOPE = 1.022029  
 R<sup>2</sup> = 0.999989

*DW*

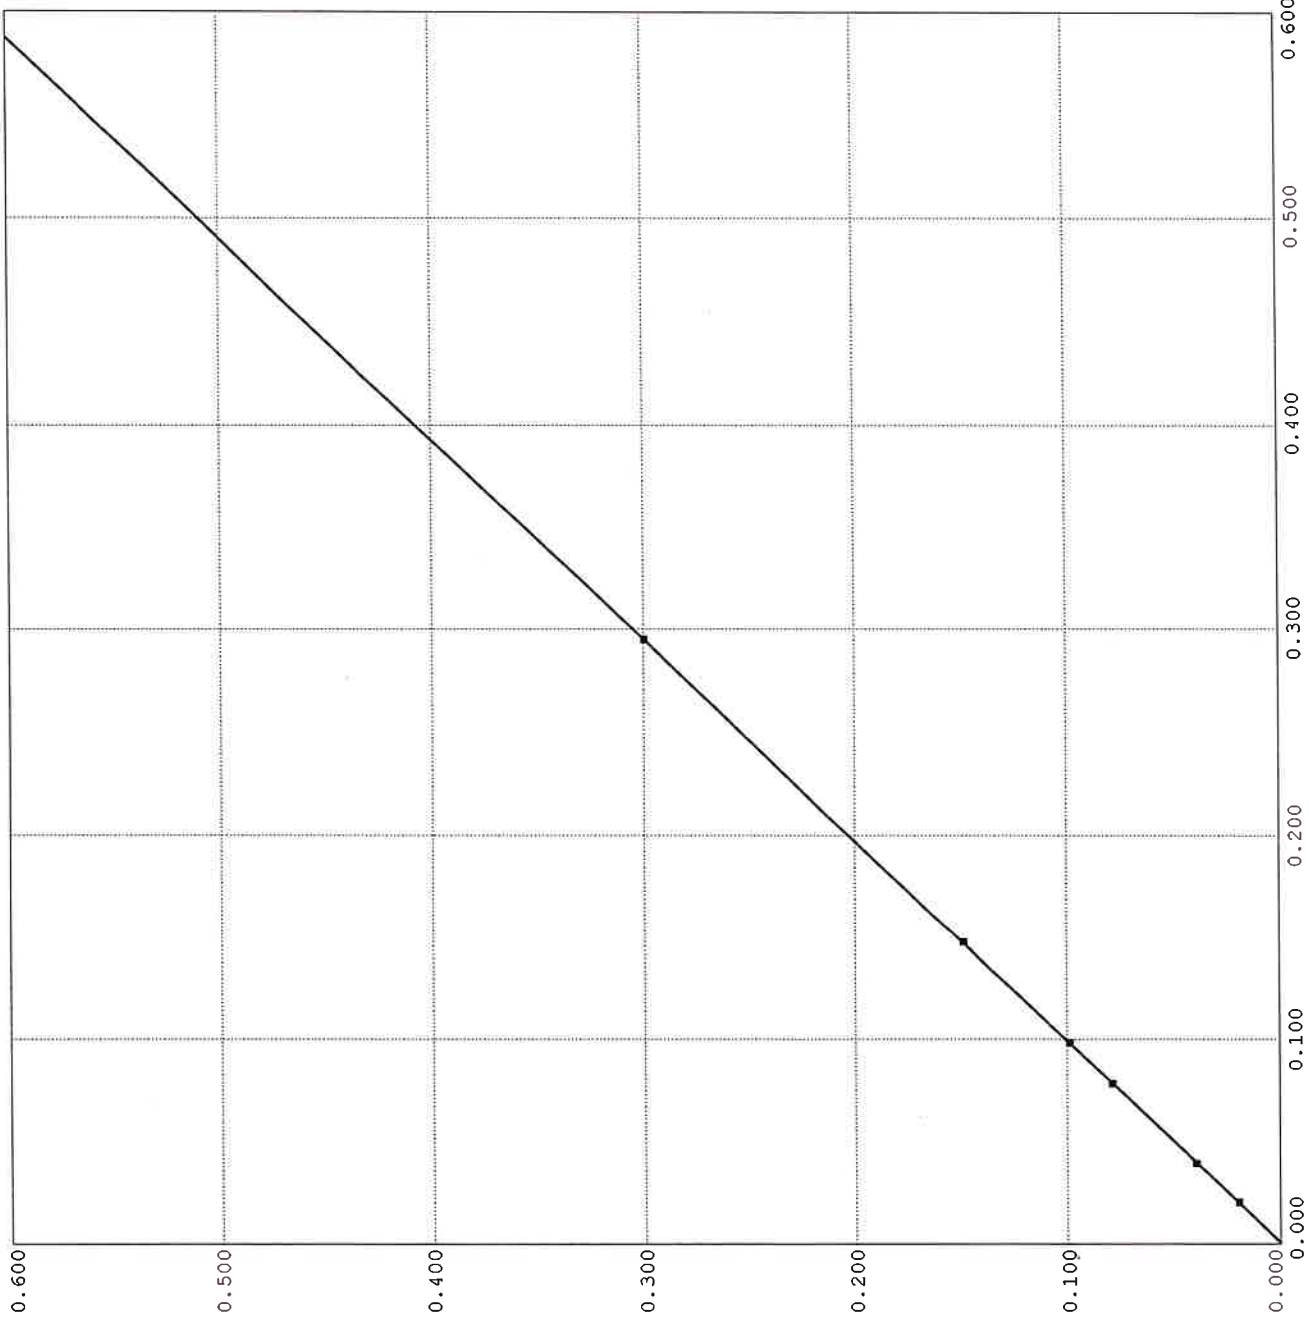



LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100390






Date: 11/03/2023  
Time: 08:25:51

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.33: 0.020  
LOT #: AG217902  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 839 psi

BLANK TEST	0.000	08:27
INTERNAL STANDARD	VERIFIED	08:27
EXTERNAL STANDARD	0.020	08:27
BLANK TEST	0.000	08:28
EXTERNAL STANDARD	0.020	08:28
BLANK TEST	0.000	08:29
EXTERNAL STANDARD	0.020	08:29
BLANK TEST	0.000	08:30
EXTERNAL STANDARD	0.020	08:30
BLANK TEST	0.000	08:31
EXTERNAL STANDARD	0.020	08:31
BLANK TEST	0.000	08:32

Average = 0.0200  
Std Dev = 0.0000

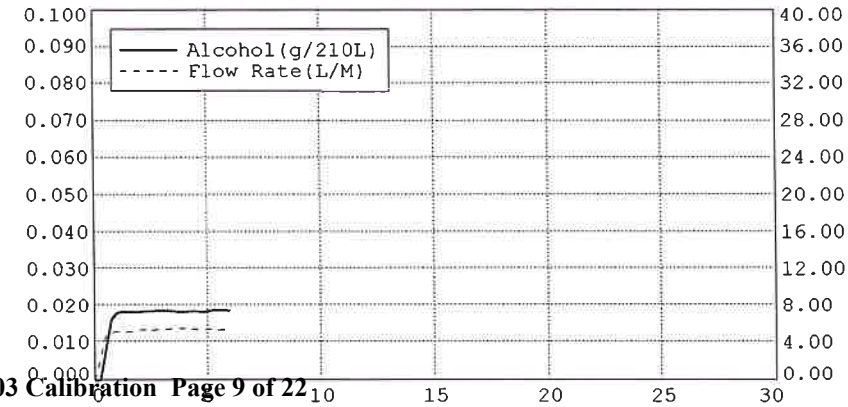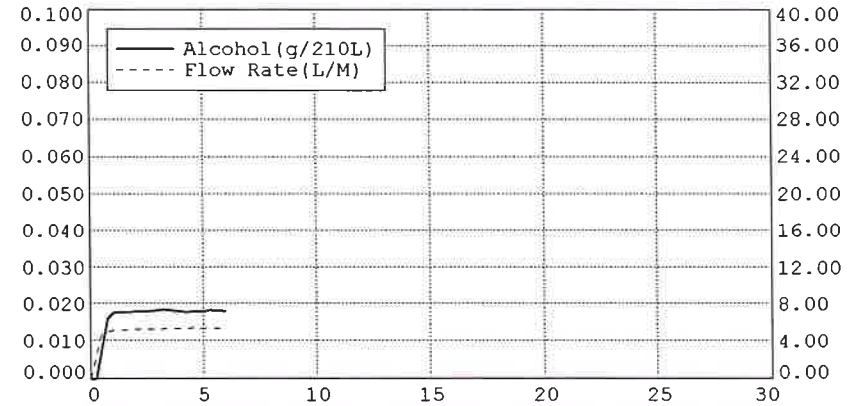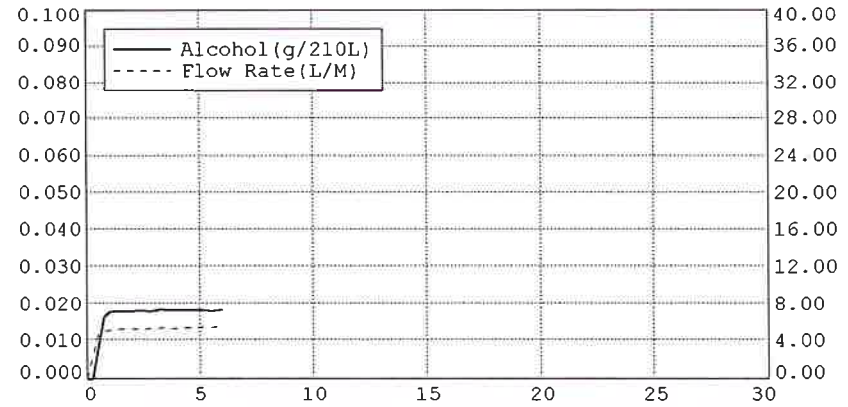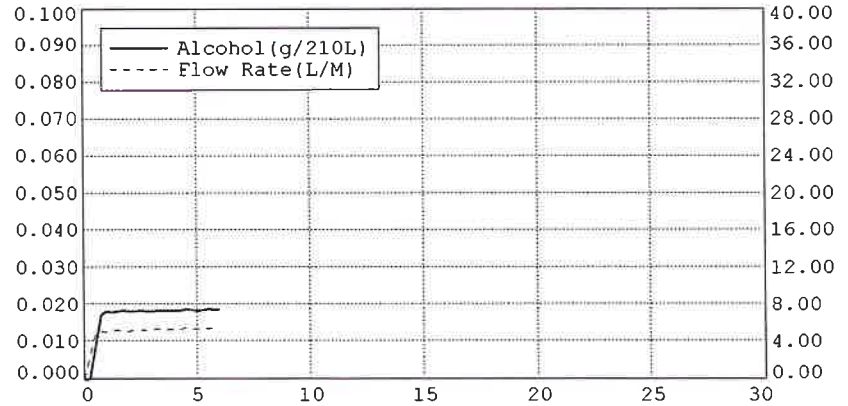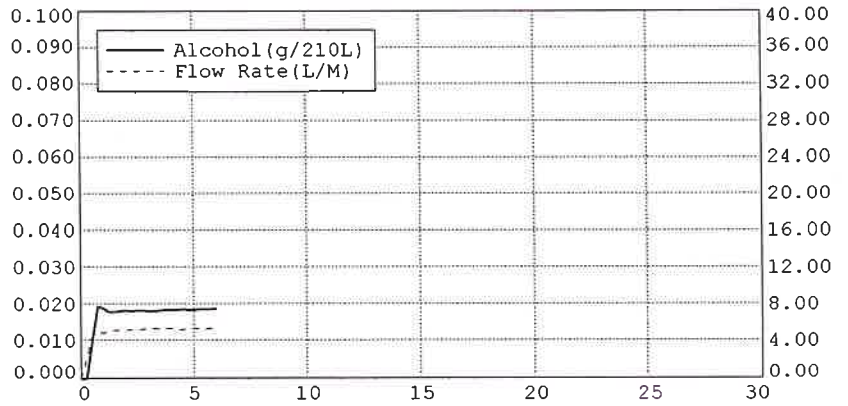

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
DATAMASTER dmt: 100390






Date: 11/03/2023  
Time: 08:34:33

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
TARGET AT 29.33: 0.039  
LOT #: AG217904  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 888 psi

BLANK TEST	0.000	08:35
INTERNAL STANDARD	VERIFIED	08:35
EXTERNAL STANDARD	0.040	08:36
BLANK TEST	0.000	08:37
EXTERNAL STANDARD	0.040	08:37
BLANK TEST	0.000	08:38
EXTERNAL STANDARD	0.040	08:38
BLANK TEST	0.000	08:39
EXTERNAL STANDARD	0.040	08:39
BLANK TEST	0.000	08:40
EXTERNAL STANDARD	0.040	08:40
BLANK TEST	0.000	08:41

Average = 0.0400  
Std Dev = 0.0000

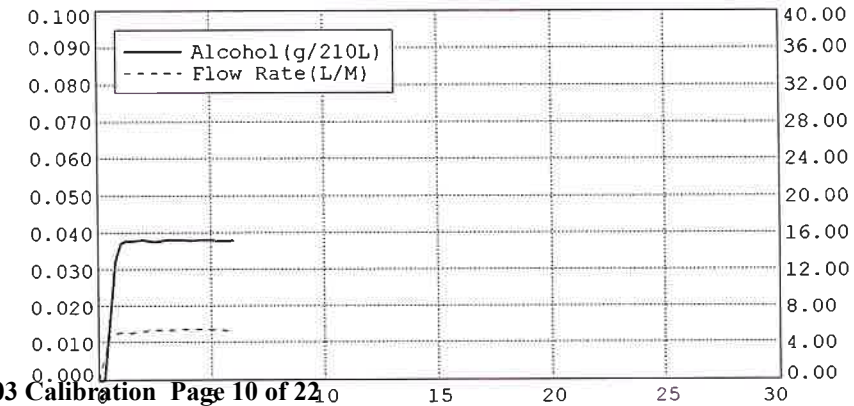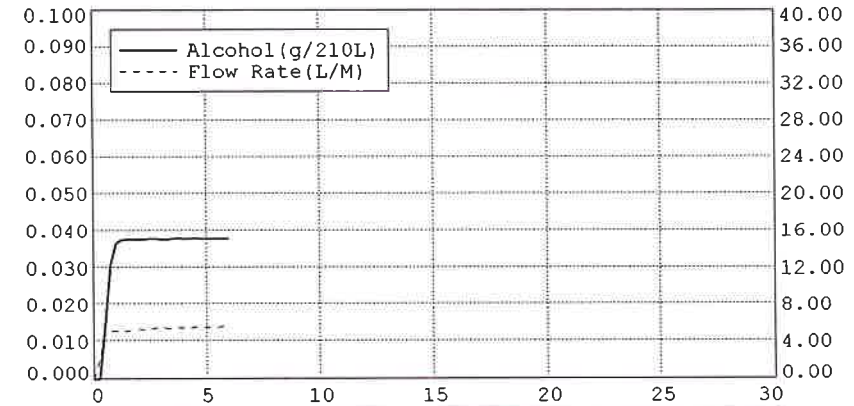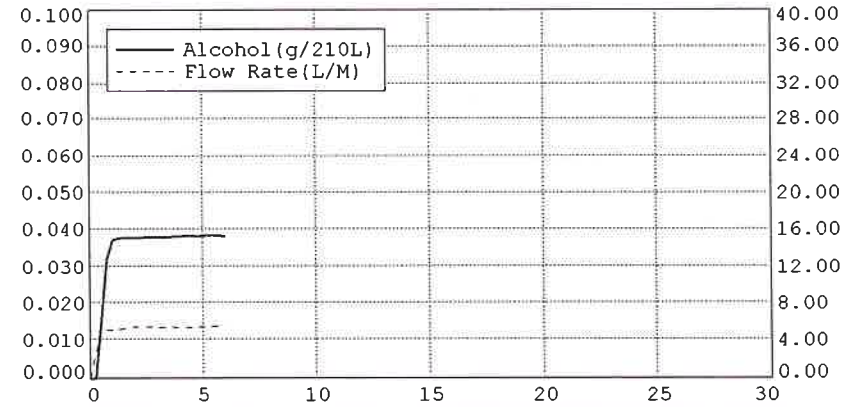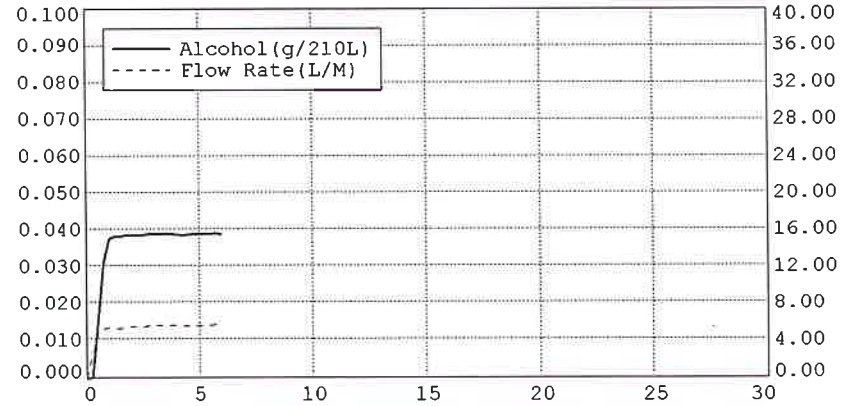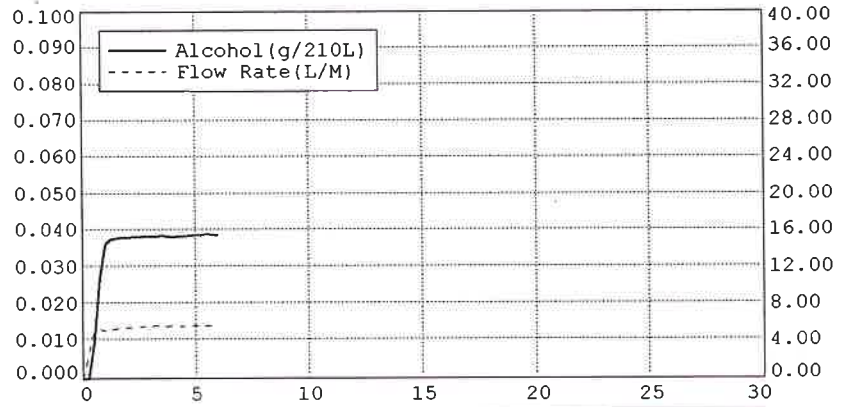

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
DATAMASTER dmt: 100390






Date: 11/03/2023  
Time: 08:43:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.33: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025  
TANK PRESSURE: 811 psi

BLANK TEST	0.000	08:45
INTERNAL STANDARD	VERIFIED	08:45
EXTERNAL STANDARD	0.080	08:45
BLANK TEST	0.000	08:46
EXTERNAL STANDARD	0.080	08:46
BLANK TEST	0.000	08:47
EXTERNAL STANDARD	0.080	08:47
BLANK TEST	0.000	08:48
EXTERNAL STANDARD	0.080	08:48
BLANK TEST	0.000	08:49
EXTERNAL STANDARD	0.079	08:49
BLANK TEST	0.000	08:50

Average = 0.0798  
Std Dev = 0.0004

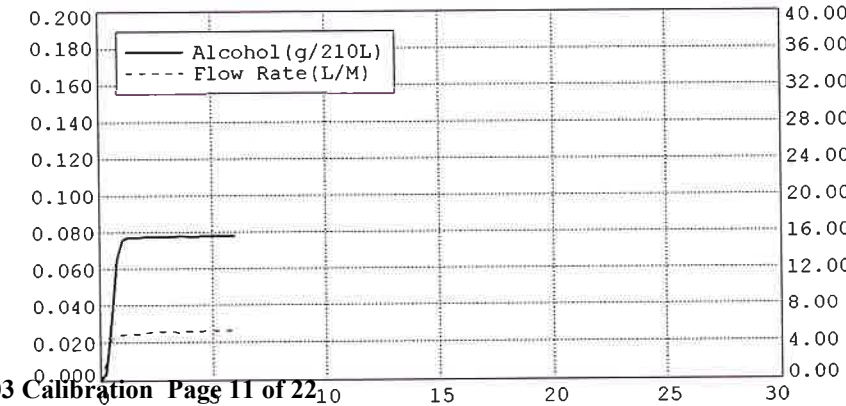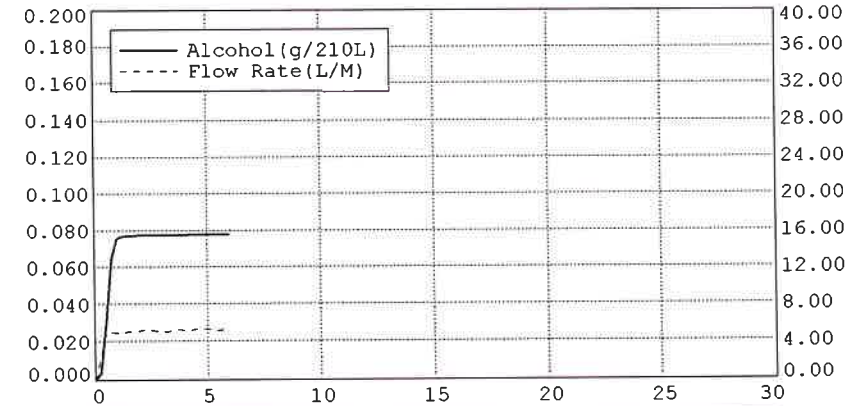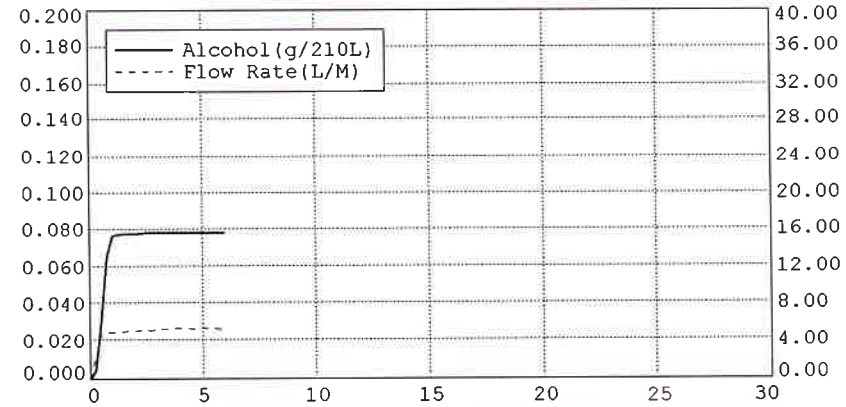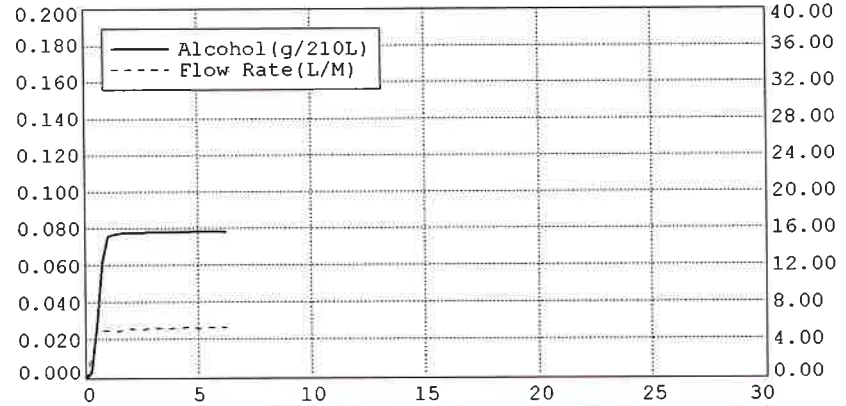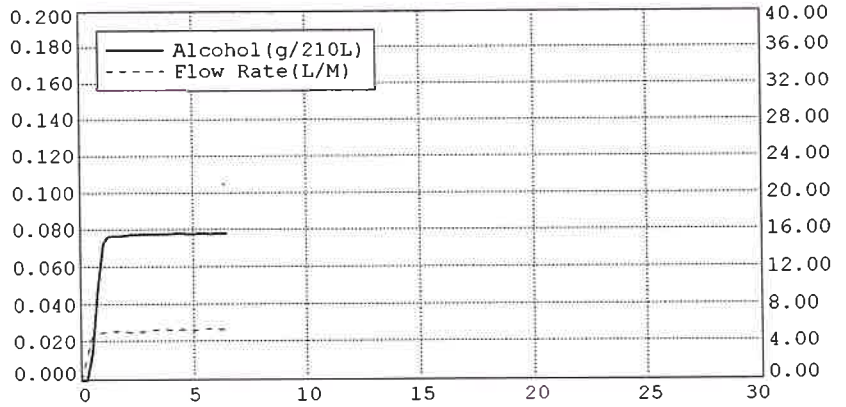



LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
DATAMASTER dmt: 100390






Date: 11/03/2023  
Time: 08:51:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
TARGET AT 29.33: 0.098  
LOT #: AG211003  
EXPIRATION: 04/20/2024  
TANK PRESSURE: 548 psi

BLANK TEST	0.000	08:52
INTERNAL STANDARD	VERIFIED	08:53
EXTERNAL STANDARD	0.100	08:53
BLANK TEST	0.000	08:54
EXTERNAL STANDARD	0.100	08:54
BLANK TEST	0.000	08:55
EXTERNAL STANDARD	0.100	08:55
BLANK TEST	0.000	08:56
EXTERNAL STANDARD	0.099	08:56
BLANK TEST	0.000	08:57
EXTERNAL STANDARD	0.099	08:57
BLANK TEST	0.000	08:58

Average = 0.0996  
Std Dev = 0.0005

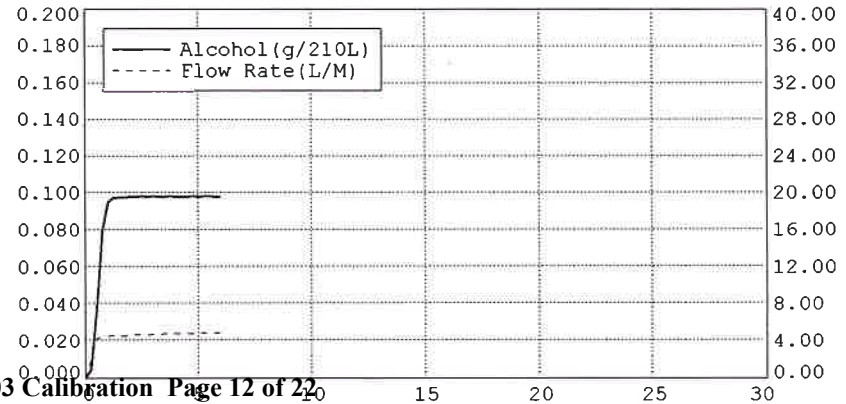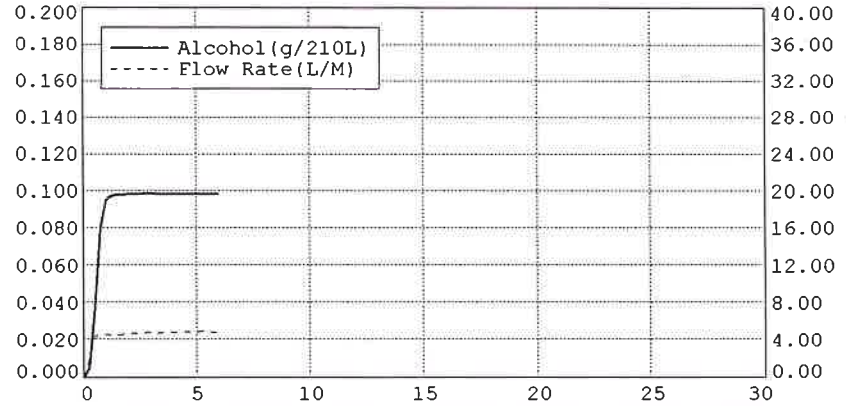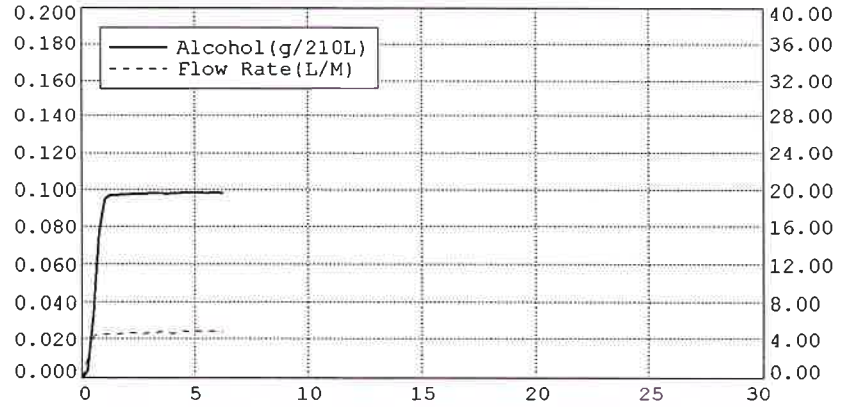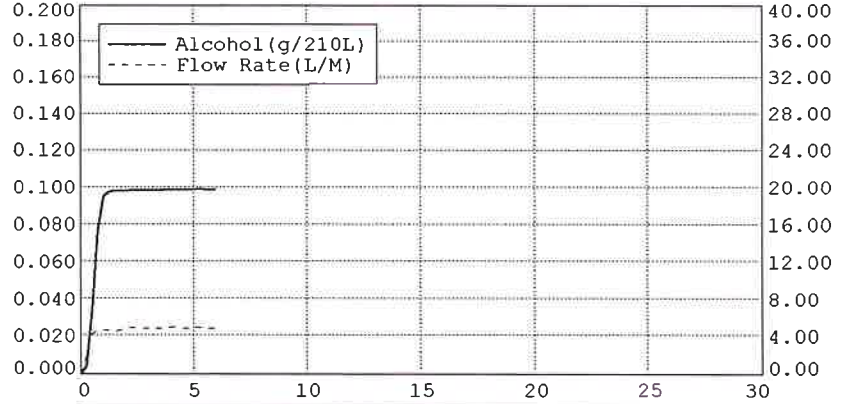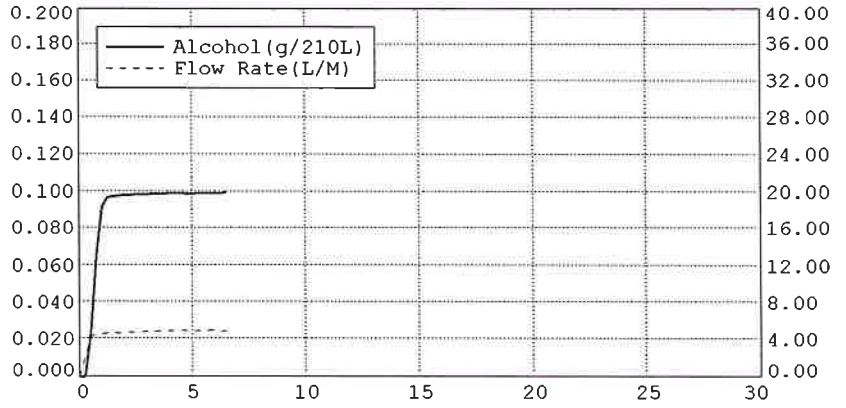

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100390






Date: 11/03/2023  
 Time: 08:59:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.34: 0.147  
 LOT #: AG134205  
 EXPIRATION: 12/08/2023  
 TANK PRESSURE: 717 psi

BLANK TEST	0.000	09:00
INTERNAL STANDARD	VERIFIED	09:01
EXTERNAL STANDARD	0.150	09:01
BLANK TEST	0.000	09:02
EXTERNAL STANDARD	0.149	09:02
BLANK TEST	0.000	09:03
EXTERNAL STANDARD	0.150	09:03
BLANK TEST	0.000	09:04
EXTERNAL STANDARD	0.150	09:04
BLANK TEST	0.000	09:05
EXTERNAL STANDARD	0.149	09:05
BLANK TEST	0.000	09:06

Average = 0.1496  
 Std Dev = 0.0005

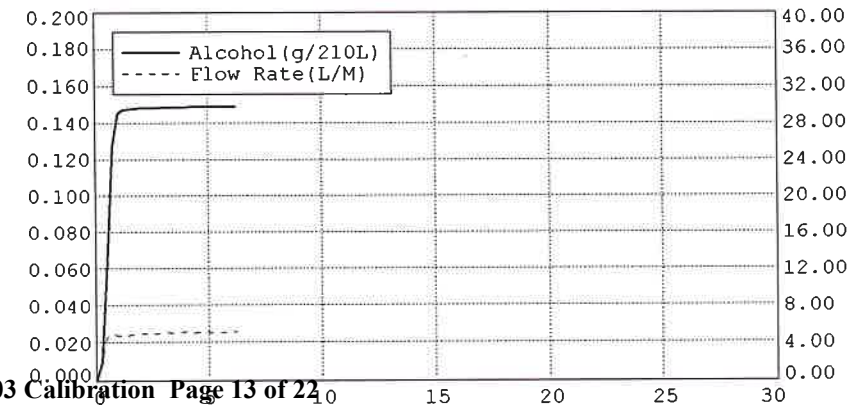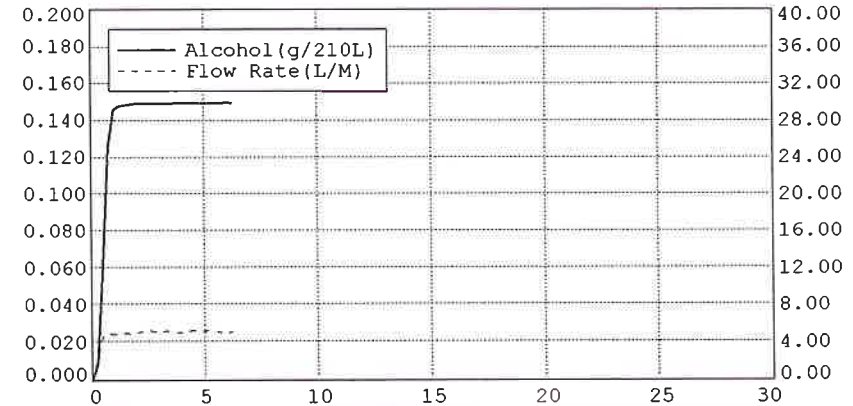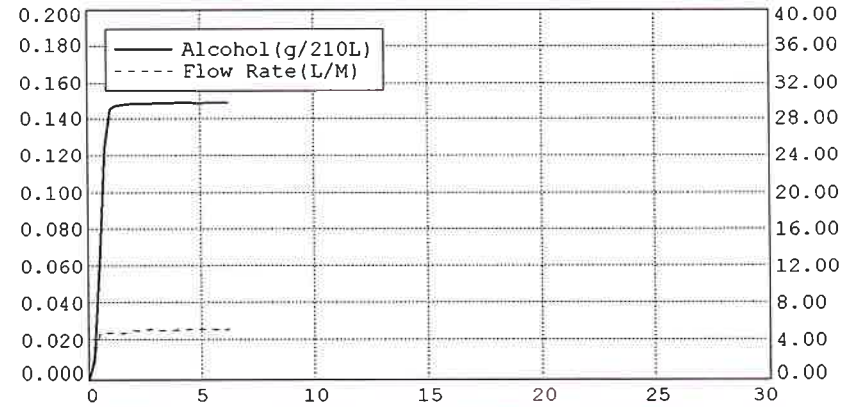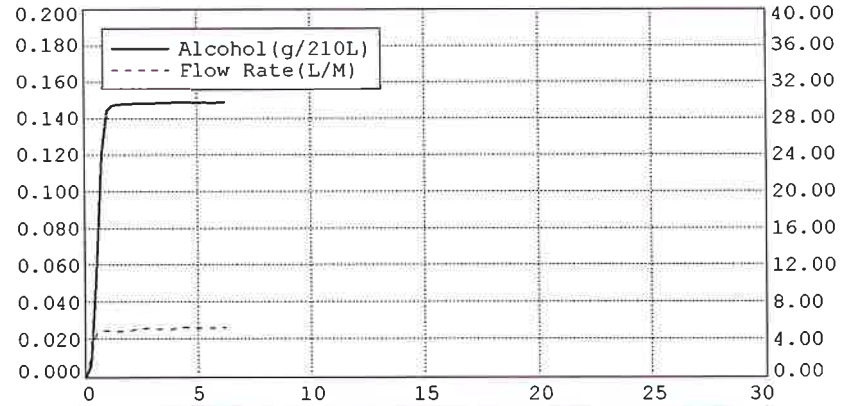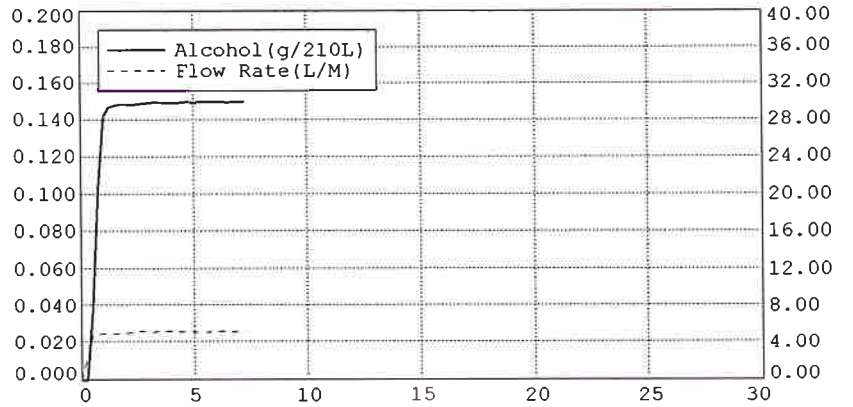

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
DATAMASTER dmt: 100390






Date: 11/03/2023  
Time: 09:08:12

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
TARGET AT 29.34: 0.294  
LOT #: AG217903  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 416 psi

BLANK TEST	0.000	09:09
INTERNAL STANDARD	VERIFIED	09:09
EXTERNAL STANDARD	0.301	09:09
BLANK TEST	0.000	09:10
EXTERNAL STANDARD	0.300	09:10
BLANK TEST	0.000	09:11
EXTERNAL STANDARD	0.301	09:12
BLANK TEST	0.000	09:13
EXTERNAL STANDARD	0.300	09:13
BLANK TEST	0.000	09:14
EXTERNAL STANDARD	0.300	09:14
BLANK TEST	0.000	09:15

Average = 0.3004  
Std Dev = 0.0005

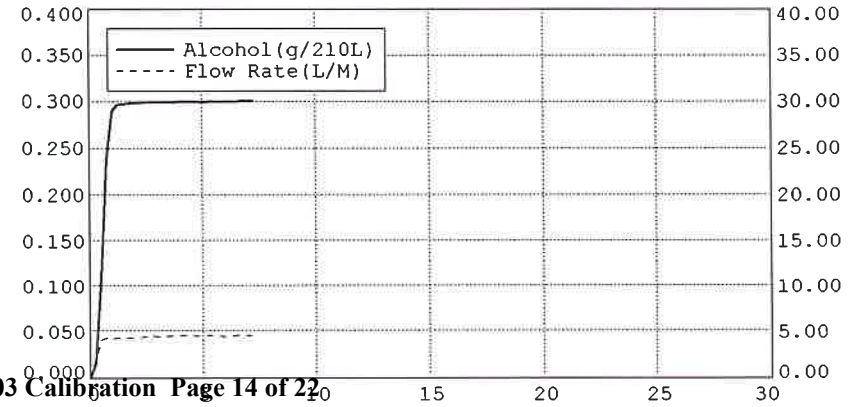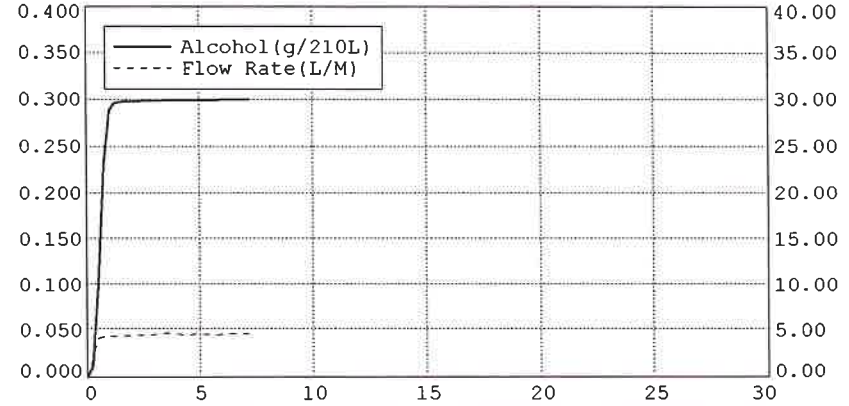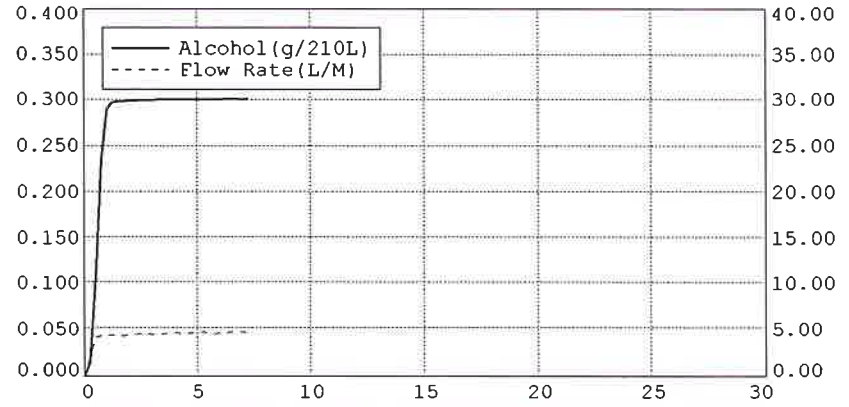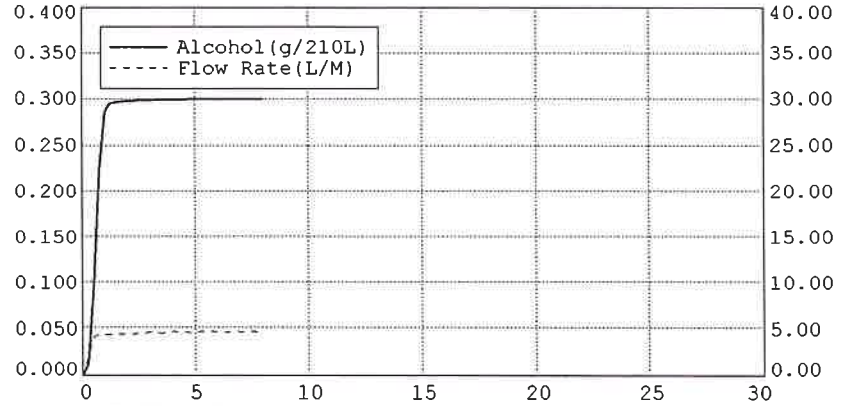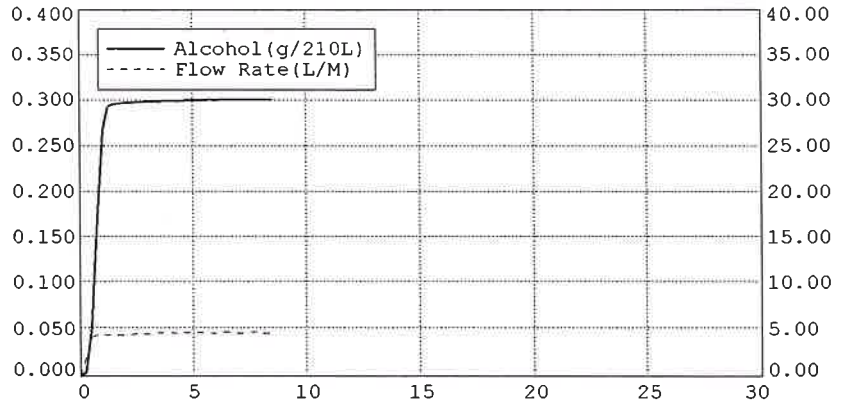



SUBJECT TEST

Alaska Department of Public Safety  
DATA MASTER dmt: 100390

Date: 11/03/2023  
Time: 10:16:53

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 10:18  
BLANK TEST 0.000 10:18  
INTERNAL STANDARD VERIFIED 10:18  
EXTERNAL STANDARD 0.079 10:18  
BLANK TEST 0.000 10:19  
SUBJECT SAMPLE INCOMPLETE 10:21

*DW*

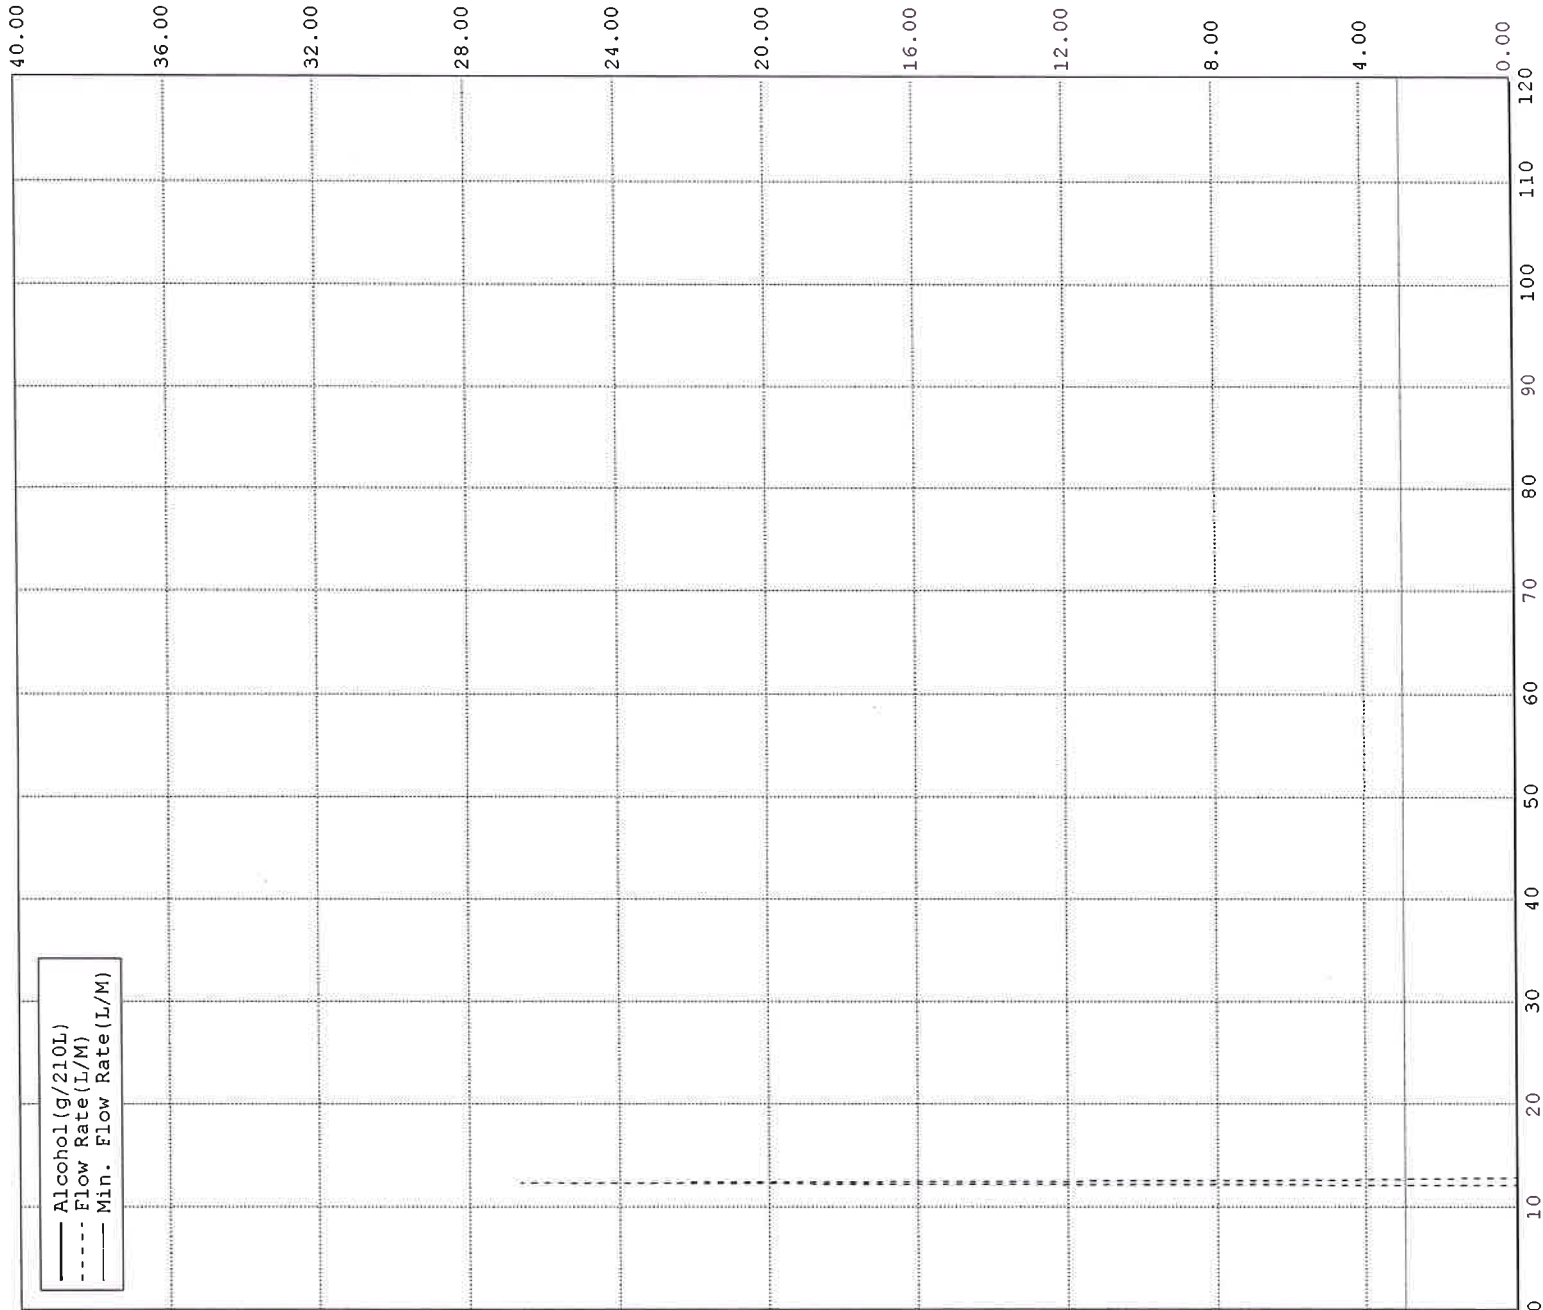

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100390

Date: 11/03/2023  
Time: 10:23:55

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
MAXIMUM ATTEMPTS  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.36: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK  
BLANK TEST PASSED 10:25  
INTERNAL STANDARD VERIFIED 10:25  
EXTERNAL STANDARD 0.080 10:25  
BLANK TEST 0.000 10:26  
SUBJECT SAMPLE XXX 10:27

Maximum Attempts Exceeded

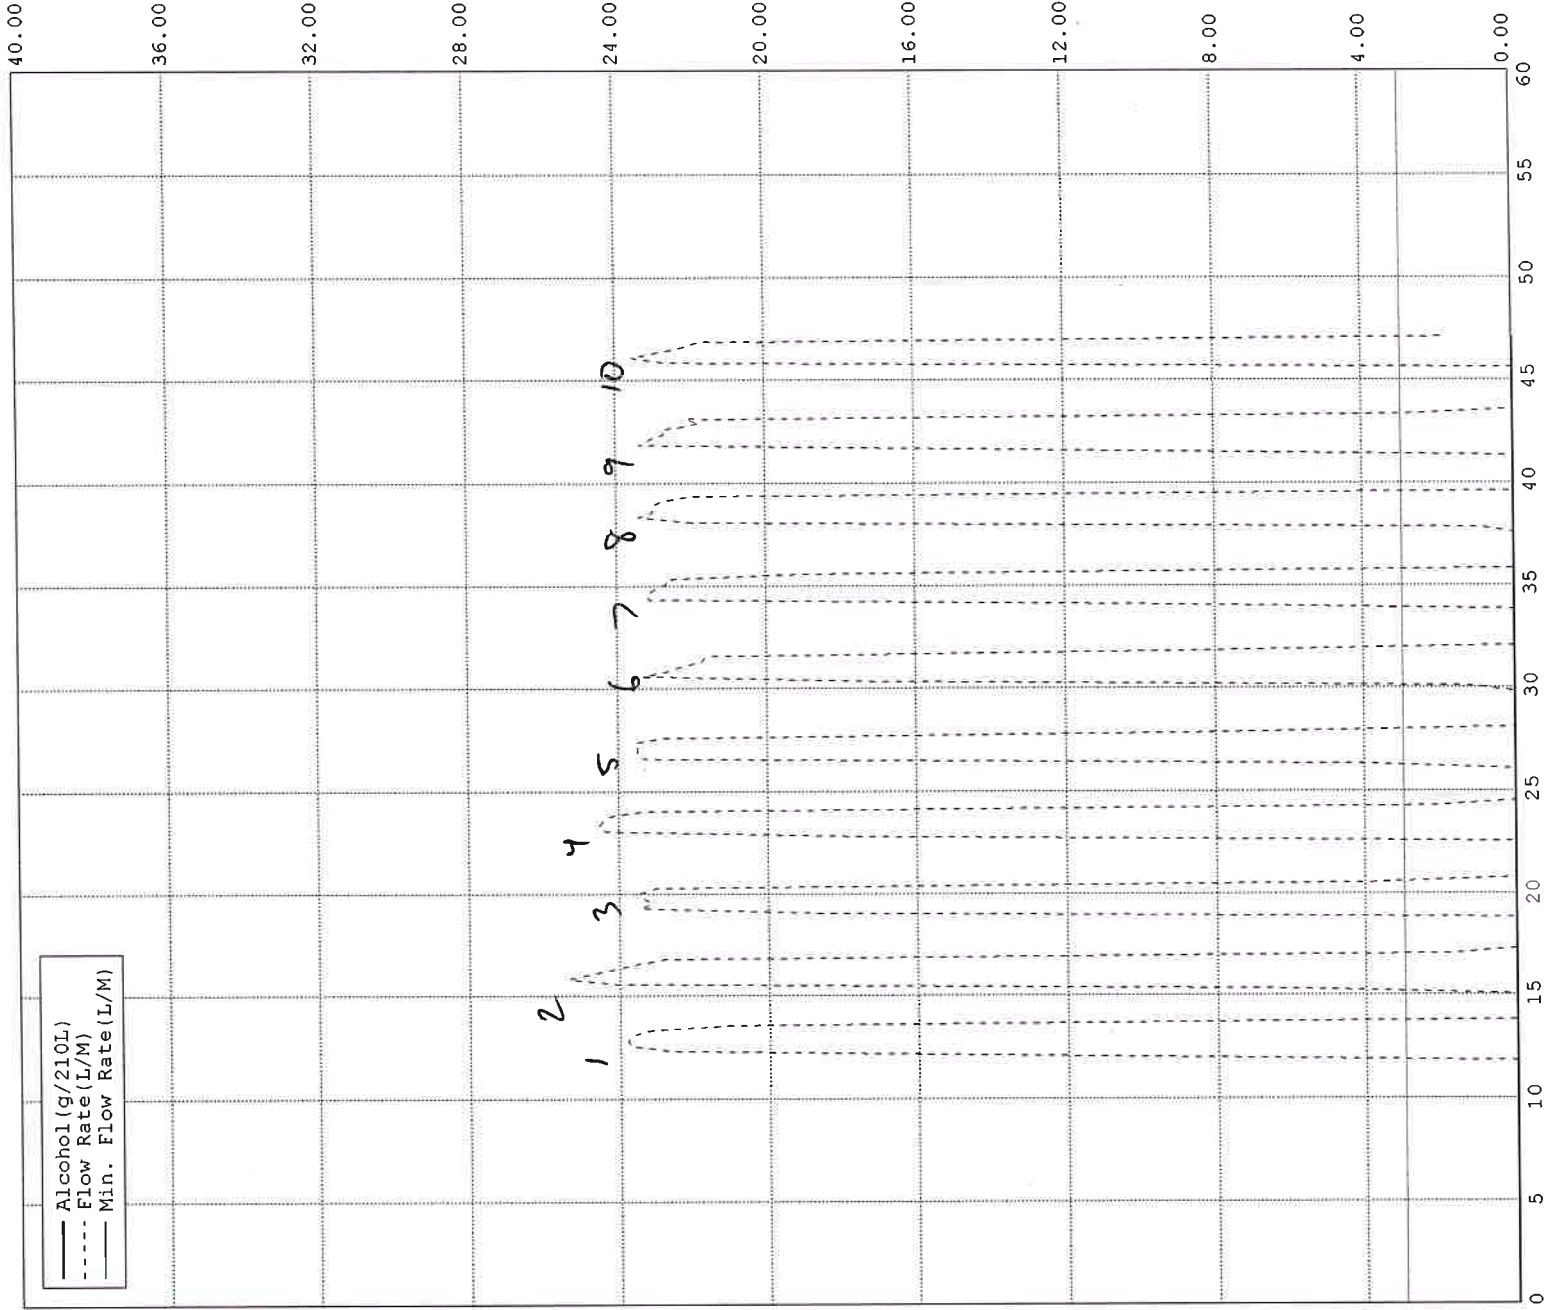



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100390

Date: 11/03/2023

Time: 10:29:00

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

DEREK WALTON

OPERATOR'S #: 9508

DEPT/AGENCY:

INVALID

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.36: 0.078

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

BLANK TEST


INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 10:30  
0.000 10:30  
VERIFIED 10:31  
0.080 10:31  
0.000 10:32  
INVALID 10:32

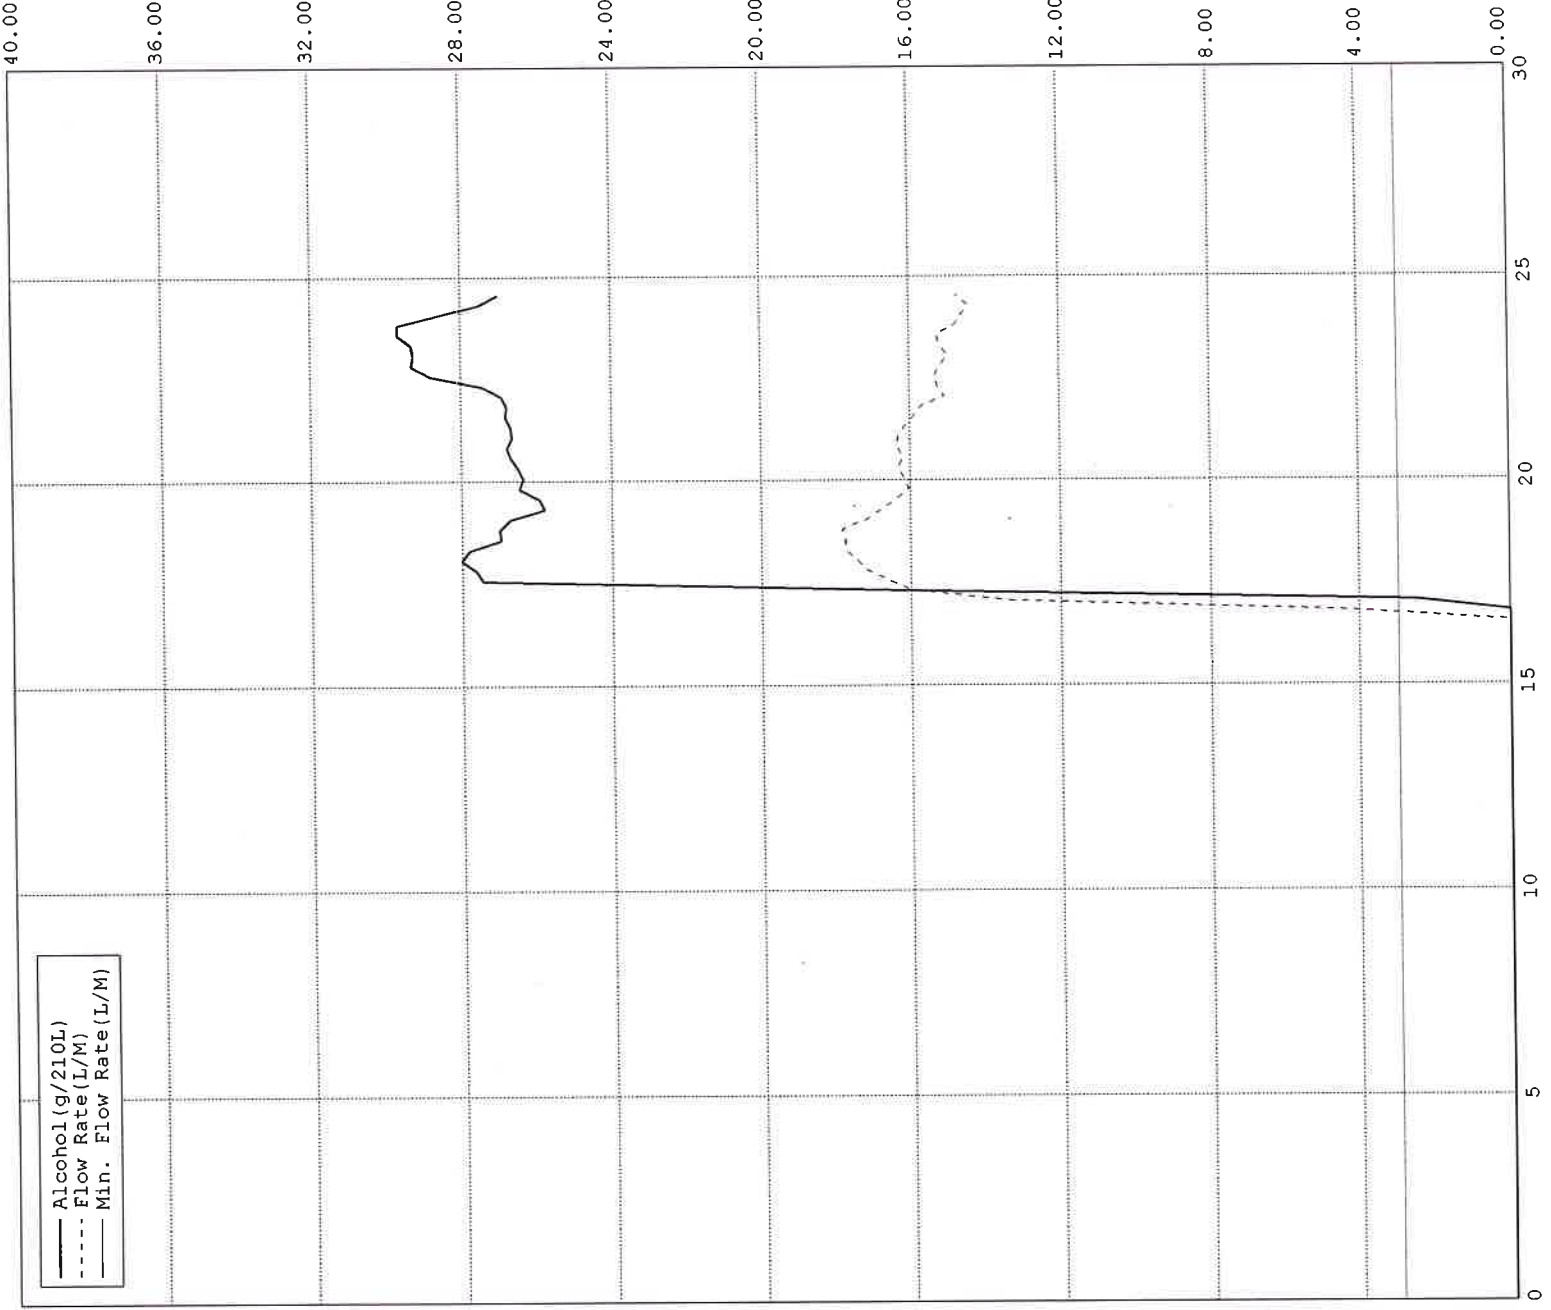

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100390

Date: 11/03/2023  
Time: 10:34:27

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508


DEPT/AGENCY:  
RADIO FREQUENCY  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.36: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 10:35  
BLANK TEST 0.000 10:35  
INTERNAL STANDARD VERIFIED 10:35  
EXTERNAL STANDARD 0.080 10:35  
BLANK TEST 0.000 10:36

RFI DETECTED

*DRW*

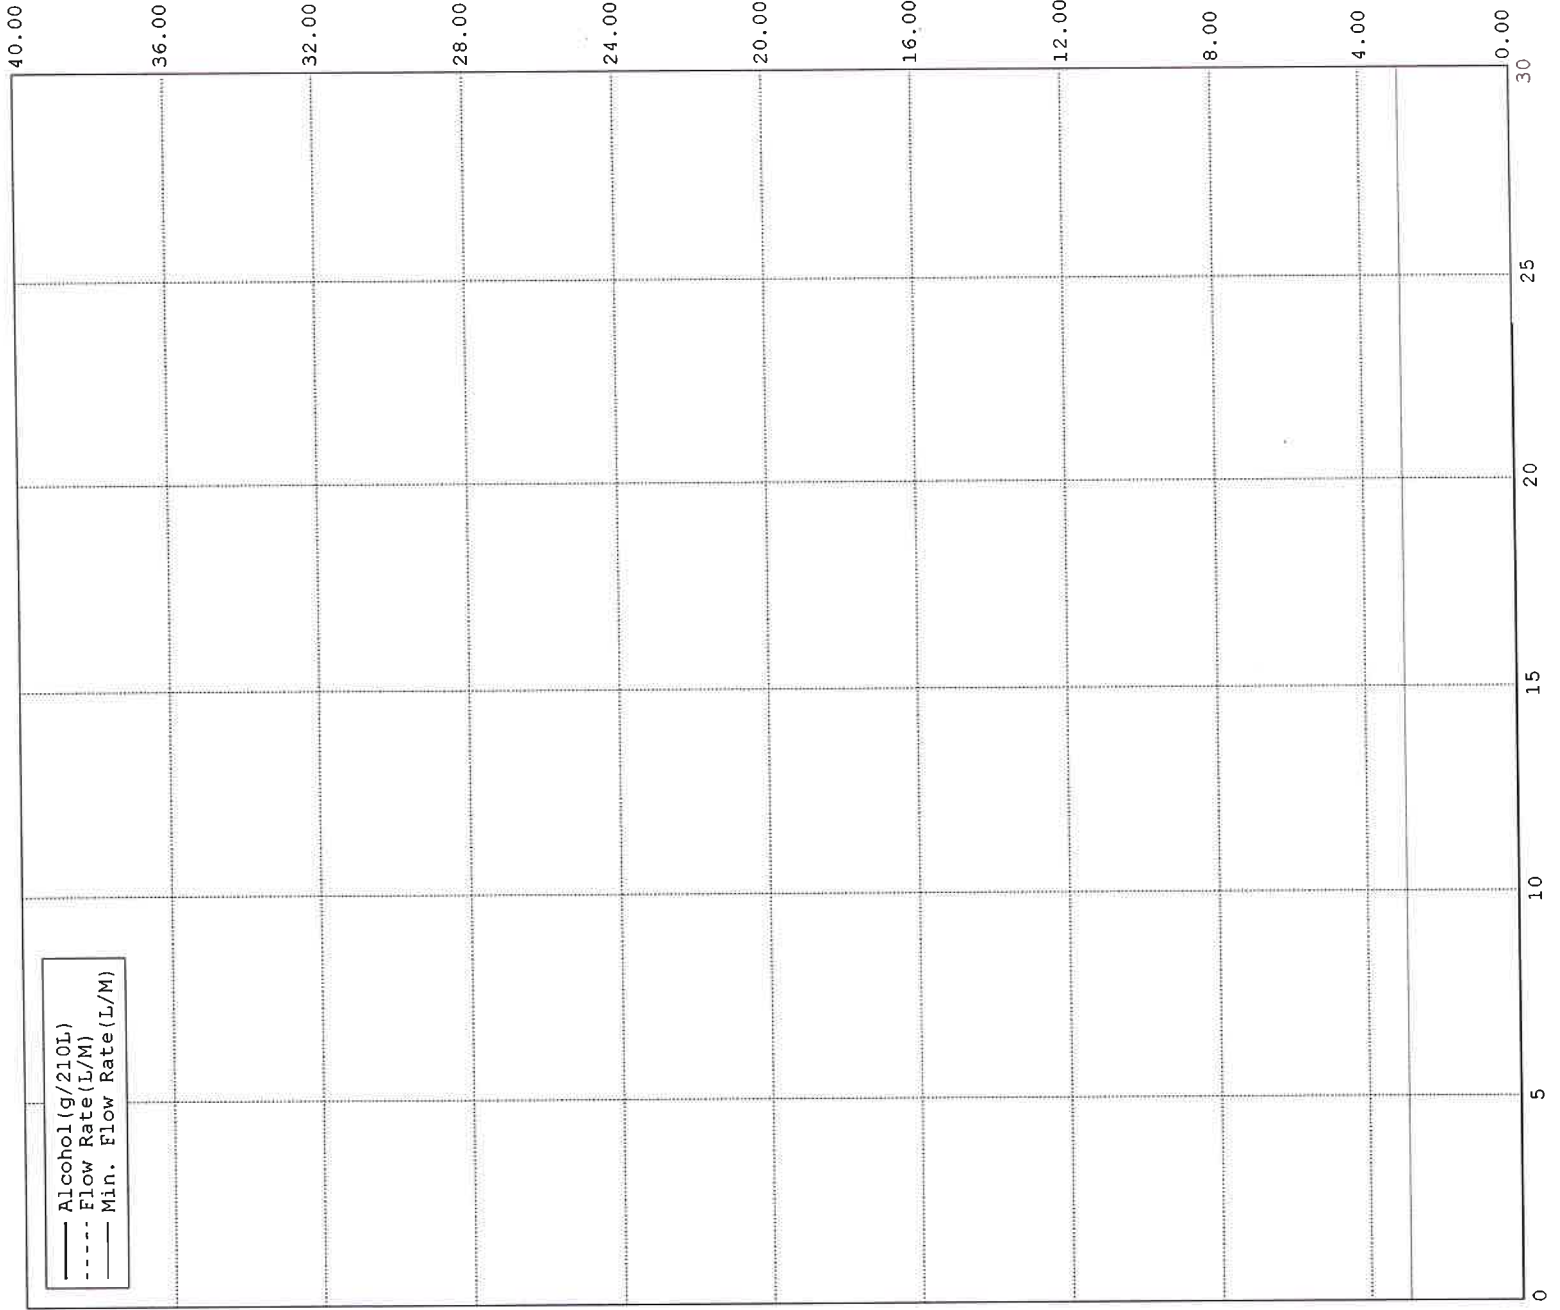

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100390

Date: 11/03/2023  
Time: 14:49:50

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
INTERFERENCE ACETONE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.36: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:50
BLANK TEST	0.000	14:50
INTERNAL STANDARD	VERIFIED	14:51
Xg = 0.097 (1.19%)		
EXTERNAL STANDARD	0.081	14:51
X[1] = 0.0805 (0.0010) (0.0009)		
BLANK TEST	0.000	14:52
SUBJECT SAMPLE	XXX	14:53
X[1] = 0.1118 (-0.0242) (0.0002)		


Interference Detected

Filter 2 average: 0.0006

Filter 3 average: 0.0020

DW 11/03/23

DW

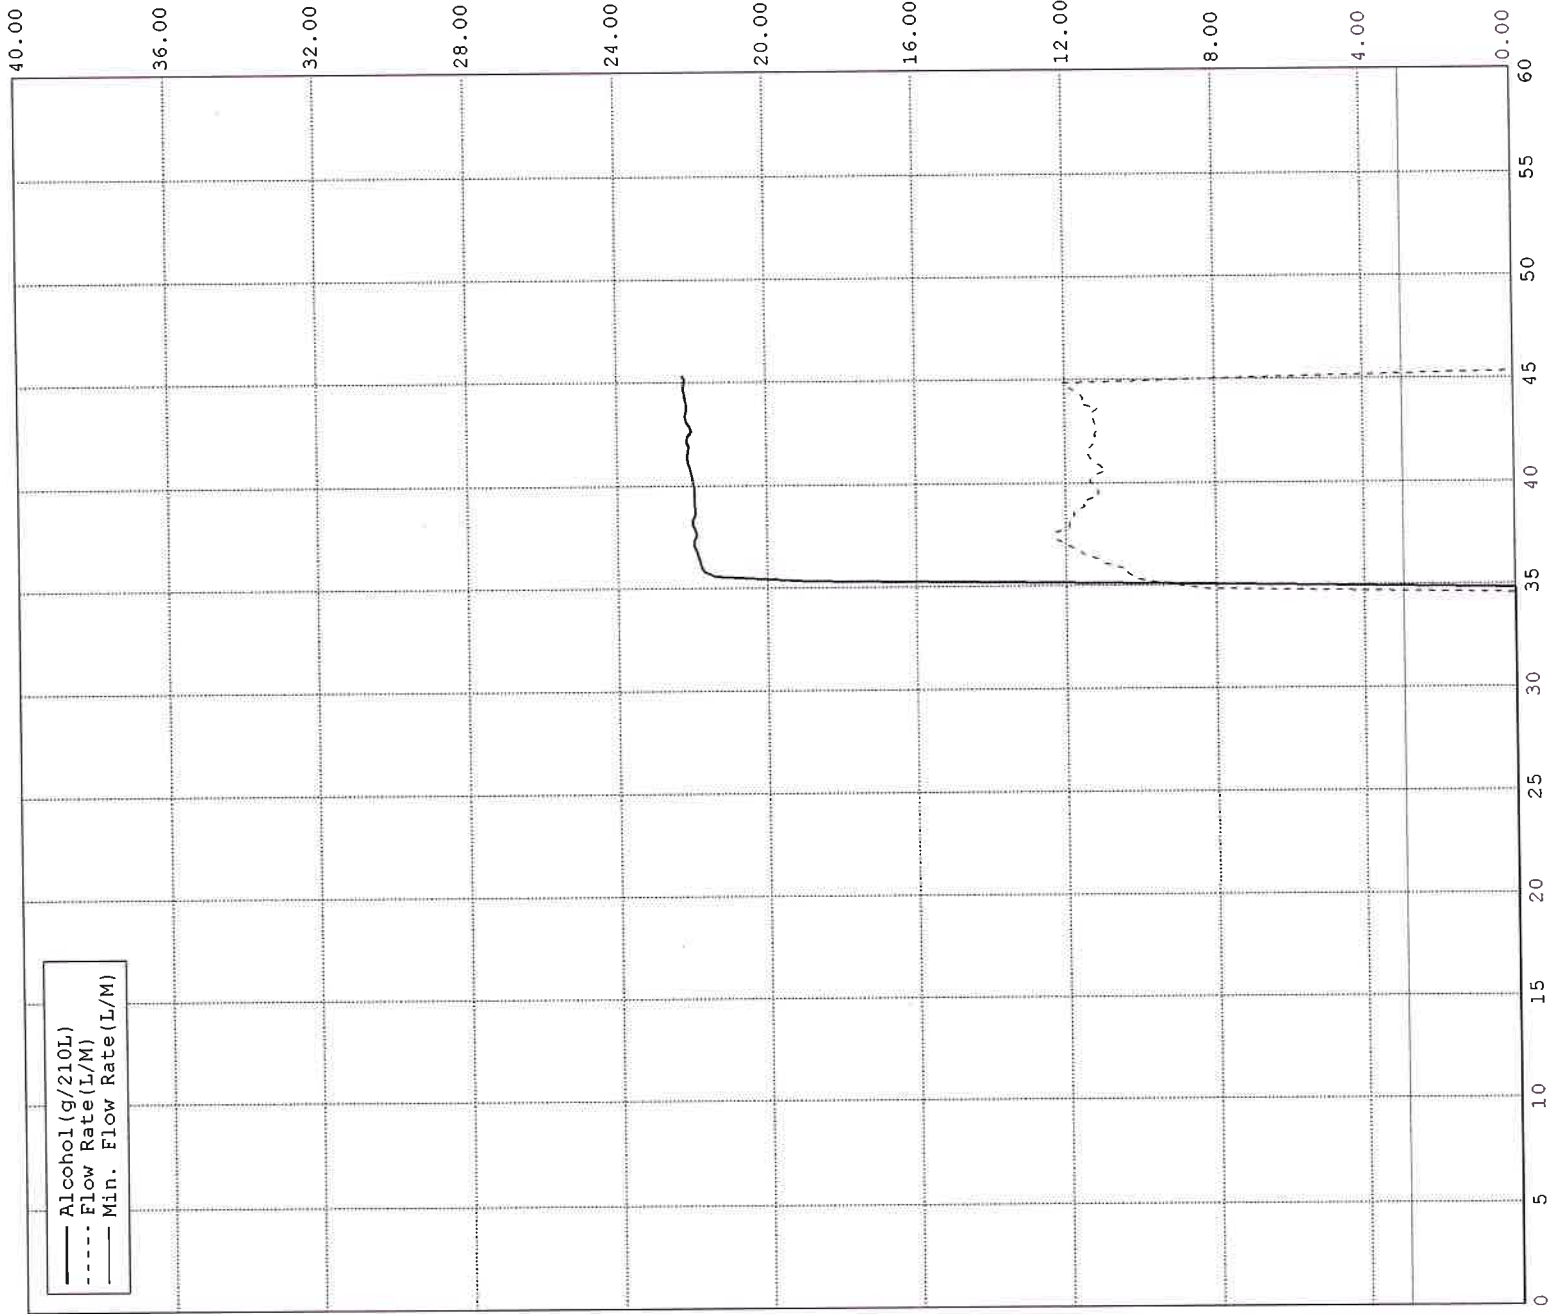

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100390

Date: 11/03/2023  
Time: 14:44:33

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
INTERFERENCE ISOPROPANOL  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 14:45  
BLANK TEST 0.000 14:45  
INTERNAL STANDARD VERIFIED 14:45  
Xq = 0.097 (1.37%) 0.079 14:46  
EXTERNAL STANDARD X[1] = 0.0795 (0.0004) (0.0026)  
BLANK TEST 0.000 14:47  
SUBJECT SAMPLE XXX 14:47  
X[1] = 0.1254 (-0.0346) (0.0013)

Interference Detected

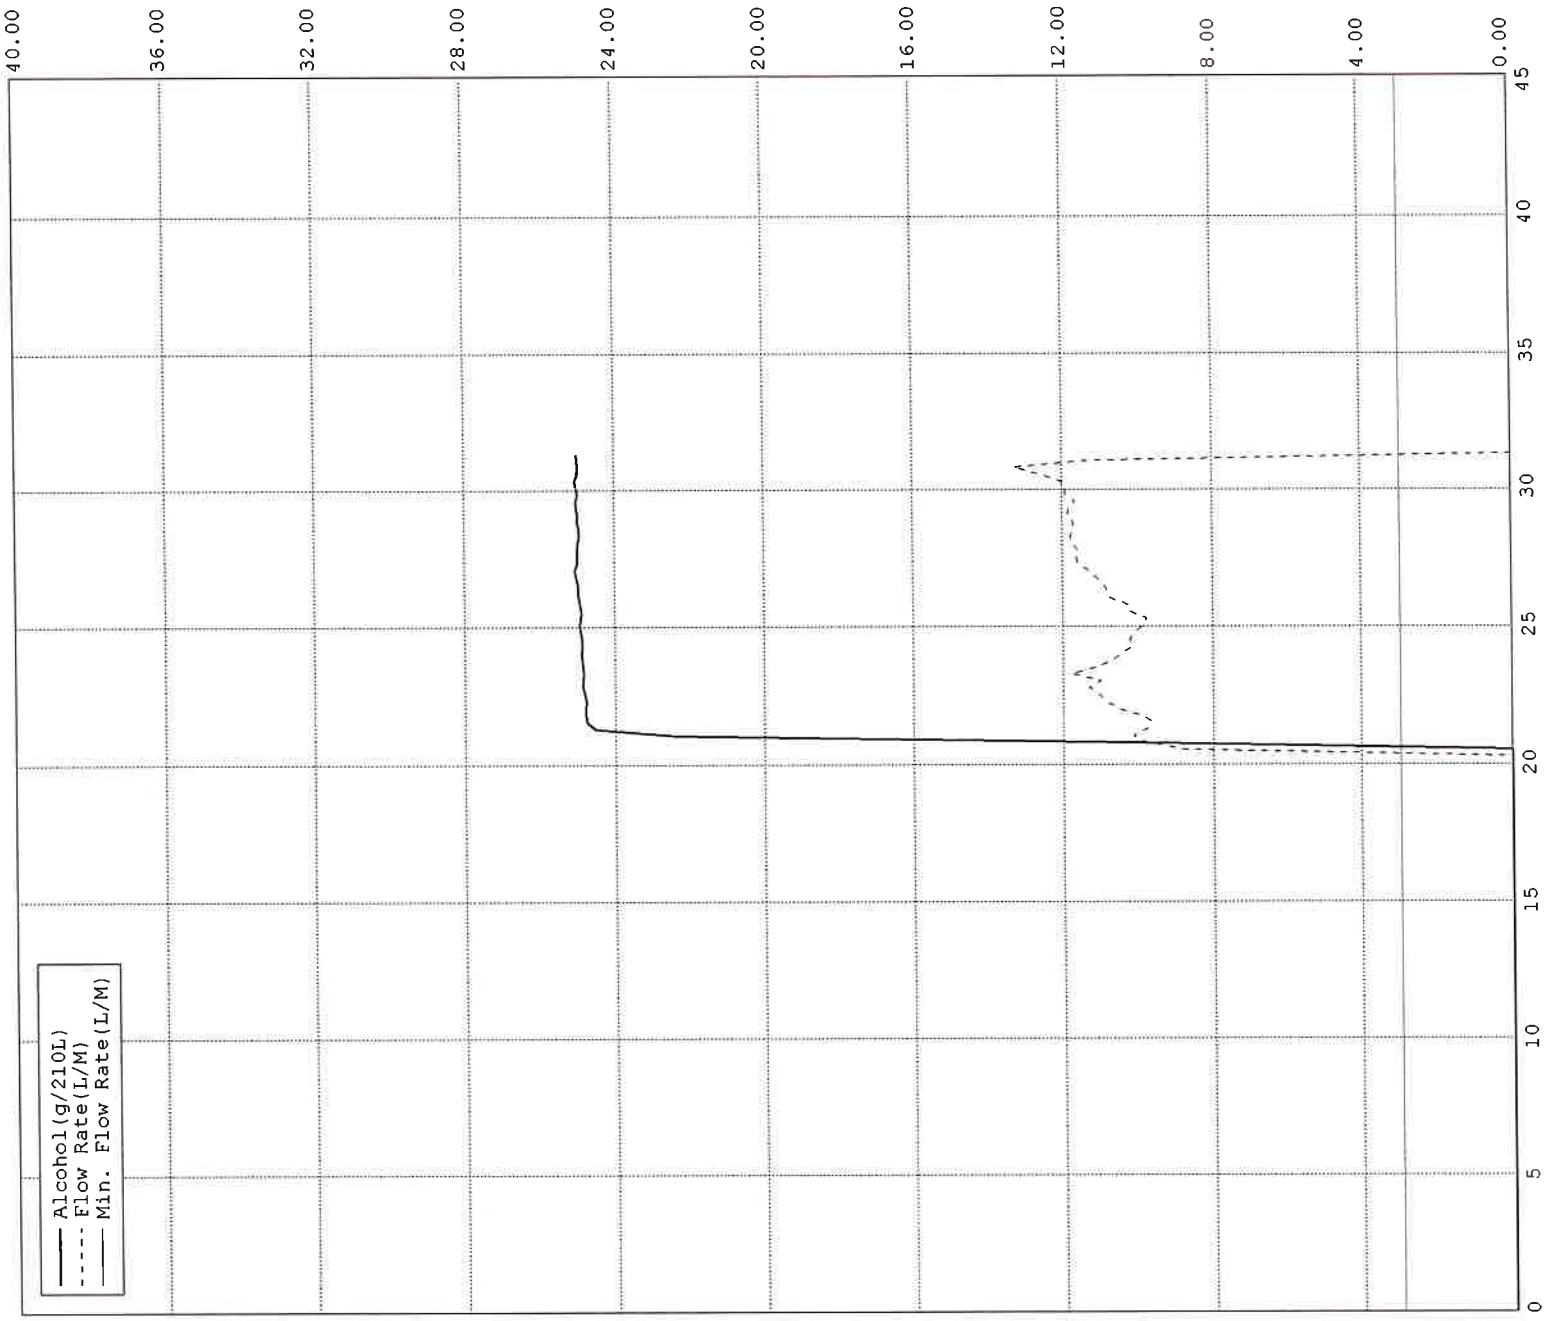

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100390

Date: 11/03/2023  
Time: 14:55:08

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508


DEPT/AGENCY:  
INTERFERENCE NEGATIVE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.36: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:56
BLANK TEST	0.000	14:56
INTERNAL STANDARD	VERIFIED	14:56
Xg = 0.097 (1.46%)		
EXTERNAL STANDARD	0.080	14:56
X[l] = 0.0801 (0.0010) (0.0021)		
BLANK TEST	0.000	14:57
SUBJECT SAMPLE (Vol=1.94L)	0.094	14:58
X[l] = 0.0940 (-0.0024) (0.0001)		
BLANK TEST	0.000	14:59
EXTERNAL STANDARD	0.079	14:59
X[l] = 0.0788 (0.0001) (0.0022)		
BLANK TEST	0.000	15:00

*DM*

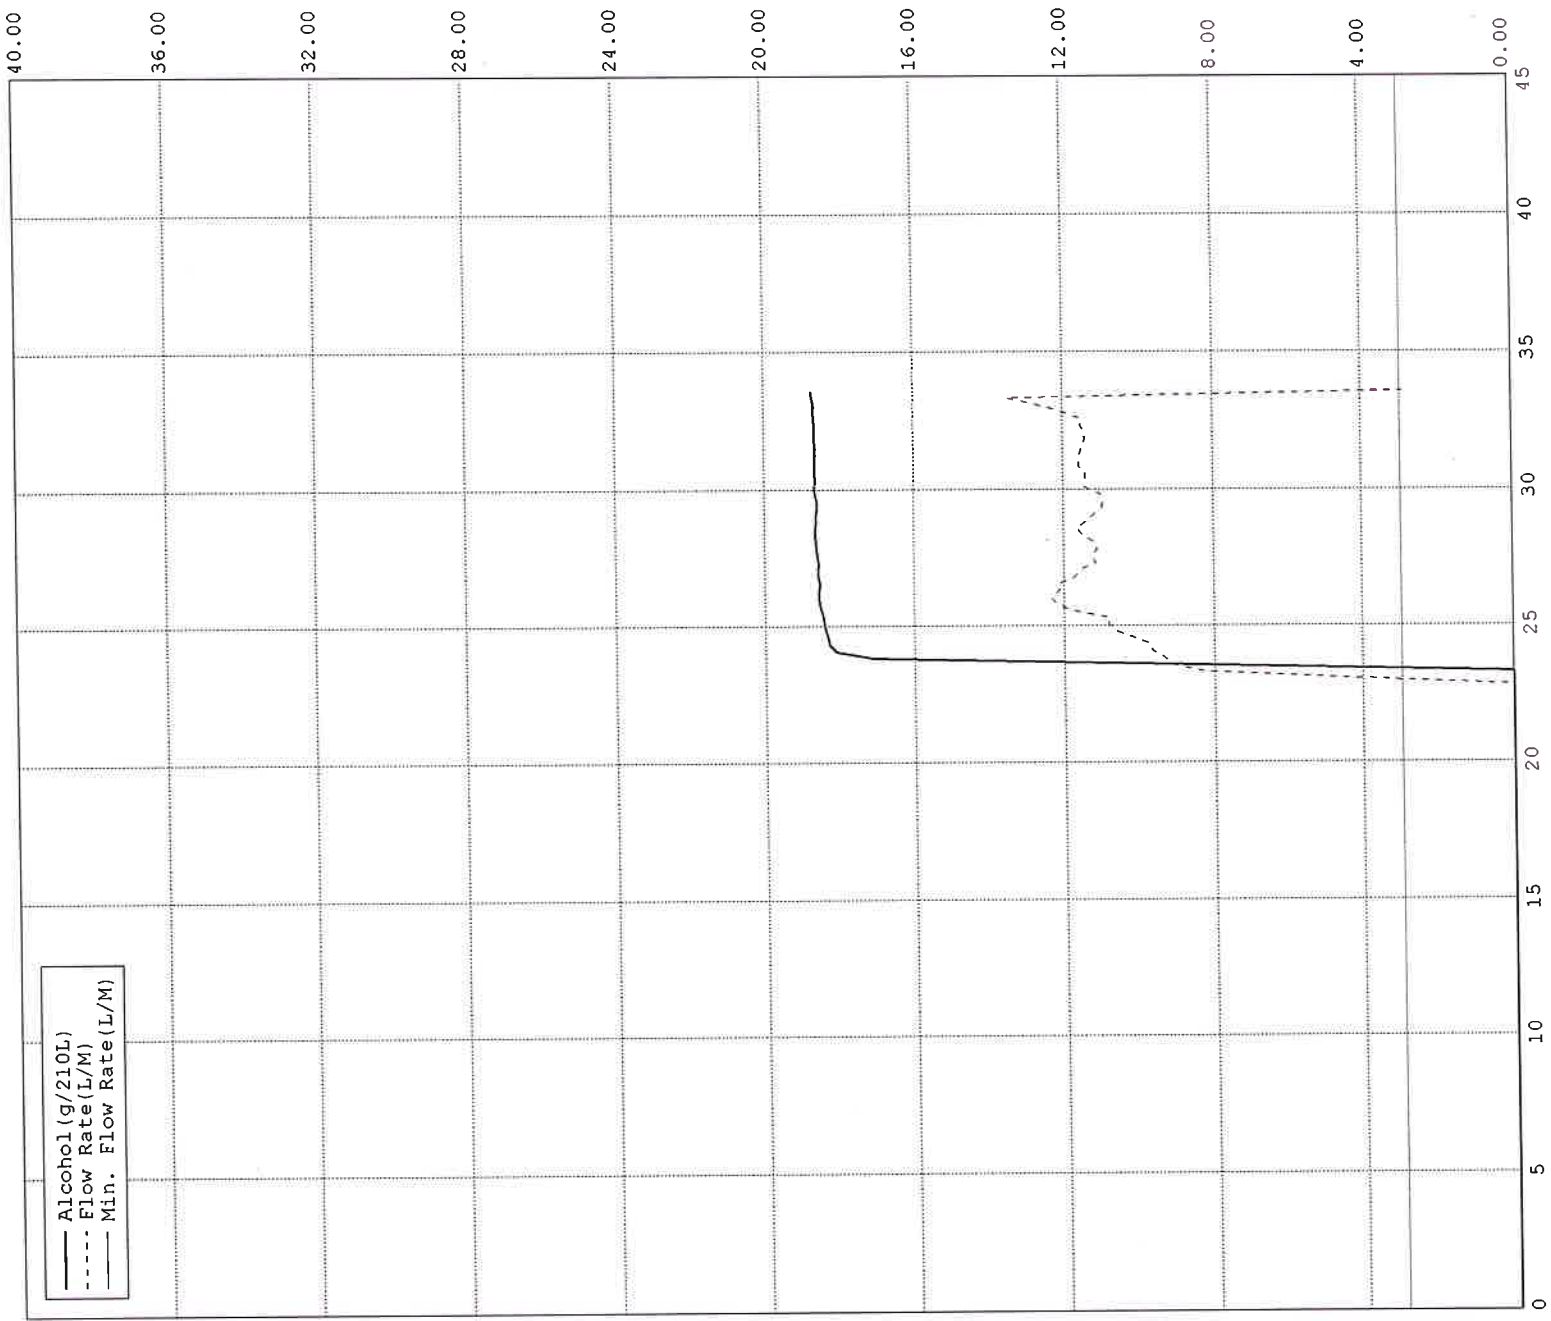



SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100390

Date: 11/03/2023

Time: 15:17:27

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

DEREK WALTON

OPERATOR'S #: 9508

DEPT/AGENCY:

NON-DRINKING SUBJECT

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.35: 0.078

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	15:18
BLANK TEST	0.000	15:18
INTERNAL STANDARD	VERIFIED	15:18
EXTERNAL STANDARD	0.079	15:18
BLANK TEST	0.000	15:19
SUBJECT SAMPLE (Vol=2.32L)	0.000	15:20
BLANK TEST	0.000	15:21
EXTERNAL STANDARD	0.080	15:21
BLANK TEST	0.000	15:22

*DW*

