

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 02/26/2015

Serial #: 100345

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 30.63: 0.082  
LOT #: 09214080A2  
EXPIRATION: 05/01/2016  
TANK PRESSURE: 993 psi

BLANK TEST	0.000	09:19
INTERNAL STANDARD	VERIFIED	09:19
EXTERNAL STANDARD	0.080	09:20
BLANK TEST	0.000	09:20
EXTERNAL STANDARD	0.080	09:21
BLANK TEST	0.000	09:22
EXTERNAL STANDARD	0.080	09:22
BLANK TEST	0.000	09:23
EXTERNAL STANDARD	0.080	09:23
BLANK TEST	0.000	09:24
EXTERNAL STANDARD	0.080	09:24
BLANK TEST	0.000	09:25

Average = 0.0800  
Std Dev = 0.0000

## Diagnostic Check

### VERSIONS

DMT: 3.00  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.8°C PASSED  
Breath Tube = 47.3°C PASSED

### PUMP INFO

Flow Rate = 5.079 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED


### FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED


INTERNAL STANDARD PASSED



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

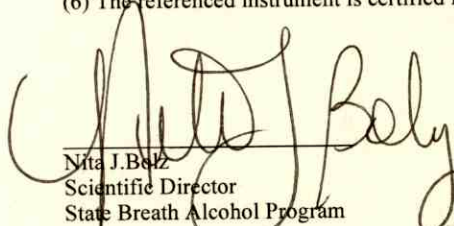 3/10/2015  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 10<sup>th</sup> day of Mar, 20 15

  
Nikki Roth, Notary Public  
My Commission Expires With Office

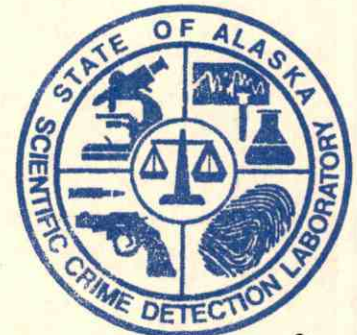

BMB  
3/2/15