



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100351

Report Issue Date: 12/27/2022
Date Received: Not Recorded
Condition of Item: Not Recorded

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

No As-Found Data Collected

Start Date 12/20/2022 - As Left - End Date 12/21/2022

As Left Conditions - Barometric Pressure (inHg): 30.06 Barometer Used: Fisher S/N 221250180 Temperature (C): 19.2 Relative Humidity (%): 4

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG111710	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.080	AG135004	0.080	0.079	0.080	0.079	0.079	0.079	+/- 0.003
0.100	0.100	AG211003	0.100	0.100	0.100	0.100	0.100	0.100	+/- 0.003
0.150	0.151	AG134205	0.150	0.150	0.151	0.150	0.151	0.150	+/- 0.004
0.300	0.301	AG130502	0.300	0.298	0.299	0.299	0.299	0.299	+/- 0.008

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Technically and administratively reviewed by Colleen O'Bryant on 12/27/2022

Brandi M Barnett

Results authorized by Brandi Barnett on 12/27/2022
brandi.barnett@alaska.gov

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100351 Analyst: Brandi Barnett Start Date: 12/20/22

- Diagnostic Test (attached)
- Adjust voltages, if needed
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Internal Standard value \leq 3.00%
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.6 L (1.3L to 1.7L)

As Left Conditions: 221250180 exp: 2/14/24 Barometer BMB 12/20/22

Barometric Pressure (in Hg): 30.06 Temperature (C): 19.2 Relative Humidity (%) 4

Linearity Test (attached)

0.020g/210L Mnf: <u>Airgas</u>	Lot: <u>AG 217902</u>	Exp: <u>6/28/24</u>
0.040g/210L Mnf: <u>Airgas</u>	Lot: <u>AG 100401</u> ^{BMB} _{12/20/22}	Exp: <u>1/4/23</u> ^{ONE} _{12/20/22}
0.080g/210L Mnf: <u>Airgas</u>	Lot: <u>AG111710</u>	Exp: <u>4/27/23</u>
0.100g/210L Mnf: <u>Airgas</u>	Lot: <u>AG135004</u>	Exp: <u>12/16/23</u>
0.150g/210L Mnf: <u>Airgas</u>	Lot: <u>AG 211003</u>	Exp: <u>4/20/24</u>
0.300g/210L Mnf: <u>Airgas</u>	Lot: <u>AG134205</u>	Exp: <u>12/08/23</u>
0.300g/210L Mnf: <u>Airgas</u>	Lot: <u>AG130502</u>	Exp: <u>11/01/23</u>

Functional Tests (attached)

- Incomplete
- Maximum Attempts Exceeded
- Interference (Volatiles)
- Invalid
- Radio Frequency Interference (RFI)

Acetone Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: DR5298 Verification Performed?

Isopropanol Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: SD1198 Verification Performed?

Neg. Control Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: SD1202 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/09/23

- Verify stylus is calibrated
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Non-Drinking Subject Test
- Upload
- Remove Tank Prior to Shutdown

Calibration End Date: 12/21/22

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: ~~12/23/2022~~ 12/20/2022 BWS
Time: 07:50:55

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.0°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 45.4°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.87 V PASSED
(1.15 V - 2.69 V)
Cooler Voltage = 1.83 V PASSED
(1.12 V - 2.60 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 528 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 30.1 in

PUMP INFO

Flow Rate = 5.288 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.001 V <= 0.010 V)
PUMP OFF PASSED
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.121 0.66% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100351

Date: ~~12/23/2022~~ 12/20/2022 *BMB*
Time: 7:58 AM

Temperatures (°C)
Sample Cell: 48.5°C
Breath Tube: 44.5°C

Current Barometer 30.1 in
Volume (Ltr) 1.46

Settings
Lamp: 1.87 V
Bias: 80 V
Cooler: 1.78 V
Chopper: 521 Hz

Voltages (V)
Flow: 1.04 V
Detector: -0.068 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: 03/18/2020
Time: 08:09:54

OPERATOR NAME:
INTOX I METERS
CERTIFICATE #: 1

Ca = 0.2000
CAL = 0.975058 0.800 <= CAL < 1.200
b1 = 0.0006 0.0000 <= b1 < 0.0040
b2 = 0.0055 0.0010 <= b2 < 0.0100
b3 = 0.0008 0.0000 <= b3 < 0.0040
Xq = 0.1217 0.0500 <= Xq < 0.2000
a21 = 1.157872 1.050 <= a21 < 1.300
a31 = 0.464353 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: 12/20/2022
Time: 08:11:48


SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
BRANDI BARNETT
OPERATOR'S #: 7038

DEPT/AGENCY:
MINIMUM VOLUME
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.06: 0.080
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	08:12
BLANK TEST	0.000	08:12
INTERNAL STANDARD	VERIFIED	08:13
EXTERNAL STANDARD	0.079	08:13
BLANK TEST	0.000	08:14
SUBJECT SAMPLE (Vol=1.61L)	0.000	08:15
BLANK TEST	0.000	08:16
EXTERNAL STANDARD	0.080	08:16
BLANK TEST	0.000	08:17

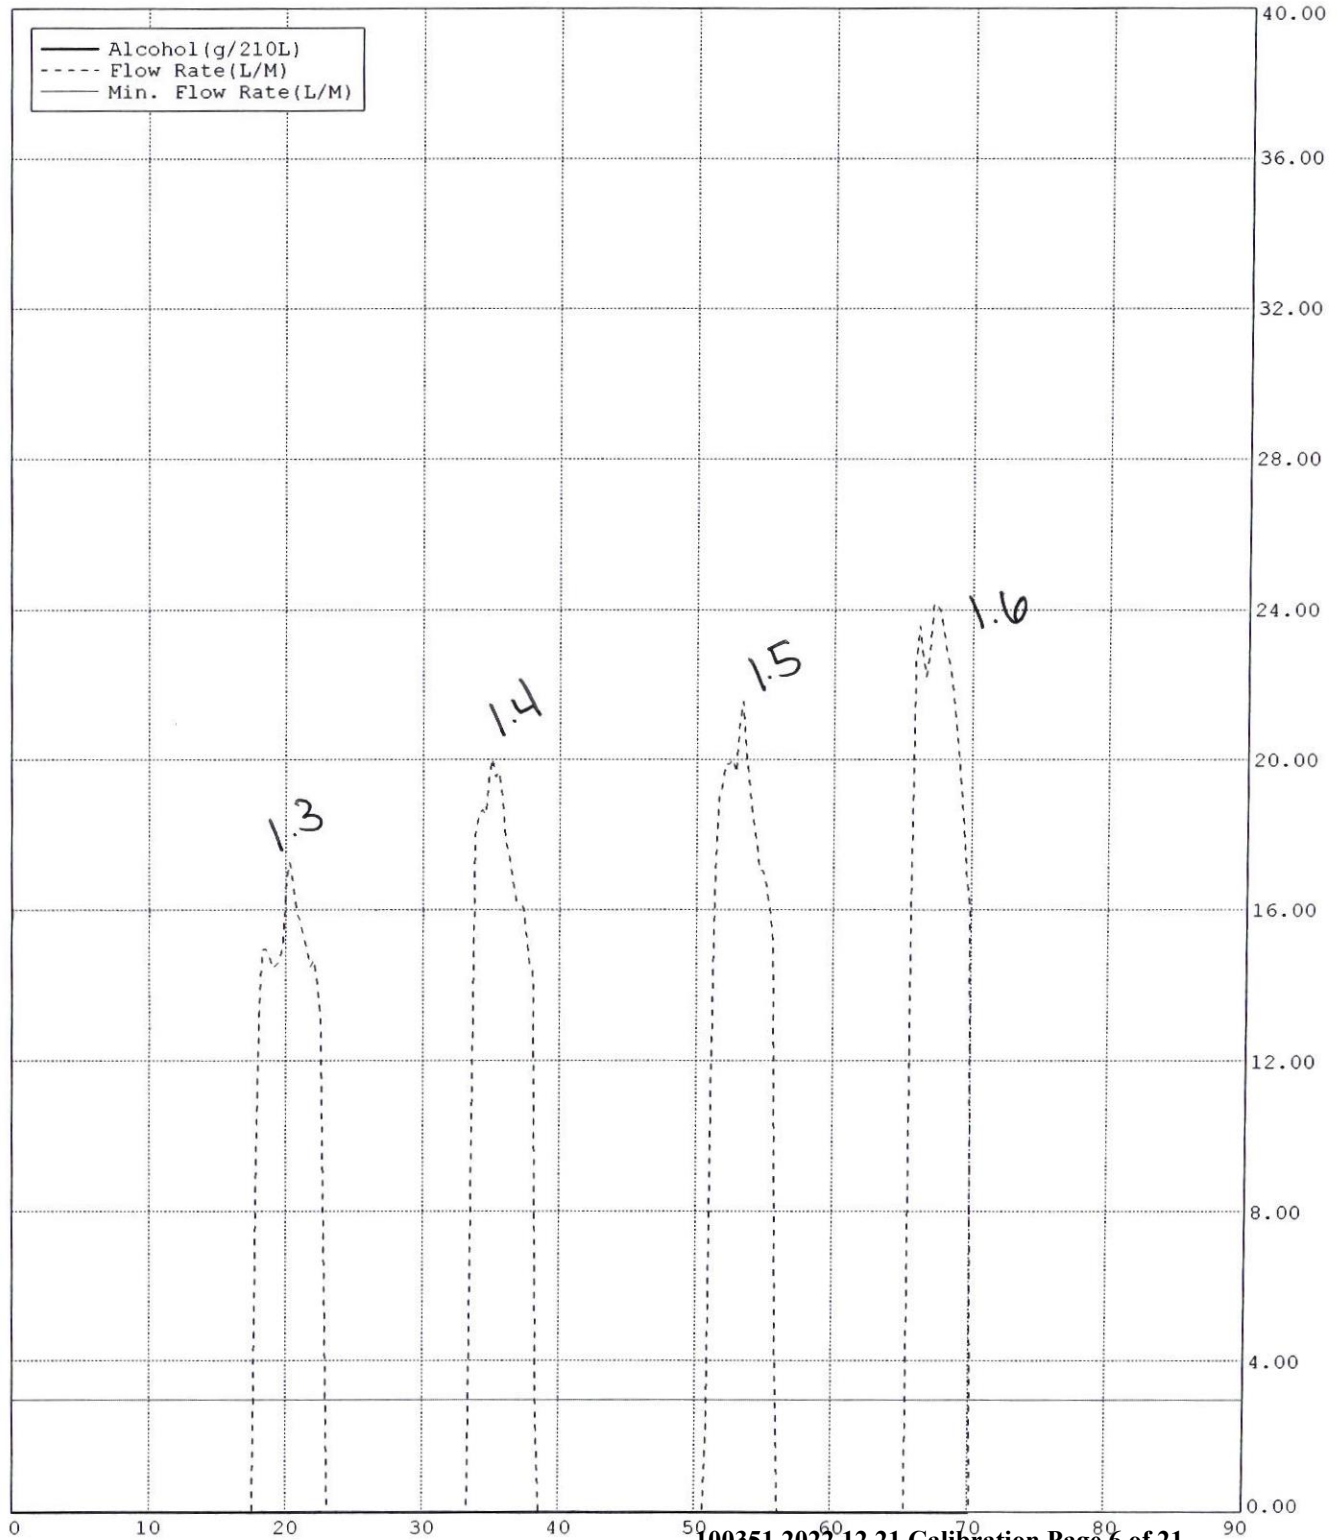

LINEARITY CHECK

Alaska Department of Public Safety
DATAMASTER dmt: 100351


Date: 12/20/2022
Time: 08:24:50

SUPERVISOR NAME:
BRANDI BARNETT
OPERATOR'S #: 7038

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.040	0.0400	0.0000
0.080	0.0794	0.0005
0.100	0.1000	0.0000
0.151	0.1504	0.0005
0.301	0.2990	0.0007

SLOPE = 0.992854
R² = 0.999993

BBB

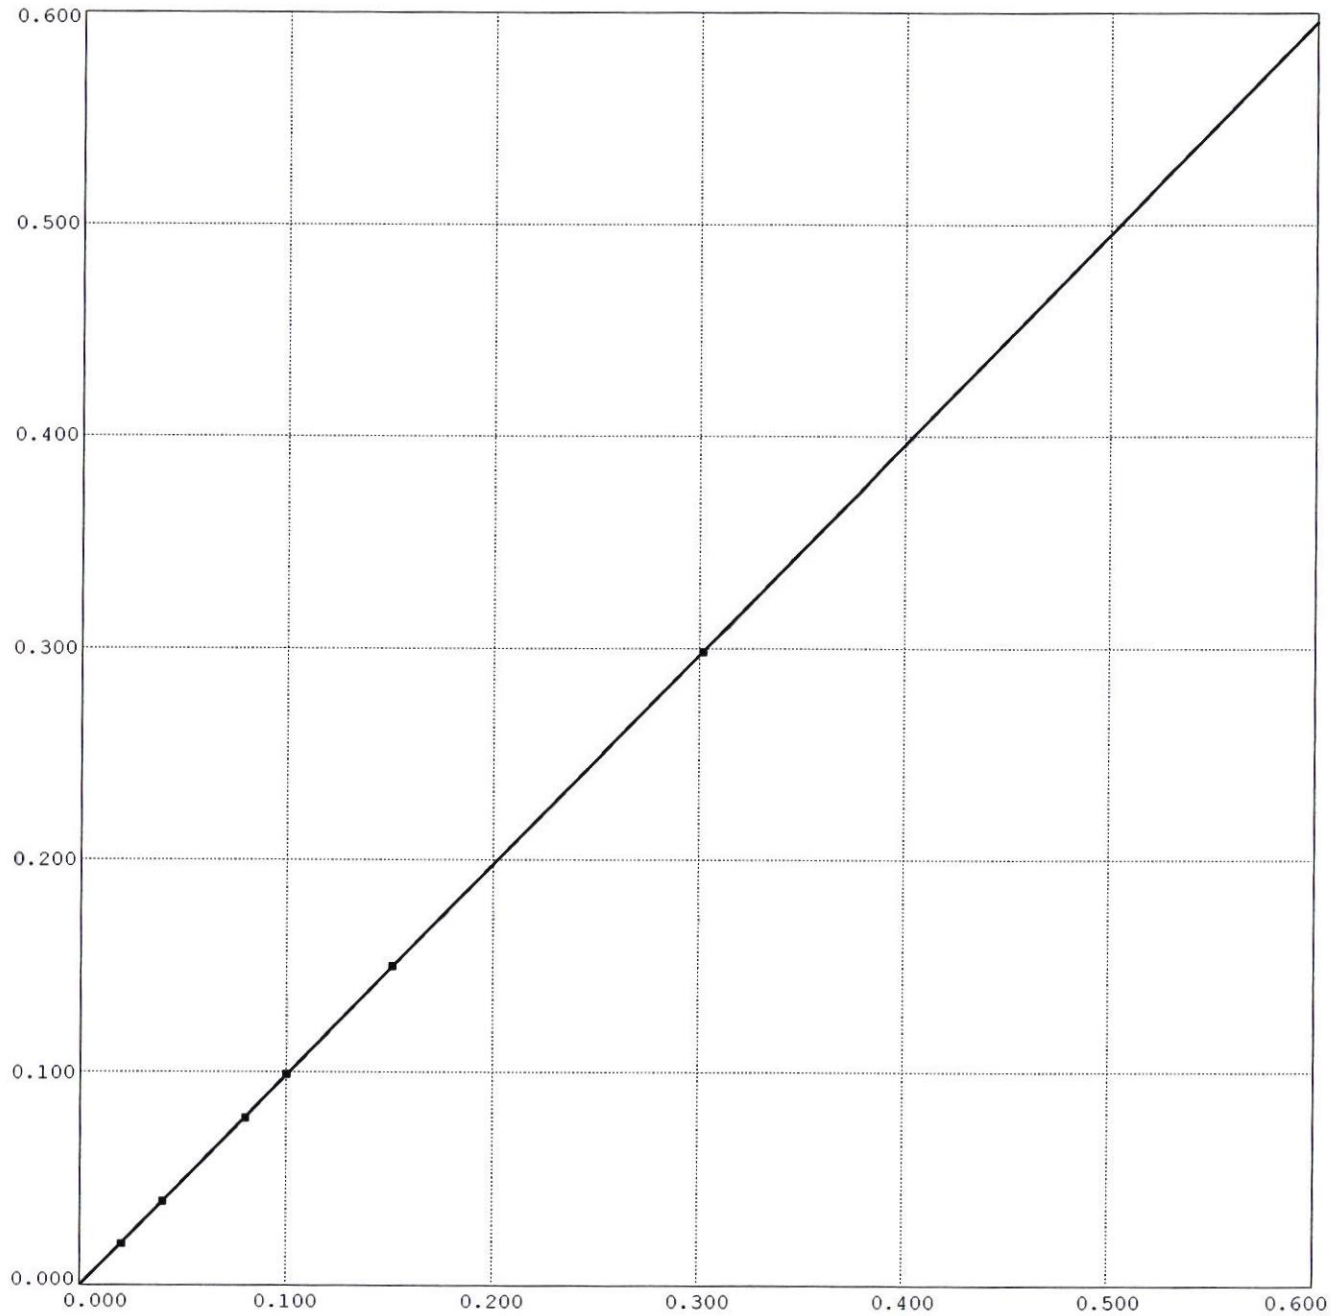

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100351






Date: 12/20/2022
 Time: 08:37:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 30.06: 0.020
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 1079 psi

BLANK TEST	0.000	08:39
INTERNAL STANDARD	VERIFIED	08:39
EXTERNAL STANDARD	0.020	08:39
BLANK TEST	0.000	08:40
EXTERNAL STANDARD	0.020	08:40
BLANK TEST	0.000	08:41
EXTERNAL STANDARD	0.020	08:41
BLANK TEST	0.000	08:42
EXTERNAL STANDARD	0.020	08:42
BLANK TEST	0.000	08:43
EXTERNAL STANDARD	0.020	08:43
BLANK TEST	0.000	08:44

Average = 0.0200
 Std Dev = 0.0000

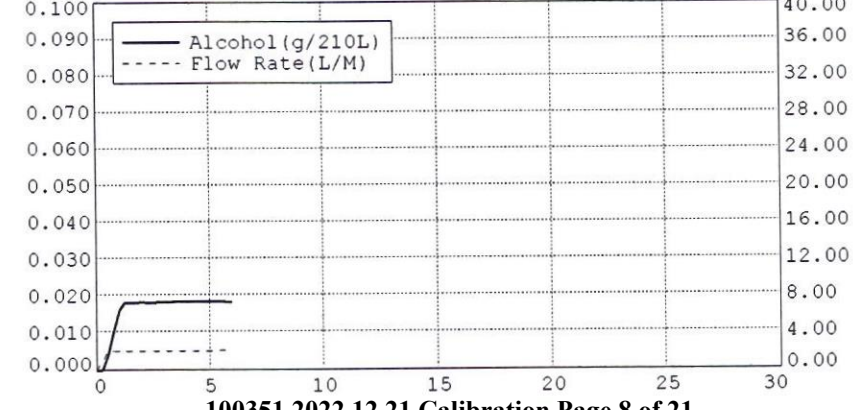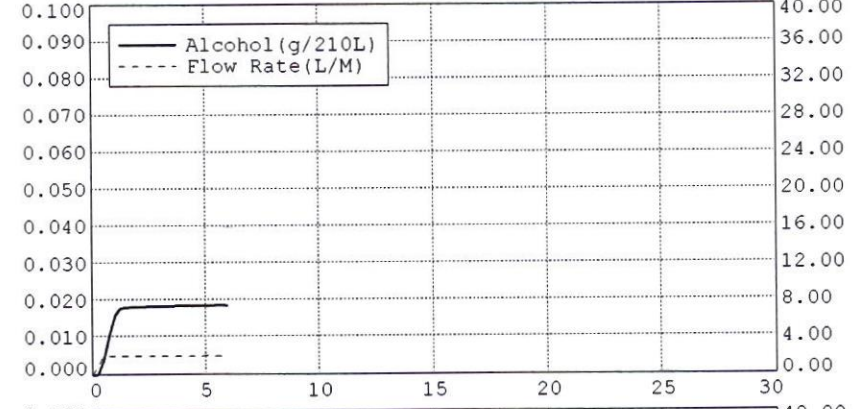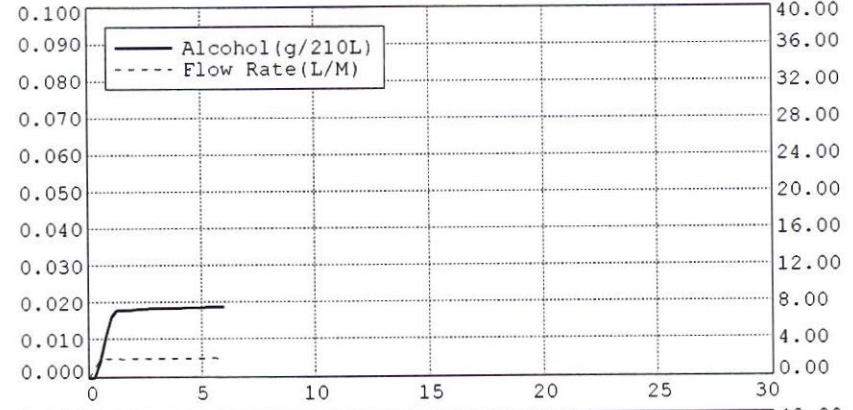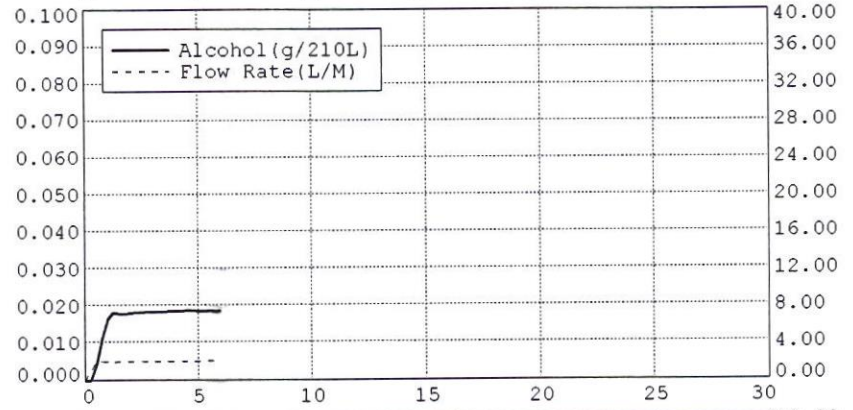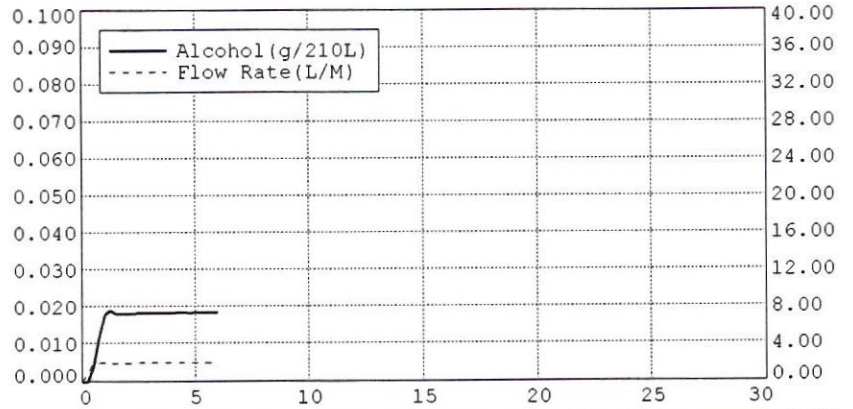

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100351






Date: 12/20/2022
 Time: 08:46:35

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 30.06: 0.040
 LOT #: AG111710
 EXPIRATION: 04/27/2023
 TANK PRESSURE: 373 psi

BLANK TEST	0.000	08:47
INTERNAL STANDARD	VERIFIED	08:47
EXTERNAL STANDARD	0.040	08:48
BLANK TEST	0.000	08:48
EXTERNAL STANDARD	0.040	08:49
BLANK TEST	0.000	08:50
EXTERNAL STANDARD	0.040	08:50
BLANK TEST	0.000	08:51
EXTERNAL STANDARD	0.040	08:51
BLANK TEST	0.000	08:52
EXTERNAL STANDARD	0.040	08:52
BLANK TEST	0.000	08:53

Average = 0.0400
 Std Dev = 0.0000

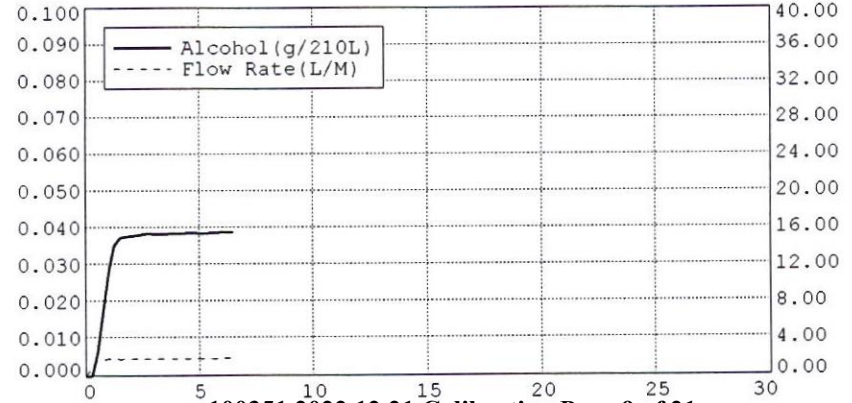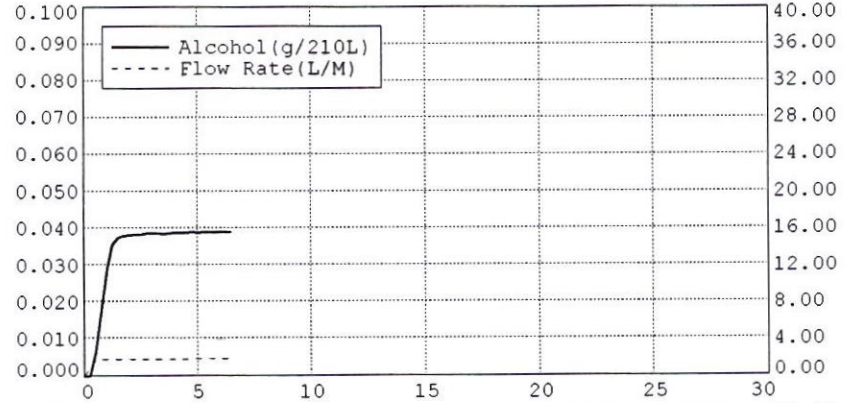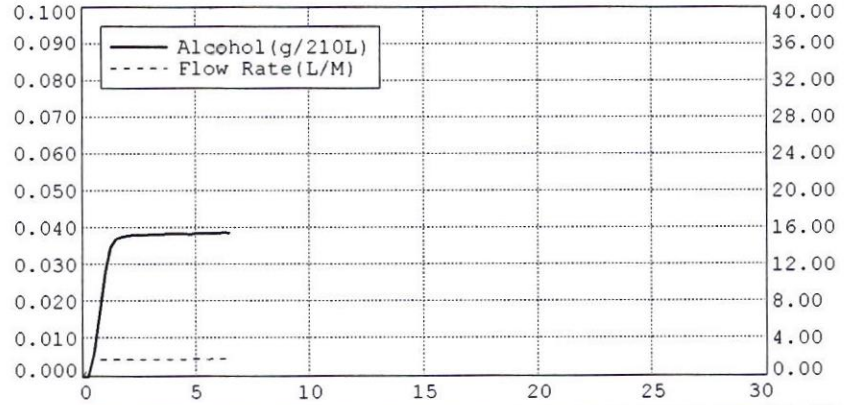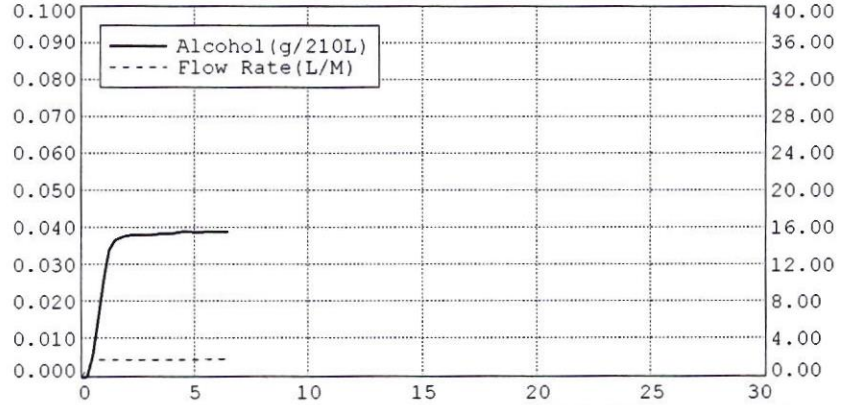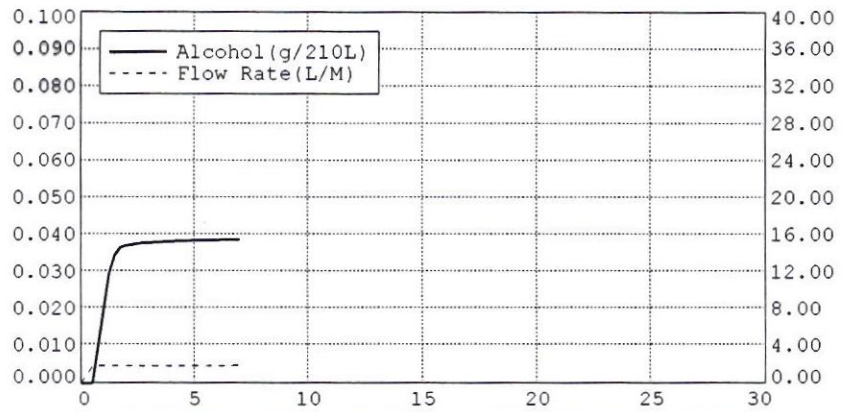

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100351






Date: 12/20/2022
 Time: 08:55:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 30.07: 0.080
 LOT #: AG135004
 EXPIRATION: 12/16/2023
 TANK PRESSURE: 1077 psi

BLANK TEST	0.000	08:57
INTERNAL STANDARD	VERIFIED	08:57
EXTERNAL STANDARD	0.080	08:57
BLANK TEST	0.000	08:58
EXTERNAL STANDARD	0.079	08:58
BLANK TEST	0.000	08:59
EXTERNAL STANDARD	0.080	08:59
BLANK TEST	0.000	09:00
EXTERNAL STANDARD	0.079	09:00
BLANK TEST	0.000	09:01
EXTERNAL STANDARD	0.079	09:01
BLANK TEST	0.000	09:02

Average = 0.0794
 Std Dev = 0.0005

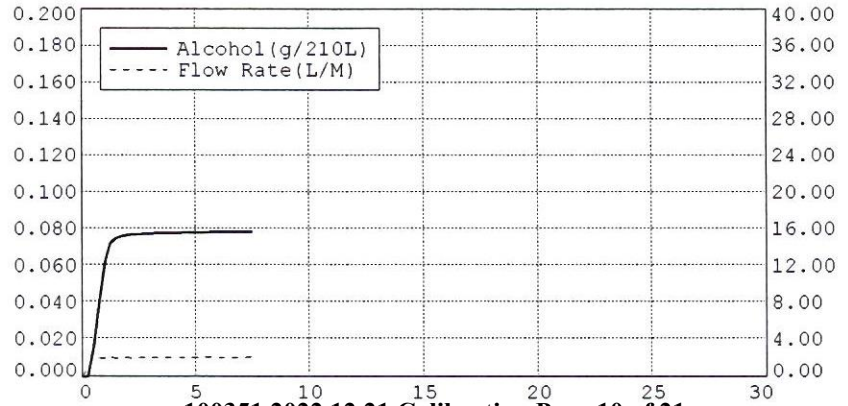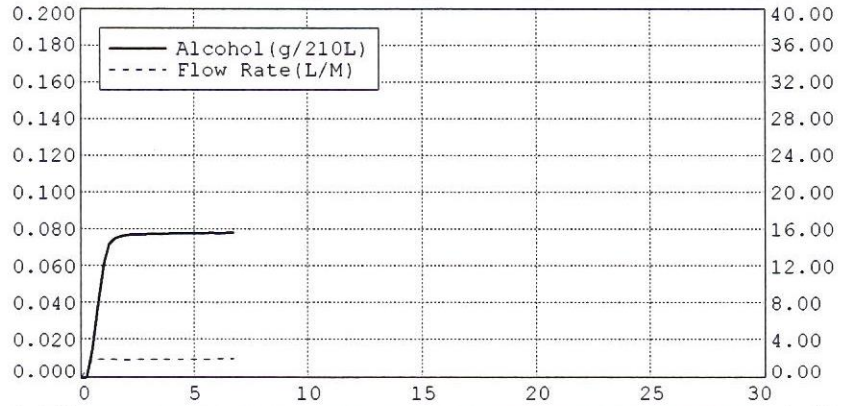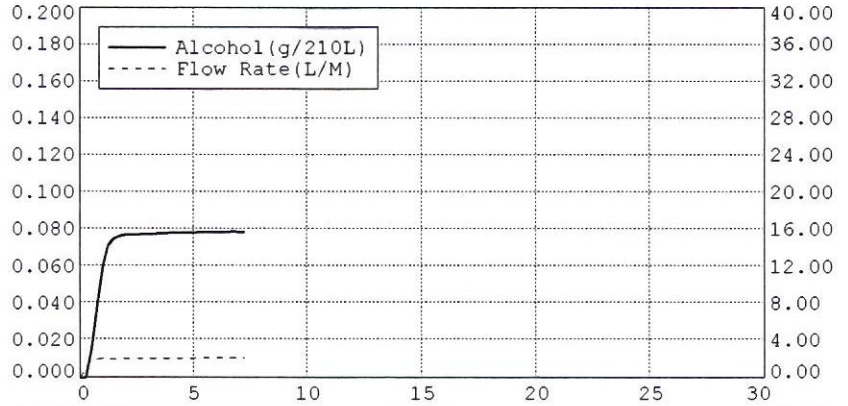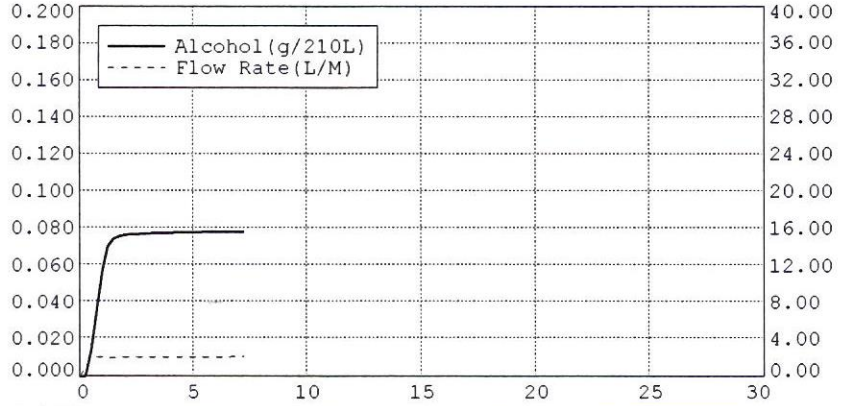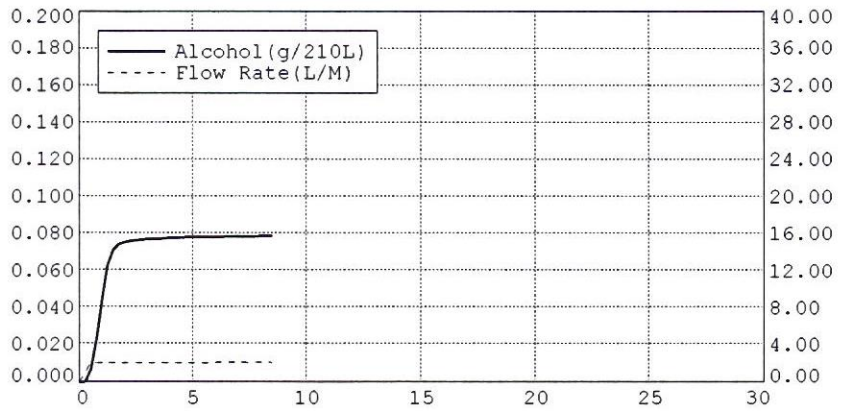

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100351






Date: 12/20/2022
 Time: 09:06:09

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 30.07: 0.100
 LOT #: AG211003
 EXPIRATION: 04/20/2024
 TANK PRESSURE: 1034 psi

BLANK TEST	0.000	09:07
INTERNAL STANDARD	VERIFIED	09:07
EXTERNAL STANDARD	0.100	09:07
BLANK TEST	0.000	09:08
EXTERNAL STANDARD	0.100	09:08
BLANK TEST	0.000	09:09
EXTERNAL STANDARD	0.100	09:09
BLANK TEST	0.000	09:10
EXTERNAL STANDARD	0.100	09:10
BLANK TEST	0.000	09:11
EXTERNAL STANDARD	0.100	09:12
BLANK TEST	0.000	09:12

Average = 0.1000
 Std Dev = 0.0000

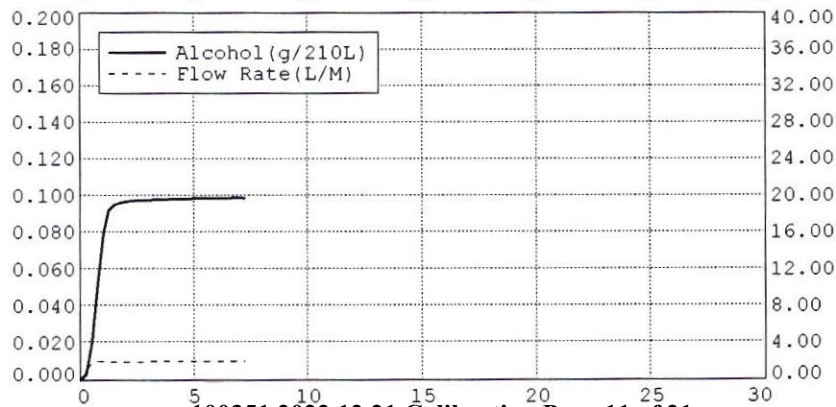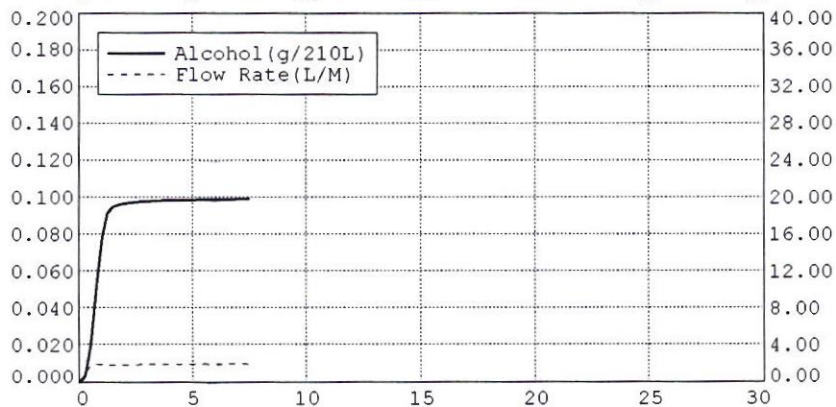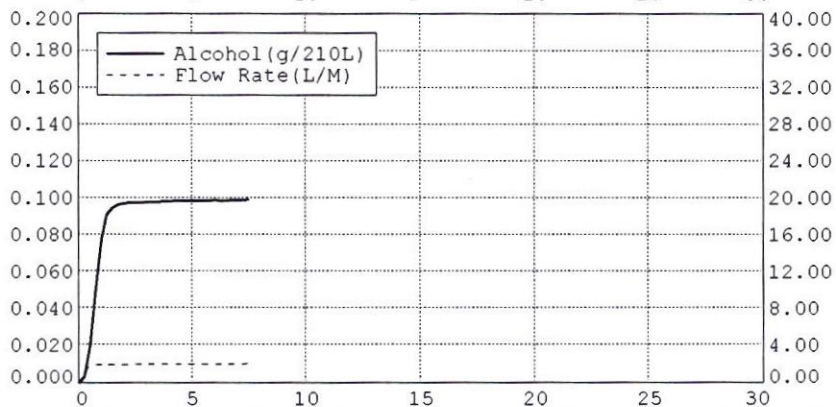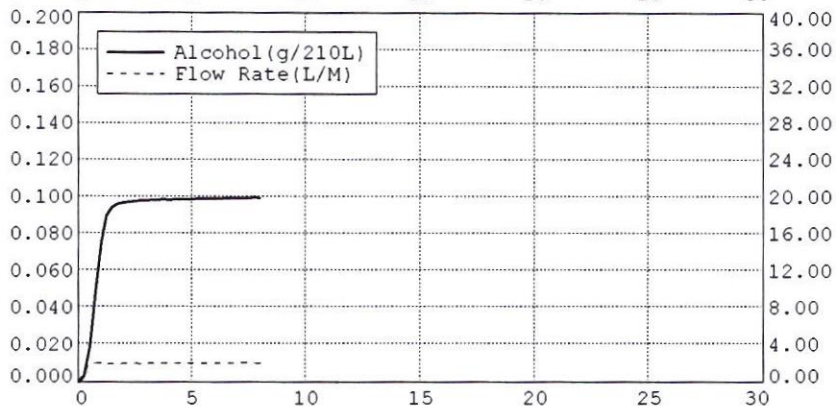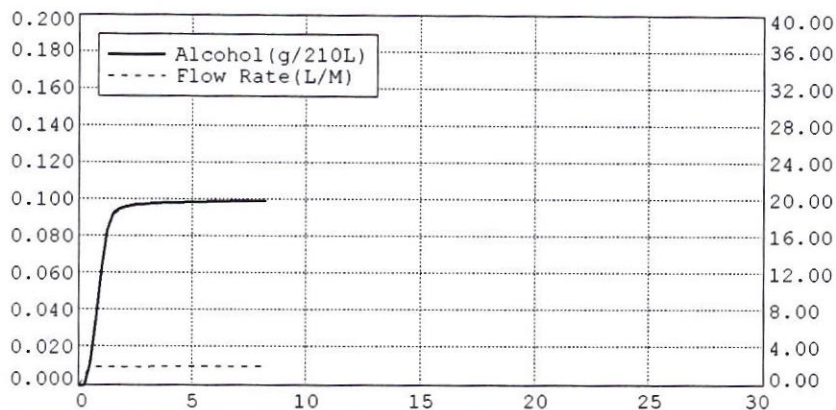

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100351






Date: 12/20/2022
 Time: 09:14:14

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 30.07: 0.151
 LOT #: AG134205
 EXPIRATION: 12/08/2023
 TANK PRESSURE: 664 psi

BLANK TEST	0.000	09:15
INTERNAL STANDARD	VERIFIED	09:15
EXTERNAL STANDARD	0.150	09:15
BLANK TEST	0.000	09:16
EXTERNAL STANDARD	0.150	09:17
BLANK TEST	0.000	09:17
EXTERNAL STANDARD	0.151	09:18
BLANK TEST	0.000	09:19
EXTERNAL STANDARD	0.150	09:19
BLANK TEST	0.000	09:20
EXTERNAL STANDARD	0.151	09:20
BLANK TEST	0.000	09:21

Average = 0.1504
 Std Dev = 0.0005

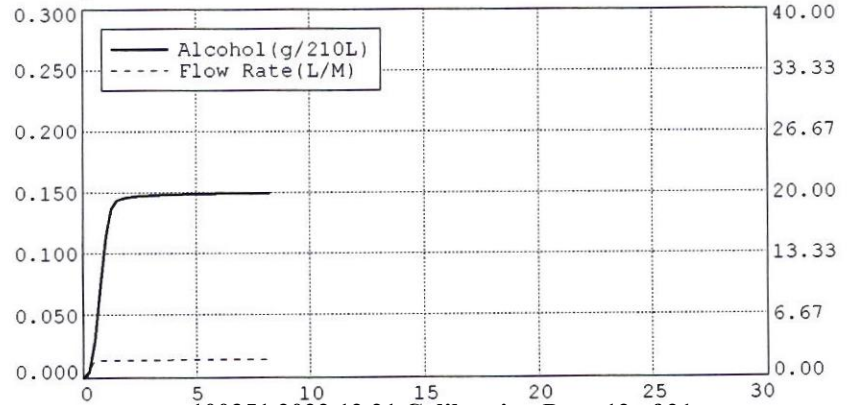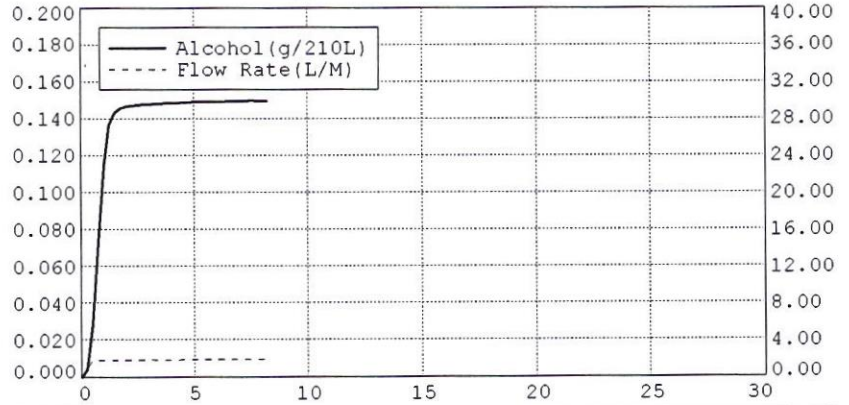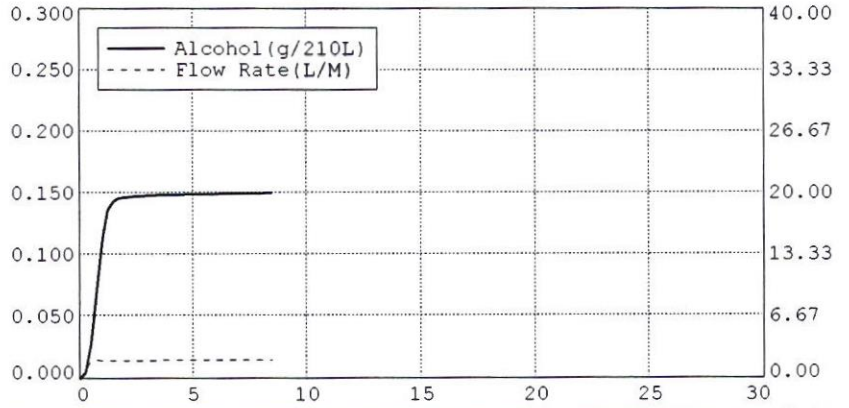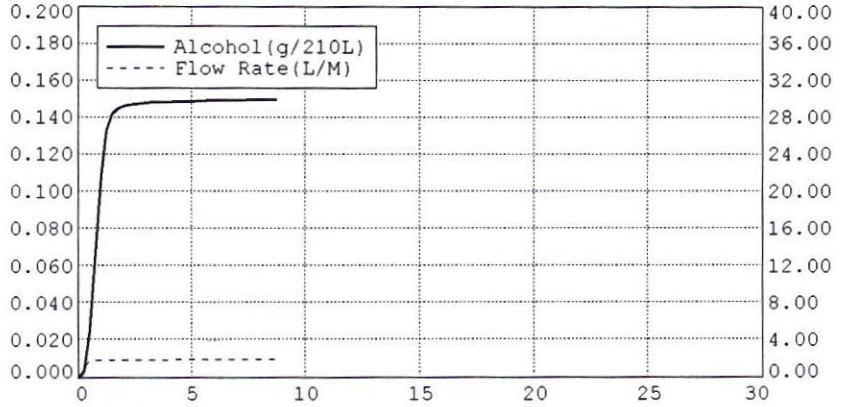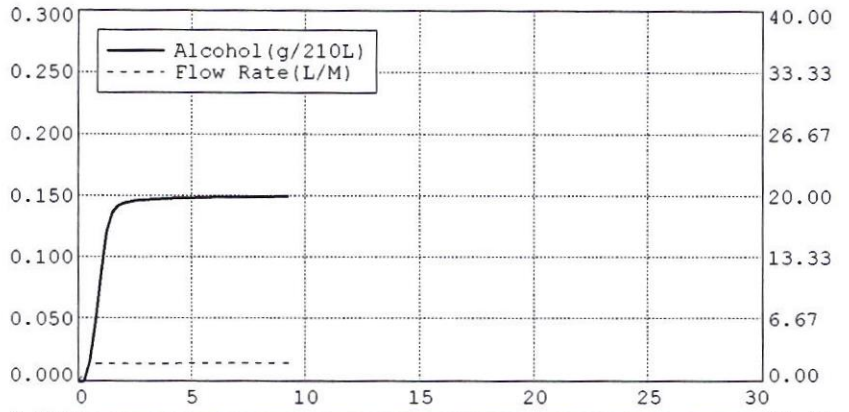

LINEARITY CHECK: Control Test 6

 Alaska Department of Public Safety
 DATAMASTER dmt: 100351






Date: 12/20/2022
 Time: 09:24:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 30.07: 0.301
 LOT #: AG130502
 EXPIRATION: 11/01/2023
 TANK PRESSURE: 336 psi

BLANK TEST	0.000	09:26
INTERNAL STANDARD	VERIFIED	09:26
EXTERNAL STANDARD	0.300	09:26
BLANK TEST	0.000	09:27
EXTERNAL STANDARD	0.298	09:27
BLANK TEST	0.000	09:28
EXTERNAL STANDARD	0.299	09:28
BLANK TEST	0.000	09:29
EXTERNAL STANDARD	0.299	09:30
BLANK TEST	0.000	09:31
EXTERNAL STANDARD	0.299	09:31
BLANK TEST	0.000	09:32

Average = 0.2990
 Std Dev = 0.0007

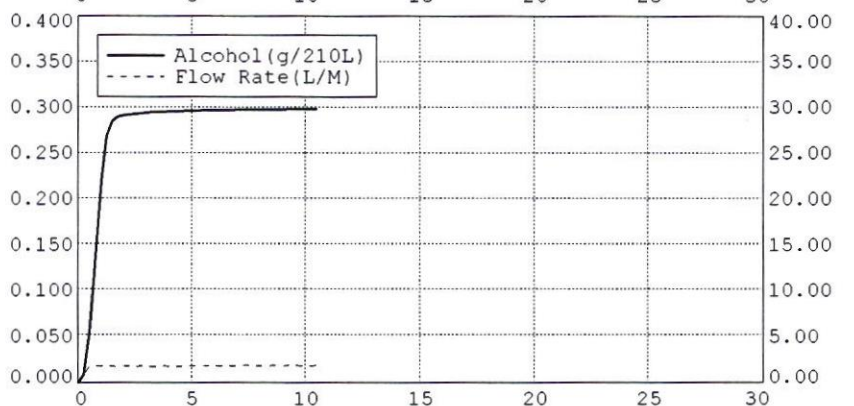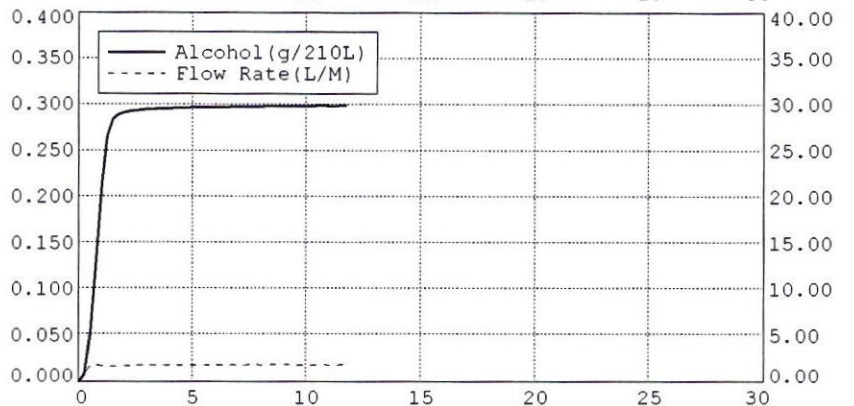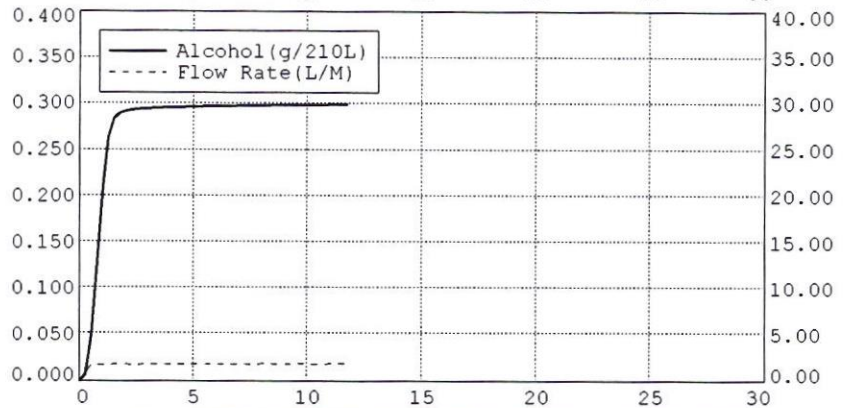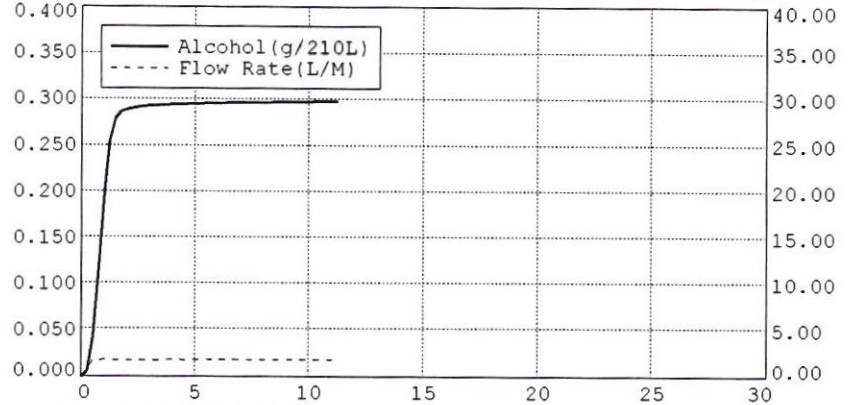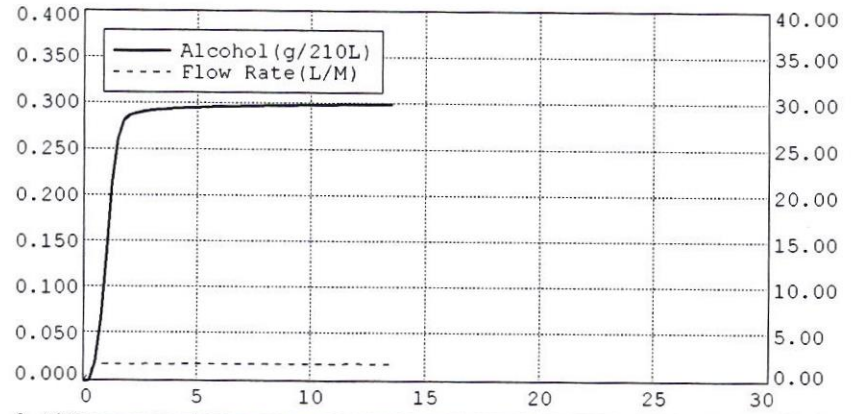

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: 12/20/2022
Time: 09:40:56

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
BRANDI BARNETT
OPERATOR'S #: 7038

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.07: 0.080
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	09:42
BLANK TEST	0.000	09:43
INTERNAL STANDARD	VERIFIED	09:43
EXTERNAL STANDARD	0.081	09:43
BLANK TEST	0.000	09:44
SUBJECT SAMPLE	INCOMPLETE	09:46

BMB

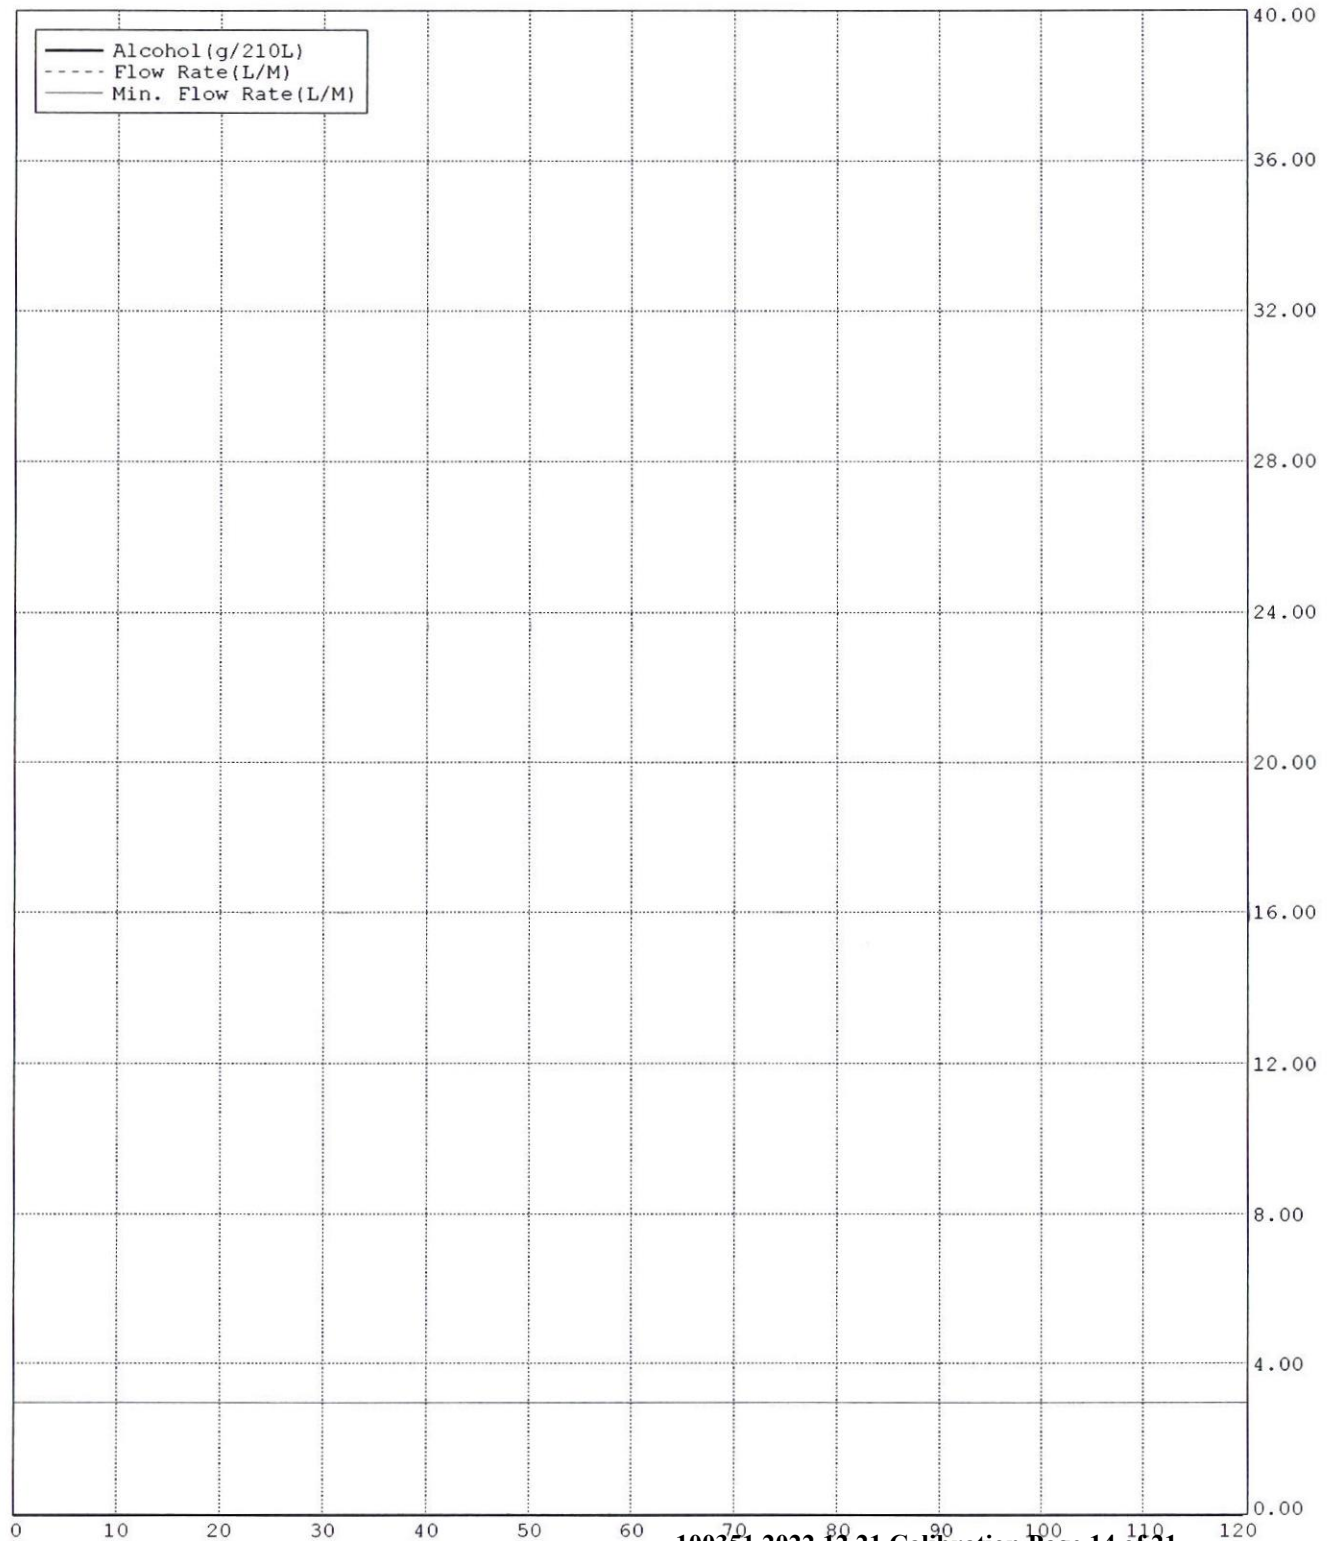

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: 12/20/2022
Time: 10:22:00


SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
BRANDI BARNETT
OPERATOR'S #: 7038

DEPT/AGENCY:
INVALID
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.06: 0.080
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	10:23
BLANK TEST	0.000	10:23
INTERNAL STANDARD	VERIFIED	10:23
EXTERNAL STANDARD	0.079	10:23
BLANK TEST	0.000	10:24
SUBJECT SAMPLE	INVALID	10:24

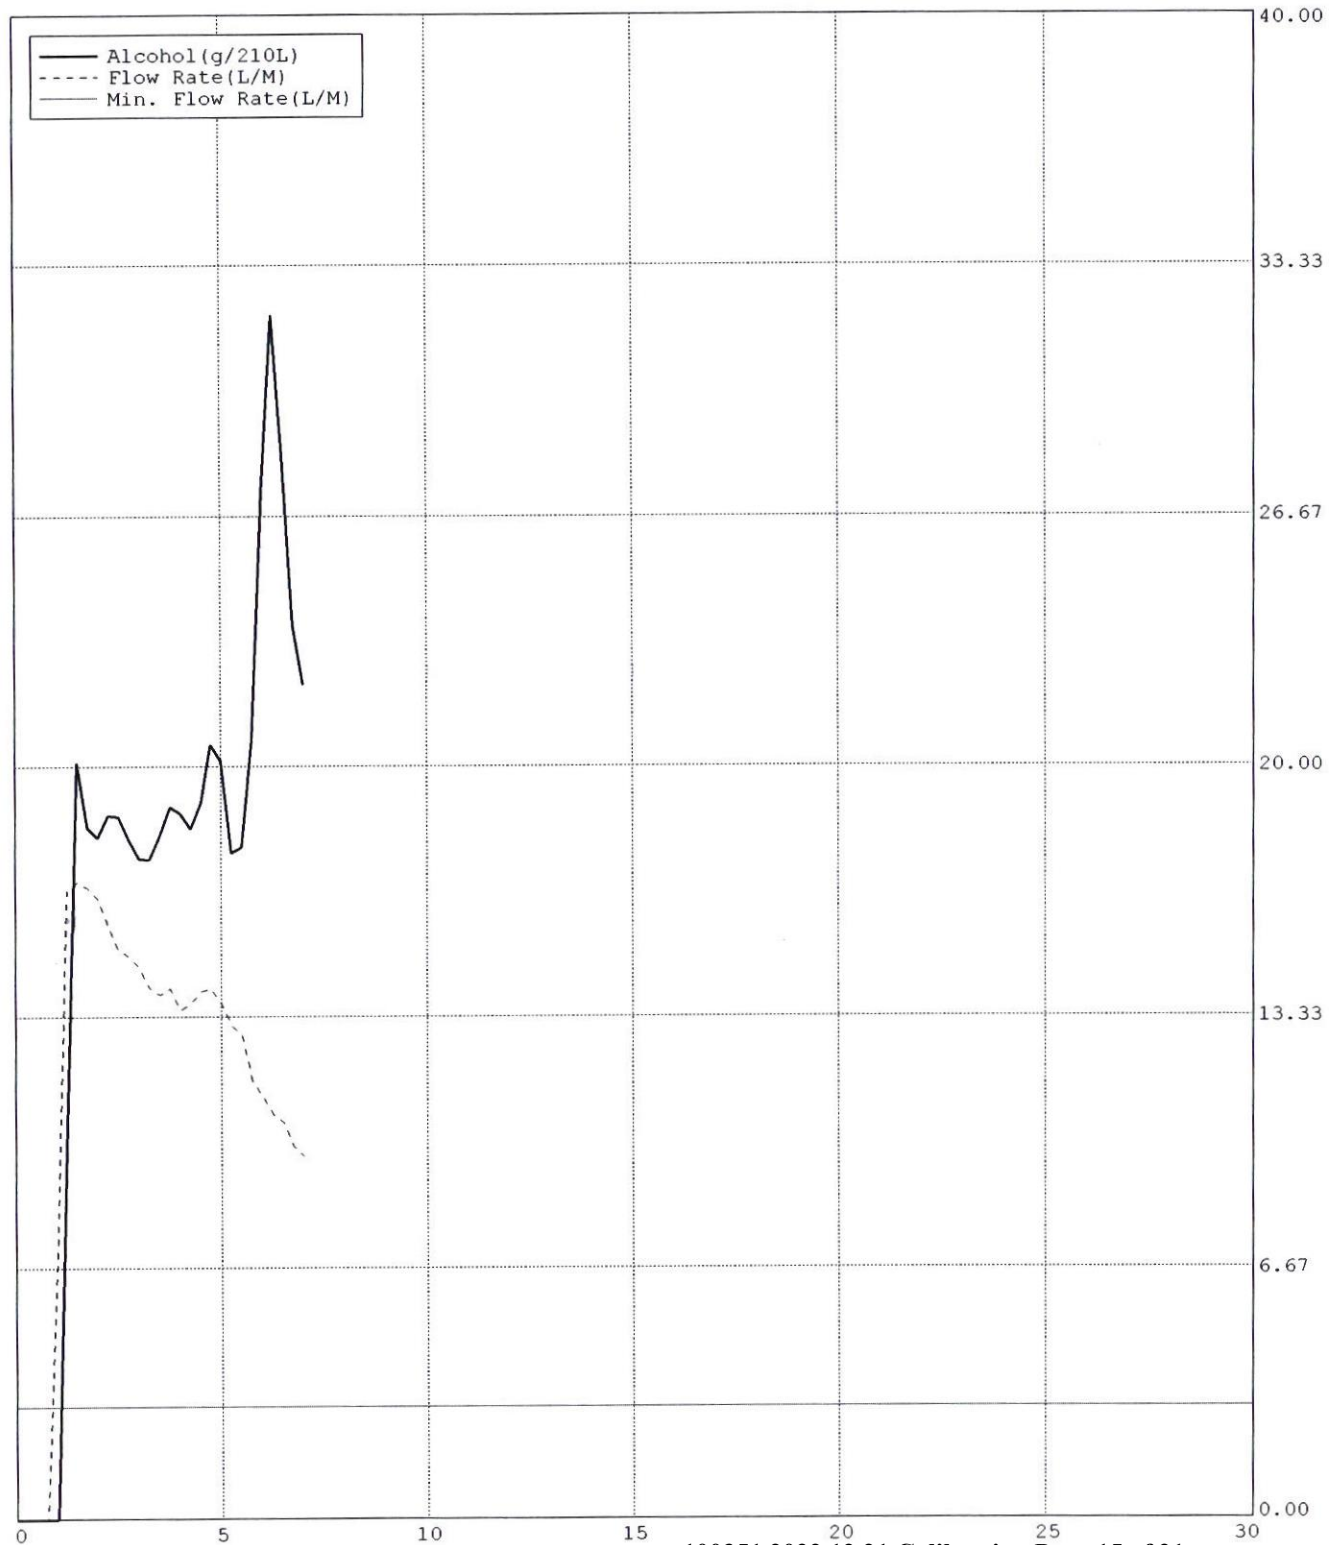

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: 12/20/2022
Time: 09:49:56

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
BRANDI BARNETT
OPERATOR'S #: 7038

DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.06: 0.080
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	09:53
BLANK TEST	0.000	09:53
INTERNAL STANDARD	VERIFIED	09:53
EXTERNAL STANDARD	0.080	09:53
BLANK TEST	0.000	09:54
SUBJECT SAMPLE	XXX	09:55

Maximum Attempts Exceeded

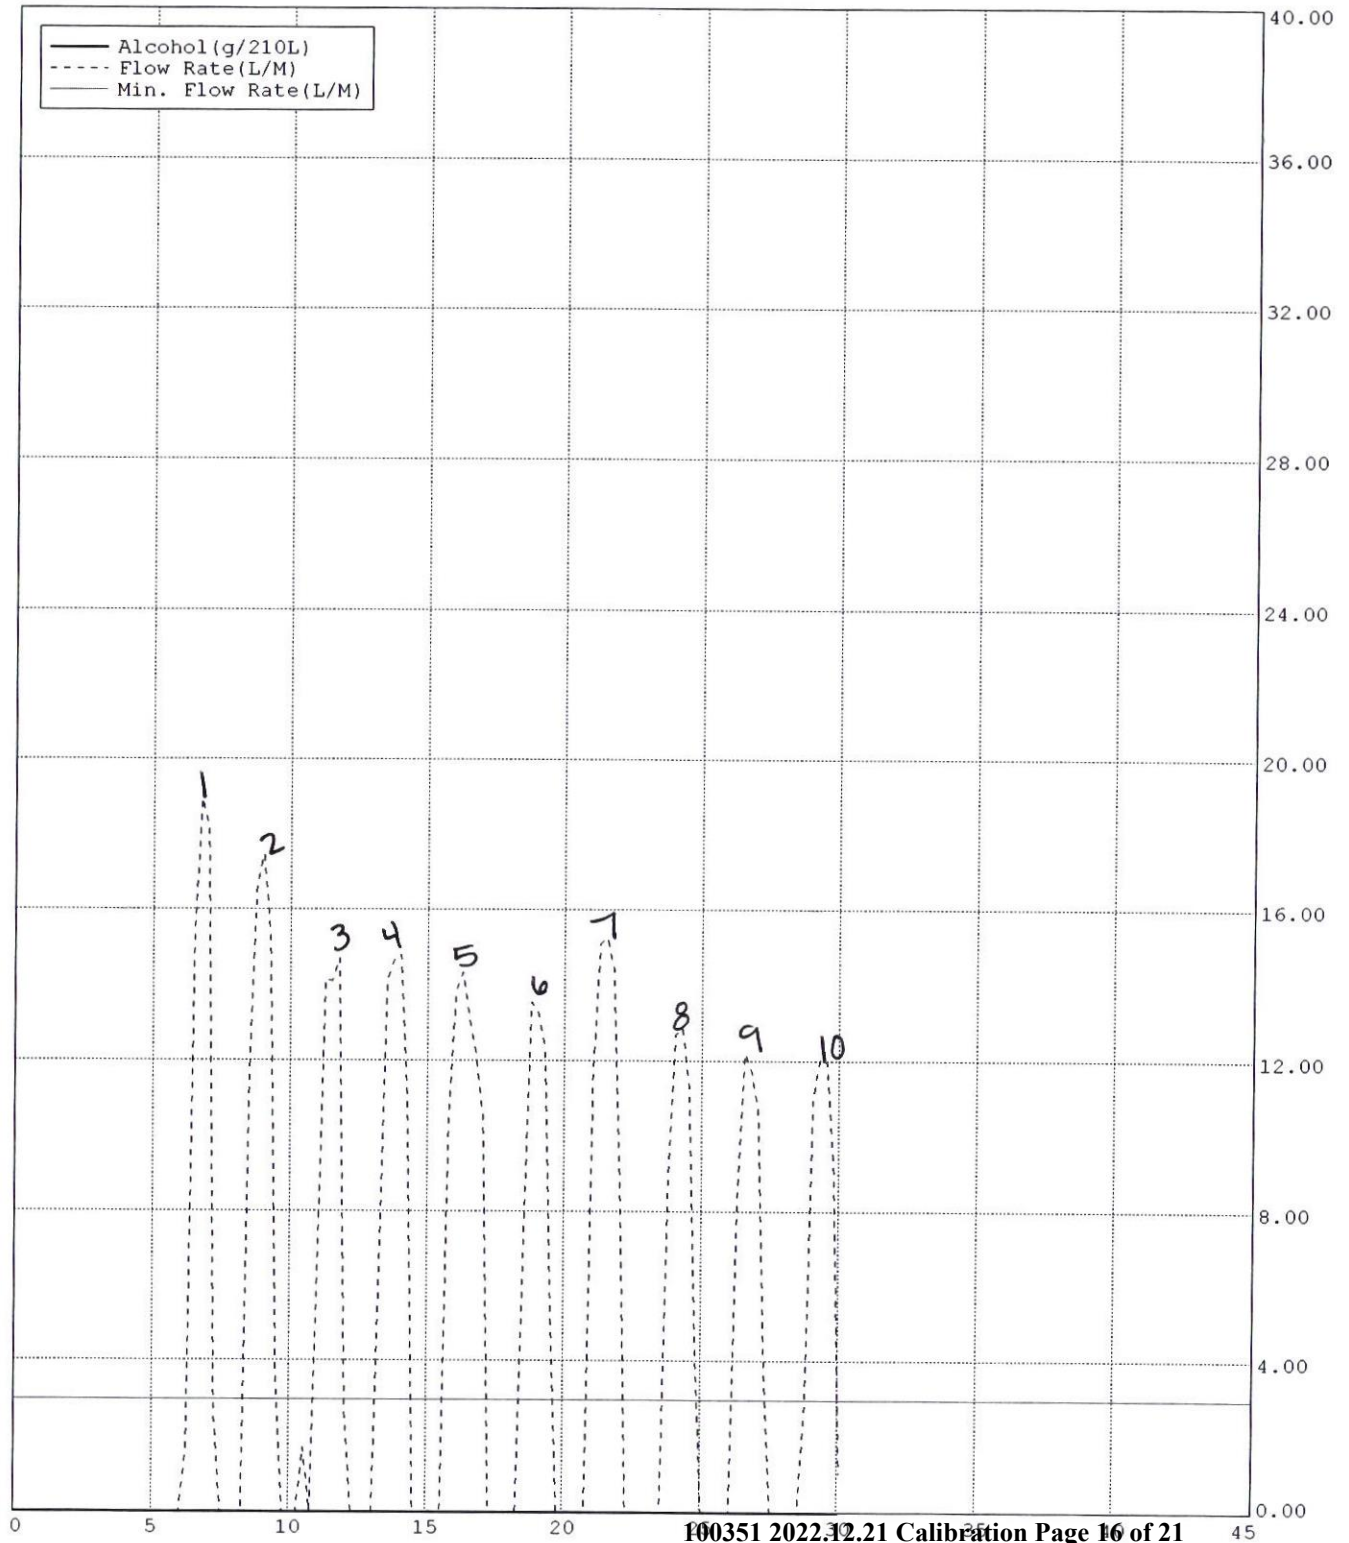

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: 12/20/2022
Time: 10:26:20

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
BRANDI BARNETT
OPERATOR'S #: 7038

DEPT/AGENCY:
RFI
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.07: 0.080
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	10:27
BLANK TEST	0.000	10:28
INTERNAL STANDARD	VERIFIED	10:28
EXTERNAL STANDARD	0.080	10:28
BLANK TEST	0.000	10:29

RFI DETECTED

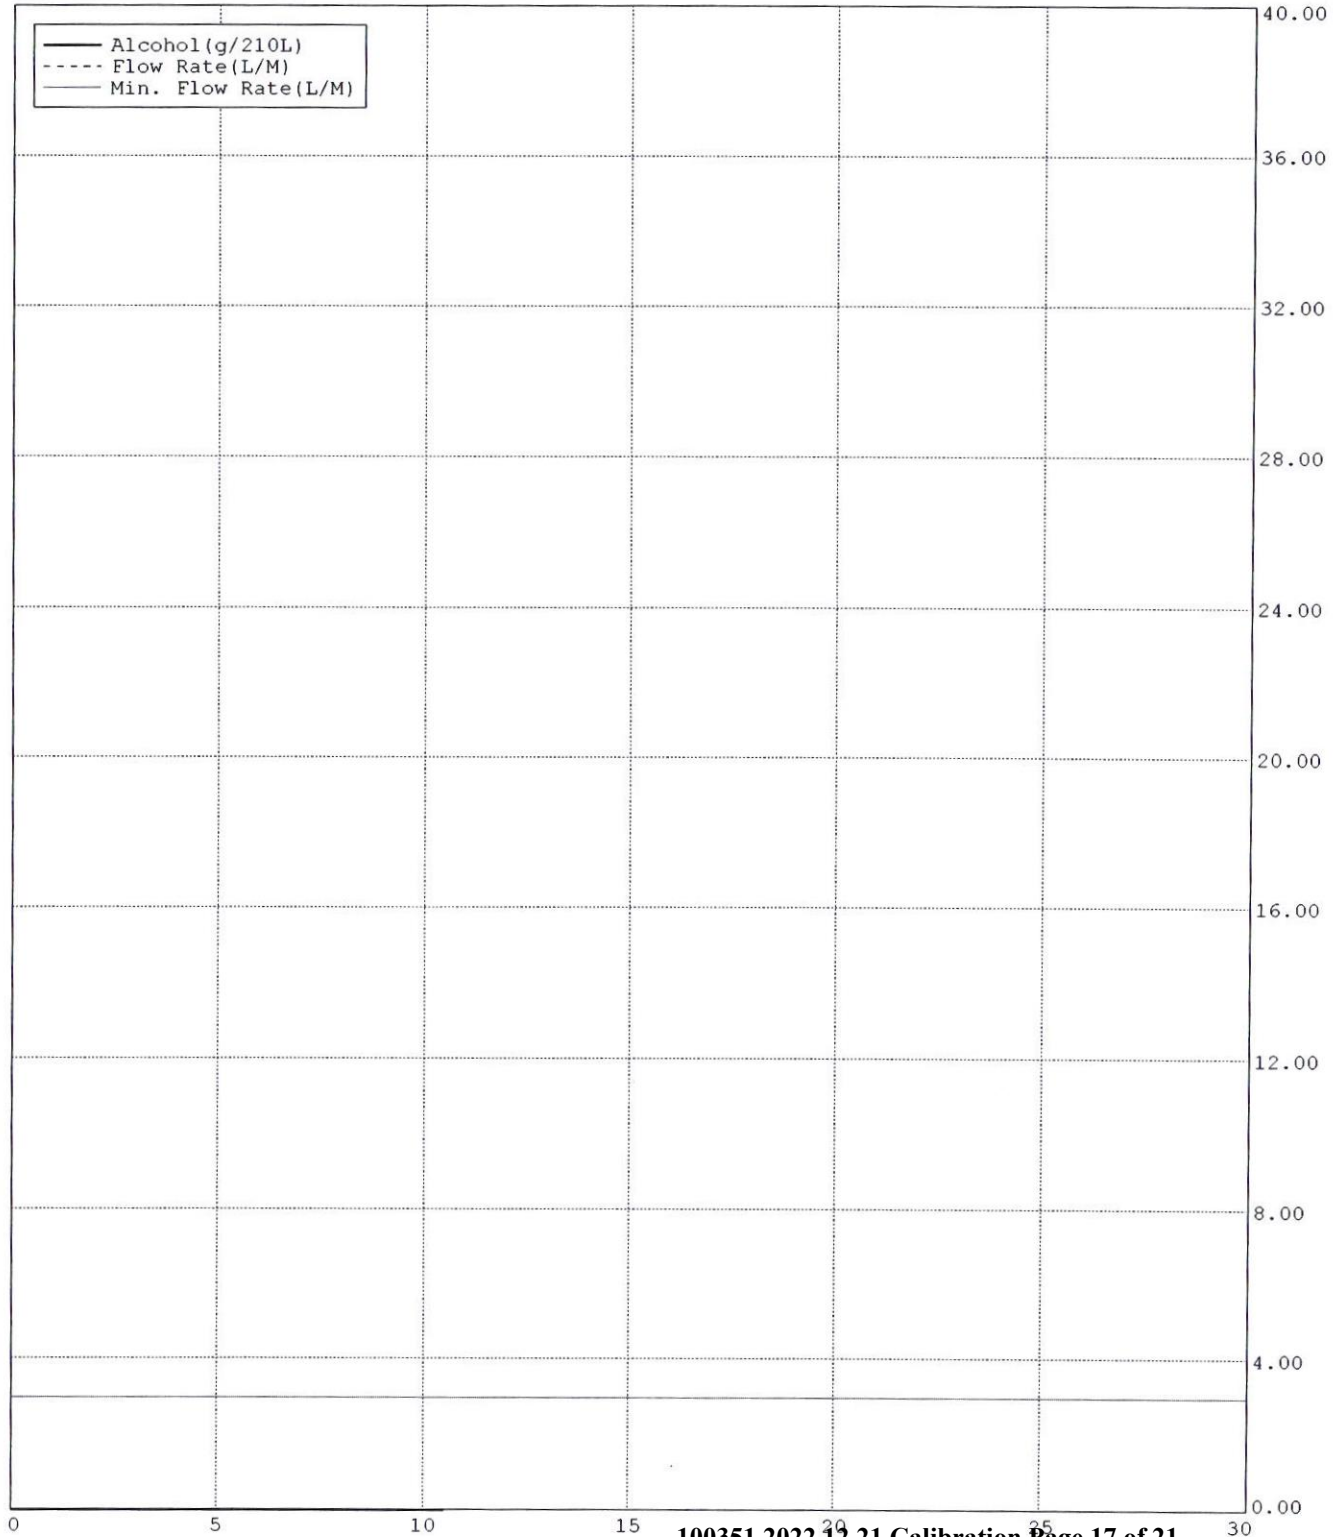

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: 12/20/2022
Time: 13:16:29

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
BRANDI BARNETT
OPERATOR'S #: 7038

DEPT/AGENCY:
INTERFERENCE ACETONE
CASE/REPORT: XXXX
TEST TYPE: TEST



EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.05: 0.080
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	13:17
BLANK TEST	0.000	13:17
INTERNAL STANDARD	VERIFIED	13:18
Xq = 0.121 (0.36%)		
EXTERNAL STANDARD	0.079	13:18
X[1] = 0.0792 (-0.0027) (0.0010)		
BLANK TEST	0.000	13:19
SUBJECT SAMPLE	XXX	13:19
X[1] = 0.1157 (-0.0189) (0.0010)		

Interference Detected

Filter 2 Average: -0.0021
Filter 3 Average: 0.0007

BMB
12/27/2022

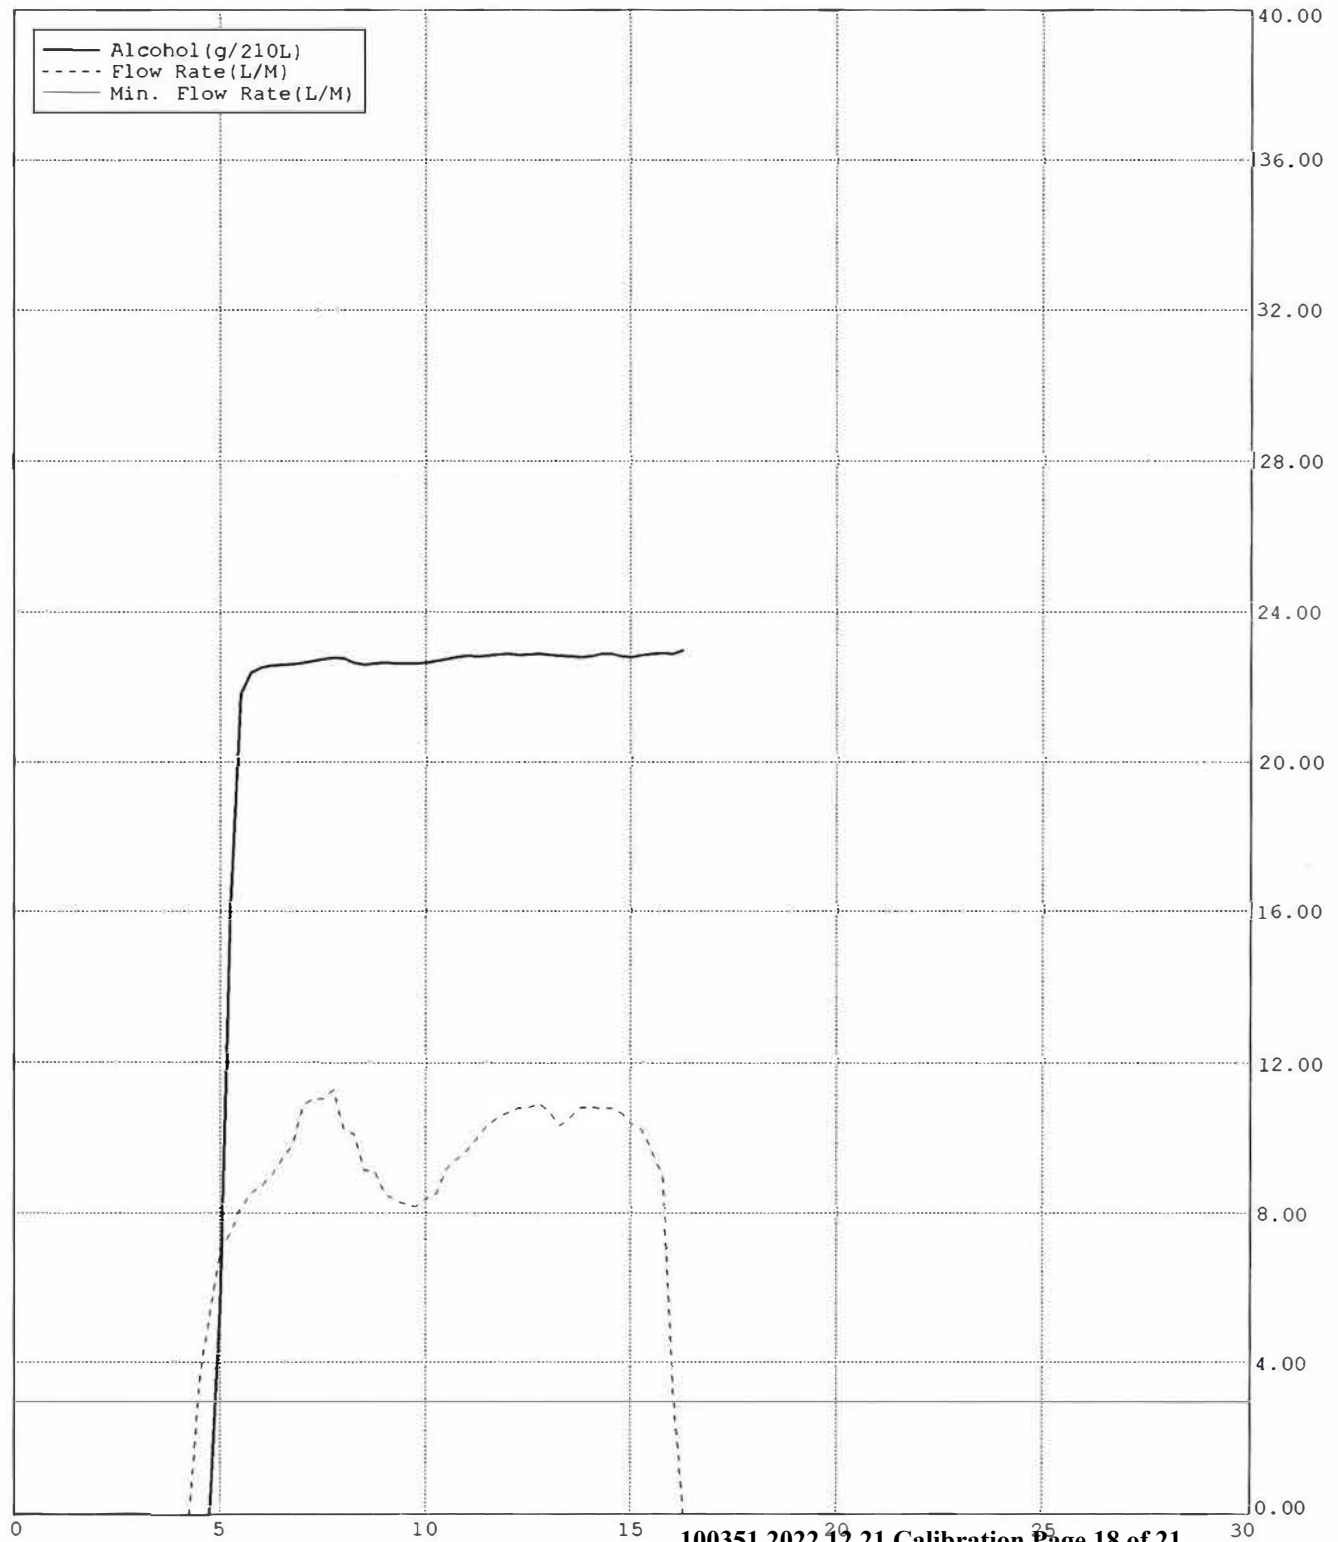

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: 12/20/2022
Time: 13:24:00

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
BRANDI BARNETT
OPERATOR'S #: 7038

DEPT/AGENCY:
INTERFERENCE ISOPROPANOL
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.05: 0.080
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	13:25
BLANK TEST	0.000	13:25
INTERNAL STANDARD	VERIFIED	13:25
Xq = 0.121 (0.22%)		
EXTERNAL STANDARD	0.080	13:25
X[1] = 0.0795 (-0.0019) (0.0005)		
BLANK TEST	0.000	13:26
SUBJECT SAMPLE	XXX	13:26
X[1] = 0.1185 (-0.0245) (-0.0008)		

Interference Detected

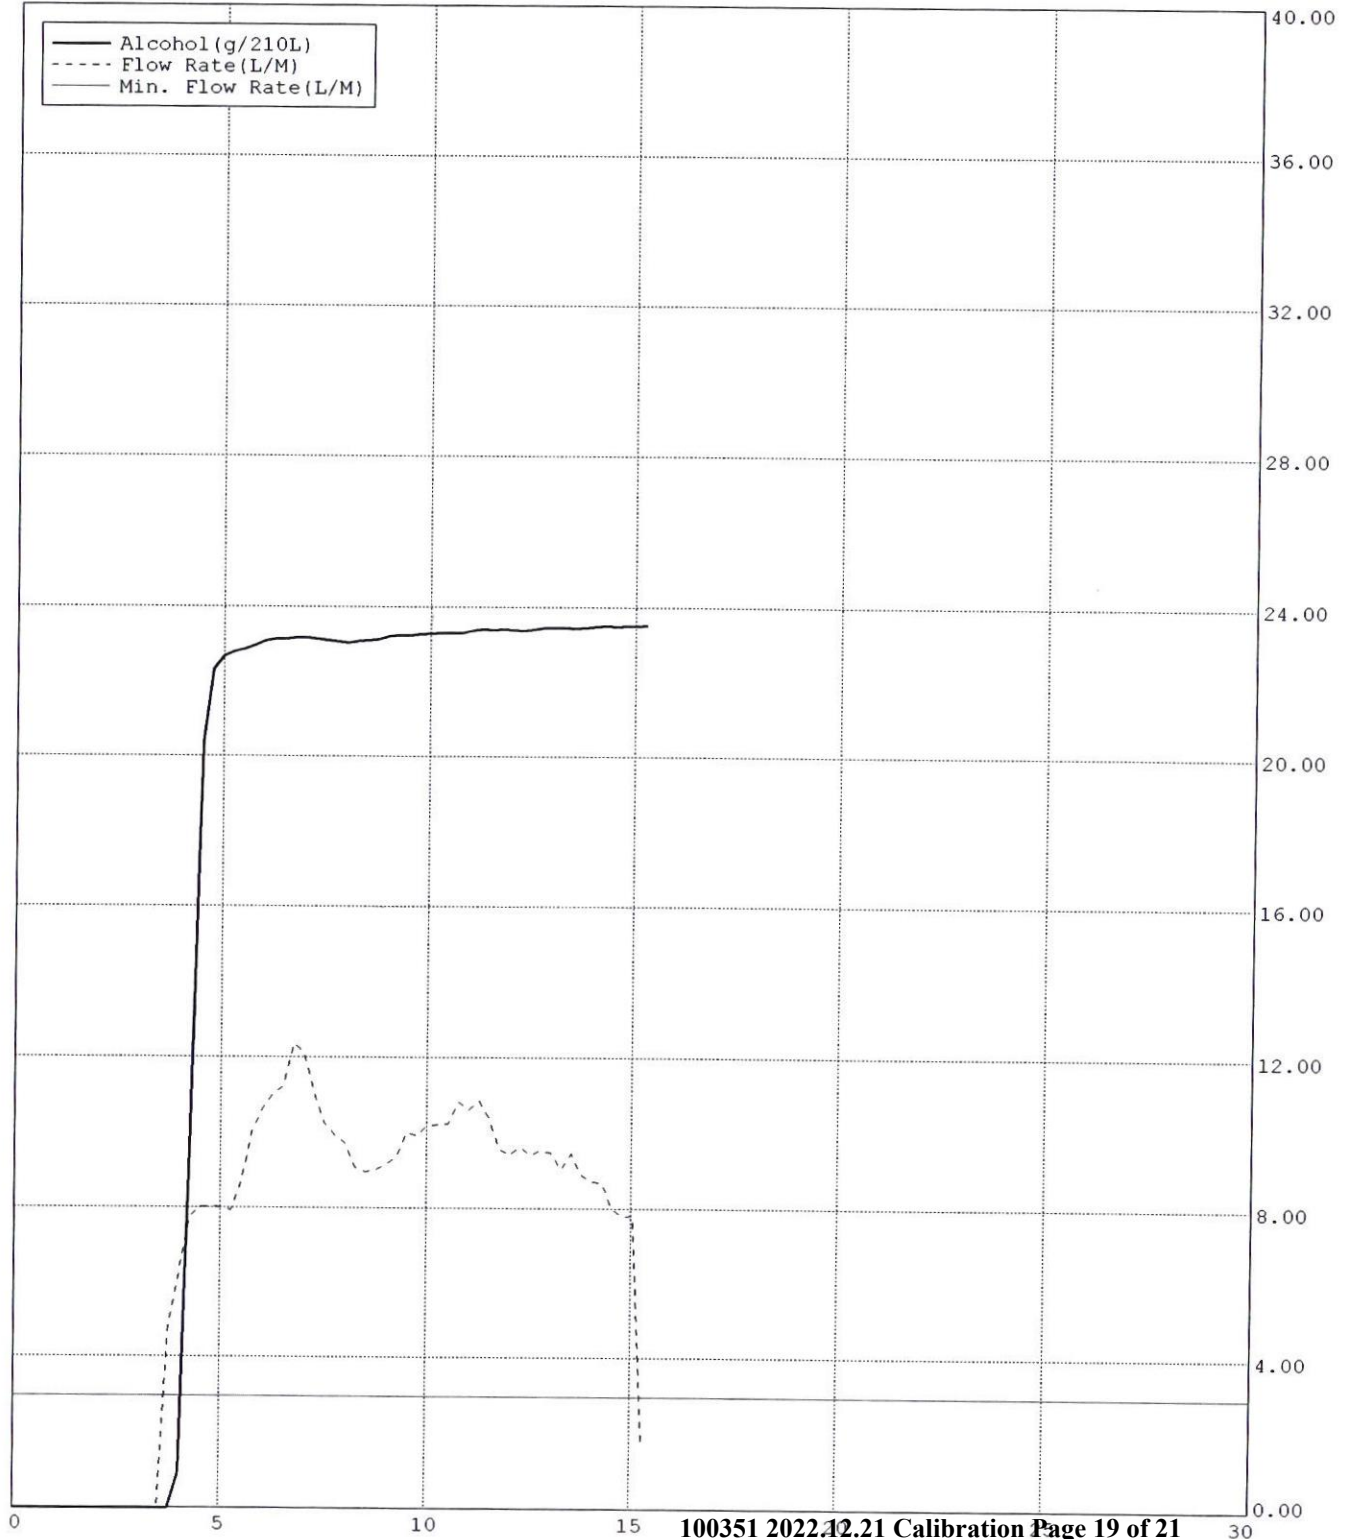

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: 12/20/2022
Time: 13:29:43


SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
BRANDI BARNETT
OPERATOR'S #: 7038

DEPT/AGENCY:
INTERFERENCE NEGATIVE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.05: 0.080
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	13:30
BLANK TEST	0.000	13:30
INTERNAL STANDARD	VERIFIED	13:30
Xq = 0.122 (0.07%)		
EXTERNAL STANDARD	0.080	13:31
X[1] = 0.0799 (-0.0019) (0.0010)		
BLANK TEST	0.000	13:32
SUBJECT SAMPLE (Vol=1.77L)	0.099	13:32
X[1] = 0.0997 (-0.0013) (-0.0006)		
BLANK TEST	0.000	13:33
EXTERNAL STANDARD	0.079	13:33
X[1] = 0.0791 (-0.0019) (0.0002)		
BLANK TEST	0.000	13:34

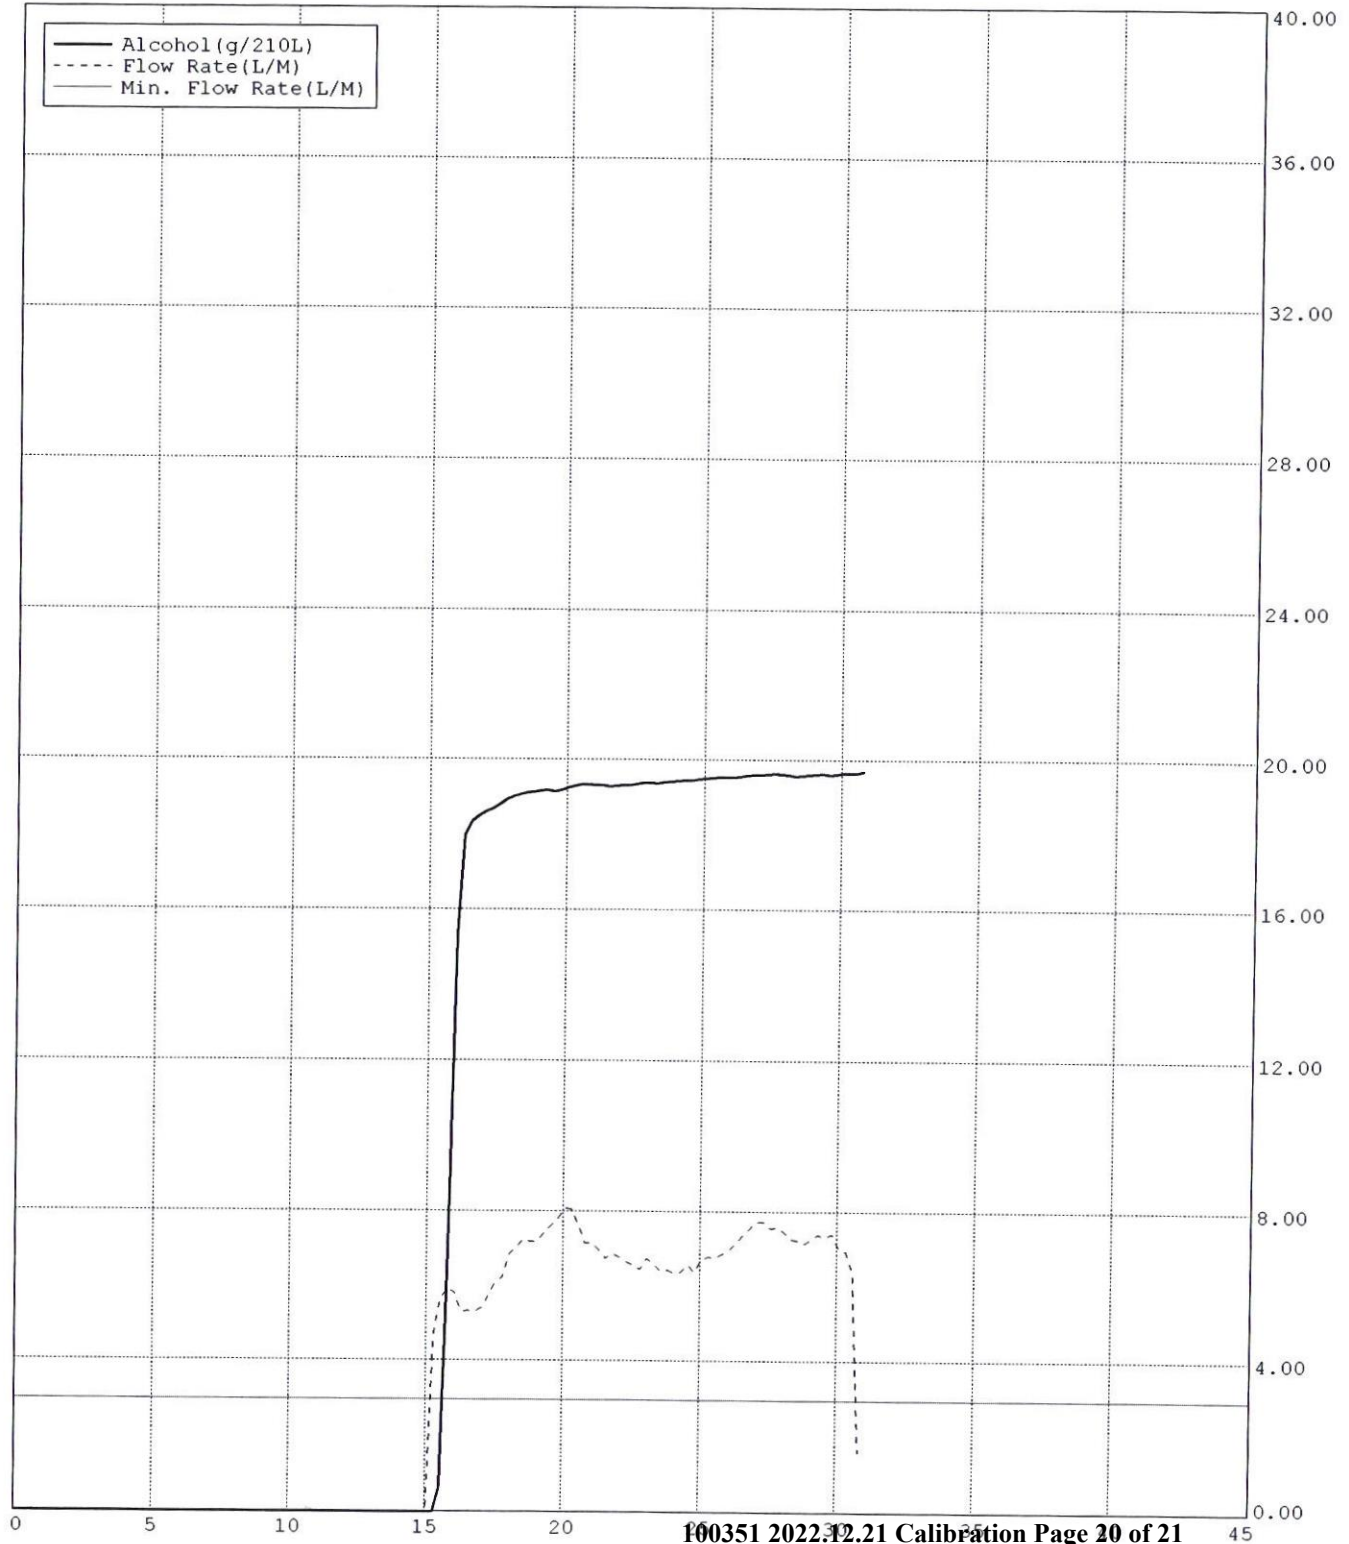

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100351

Date: 12/20/2022
Time: 13:54:38

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
BRANDI M BARNETT
OPERATOR'S #: 7038

DEPT/AGENCY:
NON DRINKING SUBJECT
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.05: 0.080
LOT #: AG135004
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	13:55
BLANK TEST	0.000	13:55
INTERNAL STANDARD	VERIFIED	13:55
EXTERNAL STANDARD	0.079	13:56
BLANK TEST	0.000	13:57
SUBJECT SAMPLE (Vol=2.08L)	0.000	13:57
BLANK TEST	0.000	13:58
EXTERNAL STANDARD	0.080	13:58
BLANK TEST	0.000	13:59

