

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument  
State of Alaska

Serial #: 100366

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 04/03/2021

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.88: 0.080  
LOT #: AG018102  
EXPIRATION: 06/29/2022  
TANK PRESSURE: 1196 psi

BLANK TEST	0.000	02:55
INTERNAL STANDARD	VERIFIED	02:56
EXTERNAL STANDARD	0.078	02:56
BLANK TEST	0.000	02:57
EXTERNAL STANDARD	0.078	02:57
BLANK TEST	0.000	02:58
EXTERNAL STANDARD	0.078	02:58
BLANK TEST	0.000	02:59
EXTERNAL STANDARD	0.078	02:59
BLANK TEST	0.000	03:00
EXTERNAL STANDARD	0.078	03:00
BLANK TEST	0.000	03:01

Average = 0.0780  
Std Dev = 0.0000

## Diagnostic Check

### VERSIONS

DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.9°C PASSED  
Breath Tube = 47.8°C PASSED

### PUMP INFO

Flow Rate = 4.734 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

### FILTER INFO


Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

### INTERNAL STANDARD

PASSED


I, Brandi M. Barnett, after being first duly sworn, depose and state as follows:



- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

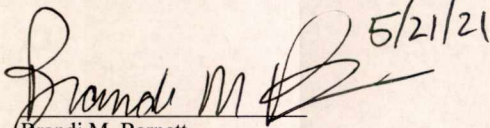 5/21/21

Brandi M. Barnett  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 21 day of 5, 20 21

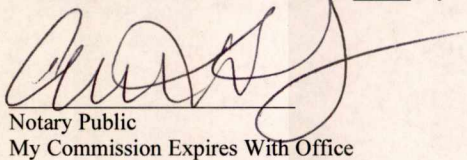  
Notary Public  
My Commission Expires With Office

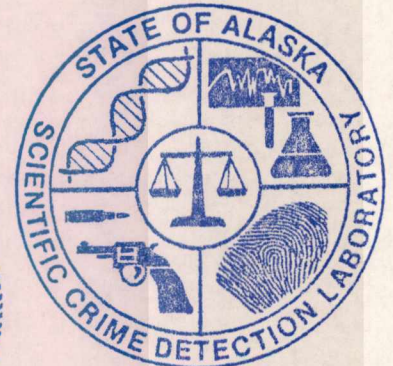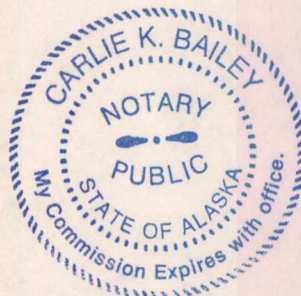

JM 04/14/21