



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100345

**Report Issue Date:** 12/28/2023  
**Date Received:** 2023-05-17  
**Condition of Item:** Needs Repair

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 05/17/2023** - As Found - **End Date 05/17/2023** As Found - Evaluation Analyst: Colleen O'Bryant  
 As Found Conditions - Barometric Pressure (inHg): 29.92 Barometer Used: Fisher S/N 221250180 Temperature (C): 21.9  
 Relative Humidity (%): 24

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.080	09523080A1	0.079	0.079	0.080	0.079	0.079	0.079	0.079
0.300	0.300	AG217903	0.298	0.297	0.296	0.297	0.296	0.296	0.297

Regulator did stick on all tanks installed but did not appear to leak. Recommend regulator replacement.

**Start Date 11/30/2023** - As Left - **End Date 12/04/2023**

As Left Conditions - Barometric Pressure (inHg): 28.83 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.3 Relative Humidity (%): 19

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.019	AG217902	0.019	0.019	0.019	0.019	0.019	0.019	+/- 0.002	
0.040	0.039	AG217904	0.038	0.038	0.038	0.038	0.038	0.038	+/- 0.003	
0.080	0.077	AG310901	0.075	0.075	0.075	0.075	0.075	0.075	+/- 0.004	
0.100	0.096	AG211003	0.094	0.095	0.095	0.095	0.095	0.095	+/- 0.004	
0.150	0.144	AG134205	0.142	0.142	0.142	0.142	0.142	0.142	+/- 0.005	
0.300	0.289	AG217903	0.287	0.285	0.286	0.286	0.286	0.286	+/- 0.011	

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Carlie Glaister on 12/04/2023

[carlie.glaister@alaska.gov](mailto:carlie.glaister@alaska.gov)

Technically and administratively reviewed by Colleen O'Bryant on 12/28/2023

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100345 Analyst: Carlie Haister Start Date: 11/30/23

- Diagnostic Test (attached)
- Adjust voltages, if needed
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
- Internal Standard value  $\leq$  3.00%
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.4 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 28.83 Temperature (C): 22.3 Relative Humidity (%) 19

Linearity Test (attached)

0.020g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217902</u>	Exp: <u>6/28/24</u>
0.040g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217904</u>	Exp: <u>6/28/24</u>
0.080g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-310901</u>	Exp: <u>4/19/25</u>
0.100g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-211003</u>	Exp: <u>4/20/24</u>
0.150g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-134205</u>	Exp: <u>12/8/23</u>
0.300g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217903</u>	Exp: <u>6/28/24</u>

Functional Tests (attached)

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles)

Acetone Mnf: Lifelog Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR4176 Verification Performed?

Isopropanol Mnf: Lifelog Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR4177 Verification Performed?

Neg. Control Mnf: Lifelog Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR6267 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 230631106 Calibration Due Date: 9/19/2025

- Verify stylus is calibrated
- Non-Drinking Subject Test
- Reset Options
- Upload
- Clear Memory
- Remove Tank Prior to Shutdown
- Verification of Calibration (VOC)
- Calibration End Date: 12/1/23

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100345  
-----

Date: 11/30/2023  
Time: 09:21:19

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 46.3°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.70 V PASSED  
(1.02 V - 2.38 V)  
Cooler Voltage = 1.64 V PASSED  
(0.98 V - 2.30 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 526 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 28.9 in

PUMP INFO

Flow Rate = 4.208 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.001 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.094 0.65% (0.00% - 4.00%) PASSED

Technician Screen

-----  
DATAMASTER dmt: 100345  
-----

Date: 11/30/2023  
Time: 10:39 AM

Temperatures (°C)  
Sample Cell: 48.8°C  
Breath Tube: 46.6°C

Current Barometer 28.8 in  
Volume (Ltr) 1.44

Settings  
Lamp: 1.75 V  
Bias: 80 V  
Cooler: 1.64 V  
Chopper: 526 Hz

Voltages (V)  
Flow: 1.06 V  
Detector: -0.084 V



CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100345  
-----

Date: 09/01/2022  
Time: 09:10:46

OPERATOR NAME:  
TATIANA MALNOSKE  
CERTIFICATE #: 10437

Ca = 0.1000  
CAL = 0.970856    0.800 <= CAL < 1.200  
b1 = 0.0014    0.0000 <= b1 < 0.0040  
b2 = 0.0059    0.0010 <= b2 < 0.0100  
b3 = 0.0008    0.0000 <= b3 < 0.0040  
Xq = 0.0945    0.0500 <= Xq < 0.2000  
a21 = 1.146871    1.050 <= a21 < 1.300  
a31 = 0.502084    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100345

Date: 11/30/2023  
Time: 10:40:15

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
MINIMUM VOLUME TEST  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.84: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	10:42
BLANK TEST	0.000	10:42
INTERNAL STANDARD	VERIFIED	10:43
EXTERNAL STANDARD	0.075	10:43
BLANK TEST	0.000	10:44
SUBJECT SAMPLE (Vol=1.56L)	0.000	10:45
BLANK TEST	0.000	10:46
EXTERNAL STANDARD	0.076	10:46
BLANK TEST	0.000	10:47

CKG

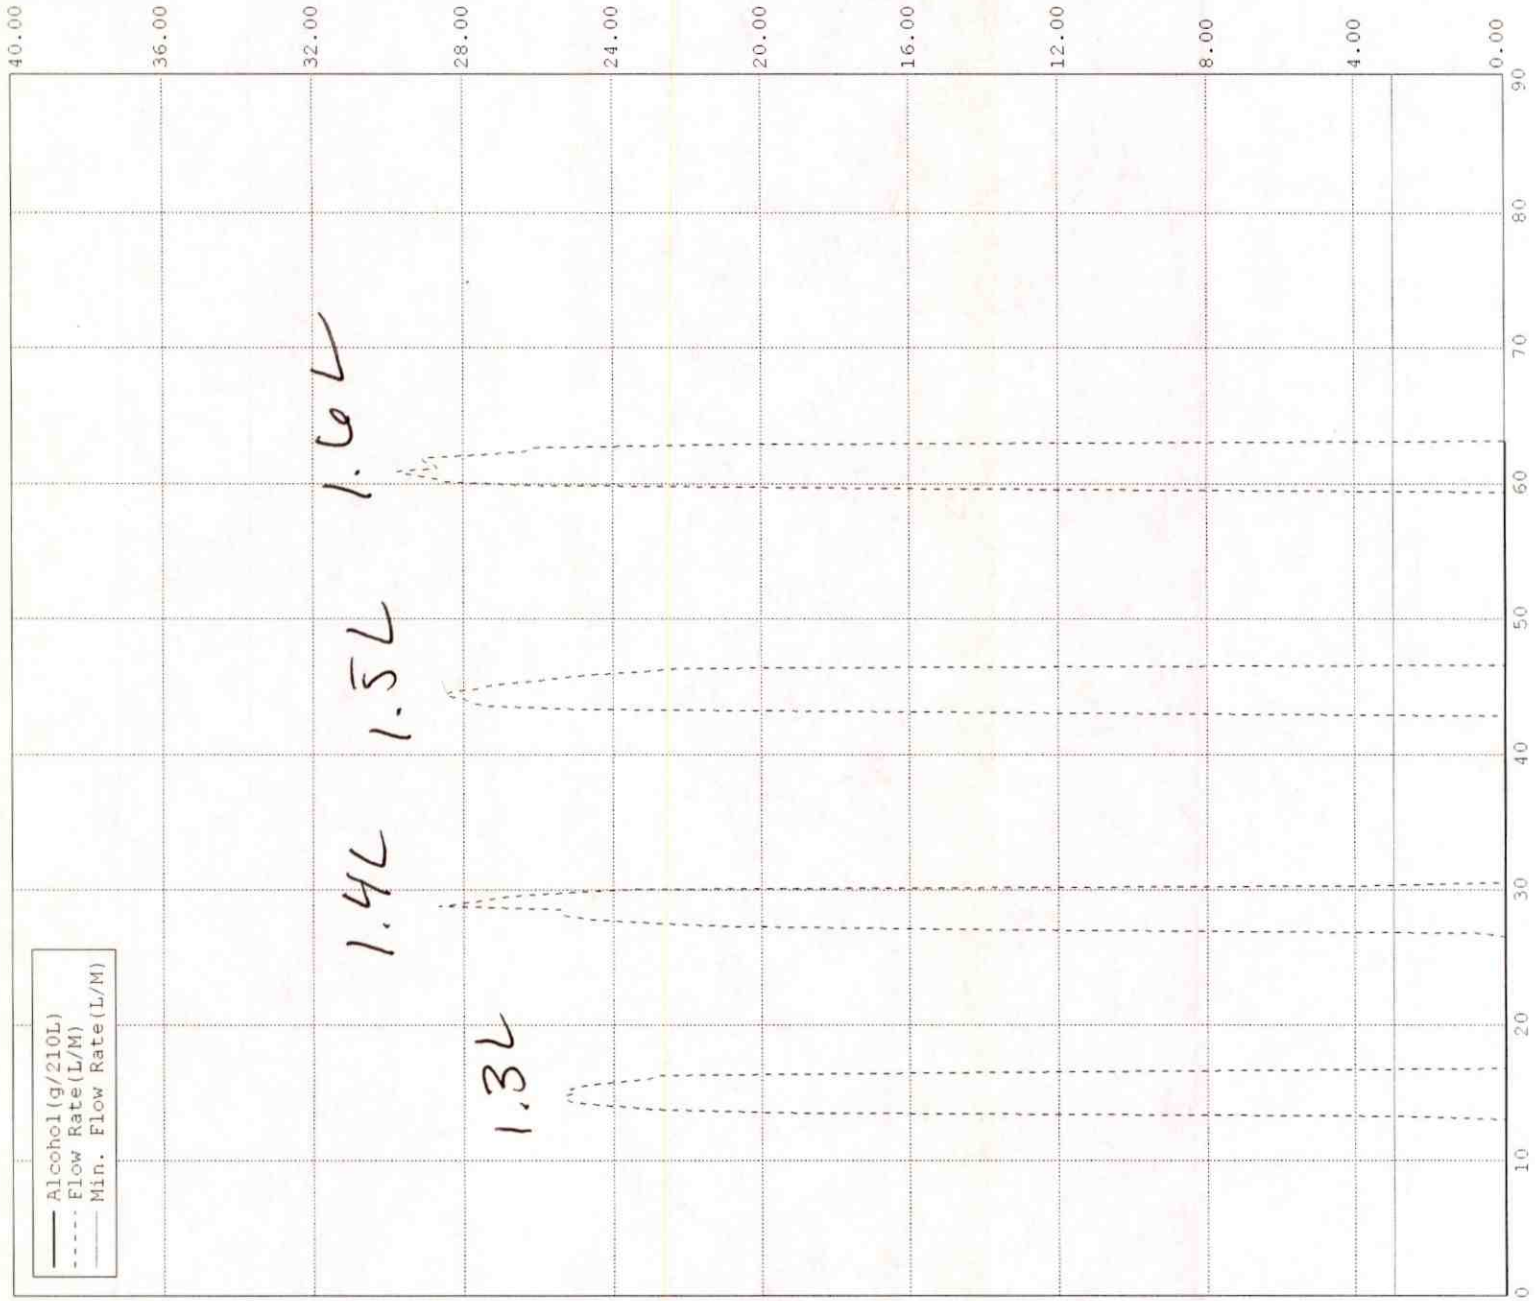

LINEARITY CHECK


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100345  
 -----

Date: 11/30/2023  
 Time: 12:02:11

SUPERVISOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.019	0.0190	0.0000
0.039	0.0380	0.0000
0.077	0.0750	0.0000
0.096	0.0948	0.0004
0.144	0.1420	0.0000
0.289	0.2860	0.0007

SLOPE = 0.990689  
 R<sup>2</sup> = 0.999975

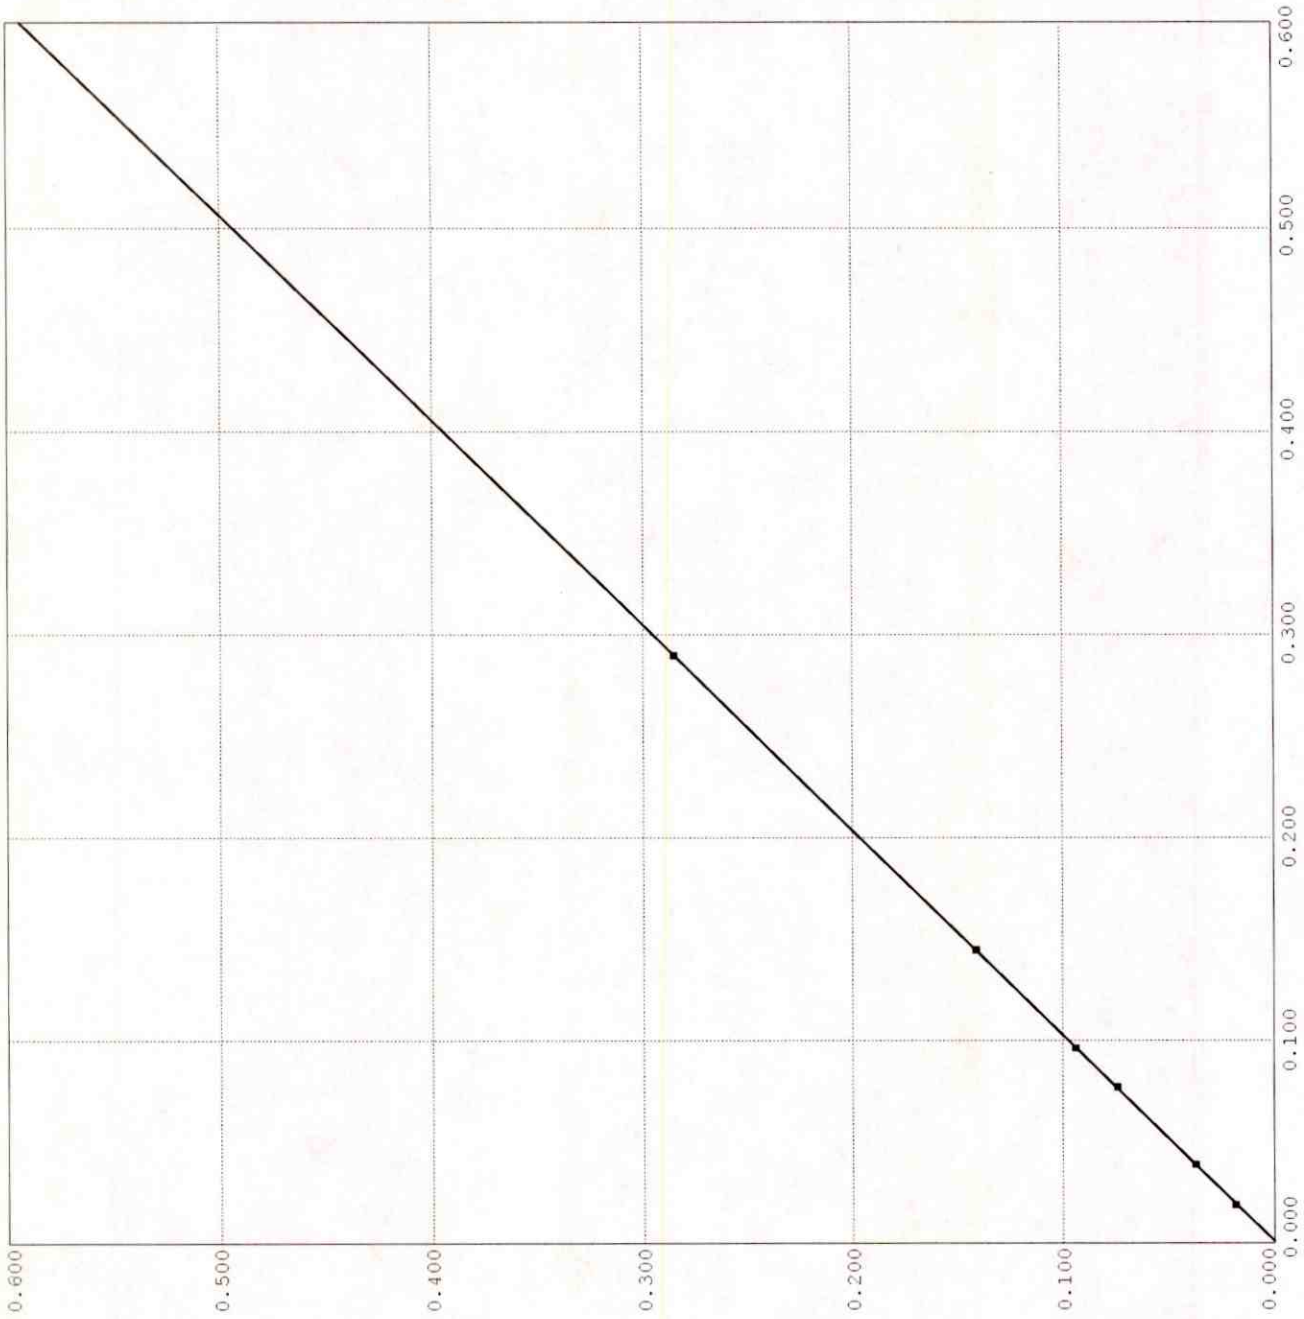

CVG



LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100345






Date: 11/30/2023  
Time: 12:02:13

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 28.82: 0.019  
LOT #: AG217902  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 700 psi

TEST TYPE	CONCENTRATION	TIME
BLANK TEST	0.000	12:03
INTERNAL STANDARD	VERIFIED	12:03
EXTERNAL STANDARD	0.019	12:03
BLANK TEST	0.000	12:04
EXTERNAL STANDARD	0.019	12:04
BLANK TEST	0.000	12:05
EXTERNAL STANDARD	0.019	12:05
BLANK TEST	0.000	12:06
EXTERNAL STANDARD	0.019	12:07
BLANK TEST	0.000	12:07
EXTERNAL STANDARD	0.019	12:08
BLANK TEST	0.000	12:09

Average = 0.0190  
Std Dev = 0.0000

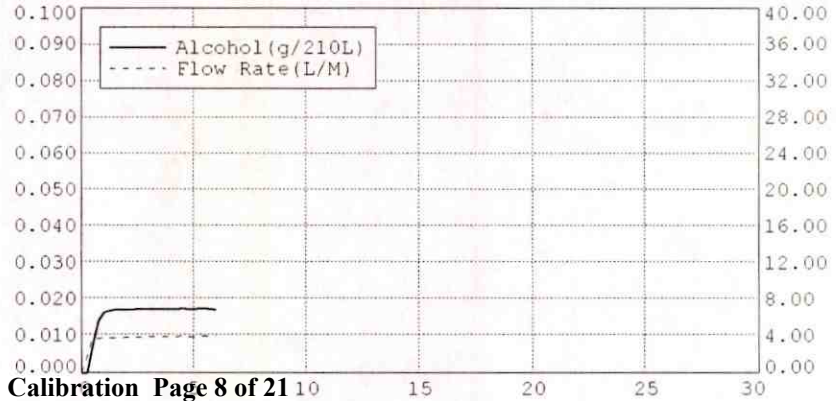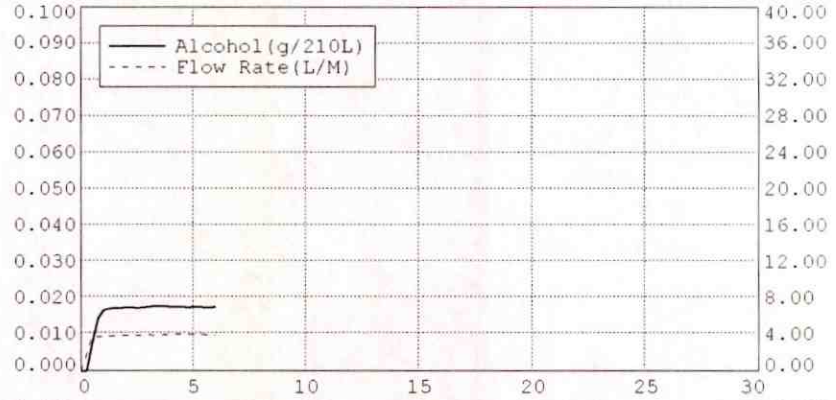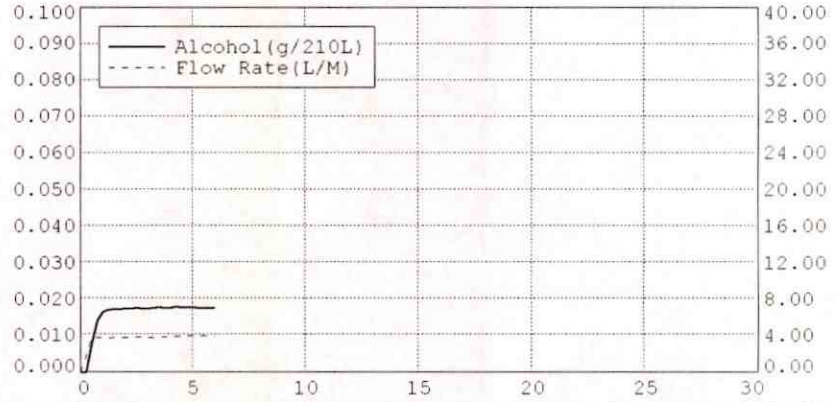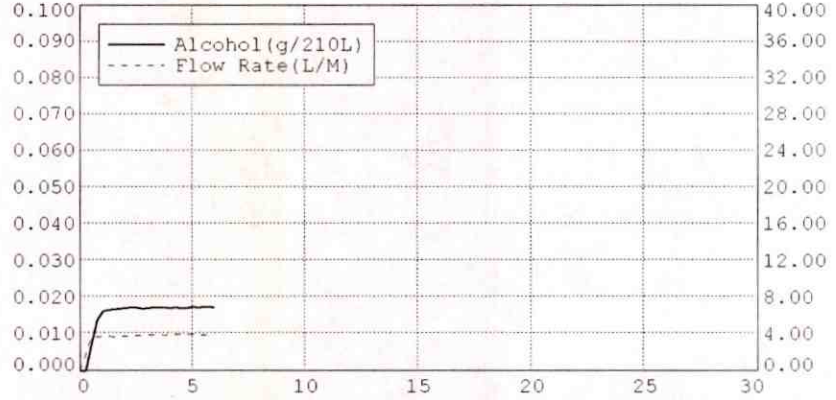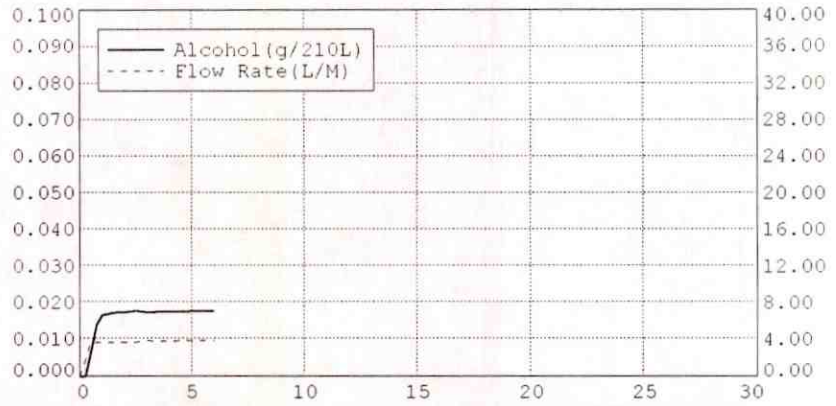



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100345






Date: 11/30/2023  
 Time: 12:12:02

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 28.81: 0.039  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 812 psi

BLANK TEST	0.000	12:13
INTERNAL STANDARD	VERIFIED	12:13
EXTERNAL STANDARD	0.038	12:13
BLANK TEST	0.000	12:14
EXTERNAL STANDARD	0.038	12:14
BLANK TEST	0.000	12:15
EXTERNAL STANDARD	0.038	12:15
BLANK TEST	0.000	12:16
EXTERNAL STANDARD	0.038	12:16
BLANK TEST	0.000	12:17
EXTERNAL STANDARD	0.038	12:17
BLANK TEST	0.000	12:18

Average = 0.0380  
 Std Dev = 0.0000

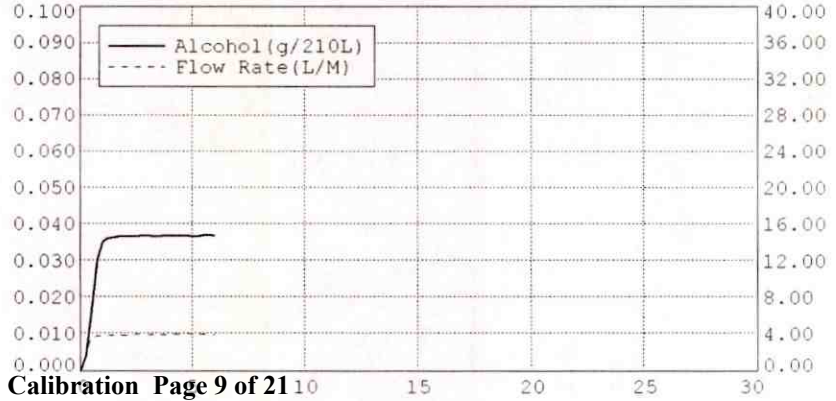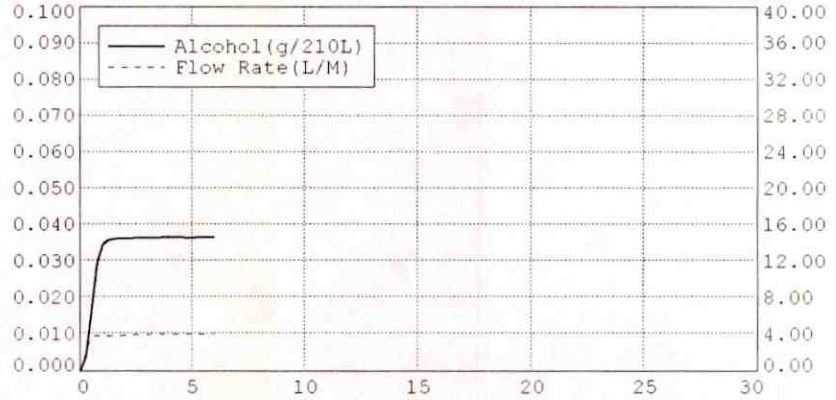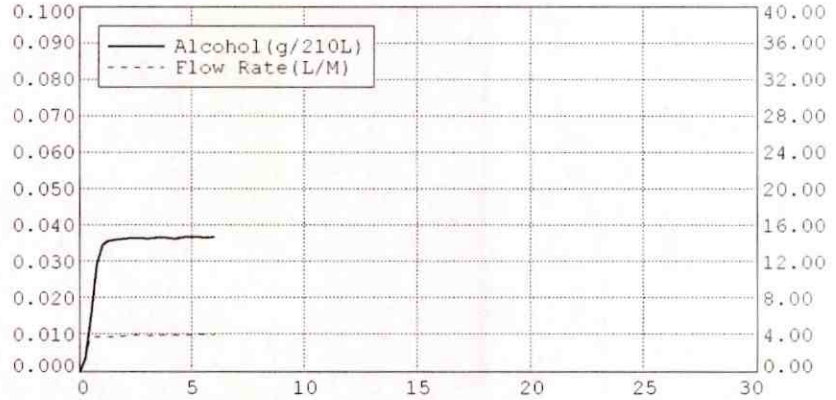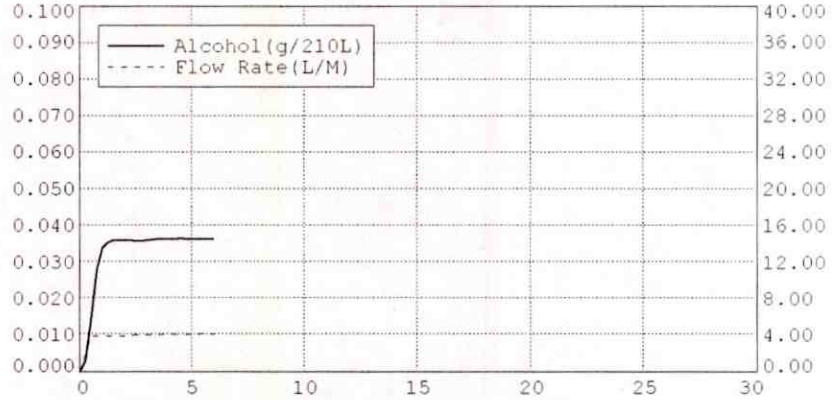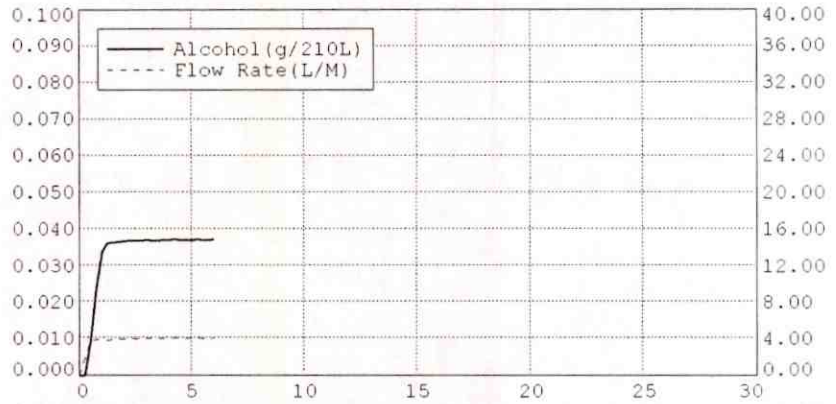

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100345






Date: 11/30/2023  
 Time: 12:25:05

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 28.82: 0.077  
 LOT #: AG310901  
 EXPIRATION: 04/19/2025  
 TANK PRESSURE: 417 psi

BLANK TEST	0.000	12:26
INTERNAL STANDARD	VERIFIED	12:26
EXTERNAL STANDARD	0.075	12:26
BLANK TEST	0.000	12:27
EXTERNAL STANDARD	0.075	12:27
BLANK TEST	0.000	12:28
EXTERNAL STANDARD	0.075	12:28
BLANK TEST	0.000	12:29
EXTERNAL STANDARD	0.075	12:29
BLANK TEST	0.000	12:30
EXTERNAL STANDARD	0.075	12:31
BLANK TEST	0.000	12:31

Average = 0.0750  
 Std Dev = 0.0000

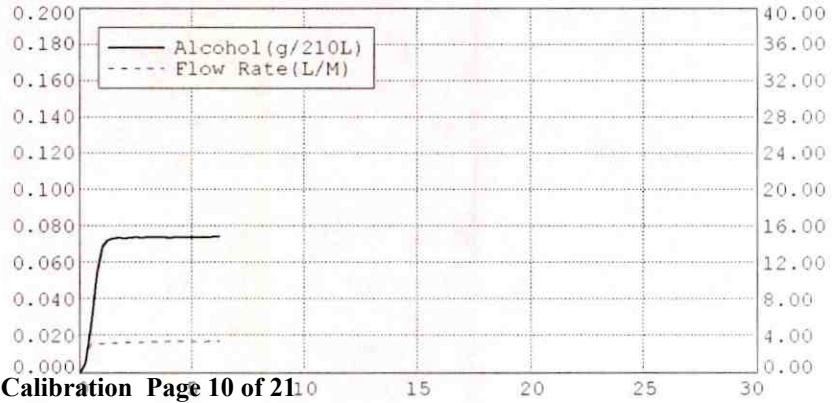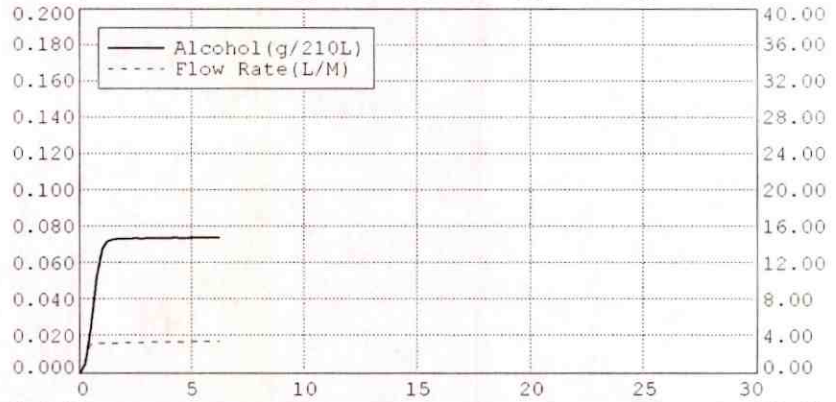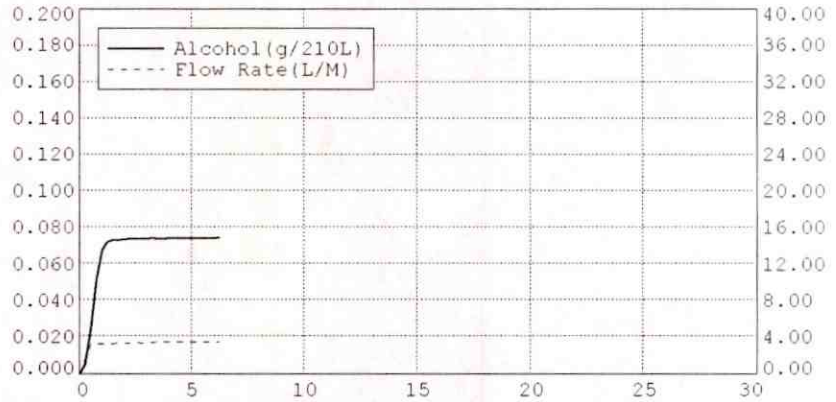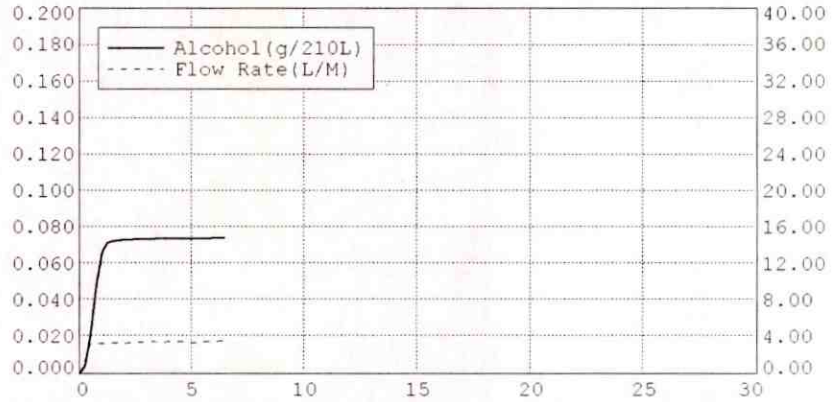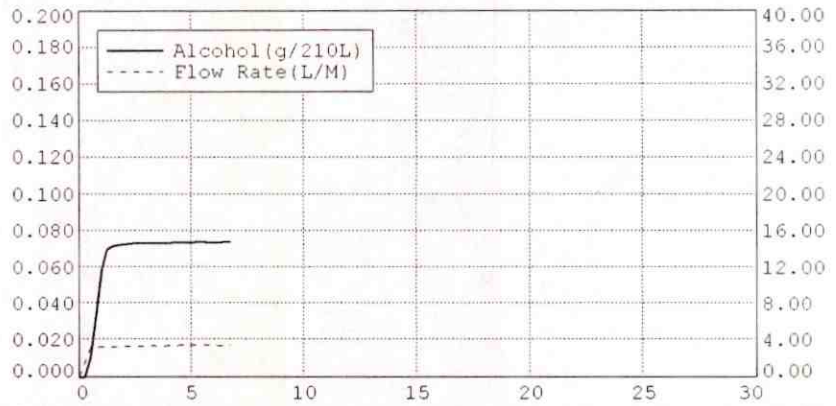



LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100345






Date: 11/30/2023  
 Time: 12:36:38

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 28.82: 0.096  
 LOT #: AG211003  
 EXPIRATION: 04/20/2024  
 TANK PRESSURE: 750 psi

BLANK TEST	0.000	12:38
INTERNAL STANDARD	VERIFIED	12:38
EXTERNAL STANDARD	0.094	12:38
BLANK TEST	0.000	12:39
EXTERNAL STANDARD	0.095	12:39
BLANK TEST	0.000	12:40
EXTERNAL STANDARD	0.095	12:40
BLANK TEST	0.000	12:41
EXTERNAL STANDARD	0.095	12:41
BLANK TEST	0.000	12:42
EXTERNAL STANDARD	0.095	12:42
BLANK TEST	0.000	12:43

Average = 0.0948  
 Std Dev = 0.0004

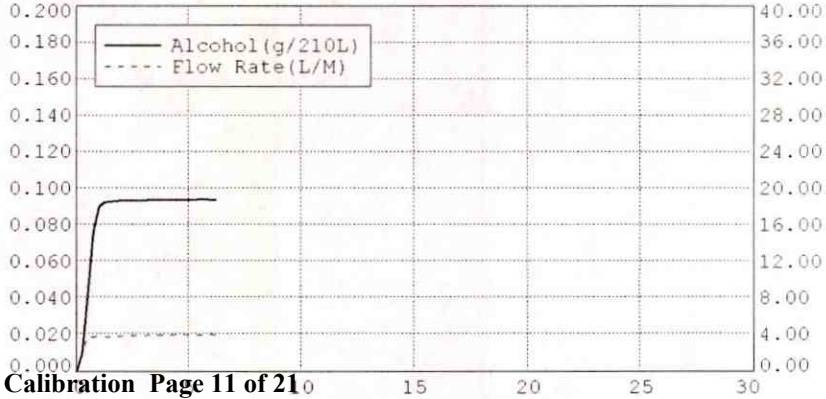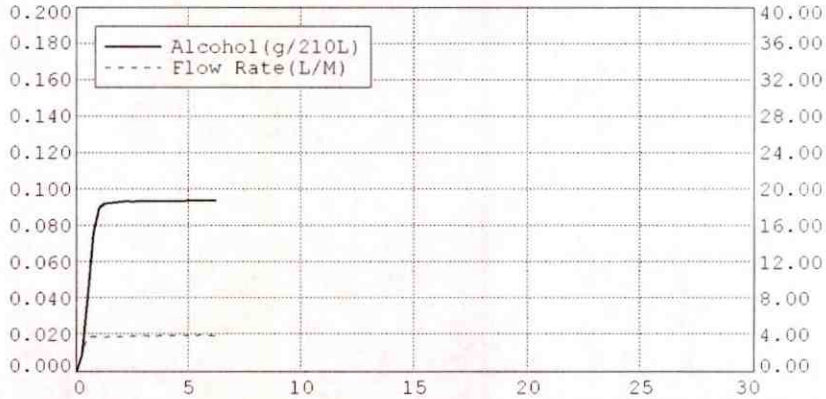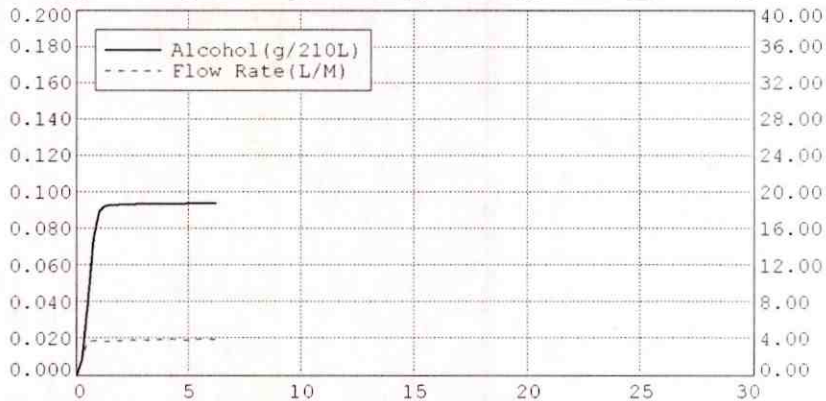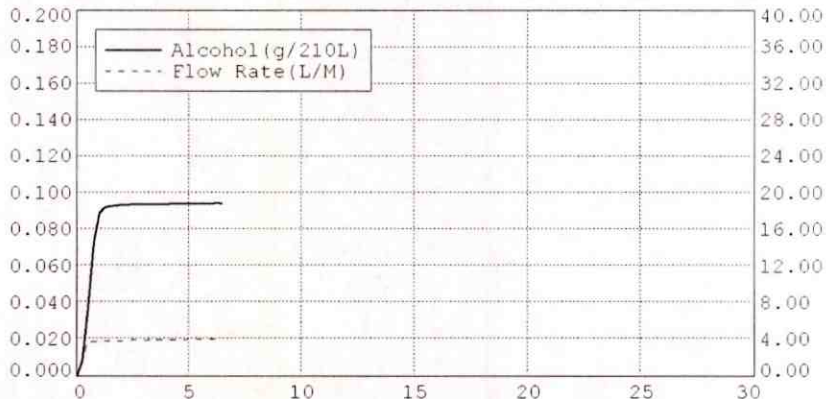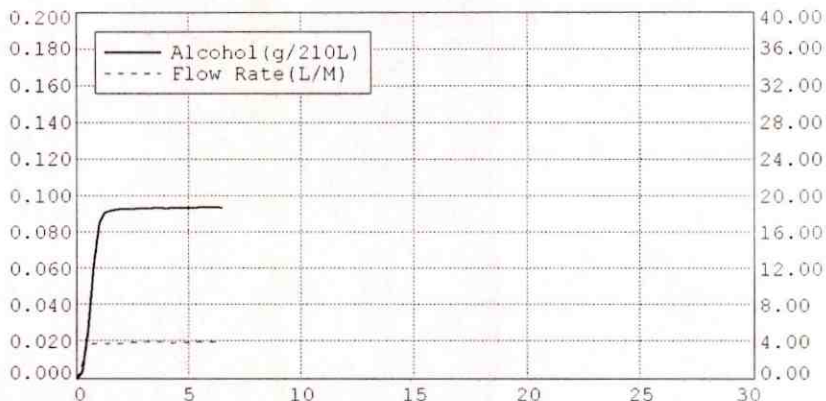



LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
DATAMASTER dmt: 100345






Date: 11/30/2023  
Time: 14:22:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
TARGET AT 28.82: 0.144  
LOT #: AG134205  
EXPIRATION: 12/08/2023  
TANK PRESSURE: 659 psi

BLANK TEST	0.000	14:23
INTERNAL STANDARD	VERIFIED	14:23
EXTERNAL STANDARD	0.142	14:24
BLANK TEST	0.000	14:25
EXTERNAL STANDARD	0.142	14:25
BLANK TEST	0.000	14:26
EXTERNAL STANDARD	0.142	14:26
BLANK TEST	0.000	14:27
EXTERNAL STANDARD	0.142	14:27
BLANK TEST	0.000	14:28
EXTERNAL STANDARD	0.142	14:28
BLANK TEST	0.000	14:29

Average = 0.1420  
Std Dev = 0.0000

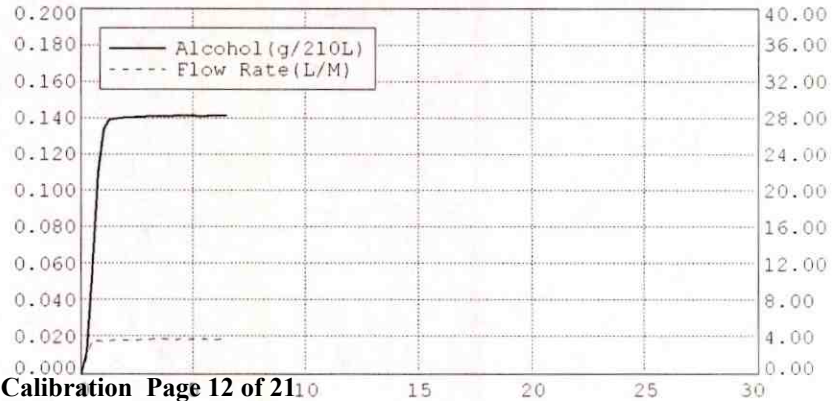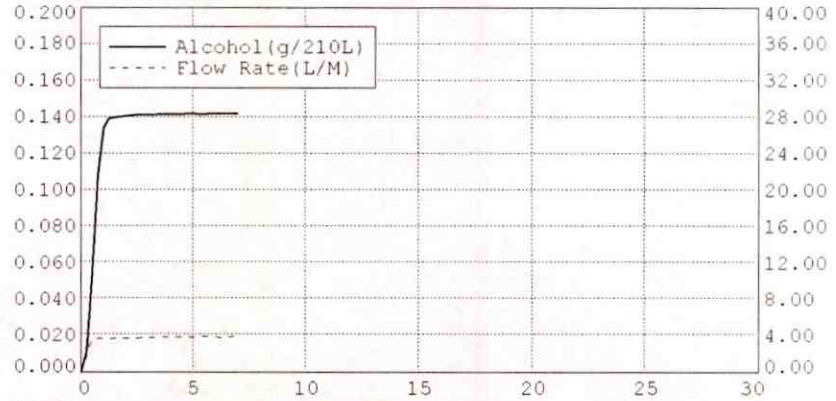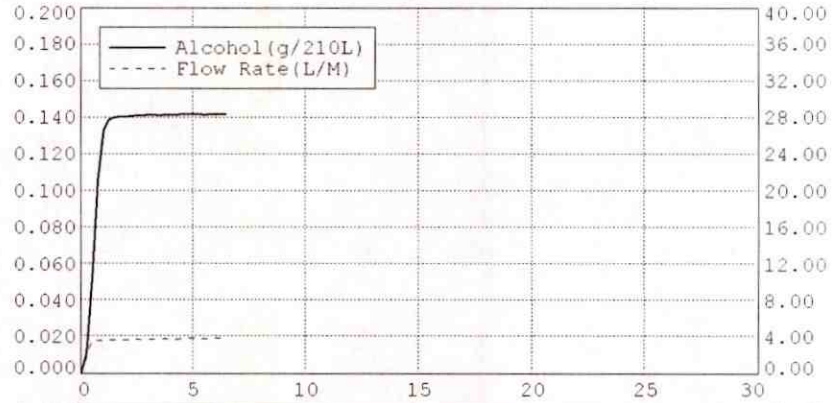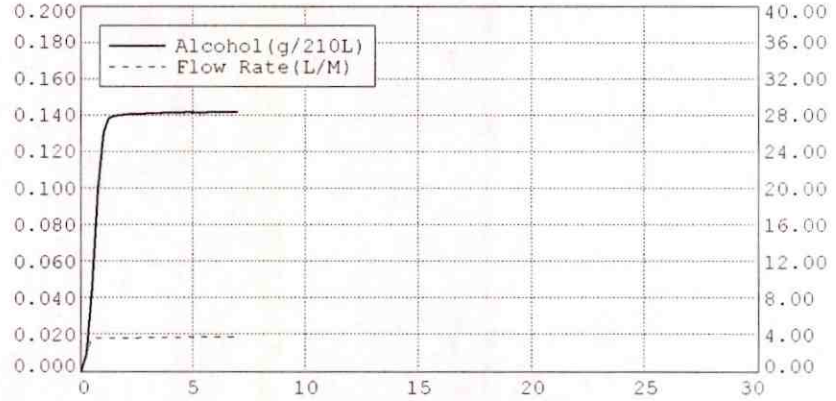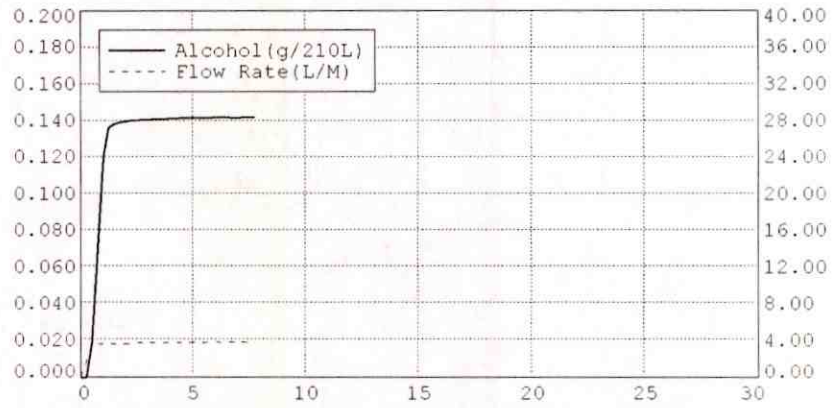

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100345






Date: 11/30/2023  
 Time: 14:39:03

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 28.81: 0.289  
 LOT #: AG217903  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 230 psi

BLANK TEST	0.000	14:40
INTERNAL STANDARD	VERIFIED	14:40
EXTERNAL STANDARD	0.287	14:40
BLANK TEST	0.000	14:41
EXTERNAL STANDARD	0.285	14:41
BLANK TEST	0.000	14:42
EXTERNAL STANDARD	0.286	14:43
BLANK TEST	0.000	14:43
EXTERNAL STANDARD	0.286	14:44
BLANK TEST	0.000	14:45
EXTERNAL STANDARD	0.286	14:45
BLANK TEST	0.000	14:46

Average = 0.2860  
 Std Dev = 0.0007

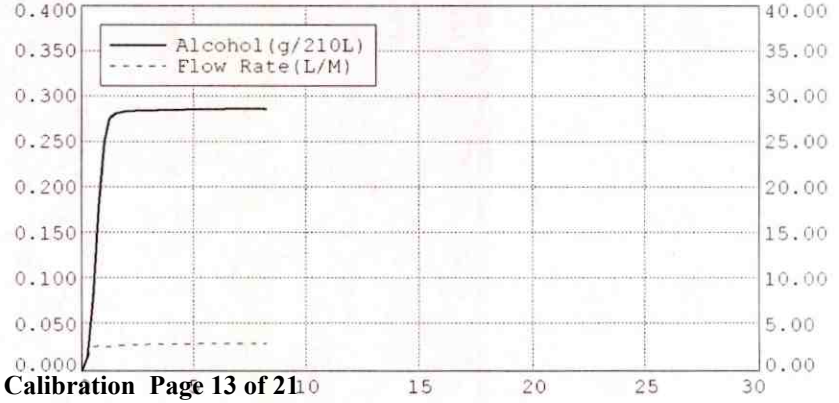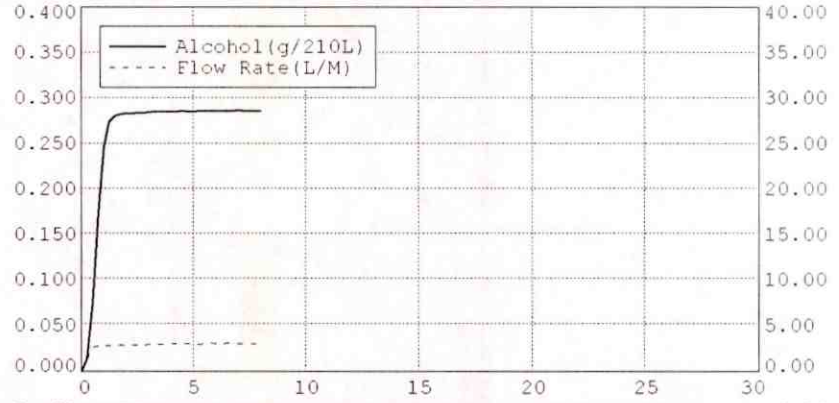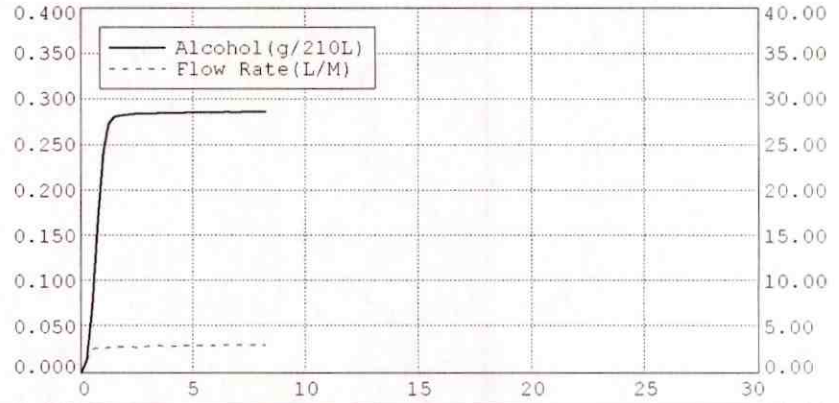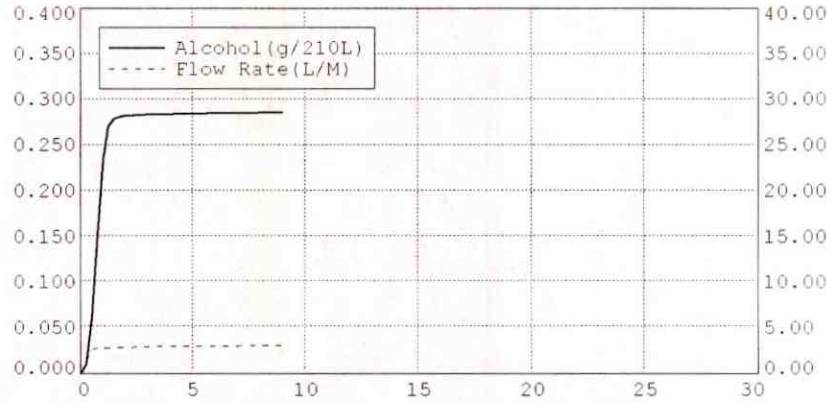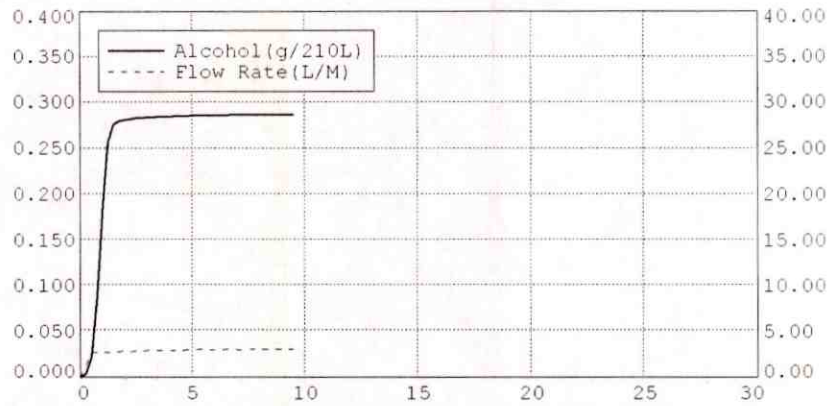

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100345  
-----

Date: 11/30/2023  
Time: 14:59:49

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.83: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 15:00  
BLANK TEST 0.000 15:00  
INTERNAL STANDARD VERIFIED 15:01  
EXTERNAL STANDARD 0.076 15:01  
BLANK TEST 0.000 15:02  
SUBJECT SAMPLE INCOMPLETE 15:04

QY6





SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100345

Date: 12/01/2023

Time: 08:51:38

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

MAXIMUM ATTEMPTS EXCEEDED

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 28.95: 0.077

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD


BLANK TEST

SUBJECT SAMPLE

PASSED	08:52
0.000	08:52
VERIFIED	08:52
0.075	08:53
0.000	08:54
XXX	08:54

Maximum Attempts Exceeded

CKG

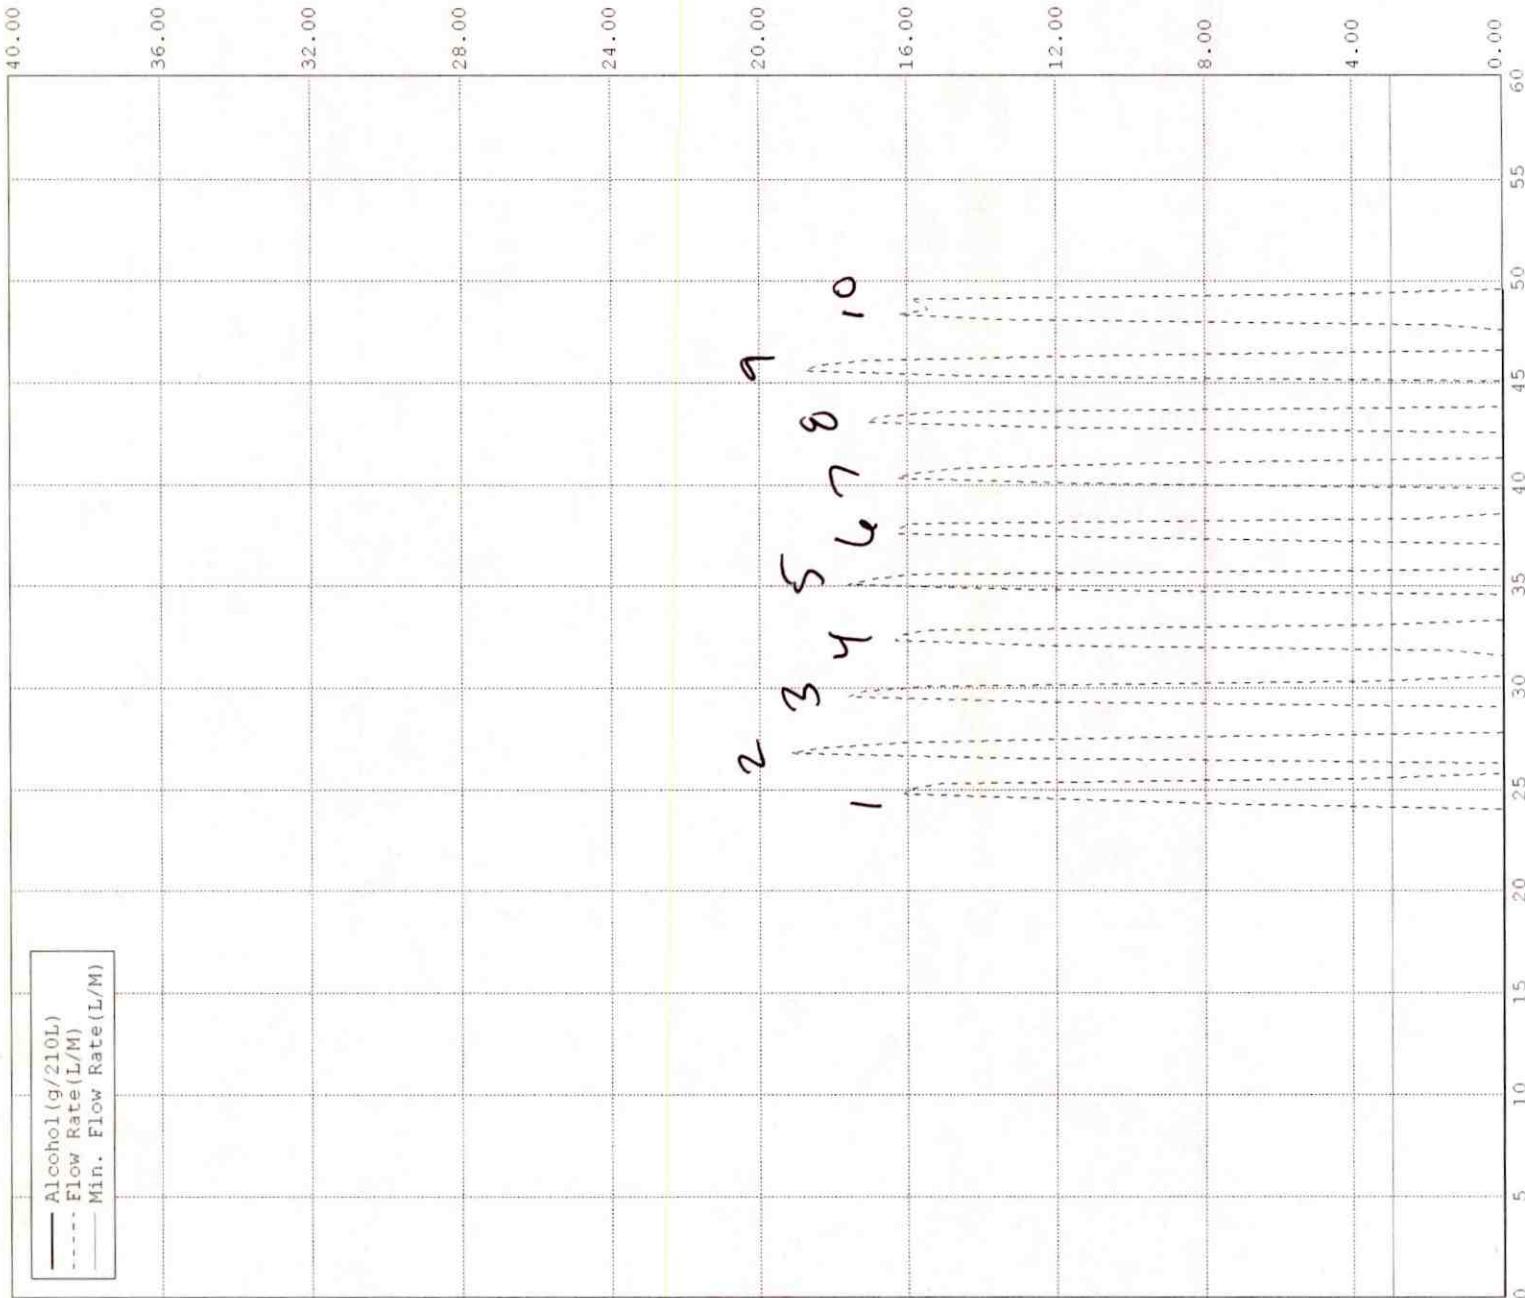

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100345

Date: 12/01/2023  
Time: 09:10:20


SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INVALID  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 28.94: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK  
BLANK TEST PASSED 09:15  
INTERNAL STANDARD VERIFIED 09:16  
EXTERNAL STANDARD 0.076 09:16  
BLANK TEST 0.000 09:17  
SUBJECT SAMPLE INVALID 09:18

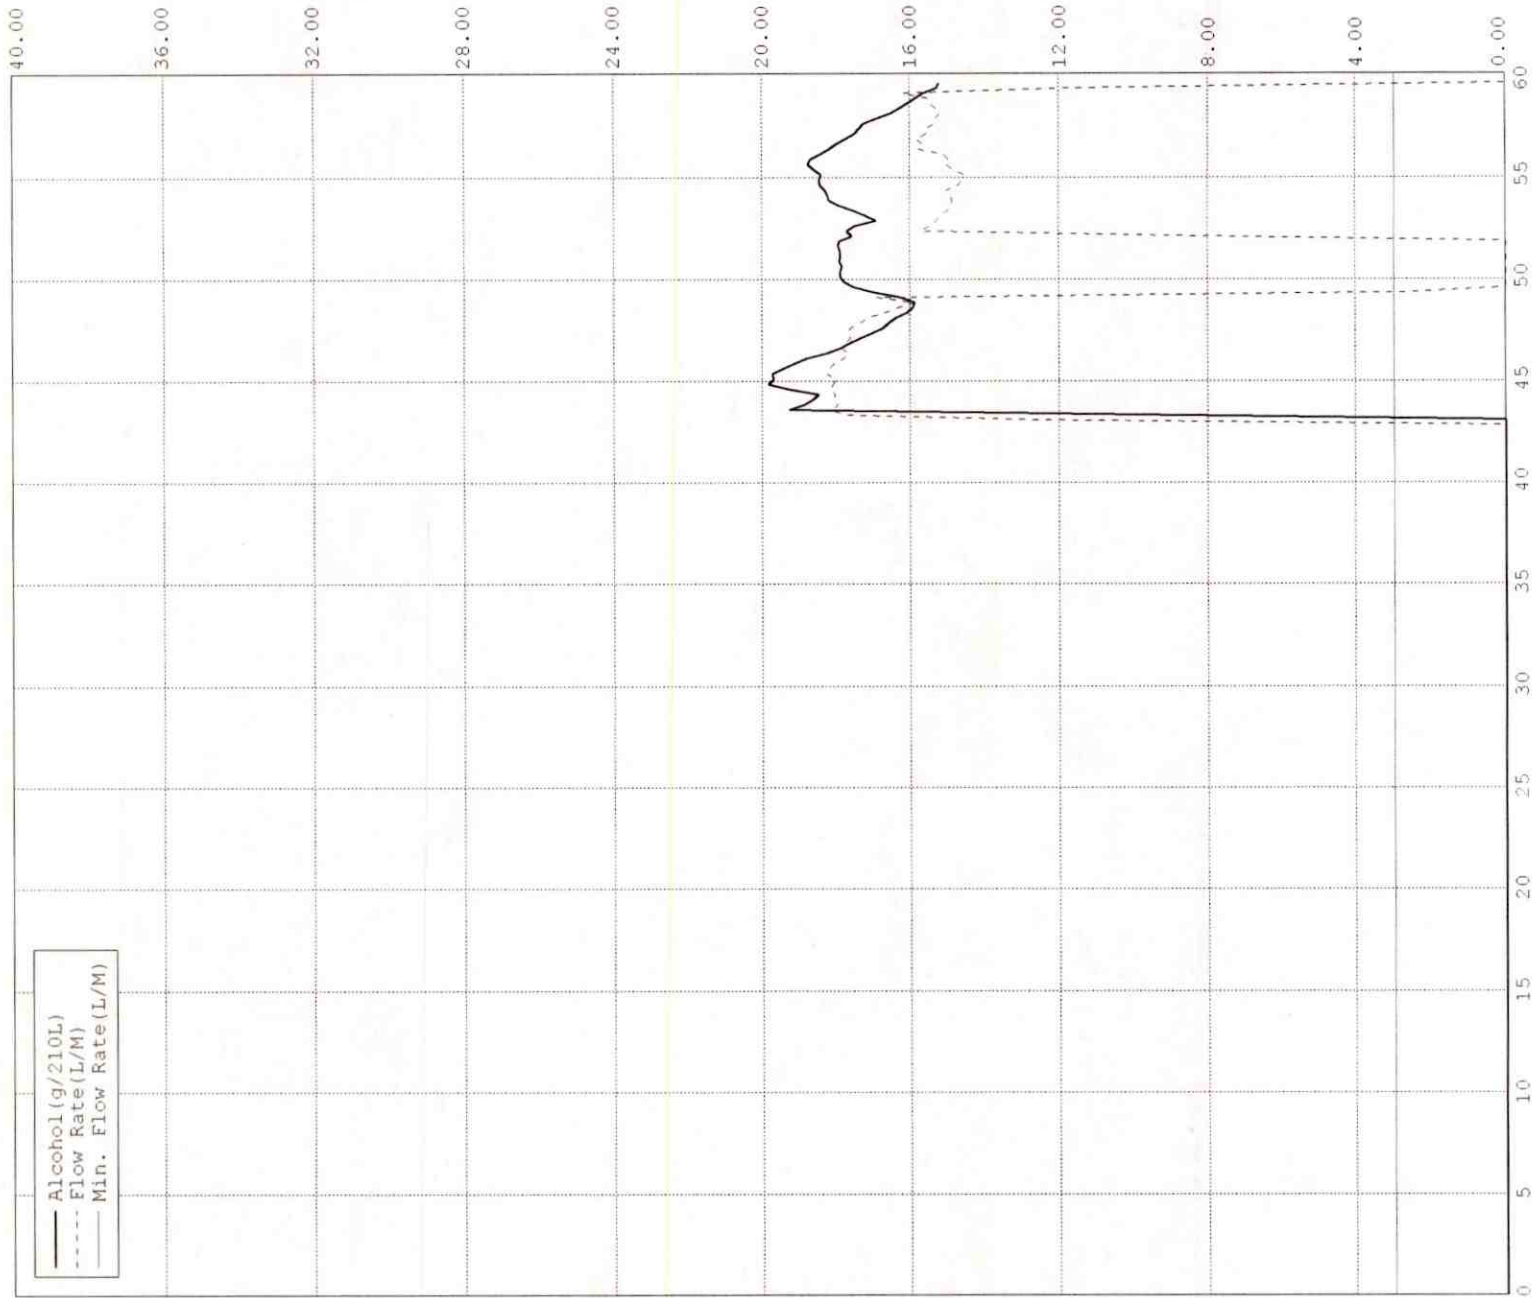

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100345

Date: 12/01/2023

Time: 09:27:32

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

RFI

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 28.94: 0.077

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

PASSED 09:29


0.000 09:29

VERIFIED 09:29

0.076 09:29

0.000 09:30

RFI DETECTED

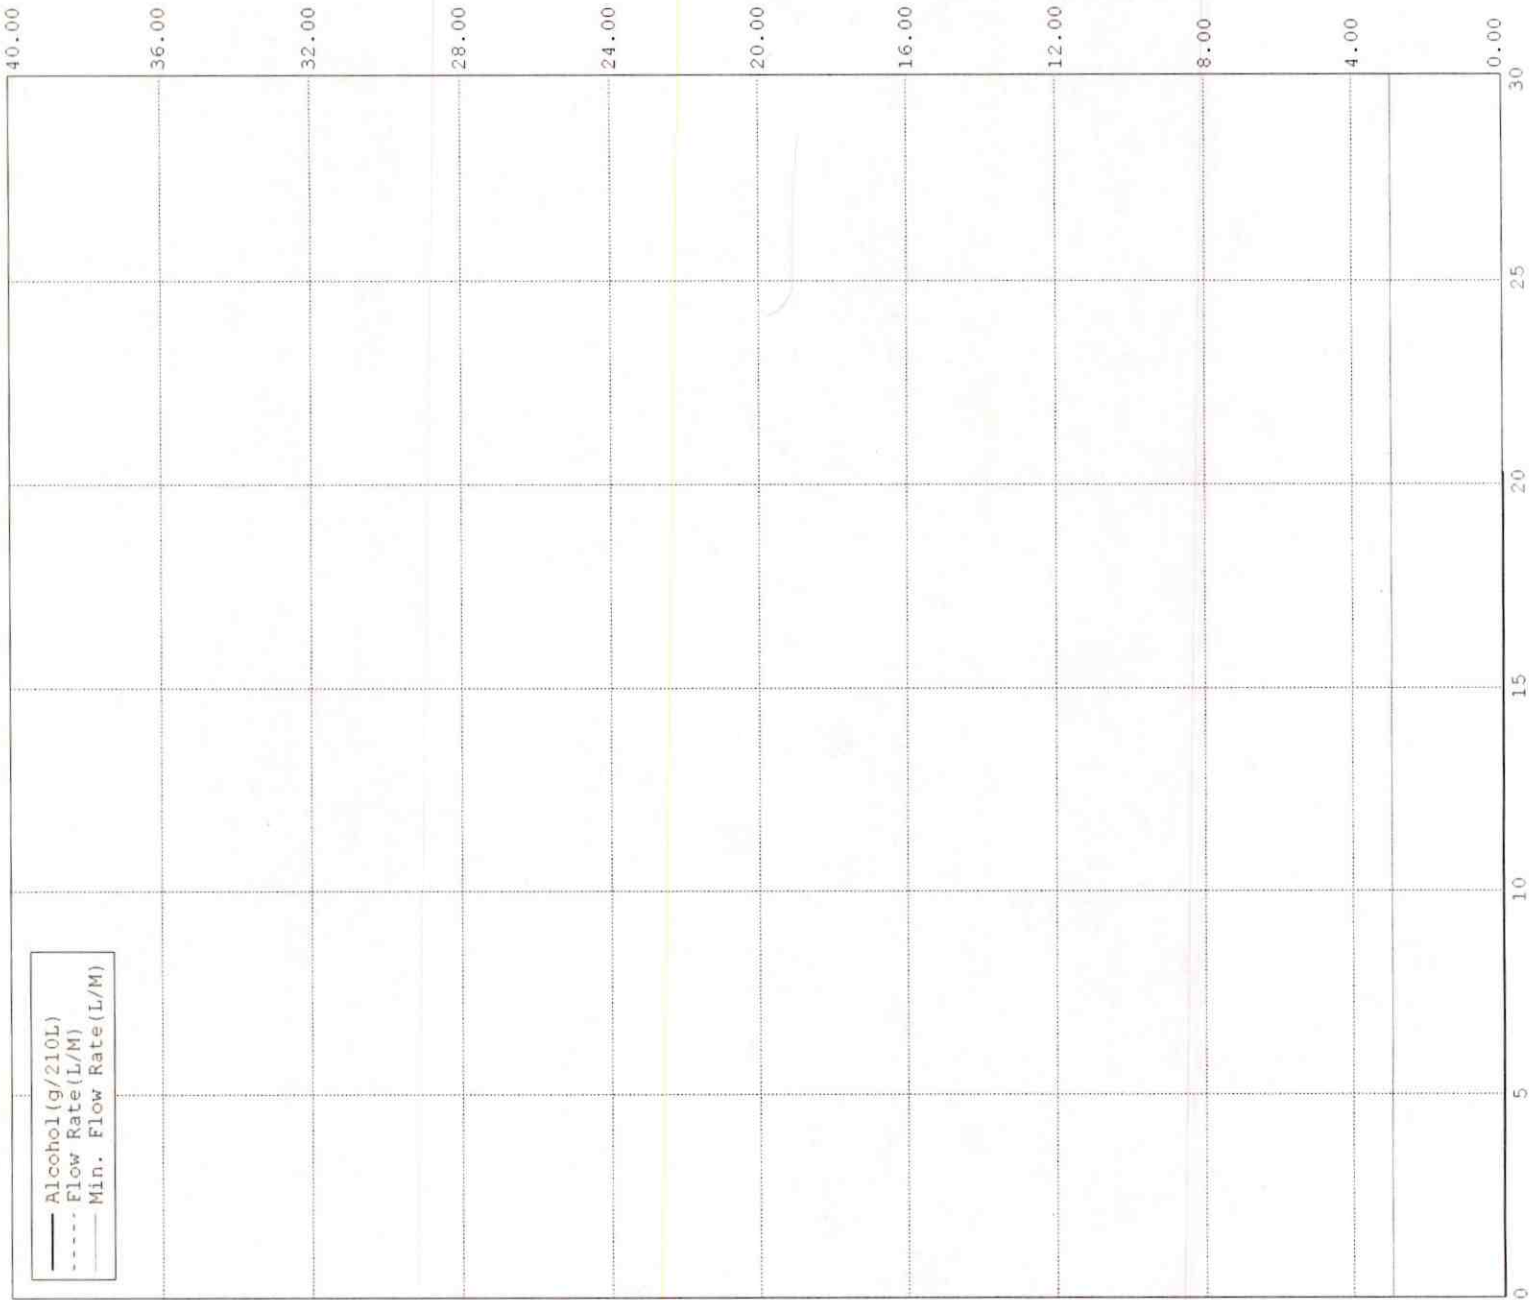



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100345

Date: 12/01/2023  
Time: 09:54:12

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE ACETONE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.96: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025


DIAGNOSTIC CHECK	PASSED	09:55
BLANK TEST	0.000	09:56
INTERNAL STANDARD	VERIFIED	09:56
Xq = 0.094 (0.09%)		
EXTERNAL STANDARD	0.076	09:56
X[1] = 0.0759 (-0.0013) (0.0016)		
BLANK TEST	0.000	09:57
SUBJECT SAMPLE	XXX	09:58
X[1] = 0.1080 (-0.0190) (0.0020)		

Interference Detected

*Filter 2 Average: -0.0011*

*Filter 3 Average: 0.0019*

*CMB 12/4/23*

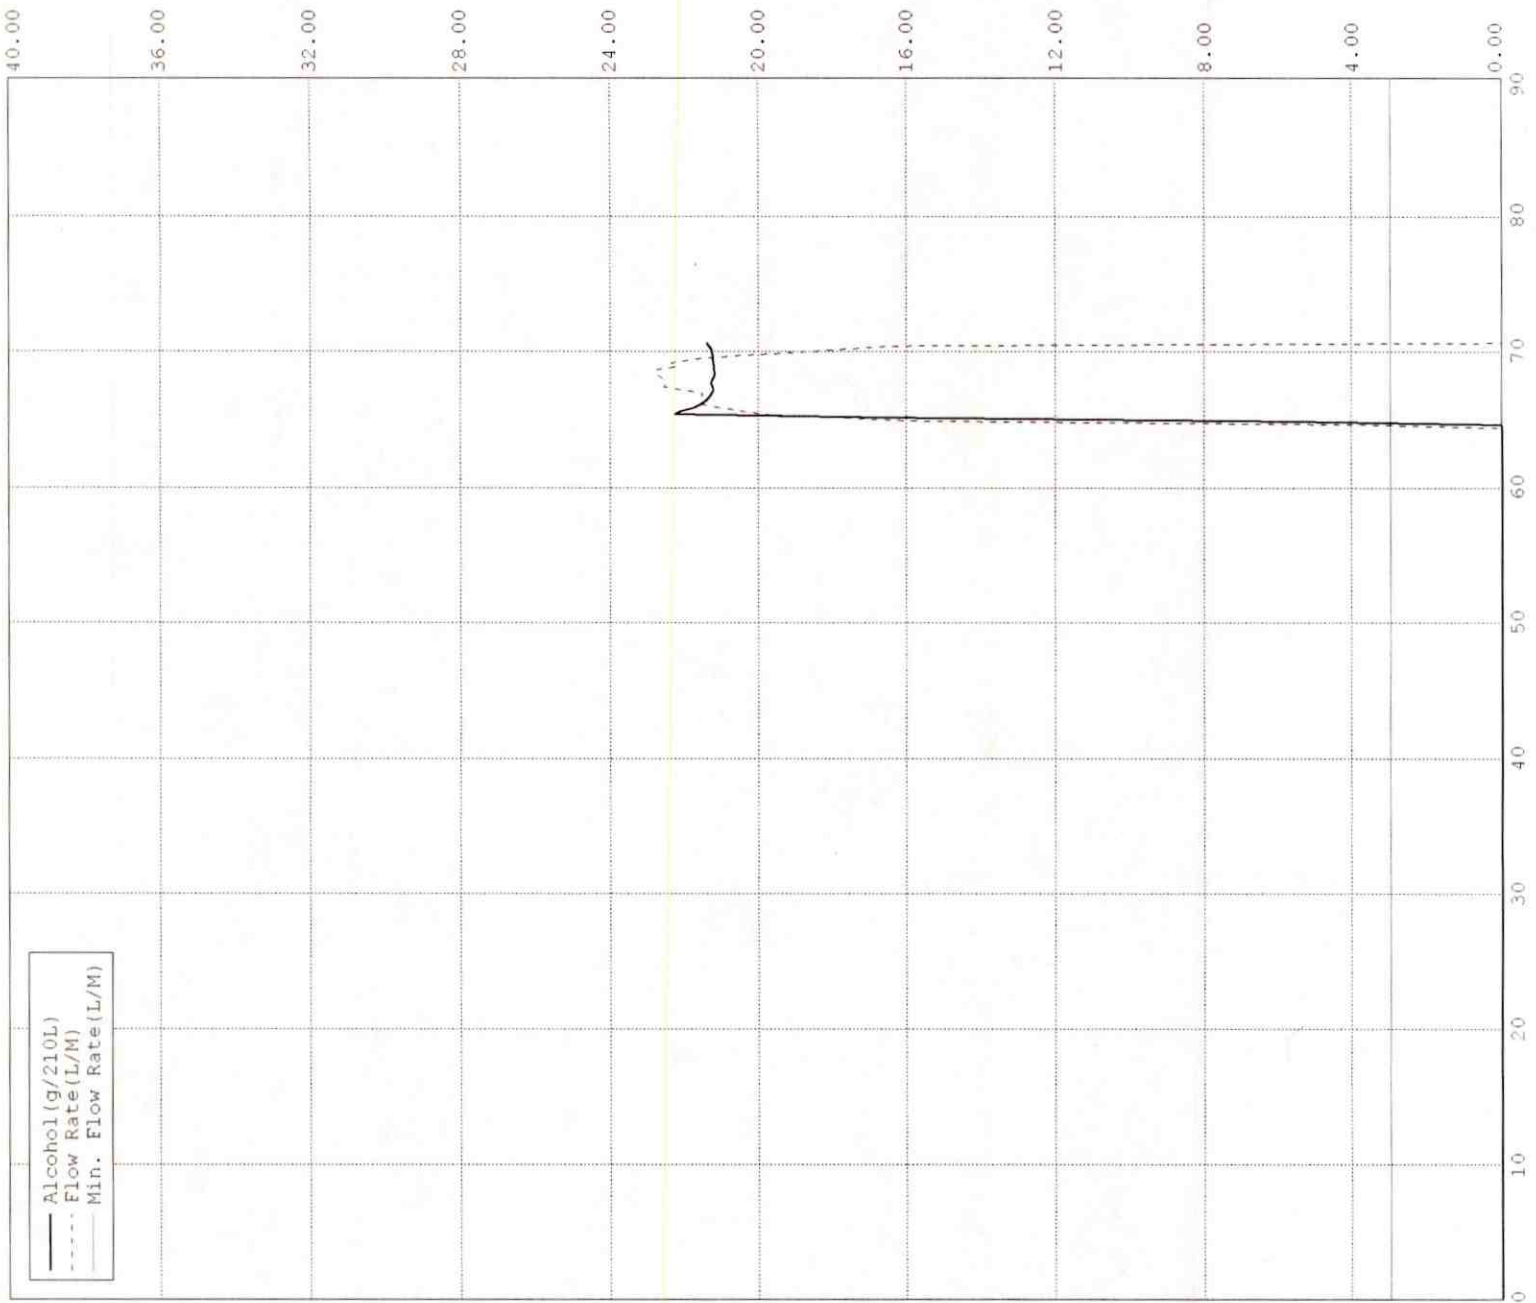

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100345

Date: 12/01/2023  
Time: 09:47:11

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
INTERFERENCE IPA  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.96: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	09:48
BLANK TEST	0.000	09:48
INTERNAL STANDARD	VERIFIED	09:48
Xq = 0.094 (0.09%)		
EXTERNAL STANDARD	0.076	09:48
X[1] = 0.0756 (-0.0012) (0.0026)		
BLANK TEST	0.000	09:49
SUBJECT SAMPLE	XXX	09:50
X[1] = 0.1183 (-0.0322) (0.0010)		

Interference Detected

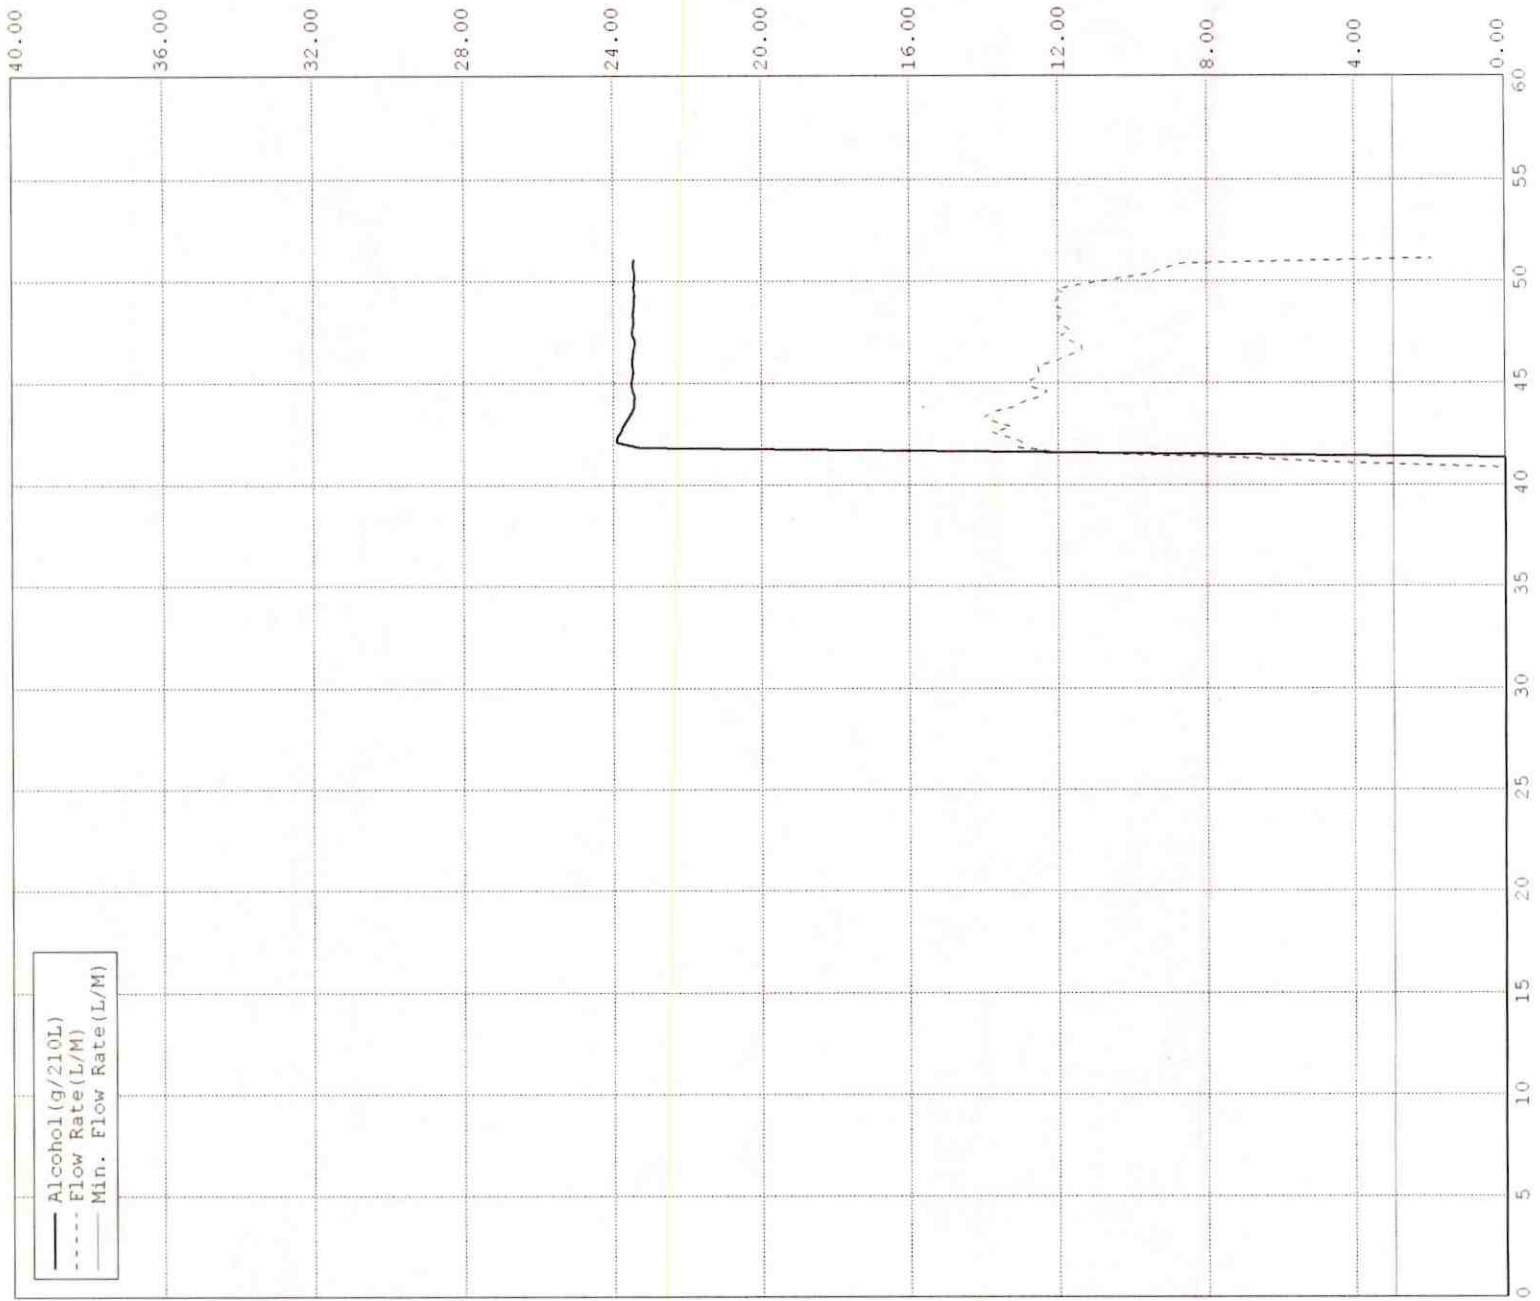

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100345  
-----

Date: 12/01/2023  
Time: 10:01:02

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE NEGATIVE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.96: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	10:02
BLANK TEST	0.000	10:02
INTERNAL STANDARD	VERIFIED	10:02
EXTERNAL STANDARD	0.076	10:02
Xq = 0.094 (0.28%)		
X[1] = 0.0758 (-0.0011)	(0.0016)	
BLANK TEST	0.000	10:03
SUBJECT SAMPLE (Vol=2.08L)	0.087	10:04
X[1] = 0.0876 (-0.0026)	(-0.0004)	
BLANK TEST	0.000	10:04
EXTERNAL STANDARD	0.075	10:05
X[1] = 0.0752 (-0.0006)	(0.0017)	
BLANK TEST	0.000	10:06

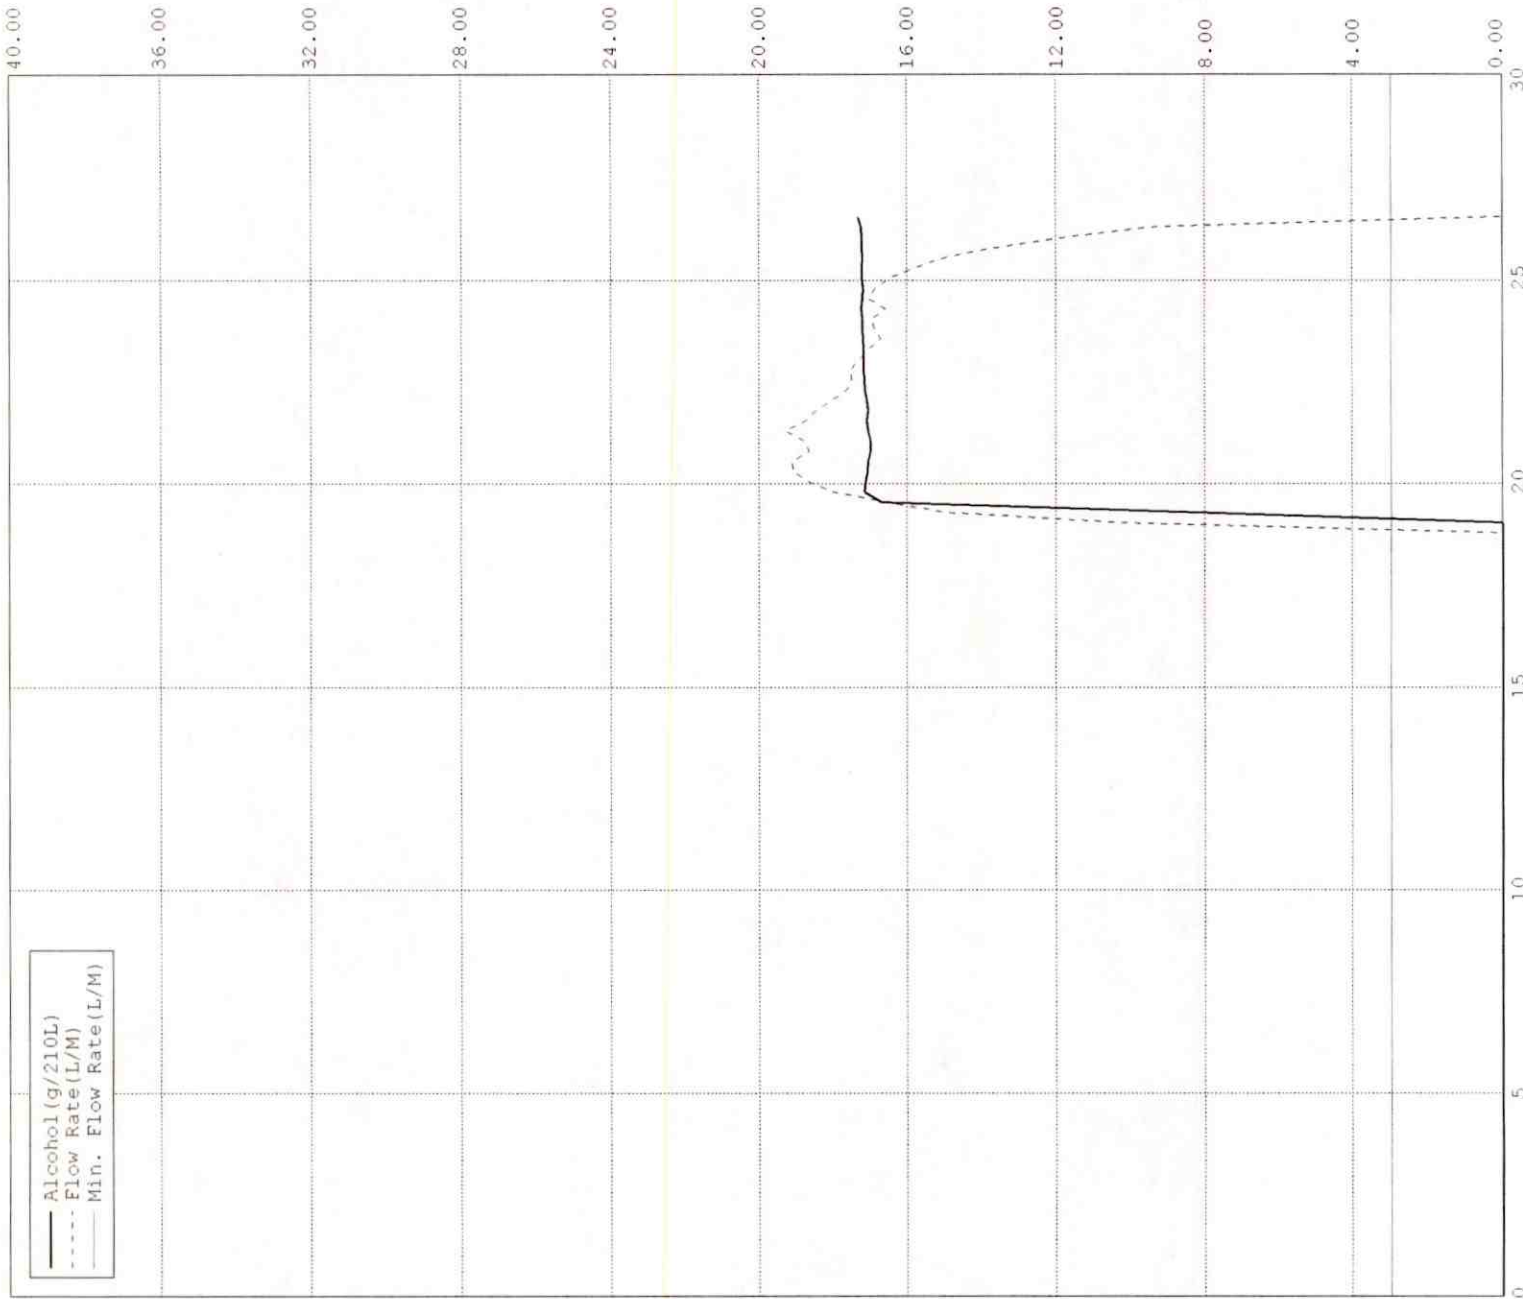



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100345

Date: 12/01/2023  
Time: 10:26:50

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 28.97: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	10:34
BLANK TEST	0.000	10:34
INTERNAL STANDARD	VERIFIED	10:34
EXTERNAL STANDARD	0.076	10:34
BLANK TEST	0.000	10:35
SUBJECT SAMPLE (Vol=1.81L)	0.000	10:35
BLANK TEST	0.000	10:36
EXTERNAL STANDARD	0.076	10:37
BLANK TEST	0.000	10:38

CKG

