

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100685

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 09/30/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.75: 0.080
LOT #: 01315080A2
EXPIRATION: 02/05/2017
TANK PRESSURE: 919 psi

BLANK TEST	0.000	14:50
INTERNAL STANDARD	VERIFIED	14:50
EXTERNAL STANDARD	0.080	14:50
BLANK TEST	0.000	14:51
EXTERNAL STANDARD	0.080	14:52
BLANK TEST	0.000	14:52
EXTERNAL STANDARD	0.080	14:53
BLANK TEST	0.000	14:54
EXTERNAL STANDARD	0.080	14:54
BLANK TEST	0.000	14:55
EXTERNAL STANDARD	0.080	14:55
BLANK TEST	0.000	14:56

Average = 0.0800
Std Dev = 0.0000

Diagnostic Check

VERSIONS

DMT: 3.01
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
Breath Tube = 47.7°C PASSED

PUMP INFO

Flow Rate = 5.606 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO

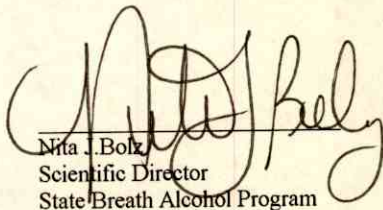
Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

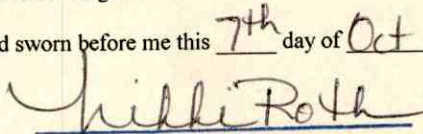
I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

10/7/2015

Subscribed and sworn before me this 7th day of Oct, 20 15


Nikki Roth, Notary Public
My Commission Expires With Office



BMB
9 BMB 10/2/15
10/2/15