




State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100365

**Report Issue Date:** 12/06/2024  
**Date Received:** 2024-10-28  
**Condition of Item:** No apparent damage

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.019	0.020	0.020	0.020	0.020	0.020
0.080	0.079	AG335202	0.079	0.078	0.078	0.078	0.078	0.078
0.300	0.296	AG427706	0.292	0.292	0.292	0.292	0.293	0.292

As Found - Evaluation Analyst: Megan Carlock  
 As Found Conditions - Barometric Pressure (inHg): 29.46 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.1 Relative Humidity (%): 17  
 As-Found Lab Activity Date Range: 10/28/2024 - 10/29/2024

Replaced O-ring. Filter wheel error occurred on first VOC; the second VOC passed.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG408002	0.019	0.019	0.019	0.019	0.020	0.019	+/- 0.002
0.040	0.039	AG407908	0.038	0.038	0.038	0.038	0.038	0.038	+/- 0.003
0.080	0.077	AG335202	0.075	0.077	0.076	0.076	0.076	0.076	+/- 0.004
0.100	0.096	AG333401	0.095	0.095	0.095	0.095	0.096	0.095	+/- 0.004
0.150	0.145	AG332004	0.140	0.140	0.141	0.140	0.140	0.140	+/- 0.006
0.300	0.289	AG427706	0.283	0.283	0.283	0.282	0.282	0.283	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 28.86 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.9 Relative Humidity (%): 19  
 As-Left Lab Activity Date Range: 11/07/2024 - 11/07/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Kaija Swisher on 12/03/2024

[kaija.swisher@alaska.gov](mailto:kaija.swisher@alaska.gov)

Technically and administratively reviewed by Carlie Glaister on 12/06/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100365 Analyst or Technician Name: Kaya Swisher

DataMaster DMT Calibration Start Date: 11/7/24

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage
  - (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 230307229  
Calibration Due Date: 5/2/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 28.86 Temperature(C) 21.9 Relative Humidity(%) 19

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20241107KS Expiration Date: 2/7/25  
Simulator S/N: DR4161 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20241107KS Expiration Date: 2/7/25  
Simulator S/N: DR5298 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 232941233 Expiration Date: 2/7/25  
Simulator S/N: DR4163 Thermometer Verification Performed?

The second exp date is  
09/20/2025  
KS 12/2/24

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 9/19/25

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 11/7/24

Data Interpretation Date (Technician): NK (if applicable)

Data Interpretation Date (Analyst): 11/7/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100365  
-----

Date: 11/07/2024  
Time: 09:18:40

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C                    PASSED  
(44.0°C - 52.0°C)  
Breath Tube        = 45.8°C                PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage     = 2.02 V                   PASSED  
(1.21 V - 2.83 V)  
Cooler Voltage   = 1.82 V                   PASSED  
(1.09 V - 2.55 V)  
Bias Voltage     = 80 V                     PASSED  
(47 V - 111 V)  
Chopper Freq    = 530 Hz                     PASSED  
(475 Hz - 575 Hz)  
Barometer        = 28.9 in

PUMP INFO

Flow Rate = 4.423 L/M                    PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON                                    PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF                                  PASSED  
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1                                   PASSED  
Filter 2                                   PASSED  
Filter 3                                   PASSED

INTERNAL STANDARD

Xq = 0.093 0.19% (0.00% - 4.00%)                    PASSED

Technician Screen

-----  
DATAMASTER dmt: 100365  
-----

Date: 11/07/2024  
Time: 9:45 AM

Temperatures (°C)  
Sample Cell: 49.0°C  
Breath Tube: 45.6°C

Current Barometer 28.9 in  
Volume (Itr) 1.59

Settings  
Lamp: 2.02 V  
Bias: 79 V  
Cooler: 1.83 V  
Chopper: 530 Hz

Voltages (V)  
Flow: 1.04 V  
Detector: 0.093 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100365  
-----

Date: 11/06/2024  
Time: 13:50:21

OPERATOR NAME:  
KAIJA SWISHER  
CERTIFICATE #: 10746

Ca = 0.1000  
CAL = 0.983493    0.800 <= CAL < 1.200  
b1 = 0.0004    0.0000 <= b1 < 0.0040  
b2 = 0.0056    0.0010 <= b2 < 0.0100  
b3 = 0.0002    0.0000 <= b3 < 0.0040  
Xq = 0.0931    0.0500 <= Xq < 0.2000  
a21 = 1.171826    1.050 <= a21 < 1.300  
a31 = 0.450343    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100365

Date: 11/07/2024  
 Time: 09:55:24

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXX

OPERATOR NAME:  
 KAIJA SWISHER  
 OPERATOR'S #: 10746


DEPT/AGENCY:  
 MINIMUM VOLUME TEST  
 CASE/REPORT: XXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 28.87: 0.077  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	09:57
BLANK TEST	0.000	09:57
INTERNAL STANDARD	VERIFIED	09:58
EXTERNAL STANDARD	0.075	09:58
BLANK TEST	0.000	09:59
SUBJECT SAMPLE (Vol=1.56L)	0.000	10:00
BLANK TEST	0.000	10:01
EXTERNAL STANDARD	0.076	10:01
BLANK TEST	0.000	10:02

KS

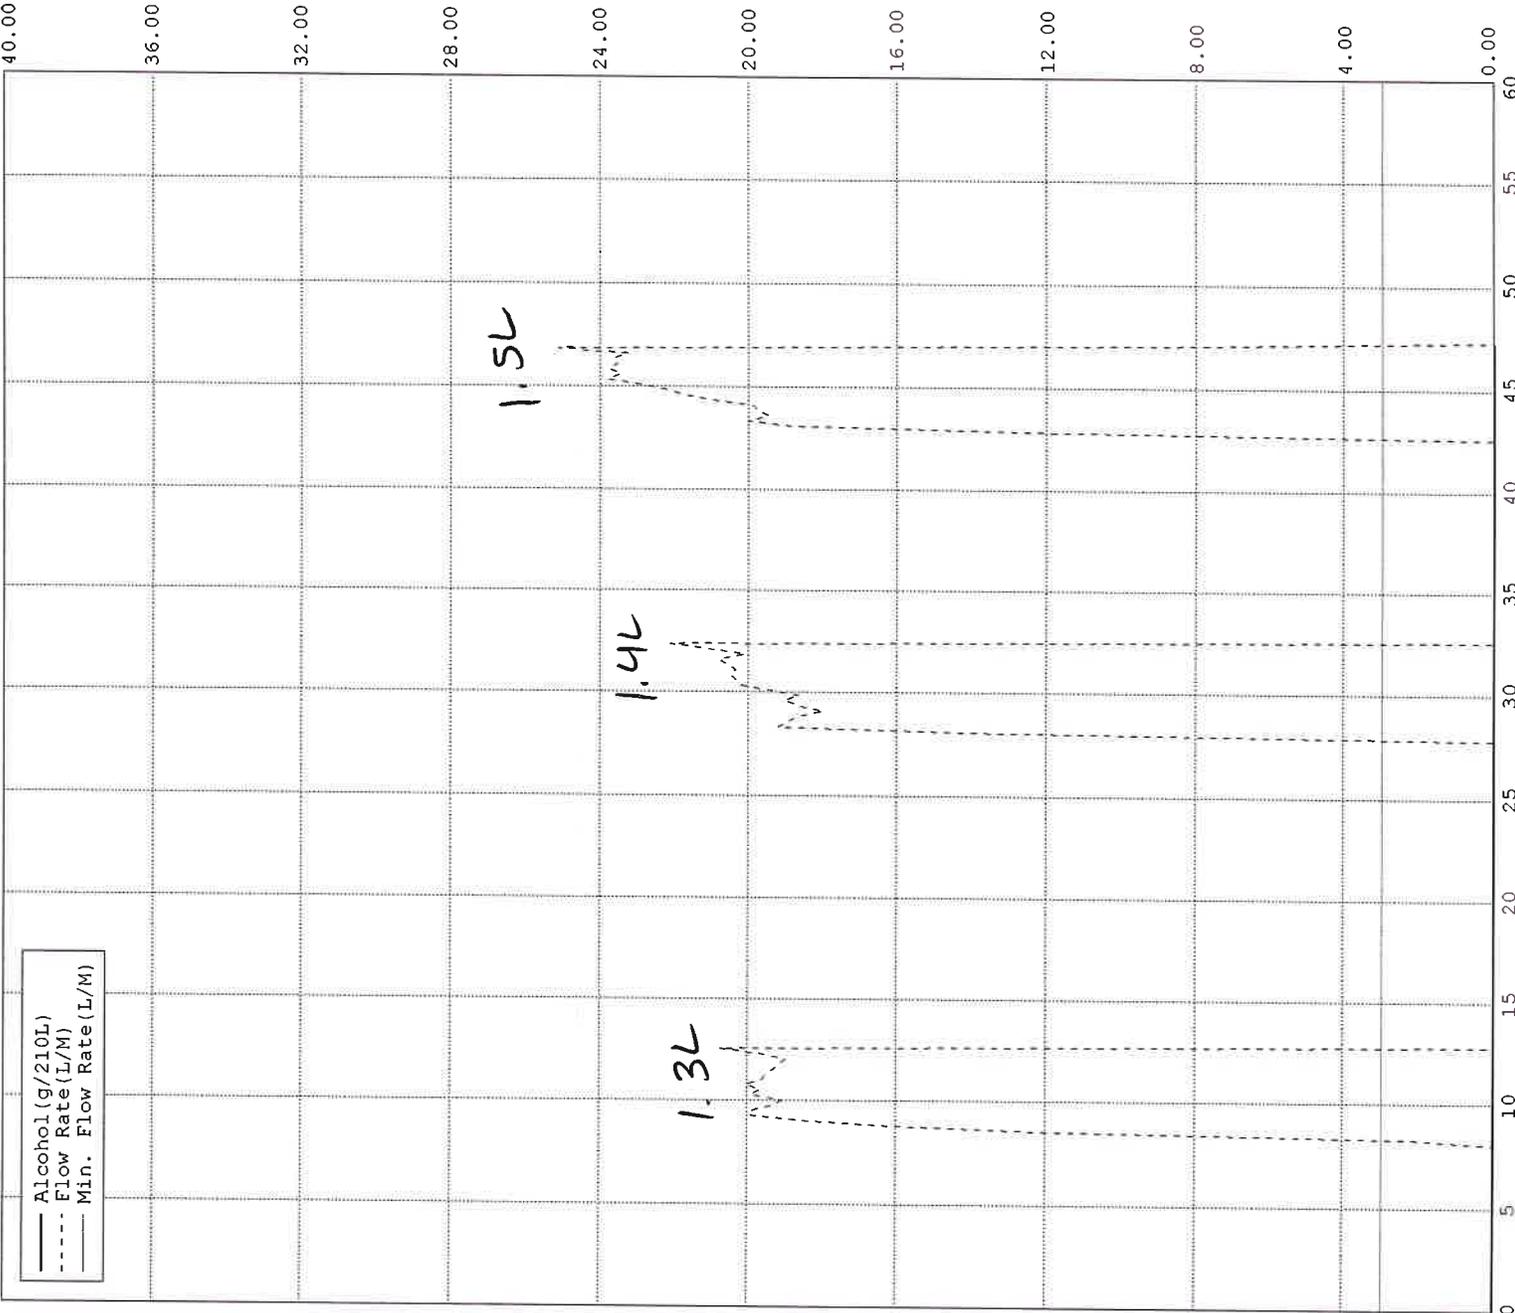

LINEARITY CHECK


Alaska Department of Public Safety  
 DATAMASTER dmt: 100365

Date: 11/07/2024  
 Time: 10:13:11

SUPERVISOR NAME:  
 KAIJA SWISHER  
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.019	0.0192	0.0004
0.039	0.0380	0.0000
0.077	0.0760	0.0007
0.096	0.0952	0.0004
0.145	0.1402	0.0004
0.289	0.2826	0.0005

SLOPE = 0.974825  
 R<sup>2</sup> = 0.999899

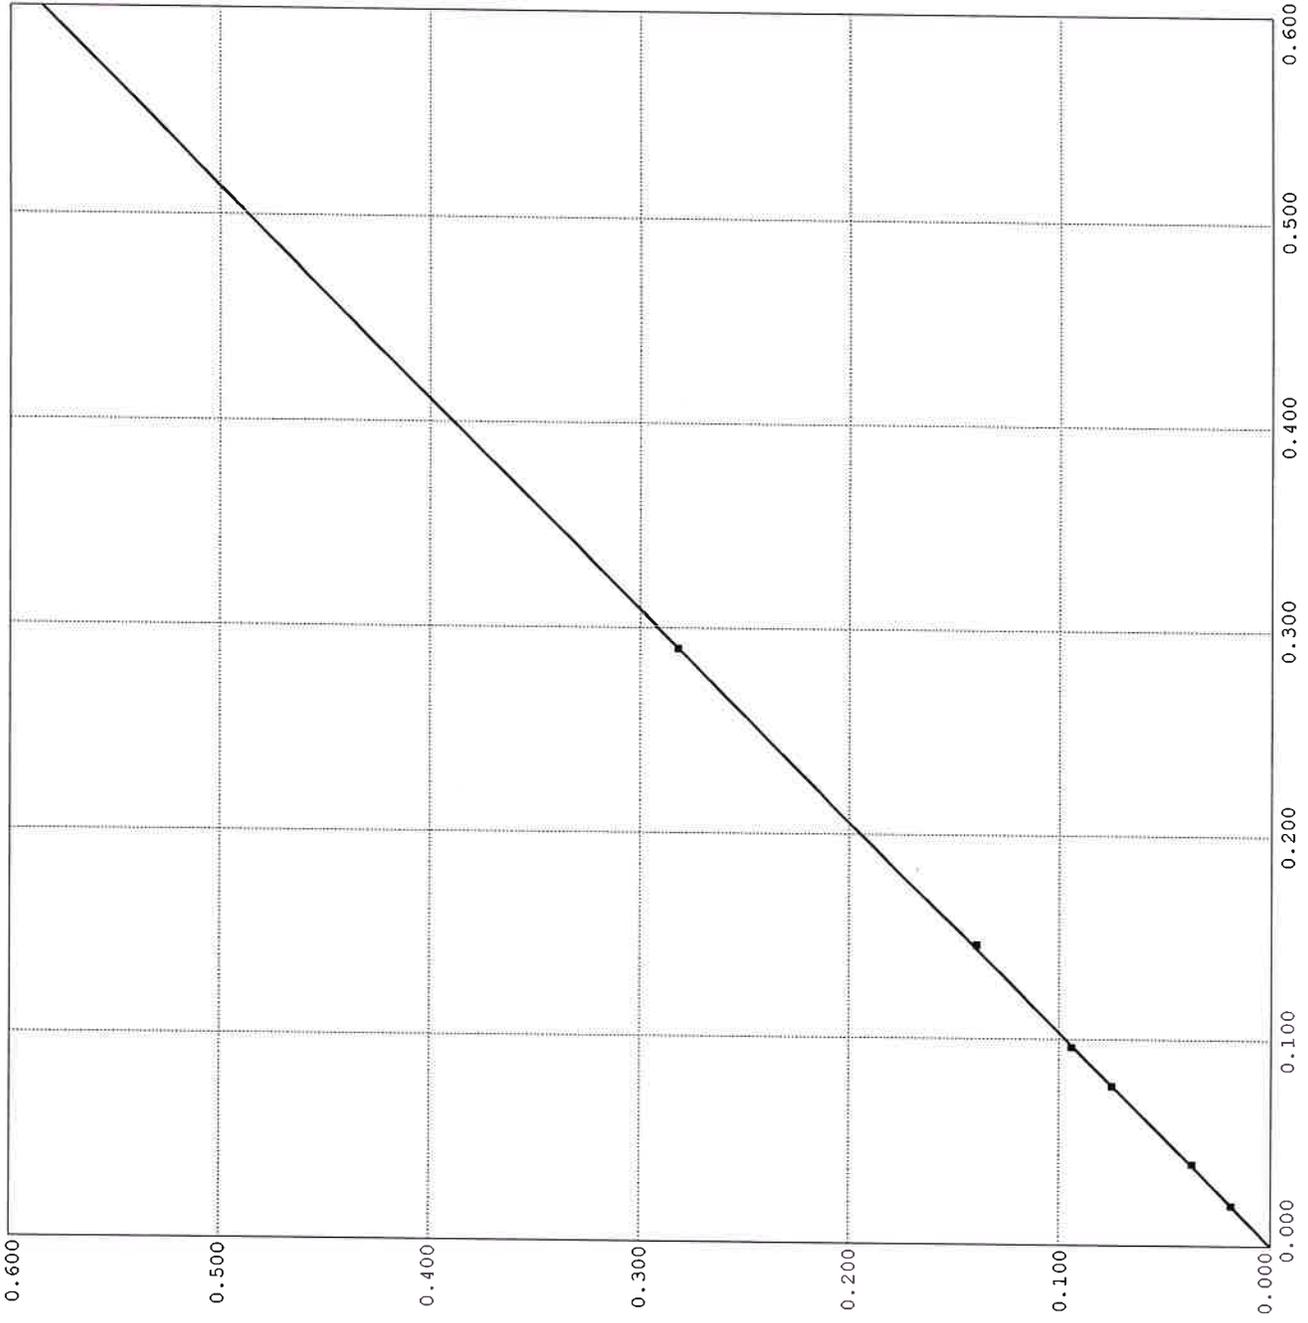

KS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100365






Date: 11/07/2024  
Time: 10:13:13

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 28.86: 0.019  
LOT #: AG408002  
EXPIRATION: 03/20/2026  
TANK PRESSURE: 1053 psi

BLANK TEST	0.000	10:15
INTERNAL STANDARD	VERIFIED	10:15
EXTERNAL STANDARD	0.019	10:16
BLANK TEST	0.000	10:17
EXTERNAL STANDARD	0.019	10:17
BLANK TEST	0.000	10:18
EXTERNAL STANDARD	0.019	10:18
BLANK TEST	0.000	10:19
EXTERNAL STANDARD	0.019	10:19
BLANK TEST	0.000	10:20
EXTERNAL STANDARD	0.020	10:20
BLANK TEST	0.000	10:21

Average = 0.0192  
Std Dev = 0.0004

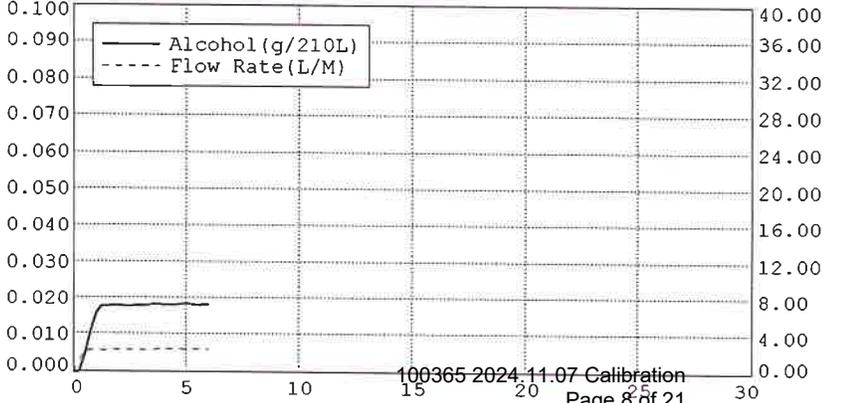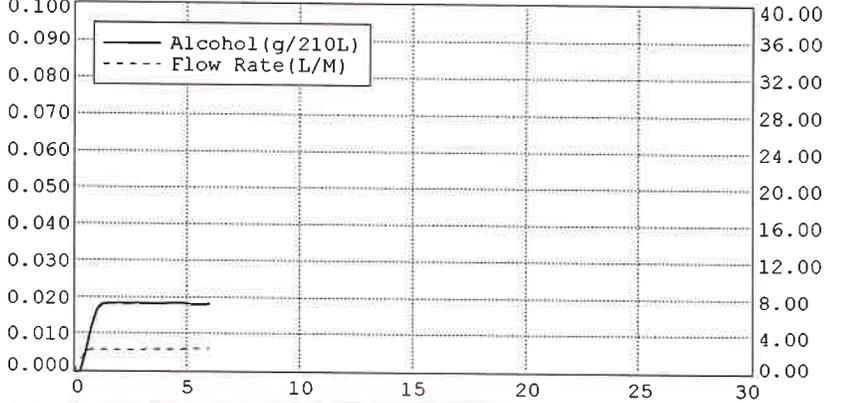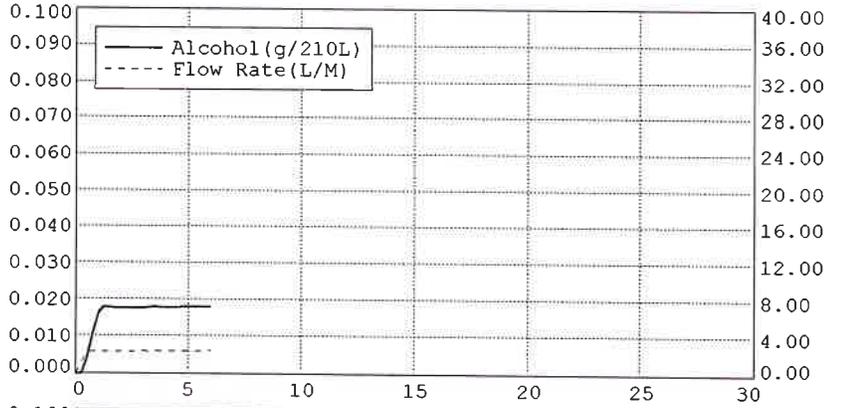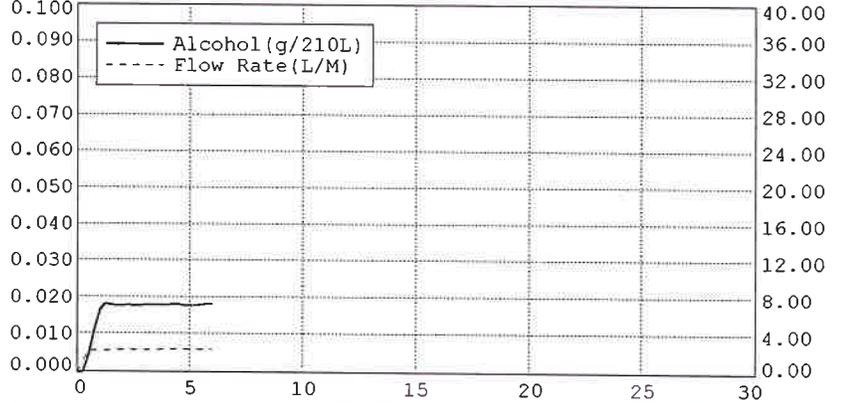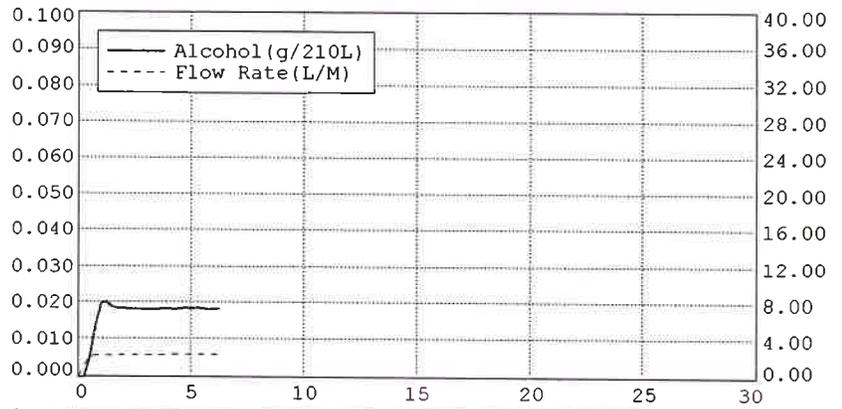

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100365






Date: 11/07/2024  
 Time: 10:24:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 28.85: 0.039  
 LOT #: AG407908  
 EXPIRATION: 03/19/2026  
 TANK PRESSURE: 1051 psi

BLANK TEST	0.000	10:25
INTERNAL STANDARD	VERIFIED	10:25
EXTERNAL STANDARD	0.038	10:25
BLANK TEST	0.000	10:26
EXTERNAL STANDARD	0.038	10:27
BLANK TEST	0.000	10:27
EXTERNAL STANDARD	0.038	10:28
BLANK TEST	0.000	10:29
EXTERNAL STANDARD	0.038	10:29
BLANK TEST	0.000	10:30
EXTERNAL STANDARD	0.038	10:30
BLANK TEST	0.000	10:31

Average = 0.0380  
 Std Dev = 0.0000

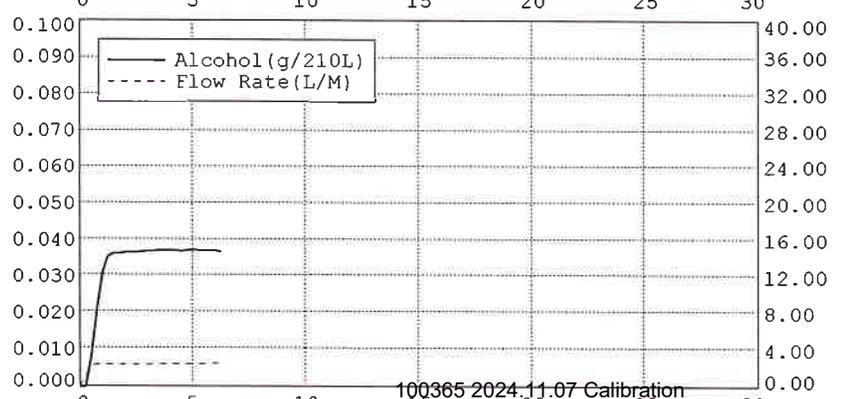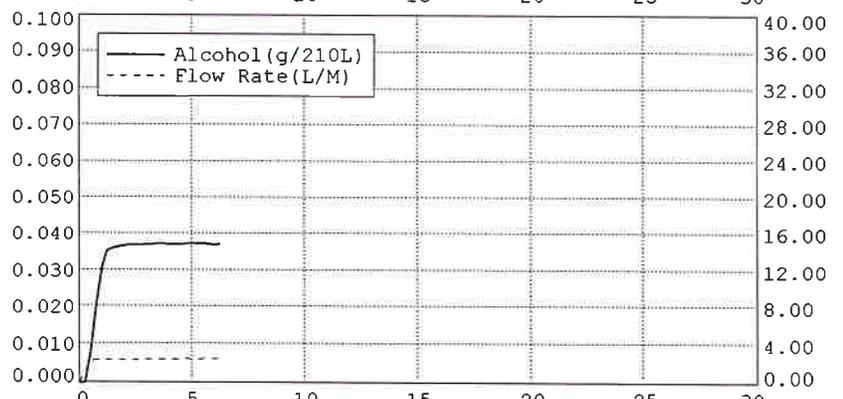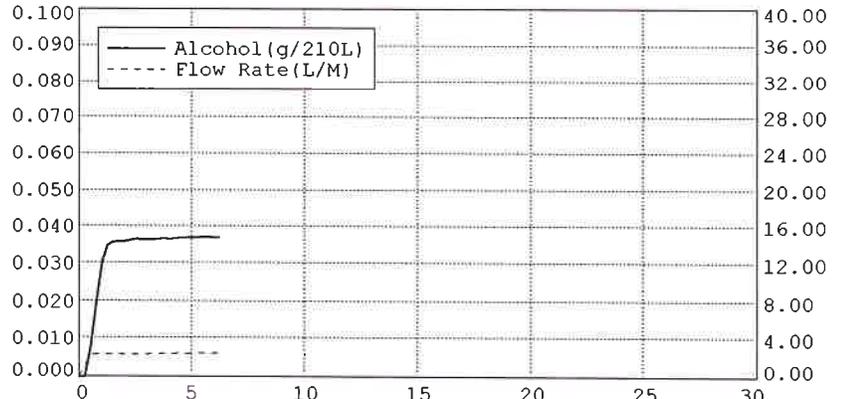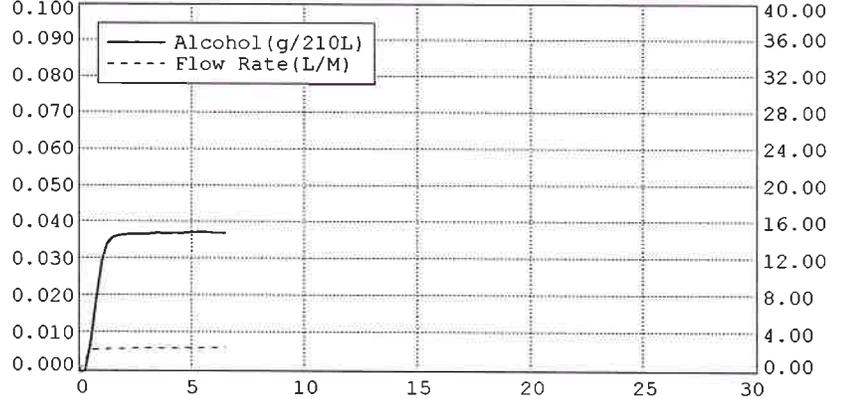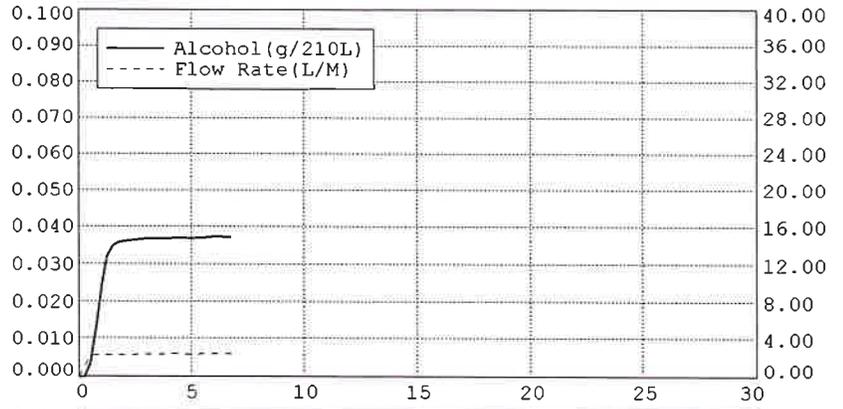

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
DATAMASTER dmt: 100365






Date: 11/07/2024  
Time: 10:32:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.86: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025  
TANK PRESSURE: 988 psi

BLANK TEST	0.000	10:34
INTERNAL STANDARD	VERIFIED	10:34
EXTERNAL STANDARD	0.075	10:34
BLANK TEST	0.000	10:35
EXTERNAL STANDARD	0.077	10:35
BLANK TEST	0.000	10:36
EXTERNAL STANDARD	0.076	10:36
BLANK TEST	0.000	10:37
EXTERNAL STANDARD	0.076	10:37
BLANK TEST	0.000	10:38
EXTERNAL STANDARD	0.076	10:38
BLANK TEST	0.000	10:39

Average = 0.0760  
Std Dev = 0.0007

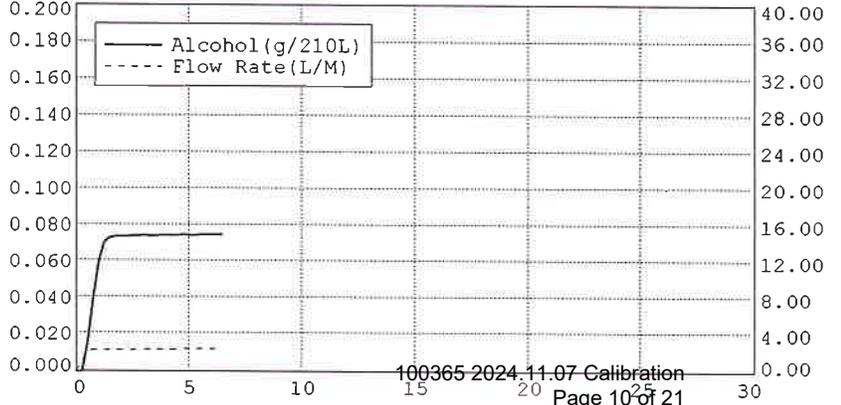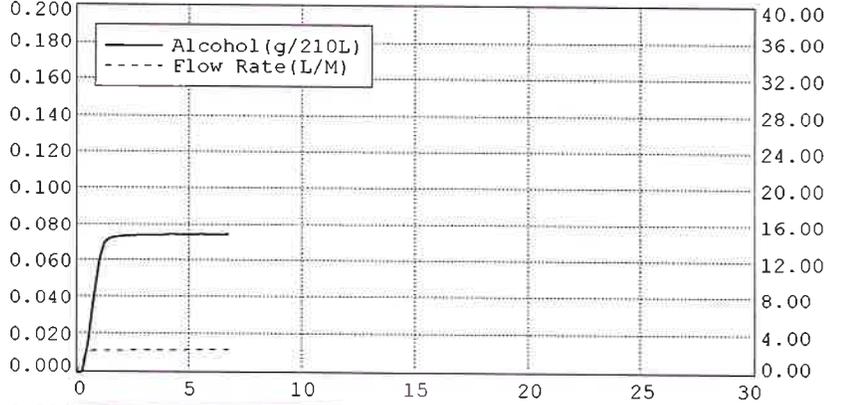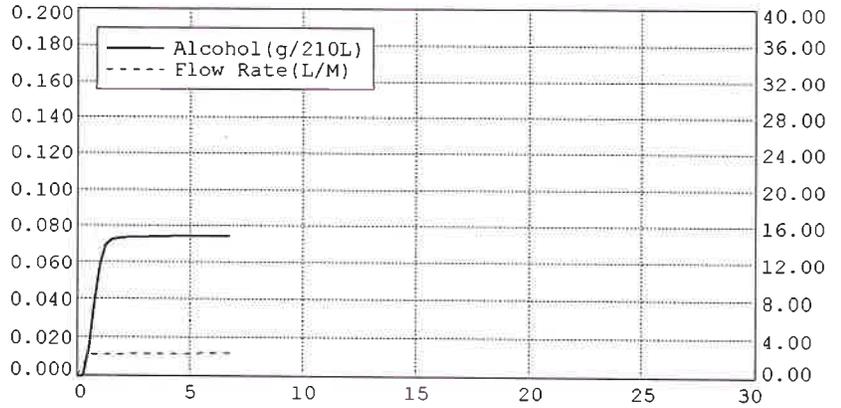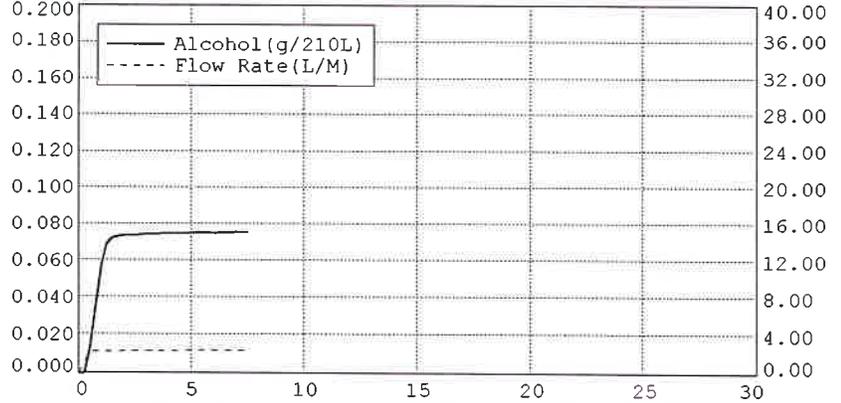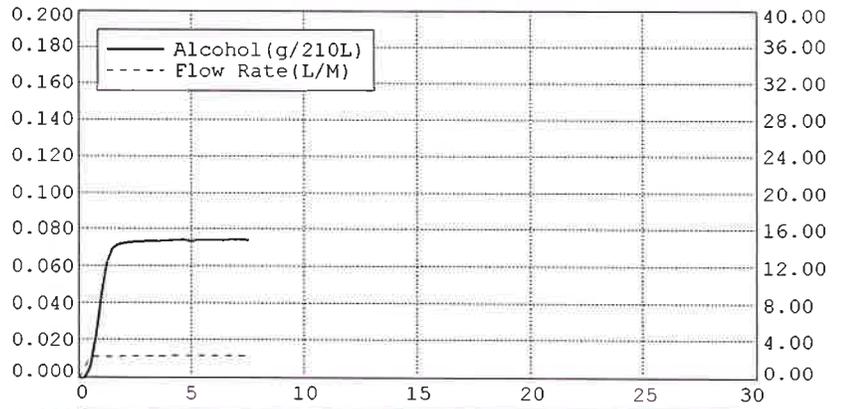

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
DATAMASTER dmt: 100365






Date: 11/07/2024  
Time: 10:40:13

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
TARGET AT 28.86: 0.096  
LOT #: AG333401  
EXPIRATION: 11/30/2025  
TANK PRESSURE: 1143 psi

BLANK TEST	0.000	10:41
INTERNAL STANDARD	VERIFIED	10:41
EXTERNAL STANDARD	0.095	10:41
BLANK TEST	0.000	10:42
EXTERNAL STANDARD	0.095	10:43
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.095	10:44
BLANK TEST	0.000	10:45
EXTERNAL STANDARD	0.095	10:45
BLANK TEST	0.000	10:46
EXTERNAL STANDARD	0.096	10:46
BLANK TEST	0.000	10:47

Average = 0.0952  
Std Dev = 0.0004

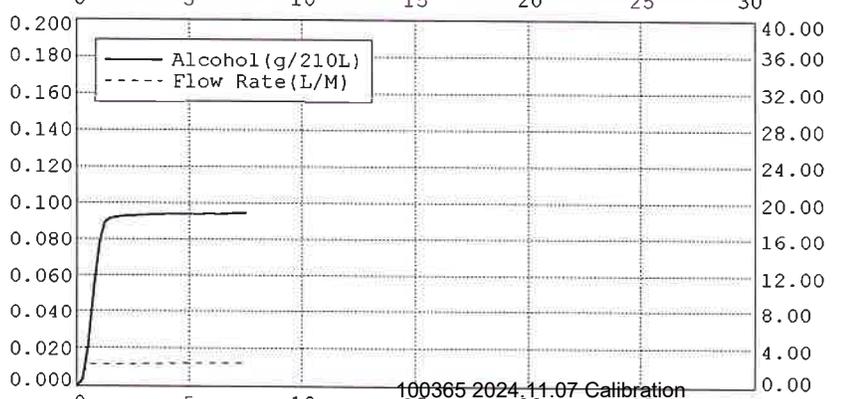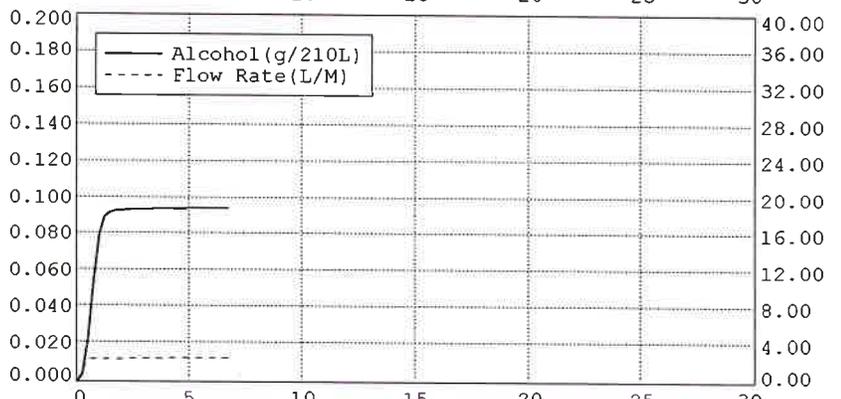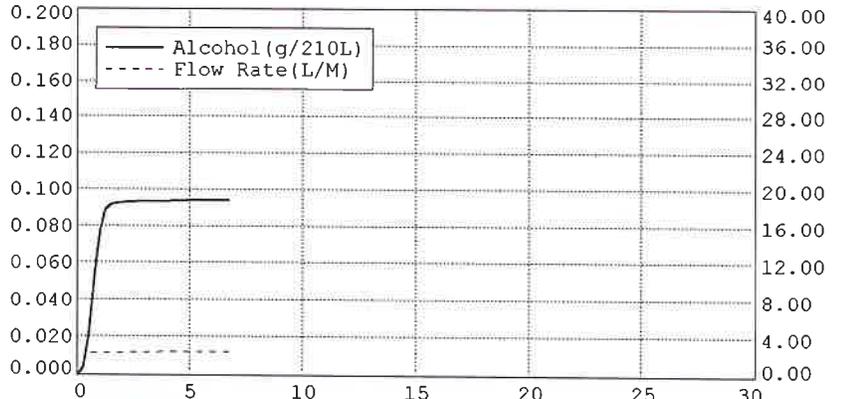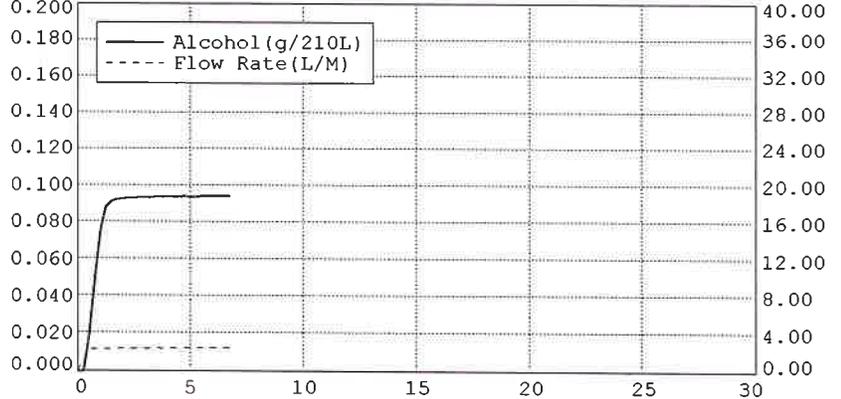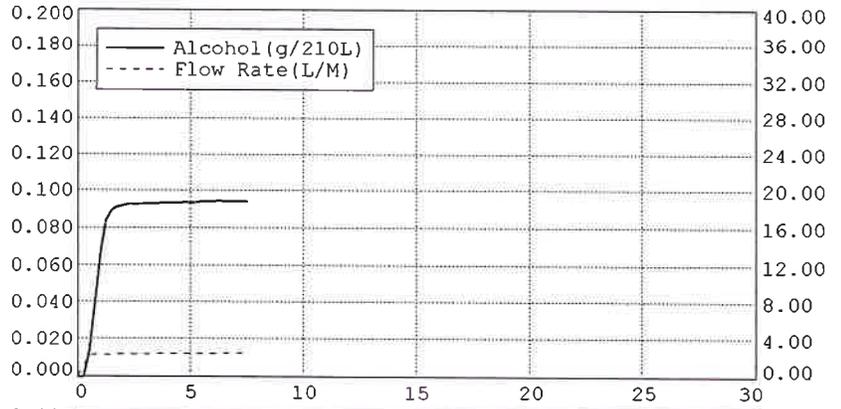

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100365






Date: 11/07/2024  
 Time: 10:47:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 28.86: 0.145  
 LOT #: AG332004  
 EXPIRATION: 11/16/2025  
 TANK PRESSURE: 608 psi

BLANK TEST	0.000	10:49
INTERNAL STANDARD	VERIFIED	10:49
EXTERNAL STANDARD	0.140	10:49
BLANK TEST	0.000	10:50
EXTERNAL STANDARD	0.140	10:50
BLANK TEST	0.000	10:51
EXTERNAL STANDARD	0.141	10:51
BLANK TEST	0.000	10:52
EXTERNAL STANDARD	0.140	10:52
BLANK TEST	0.000	10:53
EXTERNAL STANDARD	0.140	10:53
BLANK TEST	0.000	10:54

Average = 0.1402  
 Std Dev = 0.0004

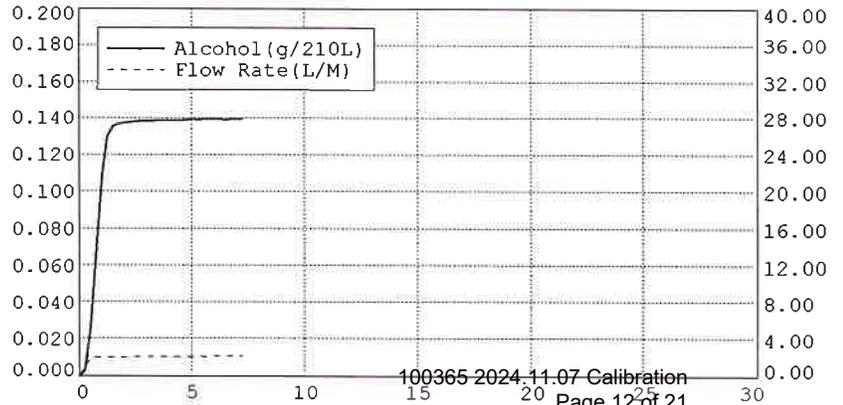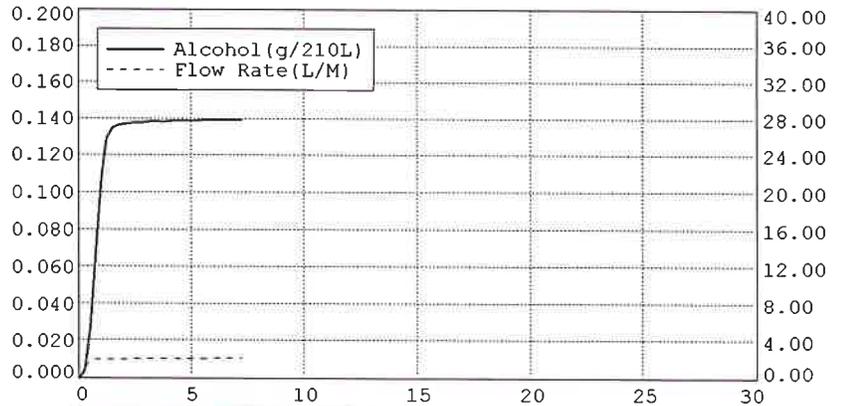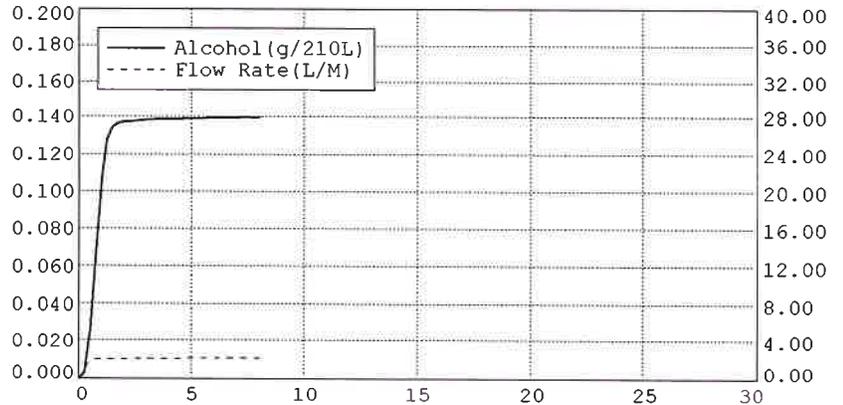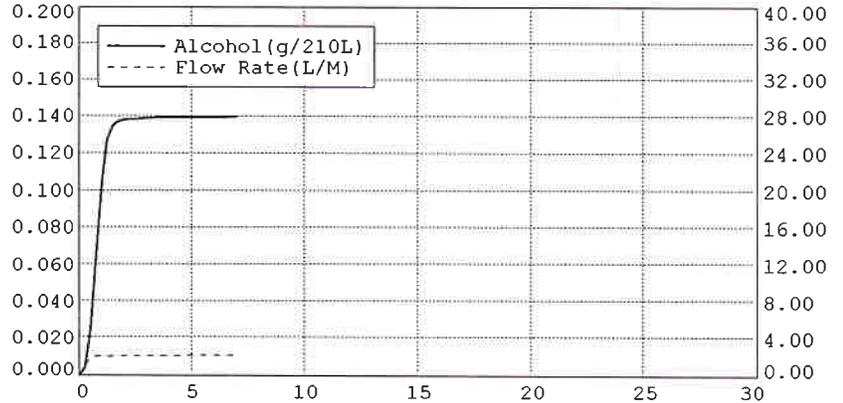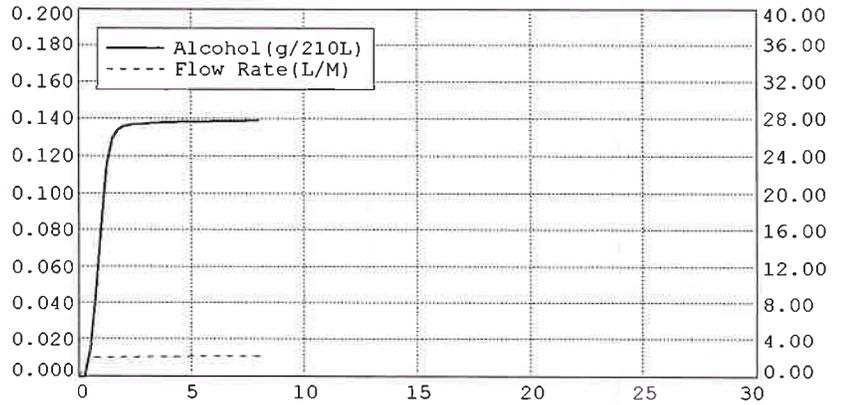

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
DATAMASTER dmt: 100365






Date: 11/07/2024  
Time: 10:56:48

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
TARGET AT 28.86: 0.289  
LOT #: AG427706  
EXPIRATION: 10/03/2026  
TANK PRESSURE: 425 psi

BLANK TEST	0.000	10:58
INTERNAL STANDARD	VERIFIED	10:58
EXTERNAL STANDARD	0.283	10:58
BLANK TEST	0.000	10:59
EXTERNAL STANDARD	0.283	10:59
BLANK TEST	0.000	11:00
EXTERNAL STANDARD	0.283	11:00
BLANK TEST	0.000	11:01
EXTERNAL STANDARD	0.282	11:02
BLANK TEST	0.000	11:02
EXTERNAL STANDARD	0.282	11:03
BLANK TEST	0.000	11:04

Average = 0.2826  
Std Dev = 0.0005

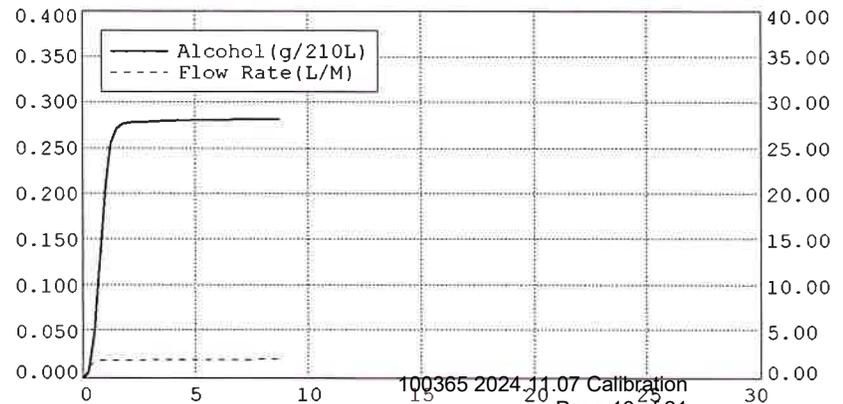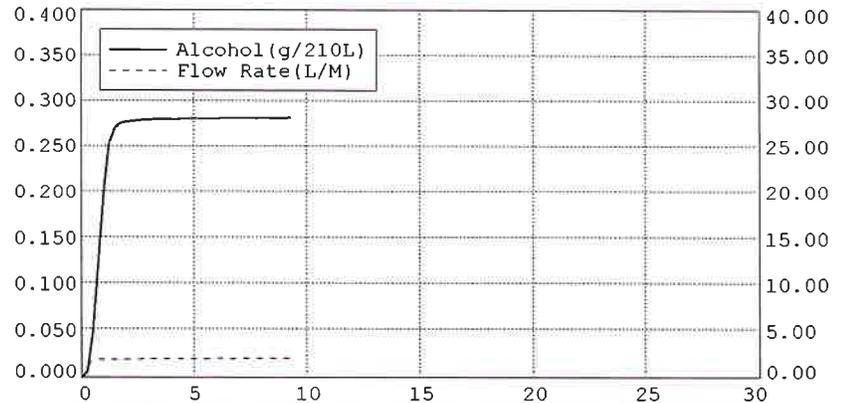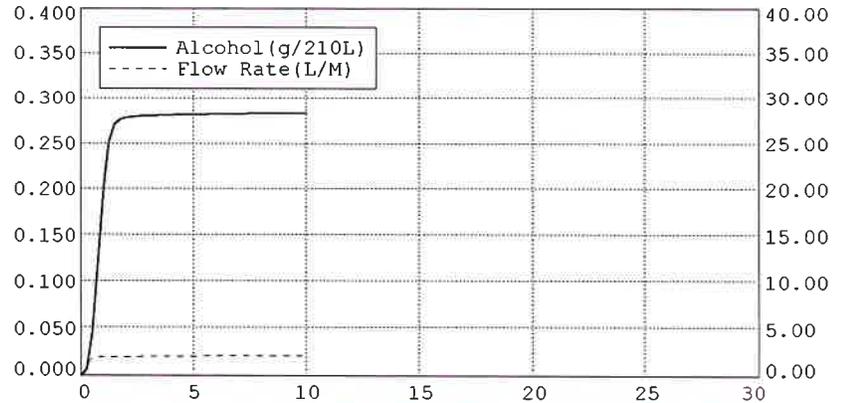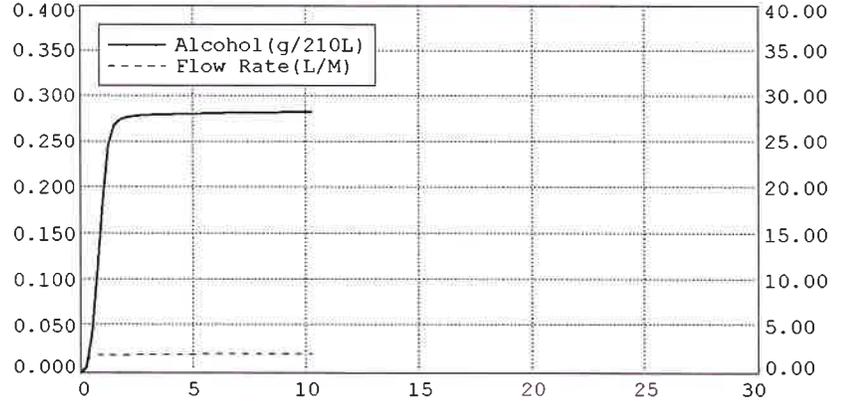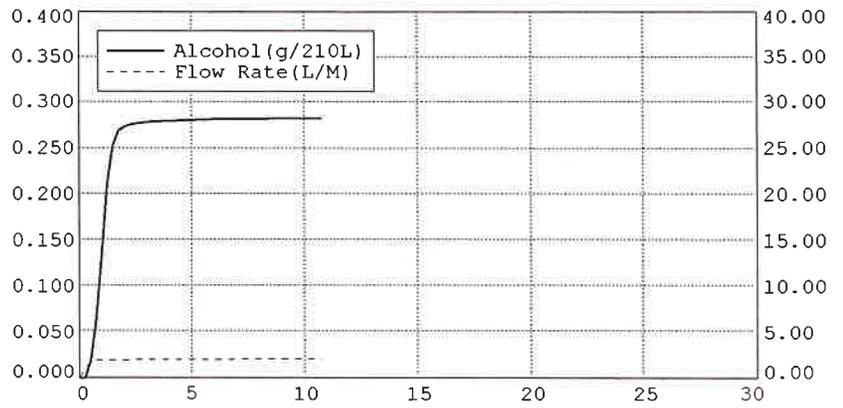

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100365

Date: 11/07/2024  
Time: 11:16:12

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 28.85: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:17  
BLANK TEST 0.000 11:17  
INTERNAL STANDARD VERIFIED 11:17  
EXTERNAL STANDARD 0.076 11:17  
BLANK TEST 0.000 11:18  
SUBJECT SAMPLE INCOMPLETE 11:22

KS

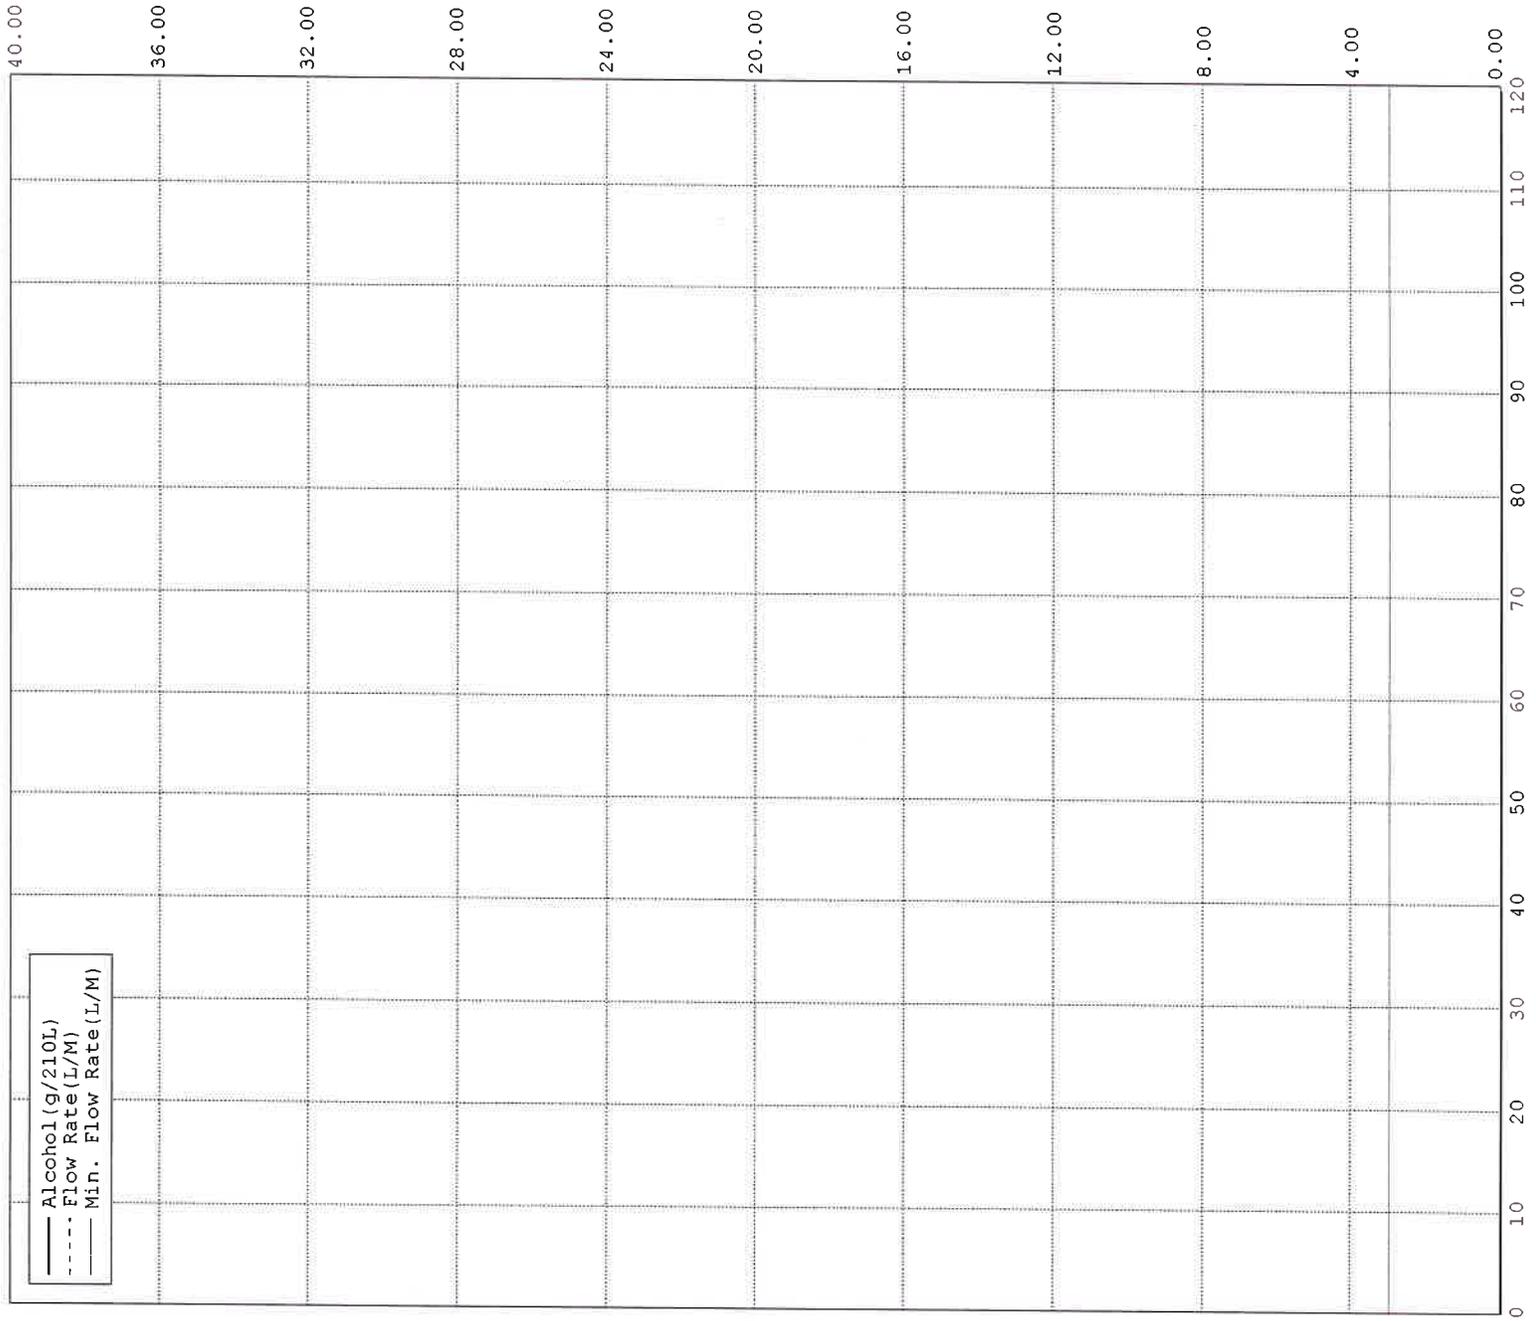

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100365

Date: 11/07/2024  
Time: 11:23:53

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746


DEPT/AGENCY:  
MAX ATTEMPTS  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 28.86: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:25  
BLANK TEST 0.000 11:25  
INTERNAL STANDARD VERIFIED 11:25  
EXTERNAL STANDARD 0.077 11:25  
BLANK TEST 0.000 11:26  
SUBJECT SAMPLE XXX 11:27

Maximum Attempts Exceeded

KS

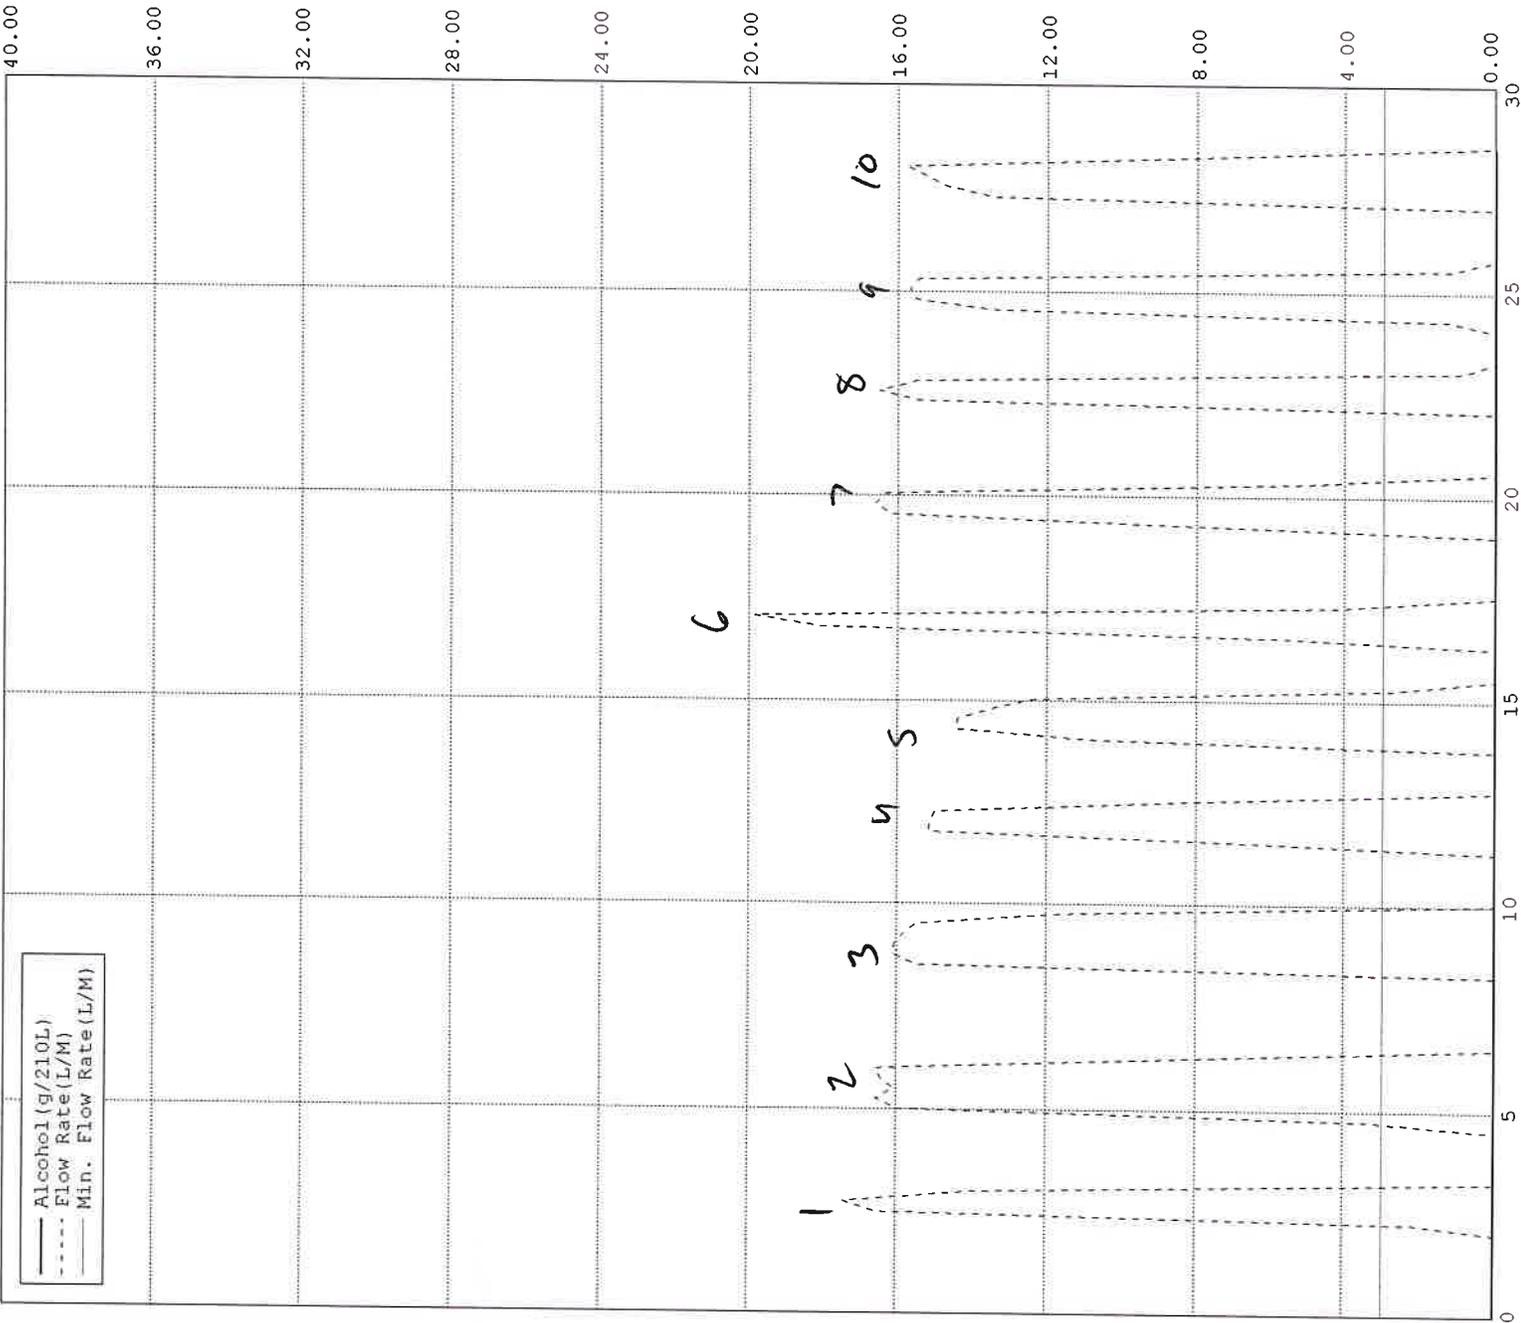

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100365

Date: 11/07/2024  
Time: 11:35:40

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
INVALID


CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.85: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:38  
BLANK TEST 0.000 11:38  
INTERNAL STANDARD VERIFIED 11:38  
EXTERNAL STANDARD 0.077 11:38  
BLANK TEST 0.000 11:39  
SUBJECT SAMPLE INVALID 11:40

KS

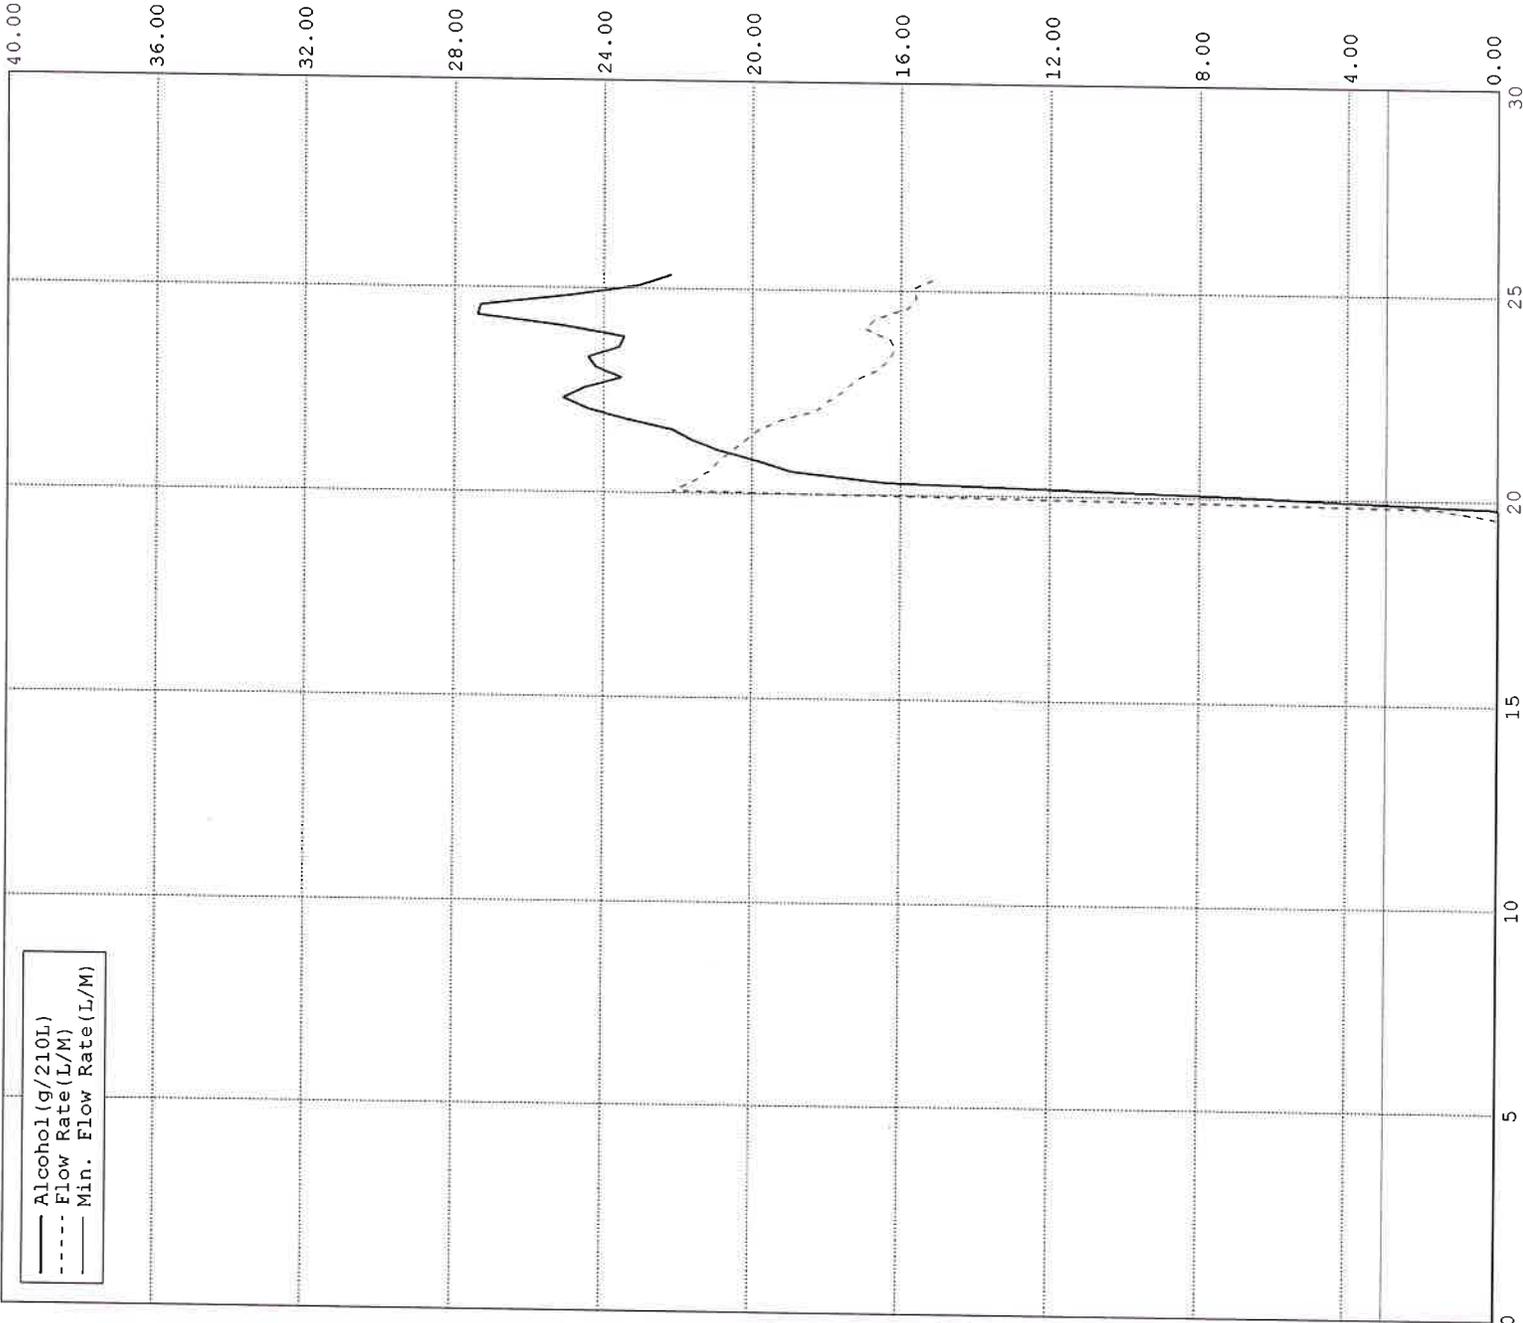

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100365

Date: 11/07/2024  
Time: 11:42:28

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
RFI  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.85: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:45  
BLANK TEST 0.000 11:45  
INTERNAL STANDARD VERIFIED 11:45  
EXTERNAL STANDARD 0.076 11:45  
BLANK TEST 0.000 11:46

RFI DETECTED

KS

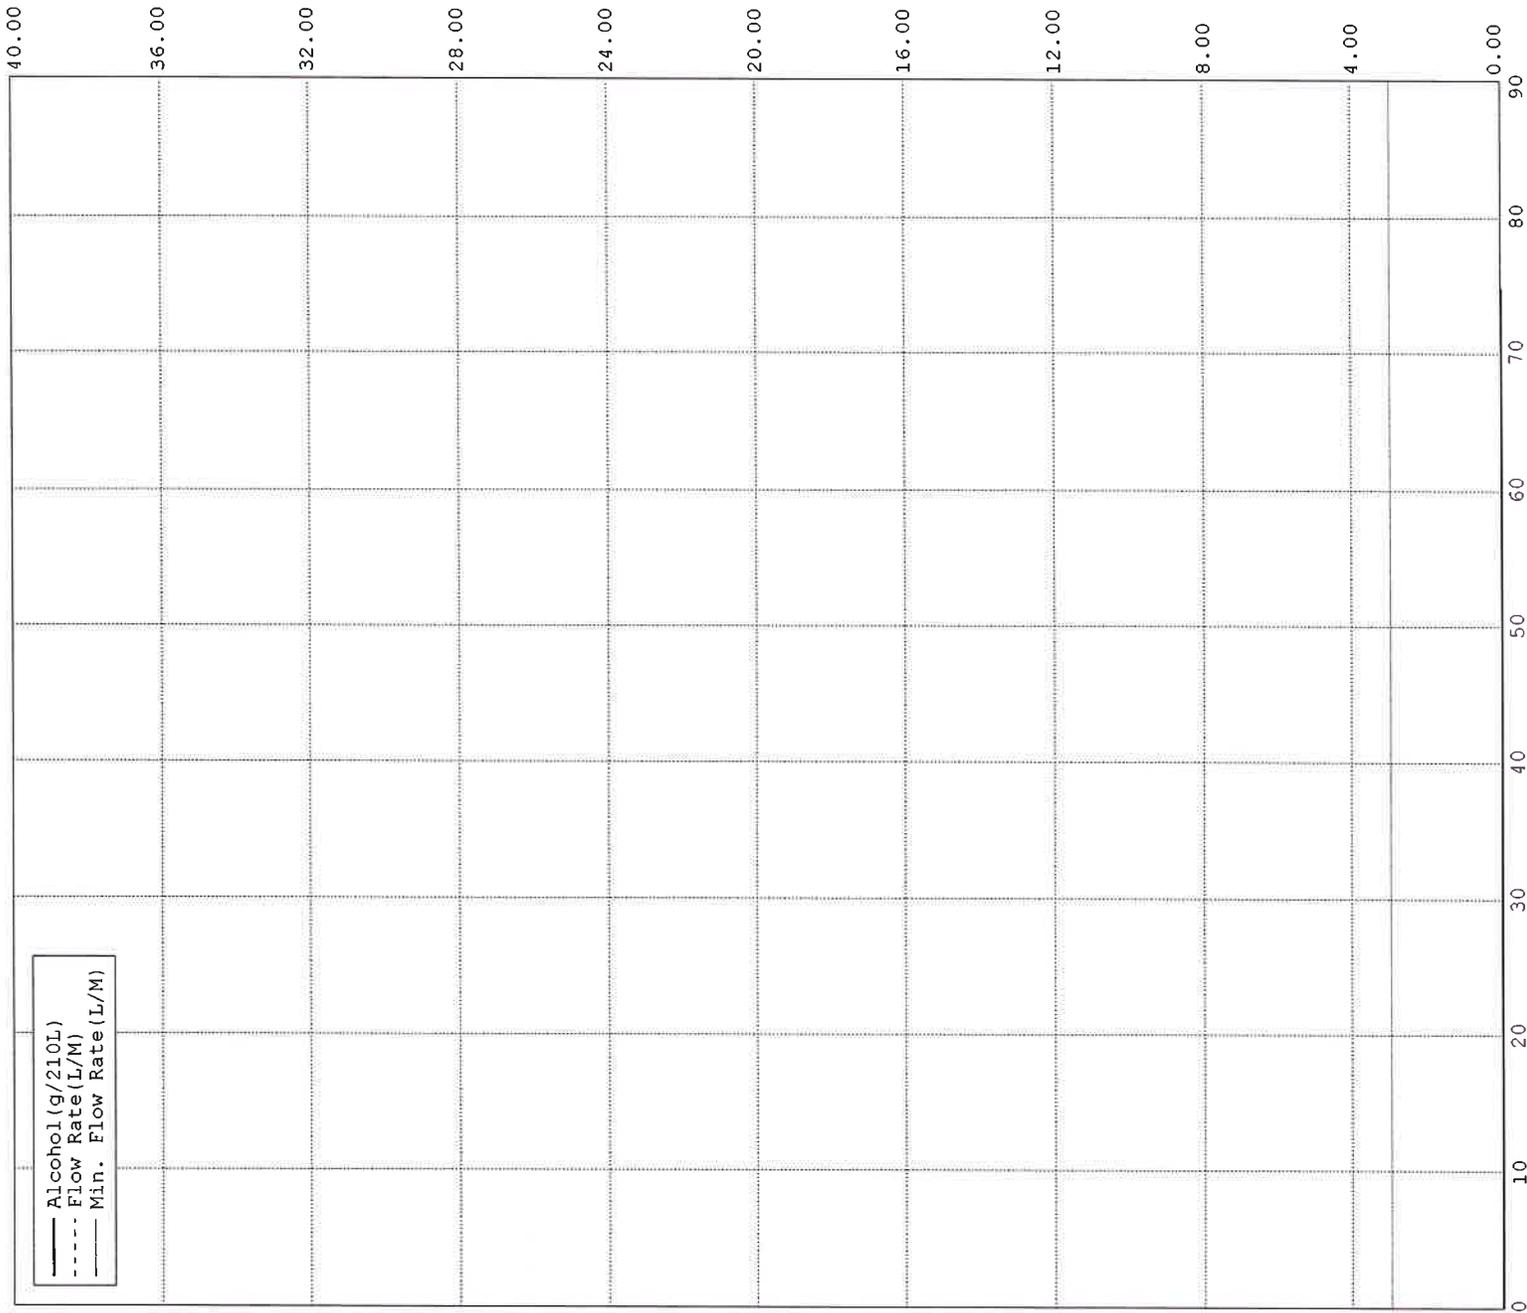

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100365

Date: 11/07/2024  
Time: 12:46:37

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAJJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
INTERFERENCE - ACETONE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.84: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 12:48  
BLANK TEST 0.000 12:48  
INTERNAL STANDARD VERIFIED 12:48  
Xg = 0.095 (1.78%)  
EXTERNAL STANDARD 0.076 12:48  
X[1] = 0.0762 (-0.0004) (0.0020)  
BLANK TEST 0.000 12:49  
SUBJECT SAMPLE XXX 12:50  
X[1] = 0.1102 (-0.0194) (0.0004)

Interference Detected

Filter 2 average is -0.0006  
Filter 3 average is 0.0021  
KS 11/7/24

KS



SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100365

Date: 11/07/2024  
Time: 12:41:32

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KALJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
INTERFERENCE - IPA  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.84: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:42
BLANK TEST	0.000	12:42
INTERNAL STANDARD	VERIFIED	12:42
$X_q = 0.094$ (0.84%)		
EXTERNAL STANDARD	0.076	12:43
$X[1] = 0.0760$ (-0.0004) (0.0029)		
BLANK TEST	0.000	12:43
SUBJECT SAMPLE	XXX	12:44
$X[1] = 0.1187$ (-0.0243) (0.0005)		

Interference Detected

KS

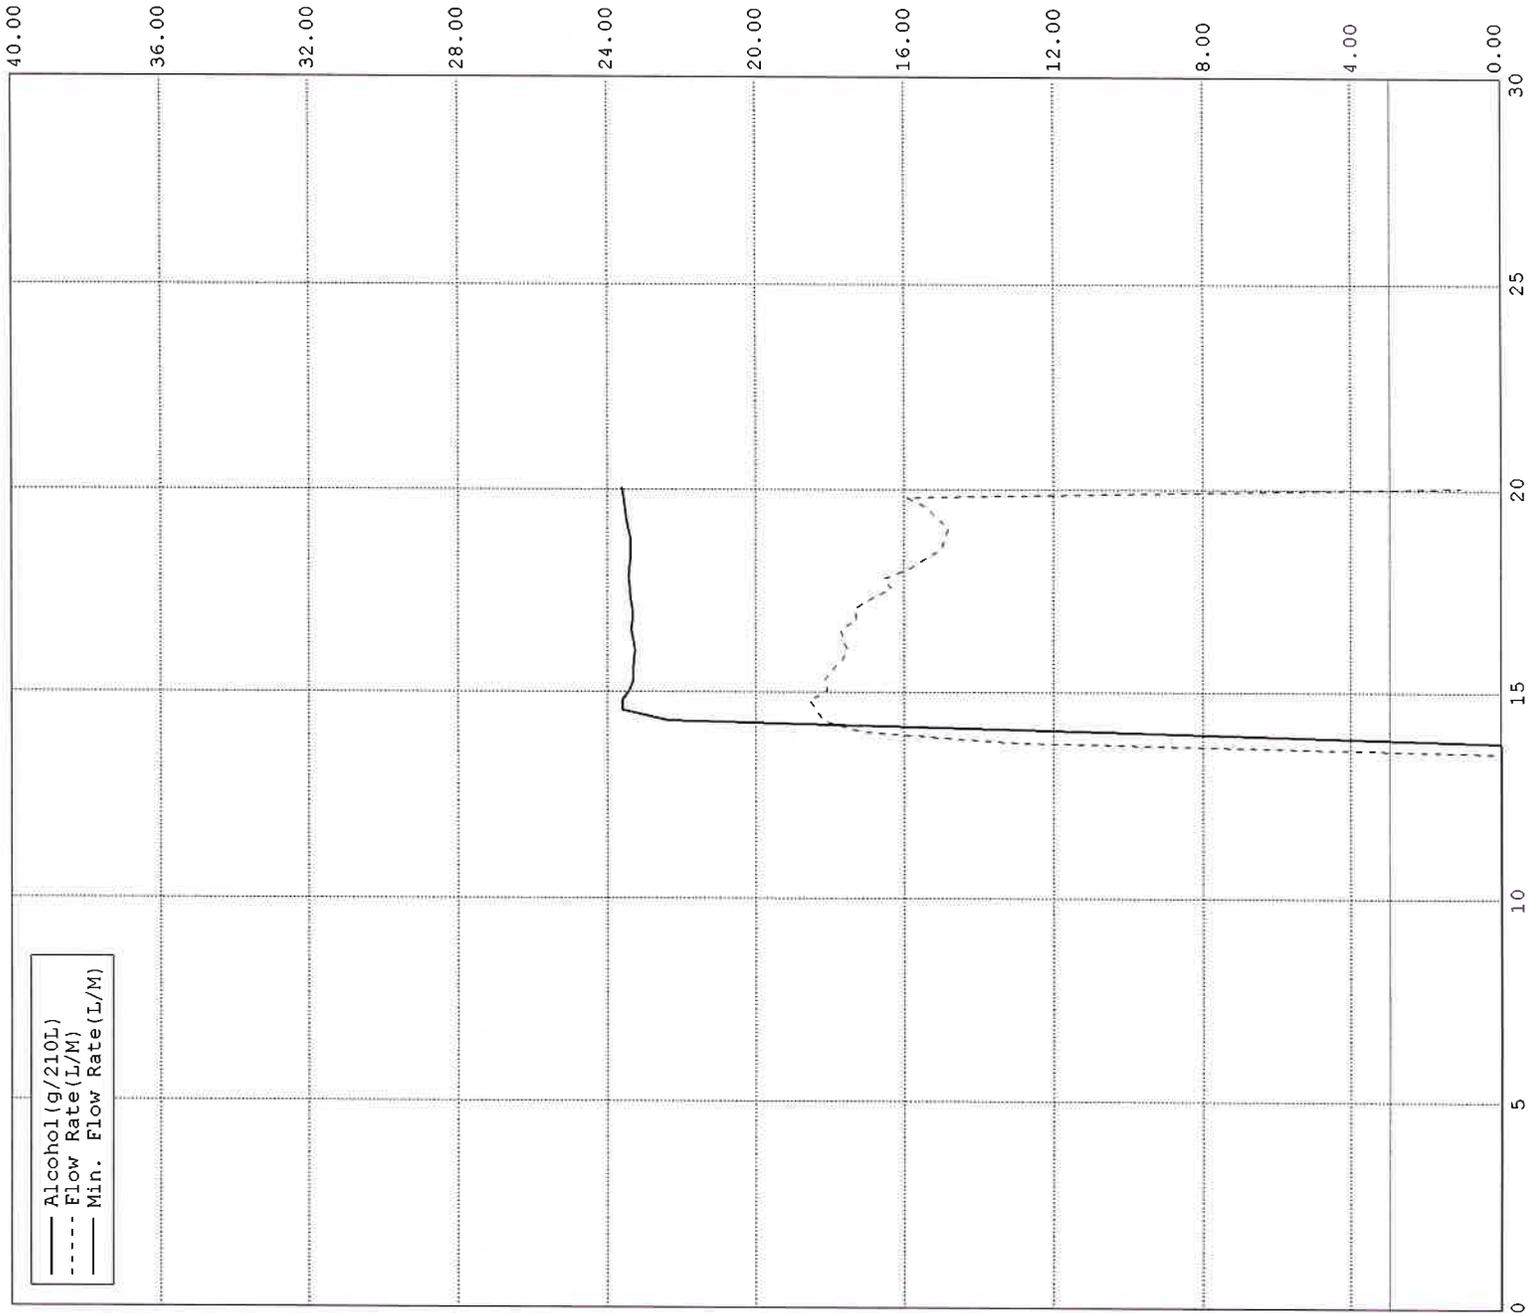

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100365

Date: 11/07/2024  
Time: 12:52:02

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
INTERFERENCE - NEGATIVE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL:	0.080		
TARGET AT	28.84:	0.077	
LOT #:	AG335202		
EXPIRATION:	12/18/2025		
DIAGNOSTIC CHECK	PASSED	12:55	
BLANK TEST	0.000	12:55	
INTERNAL STANDARD	VERIFIED	12:55	
Xg = 0.094 (0.66%)			
EXTERNAL STANDARD	0.076	12:56	
X[1] = 0.0758 (-0.0009)	(0.0021)		
BLANK TEST	0.000	12:57	
SUBJECT SAMPLE (Vol=1.75L)	0.094	12:57	
X[1] = 0.0941 (0.0007)	(0.0006)		
BLANK TEST	0.000	12:58	
EXTERNAL STANDARD	0.075	12:59	
X[1] = 0.0755 (-0.0006)	(0.0014)		
BLANK TEST	0.000	12:59	

KS

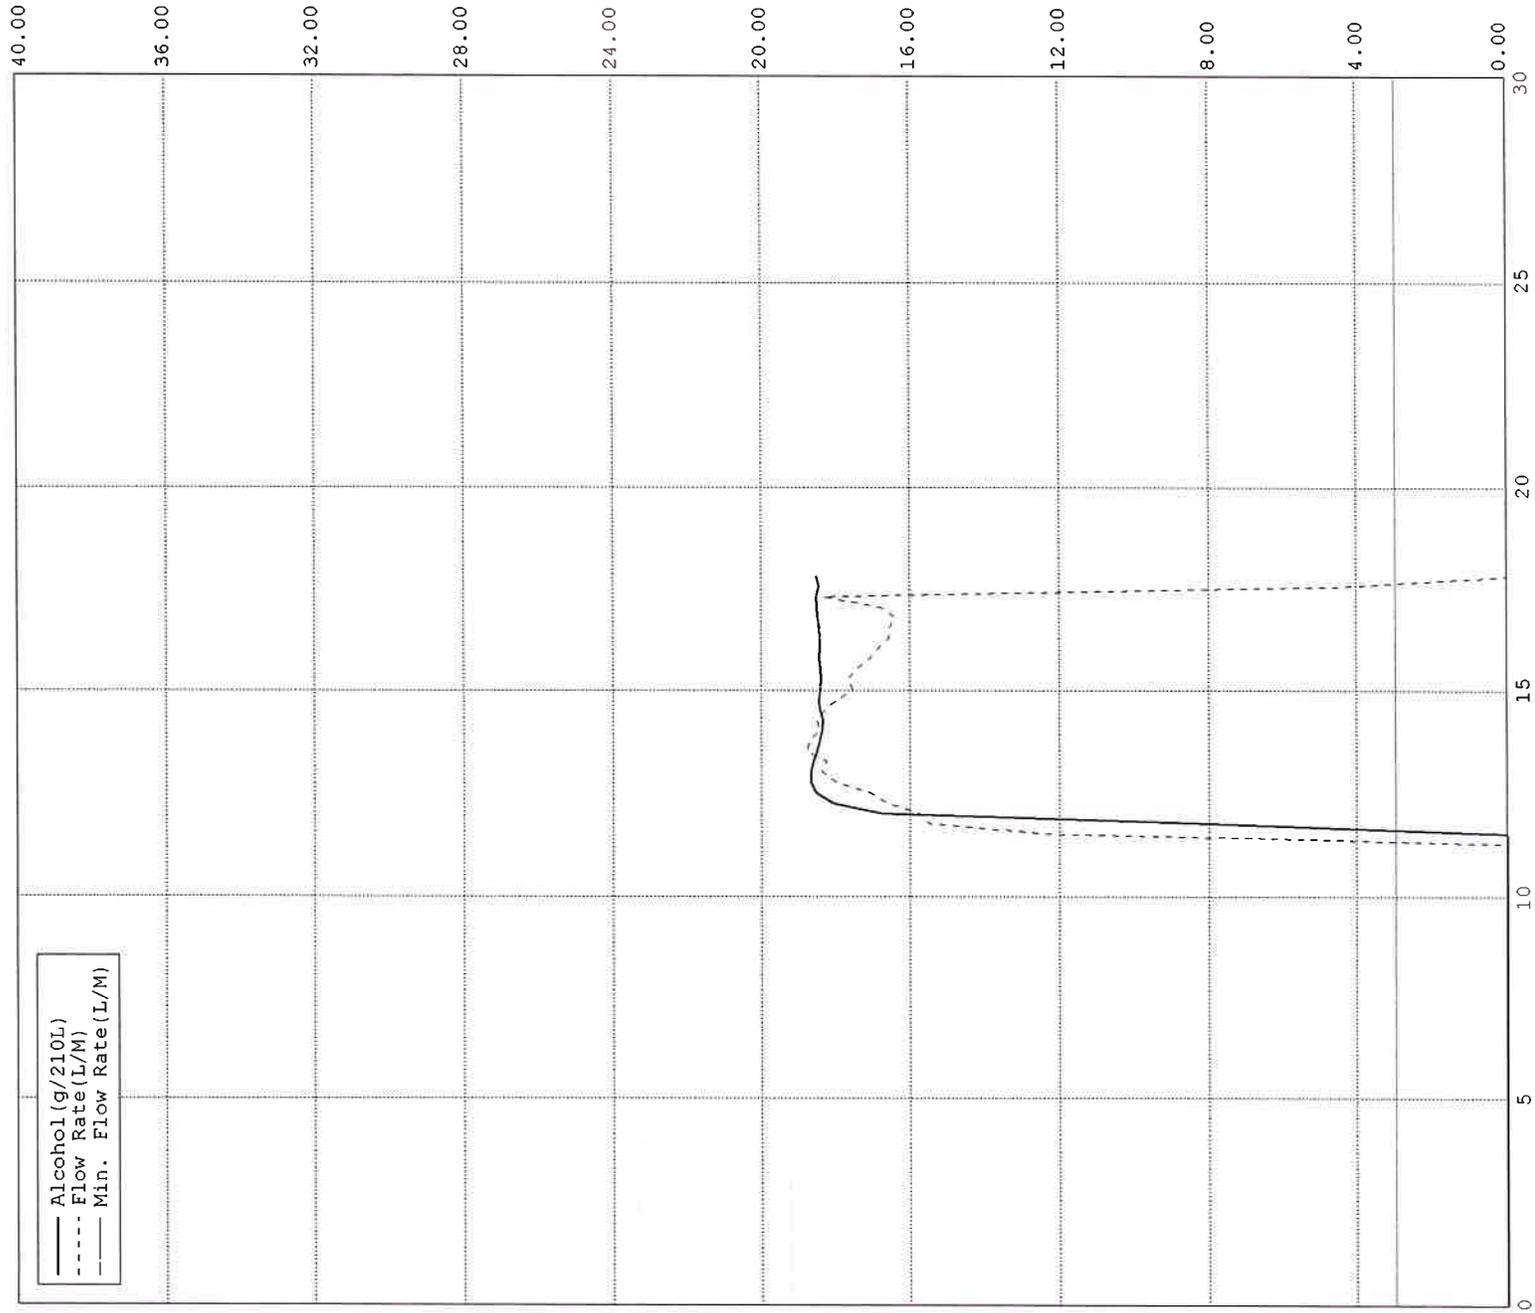

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100365

Date: 11/07/2024

Time: 13:56:06

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

NON-DRINKING SUBJECT TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 28.83: 0.077

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:57
BLANK TEST	0.000	13:57
INTERNAL STANDARD	VERIFIED	13:57
EXTERNAL STANDARD	0.075	13:57
BLANK TEST	0.000	13:58
SUBJECT SAMPLE (Vol=2.20L)	0.000	13:59
BLANK TEST	0.000	13:59
EXTERNAL STANDARD	0.076	14:00
BLANK TEST	0.000	14:01

XS

