

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100697

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 07/28/2018

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.03: 0.080
LOT #: AG634001
EXPIRATION: 12/05/2018
TANK PRESSURE: 851 psi

BLANK TEST	0.000	12:21
INTERNAL STANDARD	VERIFIED	12:21
EXTERNAL STANDARD	0.076	12:21
BLANK TEST	0.000	12:22
EXTERNAL STANDARD	0.076	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.076	12:24
BLANK TEST	0.000	12:24
EXTERNAL STANDARD	0.076	12:25
BLANK TEST	0.000	12:26
EXTERNAL STANDARD	0.077	12:26
BLANK TEST	0.000	12:27

Average = 0.0762
Std Dev = 0.0004

Diagnostic Check

VERSIONS

DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
Breath Tube = 48.1°C PASSED

PUMP INFO

Flow Rate = 4.433 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO


Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

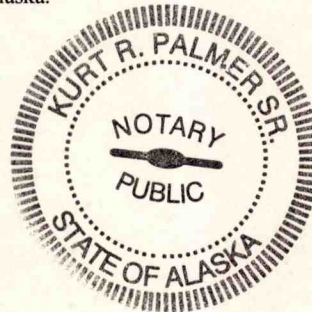
PASSED

I, Charles R. Foster, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Charles R. Foster
Scientific Director
State Breath Alcohol Program

11/21/18



Subscribed and sworn before me this 21 day of NOV 20 18


Kurt R. Palmer Sr., Notary Public
My Commission Expires With Office

BMB
11/16/18