

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100412

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 04/28/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.25: 0.078
LOT #: 11313080A1
EXPIRATION: 06/01/2015
TANK PRESSURE: 449 psi

| | | |
|-------------------|----------|-------|
| BLANK TEST | 0.000 | 08:45 |
| INTERNAL STANDARD | VERIFIED | 08:45 |
| EXTERNAL STANDARD | 0.080 | 08:45 |
| BLANK TEST | 0.000 | 08:46 |
| EXTERNAL STANDARD | 0.080 | 08:46 |
| BLANK TEST | 0.000 | 08:47 |
| EXTERNAL STANDARD | 0.080 | 08:47 |
| BLANK TEST | 0.000 | 08:48 |
| EXTERNAL STANDARD | 0.080 | 08:48 |
| BLANK TEST | 0.000 | 08:49 |
| EXTERNAL STANDARD | 0.080 | 08:49 |
| BLANK TEST | 0.000 | 08:50 |

Average = 0.0800
Std Dev = 0.0000

Diagnostic Check

VERSIONS

DMT: 3.00
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
Breath Tube = 47.3°C PASSED

PUMP INFO

Flow Rate = 4.806 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO


Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


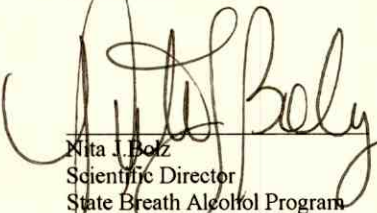

Nita J. Bolz
Scientific Director
State Breath Alcohol Program

5/15/2015

Subscribed and sworn before me this 15th day of May, 2015



Nikki Roth, Notary Public
My Commission Expires With Office

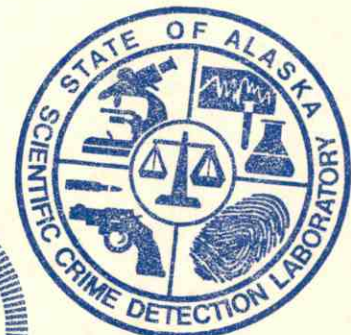

DMB
4/29/15