

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100423

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 09/19/2013

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.83: 0.077
LOT #: 11313080A1
EXPIRATION: 06/01/2015

BLANK TEST	0.000	16:31
INTERNAL STANDARD	VERIFIED	16:31
EXTERNAL STANDARD	0.079	16:31
BLANK TEST	0.000	16:32
EXTERNAL STANDARD	0.079	16:32
BLANK TEST	0.000	16:33
EXTERNAL STANDARD	0.079	16:34
BLANK TEST	0.000	16:34
EXTERNAL STANDARD	0.079	16:35
BLANK TEST	0.000	16:36
EXTERNAL STANDARD	0.079	16:36
BLANK TEST	0.000	16:37

Average = 0.0790
Std Dev = 0.0000

Diagnostic Check

VERSIONS

DMT: 2.00
PIC: 3.03
Modem: 2.3
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
Breath Tube = 48.1°C PASSED

PUMP INFO

Flow Rate = 4.427 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO

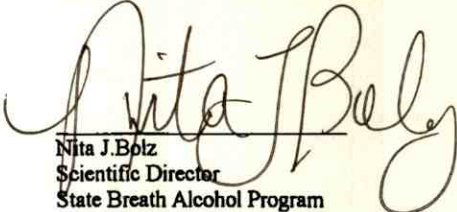
Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

9/23/2013

Subscribed and sworn before me this 23 day of Sept, 2013


Nikki Roth, Notary Public
My Commission Expires With Office



COB 9/20/13