




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100365

Report Issue Date: 10/02/2025
Date Received: 2025-06-26
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.021	0.022	0.022	0.022	0.021	0.022
0.080	0.079	AG335202	0.082	0.082	0.081	0.080	0.079	0.081
0.300	0.296	AG427706	0.290	0.289	0.290	0.290	0.289	0.290

As Found - Evaluation Analyst: Derek Walton

As Found Conditions - Barometric Pressure (inHg): 29.54 Barometer Used: VWR S/N 240680771 Temperature (C): 22.5 Relative Humidity (%): 32

As-Found Lab Activity Date Range: 06/26/2025 - 06/26/2025

Recommend Repair to resolve unable to poll via modem.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG408002	0.020	0.020	0.019	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.038	0.039	0.039	0.038	0.038	0.038	+/- 0.003
0.080	0.078	AG335202	0.076	0.076	0.076	0.076	0.077	0.076	+/- 0.004
0.100	0.097	AG333401	0.096	0.096	0.096	0.096	0.096	0.096	+/- 0.004
0.150	0.146	AG332004	0.142	0.142	0.142	0.141	0.141	0.142	+/- 0.006
0.300	0.292	AG427706	0.286	0.285	0.285	0.285	0.286	0.285	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.14 Barometer Used: VWR S/N 240680771 Temperature (C): 22.3 Relative Humidity (%): 40

As-Left Lab Activity Date Range: 09/22/2025 - 09/23/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Kaija Swisher on 10/01/2025

kaija.swisher@alaska.gov

Technically and administratively reviewed by Derek Walton on 10/02/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100365 Analyst or Technician Name: Kaya Swisher

DataMaster DMT Calibration Start Date: 9/22/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 290680771
Calibration Due Date: 9/10/26
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5L liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.14 Temperature(C) 22.3 Relative Humidity(%) 40

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)
- ☒ Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20250922K5 Expiration Date: 12/22/25
Simulator S/N: DR4178 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20250922K5 Expiration Date: 12/22/25
Simulator S/N: DR4177 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 12/22/25 / 3/19/27
Simulator S/N: DR4163 Thermometer Verification Performed? ☒ (Solutions)

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 3/14/27

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 9/22/25

Data Interpretation Date (Technician): N/A (if applicable)

Data Interpretation Date (Analyst): 9/23/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100365

Date: 09/22/2025
Time: 09:29:27

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.6°C (44.0°C - 52.0°C)	PASSED
Breath Tube = 44.5°C (38.0°C - 50.0°C)	PASSED

SETTINGS

Lamp Voltage = 2.02 V (1.21 V - 2.83 V)	PASSED
Cooler Voltage = 1.82 V (1.09 V - 2.55 V)	PASSED
Bias Voltage = 80 V (47 V - 111 V)	PASSED
Chopper Freq = 522 Hz (475 Hz - 575 Hz)	PASSED
Barometer = 29.1 in	

PUMP INFO

Flow Rate = 4.574 L/M (3.500 L/M - 6.500 L/M)	PASSED
--	--------

DETECTOR INFO

PUMP ON (0.003 V <= 0.010 V)	PASSED
PUMP OFF (0.001 V <= 0.010 V)	PASSED

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
Xq = 0.094 0.47% (0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100365

Date: 09/22/2025

Time: 10:28 AM

Temperatures (°C)

Sample Cell: 48.6°C

Breath Tube: 45.2°C

Current Barometer 29.1 in

Volume (Ltr) 1.60

Settings

Lamp: 2.02 V

Bias: 80 V

Cooler: 1.90 V

Chopper: 528 Hz

Voltages (V)

Flow: 1.04 V

Detector: -0.021 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100365

Date: 11/06/2024
Time: 13:50:21

OPERATOR NAME:
KAIJA SWISHER
CERTIFICATE #: 10746

Ca	=	0.1000		
CAL	=	0.983493	0.800	<= CAL < 1.200
b1	=	0.0004	0.0000	<= b1 < 0.0040
b2	=	0.0056	0.0010	<= b2 < 0.0100
b3	=	0.0002	0.0000	<= b3 < 0.0040
Xq	=	0.0931	0.0500	<= Xq < 0.2000
a21	=	1.171826	1.050	<= a21 < 1.300
a31	=	0.450343	0.300	<= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100365

Date: 09/22/2025
Time: 10:54:32

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.14: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:55
BLANK TEST	0.000	10:55
INTERNAL STANDARD	VERIFIED	10:55
EXTERNAL STANDARD	0.076	10:56
BLANK TEST	0.000	10:57
SUBJECT SAMPLE (Vol=1.55L)	0.000	10:57
BLANK TEST	0.000	10:58
EXTERNAL STANDARD	0.076	10:59
BLANK TEST	0.000	11:00

Alcohol(g/210L)
Flow Rate(L/M)
Min. Flow Rate(L/M)

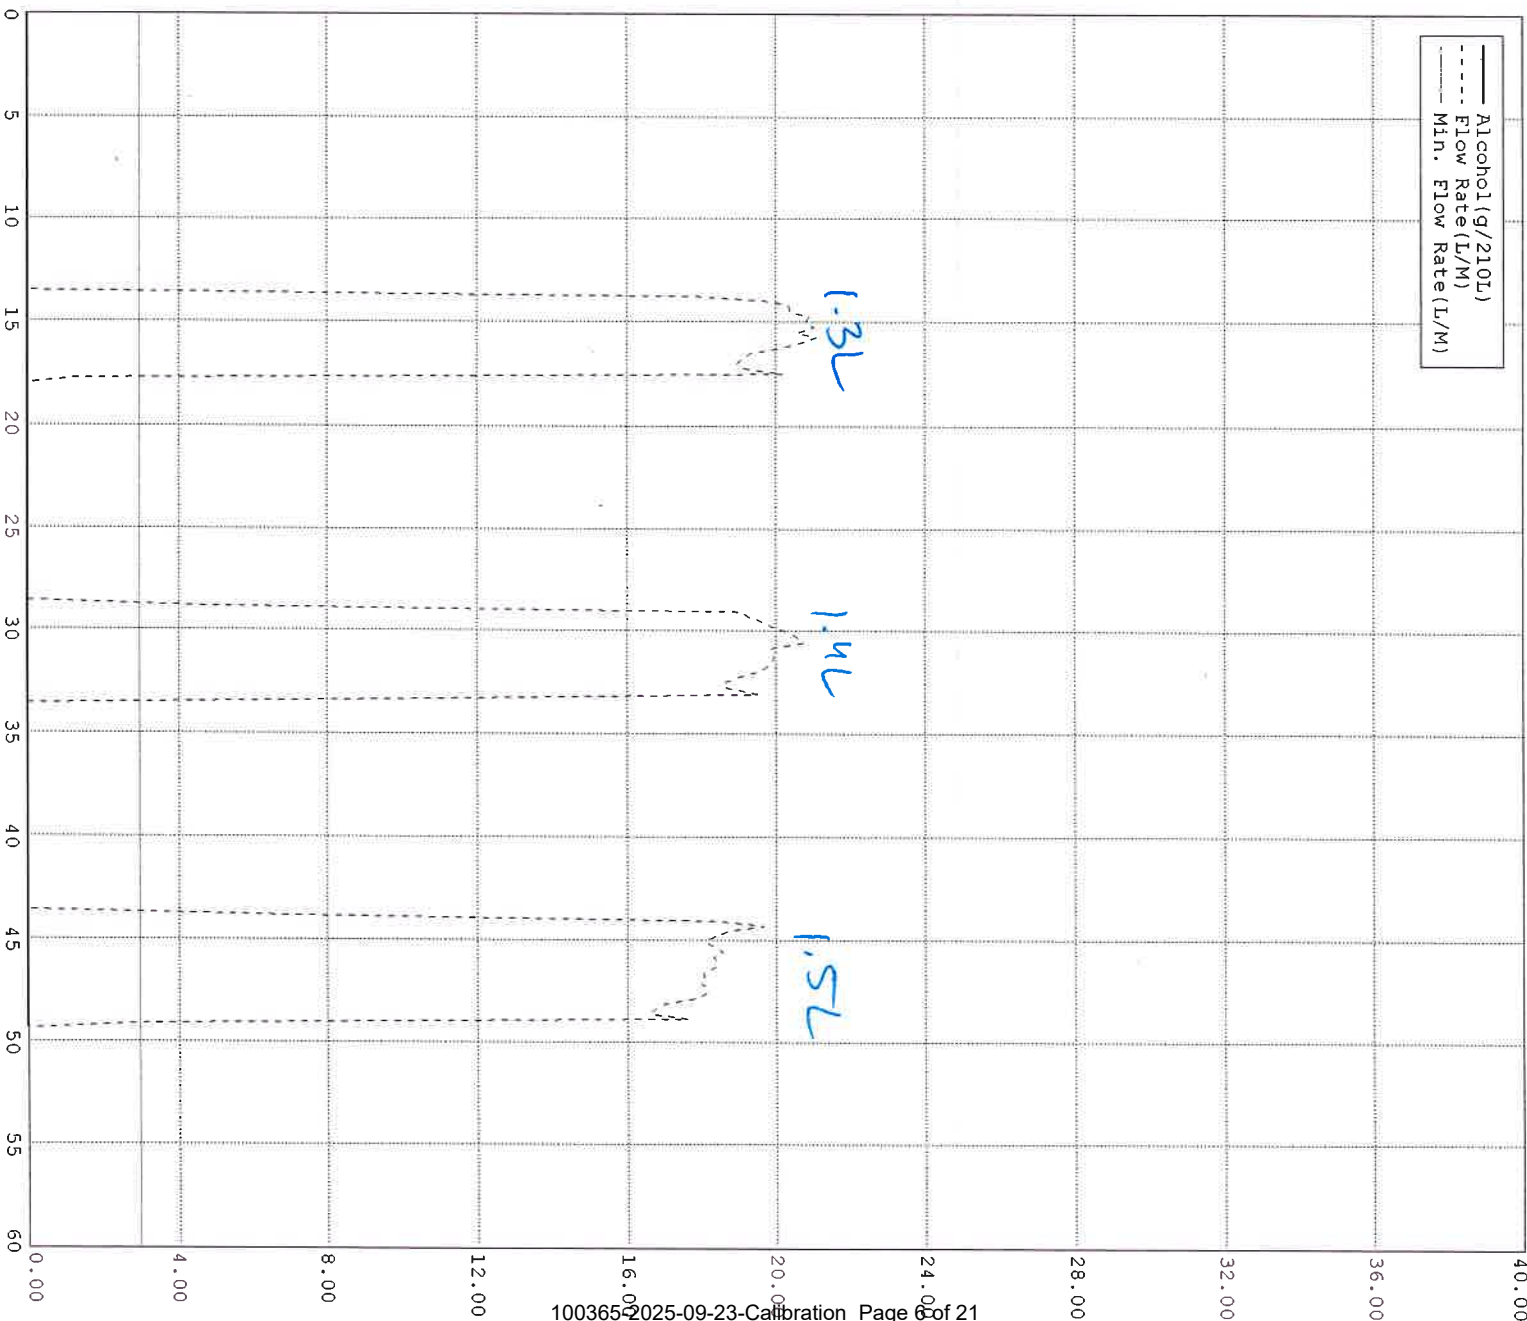

KS


LINEARITY CHECK

Alaska Department of Public Safety
 DATAMASTER dmt: 100365

Date: 09/22/2025
 Time: 11:08:25

SUPERVISOR NAME:
 KAITA SWISHER
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.019	0.0198	0.0004
0.039	0.0384	0.0005
0.078	0.0762	0.0004
0.097	0.0960	0.0000
0.146	0.1416	0.0005
0.292	0.2854	0.0005
SLOPE	= 0.973540	
R ²	= 0.999933	

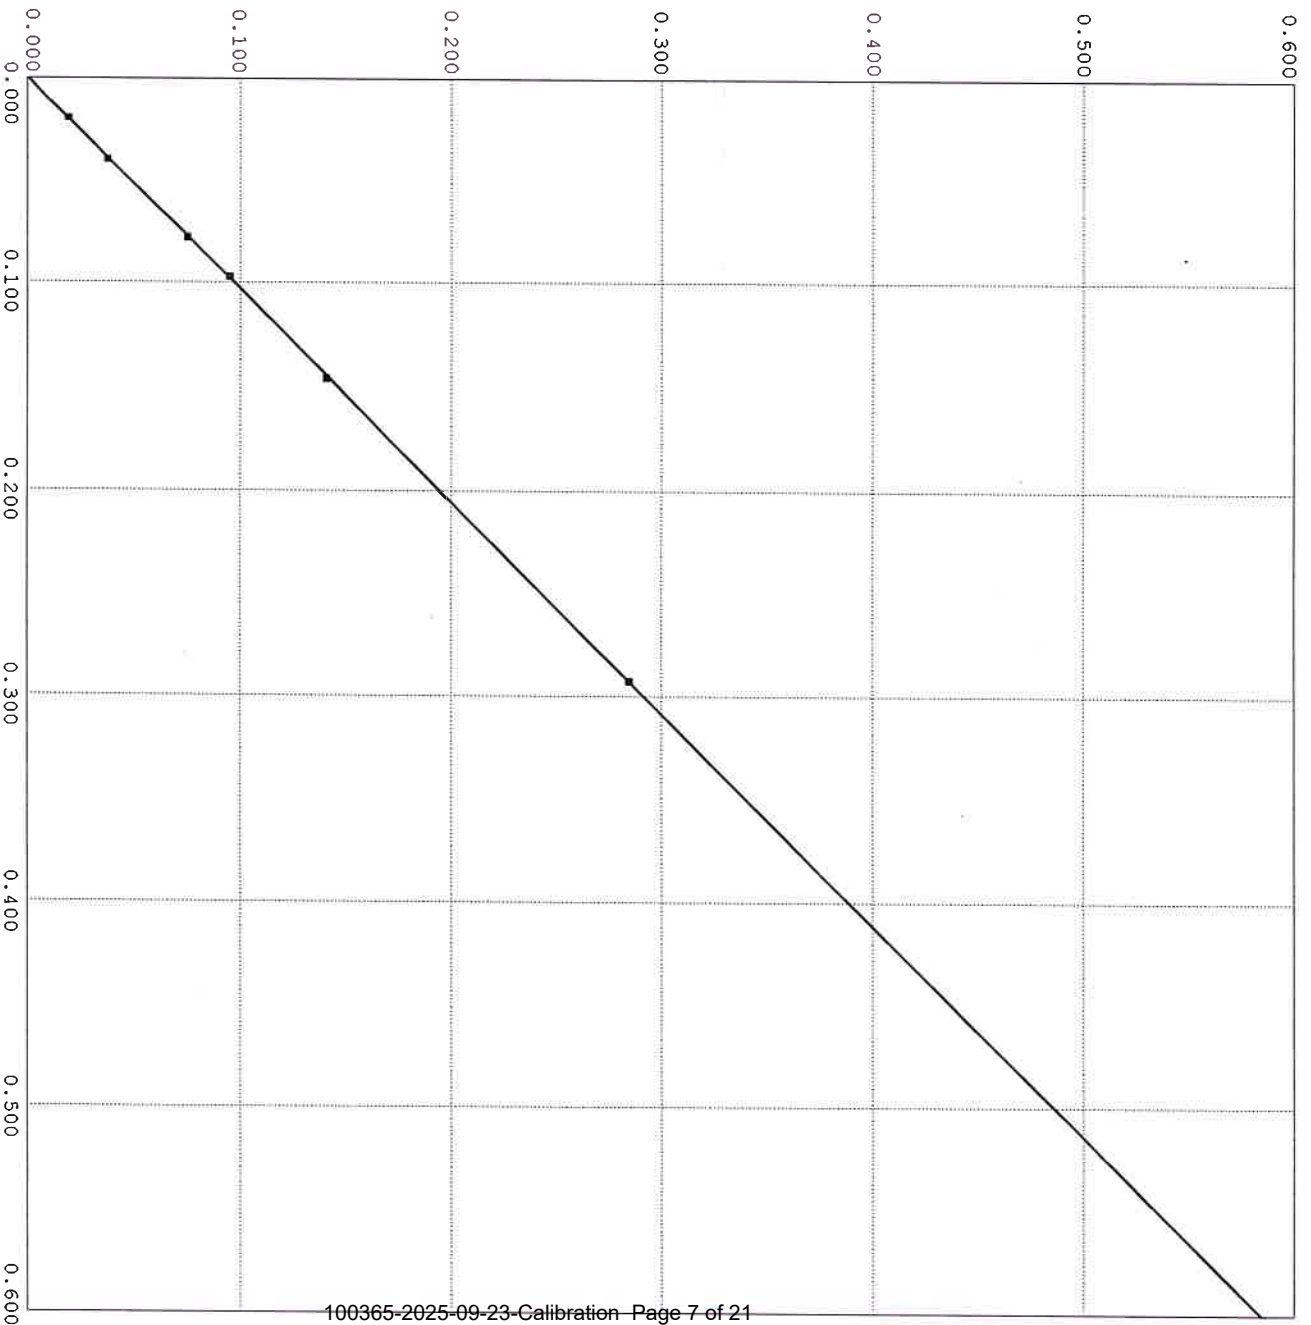

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100365






Date: 09/22/2025
Time: 11:08:27

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.14: 0.019
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 450 psi

BLANK TEST	0.000	11:10
INTERNAL STANDARD	VERIFIED	11:10
EXTERNAL STANDARD	0.020	11:10
BLANK TEST	0.000	11:11
EXTERNAL STANDARD	0.020	11:12
BLANK TEST	0.000	11:12
EXTERNAL STANDARD	0.019	11:13
BLANK TEST	0.000	11:14
EXTERNAL STANDARD	0.020	11:14
BLANK TEST	0.000	11:15
EXTERNAL STANDARD	0.020	11:15
BLANK TEST	0.000	11:16

Average = 0.0198
Std Dev = 0.0004

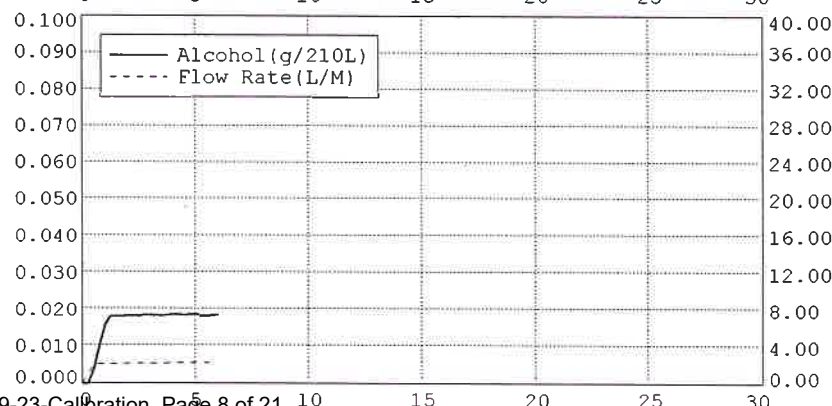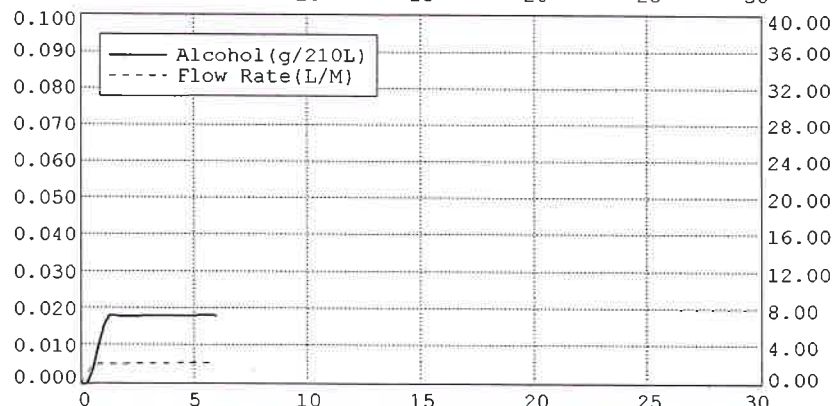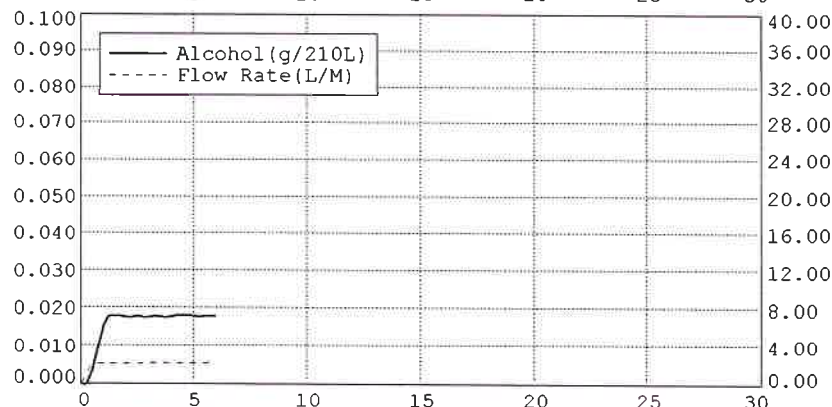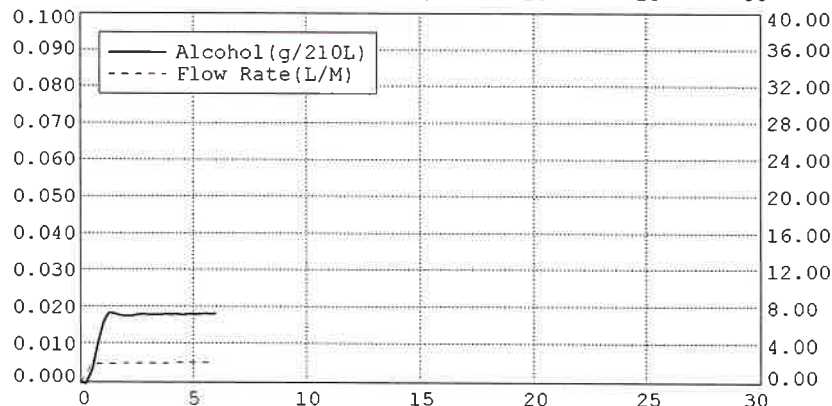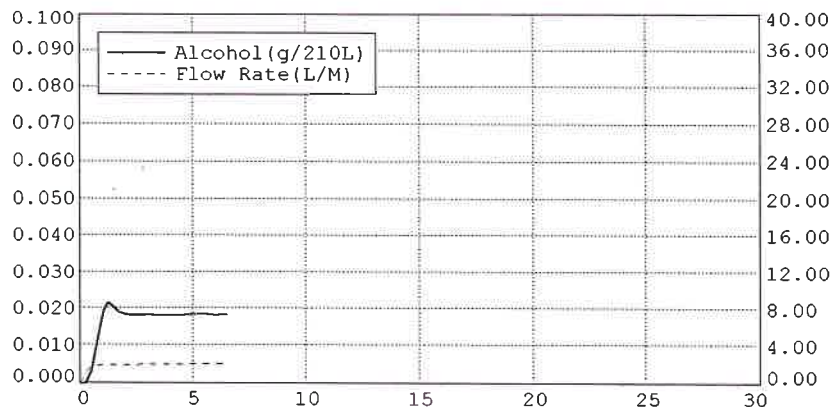

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100365






Date: 09/22/2025
Time: 11:17:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.15: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 888 psi

BLANK TEST	0.000	11:19
INTERNAL STANDARD	VERIFIED	11:19
EXTERNAL STANDARD	0.038	11:19
BLANK TEST	0.000	11:20
EXTERNAL STANDARD	0.039	11:20
BLANK TEST	0.000	11:21
EXTERNAL STANDARD	0.039	11:21
BLANK TEST	0.000	11:22
EXTERNAL STANDARD	0.038	11:22
BLANK TEST	0.000	11:23
EXTERNAL STANDARD	0.038	11:23
BLANK TEST	0.000	11:24

Average = 0.0384
Std Dev = 0.0005

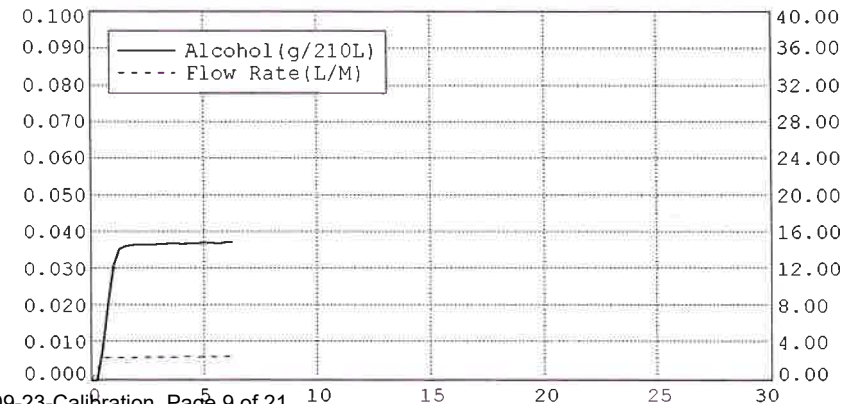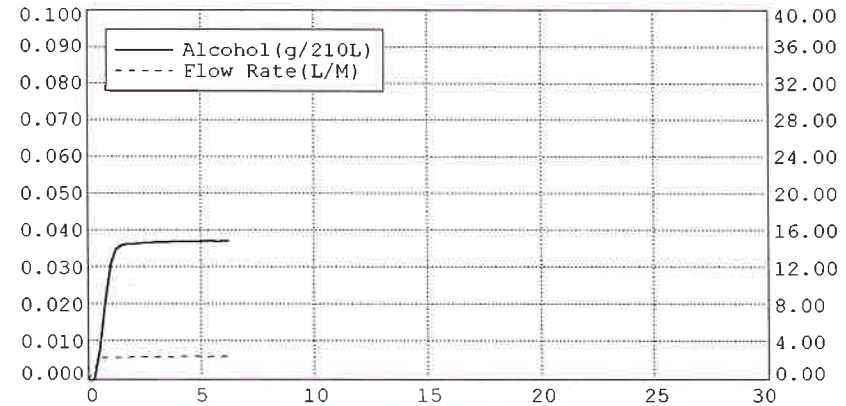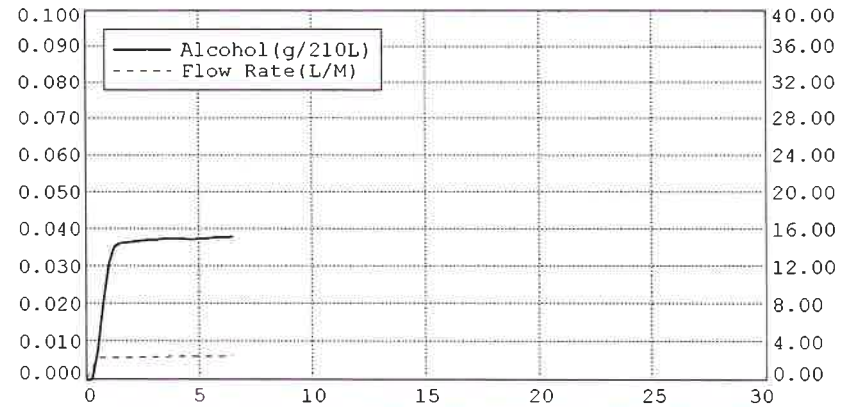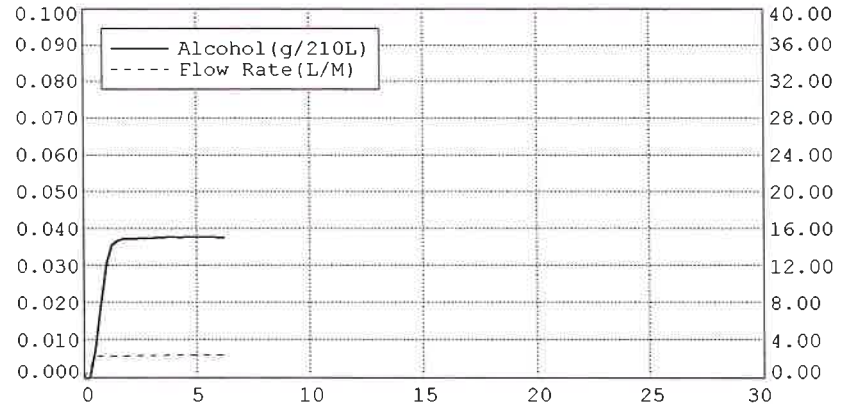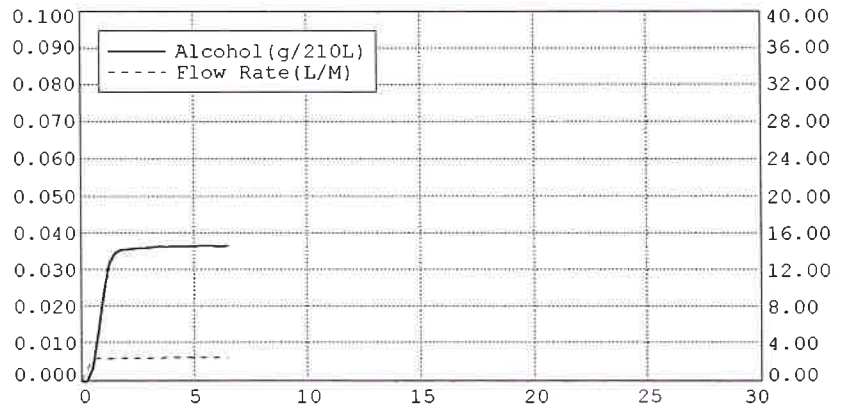

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100365






Date: 09/22/2025
Time: 11:25:26

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.15: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 1107 psi

BLANK TEST	0.000	11:26
INTERNAL STANDARD	VERIFIED	11:26
EXTERNAL STANDARD	0.076	11:27
BLANK TEST	0.000	11:27
EXTERNAL STANDARD	0.076	11:28
BLANK TEST	0.000	11:29
EXTERNAL STANDARD	0.076	11:29
BLANK TEST	0.000	11:30
EXTERNAL STANDARD	0.076	11:30
BLANK TEST	0.000	11:31
EXTERNAL STANDARD	0.077	11:31
BLANK TEST	0.000	11:32

Average = 0.0762
Std Dev = 0.0004

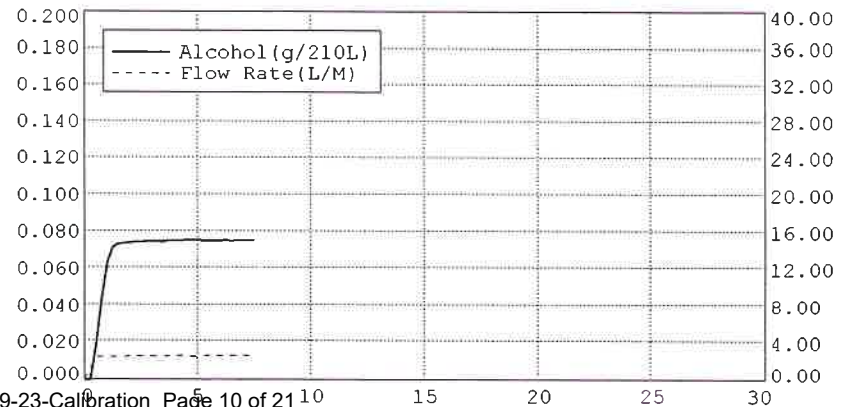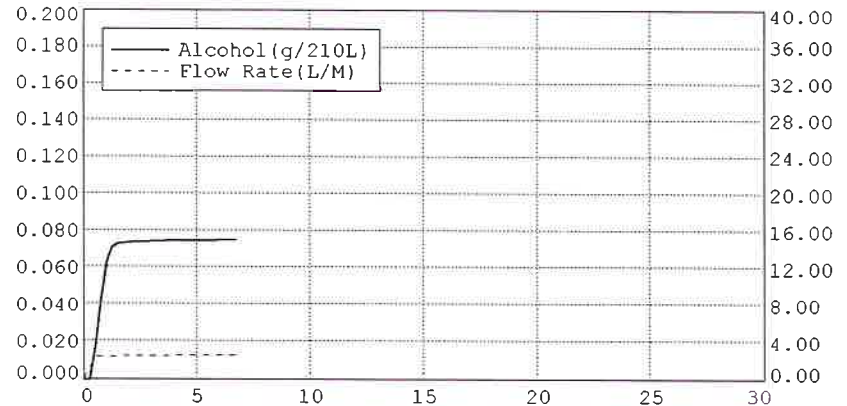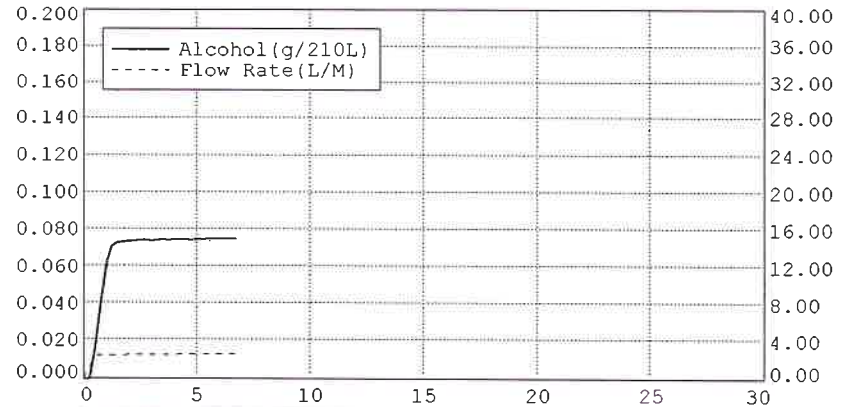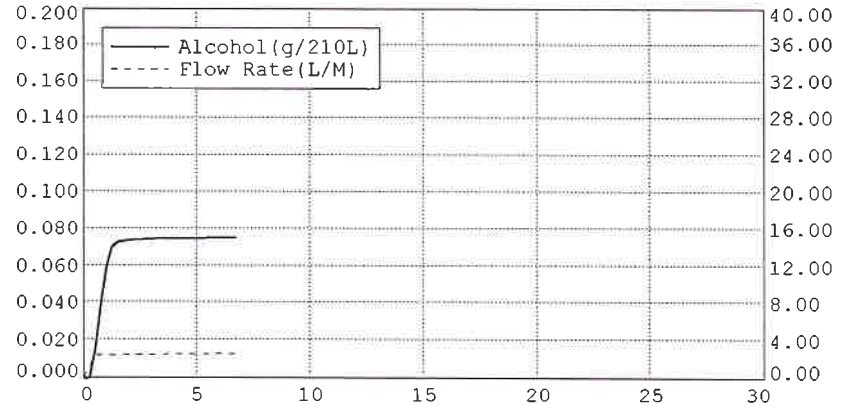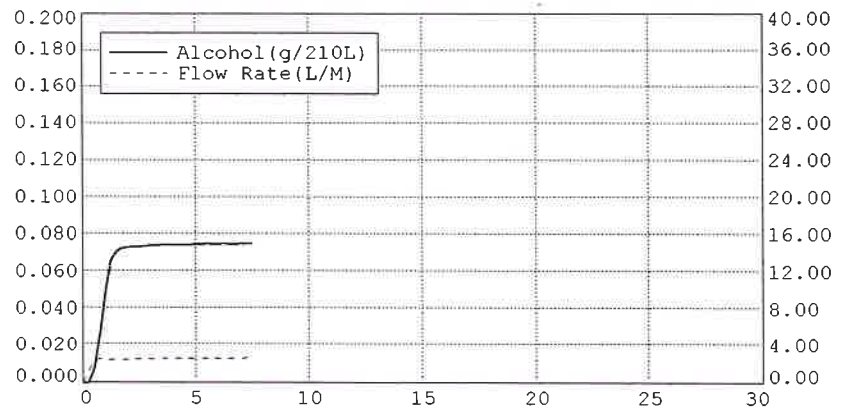

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100365






Date: 09/22/2025
Time: 11:33:03

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.15: 0.097
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 893 psi

BLANK TEST	0.000	11:34
INTERNAL STANDARD	VERIFIED	11:34
EXTERNAL STANDARD	0.096	11:34
BLANK TEST	0.000	11:35
EXTERNAL STANDARD	0.096	11:35
BLANK TEST	0.000	11:36
EXTERNAL STANDARD	0.096	11:36
BLANK TEST	0.000	11:37
EXTERNAL STANDARD	0.096	11:38
BLANK TEST	0.000	11:38
EXTERNAL STANDARD	0.096	11:39
BLANK TEST	0.000	11:40

Average = 0.0960
Std Dev = 0.0000

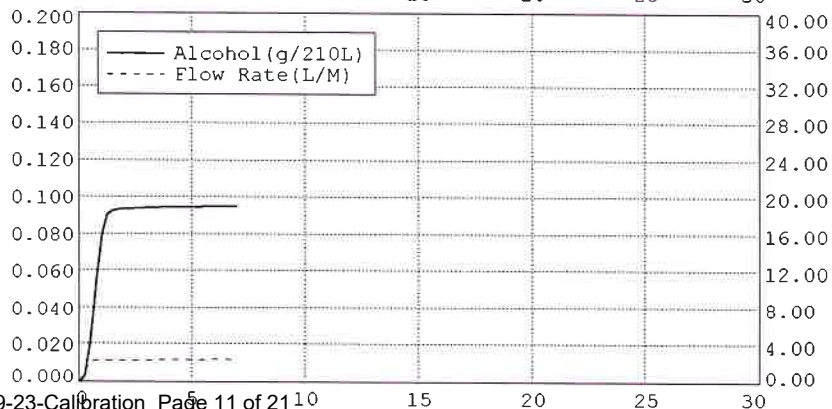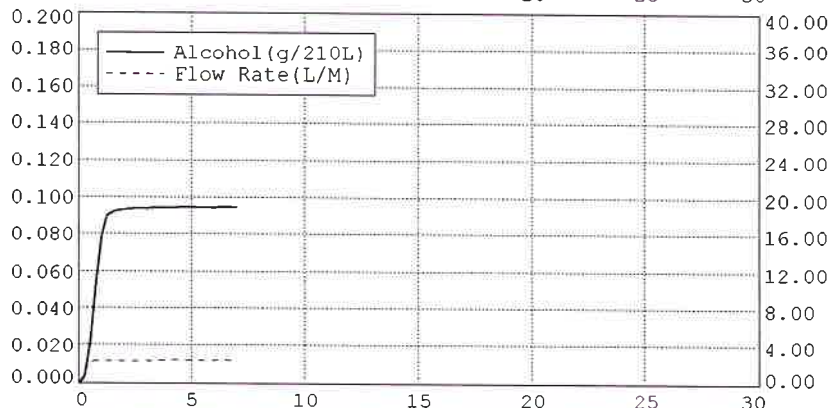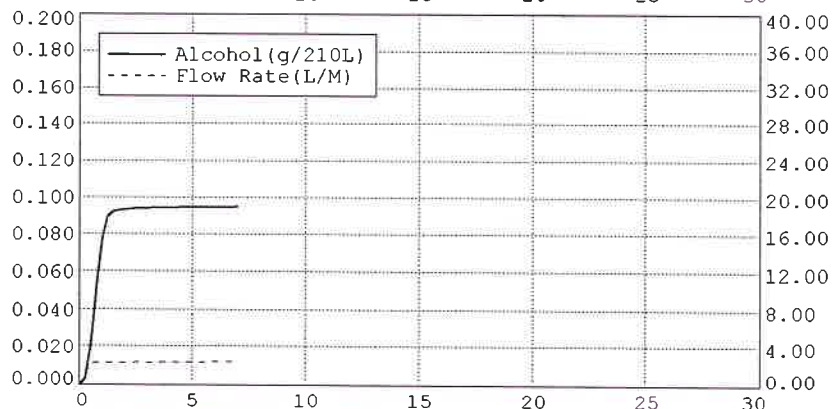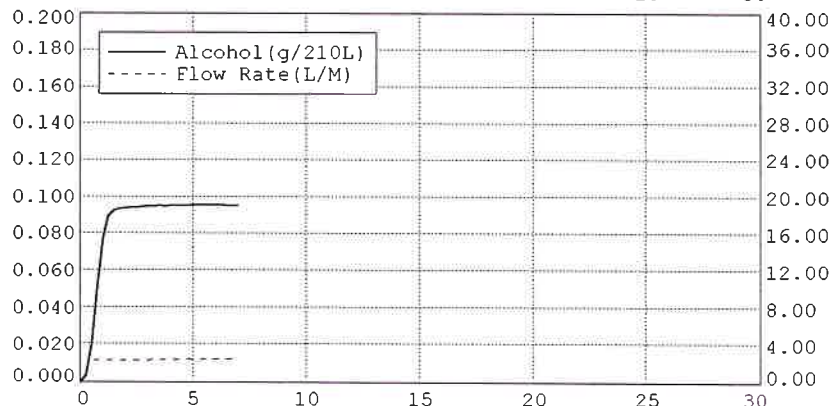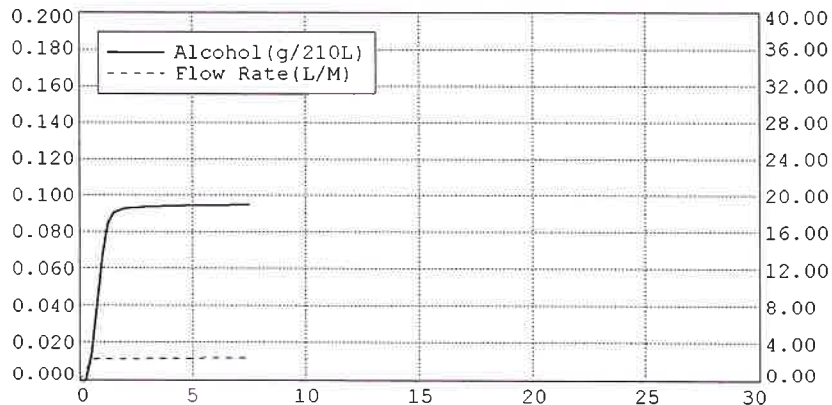

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100365






Date: 09/22/2025
Time: 11:43:34

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.15: 0.146
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 397 psi

BLANK TEST	0.000	11:45
INTERNAL STANDARD	VERIFIED	11:45
EXTERNAL STANDARD	0.142	11:45
BLANK TEST	0.000	11:46
EXTERNAL STANDARD	0.142	11:46
BLANK TEST	0.000	11:47
EXTERNAL STANDARD	0.142	11:47
BLANK TEST	0.000	11:48
EXTERNAL STANDARD	0.141	11:48
BLANK TEST	0.000	11:49
EXTERNAL STANDARD	0.141	11:49
BLANK TEST	0.000	11:50

Average = 0.1416
Std Dev = 0.0005

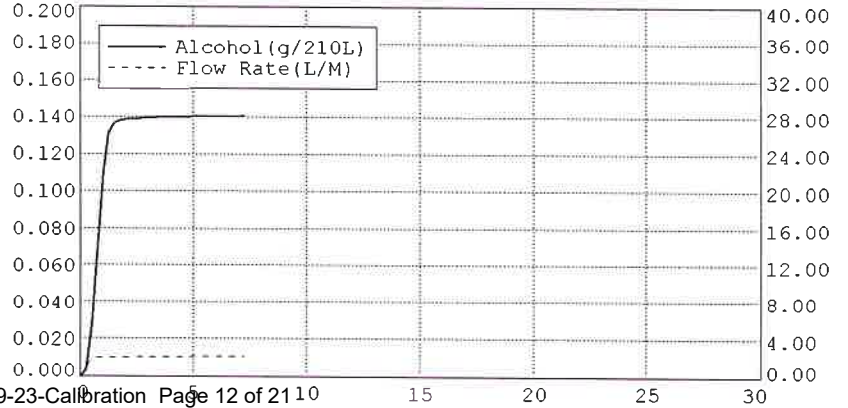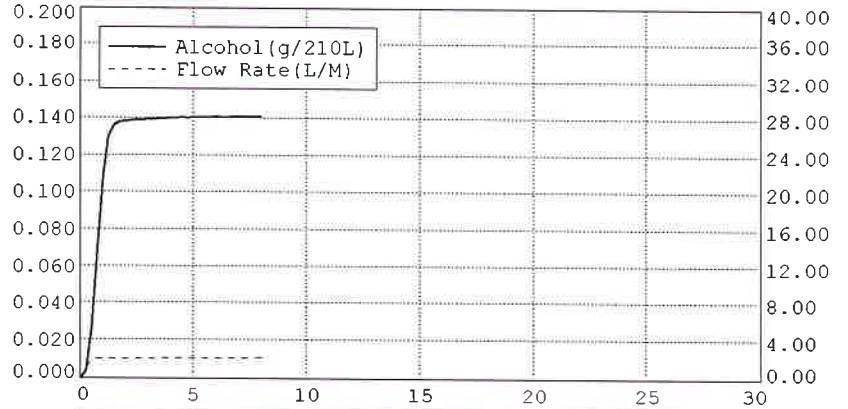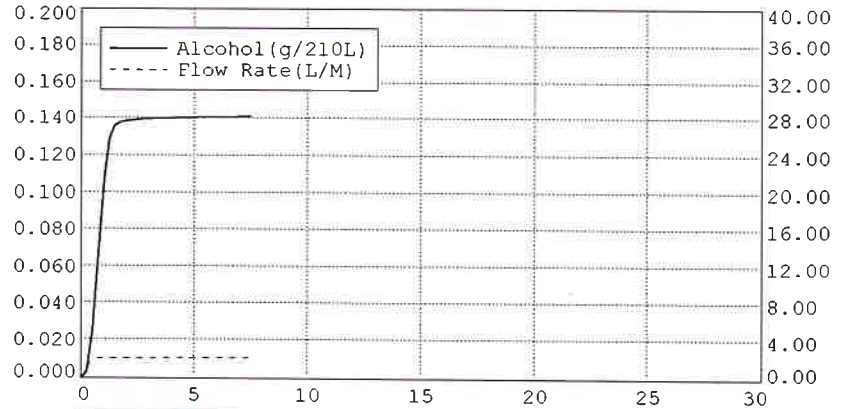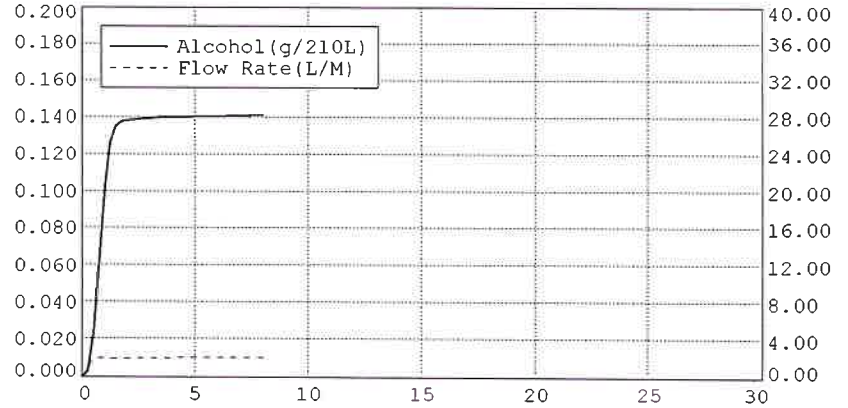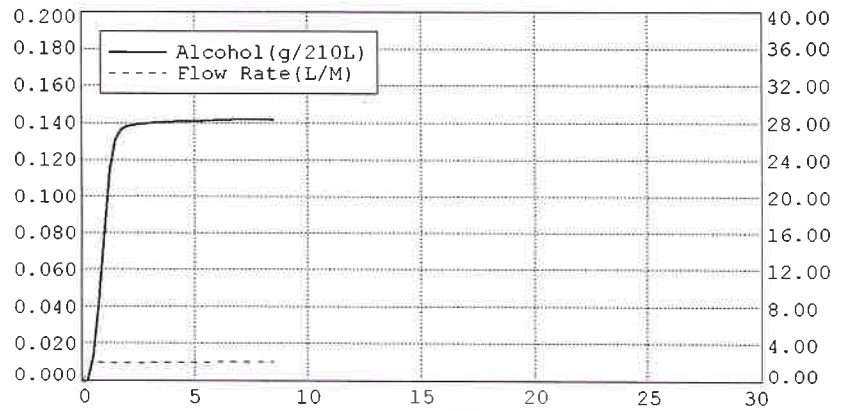

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100365






Date: 09/22/2025
Time: 11:52:02

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.15: 0.292
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 324 psi

BLANK TEST	0.000	11:53
INTERNAL STANDARD	VERIFIED	11:53
EXTERNAL STANDARD	0.286	11:53
BLANK TEST	0.000	11:54
EXTERNAL STANDARD	0.285	11:55
BLANK TEST	0.000	11:55
EXTERNAL STANDARD	0.285	11:56
BLANK TEST	0.000	11:57
EXTERNAL STANDARD	0.285	11:57
BLANK TEST	0.000	11:58
EXTERNAL STANDARD	0.286	11:58
BLANK TEST	0.000	11:59

Average = 0.2854
Std Dev = 0.0005

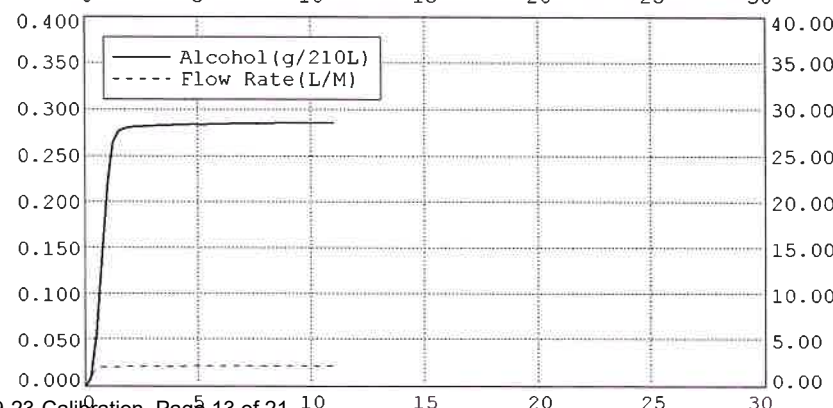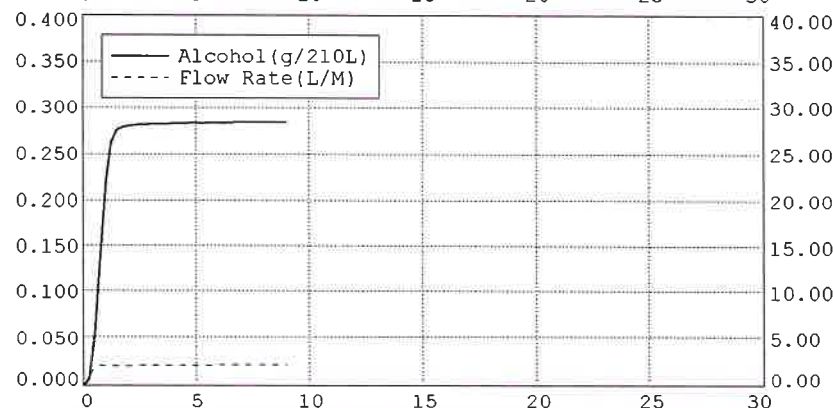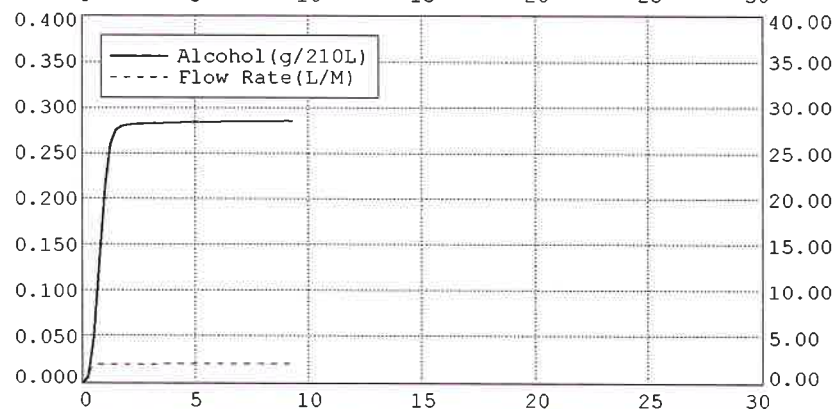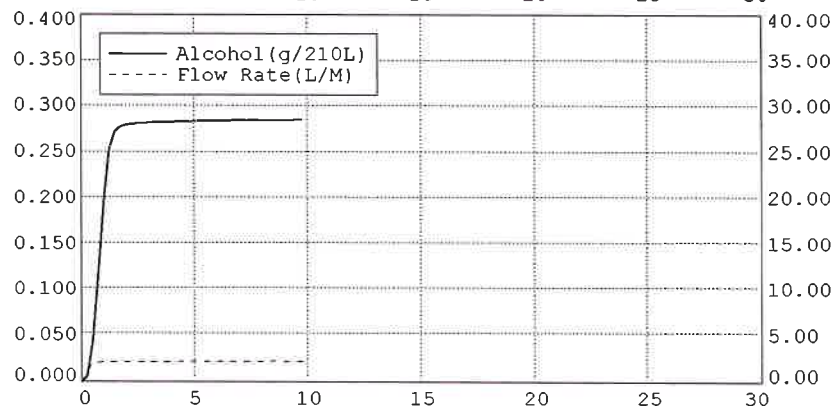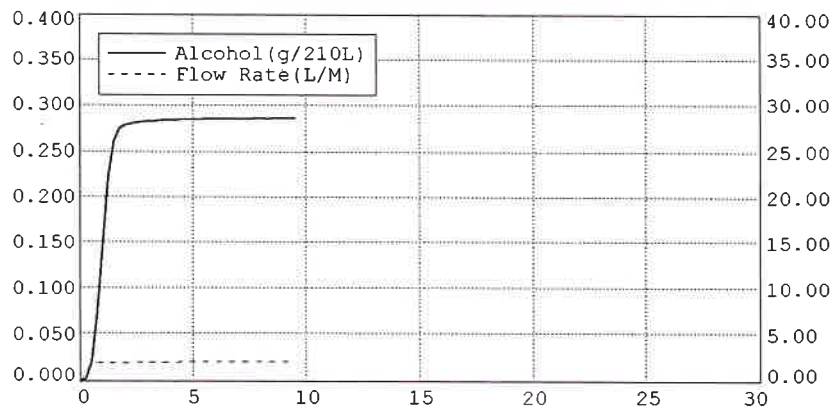

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100365

Date: 09/22/2025
Time: 12:09:01


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.15: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:10
BLANK TEST	0.000	12:10
INTERNAL STANDARD	VERIFIED	12:10
EXTERNAL STANDARD	0.077	12:10
BLANK TEST	0.000	12:11
SUBJECT SAMPLE	INCOMPLETE	12:13

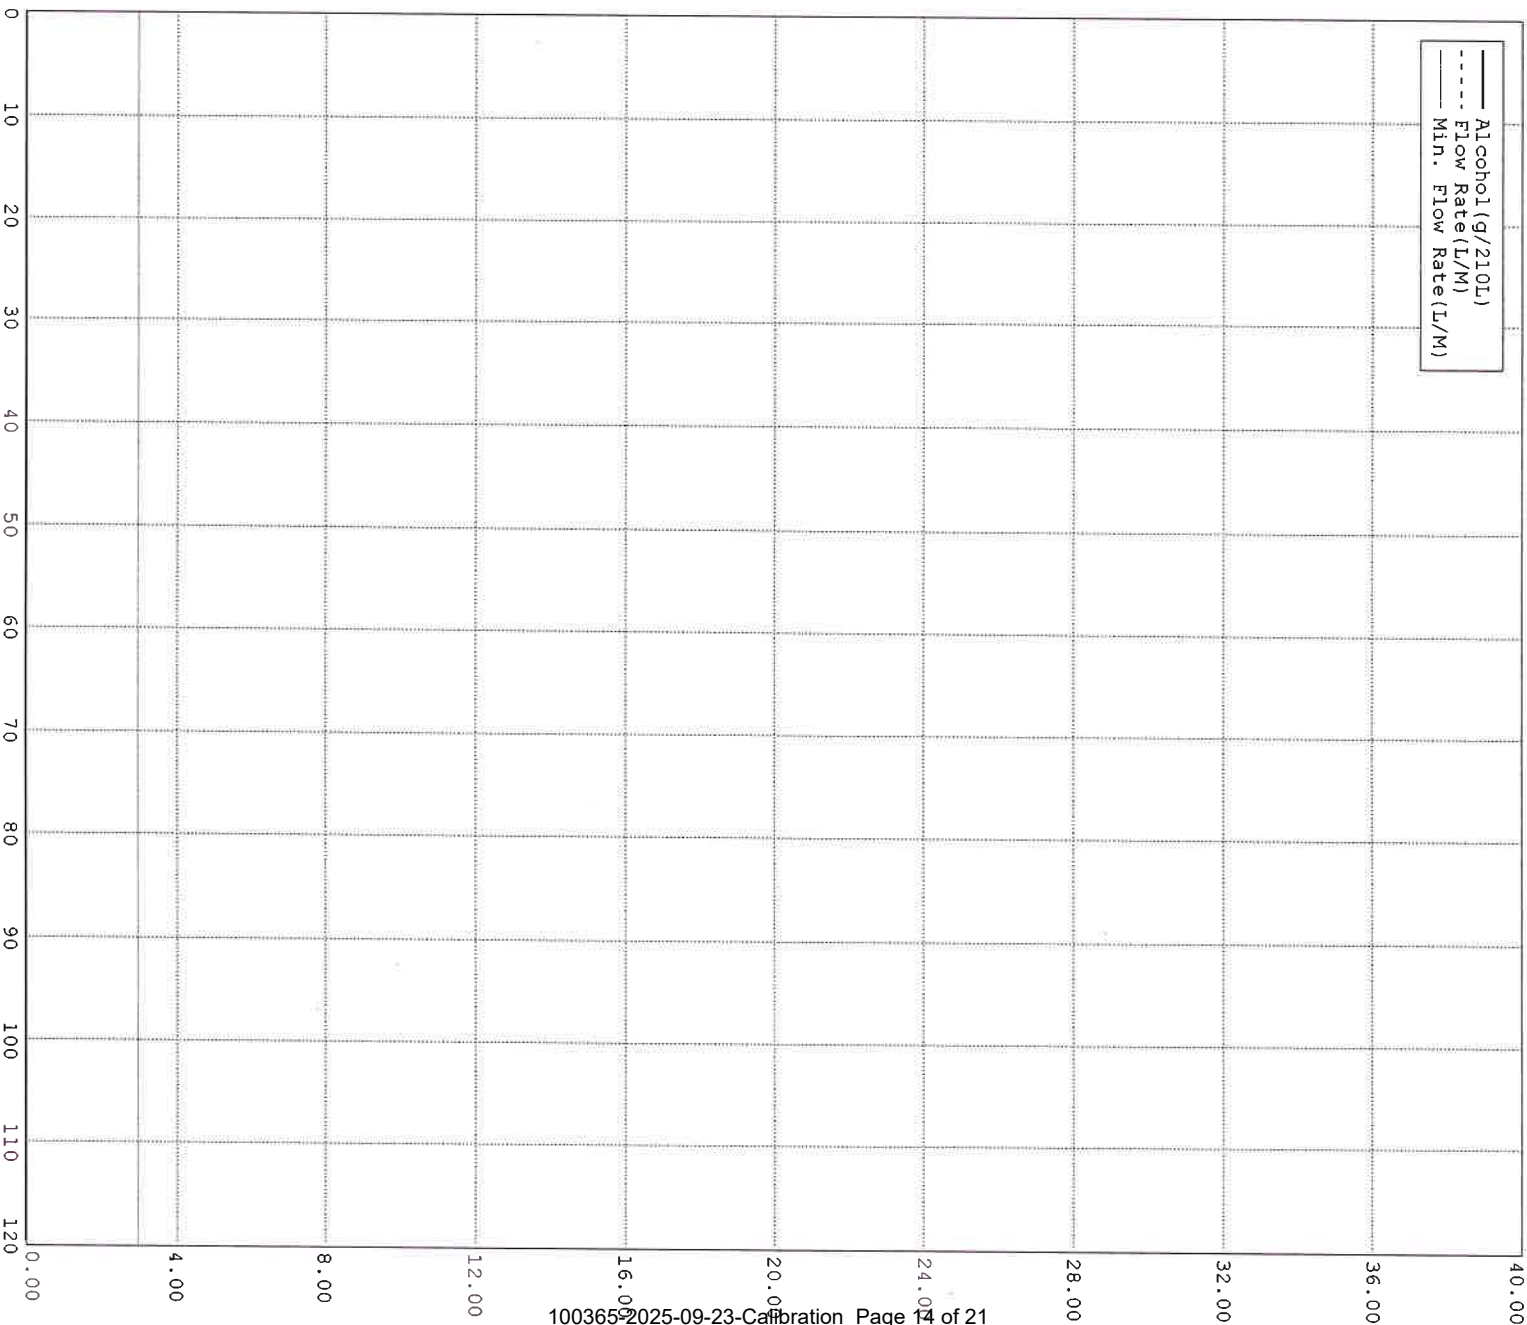

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100365

Date: 09/22/2025
Time: 12:17:37


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.16: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:18
BLANK TEST	0.000	12:18
INTERNAL STANDARD	VERIFIED	12:18
EXTERNAL STANDARD	0.077	12:19
BLANK TEST	0.000	12:20
SUBJECT SAMPLE	INVALID	12:20

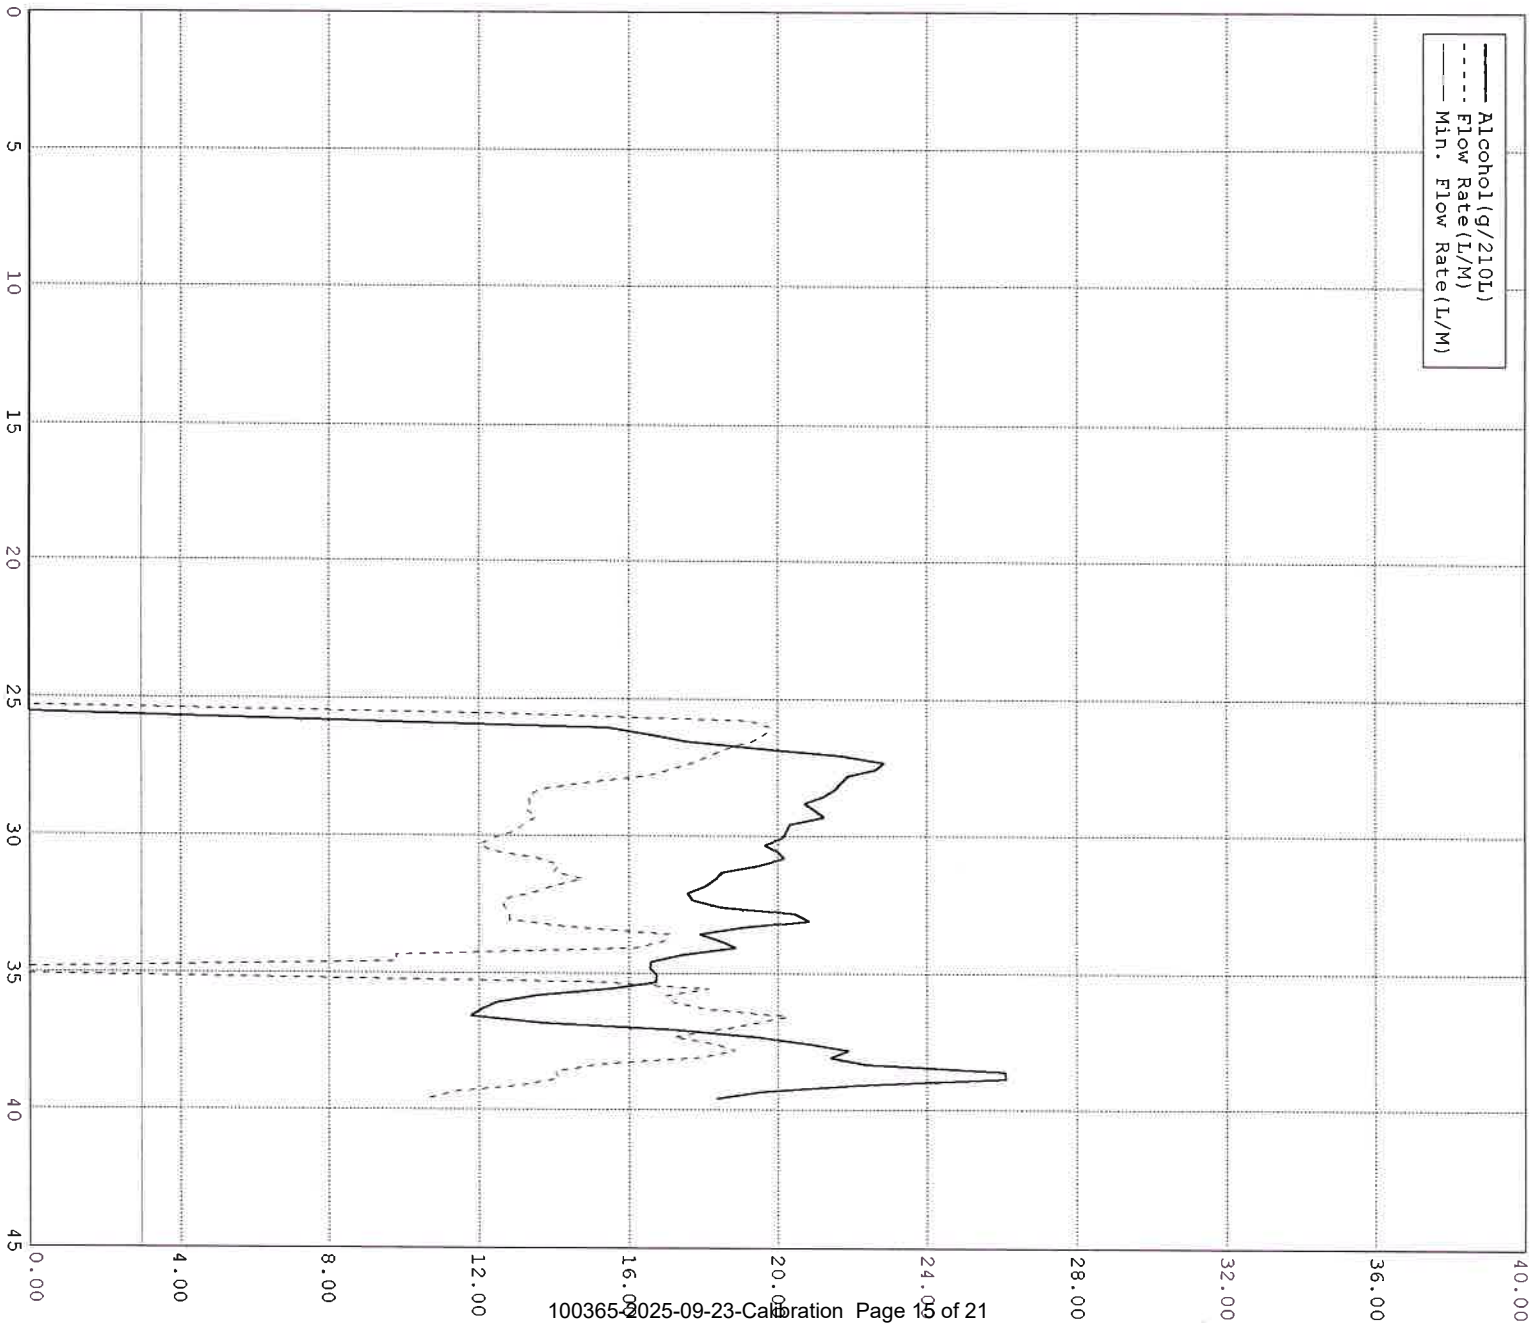

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100365

Date: 09/22/2025
Time: 13:04:01

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KALJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MAX ATTEMPTS
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:05
BLANK TEST	0.000	13:05
INTERNAL STANDARD	VERIFIED	13:05
EXTERNAL STANDARD	0.077	13:05
BLANK TEST	0.000	13:06
SUBJECT SAMPLE	XXX	13:07

Maximum Attempts Exceeded

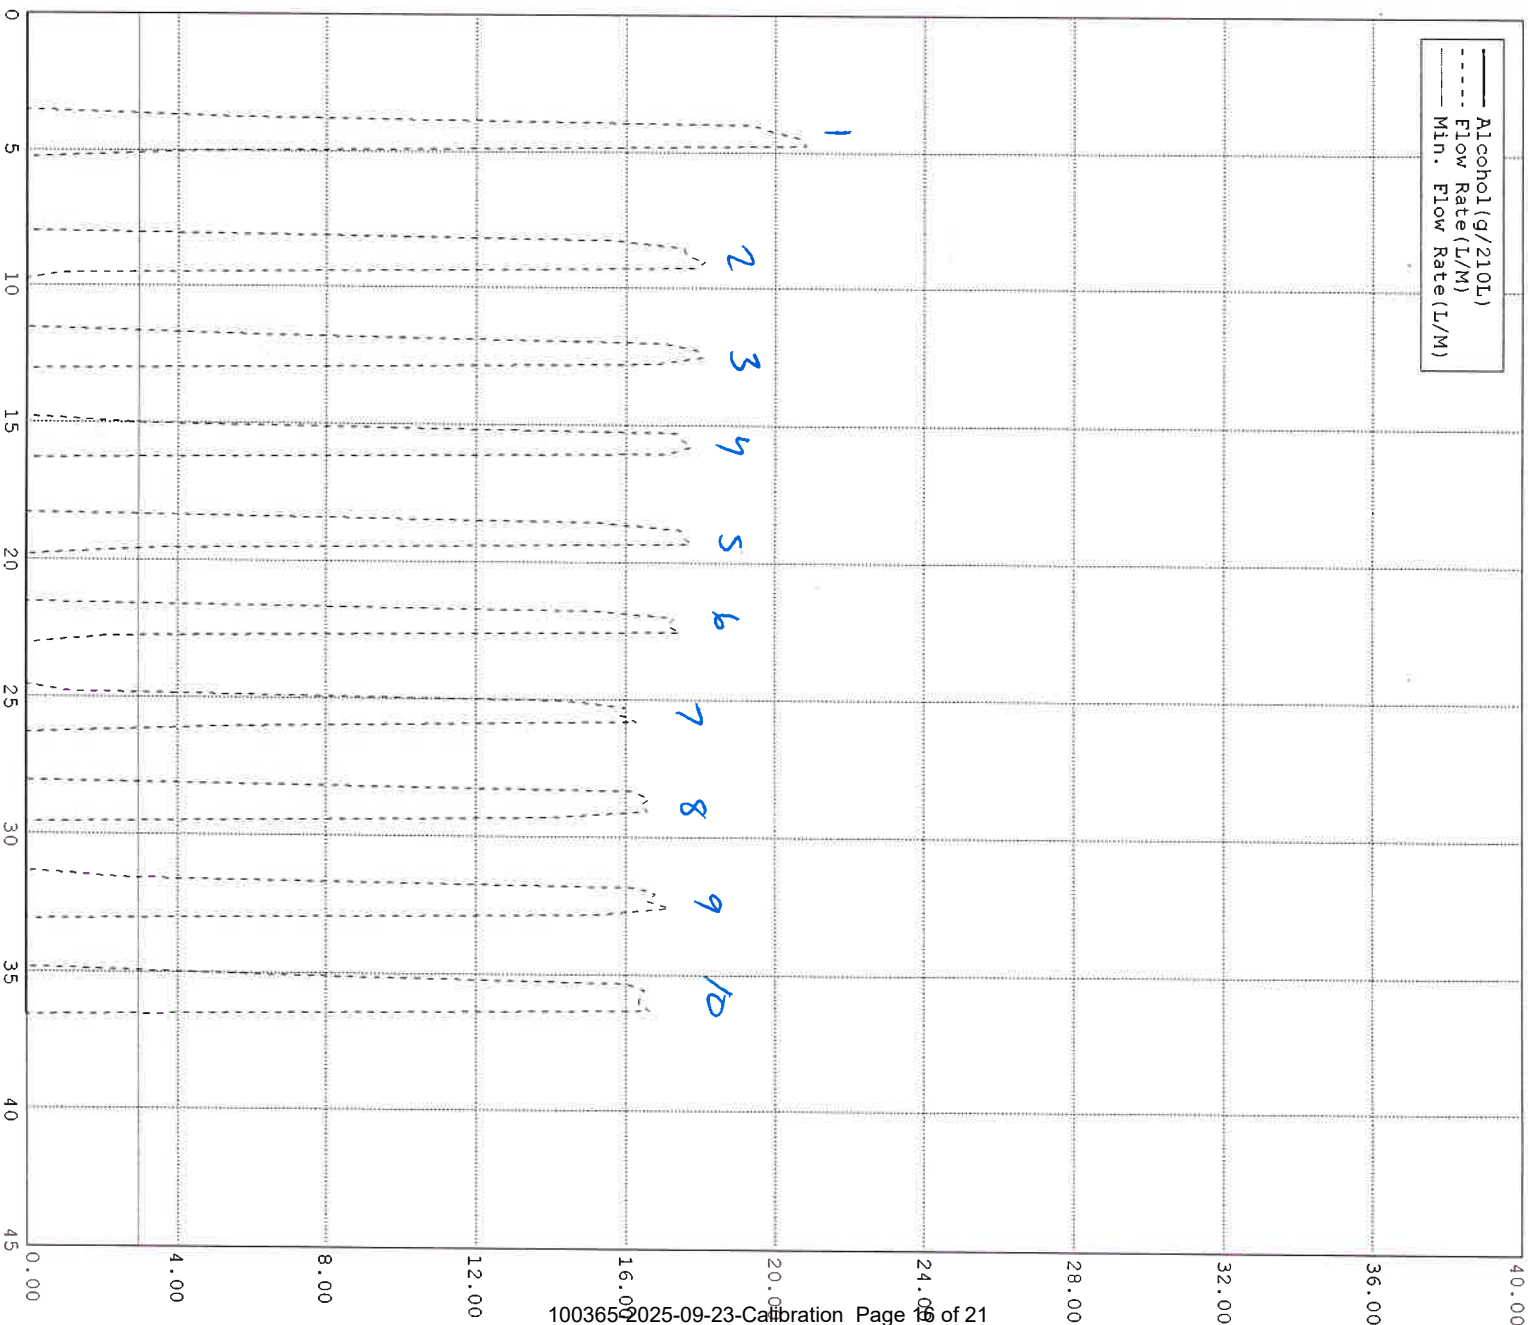

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100365

Date: 09/22/2025
Time: 13:08:47

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.16: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:09
BLANK TEST	0.000	13:09
INTERNAL STANDARD	VERIFIED	13:10
EXTERNAL STANDARD	0.076	13:10
BLANK TEST	0.000	13:11

RFI DETECTED

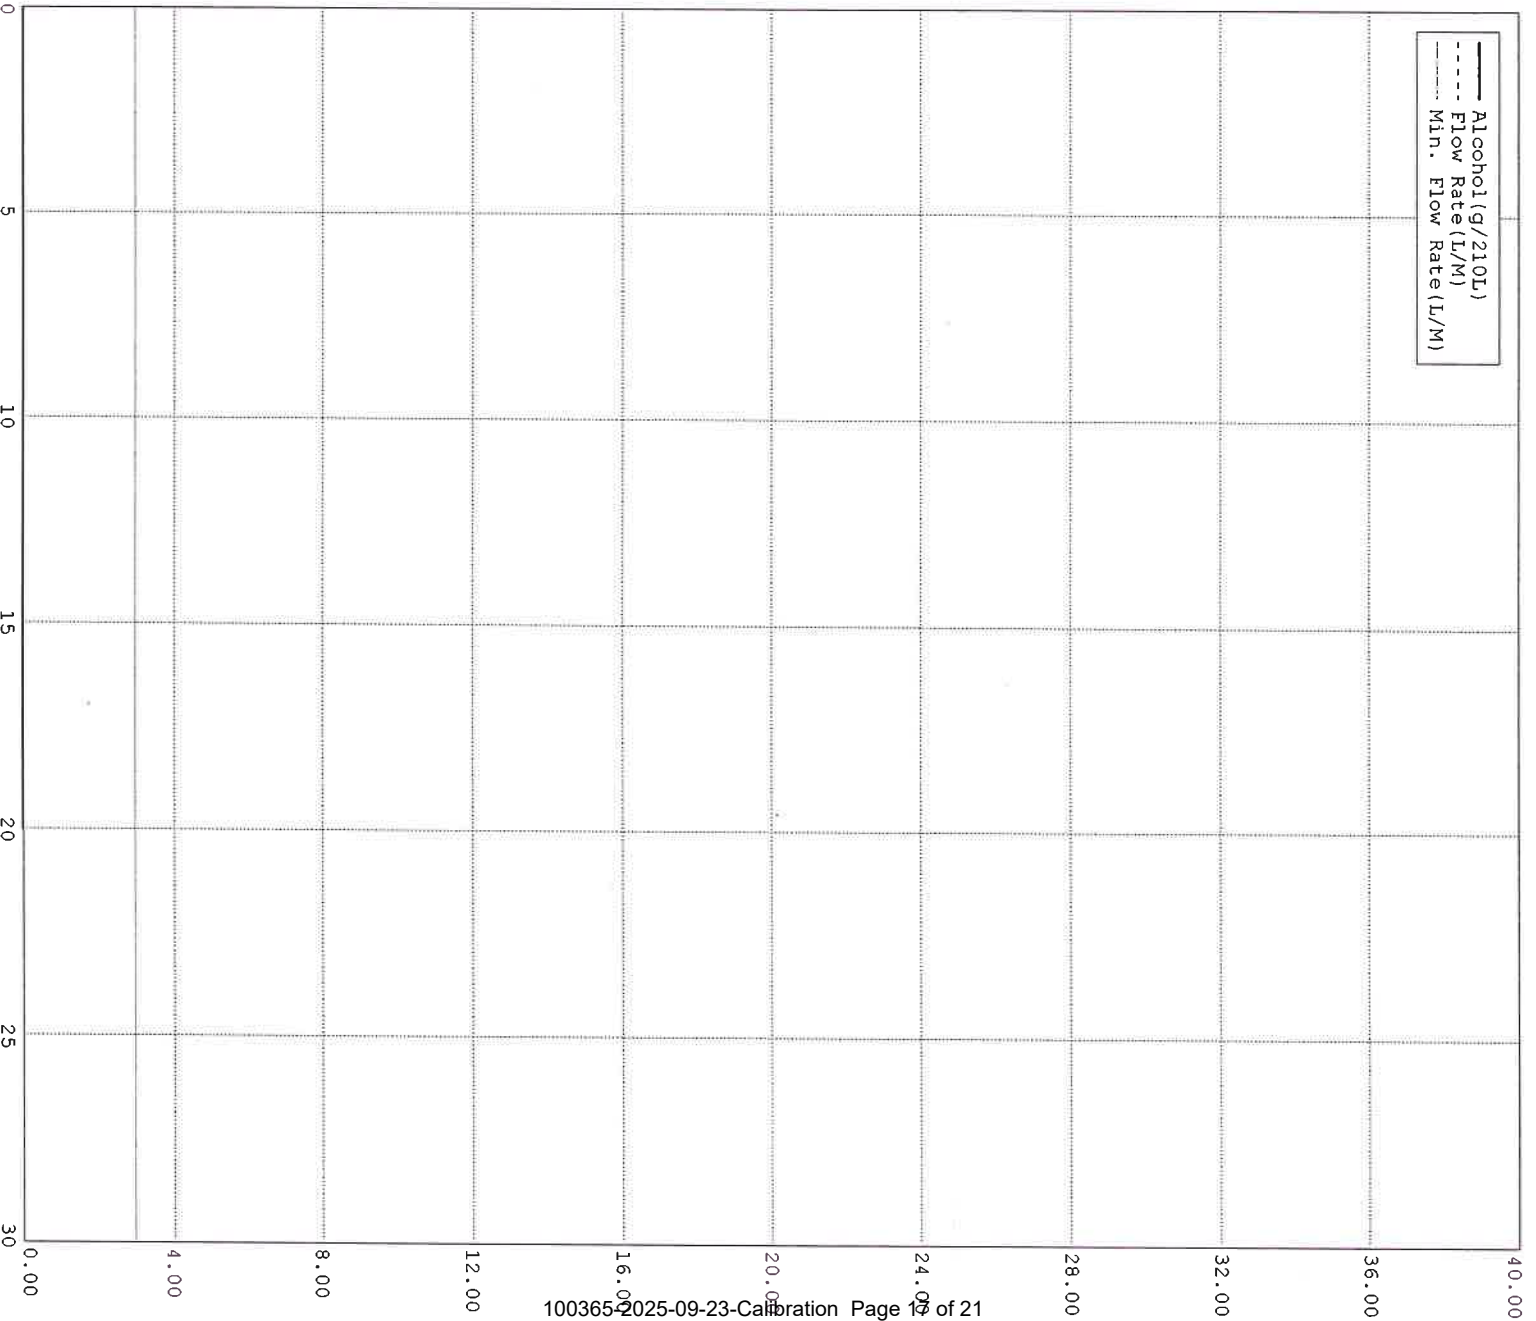

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100365

Date: 09/22/2025
Time: 13:27:22

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KALIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK		PASSED	13:28
BLANK TEST		0.000	13:28
INTERNAL STANDARD	VERIFIED		13:29
Xq = 0.093 (0.28%)			
EXTERNAL STANDARD		0.077	13:29
X[1] = 0.0770 (-0.0003)		(0.0022)	
BLANK TEST		0.000	13:30
SUBJECT SAMPLE		XXX	13:31
X[1] = 0.1091 (-0.0170)		(0.0008)	


Interference Detected

extra digit added, KS 10/1/25

Filter 2ave: 0.0060

Filter 3ave: 0.0023

KS 9/23/25

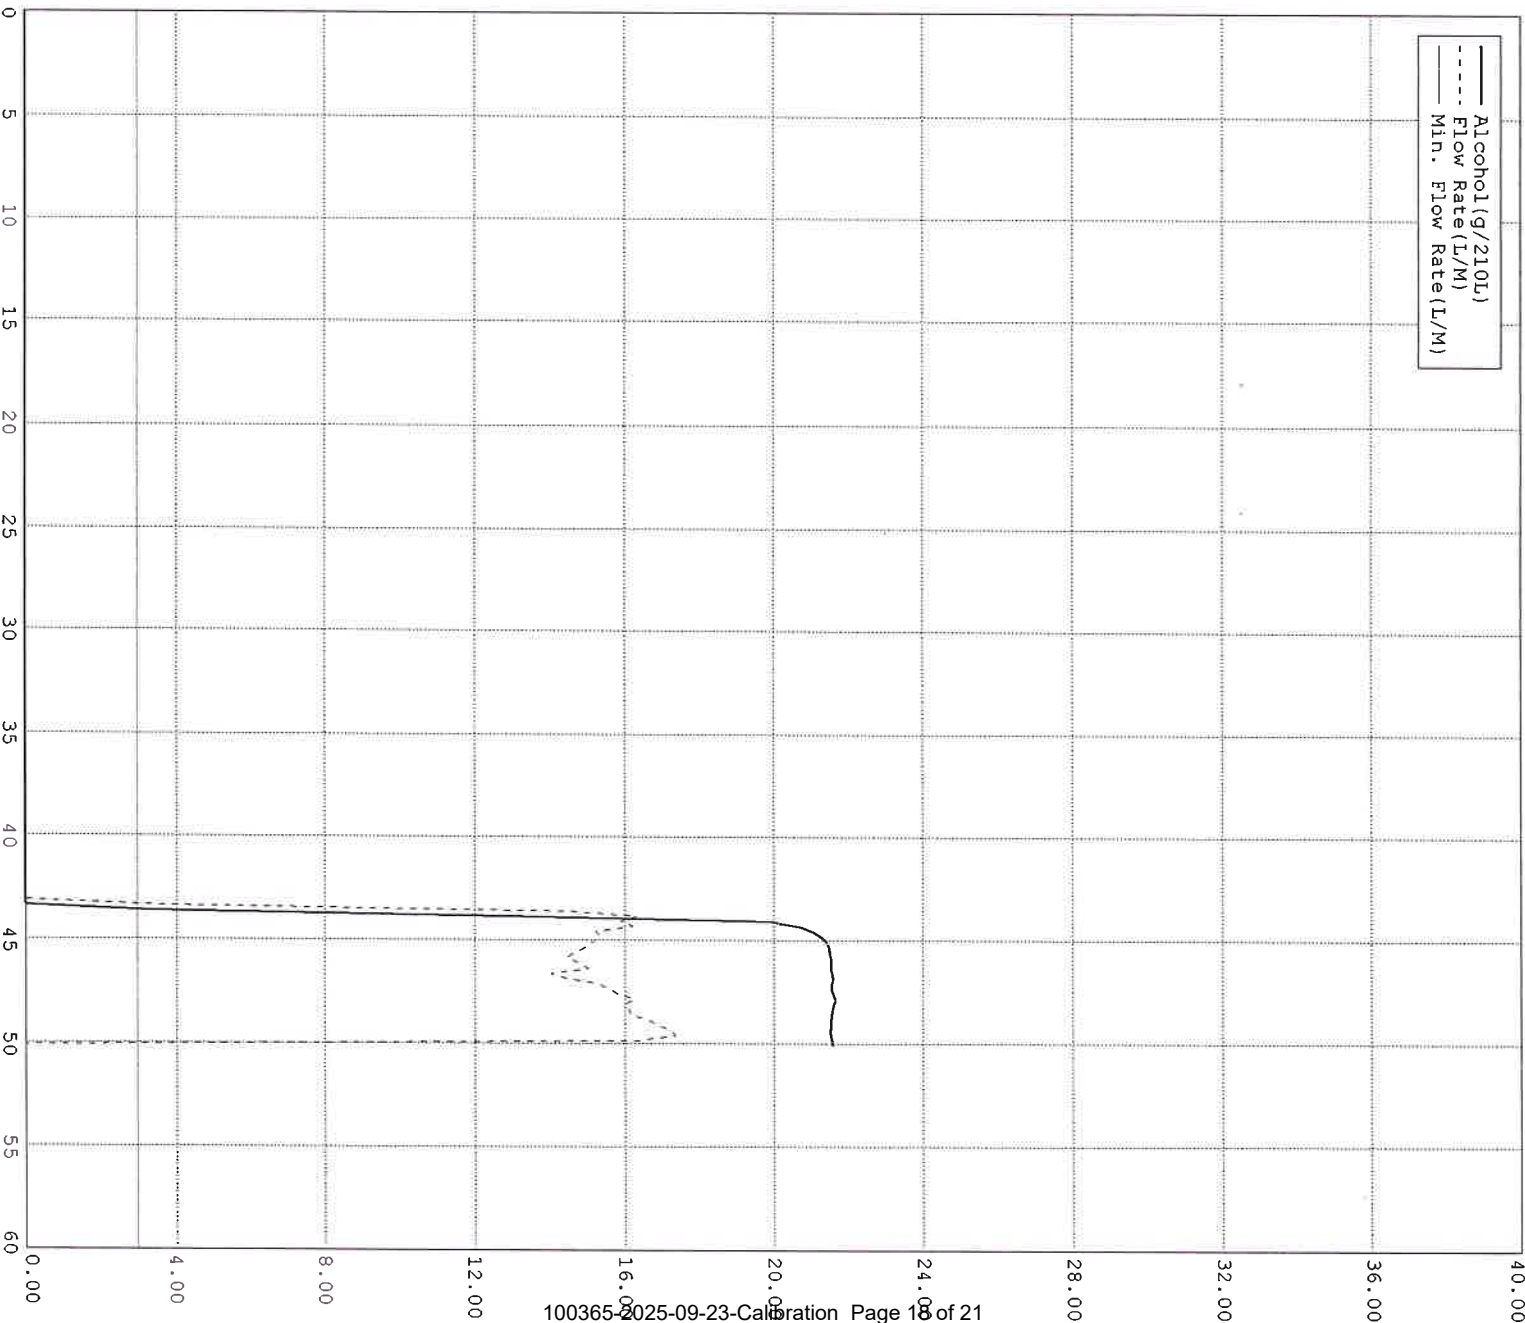

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100365

Date: 09/22/2025
Time: 13:20:07

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 13:21
INTERNAL STANDARD VERIFIED 13:21
Xq = 0.094 (0.47%)
EXTERNAL STANDARD 0.077 13:21
X[1] = 0.0767 (-0.0001) (0.0026)
BLANK TEST 0.000 13:22
SUBJECT SAMPLE XXX 13:23
X[1] = 0.1201 (-0.0240) (0.0016)

Interference Detected

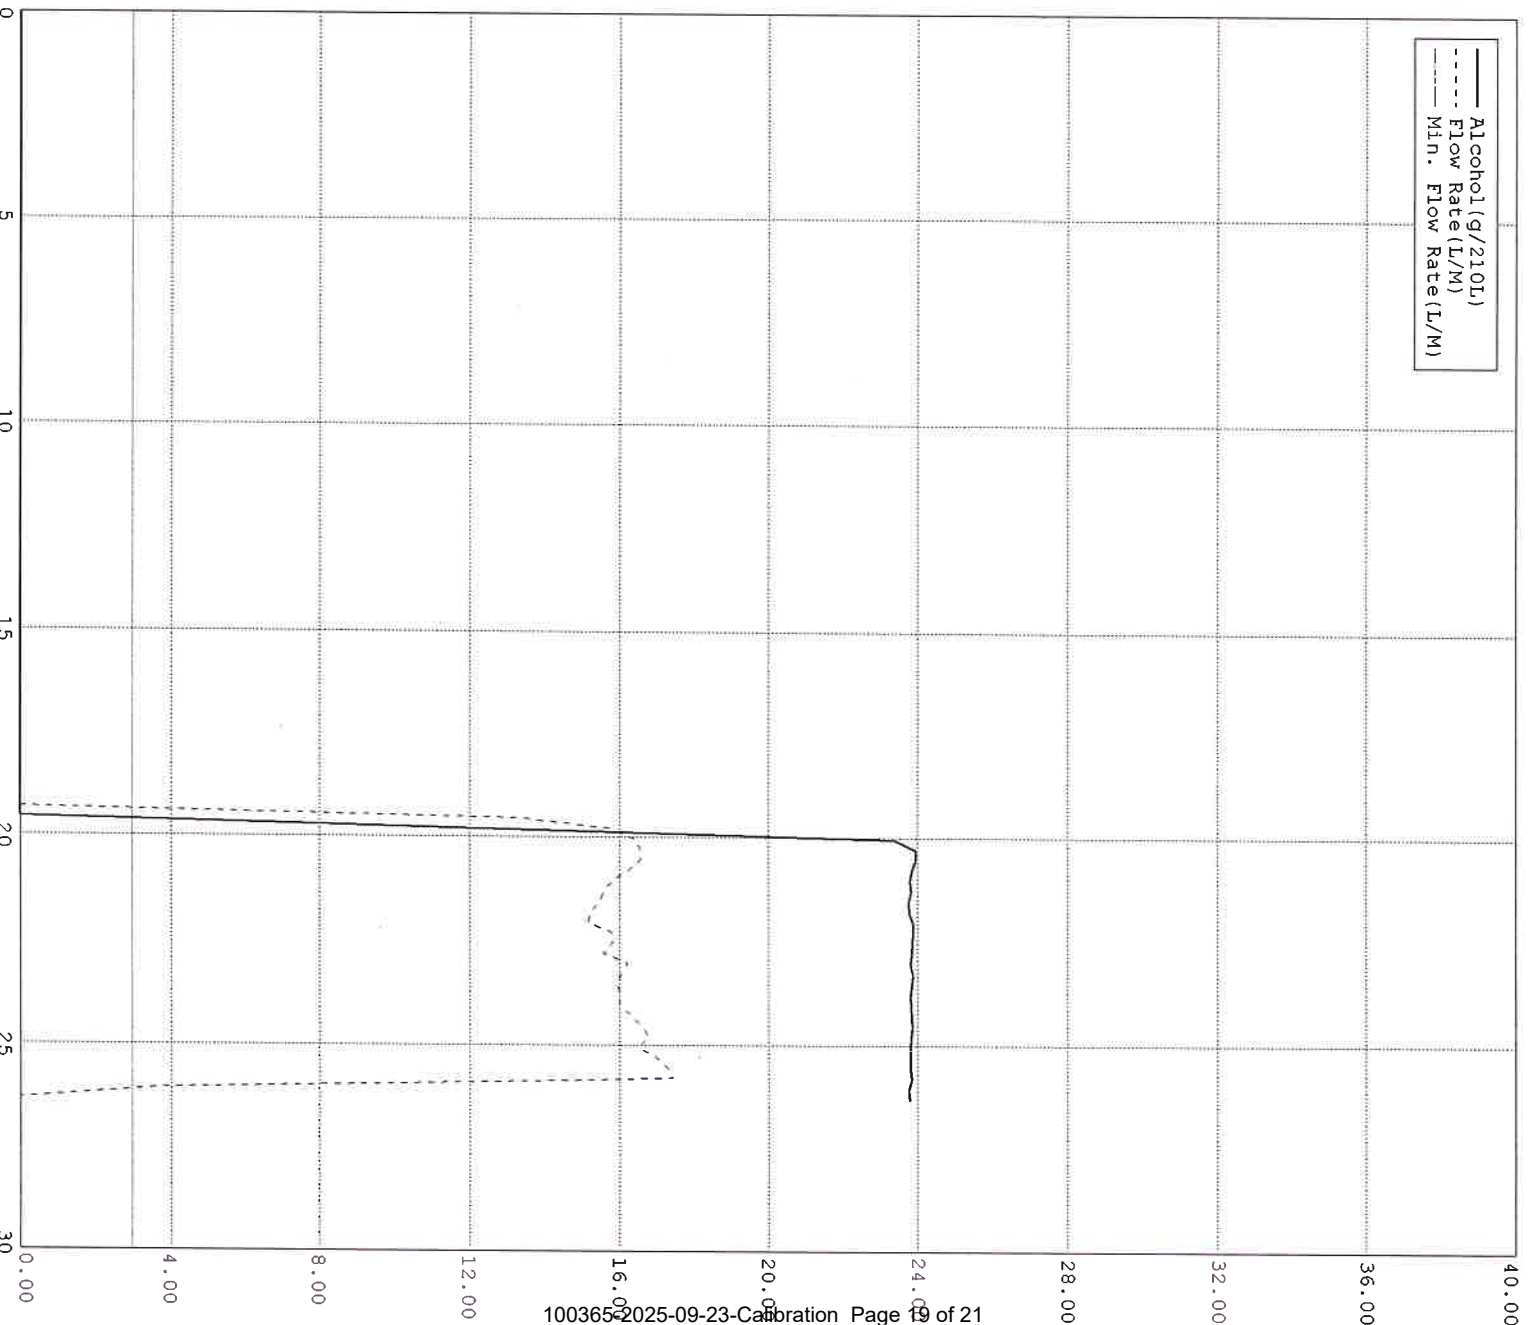

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100365

Date: 09/22/2025
Time: 13:35:03


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 13:36
INTERNAL STANDARD VERIFIED 13:36
Xq = 0.094 (0.56%)
EXTERNAL STANDARD 0.077 13:36
X[1] = 0.0772 (0.0003) (0.0027)
BLANK TEST 0.000 13:37
SUBJECT SAMPLE (Vol=1.63L) 0.096 13:38
X[1] = 0.0961 (0.0016) (0.0013)
BLANK TEST 0.000 13:39
EXTERNAL STANDARD 0.076 13:39
X[1] = 0.0761 (0.0001) (0.0016)
BLANK TEST 0.000 13:40

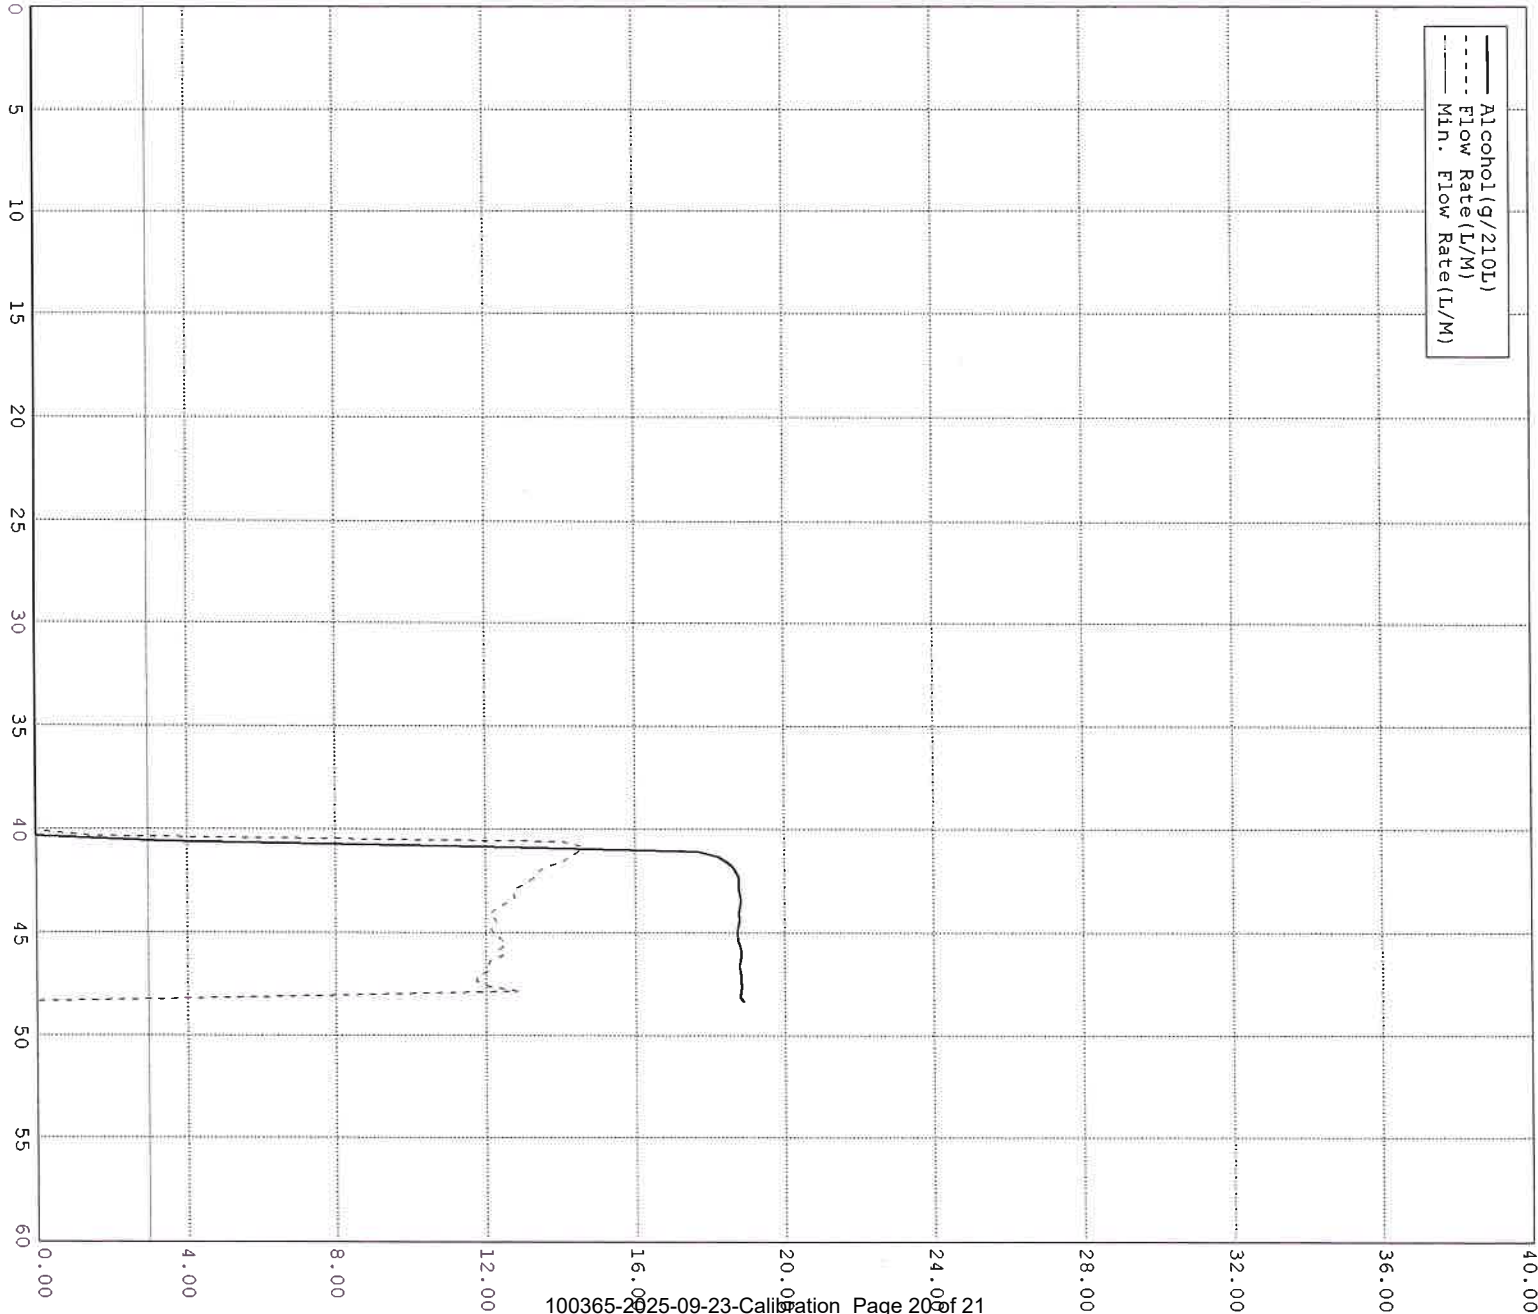

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100365

Date: 09/22/2025
Time: 14:27:51

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAJUA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON-DRINKING TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:28
BLANK TEST	0.000	14:29
INTERNAL STANDARD	VERIFIED	14:29
EXTERNAL STANDARD	0.076	14:29
BLANK TEST	0.000	14:30
SUBJECT SAMPLE (Vol=1.89L)	0.000	14:30
BLANK TEST	0.000	14:31
EXTERNAL STANDARD	0.077	14:31
BLANK TEST	0.000	14:32

