



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100675

Report Issue Date: 12/06/2023
Date Received: 2023-10-23
Condition of Item: Good

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

Start Date 11/06/2023 - As Found - **End Date 11/06/2023** As Found - Evaluation Analyst: Carlie Glaister
 As Found Conditions - Barometric Pressure (inHg): 29.12 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.2
 Relative Humidity (%): 22

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.019	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.078	AG310901	0.077	0.077	0.077	0.077	0.077	0.077	0.077
0.300	0.291	AG217903	0.299	0.297	0.297	0.298	0.298	0.298	0.298

Cleared memory & reset options before eval. Instrument would not upload at check in. Cermetex box needed to be resetted. Modem line connection was checked and it connected successfully. Modem line is now functioning properly.

Start Date 11/30/2023 - As Left - **End Date 12/04/2023**

As Left Conditions - Barometric Pressure (inHg): 28.84 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.4 Relative Humidity (%): 19

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.019	AG217902	0.019	0.019	0.019	0.019	0.019	0.019	+/- 0.002	
0.040	0.039	AG217904	0.038	0.038	0.038	0.038	0.039	0.038	+/- 0.003	
0.080	0.077	AG310901	0.075	0.075	0.076	0.076	0.076	0.076	+/- 0.004	
0.100	0.096	AG211003	0.096	0.096	0.096	0.096	0.096	0.096	+/- 0.004	
0.150	0.145	AG134205	0.144	0.144	0.144	0.144	0.144	0.144	+/- 0.005	
0.300	0.289	AG217903	0.290	0.290	0.290	0.291	0.290	0.290	+/- 0.011	

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories

Serial Number: 100675

Results authorized by Carlie Glaister on 12/04/2023

carlie.glaister@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 12/06/2023

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100675 Analyst: Carlie Glaister Start Date: 11/30/23

- Diagnostic Test (attached)
- Adjust voltages, if needed
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Internal Standard value \leq 3.00%
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.5 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 20.84 Temperature (C): 22.4 Relative Humidity (%) 19

Linearity Test (attached)

0.020g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217902</u>	Exp: <u>6/28/24</u>
0.040g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217904</u>	Exp: <u>6/28/24</u>
0.080g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-310901</u>	Exp: <u>4/19/25</u>
0.100g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-211003</u>	Exp: <u>4/20/24</u>
0.150g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-134205</u>	Exp: <u>12/8/23</u>
0.300g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217903</u>	Exp: <u>6/28/24</u>

Functional Tests (attached)

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles)
- Acetone Mnf: Lifloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24
Simulator S/N: DR4174 Verification Performed?
- Isopropanol Mnf: Lifloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24
Simulator S/N: DR4177 Verification Performed?
- Neg. Control Mnf: Lifloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24
Simulator S/N: DR4-DR6267 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 230631106 Calibration Due Date: 9/19/2025

- Verify stylus is calibrated
- Non-Drinking Subject Test
- Reset Options
- Upload
- Clear Memory
- Remove Tank Prior to Shutdown
- Verification of Calibration (VOC)
- Calibration End Date: 12/1/23

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100675

Date: 11/30/2023
Time: 09:55:11

VERSIONS

DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 46.9°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 2.04 V PASSED
(1.22 V - 2.86 V)
Cooler Voltage = 1.86 V PASSED
(1.12 V - 2.60 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 539 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 28.8 in

PUMP INFO

Flow Rate = 4.629 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.096 1.08% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100675

Date: 11/30/2023
Time: 11:51 AM

Temperatures (°C)

Sample Cell: 48.9°C
Breath Tube: 47.1°C

Current Barometer 28.8 in
Volume (Ltr) 1.50

Settings

Lamp: 1.99 V
Bias: 80 V
Cooler: 1.81 V
Chopper: 540 Hz

Voltages (V)

Flow: 1.06 V
Detector: -0.010 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100675

Date: 11/07/2023
Time: 09:12:45

OPERATOR NAME:
CARLIE GLAISTER
CERTIFICATE #: 10436

Ca = 0.1000
CAL = 0.987644 0.800 <= CAL < 1.200
b1 = 0.0013 0.0000 <= b1 < 0.0040
b2 = 0.0068 0.0010 <= b2 < 0.0100
b3 = 0.0012 0.0000 <= b3 < 0.0040
Xq = 0.0970 0.0500 <= Xq < 0.2000
a21 = 1.179594 1.050 <= a21 < 1.300
a31 = 0.439578 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100675

Date: 11/30/2023
Time: 11:53:07

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.84: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	11:54
BLANK TEST	0.000	11:54
INTERNAL STANDARD	VERIFIED	11:54
EXTERNAL STANDARD	0.076	11:55
BLANK TEST	0.000	11:55
SUBJECT SAMPLE (Vol=1.53L)	0.000	11:56
BLANK TEST	0.000	11:57
EXTERNAL STANDARD	0.075	11:57
BLANK TEST	0.000	11:58

OKS

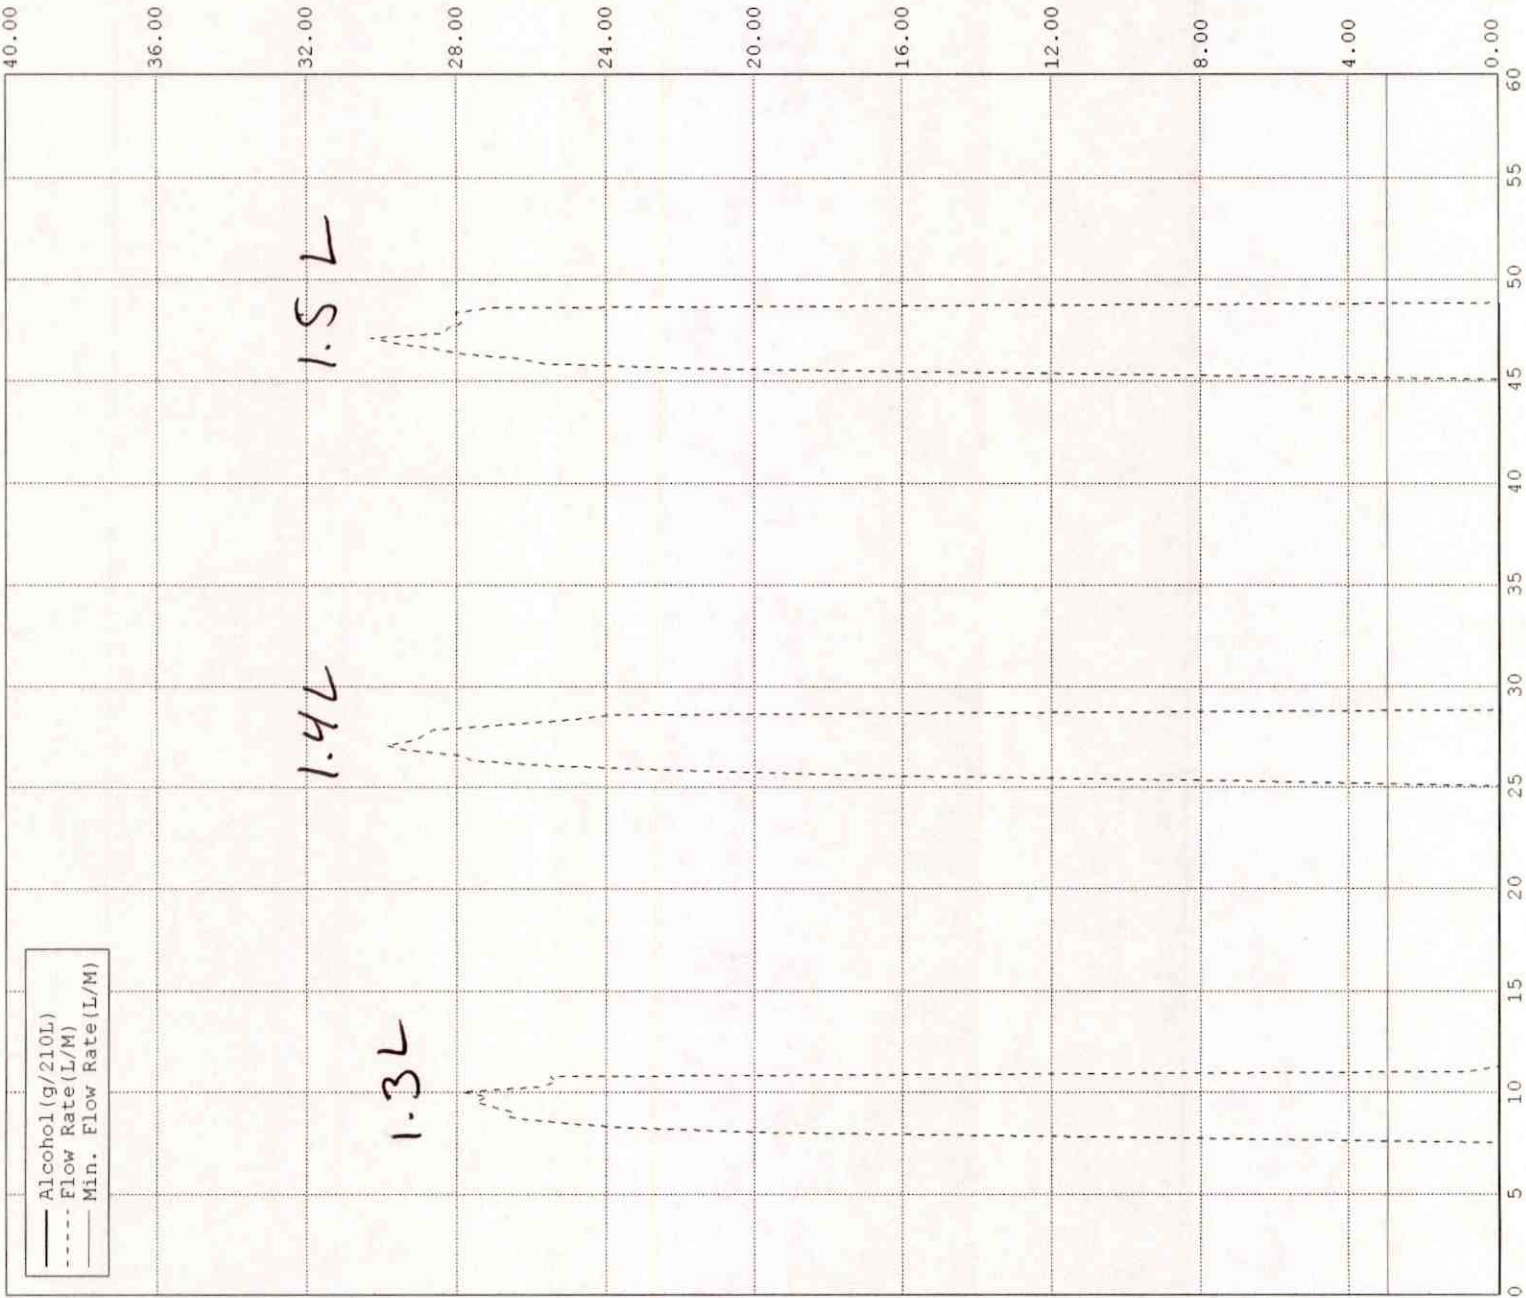

LINEARITY CHECK

 Alaska Department of Public Safety
 DATAMASTER dmt: 100675


Date: 11/30/2023
 Time: 12:21:03

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.019	0.0190	0.0000
0.039	0.0382	0.0004
0.077	0.0756	0.0005
0.096	0.0960	0.0000
0.145	0.1440	0.0000
0.289	0.2902	0.0004

SLOPE = 1.005943
 R^2 = 0.999945

100675 2023.12.01 Calibration

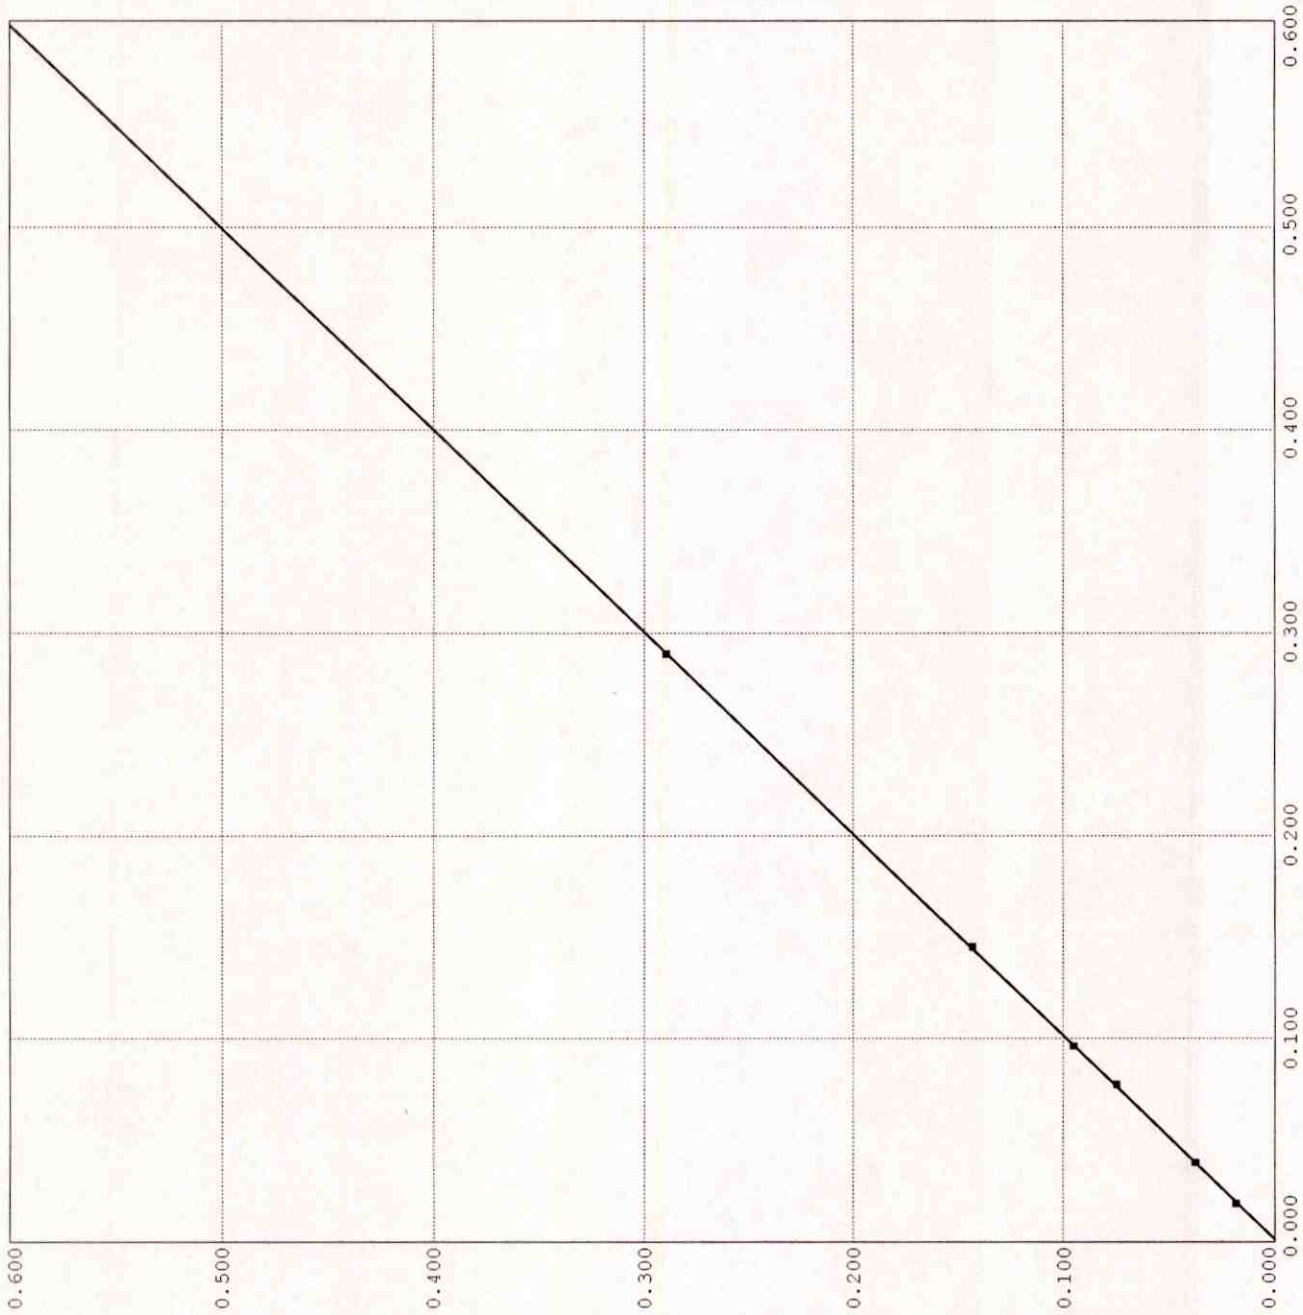

CY 6

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100675






Date: 11/30/2023
 Time: 12:21:05

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 28.85: 0.019
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 707 psi

BLANK TEST	0.000	12:22
INTERNAL STANDARD	VERIFIED	12:22
EXTERNAL STANDARD	0.019	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.019	12:23
BLANK TEST	0.000	12:24
EXTERNAL STANDARD	0.019	12:25
BLANK TEST	0.000	12:25
EXTERNAL STANDARD	0.019	12:26
BLANK TEST	0.000	12:27
EXTERNAL STANDARD	0.019	12:27
BLANK TEST	0.000	12:28

Average = 0.0190
 Std Dev = 0.0000

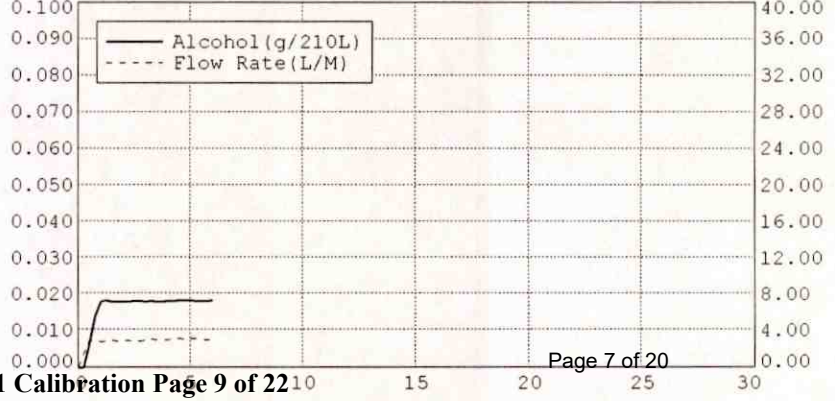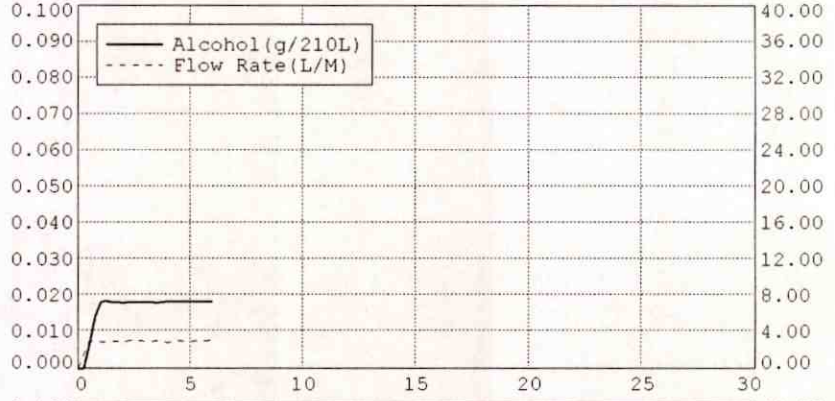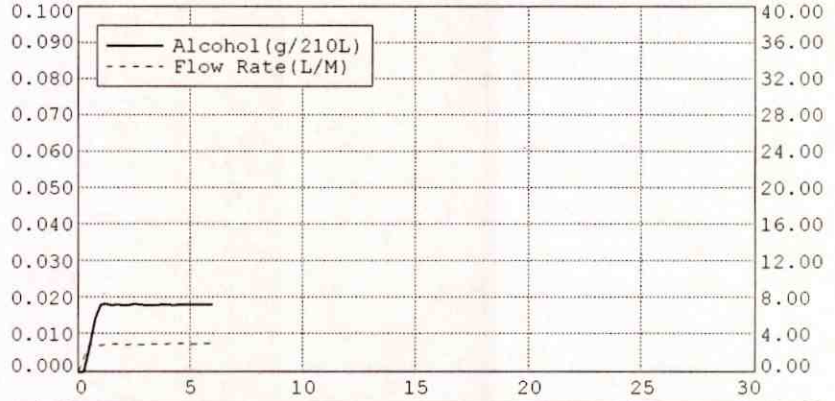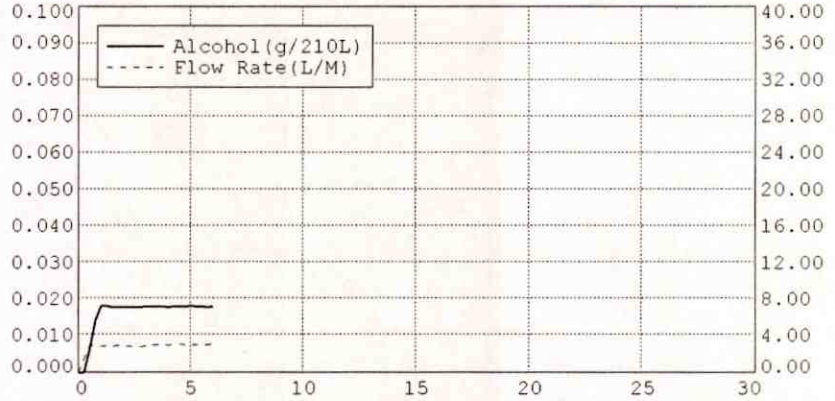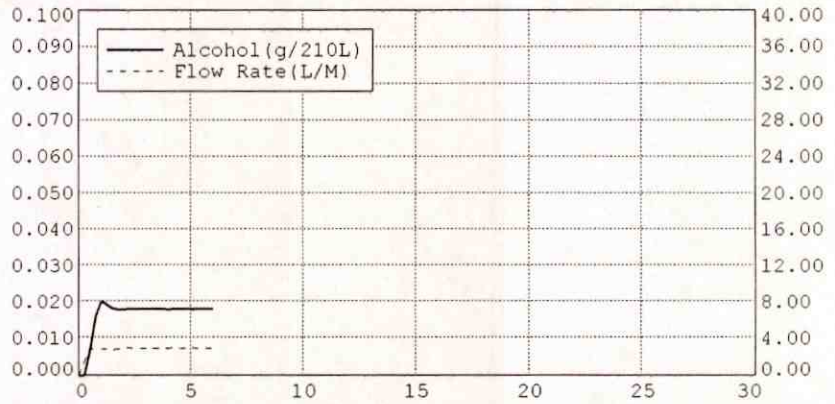

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100675






Date: 11/30/2023
 Time: 12:41:46

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 28.84: 0.039
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 775 psi

BLANK TEST	0.000	12:43
INTERNAL STANDARD	VERIFIED	12:43
EXTERNAL STANDARD	0.038	12:43
BLANK TEST	0.000	12:44
EXTERNAL STANDARD	0.038	12:44
BLANK TEST	0.000	12:45
EXTERNAL STANDARD	0.038	12:45
BLANK TEST	0.000	12:46
EXTERNAL STANDARD	0.038	12:46
BLANK TEST	0.000	12:47
EXTERNAL STANDARD	0.039	12:47
BLANK TEST	0.000	12:48

Average = 0.0382
 Std Dev = 0.0004

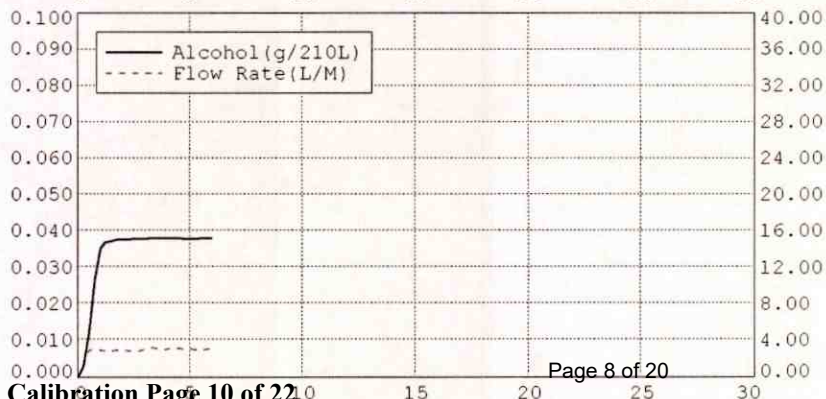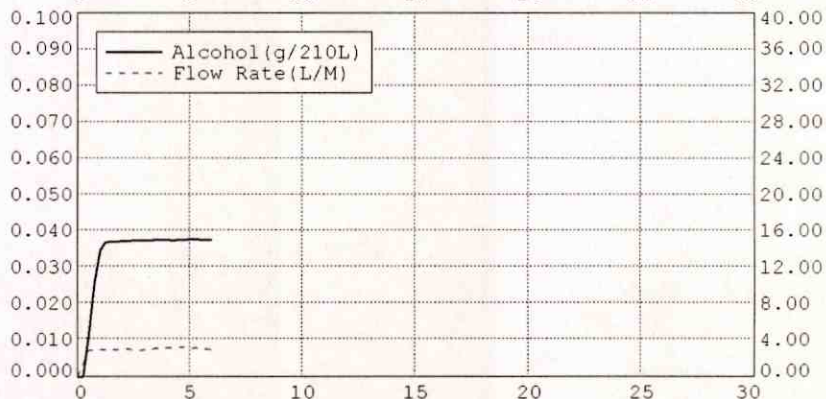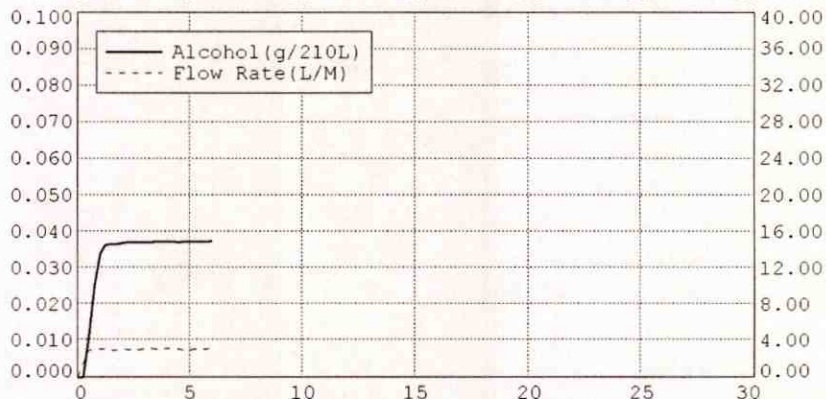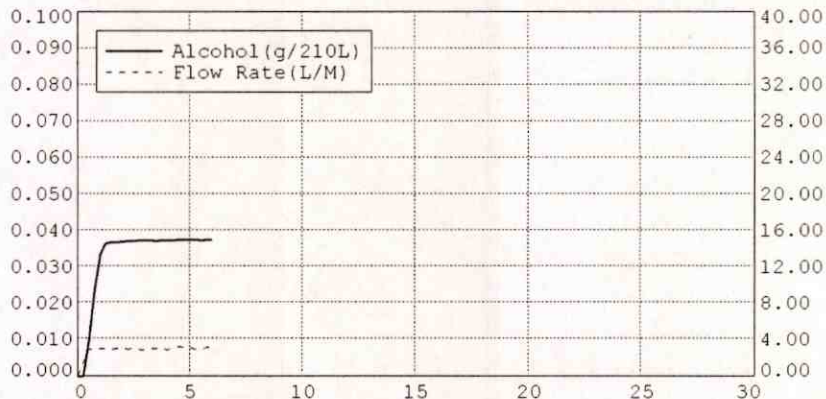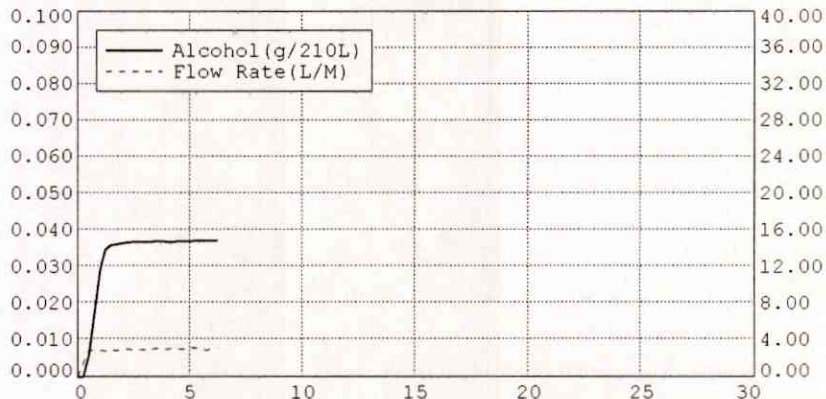

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100675






Date: 11/30/2023
 Time: 14:31:33

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 28.85: 0.077
 LOT #: AG310901
 EXPIRATION: 04/19/2025
 TANK PRESSURE: 760 psi

BLANK TEST	0.000	14:33
INTERNAL STANDARD	VERIFIED	14:33
EXTERNAL STANDARD	0.075	14:33
BLANK TEST	0.000	14:34
EXTERNAL STANDARD	0.075	14:34
BLANK TEST	0.000	14:35
EXTERNAL STANDARD	0.076	14:35
BLANK TEST	0.000	14:36
EXTERNAL STANDARD	0.076	14:36
BLANK TEST	0.000	14:37
EXTERNAL STANDARD	0.076	14:37
BLANK TEST	0.000	14:38

Average = 0.0756
 Std Dev = 0.0005

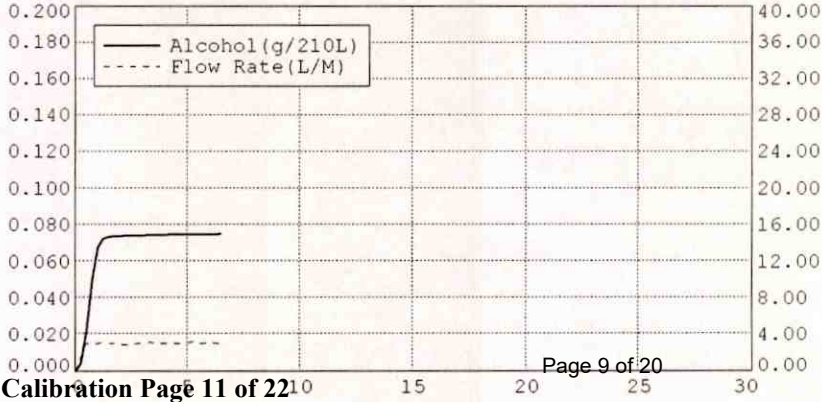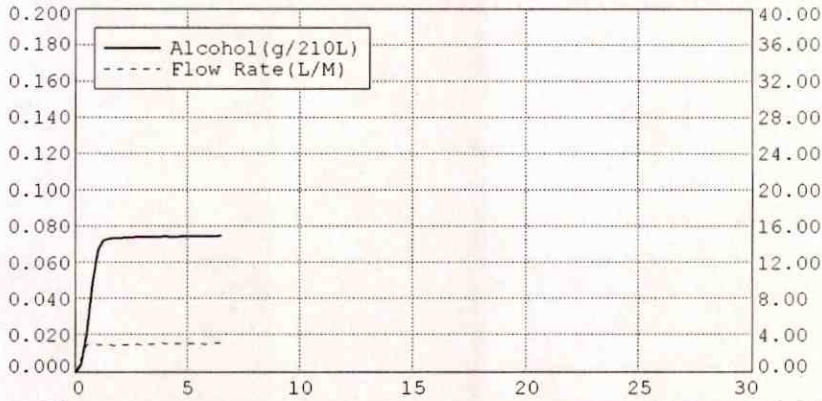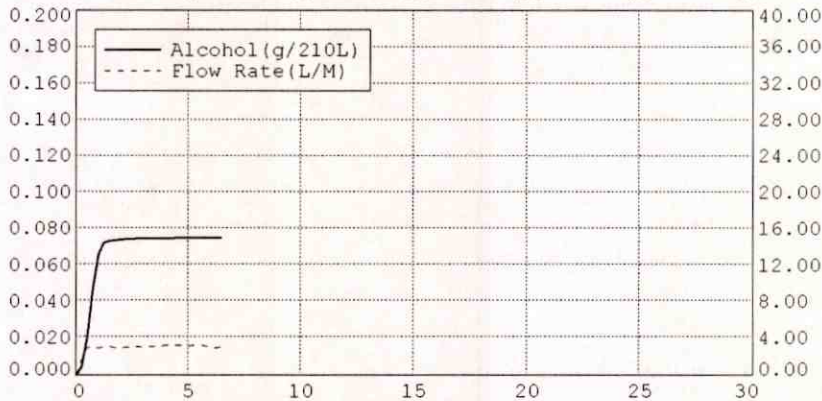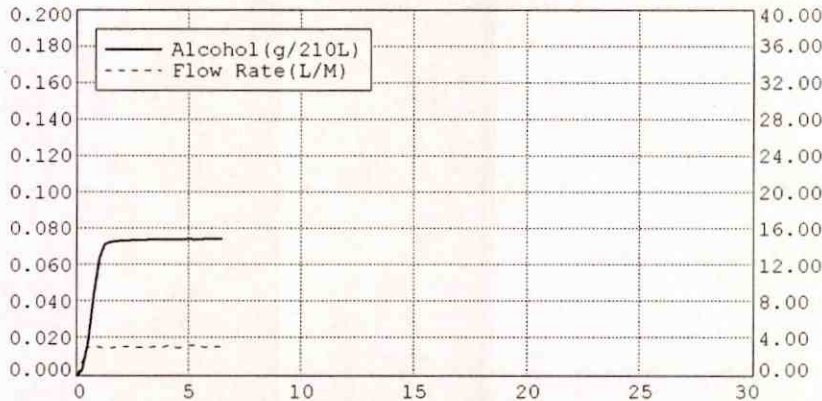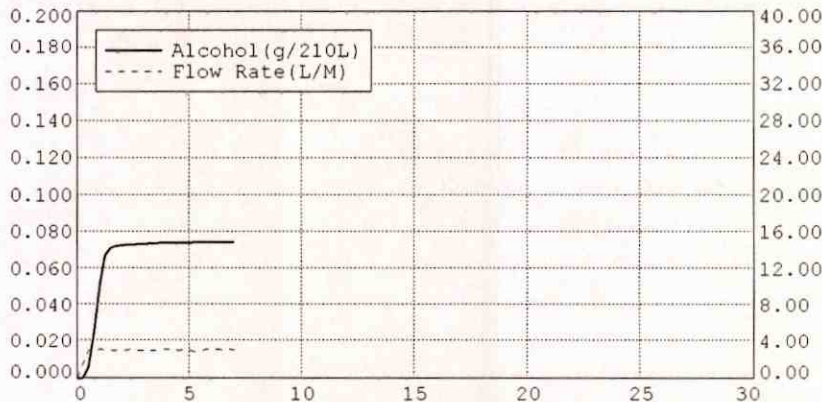

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100675






Date: 11/30/2023
 Time: 14:46:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 28.85: 0.096
 LOT #: AG211003
 EXPIRATION: 04/20/2024
 TANK PRESSURE: 988 psi

BLANK TEST	0.000	14:48
INTERNAL STANDARD	VERIFIED	14:48
EXTERNAL STANDARD	0.096	14:48
BLANK TEST	0.000	14:49
EXTERNAL STANDARD	0.096	14:49
BLANK TEST	0.000	14:50
EXTERNAL STANDARD	0.096	14:50
BLANK TEST	0.000	14:51
EXTERNAL STANDARD	0.096	14:52
BLANK TEST	0.000	14:52
EXTERNAL STANDARD	0.096	14:53
BLANK TEST	0.000	14:54

Average = 0.0960
 Std Dev = 0.0000

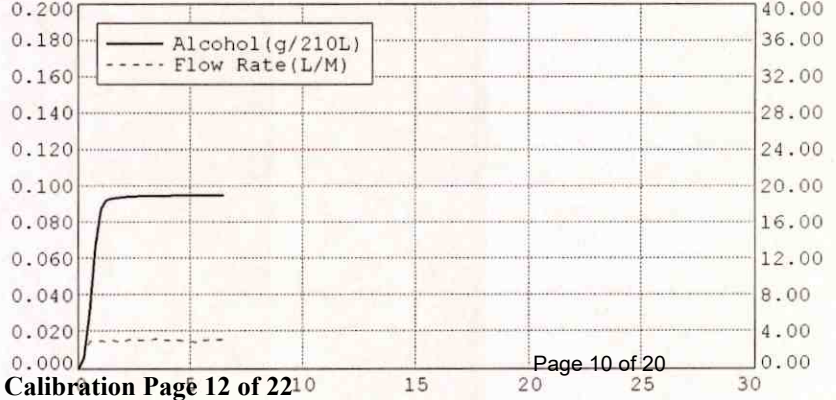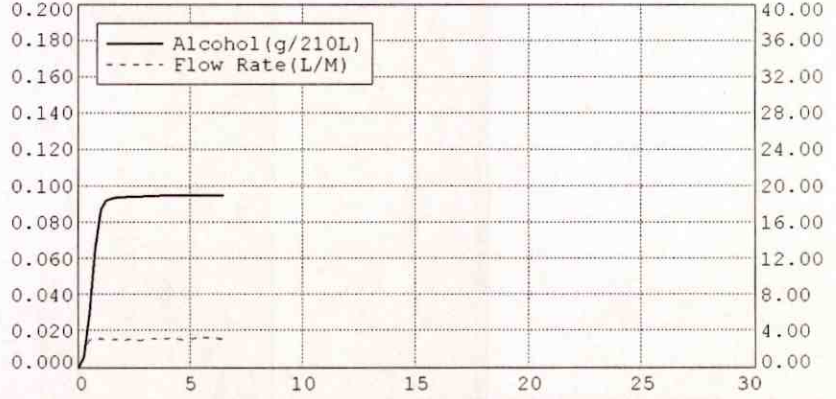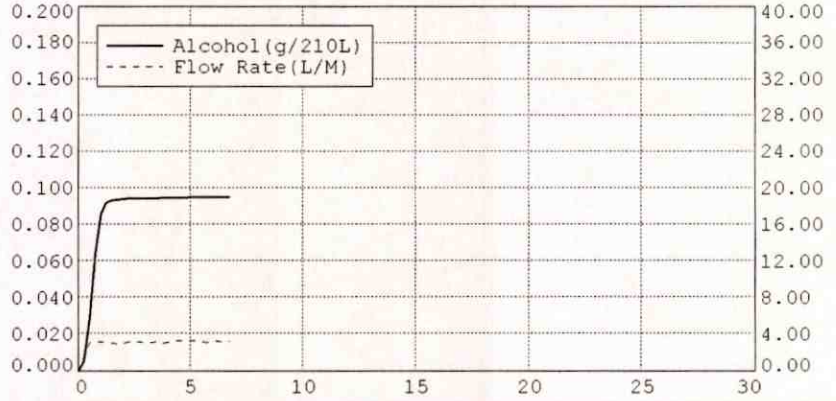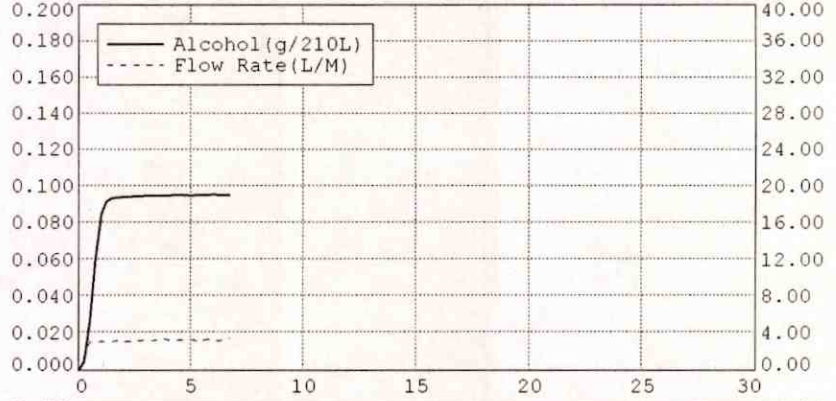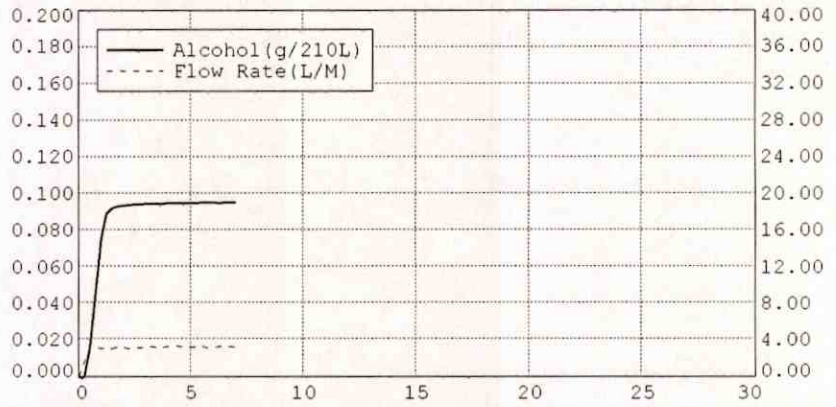

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100675






Date: 11/30/2023
 Time: 14:55:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 28.85: 0.145
 LOT #: AG134205
 EXPIRATION: 12/08/2023
 TANK PRESSURE: 750 psi

BLANK TEST	0.000	14:58
INTERNAL STANDARD	VERIFIED	14:58
EXTERNAL STANDARD	0.144	14:58
BLANK TEST	0.000	14:59
EXTERNAL STANDARD	0.144	14:59
BLANK TEST	0.000	15:00
EXTERNAL STANDARD	0.144	15:00
BLANK TEST	0.000	15:01
EXTERNAL STANDARD	0.144	15:01
BLANK TEST	0.000	15:02
EXTERNAL STANDARD	0.144	15:02
BLANK TEST	0.000	15:03

Average = 0.1440
 Std Dev = 0.0000

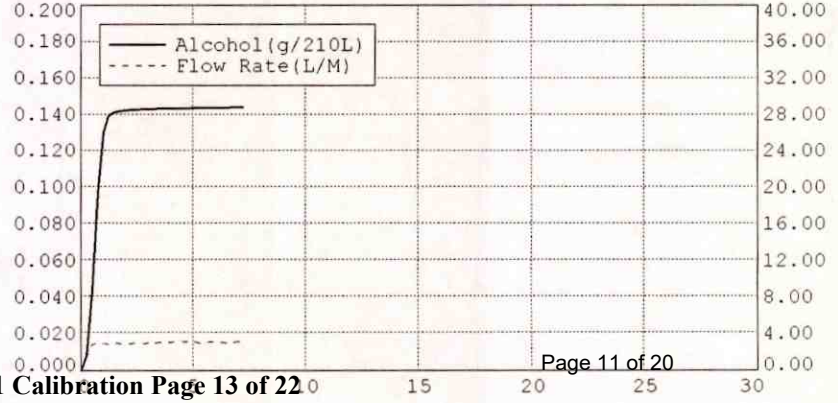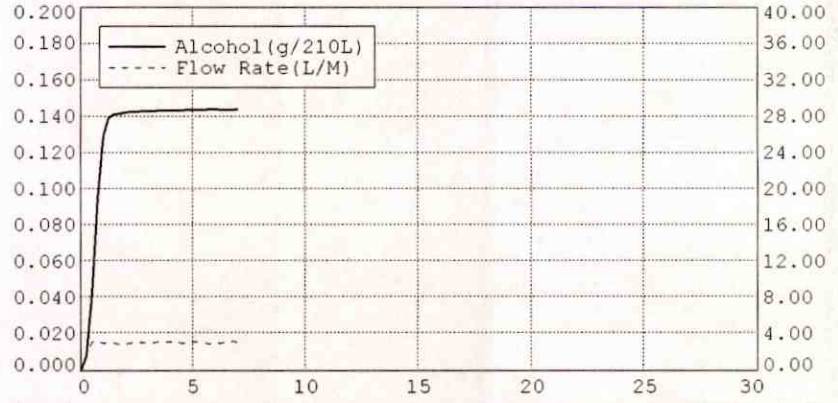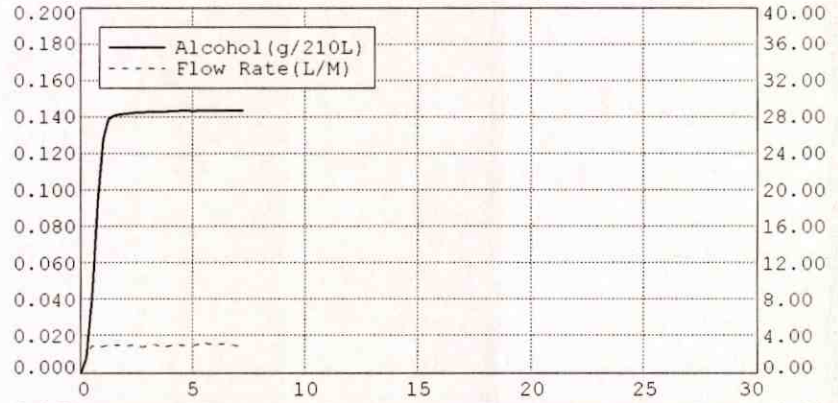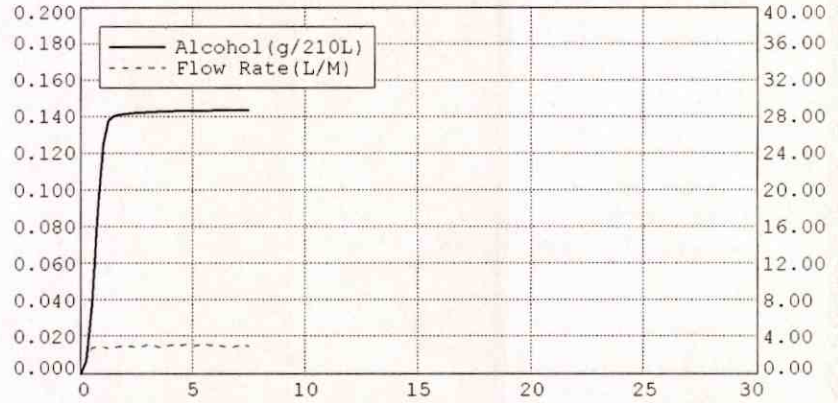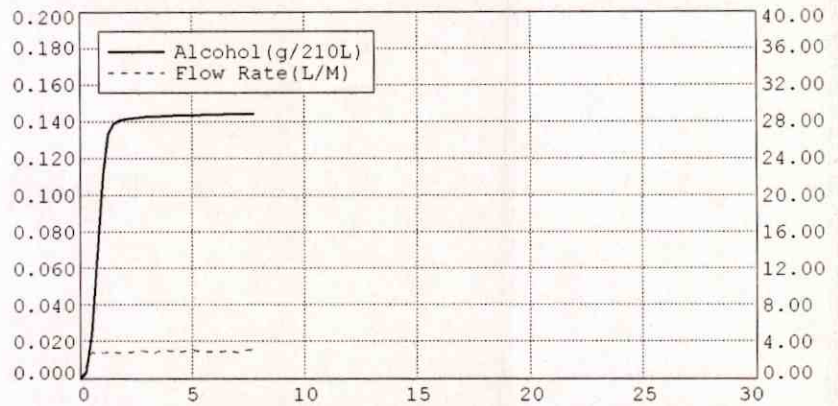

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100675






Date: 11/30/2023
Time: 15:11:11


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 28.85: 0.289
LOT #: AG217903
EXPIRATION: 06/28/2024
TANK PRESSURE: 134 psi

BLANK TEST	0.000	15:12
INTERNAL STANDARD	VERIFIED	15:12
EXTERNAL STANDARD	0.290	15:13
BLANK TEST	0.000	15:14
EXTERNAL STANDARD	0.290	15:14
BLANK TEST	0.000	15:15
EXTERNAL STANDARD	0.290	15:15
BLANK TEST	0.000	15:16
EXTERNAL STANDARD	0.291	15:16
BLANK TEST	0.000	15:17
EXTERNAL STANDARD	0.290	15:17
BLANK TEST	0.000	15:18

Average = 0.2902
Std Dev = 0.0004

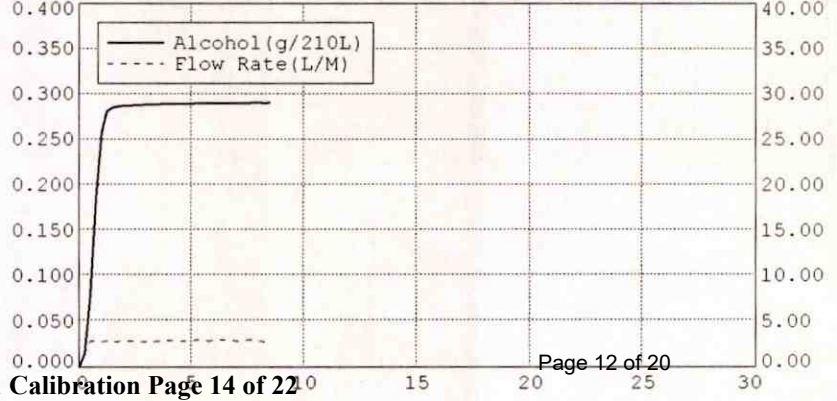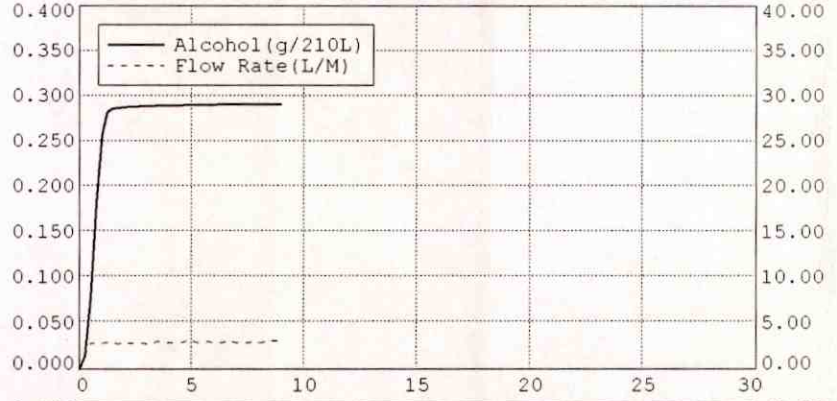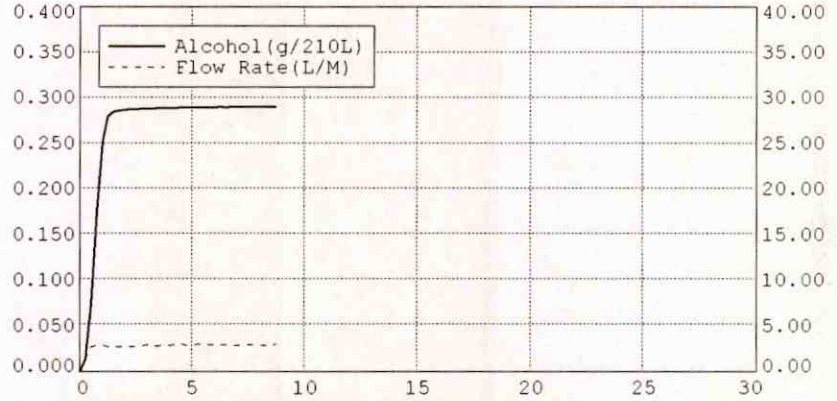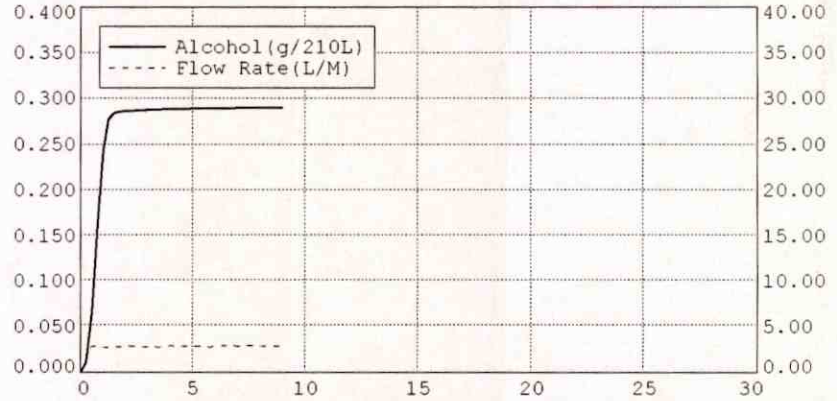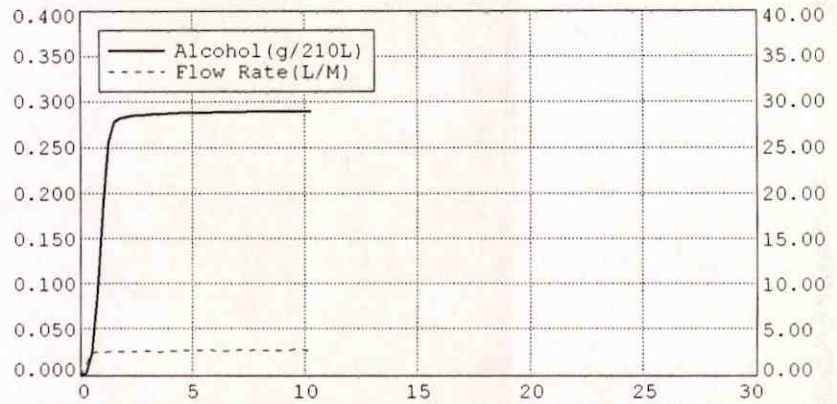

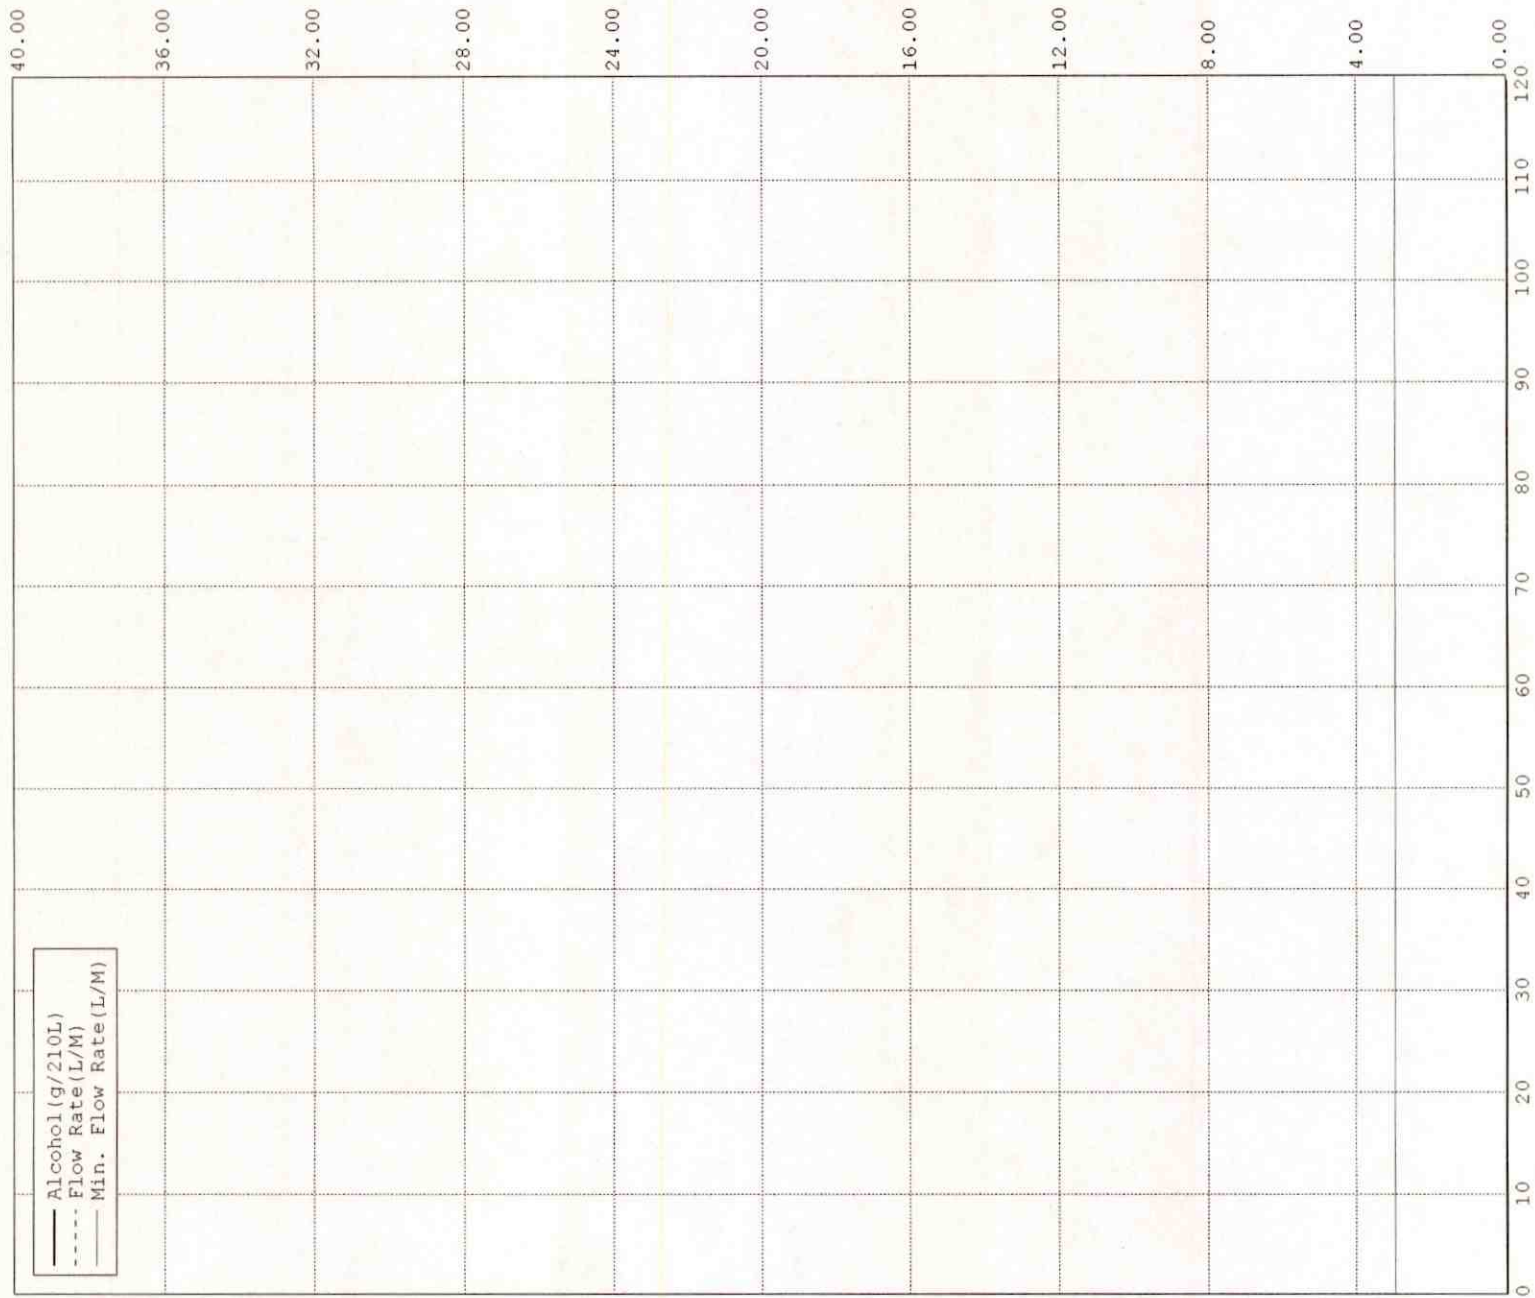

SUBJECT TEST

 Alaska Department of Public Safety
 DATAMASTER dmt: 100675

 Date: 11/30/2023
 Time: 15:28:20

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX

OPERATOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

DEPT/AGENCY:
 INCOMPLETE

CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 28.87: 0.077
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 15:29
 BLANK TEST 0.000 15:29
 INTERNAL STANDARD VERIFIED 15:29
 EXTERNAL STANDARD 0.076 15:30
 BLANK TEST 0.000 15:30
 SUBJECT SAMPLE INCOMPLETE 15:33

AKG

100675 2023.12.01 Calibration Page 15 of 22

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100675

Date: 12/01/2023
 Time: 08:59:29

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX


OPERATOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

DEPT/AGENCY:
 MAXIMUM ATTEMPTS EXCEEDED
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 28.98: 0.077
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 09:01
 BLANK TEST 0.000 09:01
 INTERNAL STANDARD VERIFIED 09:01
 EXTERNAL STANDARD 0.076 09:02
 BLANK TEST 0.000 09:03
 SUBJECT SAMPLE XXX 09:03

Maximum Attempts Exceeded

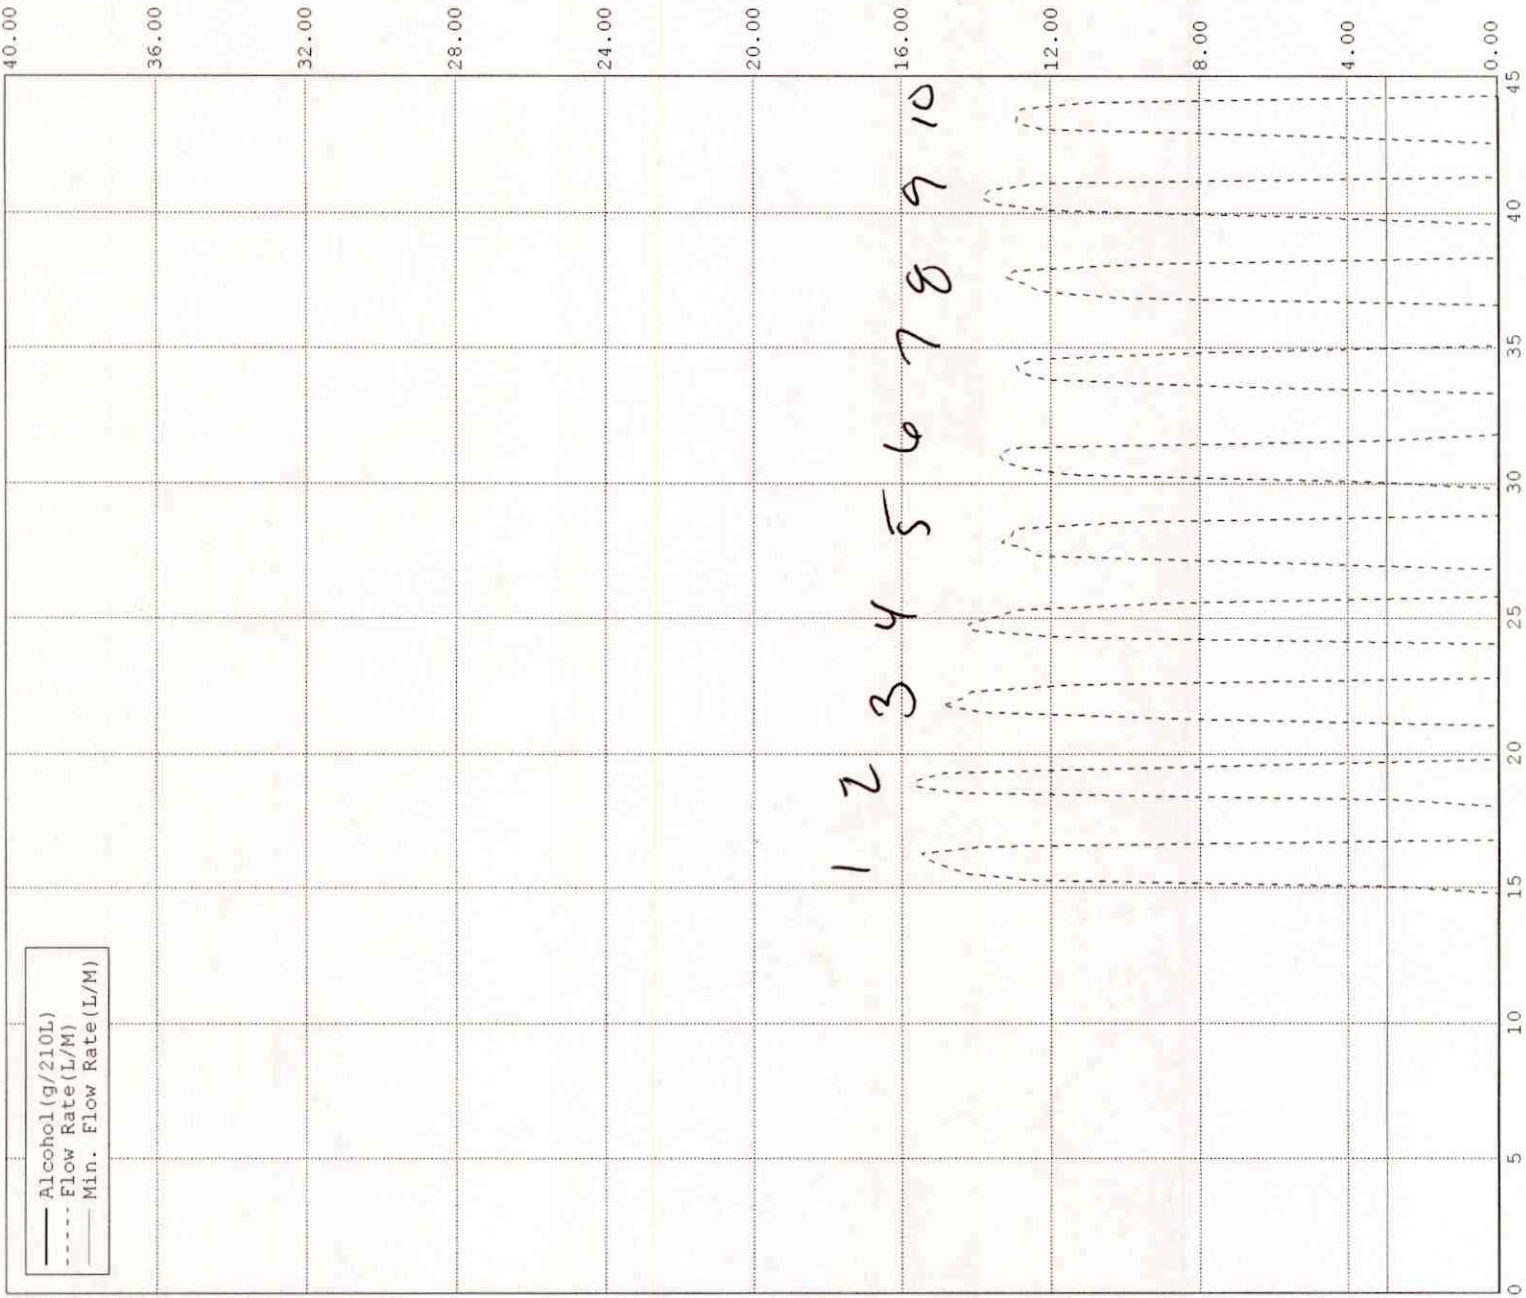

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100675

Date: 12/01/2023
Time: 09:11:40

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INVALID

CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.97: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 09:16
BLANK TEST 0.000 09:16
INTERNAL STANDARD VERIFIED 09:16
EXTERNAL STANDARD 0.076 09:17
BLANK TEST 0.000 09:17
SUBJECT SAMPLE INVALID 09:18

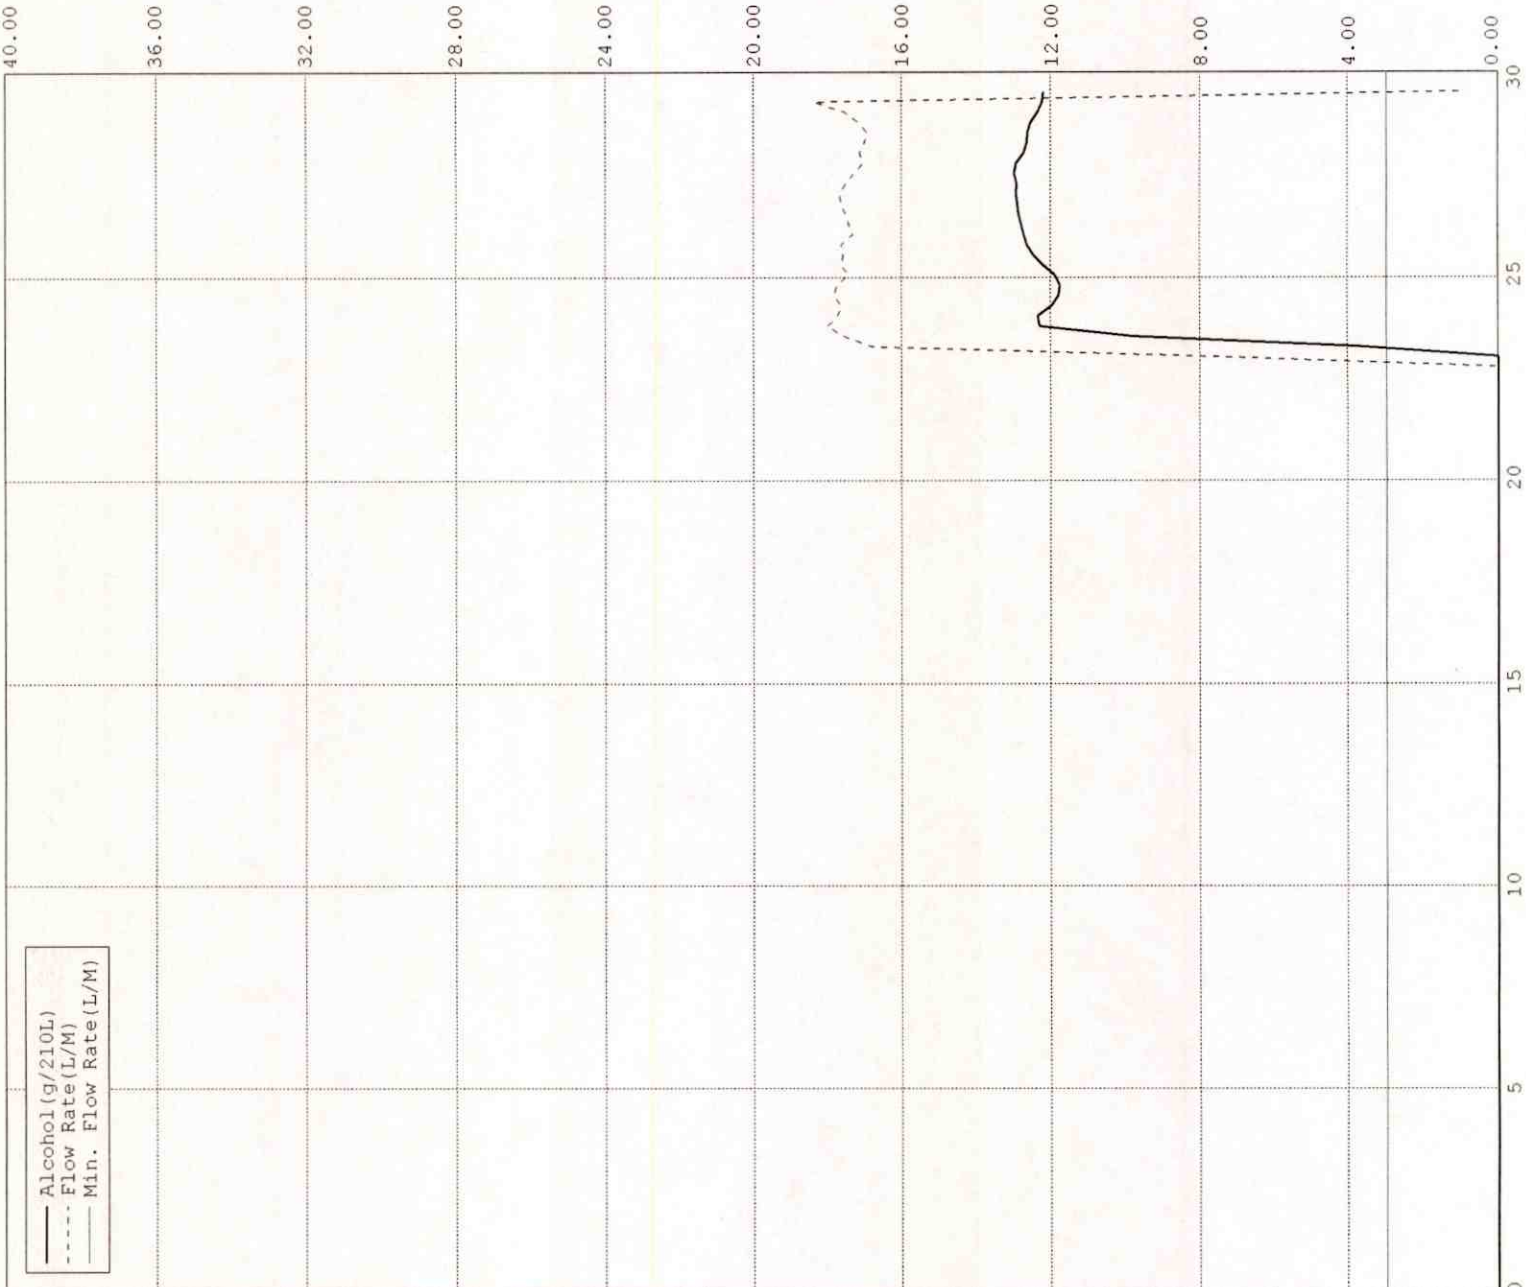

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100675

Date: 12/01/2023
Time: 09:28:06

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
RFI
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.98: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 09:30
BLANK TEST 0.000 09:30
INTERNAL STANDARD VERIFIED 09:30
EXTERNAL STANDARD 0.076 09:30
BLANK TEST 0.000 09:31

RFI DETECTED

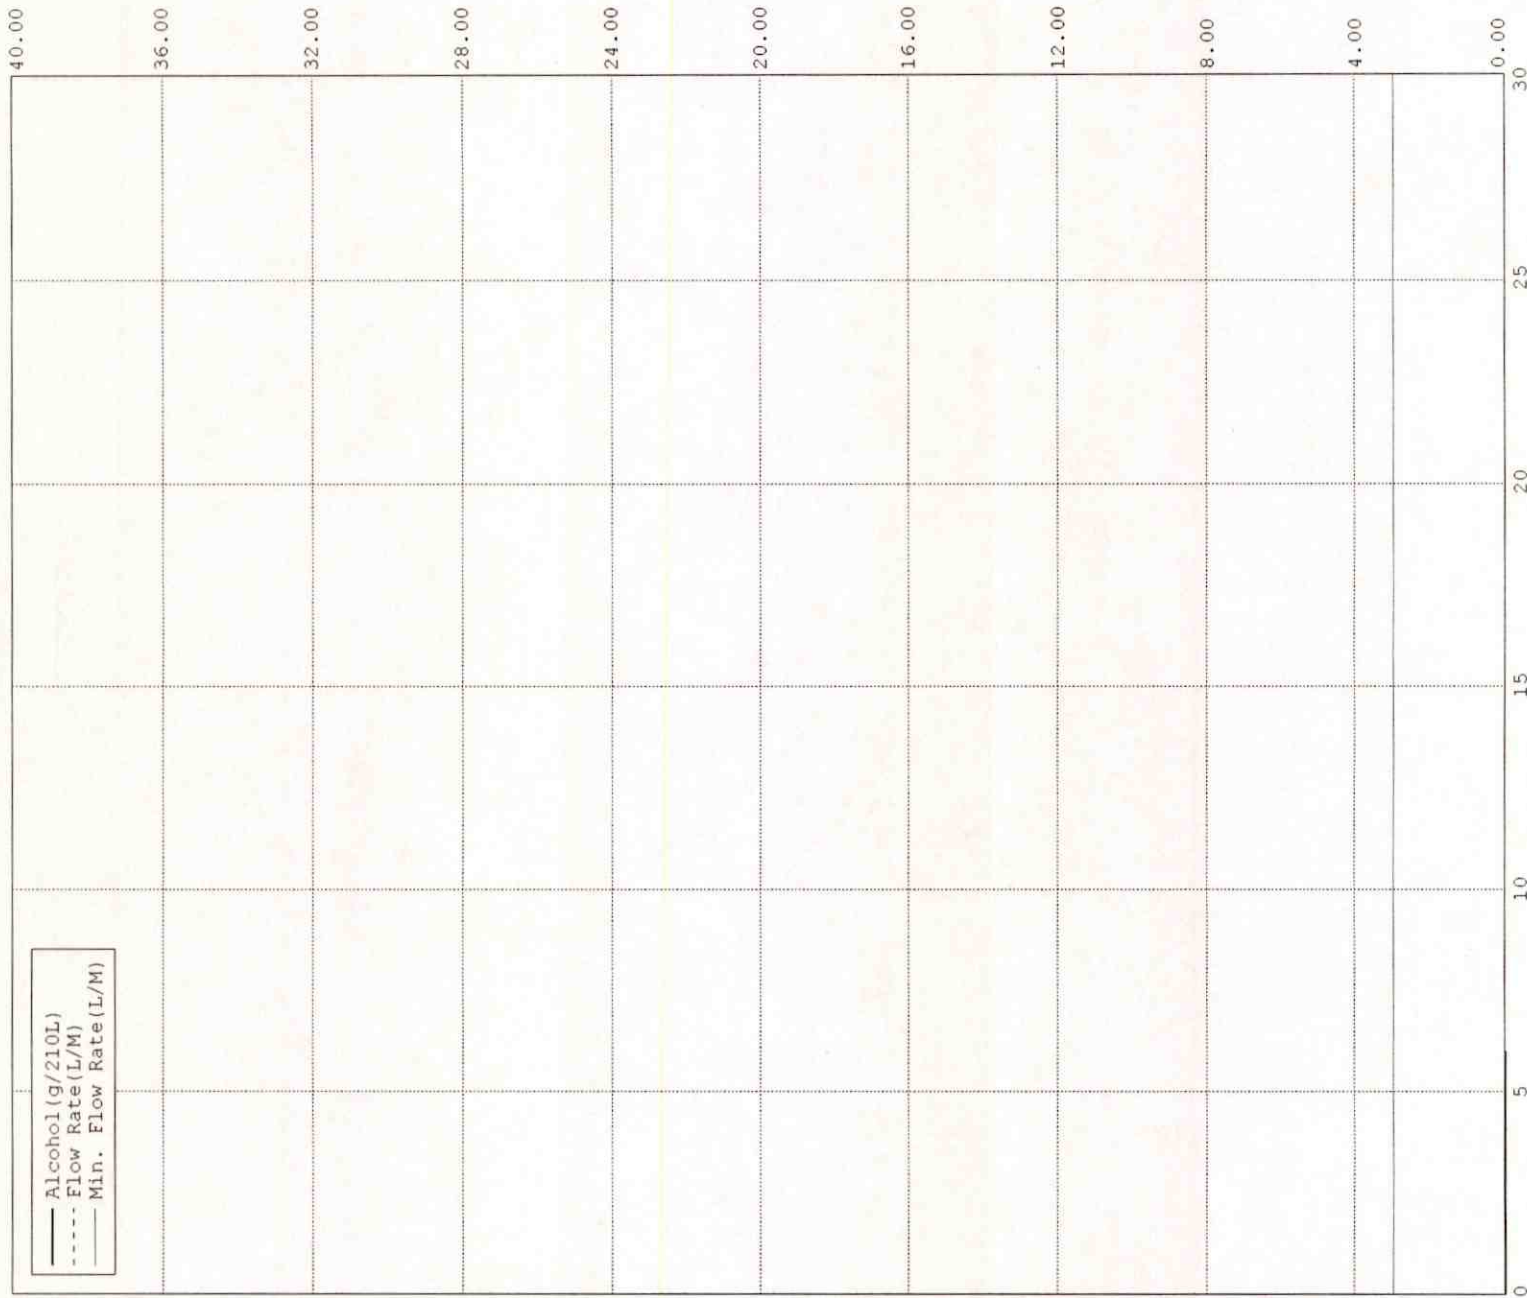

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100675

Date: 12/01/2023
Time: 10:48:03

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE ACETONE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080
TARGET AT 28.98: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 10:50
BLANK TEST 0.000 10:50
INTERNAL STANDARD VERIFIED 10:50
Xg = 0.096 (0.54%)
EXTERNAL STANDARD 0.076 10:50
X[1] = 0.0761 (-0.0006) (0.0018)
BLANK TEST 0.000 10:51
SUBJECT SAMPLE XXX 10:52
X[1] = 0.1101 (-0.0169) (0.0025)

Interference Detected

Filter 2 Average: -0.0009

Filter 3 Average: 0.0018

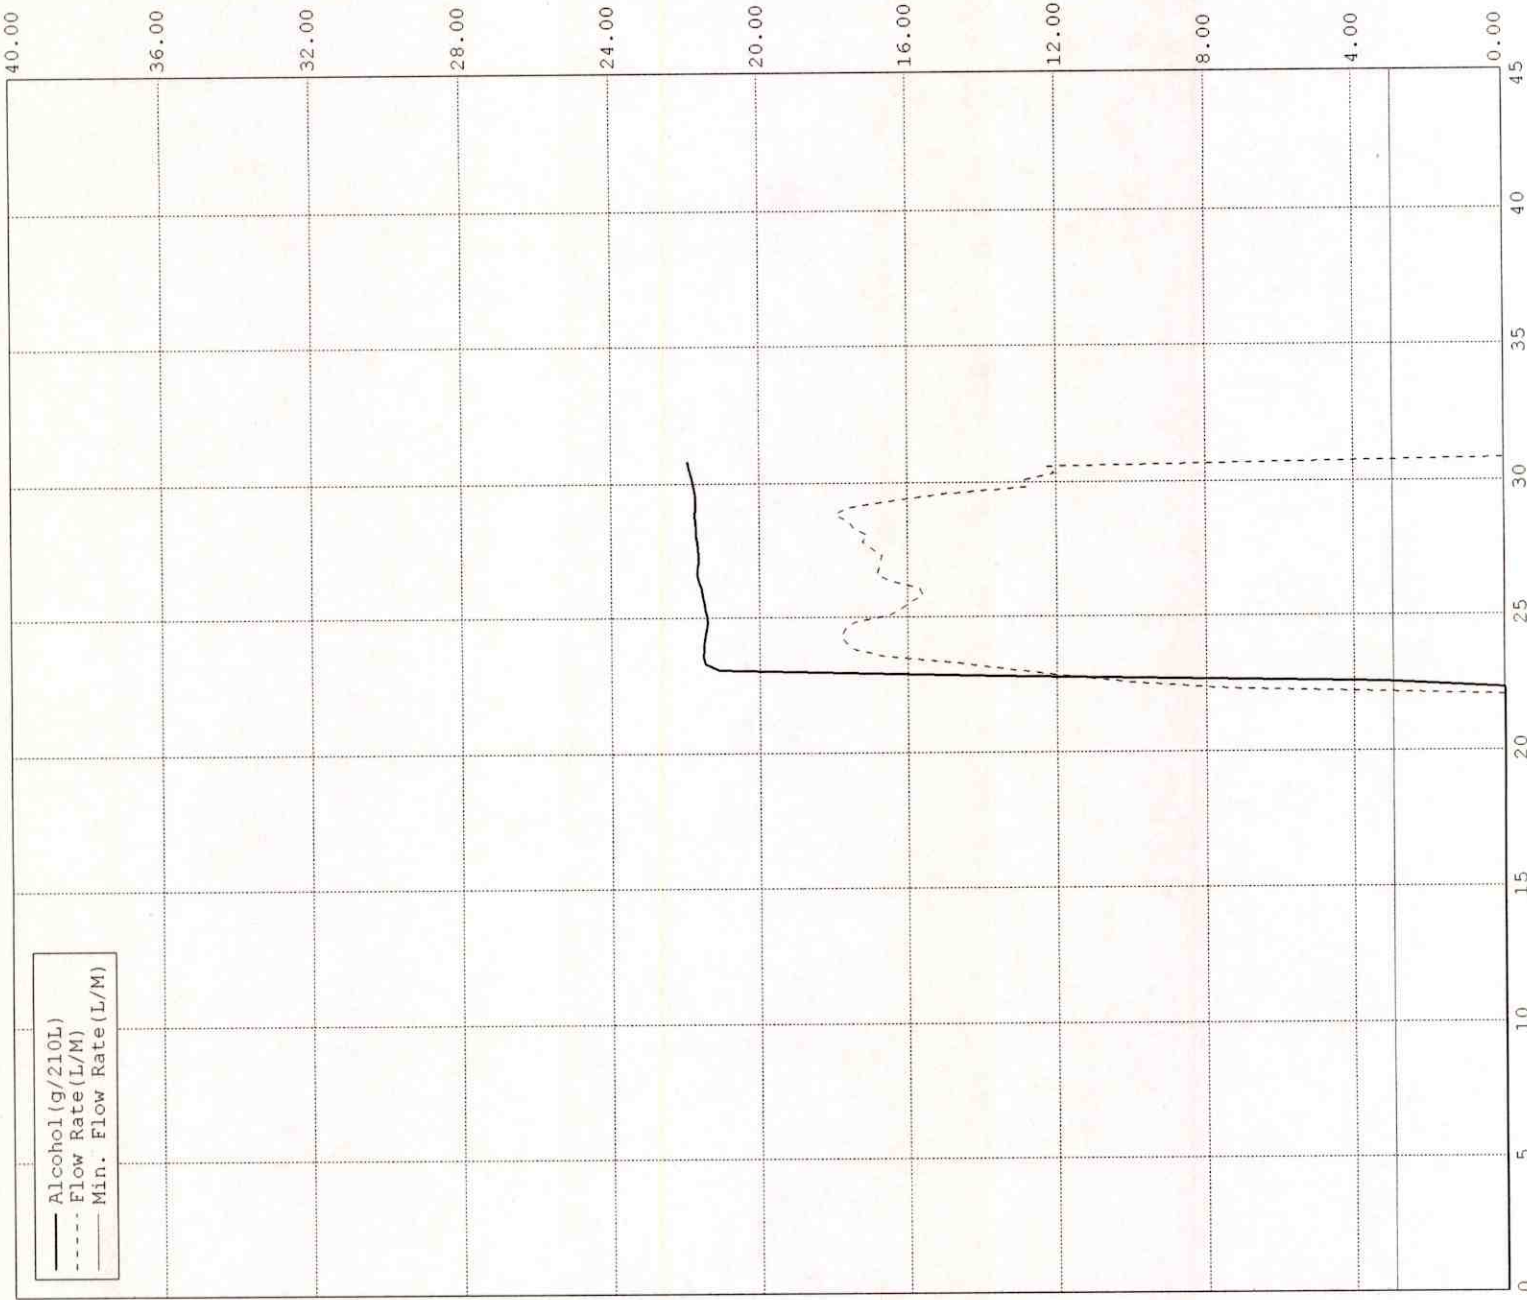

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100675

Date: 12/01/2023
Time: 10:40:34

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INTERFERENCE IPA
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.98: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 10:43
BLANK TEST 0.000 10:44
INTERNAL STANDARD VERIFIED 10:44
Xg = 0.097 (0.36%)
EXTERNAL STANDARD 0.076 10:44
X[1] = 0.0760 (-0.0010) (0.0019)
BLANK TEST 0.000 10:45
SUBJECT SAMPLE XXX 10:45
X[1] = 0.1176 (-0.0342) (0.0013)

Interference Detected

CVG

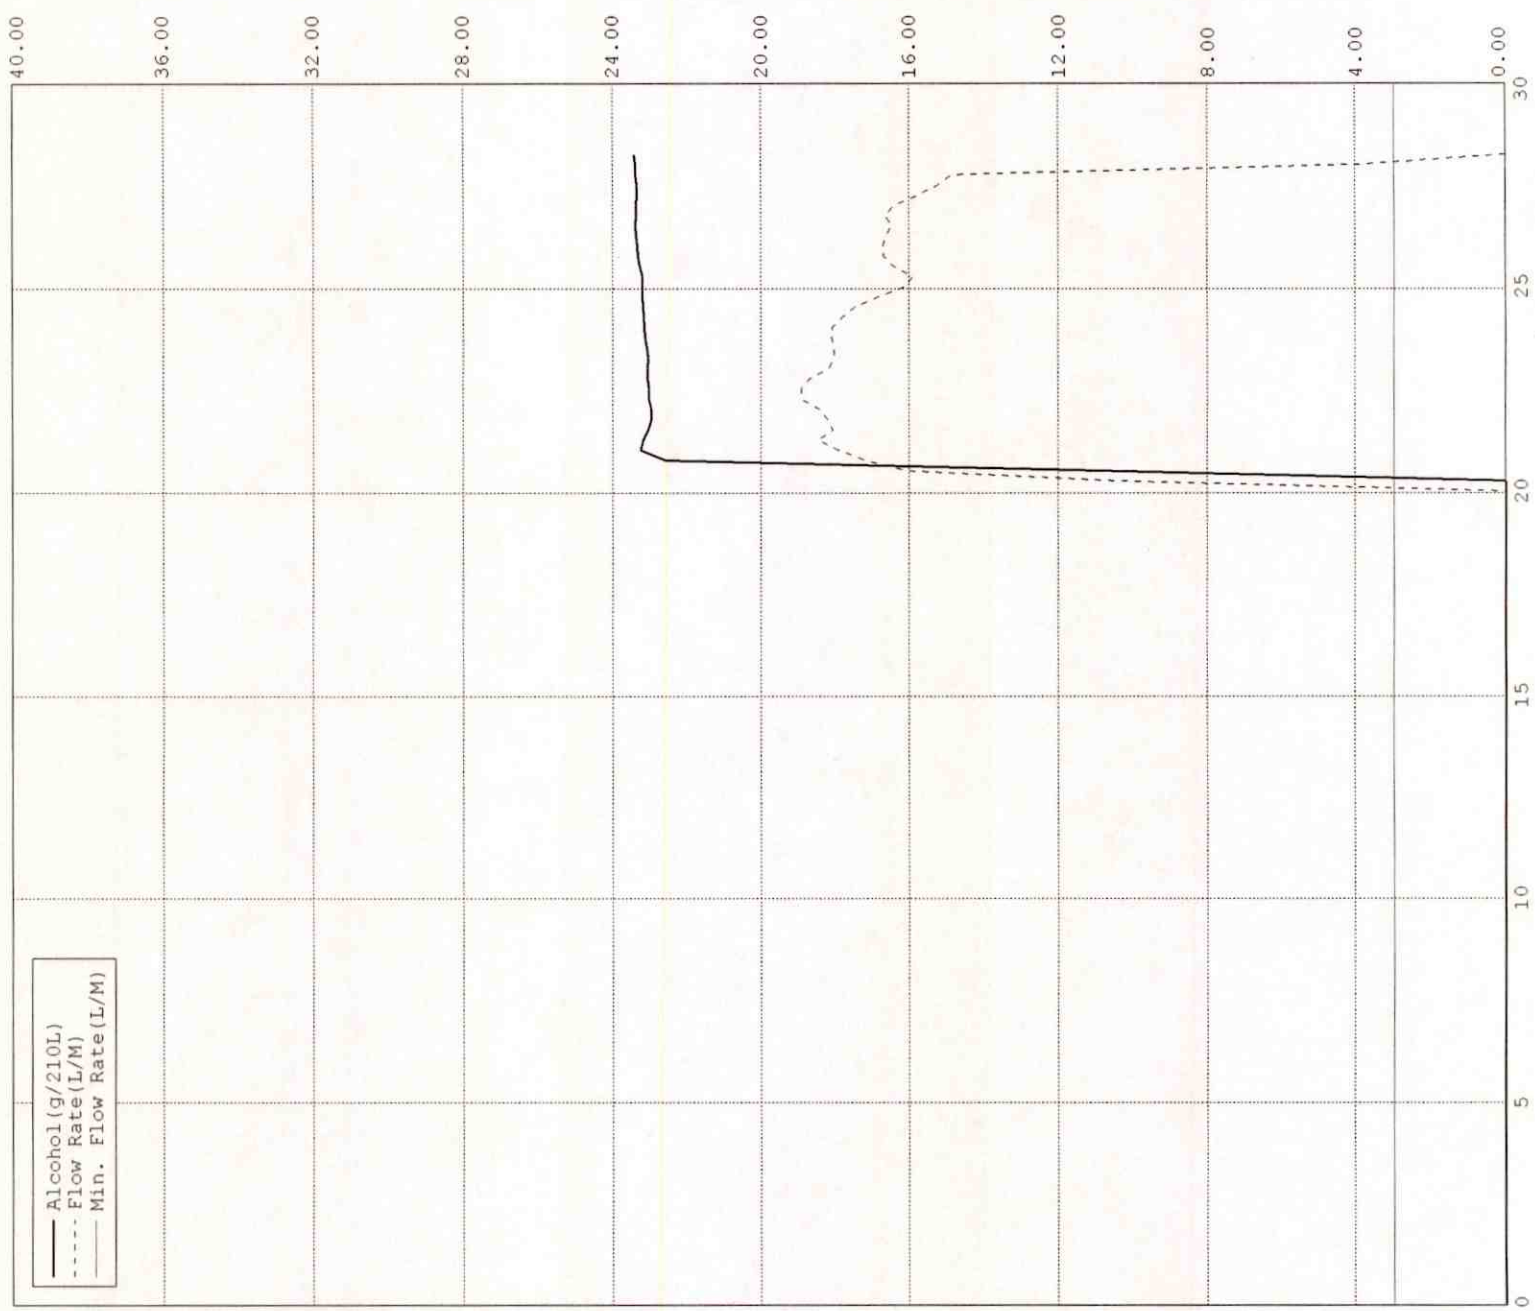

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100675

Date: 12/01/2023

Time: 10:29:26

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INTERFERENCE NEGATIVE

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 28.98: 0.077

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

BLANK TEST 10:30 PASSED 10:30

INTERNAL STANDARD 10:30 VERIFIED 10:30

Xq = 0.096 (0.99%) 0.076 10:31

X[1] = 0.0755 (-0.0009) (0.0025) 0.000 10:31

BLANK TEST 10:32 0.000 10:32

SUBJECT SAMPLE (Vol=2.23L) 0.089 10:32

X[1] = 0.0891 (-0.0015) (0.0000) 0.000 10:33


BLANK TEST 10:34 0.075 10:34

EXTERNAL STANDARD 0.075 10:34

X[1] = 0.0753 (-0.0010) (0.0010) 0.000 10:35

BLANK TEST 10:35 0.000 10:35

OK

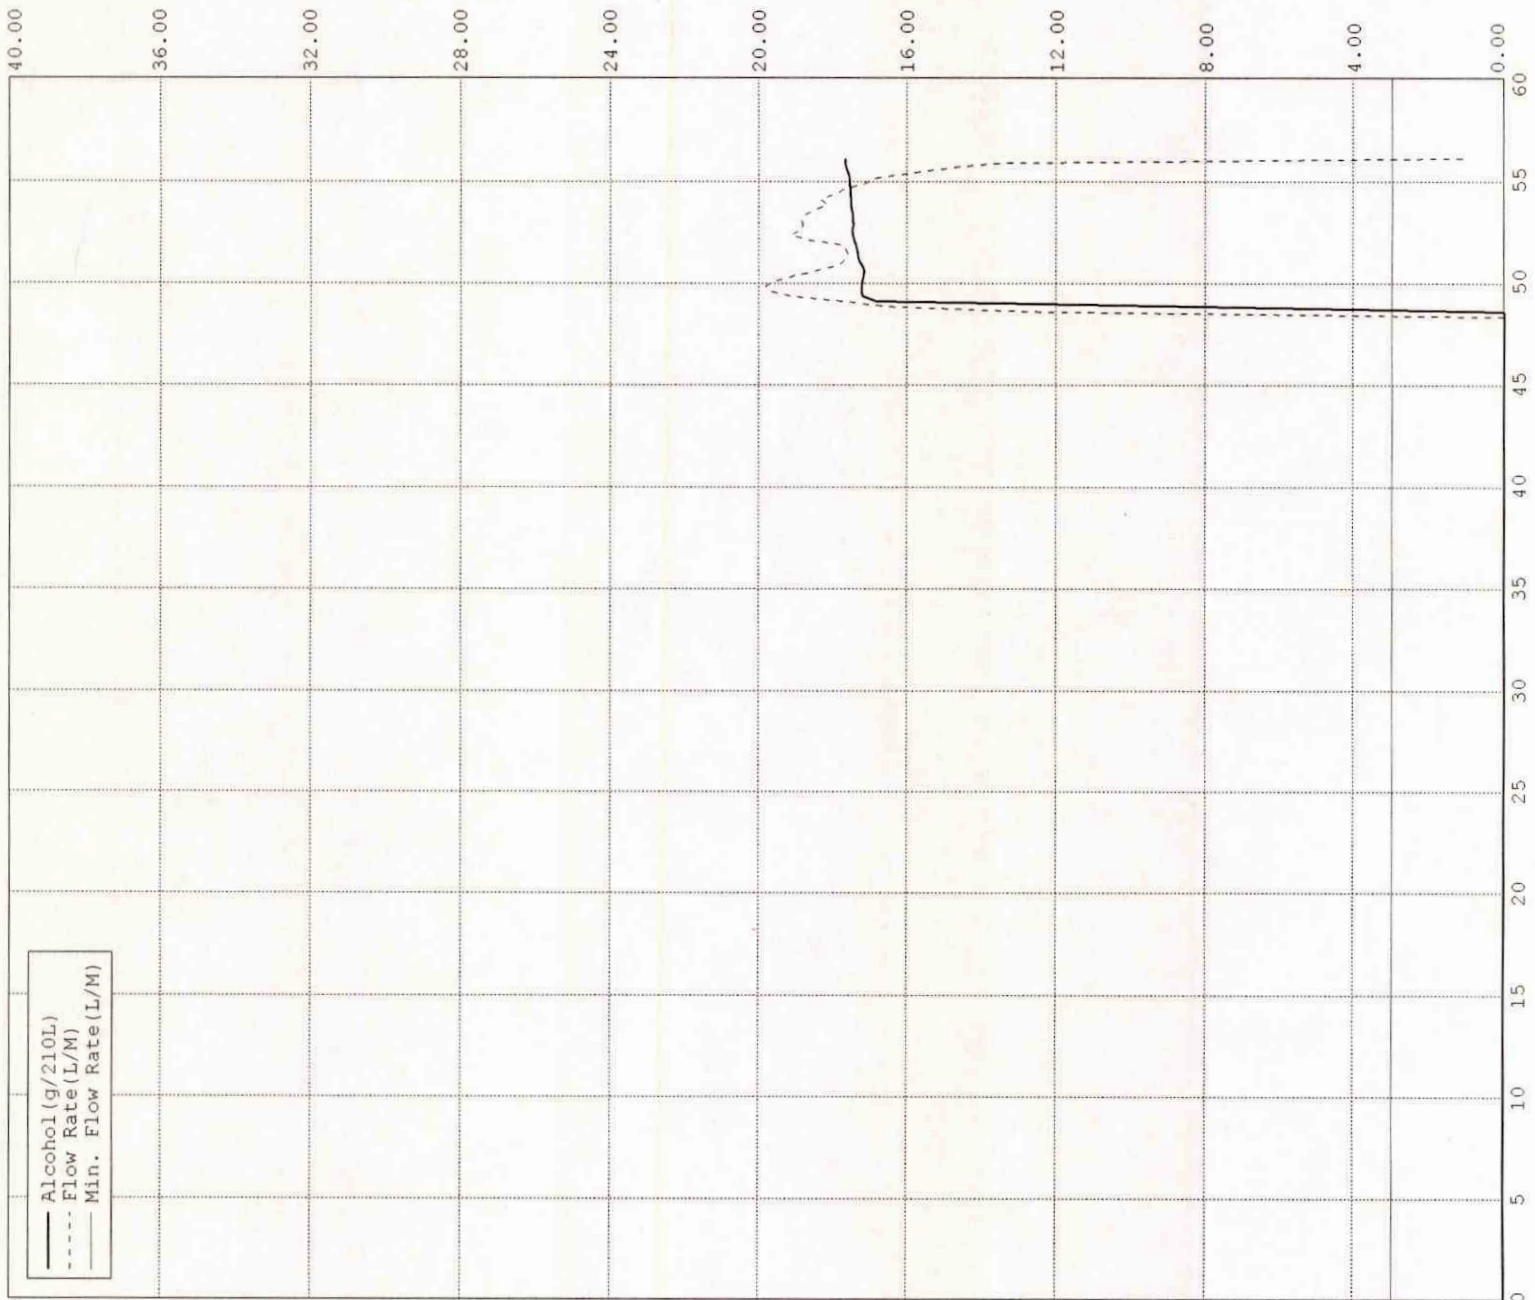

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100675

Date: 12/01/2023
Time: 11:12:42

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.98: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	11:13
BLANK TEST	0.000	11:13
INTERNAL STANDARD	VERIFIED	11:13
EXTERNAL STANDARD	0.075	11:14
BLANK TEST	0.000	11:15
SUBJECT SAMPLE (Vol=1.71L)	0.000	11:15
BLANK TEST	0.000	11:16
EXTERNAL STANDARD	0.076	11:16
BLANK TEST	0.000	11:17

