

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100389

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 08/03/2020

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.87: 0.080
LOT #: AG923401
EXPIRATION: 08/22/2021
TANK PRESSURE: 1218 psi

BLANK TEST	0.000	14:25
INTERNAL STANDARD	VERIFIED	14:26
EXTERNAL STANDARD	0.081	14:26
BLANK TEST	0.000	14:27
EXTERNAL STANDARD	0.080	14:27
BLANK TEST	0.000	14:28
EXTERNAL STANDARD	0.081	14:28
BLANK TEST	0.000	14:29
EXTERNAL STANDARD	0.081	14:29
BLANK TEST	0.000	14:30
EXTERNAL STANDARD	0.080	14:30
BLANK TEST	0.000	14:31

Average = 0.0806
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.1°C PASSED
Breath Tube = 48.1°C PASSED

PUMP INFO

Flow Rate = 4.905 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED


FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED


I, Brandi M. Barnett, after being first duly sworn, depose and state as follows:

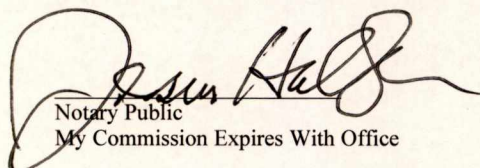
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

 10/16/20

Brandi M. Barnett
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 16 day of Oct, 2020




Notary Public
My Commission Expires With Office

JMB 09/17/20