



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

Certificate of Analysis

Customer Name

Exclusive Supplier

Intoximeters, Inc.

2081 Craig Road

St. Louis, Mo 63146

Test Date: 5-Mar-2018

Lot # AG805903 Model 108cacc

<u>Exp. Date</u>	<u>Cyl. Type</u>	<u>Component</u>	<u>Certified Concentration</u>
28-Feb-2020	108	Ethanol Nitrogen	0.100 ± 2% BrAC (260 ppm) Balance

Certification Traceable to N.I.S.T. RGM Ethanol Standards:

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

Analytical Method: NDIR

Digitally signed by Quality Control
Date: 2018.03.05 10:15:15 -06:00
Reason: Dry gas standard certification of analysis
Location: Airgas USA LLC (Lab)

Approved for Release:

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100353

Date: 05/15/2018
 Time: 11:22:36

SUPERVISOR NAME:
 DEREK WALTON
 OPERATOR'S #: 9508

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.100
 TARGET AT 29.82: 0.100
 TANK PRESSURE: 1175 psi

BLANK TEST	0.000	11:39
INTERNAL STANDARD	VERIFIED	11:39
EXTERNAL STANDARD	0.100	11:39
BLANK TEST	0.000	11:40
EXTERNAL STANDARD	0.101	11:40
BLANK TEST	0.000	11:41
EXTERNAL STANDARD	0.101	11:41
BLANK TEST	0.000	11:42
EXTERNAL STANDARD	0.100	11:42
BLANK TEST	0.000	11:43
EXTERNAL STANDARD	0.101	11:43
BLANK TEST	0.000	11:44

Average = 0.1006
 Std Dev = 0.0005

Lot # A6805903

Tank # 009

EXP. 02/28/2020

DMR 05/15/2018

0.1006

0.1004






0.0990

Avg = 0.100

DMR 05/16/18

Target = 0.100

Supervised by CAB 5/16/18

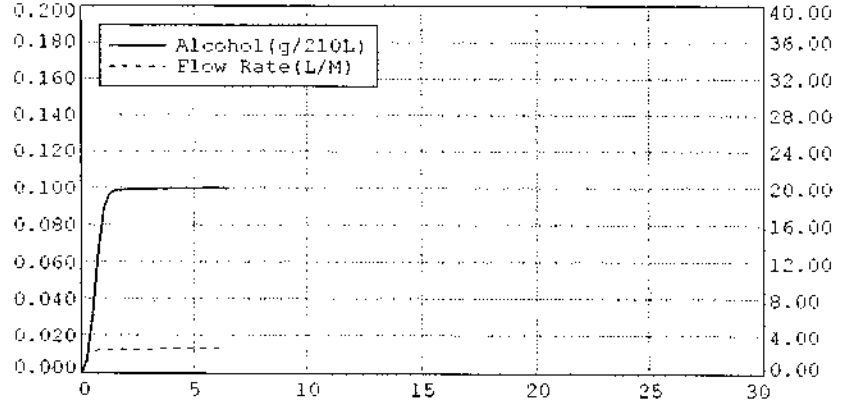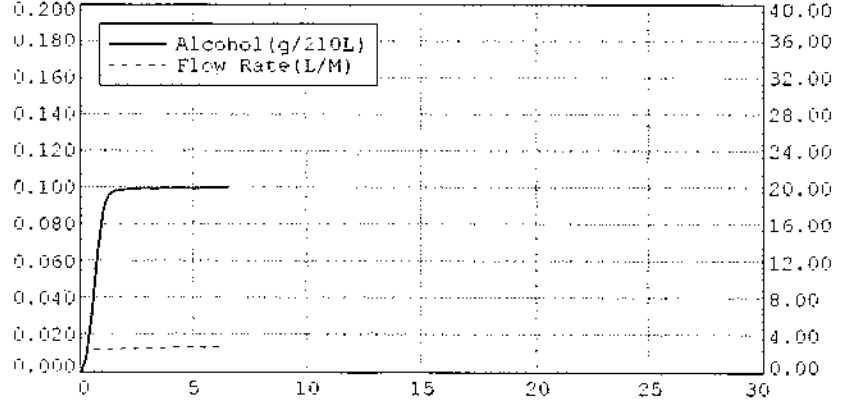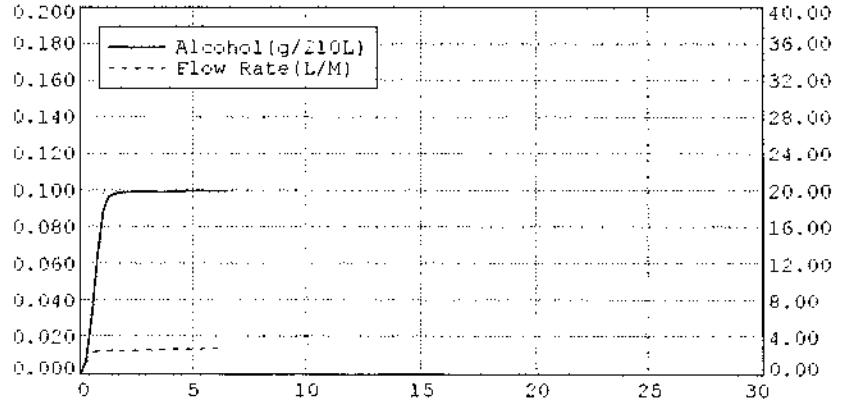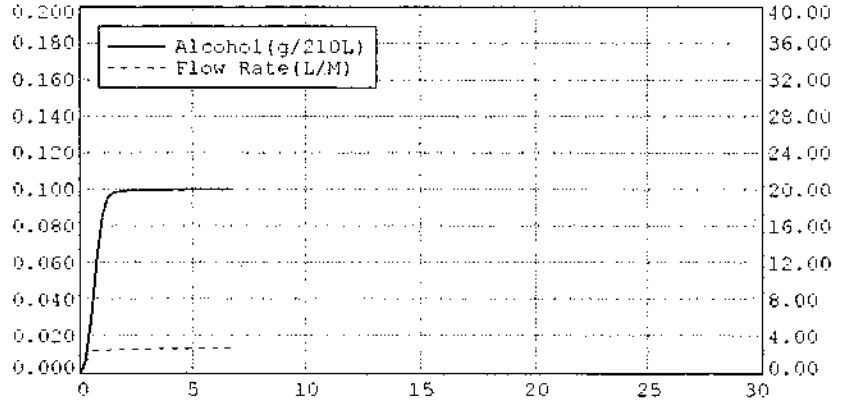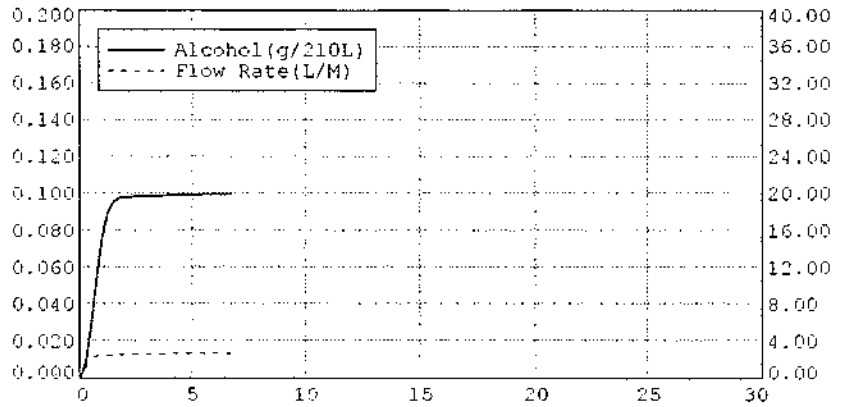

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100411

Date: 05/15/2018
 Time: 11:02:14

SUPERVISOR NAME:
 DEREK WALTON
 OPERATOR'S #: 9508

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.100
 TARGET AT 29.80: 0.100
 TANK PRESSURE: 1211 psi

BLANK TEST	0.000	11:03
INTERNAL STANDARD	VERIFIED	11:03
EXTERNAL STANDARD	0.101	11:04
BLANK TEST	0.000	11:05
EXTERNAL STANDARD	0.101	11:05
BLANK TEST	0.000	11:06
EXTERNAL STANDARD	0.100	11:06
BLANK TEST	0.000	11:07
EXTERNAL STANDARD	0.100	11:07
BLANK TEST	0.000	11:08
EXTERNAL STANDARD	0.100	11:08
BLANK TEST	0.000	11:09






Average = 0.1004
 Std Dev = 0.0005

*Lot # 8 DM 05/15/2018
 AG805903*

Tank # 009

Exp. 02/28/2020

DM 05/15/2018

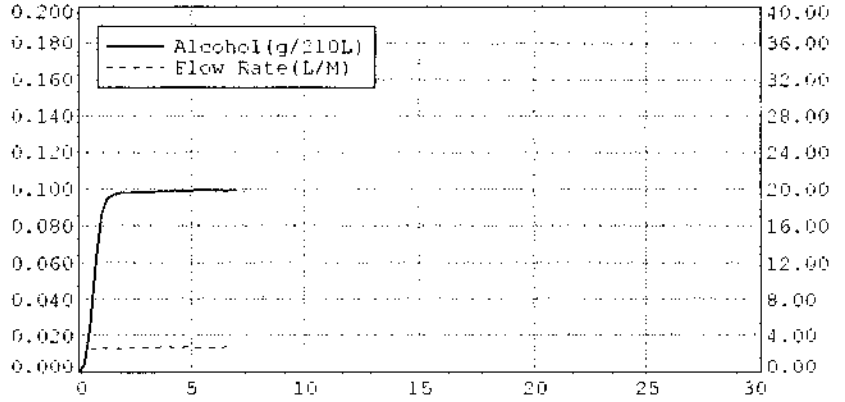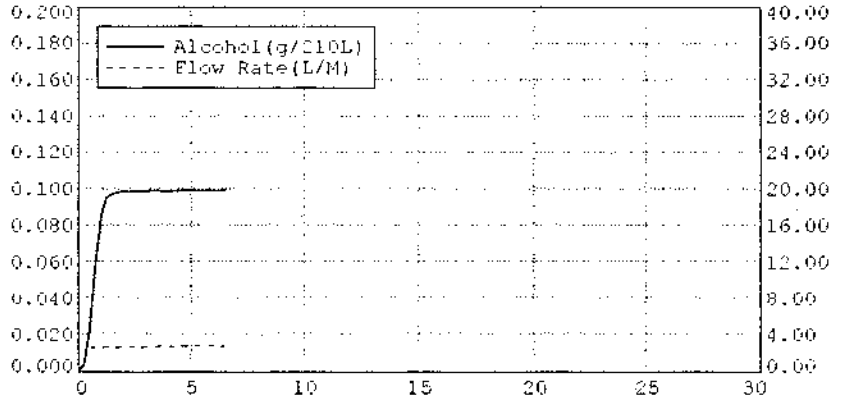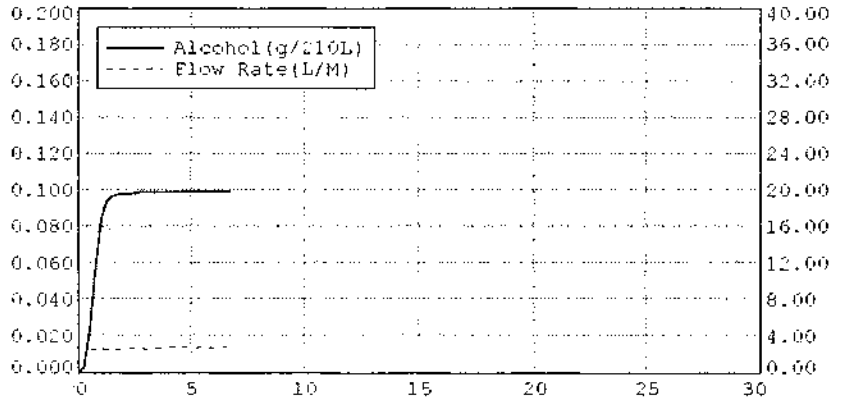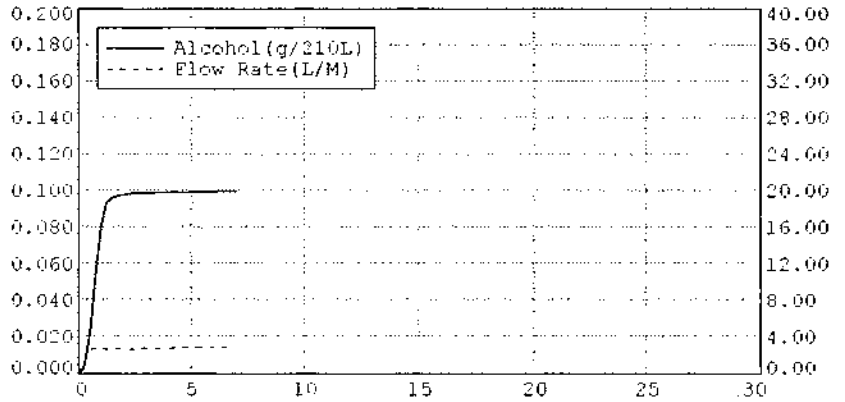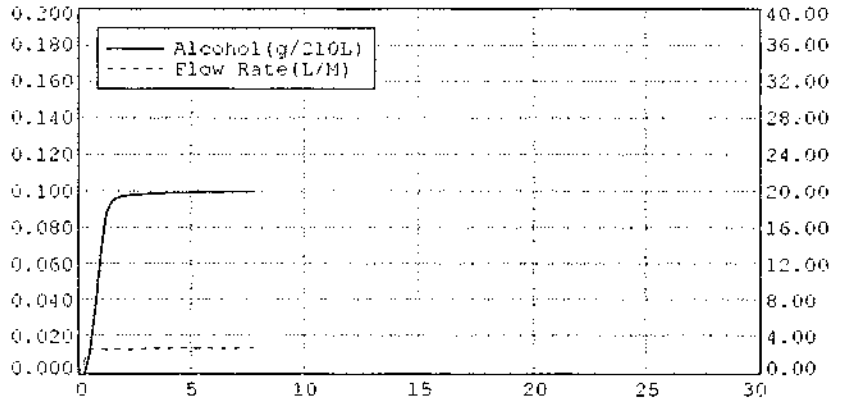

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100671

Date: 05/15/2018
 Time: 11:37:00

SUPERVISOR NAME:
 DEREK WALTON
 OPERATOR'S #: 9508

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.100
 TARGET AT 29.80: 0.100
 TANK PRESSURE: 1198 psi

BLANK TEST	0.000	11:38
INTERNAL STANDARD	VERIFIED	11:38
EXTERNAL STANDARD	0.099	11:38
BLANK TEST	0.000	11:39
EXTERNAL STANDARD	0.099	11:39
BLANK TEST	0.000	11:40
EXTERNAL STANDARD	0.099	11:41
BLANK TEST	0.000	11:41
EXTERNAL STANDARD	0.099	11:42
BLANK TEST	0.000	11:43
EXTERNAL STANDARD	0.099	11:43
BLANK TEST	0.000	11:44






Average = 0.0990
 Std Dev = 0.0000

Lot # AG805903

Tank # 009

Exp. 02/28/2020

DW 05/15/2018

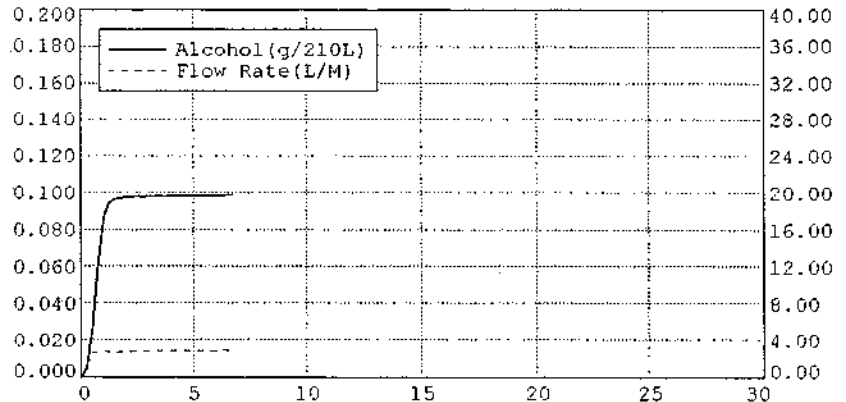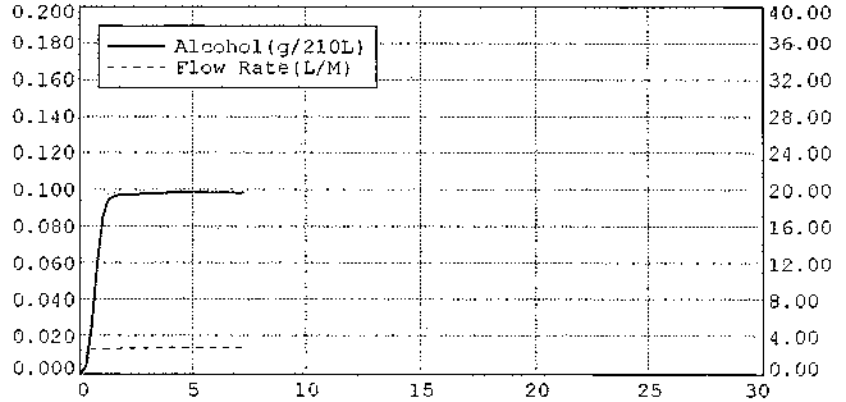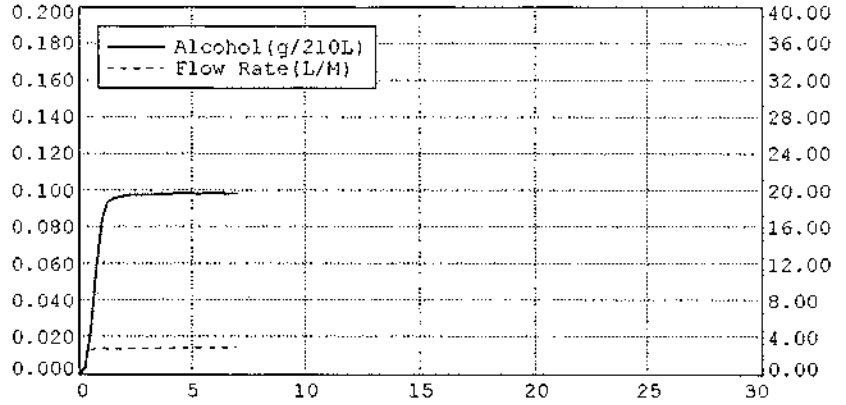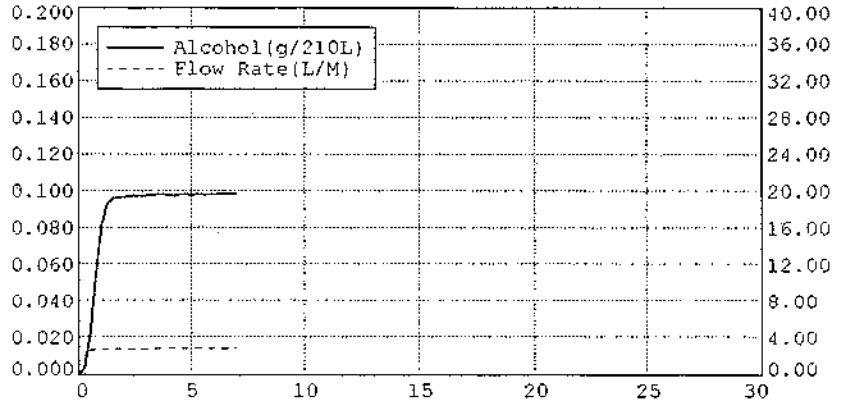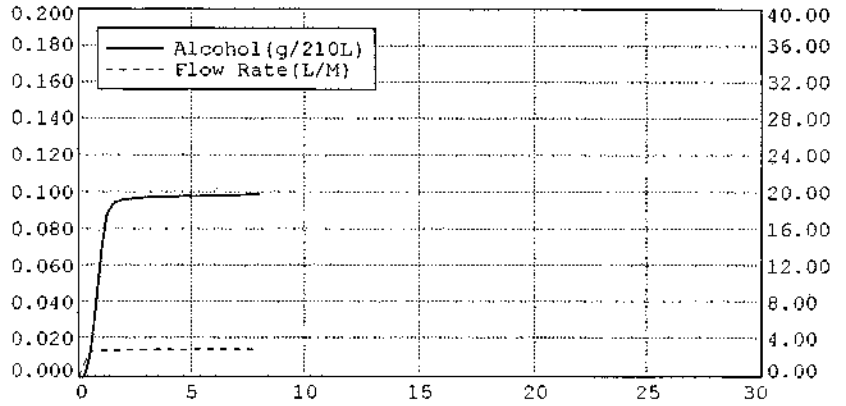

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100353

Date: 05/15/2018
 Time: 11:14:10

SUPERVISOR NAME:
 DEREK WALTON
 OPERATOR'S #: 9508

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.100
 TARGET AT 29.82: 0.100
 TANK PRESSURE: 1200 psi

BLANK TEST	0.000	11:15
INTERNAL STANDARD	VERIFIED	11:15
EXTERNAL STANDARD	0.101	11:15
BLANK TEST	0.000	11:16
EXTERNAL STANDARD	0.101	11:17
BLANK TEST	0.000	11:17
EXTERNAL STANDARD	0.101	11:18
BLANK TEST	0.000	11:19
EXTERNAL STANDARD	0.101	11:19
BLANK TEST	0.000	11:20
EXTERNAL STANDARD	0.100	11:20
BLANK TEST	0.000	11:21

Average = 0.1008
 Std Dev = 0.0004

Lot # AG 805903

Tank # 010

Exp. 02/28/2020

DW 05/15/2018

0.1008






0.1004

0.0996

Arg = 0.100

DW
 05/16/18

Target = 0.100

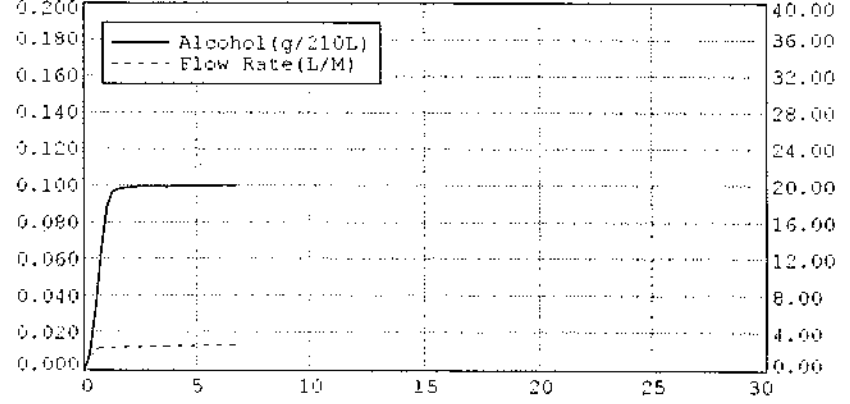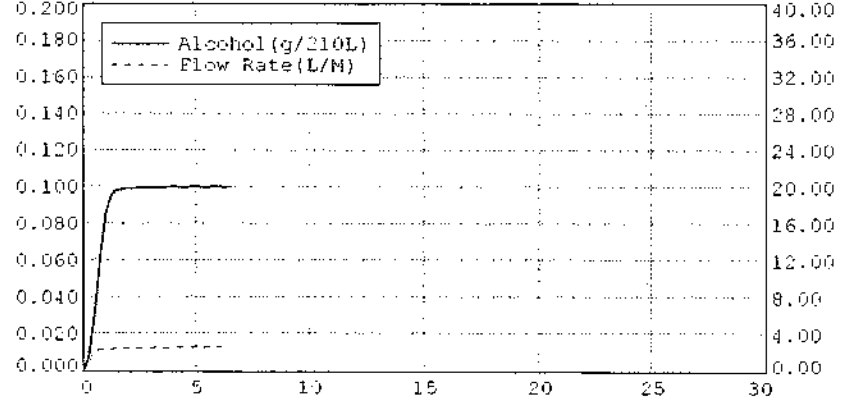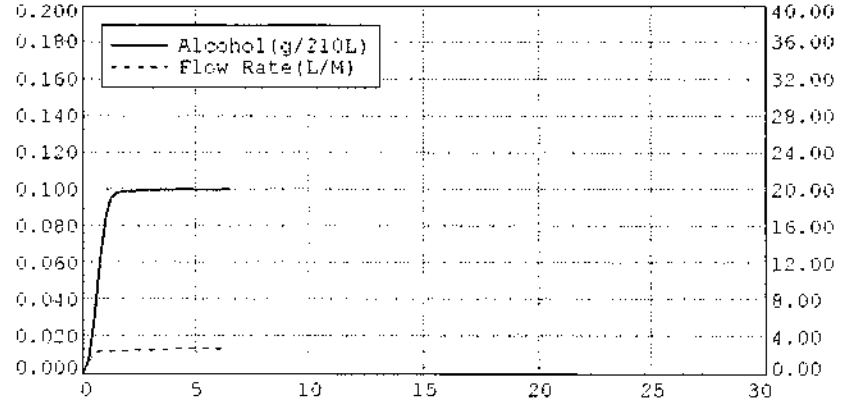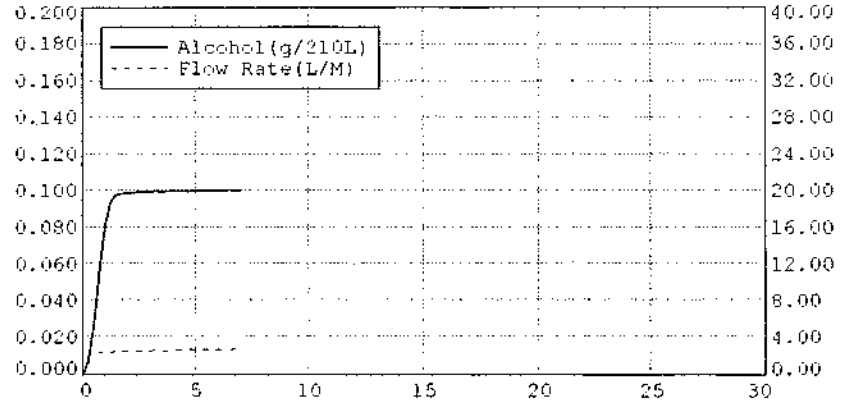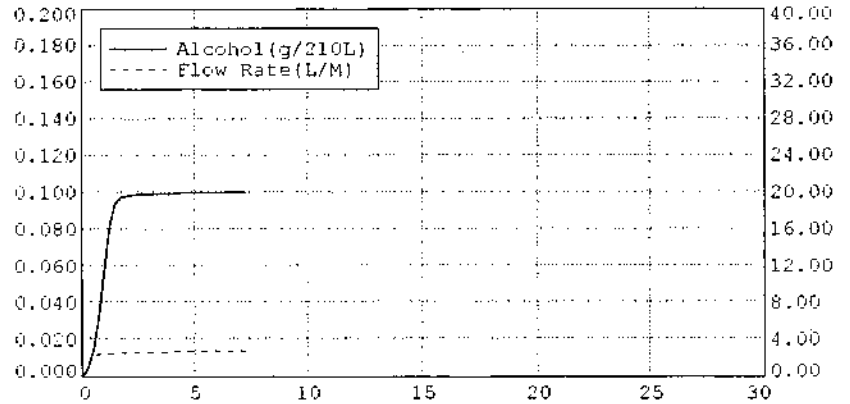

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100411

Date: 05/15/2018
 Time: 11:11:58

SUPERVISOR NAME:
 DEREK WALTON
 OPERATOR'S #: 9508

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.100
 TARGET AT 29.80: 0.100
 TANK PRESSURE: 1195 psi

BLANK TEST	0.000	11:13
INTERNAL STANDARD	VERIFIED	11:13
EXTERNAL STANDARD	0.100	11:13
BLANK TEST	0.000	11:14
EXTERNAL STANDARD	0.101	11:14
BLANK TEST	0.000	11:15
EXTERNAL STANDARD	0.101	11:15
BLANK TEST	0.000	11:16
EXTERNAL STANDARD	0.100	11:17
BLANK TEST	0.000	11:18
EXTERNAL STANDARD	0.100	11:18
BLANK TEST	0.000	11:19






Average = 0.1004
 Std Dev = 0.0005

Lot # AG805903

Tank # 010

Exp. 02/28/2020

DW 05/15/2018

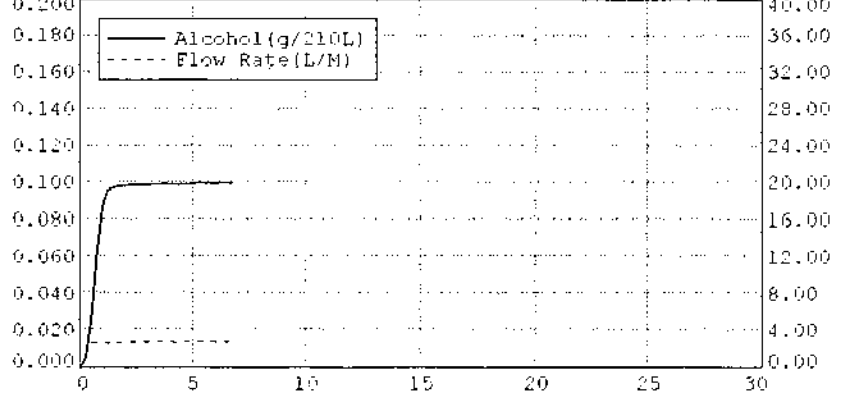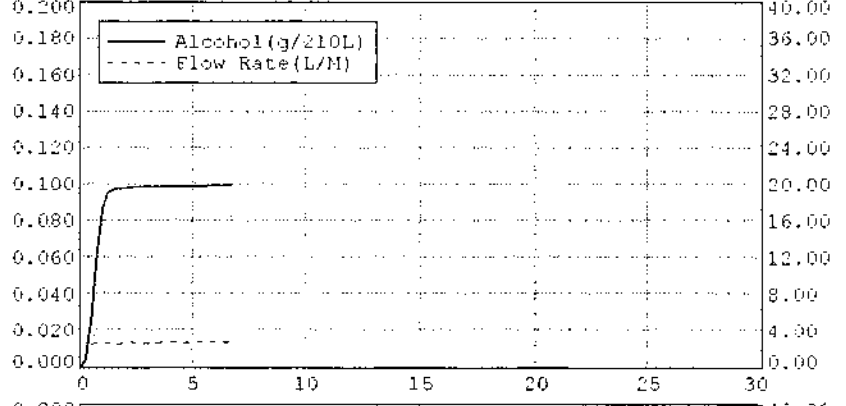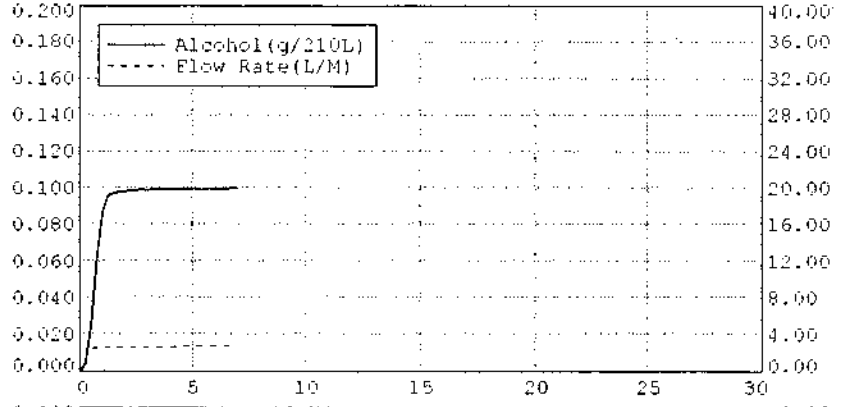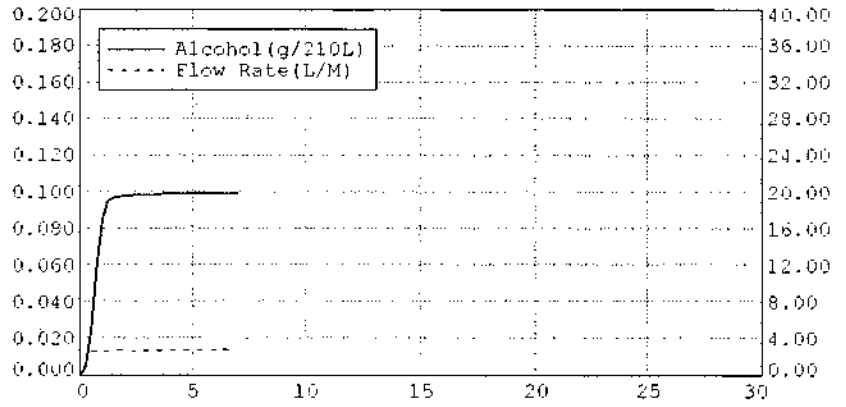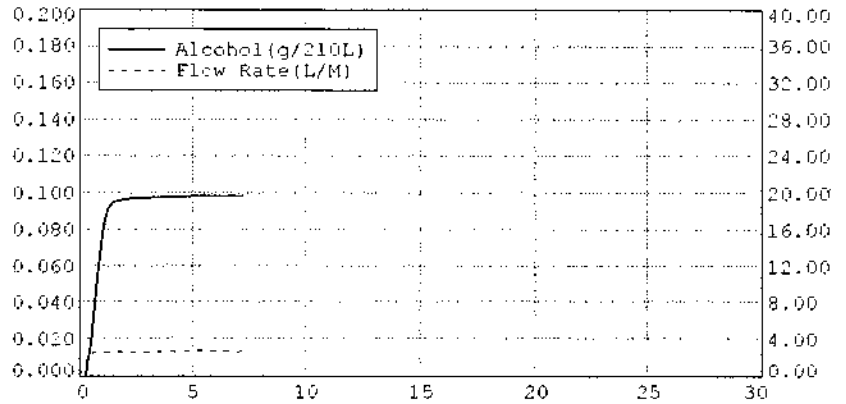

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100671

Date: 05/15/2018
 Time: 11:45:12

SUPERVISOR NAME:
 DEREK WALTON
 OPERATOR'S #: 9508

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.80: 0.100
 TANK PRESSURE: 1175 psi

BLANK TEST	0.000	11:46
INTERNAL STANDARD	VERIFIED	11:46
EXTERNAL STANDARD	0.100	11:47
BLANK TEST	0.000	11:47
EXTERNAL STANDARD	0.100	11:48
BLANK TEST	0.000	11:49
EXTERNAL STANDARD	0.099	11:49
BLANK TEST	0.000	11:50
EXTERNAL STANDARD	0.099	11:50
BLANK TEST	0.000	11:51
EXTERNAL STANDARD	0.100	11:51
BLANK TEST	0.000	11:52






Average = 0.0996
 Std Dev = 0.0005

Lot # AG805903

Tank # 010

Exp. 02/28/2020

DMV 05/15/2018

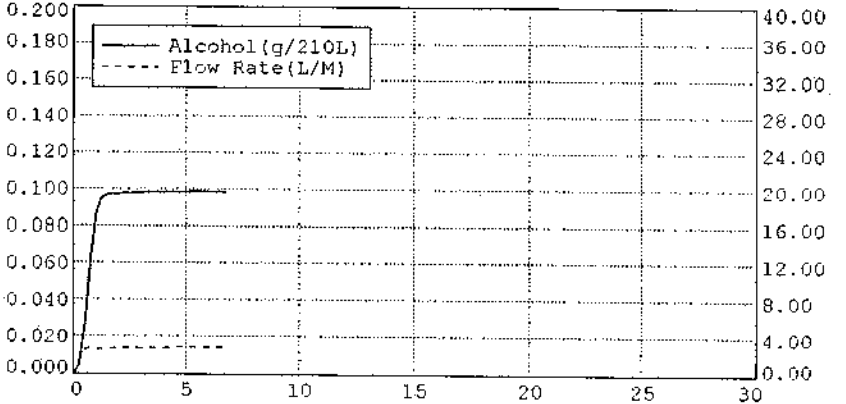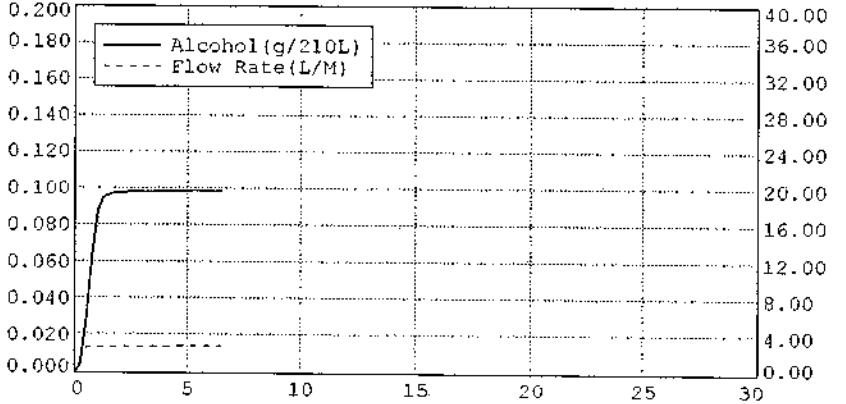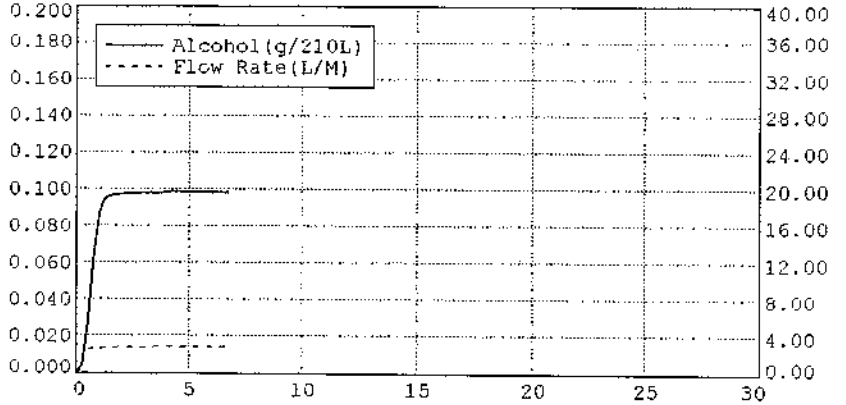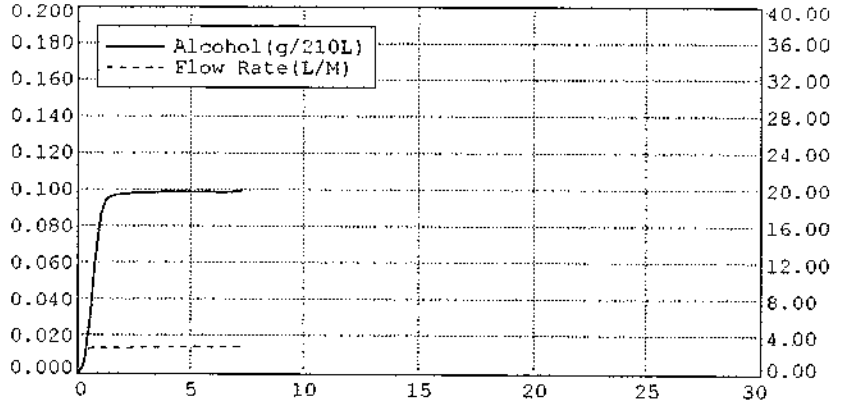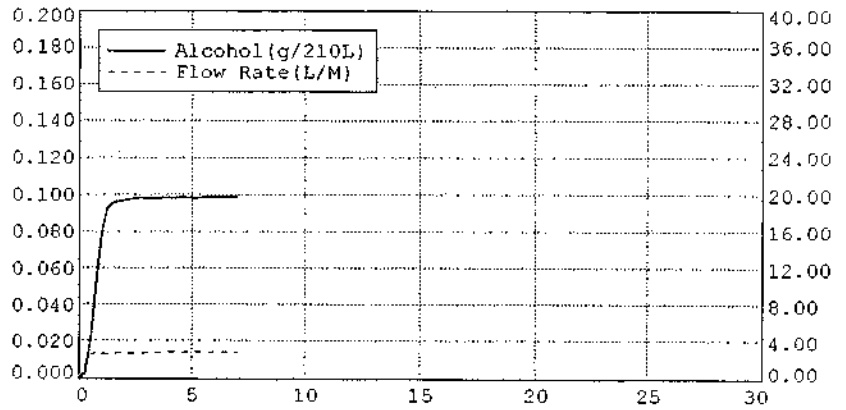

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100353

Date: 05/15/2018
Time: 09:19:42

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 2.15 V PASSED
(1.30 V - 3.04 V)
Cooler Voltage = 2.10 V PASSED
(1.26 V - 2.94 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 538 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.8 in

PUMP INFO

Flow Rate = 4.785 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.093 1.39% (0.00% - 4.00%) PASSED

LINEARITY CHECK


Alaska Department of Public Safety
DATAMASTER dmt: 100353

Date: 05/15/2018
Time: 09:34:54

SUPERVISOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

TARGET	AVERAGE	STD. DEV.
0.020	0.0208	0.0004
0.100	0.1008	0.0004
0.300	0.2994	0.0011

SLOPE = 0.994615
R² = 0.999998

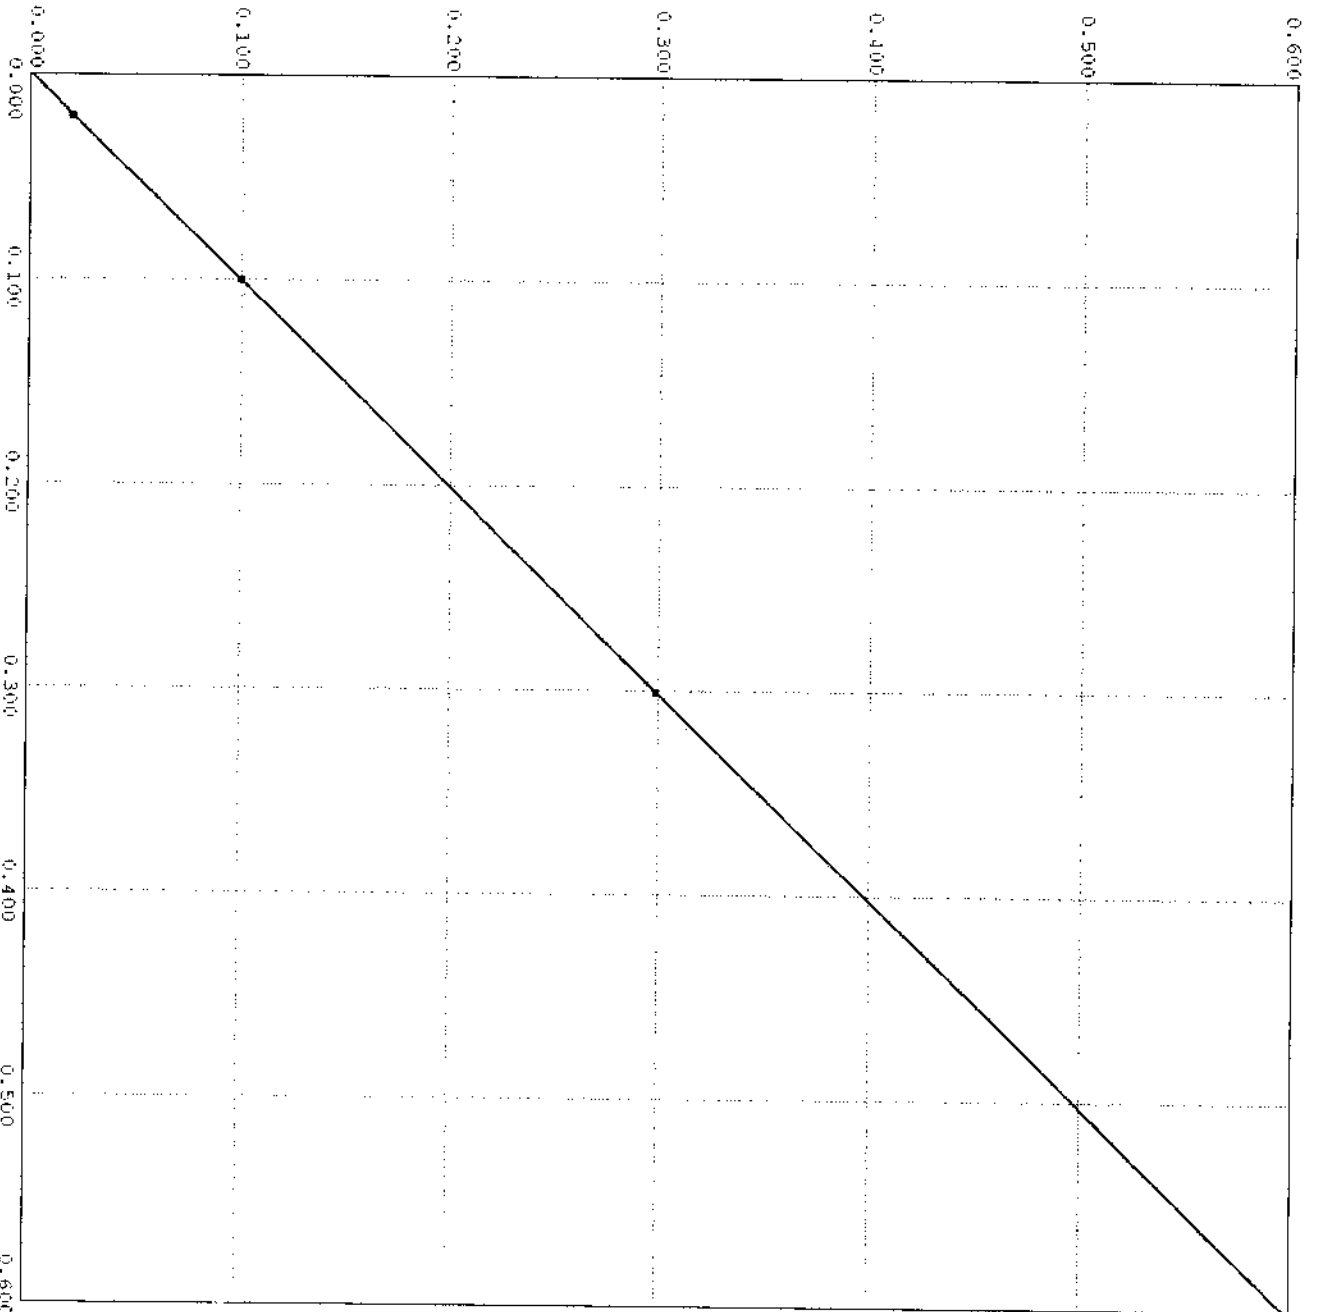

DM

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100353






Date: 05/15/2018
Time: 09:34:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.80: 0.020
LOT #: AG616504
EXPIRATION: 06/13/2018
TANK PRESSURE: 990 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	09:36
INTERNAL STANDARD	VERIFIED	09:36
EXTERNAL STANDARD	0.021	09:36
BLANK TEST	0.000	09:37
EXTERNAL STANDARD	0.021	09:37
BLANK TEST	0.000	09:38
EXTERNAL STANDARD	0.021	09:39
BLANK TEST	0.000	09:39
EXTERNAL STANDARD	0.021	09:40
BLANK TEST	0.000	09:41
EXTERNAL STANDARD	0.020	09:41
BLANK TEST	0.000	09:42

Average = 0.0208
Std Dev = 0.0004

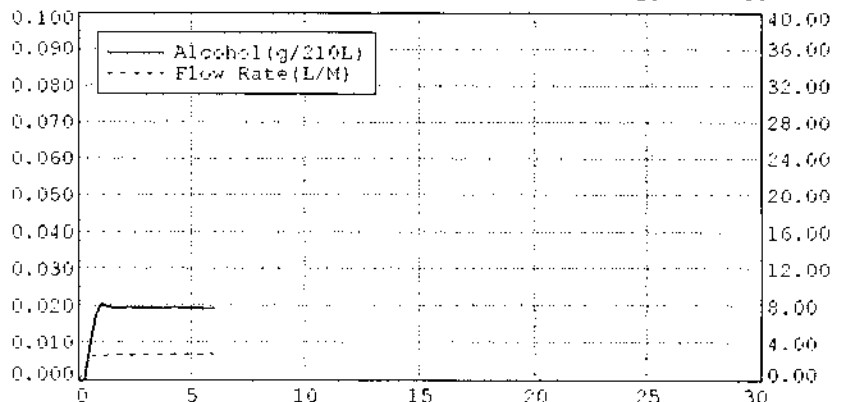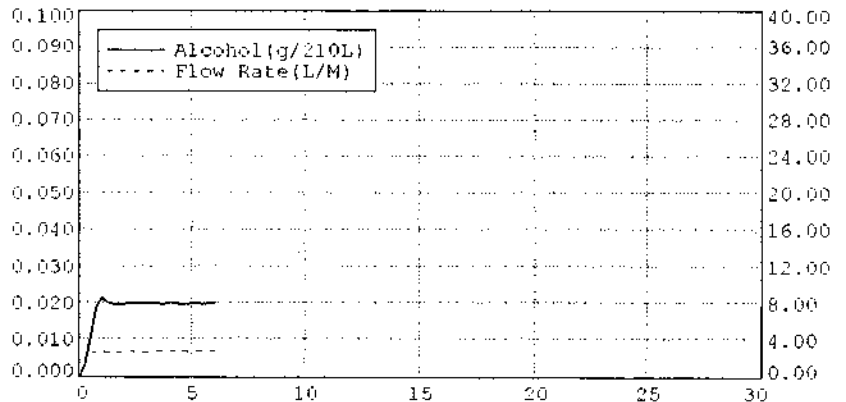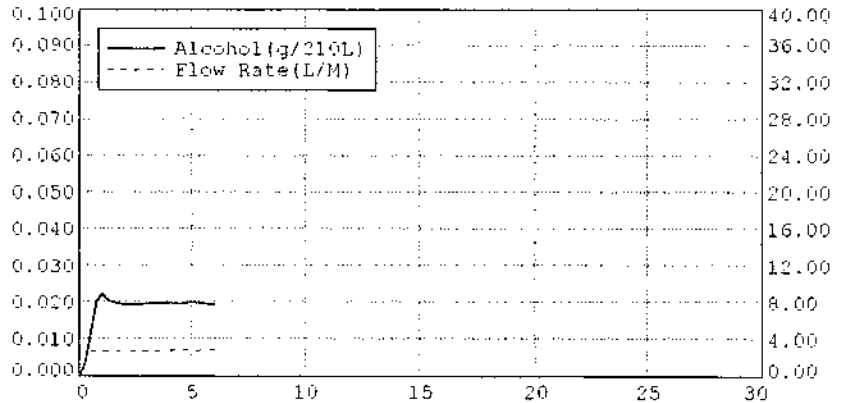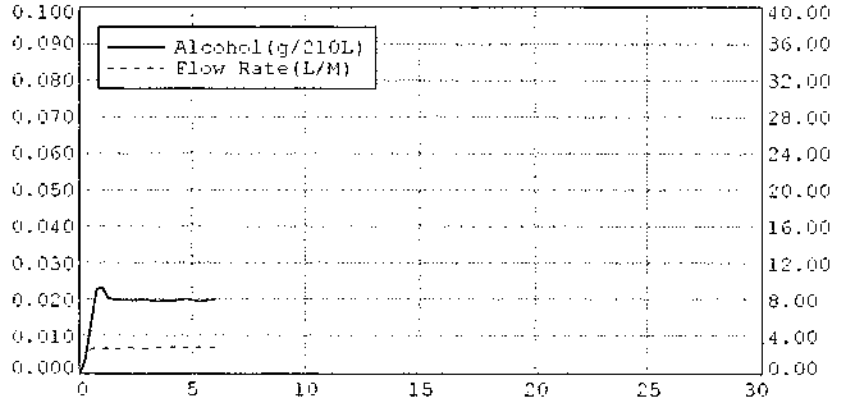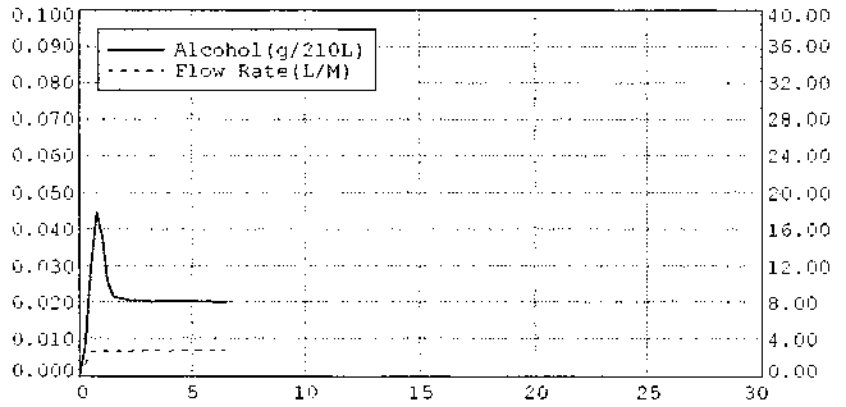

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100353






Date: 05/15/2018
 Time: 09:44:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.80: 0.100
 LOT #: AG629304
 EXPIRATION: 10/19/2018
 TANK PRESSURE: 948 psi

BLANK TEST	0.000	09:46
INTERNAL STANDARD	VERIFIED	09:46
EXTERNAL STANDARD	0.101	09:46
BLANK TEST	0.000	09:47
EXTERNAL STANDARD	0.101	09:47
BLANK TEST	0.000	09:48
EXTERNAL STANDARD	0.101	09:48
BLANK TEST	0.000	09:49
EXTERNAL STANDARD	0.100	09:49
BLANK TEST	0.000	09:50
EXTERNAL STANDARD	0.101	09:51
BLANK TEST	0.000	09:51

Average = 0.1008
 Std Dev = 0.0004

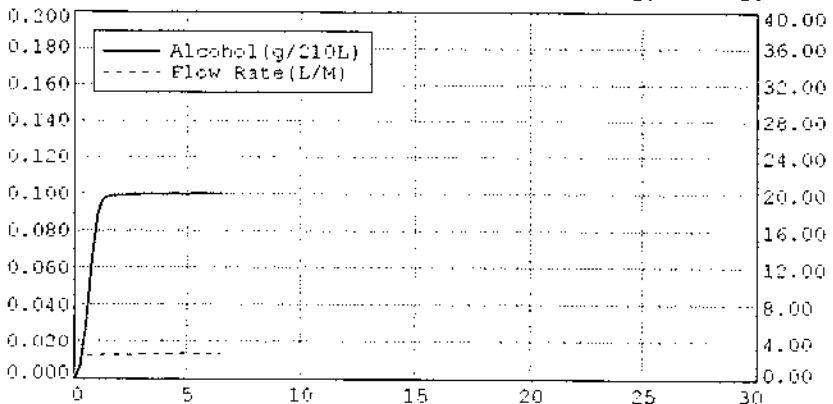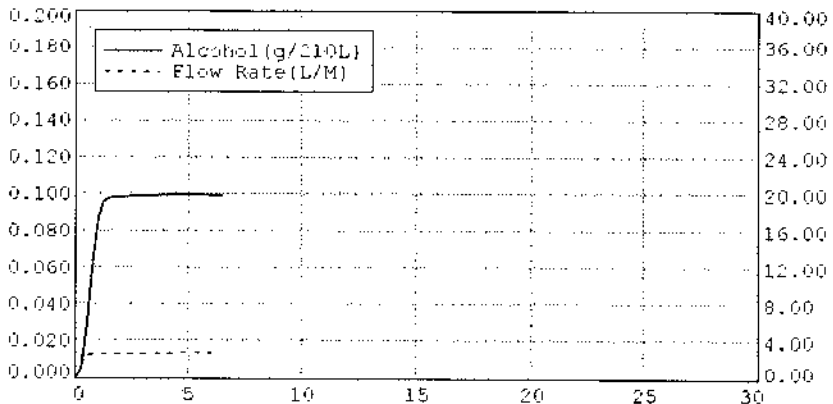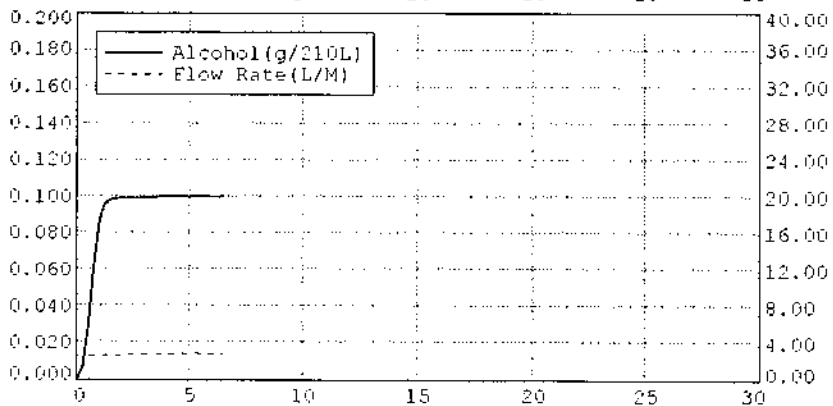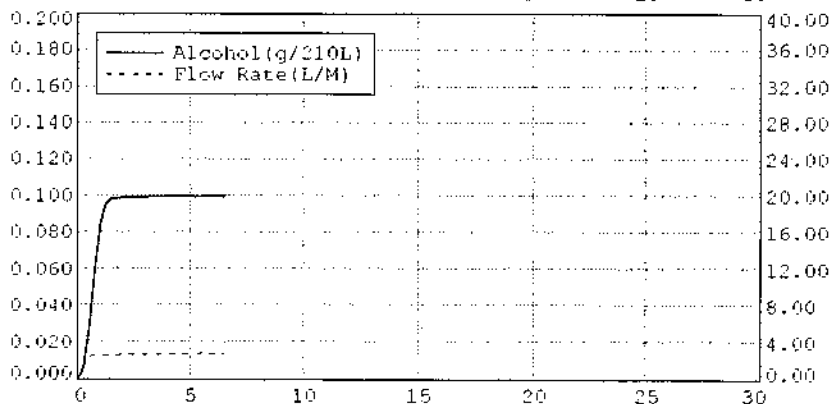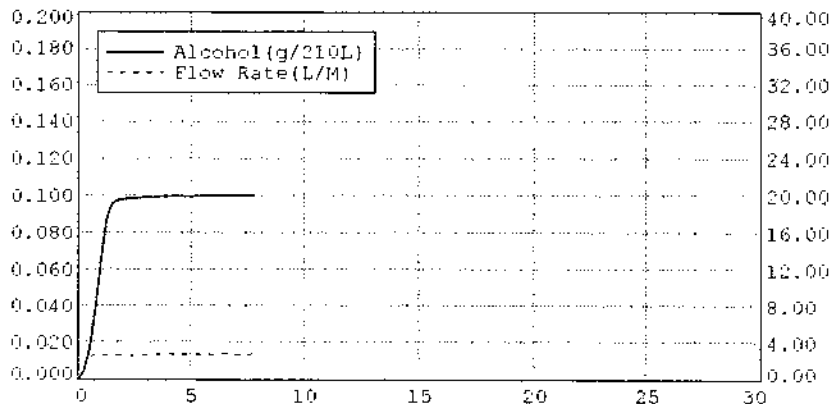

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100353

Date: 05/15/2018
 Time: 09:56:31

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 LOT #: 17140
 EXPIRATION: 05/15/2019






BLANK TEST	0.000	09:58
INTERNAL STANDARD	VERIFIED	09:58
EXTERNAL STANDARD	0.298	09:59
BLANK TEST	0.000	10:00
EXTERNAL STANDARD	0.299	10:01
BLANK TEST	0.000	10:02
EXTERNAL STANDARD	0.299	10:02
BLANK TEST	0.000	10:03
EXTERNAL STANDARD	0.300	10:03
BLANK TEST	0.000	10:04
EXTERNAL STANDARD	0.301	10:05
BLANK TEST	0.000	10:06

Average = 0.2994
 Std Dev = 0.0011

Simulator S/N: SD1202

Calibrated: 01/24/2018

JM 05/15/2018

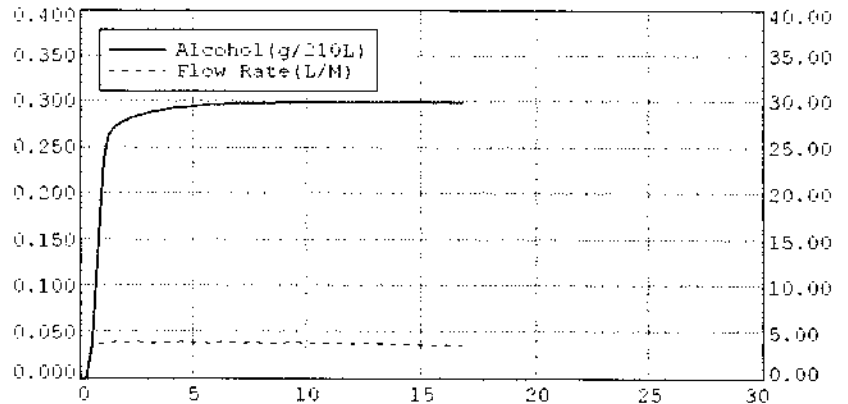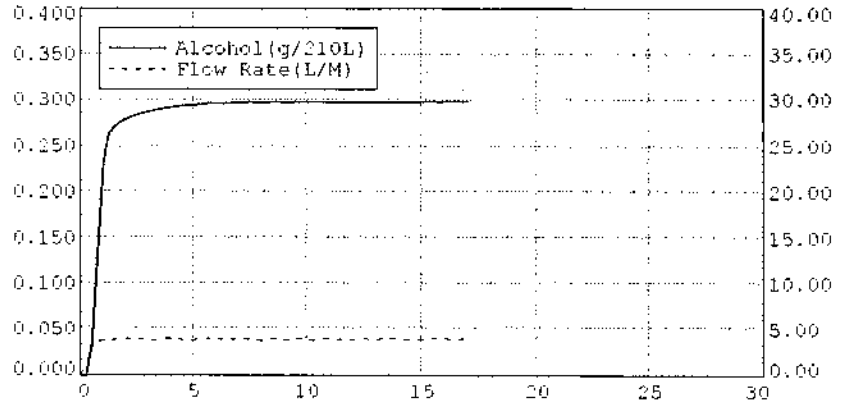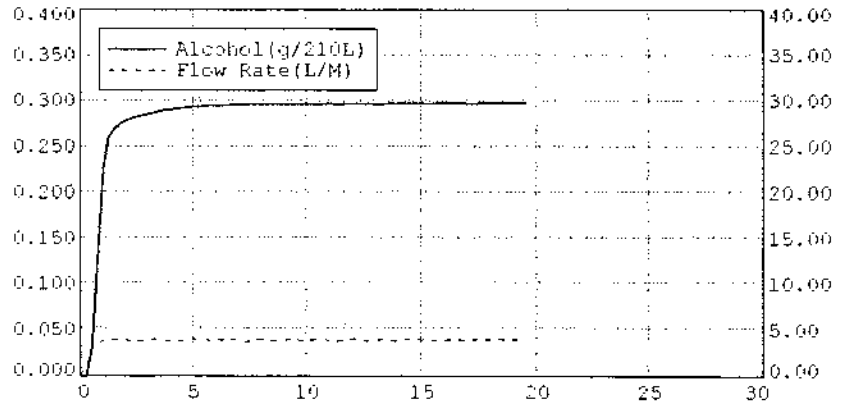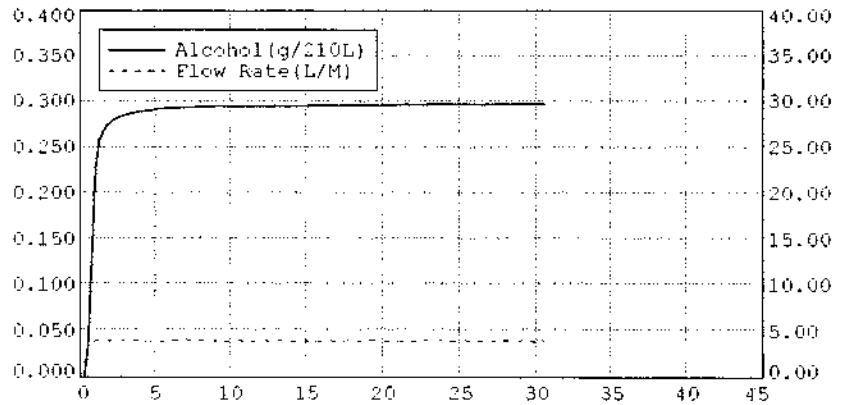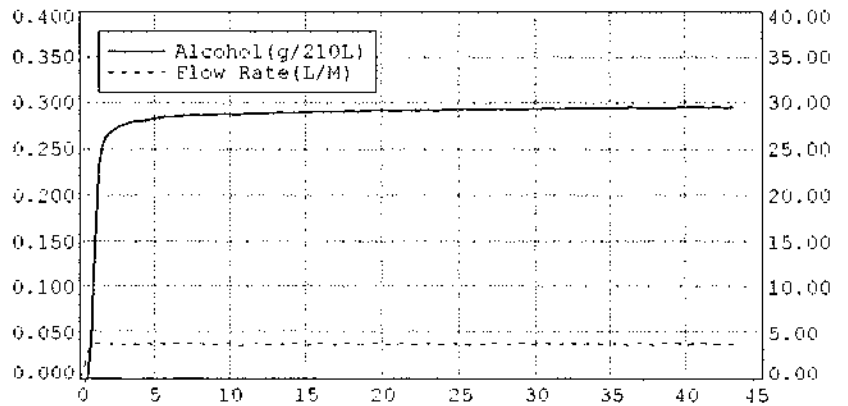

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100411

Date: 05/15/2018
Time: 09:05:17

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 47.8°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.82 V PASSED
(1.10 V - 2.58 V)
Cooler Voltage = 1.92 V PASSED
(1.06 V - 2.48 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 537 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.8 in

PUMP INFO

Flow Rate = 5.237 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED

Xq = 0.084 1.92% (0.00% - 4.00%)

LINEARITY CHECK


Alaska Department of Public Safety
DATAMASTER dmt: 100411

Date: 05/15/2018
Time: 09:39:50

SUPERVISOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

TARGET	AVERAGE	STD. DEV.
0.020	0.0208	0.0004
0.100	0.1006	0.0005
0.300	0.2986	0.0005

SLOPE = 0.991731
R² = 0.999997

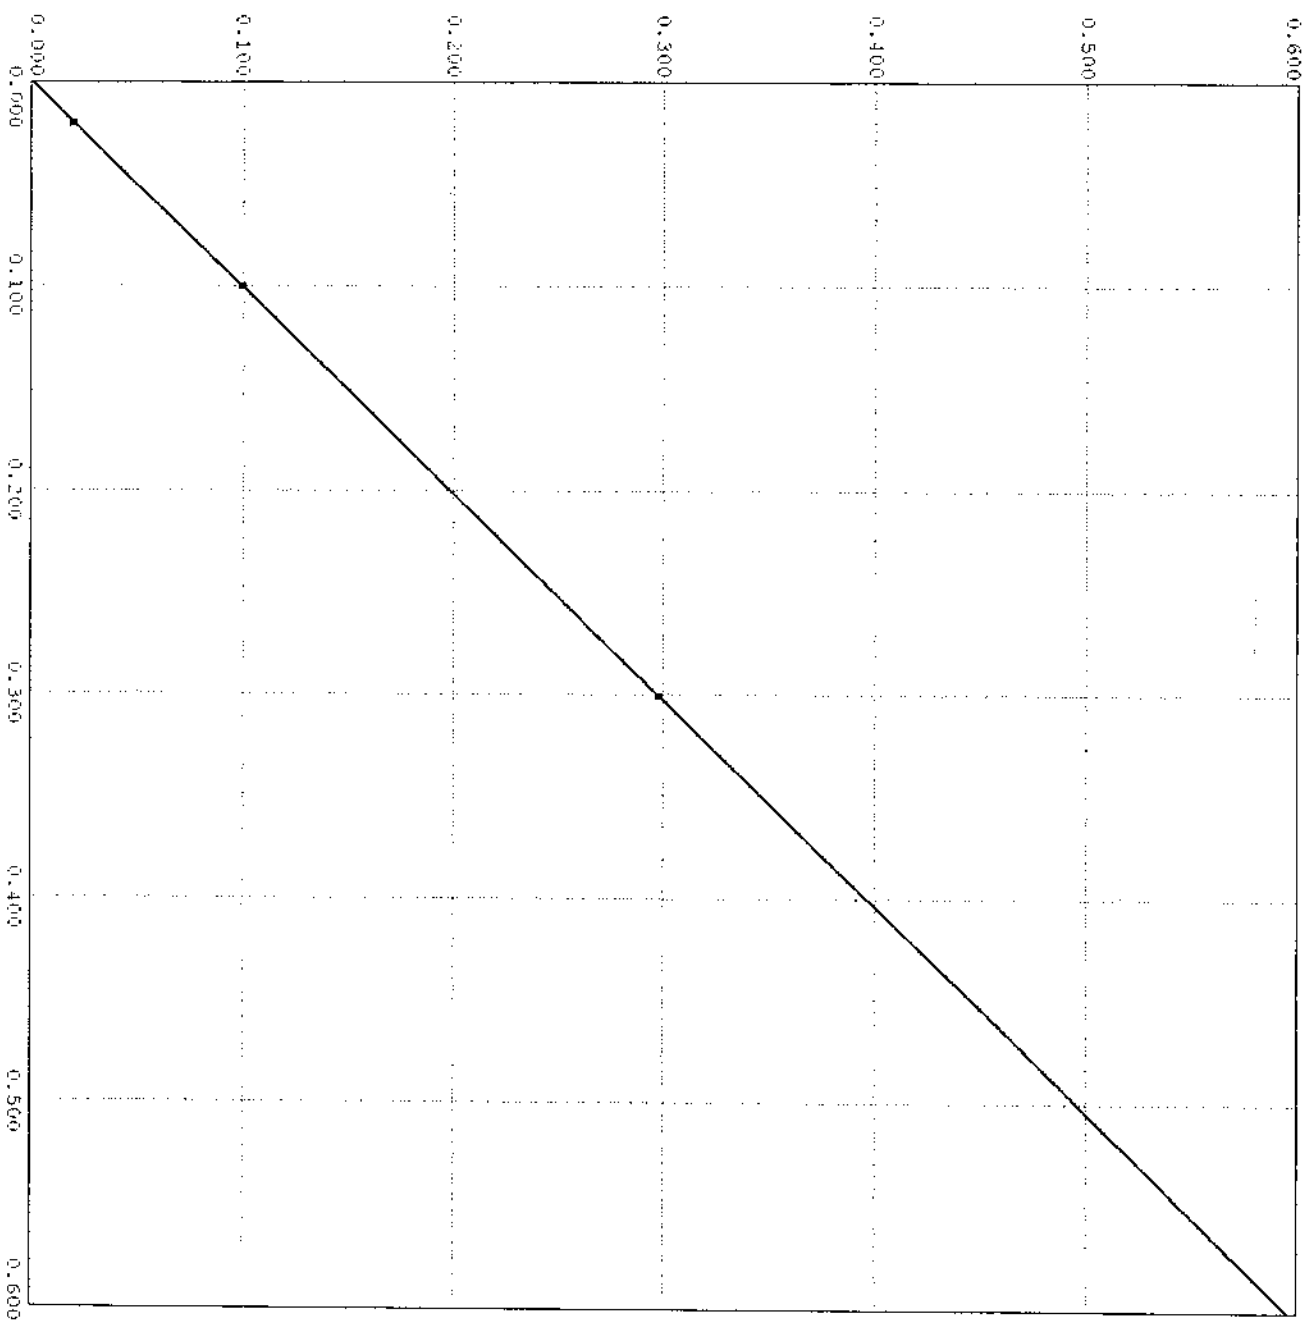

DM

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dnt: 100411






Date: 05/15/2018
 Time: 09:39:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.79: 0.020
 LOT #: AG616504
 EXPIRATION: 06/13/2018
 TANK PRESSURE: 976 psi

BLANK TEST	0.000	09:41
INTERNAL STANDARD	VERIFIED	09:41
EXTERNAL STANDARD	0.020	09:41
BLANK TEST	0.000	09:42
EXTERNAL STANDARD	0.021	09:42
BLANK TEST	0.000	09:43
EXTERNAL STANDARD	0.021	09:43
BLANK TEST	0.000	09:44
EXTERNAL STANDARD	0.021	09:45
BLANK TEST	0.000	09:45
EXTERNAL STANDARD	0.021	09:46
BLANK TEST	0.000	09:47

Average = 0.0208
 Std Dev = 0.0004

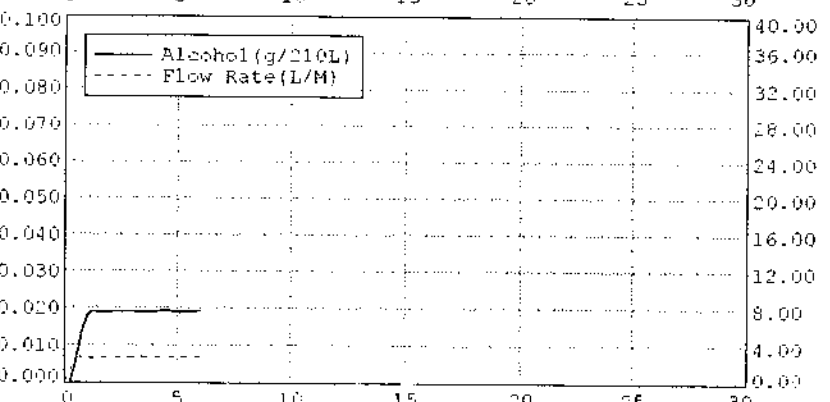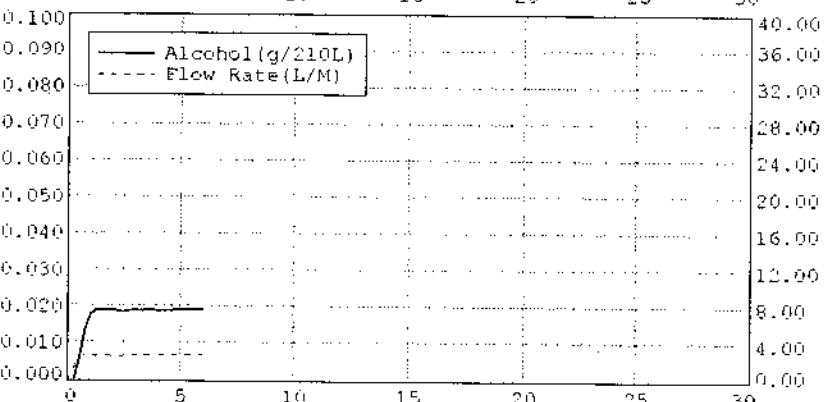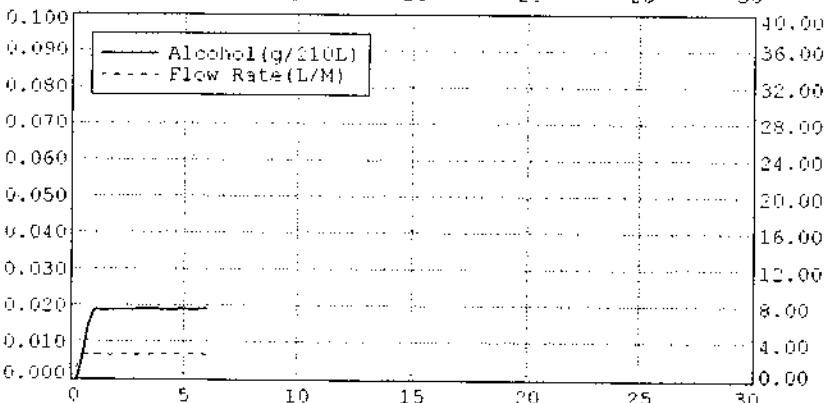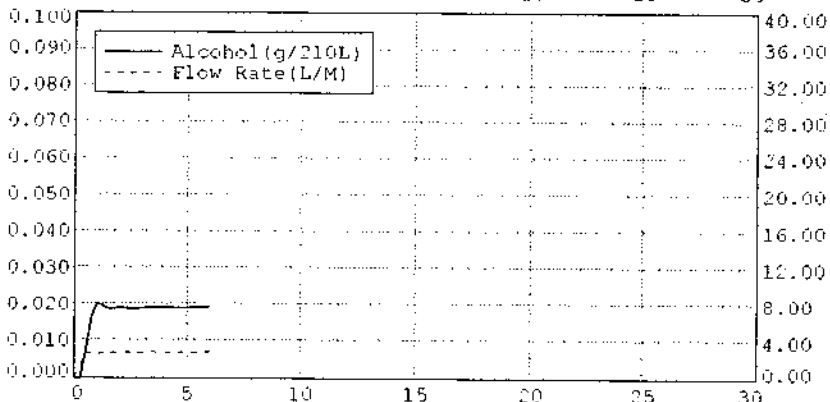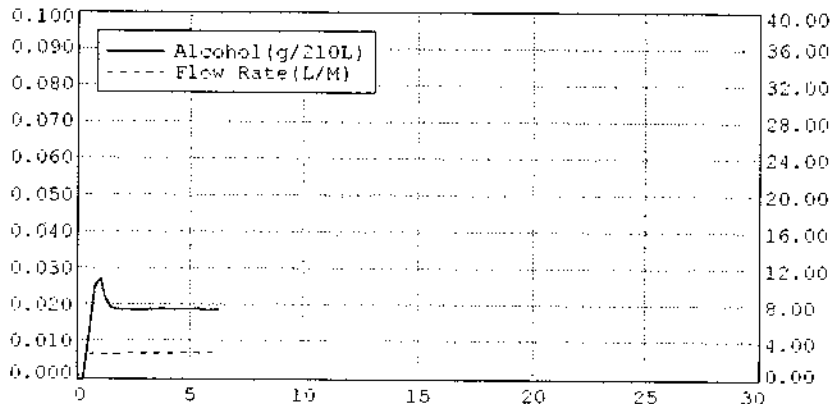

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100411






Date: 05/15/2018
 Time: 09:50:11

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.79: 0.100
 LOT #: AG629304
 EXPIRATION: 10/19/2018
 TANK PRESSURE: 473 psi

BLANK TEST	0.000	09:51
INTERNAL STANDARD	VERIFIED	09:51
EXTERNAL STANDARD	0.101	09:51
BLANK TEST	0.000	09:52
EXTERNAL STANDARD	0.100	09:53
BLANK TEST	0.000	09:53
EXTERNAL STANDARD	0.101	09:54
BLANK TEST	0.000	09:55
EXTERNAL STANDARD	0.100	09:55
BLANK TEST	0.000	09:56
EXTERNAL STANDARD	0.101	09:56
BLANK TEST	0.000	09:57

Average = 0.1006
 Std Dev = 0.0005

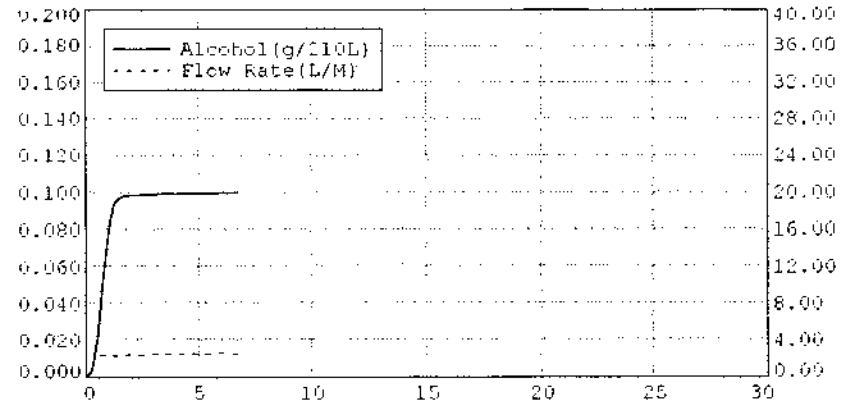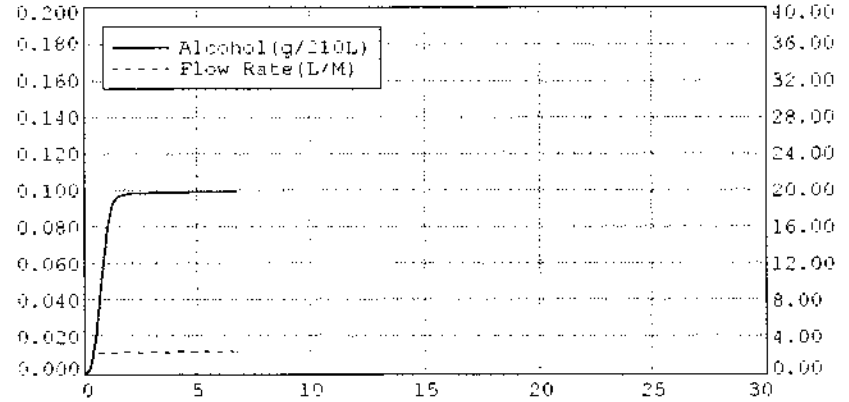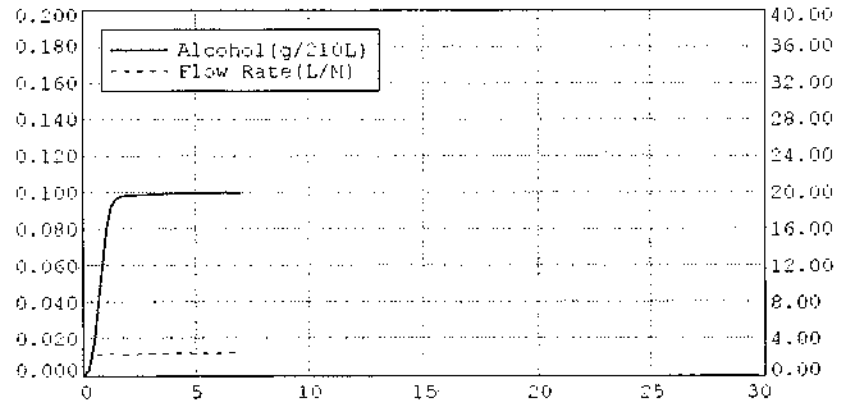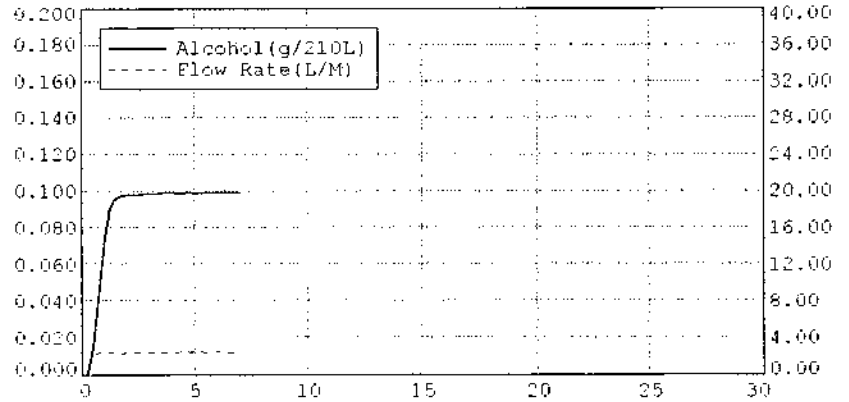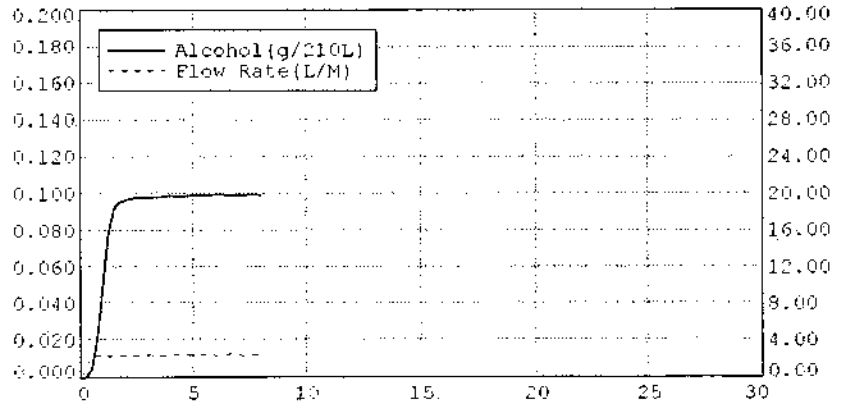

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dnt: 100411

Date: 05/15/2018
 Time: 10:01:54

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 LOT #: 17140
 EXPIRATION: 05/15/2019






BLANK TEST	0.000	10:03
INTERNAL STANDARD	VERIFIED	10:03
EXTERNAL STANDARD	0.299	10:03
BLANK TEST	0.000	10:04
EXTERNAL STANDARD	0.298	10:05
BLANK TEST	0.000	10:06
EXTERNAL STANDARD	0.299	10:06
BLANK TEST	0.000	10:07
EXTERNAL STANDARD	0.299	10:08
BLANK TEST	0.000	10:09
EXTERNAL STANDARD	0.298	10:09
BLANK TEST	0.000	10:10

Average = 0.2986
 Std Dev = 0.0005

Simulator S/N: SD1202

Calibrated 01/24/2018

JMY 05/15/2018

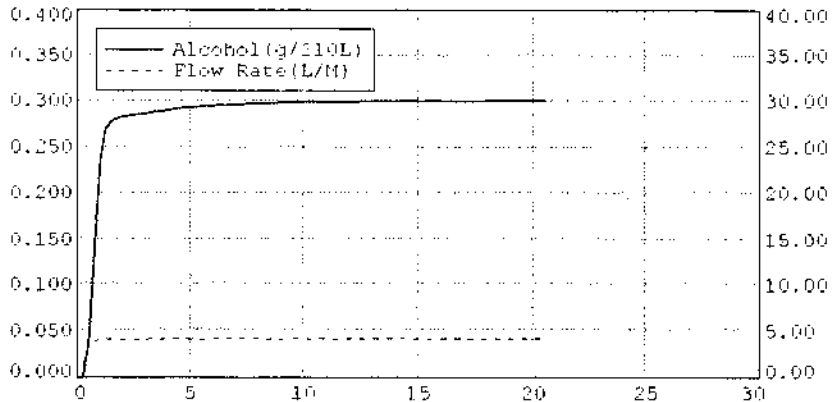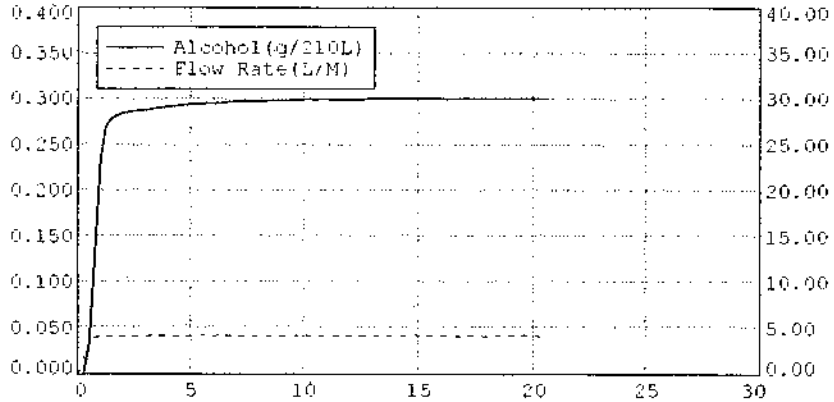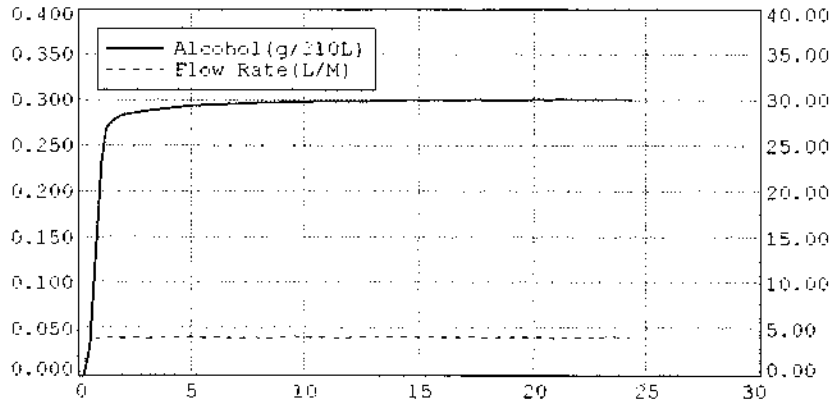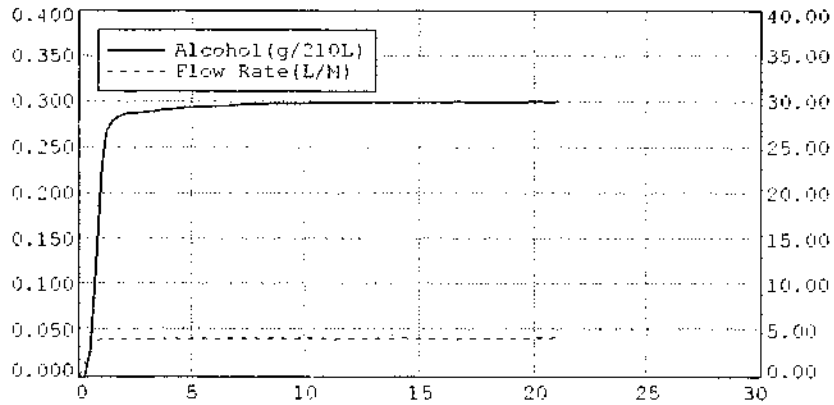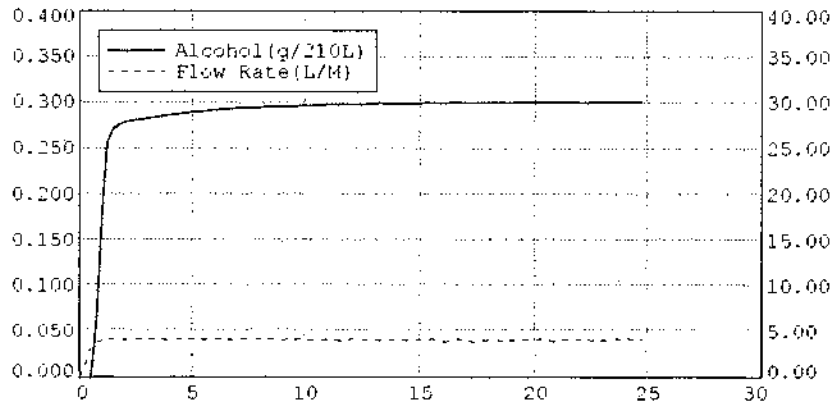

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 05/15/2018
Time: 09:28:39

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 46.9°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.64 V PASSED
(1.01 V - 2.37 V)
Cooler Voltage = 1.76 V PASSED
(1.00 V - 2.32 V)
Bias Voltage = 80 V PASSED
(47 V - 111 V)
Chopper Freq = 545 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.8 in

PUMP INFO

Flow Rate = 4.705 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED

Xq = 0.100 1.42% (0.00% - 4.00%)

LINEARITY CHECK


Alaska Department of Public Safety
DATA MASTER dmt: 100671

Date: 05/15/2018
Time: 09:47:13

SUPERVISOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0004
0.100	0.0992	0.0004
0.300	0.2960	0.0012

SLOPE = 0.984808
R² = 0.999999

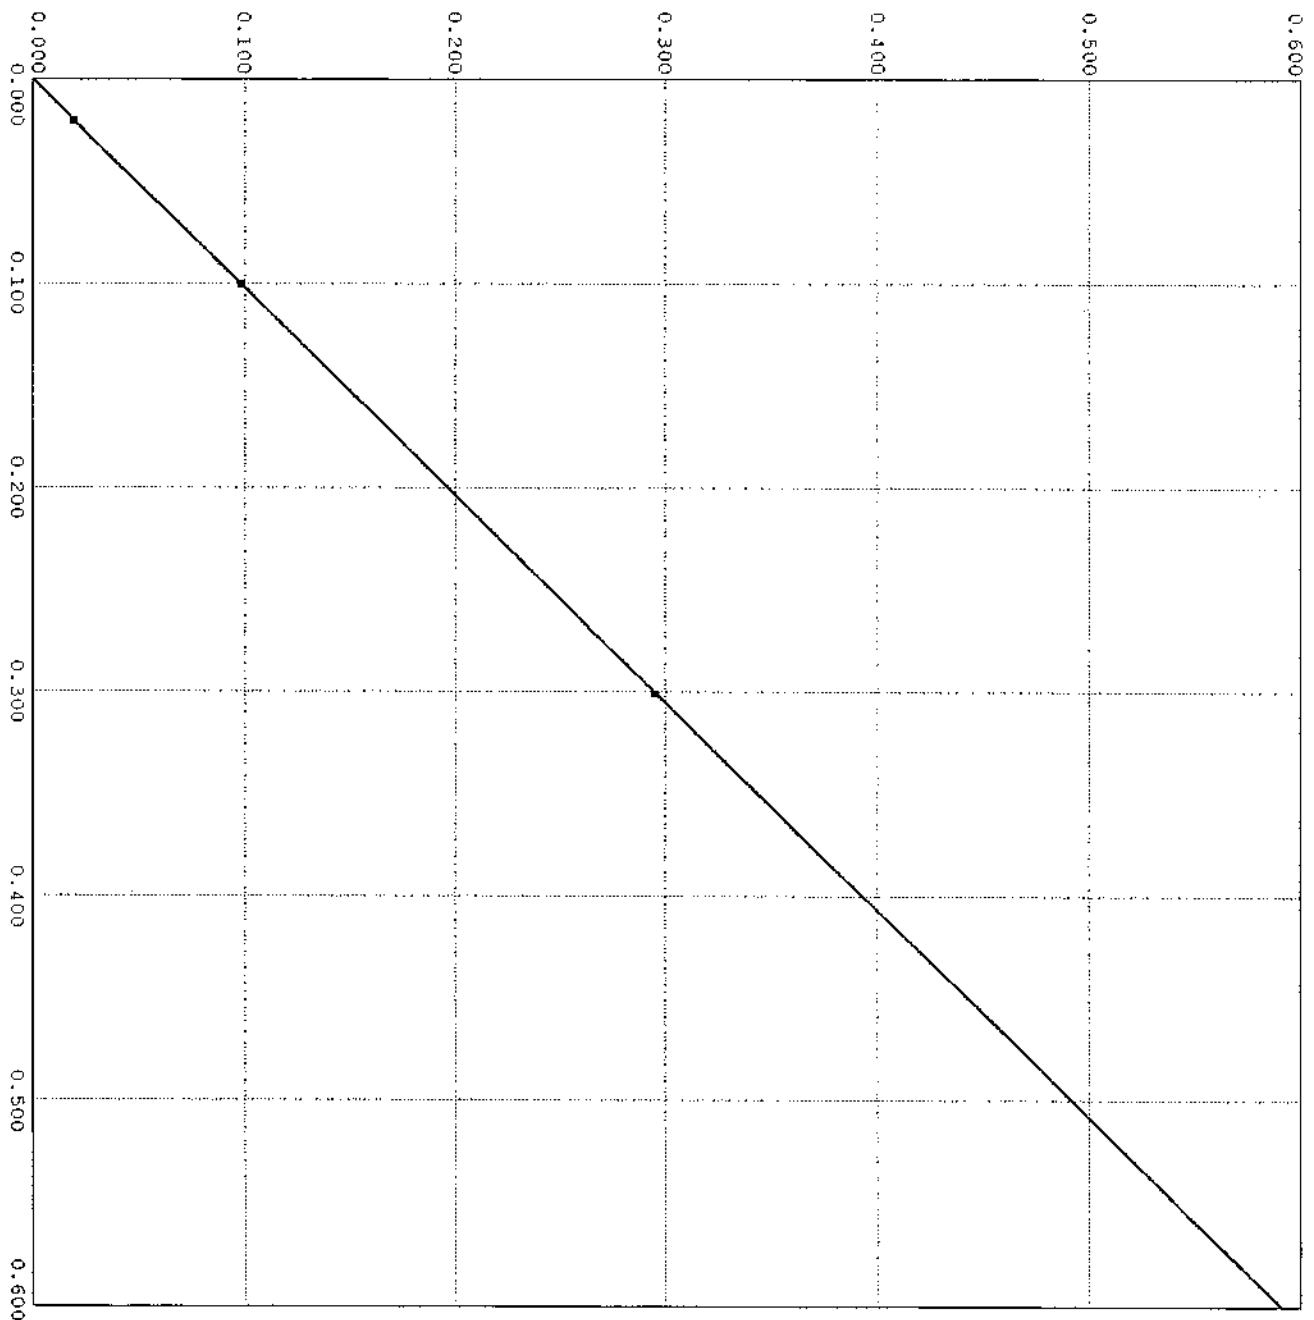

DW

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100671






Date: 05/15/2018
 Time: 09:47:15

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.79: 0.020
 LOT #: AG616504
 EXPIRATION: 06/13/2018
 TANK PRESSURE: 1087 psi

BLANK TEST	0.000	09:48
INTERNAL STANDARD	VERIFIED	09:48
EXTERNAL STANDARD	0.020	09:49
BLANK TEST	0.000	09:50
EXTERNAL STANDARD	0.020	09:50
BLANK TEST	0.000	09:51
EXTERNAL STANDARD	0.020	09:51
BLANK TEST	0.000	09:52
EXTERNAL STANDARD	0.020	09:52
BLANK TEST	0.000	09:53
EXTERNAL STANDARD	0.021	09:53
BLANK TEST	0.000	09:54

Average = 0.0202
 Std Dev = 0.0004

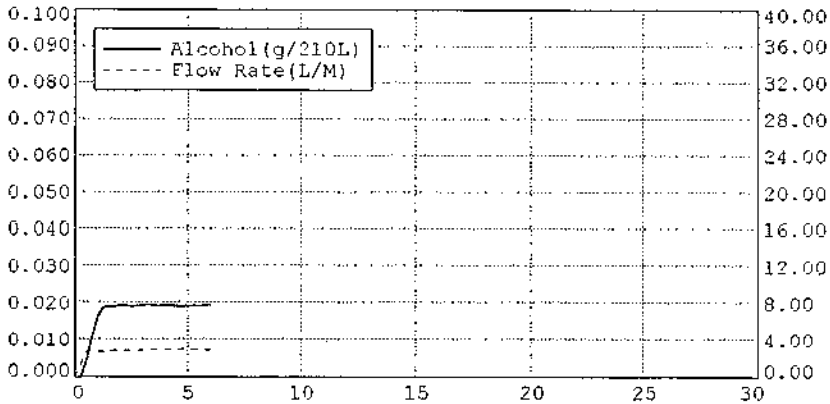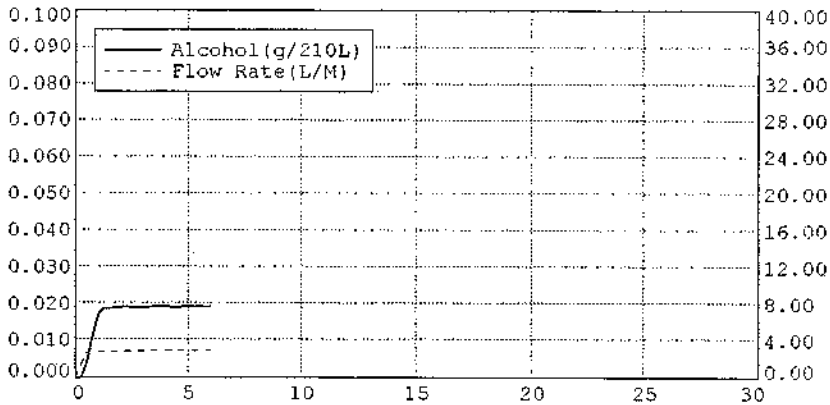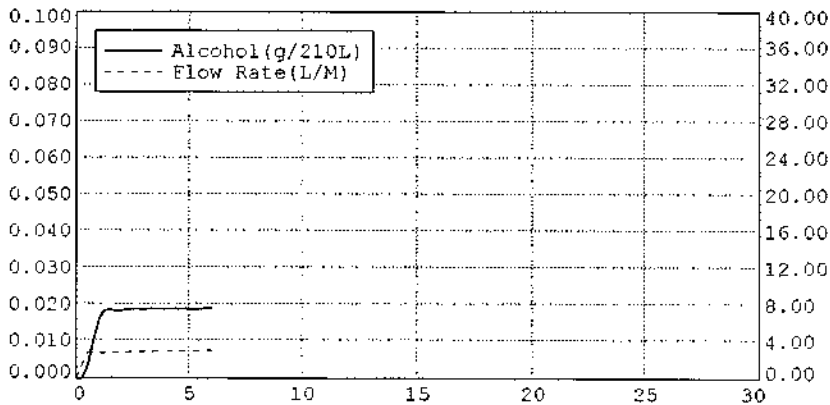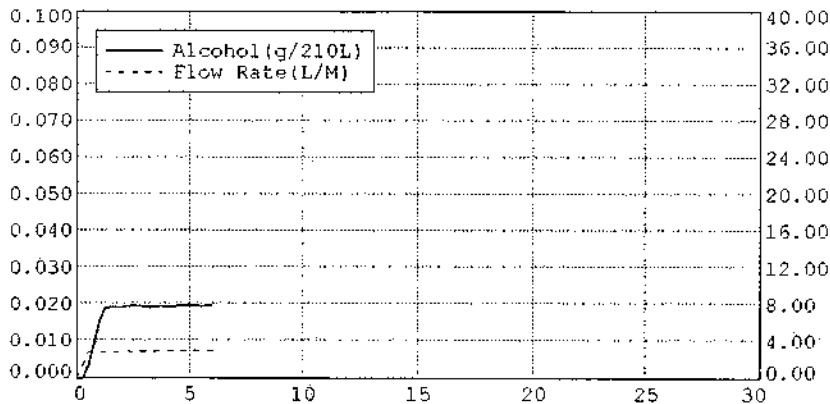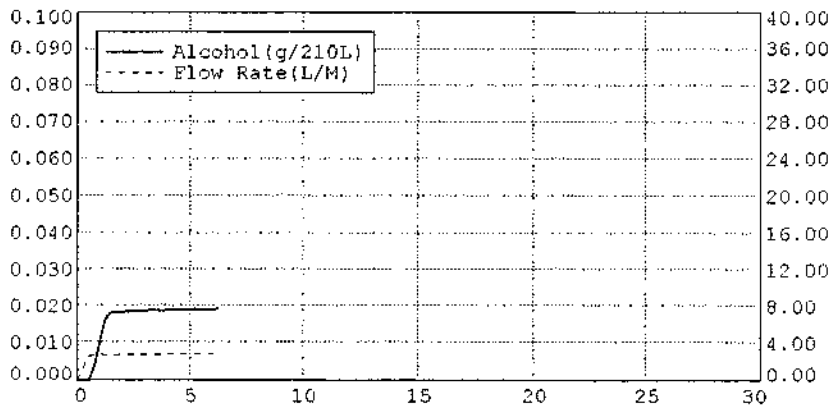

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100671






Date: 05/15/2018
 Time: 09:54:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.79: 0.100
 LOT #: AG629304
 EXPIRATION: 10/19/2018
 TANK PRESSURE: 584 psi

BLANK TEST	0.000	09:56
INTERNAL STANDARD	VERIFIED	09:56
EXTERNAL STANDARD	0.099	09:56
BLANK TEST	0.000	09:57
EXTERNAL STANDARD	0.099	09:57
BLANK TEST	0.000	09:58
EXTERNAL STANDARD	0.099	09:59
BLANK TEST	0.000	09:59
EXTERNAL STANDARD	0.099	10:00
BLANK TEST	0.000	10:01
EXTERNAL STANDARD	0.100	10:01
BLANK TEST	0.000	10:02

Average = 0.0992
 Std Dev = 0.0004

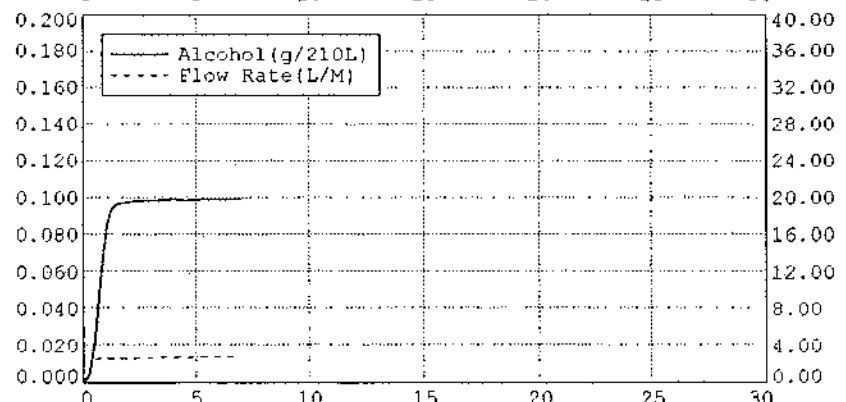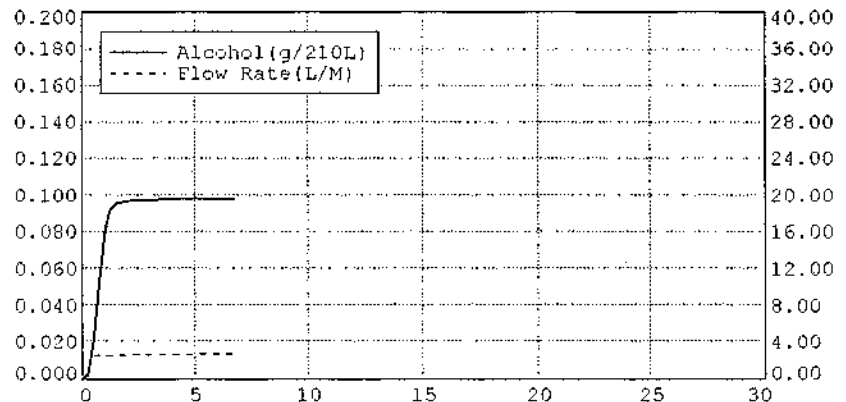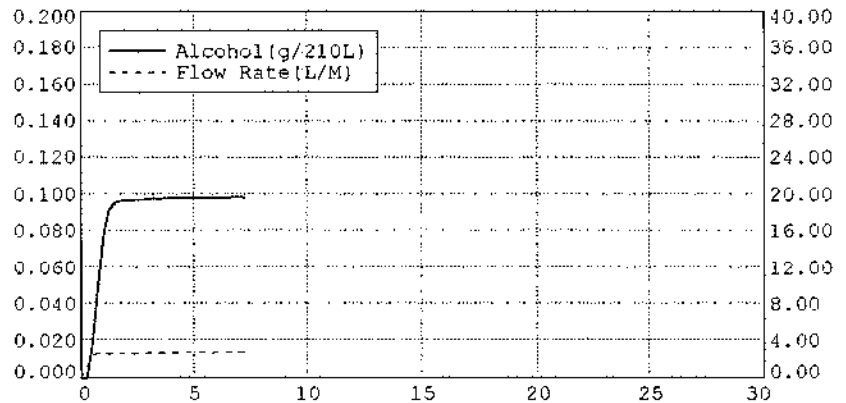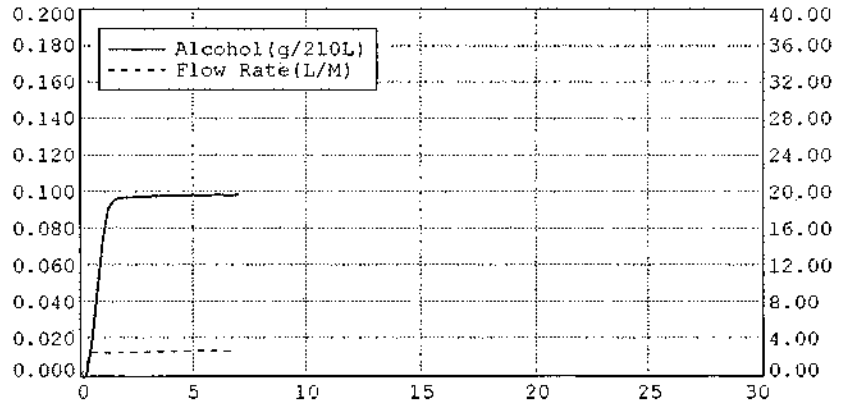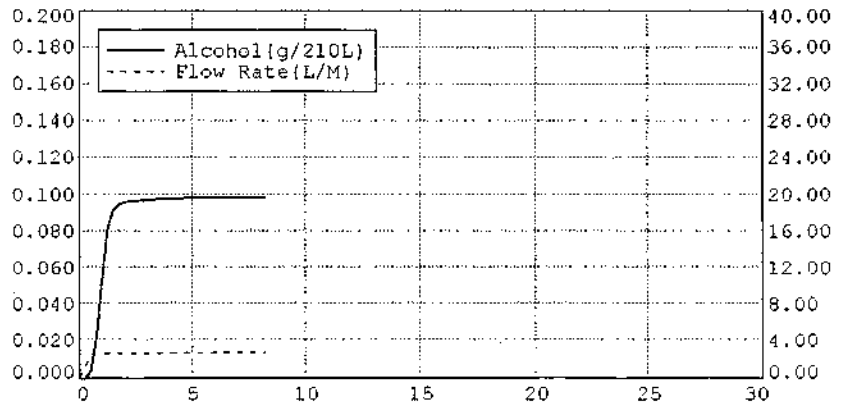

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100671

Date: 05/15/2018
 Time: 10:15:49

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 LOT #: 17140
 EXPIRATION: 05/15/2019

BLANK TEST	0.000	10:17
INTERNAL STANDARD	VERIFIED	10:17
EXTERNAL STANDARD	0.295	10:17
BLANK TEST	0.000	10:18
EXTERNAL STANDARD	0.295	10:19
BLANK TEST	0.000	10:20
EXTERNAL STANDARD	0.296	10:20
BLANK TEST	0.000	10:21
EXTERNAL STANDARD	0.296	10:21
BLANK TEST	0.000	10:22
EXTERNAL STANDARD	0.298	10:23
BLANK TEST	0.000	10:24

Average = 0.2960
 Std Dev = 0.0012

Simulator S/N: SD1202

Calibrated: 01/24/2018

JW 05/15/2018

