

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument  
State of Alaska

Serial #: 100388

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 01/06/2021

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 26.74: 0.071  
LOT #: AG923401  
EXPIRATION: 08/22/2021  
TANK PRESSURE: 1042 psi

BLANK TEST	0.000	09:17
INTERNAL STANDARD	VERIFIED	09:17
EXTERNAL STANDARD	0.071	09:18
BLANK TEST	0.000	09:19
EXTERNAL STANDARD	0.071	09:19
BLANK TEST	0.000	09:20
EXTERNAL STANDARD	0.071	09:20
BLANK TEST	0.000	09:21
EXTERNAL STANDARD	0.071	09:21
BLANK TEST	0.000	09:22
EXTERNAL STANDARD	0.071	09:22
BLANK TEST	0.000	09:23

Average = 0.0710  
Std Dev = 0.0000

## Diagnostic Check

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.7°C PASSED  
Breath Tube = 48.1°C PASSED

### PUMP INFO

Flow Rate = 4.291 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

### FILTER INFO


Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

### INTERNAL STANDARD

PASSED

I, Brandi M. Barnett, after being first duly sworn, depose and state as follows:



- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

 2/4/21

Brandi M. Barnett  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this Feb day of 04, 2021

  
Notary Public  
My Commission Expires With Office

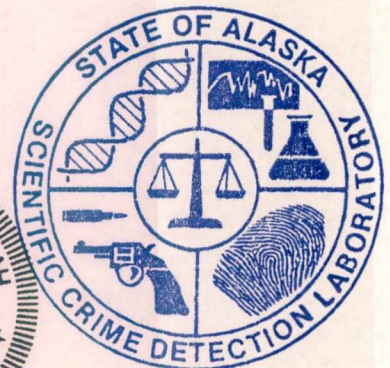

003 1/18/21