



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100343

Report Issue Date: 12/05/2024
Date Received: 2024-05-06
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.079	AG335202	0.079	0.079	0.079	0.078	0.079	0.079	0.079
0.300	0.295	AG327804	0.303	0.303	0.303	0.302	0.304	0.303	0.303

As Found - Evaluation Analyst: Colleen O'Bryant
 As Found Conditions - Barometric Pressure (inHg): 29.29 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.5 Relative Humidity (%): 29
 As-Found Lab Activity Date Range: 05/06/2024 - 05/07/2024

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.019	AG408002	0.020	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.039	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.077	AG335202	0.078	0.078	0.078	0.078	0.078	0.078	0.078	+/- 0.004
0.100	0.096	AG333401	0.098	0.098	0.098	0.098	0.099	0.098	0.098	+/- 0.004
0.150	0.145	AG332004	0.146	0.145	0.145	0.145	0.145	0.145	0.145	+/- 0.006
0.300	0.289	AG427706	0.298	0.297	0.297	0.297	0.296	0.297	0.297	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 28.86 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.8 Relative Humidity (%): 19
 As-Left Lab Activity Date Range: 11/07/2024 - 11/07/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Kaija Swisher on 12/04/2024

kaija.swisher@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 12/05/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 160343 Analyst or Technician Name: Kaja Swisher

DataMaster DMT Calibration Start Date: 11/7/24

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: 5/2/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 28.86 Temperature(C) 21.8 Relative Humidity(%) 19
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20241107KS Expiration Date: 2/7/25
Simulator S/N: DR4161 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20241107KS Expiration Date: 2/7/25
Simulator S/N: DR5298 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 23IP41233 Expiration Date: 2/7/25
Simulator S/N: DR4163 Thermometer Verification Performed?

The second exp date is
09/20/2025
KS 12/2/24

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 9/19/25

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 11/7/24
Data Interpretation Date (Technician): NA (if applicable)
Data Interpretation Date (Analyst): 11/7/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 09:25:32

VERSIONS
DMT: 3.02
PIC: 3.06
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 43.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.84 V PASSED
(1.10 V - 2.58 V)
Cooler Voltage = 1.78 V PASSED
(1.07 V - 2.49 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 533 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 28.8 in

PUMP INFO

Flow Rate = 4.123 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.091 0.48% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 9:58 AM

Temperatures (°C)

Sample Cell: 49.1°C
Breath Tube: 43.1°C

Current Barometer 28.9 in
Volume (Ltr) 1.41

Settings

Lamp: 1.89 V
Bias: 80 V
Cooler: 1.68 V
Chopper: 532 Hz

Voltages (V)

Flow: 1.05 V
Detector: 0.055 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/06/2024
Time: 14:11:28

OPERATOR NAME:
KAIJA SWISHER
CERTIFICATE #: 10746

Ca = 0.1000
CAL = 0.989777 0.800 <= CAL < 1.200
b1 = 0.0004 0.0000 <= b1 < 0.0040
b2 = 0.0053 0.0010 <= b2 < 0.0100
b3 = 0.0004 0.0000 <= b3 < 0.0040
Xq = 0.0918 0.0500 <= Xq < 0.2000
a21 = 1.158225 1.050 <= a21 < 1.300
a31 = 0.507724 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 10:05:09

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.86: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:08
BLANK TEST	0.000	10:08
INTERNAL STANDARD	VERIFIED	10:08
EXTERNAL STANDARD	0.078	10:08
BLANK TEST	0.000	10:09
SUBJECT SAMPLE (Vol=1.53L)	0.000	10:10
BLANK TEST	0.000	10:11
EXTERNAL STANDARD	0.078	10:11
BLANK TEST	0.000	10:12

KS

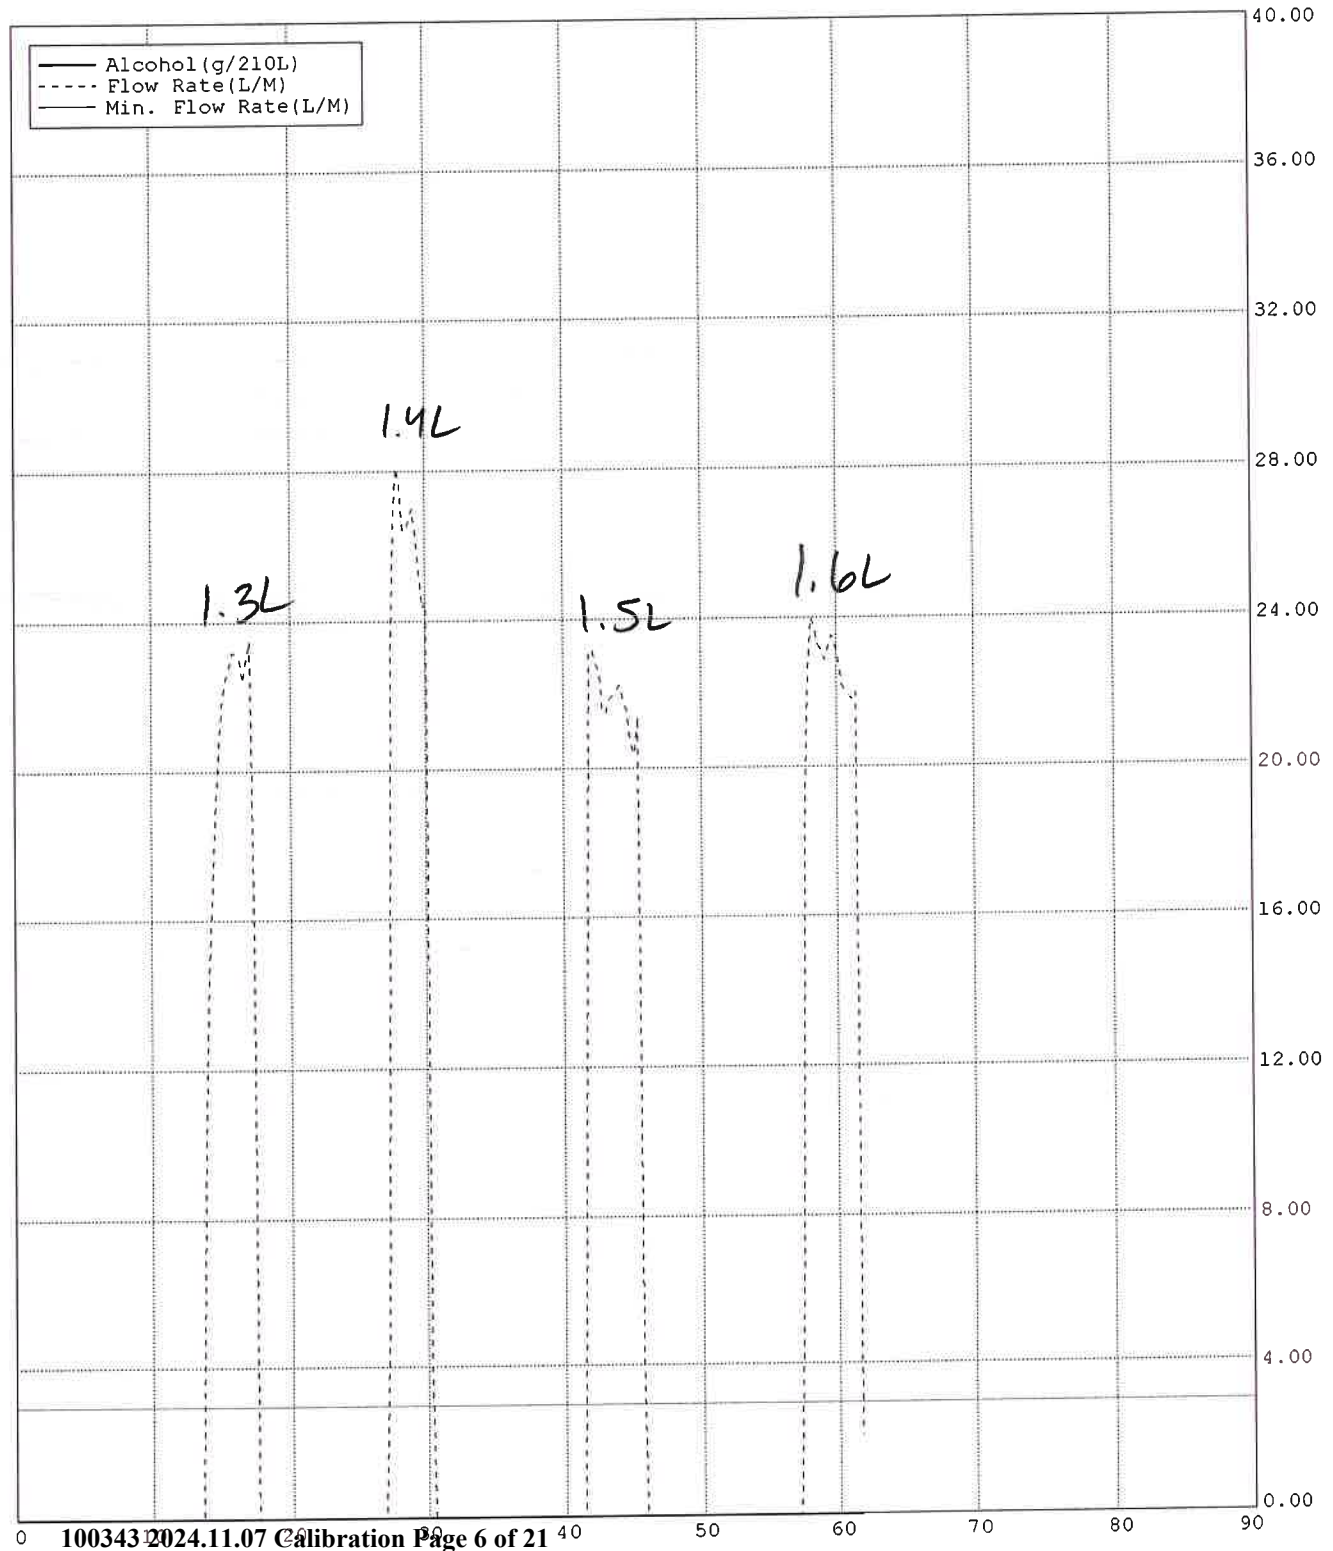

LINEARITY CHECK

Alaska Department of Public Safety
DATAMASTER dmt: 100343


Date: 11/07/2024
Time: 10:22:39

SUPERVISOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.019	0.0200	0.0000
0.039	0.0390	0.0000
0.077	0.0780	0.0000
0.096	0.0982	0.0004
0.145	0.1452	0.0004
0.289	0.2970	0.0007

SLOPE = 1.026612
R² = 0.999775

KS

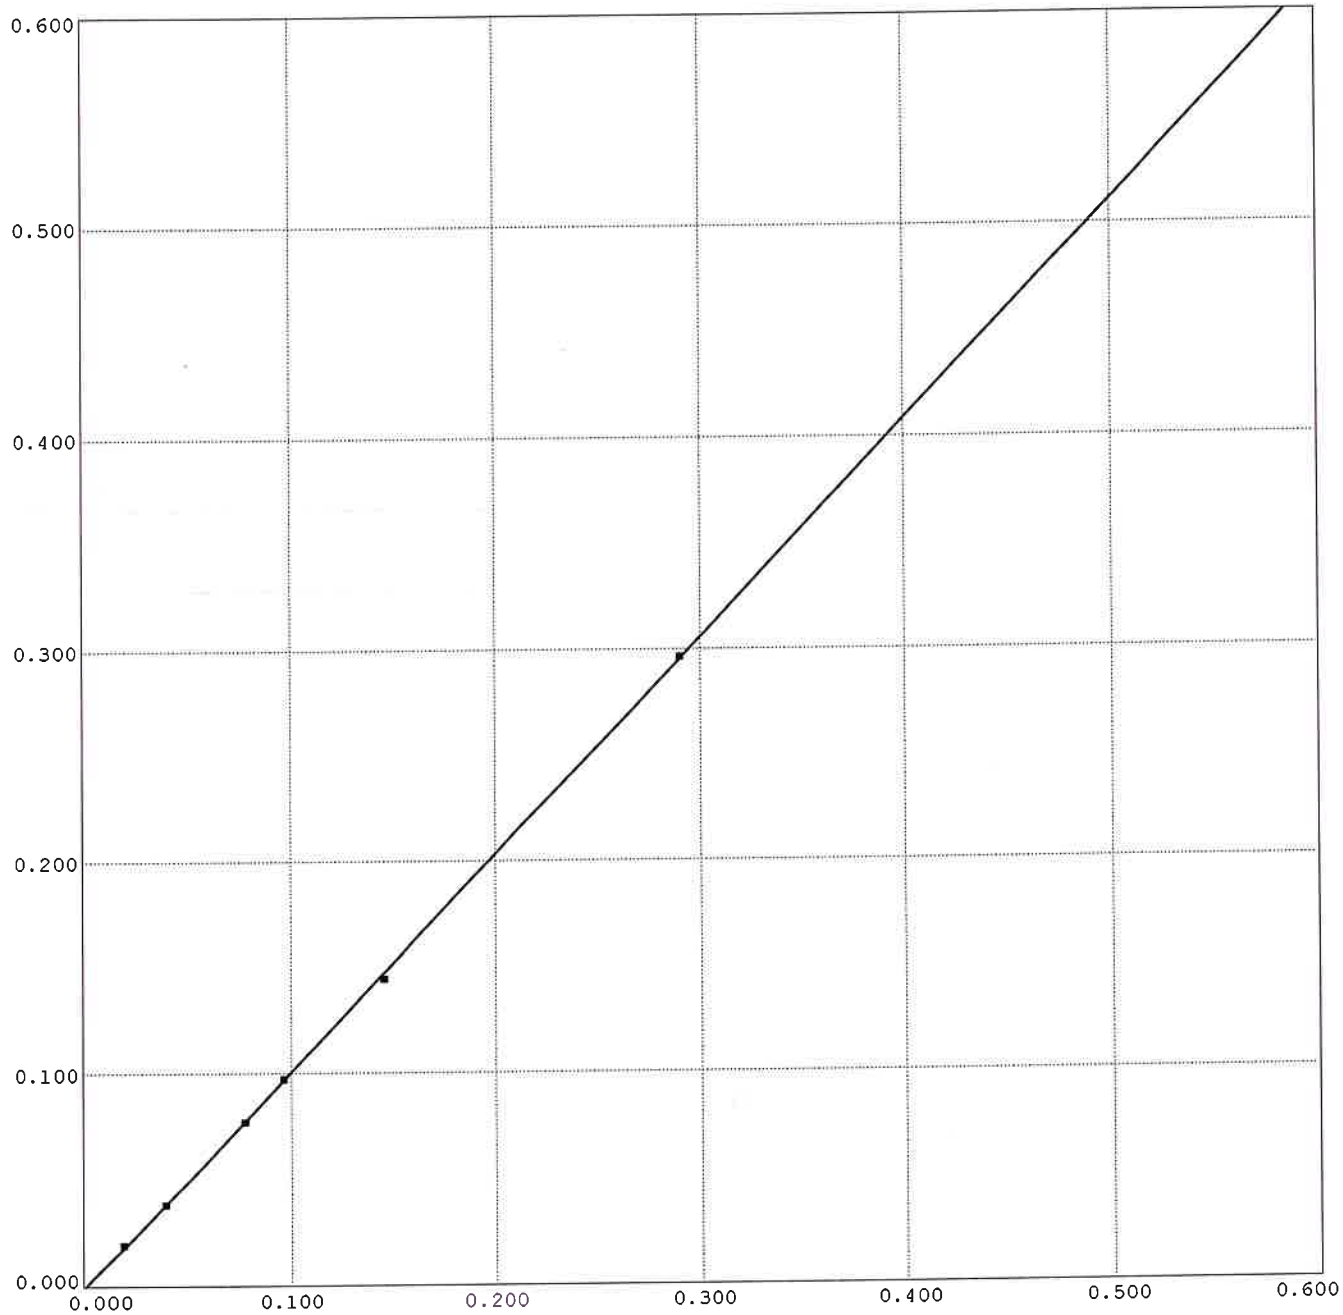

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100343






Date: 11/07/2024
 Time: 10:22:41

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 28.85: 0.019
 LOT #: AG408002
 EXPIRATION: 03/20/2026
 TANK PRESSURE: 348 psi

BLANK TEST	0.000	10:24
INTERNAL STANDARD	VERIFIED	10:25
EXTERNAL STANDARD	0.020	10:25
BLANK TEST	0.000	10:26
EXTERNAL STANDARD	0.020	10:26
BLANK TEST	0.000	10:27
EXTERNAL STANDARD	0.020	10:27
BLANK TEST	0.000	10:28
EXTERNAL STANDARD	0.020	10:28
BLANK TEST	0.000	10:29
EXTERNAL STANDARD	0.020	10:29
BLANK TEST	0.000	10:30

Average = 0.0200
 Std Dev = 0.0000

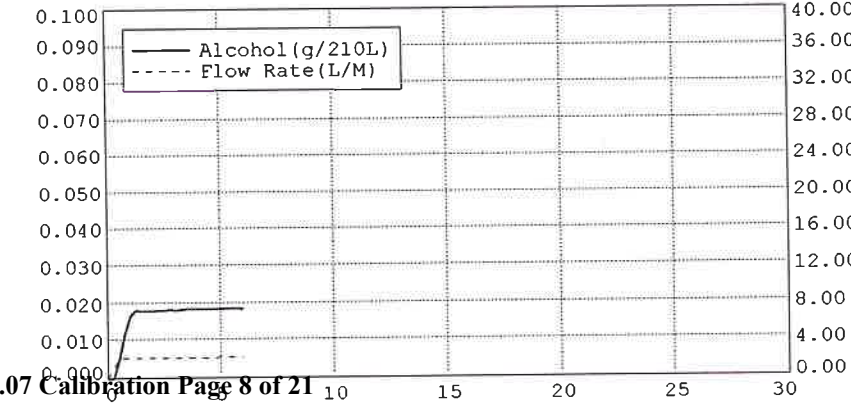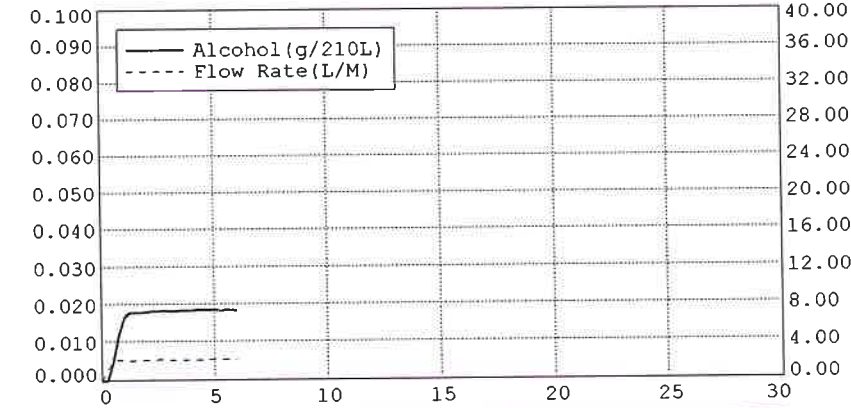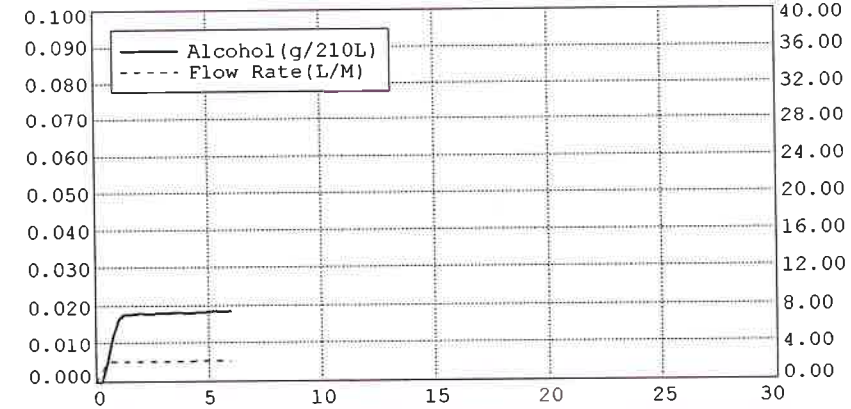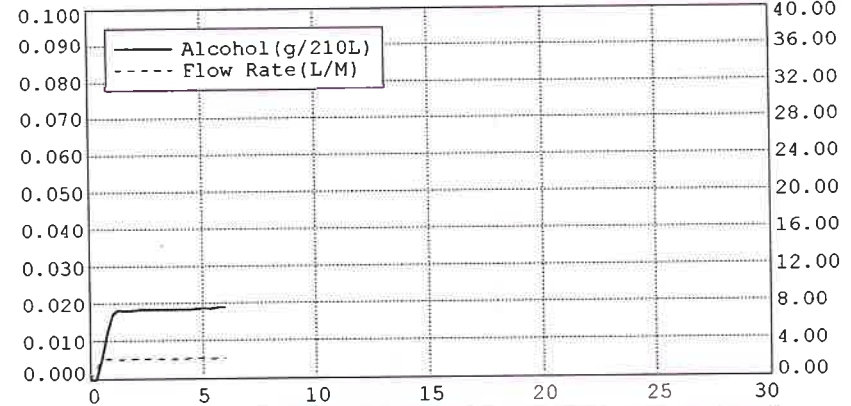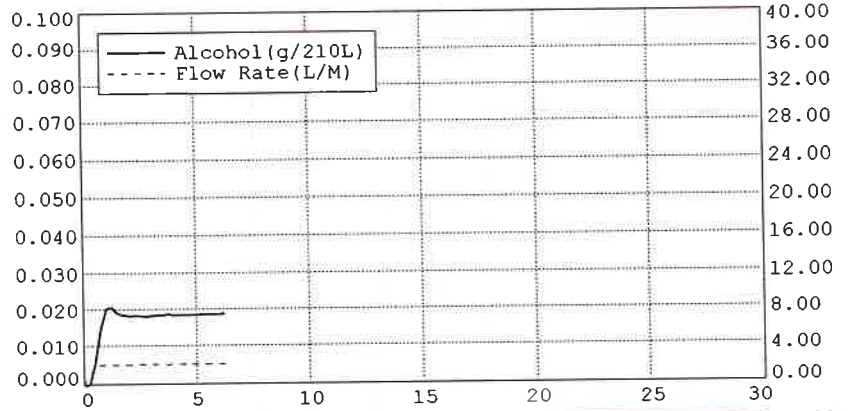

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100343






Date: 11/07/2024
Time: 10:31:35

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 28.85: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 1006 psi

BLANK TEST	0.000	10:33
INTERNAL STANDARD	VERIFIED	10:33
EXTERNAL STANDARD	0.039	10:33
BLANK TEST	0.000	10:34
EXTERNAL STANDARD	0.039	10:34
BLANK TEST	0.000	10:35
EXTERNAL STANDARD	0.039	10:35
BLANK TEST	0.000	10:36
EXTERNAL STANDARD	0.039	10:36
BLANK TEST	0.000	10:37
EXTERNAL STANDARD	0.039	10:37
BLANK TEST	0.000	10:38

Average = 0.0390
Std Dev = 0.0000

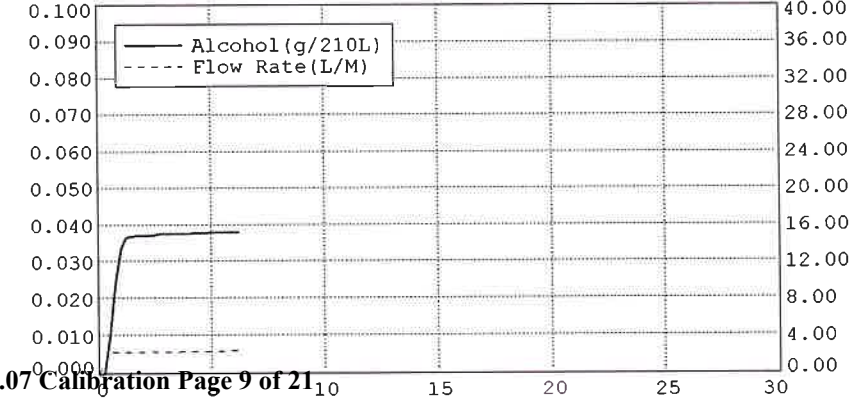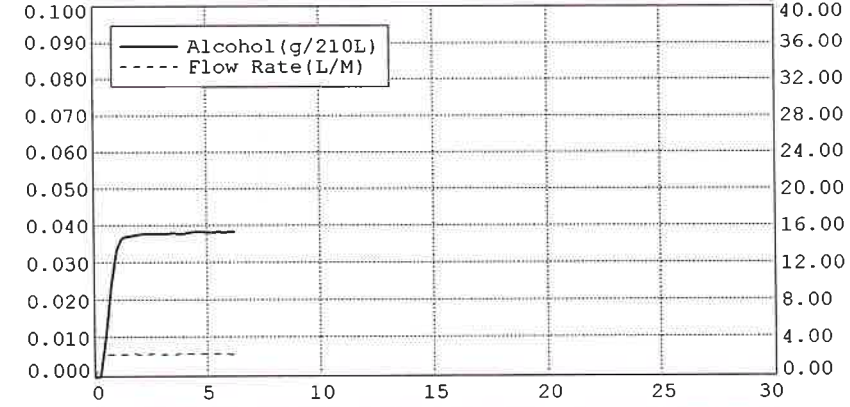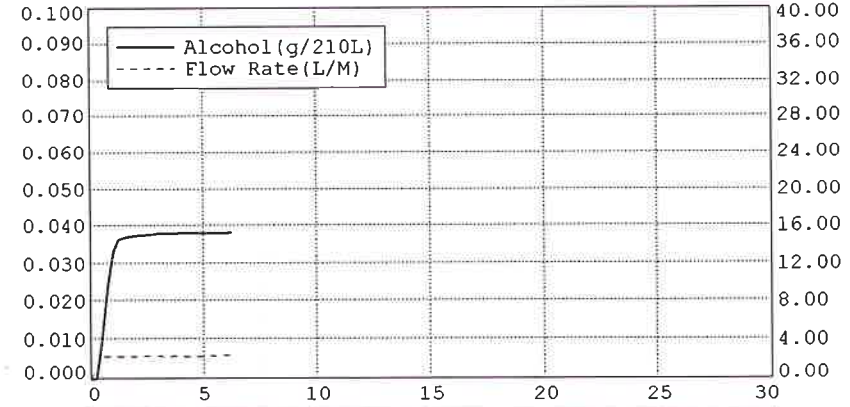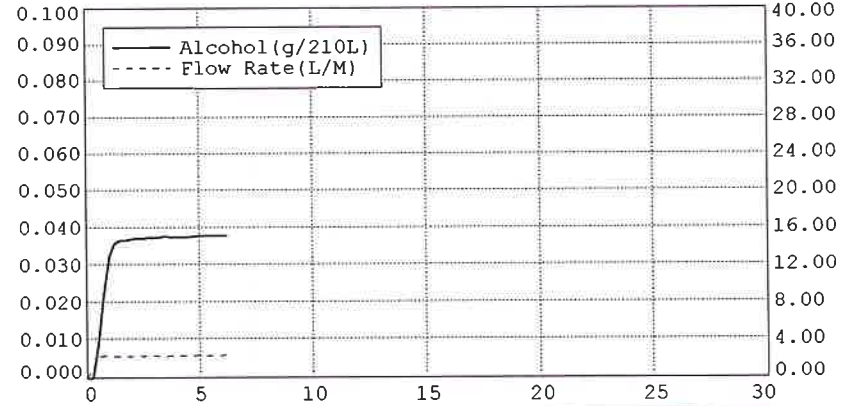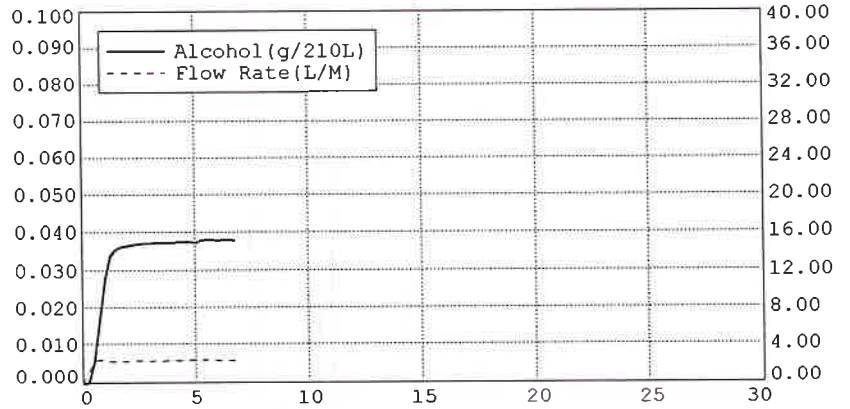

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100343






Date: 11/07/2024
 Time: 10:40:02

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 28.85: 0.077
 LOT #: AG335202
 EXPIRATION: 12/18/2025
 TANK PRESSURE: 779 psi

BLANK TEST	0.000	10:41
INTERNAL STANDARD	VERIFIED	10:41
EXTERNAL STANDARD	0.078	10:41
BLANK TEST	0.000	10:42
EXTERNAL STANDARD	0.078	10:42
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.078	10:44
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.078	10:45
BLANK TEST	0.000	10:46
EXTERNAL STANDARD	0.078	10:46
BLANK TEST	0.000	10:47

Average = 0.0780
 Std Dev = 0.0000

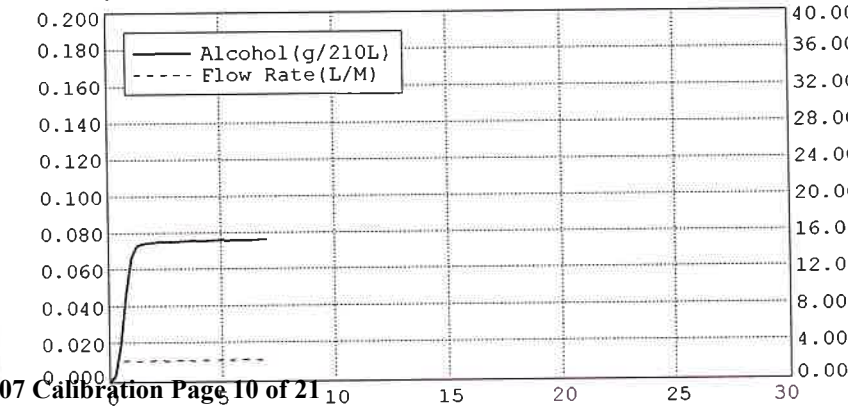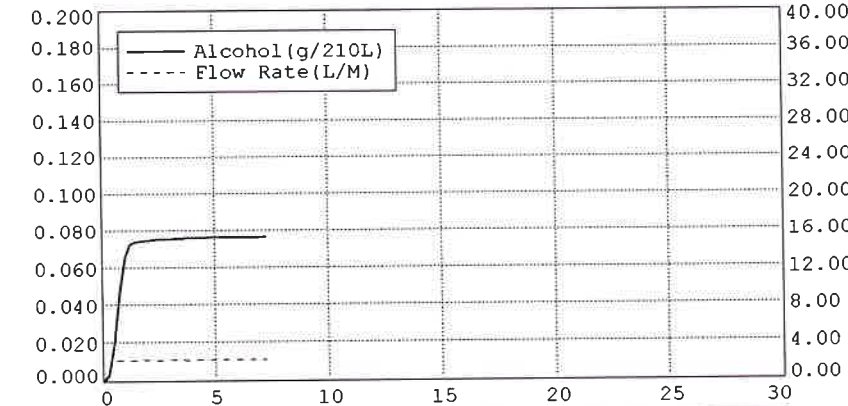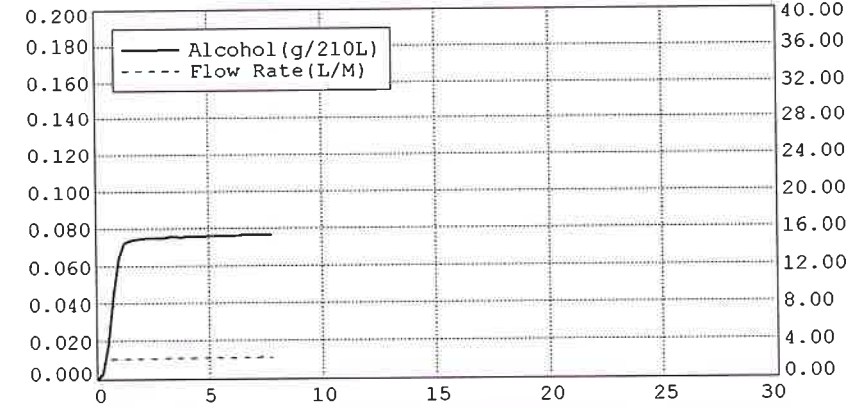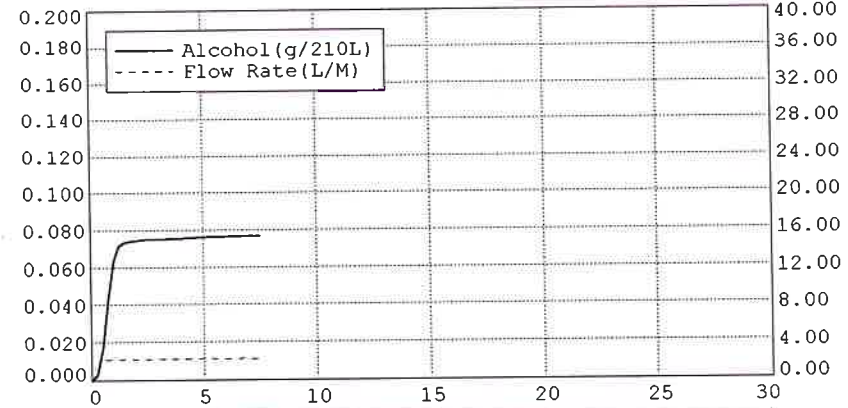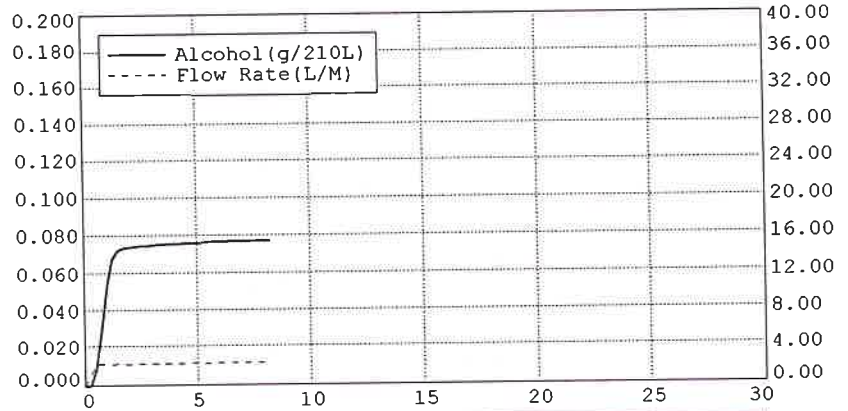

LINEARITY CHECK: Control Test 4






Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 10:49:31

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.100
TARGET AT 28.85: 0.096
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 976 psi

BLANK TEST	0.000	10:50
INTERNAL STANDARD	VERIFIED	10:51
EXTERNAL STANDARD	0.098	10:51
BLANK TEST	0.000	10:52
EXTERNAL STANDARD	0.098	10:52
BLANK TEST	0.000	10:53
EXTERNAL STANDARD	0.098	10:53
BLANK TEST	0.000	10:54
EXTERNAL STANDARD	0.098	10:54
BLANK TEST	0.000	10:55
EXTERNAL STANDARD	0.099	10:55
BLANK TEST	0.000	10:56

Average = 0.0982
Std Dev = 0.0004

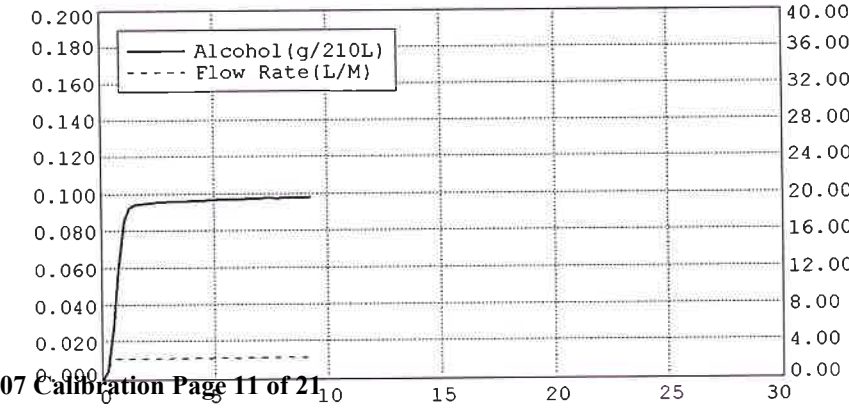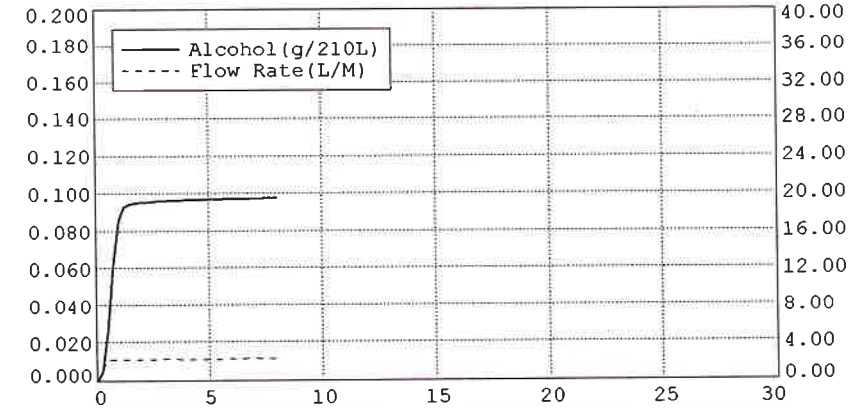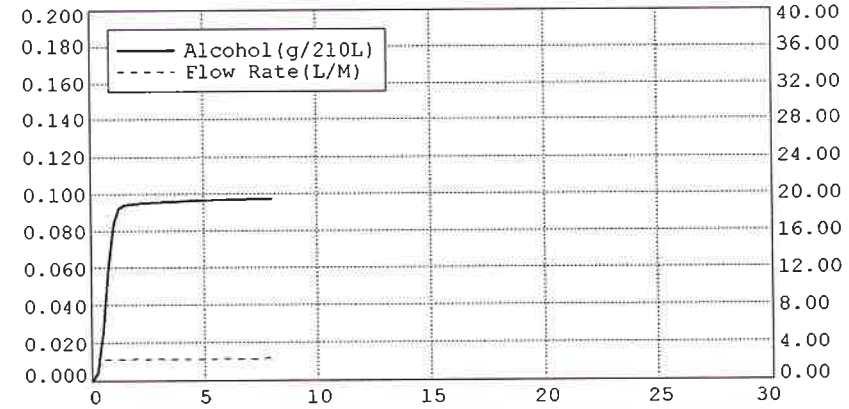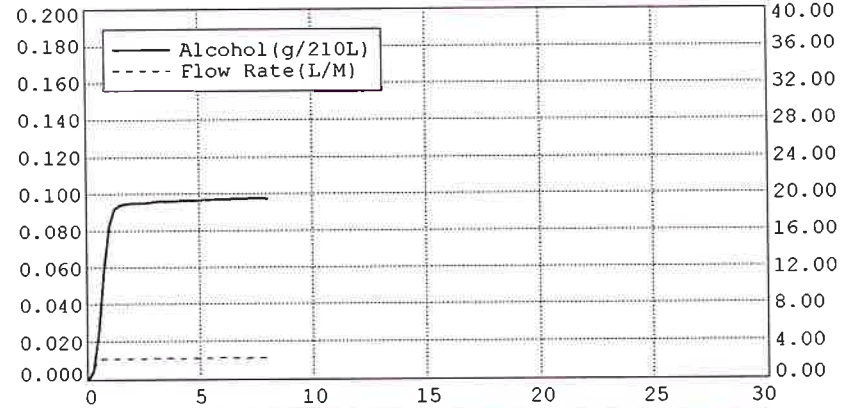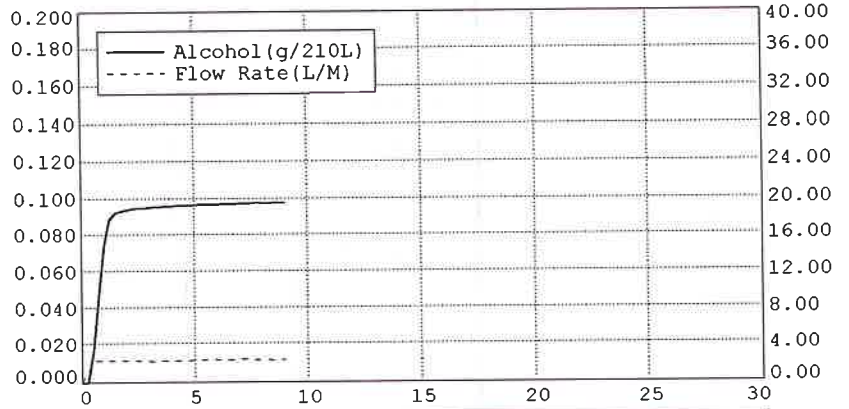

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100343






Date: 11/07/2024
 Time: 10:58:57

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 28.86: 0.145
 LOT #: ~~AG332044~~ AG332004 KS11/08/2024
 EXPIRATION: 11/16/2025
 TANK PRESSURE: 457 psi

BLANK TEST	0.000	11:00
INTERNAL STANDARD	VERIFIED	11:00
EXTERNAL STANDARD	0.146	11:00
BLANK TEST	0.000	11:01
EXTERNAL STANDARD	0.145	11:01
BLANK TEST	0.000	11:02
EXTERNAL STANDARD	0.145	11:03
BLANK TEST	0.000	11:04
EXTERNAL STANDARD	0.145	11:04
BLANK TEST	0.000	11:05
EXTERNAL STANDARD	0.145	11:05
BLANK TEST	0.000	11:06

Average = 0.1452
 Std Dev = 0.0004

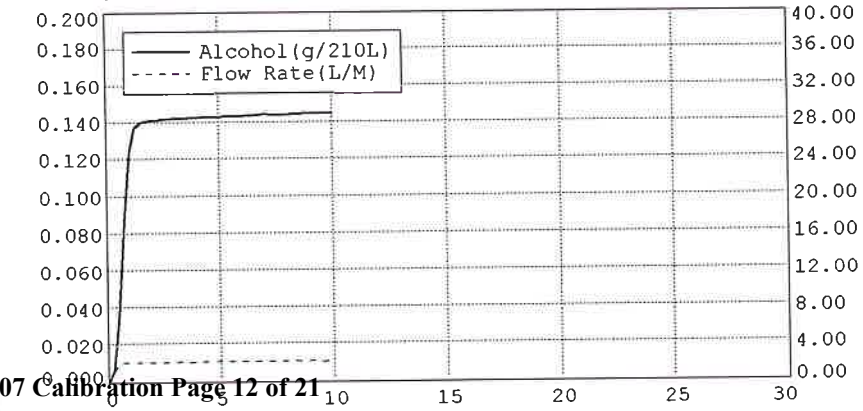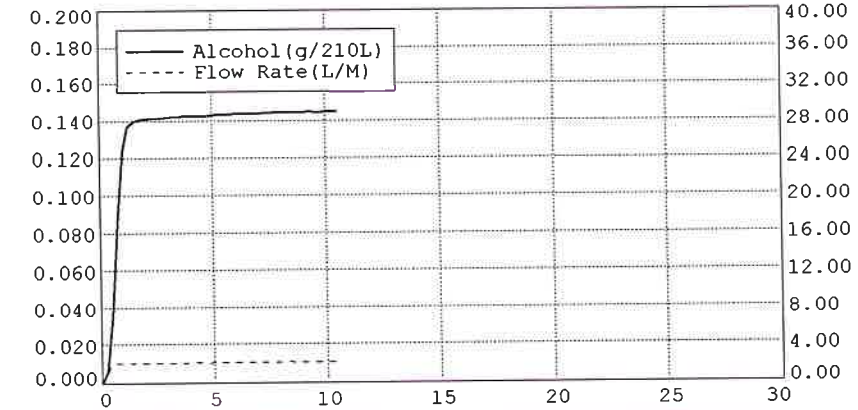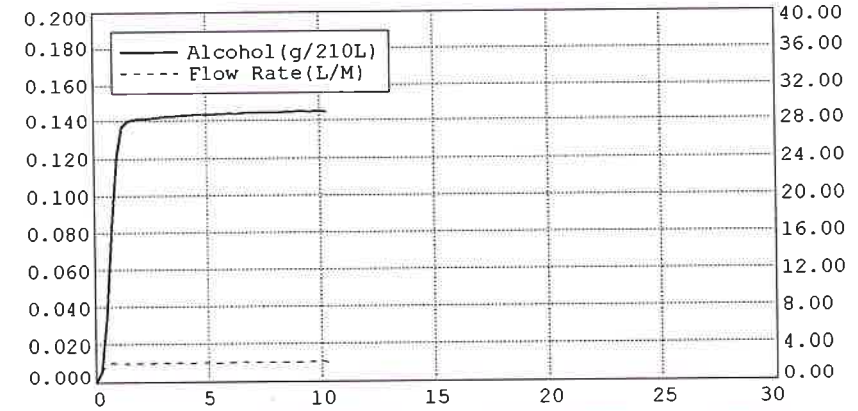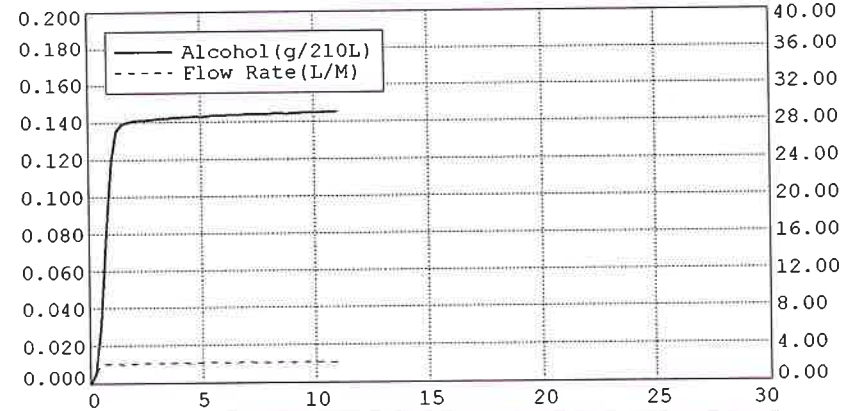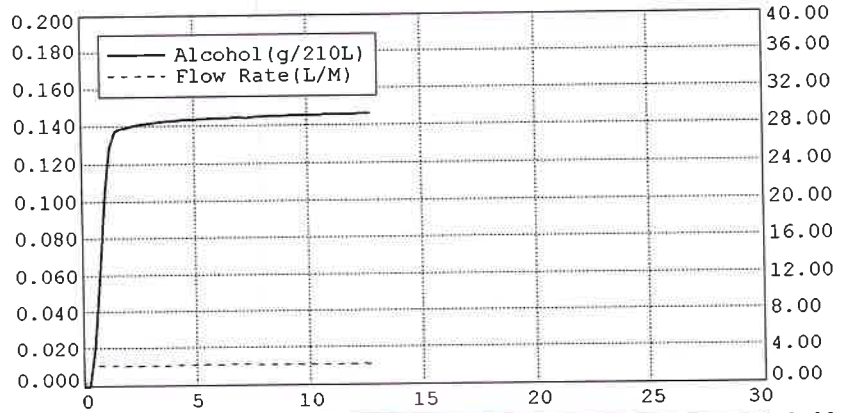

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100343






Date: 11/07/2024
 Time: 11:07:54

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 28.85: 0.289
 LOT #: AG427706
 EXPIRATION: 10/03/2026
 TANK PRESSURE: 389 psi

BLANK TEST	0.000	11:09
INTERNAL STANDARD	VERIFIED	11:09
EXTERNAL STANDARD	0.298	11:10
BLANK TEST	0.000	11:11
EXTERNAL STANDARD	0.297	11:11
BLANK TEST	0.000	11:12
EXTERNAL STANDARD	0.297	11:13
BLANK TEST	0.000	11:14
EXTERNAL STANDARD	0.297	11:14
BLANK TEST	0.000	11:15
EXTERNAL STANDARD	0.296	11:16
BLANK TEST	0.000	11:17

Average = 0.2970
 Std Dev = 0.0007

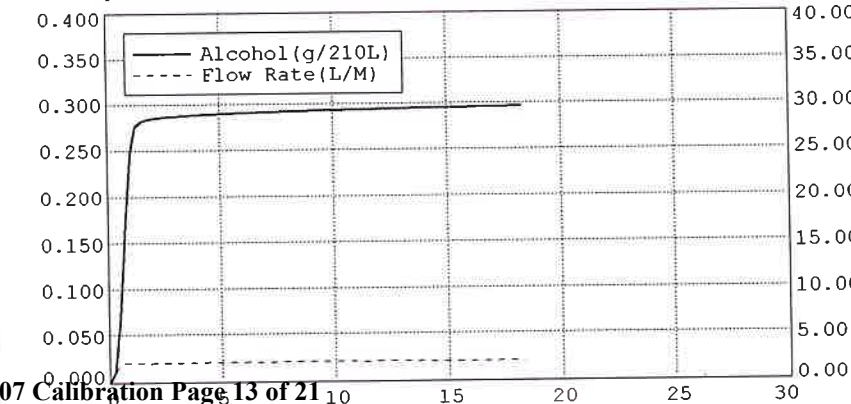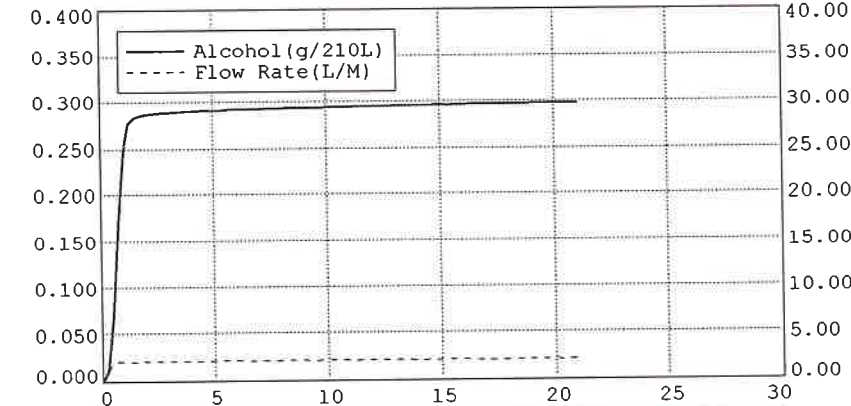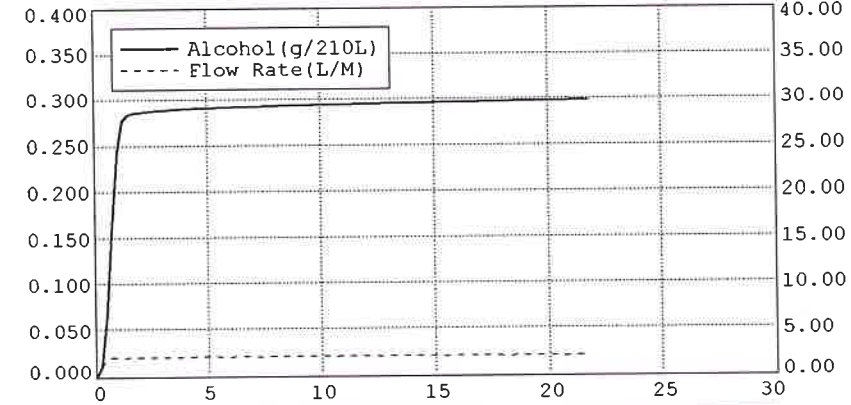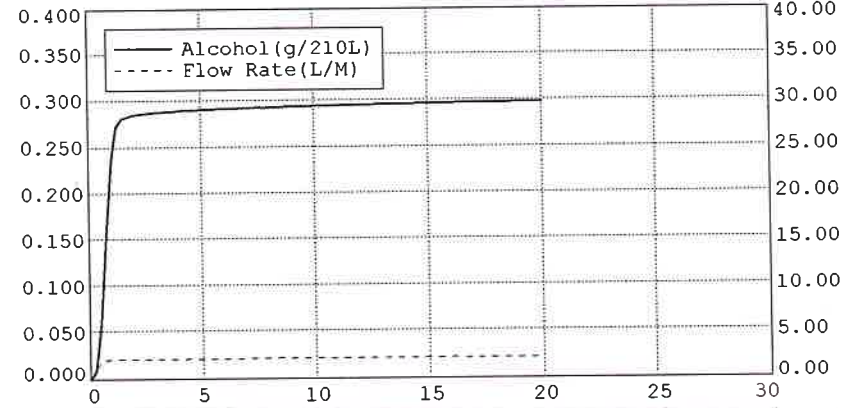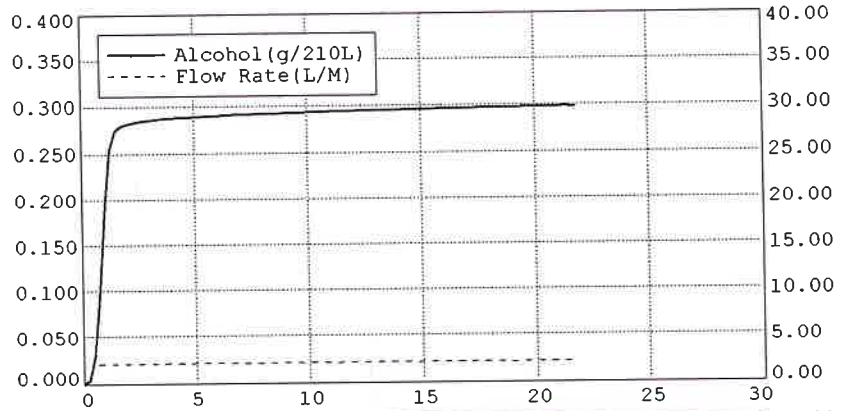

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 11:23:16

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.85: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:24
BLANK TEST	0.000	11:24
INTERNAL STANDARD	VERIFIED	11:24
EXTERNAL STANDARD	0.078	11:24
BLANK TEST	0.000	11:25
SUBJECT SAMPLE	INCOMPLETE	11:27

KS

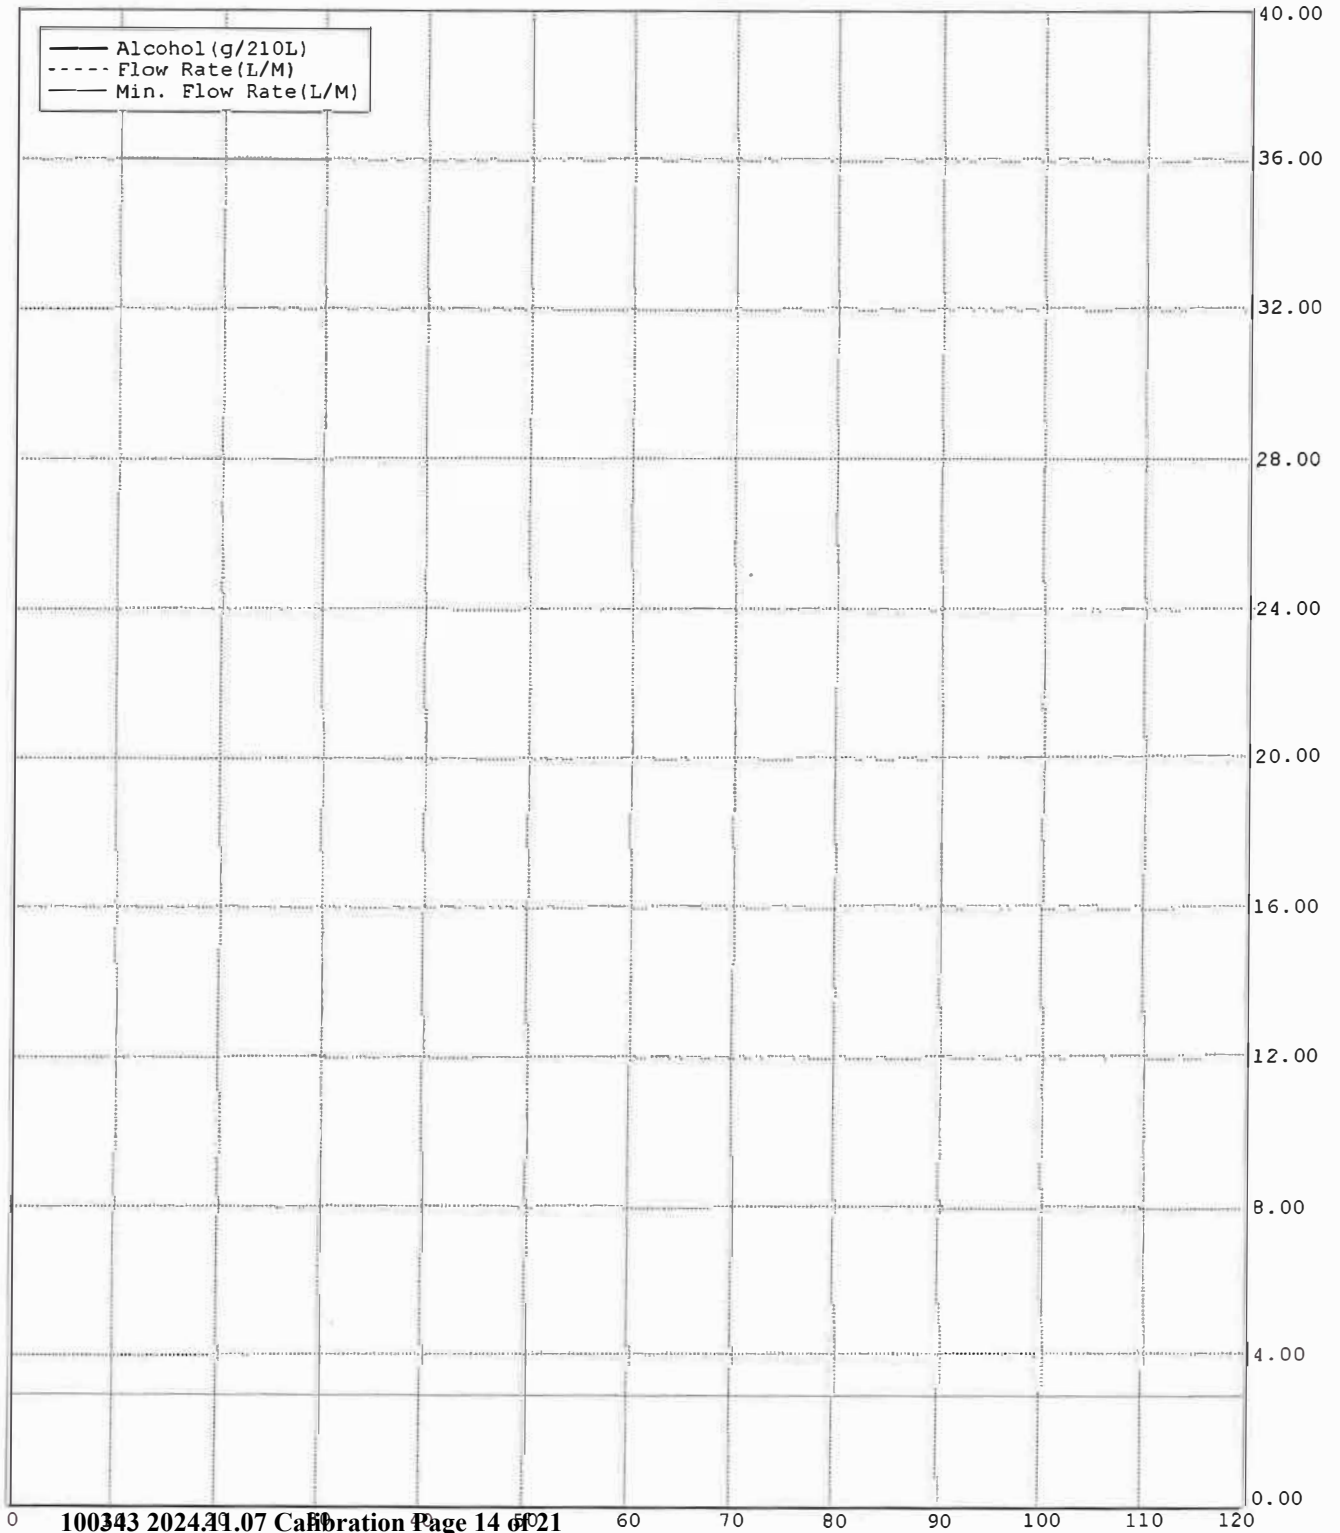

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 11:29:27

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
MAX ATTEMPTS
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.85: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:30
BLANK TEST	0.000	11:30
INTERNAL STANDARD	VERIFIED	11:30
EXTERNAL STANDARD	0.078	11:30
BLANK TEST	0.000	11:31
SUBJECT SAMPLE	XXX	11:32

Maximum Attempts Exceeded

KS

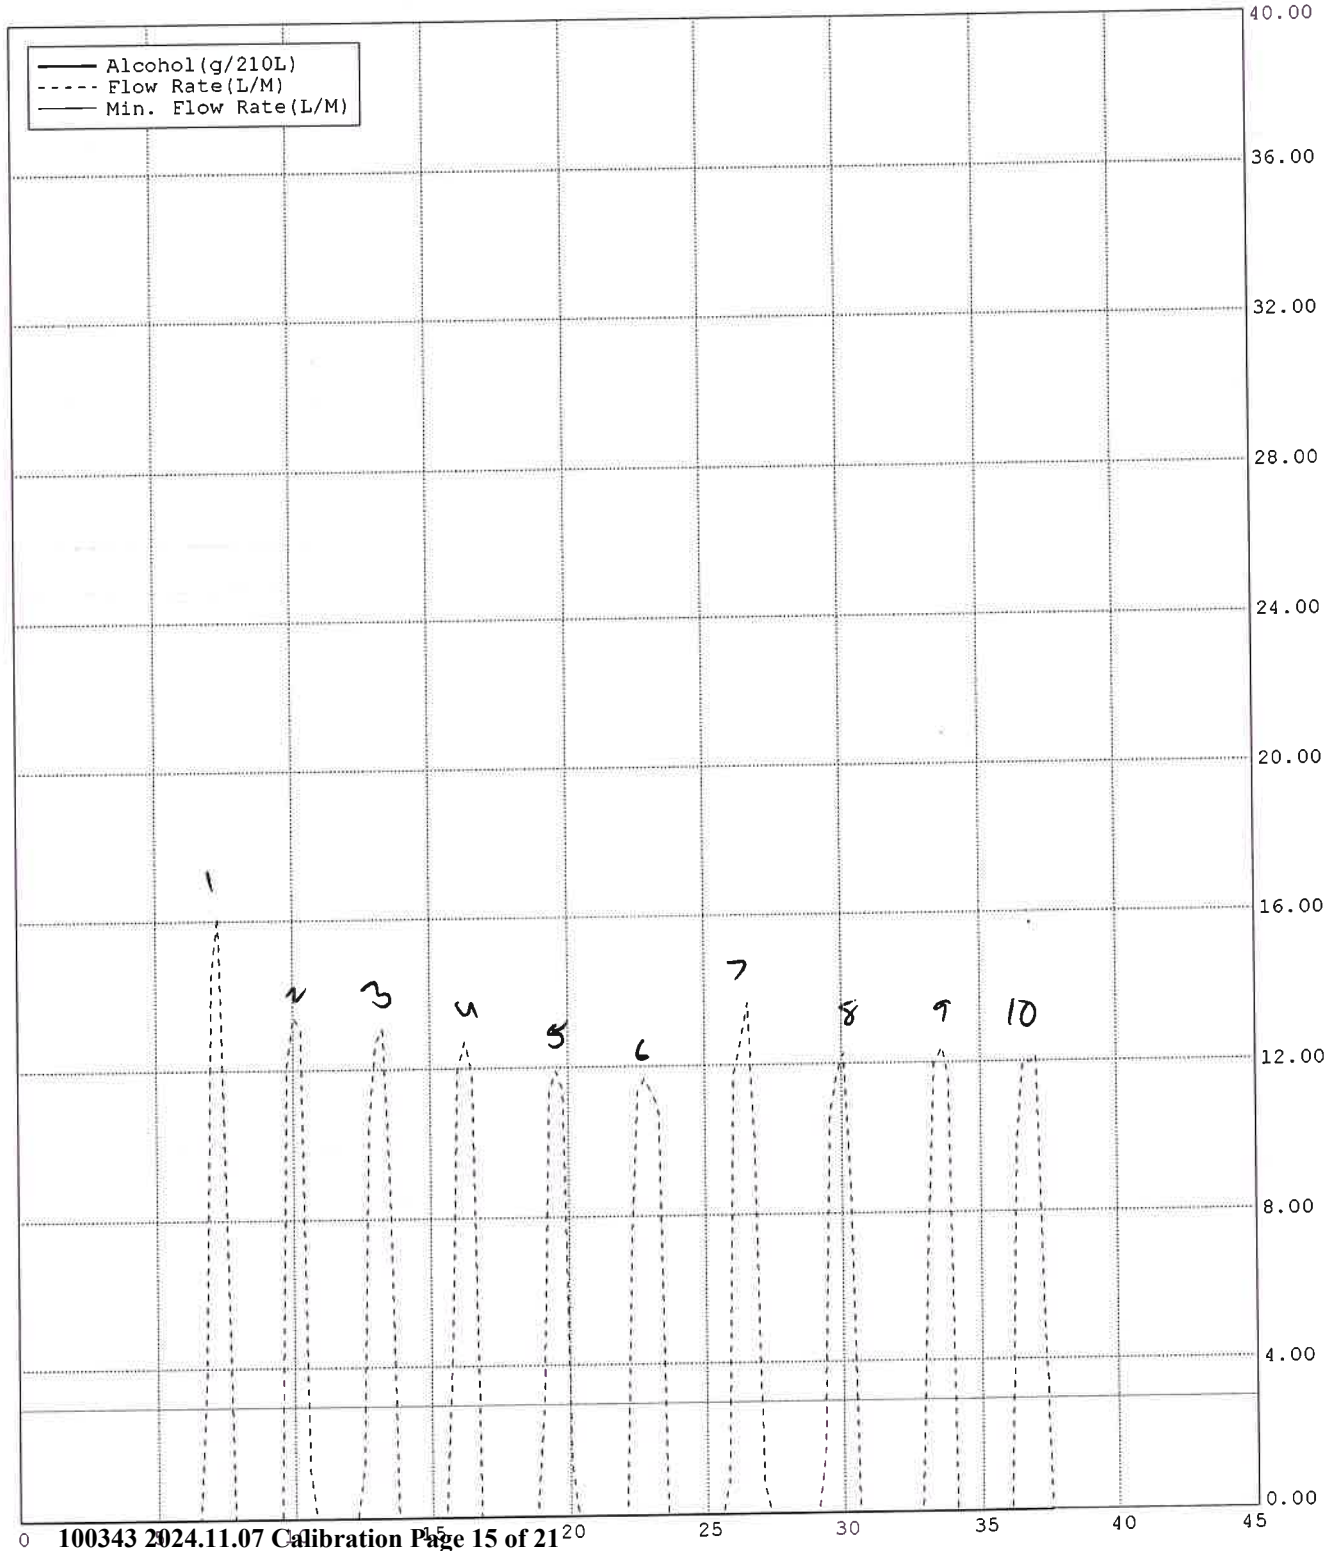

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 11:41:59

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.85: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:44
BLANK TEST	0.000	11:44
INTERNAL STANDARD	VERIFIED	11:44
EXTERNAL STANDARD	0.078	11:44
BLANK TEST	0.000	11:45
SUBJECT SAMPLE	INVALID	11:46

KS

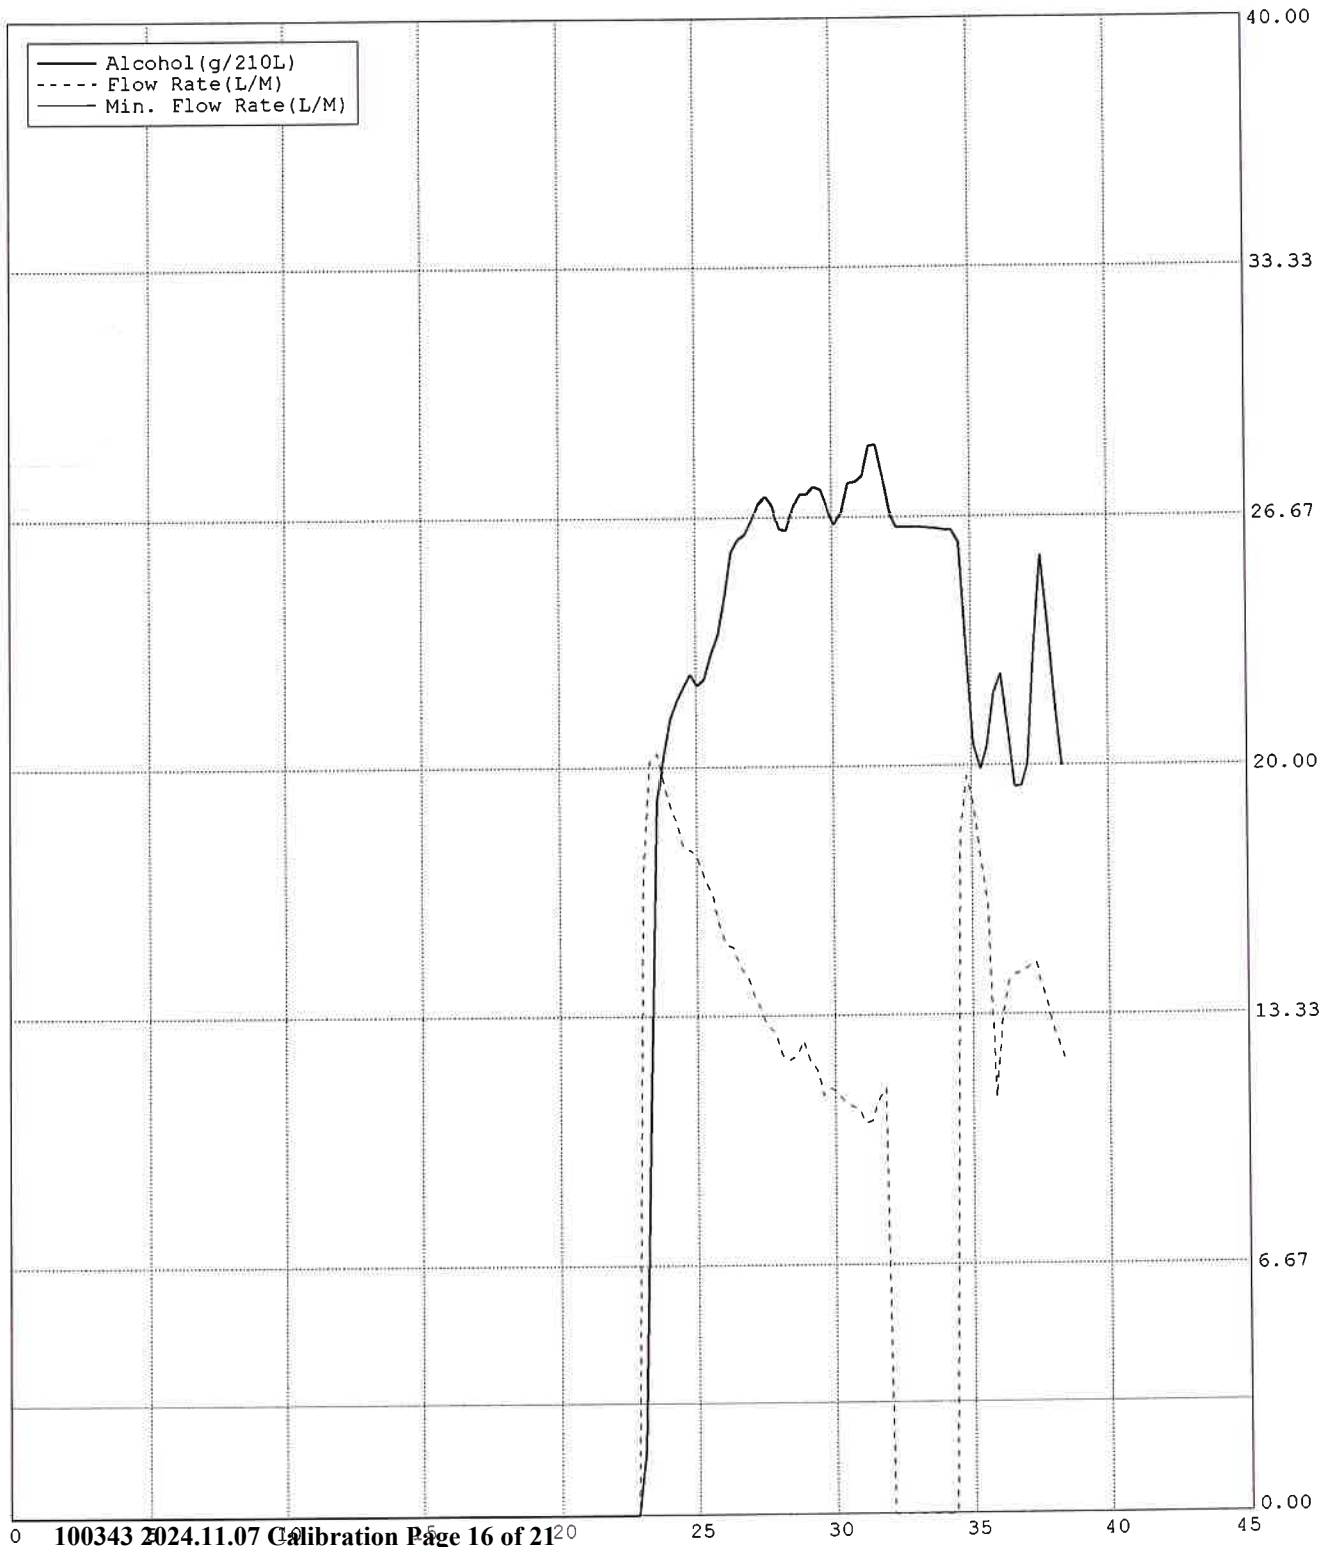

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 11:49:21

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.85: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:51
BLANK TEST	0.000	11:51
INTERNAL STANDARD	VERIFIED	11:51
EXTERNAL STANDARD	0.078	11:51
BLANK TEST	0.000	11:52

RFI DETECTED

KS

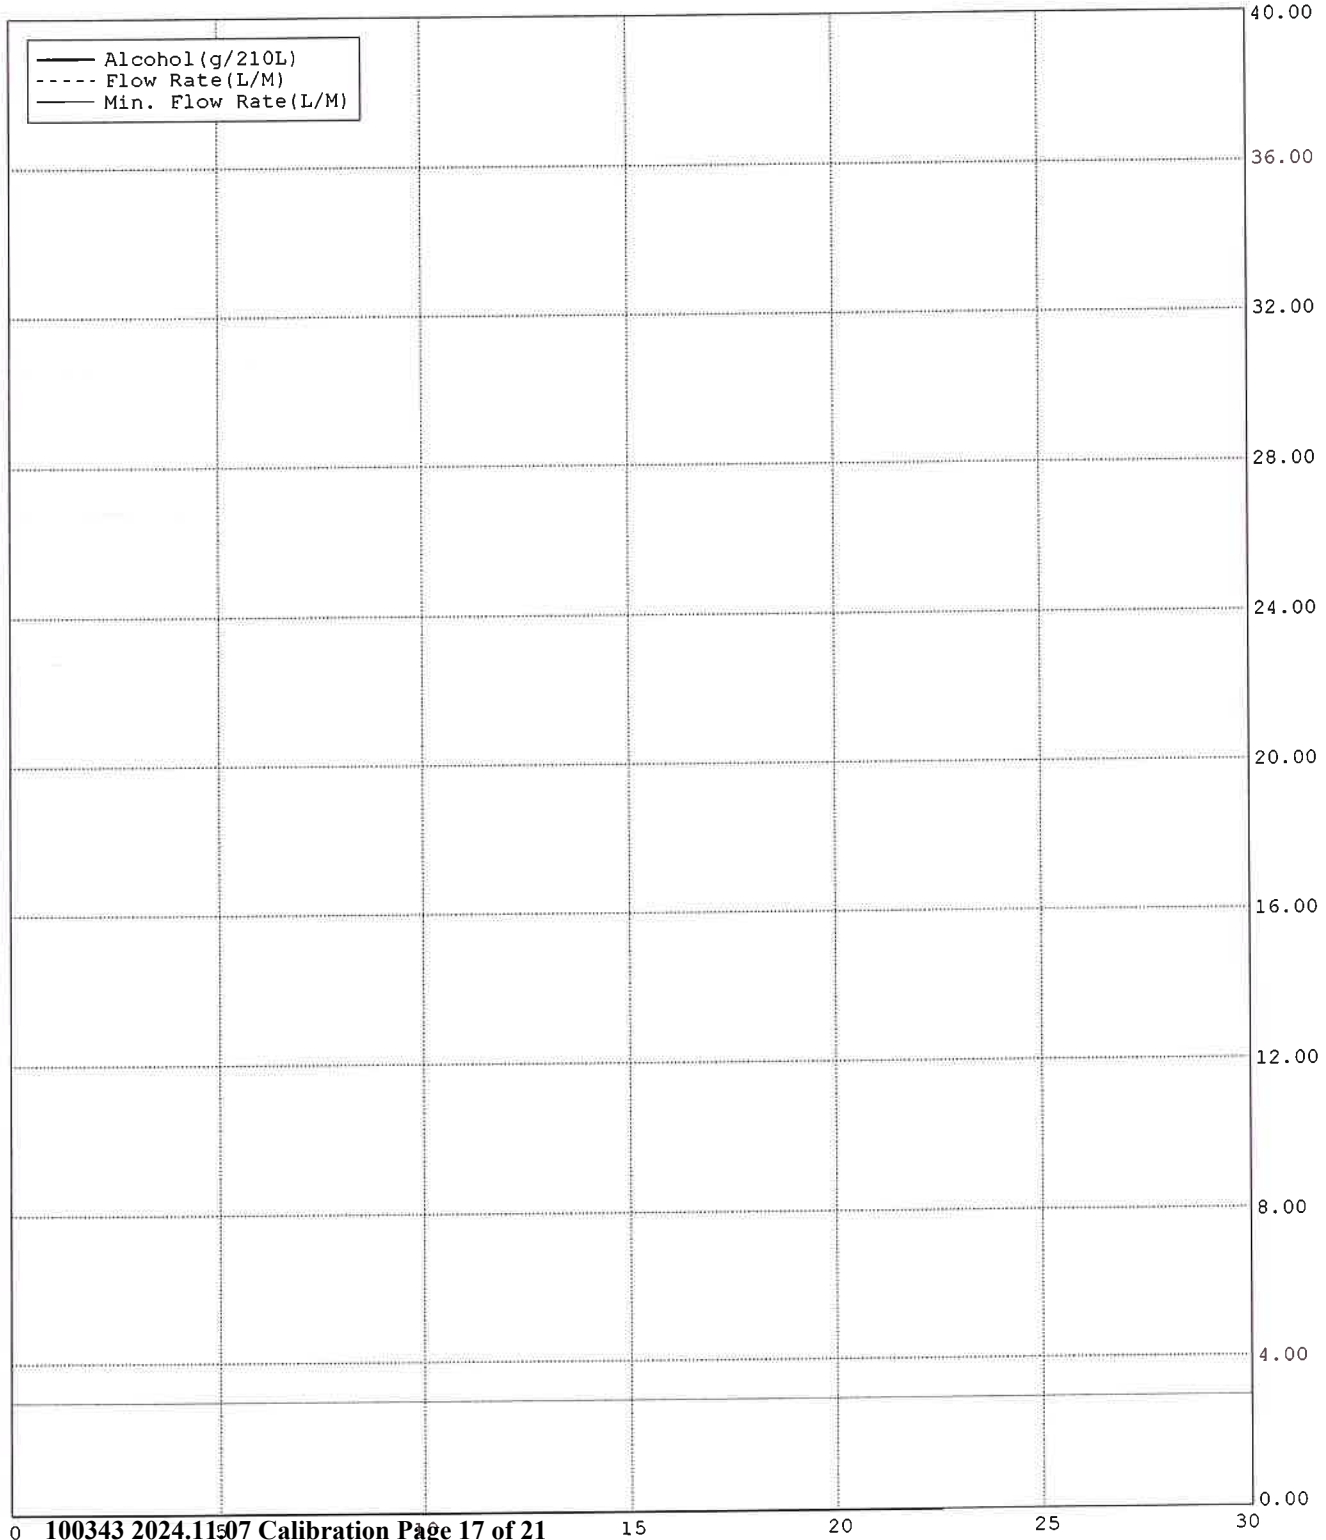

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 12:59:22

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.83: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:00
BLANK TEST	0.000	13:00
INTERNAL STANDARD	VERIFIED	13:00
X _q = 0.092 (0.00%)		
EXTERNAL STANDARD	0.078	13:00
X[1] = 0.0781 (-0.0008) (0.0020)		
BLANK TEST	0.000	13:01
SUBJECT SAMPLE	XXX	13:02
X[1] = 0.1165 (-0.0213) (0.0014)		

Interference Detected


KS 12/4/2024
-0.0007

Filter 2 average is ~~-0.007~~

Filter 3 average is 0.0014

KS 11/7/24

KS

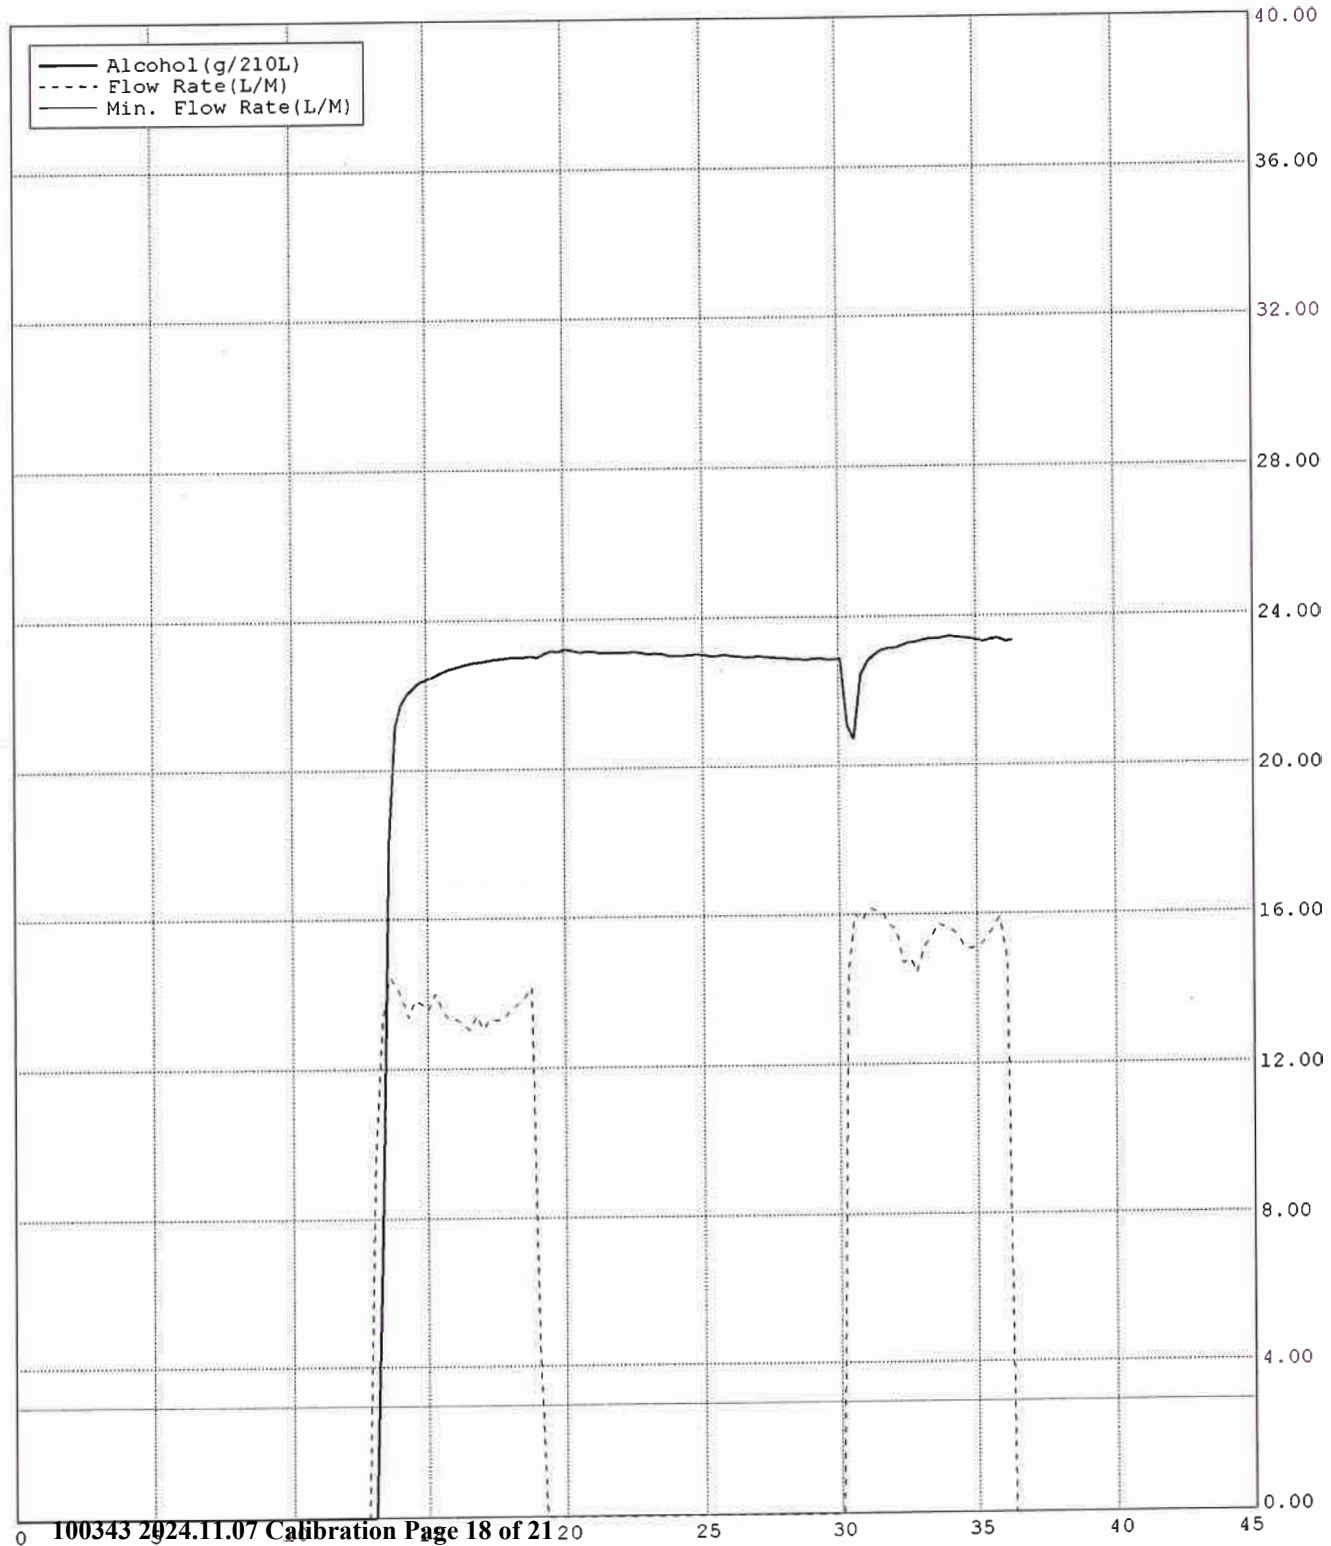

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 13:04:38

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.83: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:05
BLANK TEST	0.000	13:05
INTERNAL STANDARD	VERIFIED	13:05
Xq = 0.092 (0.67%)		
EXTERNAL STANDARD	0.079	13:06
X[1] = 0.0788 (-0.0005) (0.0012)		
BLANK TEST	0.000	13:07
SUBJECT SAMPLE	XXX	13:08
X[1] = 0.1290 (-0.0256) (0.0006)		

Interference Detected

FS

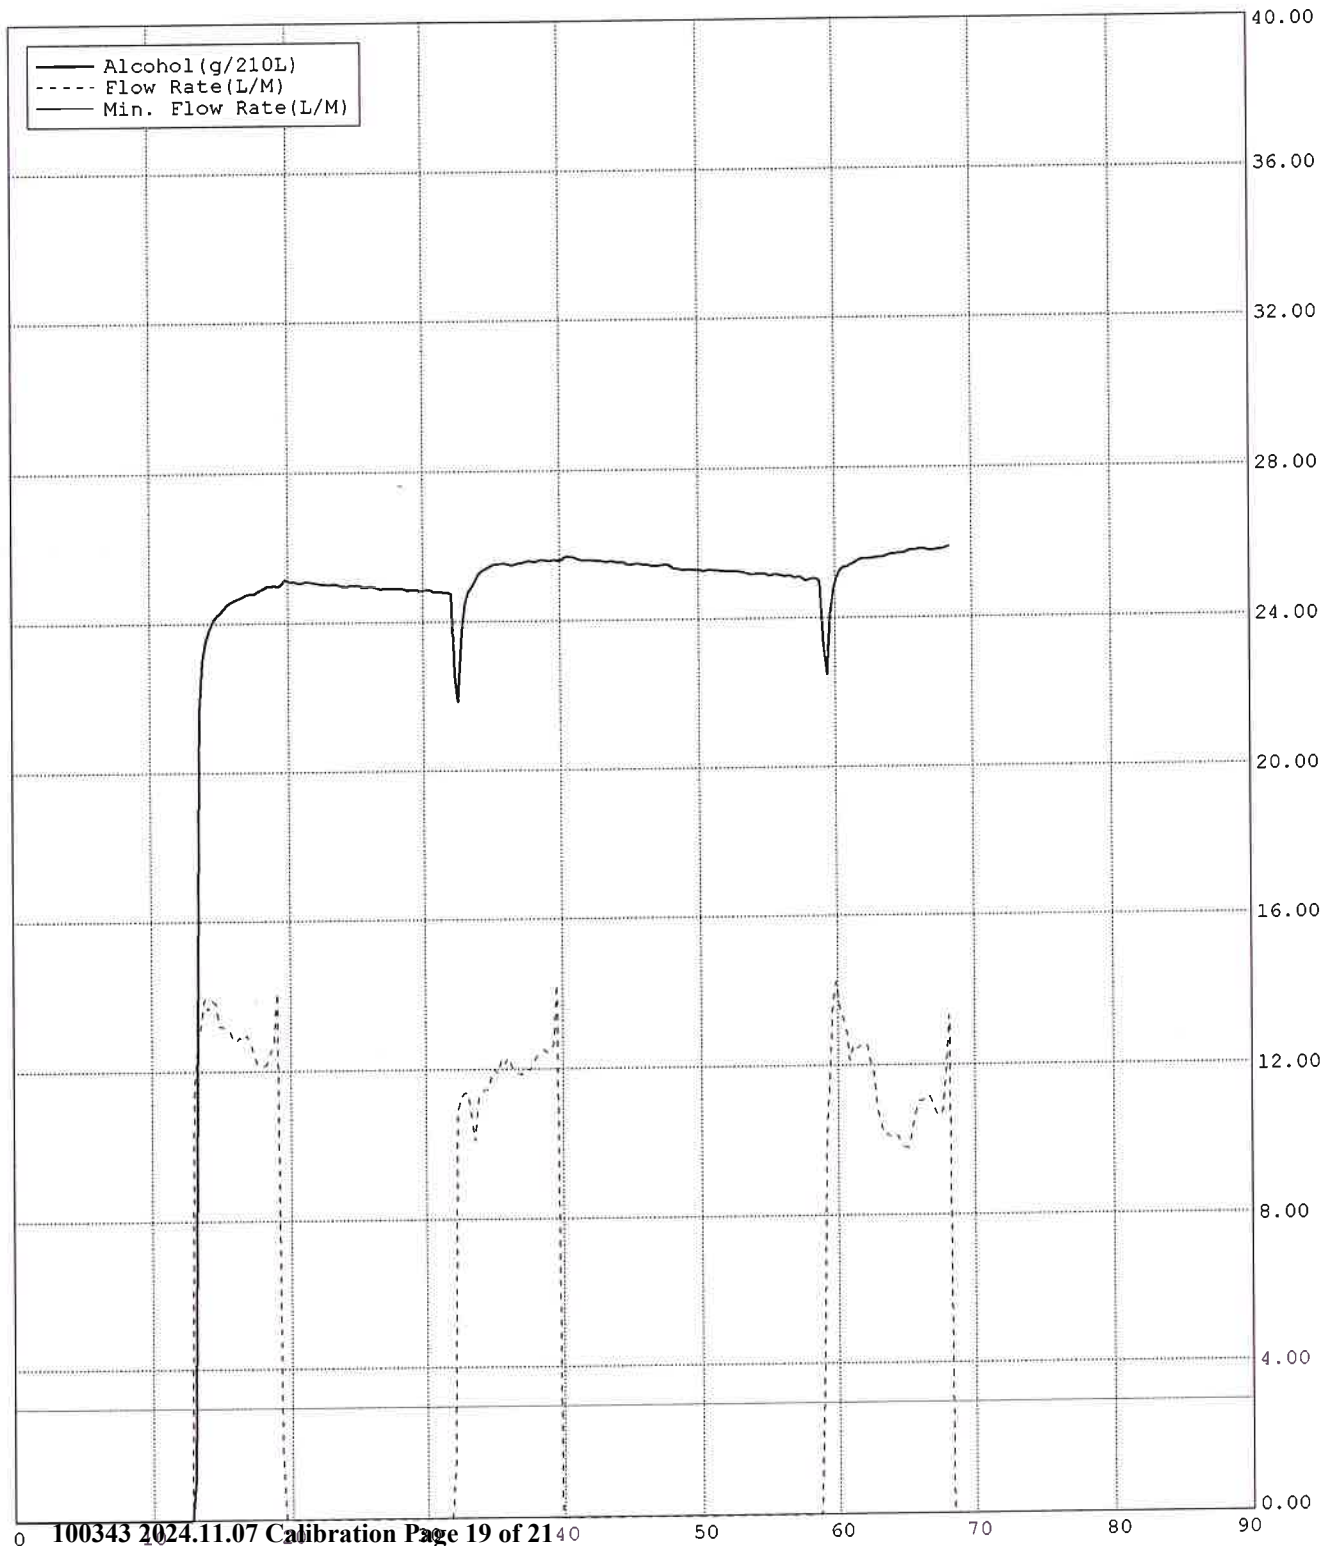

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 13:10:44

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.83: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:11
BLANK TEST	0.000	13:11
INTERNAL STANDARD	VERIFIED	13:11
Xq = 0.092 (0.10%)		
EXTERNAL STANDARD	0.077	13:12
X[1] = 0.0775 (-0.0011) (0.0006)		
BLANK TEST	0.000	13:13
SUBJECT SAMPLE (Vol=1.59L)	0.099	13:13
X[1] = 0.0991 (0.0004) (0.0006)		
BLANK TEST	0.000	13:14
EXTERNAL STANDARD	0.078	13:14
X[1] = 0.0778 (-0.0005) (0.0016)		
BLANK TEST	0.000	13:15

KS

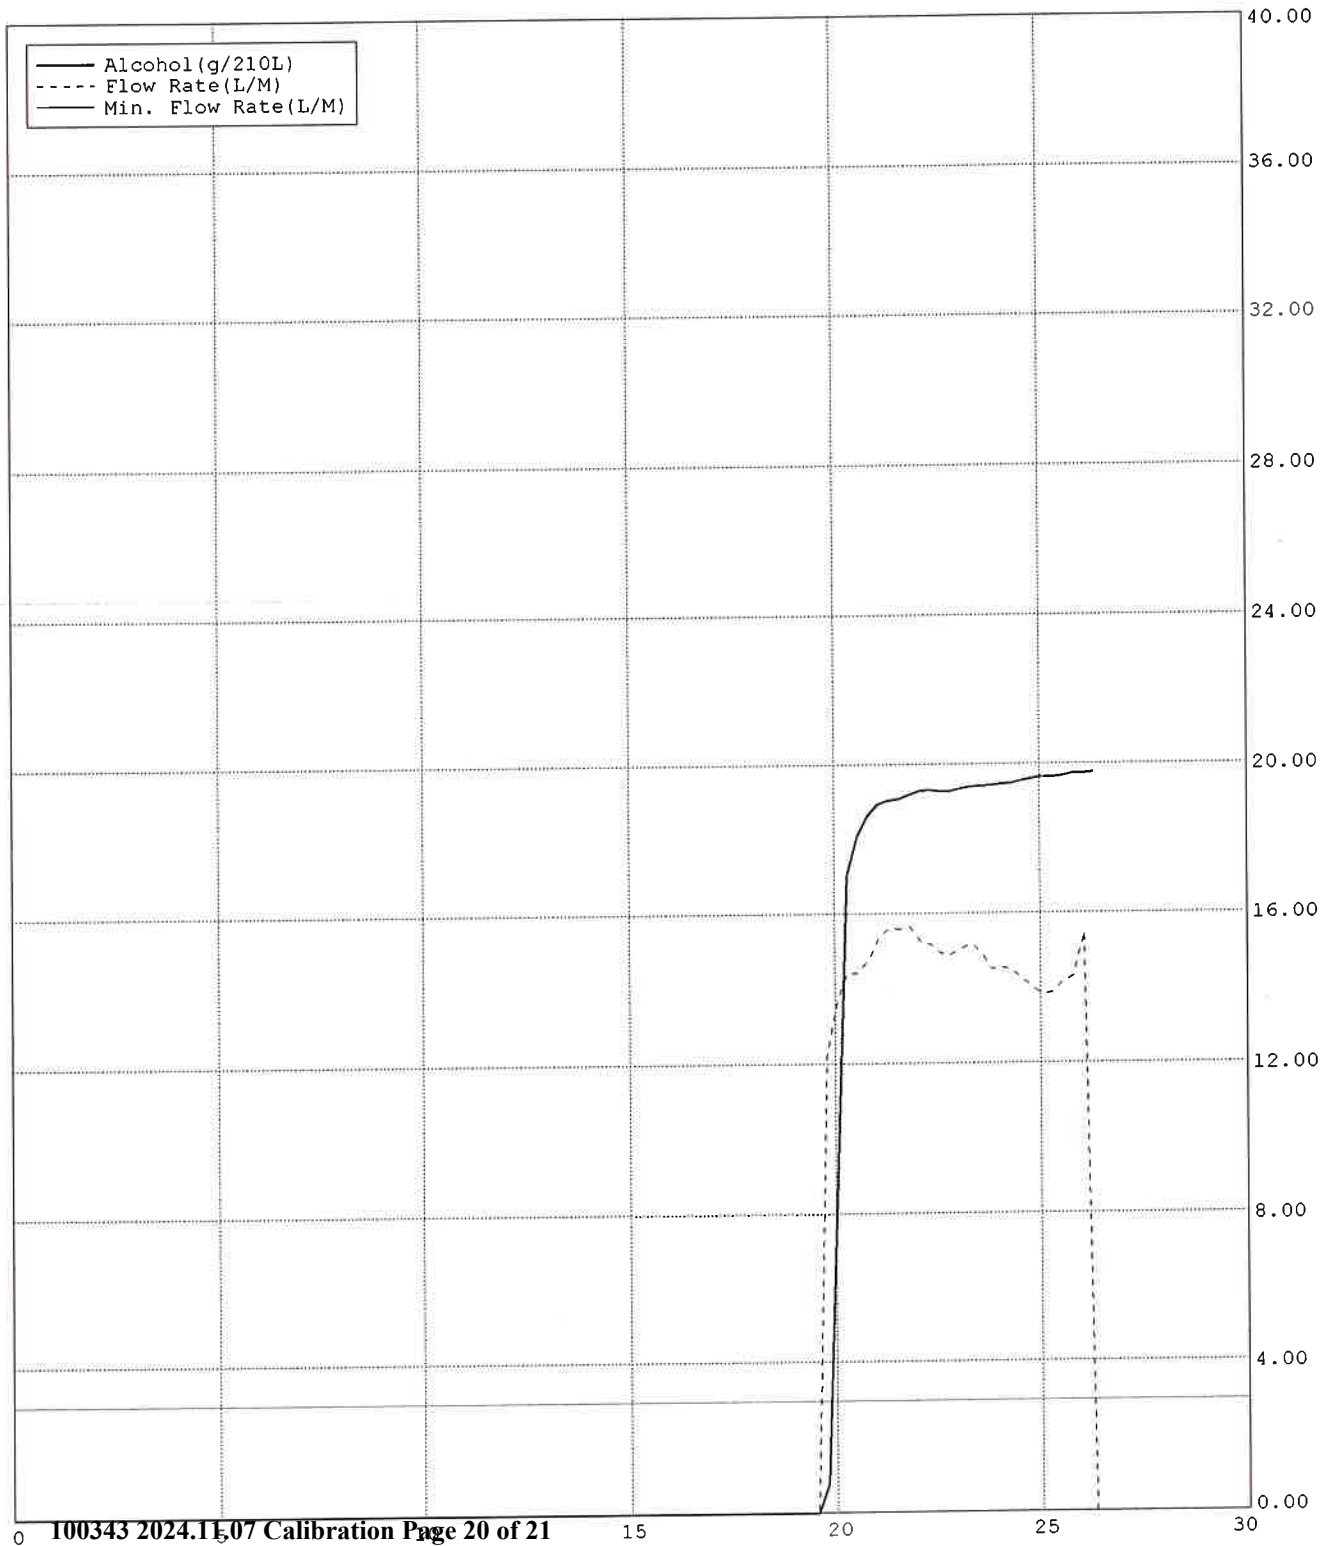

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100343

Date: 11/07/2024
Time: 14:00:46

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.82: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:01
BLANK TEST	0.000	14:01
INTERNAL STANDARD	VERIFIED	14:02
EXTERNAL STANDARD	0.078	14:02
BLANK TEST	0.000	14:03
SUBJECT SAMPLE (Vol=2.00L)	0.000	14:03
BLANK TEST	0.000	14:04
EXTERNAL STANDARD	0.078	14:04
BLANK TEST	0.000	14:05

K-S

