

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100692

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 10/09/2020

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.10: 0.078  
LOT #: AG018102  
EXPIRATION: 06/29/2022  
TANK PRESSURE: 1216 psi

BLANK TEST	0.000	15:32
INTERNAL STANDARD	VERIFIED	15:32
EXTERNAL STANDARD	0.079	15:33
BLANK TEST	0.000	15:34
EXTERNAL STANDARD	0.078	15:34
BLANK TEST	0.000	15:35
EXTERNAL STANDARD	0.078	15:35
BLANK TEST	0.000	15:36
EXTERNAL STANDARD	0.079	15:36
BLANK TEST	0.000	15:37
EXTERNAL STANDARD	0.079	15:37
BLANK TEST	0.000	15:38

Average = 0.0786  
Std Dev = 0.0005

## Diagnostic Check

VERSIONS  
DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.7°C PASSED  
Breath Tube = 48.1°C PASSED

### PUMP INFO

Flow Rate = 3.992 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

### FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED

I, Brandi M. Barnett, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.



*Brandi M Barnett* 12/4/20

Brandi M. Barnett  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this

4 day of 12, 20 20

*Carlie K. Bailey*  
Notary Public  
My Commission Expires With Office

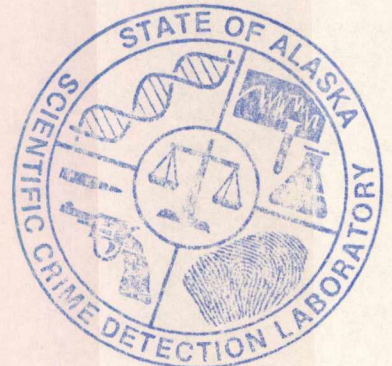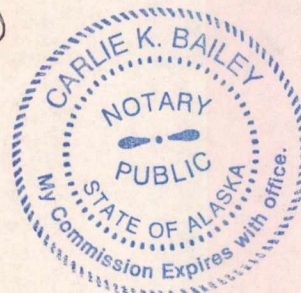

CORB 11/14/20