

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100352

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 12/26/2019

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 28.92: 0.077

LOT #: AG826101

EXPIRATION: ~~05/18/2020~~ 09/18/2020 JMW 12/27/19

TANK PRESSURE: 1100 psi

BLANK TEST	0.000	03:22
INTERNAL STANDARD	VERIFIED	03:22
EXTERNAL STANDARD	0.075	03:23
BLANK TEST	0.000	03:23
EXTERNAL STANDARD	0.076	03:24
BLANK TEST	0.000	03:25
EXTERNAL STANDARD	0.076	03:25
BLANK TEST	0.000	03:26
EXTERNAL STANDARD	0.076	03:26
BLANK TEST	0.000	03:27
EXTERNAL STANDARD	0.076	03:27
BLANK TEST	0.000	03:28

Average = 0.0758

Std Dev = 0.0004

Diagnostic Check

VERSIONS

DMT: 3.02

PIC: 3.03

Modem: 2.6

Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C

PASSED

Breath Tube = 41.7°C

PASSED

PUMP INFO

Flow Rate = 4.880 L/M

PASSED

DETECTOR INFO

PUMP ON

PASSED

PUMP OFF

PASSED

FILTER INFO

Filter 1

PASSED

Filter 2

PASSED

Filter 3

PASSED

INTERNAL STANDARD

PASSED

I, Brandi M. Barnett, after being first duly sworn, depose and state as follows:

(1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.

(2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.

(3) I am the Scientific Director of the State Breath Alcohol Program.

(4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.

(5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.



(6) The referenced instrument is certified for evidentiary use in the State of Alaska.

 1/10/20

Brandi M. Barnett
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 10 day of Jan, 20 20


Notary Public
My Commission Expires With Office

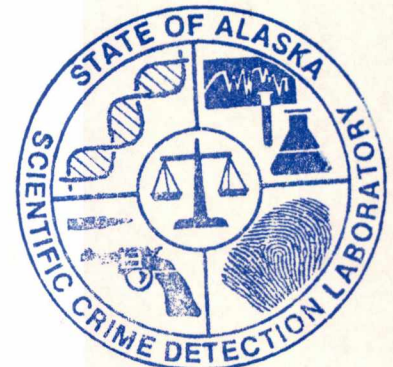

JMW 12/27/19