



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100667

**Report Issue Date:** 12/18/2023  
**Date Received:** 2023-11-07  
**Condition of Item:** Needs Repair

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 11/07/2023** - As Found - **End Date 11/08/2023** As Found - Evaluation Analyst: Carlie Glaister  
 As Found Conditions - Barometric Pressure (inHg): 29.19 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.6  
 Relative Humidity (%): 18

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.078	AG310901	0.077	0.078	0.077	0.077	0.077	0.077	0.077
0.300	0.293	AG217903	0.293	0.293	0.293	0.292	0.293	0.293	0.293

5 way valve was stuck. Moved the mechanism to un-jam it. While testing the mechanism, it continues to get stuck. Recommend replacing the 5 way valve. Reset options.

**Start Date 11/30/2023** - As Left - **End Date 12/04/2023**

As Left Conditions - Barometric Pressure (inHg): 28.83 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.4 Relative Humidity (%): 19

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG217902	0.020	0.020	0.020	0.019	0.020	0.020	+/- 0.002
0.040	0.039	AG217904	0.039	0.038	0.039	0.039	0.038	0.039	+/- 0.003
0.080	0.077	AG310901	0.076	0.077	0.076	0.076	0.076	0.076	+/- 0.004
0.100	0.096	AG211003	0.096	0.096	0.096	0.096	0.096	0.096	+/- 0.004
0.150	0.145	AG134205	0.144	0.144	0.144	0.144	0.144	0.144	+/- 0.005
0.300	0.289	AG217903	0.289	0.289	0.289	0.289	0.289	0.289	+/- 0.011

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**



State of Alaska  
Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
Anchorage, Alaska 99507  
David Kanaris, Chief, Forensic Laboratories

---

**Serial Number:** 100667

---

Results authorized by Carlie Glaister on 12/04/2023

[carlie.glaister@alaska.gov](mailto:carlie.glaister@alaska.gov)

Technically and administratively reviewed by Colleen O'Bryant on 12/18/2023

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100667 Analyst: Carlie Haister Start Date: 11/30/23

- Diagnostic Test (attached)
- Adjust voltages, if needed
  - o Lamp (2.60 V Maximum)
  - o Bias
  - o Cooler (2.00 V Maximum)
- Internal Standard value  $\leq$  3.00%
  - o Chopper Frequency
  - o Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.7 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 28.83 Temperature (C): 22.4 Relative Humidity (%): 19

Linearity Test (attached)

0.020g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217902</u>	Exp: <u>6/28/24</u>
0.040g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217904</u>	Exp: <u>6/28/24</u>
0.080g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-310901</u>	Exp: <u>4/19/25</u>
0.100g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-211003</u>	Exp: <u>4/20/24</u>
0.150g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-134205</u>	Exp: <u>12/8/23</u>
0.300g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217903</u>	Exp: <u>6/28/24</u>

Functional Tests (attached)

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles)
- Acetone Mnf: Lifloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24
  - Simulator S/N: DR4174 Verification Performed?
- Isopropanol Mnf: Lifloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24
  - Simulator S/N: DR4177 Verification Performed?
- Neg. Control Mnf: Lifloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24
  - Simulator S/N: DR6267 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 230631106 Calibration Due Date: 9/19/2025

- Verify stylus is calibrated
- Non-Drinking Subject Test
- Reset Options
- Upload
- Clear Memory
- Remove Tank Prior to Shutdown
- Verification of Calibration (VOC)
- Calibration End Date: 12/1/23

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100667  
-----

Date: 11/30/2023  
Time: 12:19:09

VERSIONS

DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 44.2°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 2.15 V PASSED  
(1.15 V - 2.67 V)  
Cooler Voltage = 1.75 V PASSED  
(1.16 V - 2.70 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 532 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 28.8 in

PUMP INFO

Flow Rate = 4.513 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.106 0.33% (0.00% - 4.00%) PASSED



Technician Screen

-----  
DATAMASTER dmt: 100667  
-----

Date: 11/30/2023  
Time: 12:23 PM

Temperatures (°C)

Sample Cell: 48.7°C  
Breath Tube: 44.3°C

Current Barometer 28.8 in  
Volume (Ltr) 1.44

Settings

Lamp: 2.21 V  
Bias: 80 V  
Cooler: 1.81 V  
Chopper: 532 Hz

Voltages (V)

Flow: 1.07 V  
Detector: -0.021 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100667  
-----

Date: 12/29/2021  
Time: 11:35:09

OPERATOR NAME:  
CARLIE GLAISTER  
CERTIFICATE #: 10436

Ca = 0.1000  
CAL = 0.984050    0.800 <= CAL < 1.200  
b1 = 0.0010    0.0000 <= b1 < 0.0040  
b2 = 0.0079    0.0010 <= b2 < 0.0100  
b3 = 0.0005    0.0000 <= b3 < 0.0040  
Xq = 0.1060    0.0500 <= Xq < 0.2000  
a21 = 1.213621    1.050 <= a21 < 1.300  
a31 = 0.486925    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100667

Date: 11/30/2023  
Time: 12:24:38

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
MINIMUM VOLUME TEST  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 28.84: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	12:25
BLANK TEST	0.000	12:25
INTERNAL STANDARD	VERIFIED	12:25
EXTERNAL STANDARD	0.076	12:26
BLANK TEST	0.000	12:27
SUBJECT SAMPLE (Vol=1.53L)	0.000	12:28
BLANK TEST	0.000	12:29
EXTERNAL STANDARD	0.076	12:29
BLANK TEST	0.000	12:30

OK

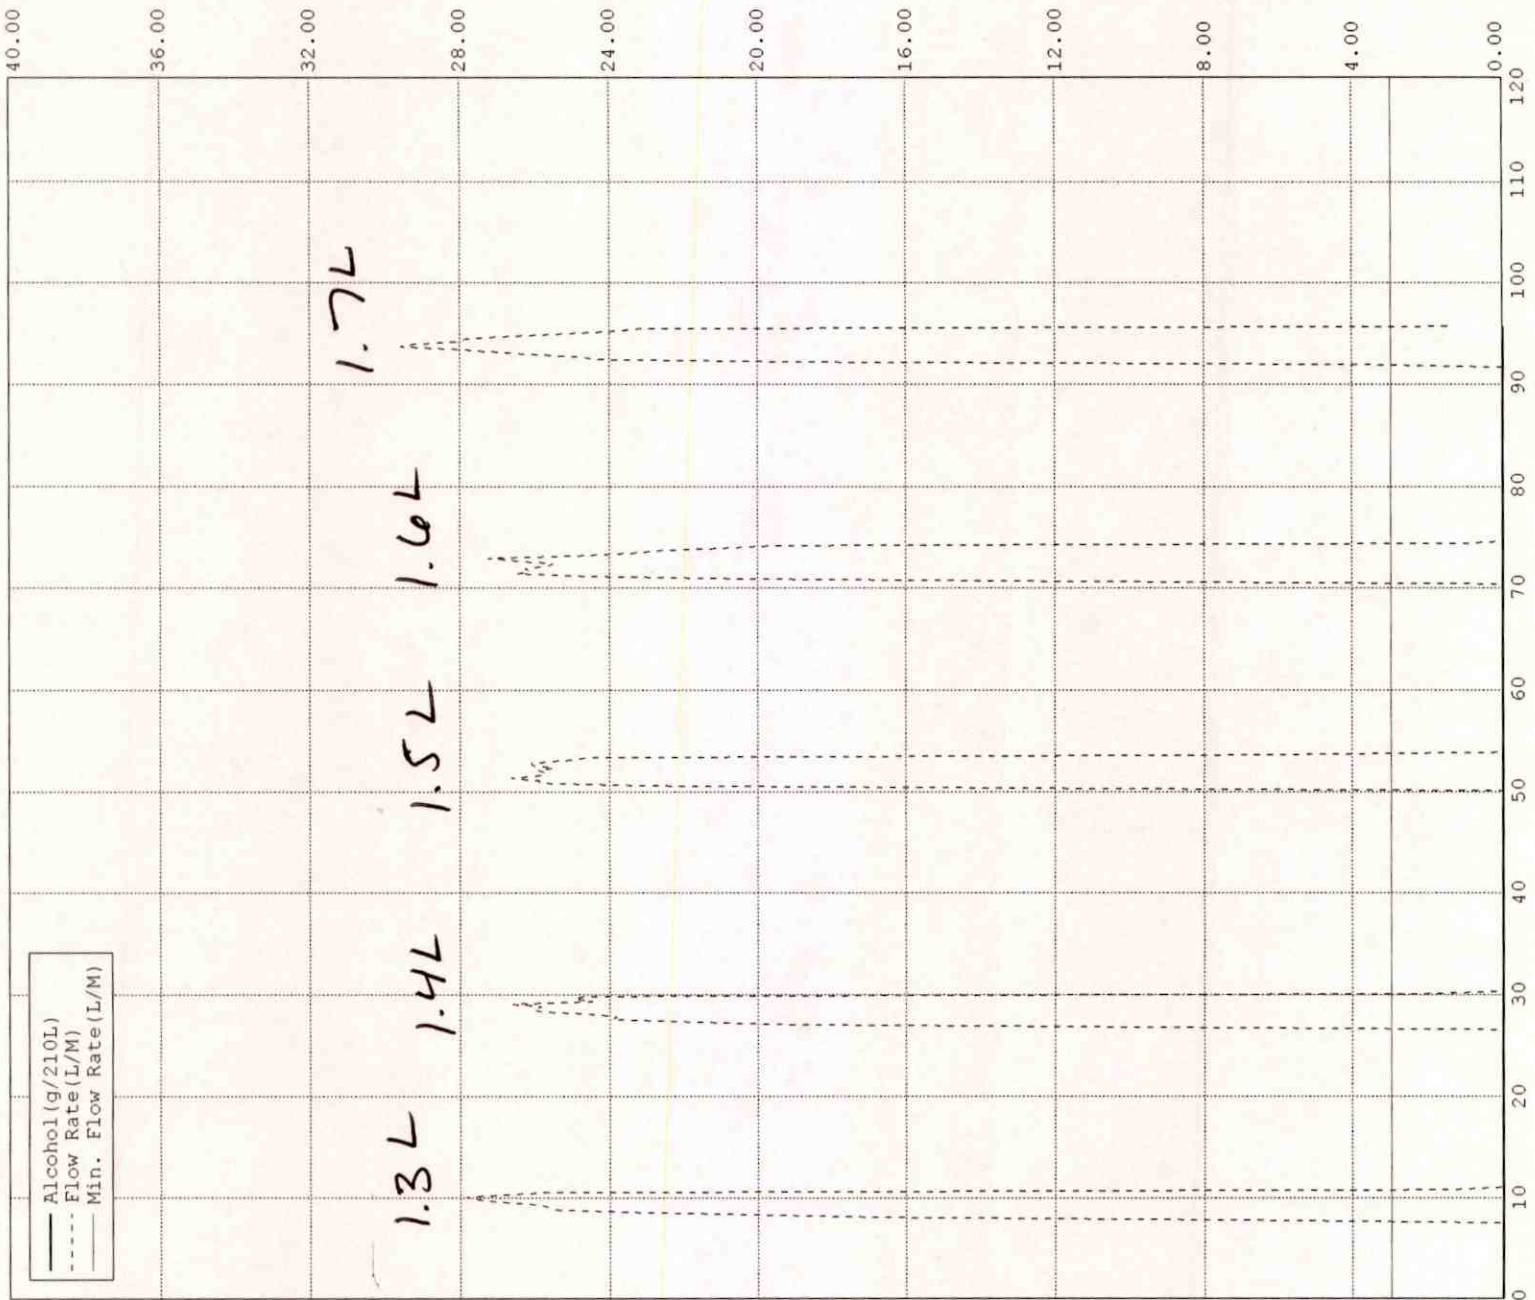

LINEARITY CHECK


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100667  
 -----

Date: 11/30/2023  
 Time: 12:35:21

SUPERVISOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.019	0.0198	0.0004
0.039	0.0386	0.0005
0.077	0.0762	0.0004
0.096	0.0960	0.0000
0.145	0.1440	0.0000
0.289	0.2890	0.0000

SLOPE = 0.998917  
 $R^2$  = 0.999957

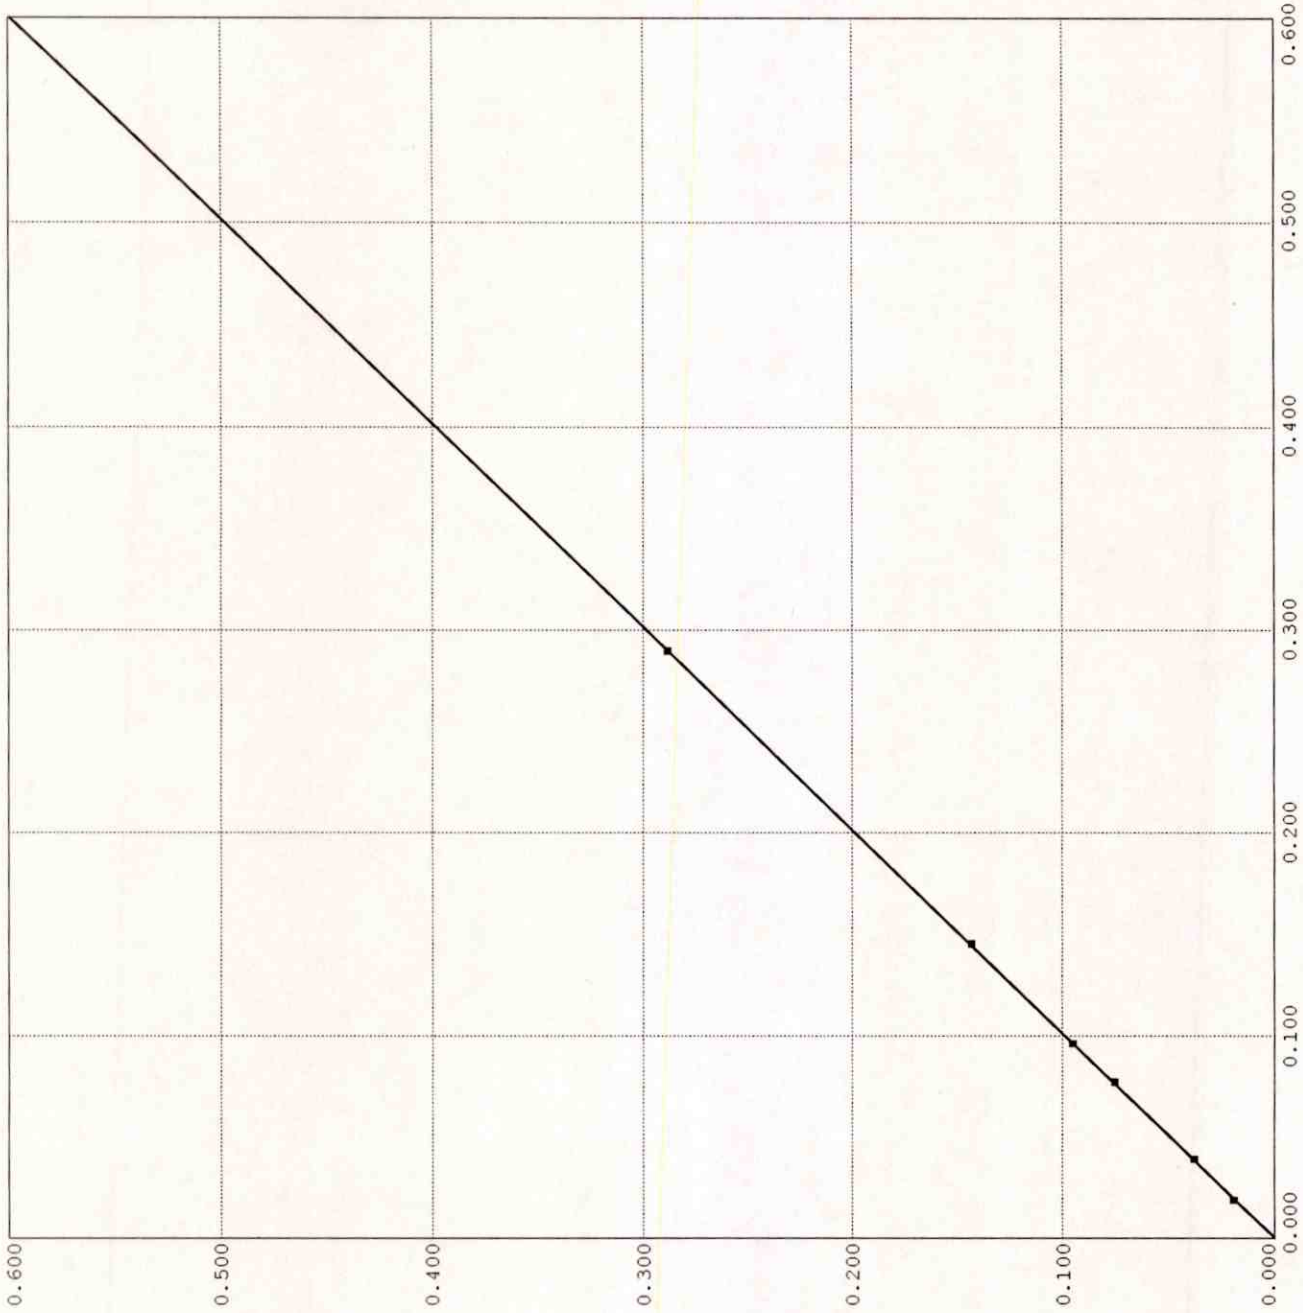

OK



LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100667






Date: 11/30/2023  
Time: 12:35:23

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 28.84: 0.019  
LOT #: AG217902  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 779 psi

BLANK TEST	0.000	12:36
INTERNAL STANDARD	VERIFIED	12:36
EXTERNAL STANDARD	0.020	12:37
BLANK TEST	0.000	12:37
EXTERNAL STANDARD	0.020	12:38
BLANK TEST	0.000	12:39
EXTERNAL STANDARD	0.020	12:39
BLANK TEST	0.000	12:40
EXTERNAL STANDARD	0.019	12:40
BLANK TEST	0.000	12:41
EXTERNAL STANDARD	0.020	12:41
BLANK TEST	0.000	12:42

Average = 0.0198  
Std Dev = 0.0004

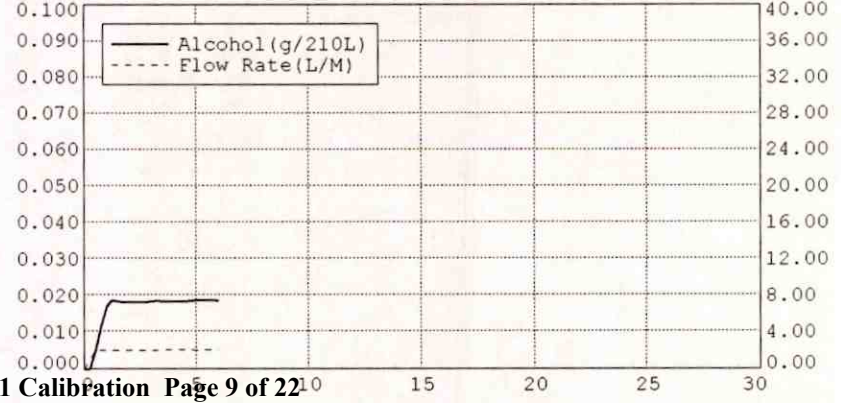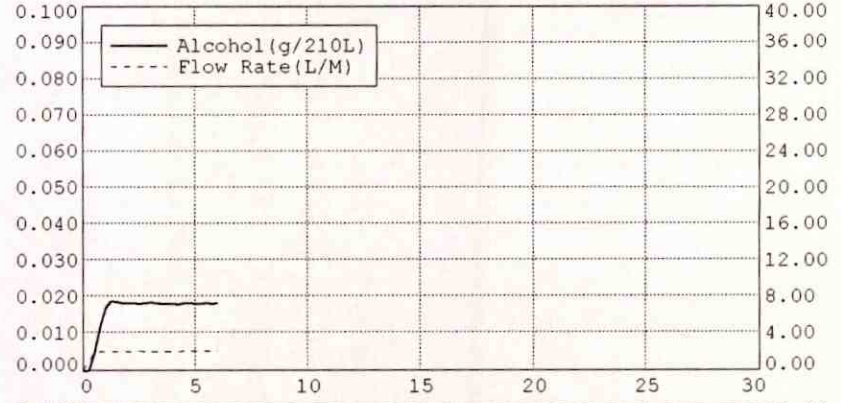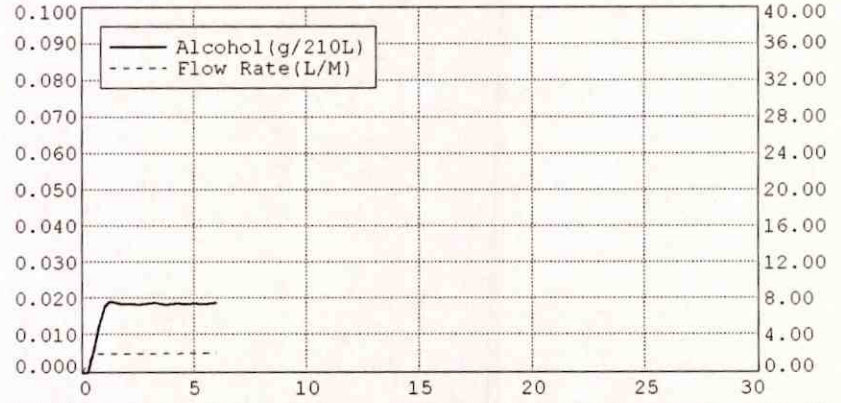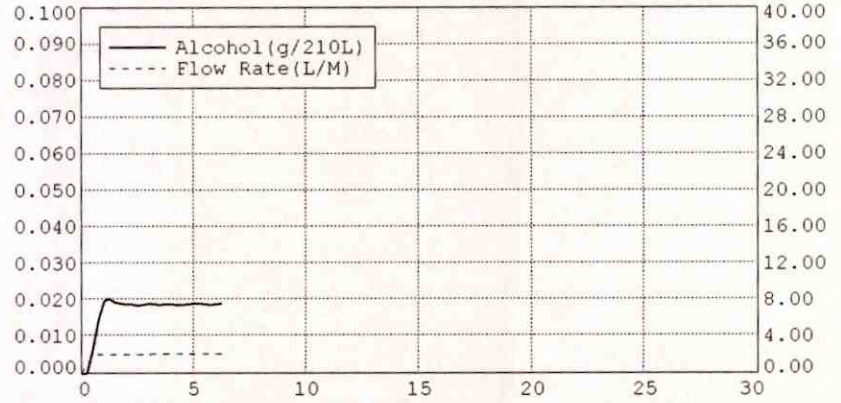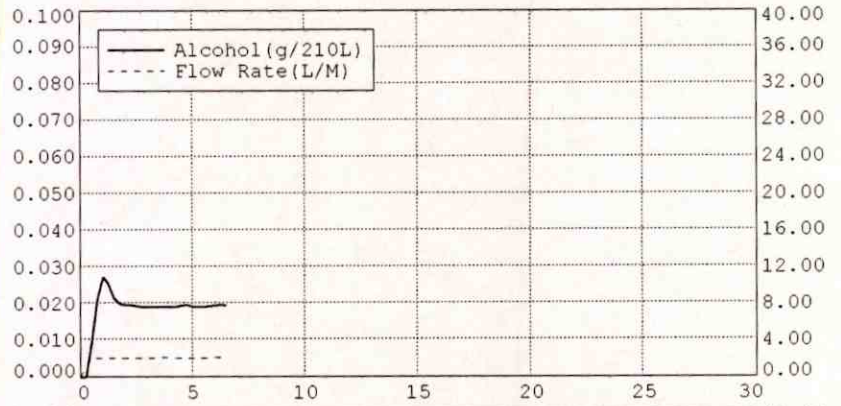

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100667






Date: 11/30/2023  
 Time: 12:43:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 28.84: 0.039  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 806 psi

BLANK TEST	0.000	12:45
INTERNAL STANDARD	VERIFIED	12:45
EXTERNAL STANDARD	0.039	12:45
BLANK TEST	0.000	12:46
EXTERNAL STANDARD	0.038	12:46
BLANK TEST	0.000	12:47
EXTERNAL STANDARD	0.039	12:47
BLANK TEST	0.000	12:48
EXTERNAL STANDARD	0.039	12:48
BLANK TEST	0.000	12:49
EXTERNAL STANDARD	0.038	12:49
BLANK TEST	0.000	12:50

Average = 0.0386  
 Std Dev = 0.0005

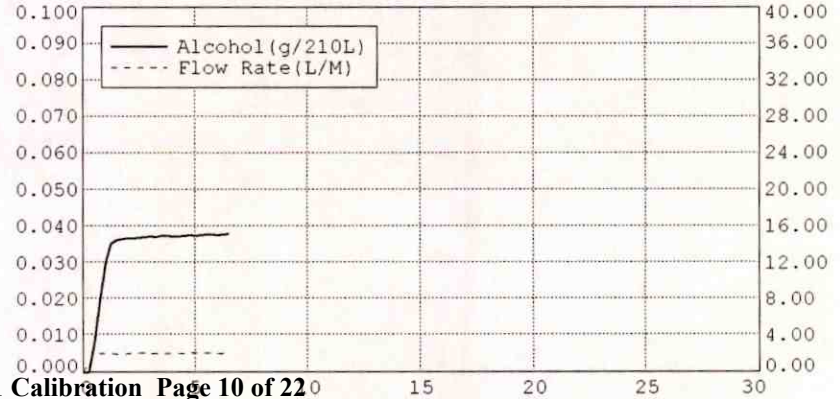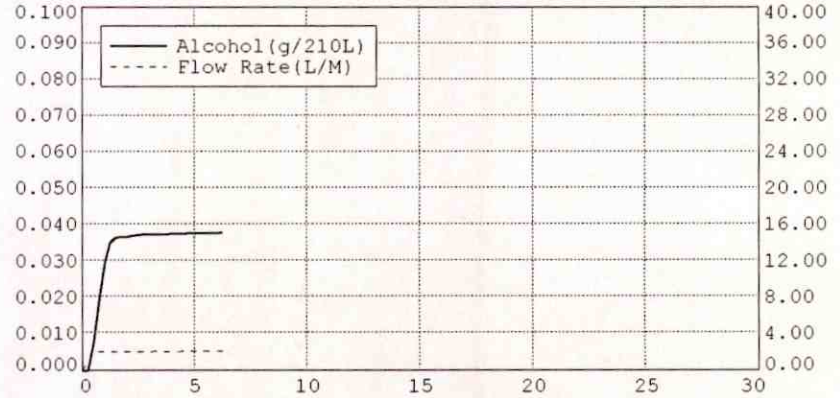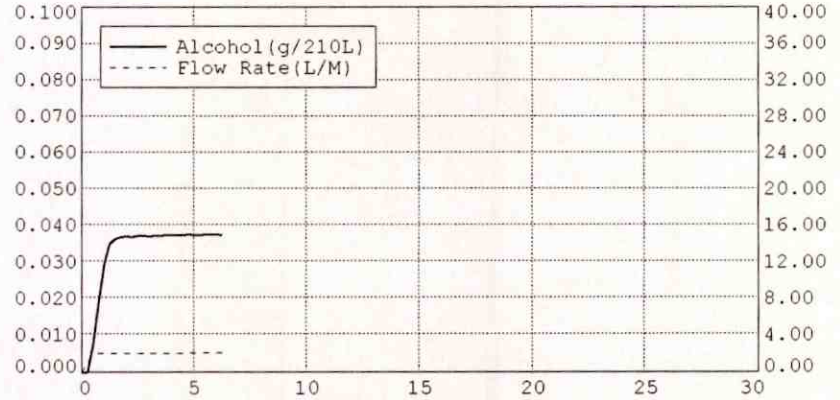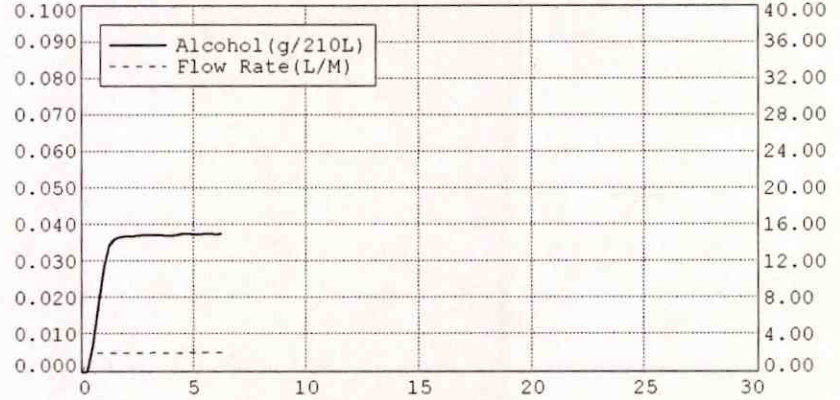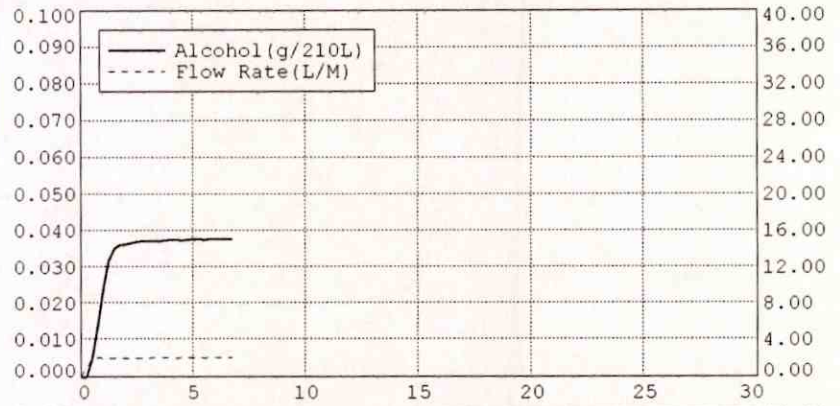



LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100667






Date: 11/30/2023  
 Time: 14:33:42

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 28.83: 0.077  
 LOT #: AG310901  
 EXPIRATION: 04/19/2025  
 TANK PRESSURE: 638 psi

BLANK TEST	0.000	14:35
INTERNAL STANDARD	VERIFIED	14:35
EXTERNAL STANDARD	0.076	14:35
BLANK TEST	0.000	14:36
EXTERNAL STANDARD	0.077	14:36
BLANK TEST	0.000	14:37
EXTERNAL STANDARD	0.076	14:37
BLANK TEST	0.000	14:38
EXTERNAL STANDARD	0.076	14:39
BLANK TEST	0.000	14:39
EXTERNAL STANDARD	0.076	14:40
BLANK TEST	0.000	14:41

Average = 0.0762  
 Std Dev = 0.0004

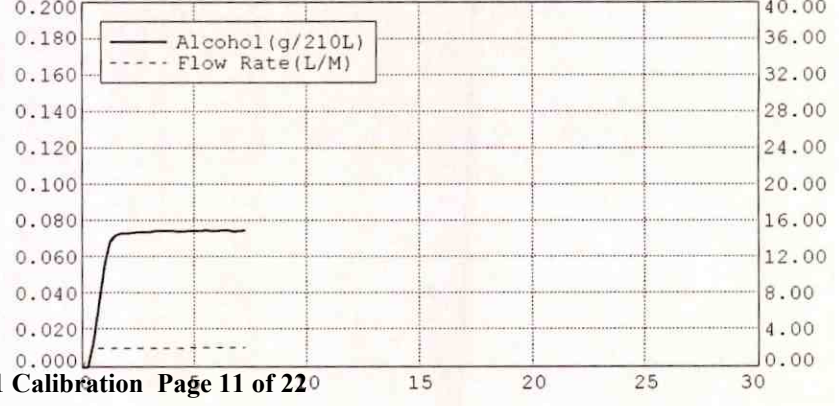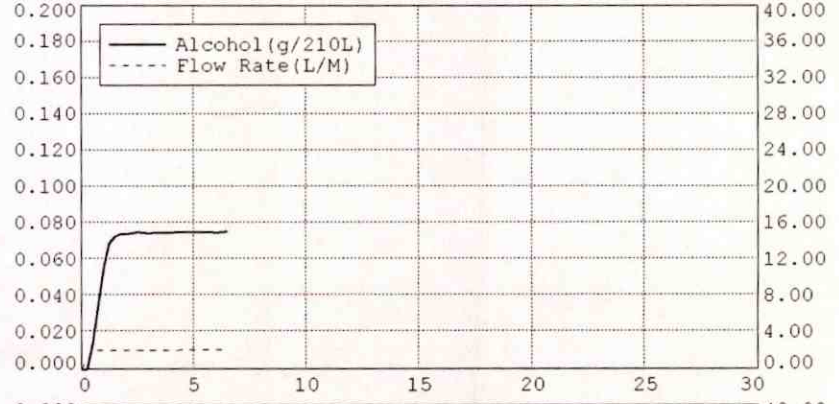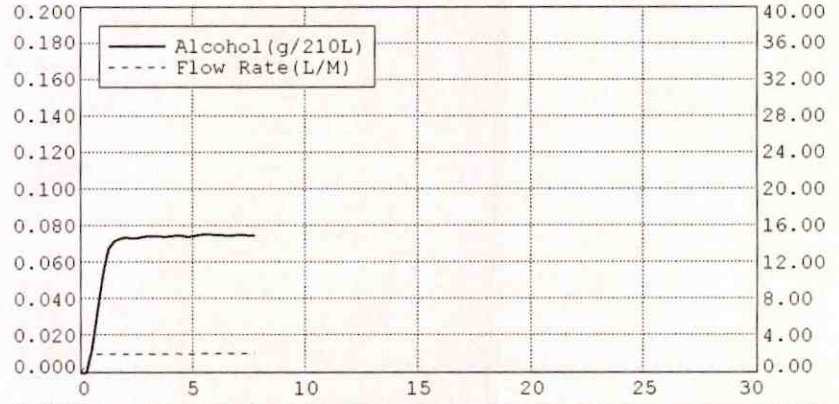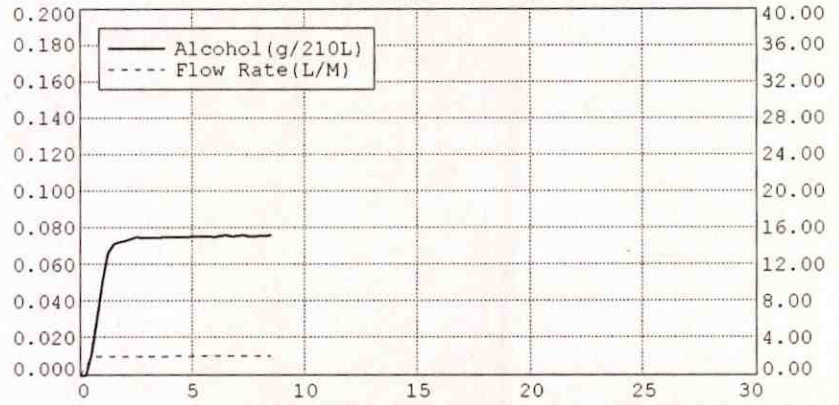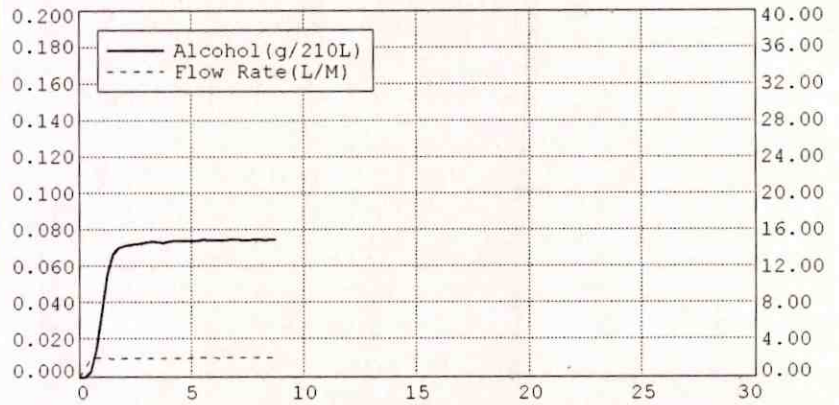

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100667






Date: 11/30/2023  
 Time: 14:48:08

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 28.84: 0.096  
 LOT #: AG211003  
 EXPIRATION: 04/20/2024  
 TANK PRESSURE: 710 psi

BLANK TEST	0.000	14:49
INTERNAL STANDARD	VERIFIED	14:49
EXTERNAL STANDARD	0.096	14:49
BLANK TEST	0.000	14:50
EXTERNAL STANDARD	0.096	14:50
BLANK TEST	0.000	14:51
EXTERNAL STANDARD	0.096	14:52
BLANK TEST	0.000	14:52
EXTERNAL STANDARD	0.096	14:53
BLANK TEST	0.000	14:54
EXTERNAL STANDARD	0.096	14:54
BLANK TEST	0.000	14:55

Average = 0.0960  
 Std Dev = 0.0000

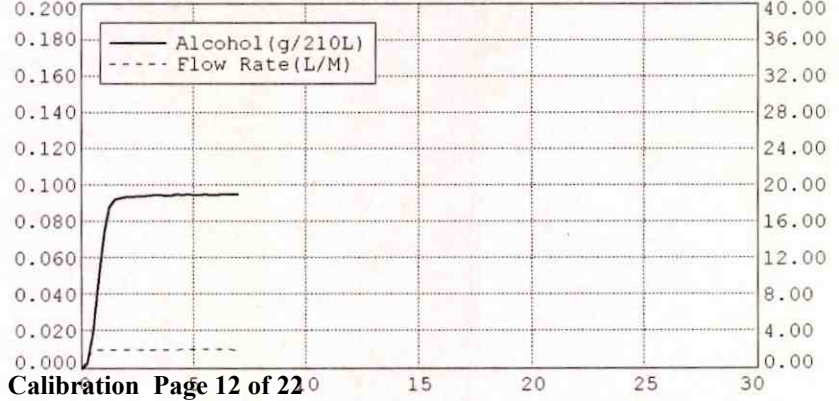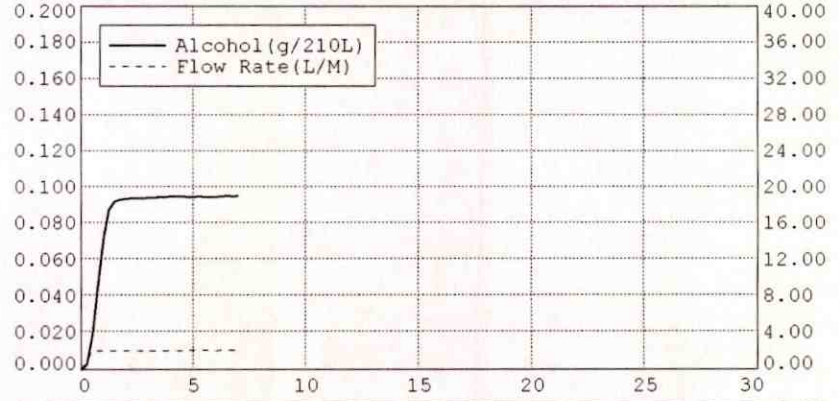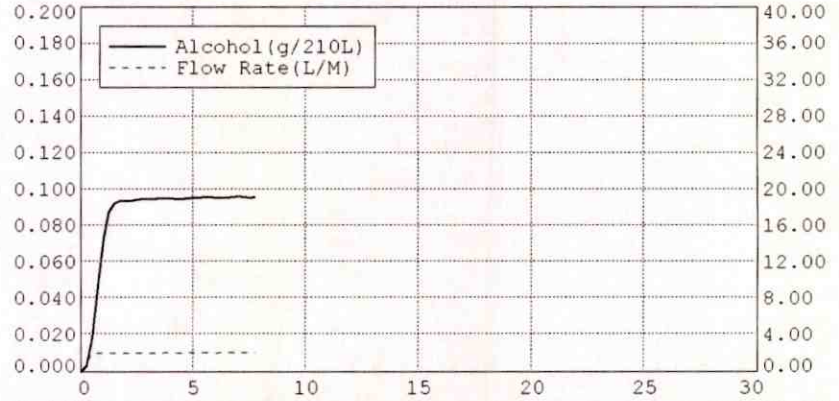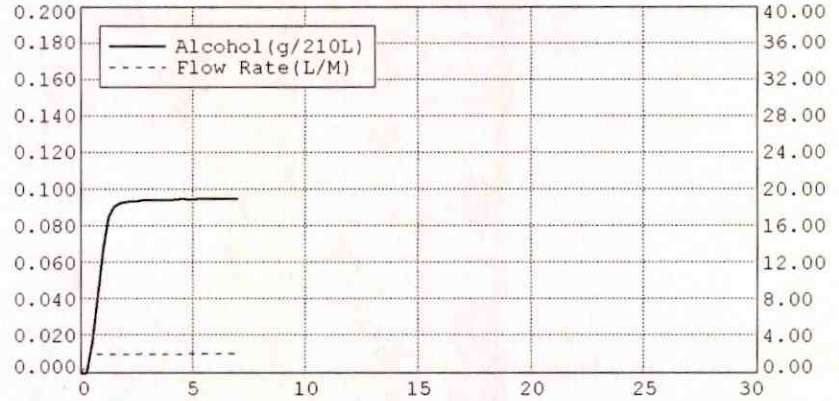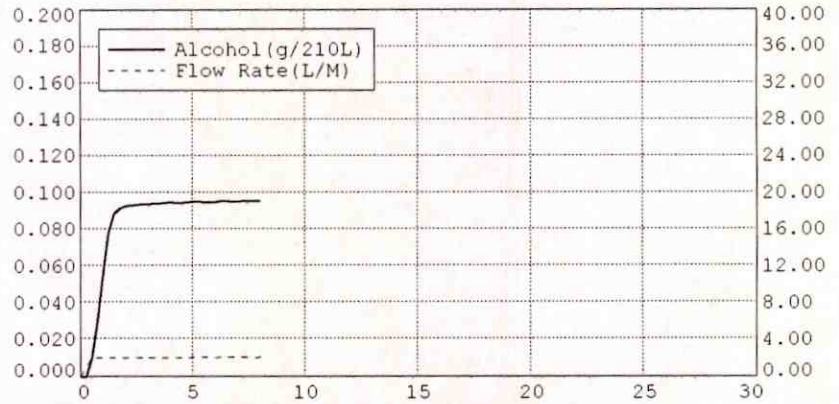



LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100667






Date: 11/30/2023  
 Time: 14:57:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 28.84: 0.145  
 LOT #: AG134205  
 EXPIRATION: 12/08/2023  
 TANK PRESSURE: 613 psi

BLANK TEST	0.000	14:59
INTERNAL STANDARD	VERIFIED	14:59
EXTERNAL STANDARD	0.144	14:59
BLANK TEST	0.000	15:00
EXTERNAL STANDARD	0.144	15:00
BLANK TEST	0.000	15:01
EXTERNAL STANDARD	0.144	15:01
BLANK TEST	0.000	15:02
EXTERNAL STANDARD	0.144	15:02
BLANK TEST	0.000	15:03
EXTERNAL STANDARD	0.144	15:04
BLANK TEST	0.000	15:04

Average = 0.1440  
 Std Dev = 0.0000

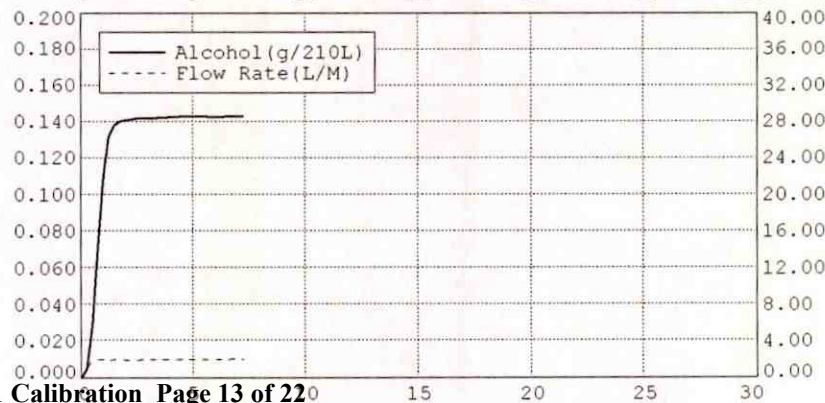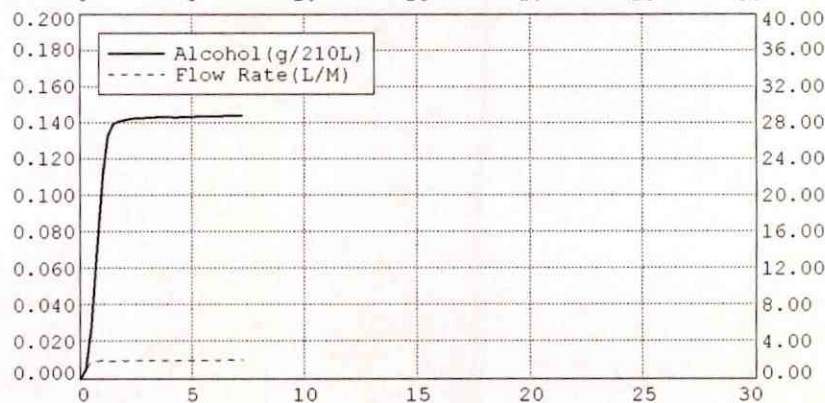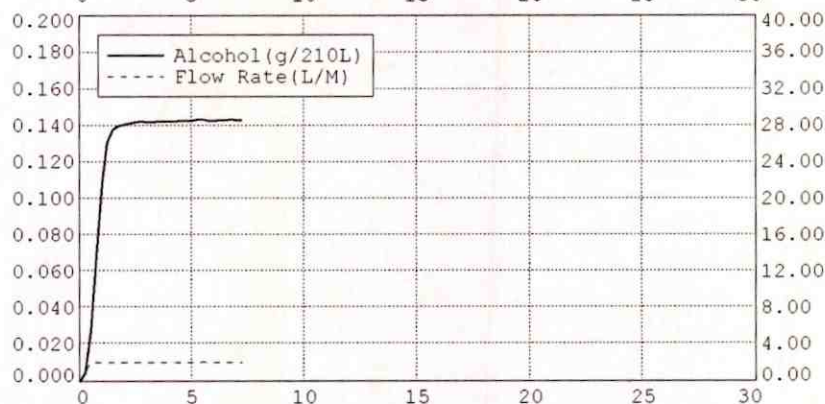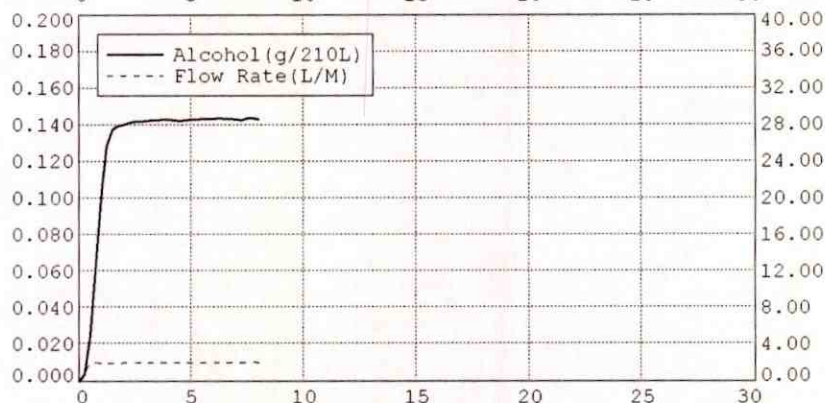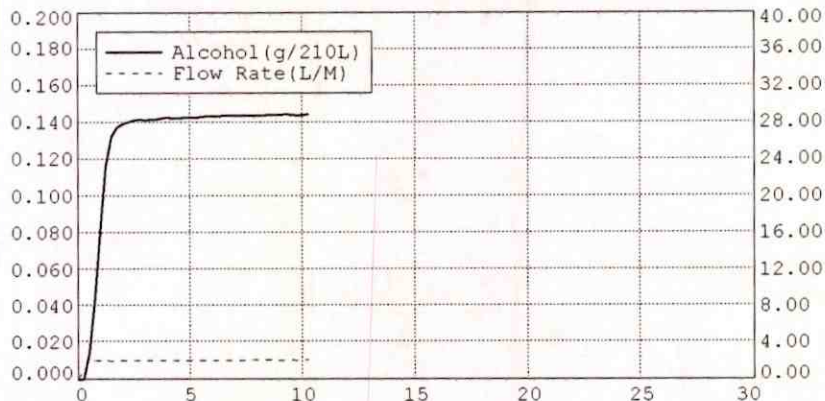

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
DATAMASTER dmt: 100667






Date: 11/30/2023  
Time: 15:21:55

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
TARGET AT 28.87: 0.289  
LOT #: AG217903  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 181 psi

BLANK TEST	0.000	15:24
INTERNAL STANDARD	VERIFIED	15:24
EXTERNAL STANDARD	0.289	15:25
BLANK TEST	0.000	15:26
EXTERNAL STANDARD	0.289	15:26
BLANK TEST	0.000	15:27
EXTERNAL STANDARD	0.289	15:27
BLANK TEST	0.000	15:28
EXTERNAL STANDARD	0.289	15:28
BLANK TEST	0.000	15:29
EXTERNAL STANDARD	0.289	15:30
BLANK TEST	0.000	15:30

Average = 0.2890  
Std Dev = 0.0000

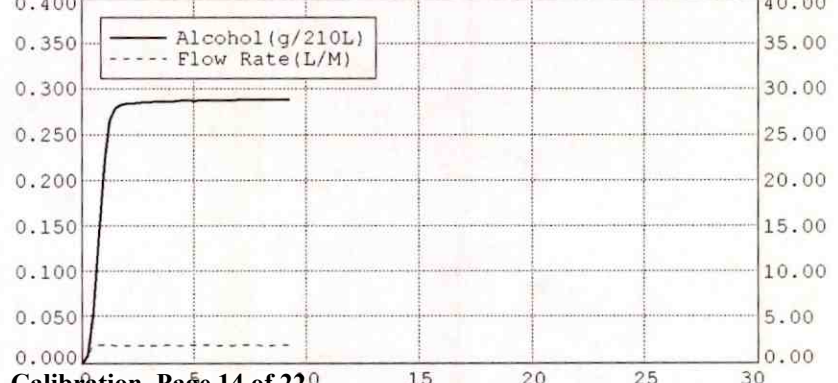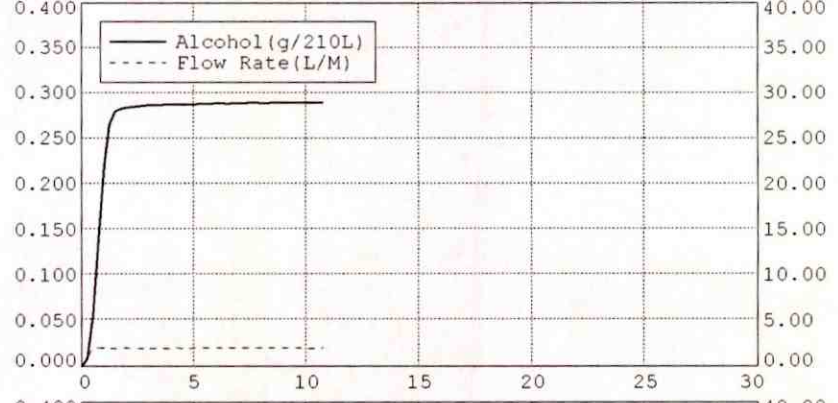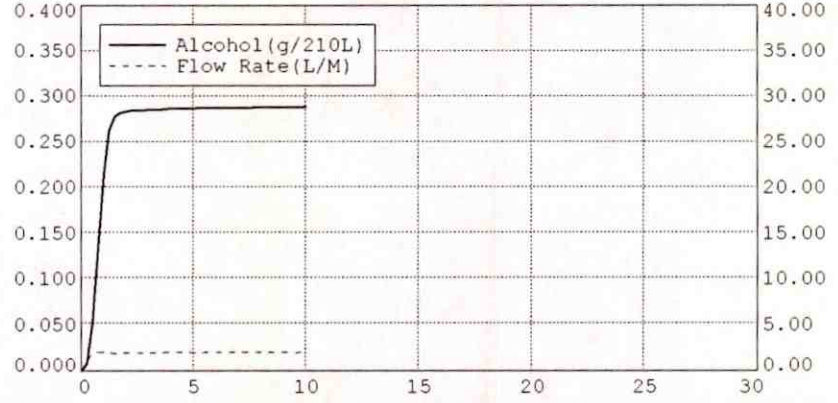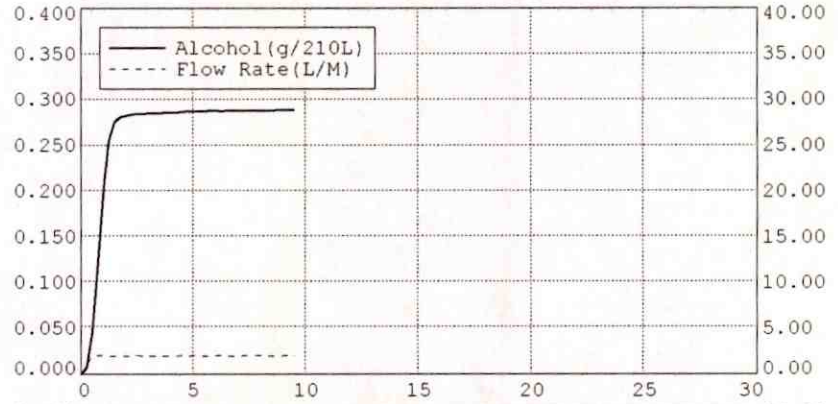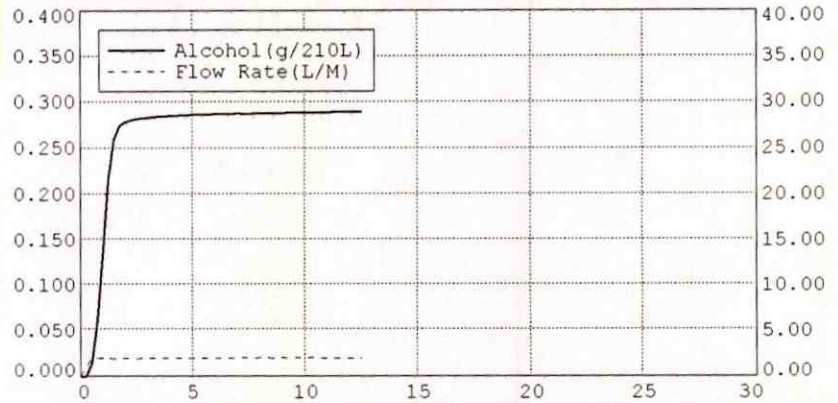



SUBJECT TEST

-----  
Alaska Department of Public Safety

DATAMASTER dmt: 100667

-----  
Date: 11/30/2023

Time: 15:36:45

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INCOMPLETE

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 28.87: 0.077

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

PASSED 15:37

BLANK TEST 0.000 15:37

INTERNAL STANDARD

VERIFIED 15:38

0.078 15:38

EXTERNAL STANDARD

0.000 15:39

BLANK TEST

INCOMPLETE 15:41

Alcohol (g/210L)  
Flow Rate (L/M)  
Min. Flow Rate (L/M)



*Handwritten signature/initials*

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100667

Date: 12/01/2023  
Time: 09:05:55

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
MAXIMUM ATTEMPTS EXCEEDED  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 28.97: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 09:06  
BLANK TEST 0.000 09:07  
INTERNAL STANDARD VERIFIED 09:07  
EXTERNAL STANDARD 0.076 09:07  
BLANK TEST 0.000 09:08  
SUBJECT SAMPLE XXX 09:09

Maximum Attempts Exceeded

OK

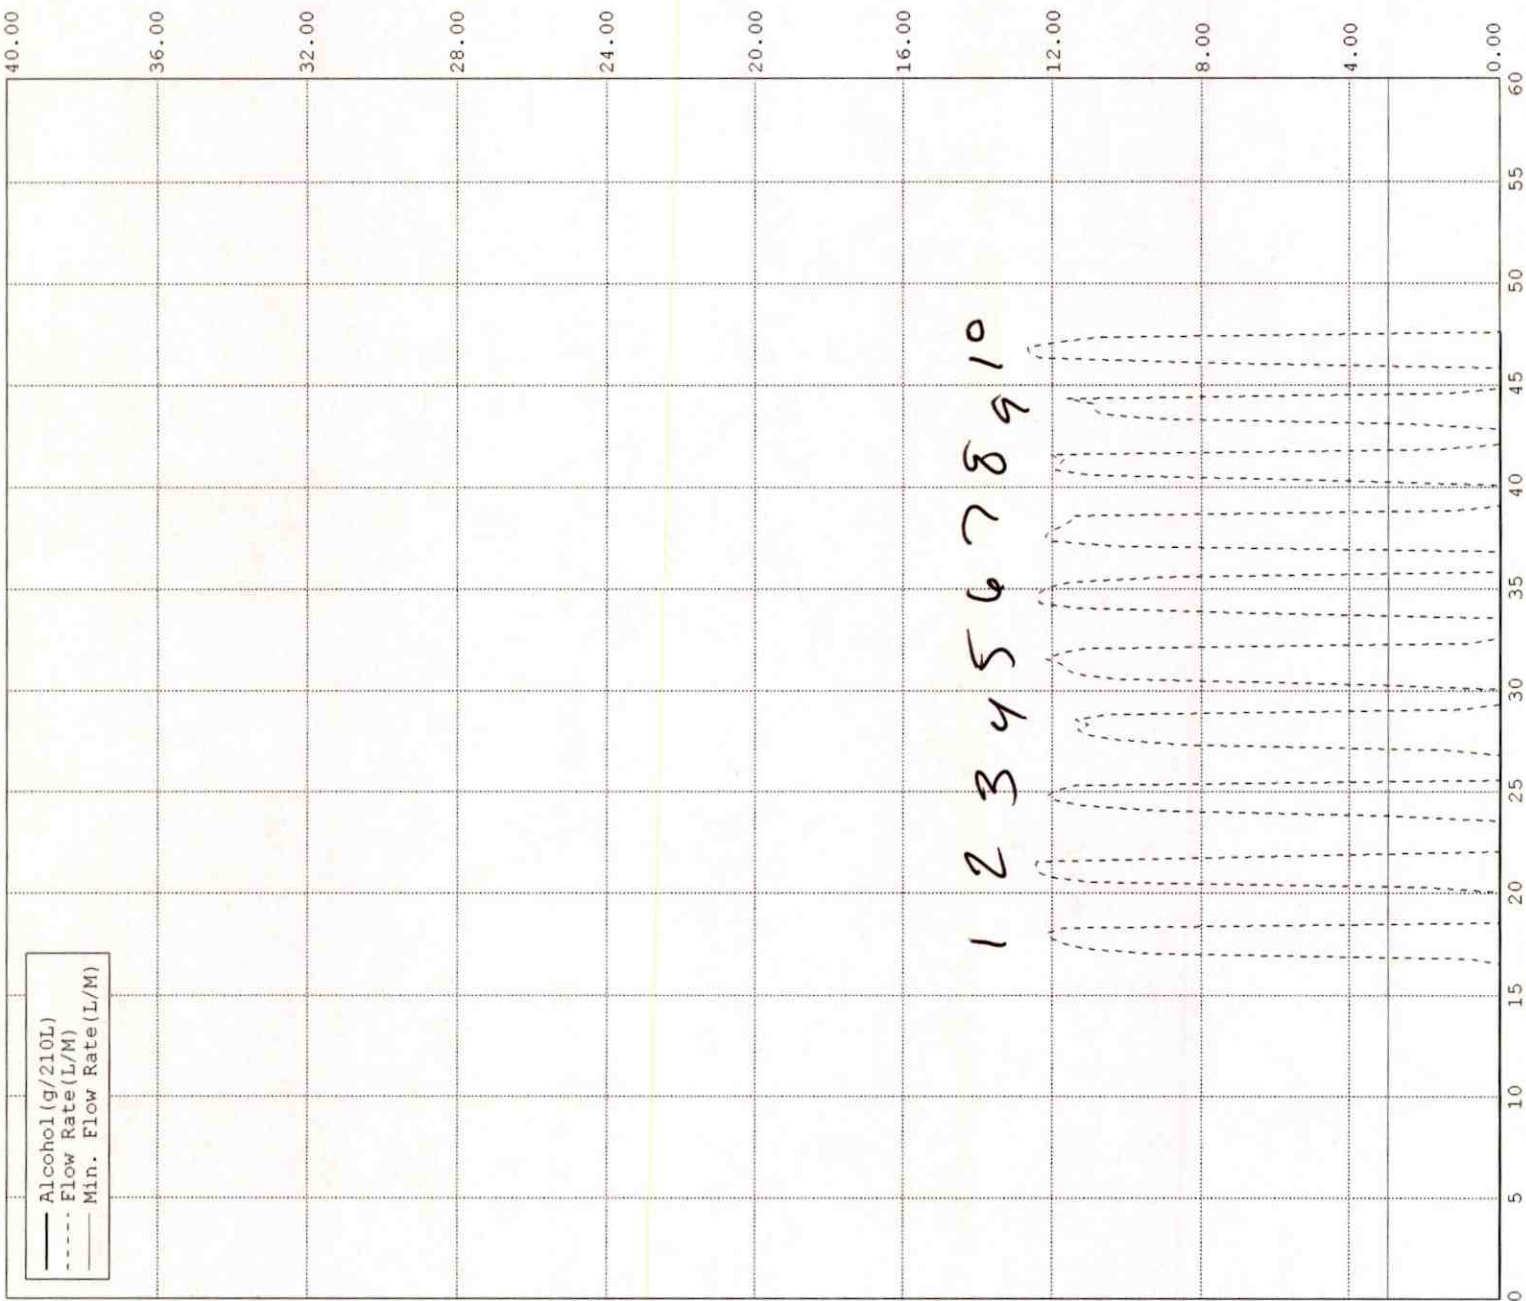



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100667

Date: 12/01/2023  
Time: 09:13:33

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
INVALID  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.97: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 09:16  
BLANK TEST 0.000 09:16  
INTERNAL STANDARD VERIFIED 09:16  
EXTERNAL STANDARD 0.077 09:16  
BLANK TEST 0.000 09:17  
SUBJECT SAMPLE INVALID 09:19

OK

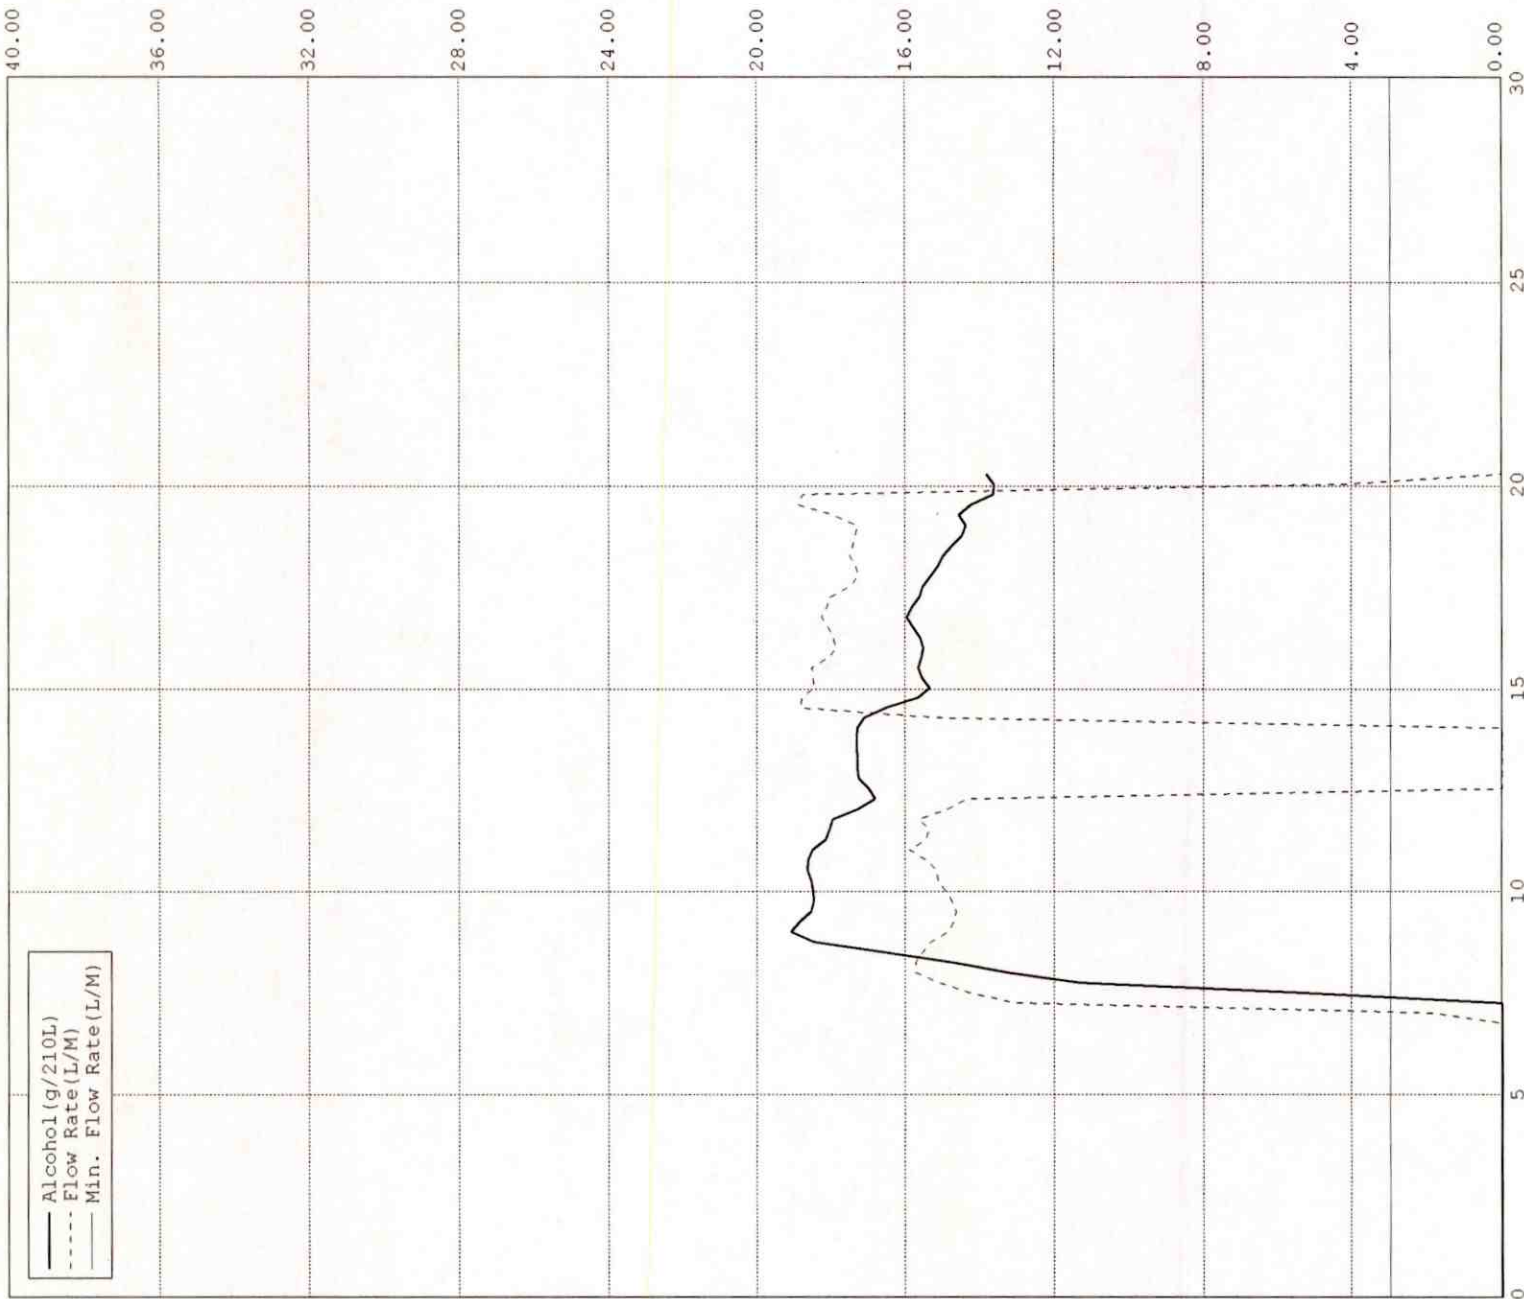

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100667  
-----

Date: 12/01/2023  
Time: 09:28:35

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
RFI  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 28.97: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 09:30  
BLANK TEST 0.000 09:30  
INTERNAL STANDARD VERIFIED 09:30  
EXTERNAL STANDARD 0.076 09:30  
BLANK TEST 0.000 09:31

RFI DETECTED



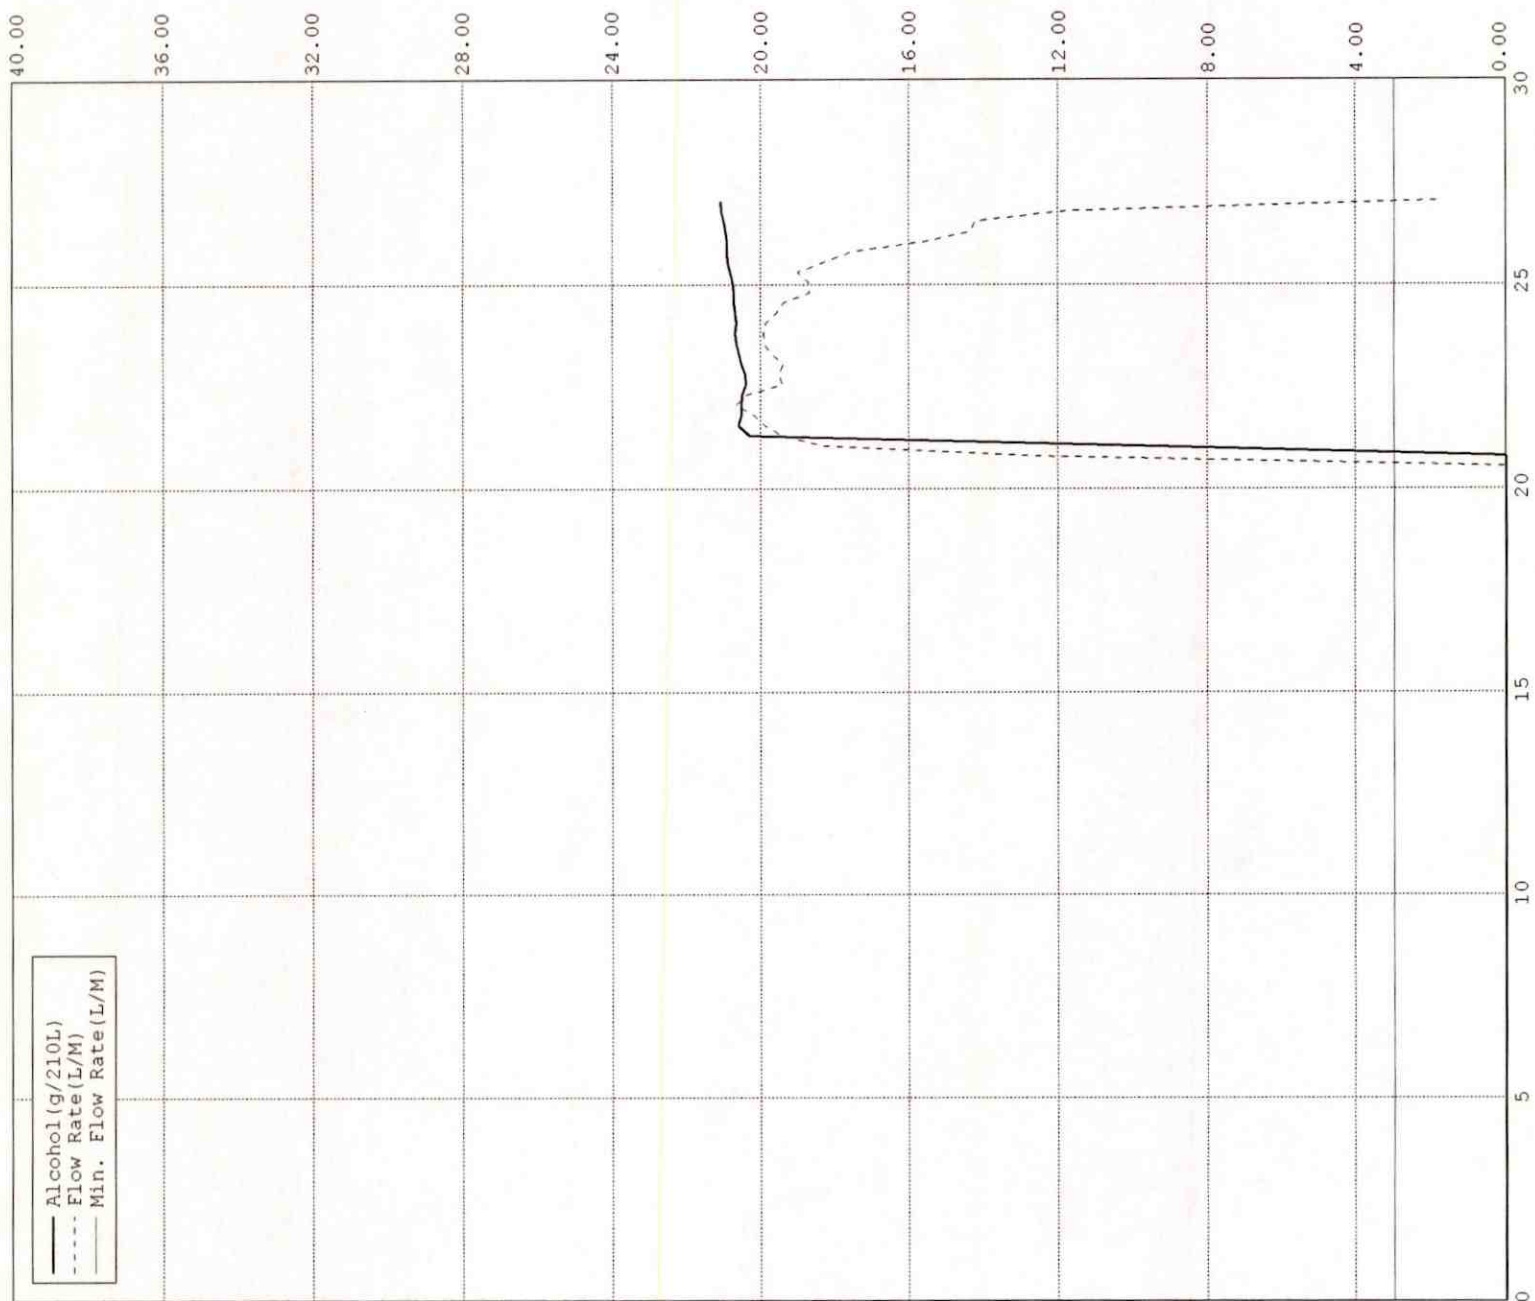

SUBJECT TEST

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100667  
 -----  
 Date: 12/01/2023  
 Time: 10:51:27

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX

OPERATOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

DEPT/AGENCY:  
 INTERFERENCE ACETONE  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 28.99: 0.078  
 Lot # AG-310901 Exp: 4/19/25 OVV 12/1/23  
 DIAGNOSTIC CHECK PASSED 10:52  
 BLANK TEST 0.000 10:52  
 INTERNAL STANDARD VERIFIED 10:52  
 Xq = 0.106 (0.08%)  
 EXTERNAL STANDARD 0.076 10:52  
 X[1] = 0.0764 (-0.0020) (0.0019)  
 BLANK TEST 0.000 10:53  
 SUBJECT SAMPLE XXX 10:54  
 X[1] = 0.1061 (-0.0207) (0.0005)

Interference Detected

Filter 2 Average: -0.0021  
 Filter 3 Average: 0.0019  
 OVV 12/4/23

OVV



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100667

Date: 12/01/2023  
Time: 10:45:07

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE IPA  
CASE/REPORT: XXXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.98: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	10:46
BLANK TEST	0.000	10:46
INTERNAL STANDARD	VERIFIED	10:47
Xq = 0.106 (0.08%)		
EXTERNAL STANDARD	0.076	10:47
X[1] = 0.0764 (-0.0020)	(0.0021)	
BLANK TEST	0.000	10:48
SUBJECT SAMPLE	XXX	10:48
X[1] = 0.1182 (-0.0372)	(0.0010)	

Interference Detected

CV6

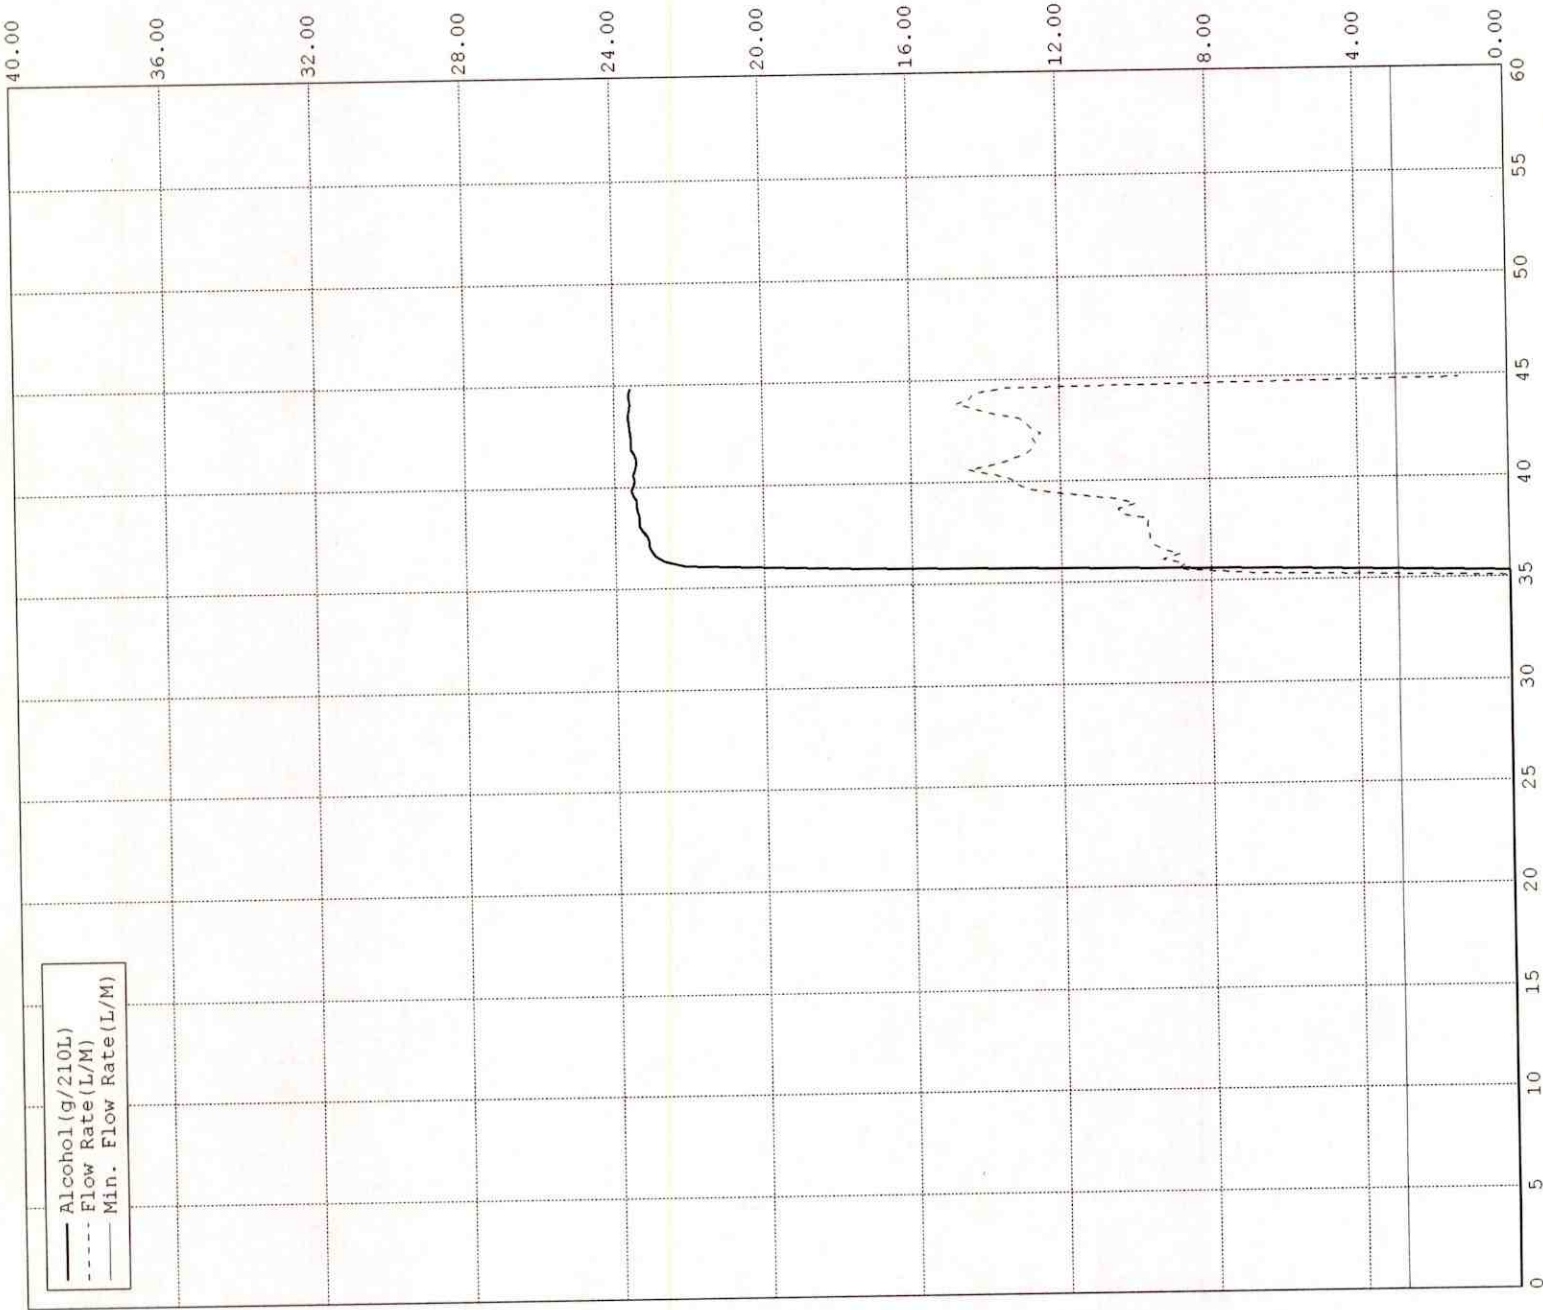



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100667

Date: 12/01/2023  
Time: 10:33:56

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
INTERFERENCE NEGATIVE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.98: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	10:34
BLANK TEST	0.000	10:35
INTERNAL STANDARD	VERIFIED	10:35
Xq = 0.106 (0.17%)	0.076	10:35
EXTERNAL STANDARD	X[1] = 0.0762 (-0.0022)	(0.0024)
BLANK TEST	0.000	10:36
SUBJECT SAMPLE (Vol=1.90L)	0.089	10:37
X[1] = 0.0895 (-0.0018)	(0.0000)	10:38
BLANK TEST	0.076	10:38
EXTERNAL STANDARD	X[1] = 0.0759 (-0.0021)	(0.0012)
BLANK TEST	0.000	10:39

CVG

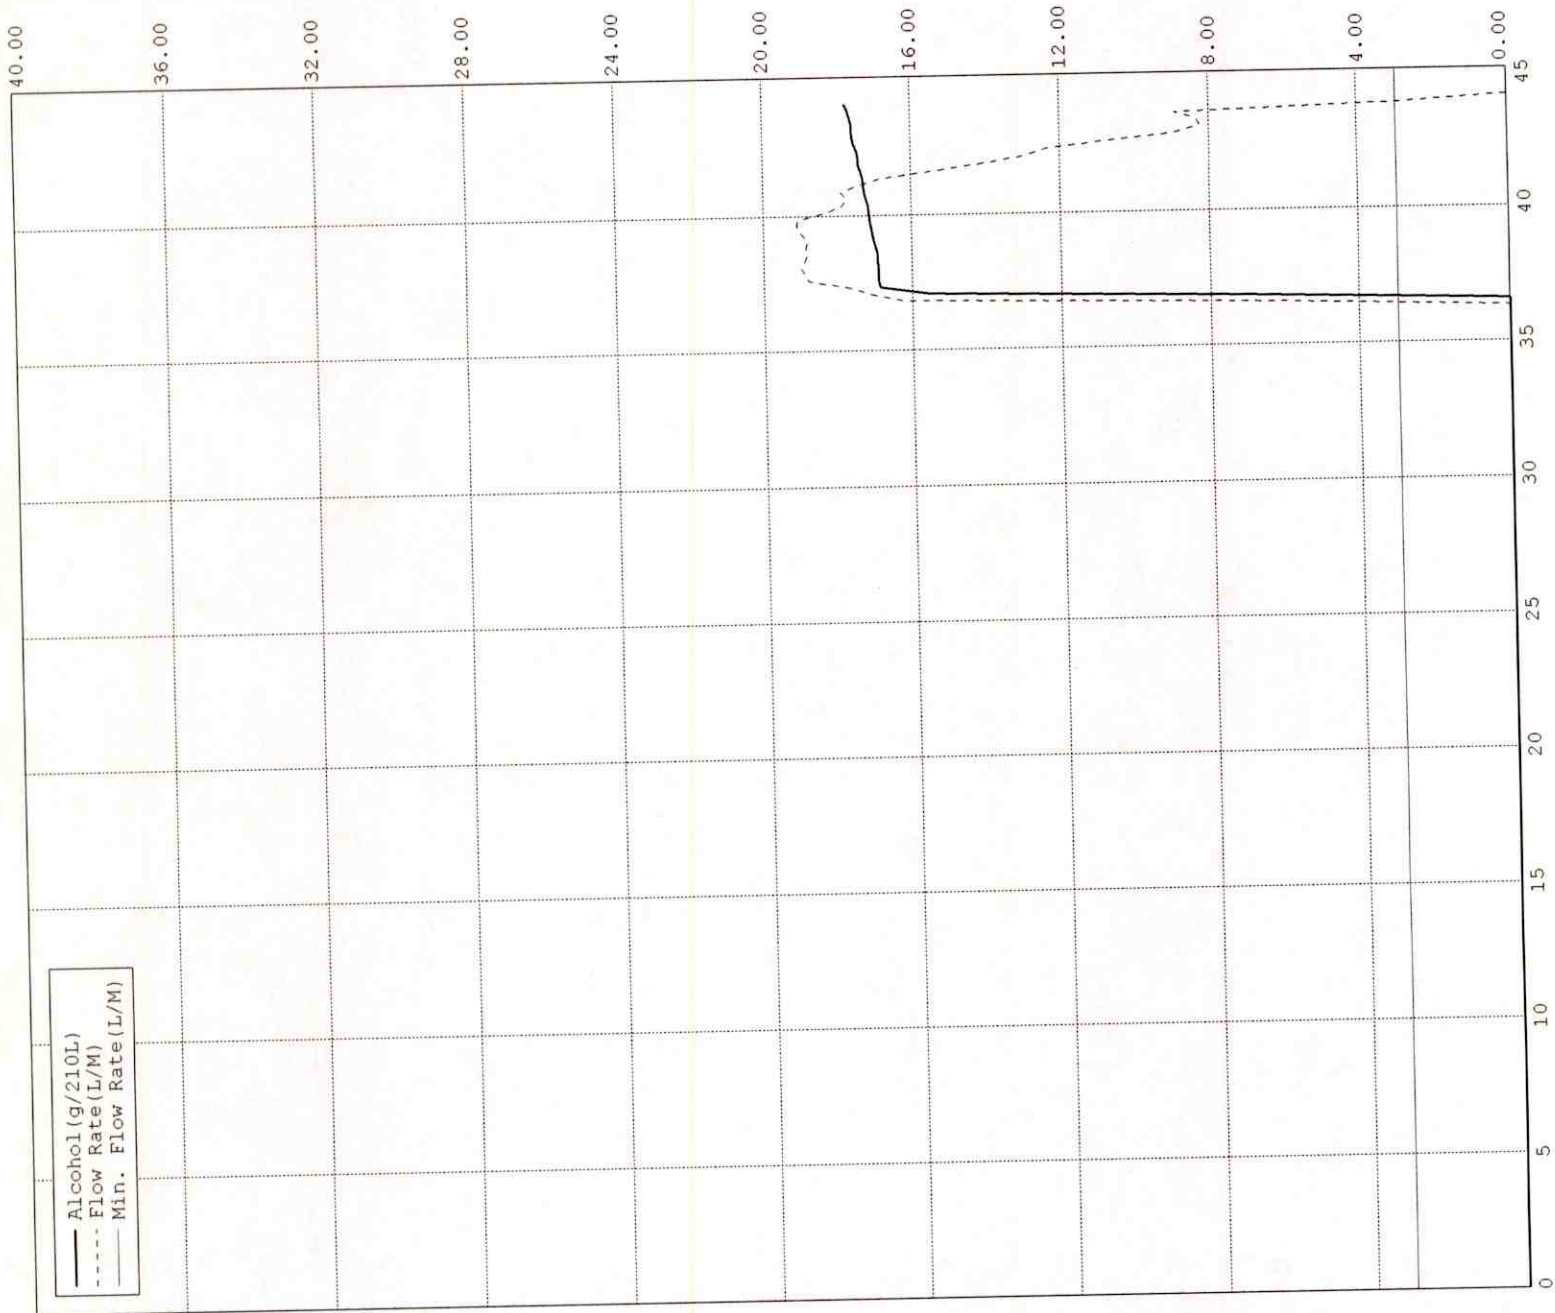

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100667

Date: 12/01/2023  
Time: 11:13:14

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 28.99: 0.077  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	11:14
BLANK TEST	0.000	11:14
INTERNAL STANDARD	VERIFIED	11:14
EXTERNAL STANDARD	0.077	11:14
BLANK TEST	0.000	11:15
SUBJECT SAMPLE (Vol=1.60L)	0.000	11:16
BLANK TEST	0.000	11:17
EXTERNAL STANDARD	0.076	11:17
BLANK TEST	0.000	11:18

