

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100386

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 09/17/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.72: 0.077
LOT #: 09214080A3
EXPIRATION: 05/01/2016
TANK PRESSURE: 493 psi

BLANK TEST	0.000	13:27
INTERNAL STANDARD	VERIFIED	13:27
EXTERNAL STANDARD	0.076	13:28
BLANK TEST	0.000	13:28
EXTERNAL STANDARD	0.075	13:29
BLANK TEST	0.000	13:30
EXTERNAL STANDARD	0.075	13:30
BLANK TEST	0.000	13:31
EXTERNAL STANDARD	0.075	13:31
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.076	13:32
BLANK TEST	0.000	13:33

Average = 0.0754
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 3.01
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
Breath Tube = 45.0°C PASSED

PUMP INFO

Flow Rate = 4.745 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO


Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

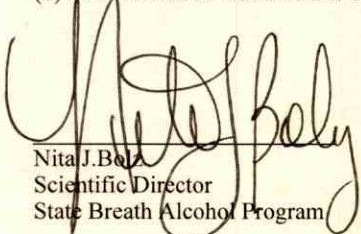
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

11/6/2015

Subscribed and sworn before me this 6th day of NOV, 20 15


Nikki Roth, Notary Public
My Commission Expires With Office

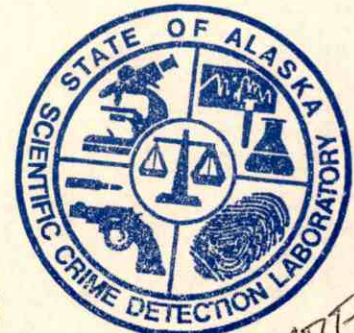

CRT
10/26/15