



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100363

**Report Issue Date:** 12/05/2022  
**Date Received:** Not Recorded  
**Condition of Item:** Not Recorded

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**No As-Found Data Collected**

**Start Date 11/14/2022 - As Left - End Date 11/15/2022**

As Left Conditions - Barometric Pressure (inHg): 29.97 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.7 Relative Humidity (%): 21

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG100401	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG111710	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.080	AG113402	0.080	0.080	0.079	0.079	0.080	0.080	+/- 0.003
0.100	0.100	AG108404	0.101	0.100	0.100	0.100	0.100	0.100	+/- 0.003
0.150	0.150	AG134205	0.151	0.150	0.150	0.150	0.150	0.150	+/- 0.004
0.300	0.301	AG130502	0.298	0.298	0.298	0.298	0.298	0.298	+/- 0.008

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Technically and administratively reviewed by Brandi Barnett on 12/05/2022

Results authorized by Colleen O'Bryant on 12/05/2022  
[colleen.obryant@alaska.gov](mailto:colleen.obryant@alaska.gov)

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100363 Analyst: C. O'Bryant Start Date: 11/14/22

- Diagnostic Test (attached)
- Adjust voltages, if needed
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Internal Standard value  $\leq$  3.00%
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.5 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.97 Temperature (C): 22.7 Relative Humidity (%): 21

Linearity Test (attached)

0.020g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG100401</u>	Exp:	<u>1/4/23</u>
0.040g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG111710</u>	Exp:	<u>4/07/23</u>
0.080g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG113402</u>	Exp:	<u>5/14/23</u>
0.100g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG108404</u>	Exp:	<u>3/25/23</u>
0.150g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG134205</u>	Exp:	<u>12/8/23</u>
0.300g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG130502</u>	Exp:	<u>11/01/23</u>

Functional Tests (attached)

- Incomplete
- Maximum Attempts Exceeded
- Interference (Volatiles)
- Invalid
- Radio Frequency Interference (RFI)

Acetone Mnf: Lifeloc Lot: 21DP41158 Level: 0.100 Exp: 4/29/23

Simulator S/N: SD1200 Verification Performed?

Isopropanol Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: DR4176 Verification Performed?

Neg. Control Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: DR4162 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/9/23

- Verify stylus is calibrated
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Non-Drinking Subject Test
- Upload
- Remove Tank Prior to Shutdown
- COB  
Calibration End Date: 2022.11.15 2022.11.15

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100363  
-----

Date: 11/14/2022  
Time: 13:45:39

VERSIONS  
DMT: 3.02 ✓  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 48.1°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.77 V PASSED  
(1.06 V - 2.48 V)  
Cooler Voltage = 1.81 V PASSED  
(1.09 V - 2.53 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 519 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 30.0 in

PUMP INFO

Flow Rate = 4.106 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED

Xq = 0.080 0.11% (0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100363  
-----

Date: 11/14/2022  
Time: 1:54 PM

Temperatures (°C)  
Sample Cell: 48.9°C  
Breath Tube: 48.1°C

Current Barometer 30.0 in  
Volume (Ltr) 1.54

Settings  
Lamp: 1.77 V  
Bias: 80 V  
Cooler: 1.79 V  
Chopper: 518 Hz

Voltages (V)  
Flow: 1.05 V  
Detector: -0.061 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100363  
-----

Date: 08/30/2022  
Time: 07:45:41

OPERATOR NAME:  
CARLIE GLAISTER  
CERTIFICATE #: 10436

Ca = 0.1000  
CAL = 0.976806    0.800 <= CAL < 1.200  
b1 = 0.0009    0.0000 <= b1 < 0.0040  
b2 = 0.0040    0.0010 <= b2 < 0.0100  
b3 = 0.0003    0.0000 <= b3 < 0.0040  
Xq = 0.0803    0.0500 <= Xq < 0.2000  
a21 = 1.070752    1.050 <= a21 < 1.300  
a31 = 0.466291    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100363

Date: 11/14/2022

Time: 13:56:37

SUBJECT NAME:

TEST TEST

LICENSE #: VOLUME TEST

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 22-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.97: 0.080


LOT #: AG113402

EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK

BLANK TEST	0.000	PASSED	13:58
INTERNAL STANDARD	0.080	VERIFIED	13:58
EXTERNAL STANDARD	0.080		13:59
BLANK TEST	0.000		14:00
SUBJECT SAMPLE (Vol=1.58L)	0.000		14:01
BLANK TEST	0.000		14:01
EXTERNAL STANDARD	0.080		14:02
BLANK TEST	0.000		14:03

Alcohol (g/210L)  
Flow Rate (L/M)  
Min. Flow Rate (L/M)

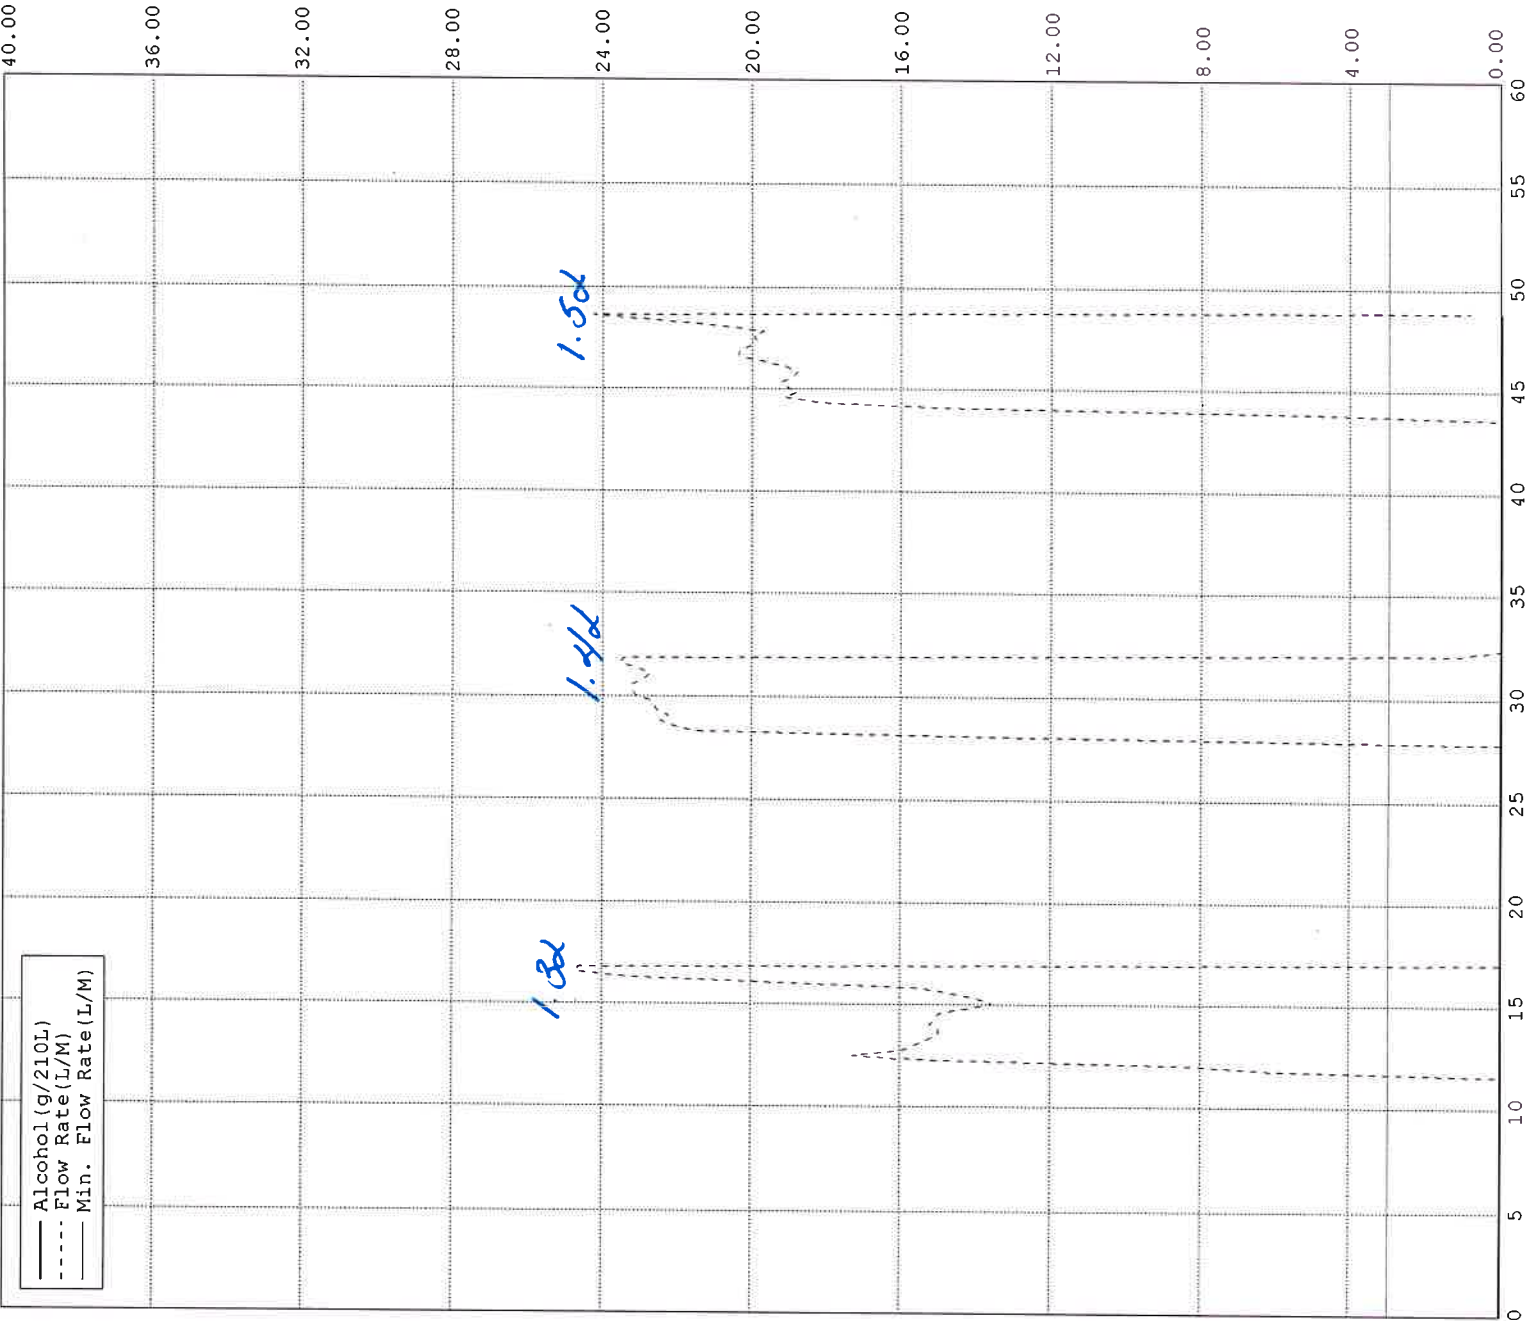

LINEARITY CHECK

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100363  
 -----


Date: 11/14/2022  
 Time: 14:08:26

SUPERVISOR NAME:  
 COLLEEN S O'BRYAN  
 OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.040	0.0400	0.0000
0.080	0.0796	0.0005
0.100	0.1002	0.0004
0.150	0.1502	0.0004
0.301	0.2980	0.0000

SLOPE = 0.989609  
 R<sup>2</sup> = 0.999958

*COS*

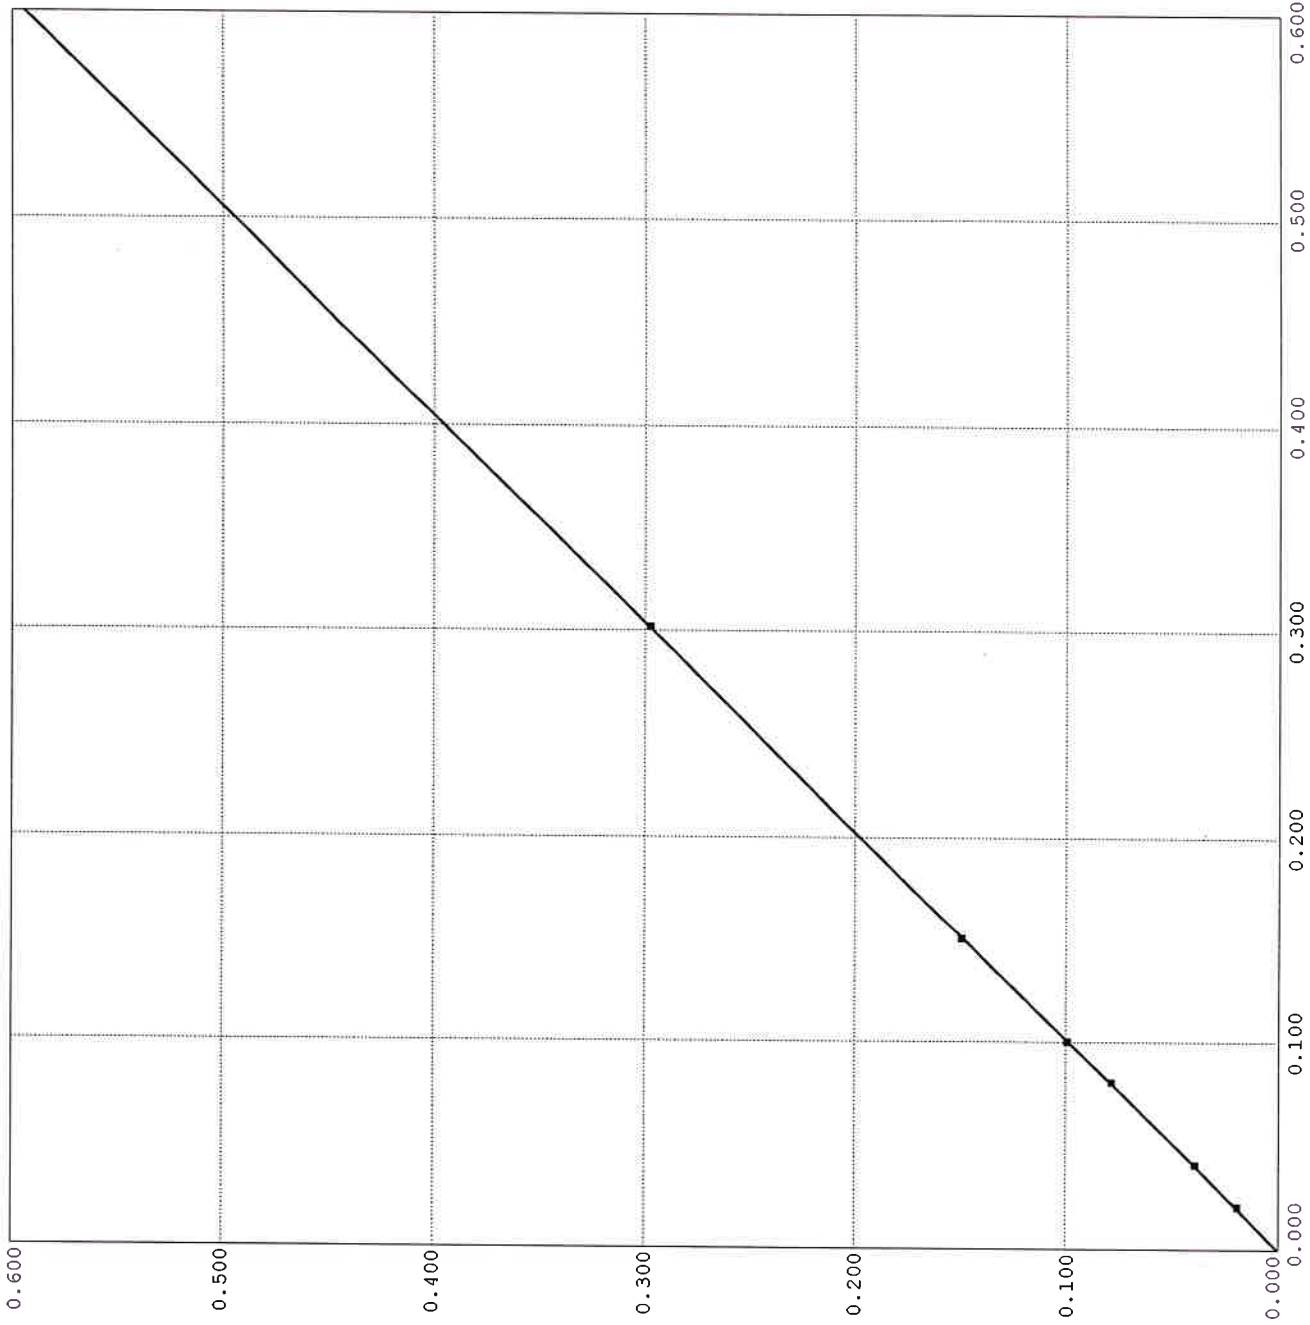

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100363






Date: 11/14/2022  
Time: 14:08:28

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.98: 0.020  
LOT #: AG100401  
EXPIRATION: 01/04/2023  
TANK PRESSURE: 241 psi

BLANK TEST	0.000	14:09
INTERNAL STANDARD	VERIFIED	14:10
EXTERNAL STANDARD	0.020	14:10
BLANK TEST	0.000	14:11
EXTERNAL STANDARD	0.020	14:11
BLANK TEST	0.000	14:12
EXTERNAL STANDARD	0.020	14:12
BLANK TEST	0.000	14:13
EXTERNAL STANDARD	0.020	14:13
BLANK TEST	0.000	14:14
EXTERNAL STANDARD	0.020	14:14
BLANK TEST	0.000	14:15

Average = 0.0200  
Std Dev = 0.0000

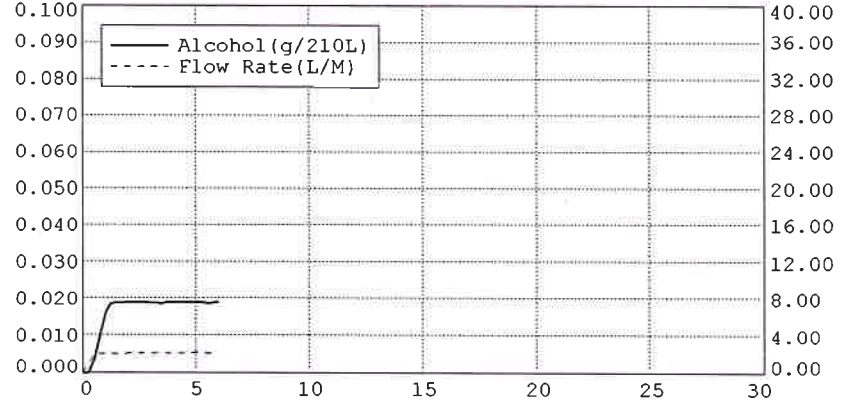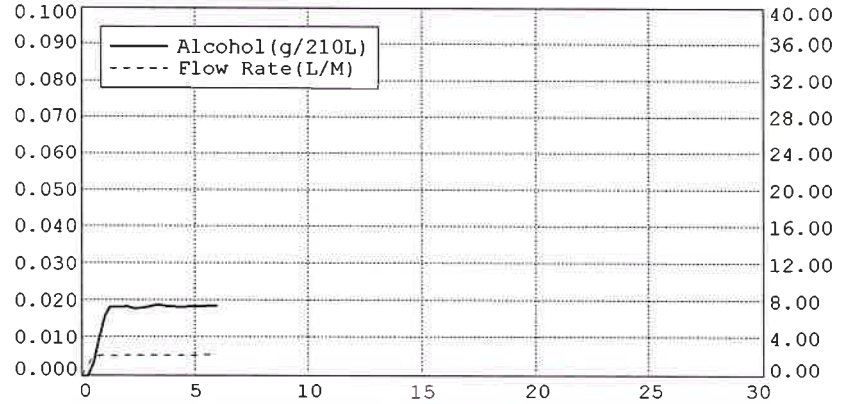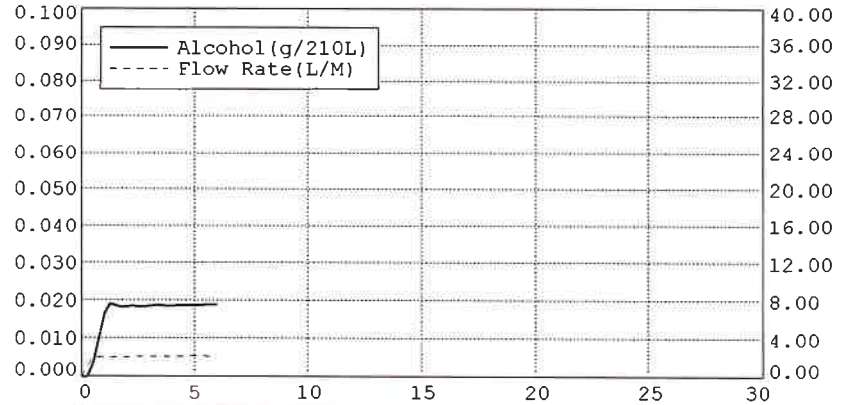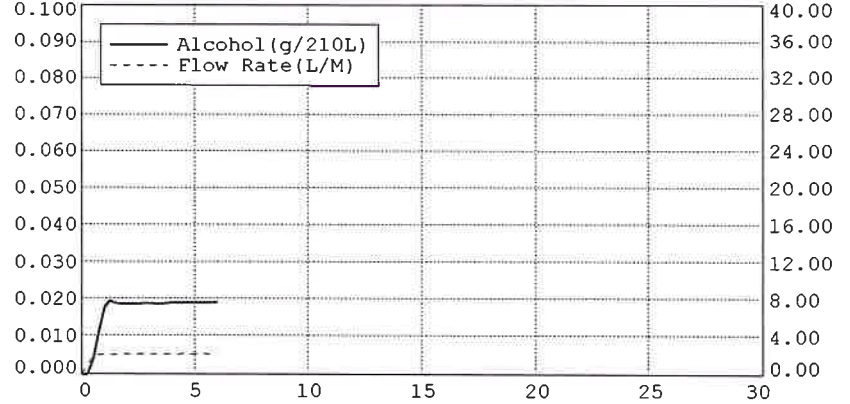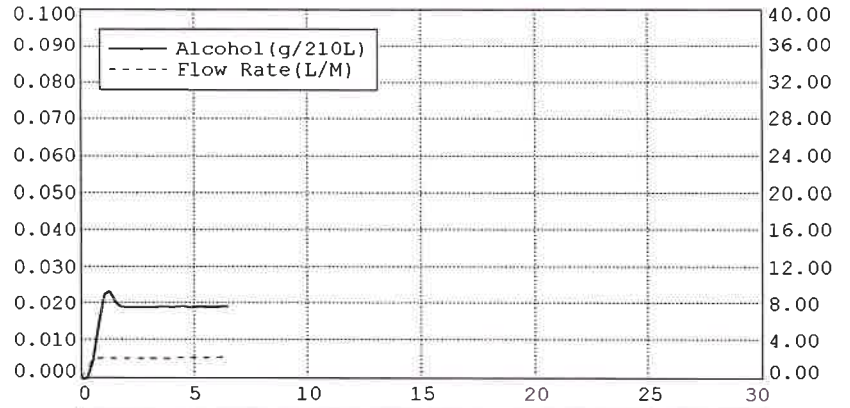



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100363






Date: 11/14/2022  
 Time: 14:16:05

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.98: 0.040  
 LOT #: AG111710  
 EXPIRATION: 04/27/2023  
 TANK PRESSURE: 417 psi

BLANK TEST	0.000	14:17
INTERNAL STANDARD	VERIFIED	14:17
EXTERNAL STANDARD	0.040	14:17
BLANK TEST	0.000	14:18
EXTERNAL STANDARD	0.040	14:18
BLANK TEST	0.000	14:19
EXTERNAL STANDARD	0.040	14:20
BLANK TEST	0.000	14:20
EXTERNAL STANDARD	0.040	14:21
BLANK TEST	0.000	14:22
EXTERNAL STANDARD	0.040	14:22
BLANK TEST	0.000	14:23

Average = 0.0400  
 Std Dev = 0.0000

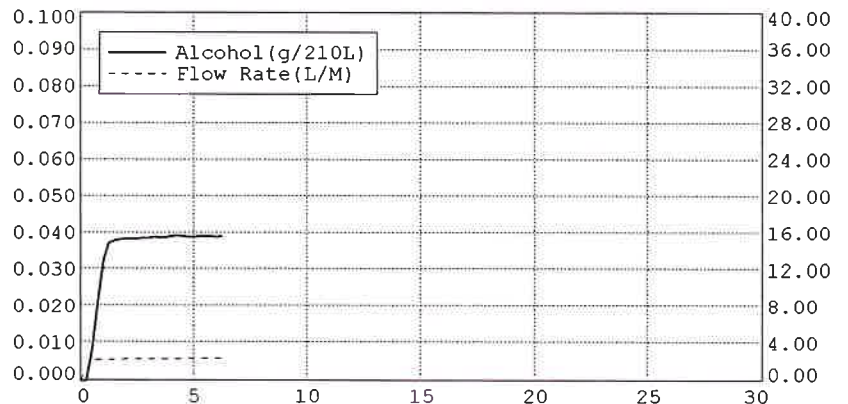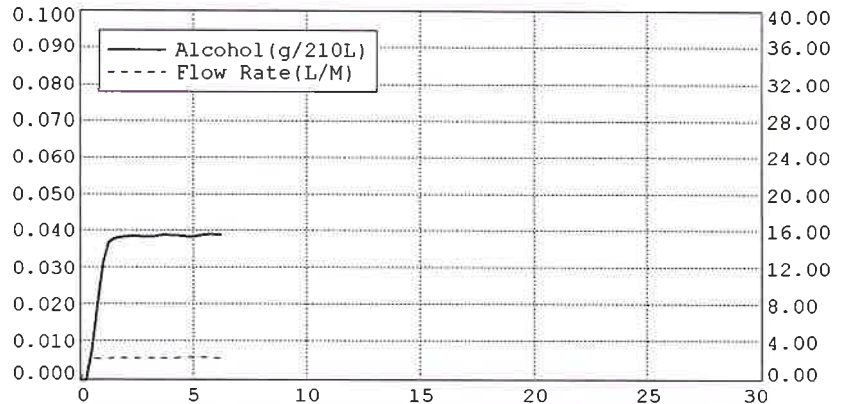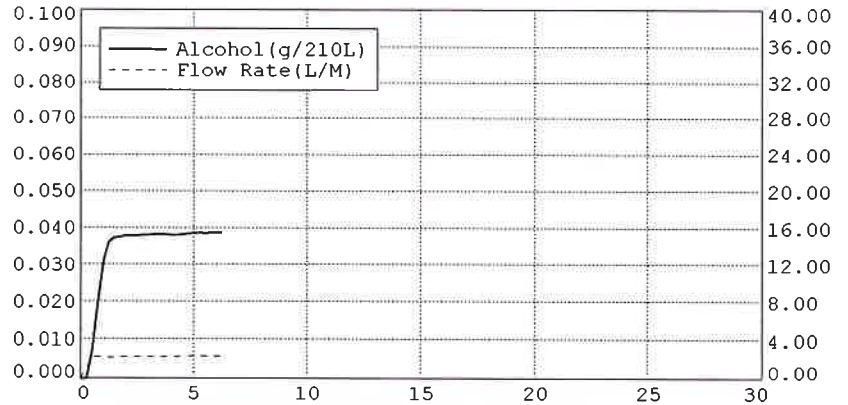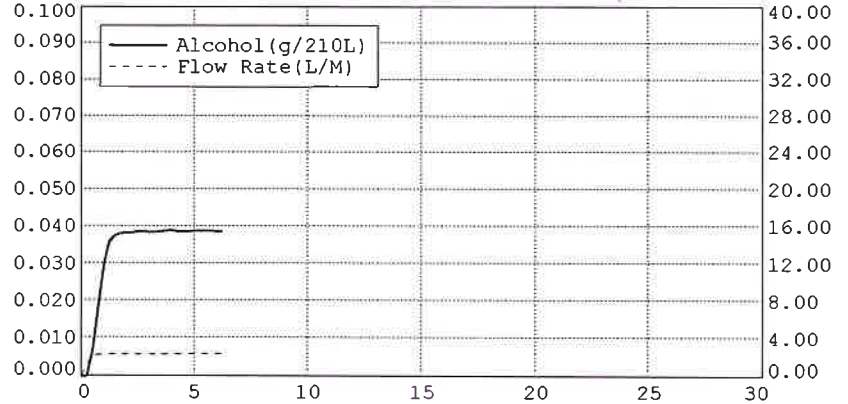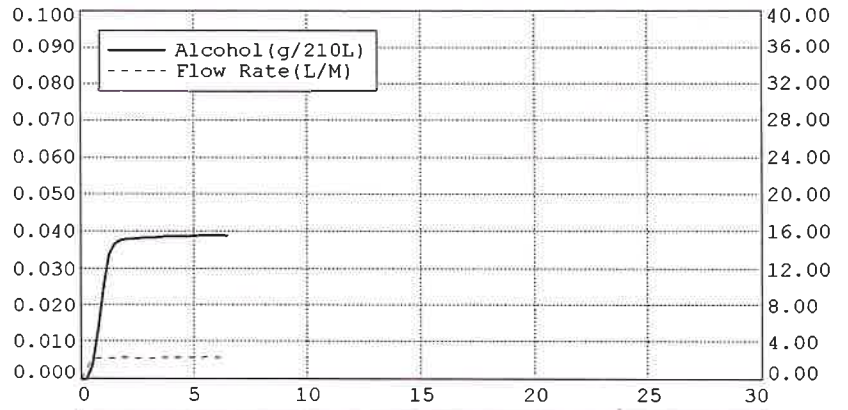

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100363






Date: 11/14/2022  
 Time: 14:23:34

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.98: 0.080  
 LOT #: AG113402  
 EXPIRATION: 05/14/2023  
 TANK PRESSURE: 1042 psi

BLANK TEST	0.000	14:26
INTERNAL STANDARD	VERIFIED	14:26
EXTERNAL STANDARD	0.080	14:26
BLANK TEST	0.000	14:27
EXTERNAL STANDARD	0.080	14:27
BLANK TEST	0.000	14:28
EXTERNAL STANDARD	0.079	14:28
BLANK TEST	0.000	14:29
EXTERNAL STANDARD	0.079	14:29
BLANK TEST	0.000	14:30
EXTERNAL STANDARD	0.080	14:31
BLANK TEST	0.000	14:32

Average = 0.0796  
 Std Dev = 0.0005

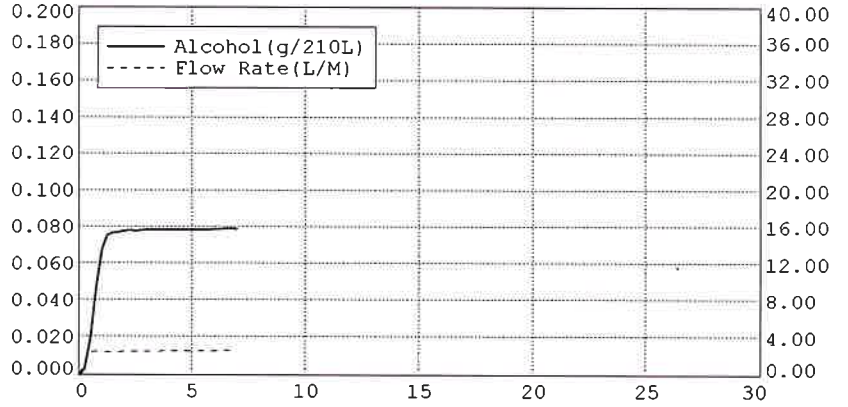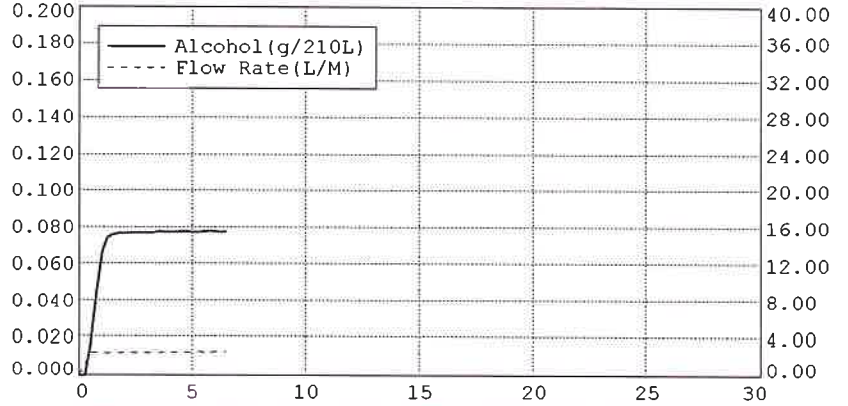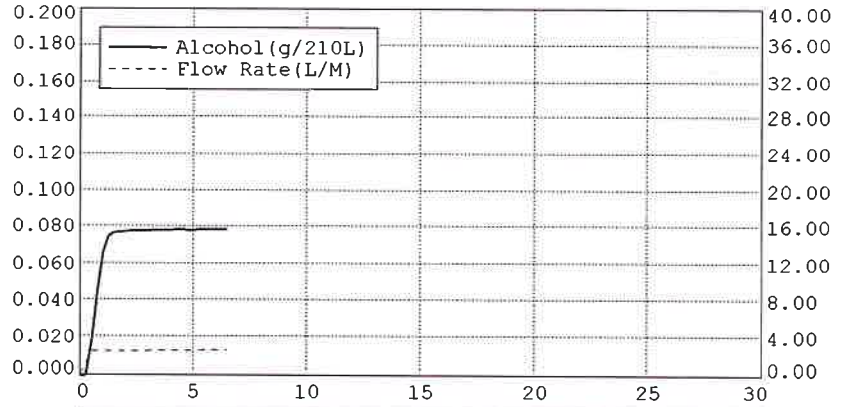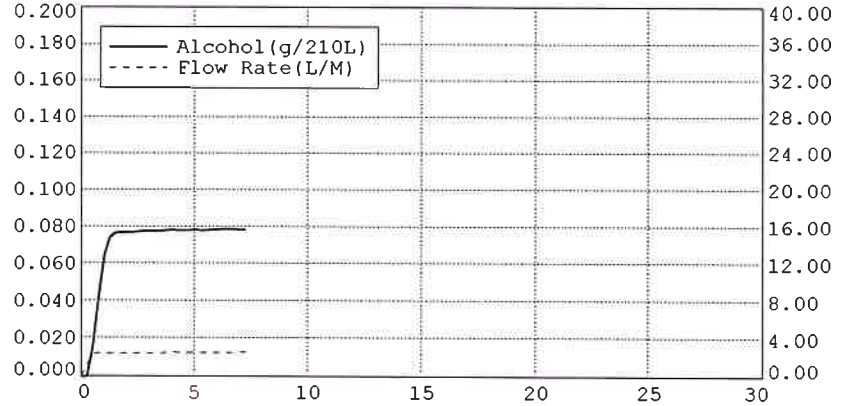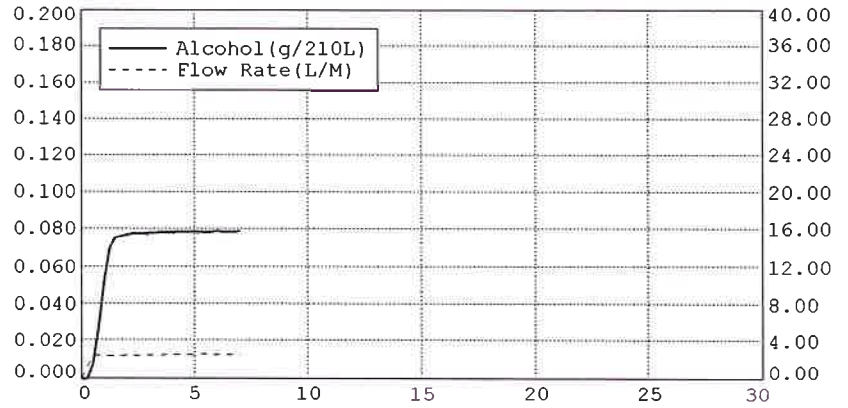

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100363






Date: 11/14/2022  
 Time: 14:32:28

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.98: 0.100  
 LOT #: AG108404  
 EXPIRATION: 03/25/2023  
 TANK PRESSURE: 126 psi

BLANK TEST	0.000	14:33
INTERNAL STANDARD	VERIFIED	14:33
EXTERNAL STANDARD	0.101	14:34
BLANK TEST	0.000	14:34
EXTERNAL STANDARD	0.100	14:35
BLANK TEST	0.000	14:36
EXTERNAL STANDARD	0.100	14:36
BLANK TEST	0.000	14:37
EXTERNAL STANDARD	0.100	14:37
BLANK TEST	0.000	14:38
EXTERNAL STANDARD	0.100	14:38
BLANK TEST	0.000	14:39

Average = 0.1002  
 Std Dev = 0.0004

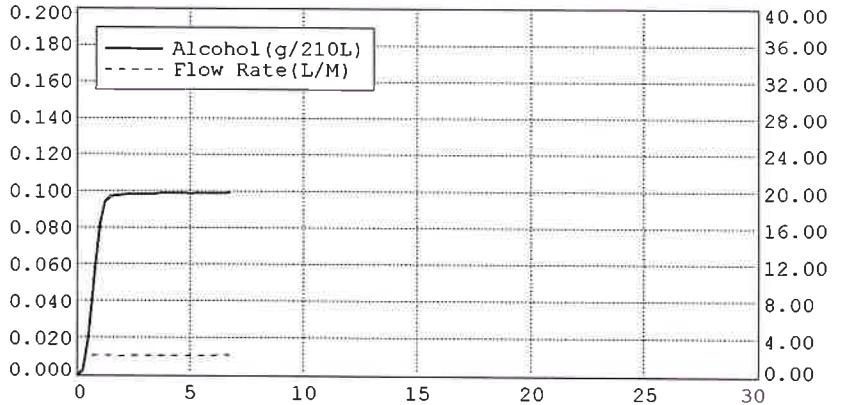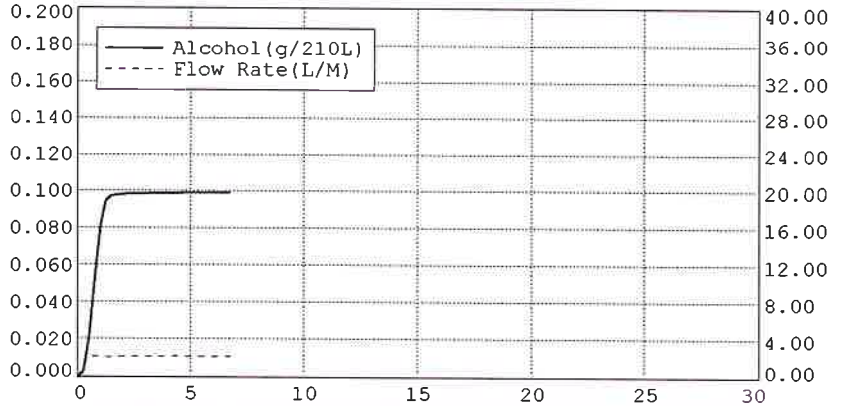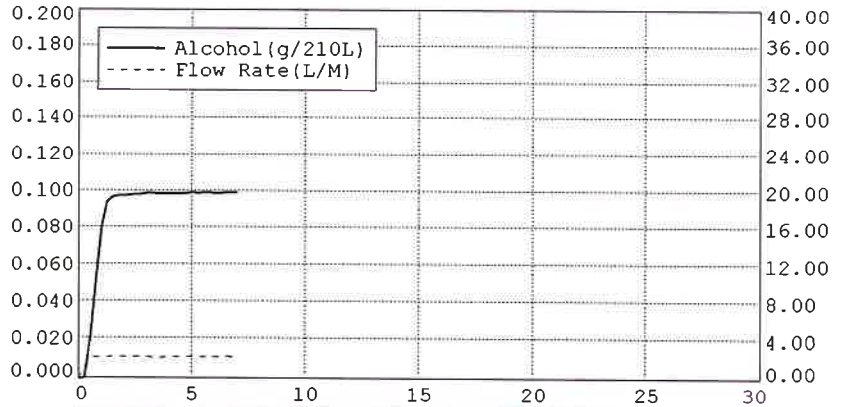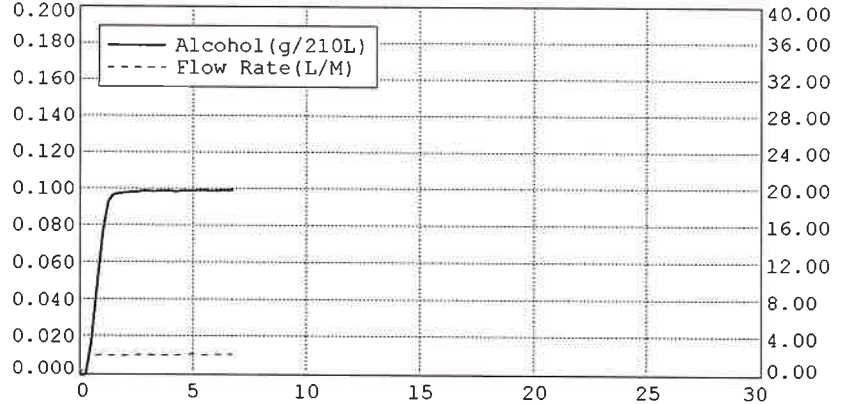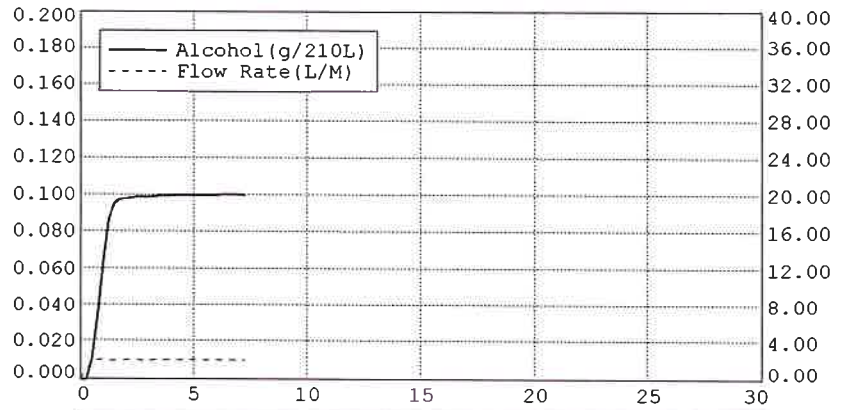

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100363






Date: 11/14/2022  
 Time: 14:41:14

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.98: 0.150  
 LOT #: AG134205  
 EXPIRATION: 12/08/2023  
 TANK PRESSURE: 716 psi

BLANK TEST	0.000	14:42
INTERNAL STANDARD	VERIFIED	14:42
EXTERNAL STANDARD	0.151	14:42
BLANK TEST	0.000	14:43
EXTERNAL STANDARD	0.150	14:43
BLANK TEST	0.000	14:44
EXTERNAL STANDARD	0.150	14:45
BLANK TEST	0.000	14:45
EXTERNAL STANDARD	0.150	14:46
BLANK TEST	0.000	14:47
EXTERNAL STANDARD	0.150	14:47
BLANK TEST	0.000	14:48

Average = 0.1502  
 Std Dev = 0.0004

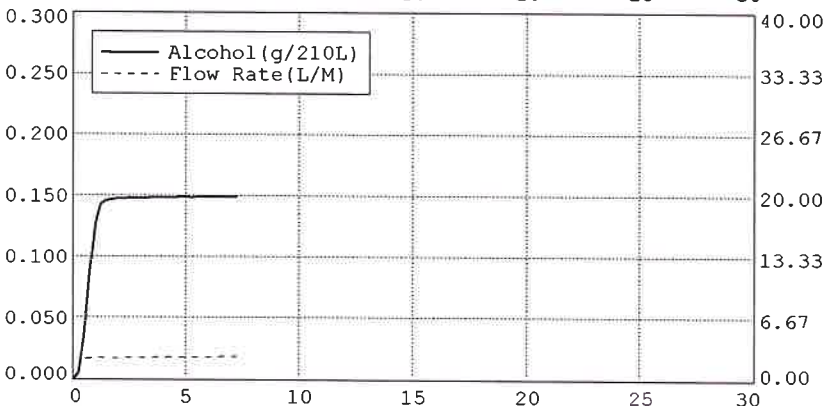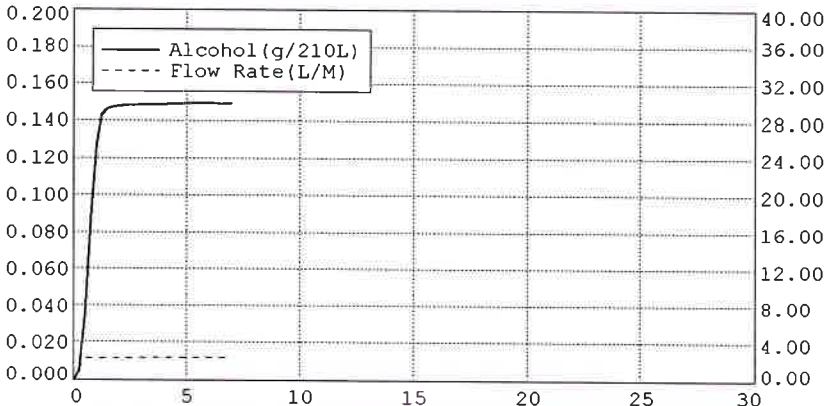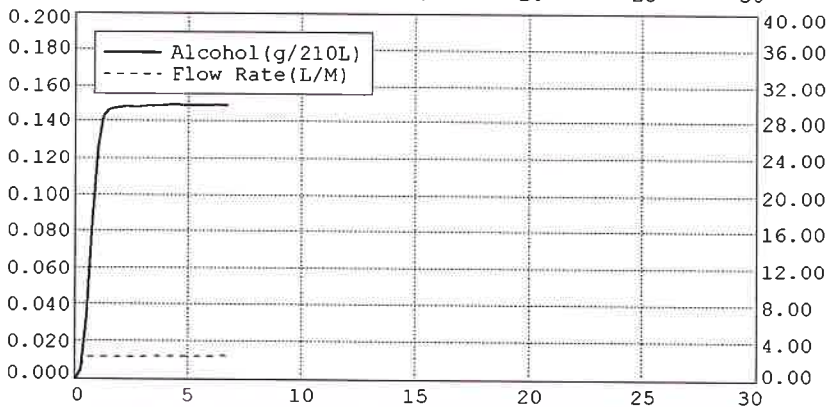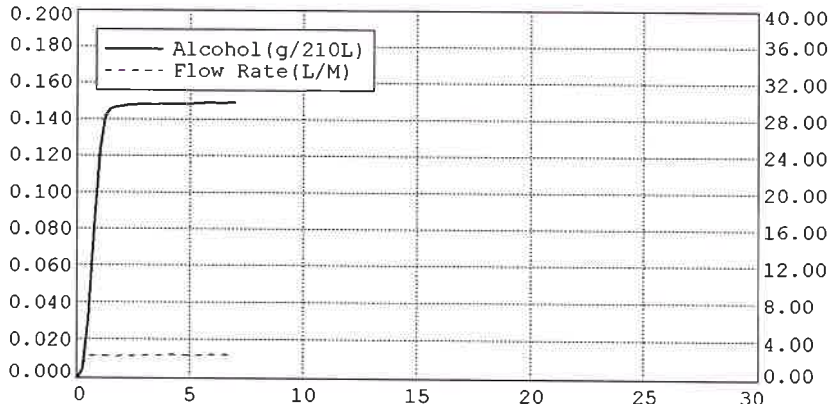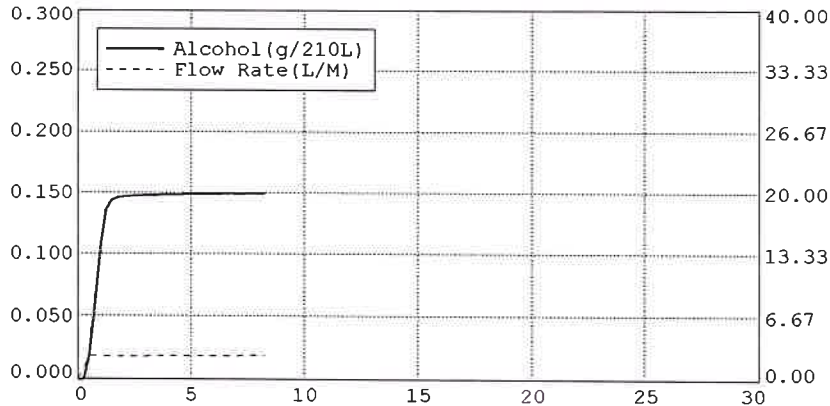

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100363






Date: 11/14/2022  
 Time: 14:48:57

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.99: 0.301  
 LOT #: AG130502  
 EXPIRATION: 11/01/2023  
 TANK PRESSURE: 383 psi

BLANK TEST	0.000	14:50
INTERNAL STANDARD	VERIFIED	14:50
EXTERNAL STANDARD	0.298	14:50
BLANK TEST	0.000	14:51
EXTERNAL STANDARD	0.298	14:51
BLANK TEST	0.000	14:52
EXTERNAL STANDARD	0.298	14:52
BLANK TEST	0.000	14:53
EXTERNAL STANDARD	0.298	14:54
BLANK TEST	0.000	14:54
EXTERNAL STANDARD	0.298	14:55
BLANK TEST	0.000	14:56

Average = 0.2980  
 Std Dev = 0.0000

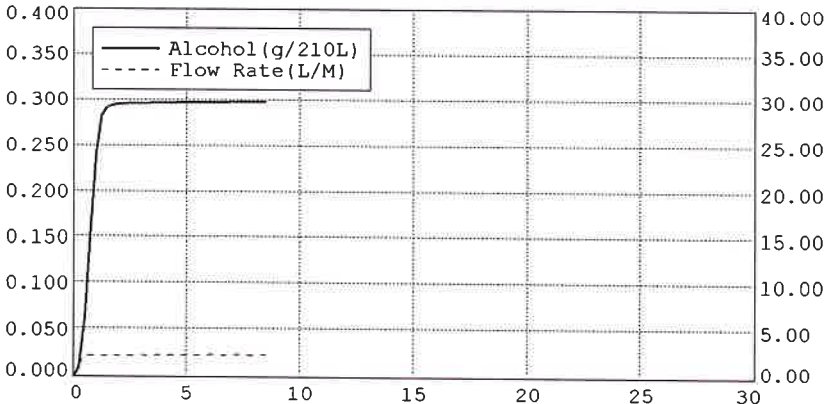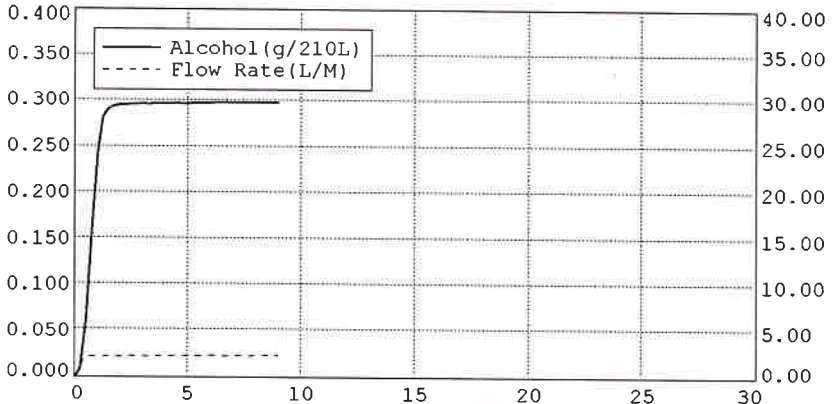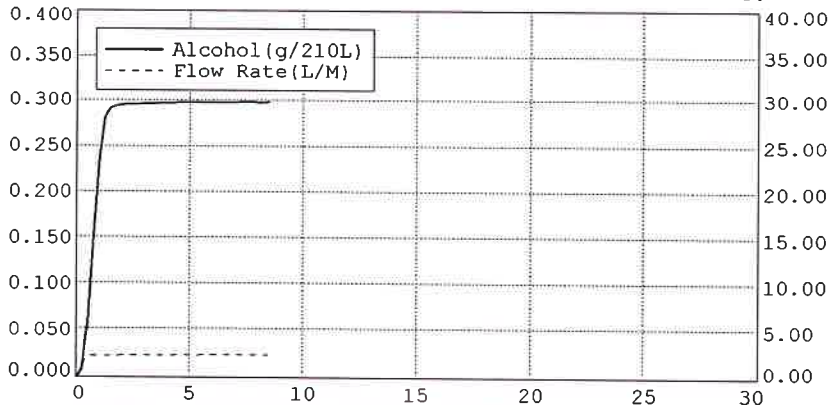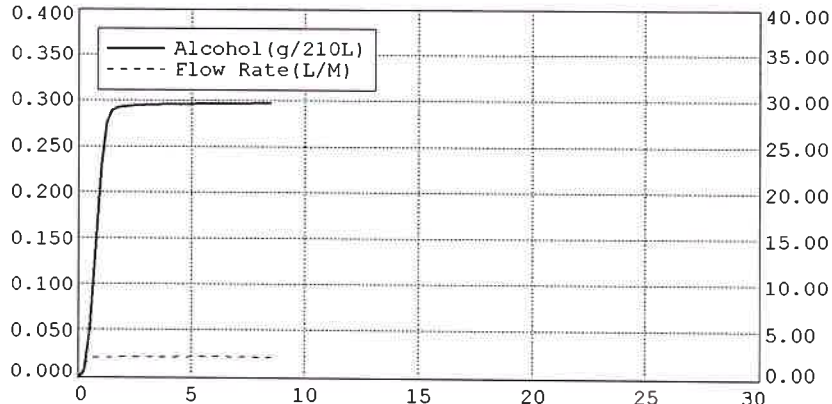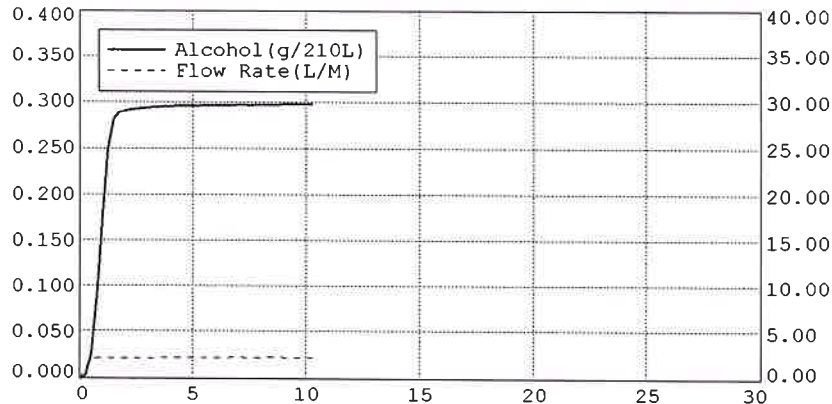

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100363

Date: 11/14/2022

Time: 15:02:08

SUBJECT NAME:

TEST TEST

LICENSE #: INCOMPLETE

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 22-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 30.00: 0.080

LOT #: AG113402

EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED

0.000

VERIFIED

0.081

0.000

INCOMPLETE

15:04


15:04

15:04

15:04

15:05

15:07

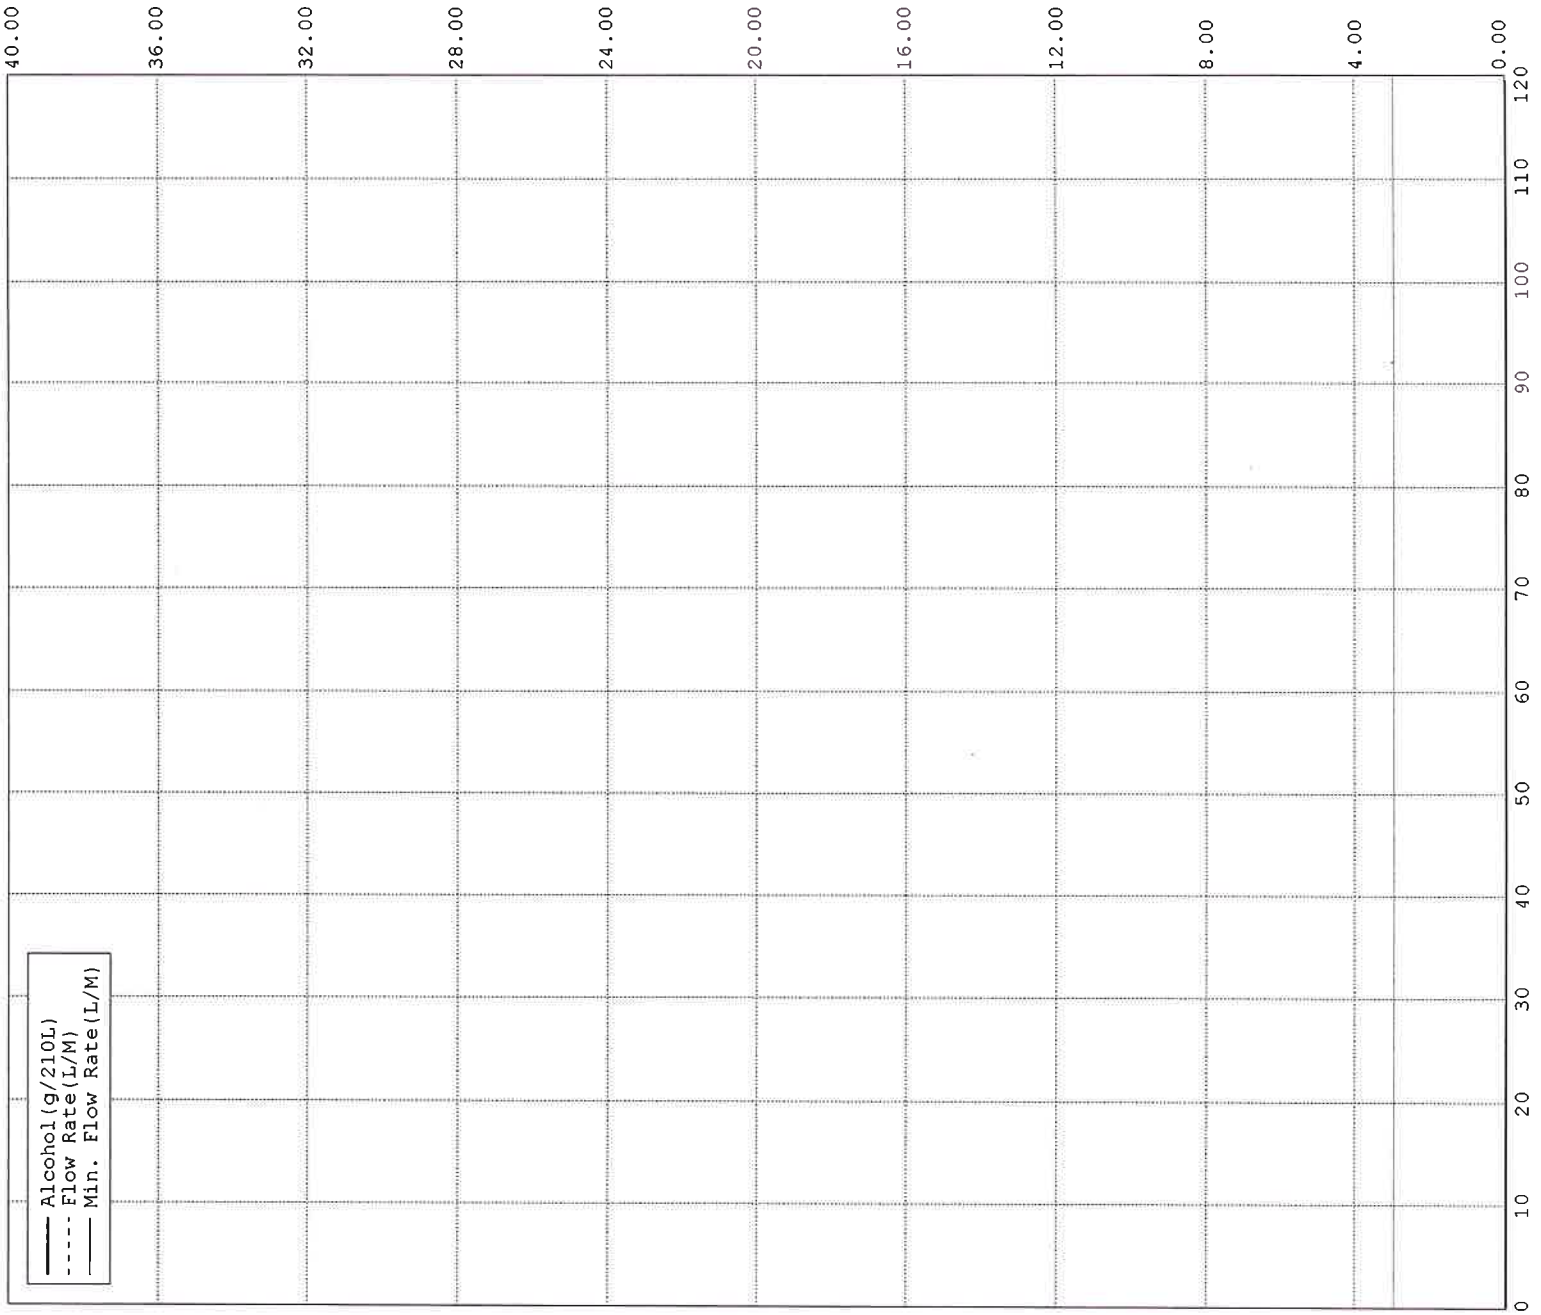

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100363

Date: 11/14/2022

Time: 15:11:22

SUBJECT NAME:

TEST TEST

LICENSE #: MAX ATTEMPTS

OPERATOR NAME:

COLLEEN S OBRyant

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 22-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 30.01: 0.080

LOT #: AG113402

EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 15:12  
0.000 15:12  
VERIFIED 15:13  
0.080 15:13  
0.000 15:14  
XXX 15:15

Maximum Attempts Exceeded

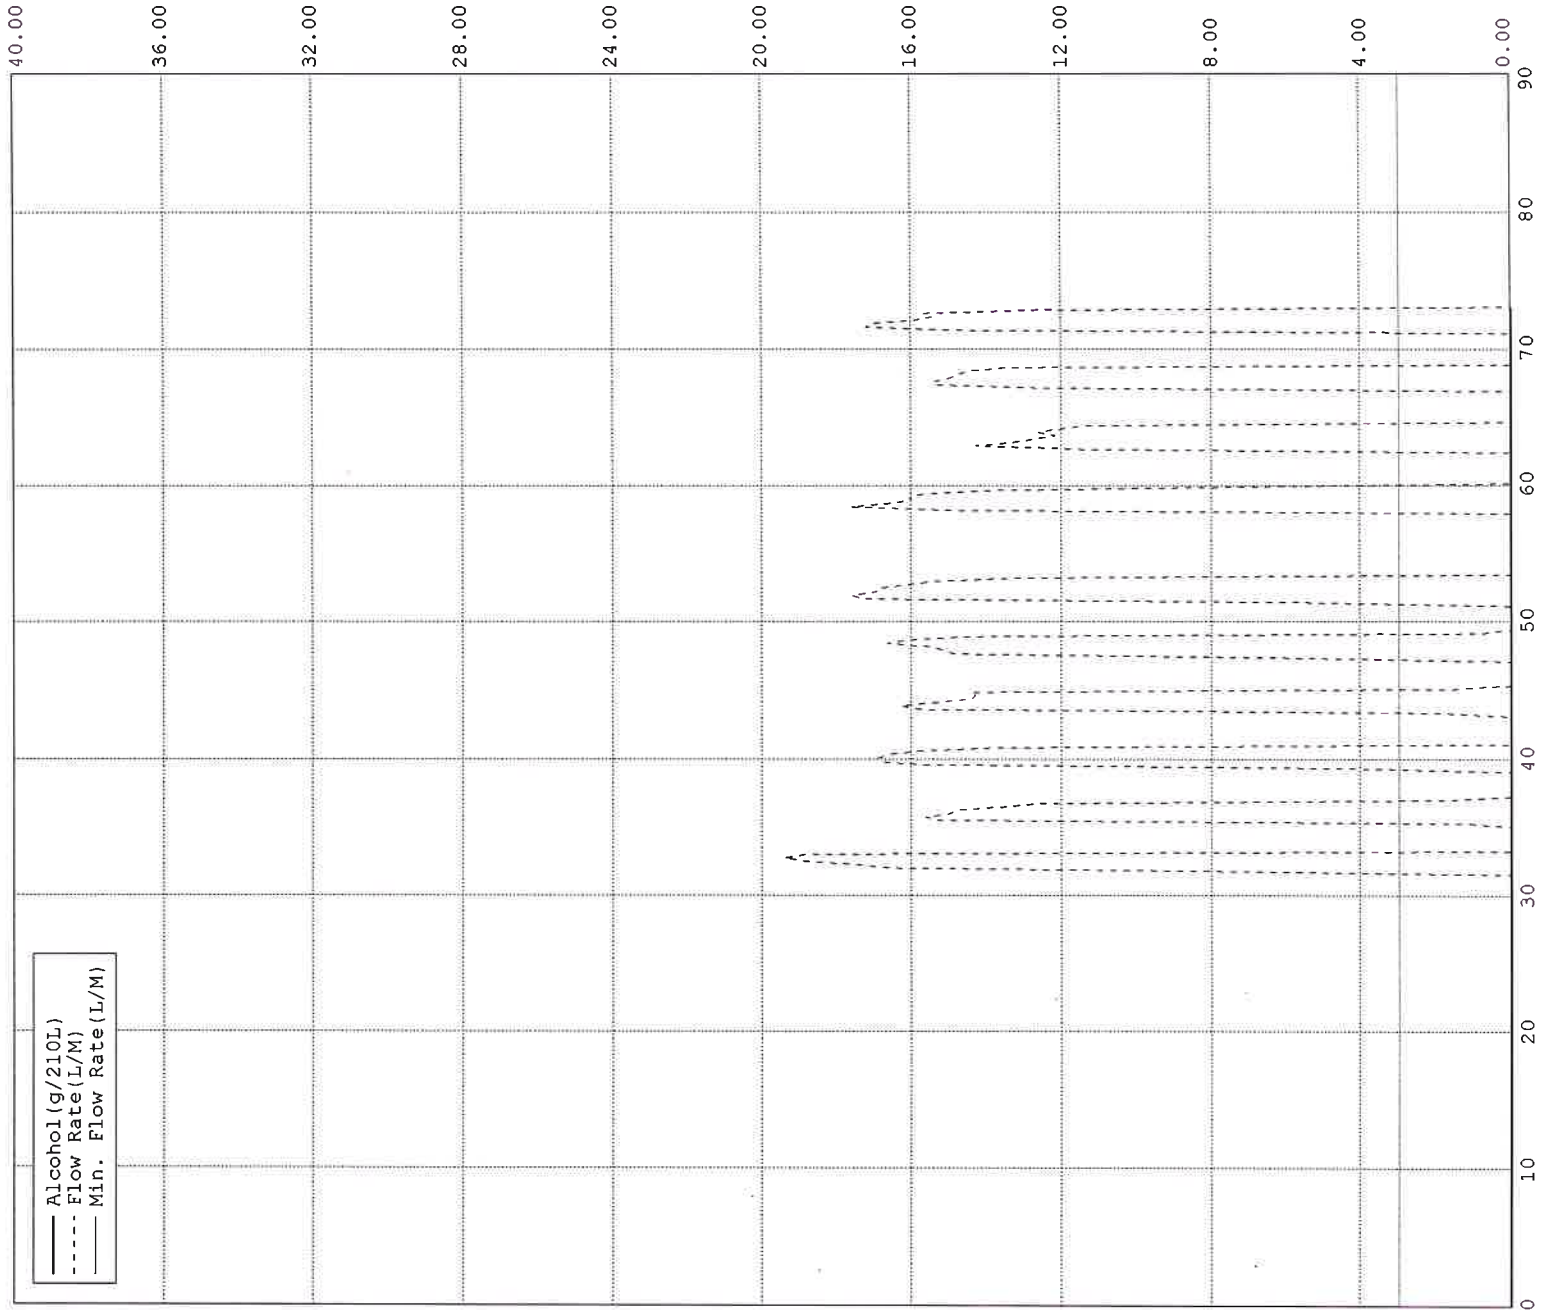

SUBJECT TEST

Alaska Department of Public Safety  
DATA MASTER dmt: 100363

Date: 11/14/2022  
Time: 15:21:13

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-ACETONE

OPERATOR NAME:  
COLLIEN S OBRVANT  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 22-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 30.00: 0.080  
LOT #: AG113402  
EXPIRATION: 05/14/2023


DIAGNOSTIC CHECK PASSED 15:22  
BLANK TEST 0.000 15:22  
INTERNAL STANDARD VERIFIED 15:23  
Xq = 0.080 (0.00%) 0.080 15:23  
EXTERNAL STANDARD (0.0033)  
X[1] = 0.0799 (-0.0007) (0.0033)  
BLANK TEST 0.000 15:24  
SUBJECT SAMPLE XXX 15:24  
X[1] = 0.1078 (-0.0157) (0.0028)

Interference Detected

*Filter 2 Avg = -0.0004*

*Filter 3 Avg = 0.0034*

*CO2*

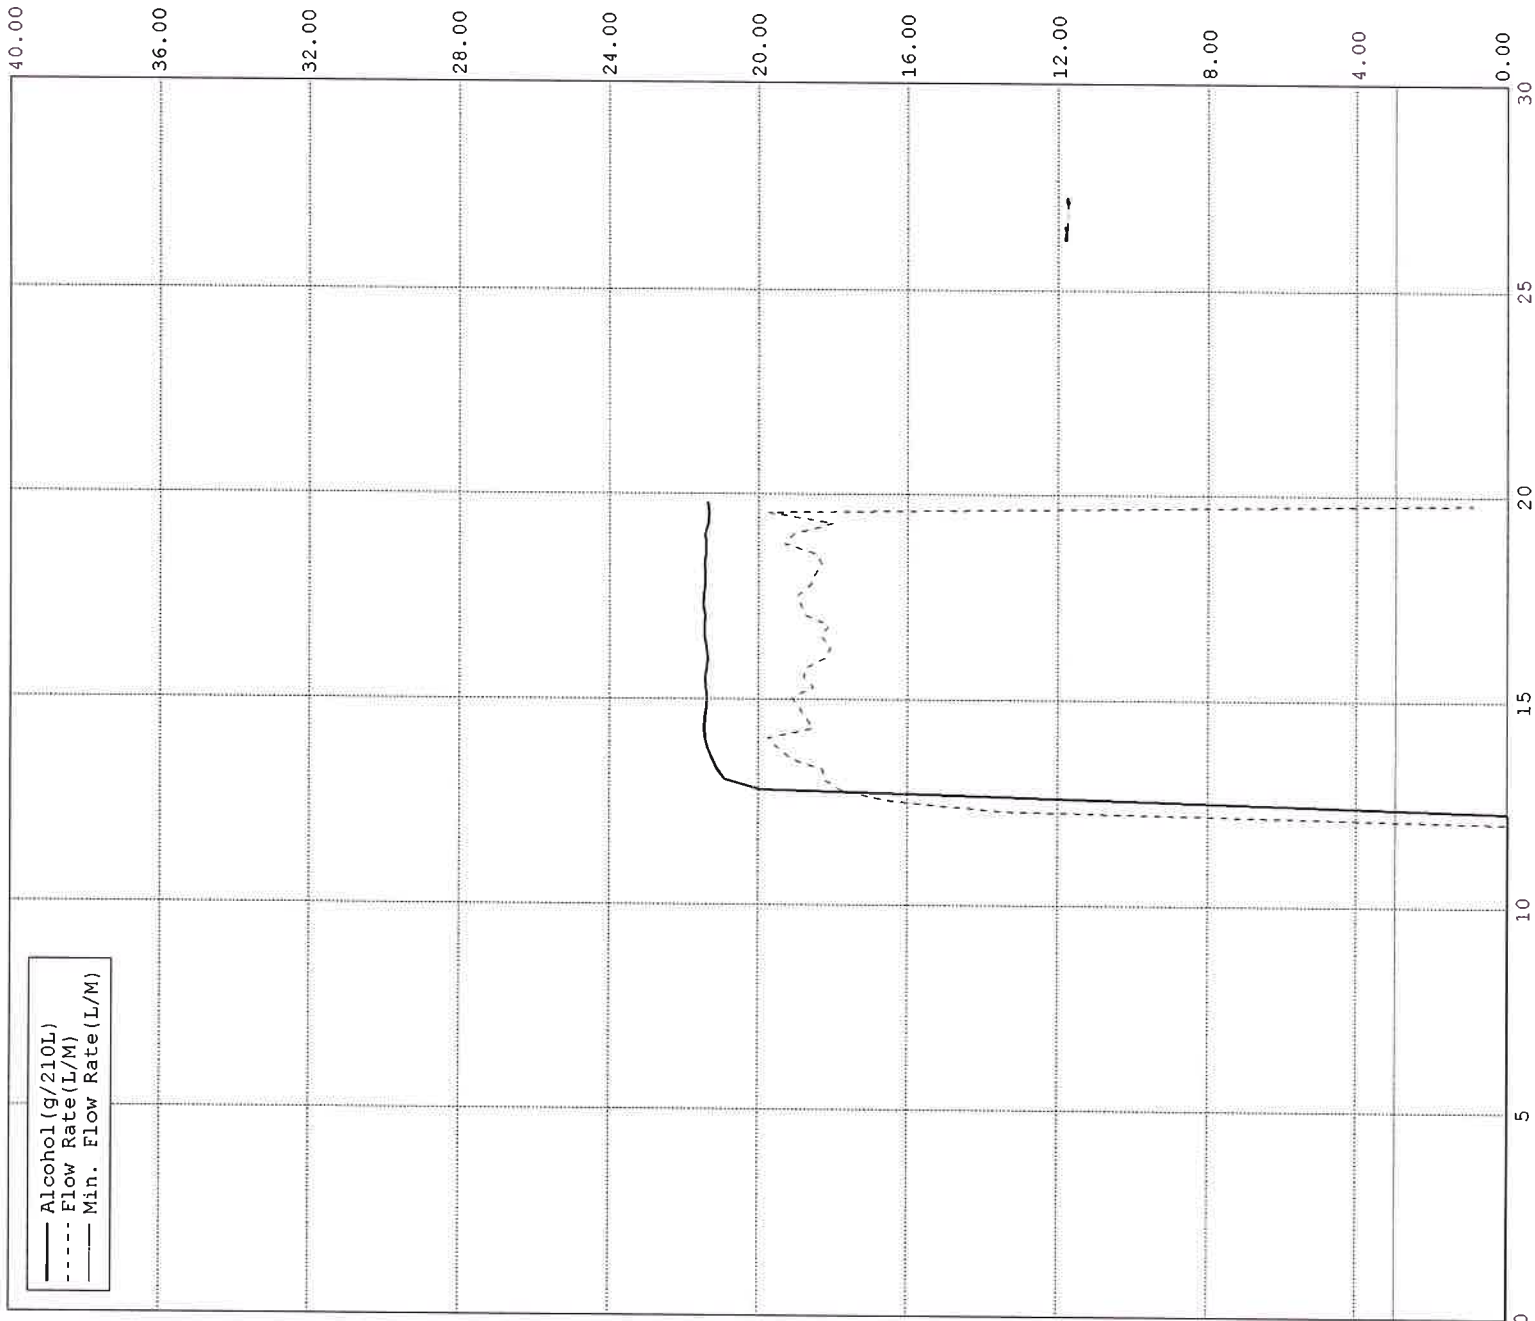



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100363

Date: 11/14/2022

Time: 15:27:49

SUBJECT NAME:

TEST TEST

LICENSE #: INT-IPA

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAAA

CASE/REPORT: 22-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 30.00: 0.080

LOT #: AG113402

EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK PASSED 15:28

BLANK TEST 0.000 15:29

INTERNAL STANDARD VERIFIED 15:29

Xq = 0.081 (1.41%)

EXTERNAL STANDARD 0.080 15:29

X[1] = 0.0802 (-0.0001) (0.0039)


BLANK TEST 0.000 15:30

SUBJECT SAMPLE XXX 15:30

X[1] = 0.1170 (-0.0160) (0.0025)

Interference Detected

CAB

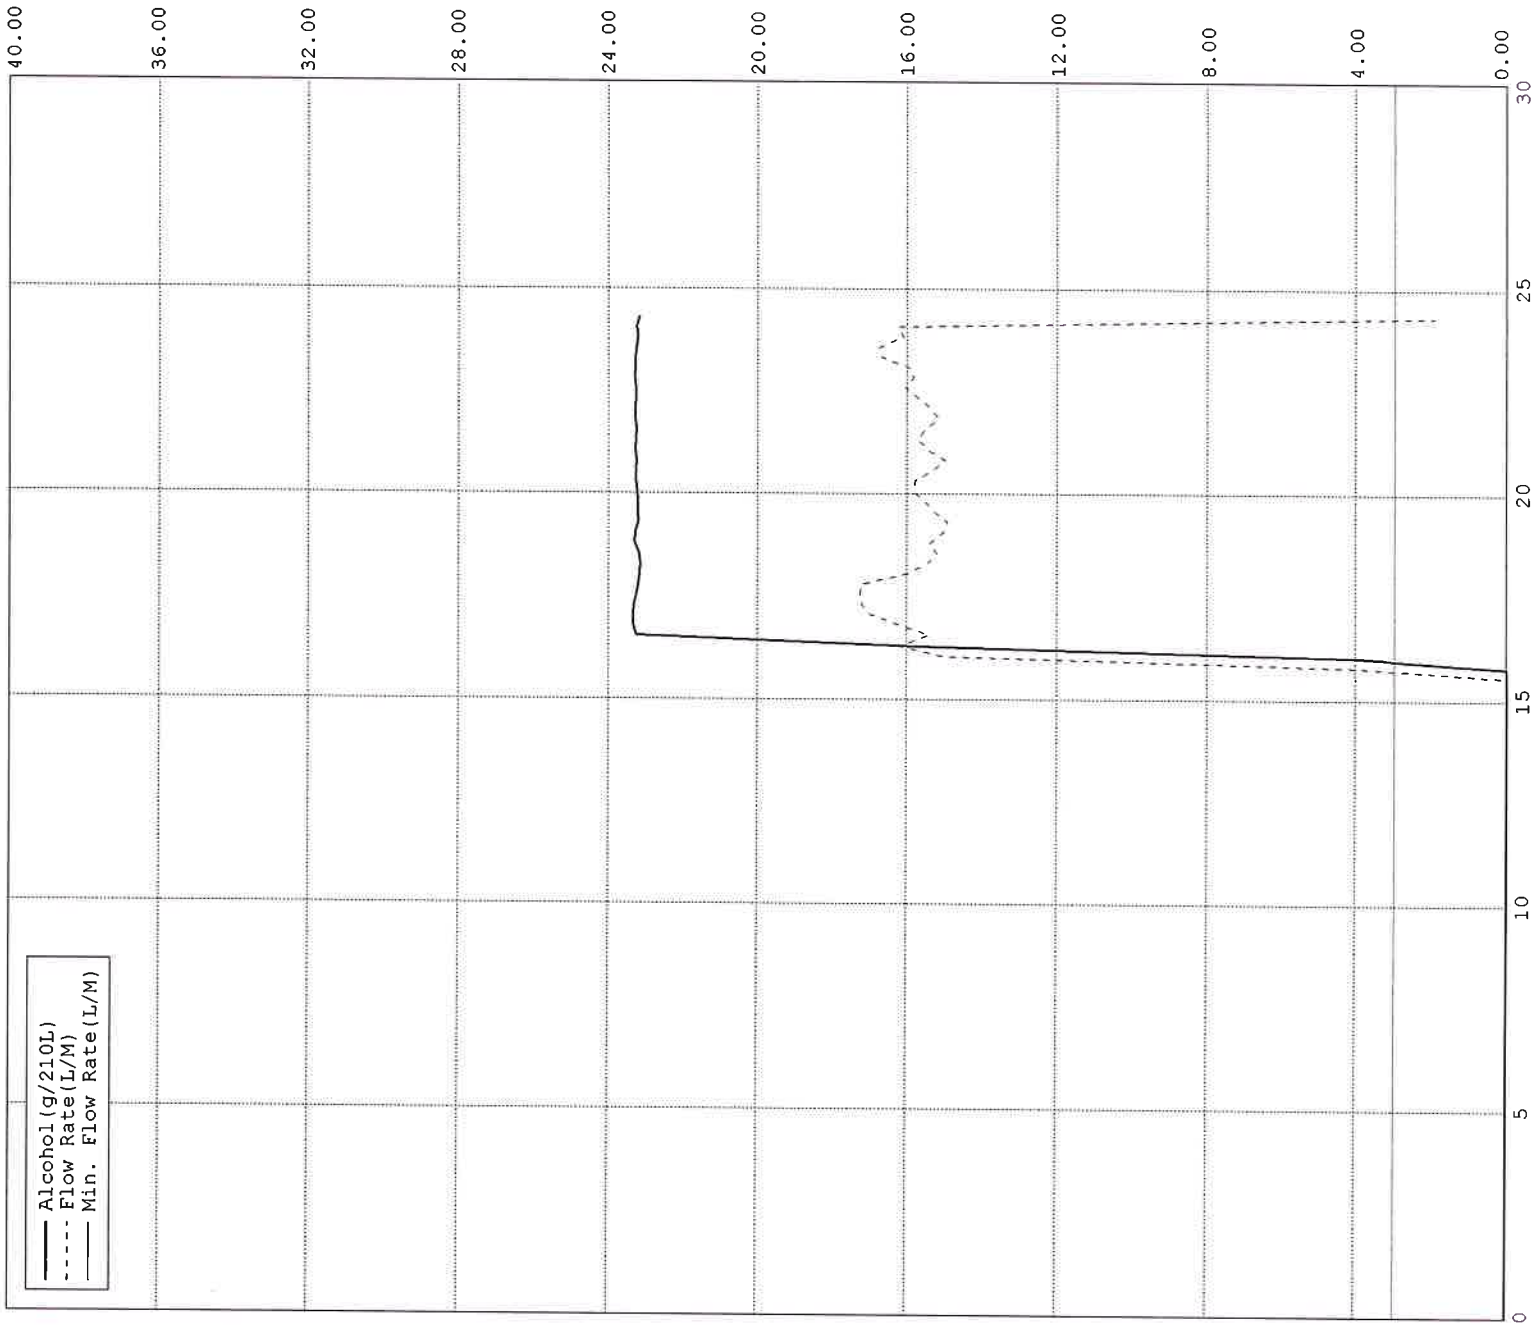

SUBJECT TEST

Alaska Department of Public Safety  
DATA MASTER dmt: 100363

Date: 11/14/2022  
Time: 15:36:03

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-NEGATIVE

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237


DEPT/AGENCY:  
AAA1

CASE/REPORT: 22-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 30.00: 0.080  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	15:37
BLANK TEST	0.000	15:37
INTERNAL STANDARD	VERIFIED	15:37
$X_q = 0.081$ (0.87%)		
EXTERNAL STANDARD	0.080	15:37
$X[1] = 0.0801$ (0.0005) (0.0037)		
BLANK TEST	0.000	15:38
SUBJECT SAMPLE (Vol=2.32L)	0.091	15:39
$X[1] = 0.0915$ (-0.0001) (0.0019)		
BLANK TEST	0.000	15:40
EXTERNAL STANDARD	0.079	15:40
$X[1] = 0.0793$ (-0.0011) (0.0027)		
BLANK TEST	0.000	15:41

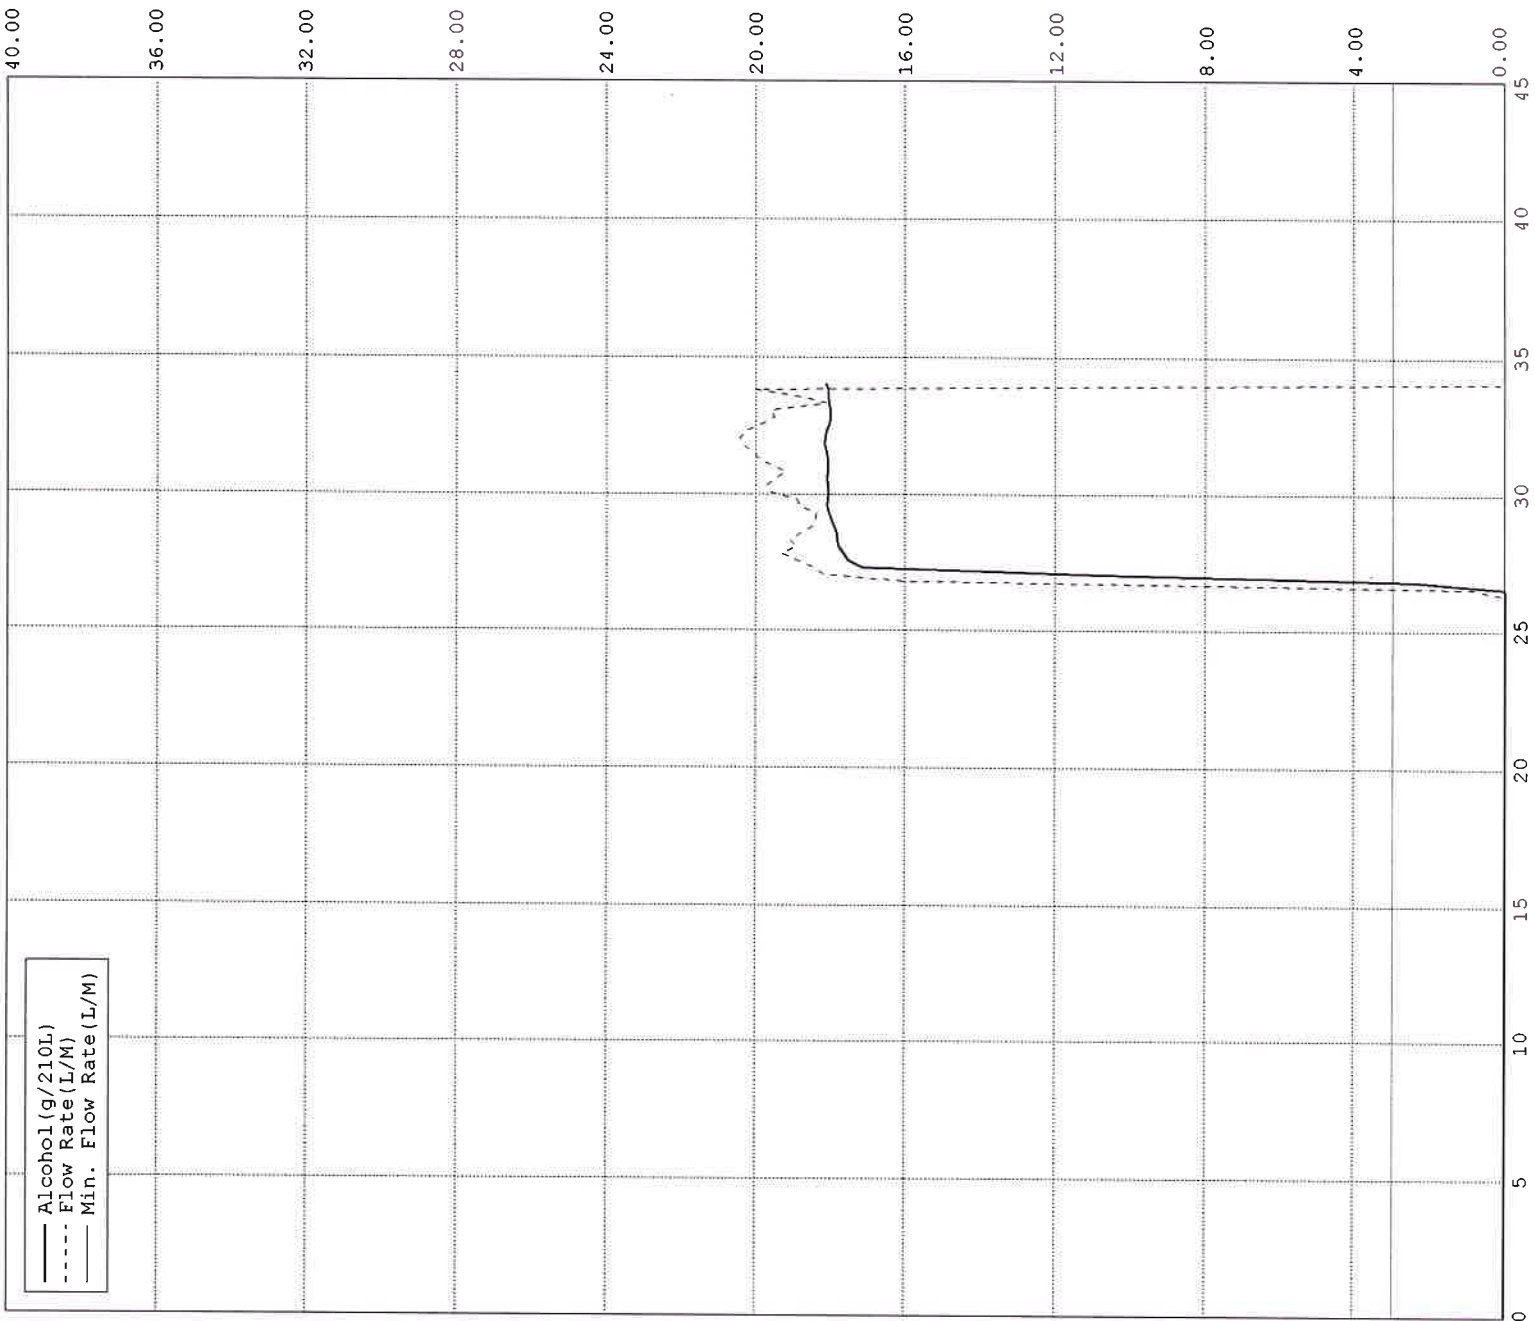

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100363

Date: 11/14/2022

Time: 16:00:00

SUBJECT NAME:

TEST TEST

LICENSE #: INVALID

OPERATOR NAME:

COLLEEN S OBRVANT

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 22-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 30.02: 0.080

LOT #: AG113402

EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK

BLANK TEST

PASSED

16:01

INTERNAL STANDARD

0.000

16:01

EXTERNAL STANDARD

VERIFIED

16:01

BLANK TEST

0.080

16:01


SUBJECT SAMPLE

0.000

16:02

INVALID

16:03

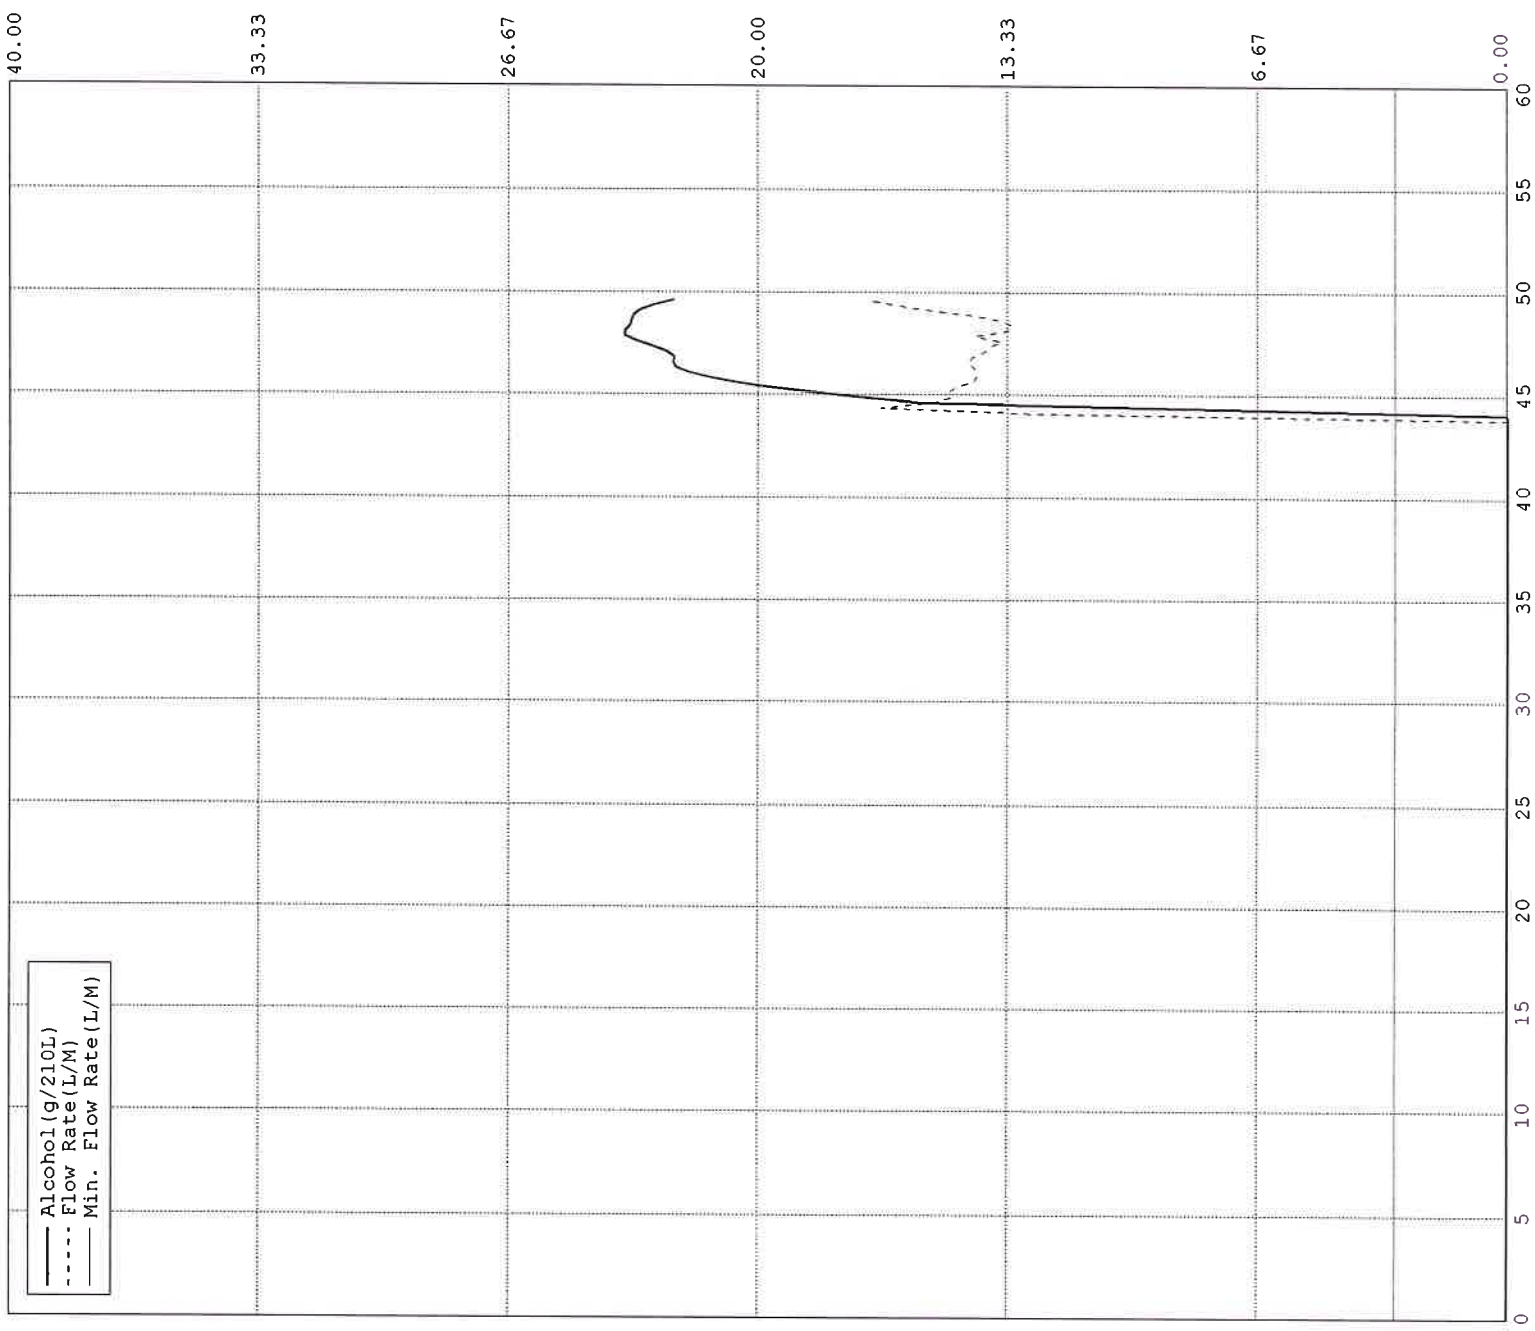

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100363

Date: 11/14/2022  
Time: 16:06:41

SUBJECT NAME:  
TEST TEST  
LICENSE #: RFI


OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 22-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 30.02: 0.080  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK  
BLANK TEST PASSED 16:08  
INTERNAL STANDARD 0.000 16:08  
EXTERNAL STANDARD VERIFIED 16:08  
BLANK TEST 0.080 16:08  
BLANK TEST 0.000 16:09

RFI DETECTED

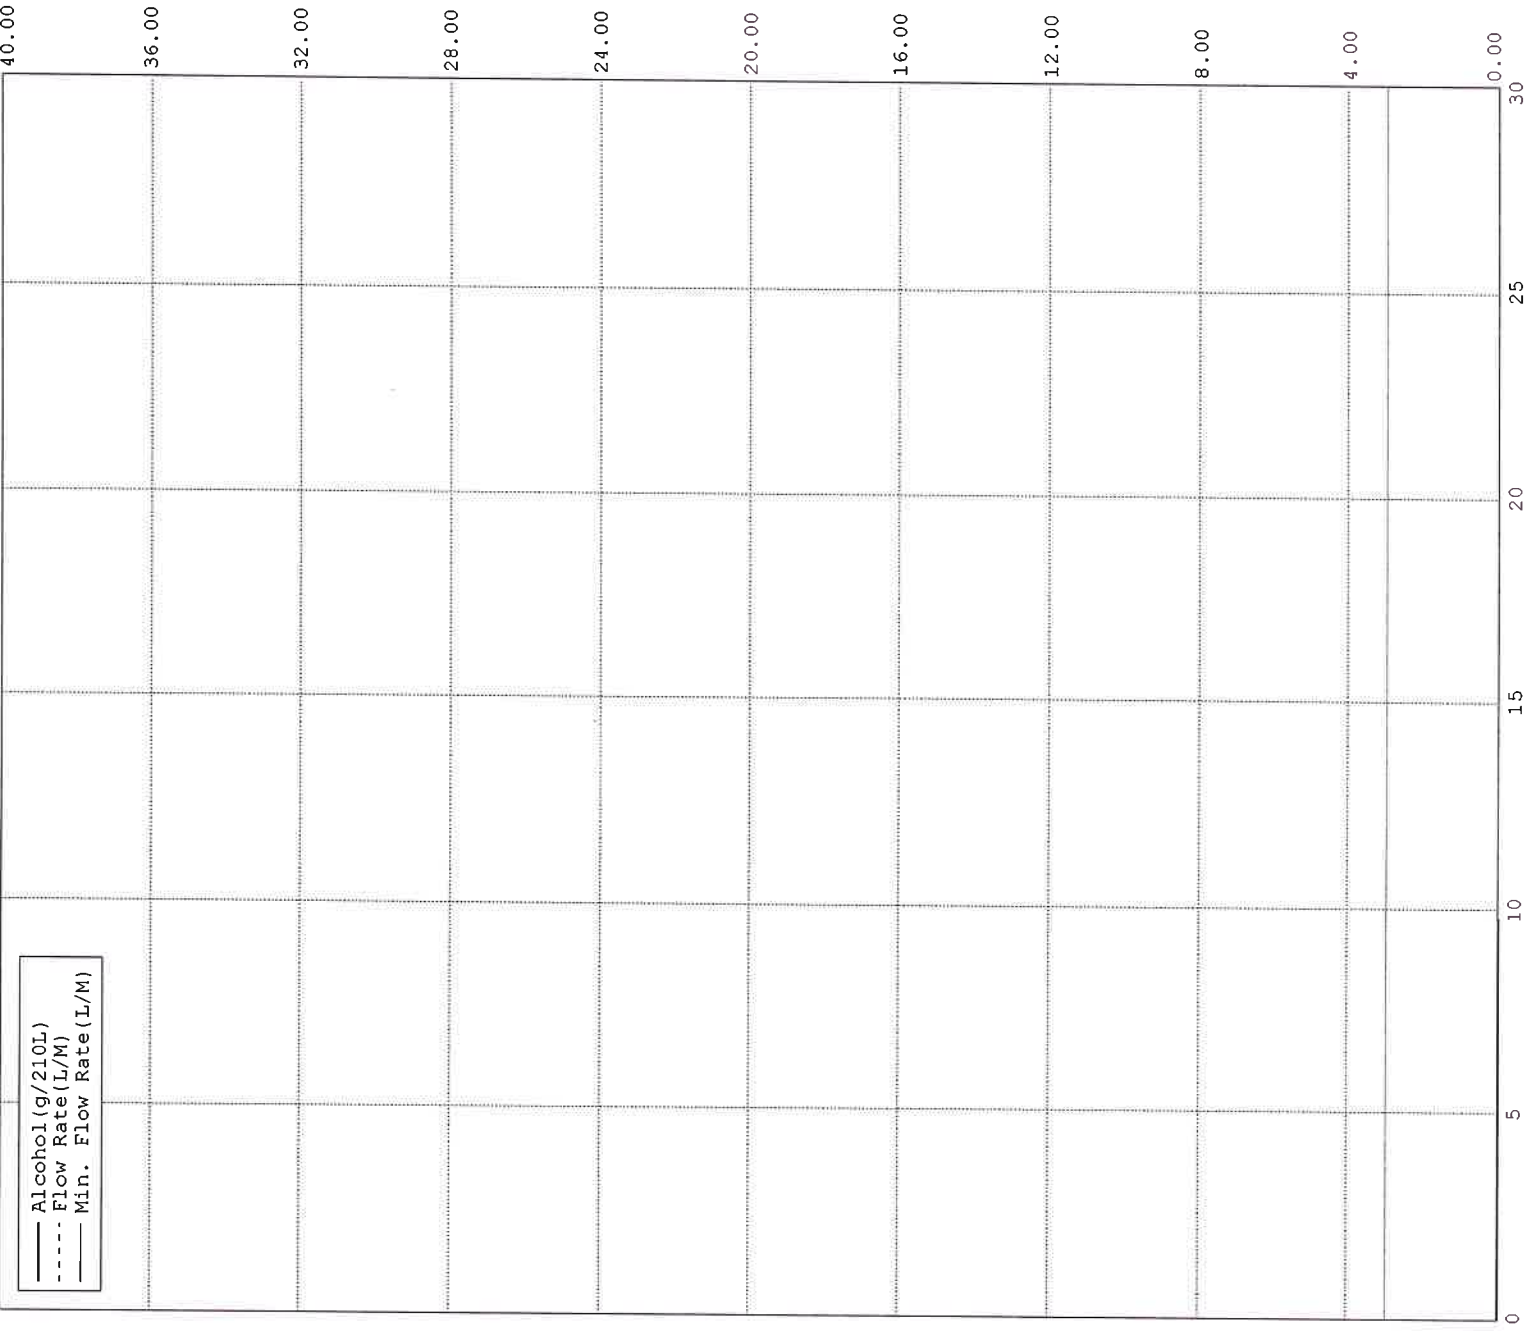

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100363

Date: 11/14/2022  
Time: 16:21:43

SUBJECT NAME:  
TEST TEST  
LICENSE #: NON-DRINKING

OPERATOR NAME:  
COLLEEN S OBRyant  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1

CASE/REPORT: 22-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 30.02: 0.080  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	16:22
BLANK TEST	0.000	16:22
INTERNAL STANDARD	VERIFIED	16:23
EXTERNAL STANDARD	0.080	16:23
BLANK TEST	0.000	16:24
SUBJECT SAMPLE (Vol=1.97L)	0.000	16:24
BLANK TEST	0.000	16:25
EXTERNAL STANDARD	0.081	16:25
BLANK TEST	0.000	16:26

