




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100421

Report Issue Date: 11/13/2025
Date Received: 2025-10-06
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.019	0.020	0.020	0.020	0.020	0.020
0.080	0.078	AG335202	0.077	0.077	0.077	0.077	0.077	0.077
0.300	0.294	AG427706	0.287	0.286	0.286	0.286	0.286	0.286

As Found - Evaluation Analyst: Carlie Glaister

As Found Conditions - Barometric Pressure (inHg): 29.30 Barometer Used: VWR S/N 240680771 Temperature (C): 21.6 Relative Humidity (%): 37

As-Found Lab Activity Date Range: 10/06/2025 - 10/06/2025

Internal standard observed on screen during non-drinking subject test was 3.90%. Due to recent repeated internal standard errors in the field Adjustment is recommended.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG408002	0.020	0.021	0.021	0.021	0.020	0.021	+/- 0.002
0.040	0.039	AG407908	0.041	0.040	0.040	0.040	0.039	0.040	+/- 0.003
0.080	0.078	AG335202	0.079	0.079	0.079	0.079	0.078	0.079	+/- 0.004
0.100	0.097	AG333401	0.099	0.099	0.100	0.099	0.099	0.099	+/- 0.004
0.150	0.146	AG515604	0.147	0.146	0.146	0.147	0.146	0.146	+/- 0.006
0.300	0.292	AG427706	0.293	0.292	0.292	0.292	0.292	0.292	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.17 Barometer Used: VWR S/N 240680771 Temperature (C): 21.6 Relative Humidity (%): 16

As-Left Lab Activity Date Range: 10/29/2025 - 10/29/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Kaija Swisher on 10/29/2025

kaija.swisher@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 11/13/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100421 Analyst or Technician Name: Kaya Swisher

DataMaster DMT Calibration Start Date: 10/29/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 9/10/26
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.17 Temperature(C) 21.6 Relative Humidity(%) 16
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) - *Print with View Details*
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20250922KS Expiration Date: 12/22/25
Simulator S/N: DR4178 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20250922KS Expiration Date: 12/22/25
Simulator S/N: DR4177 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 12/22/25
Simulator S/N: DR4163 Thermometer Verification Performed? ☒ 3/19/27 (Solution)
27 KS 10/29/25

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 3/14/27

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 10/29/25

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): 10/29/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

 Alaska Department of Public Safety
 DATAMASTER dmt: 100421

Date: 10/29/2025
 Time: 08:08:19

VERSIONS
 DMT: 3.02
 PIC: 3.02
 Modem: 2.6
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 42.0°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.74 V	PASSED
(1.04 V - 2.44 V)	
Cooler Voltage = 1.80 V	PASSED
(1.08 V - 2.52 V)	
Bias Voltage = 80 V	PASSED
(48 V - 112 V)	
Chopper Freq = 530 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.2 in	

PUMP INFO

Flow Rate = 4.620 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.002 V <= 0.010 V)	
PUMP OFF	PASSED
(0.002 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

	PASSED
Xq = 0.098 0.36% (0.00% - 4.00%)	

Technician Screen

Joint Base Elmendorf - Richardson
DATAMASTER dmt: 100421

Date: 10/29/2025
Time: 8:16 AM

Temperatures (°C)

Sample Cell: 48.8°C
Breath Tube: 41.7°C

Current Barometer 29.2 in
Volume (Ltr) 1.54

Settings

Lamp: 1.74 V
Bias: 80 V
Cooler: 1.80 V
Chopper: 529 Hz

Voltages (V)

Flow: 1.09 V
Detector: 0.075 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100421

Date: 10/20/2025
Time: 12:44:11

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca	=	0.1000		
CAL	=	0.990551	0.800	<= CAL < 1.200
b1	=	0.0018	0.0000	<= b1 < 0.0040
b2	=	0.0051	0.0010	<= b2 < 0.0100
b3	=	0.0012	0.0000	<= b3 < 0.0040
Xq	=	0.0987	0.0500	<= Xq < 0.2000
a21	=	1.124461	1.050	<= a21 < 1.300
a31	=	0.458046	0.300	<= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100421

Date: 10/29/2025
 Time: 08:17:24


SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

DEPT/AGENCY:
 MINIMUM VOLUME TEST
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.17: 0.078
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	08:18
BLANK TEST	0.000	08:18
INTERNAL STANDARD	VERIFIED	08:18
EXTERNAL STANDARD	0.079	08:19
BLANK TEST	0.000	08:20
SUBJECT SAMPLE (Vol=1.59L)	0.000	08:22
BLANK TEST	0.000	08:23
EXTERNAL STANDARD	0.079	08:23
BLANK TEST	0.000	08:24

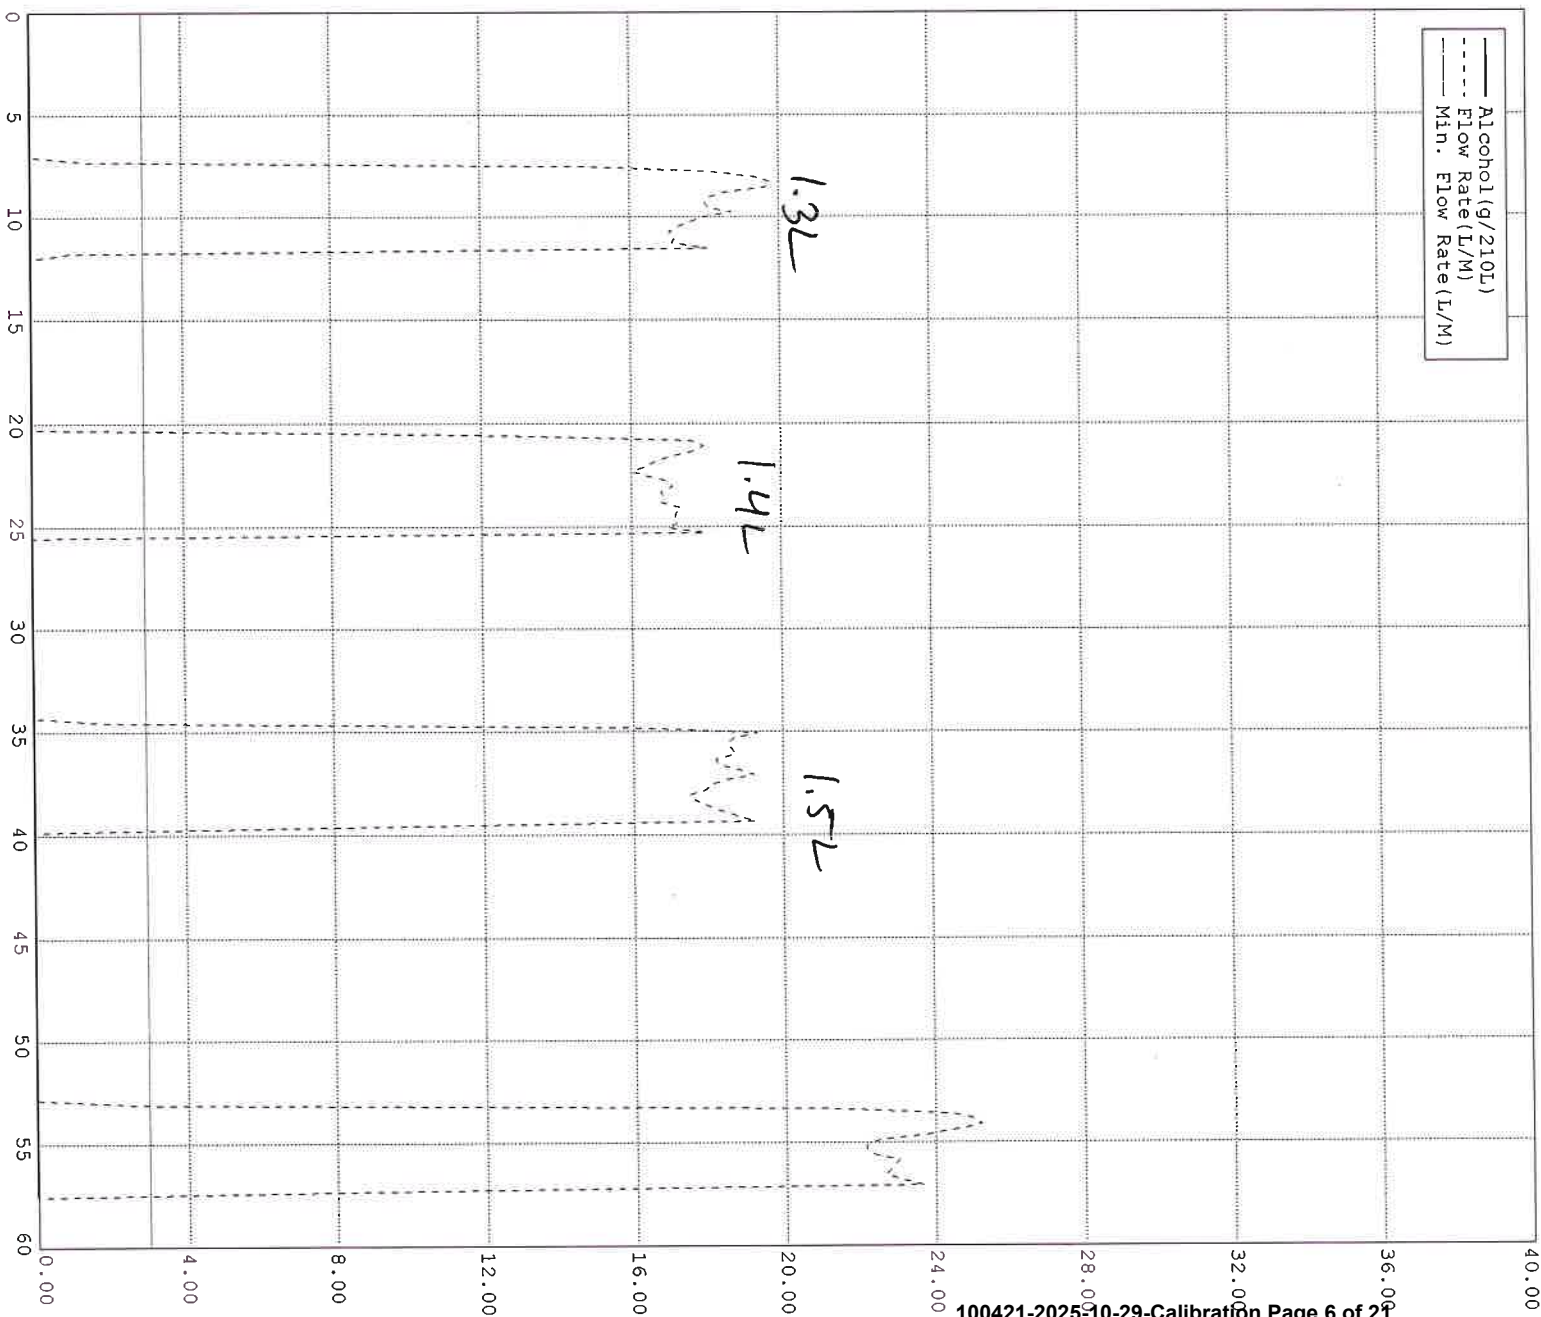


LINEARITY CHECK

Alaska Department of Public Safety
 DATA MASTER dmt: 100421

Date: 10/29/2025
 Time: 09:12:54

SUPERVISOR NAME:
 KAITA SWISHER
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.019	0.0206	0.0005
0.039	0.0400	0.0007
0.078	0.0788	0.0004
0.097	0.0992	0.0004
0.146	0.1464	0.0005
0.292	0.2922	0.0004
SLOPE	= 0.995270	
R ²	= 0.999964	

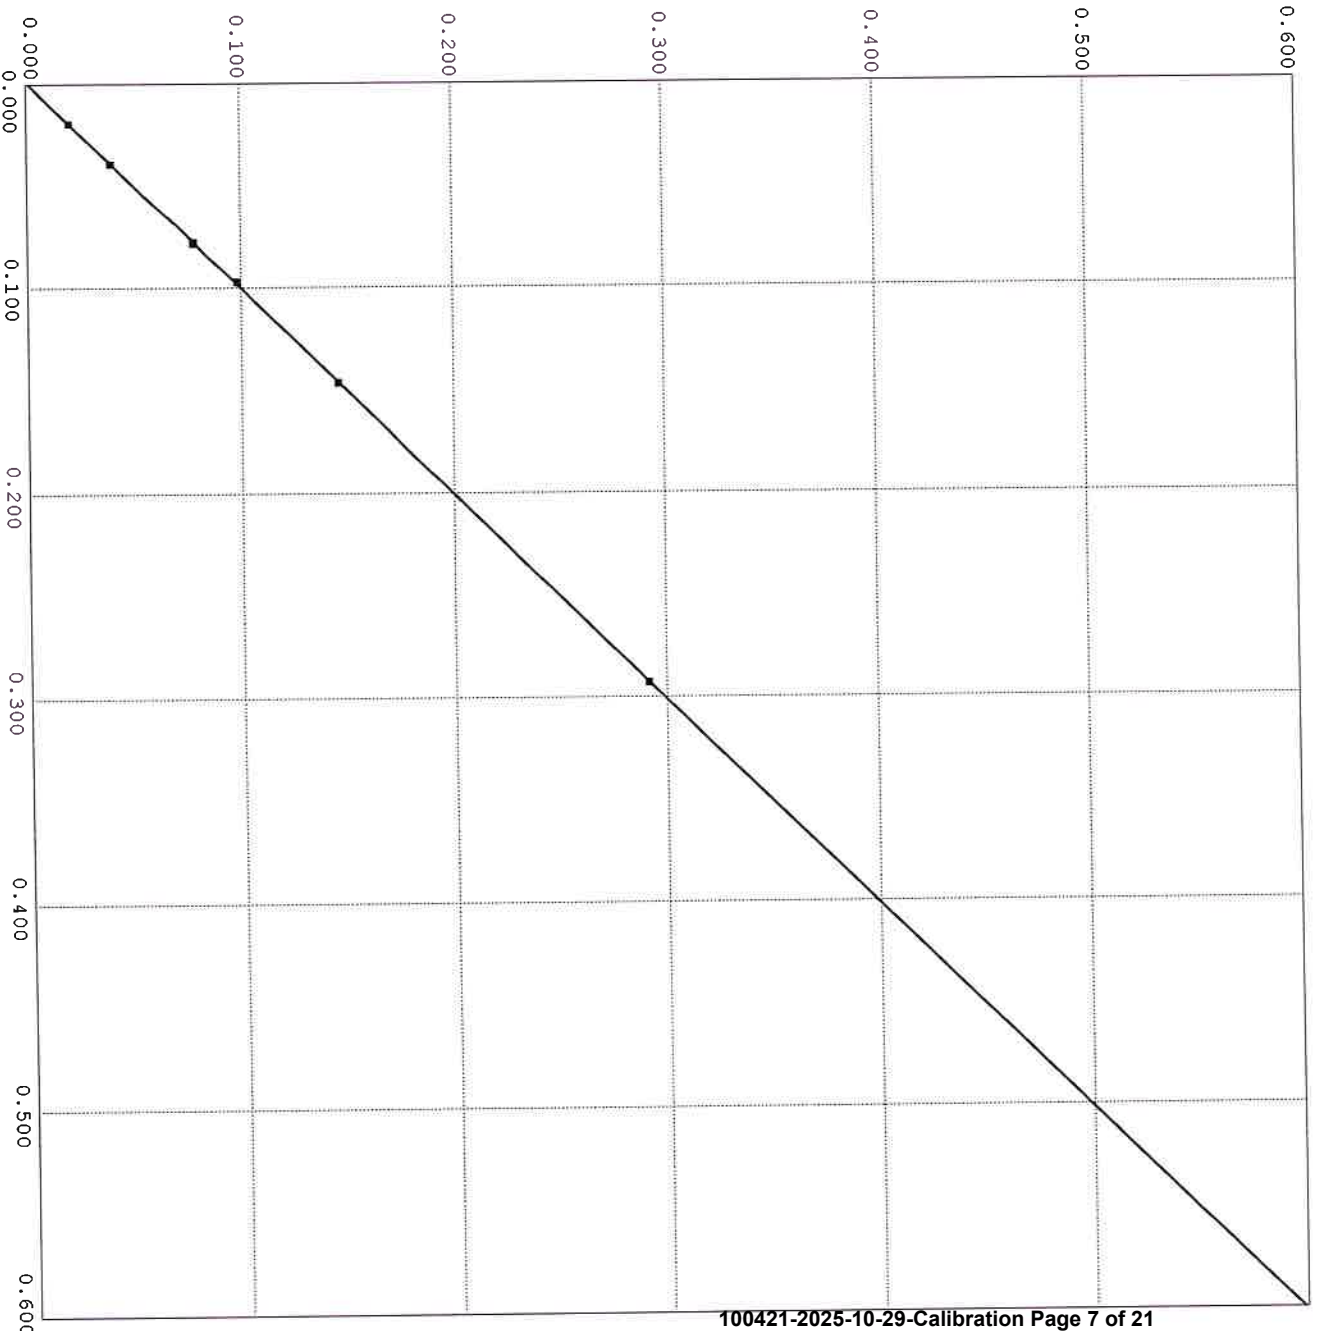

145

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100421






Date: 10/29/2025
Time: 09:12:57

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.12: 0.019
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 780 psi

BLANK TEST	0.000	09:14
INTERNAL STANDARD	VERIFIED	09:14
EXTERNAL STANDARD	0.020	09:14
BLANK TEST	0.000	09:15
EXTERNAL STANDARD	0.021	09:15
BLANK TEST	0.000	09:16
EXTERNAL STANDARD	0.021	09:16
BLANK TEST	0.000	09:17
EXTERNAL STANDARD	0.021	09:17
BLANK TEST	0.000	09:18
EXTERNAL STANDARD	0.020	09:18
BLANK TEST	0.000	09:19

Average = 0.0206
Std Dev = 0.0005

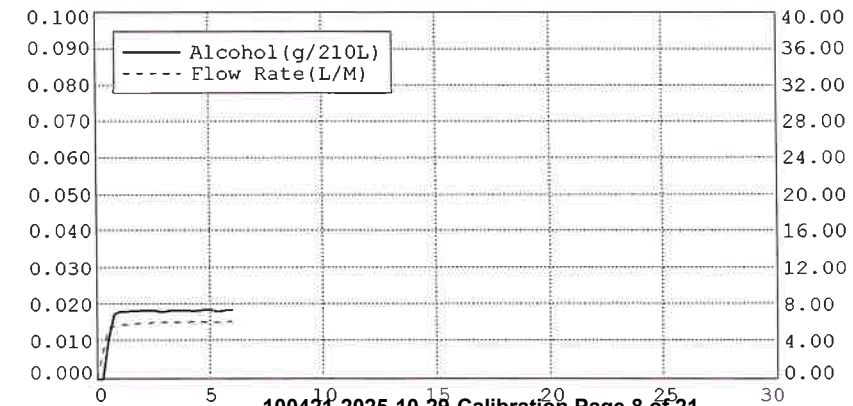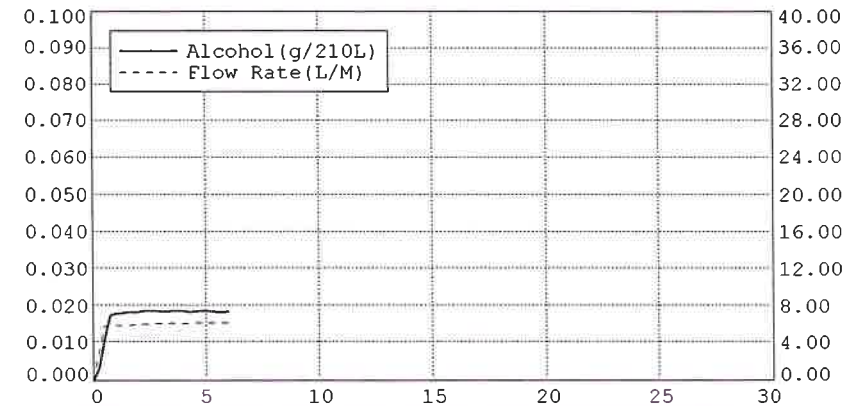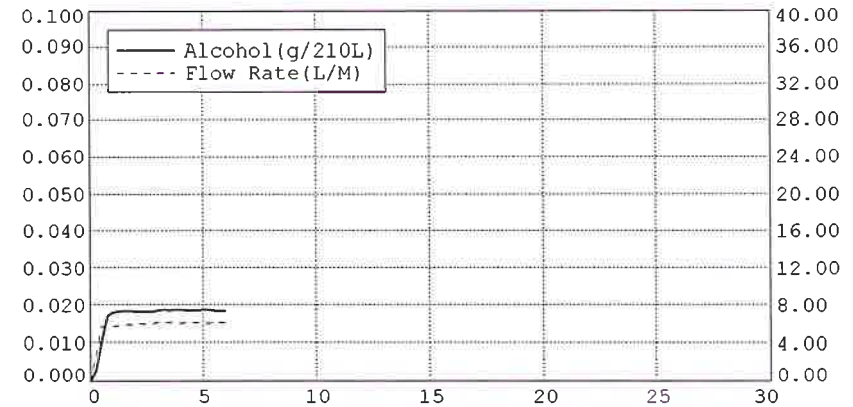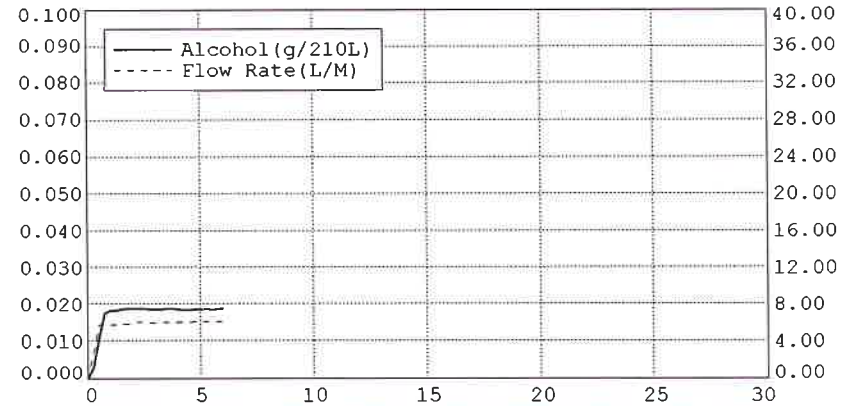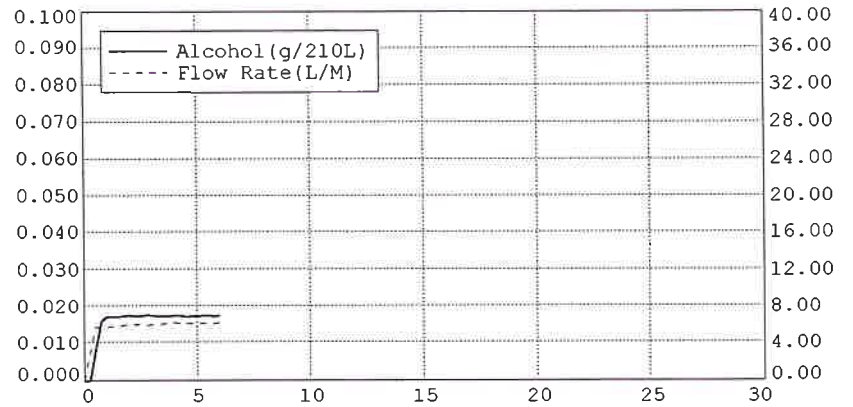

LINEARITY CHECK: Control Test 2






Alaska Department of Public Safety
DATAMASTER dmt: 100421

Date: 10/29/2025
Time: 09:20:47

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.040
TARGET AT 29.12: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 805 psi

BLANK TEST	0.000	09:22
INTERNAL STANDARD	VERIFIED	09:22
EXTERNAL STANDARD	0.041	09:22
BLANK TEST	0.000	09:23
EXTERNAL STANDARD	0.040	09:23
BLANK TEST	0.000	09:24
EXTERNAL STANDARD	0.040	09:24
BLANK TEST	0.000	09:25
EXTERNAL STANDARD	0.040	09:25
BLANK TEST	0.000	09:26
EXTERNAL STANDARD	0.039	09:27
BLANK TEST	0.000	09:27

Average = 0.0400
Std Dev = 0.0007

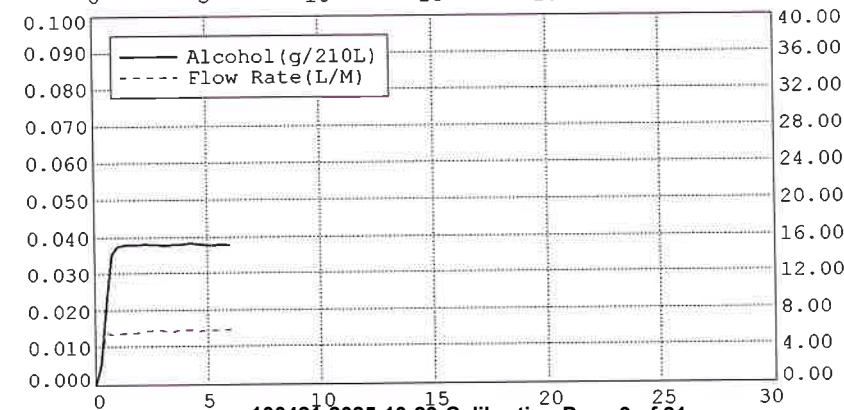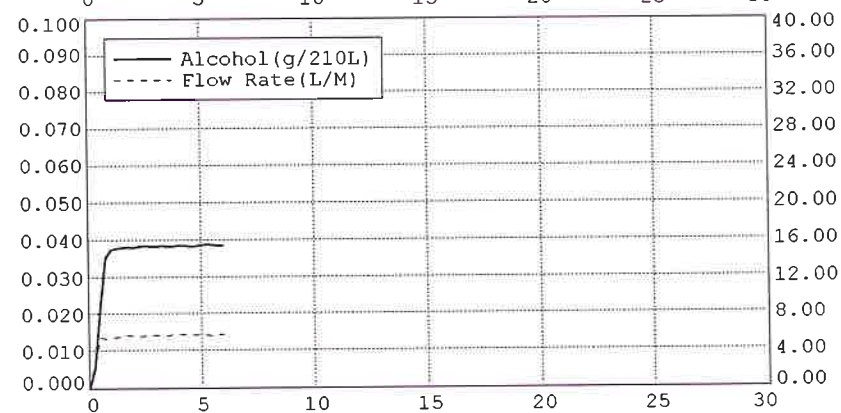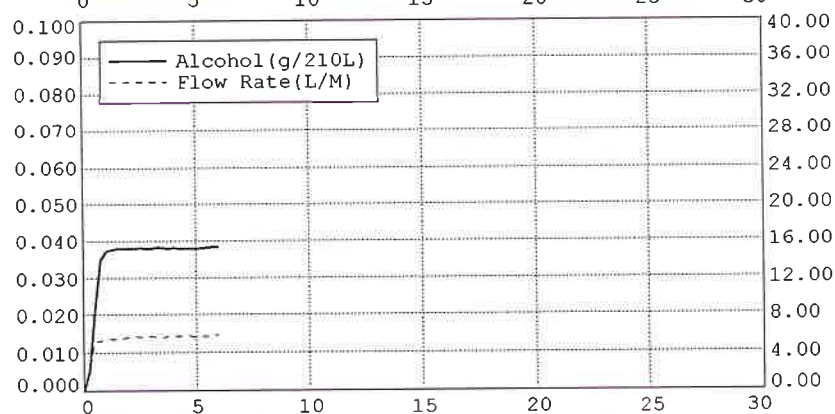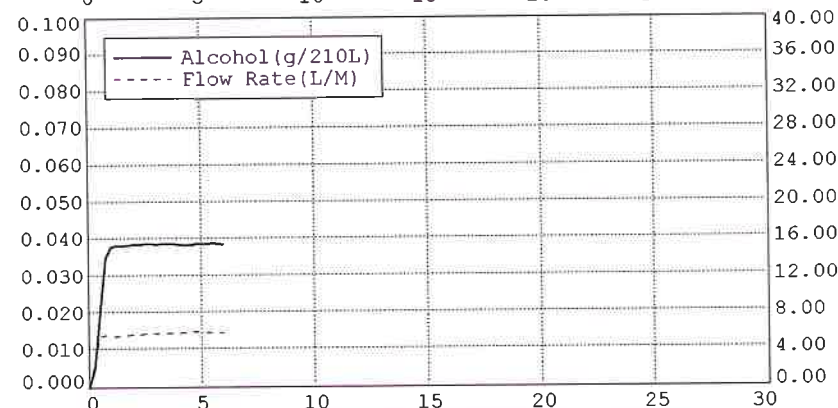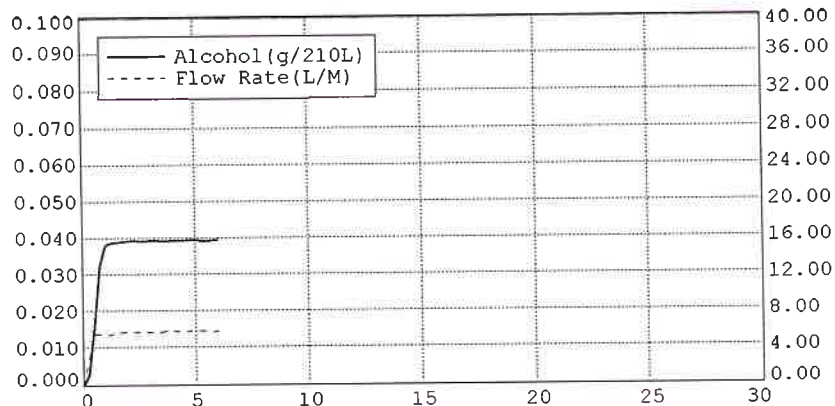

LINEARITY CHECK: Control Test 3






Alaska Department of Public Safety
DATAMASTER dmt: 100421

Date: 10/29/2025
Time: 09:28:39

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.12: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 770 psi

BLANK TEST	0.000	09:30
INTERNAL STANDARD	VERIFIED	09:30
EXTERNAL STANDARD	0.079	09:30
BLANK TEST	0.000	09:31
EXTERNAL STANDARD	0.079	09:31
BLANK TEST	0.000	09:32
EXTERNAL STANDARD	0.079	09:32
BLANK TEST	0.000	09:33
EXTERNAL STANDARD	0.079	09:33
BLANK TEST	0.000	09:34
EXTERNAL STANDARD	0.078	09:35
BLANK TEST	0.000	09:35

Average = 0.0788
Std Dev = 0.0004

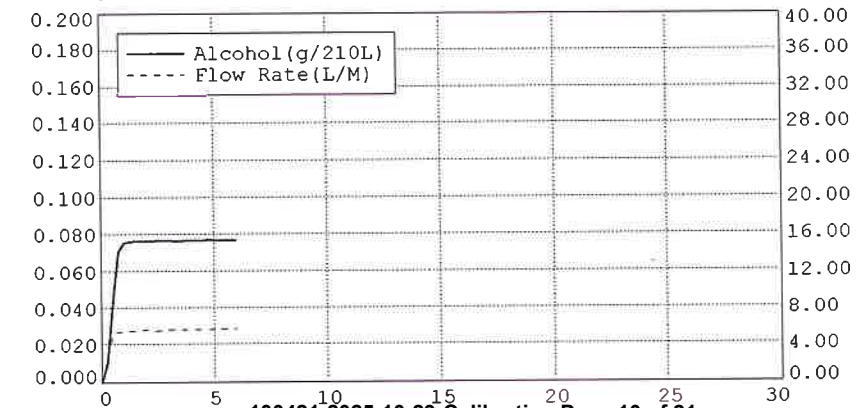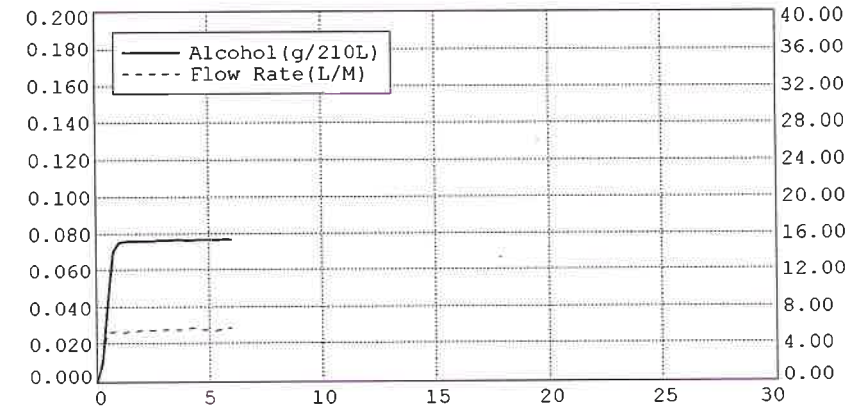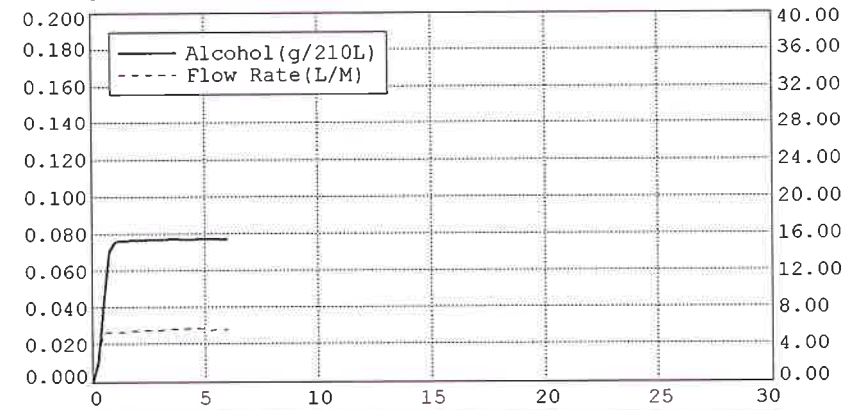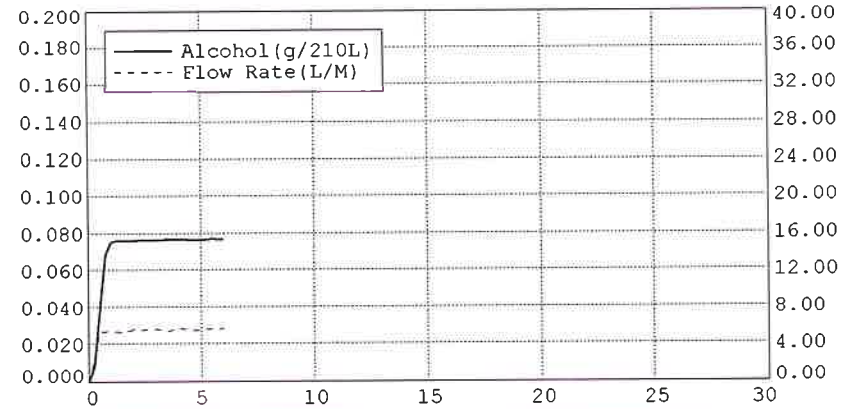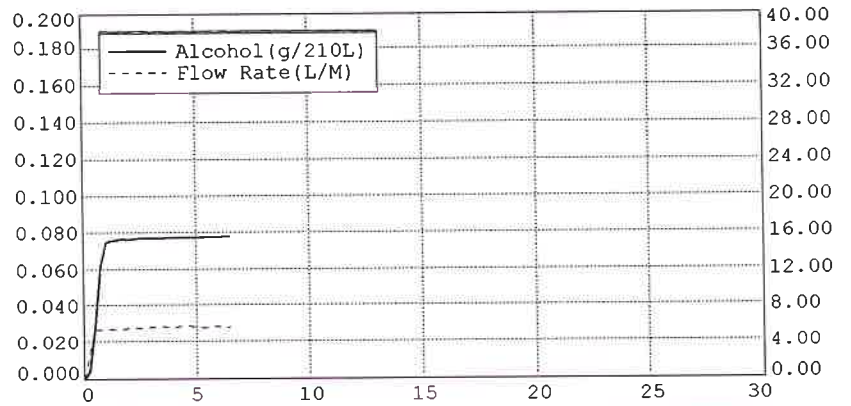

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100421






Date: 10/29/2025
Time: 09:36:33

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.11: 0.097
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 847 psi

BLANK TEST	0.000	09:38
INTERNAL STANDARD	VERIFIED	09:38
EXTERNAL STANDARD	0.099	09:38
BLANK TEST	0.000	09:39
EXTERNAL STANDARD	0.099	09:39
BLANK TEST	0.000	09:40
EXTERNAL STANDARD	0.100	09:40
BLANK TEST	0.000	09:41
EXTERNAL STANDARD	0.099	09:41
BLANK TEST	0.000	09:42
EXTERNAL STANDARD	0.099	09:42
BLANK TEST	0.000	09:43

Average = 0.0992
Std Dev = 0.0004

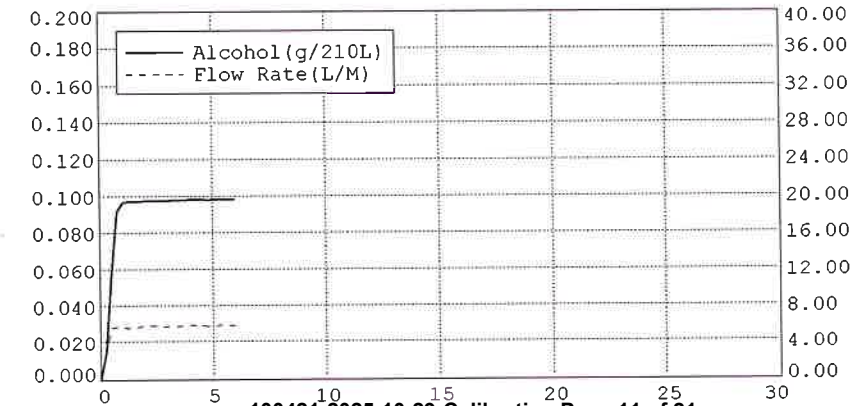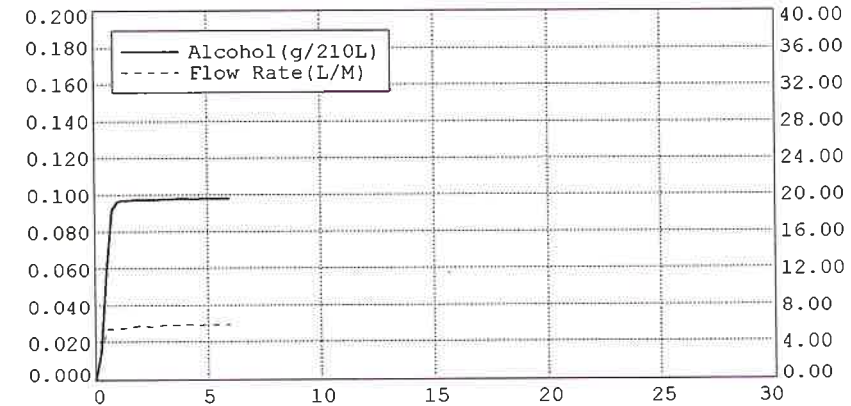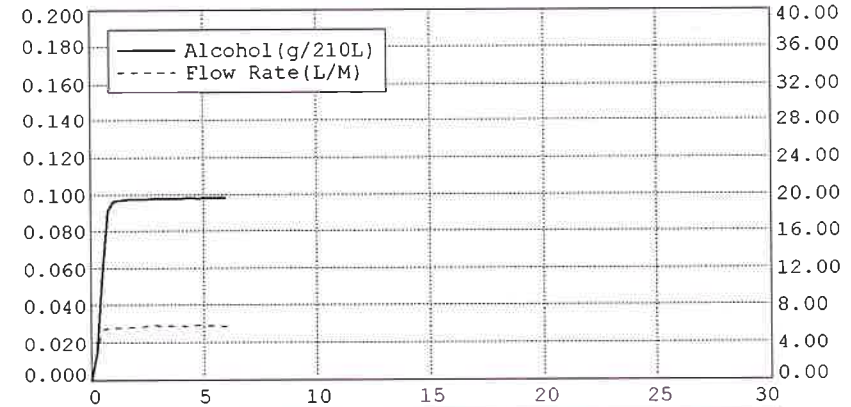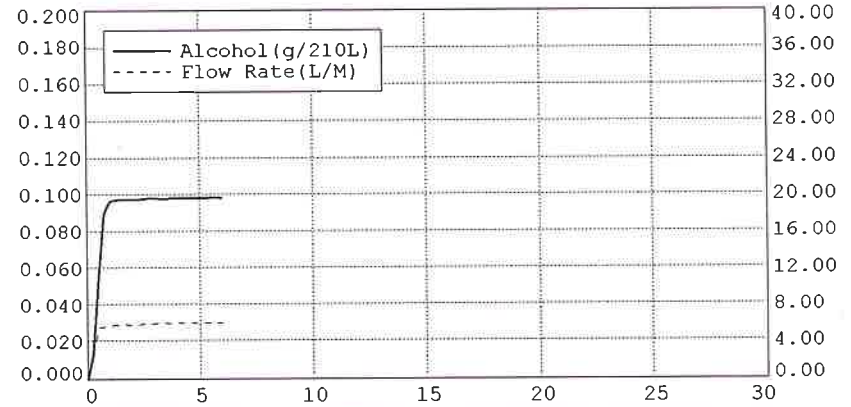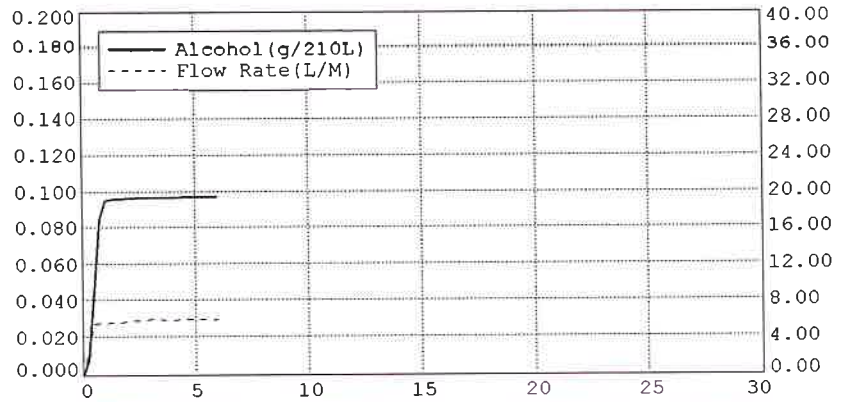

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100421






Date: 10/29/2025
Time: 09:48:30

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.11: 0.146
LOT #: AG515604
EXPIRATION: 06/05/2027
TANK PRESSURE: 712 psi

TEST TYPE	CONCENTRATION (g/210L)	TIME
BLANK TEST	0.000	09:49
INTERNAL STANDARD	VERIFIED	09:50
EXTERNAL STANDARD	0.147	09:50
BLANK TEST	0.000	09:51
EXTERNAL STANDARD	0.146	09:51
BLANK TEST	0.000	09:52
EXTERNAL STANDARD	0.146	09:52
BLANK TEST	0.000	09:53
EXTERNAL STANDARD	0.147	09:53
BLANK TEST	0.000	09:54
EXTERNAL STANDARD	0.146	09:54
BLANK TEST	0.000	09:55

Average = 0.1464
Std Dev = 0.0005

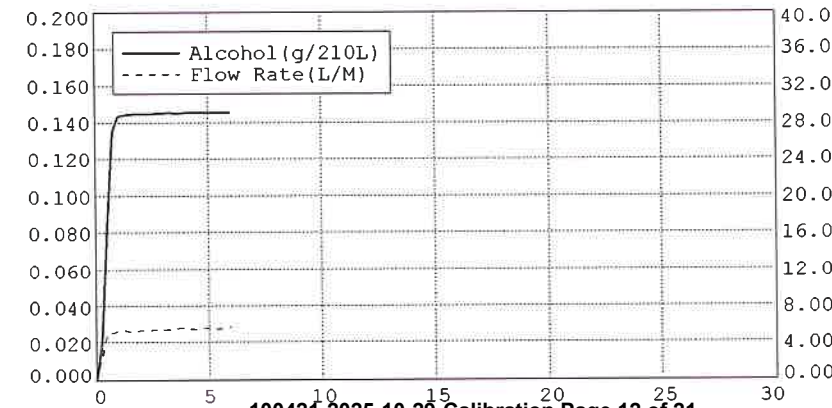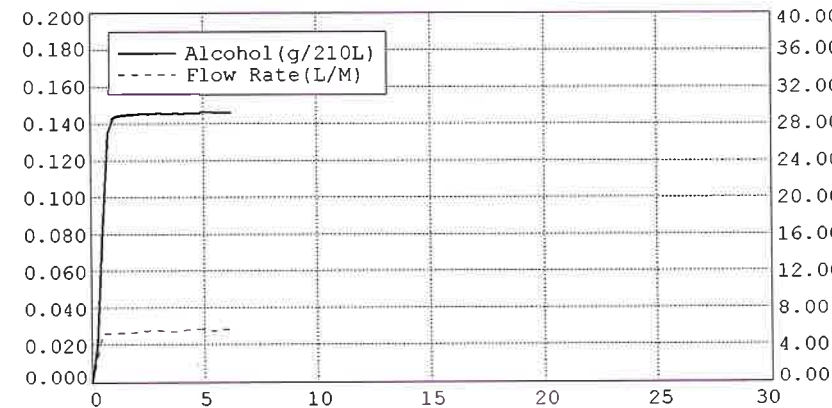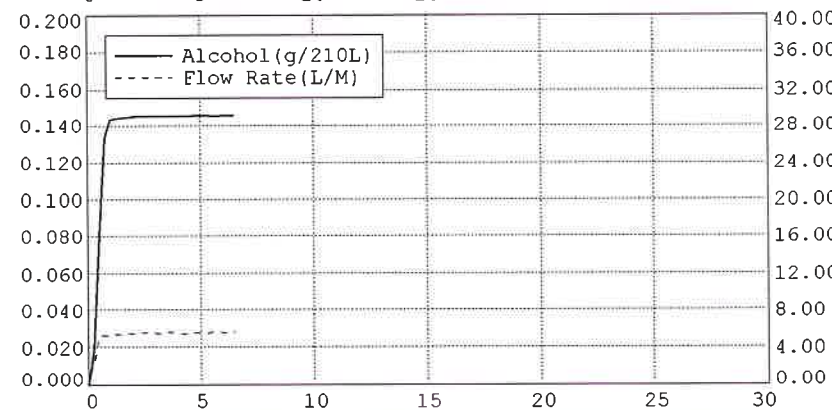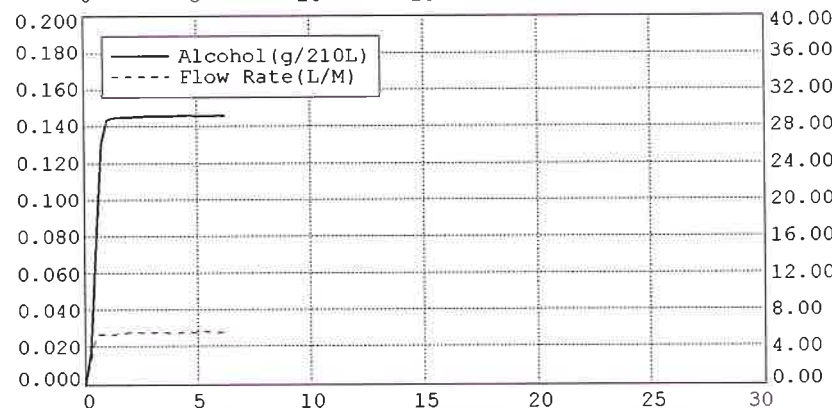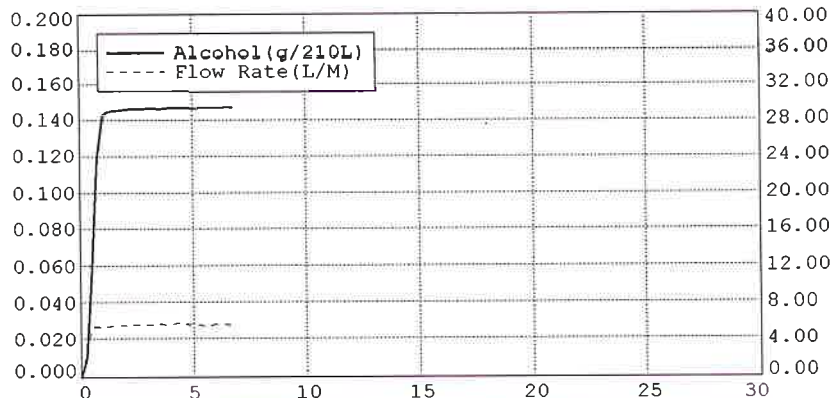

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100421






Date: 10/29/2025
Time: 09:58:27

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.10: 0.292
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 484 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	10:00
INTERNAL STANDARD	VERIFIED	10:00
EXTERNAL STANDARD	0.293	10:00
BLANK TEST	0.000	10:01
EXTERNAL STANDARD	0.292	10:01
BLANK TEST	0.000	10:02
EXTERNAL STANDARD	0.292	10:02
BLANK TEST	0.000	10:03
EXTERNAL STANDARD	0.292	10:03
BLANK TEST	0.000	10:04
EXTERNAL STANDARD	0.292	10:04
BLANK TEST	0.000	10:05

Average = 0.2922
Std Dev = 0.0004

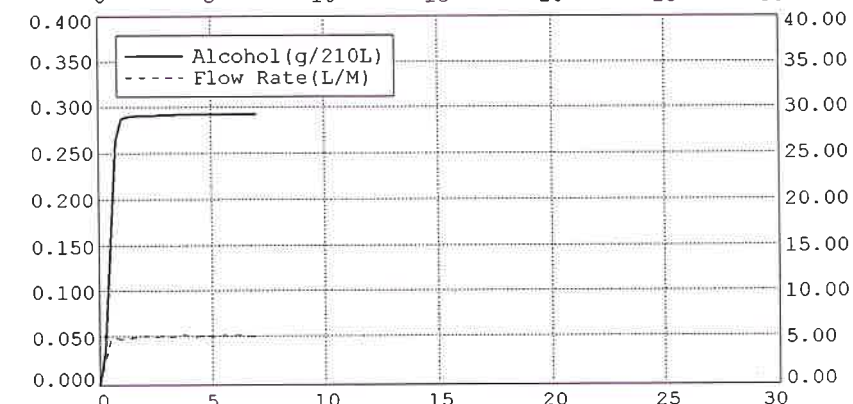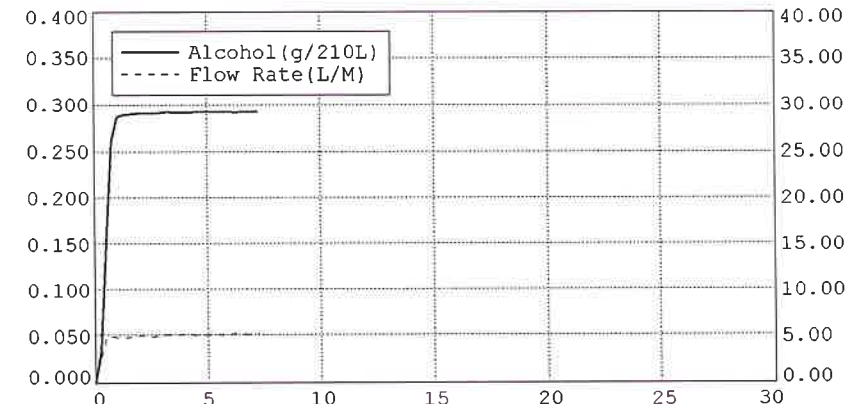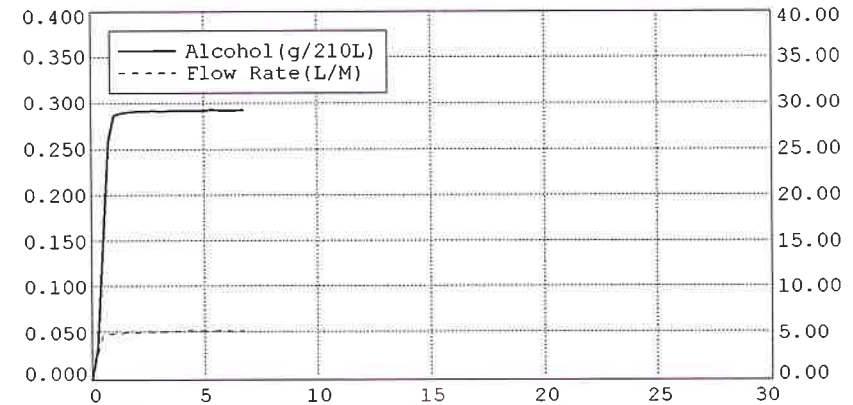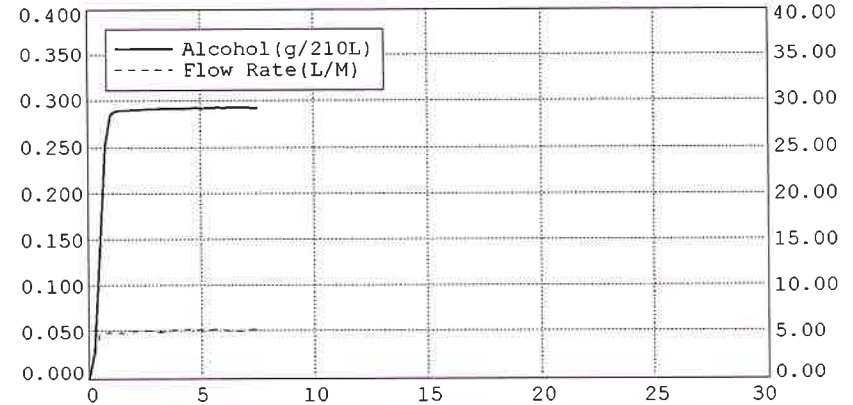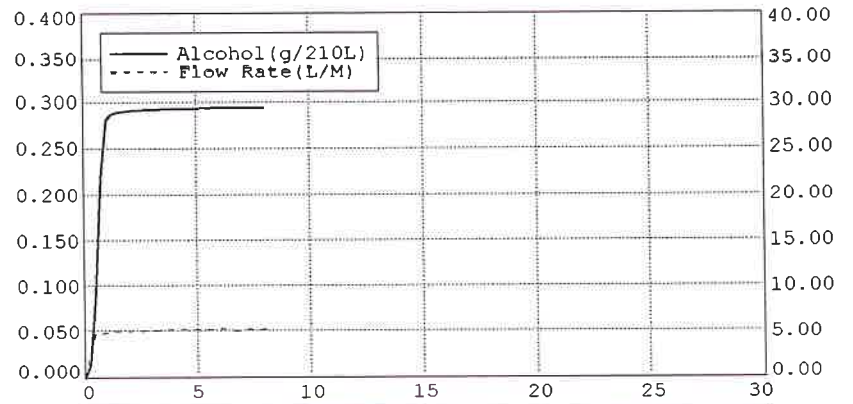

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100421

Date: 10/29/2025
Time: 10:13:01


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.09: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:14
BLANK TEST	0.000	10:14
INTERNAL STANDARD	VERIFIED	10:14
EXTERNAL STANDARD	0.079	10:14
BLANK TEST	0.000	10:15
SUBJECT SAMPLE	INCOMPLETE	10:18

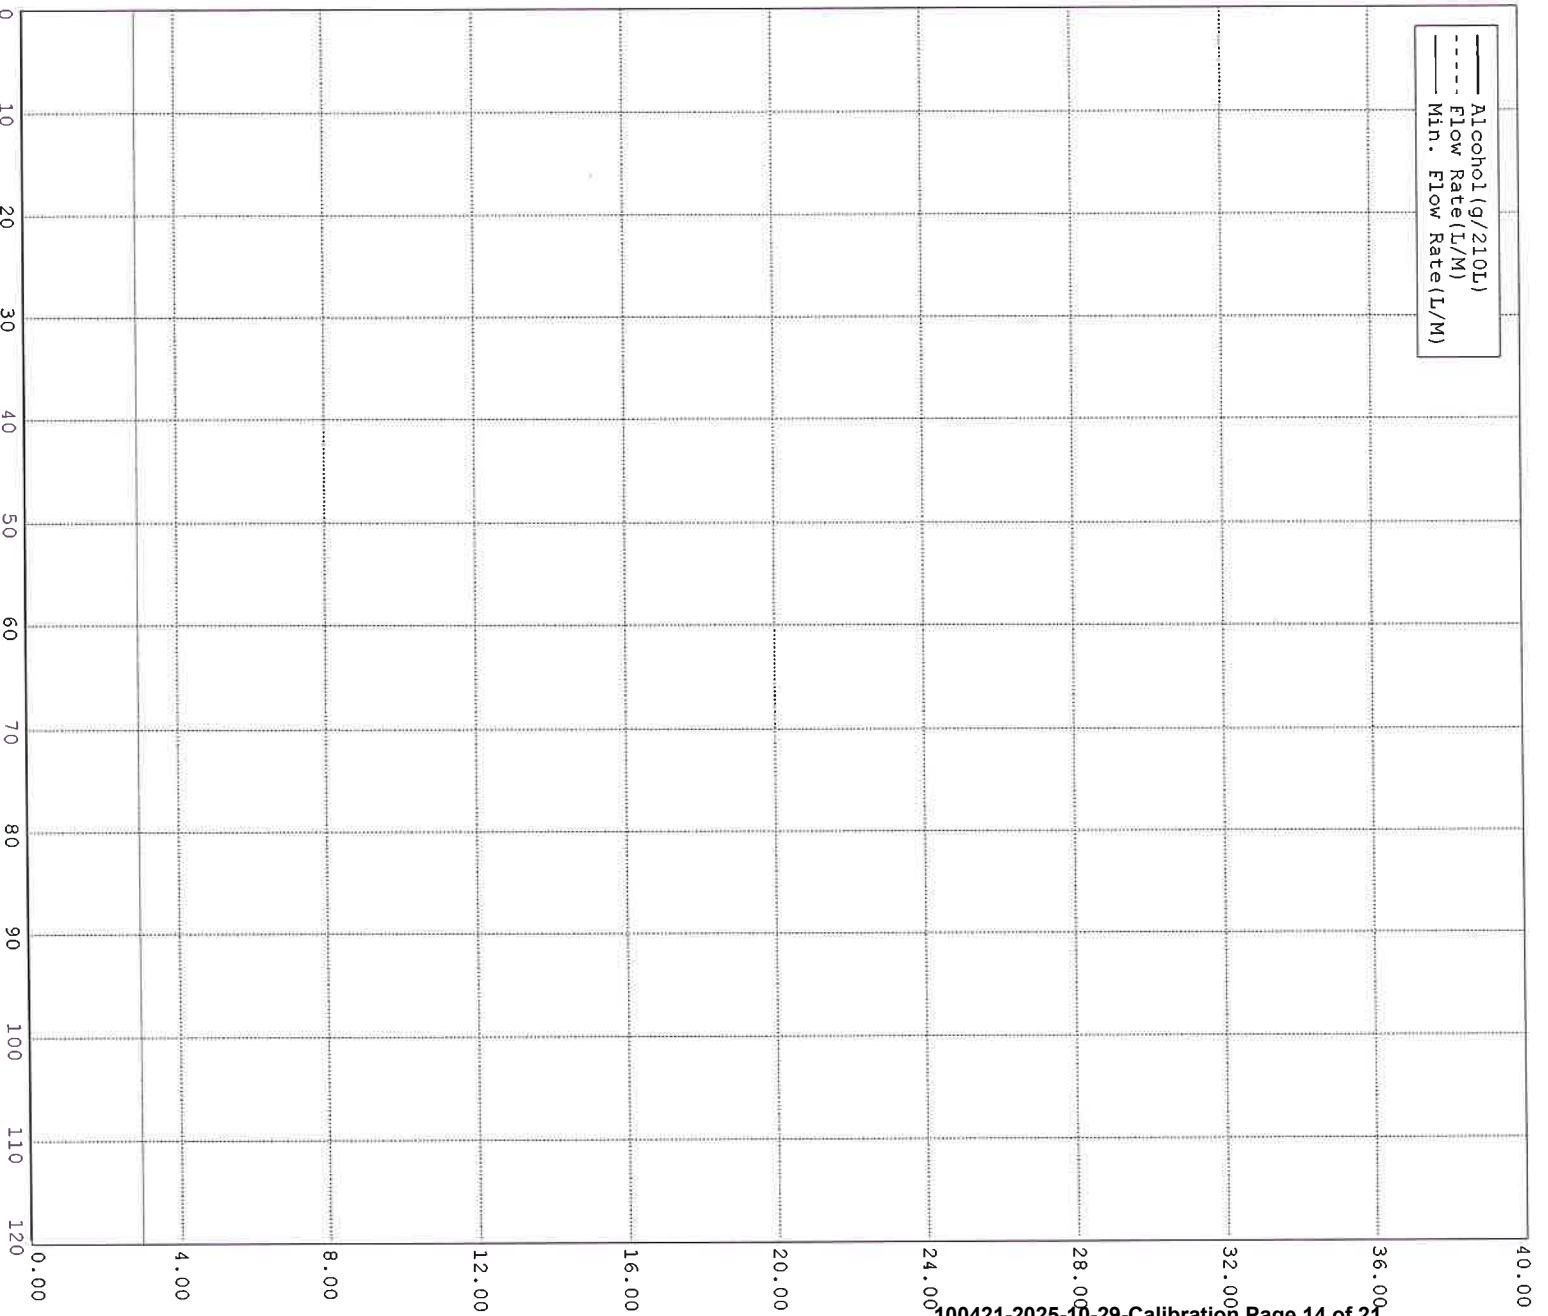

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100421

Date: 10/29/2025
Time: 10:21:53

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MAX ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.08: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:23
BLANK TEST	0.000	10:23
INTERNAL STANDARD	VERIFIED	10:23
EXTERNAL STANDARD	0.080	10:23
BLANK TEST	0.000	10:24
SUBJECT SAMPLE	XXX	10:25

Maximum Attempts Exceeded

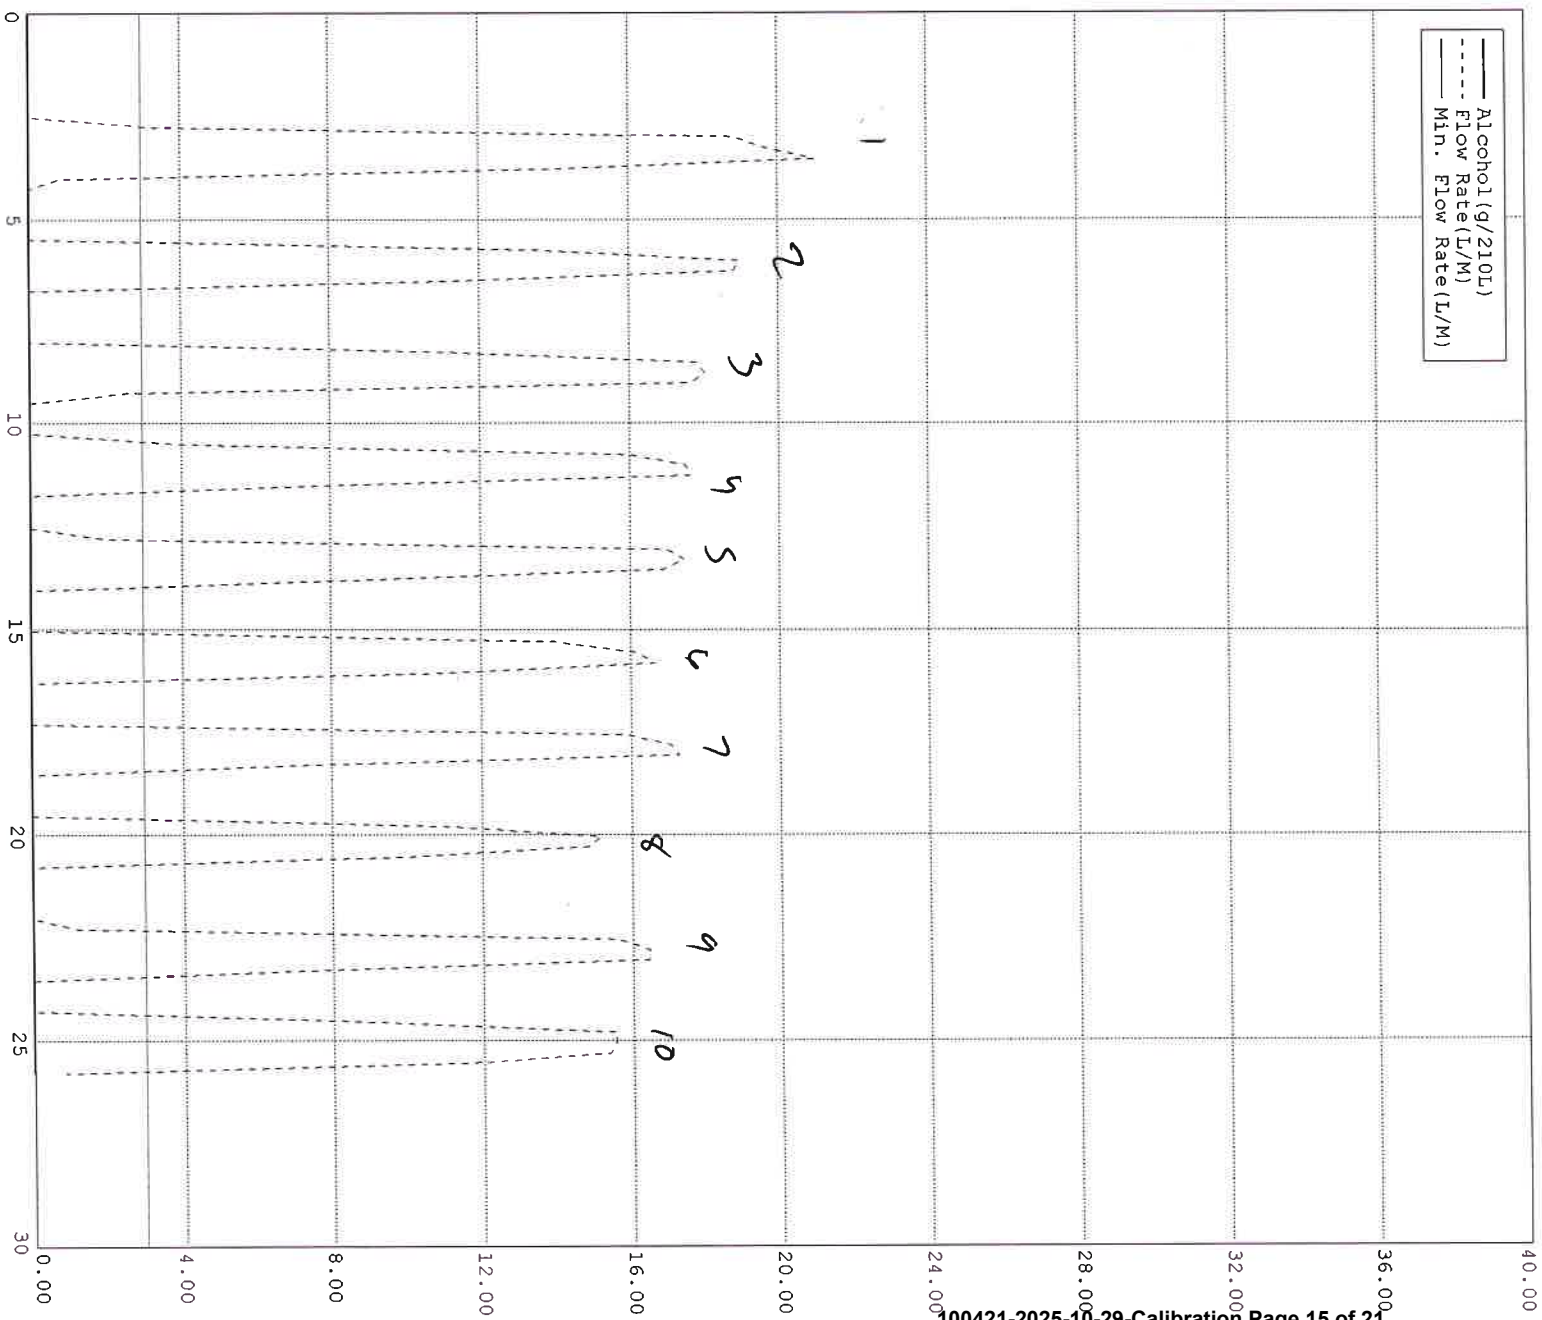

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100421

Date: 10/29/2025
Time: 10:27:10

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.06: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 10:36
INTERNAL STANDARD VERIFIED 10:37
EXTERNAL STANDARD 0.080 10:37
BLANK TEST 0.000 10:38
SUBJECT SAMPLE INVALID 10:38



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dnt: 100421

Date: 10/29/2025
Time: 10:40:25

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.07: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 10:41
INTERNAL STANDARD VERIFIED 10:42
EXTERNAL STANDARD 0.079 10:42
BLANK TEST 0.000 10:43

RFI DETECTED

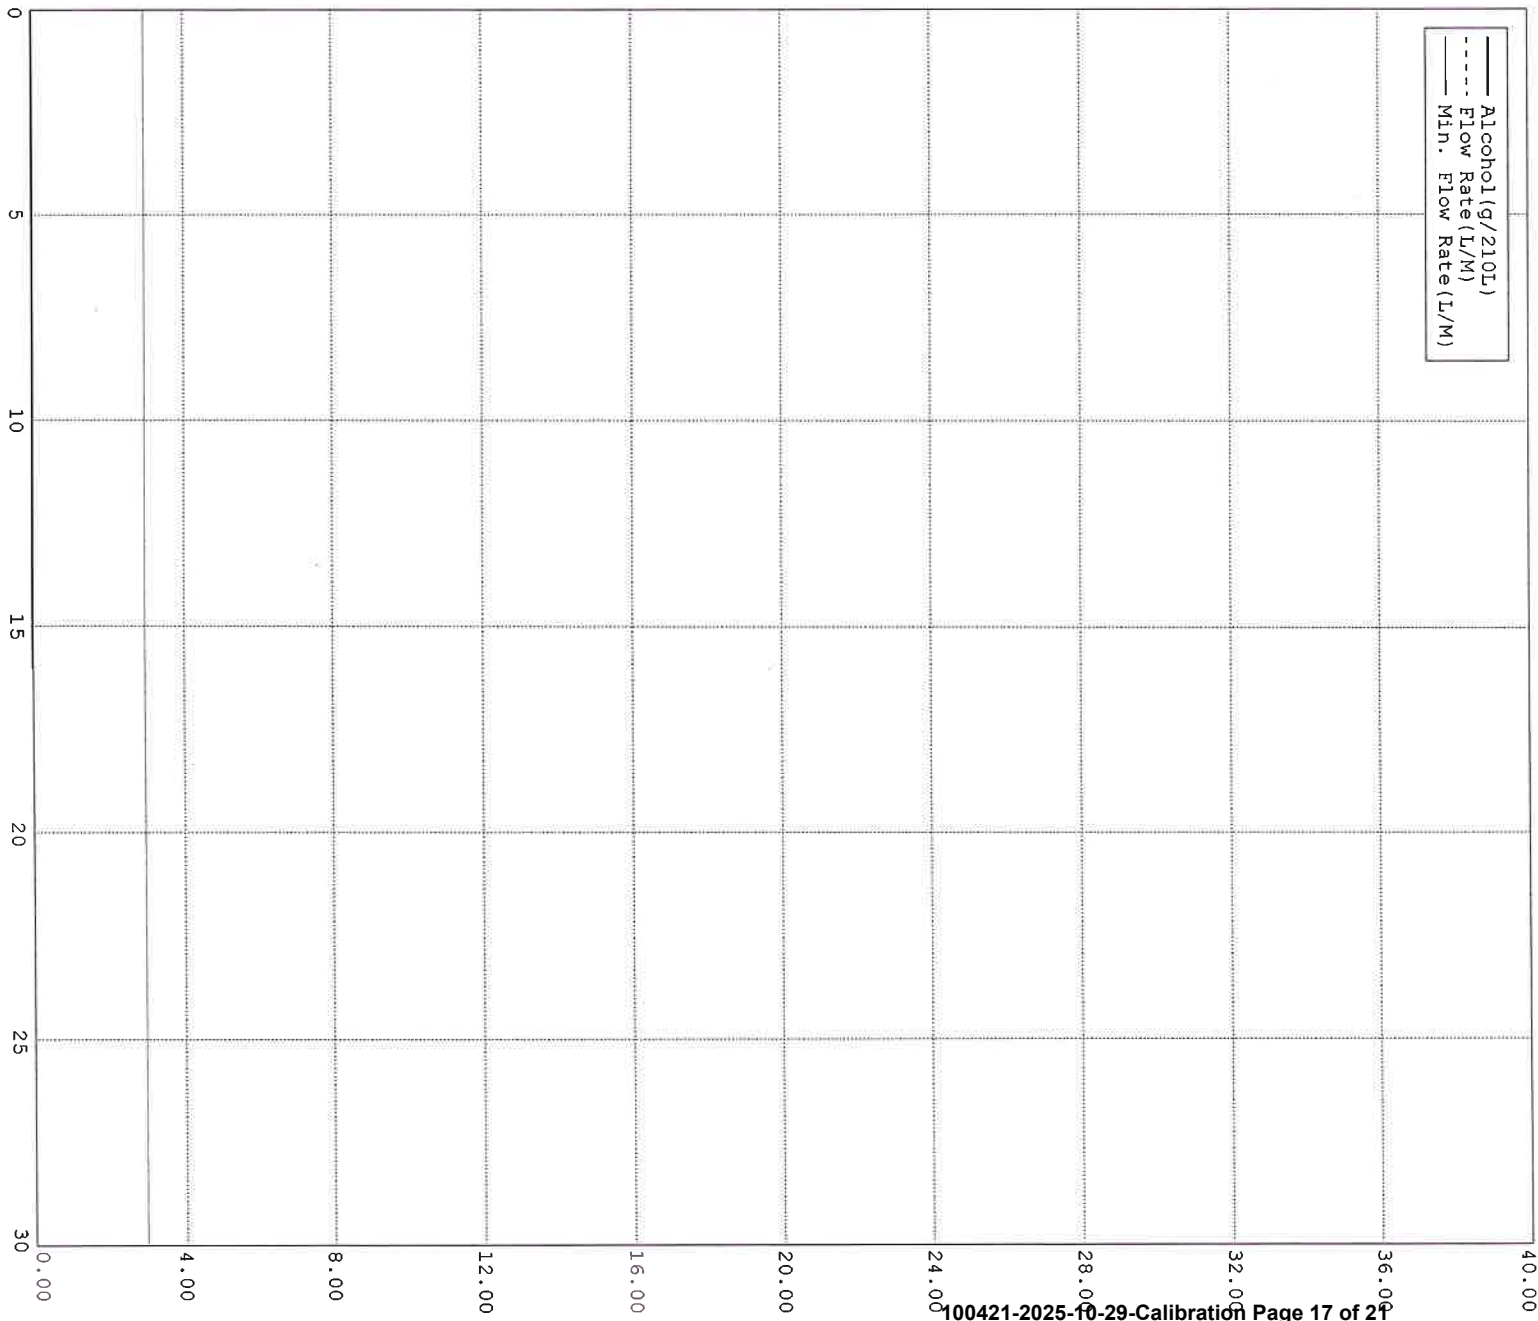

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100421

Date: 10/29/2025
Time: 12:31:30

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.00: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025


DIAGNOSTIC CHECK
BLANK TEST PASSED 12:33
INTERNAL STANDARD VERIFIED 12:33
Xq = 0.098 (0.98%)
EXTERNAL STANDARD 0.078 12:33
X[1] = 0.0779 (0.0003) (0.0012)
BLANK TEST 0.000 12:34
SUBJECT SAMPLE XXX 12:35
X[1] = 0.1096 (-0.0192) (0.0000)

Interference Detected

Filter Lav: -0.0008

Filter Sav: 0.0010

KS 10/29/25

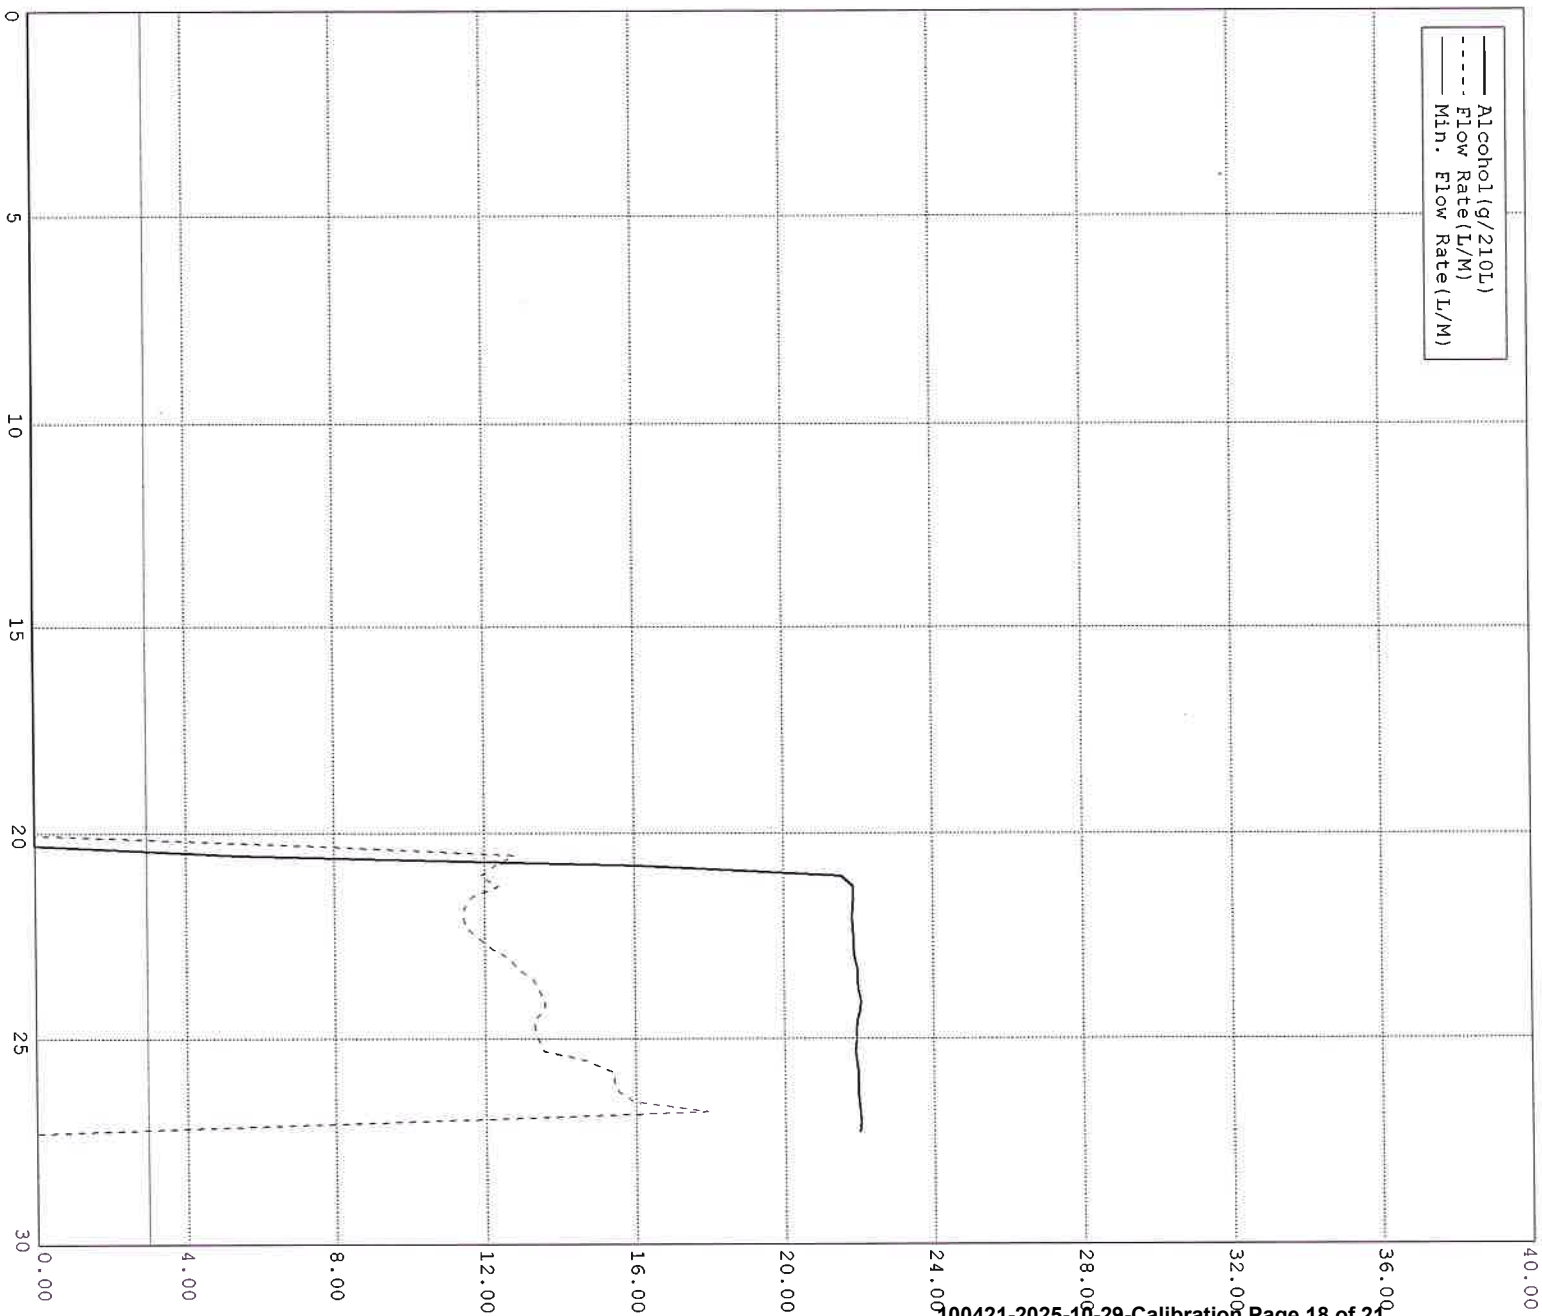

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100421

Date: 10/29/2025
Time: 12:39:00

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.00: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST
INTERNAL STANDARD
Xq = 0.098 (0.27%)
EXTERNAL STANDARD
X[1] = 0.0792 (-0.0001)
BLANK TEST
SUBJECT SAMPLE
X[1] = 0.1199 (-0.0211)

	PASSED	12:40
0.000	12:40	
VERIFIED	12:40	
0.079	12:40	
(0.0011)		
0.000	12:41	
XXX	12:42	
(0.0010)		

Interference Detected

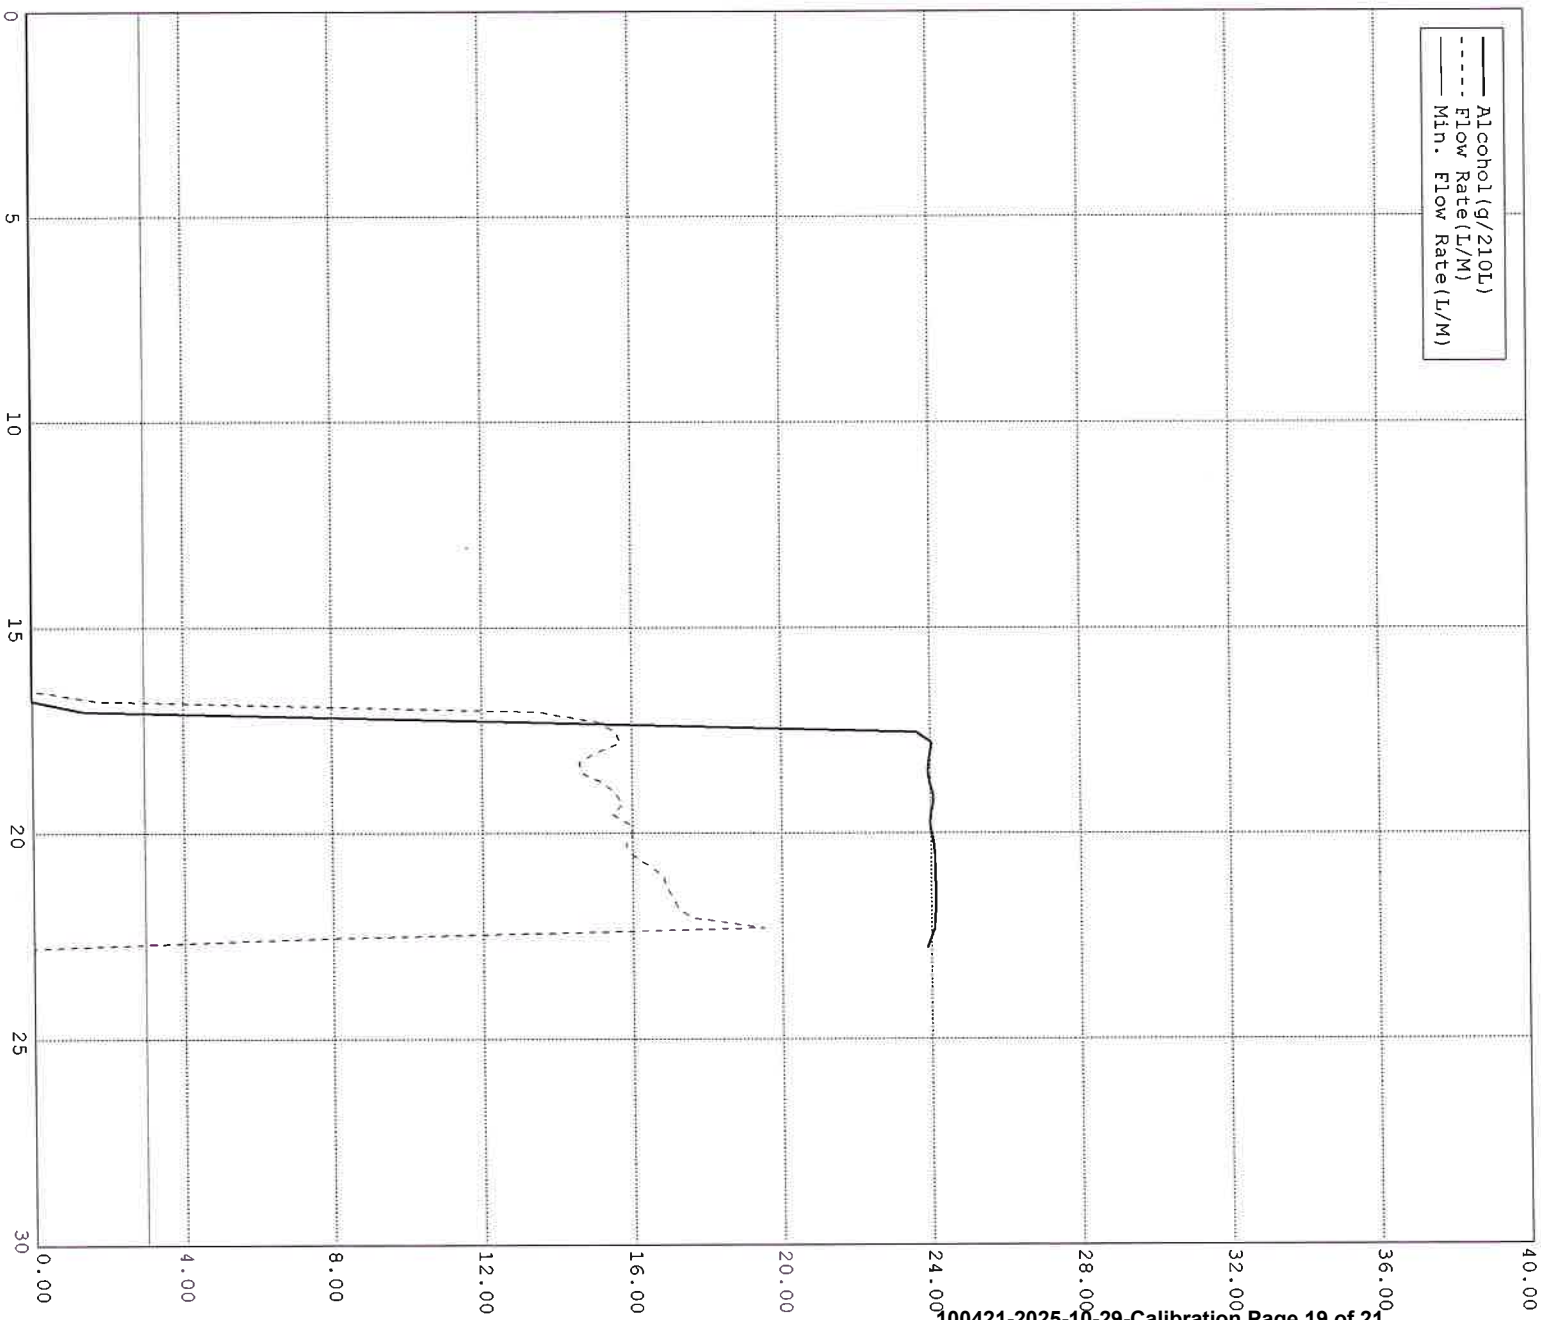

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100421

Date: 10/29/2025
Time: 12:44:57


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.99: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:46
BLANK TEST	0.000	12:46
INTERNAL STANDARD	VERIFIED	12:46
Xg = 0.100 (0.98%)		
EXTERNAL STANDARD	0.079	12:46
X[1] = 0.0789 (-0.0015)	(0.0008)	
BLANK TEST	0.000	12:47
SUBJECT SAMPLE (Vol=1.51L)	0.096	12:49
X[1] = 0.0962 (-0.0027)	(-0.0005)	
BLANK TEST	0.000	12:50
EXTERNAL STANDARD	0.078	12:50
X[1] = 0.0781 (-0.0017)	(0.0010)	
BLANK TEST	0.000	12:51

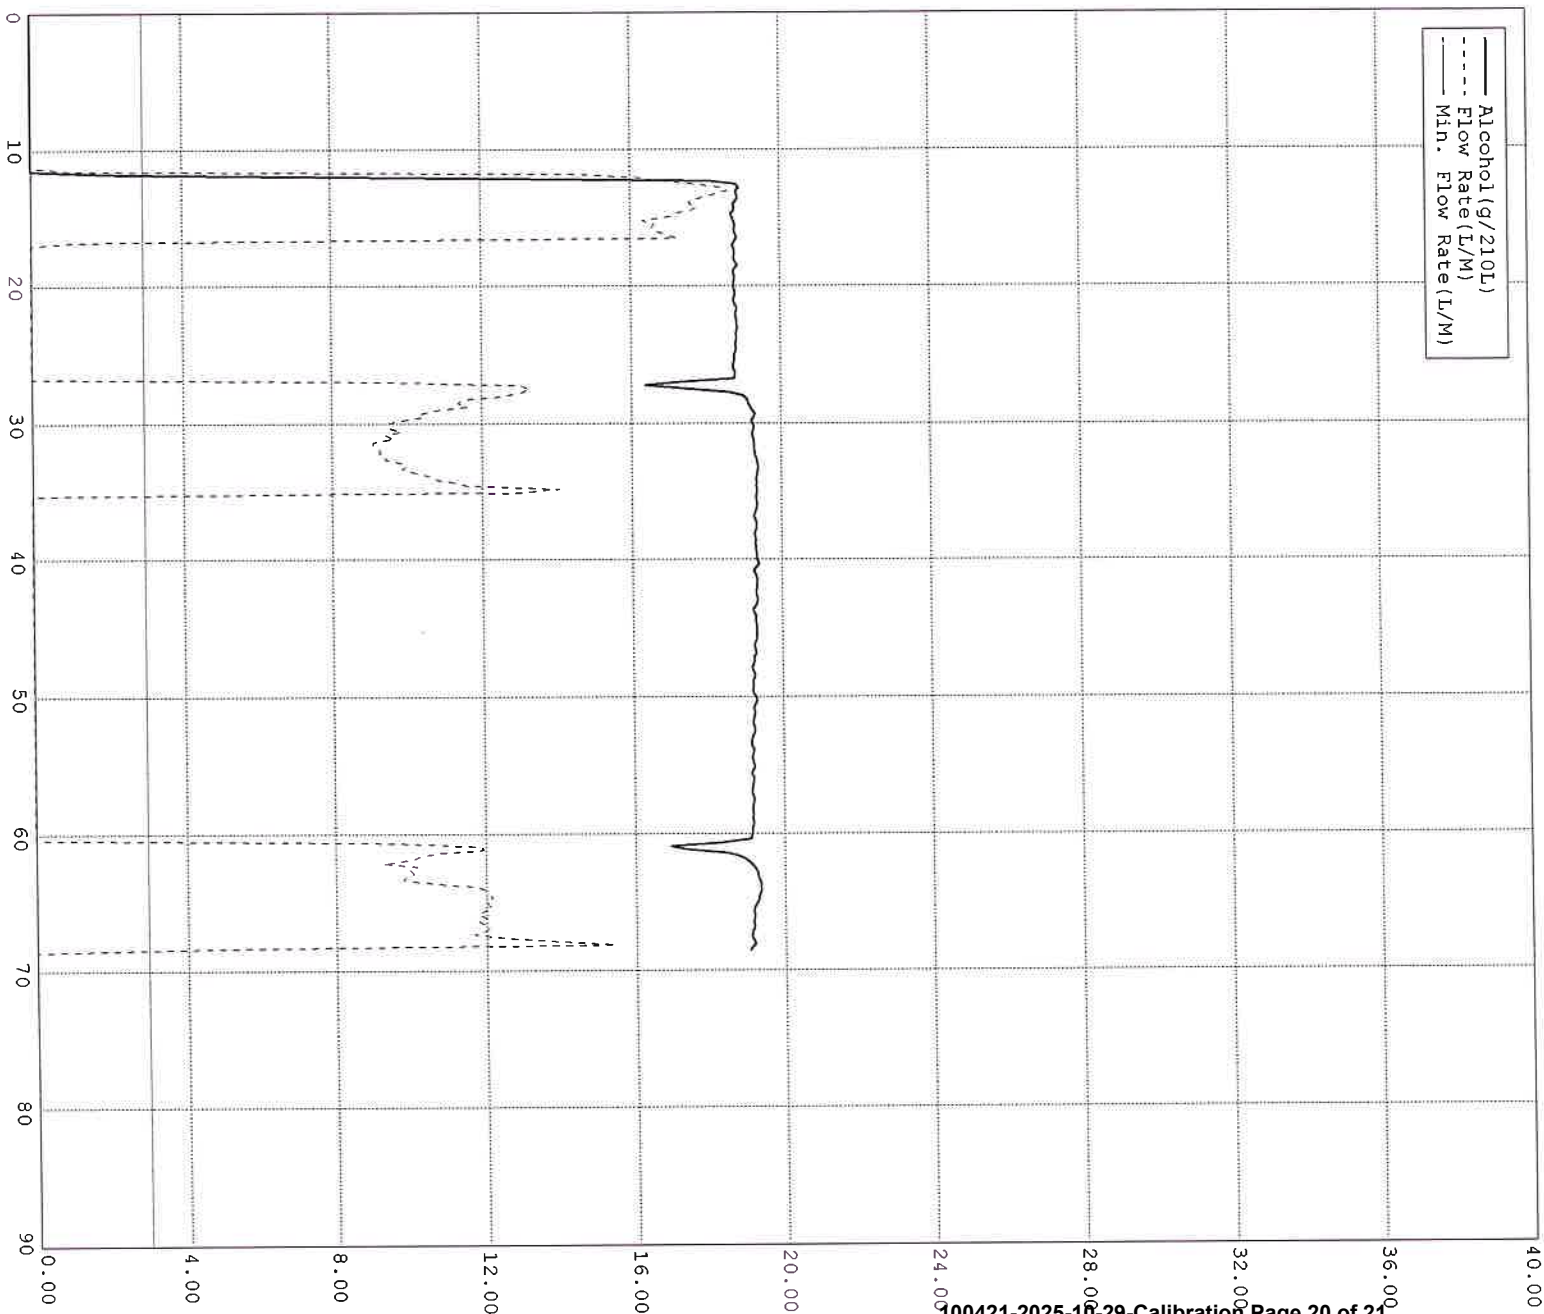

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100421

Date: 10/29/2025
Time: 13:13:56

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.97: 0.077
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:14
BLANK TEST	0.000	13:15
INTERNAL STANDARD	VERIFIED	13:15
EXTERNAL STANDARD	0.080	13:15
BLANK TEST	0.000	13:16
SUBJECT SAMPLE (Vol=2.10L)	0.000	13:16
BLANK TEST	0.000	13:17
EXTERNAL STANDARD	0.079	13:18
BLANK TEST	0.000	13:18

