



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100349

Report Issue Date: 07/15/2024
Date Received: 2024-02-20
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG217902	0.019	0.019	0.020	0.020	0.020	0.020
0.080	0.078	AG310901	0.076	0.077	0.077	0.077	0.077	0.077
0.300	0.294	AG327804	0.291	0.291	0.291	0.291	0.292	0.291

As Found - Evaluation Analyst: Carlie Glaister
 As Found Conditions - Barometric Pressure (inHg): 29.46 Barometer Used: Fisher S/N 230307229 Temperature (C): 22.5 Relative Humidity (%): 12
 As-Found Lab Activity Date Range: 02/22/2024 - 02/22/2024

Replaced o-ring.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG217904	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.080	AG310901	0.079	0.079	0.079	0.080	0.080	0.079	+/- 0.004
0.100	0.100	AG333401	0.100	0.100	0.100	0.100	0.100	0.100	+/- 0.004
0.150	0.150	AG332004	0.147	0.147	0.147	0.147	0.147	0.147	+/- 0.005
0.300	0.299	AG327804	0.298	0.298	0.298	0.299	0.299	0.298	+/- 0.011

As Left Conditions - Barometric Pressure (inHg): 29.83 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.3 Relative Humidity (%): 37
 As-Left Lab Activity Date Range: 06/13/2024 - 07/12/2024

Supervised casework with Kaija Swisher.

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Derek Walton on 07/12/2024

derek.walton@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 07/15/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100349 Analyst or Technician Name: Kaija Swisher

DataMaster DMT Calibration Start Date: 6/13/24

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

*Supervised casework with
Derek Walton 07/11/24*

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: May 2, 2025
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.83 Temperature(C) 20.3 Relative Humidity(%) 37
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
 - Invalid
 - Interference (Volatiles) - *Print with View Details*
 - Maximum Attempts Exceeded
 - Radio Frequency Interference (RFI)
- ✓ 1. Acetone Reagent Lot Number: 20240501KS Expiration Date: 8/1/24
Simulator S/N: SD1088 Thermometer Verification Performed?
 - ✓ 2. Isopropanol Reagent Lot Number: 20240501MNC Expiration Date: 8/1/24
Simulator S/N: DR4161 Thermometer Verification Performed?
 - ✓ 3. Negative (Ethanol Only) Lot Number: 224P41201 Expiration Date: 8/1/24
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: Sept. 19, 2025

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 6/13/24

Data Interpretation Date (Technician): _____ (if applicable)

Data Interpretation Date (Analyst): 6/13/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 05:30:38

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 47.3°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.75 V PASSED
(1.05 V - 2.45 V)
Cooler Voltage = 1.73 V PASSED
(1.04 V - 2.42 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 530 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 30.0 in

PUMP INFO

Flow Rate = 4.657 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.078 0.67% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 5:35 AM

Temperatures (°C)
Sample Cell: 48.7°C
Breath Tube: 46.8°C

Current Barometer 29.8 in
Volume (Ltr) 1.49

Settings
Lamp: 1.75 V
Bias: 80 V
Cooler: 1.73 V
Chopper: 530 Hz

Voltages (V)
Flow: 1.06 V
Detector: 0.071 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 04/29/2024
Time: 12:41:52

OPERATOR NAME:
KAIJA SWISHER
CERTIFICATE #: 10746

Ca = 0.1000
CAL = 0.980299 0.800 <= CAL < 1.200
b1 = 0.0005 0.0000 <= b1 < 0.0040
b2 = 0.0057 0.0010 <= b2 < 0.0100
b3 = 0.0009 0.0000 <= b3 < 0.0040
Xq = 0.0777 0.0500 <= Xq < 0.2000
a21 = 1.191043 1.050 <= a21 < 1.300
a31 = 0.569042 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100349

Date: 06/13/2024
Time: 05:39:55

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


Lot # A69310901
Exp 4/17/25
KS 6/18/24

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK	PASSED	05:41
BLANK TEST	0.000	05:41
INTERNAL STANDARD	VERIFIED	05:41
EXTERNAL STANDARD	0.079	05:41
BLANK TEST	0.000	05:42
SUBJECT SAMPLE (Vol=1.51L)	0.000	05:43
BLANK TEST	0.000	05:44
EXTERNAL STANDARD	0.079	05:44
BLANK TEST	0.000	05:45

KS

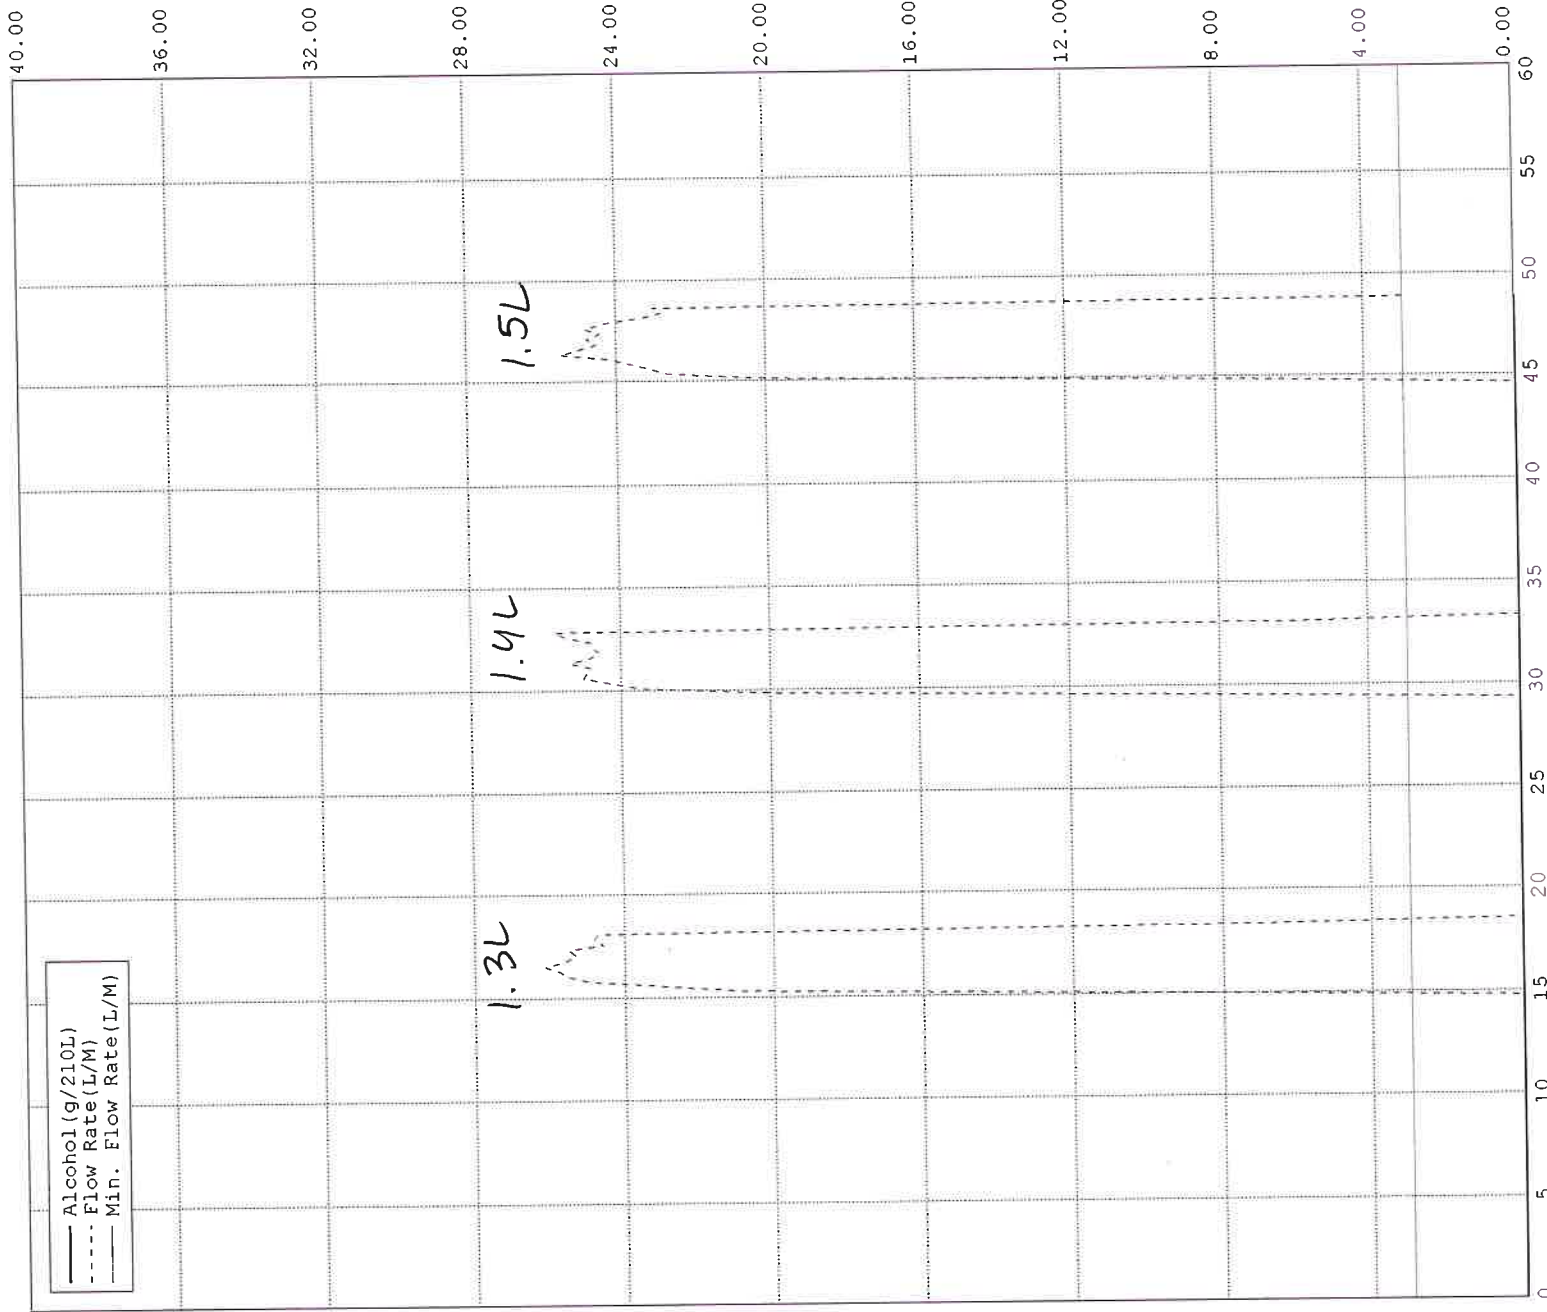

LINEARITY CHECK


Alaska Department of Public Safety
 DATAMASTER dmt: 100349

Date: 06/13/2024
 Time: 05:55:00

SUPERVISOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.040	0.0400	0.0000
0.080	0.0794	0.0005
0.100	0.1000	0.0000
0.150	0.1470	0.0000
0.299	0.2984	0.0005

SLOPE = 0.996188
 R² = 0.999881

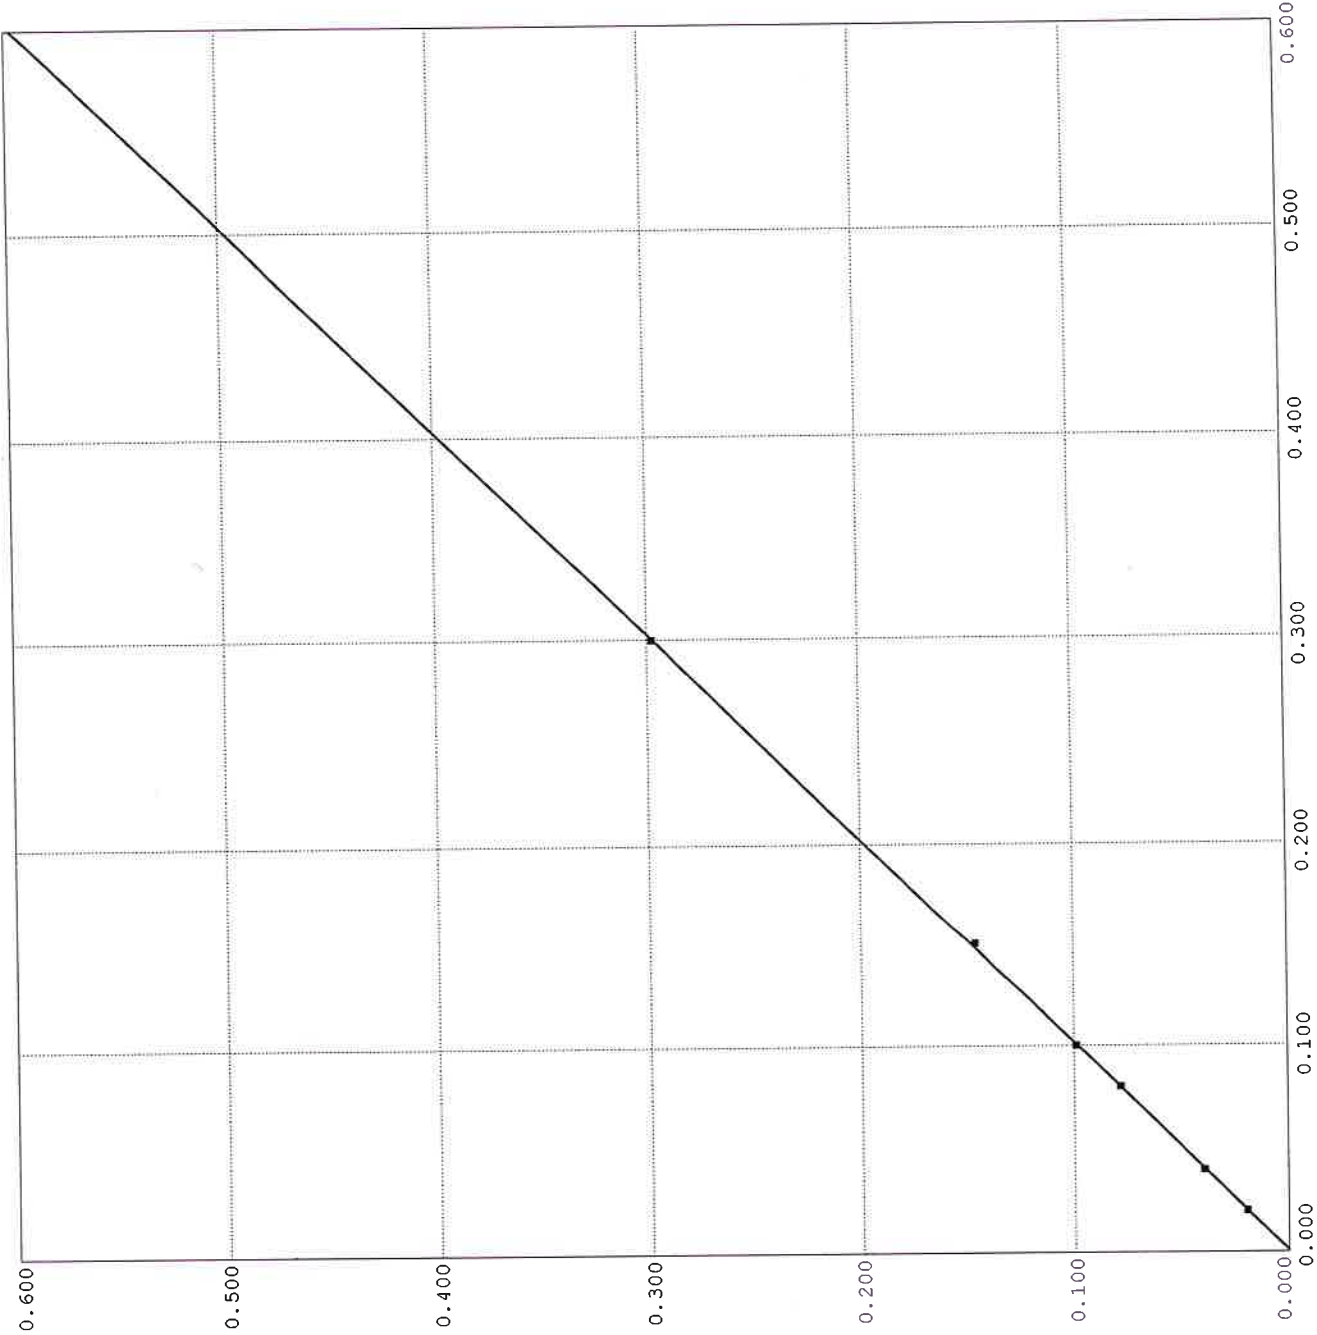

KS

LINEARITY CHECK: Control Test 1






Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 05:55:02

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.020
TARGET AT 29.83: 0.020
LOT #: AG217902
EXPIRATION: 06/28/2024
TANK PRESSURE: 250 psi

BLANK TEST	0.000	05:56
INTERNAL STANDARD	VERIFIED	05:56
EXTERNAL STANDARD	0.020	05:56
BLANK TEST	0.000	05:57
EXTERNAL STANDARD	0.020	05:57
BLANK TEST	0.000	05:58
EXTERNAL STANDARD	0.020	05:58
BLANK TEST	0.000	05:59
EXTERNAL STANDARD	0.020	06:00
BLANK TEST	0.000	06:00
EXTERNAL STANDARD	0.020	06:01
BLANK TEST	0.000	06:02

Average = 0.0200
Std Dev = 0.0000

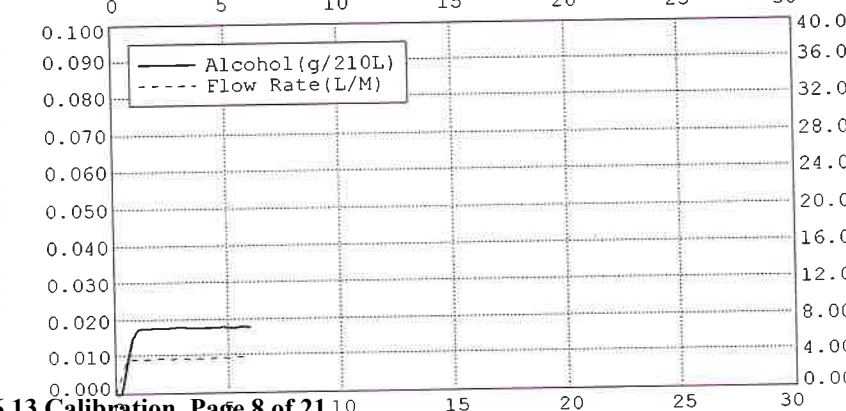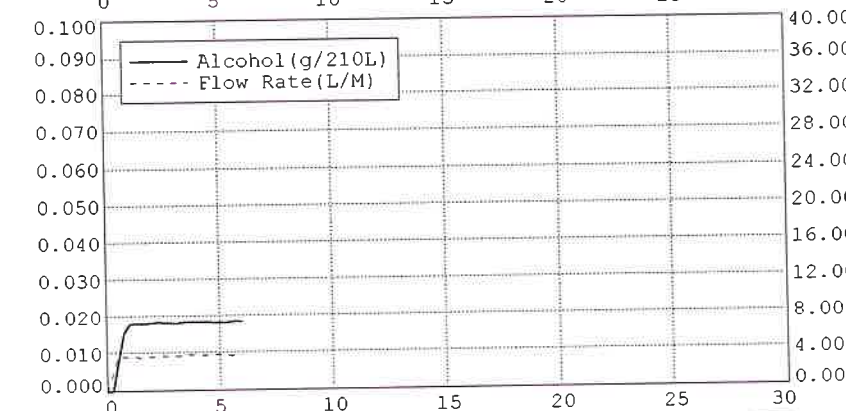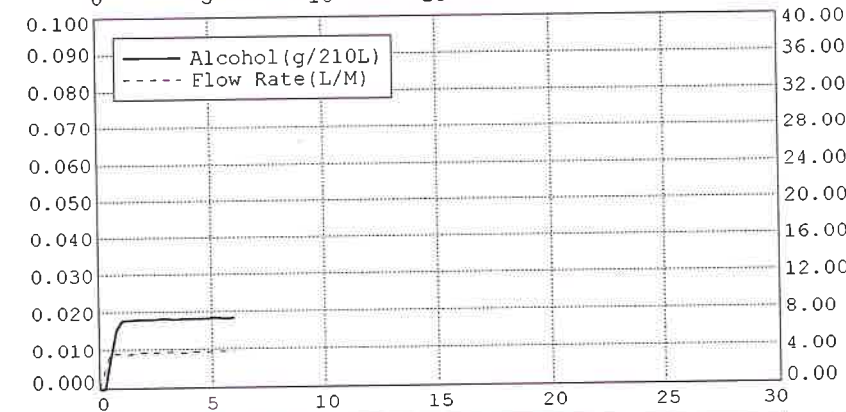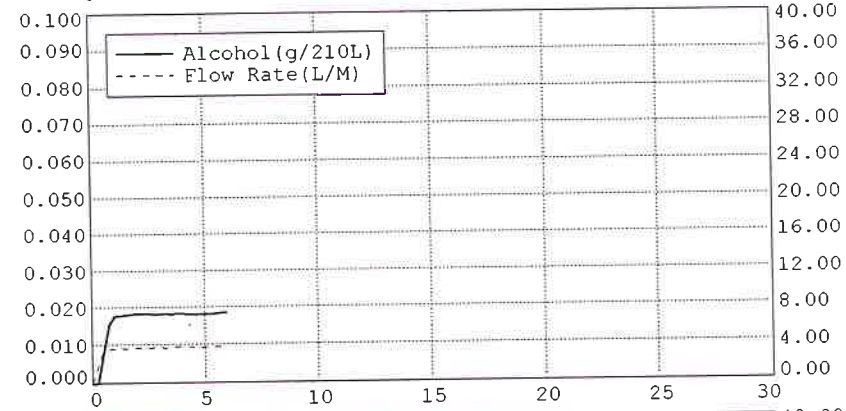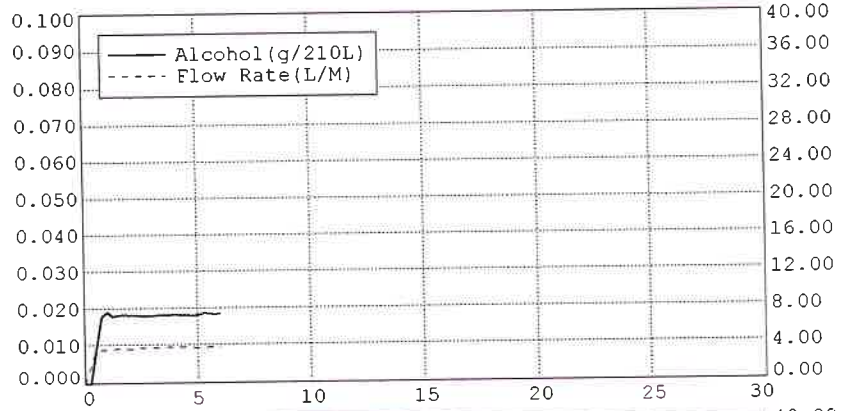

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100349






Date: 06/13/2024
Time: 06:02:51

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.83: 0.040
LOT #: AG217904
EXPIRATION: 06/28/2024
TANK PRESSURE: 756 psi

BLANK TEST	0.000	06:04
INTERNAL STANDARD	VERIFIED	06:04
EXTERNAL STANDARD	0.040	06:04
BLANK TEST	0.000	06:05
EXTERNAL STANDARD	0.040	06:05
BLANK TEST	0.000	06:06
EXTERNAL STANDARD	0.040	06:06
BLANK TEST	0.000	06:07
EXTERNAL STANDARD	0.040	06:07
BLANK TEST	0.000	06:08
EXTERNAL STANDARD	0.040	06:08
BLANK TEST	0.000	06:09

Average = 0.0400
Std Dev = 0.0000

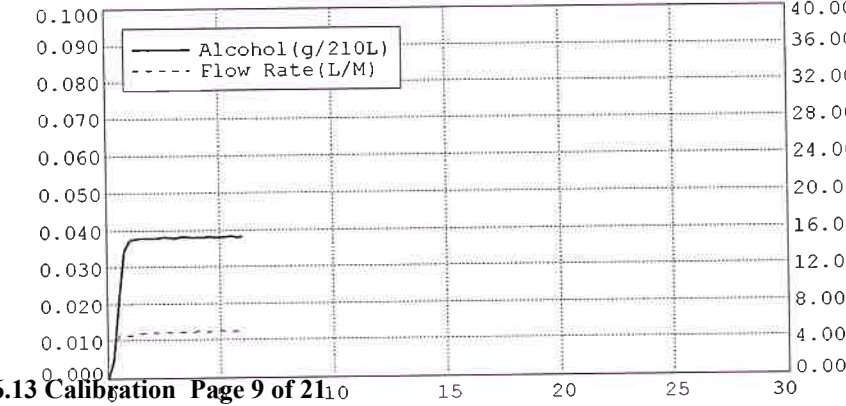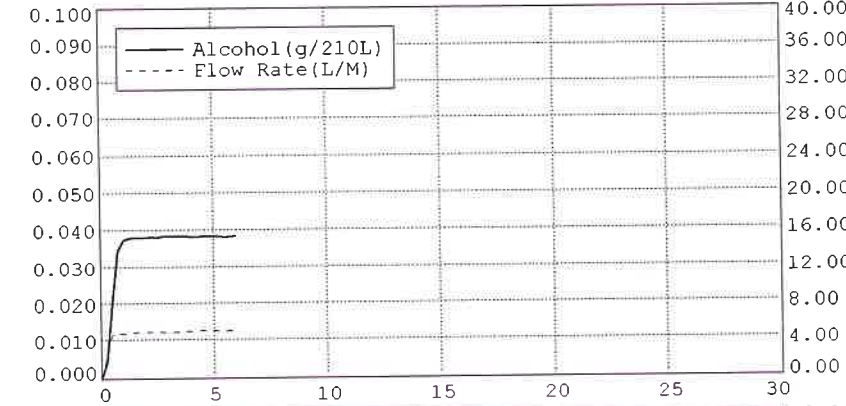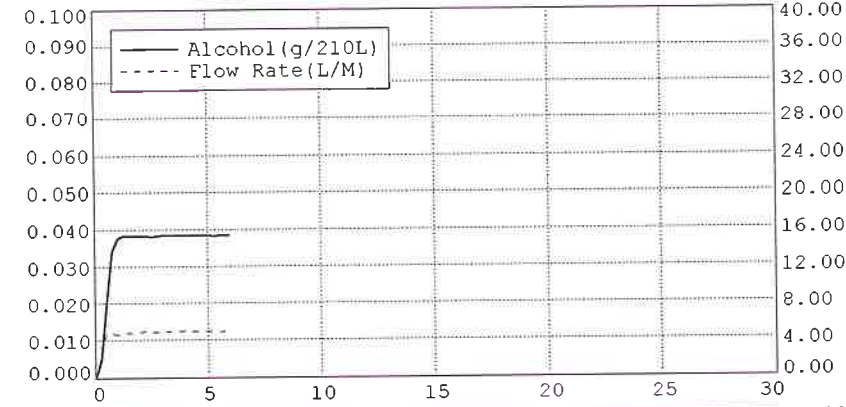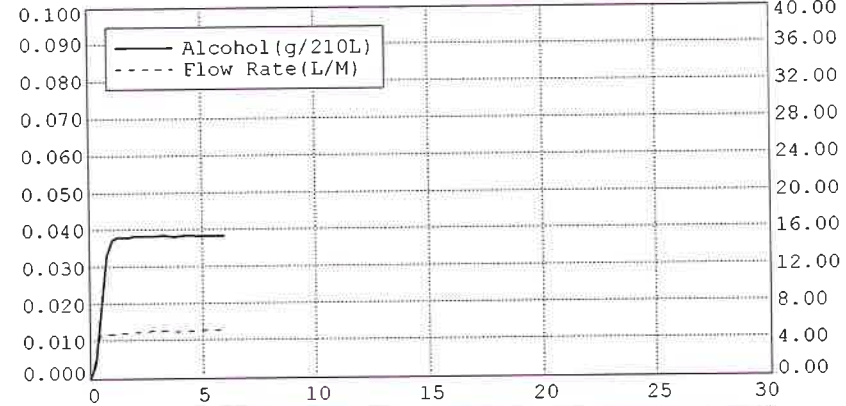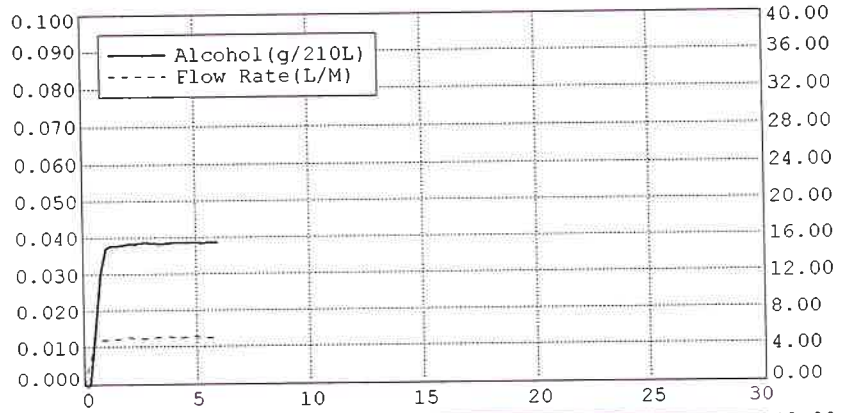

LINEARITY CHECK: Control Test 3






Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 06:10:37

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.84: 0.080
LOT #: AG310901
EXPIRATION: 04/19/2025
TANK PRESSURE: 714 psi

BLANK TEST	0.000	06:11
INTERNAL STANDARD	VERIFIED	06:11
EXTERNAL STANDARD	0.079	06:12
BLANK TEST	0.000	06:13
EXTERNAL STANDARD	0.079	06:13
BLANK TEST	0.000	06:14
EXTERNAL STANDARD	0.079	06:14
BLANK TEST	0.000	06:15
EXTERNAL STANDARD	0.080	06:15
BLANK TEST	0.000	06:16
EXTERNAL STANDARD	0.080	06:16
BLANK TEST	0.000	06:17

Average = 0.0794
Std Dev = 0.0005

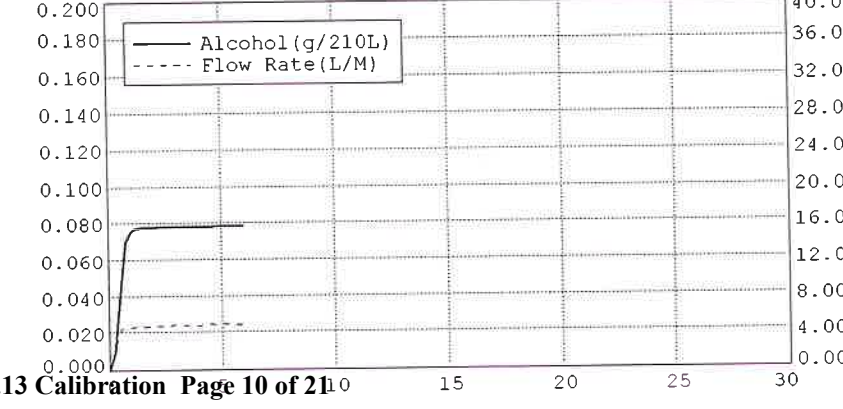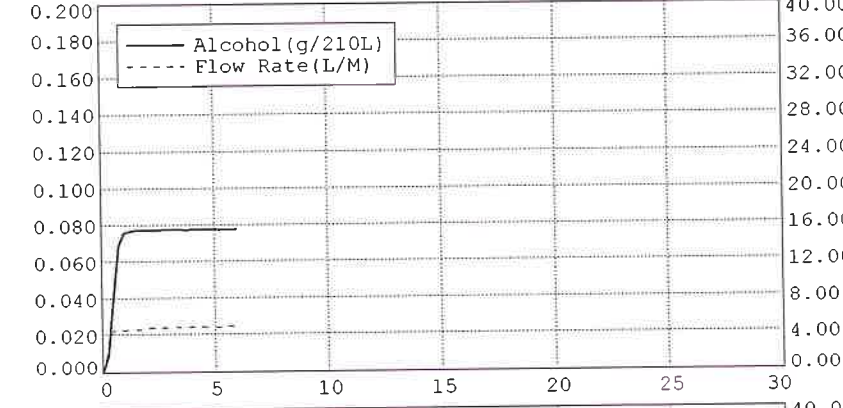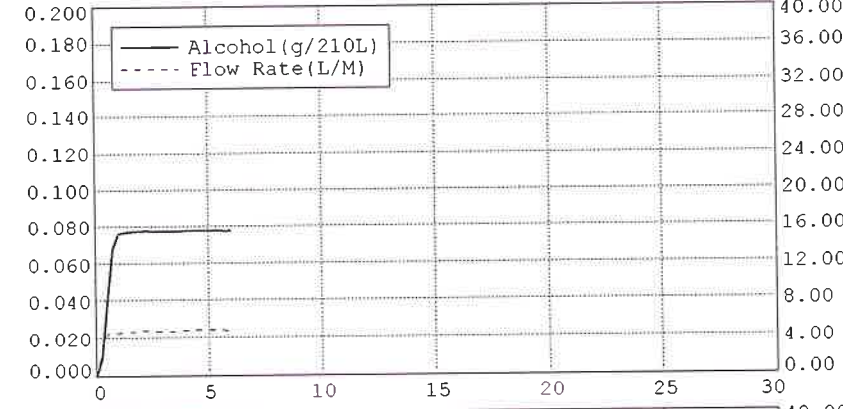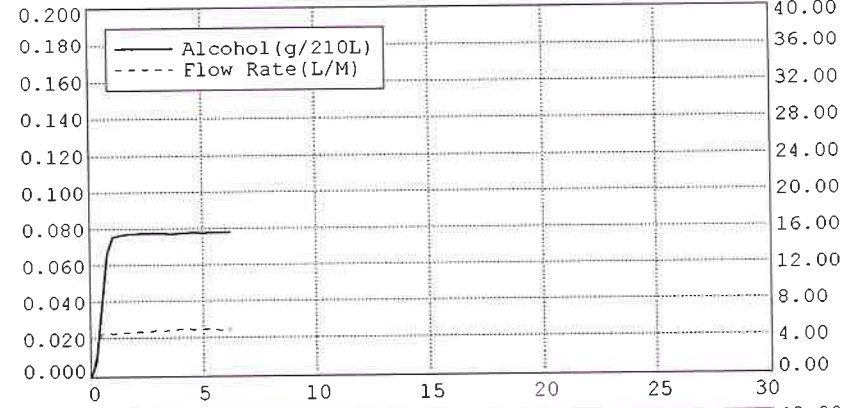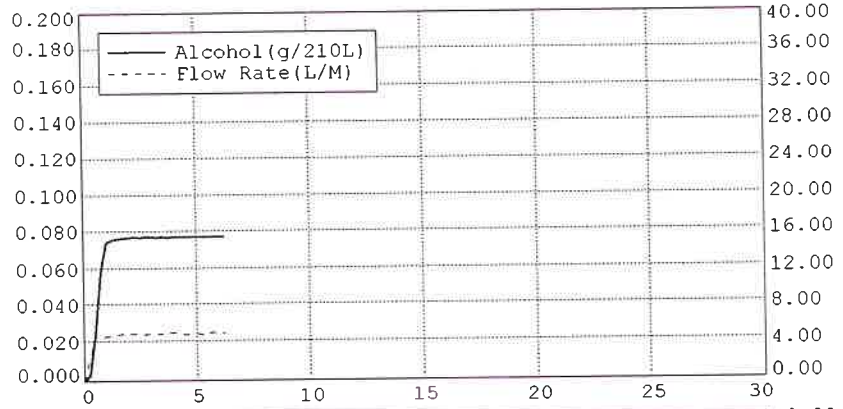

LINEARITY CHECK: Control Test 4






Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 06:18:43

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.100
TARGET AT 29.83: 0.100
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 1064 psi

BLANK TEST	0.000	06:20
INTERNAL STANDARD	VERIFIED	06:20
EXTERNAL STANDARD	0.100	06:20
BLANK TEST	0.000	06:21
EXTERNAL STANDARD	0.100	06:21
BLANK TEST	0.000	06:22
EXTERNAL STANDARD	0.100	06:22
BLANK TEST	0.000	06:23
EXTERNAL STANDARD	0.100	06:23
BLANK TEST	0.000	06:24
EXTERNAL STANDARD	0.100	06:24
BLANK TEST	0.000	06:25

Average = 0.1000
Std Dev = 0.0000

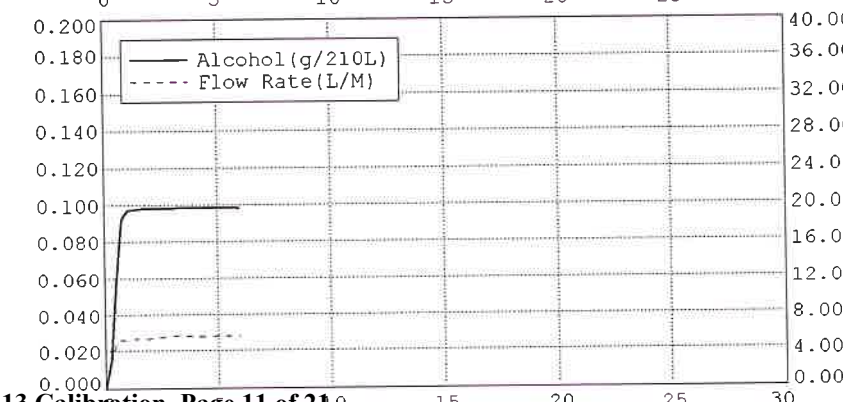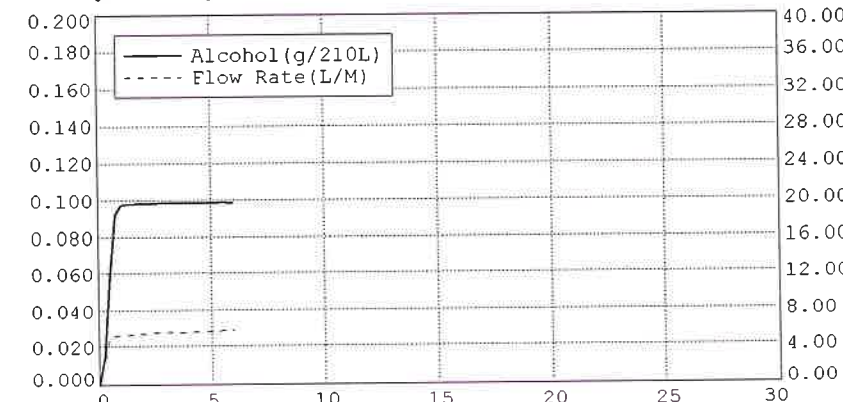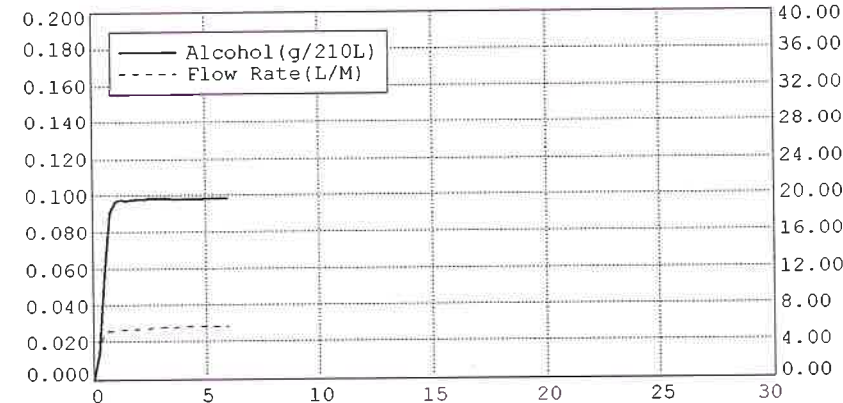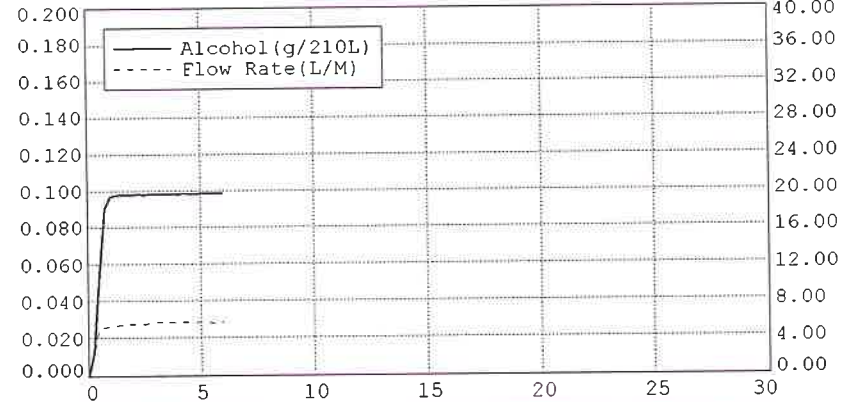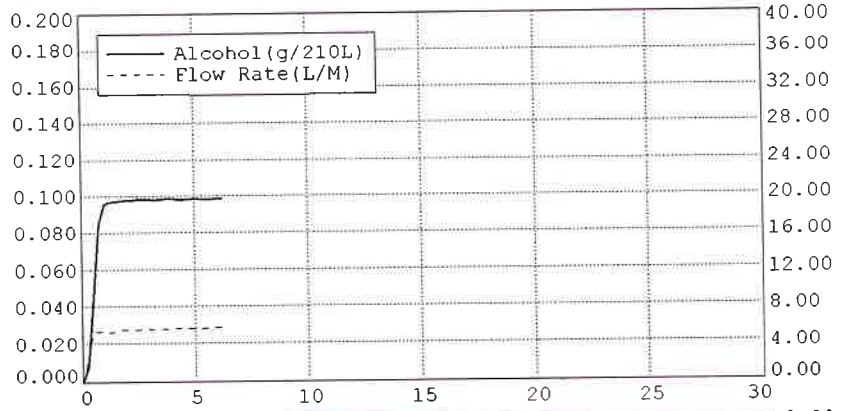

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100349






Date: 06/13/2024
Time: 06:26:48

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.84: 0.150
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 494 psi

BLANK TEST	0.000	06:28
INTERNAL STANDARD	VERIFIED	06:28
EXTERNAL STANDARD	0.147	06:28
BLANK TEST	0.000	06:29
EXTERNAL STANDARD	0.147	06:29
BLANK TEST	0.000	06:30
EXTERNAL STANDARD	0.147	06:30
BLANK TEST	0.000	06:31
EXTERNAL STANDARD	0.147	06:31
BLANK TEST	0.000	06:32
EXTERNAL STANDARD	0.147	06:32
BLANK TEST	0.000	06:33

Average = 0.1470
Std Dev = 0.0000

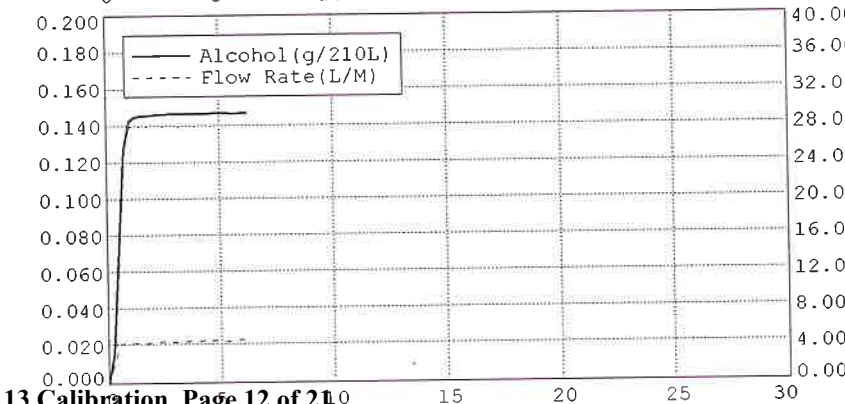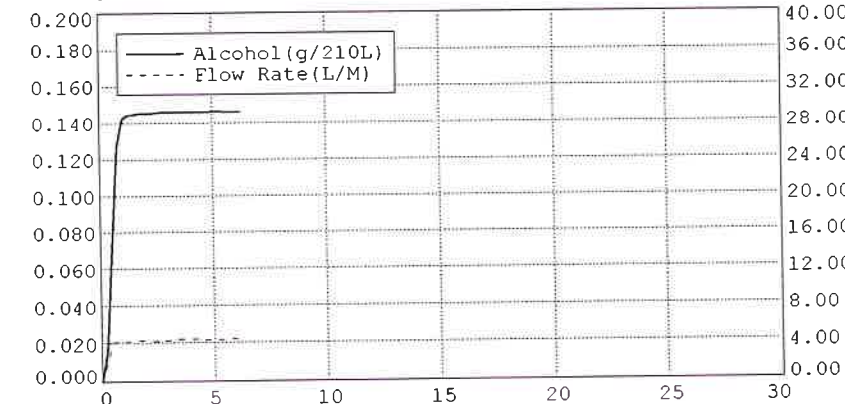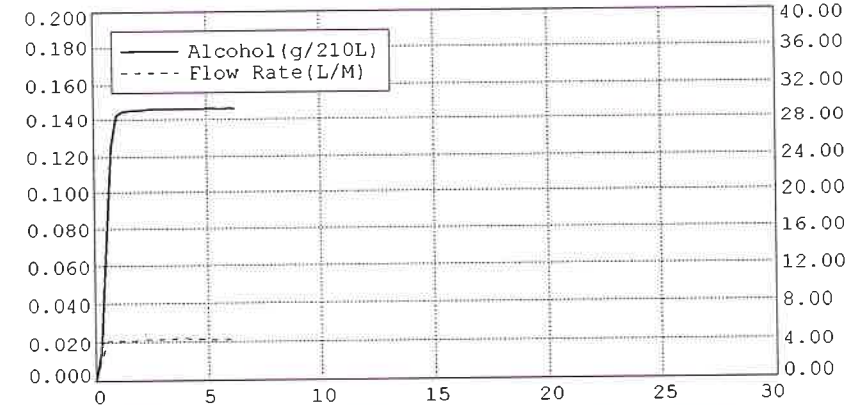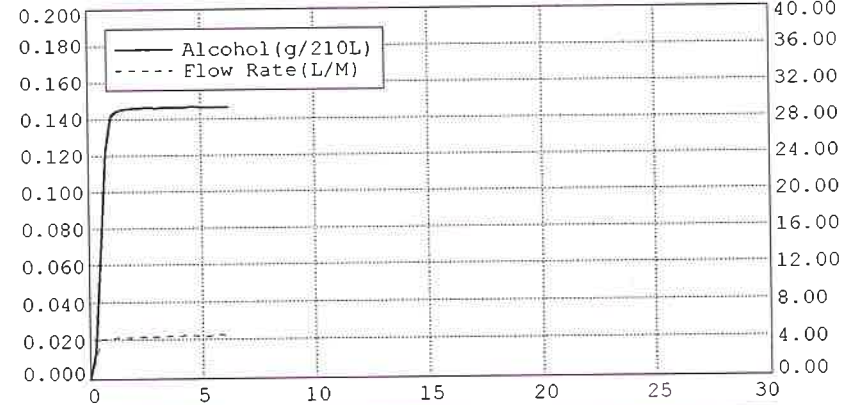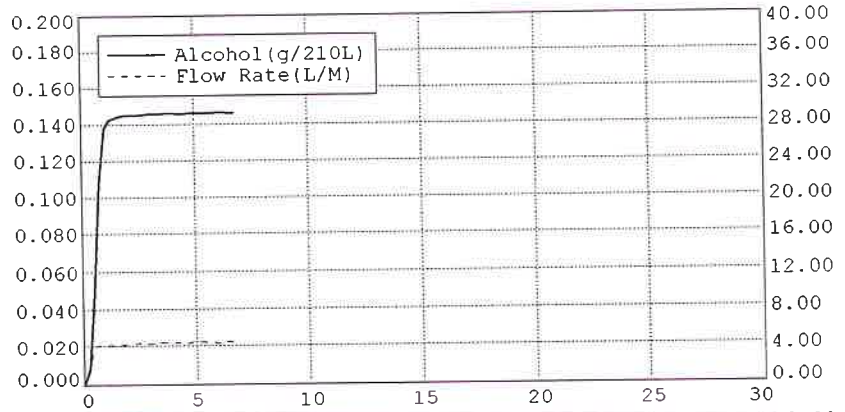

LINEARITY CHECK: Control Test 6






Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 07:04:23

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.300
TARGET AT 29.83: 0.299
LOT #: AG327804
EXPIRATION: 10/05/2025
TANK PRESSURE: 338 psi

BLANK TEST	0.000	07:05
INTERNAL STANDARD	VERIFIED	07:05
EXTERNAL STANDARD	0.298	07:06
BLANK TEST	0.000	07:07
EXTERNAL STANDARD	0.298	07:07
BLANK TEST	0.000	07:08
EXTERNAL STANDARD	0.298	07:08
BLANK TEST	0.000	07:09
EXTERNAL STANDARD	0.299	07:09
BLANK TEST	0.000	07:10
EXTERNAL STANDARD	0.299	07:10
BLANK TEST	0.000	07:11

Average = 0.2984
Std Dev = 0.0005

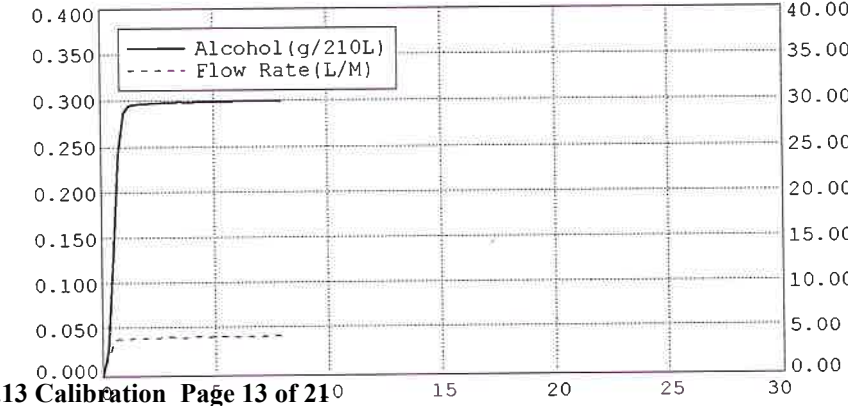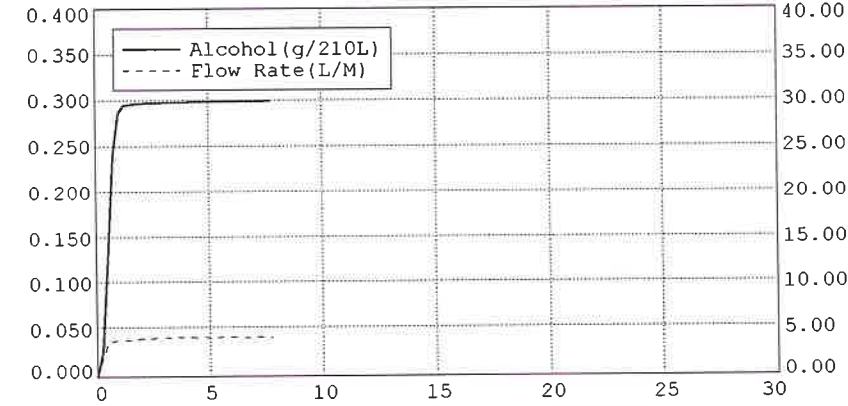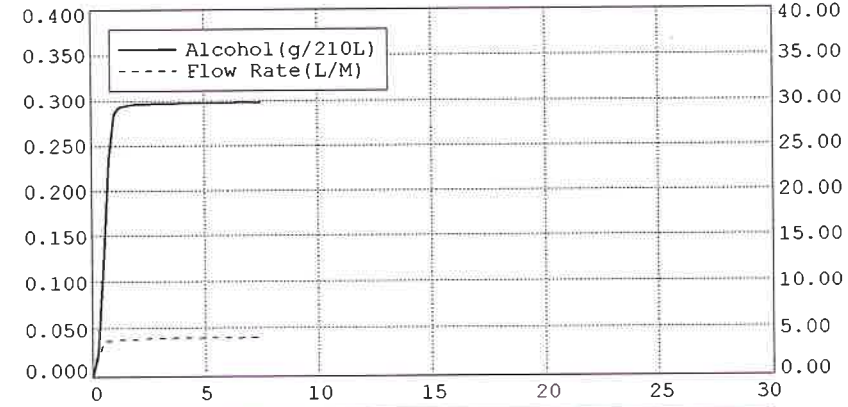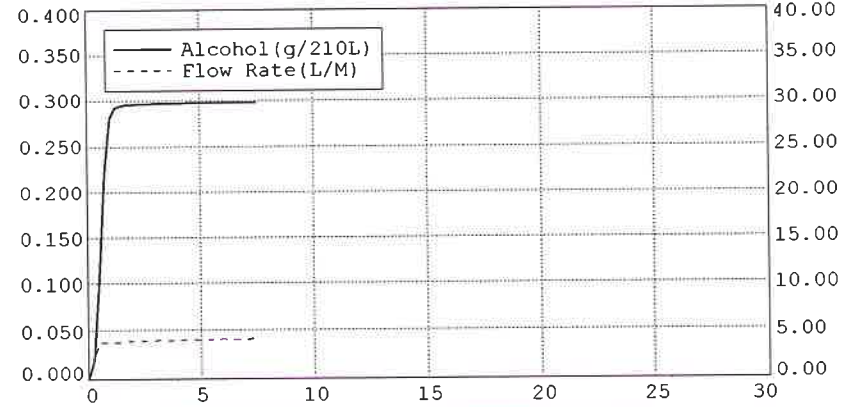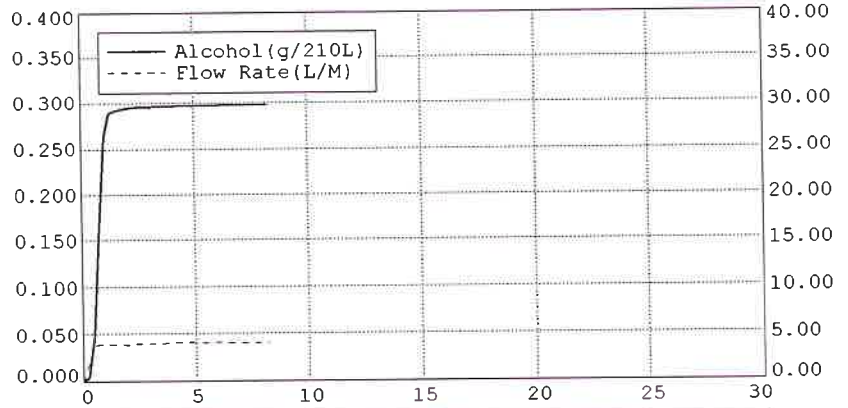

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 07:28:30

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST
*lot # AG316901
Exp 4/19/25
KS 6/18/24*

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK PASSED 07:29
BLANK TEST 0.000 07:29
INTERNAL STANDARD VERIFIED 07:29
INTERNAL STANDARD 0.079 07:29
BLANK TEST 0.000 07:30
SUBJECT SAMPLE INCOMPLETE 07:32

KS

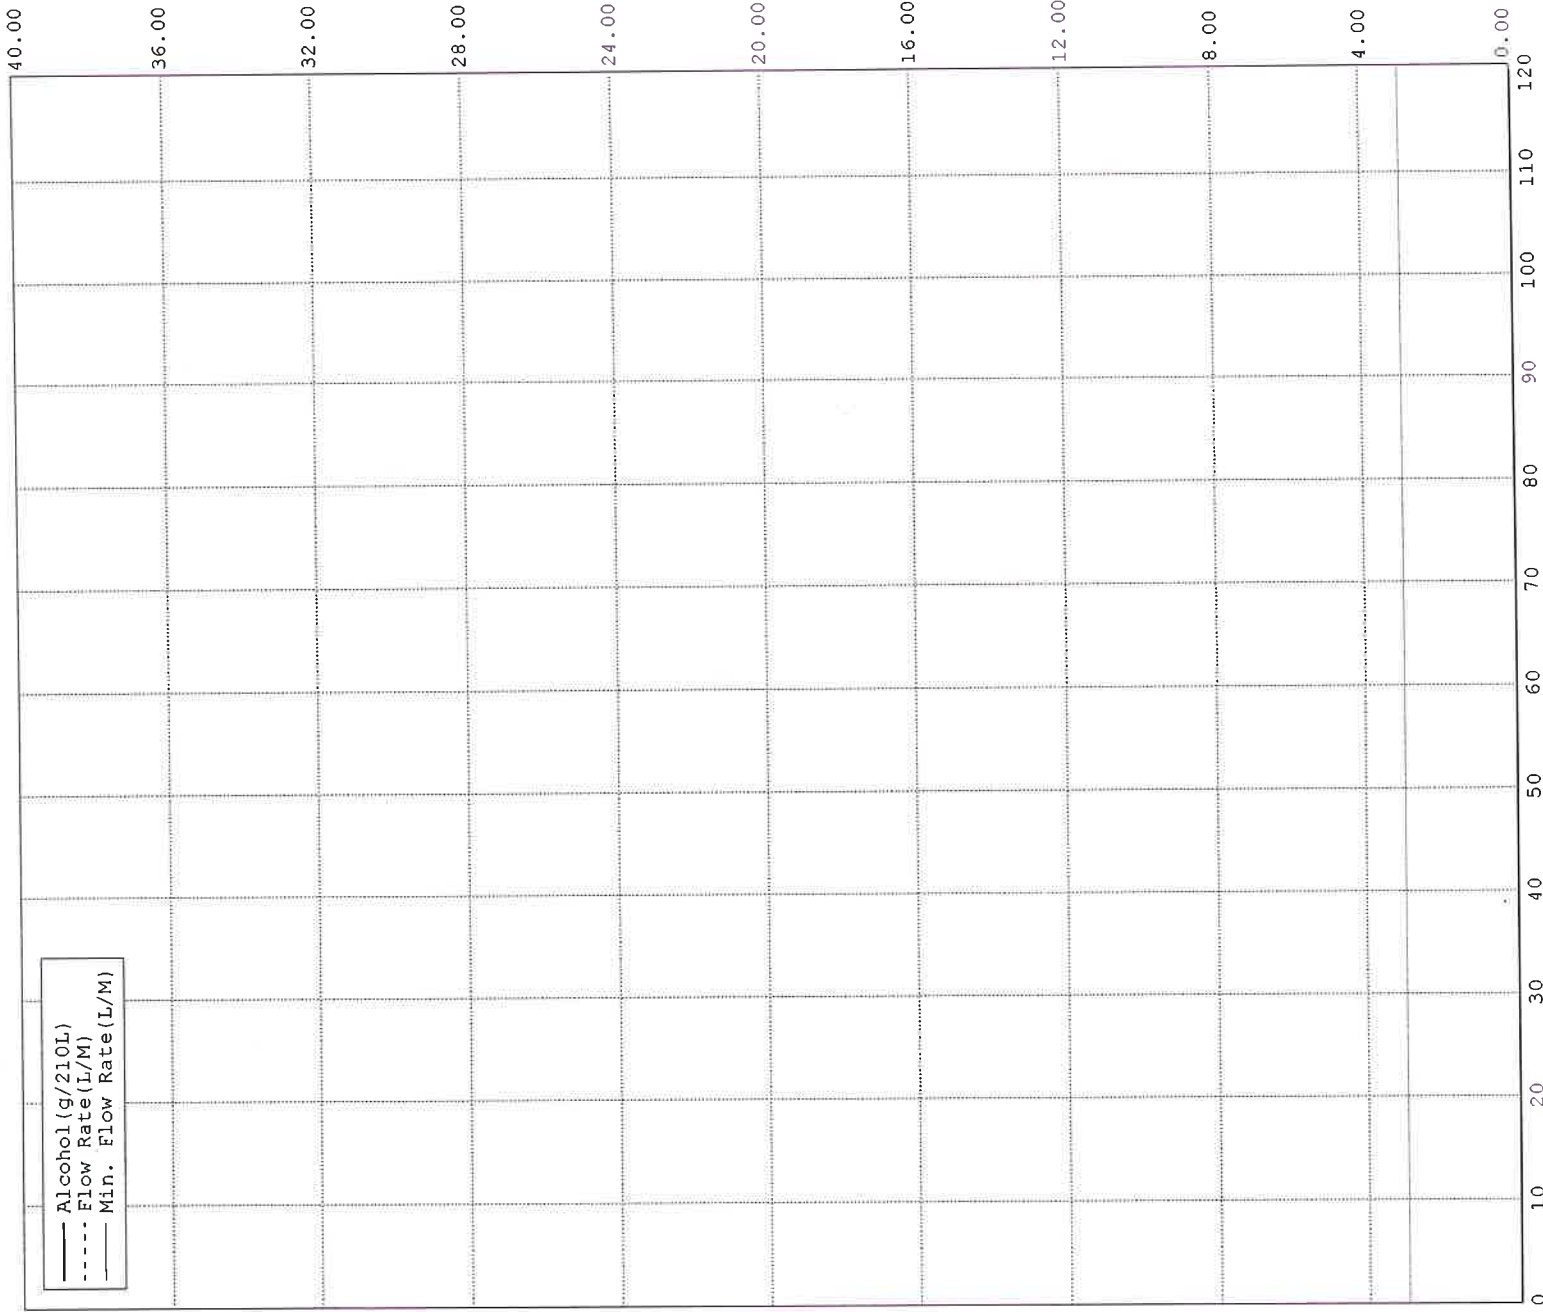

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100349

Date: 06/13/2024
 Time: 07:49:50

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

*Lot # A620901
 Exp 4/19/25
 KS 6/18/24*

OPERATOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746


DEPT/AGENCY:
 MAX ATTEMPTS EXCEEDED
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK PASSED 07:50
 BLANK TEST 0.000 07:50
 VERIFIED 07:51
 INTERNAL STANDARD 0.079 07:51
 EXTERNAL STANDARD 0.000 07:52
 BLANK TEST XXX 07:52
 SUBJECT SAMPLE

Maximum Attempts Exceeded

KS

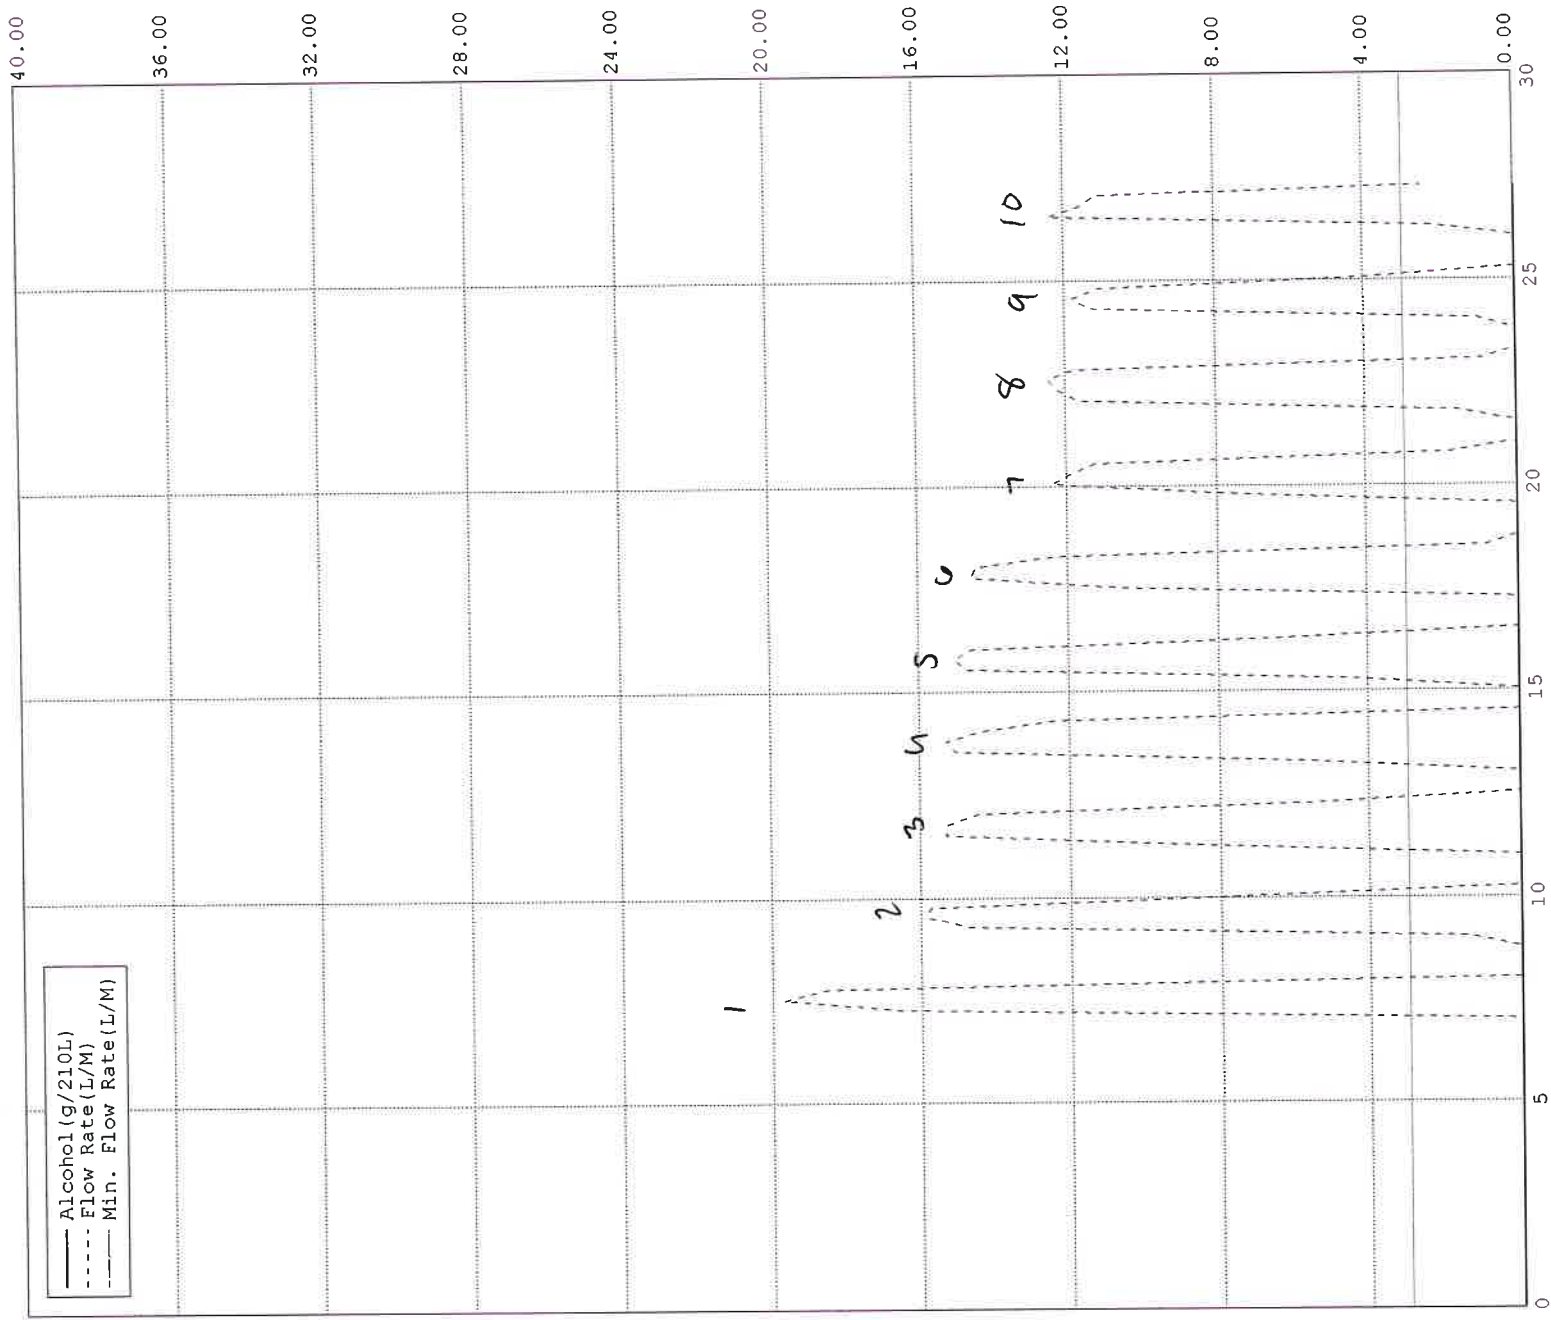

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 07:58:16

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

Lot # A69310901
Exp 4/17/25
LS 6/18/24

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK PASSED 07:59
BLANK TEST 0.000 07:59
INTERNAL STANDARD VERIFIED 07:59
EXTERNAL STANDARD 0.079 07:59
BLANK TEST 0.000 08:00
SUBJECT SAMPLE INVALID 08:01

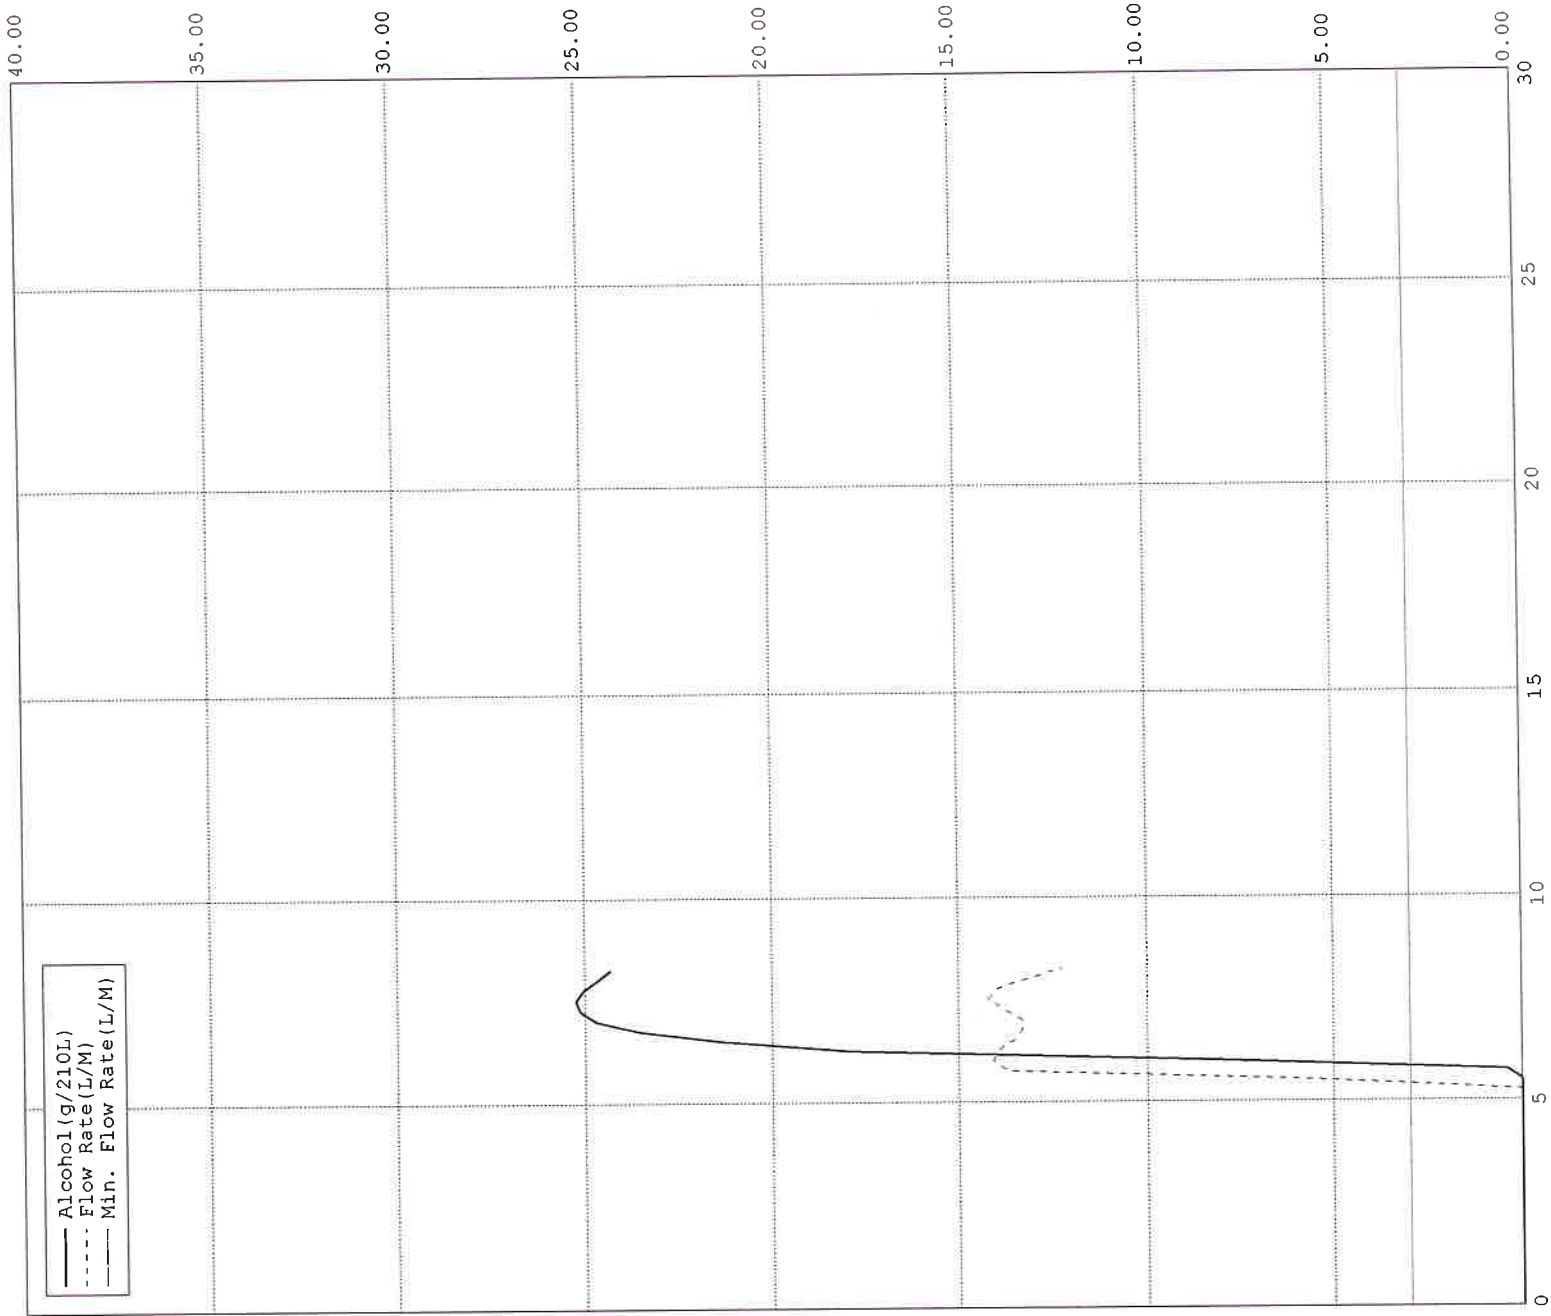

15

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100349

Date: 06/13/2024
Time: 08:04:13

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

*Lot # AG310901
Exp 4/19/25
KS 6/18/24*


DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK PASSED 08:05
BLANK TEST 0.000 08:05
INTERNAL STANDARD VERIFIED 08:05
EXTERNAL STANDARD 0.080 08:05
BLANK TEST 0.000 08:06

RFI DETECTED

KS

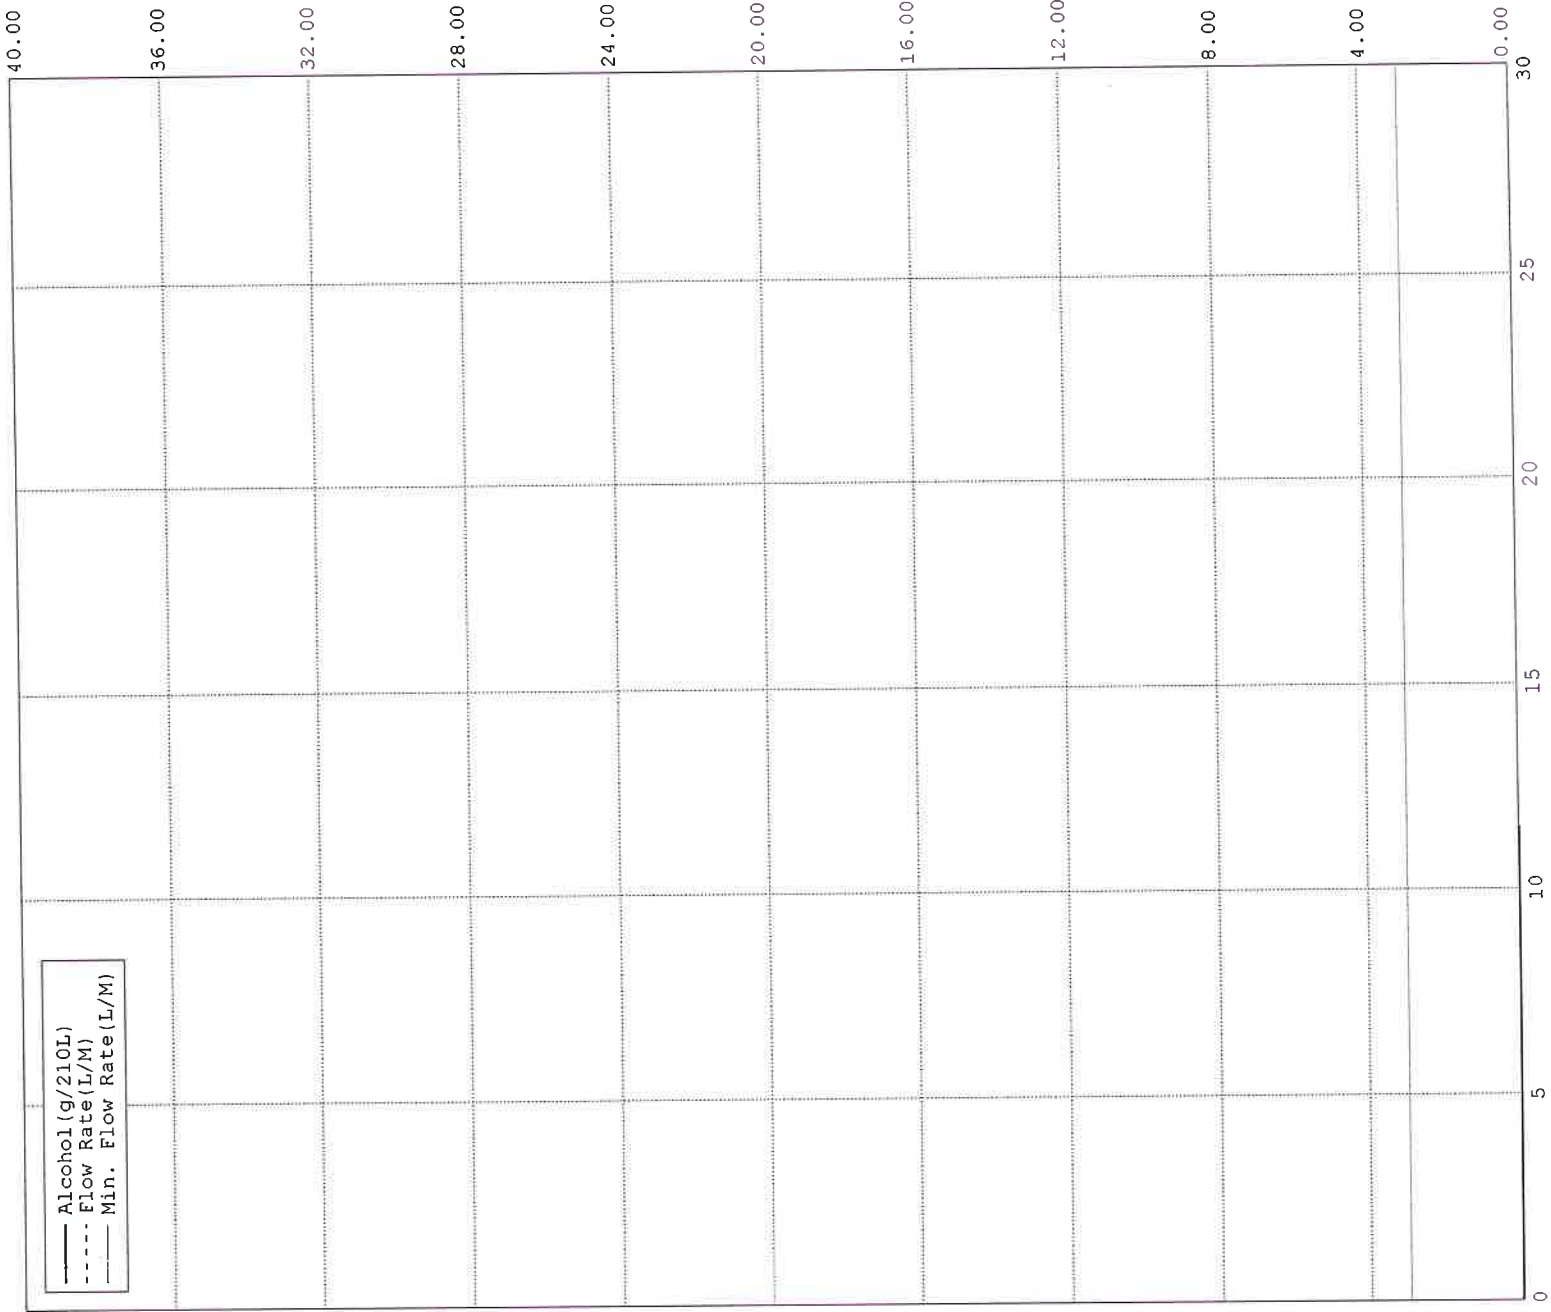

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 08:33:59

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
ACETONE

CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK	PASSED	08:35
BLANK TEST	0.000	08:35
INTERNAL STANDARD	VERIFIED	08:35
xq = 0.078 (0.56%)		
EXTERNAL STANDARD	0.079	08:35
x[1] = 0.0794 (0.0000) (0.0018)		
BLANK TEST	0.000	08:36
SUBJECT SAMPLE	XXX	08:37
x[1] = 0.1044 (-0.0156) (0.0025)		


Interference Detected

Filter 2 ave → -0.0005

Filter 3 ave → 0.0017

KS 6/13/24

KS

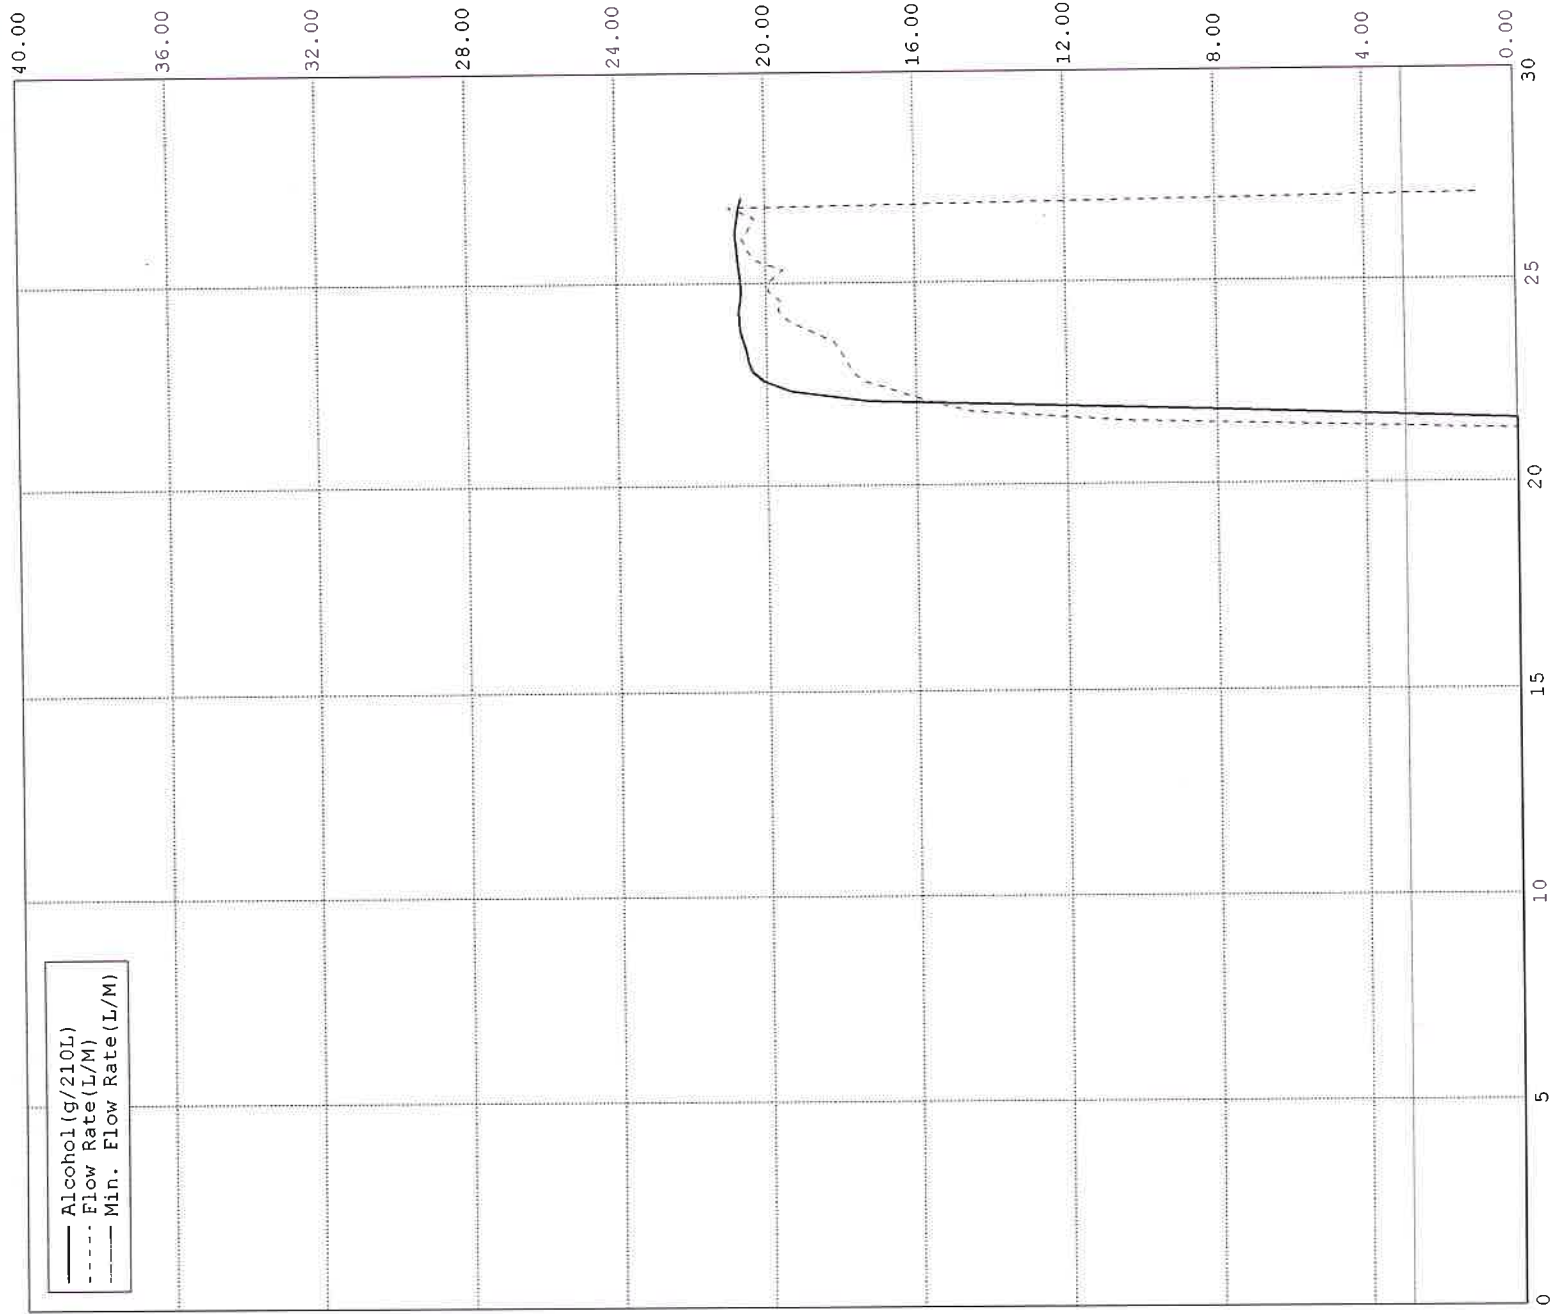

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 08:21:26

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
IPA
Lot # A6310901
Exp 9/19/25
ICS 6/18/24


CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK	PASSED	08:22
BLANK TEST	0.000	08:22
INTERNAL STANDARD	VERIFIED	08:22
Xq = 0.078 (0.22%)		
EXTERNAL STANDARD	0.078	08:22
X[1] = 0.0782 (-0.0010)	(0.0019)	
BLANK TEST	0.000	08:23
SUBJECT SAMPLE	XXX	08:25
X[1] = 0.1098 (-0.0236)	(0.0020)	

Interference Detected

KS

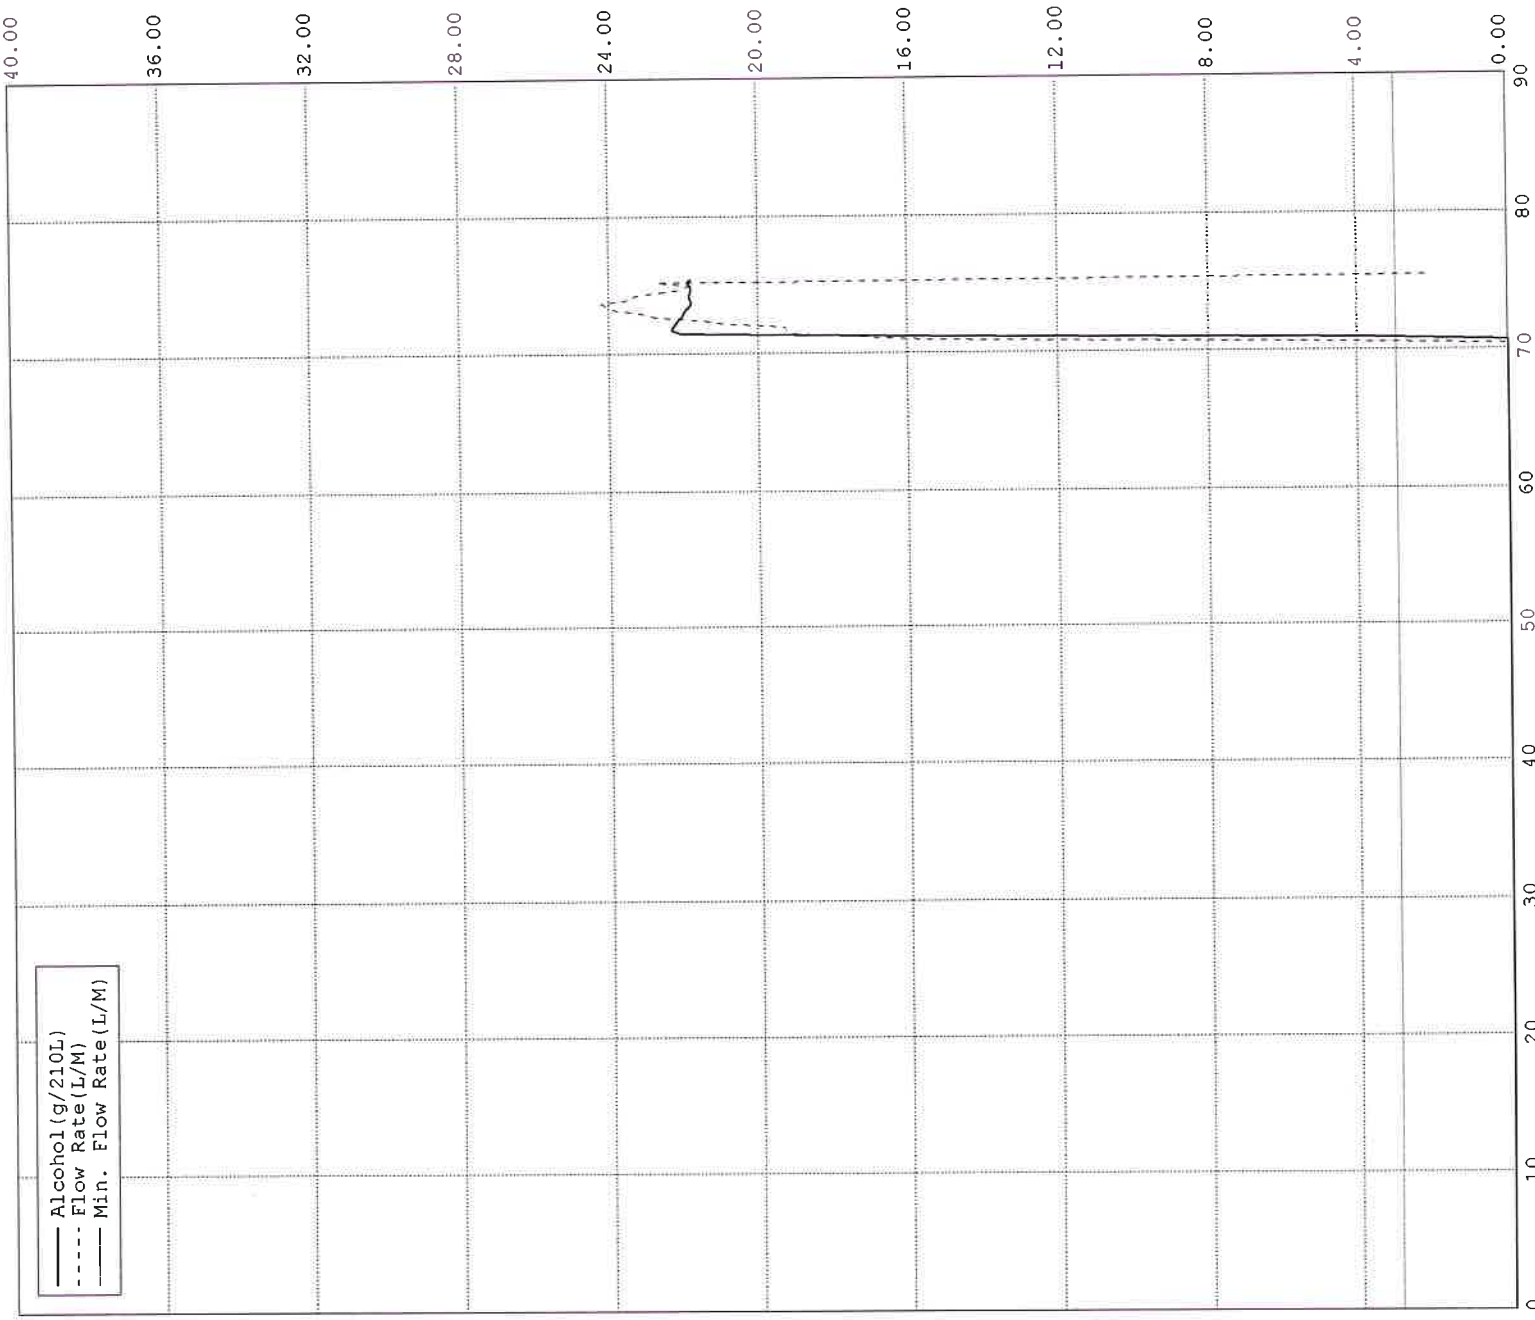

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100349

Date: 06/13/2024
Time: 08:27:14

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME: *Lot # A0310901*
KAIJA SWISHER *Exp 4/19/25*
OPERATOR'S #: 10746 *ICS 6/18/24*

DEPT/AGENCY:
NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080

DIAGNOSTIC CHECK	PASSED	08:28
BLANK TEST	0.000	08:28
INTERNAL STANDARD	VERIFIED	08:28
Xq = 0.078 (0.78%)	0.079	08:28
EXTERNAL STANDARD	(0.0017)	08:29
BLANK TEST	0.000	08:30
SUBJECT SAMPLE (Vol=1.60L)	0.089	08:30
X[1] = 0.0898 (-0.0001)	(0.0007)	08:31
BLANK TEST	0.000	08:31
EXTERNAL STANDARD	0.079	08:31
X[1] = 0.0789 (-0.0001)	(0.0012)	08:32
BLANK TEST	0.000	08:32

FS

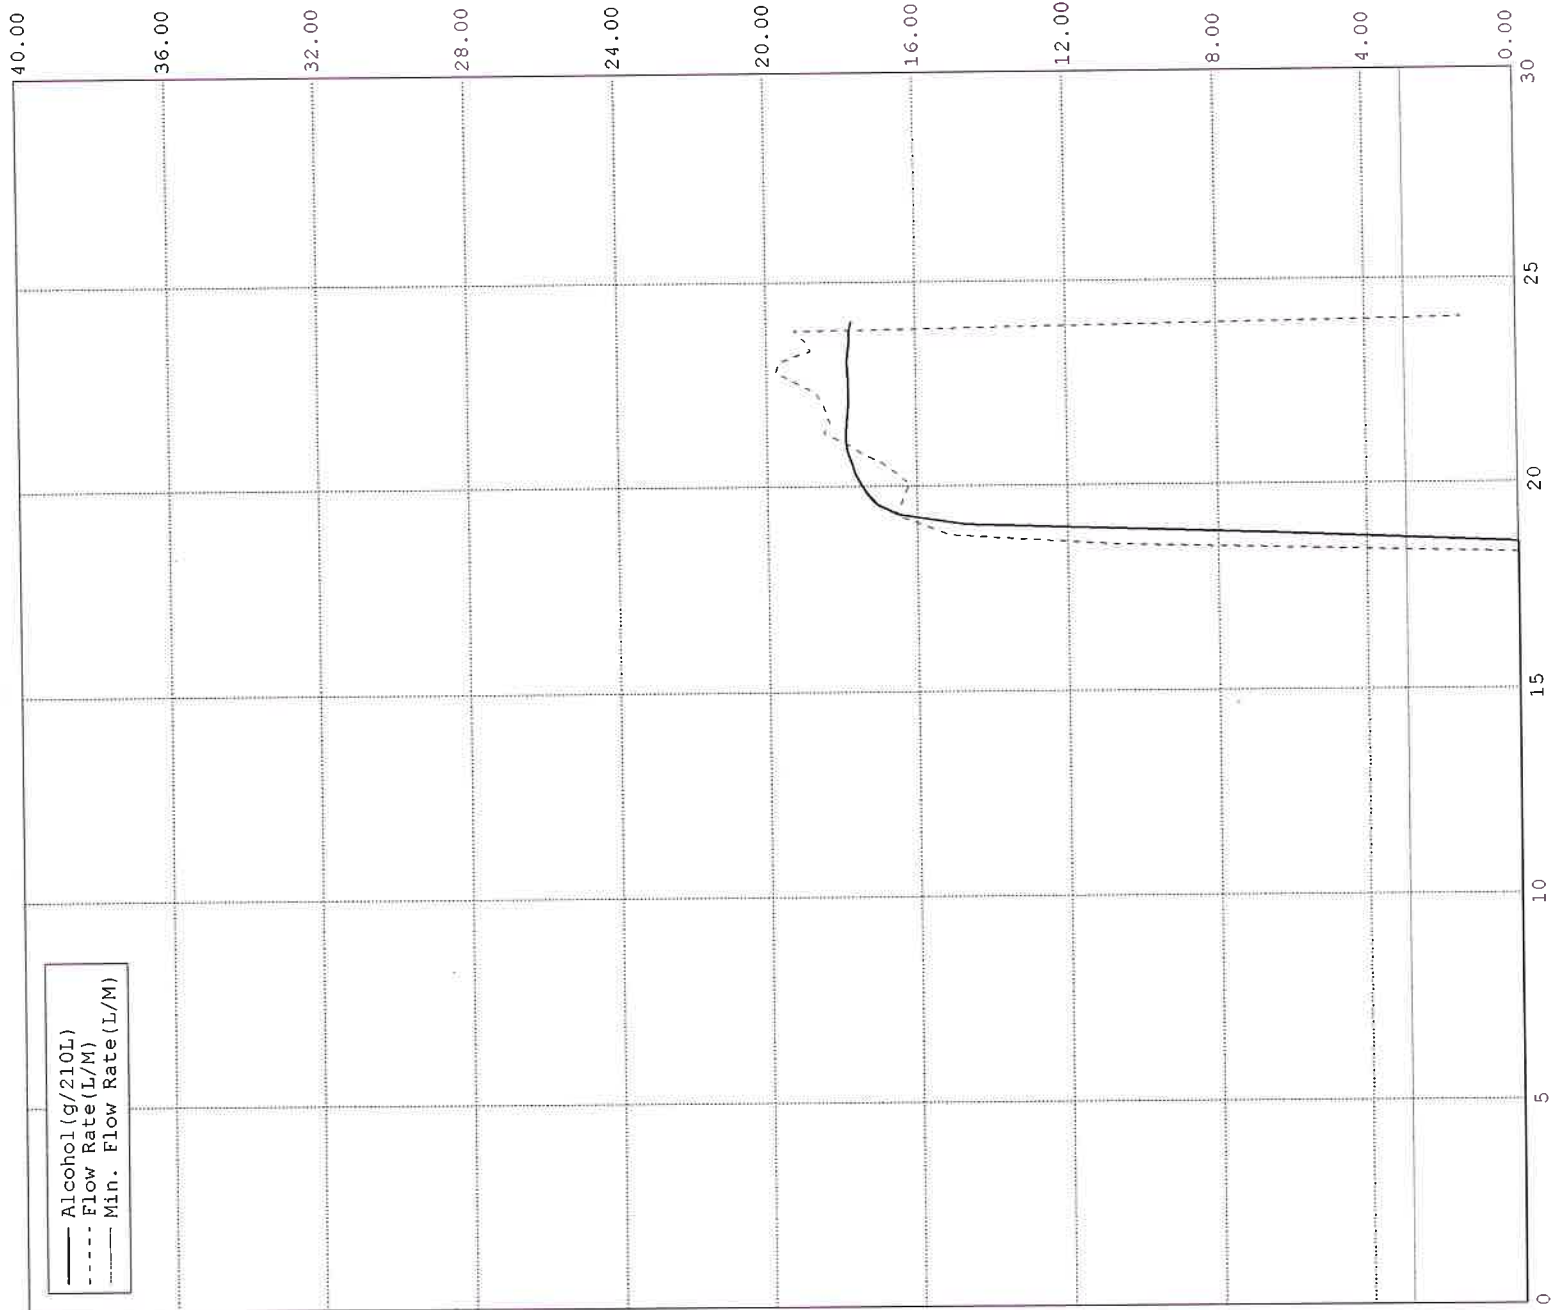

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100349

Date: 06/13/2024
 Time: 08:54:03

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

*Lot # AG810901
 Exp 4/19/25
 KS 6/18/24*

DEPT/AGENCY:
 NON DRINKING SUBJECT TEST
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.82: 0.080

DIAGNOSTIC CHECK	PASSED	08:55
BLANK TEST	0.000	08:55
INTERNAL STANDARD	VERIFIED	08:55
EXTERNAL STANDARD	0.080	08:55
BLANK TEST	0.000	08:56
SUBJECT SAMPLE (Vol=2.07L)	0.000	08:56
BLANK TEST	0.000	08:57
EXTERNAL STANDARD	0.080	08:57
BLANK TEST	0.000	08:58

KS

