



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100418

**Report Issue Date:** 09/05/2024  
**Date Received:** 2024-08-27  
**Condition of Item:** No apparent damage

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG408002	0.020	0.019	0.019	0.019	0.019	0.019	0.019
0.080	0.078	AG335202	0.077	0.077	0.077	0.078	0.077	0.077	0.077
0.300	0.294	AG327804	0.293	0.293	0.293	0.293	0.293	0.293	0.293

As Found - Evaluation Analyst: Kaija Swisher  
 As Found Conditions - Barometric Pressure (inHg): 29.59 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.5 Relative Humidity (%): 40  
 As-Found Lab Activity Date Range: 08/27/2024 - 08/27/2024

Double check valve not secured to wall. Repair recommended. Replaced O-ring.

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002	
0.040	0.040	AG407908	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003	
0.080	0.079	AG335202	0.079	0.079	0.079	0.079	0.079	0.079	+/- 0.004	
0.100	0.099	AG333401	0.100	0.100	0.100	0.100	0.100	0.100	+/- 0.004	
0.150	0.149	AG332004	0.147	0.147	0.146	0.147	0.147	0.147	+/- 0.006	
0.300	0.298	AG327804	0.299	0.298	0.299	0.299	0.299	0.299	+/- 0.012	

As Left Conditions - Barometric Pressure (inHg): 29.70 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.4 Relative Humidity (%): 45  
 As-Left Lab Activity Date Range: 09/03/2024 - 09/03/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Carlie Glaister on 09/03/2024

[carlie.glaister@alaska.gov](mailto:carlie.glaister@alaska.gov)

Technically and administratively reviewed by Derek Walton on 09/05/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100418 Analyst or Technician Name: Carlie Glaister

DataMaster DMT Calibration Start Date: 9/3/2024

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 230307229  
Calibration Due Date: 5/2/2025
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.70 Temperature(C) 21.4 Relative Humidity(%) 45  
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
  - 1. Acetone Reagent Lot Number: 2024673/MNC Expiration Date: 10/31/2024  
Simulator S/N: DR4178 Thermometer Verification Performed?
  - 2. Isopropanol Reagent Lot Number: 2024073/MNC Expiration Date: 10/31/2024  
Simulator S/N: DR6267 Thermometer Verification Performed?
  - 3. Negative (Ethanol Only) Lot Number: 23TP41233 Expiration Date: 9/20/25  
Simulator S/N: DR4163 Thermometer Verification Performed?
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

Calibrated External Thermometer S/N: 230631106  
Calibration Due Date: 9/19/2025

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 9/3/2025  
Data Interpretation Date (Technician): NA (if applicable)  
Data Interpretation Date (Analyst): 9/3/2024 OLG

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100418  
-----

Date: 09/03/2024  
Time: 11:59:41

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 48.1°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.85 V PASSED  
(1.12 V - 2.60 V)  
Cooler Voltage = 1.74 V PASSED  
(1.12 V - 2.60 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 525 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.9 in

PUMP INFO

Flow Rate = 4.885 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED

Xq = 0.065 1.57% (0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100418  
-----

Date: 09/03/2024  
Time: 12:04 PM

Temperatures (°C)  
Sample Cell: 49.0°C  
Breath Tube: 47.5°C

Current Barometer 29.7 in  
Volume (Ltr) 1.57

Settings  
Lamp: 1.85 V  
Bias: 80 V  
Cooler: 1.73 V  
Chopper: 524 Hz

Voltages (V)  
Flow: 1.07 V  
Detector: 0.096 V

CALIBRATION FACTORS


-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100418  
-----

Date: 08/12/2020  
Time: 11:52:02

OPERATOR NAME:  
ST LOUIS INTOX A TECH  
CERTIFICATE #: OU812

Ca = 0.0970  
CAL = 0.969762    0.800 <= CAL < 1.200  
b1 = 0.0003    0.0000 <= b1 < 0.0040  
b2 = 0.0053    0.0010 <= b2 < 0.0100  
b3 = 0.0001    0.0000 <= b3 < 0.0040  
Xq = 0.0660    0.0500 <= Xq < 0.2000  
a21 = 1.176228    1.050 <= a21 < 1.300  
a31 = 0.458989    0.300 <= a31 < 0.800



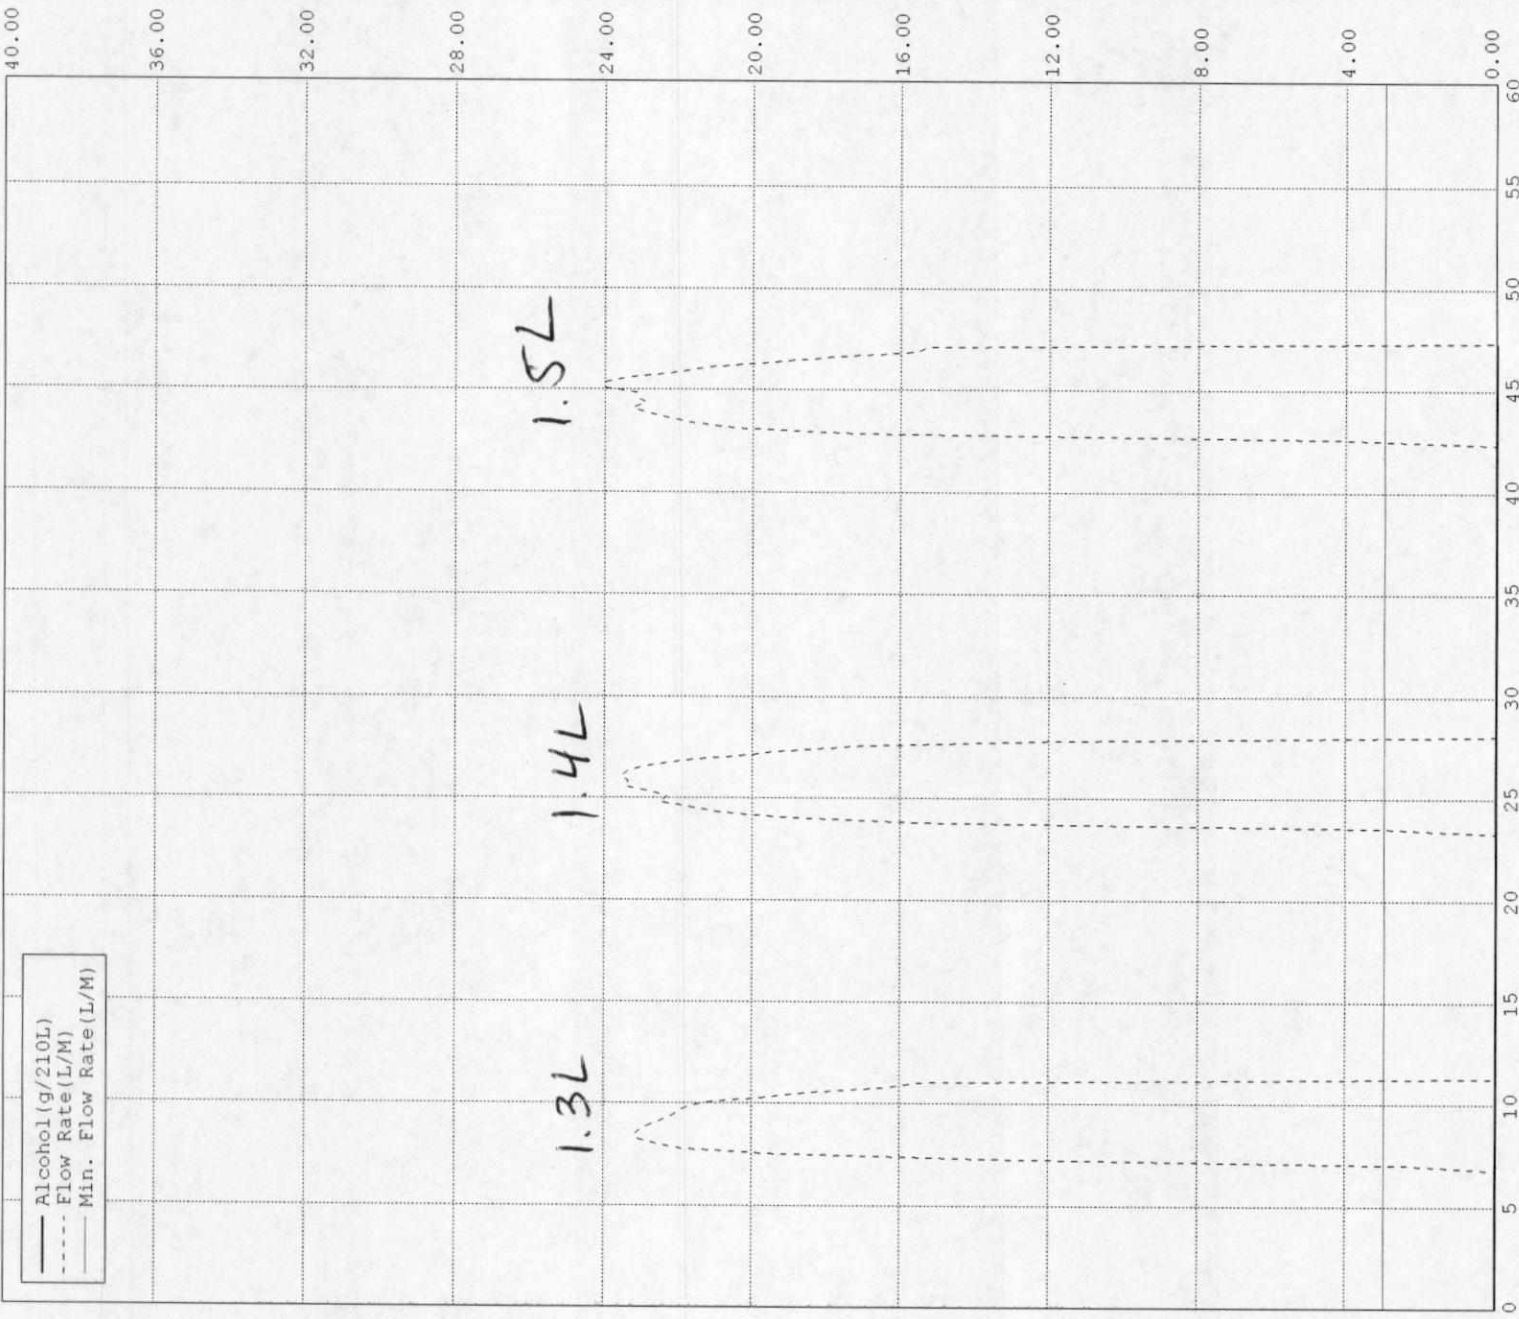

SUBJECT TEST

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100418  
 -----  
 Date: 09/03/2024  
 Time: 12:06:41  
 -----  
 SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX  
 OPERATOR NAME:  
 CHARLIE GLAISTER  
 OPERATOR'S #: 10436  
 DEPT/AGENCY:  
 MINIMUM VOLUME TEST  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST  
 -----  
 EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.69: 0.079  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025  
 -----  
 DIAGNOSTIC CHECK PASSED 12:07  
 BLANK TEST 0.000 12:07  
 INTERNAL STANDARD VERIFIED 12:07  
 EXTERNAL STANDARD 0.079 12:08  
 BLANK TEST 0.000 12:09  
 SUBJECT SAMPLE (Vol=1.60L) 0.000 12:11  
 BLANK TEST 0.000 12:12  
 EXTERNAL STANDARD 0.079 12:12  
 BLANK TEST 0.000 12:13

CKG

LINEARITY CHECK


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100418  
 -----

Date: 09/03/2024  
 Time: 12:17:29

SUPERVISOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.040	0.0400	0.0000
0.079	0.0790	0.0000
0.099	0.1000	0.0000
0.149	0.1468	0.0004
0.298	0.2988	0.0004

SLOPE = 1.001087  
 R<sup>2</sup> = 0.999875

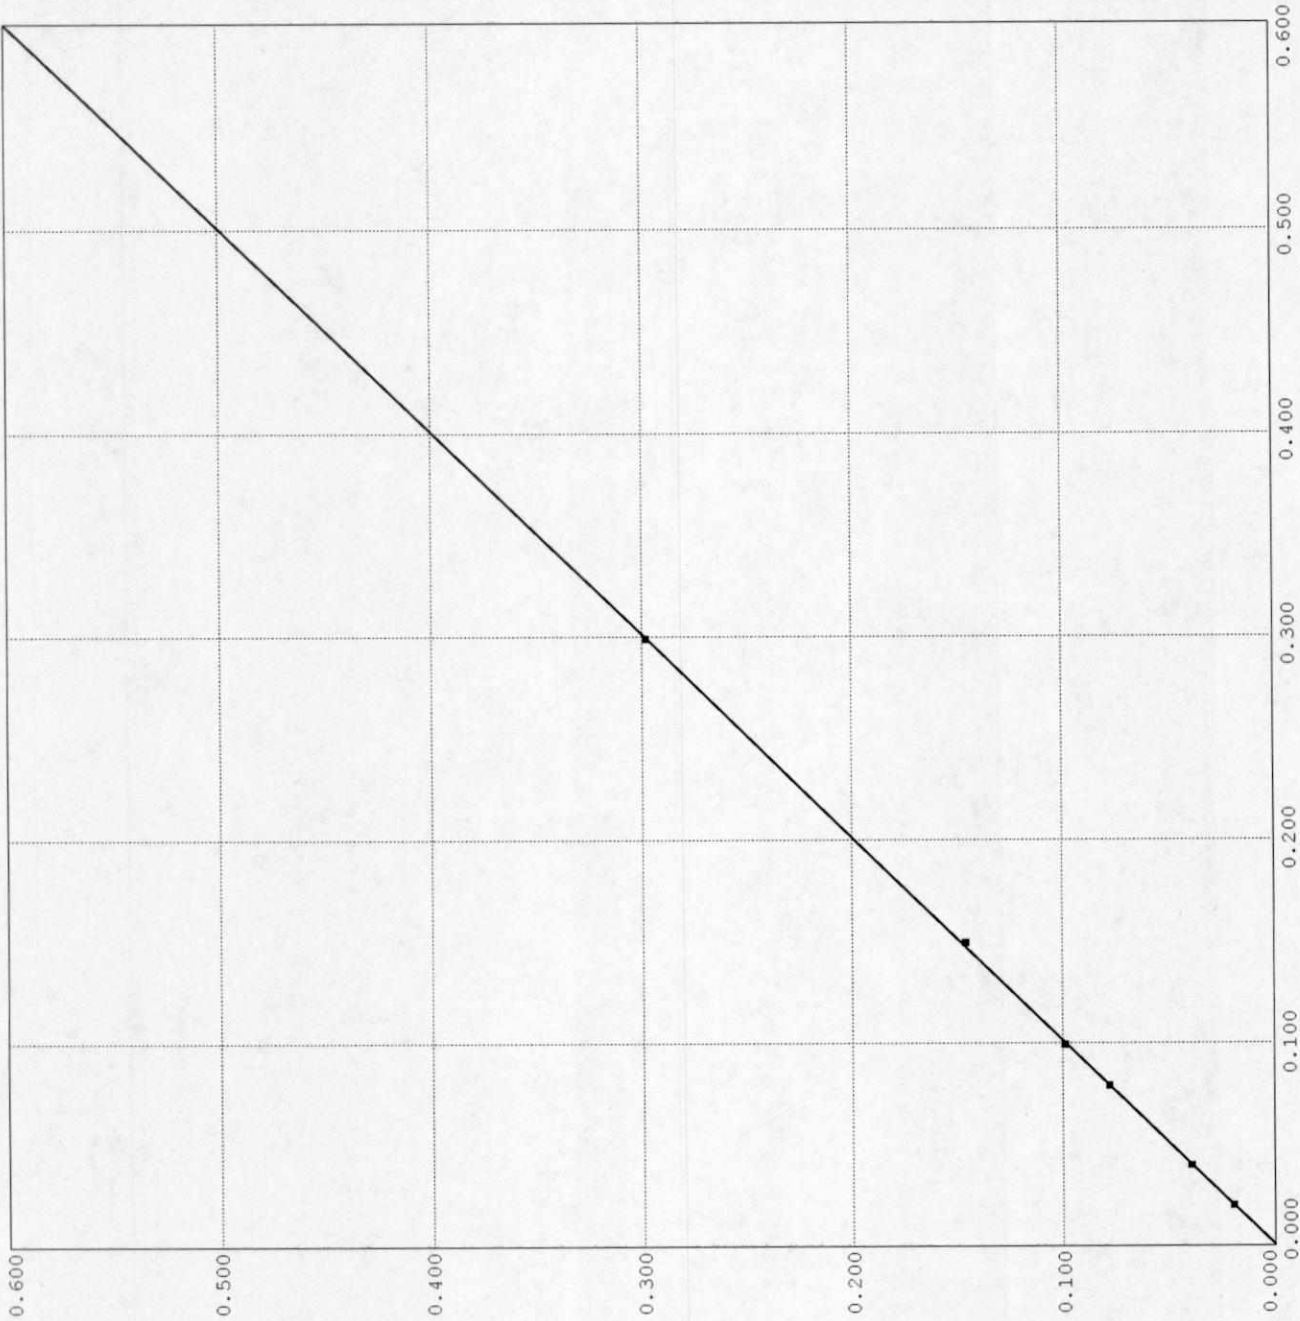

CKG

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100418






Date: 09/03/2024  
 Time: 12:17:31

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.69: 0.020  
 LOT #: AG408002  
 EXPIRATION: 03/20/2026  
 TANK PRESSURE: 898 psi

BLANK TEST	0.000	12:19
INTERNAL STANDARD	VERIFIED	12:19
EXTERNAL STANDARD	0.020	12:19
BLANK TEST	0.000	12:20
EXTERNAL STANDARD	0.020	12:20
BLANK TEST	0.000	12:21
EXTERNAL STANDARD	0.020	12:21
BLANK TEST	0.000	12:22
EXTERNAL STANDARD	0.020	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.020	12:23
BLANK TEST	0.000	12:24

Average = 0.0200  
 Std Dev = 0.0000

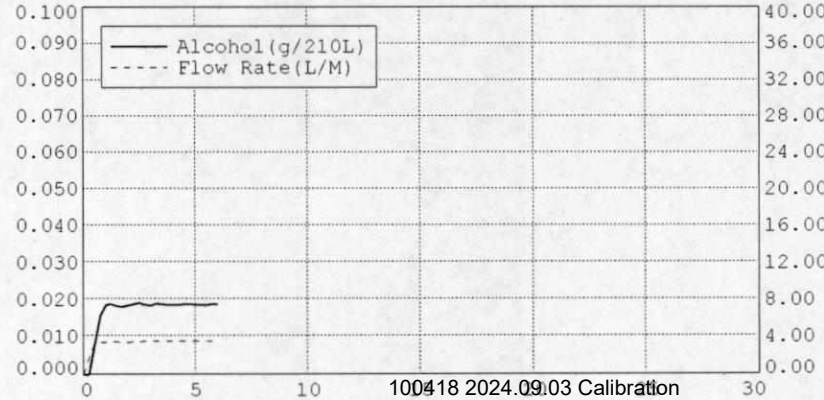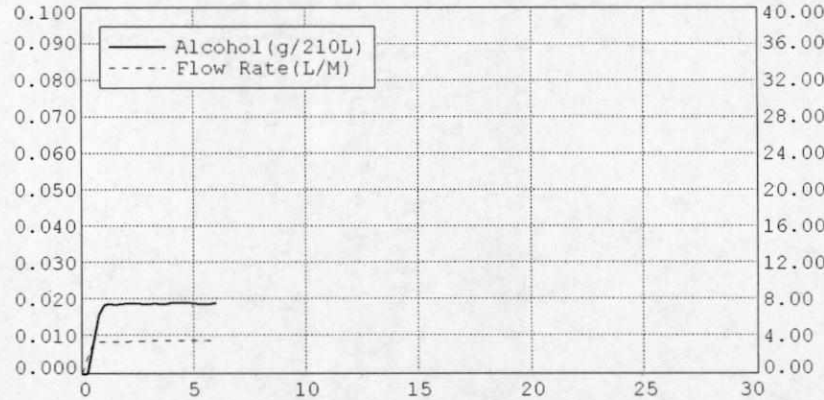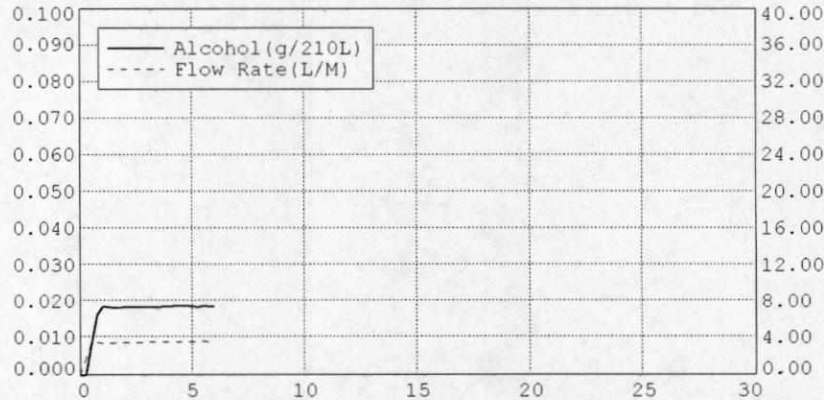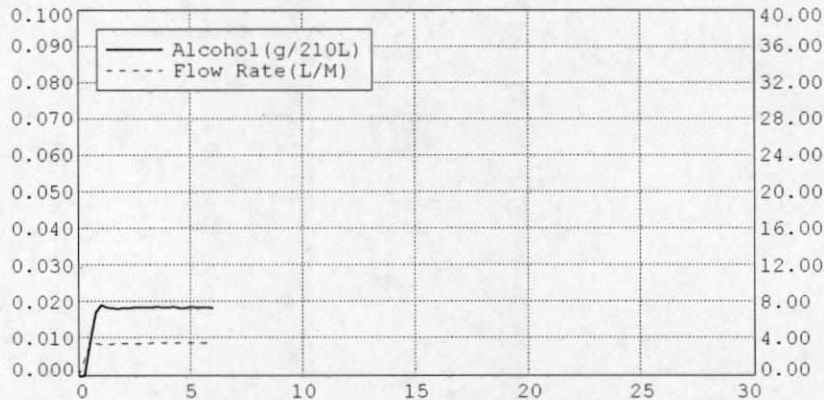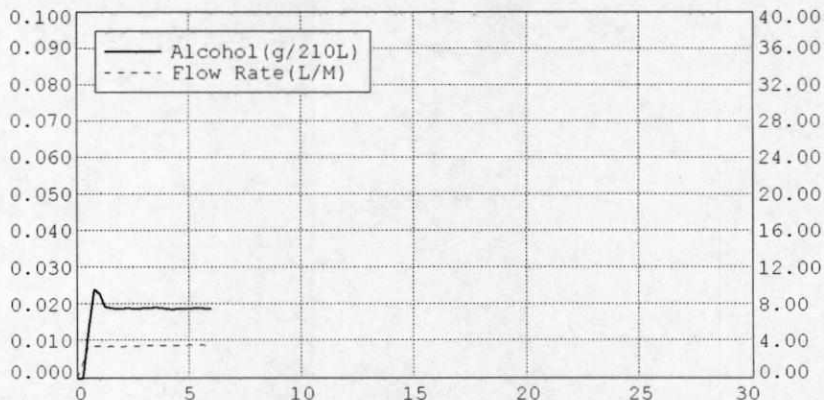



LINEARITY CHECK: Control Test 2






Alaska Department of Public Safety  
DATAMASTER dmt: 100418

Date: 09/03/2024  
Time: 12:26:10

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.040  
TARGET AT 29.70: 0.040  
LOT #: AG407908  
EXPIRATION: 03/19/2026  
TANK PRESSURE: 1097 psi

BLANK TEST	0.000	12:27
INTERNAL STANDARD	VERIFIED	12:27
EXTERNAL STANDARD	0.040	12:27
BLANK TEST	0.000	12:28
EXTERNAL STANDARD	0.040	12:28
BLANK TEST	0.000	12:29
EXTERNAL STANDARD	0.040	12:29
BLANK TEST	0.000	12:30
EXTERNAL STANDARD	0.040	12:30
BLANK TEST	0.000	12:31
EXTERNAL STANDARD	0.040	12:31
BLANK TEST	0.000	12:32

Average = 0.0400  
Std Dev = 0.0000

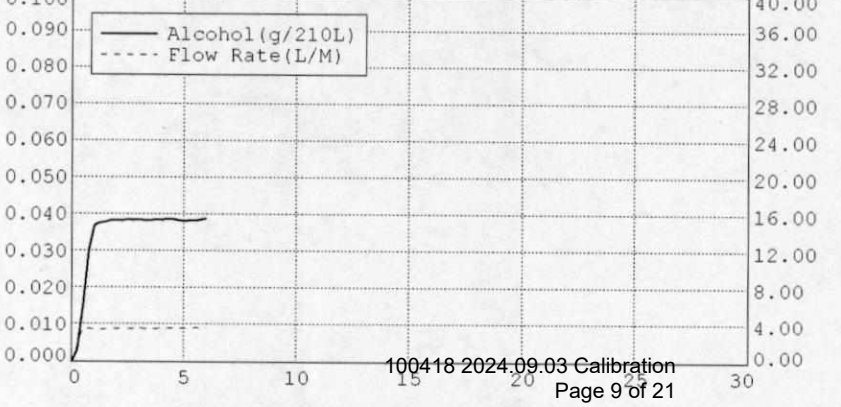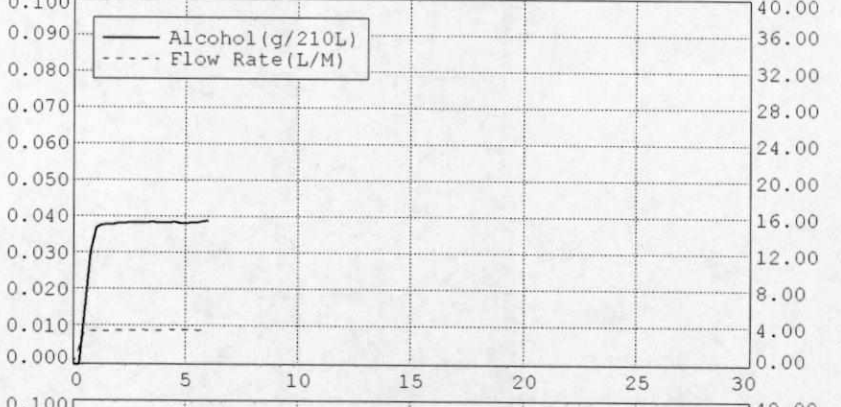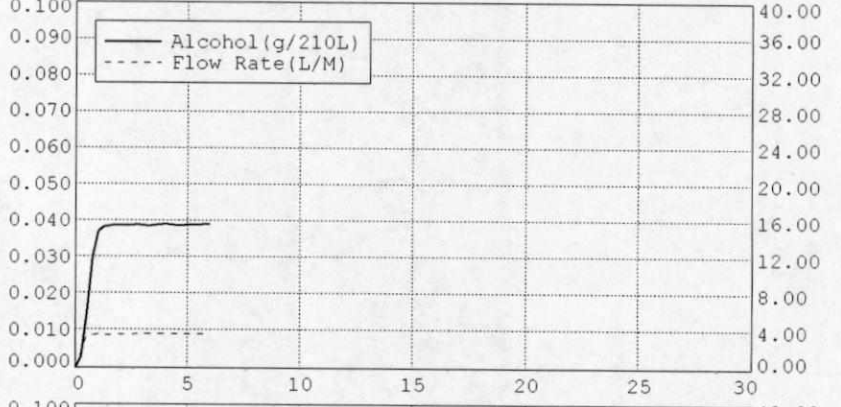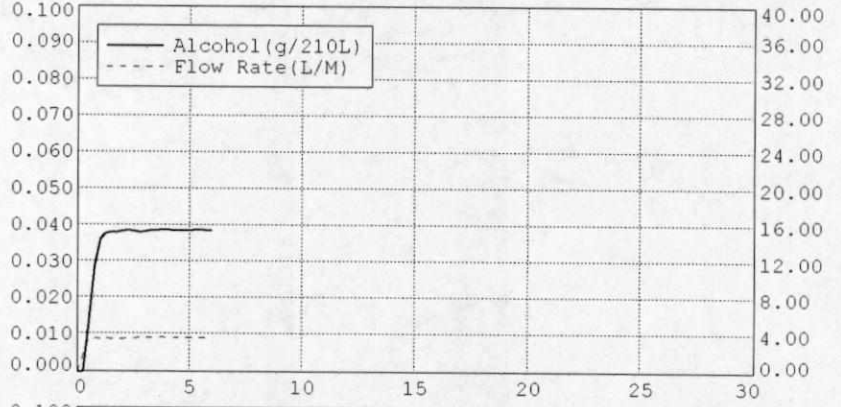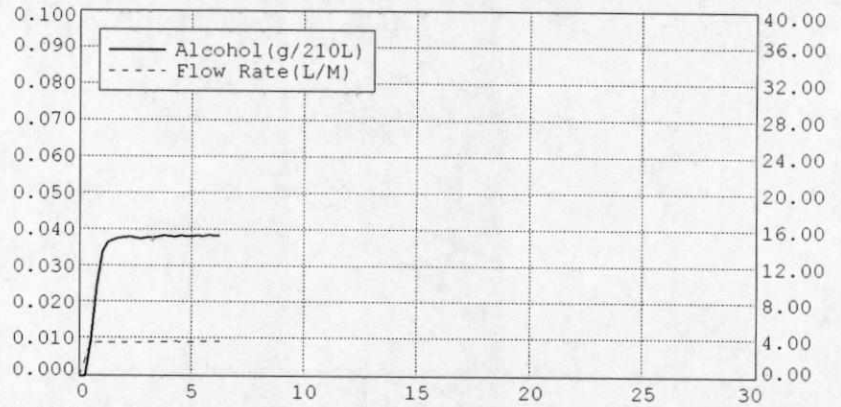

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100418






Date: 09/03/2024  
 Time: 12:33:32

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.69: 0.079  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025  
 TANK PRESSURE: 683 psi

BLANK TEST	0.000	12:34
INTERNAL STANDARD	VERIFIED	12:35
EXTERNAL STANDARD	0.079	12:35
BLANK TEST	0.000	12:36
EXTERNAL STANDARD	0.079	12:36
BLANK TEST	0.000	12:37
EXTERNAL STANDARD	0.079	12:37
BLANK TEST	0.000	12:38
EXTERNAL STANDARD	0.079	12:38
BLANK TEST	0.000	12:39
EXTERNAL STANDARD	0.079	12:39
BLANK TEST	0.000	12:40

Average = 0.0790  
 Std Dev = 0.0000

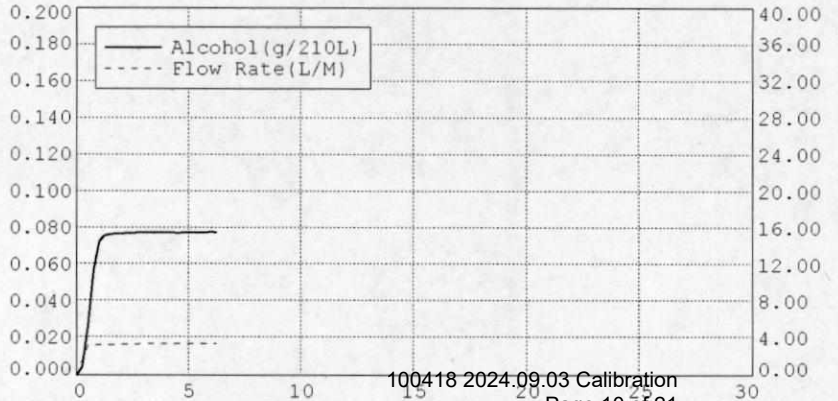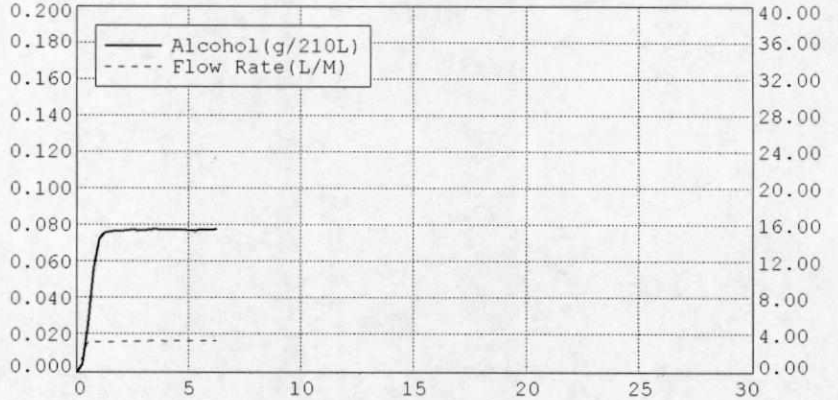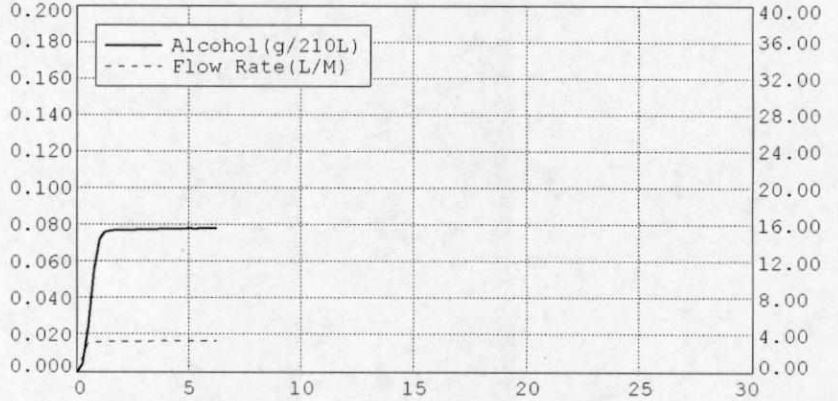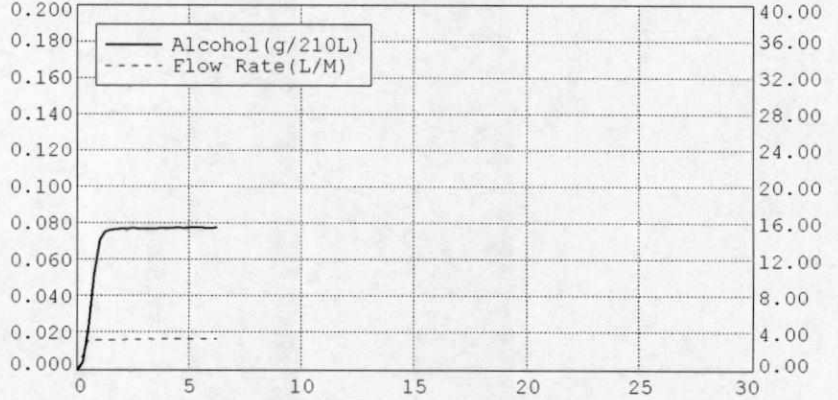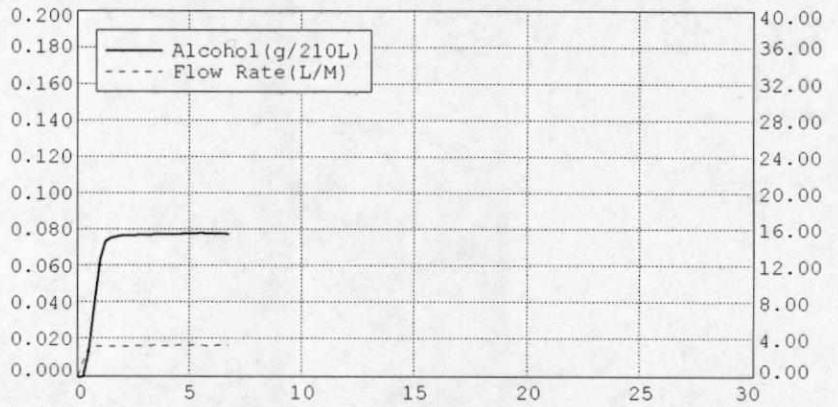

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100418






Date: 09/03/2024  
 Time: 12:42:30

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.70: 0.099  
 LOT #: AG333401  
 EXPIRATION: 11/30/2025  
 TANK PRESSURE: 999 psi

BLANK TEST	0.000	12:43
INTERNAL STANDARD	VERIFIED	12:43
EXTERNAL STANDARD	0.100	12:44
BLANK TEST	0.000	12:45
EXTERNAL STANDARD	0.100	12:45
BLANK TEST	0.000	12:46
EXTERNAL STANDARD	0.100	12:46
BLANK TEST	0.000	12:47
EXTERNAL STANDARD	0.100	12:47
BLANK TEST	0.000	12:48
EXTERNAL STANDARD	0.100	12:48
BLANK TEST	0.000	12:49

Average = 0.1000  
 Std Dev = 0.0000

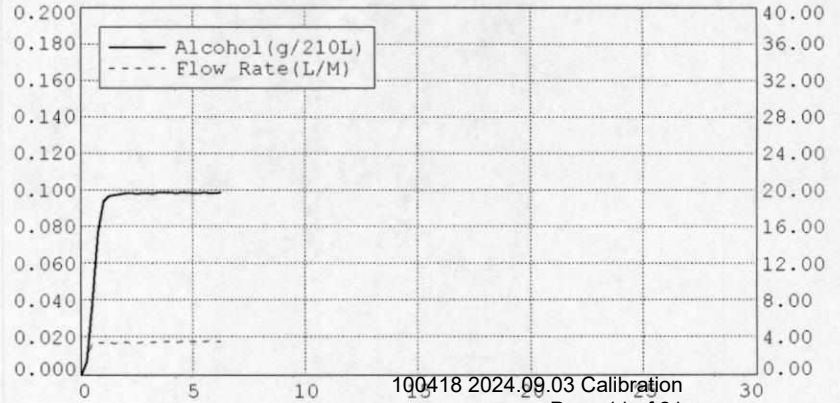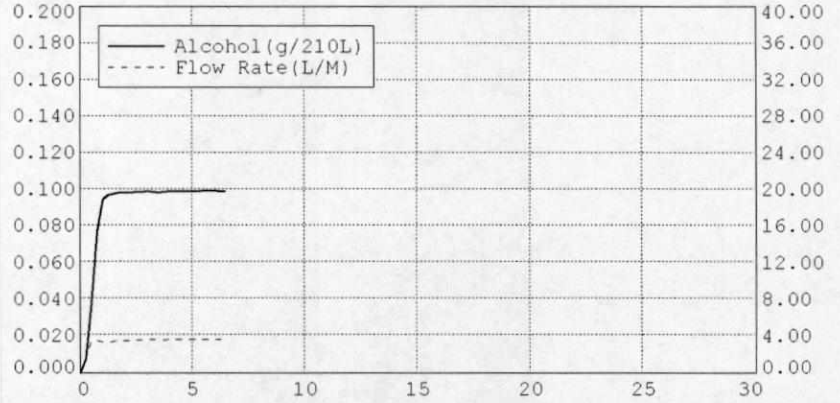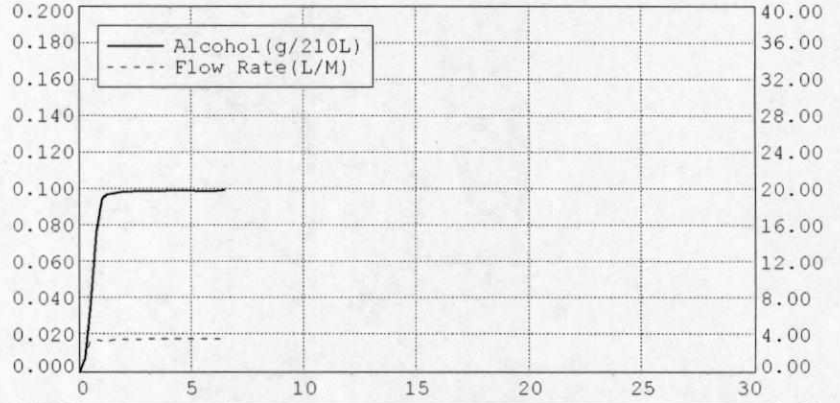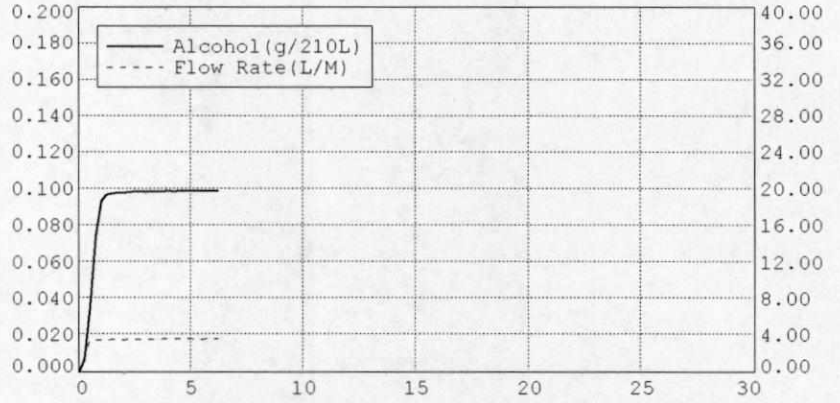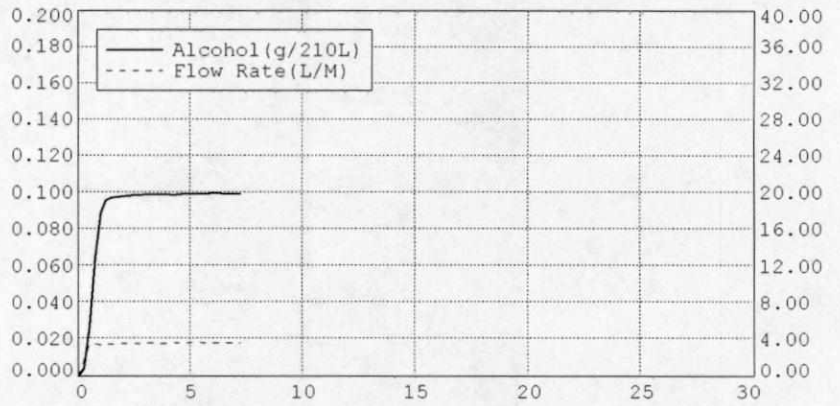



LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100418






Date: 09/03/2024  
 Time: 12:50:18

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.70: 0.149  
 LOT #: AG332004  
 EXPIRATION: 11/16/2025  
 TANK PRESSURE: 622 psi

BLANK TEST	0.000	12:51
INTERNAL STANDARD	VERIFIED	12:51
EXTERNAL STANDARD	0.147	12:51
BLANK TEST	0.000	12:52
EXTERNAL STANDARD	0.147	12:53
BLANK TEST	0.000	12:54
EXTERNAL STANDARD	0.146	12:54
BLANK TEST	0.000	12:55
EXTERNAL STANDARD	0.147	12:55
BLANK TEST	0.000	12:56
EXTERNAL STANDARD	0.147	12:56
BLANK TEST	0.000	12:57

Average = 0.1468  
 Std Dev = 0.0004

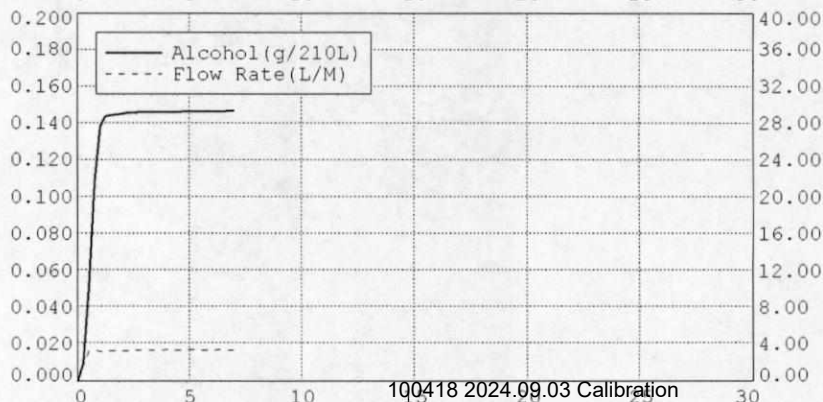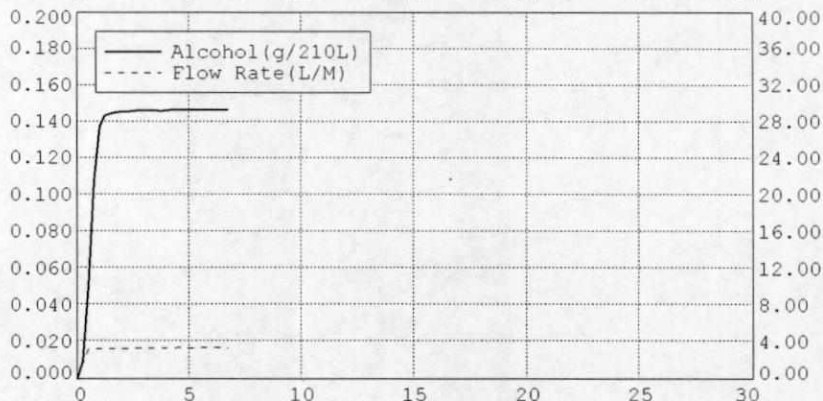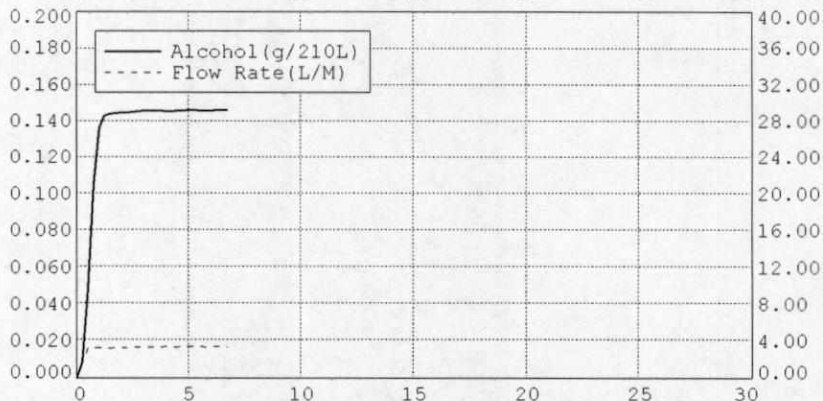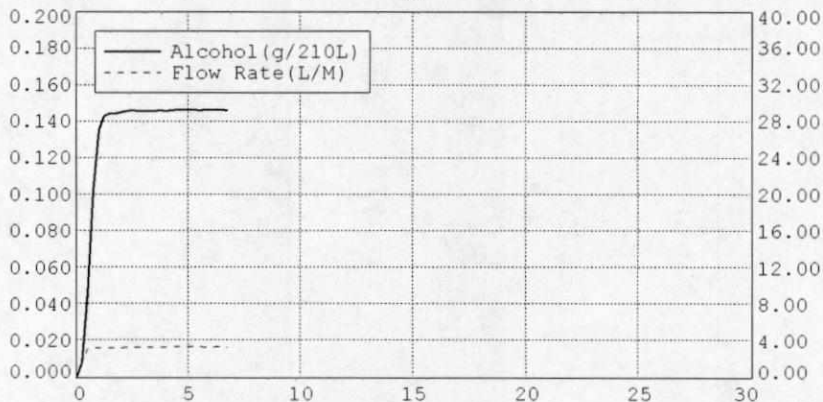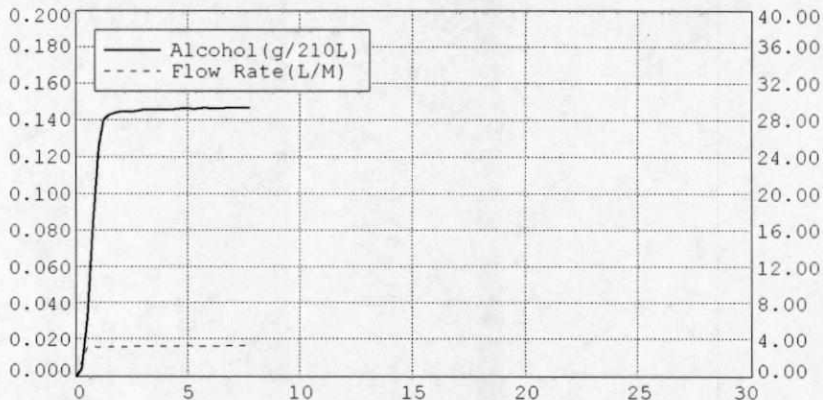



LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100418






Date: 09/03/2024  
 Time: 12:59:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.69: 0.298  
 LOT #: AG327804  
 EXPIRATION: 10/05/2025  
 TANK PRESSURE: 279 psi

BLANK TEST	0.000	13:01
INTERNAL STANDARD	VERIFIED	13:01
EXTERNAL STANDARD	0.299	13:01
BLANK TEST	0.000	13:02
EXTERNAL STANDARD	0.298	13:02
BLANK TEST	0.000	13:03
EXTERNAL STANDARD	0.299	13:03
BLANK TEST	0.000	13:04
EXTERNAL STANDARD	0.299	13:05
BLANK TEST	0.000	13:06
EXTERNAL STANDARD	0.299	13:06
BLANK TEST	0.000	13:07

Average = 0.2988  
 Std Dev = 0.0004

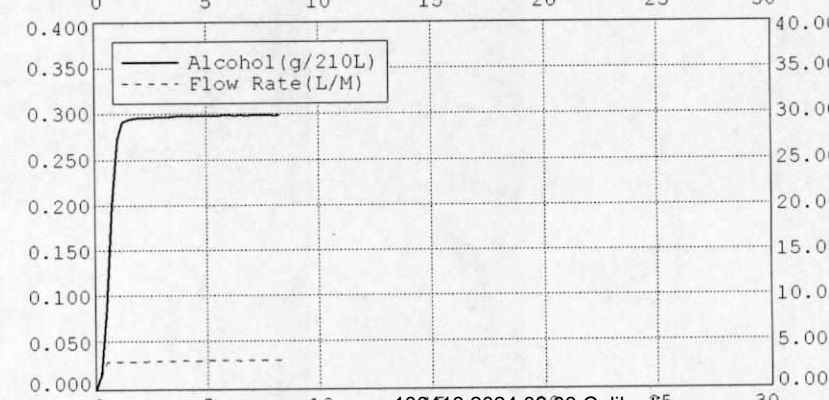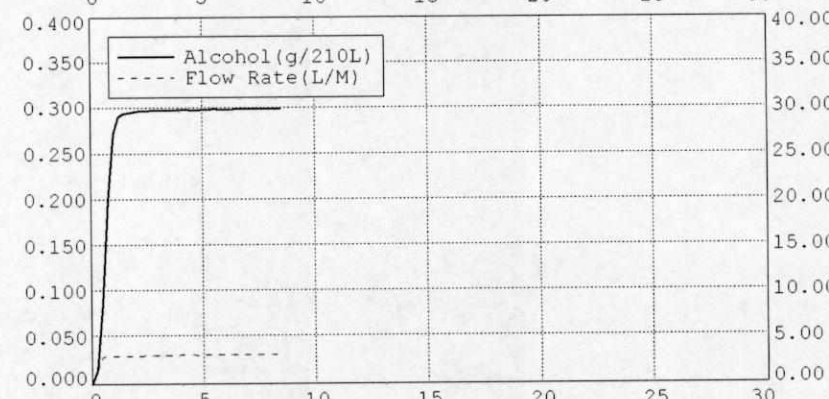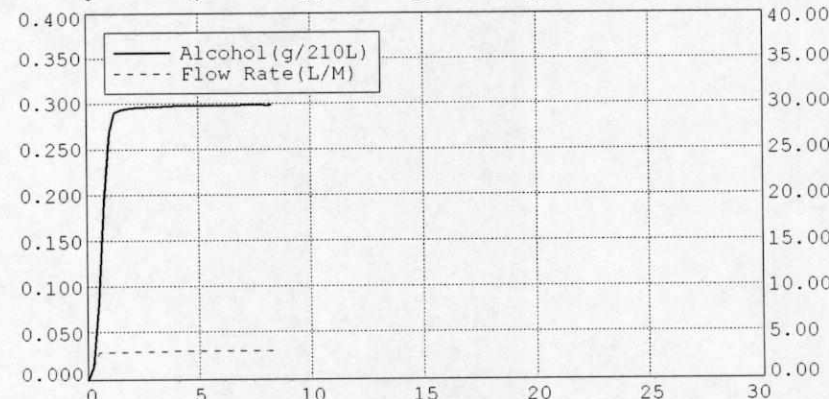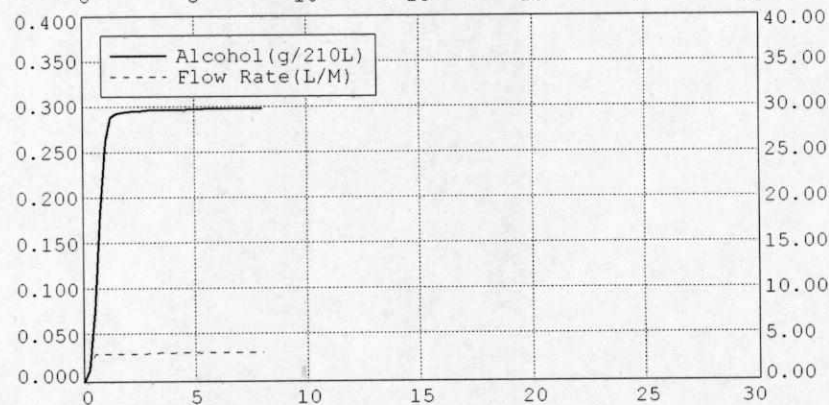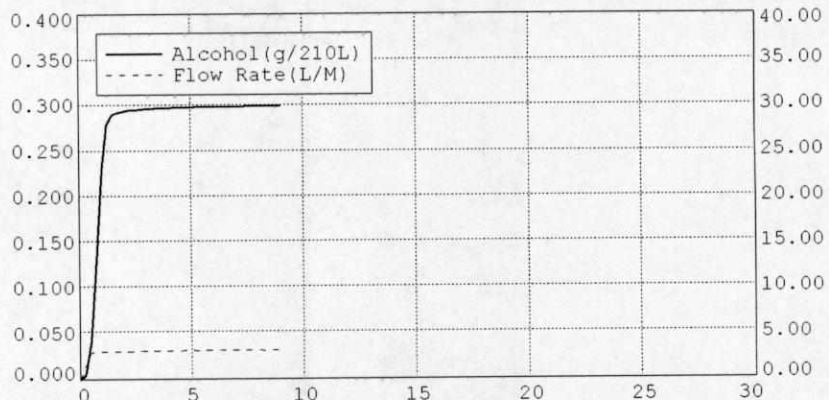

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100418

Date: 09/03/2024  
Time: 13:12:51

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.70: 0.079  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:14
BLANK TEST	0.000	13:14
INTERNAL STANDARD	VERIFIED	13:14
EXTERNAL STANDARD	0.080	13:15
BLANK TEST	0.000	13:15
SUBJECT SAMPLE	INCOMPLETE	13:18

CX6

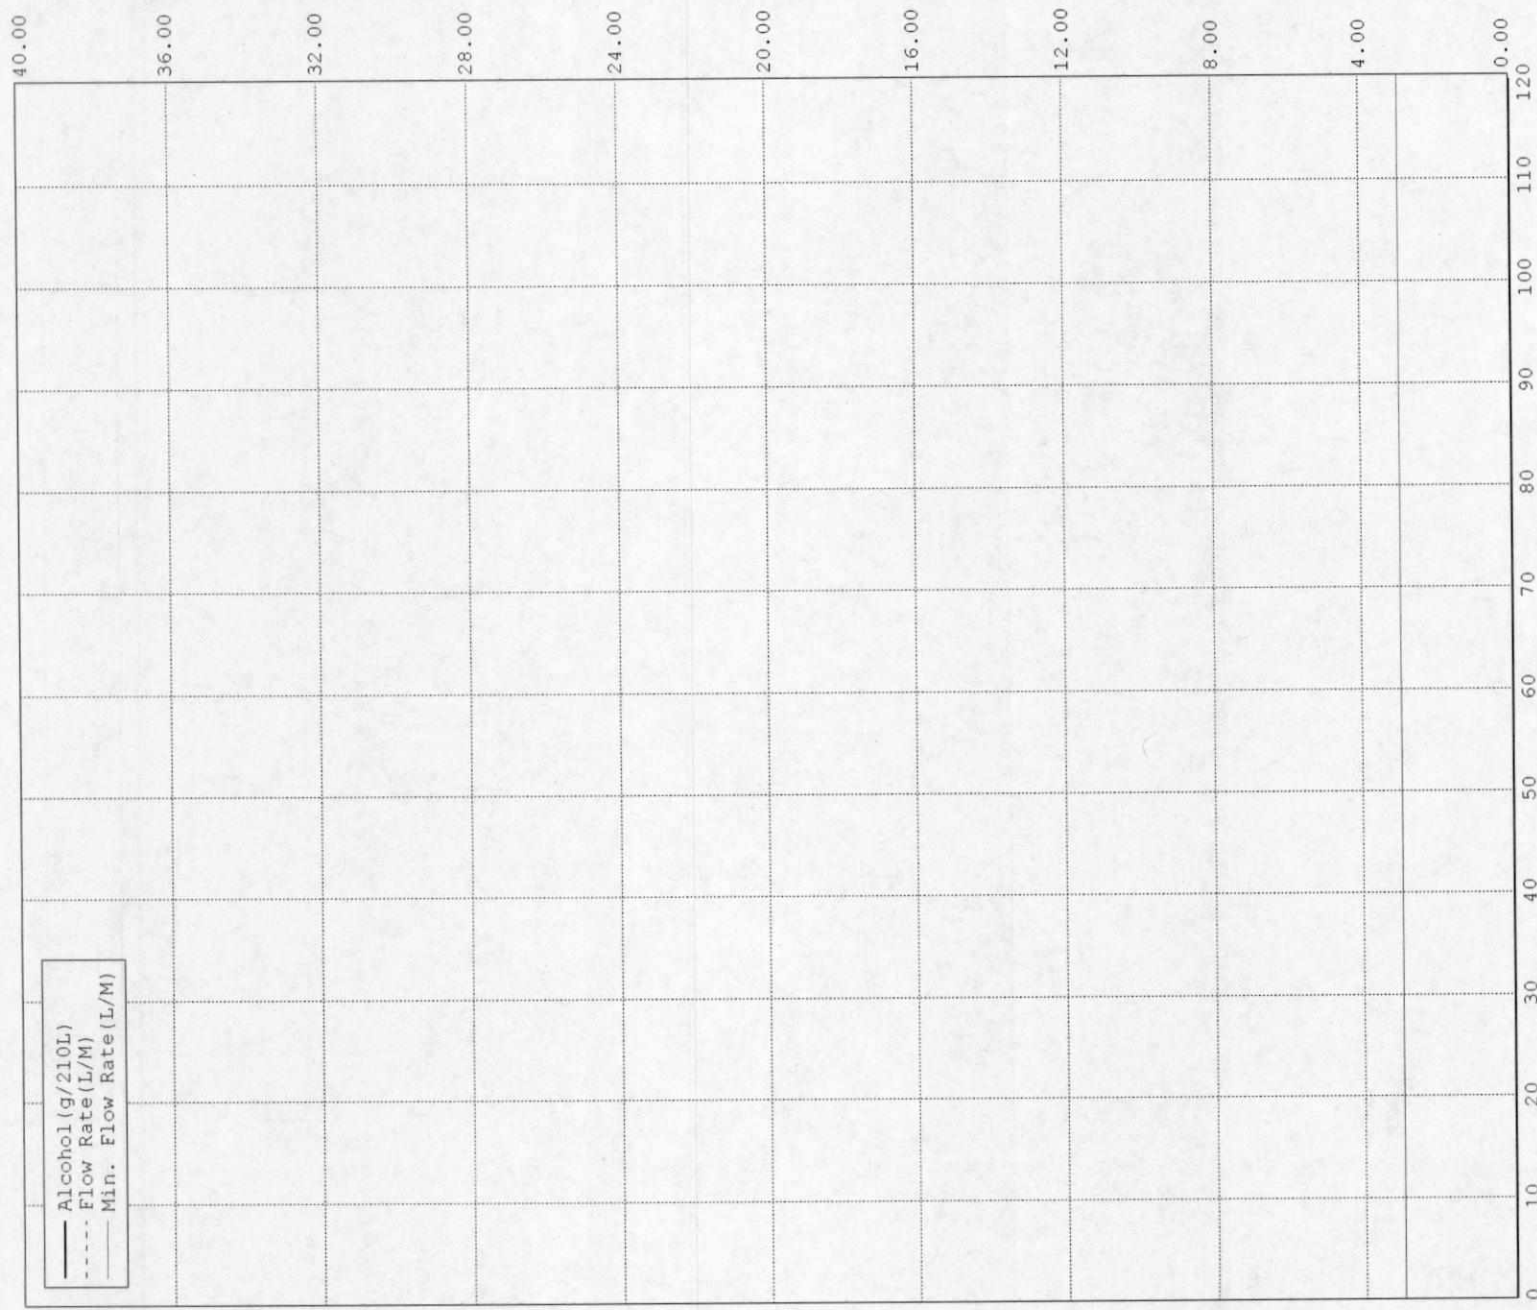

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100418

Date: 09/03/2024  
Time: 13:22:56

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
MAXIMUM ATTEMPTS EXCEEDED  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.70: 0.079  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:23  
BLANK TEST 0.000 13:24  
INTERNAL STANDARD VERIFIED 13:24  
EXTERNAL STANDARD 0.079 13:24  
BLANK TEST 0.000 13:25  
SUBJECT SAMPLE XXX 13:26

Maximum Attempts Exceeded

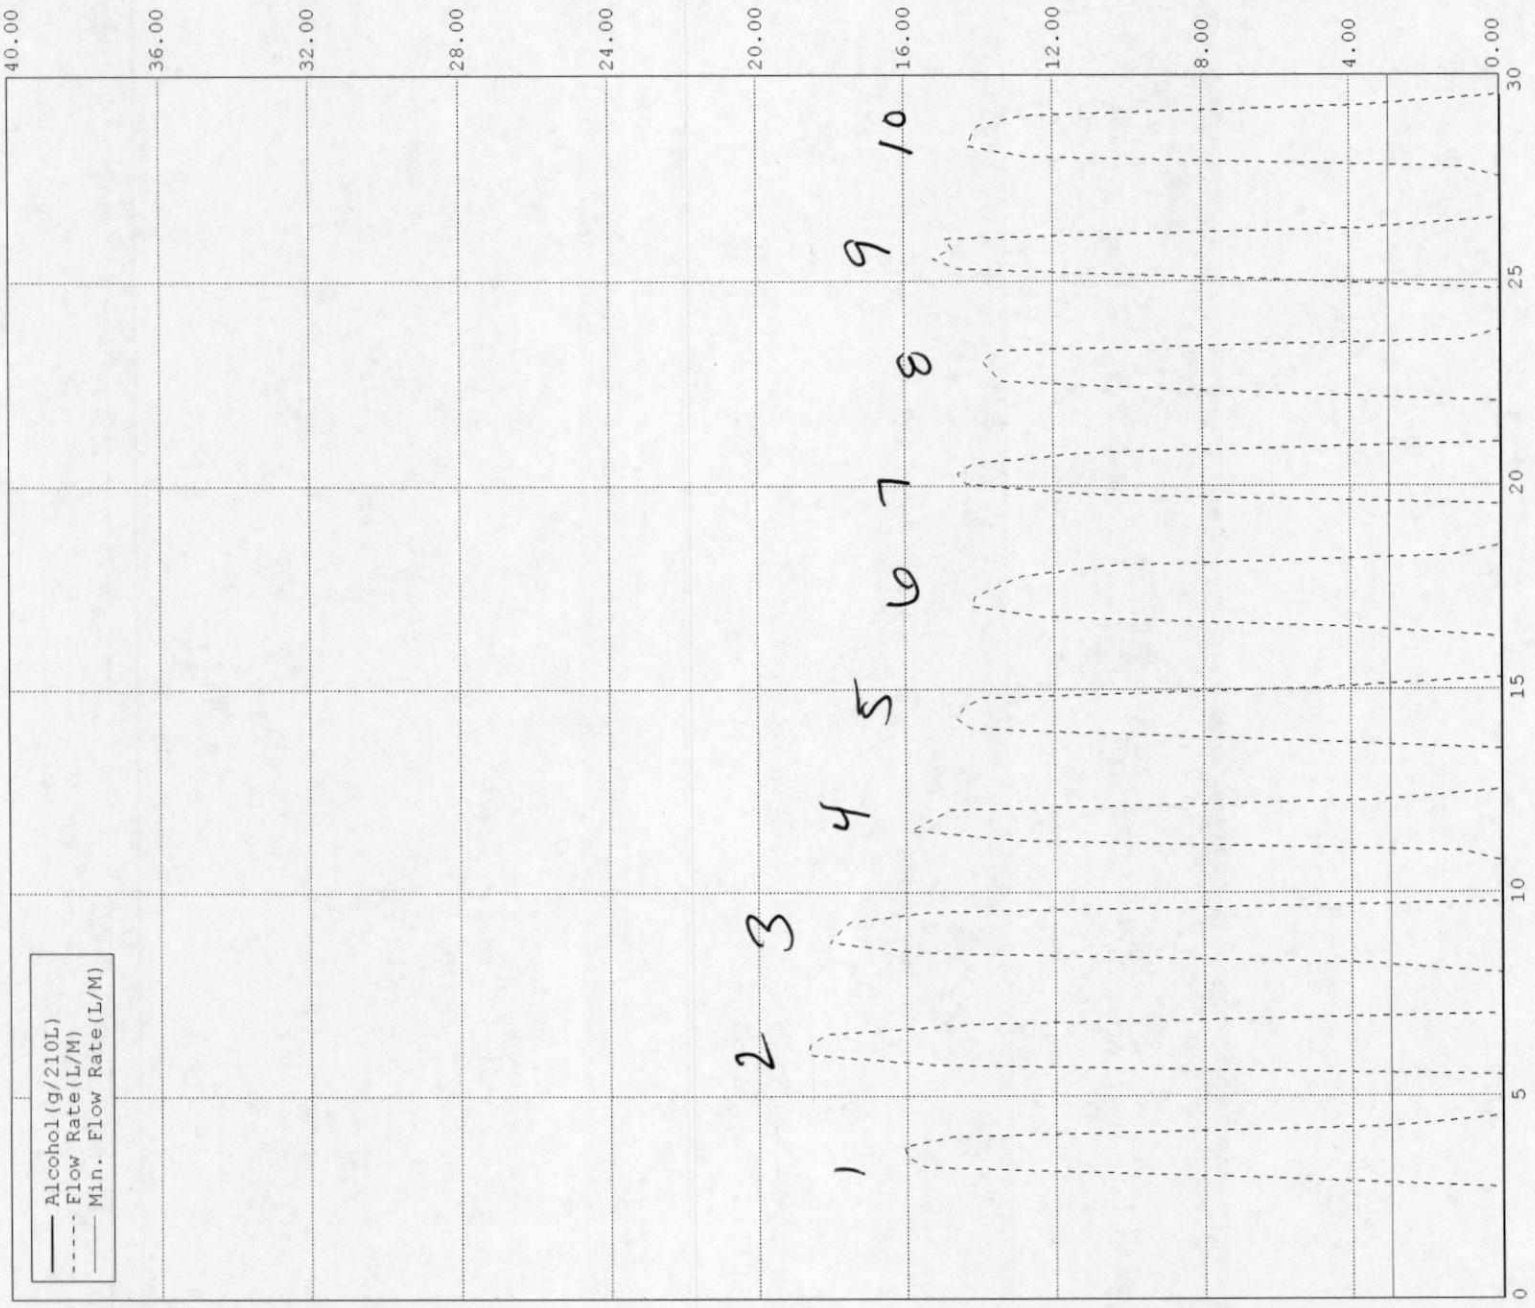

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100418

Date: 09/03/2024  
Time: 13:30:35


SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INVALID  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:31  
BLANK TEST 0.000 13:31  
INTERNAL STANDARD VERIFIED 13:32  
EXTERNAL STANDARD 0.080 13:32  
BLANK TEST 0.000 13:33  
SUBJECT SAMPLE INVALID 13:33

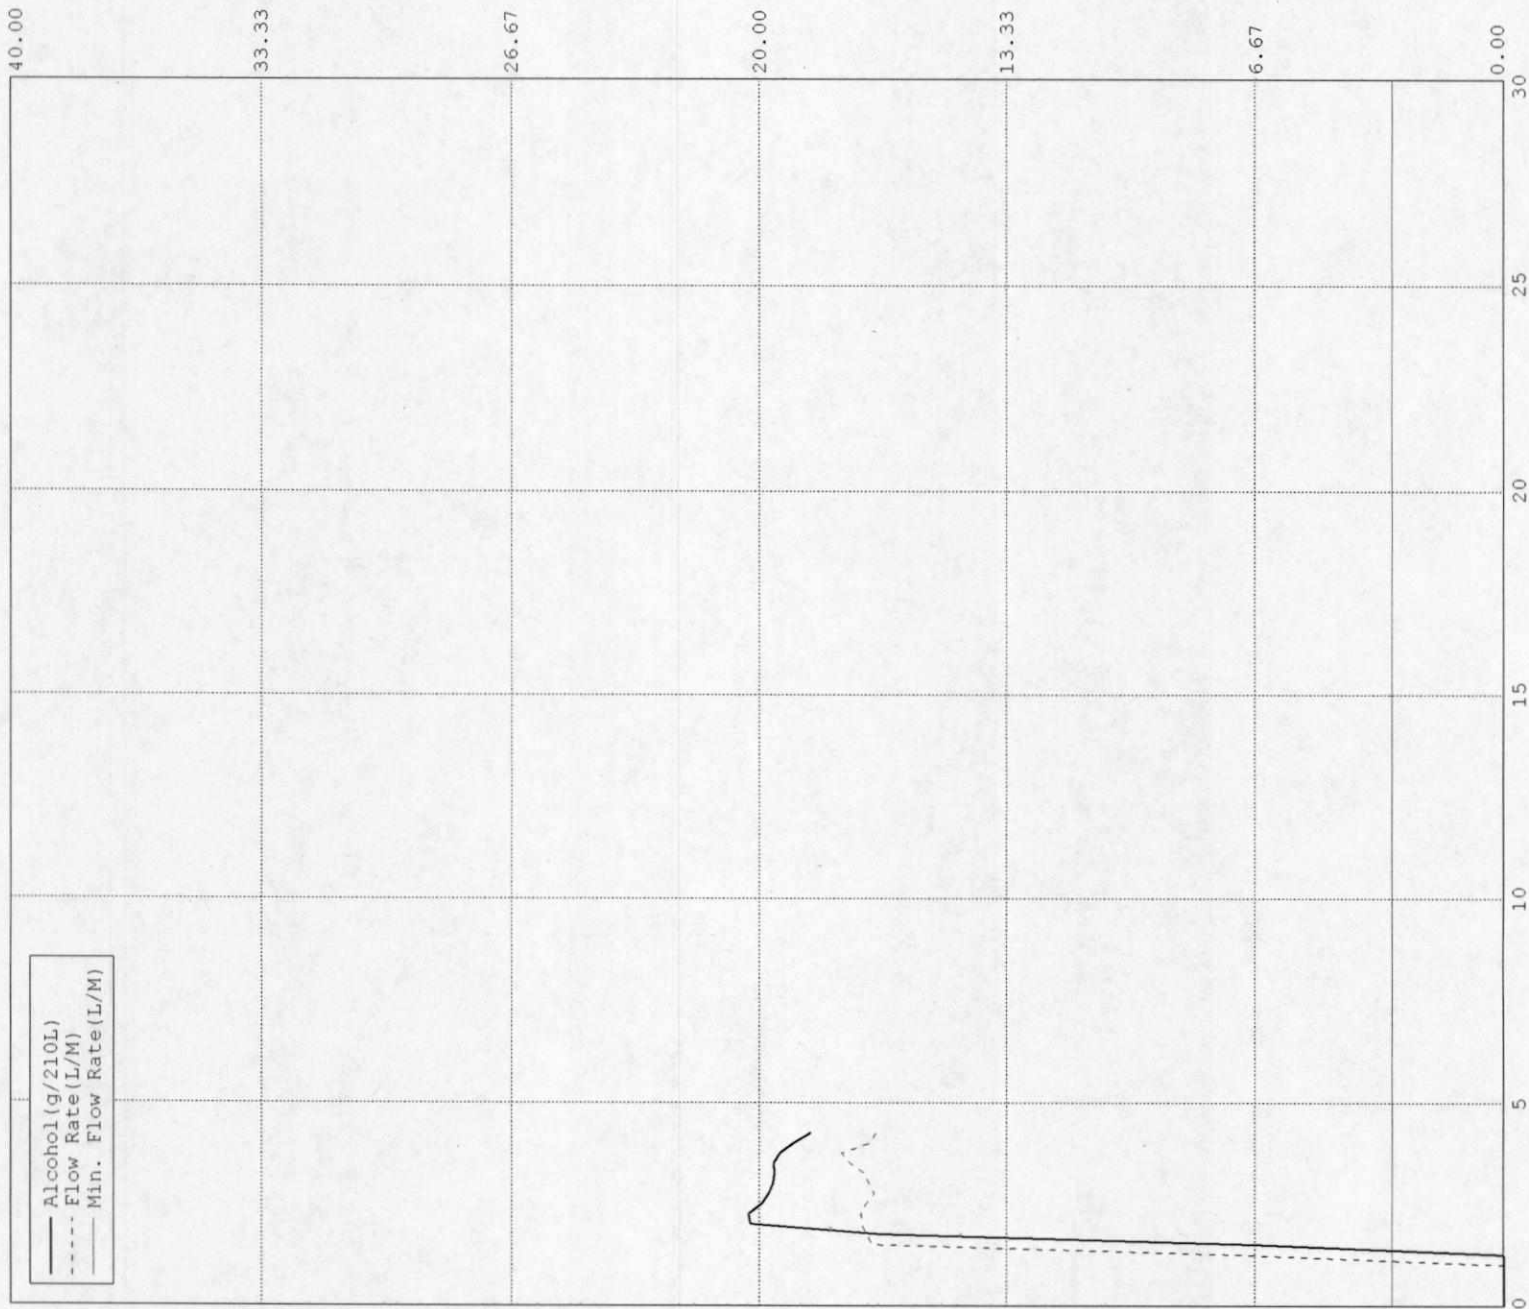



SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100418  
-----

Date: 09/03/2024  
Time: 13:40:44

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
RFI  
CASE/REPORT: XXXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:41  
BLANK TEST 0.000 13:41  
INTERNAL STANDARD VERIFIED 13:41  
EXTERNAL STANDARD 0.079 13:42  
BLANK TEST 0.000 13:43

RFI DETECTED

*OK*



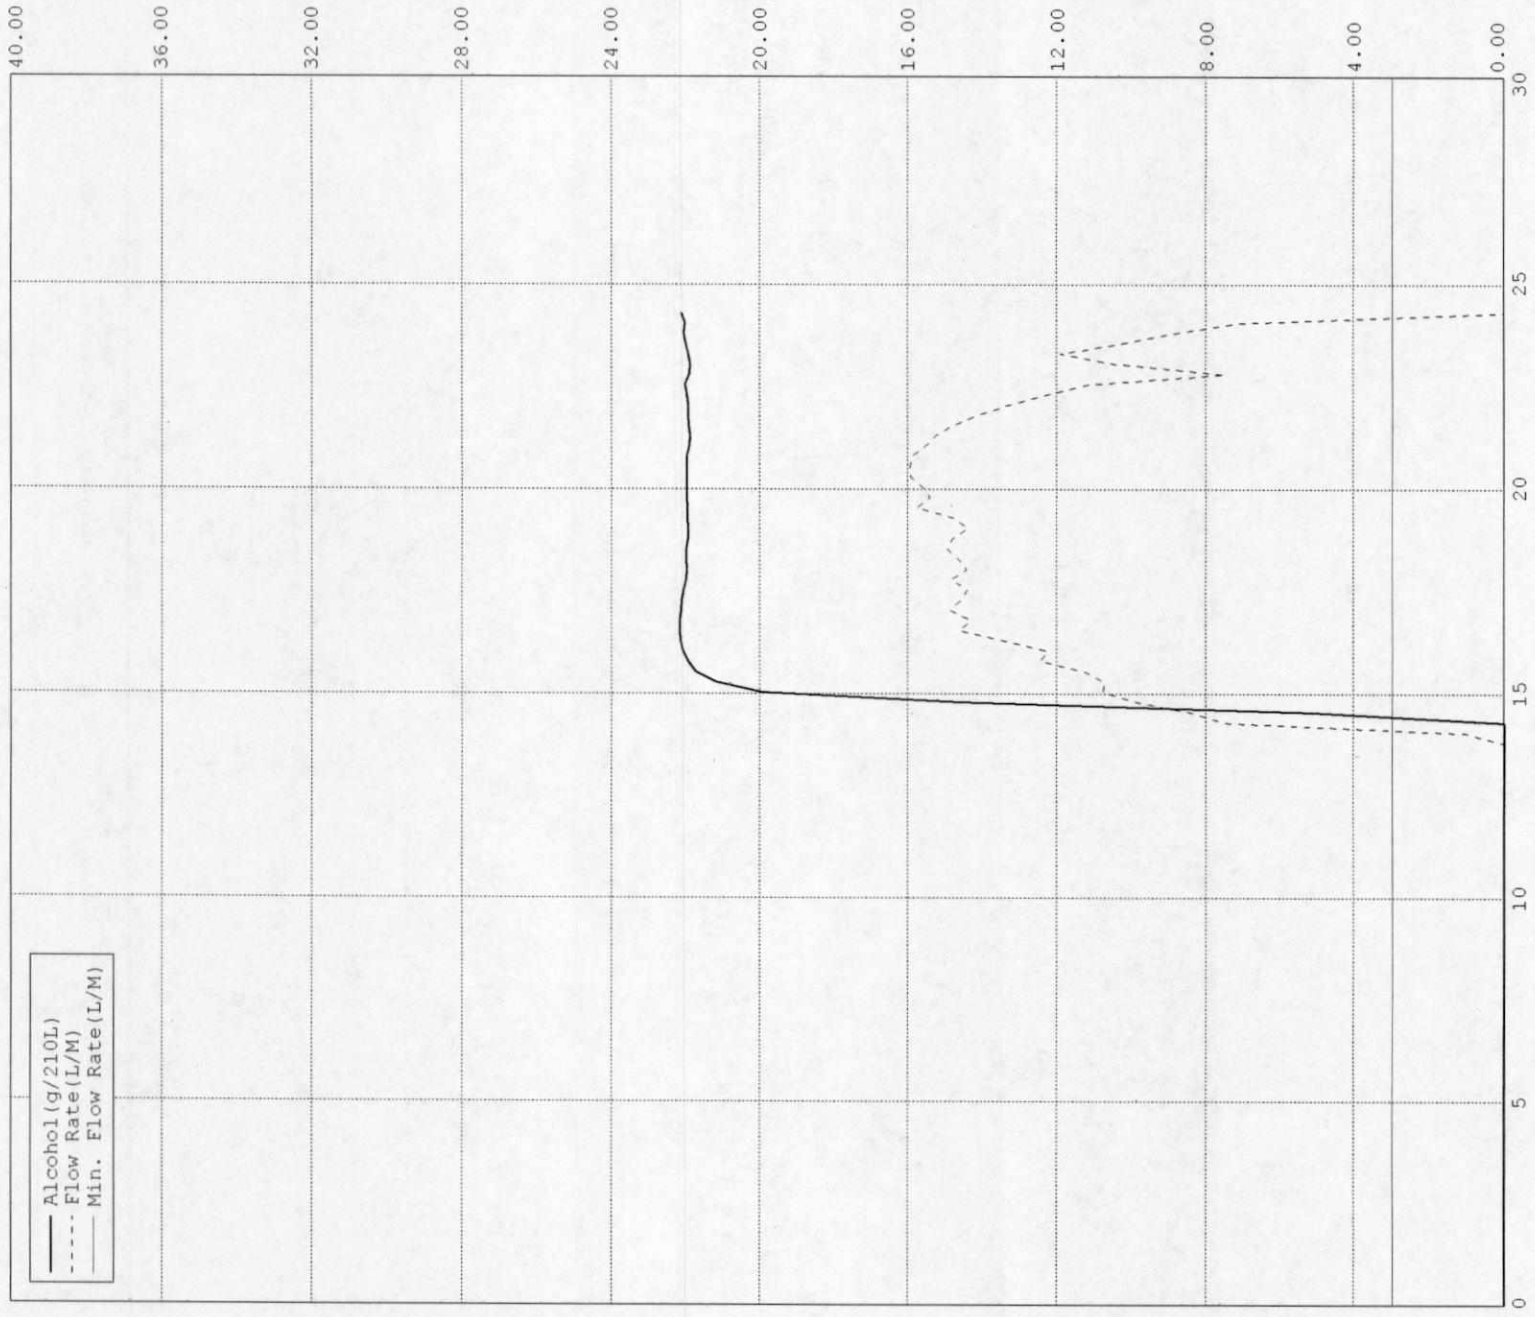

SUBJECT TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100418

Date: 09/03/2024  
 Time: 14:17:13

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX

OPERATOR NAME:  
 CHARLIE GLAISTER  
 OPERATOR'S #: 10436

DEPT/AGENCY:  
 INTERFERENCE - ACETONE  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.69: 0.079  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:18
BLANK TEST	0.000	14:18
INTERNAL STANDARD	VERIFIED	14:18
Xq = 0.065 (0.78%)		
EXTERNAL STANDARD	0.079	14:18
X[1] = 0.0791 (-0.0003) (0.0036)		
BLANK TEST	0.000	14:19
SUBJECT SAMPLE	XXX	14:20
X[1] = 0.1109 (-0.0206) (0.0019)		

Interference Detected

Filter 2 Avg: -0.0008  
 Filter 3 Avg: 0.0020  
 CWG- 9/3/2024

CWG

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100418  
-----

Date: 09/03/2024  
Time: 14:22:26

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
INTERFERENCE - IPA  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:23
BLANK TEST	0.000	14:23
INTERNAL STANDARD	VERIFIED	14:23
Xq = 0.066 (0.13%)		
EXTERNAL STANDARD	0.079	14:23
X[1] = 0.0793 (-0.0008) (0.0026)		
BLANK TEST	0.000	14:24
SUBJECT SAMPLE	XXX	14:25
X[1] = 0.1226 (-0.0296) (0.0022)		

Interference Detected

CKG

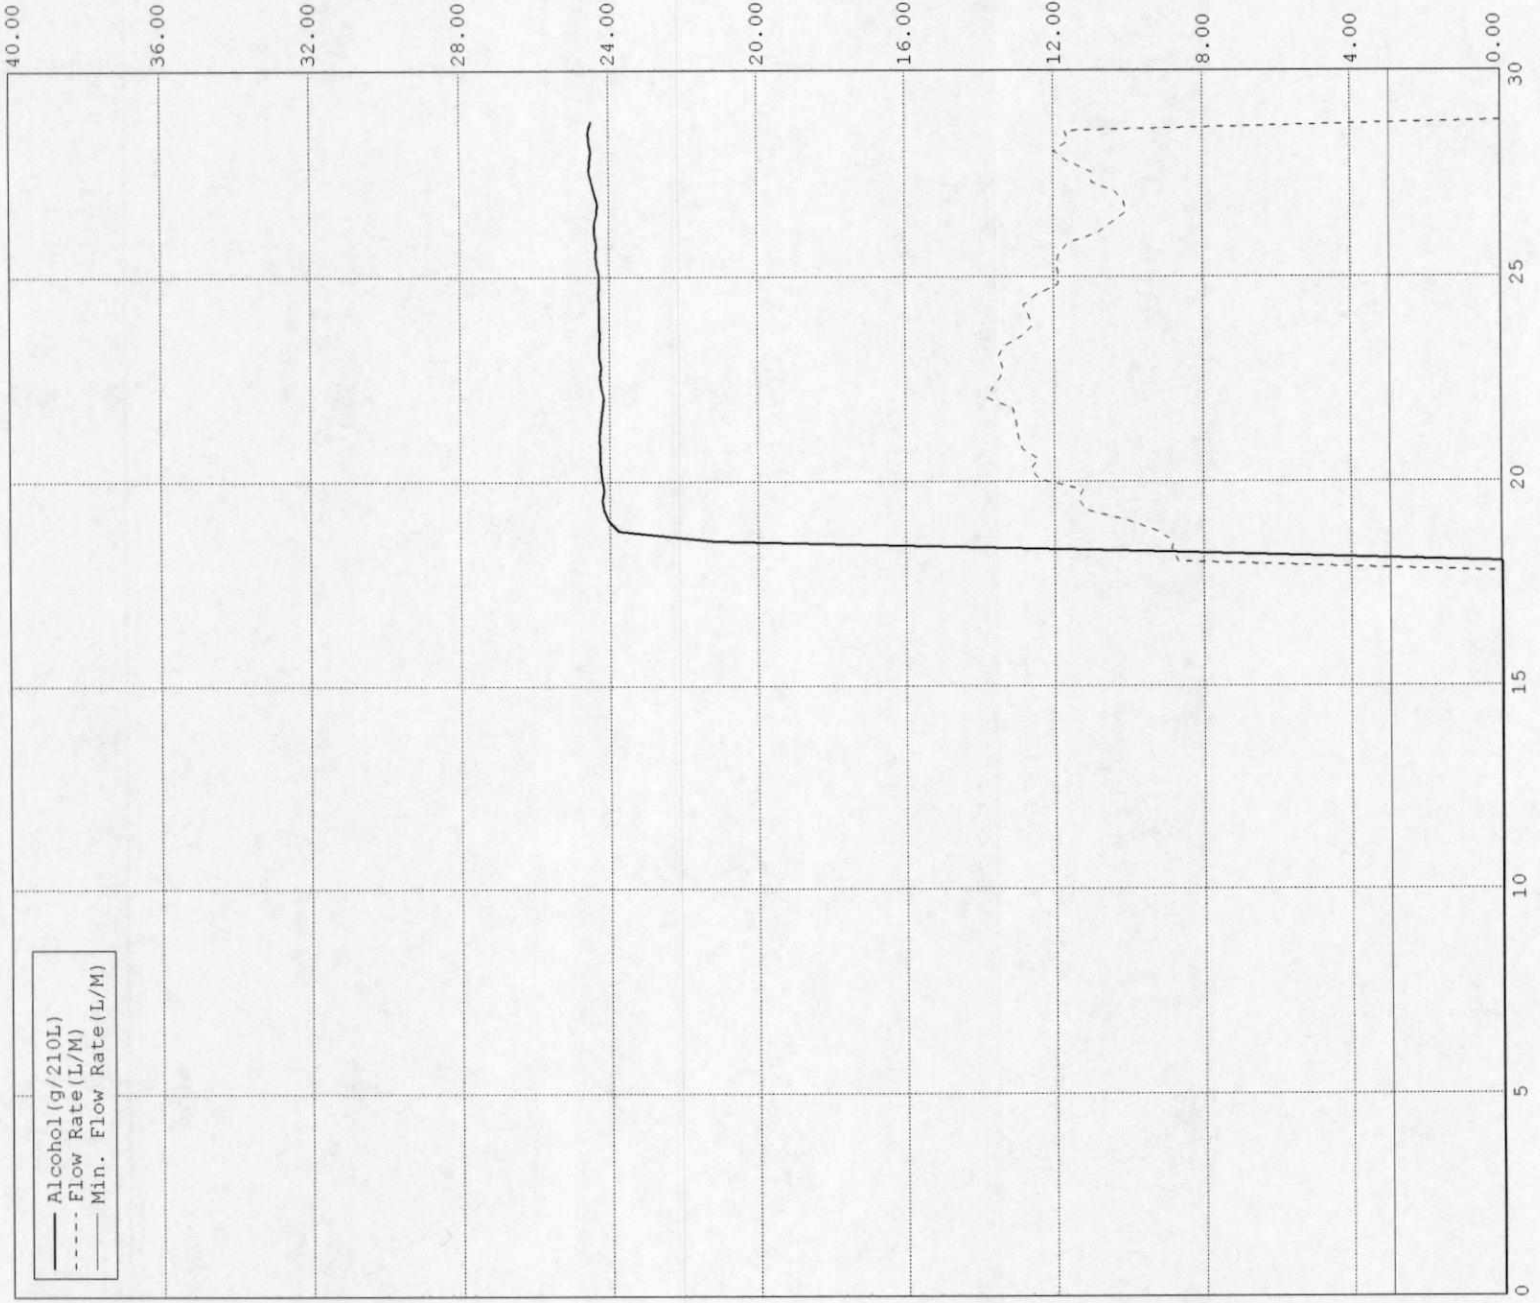

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100418

Date: 09/03/2024  
Time: 14:00:38

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE - NEGATIVE  
CASE/REPORT: XXXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:01
BLANK TEST	0.000	14:02
INTERNAL STANDARD	VERIFIED	14:02
$X_q = 0.065$ (1.57%)		
EXTERNAL STANDARD	0.079	14:02
$X[1] = 0.0793$ (-0.0007) (0.0011)		
BLANK TEST	0.000	14:03
SUBJECT SAMPLE (Vol=2.19L)	0.099	14:05
$X[1] = 0.0992$ (0.0005) (-0.0018)		
BLANK TEST	0.000	14:06
EXTERNAL STANDARD	0.079	14:06
$X[1] = 0.0788$ (-0.0013) (0.0008)		
BLANK TEST	0.000	14:07

CKG

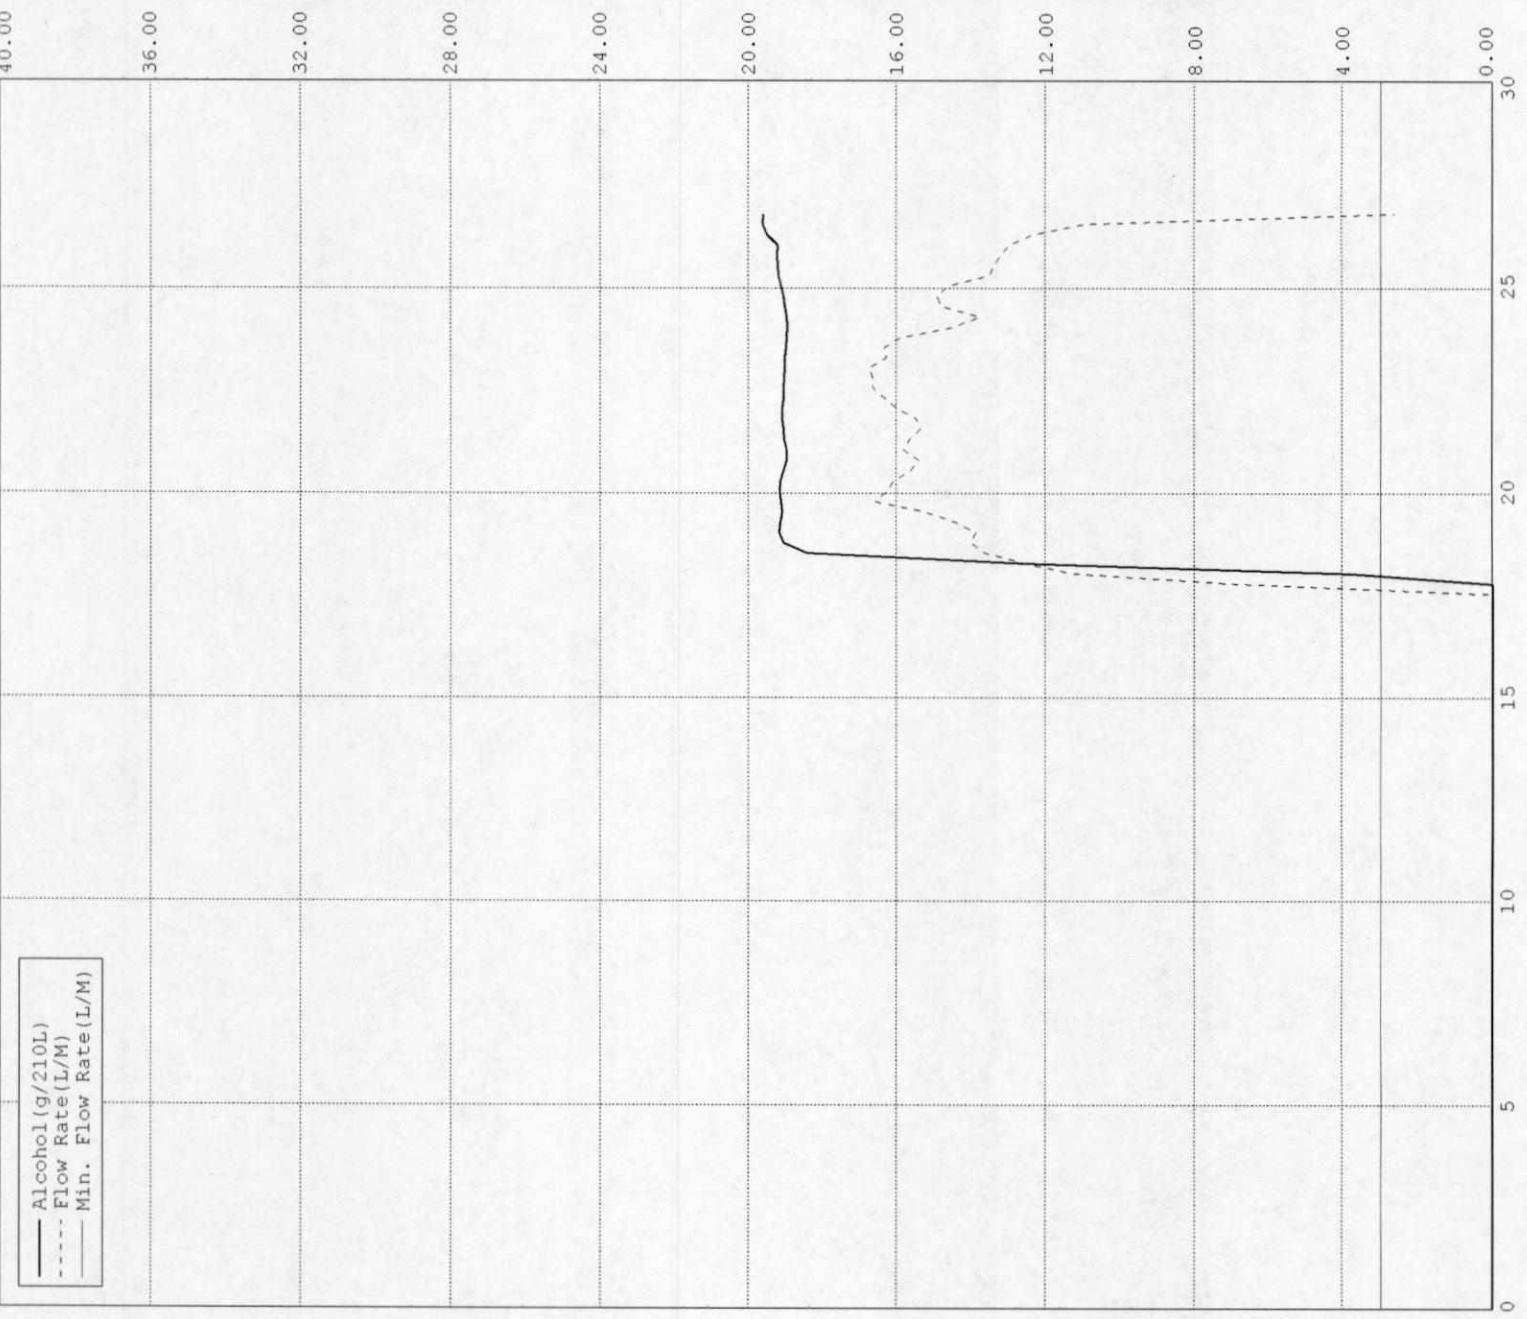



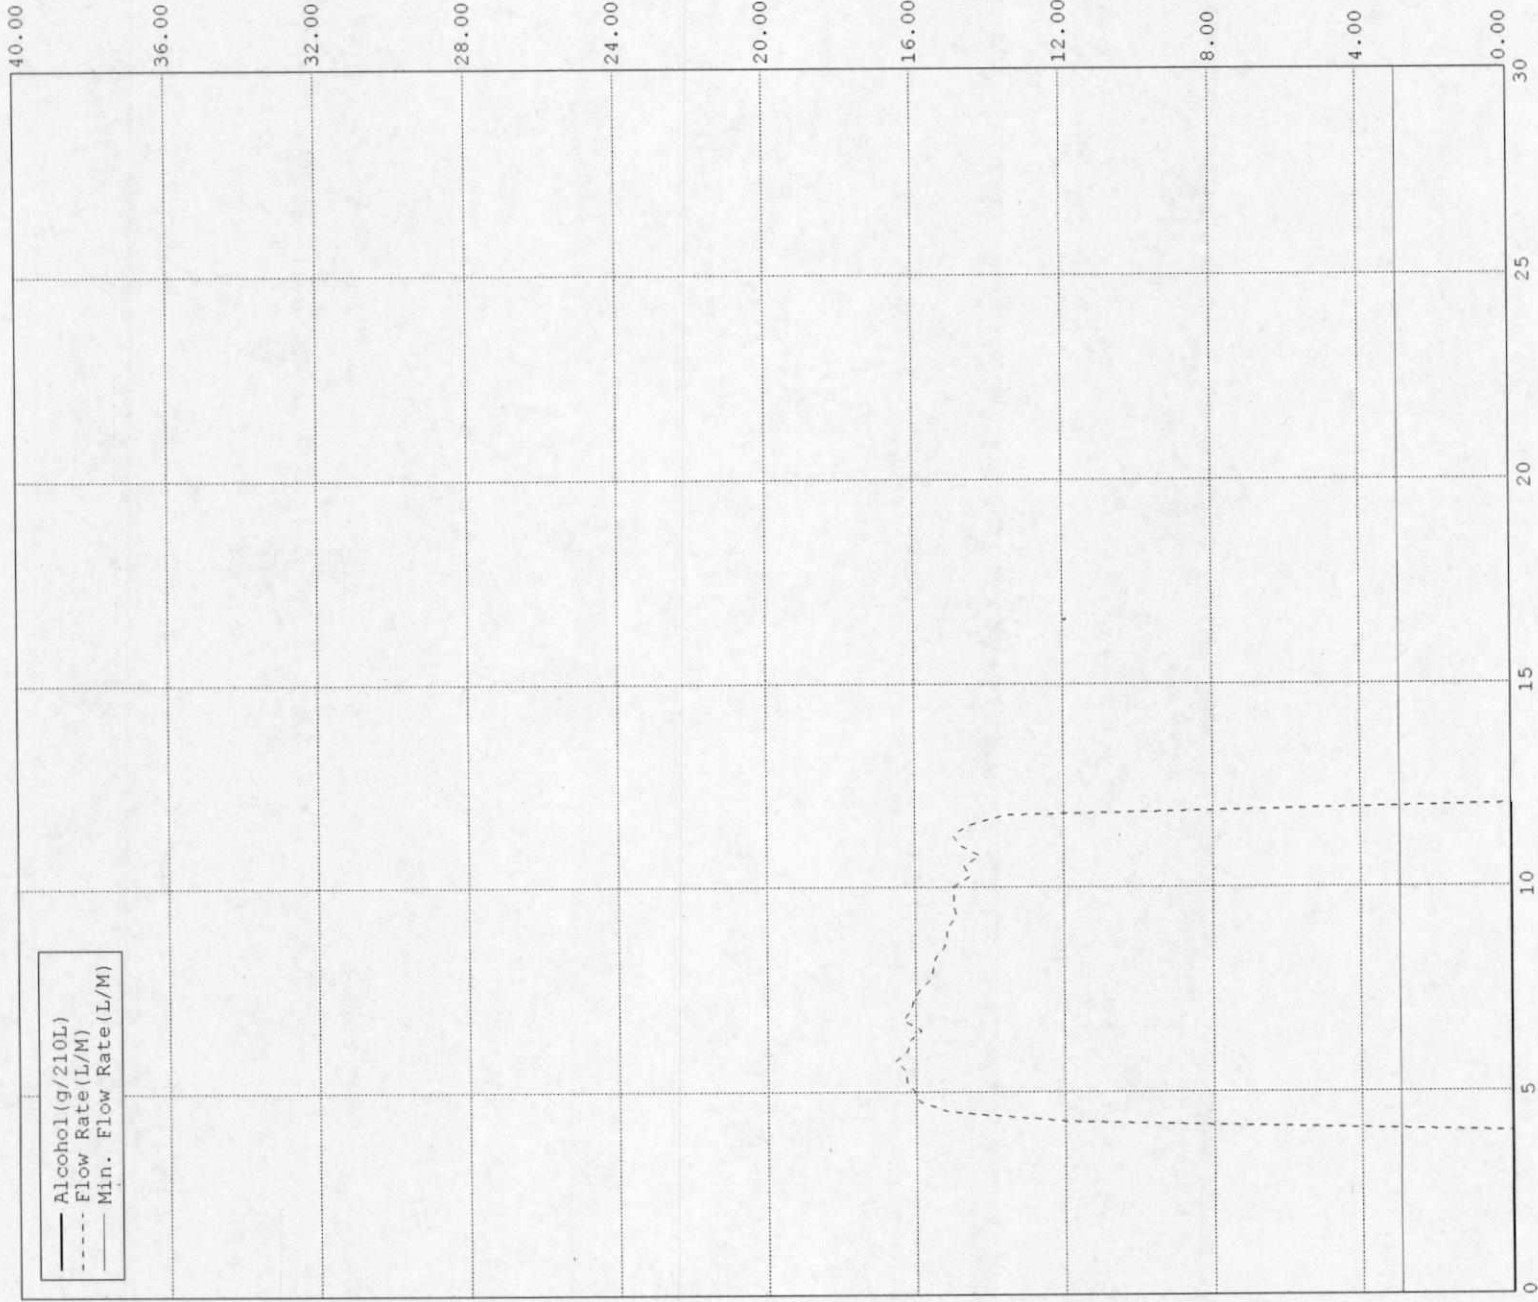

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100418

Date: 09/03/2024  
Time: 14:43:51

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.69: 0.079  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	TIME
BLANK TEST	0.000	14:45
INTERNAL STANDARD	VERIFIED	14:45
EXTERNAL STANDARD	0.079	14:45
BLANK TEST	0.000	14:46
SUBJECT SAMPLE (Vol=1.98L)	0.000	14:46
BLANK TEST	0.000	14:47
EXTERNAL STANDARD	0.079	14:47
BLANK TEST	0.000	14:48

CK6