



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100421

**Report Issue Date:** 10/02/2023  
**Date Received:** 2023-08-16  
**Condition of Item:** Good

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 08/17/2023** - As Found - **End Date 08/17/2023** As Found - Evaluation Analyst: Tatiana Malnoske  
 As Found Conditions - Barometric Pressure (inHg): 29.84 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.6  
 Relative Humidity (%): 39%

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.080	AG310901	0.078	0.079	0.079	0.079	0.079	0.079	0.079
0.300	0.300	AG217903	0.296	0.295	0.295	0.295	0.295	0.295	0.295

**Start Date 09/26/2023** - As Left - **End Date 09/27/2023**  
 As Left Conditions - Barometric Pressure (inHg): 29.30 Barometer Used: Fisher S/N 221250180 Temperature (C): 23.5 Relative Humidity (%): 31

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.021	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG217904	0.039	0.040	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.078	AG310901	0.078	0.078	0.077	0.077	0.078	0.078	+/- 0.004
0.100	0.098	AG211003	0.097	0.097	0.096	0.096	0.097	0.097	+/- 0.004
0.150	0.147	AG134205	0.144	0.145	0.145	0.145	0.145	0.145	+/- 0.005
0.300	0.294	AG217903	0.290	0.290	0.290	0.290	0.291	0.290	+/- 0.011

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Carlie Glaister on 09/27/2023

[carlie.glaister@alaska.gov](mailto:carlie.glaister@alaska.gov)

Technically and administratively reviewed by Colleen O'Bryant on 10/02/2023

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100421 Analyst: Carlie Glaister Start Date: 9/26/2023

- Diagnostic Test (attached)
- Adjust voltages, if needed
  - o Lamp (2.60 V Maximum)
  - o Bias
  - o Cooler (2.00 V Maximum)
- Internal Standard value  $\leq$  3.00%
  - o Chopper Frequency
  - o Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.6 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.30 Temperature (C): 23.5 Relative Humidity (%): 31

Linearity Test (attached)

0.020g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217902</u>	Exp: <u>6/28/24</u>
0.040g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217904</u>	Exp: <u>6/28/24</u>
0.080g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-310901</u>	Exp: <u>4/19/25</u>
0.100g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-211003</u>	Exp: <u>4/20/24</u>
0.150g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-134205</u>	Exp: <u>12/8/23</u>
0.300g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217903</u>	Exp: <u>6/28/24</u>

Functional Tests (attached)

- Incomplete
  - Maximum Attempts Exceeded
  - Interference (Volatiles)
  - Invalid
  - Radio Frequency Interference (RFI)
- Acetone Mnf: Lifeloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24  
Simulator S/N: DR4176 Verification Performed?
- Isopropanol Mnf: Lifeloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24  
Simulator S/N: DR4177 Verification Performed?
- Neg. Control Mnf: Lifeloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24  
Simulator S/N: DR6267 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/9/2023

- Verify stylus is calibrated
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Non-Drinking Subject Test
- Upload
- Remove Tank Prior to Shutdown
- Calibration End Date: 9/27/2023

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100421  
-----

Date: 09/26/2023  
Time: 08:16:36

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 44.6°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.71 V PASSED  
(1.03 V - 2.39 V)  
Cooler Voltage = 1.80 V PASSED  
(1.08 V - 2.52 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 529 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.4 in

PUMP INFO

Flow Rate = 4.607 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.097 0.63% (0.00% - 4.00%) PASSED

Technician Screen

-----  
Joint Base Elmendorf - Richardson  
DATAMASTER dmt: 100421  
-----

Date: 09/26/2023  
Time: 9:14 AM

Temperatures (°C)

Sample Cell: 48.7°C  
Breath Tube: 44.5°C

Current Barometer 29.3 in  
Volume (Ltr) 1.51

Settings

Lamp: 1.74 V  
Bias: 80 V  
Cooler: 1.80 V  
Chopper: 528 Hz

Voltages (V)

Flow: 1.08 V  
Detector: -0.047 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100421  
-----

Date: 04/21/2020  
Time: 09:14:36

OPERATOR NAME:  
COLLEEN S OBRYANT  
CERTIFICATE #: 6237

Ca = 0.1000  
CAL = 0.965698    0.800 <= CAL < 1.200  
b1 = 0.0009    0.0000 <= b1 < 0.0040  
b2 = 0.0043    0.0010 <= b2 < 0.0100  
b3 = 0.0014    0.0000 <= b3 < 0.0040  
Xq = 0.0966    0.0500 <= Xq < 0.2000  
a21 = 1.141766    1.050 <= a21 < 1.300  
a31 = 0.455042    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100421

Date: 09/26/2023

Time: 09:28:27

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080 Lot # AG310901

TARGET AT 29.30: 0.078 Exp: 4/19/25

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE (Vol=1.54L)

BLANK TEST

EXTERNAL STANDARD

BLANK TEST

PASSED 09:29

0.000 09:29

VERIFIED 09:29


0.078 09:30

0.000 09:31

0.000 09:32

0.078 09:33

0.000 09:34

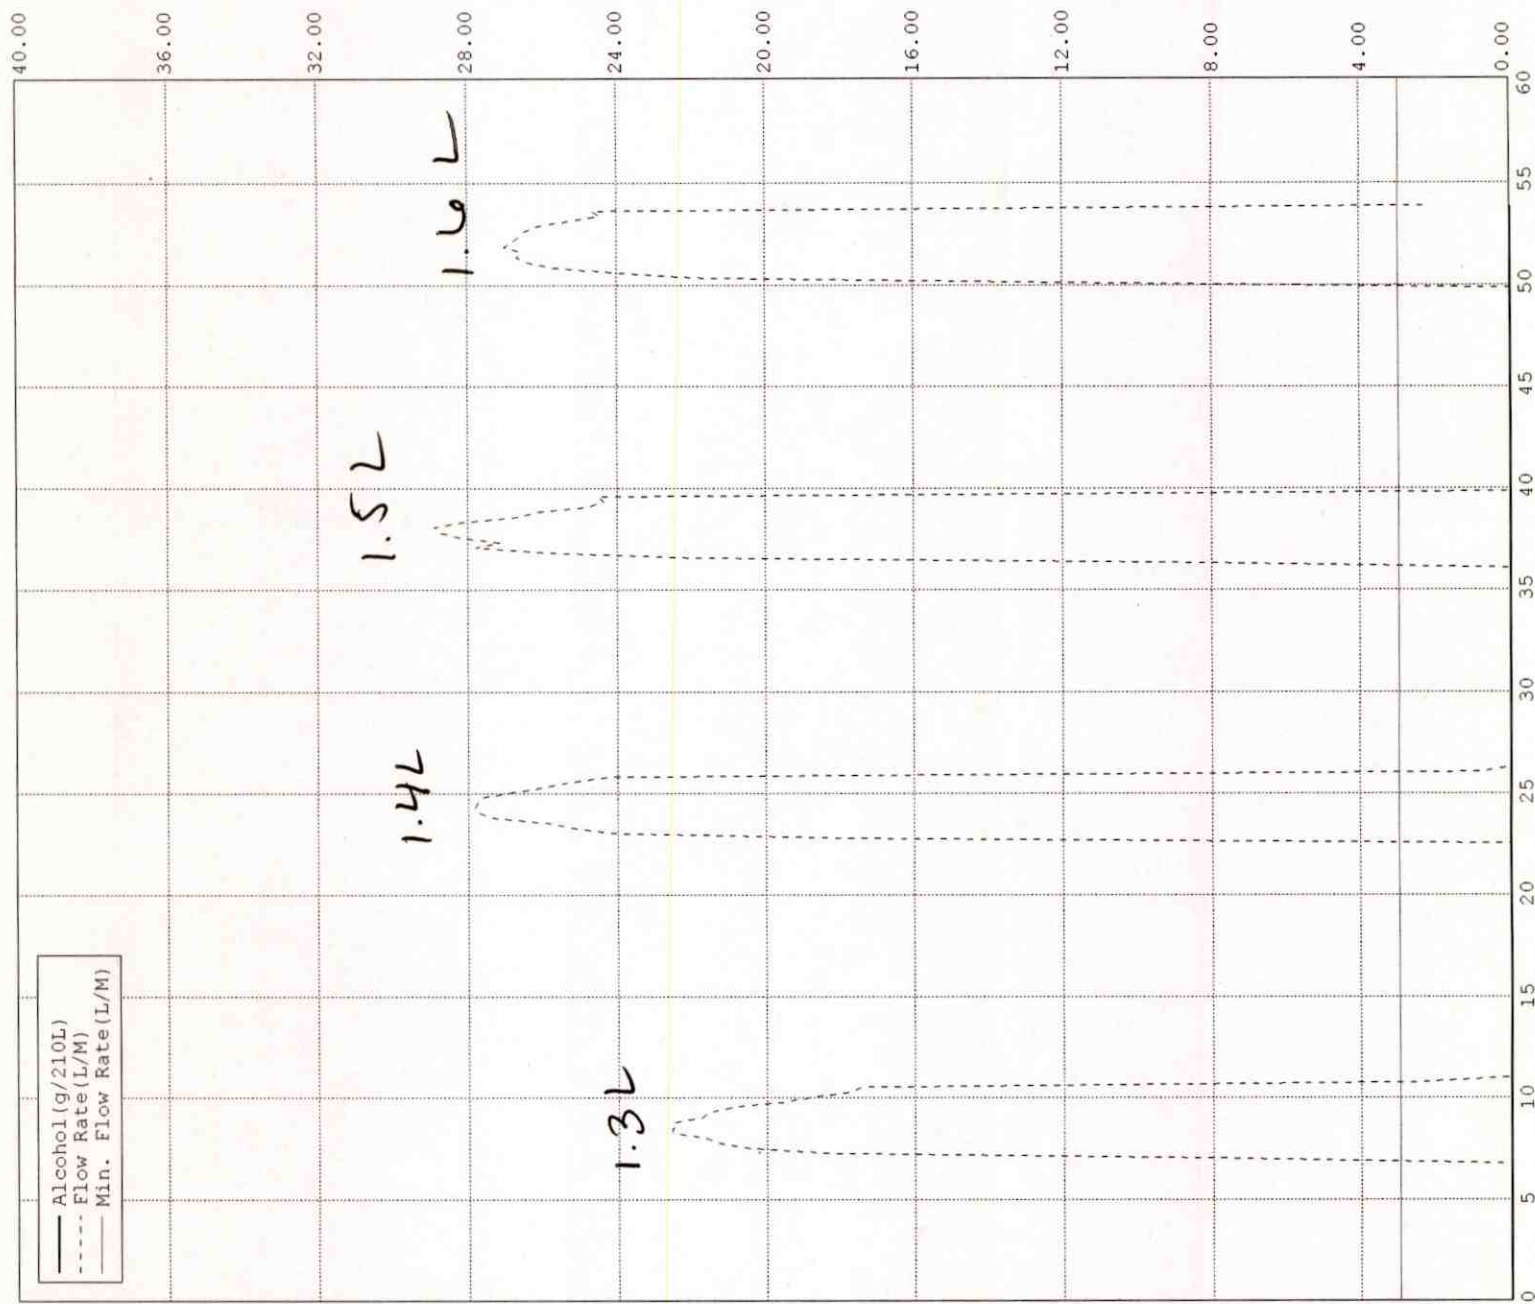

LINEARITY CHECK


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100421  
 -----

Date: 09/26/2023  
 Time: 13:18:41

SUPERVISOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0004
0.039	0.0392	0.0004
0.078	0.0776	0.0005
0.098	0.0966	0.0005
0.147	0.1448	0.0004
0.294	0.2902	0.0004

SLOPE = 0.984574  
 R<sup>2</sup> = 0.999988

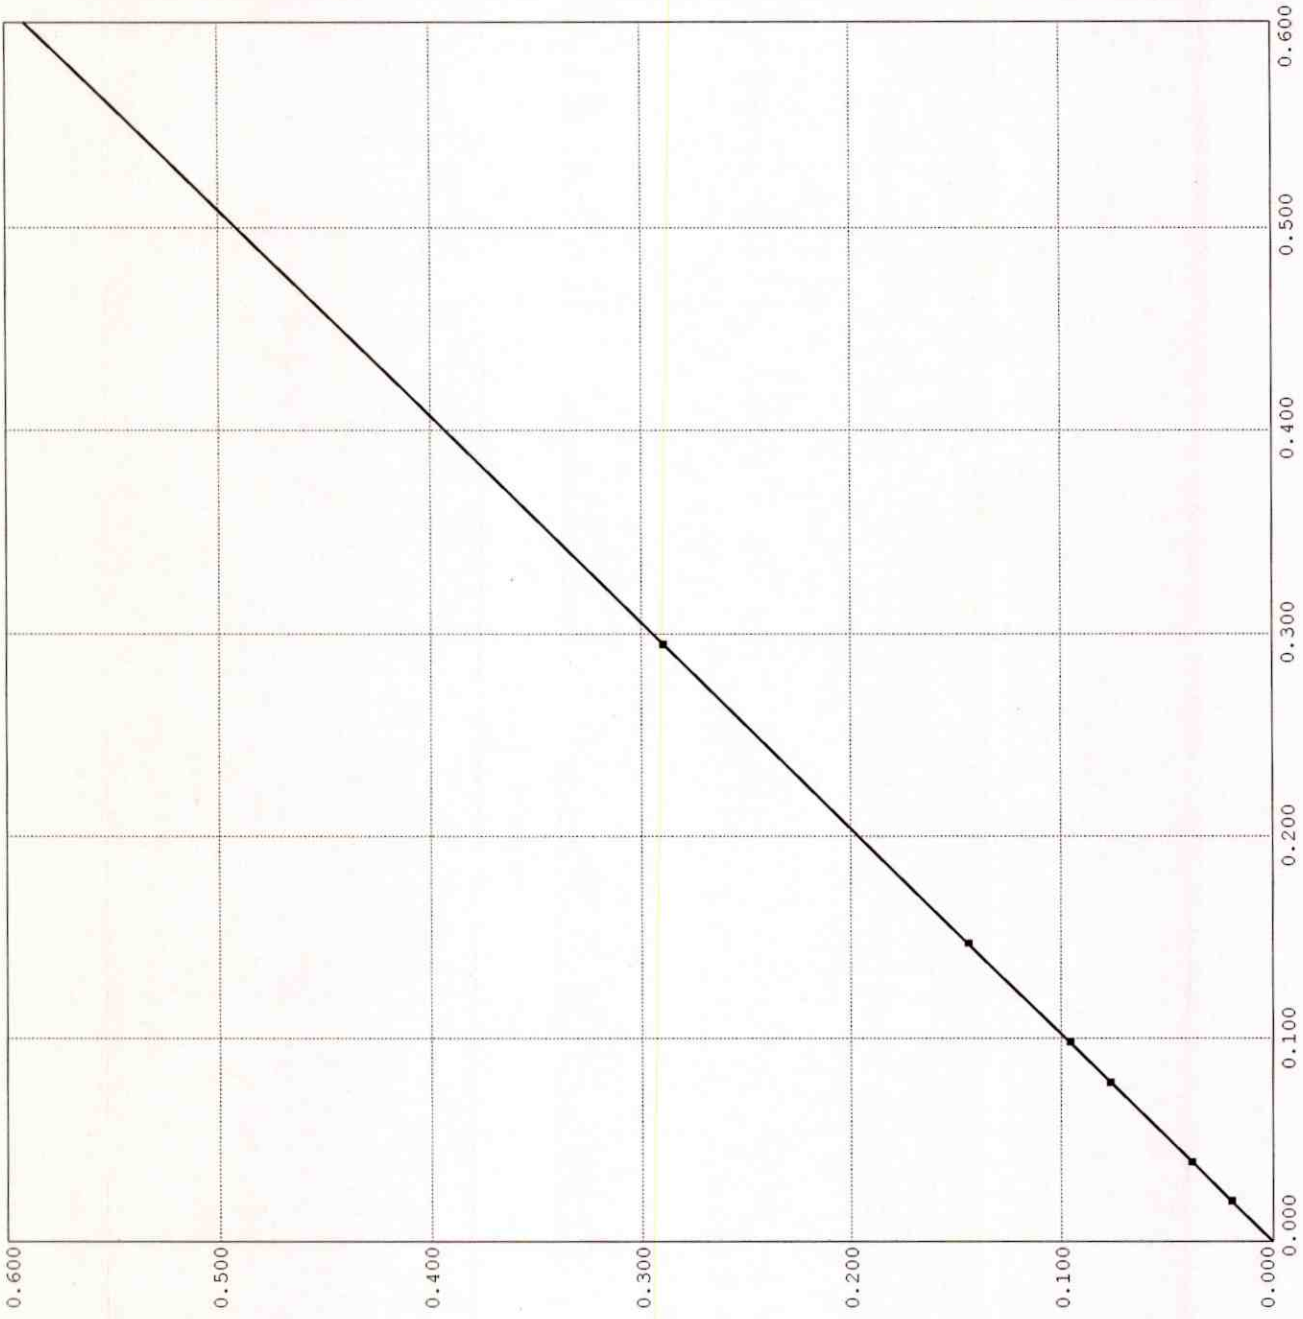

OK

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100421






Date: 09/26/2023  
 Time: 13:18:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.30: 0.020  
 LOT #: AG217902  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 864 psi

BLANK TEST	0.000	13:20
INTERNAL STANDARD	VERIFIED	13:20
EXTERNAL STANDARD	0.021	13:20
BLANK TEST	0.000	13:21
EXTERNAL STANDARD	0.020	13:21
BLANK TEST	0.000	13:22
EXTERNAL STANDARD	0.020	13:22
BLANK TEST	0.000	13:23
EXTERNAL STANDARD	0.020	13:23
BLANK TEST	0.000	13:24
EXTERNAL STANDARD	0.020	13:24
BLANK TEST	0.000	13:25

Average = 0.0202  
 Std Dev = 0.0004

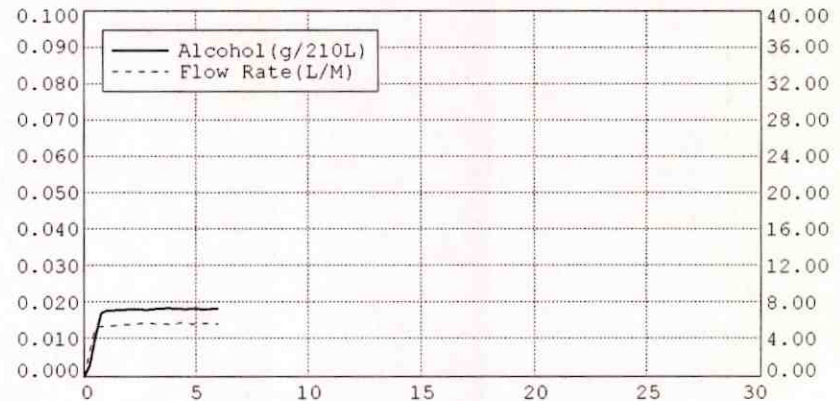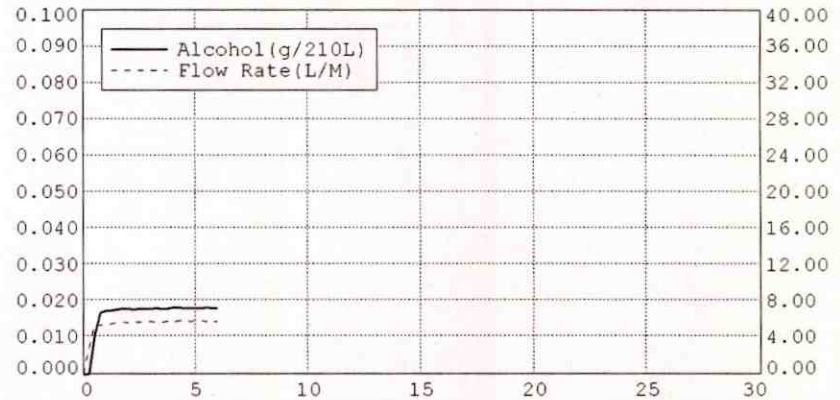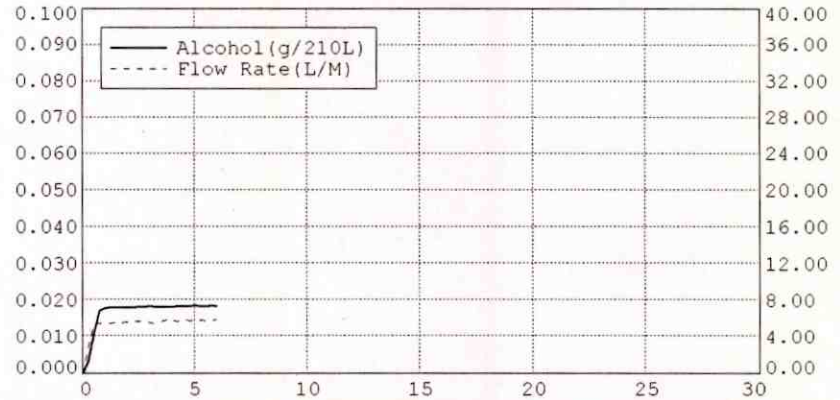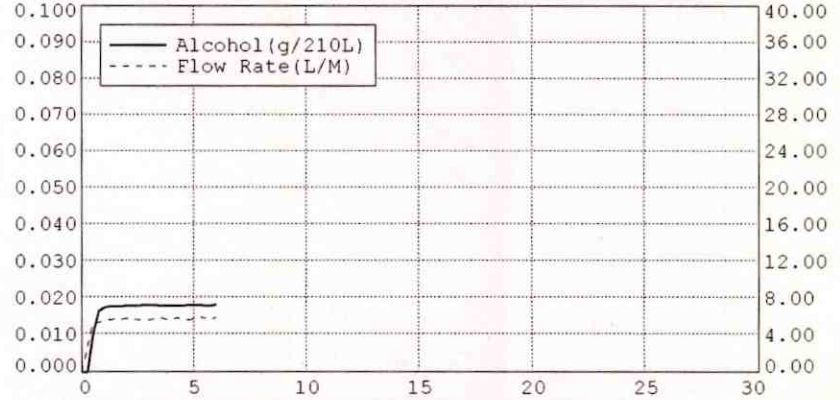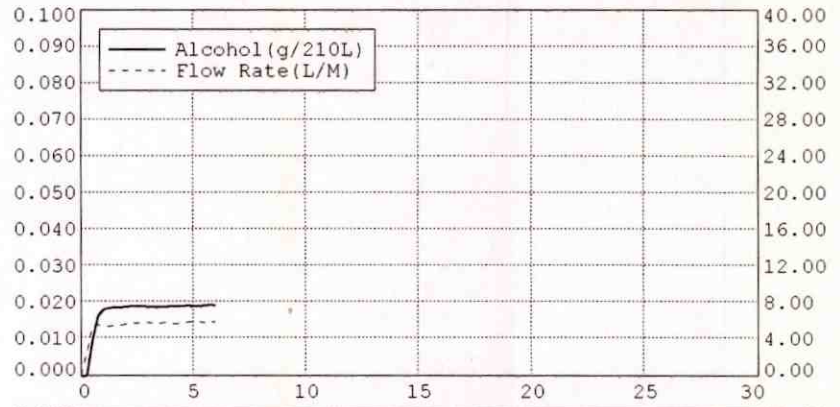



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100421






Date: 09/26/2023  
 Time: 13:27:41

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.30: 0.039  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 924 psi

BLANK TEST	0.000	13:28
INTERNAL STANDARD	VERIFIED	13:29
EXTERNAL STANDARD	0.039	13:29
BLANK TEST	0.000	13:30
EXTERNAL STANDARD	0.040	13:30
BLANK TEST	0.000	13:31
EXTERNAL STANDARD	0.039	13:31
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.039	13:32
BLANK TEST	0.000	13:33
EXTERNAL STANDARD	0.039	13:33
BLANK TEST	0.000	13:34

Average = 0.0392  
 Std Dev = 0.0004

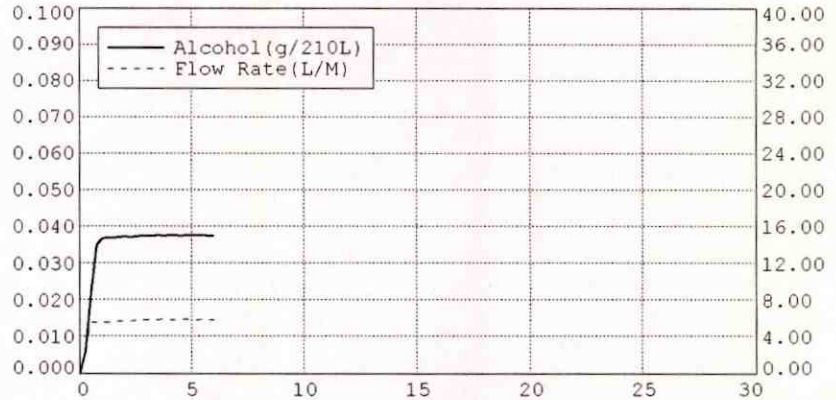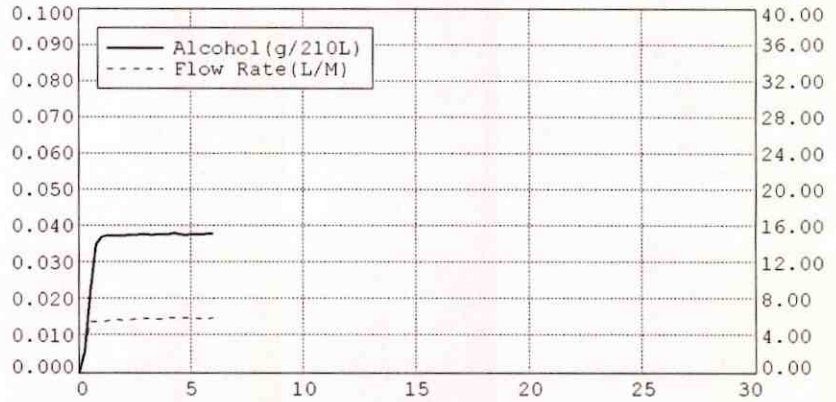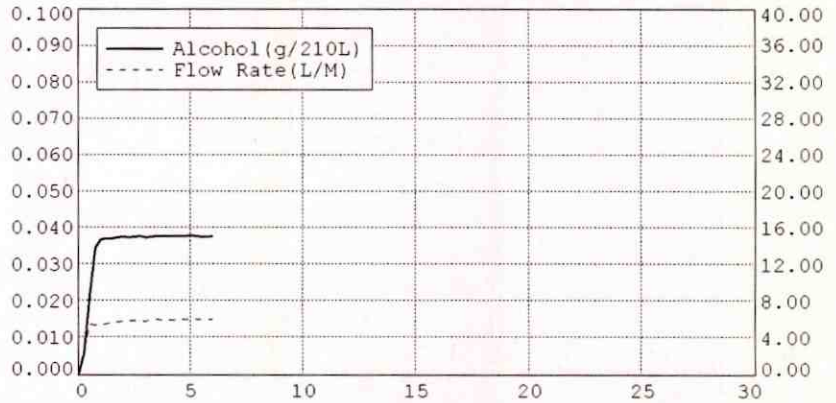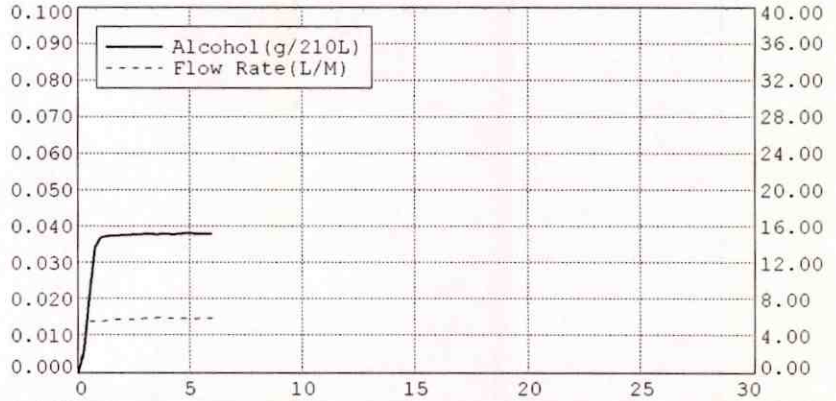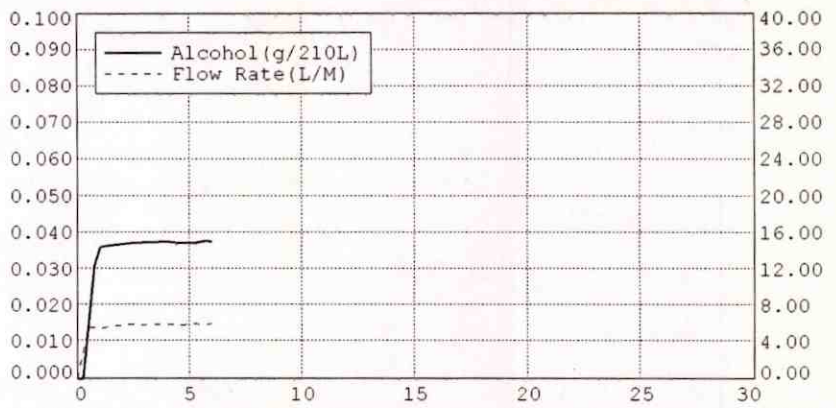

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100421






Date: 09/26/2023  
 Time: 13:36:43

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.29: 0.078  
 LOT #: AG310901  
 EXPIRATION: 04/19/2025  
 TANK PRESSURE: 969 psi

BLANK TEST	0.000	13:38
INTERNAL STANDARD	VERIFIED	13:38
EXTERNAL STANDARD	0.078	13:38
BLANK TEST	0.000	13:39
EXTERNAL STANDARD	0.078	13:39
BLANK TEST	0.000	13:40
EXTERNAL STANDARD	0.077	13:40
BLANK TEST	0.000	13:41
EXTERNAL STANDARD	0.077	13:41
BLANK TEST	0.000	13:42
EXTERNAL STANDARD	0.078	13:42
BLANK TEST	0.000	13:43

Average = 0.0776  
 Std Dev = 0.0005

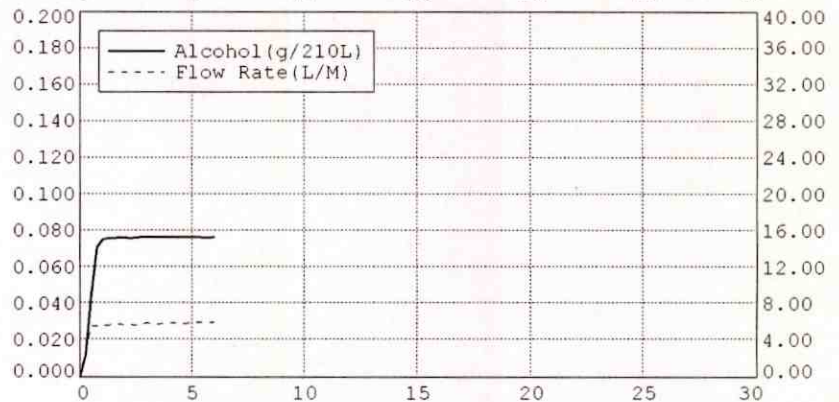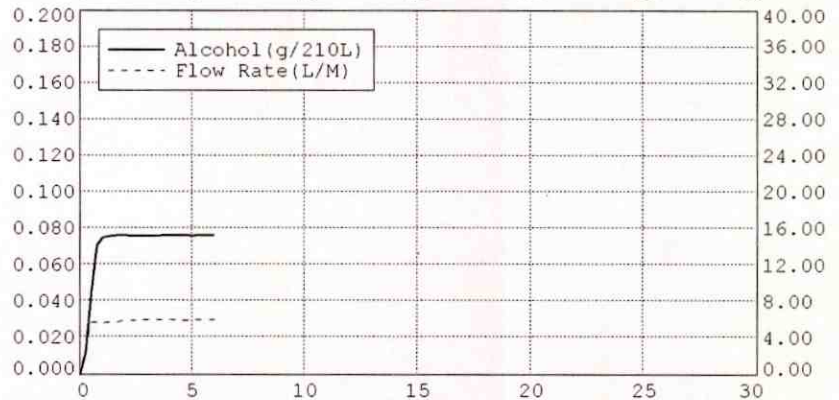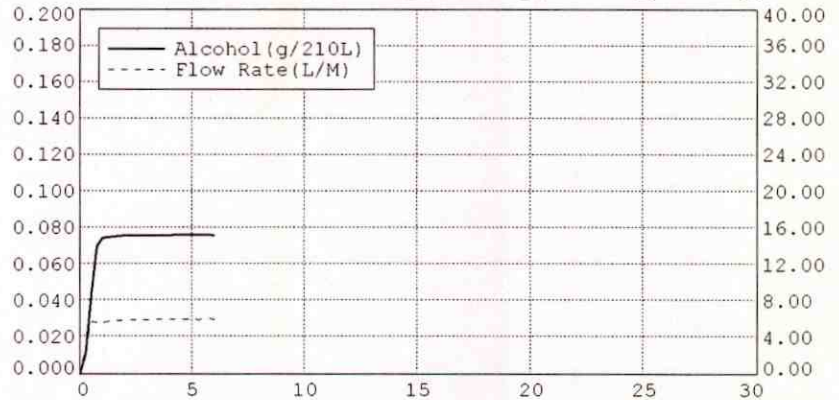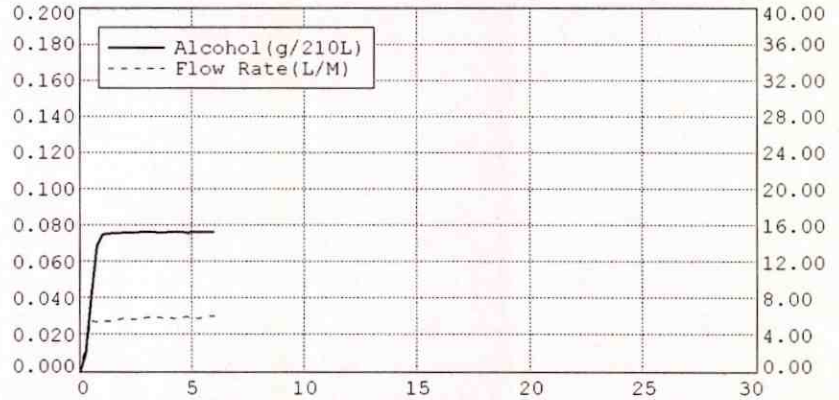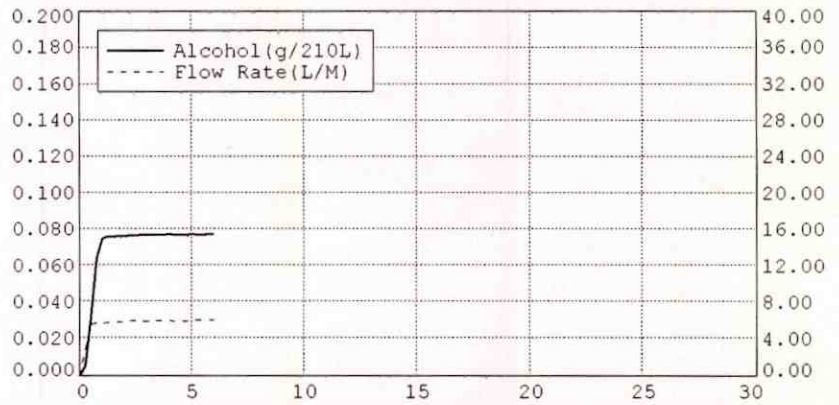

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100421






Date: 09/26/2023  
 Time: 13:45:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.30: 0.098  
 LOT #: AG211003  
 EXPIRATION: 04/20/2024  
 TANK PRESSURE: 572 psi

BLANK TEST	0.000	13:47
INTERNAL STANDARD	VERIFIED	13:47
EXTERNAL STANDARD	0.097	13:47
BLANK TEST	0.000	13:48
EXTERNAL STANDARD	0.097	13:48
BLANK TEST	0.000	13:49
EXTERNAL STANDARD	0.096	13:49
BLANK TEST	0.000	13:50
EXTERNAL STANDARD	0.096	13:51
BLANK TEST	0.000	13:51
EXTERNAL STANDARD	0.097	13:52
BLANK TEST	0.000	13:53

Average = 0.0966  
 Std Dev = 0.0005

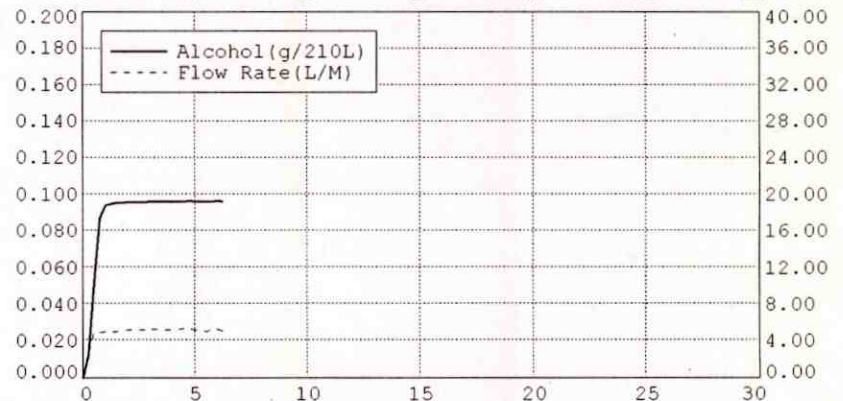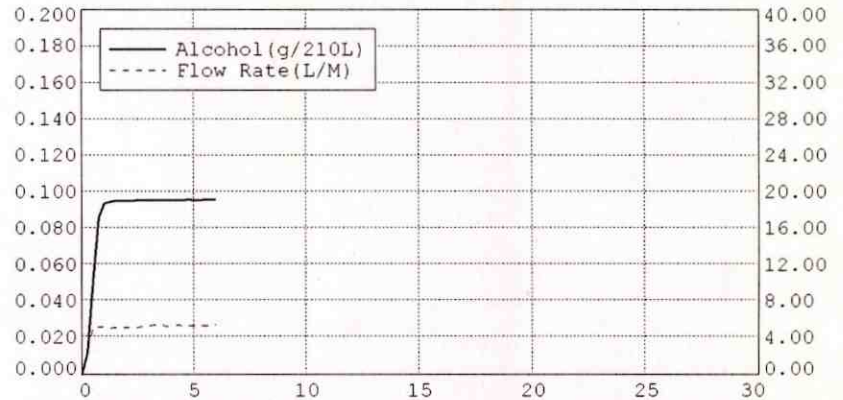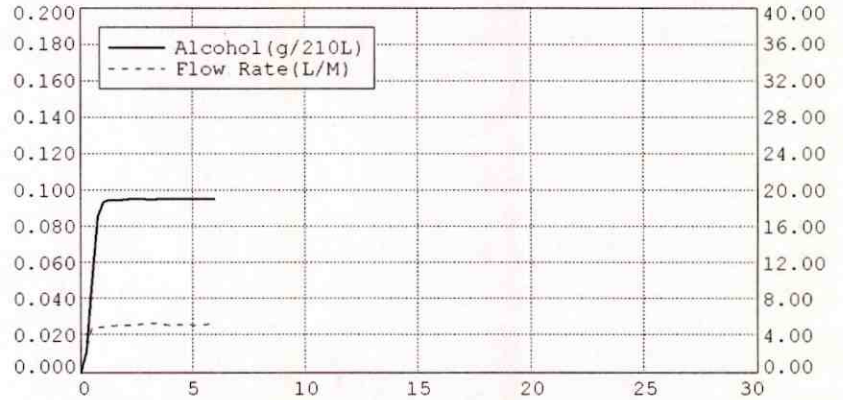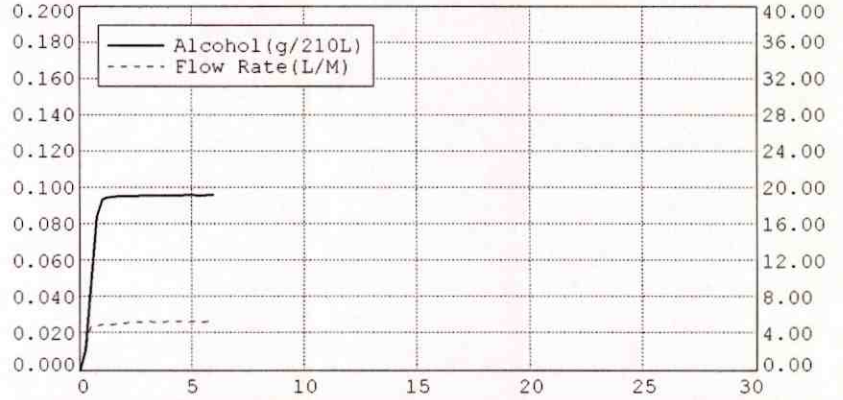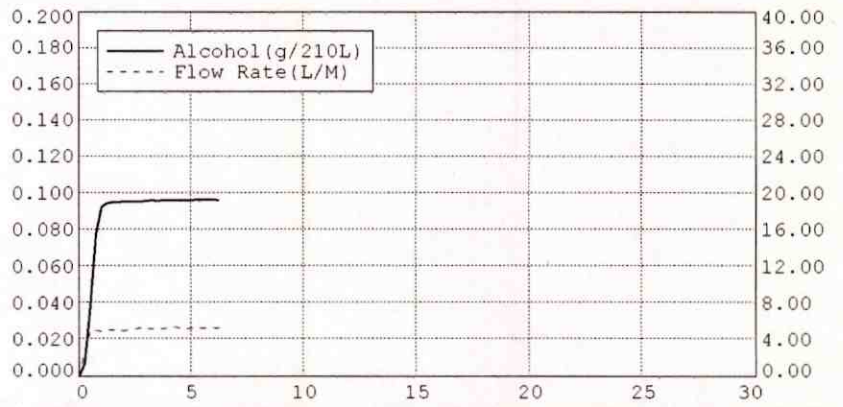

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100421






Date: 09/26/2023  
 Time: 13:53:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.30: 0.147  
 LOT #: AG134205  
 EXPIRATION: 12/08/2023  
 TANK PRESSURE: 525 psi

BLANK TEST	0.000	13:55
INTERNAL STANDARD	VERIFIED	13:55
EXTERNAL STANDARD	0.144	13:55
BLANK TEST	0.000	13:56
EXTERNAL STANDARD	0.145	13:56
BLANK TEST	0.000	13:57
EXTERNAL STANDARD	0.145	13:58
BLANK TEST	0.000	13:58
EXTERNAL STANDARD	0.145	13:59
BLANK TEST	0.000	14:00
EXTERNAL STANDARD	0.145	14:00
BLANK TEST	0.000	14:01

Average = 0.1448  
 Std Dev = 0.0004

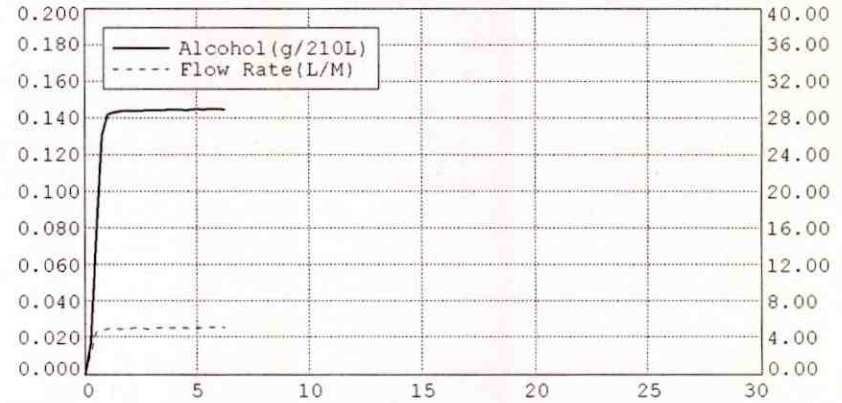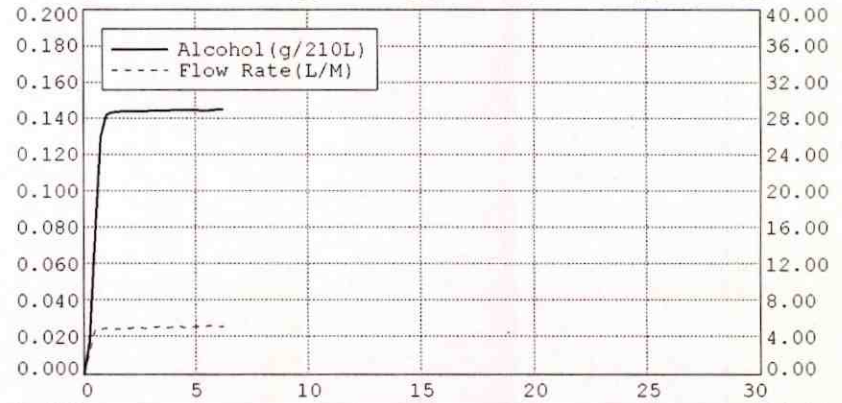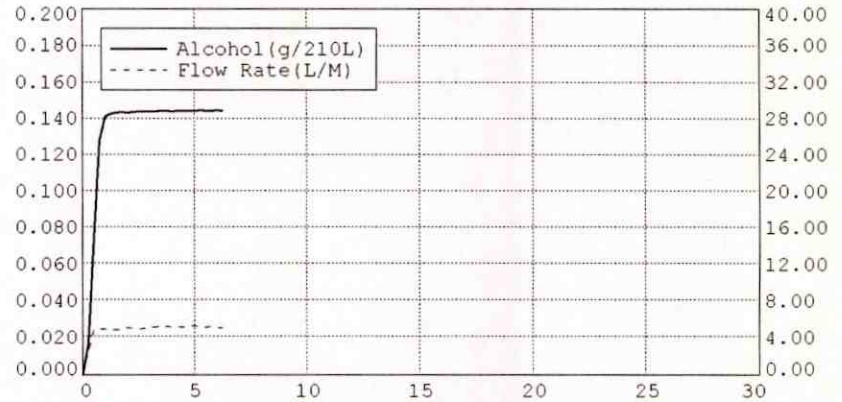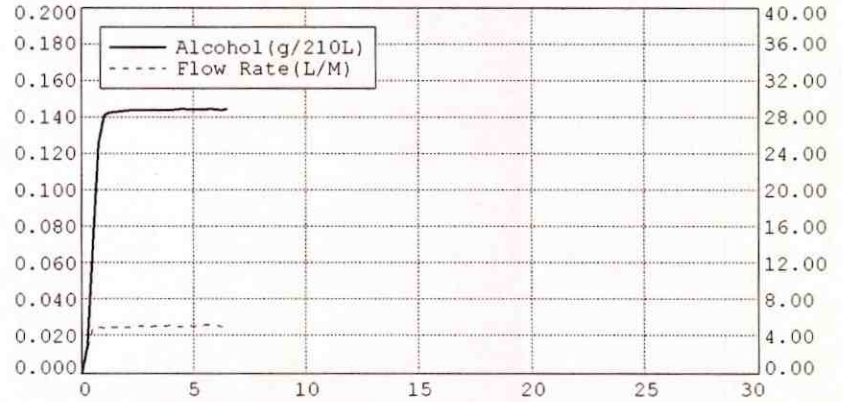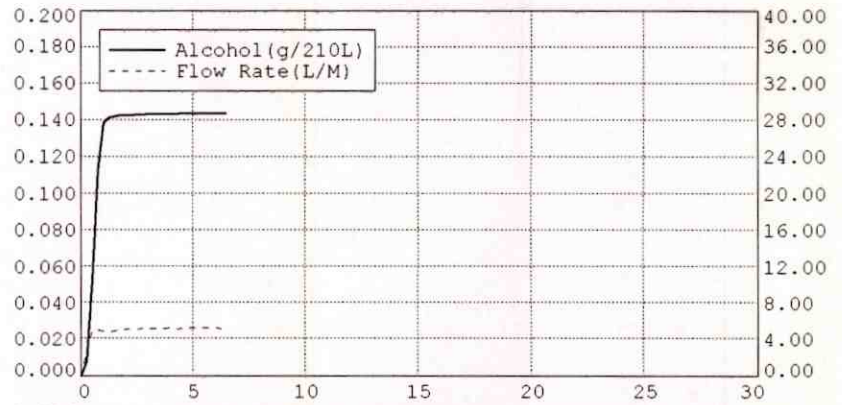

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
DATAMASTER dmt: 100421






Date: 09/26/2023  
Time: 14:02:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
TARGET AT 29.29: 0.294  
LOT #: AG217903  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 227 psi

BLANK TEST	0.000	14:03
INTERNAL STANDARD	VERIFIED	14:04
EXTERNAL STANDARD	0.290	14:04
BLANK TEST	0.000	14:05
EXTERNAL STANDARD	0.290	14:05
BLANK TEST	0.000	14:06
EXTERNAL STANDARD	0.290	14:06
BLANK TEST	0.000	14:07
EXTERNAL STANDARD	0.290	14:07
BLANK TEST	0.000	14:08
EXTERNAL STANDARD	0.291	14:08
BLANK TEST	0.000	14:09

Average = 0.2902  
Std Dev = 0.0004

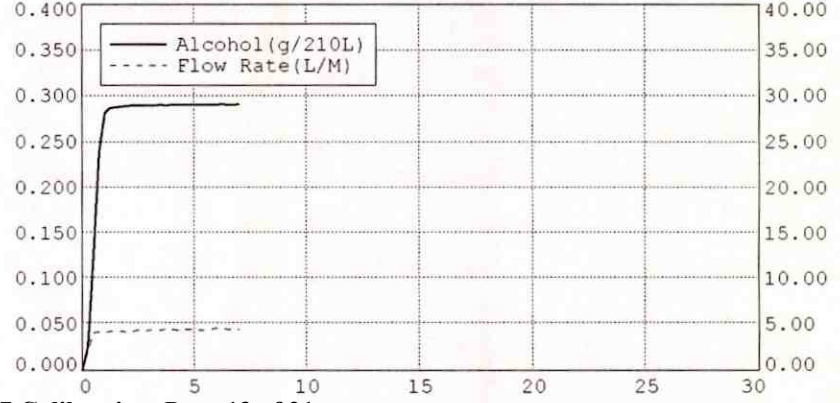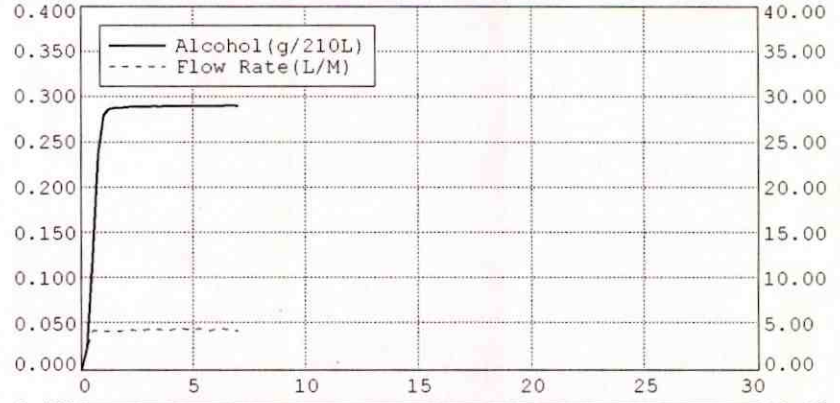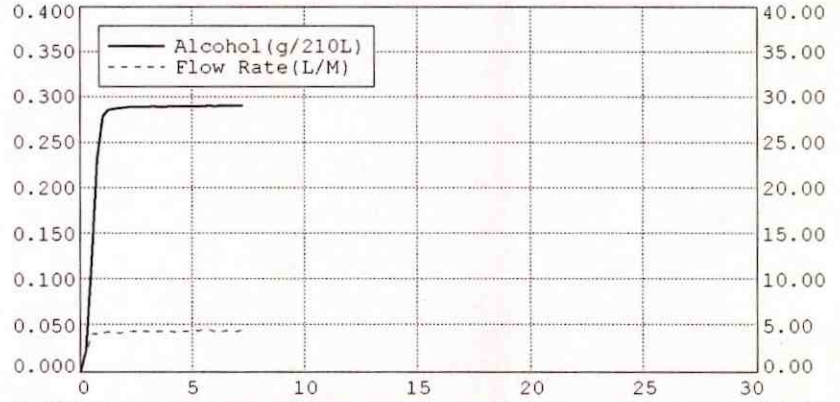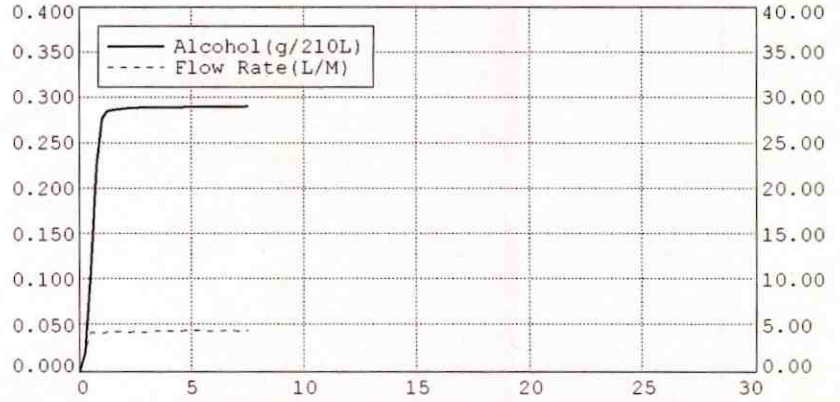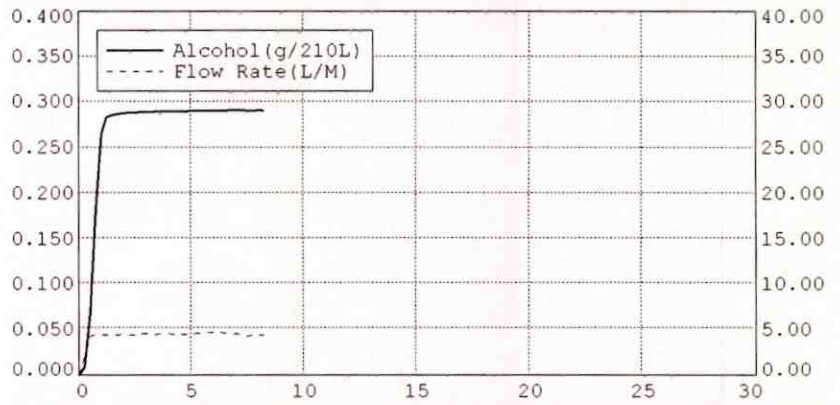

SUBJECT TEST

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100421  
 -----

Date: 09/26/2023  
 Time: 14:19:24

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX


OPERATOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

DEPT/AGENCY:  
 INCOMPLETE  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080 Lot # AG-310901 <sup>0.065</sup> 9/26/23  
 TARGET AT 29.29: 0.078 Exp: 4/19/25

DIAGNOSTIC CHECK PASSED 14:24  
 BLANK TEST 0.000 14:24  
 INTERNAL STANDARD VERIFIED 14:24  
 EXTERNAL STANDARD 0.079 14:24  
 BLANK TEST 0.000 14:25  
 SUBJECT SAMPLE INCOMPLETE 14:28

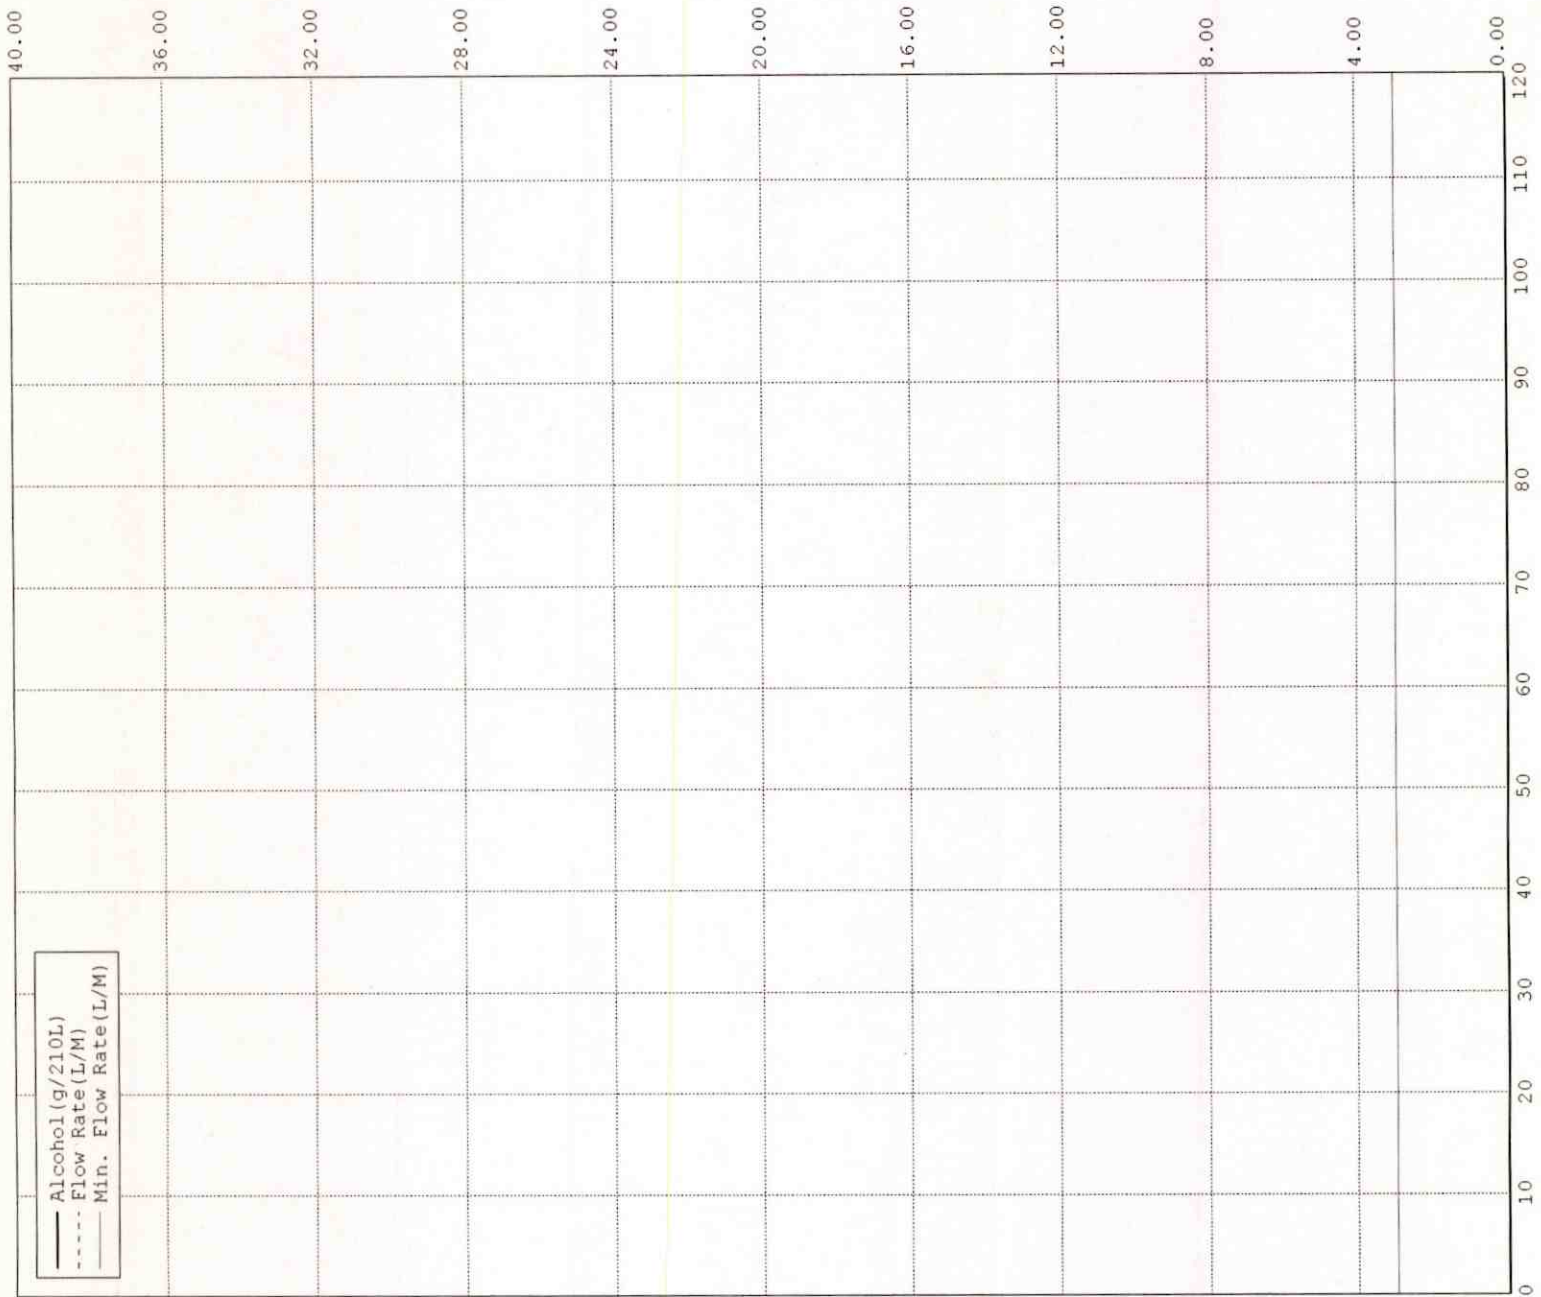

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100421

Date: 09/26/2023

Time: 14:31:26

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

MAXIMUM ATTEMPTS EXCEEDED

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080 Lot # *AK-310901*

TARGET AT 29.29: 0.078 Exp: *4/19/25*

DIAGNOSTIC CHECK

PASSED 14:32

BLANK TEST

0.000 14:33

INTERNAL STANDARD

VERIFIED 14:33

EXTERNAL STANDARD

0.078 14:33


BLANK TEST

0.000 14:34

SUBJECT SAMPLE

XXX 14:34

Maximum Attempts Exceeded

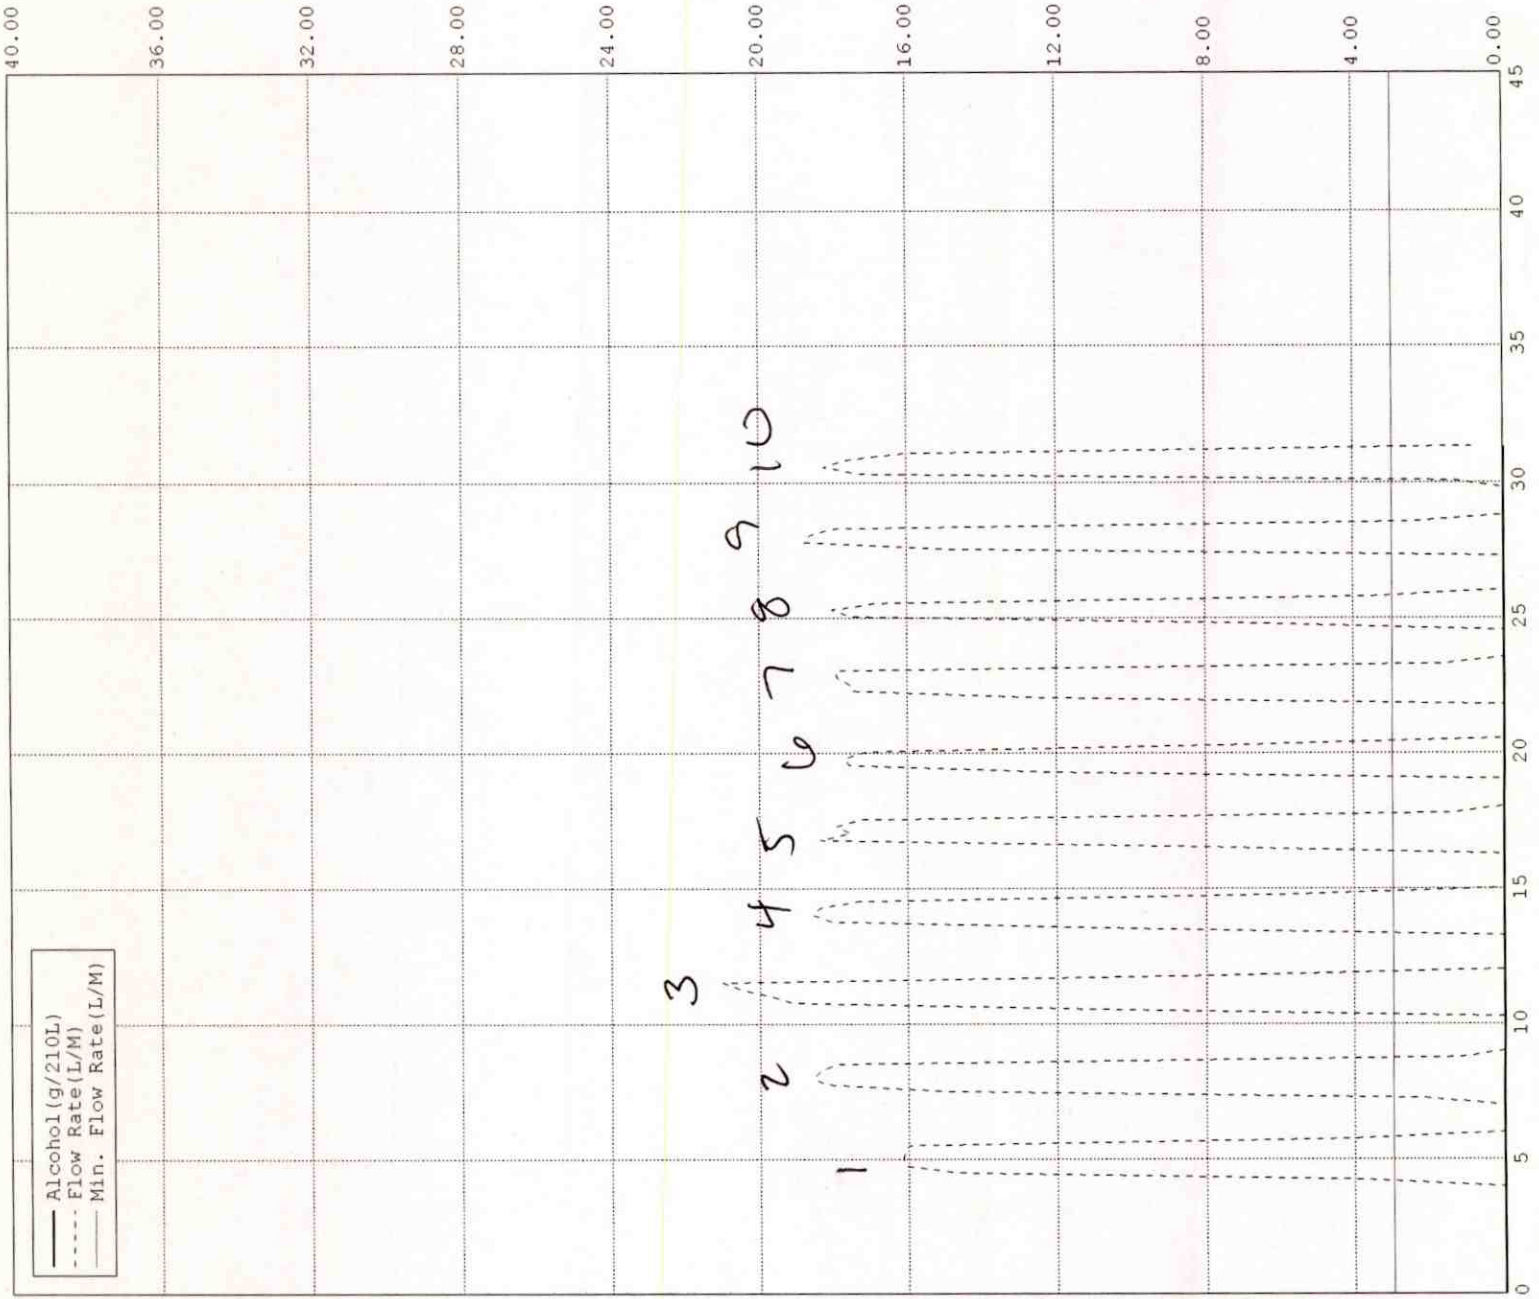

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100421

Date: 09/26/2023  
Time: 15:15:58


SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INVALID  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.29: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	15:17
BLANK TEST	0.000	15:17
INTERNAL STANDARD	VERIFIED	15:17
EXTERNAL STANDARD	0.078	15:17
BLANK TEST	0.000	15:18
SUBJECT SAMPLE	INVALID	15:19

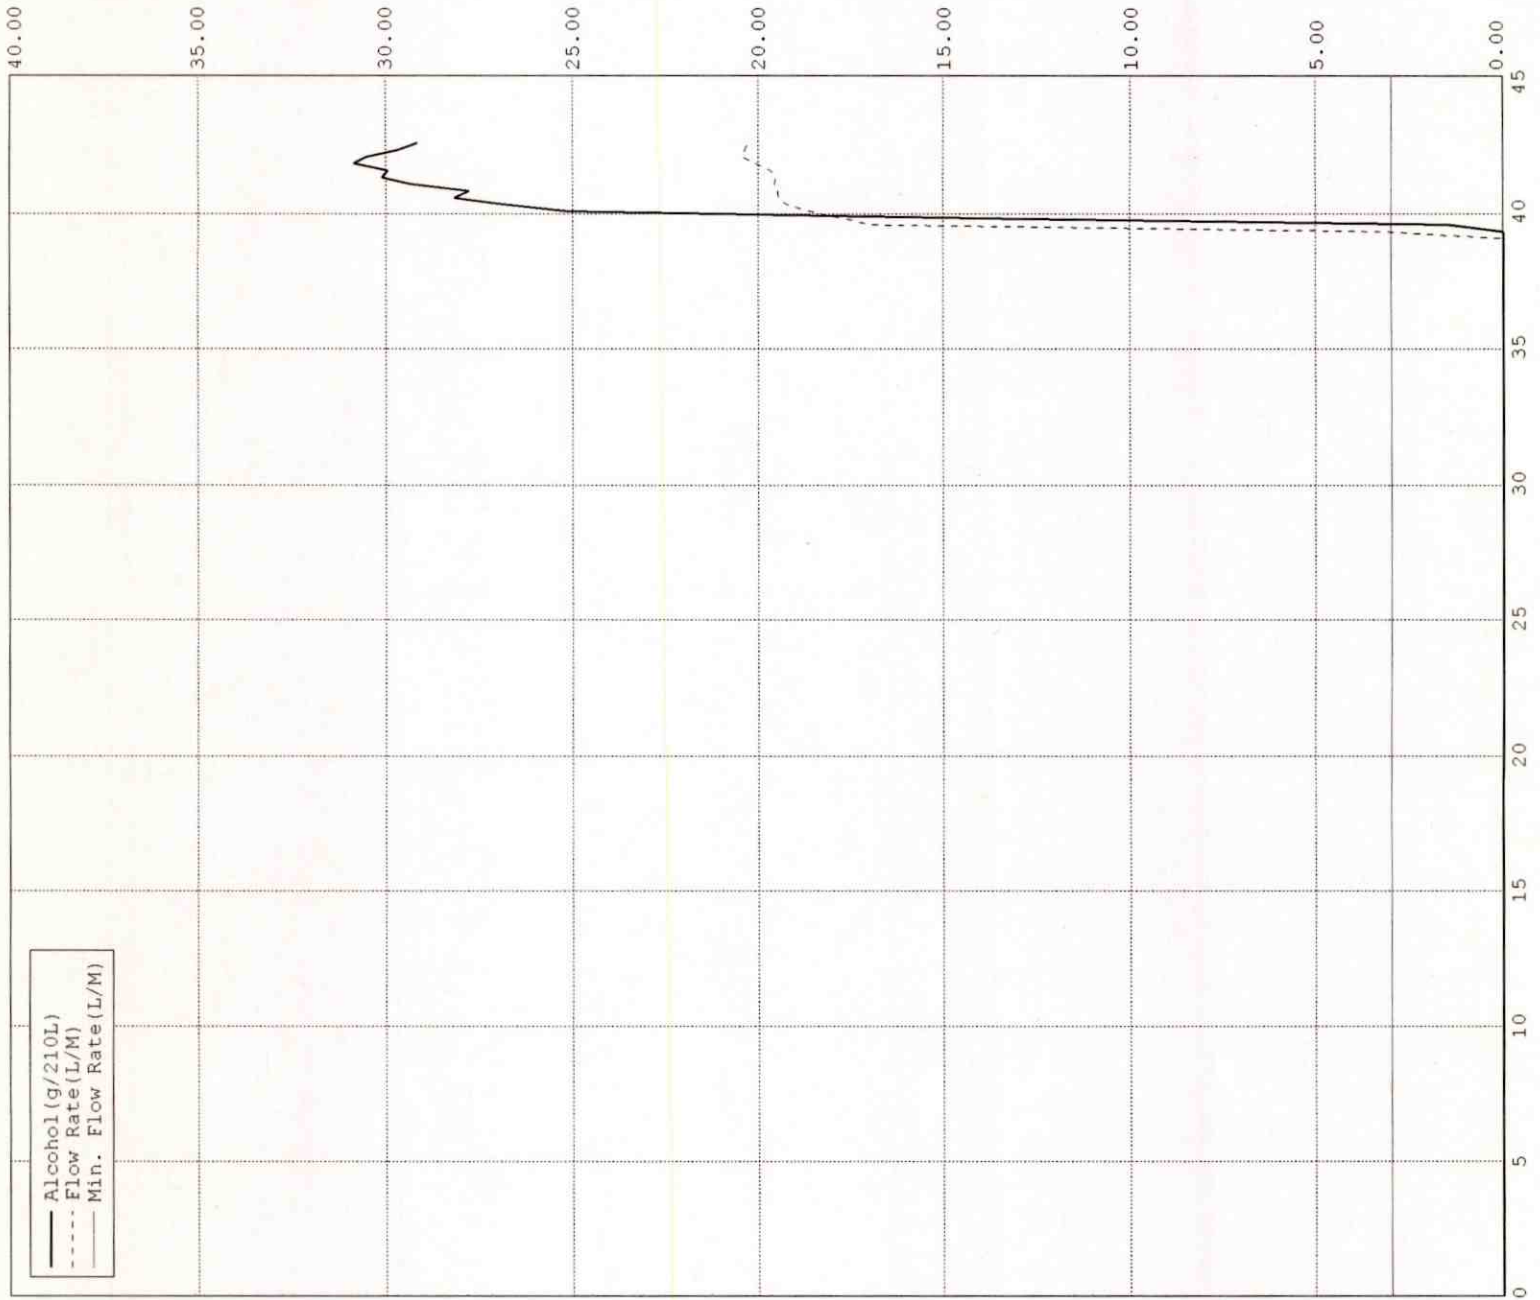



SUBJECT TEST

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100421  
 -----

Date: 09/26/2023  
 Time: 14:44:56

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX


OPERATOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

DEPT/AGENCY:  
 RFI  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.29: 0.078  
 LOT #: AG310901  
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK  
 BLANK TEST PASSED 14:46  
 INTERNAL STANDARD 0.000 14:46  
 EXTERNAL STANDARD VERIFIED 14:46  
 BLANK TEST 0.077 14:46  
 0.000 14:47

RFI DETECTED

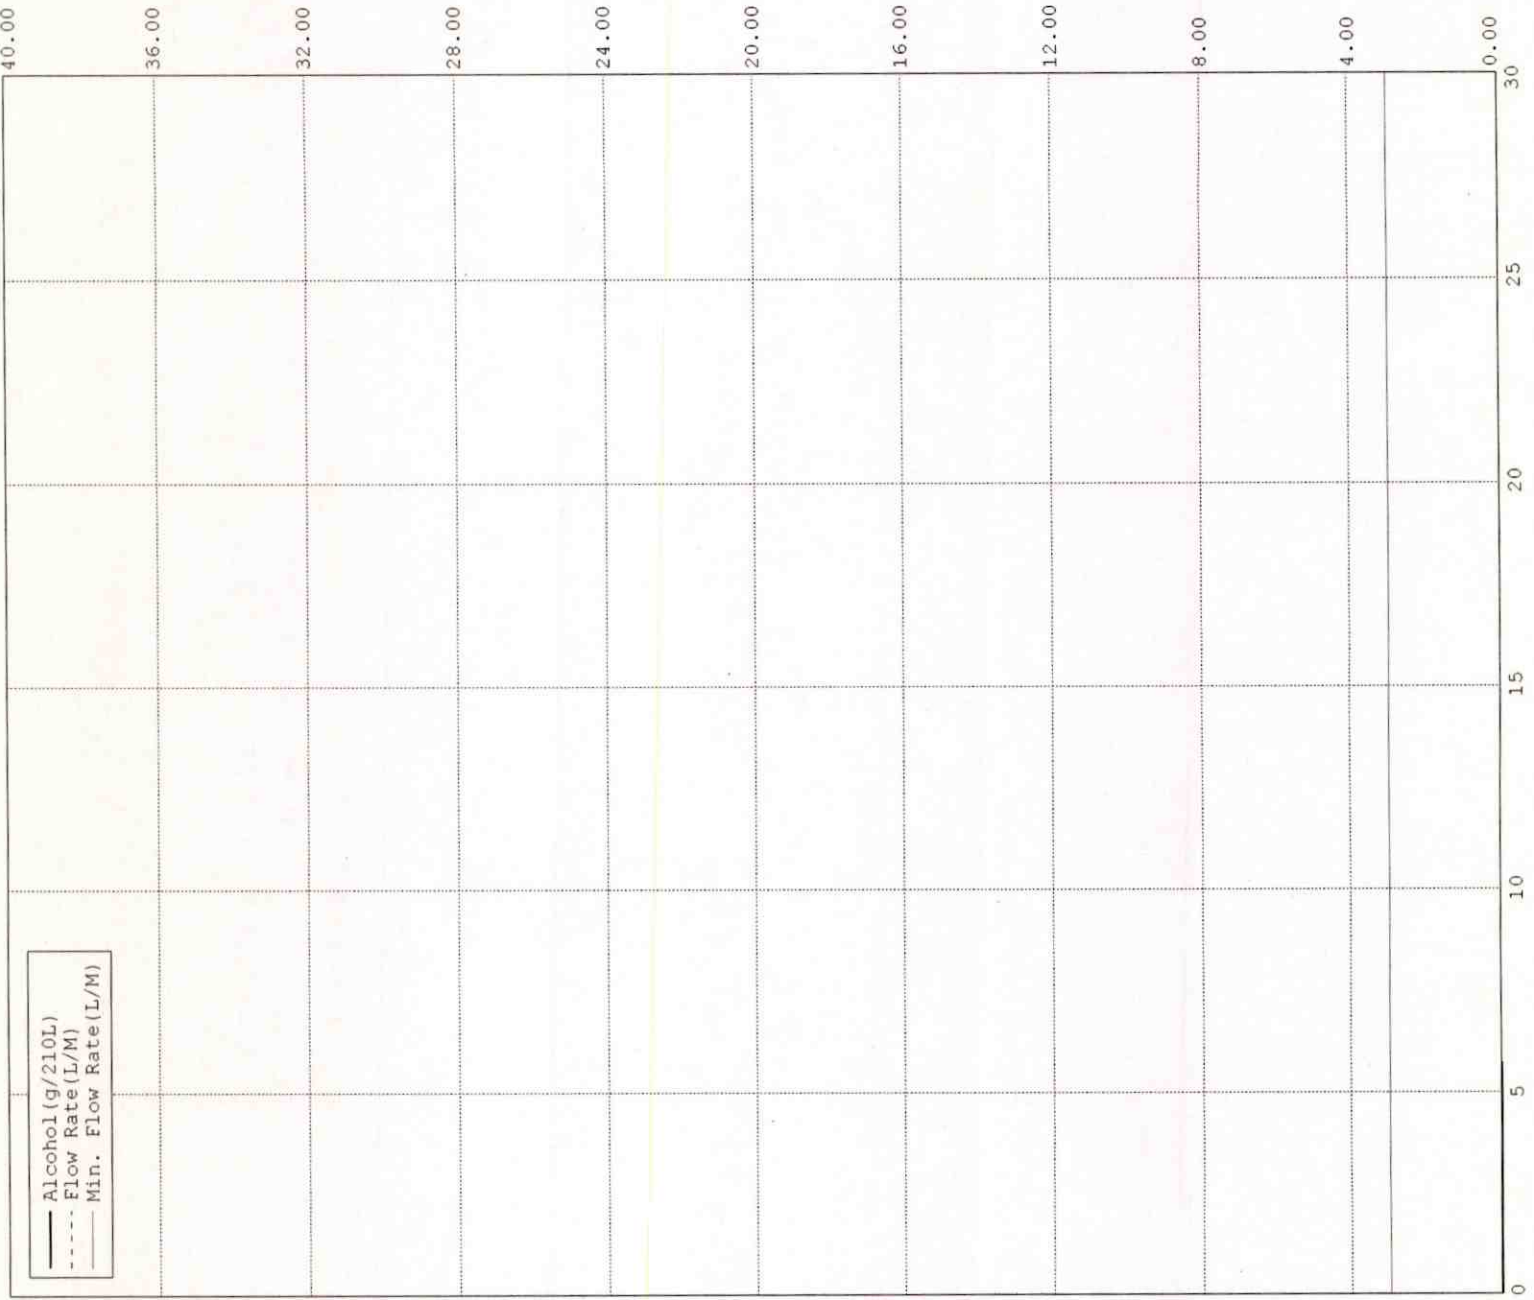

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100421

Date: 09/26/2023

Time: 15:38:03

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INTERFERENCE - ACETONE

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.28: 0.078

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 15:39

BLANK TEST 0.000 15:39

INTERNAL STANDARD VERIFIED 15:39

Xq = 0.098 (1.00%)

EXTERNAL STANDARD 0.076 15:39

X[1] = 0.0765 (-0.0005) (0.0015)

BLANK TEST 0.000 15:40

SUBJECT SAMPLE XXX 15:41


X[1] = 0.1106 (-0.0182) (0.0008)

Interference Detected

Filter 2 Average = 0.0008

Filter 3 Average = 0.0014

CVG 9/27/23

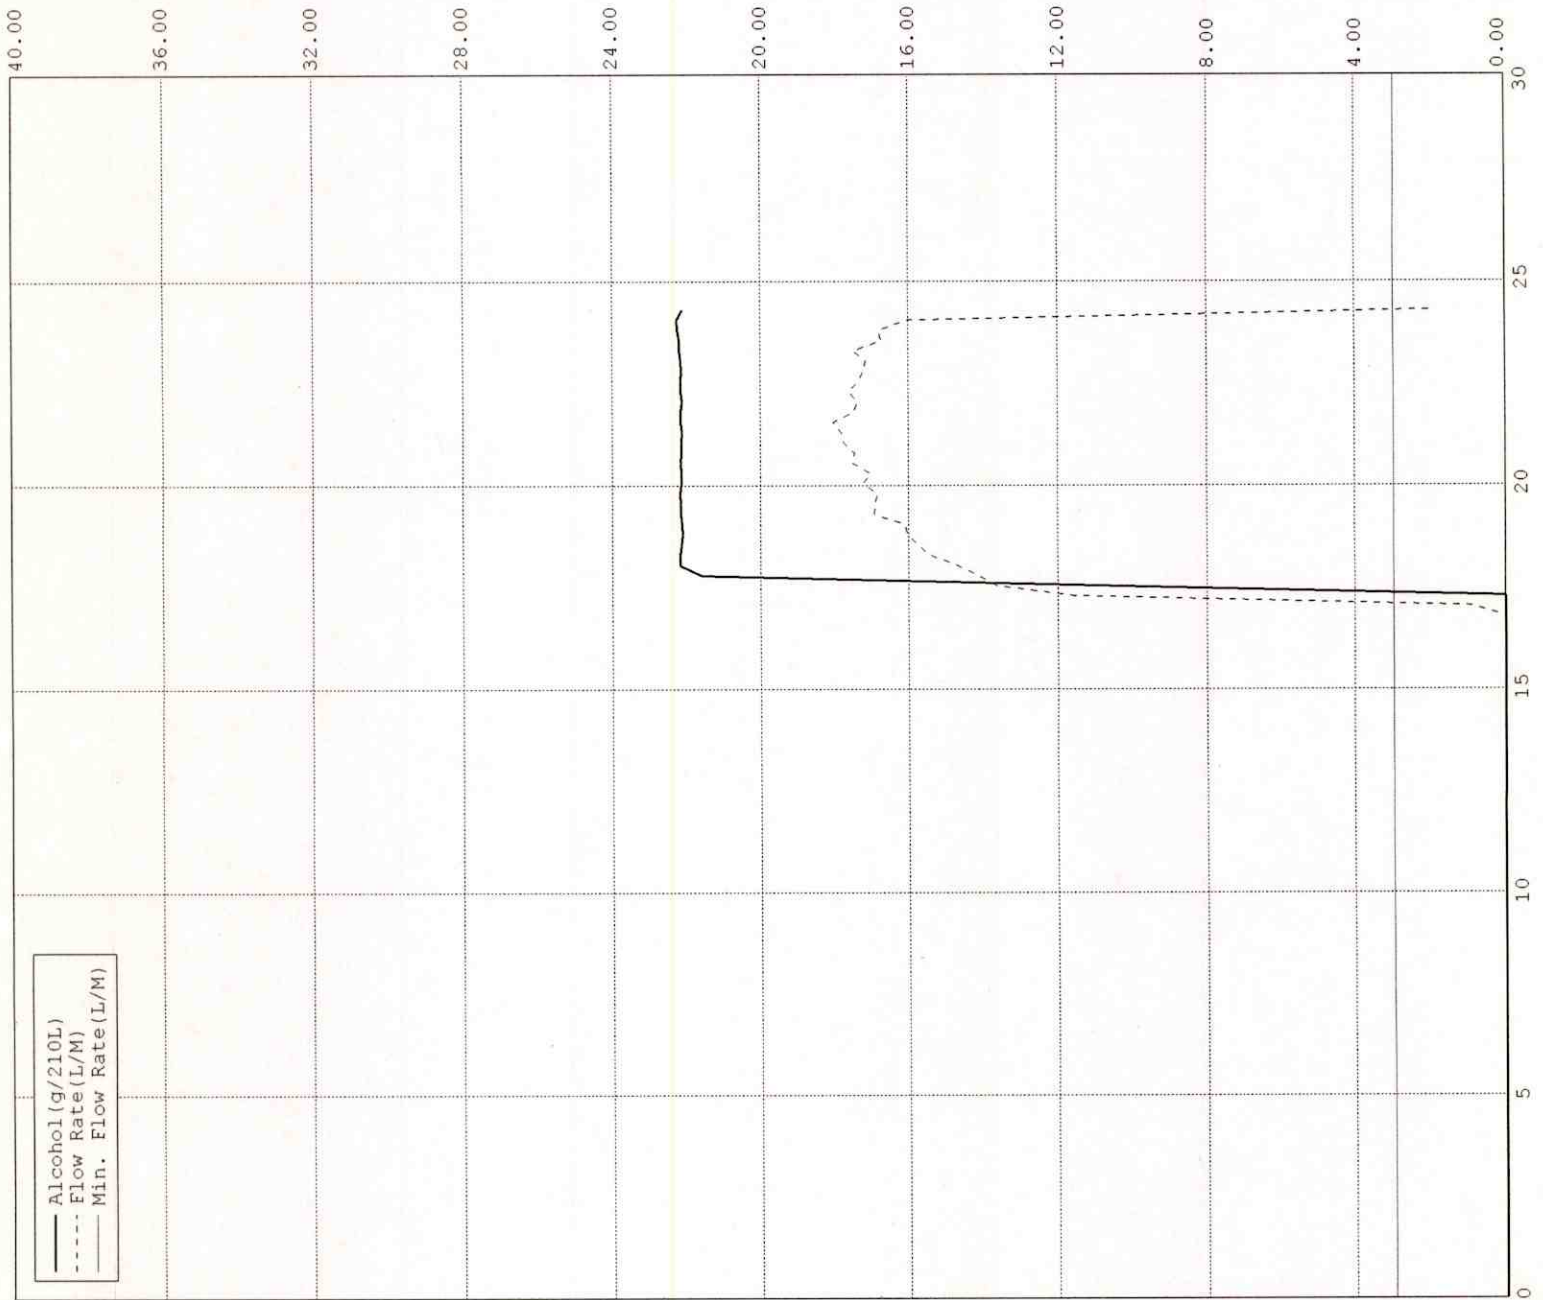

SUBJECT TEST

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100421  
 -----

Date: 09/26/2023  
 Time: 15:31:44

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX  
 OPERATOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436


DEPT/AGENCY:  
 INTERFERENCE - IPA  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.28: 0.078  
 LOT #: AG310901  
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	15:32
BLANK TEST	0.000	15:33
INTERNAL STANDARD	VERIFIED	15:33
Xq = 0.099 (2.45%)	0.077	15:33
EXTERNAL STANDARD	0.000	15:34
X[1] = 0.0773 (0.0004)	0.000	15:35
BLANK TEST	XXX	15:35
SUBJECT SAMPLE	X[1] = 0.1210 (-0.0231)	(0.0019)

Interference Detected

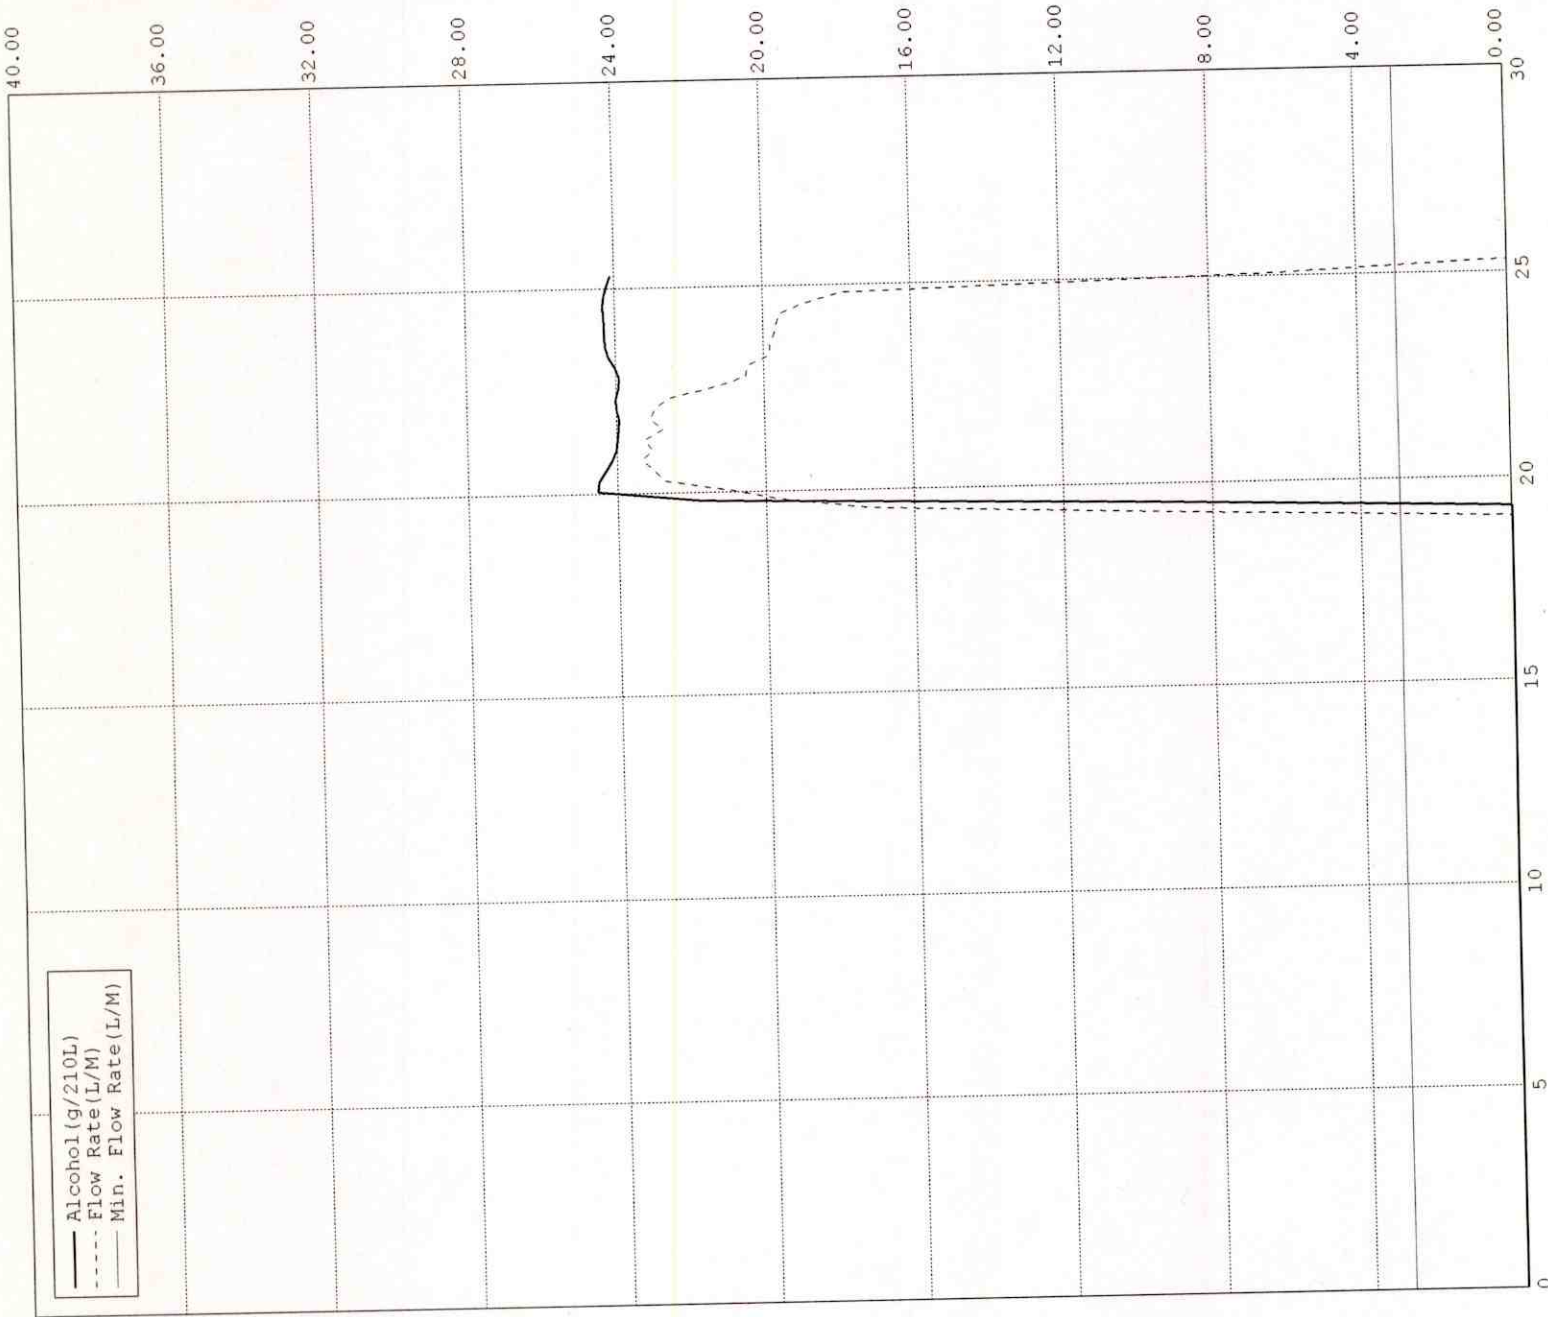

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100421  
-----

Date: 09/26/2023  
Time: 15:22:41

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE - NEGATIVE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.29: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	15:24
BLANK TEST	0.000	15:24
INTERNAL STANDARD	VERIFIED	15:24
Xq = 0.098 (1.27%)	0.077	15:24
EXTERNAL STANDARD	X[1] = 0.0773 (0.0023)	(0.0013) 0.000 15:25
BLANK TEST	SUBJECT SAMPLE (Vol=1.96L)	0.095 15:27
X[1] = 0.0956 (0.0015)	(0.0009)	0.000 15:28
BLANK TEST	0.077	15:29
EXTERNAL STANDARD	X[1] = 0.0766 (0.0008)	(0.0010) 0.000 15:30
BLANK TEST	0.000	15:30

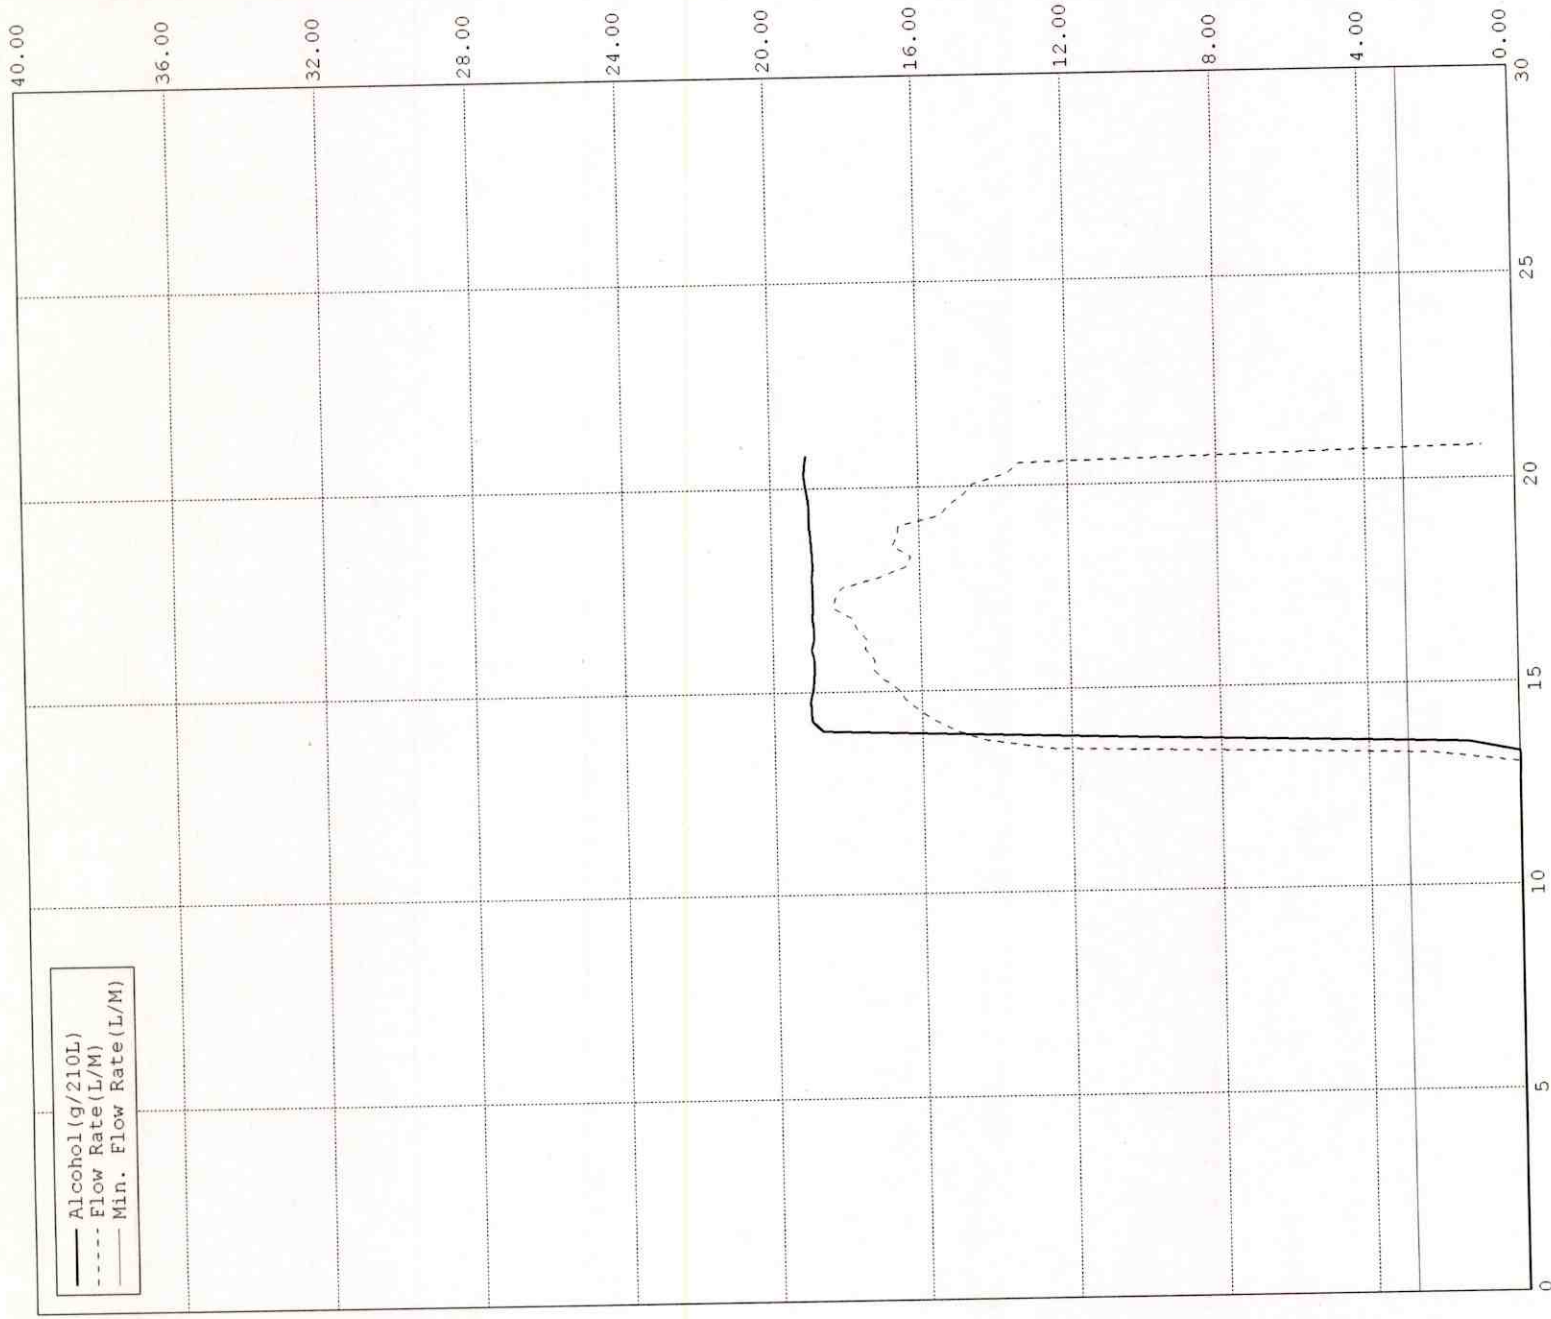

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100421

Date: 09/27/2023  
Time: 11:14:28

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.51: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	11:16
BLANK TEST	0.000	11:16
INTERNAL STANDARD	VERIFIED	11:16
EXTERNAL STANDARD	0.077	11:17
BLANK TEST	0.000	11:18
SUBJECT SAMPLE (Vol=2.10L)	0.000	11:18
BLANK TEST	0.000	11:19
EXTERNAL STANDARD	0.078	11:19
BLANK TEST	0.000	11:20

OKG

