



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100404

**Report Issue Date:** 03/29/2023  
**Date Received:** 2023-02-22  
**Condition of Item:** Good

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 02/22/2023** - As Found - **End Date 02/22/2023** As Found - Evaluation Analyst: Colleen O'Bryant  
 As Found Conditions - Barometric Pressure (inHg): 30.19 Barometer Used: Fisher S/N 221250180 Temperature (C): 21.6  
 Relative Humidity (%): 13

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.081	AG113402	0.080	0.080	0.079	0.080	0.080	0.080	0.080
0.300	0.305	AG217903	0.302	0.302	0.303	0.302	0.302	0.302	0.302

**Start Date 03/14/2023** - As Left - **End Date 03/14/2023**  
 As Left Conditions - Barometric Pressure (inHg): 29.26 Barometer Used: Fisher S/N 221250180 Temperature (C): 21.4 Relative Humidity (%): 4

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002	
0.040	0.039	AG217904	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003	
0.080	0.078	AG113402	0.078	0.077	0.078	0.078	0.078	0.078	+/- 0.003	
0.100	0.098	AG211003	0.098	0.097	0.098	0.098	0.098	0.098	+/- 0.003	
0.150	0.147	AG134205	0.147	0.147	0.147	0.147	0.147	0.147	+/- 0.004	
0.300	0.293	AG217903	0.294	0.294	0.293	0.293	0.293	0.293	+/- 0.008	

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Technically and administratively reviewed by Colleen O'Bryant on 03/29/2023

Results authorized by Derek Walton on 03/16/2023  
[derek.walton@alaska.gov](mailto:derek.walton@alaska.gov)

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100404 Analyst: Tatiana Malnoske Start Date: 03-14-2023

- Diagnostic Test (attached)
- Internal Standard value  $\leq$  3.00%
- Adjust voltages, if needed
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.6 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.26 Temperature (C): 21.4 Relative Humidity (%): 4%

Linearity Test (attached)

0.020g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG217A02</u>	Exp:	<u>06-28-2024</u>
0.040g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG217A04</u>	Exp:	<u>06-28-2024</u>
0.080g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG113402</u>	Exp:	<u>05-14-2023</u>
0.100g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG211003</u>	Exp:	<u>04-20-2024</u>
0.150g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG1134205</u>	Exp:	<u>12-08-2023</u>
0.300g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG217A03</u>	Exp:	<u>06-28-2024</u>

Functional Tests (attached)

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles)
- Acetone Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11-09-2023  
Simulator S/N: DK4161 Verification Performed?
- Isopropanol Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11-09-2023  
Simulator S/N: JD1088 Verification Performed?
- Neg. Control Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11-09-2023  
Simulator S/N: JD1177 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11-09-2023

- Verify stylus is calibrated
- Non-Drinking Subject Test
- Reset Options
- Upload
- Clear Memory
- Remove Tank Prior to Shutdown
- Verification of Calibration (VOC)
- Calibration End Date: 03-14-2023

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100404  
-----

Date: 03/14/2023  
Time: 07:41:02

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.0°C                    PASSED  
(44.0°C - 52.0°C)  
Breath Tube       = 46.1°C                PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage     = 1.77 V                PASSED  
(1.06 V - 2.48 V)  
Cooler Voltage   = 1.73 V                PASSED  
(1.01 V - 2.35 V)  
Bias Voltage     = 82 V                    PASSED  
(49 V - 115 V)  
Chopper Freq    = 535 Hz                    PASSED  
(475 Hz - 575 Hz)  
Barometer        = 29.5 in

PUMP INFO

Flow Rate = 4.525 L/M                    PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON                                    PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF                                  PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1                                   PASSED  
Filter 2                                   PASSED  
Filter 3                                   PASSED

INTERNAL STANDARD

Xq = 0.090 0.98% (0.00% - 4.00%)      PASSED

Technician Screen

-----  
DATAMASTER dmt: 100404  
-----

Date: 03/14/2023  
Time: 7:55 AM

Temperatures (°C)

Sample Cell: 49.0°C  
Breath Tube: 47.4°C

Current Barometer 29.3 in  
Volume (Ltr) 1.51

Settings

Lamp: 1.85 V  
Bias: 82 V  
Cooler: 1.68 V  
Chopper: 534 Hz

Voltages (V)

Flow: 1.06 V  
Detector: 0.026 V



CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100404  
-----

Date: 05/18/2011  
Time: 14:02:44

OPERATOR NAME:  
COLLEEN S OBRYANT  
CERTIFICATE #: 6237

LOT #: GUTH100  
BOTTLE #: 10260  
EXPIRATION: 01/01/2012

Ca = 0.1000  
CAL = 0.970035    0.800 <= CAL < 1.200  
b1 = 0.0005    0.0000 <= b1 < 0.0040  
b2 = 0.0071    0.0010 <= b2 < 0.0100  
b3 = 0.0001    0.0000 <= b3 < 0.0040  
Xq = 0.0888    0.0500 <= Xq < 0.2000  
a21 = 1.183100    1.050 <= a21 < 1.300  
a31 = 0.434619    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100404

Date: 03/14/2023  
Time: 07:56:27

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
MINIMUM VOLUME TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.26: 0.078  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	07:57
BLANK TEST	0.000	07:57
INTERNAL STANDARD	VERIFIED	07:57
EXTERNAL STANDARD	0.077	07:57
BLANK TEST	0.000	07:58
SUBJECT SAMPLE (Vol=1.60L)	0.000	08:00
BLANK TEST	0.000	08:00
EXTERNAL STANDARD	0.078	08:01
BLANK TEST	0.000	08:02

TLM

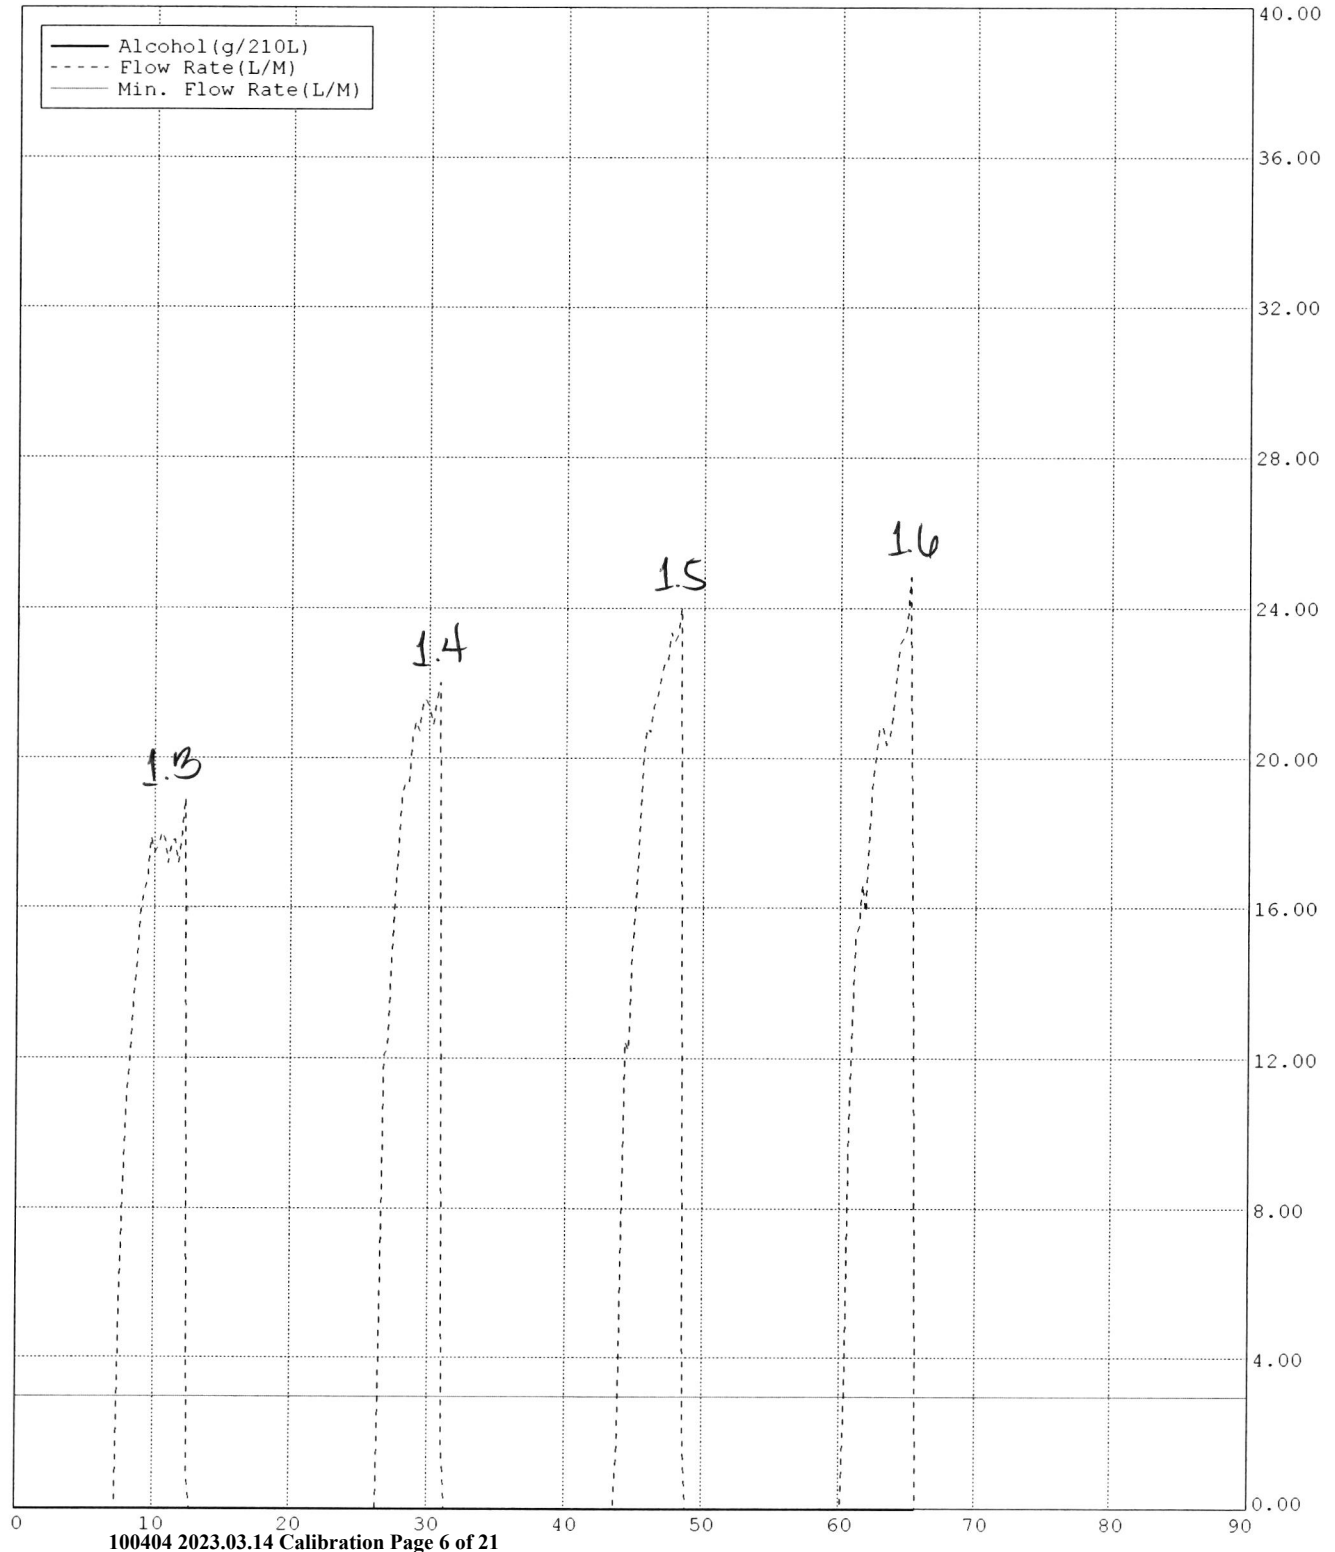

LINEARITY CHECK

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100404  
-----


Date: 03/14/2023  
Time: 08:12:16

SUPERVISOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.039	0.0390	0.0000
0.078	0.0778	0.0004
0.098	0.0978	0.0004
0.147	0.1470	0.0000
0.293	0.2934	0.0005

SLOPE = 1.001669  
R<sup>2</sup> = 0.999998

TLM

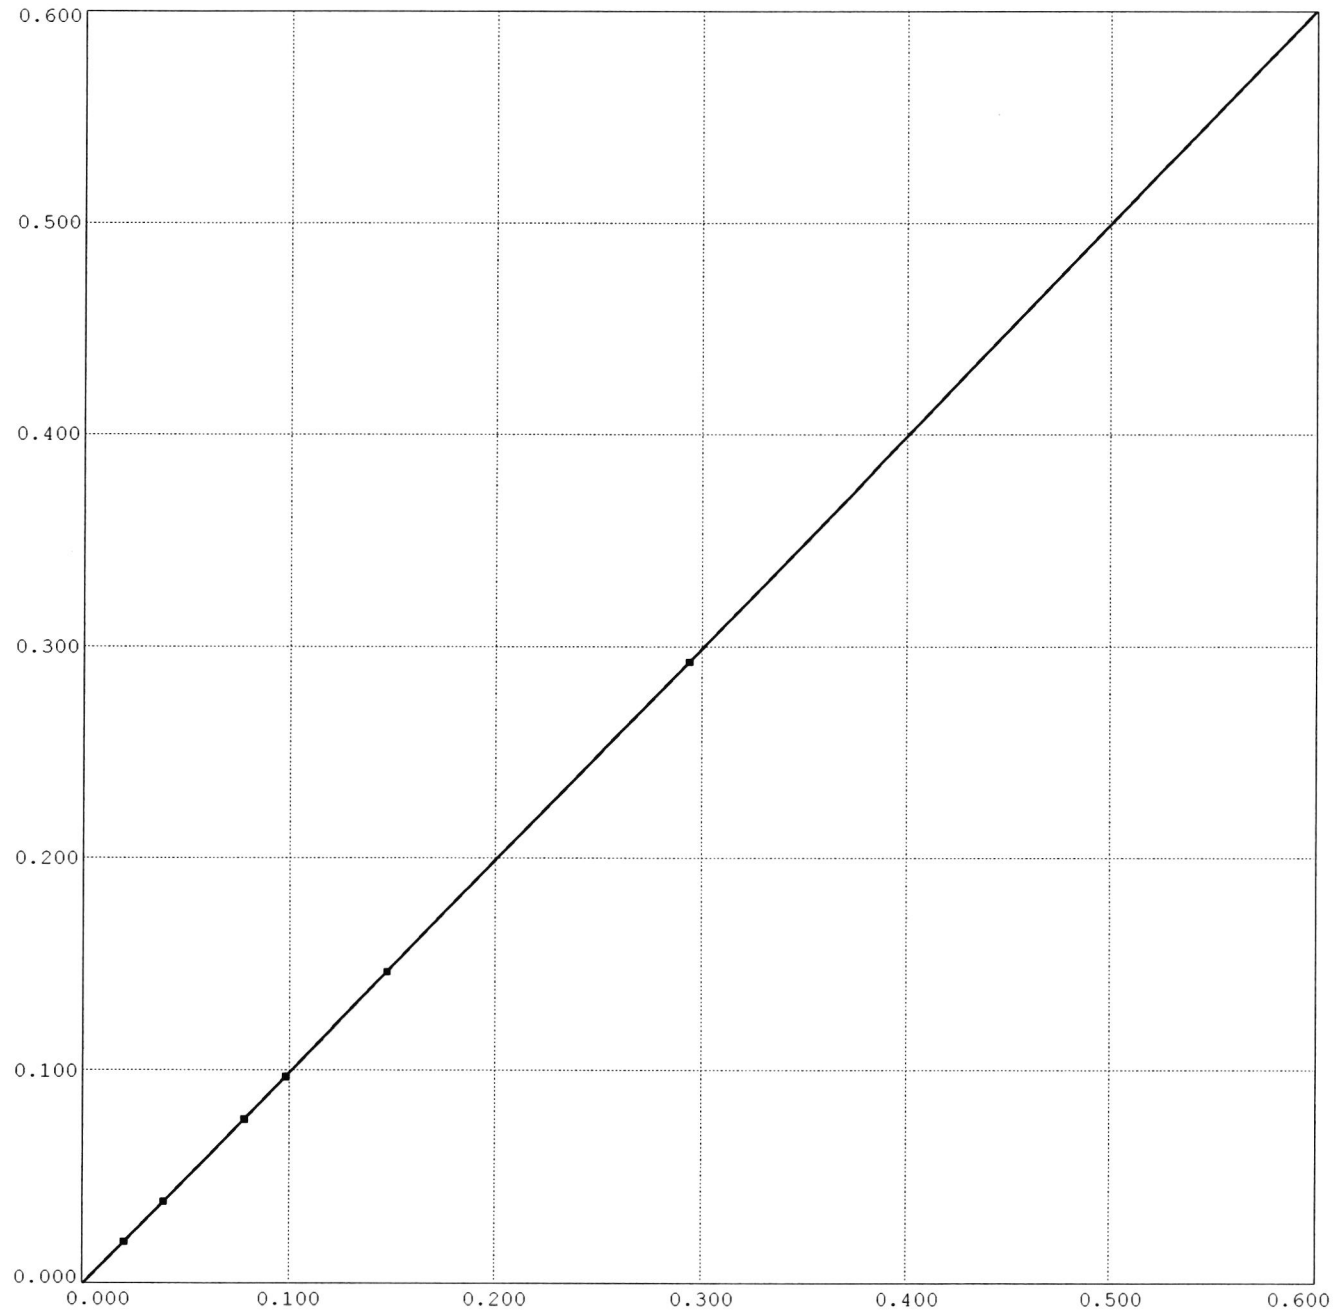

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100404






Date: 03/14/2023  
Time: 08:12:18

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.25: 0.020  
LOT #: AG217902  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 1173 psi

BLANK TEST	0.000	08:13
INTERNAL STANDARD	VERIFIED	08:13
EXTERNAL STANDARD	0.020	08:14
BLANK TEST	0.000	08:15
EXTERNAL STANDARD	0.020	08:15
BLANK TEST	0.000	08:16
EXTERNAL STANDARD	0.020	08:16
BLANK TEST	0.000	08:17
EXTERNAL STANDARD	0.020	08:17
BLANK TEST	0.000	08:18
EXTERNAL STANDARD	0.020	08:18
BLANK TEST	0.000	08:19

Average = 0.0200  
Std Dev = 0.0000

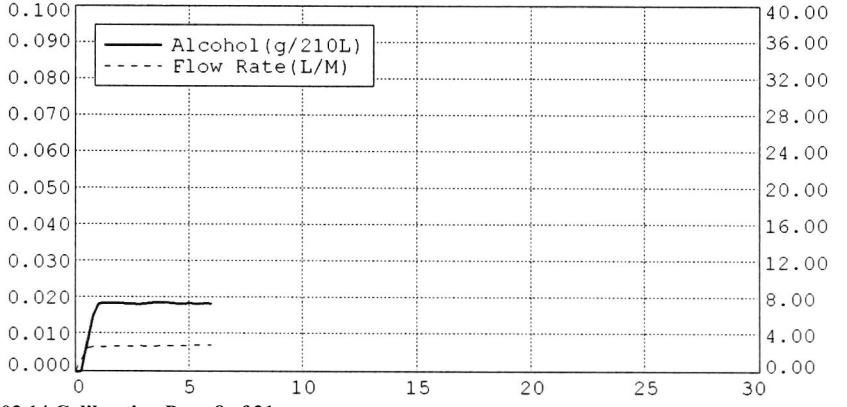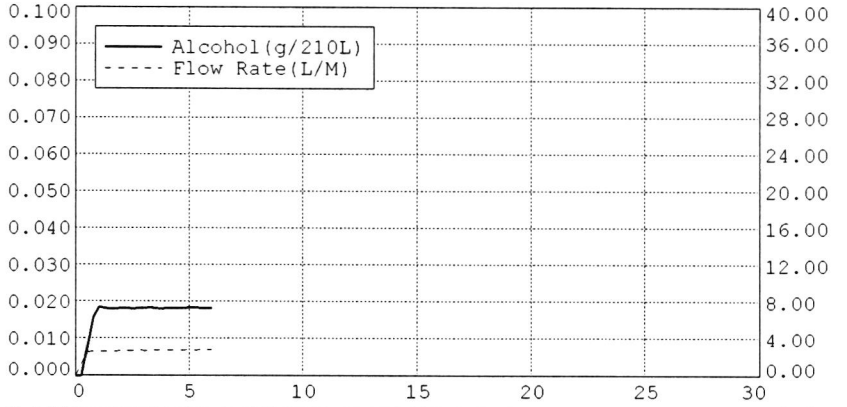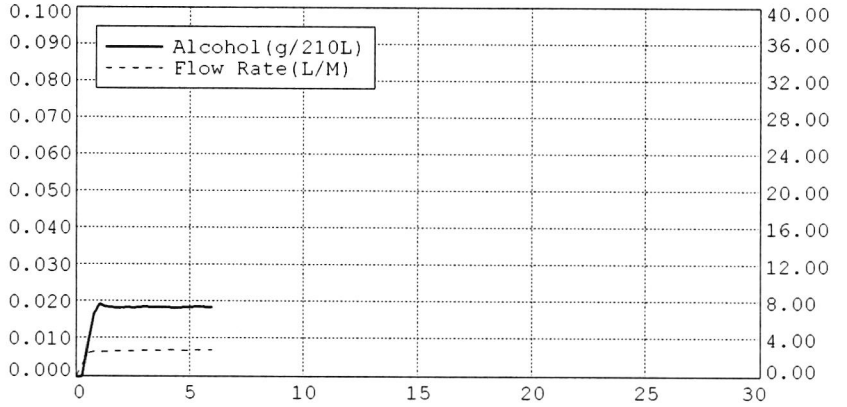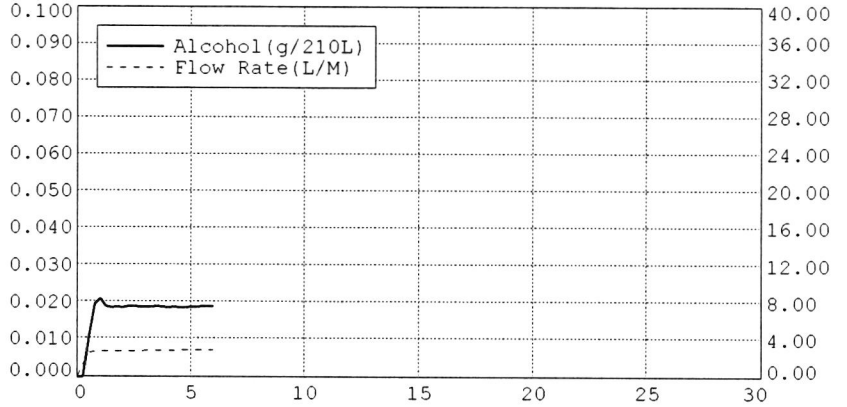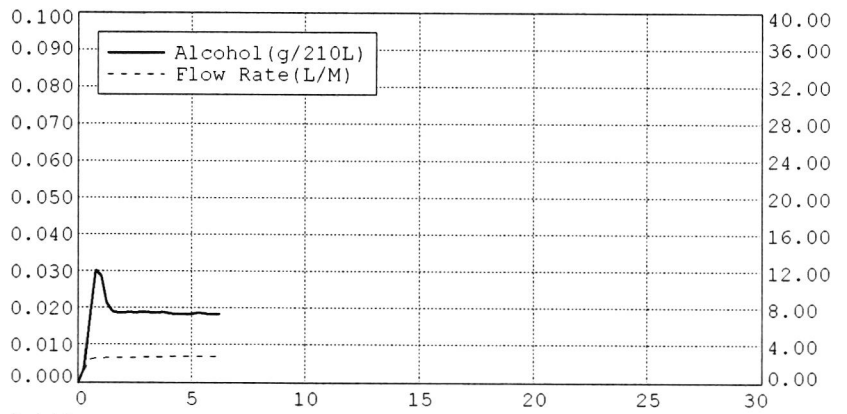

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100404






Date: 03/14/2023  
 Time: 08:19:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.25: 0.039  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 1116 psi

BLANK TEST	0.000	08:21
INTERNAL STANDARD	VERIFIED	08:21
EXTERNAL STANDARD	0.039	08:21
BLANK TEST	0.000	08:22
EXTERNAL STANDARD	0.039	08:22
BLANK TEST	0.000	08:23
EXTERNAL STANDARD	0.039	08:23
BLANK TEST	0.000	08:24
EXTERNAL STANDARD	0.039	08:24
BLANK TEST	0.000	08:25
EXTERNAL STANDARD	0.039	08:25
BLANK TEST	0.000	08:26

Average = 0.0390  
 Std Dev = 0.0000

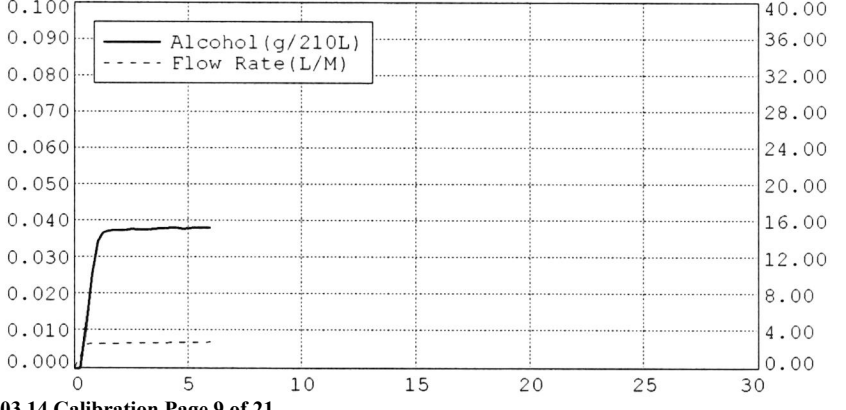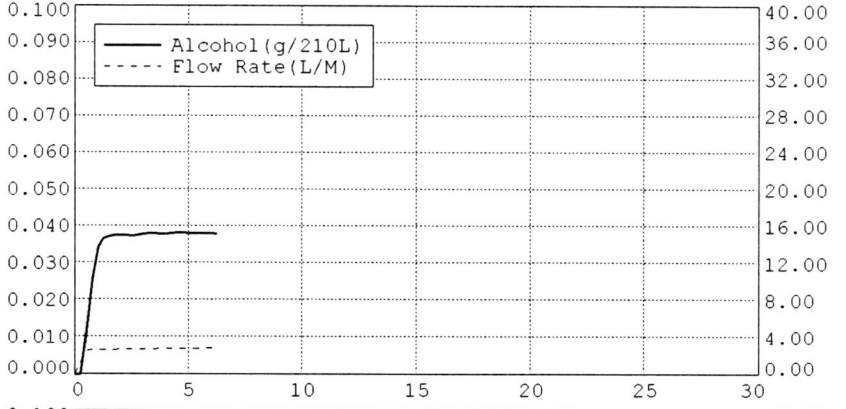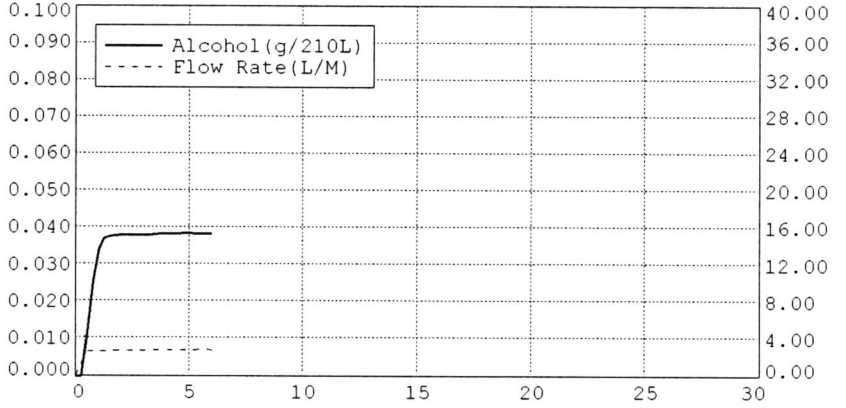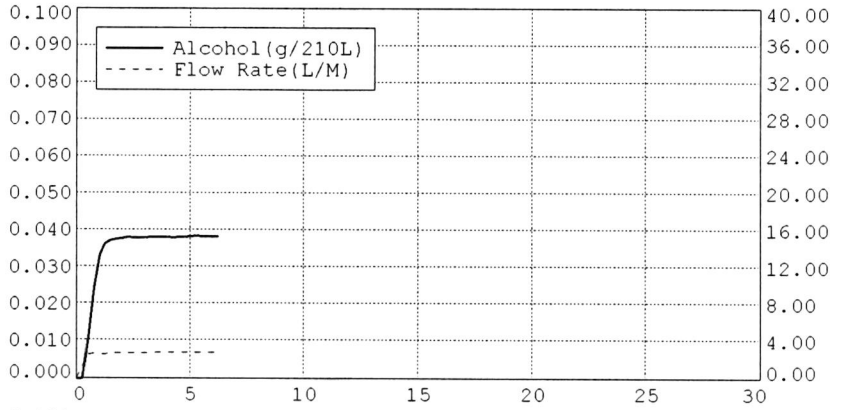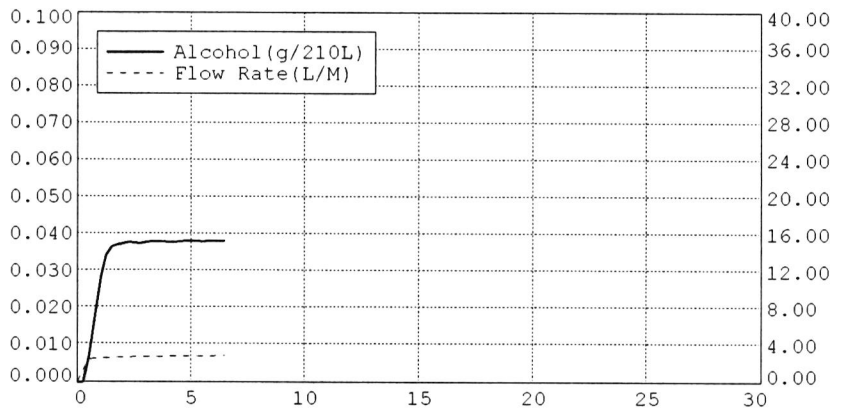

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100404






Date: 03/14/2023  
 Time: 08:28:05

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.26: 0.078  
 LOT #: AG113402  
 EXPIRATION: 05/14/2023  
 TANK PRESSURE: 441 psi

BLANK TEST	0.000	08:29
INTERNAL STANDARD	VERIFIED	08:29
EXTERNAL STANDARD	0.078	08:30
BLANK TEST	0.000	08:30
EXTERNAL STANDARD	0.077	08:31
BLANK TEST	0.000	08:32
EXTERNAL STANDARD	0.078	08:32
BLANK TEST	0.000	08:33
EXTERNAL STANDARD	0.078	08:33
BLANK TEST	0.000	08:34
EXTERNAL STANDARD	0.078	08:34
BLANK TEST	0.000	08:35

Average = 0.0778  
 Std Dev = 0.0004

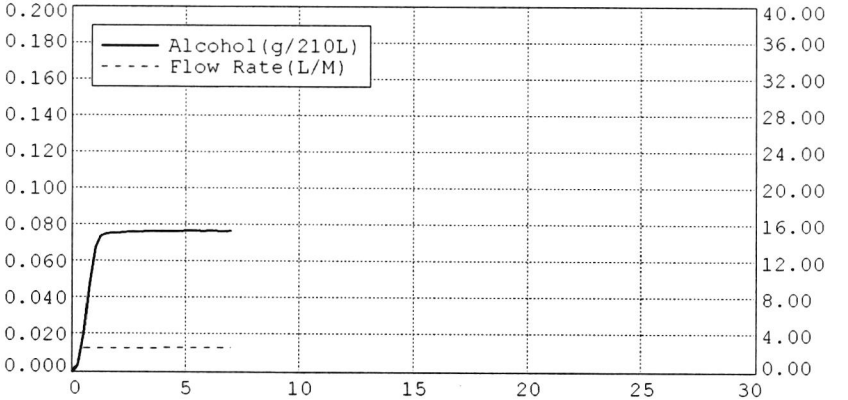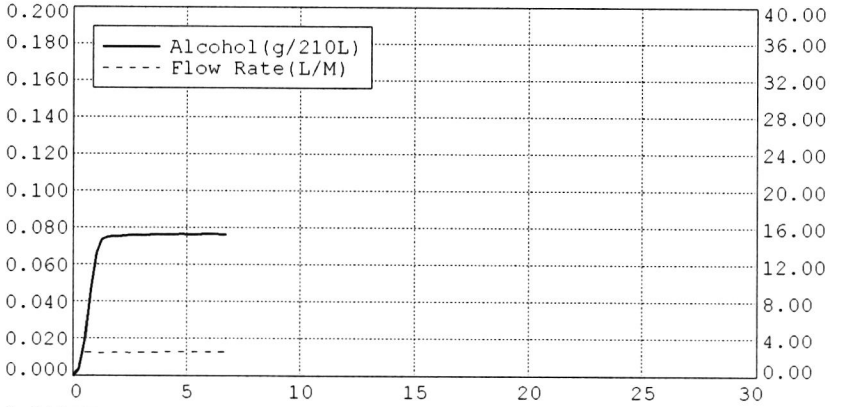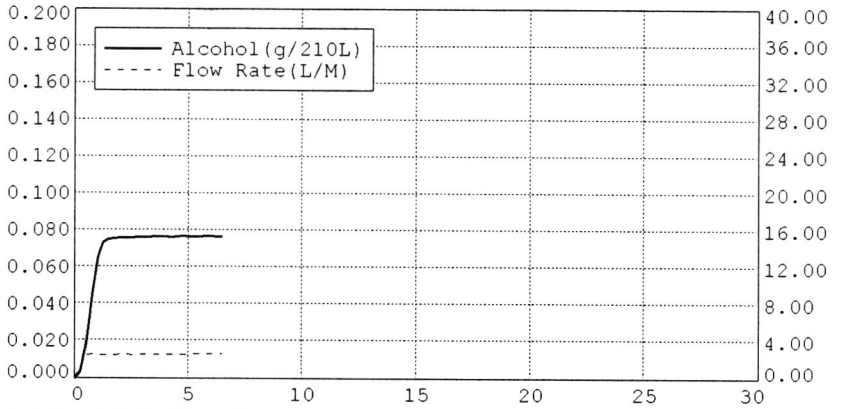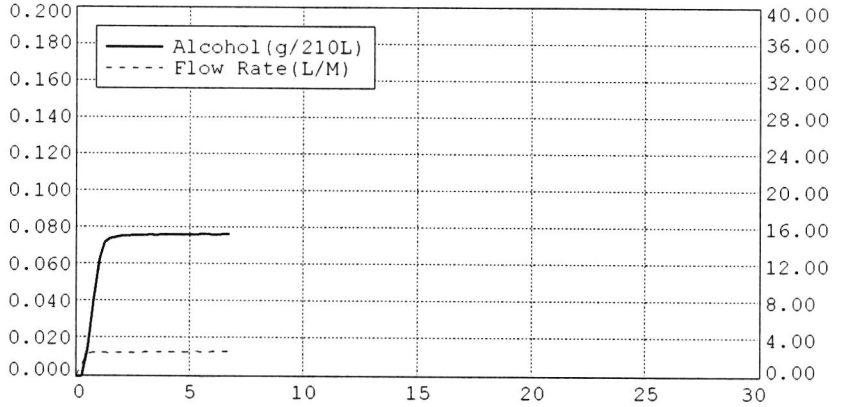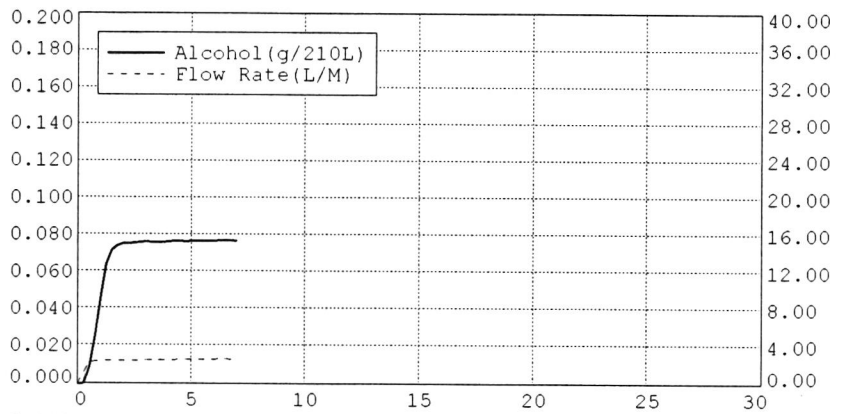



LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100404






Date: 03/14/2023  
 Time: 08:35:50

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.26: 0.098  
 LOT #: AG211003  
 EXPIRATION: 04/20/2024  
 TANK PRESSURE: 999 psi

BLANK TEST	0.000	08:37
INTERNAL STANDARD	VERIFIED	08:37
EXTERNAL STANDARD	0.098	08:37
BLANK TEST	0.000	08:38
EXTERNAL STANDARD	0.097	08:38
BLANK TEST	0.000	08:39
EXTERNAL STANDARD	0.098	08:39
BLANK TEST	0.000	08:40
EXTERNAL STANDARD	0.098	08:41
BLANK TEST	0.000	08:41
EXTERNAL STANDARD	0.098	08:42
BLANK TEST	0.000	08:43

Average = 0.0978  
 Std Dev = 0.0004

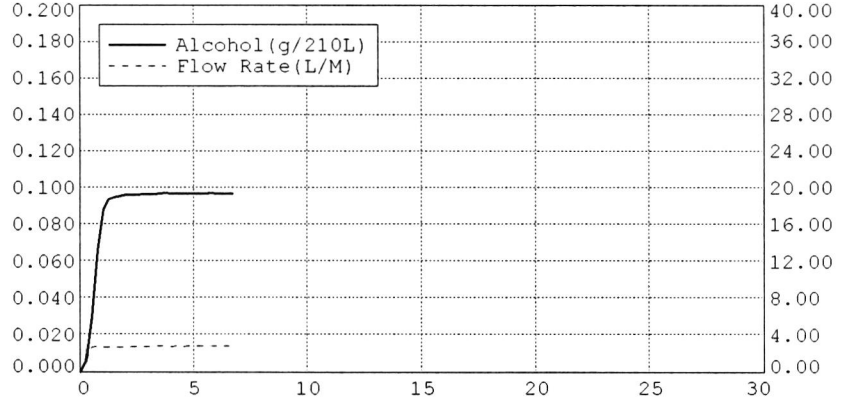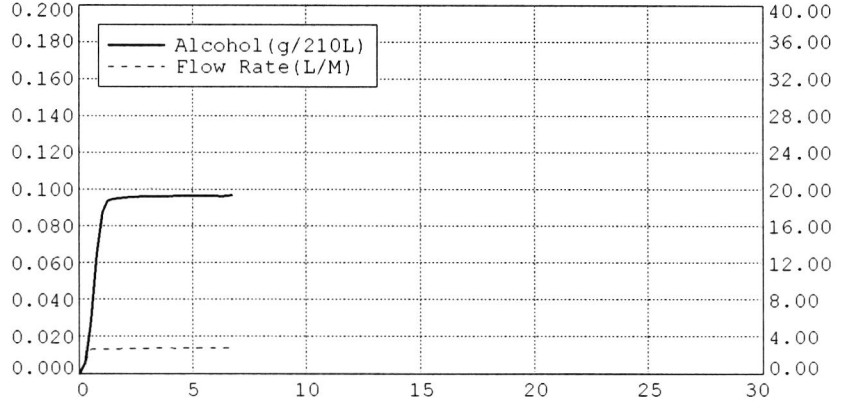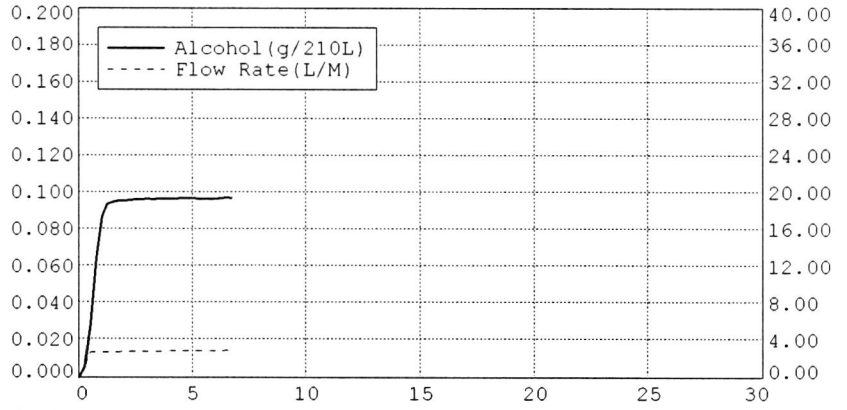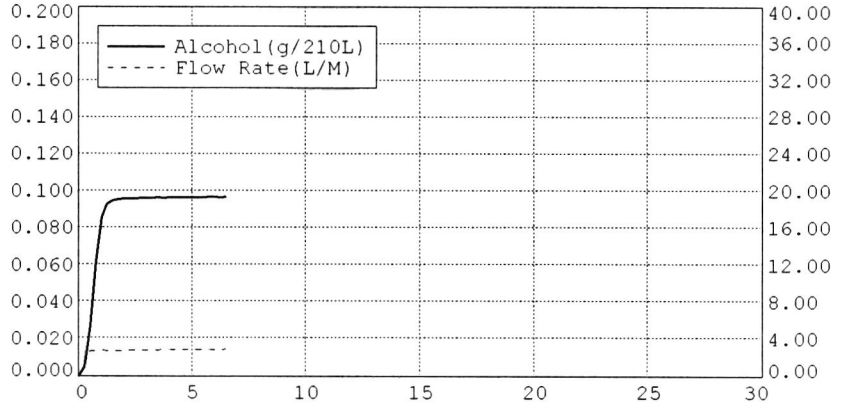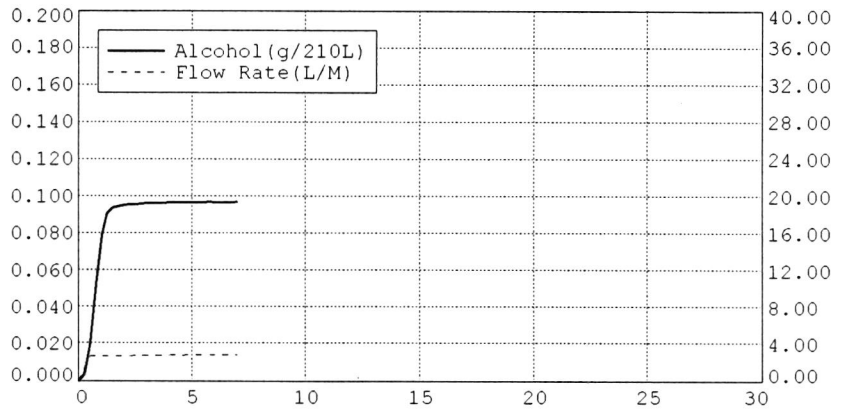

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
DATAMASTER dmt: 100404






Date: 03/14/2023  
Time: 08:43:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
TARGET AT 29.26: 0.147  
LOT #: AG134205  
EXPIRATION: 12/08/2023  
TANK PRESSURE: 1025 psi

BLANK TEST	0.000	08:45
INTERNAL STANDARD	VERIFIED	08:45
EXTERNAL STANDARD	0.147	08:45
BLANK TEST	0.000	08:46
EXTERNAL STANDARD	0.147	08:46
BLANK TEST	0.000	08:47
EXTERNAL STANDARD	0.147	08:47
BLANK TEST	0.000	08:48
EXTERNAL STANDARD	0.147	08:48
BLANK TEST	0.000	08:49
EXTERNAL STANDARD	0.147	08:49
BLANK TEST	0.000	08:50

Average = 0.1470  
Std Dev = 0.0000

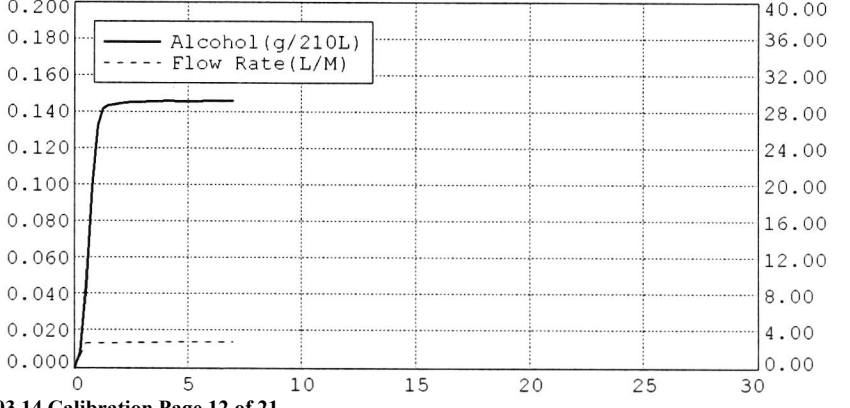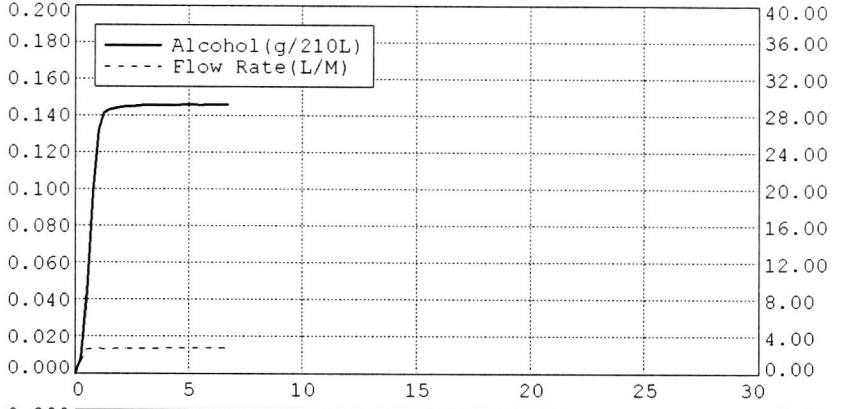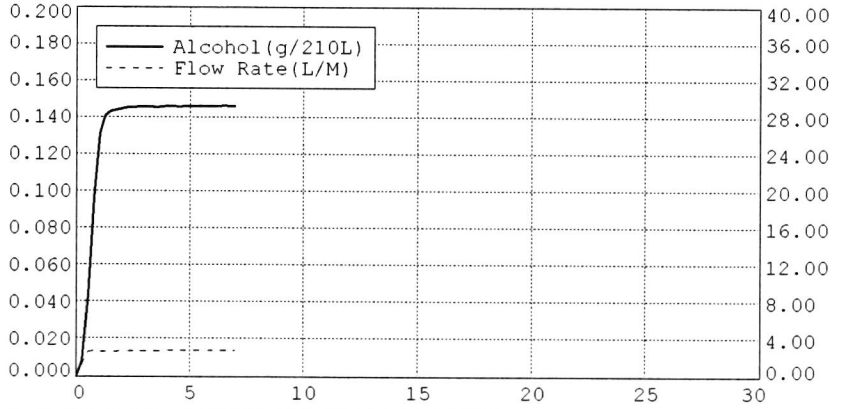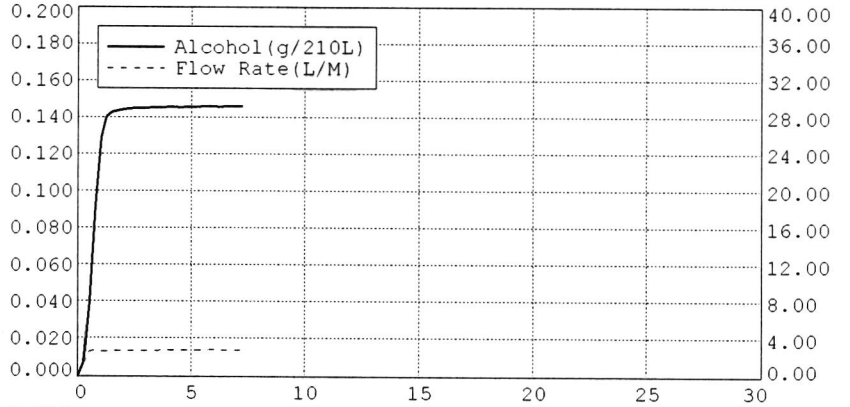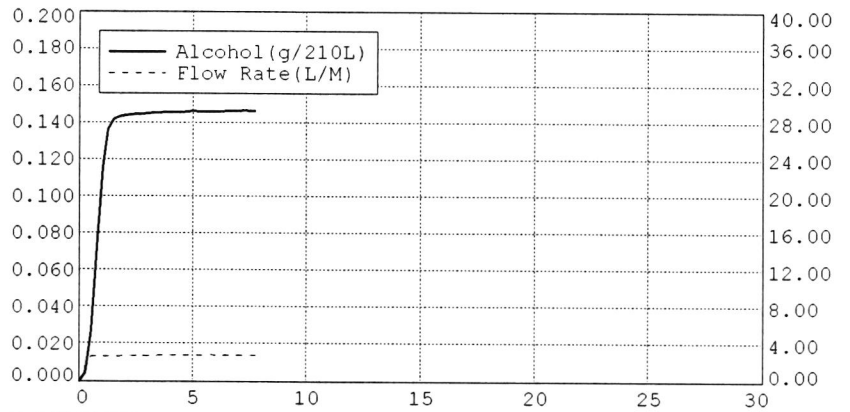

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100404






Date: 03/14/2023  
 Time: 08:51:50

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.26: 0.293  
 LOT #: AG217903  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 281 psi

BLANK TEST	0.000	08:53
INTERNAL STANDARD	VERIFIED	08:53
EXTERNAL STANDARD	0.294	08:53
BLANK TEST	0.000	08:54
EXTERNAL STANDARD	0.294	08:54
BLANK TEST	0.000	08:55
EXTERNAL STANDARD	0.293	08:55
BLANK TEST	0.000	08:56
EXTERNAL STANDARD	0.293	08:57
BLANK TEST	0.000	08:57
EXTERNAL STANDARD	0.293	08:58
BLANK TEST	0.000	08:59

Average = 0.2934  
 Std Dev = 0.0005

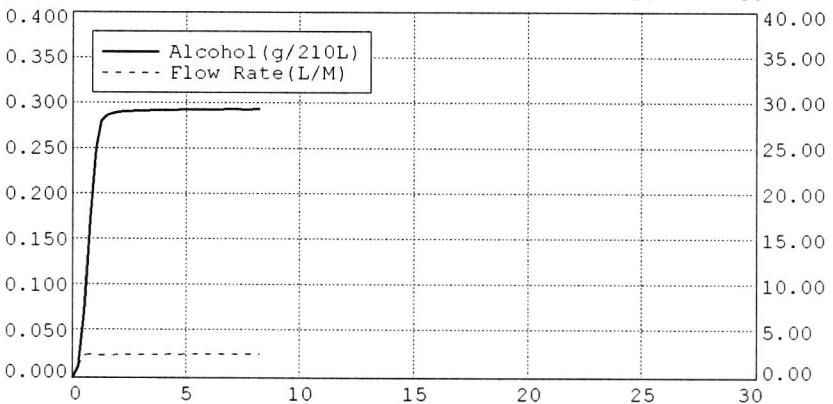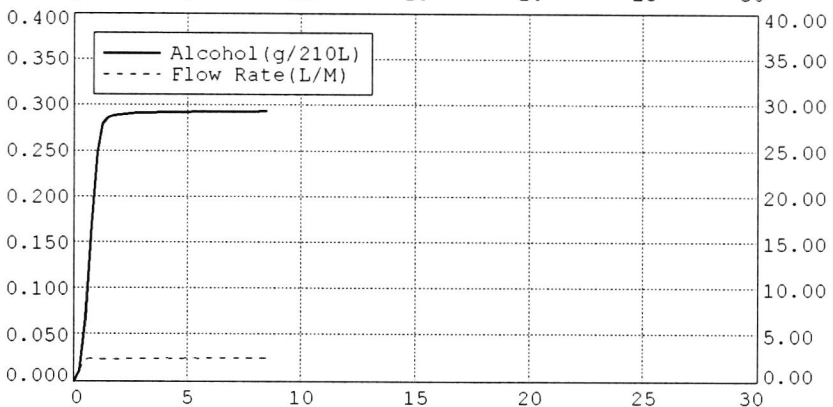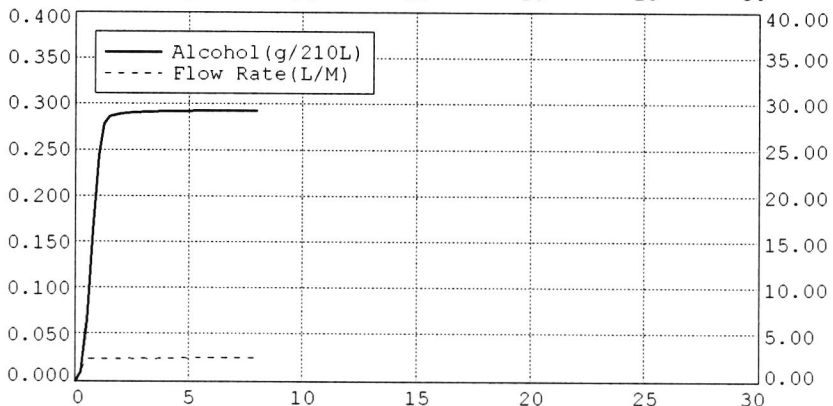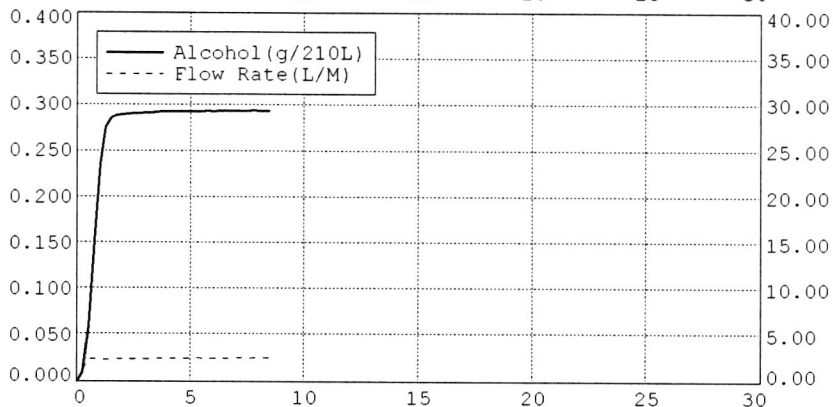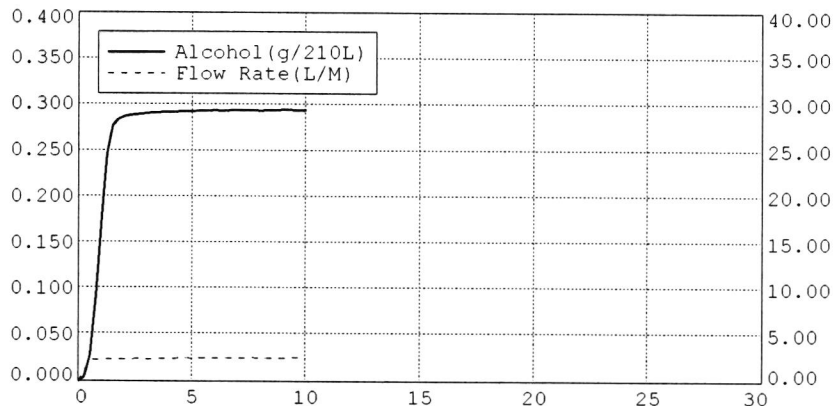

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100404  
-----

Date: 03/14/2023  
Time: 09:11:20

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.26: 0.078  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:12
BLANK TEST	0.000	09:12
INTERNAL STANDARD	VERIFIED	09:12
EXTERNAL STANDARD	0.078	09:12
BLANK TEST	0.000	09:13
SUBJECT SAMPLE	INCOMPLETE	09:15

TLM

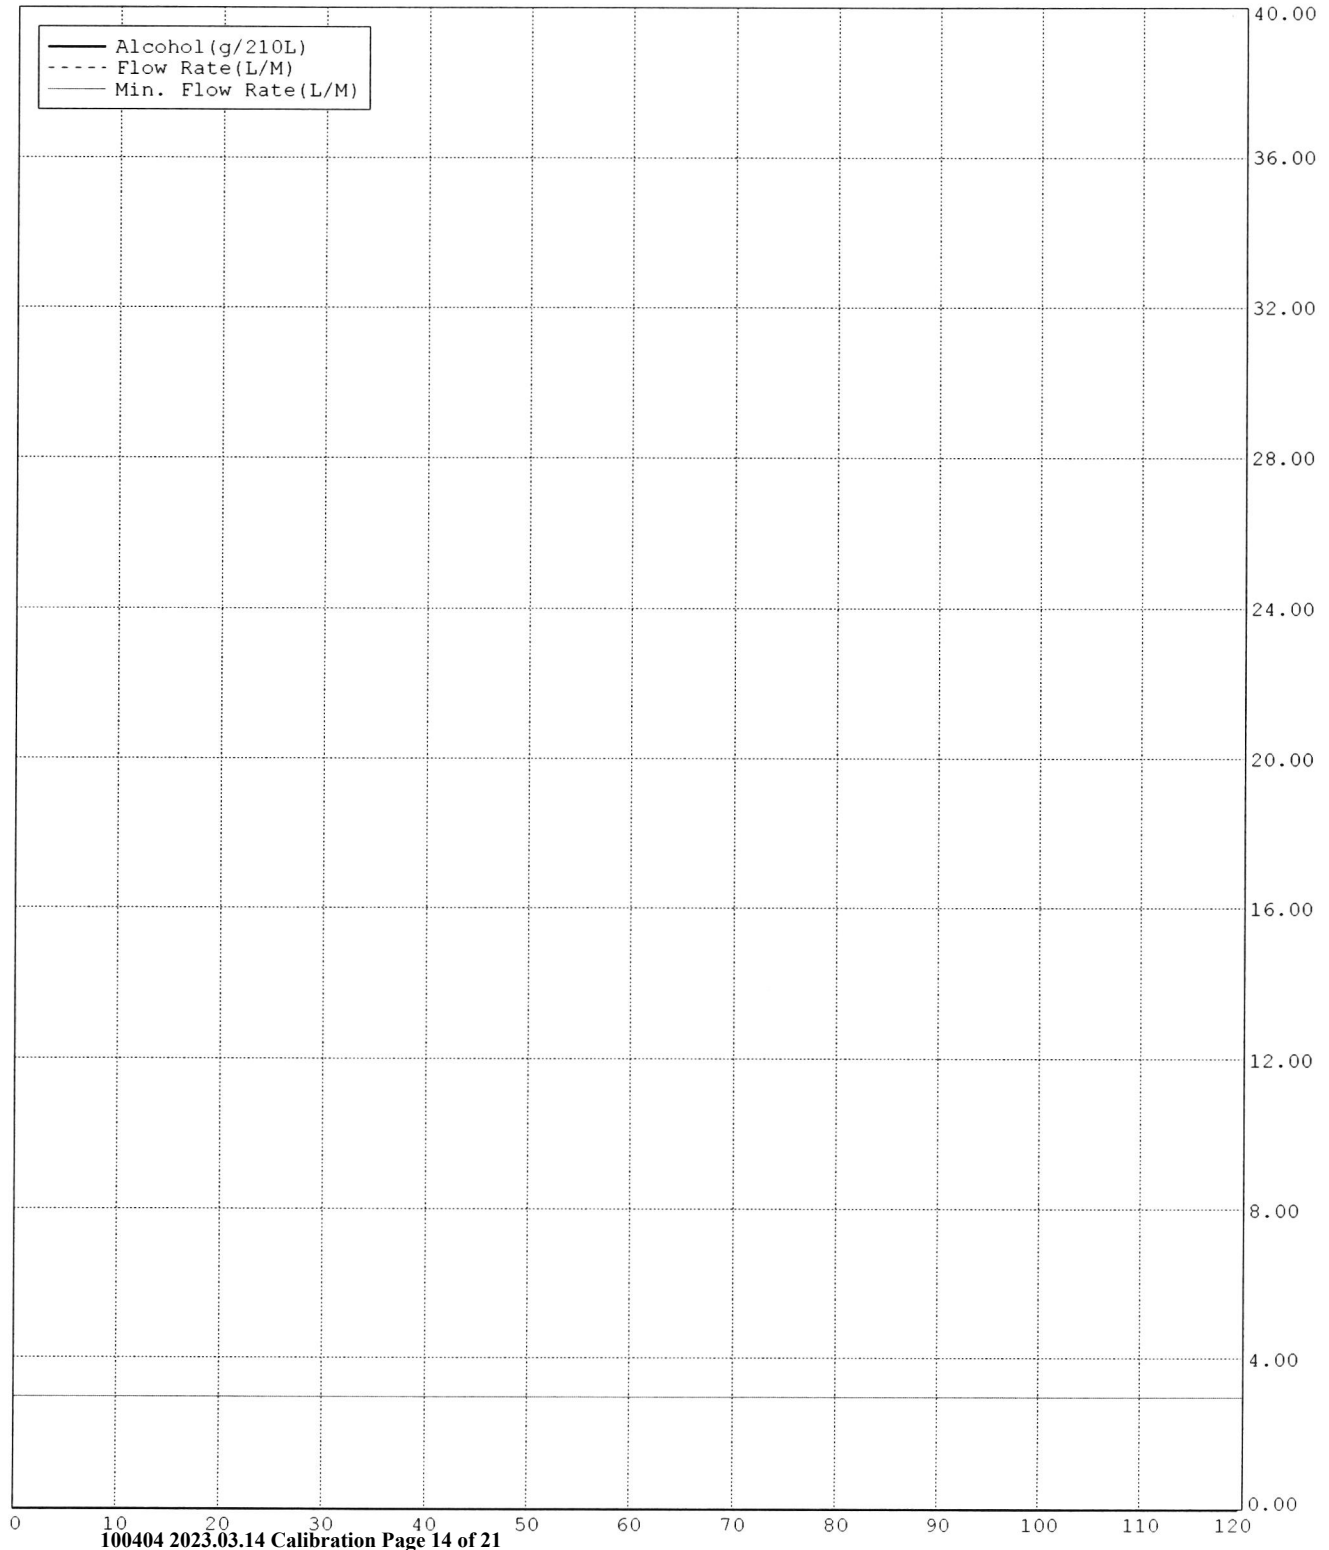

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100404

Date: 03/14/2023  
Time: 09:22:52

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437


DEPT/AGENCY:  
MAXIMUM ATTEMPTS EXCEEDED  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.26: 0.078  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:23
BLANK TEST	0.000	09:23
INTERNAL STANDARD	VERIFIED	09:24
EXTERNAL STANDARD	0.078	09:24
BLANK TEST	0.000	09:25
SUBJECT SAMPLE	XXX	09:25

Maximum Attempts Exceeded

TUM

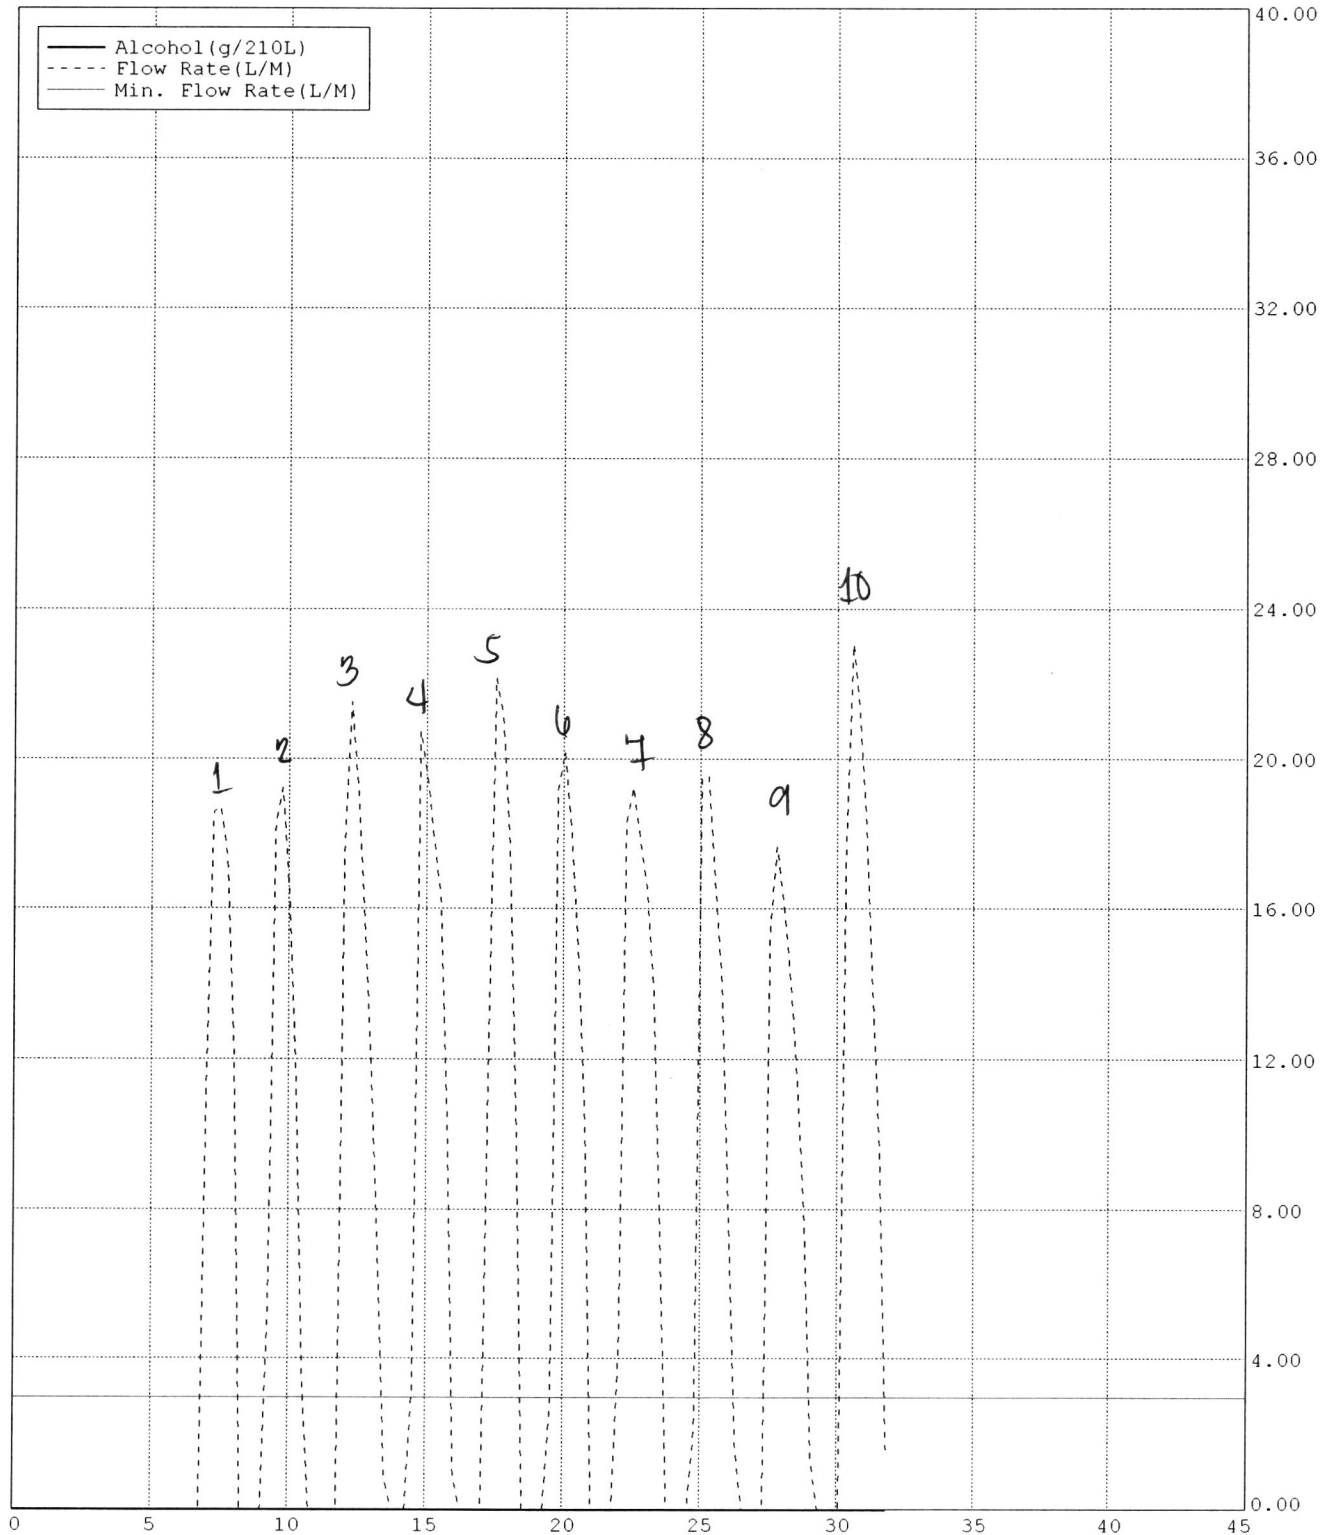

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100404

Date: 03/14/2023  
Time: 09:49:16

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
INVALID  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.26: 0.078  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:50
BLANK TEST	0.000	09:50
INTERNAL STANDARD	VERIFIED	09:50
EXTERNAL STANDARD	0.078	09:50
BLANK TEST	0.000	09:51
SUBJECT SAMPLE	INVALID	09:52

TLM

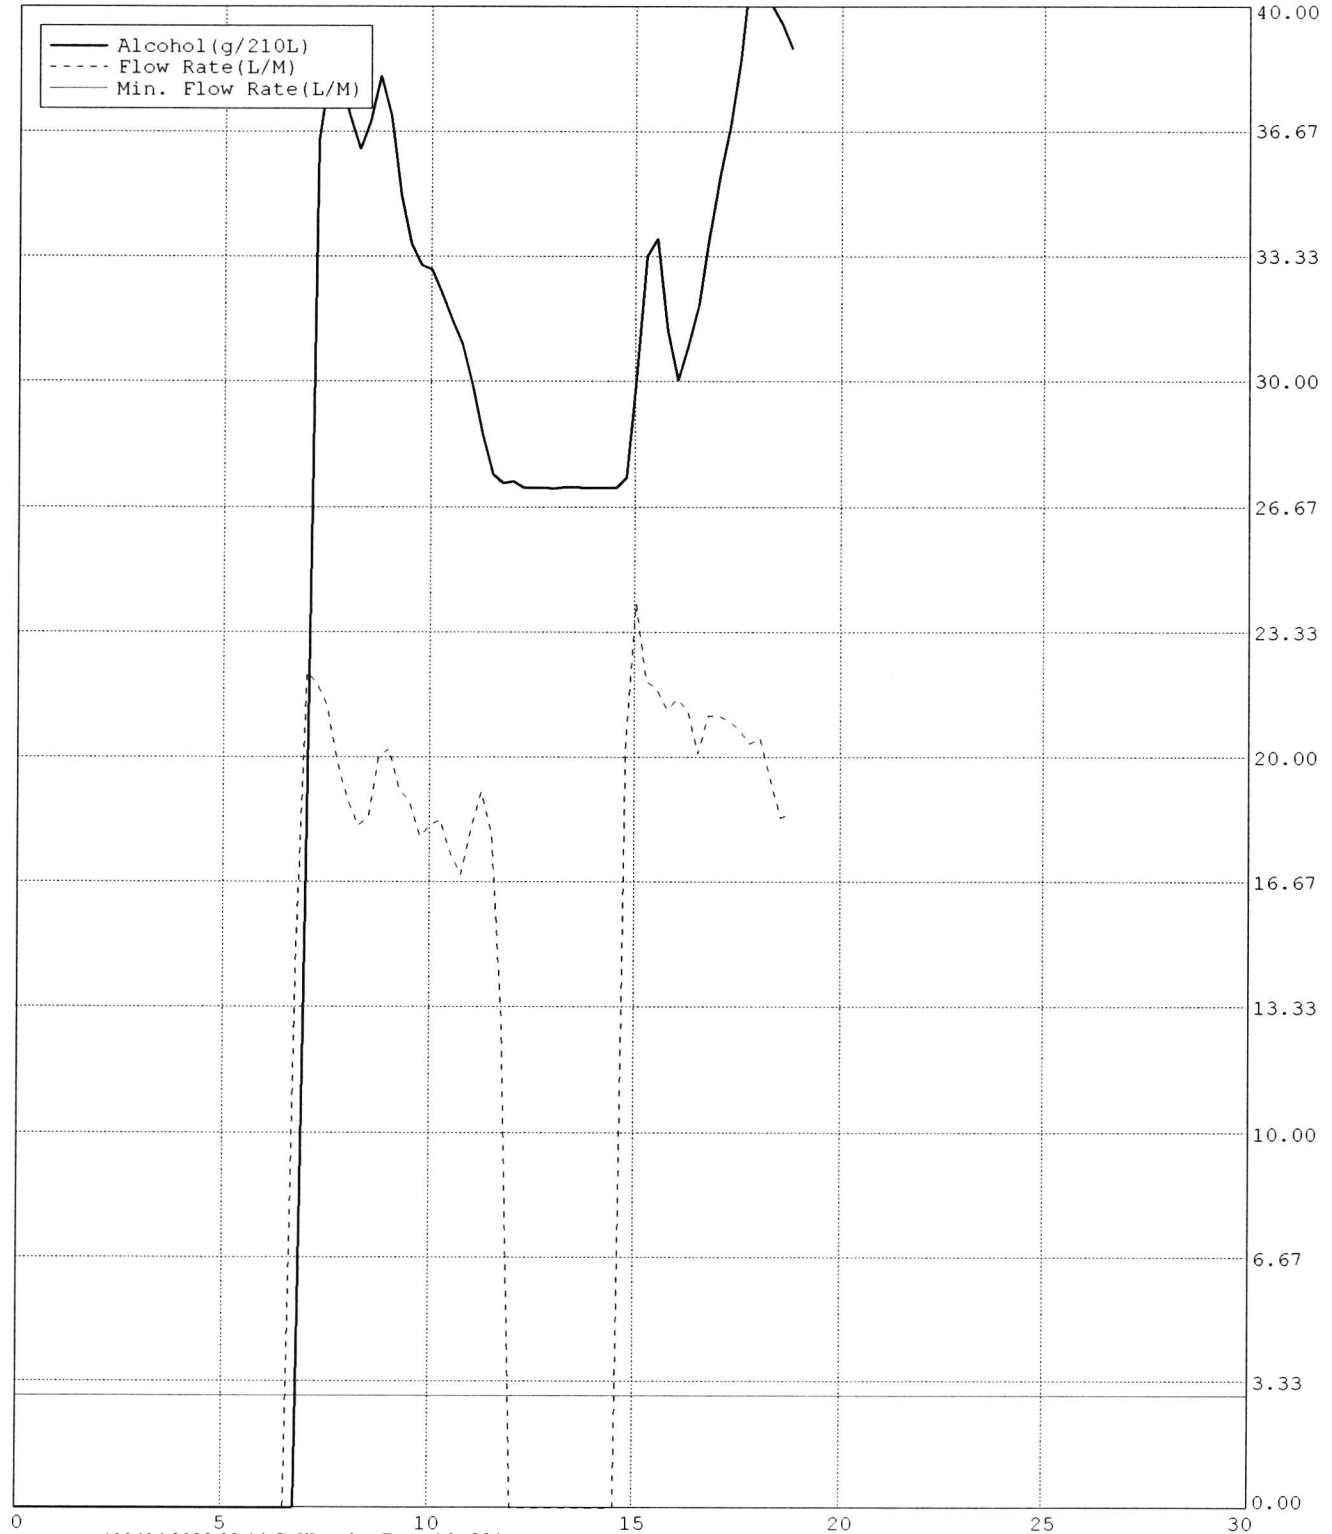



SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100404  
-----

Date: 03/14/2023  
Time: 10:07:03

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437


DEPT/AGENCY:  
RADIO FREQUENCY INTERFERENCE (RFI)  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.25: 0.078  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:08
BLANK TEST	0.000	10:08
INTERNAL STANDARD	VERIFIED	10:08
EXTERNAL STANDARD	0.077	10:08
BLANK TEST	0.000	10:09

RFI DETECTED

TLM

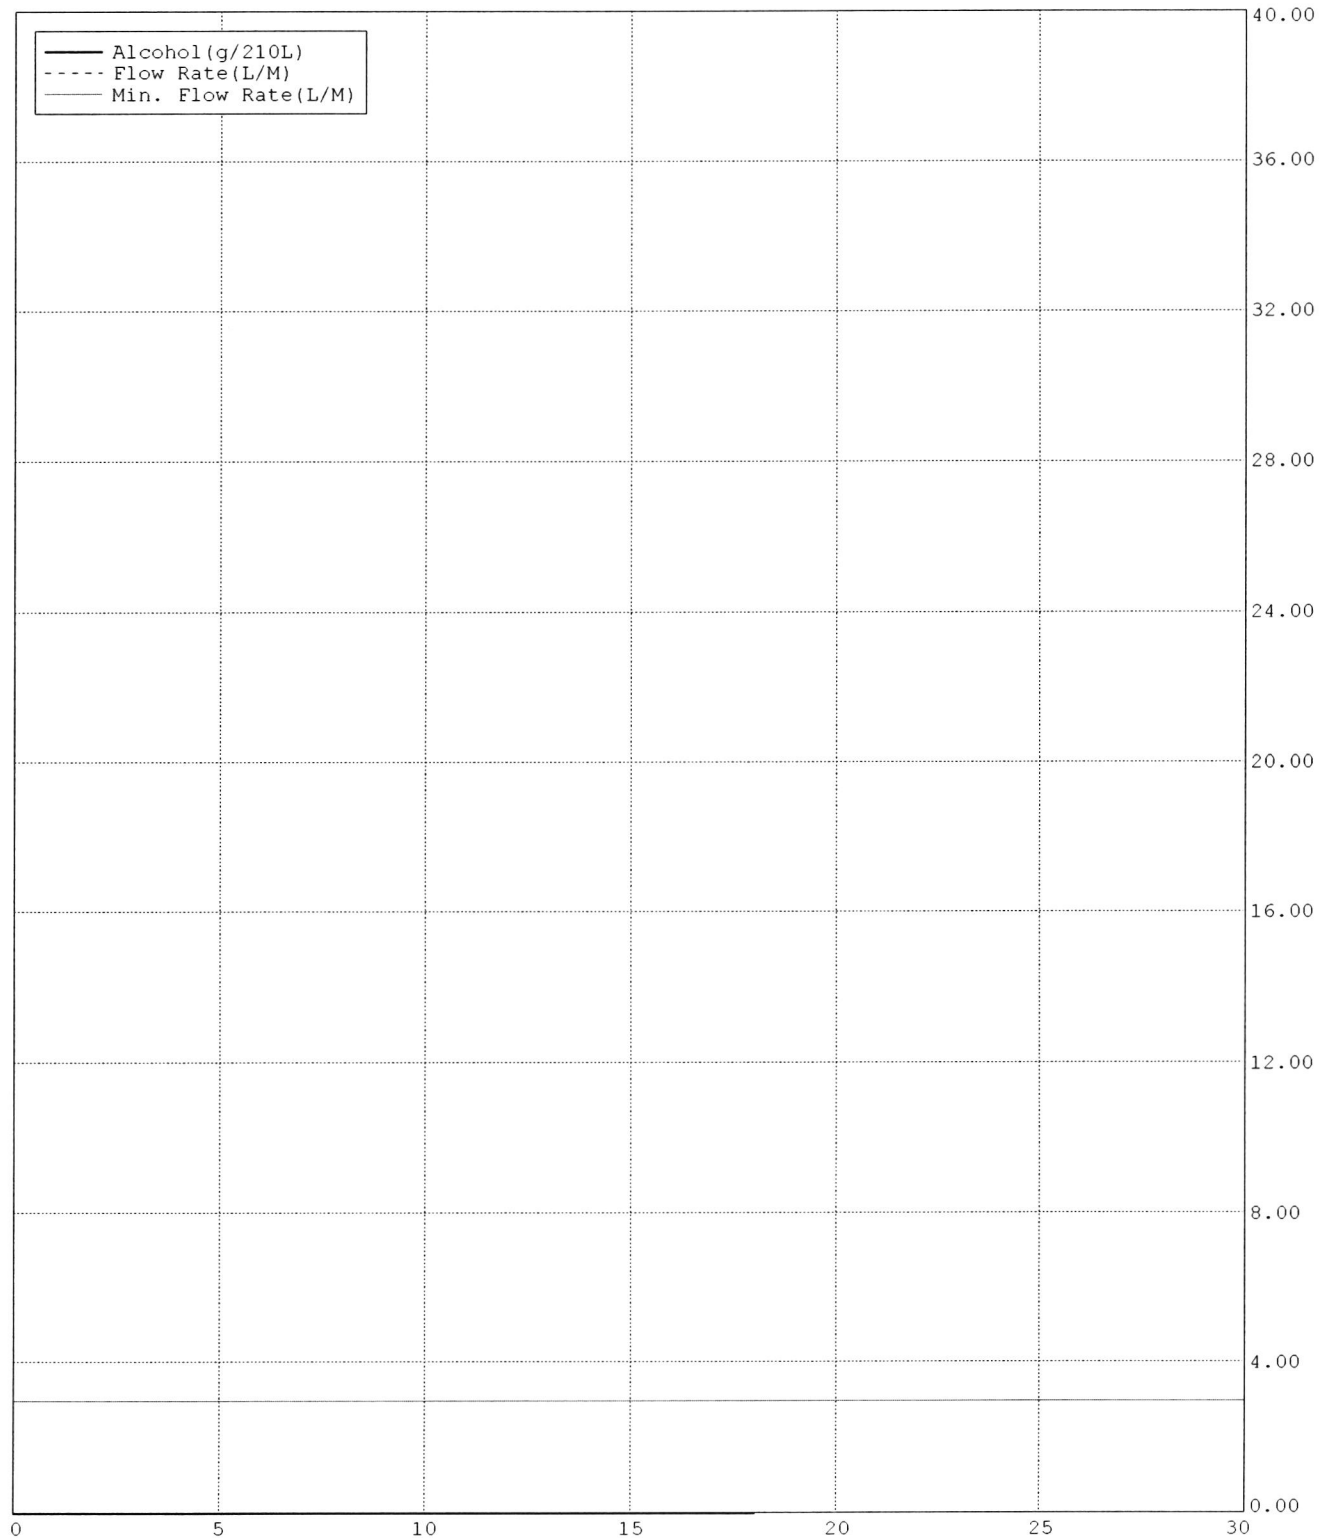

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100404

Date: 03/14/2023  
Time: 10:26:44

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
INTERFERENCE - ACETONE  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.25: 0.078  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:27
BLANK TEST	0.000	10:27
INTERNAL STANDARD	VERIFIED	10:27
Xq = 0.090 (1.38%)		
EXTERNAL STANDARD	0.078	10:28
X[1] = 0.0780 (-0.0034) (0.0025)		
BLANK TEST	0.000	10:29
SUBJECT SAMPLE	XXX	10:29
X[1] = 0.1108 (-0.0150) (0.0020)		

Interference Detected

Filter 2 Average: -0.0037  
Filter 3 Average: 0.0022  
TLN 03/14/23

TLN

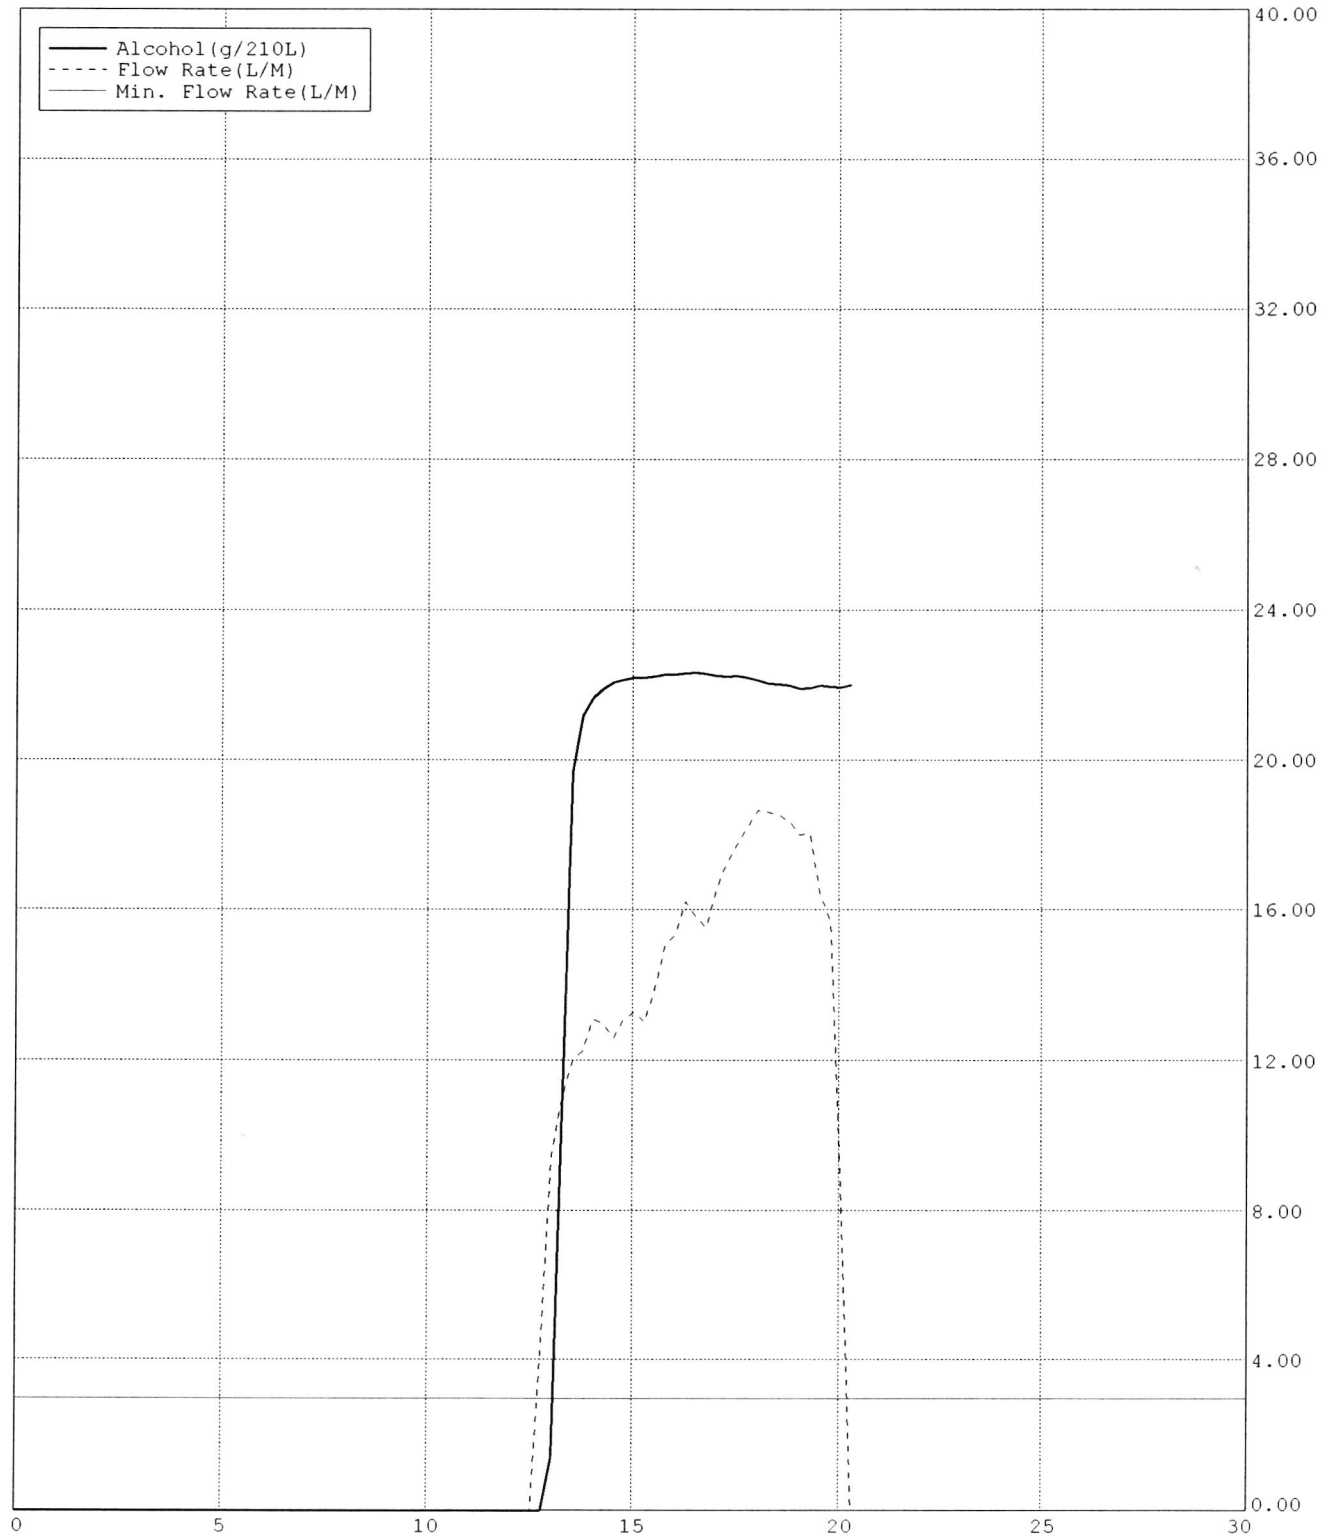

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100404

Date: 03/14/2023  
Time: 10:13:37

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437


DEPT/AGENCY:  
INTERFERENCE - ISOPROPANOL  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.26: 0.078  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:14
BLANK TEST	0.000	10:14
INTERNAL STANDARD	VERIFIED	10:14
Xq = 0.089 (0.79%)		
EXTERNAL STANDARD	0.077	10:15
X[1] = 0.0771 (-0.0043) (0.0022)		
BLANK TEST	0.000	10:16
SUBJECT SAMPLE	XXX	10:16
X[1] = 0.1174 (-0.0335) (0.0000)		

Interference Detected

TUN

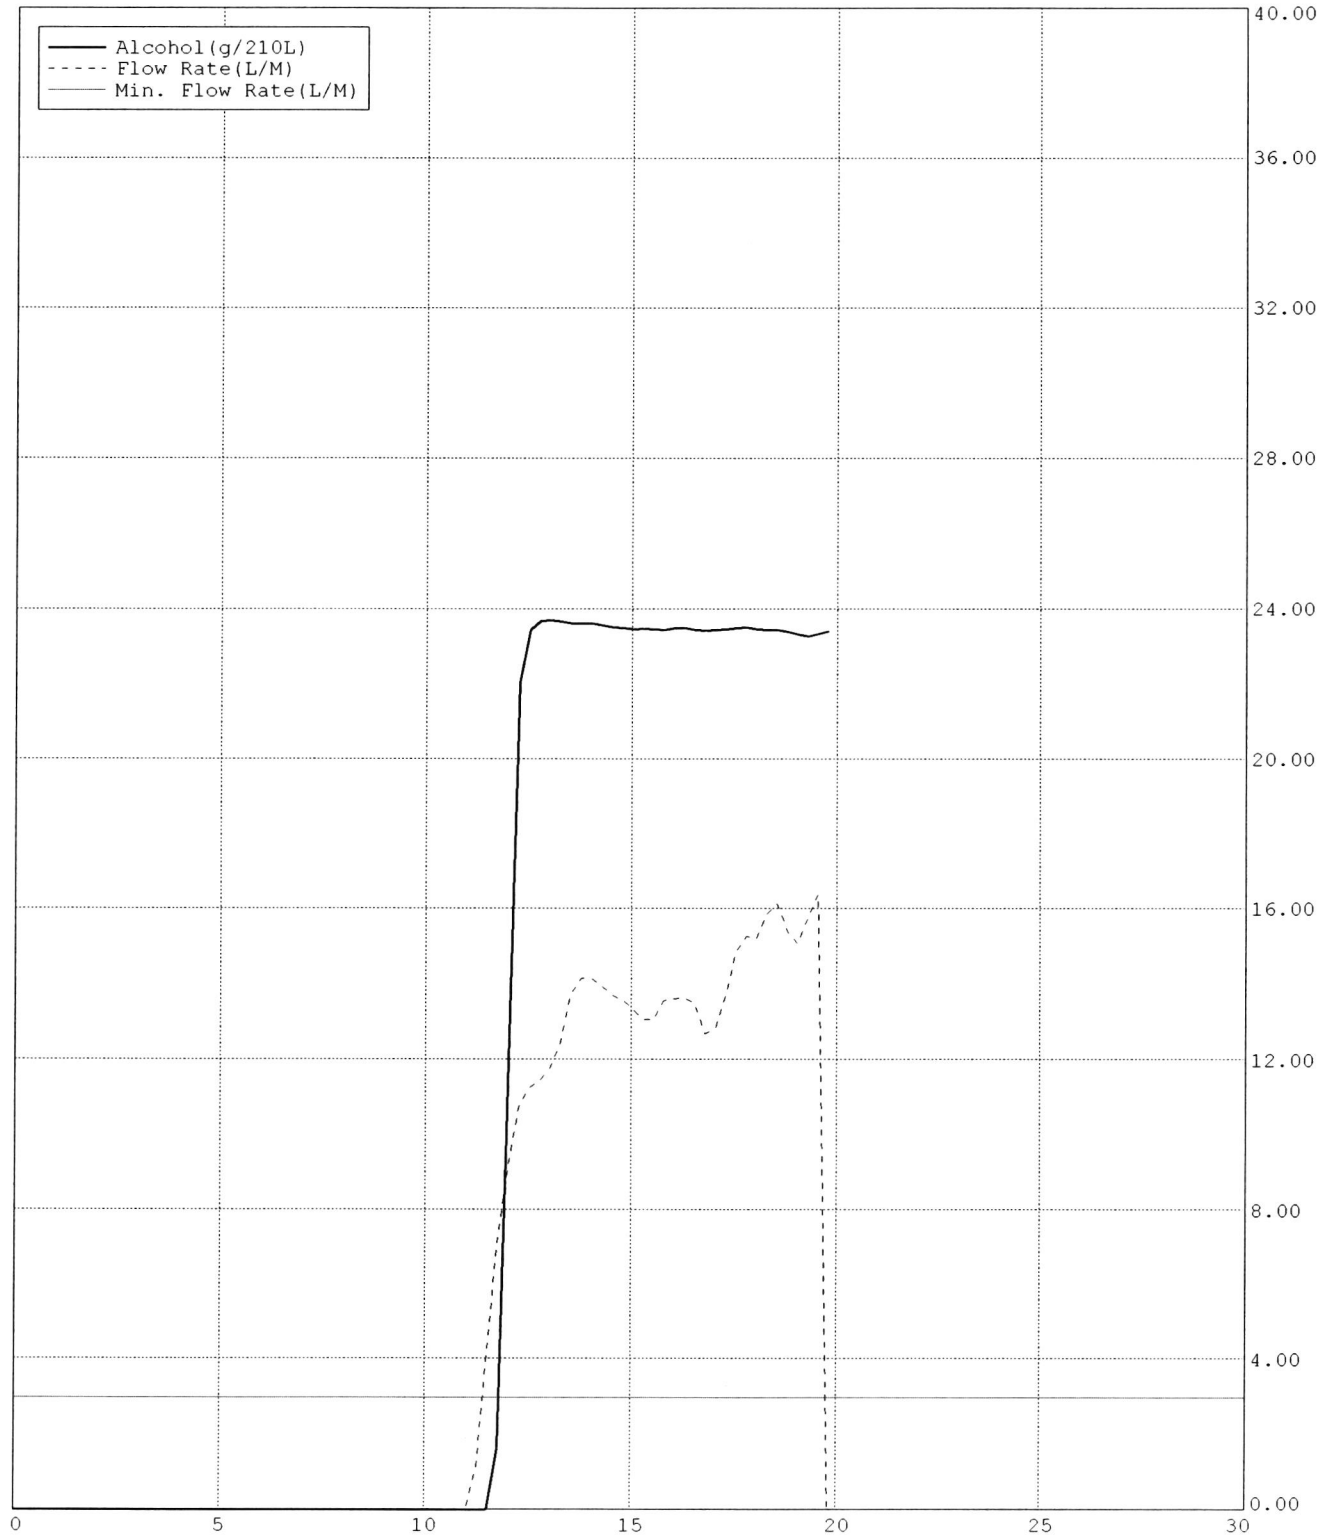

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100404

Date: 03/14/2023  
Time: 10:19:07

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
INTERFERENCE - NEGATIVE CONTROL  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.26: 0.078  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:20
BLANK TEST	0.000	10:20
INTERNAL STANDARD	VERIFIED	10:20
Xq = 0.090 (1.28%)		
EXTERNAL STANDARD	0.077	10:20
X[1] = 0.0774 (-0.0037) (0.0024)		
BLANK TEST	0.000	10:21
SUBJECT SAMPLE (Vol=1.88L)	0.091	10:21
X[1] = 0.0912 (-0.0018) (0.0015)		
BLANK TEST	0.000	10:22
EXTERNAL STANDARD	0.077	10:23
X[1] = 0.0772 (-0.0034) (0.0016)		
BLANK TEST	0.000	10:23

TUM

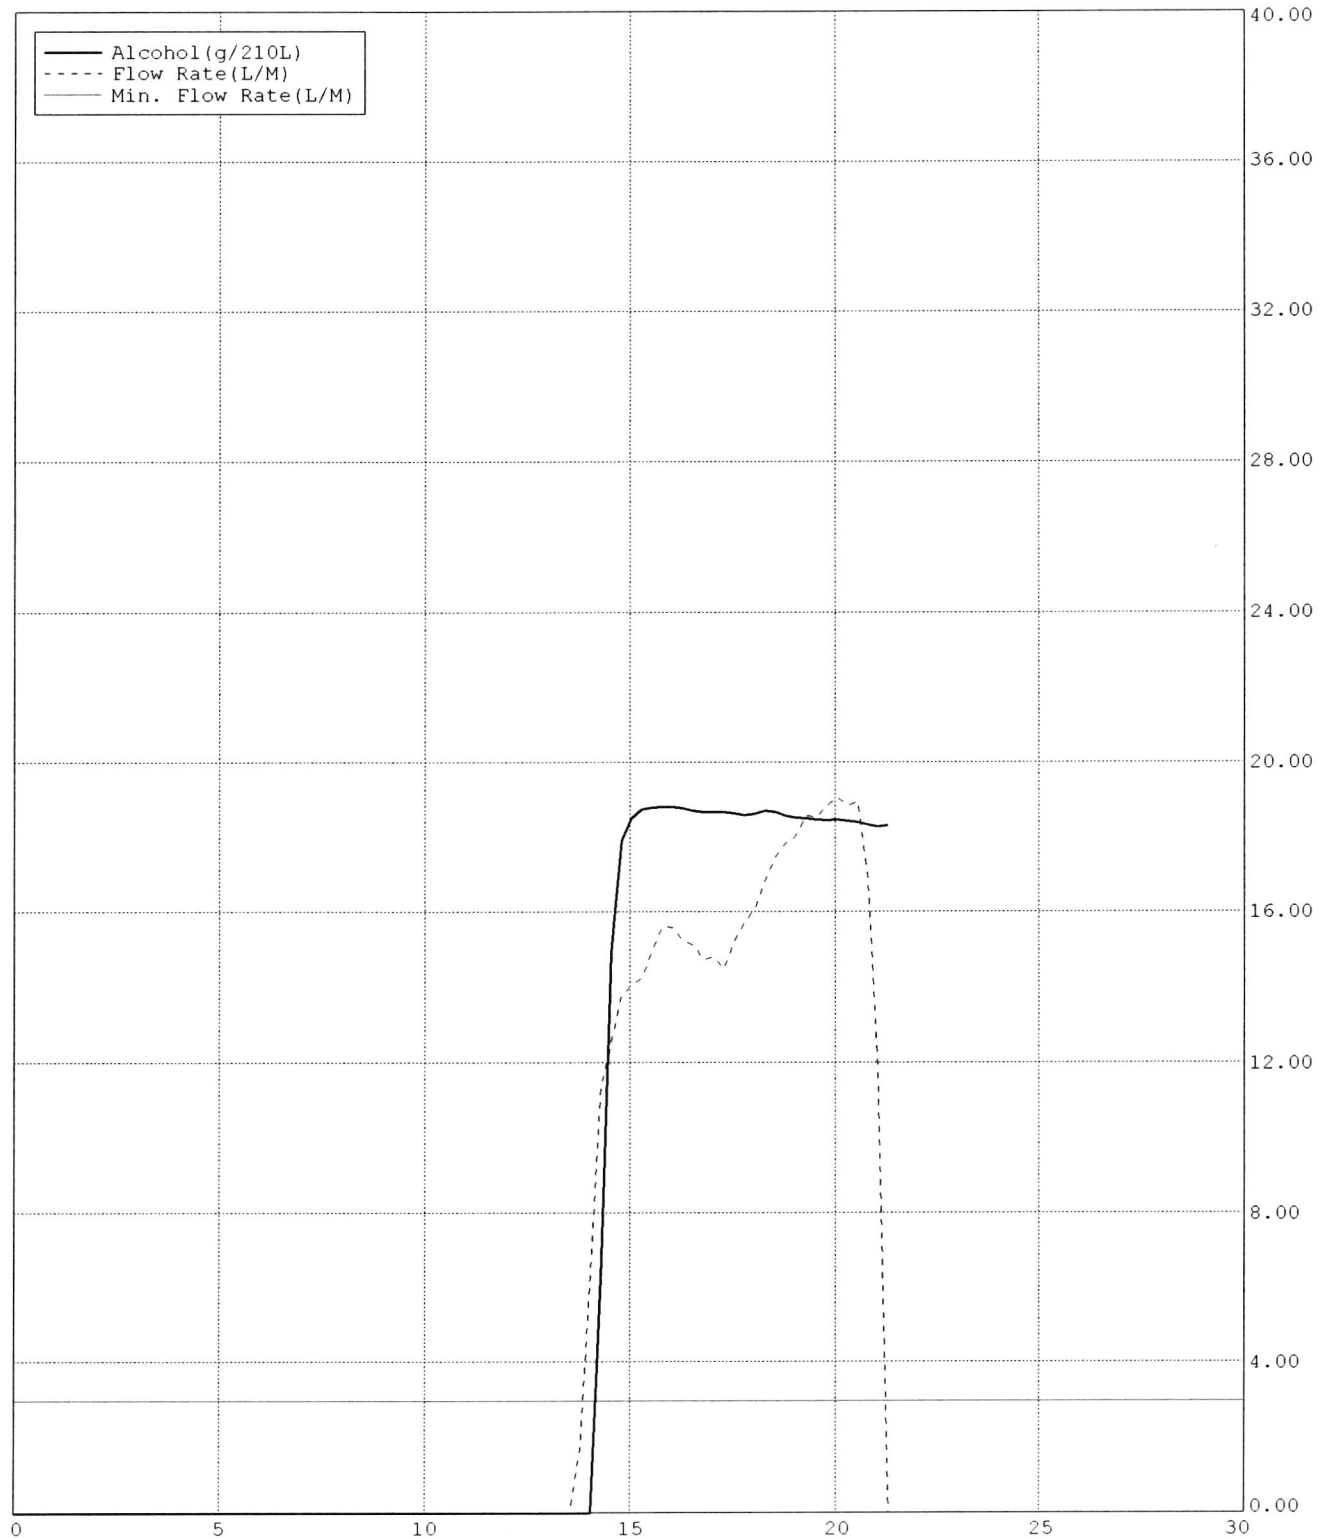

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100404  
-----

Date: 03/14/2023  
Time: 11:05:42

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.26: 0.078  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	11:06
BLANK TEST	0.000	11:06
INTERNAL STANDARD	VERIFIED	11:06
EXTERNAL STANDARD	0.078	11:07
BLANK TEST	0.000	11:08
SUBJECT SAMPLE (Vol=1.60L)	0.000	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.078	11:09
BLANK TEST	0.000	11:10

TMM

