

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument
State of Alaska

Serial #: 100355

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 02/17/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 27.67: 0.074
LOT #: 11313080A1
EXPIRATION: 06/01/2015
TANK PRESSURE: 947 psi

BLANK TEST	0.000	09:13
INTERNAL STANDARD	VERIFIED	09:13
EXTERNAL STANDARD	0.072	09:13
BLANK TEST	0.000	09:14
EXTERNAL STANDARD	0.072	09:14
BLANK TEST	0.000	09:15
EXTERNAL STANDARD	0.072	09:16
BLANK TEST	0.000	09:16
EXTERNAL STANDARD	0.072	09:17
BLANK TEST	0.000	09:18
EXTERNAL STANDARD	0.072	09:18
BLANK TEST	0.000	09:19

Average = 0.0720
Std Dev = 0.0000

Diagnostic Check

VERSIONS

DMT: 3.00
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
Breath Tube = 48.1°C PASSED

PUMP INFO

Flow Rate = 4.301 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO

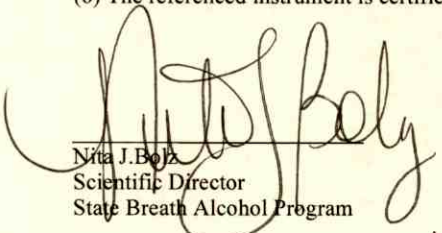
Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

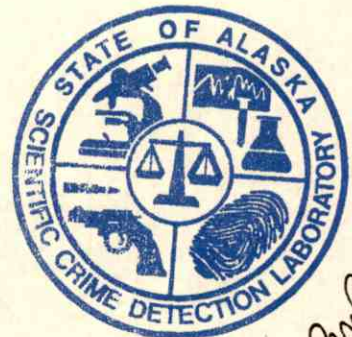
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.



Nita J. Bolz
Scientific Director
State Breath Alcohol Program

3/10/2015

Subscribed and sworn before me this 10th day of Mar, 20 15


Nikki Roth, Notary Public
My Commission Expires With Office




BMB
3/2/15