



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100672

**Report Issue Date:** 07/10/2024  
**Date Received:** 2023-12-01  
**Condition of Item:** Good

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.019	AG217902	0.018	0.019	0.019	0.019	0.018	0.019	
0.080	0.077	AG310901	0.075	0.076	0.076	0.076	0.076	0.076	
0.300	0.290	AG327804	0.285	0.285	0.286	0.285	0.286	0.285	

As Found - Evaluation Analyst: Carlie Glaister  
 As Found Conditions - Barometric Pressure (inHg): 28.98 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.6 Relative Humidity (%): 14  
 As-Found Lab Activity Date Range: 01/03/2024 - 01/03/2024

Secured double check value to wall. Replaced o-ring. 1st VOC - blank error & wrong software version. Installed 3.02. Blank error could be from recent use of dust off.

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG217902	0.019	0.019	0.019	0.020	0.020	0.019	+/- 0.002	
0.040	0.039	AG217904	0.039	0.039	0.040	0.040	0.039	0.039	+/- 0.003	
0.080	0.078	AG310901	0.077	0.076	0.078	0.078	0.077	0.077	+/- 0.004	
0.100	0.098	AG333401	0.099	0.099	0.099	0.099	0.099	0.099	+/- 0.004	
0.150	0.147	AG332004	0.145	0.145	0.145	0.145	0.146	0.145	+/- 0.005	
0.300	0.294	AG327804	0.295	0.294	0.295	0.294	0.295	0.295	+/- 0.011	

As Left Conditions - Barometric Pressure (inHg): 29.26 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.7 Relative Humidity (%): 37  
 As-Left Lab Activity Date Range: 06/06/2024 - 06/06/2024

Supervised casework with Kaija Swisher.

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**



State of Alaska  
Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
Anchorage, Alaska 99507  
David Kanaris, Chief, Forensic Laboratories



---

**Serial Number:** 100672

---

Results authorized by Derek Walton on 07/10/2024

[derek.walton@alaska.gov](mailto:derek.walton@alaska.gov)

Technically and administratively reviewed by Colleen O'Bryant on 07/10/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100672 Analyst or Technician Name: Kaja Swisher

DataMaster DMT Calibration Start Date: 6/6/24

*Supervised case work with  
Derck Walton 06/21/24 JMW*

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 230307229  
Calibration Due Date: 5/2/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.26 Temperature(C) 20.7 Relative Humidity(%) 37

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20240501KS Expiration Date: 8/1/24  
Simulator S/N: SD1088 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240501MNC Expiration Date: 8/1/24  
Simulator S/N: DE4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 22HP41201 Expiration Date: 8/1/24  
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 9/19/25

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 6/6/24

Data Interpretation Date (Technician): \_\_\_\_\_ (if applicable)

Data Interpretation Date (Analyst): 6/6/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety  
DATAMASTER dmt: 100672

Date: 06/06/2024  
Time: 07:49:58

VERSIONS  
DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 45.7°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 2.10 V PASSED  
(1.26 V - 2.94 V)  
Cooler Voltage = 1.96 V PASSED  
(1.18 V - 2.76 V)  
Bias Voltage = 80 V PASSED  
(47 V - 111 V)  
Chopper Freq = 552 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.910 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 v <= 0.010 v)  
PUMP OFF PASSED  
(0.003 v <= 0.010 v)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.114 0.94% (0.00% - 4.00%) PASSED

Technician Screen

-----  
DATAMASTER dmt: 100672  
-----

Date: 06/06/2024  
Time: 7:54 AM

Temperatures (°C)

Sample Cell: 48.9°C  
Breath Tube: 45.2°C

Current Barometer 29.3 in  
Volume (Ltr) 1.53

Settings

Lamp: 2.26 V  
Bias: 80 V  
Cooler: 1.96 V  
Chopper: 551 Hz

Voltages (V)

Flow: 1.06 V  
Detector: -0.062 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100672  
-----

Date: 04/29/2024  
Time: 12:07:38

OPERATOR NAME:  
COLLEEN S OBRYANT  
CERTIFICATE #: 6237

Ca = 0.1000  
CAL = 0.978329    0.800 <= CAL < 1.200  
b1 = 0.0013    0.0000 <= b1 < 0.0040  
b2 = 0.0058    0.0010 <= b2 < 0.0100  
b3 = 0.0012    0.0000 <= b3 < 0.0040  
Xq = 0.1127    0.0500 <= Xq < 0.2000  
a21 = 1.148807    1.050 <= a21 < 1.300  
a31 = 0.554893    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100672

Date: 06/06/2024  
 Time: 07:56:12

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXX

OPERATOR NAME:  
 KAIJA SWISHER  
 OPERATOR'S #: 10746


DEPT/AGENCY: Lot # AG310901  
 MINIMUM VOLUME TEST Exp 4/19/25  
 CASE/REPORT: XXX KS 6/18/24  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.26: 0.078

DIAGNOSTIC CHECK	PASSED	07:57
BLANK TEST	0.000	07:57
INTERNAL STANDARD	VERIFIED	07:57
EXTERNAL STANDARD	0.077	07:57
BLANK TEST	0.000	07:58
SUBJECT SAMPLE (Vol=1.57L)	0.000	07:59
BLANK TEST	0.000	08:00
EXTERNAL STANDARD	0.078	08:00
BLANK TEST	0.000	08:01

KS

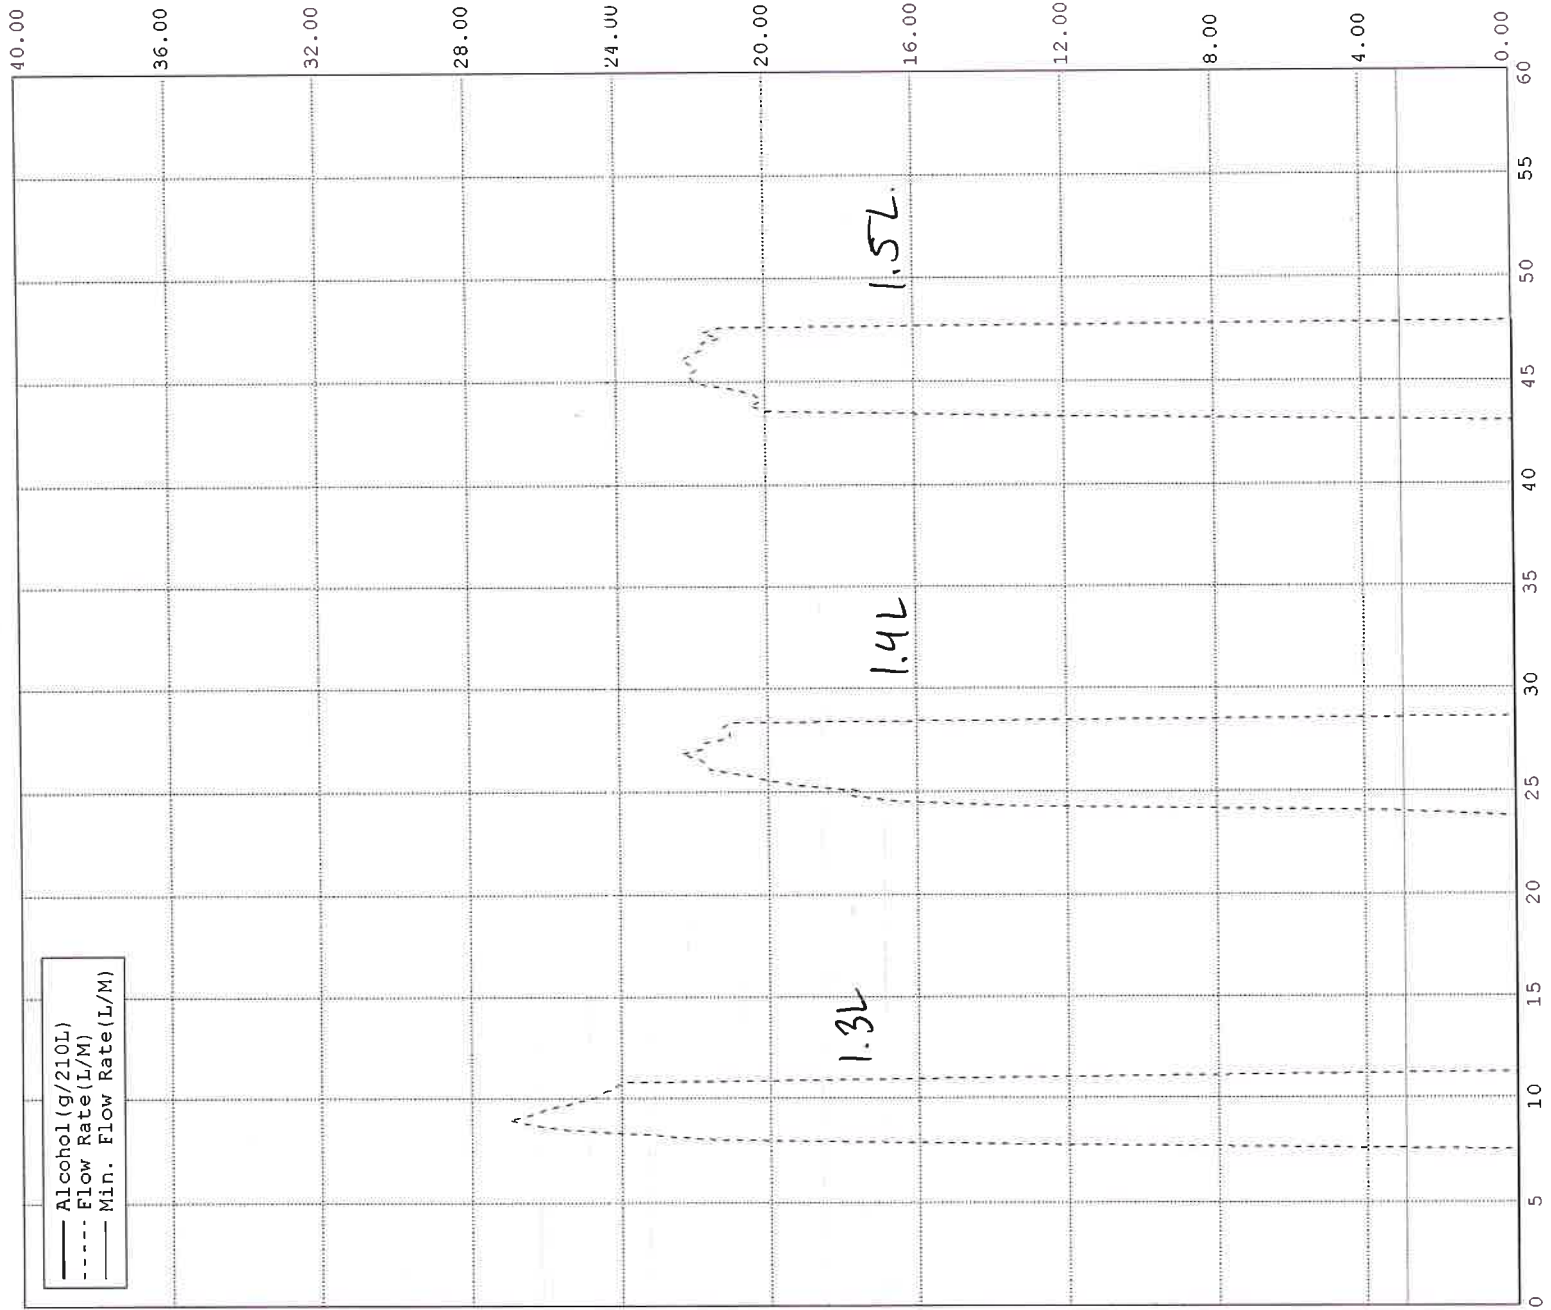

LINEARITY CHECK


Alaska Department of Public Safety  
 DATAMASTER dmt: 100672

Date: 06/06/2024  
 Time: 08:22:53

SUPERVISOR NAME:  
 KAIJA SWISHER  
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.020	0.0194	0.0005
0.039	0.0394	0.0005
0.078	0.0772	0.0008
0.098	0.0990	0.0000
0.147	0.1452	0.0004
0.294	0.2946	0.0005

SLOPE = 1.001742  
 $R^2$  = 0.999892

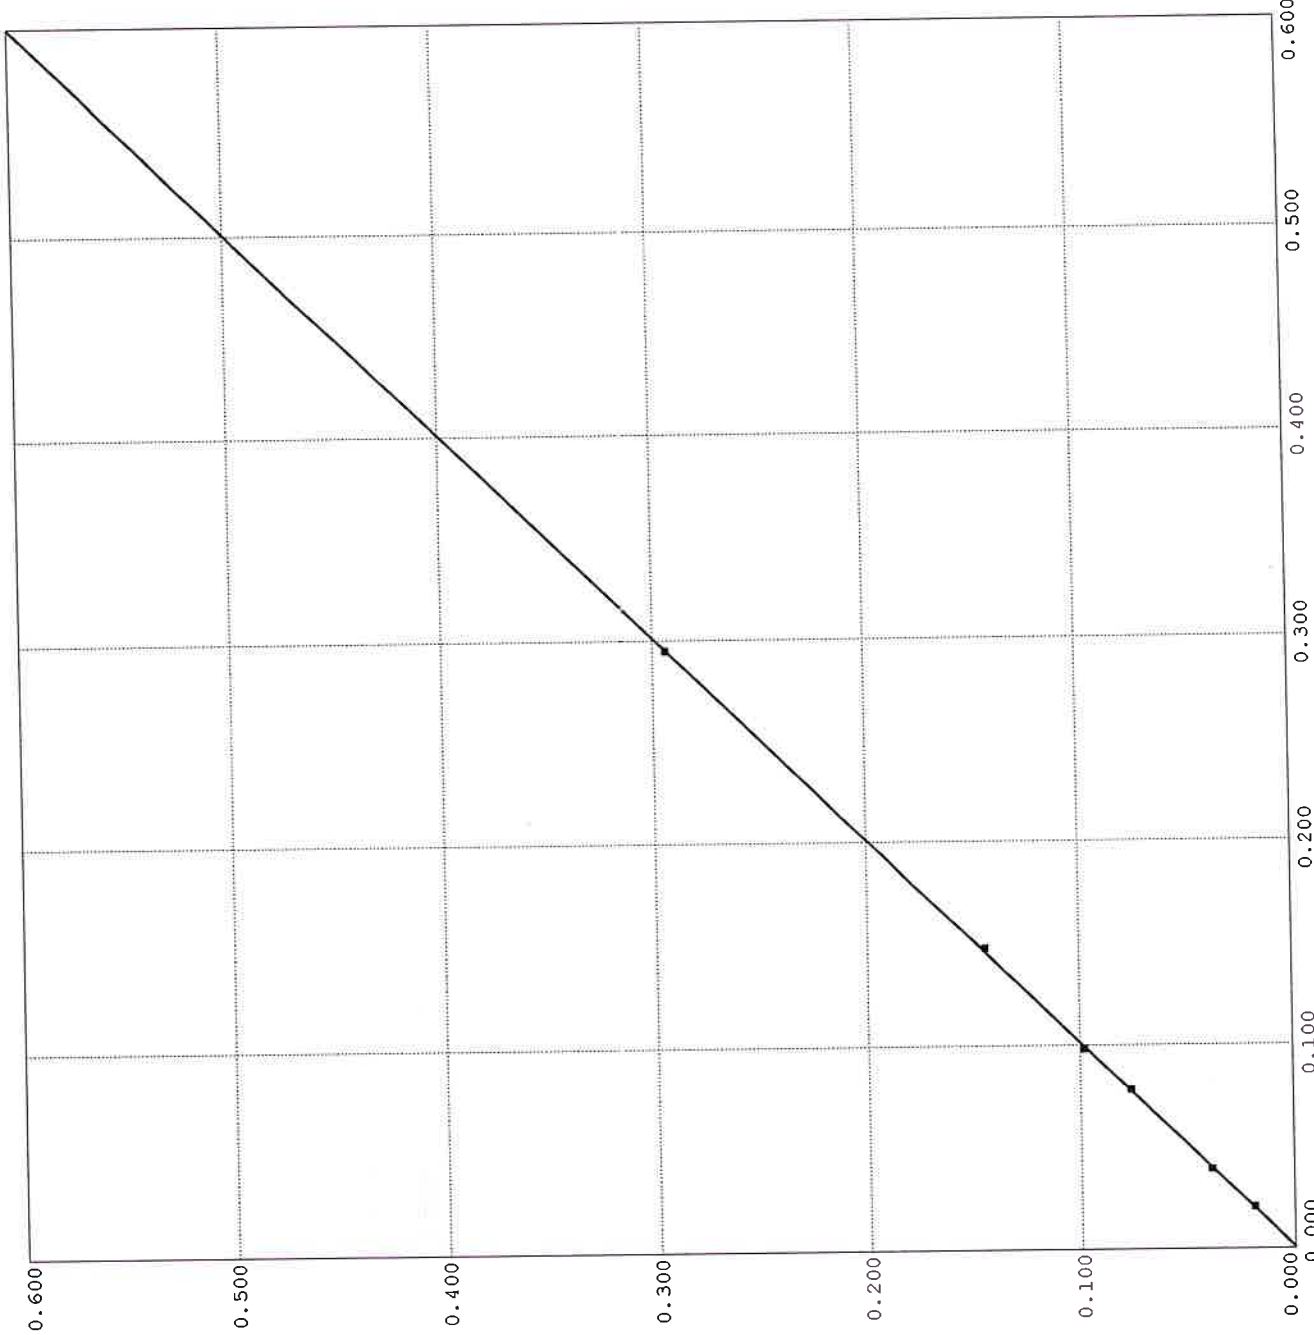

KS



LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100672






Date: 06/06/2024  
Time: 08:22:55

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.26: 0.020  
LOT #: AG217902  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 272 psi

BLANK TEST	0.000	08:24
INTERNAL STANDARD	VERIFIED	08:24
EXTERNAL STANDARD	0.019	08:24
BLANK TEST	0.000	08:25
EXTERNAL STANDARD	0.019	08:26
BLANK TEST	0.000	08:26
EXTERNAL STANDARD	0.019	08:27
BLANK TEST	0.000	08:28
EXTERNAL STANDARD	0.020	08:28
BLANK TEST	0.000	08:29
EXTERNAL STANDARD	0.020	08:29
BLANK TEST	0.000	08:30

Average = 0.0194  
Std Dev = 0.0005

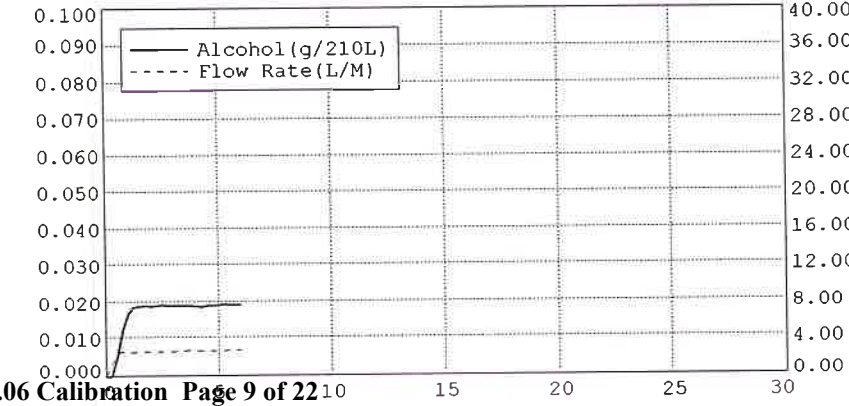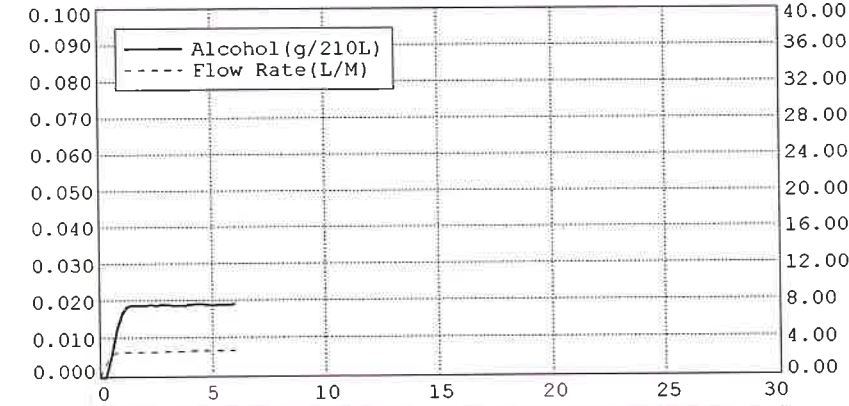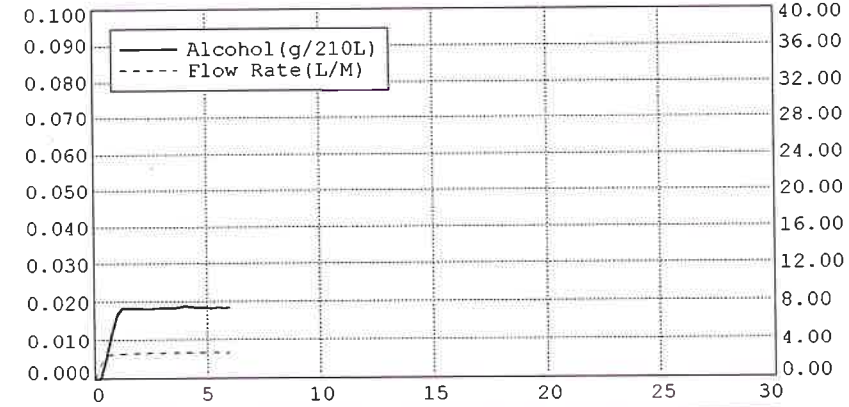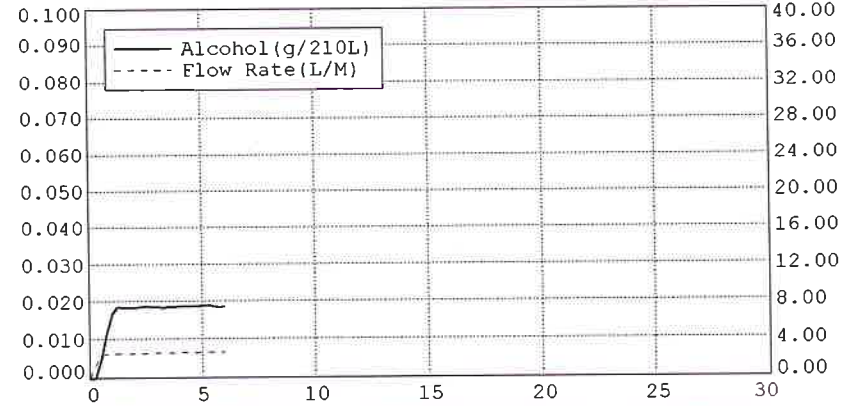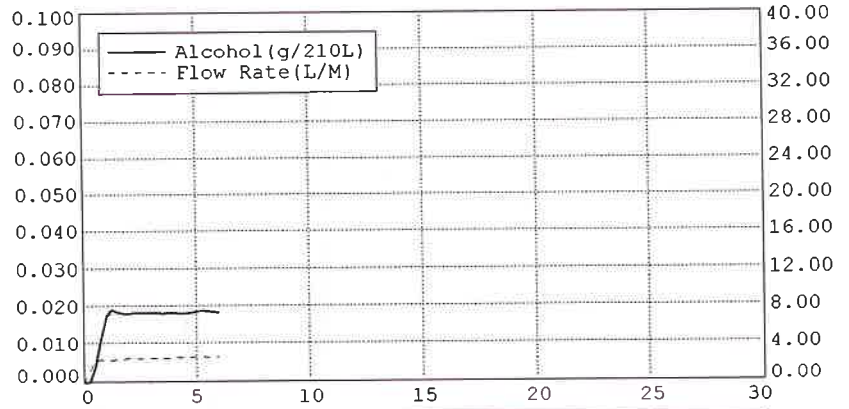

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
DATAMASTER dmt: 100672






Date: 06/06/2024  
Time: 08:31:16

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
TARGET AT 29.27: 0.039  
LOT #: AG217904  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 649 psi

BLANK TEST	0.000	08:32
INTERNAL STANDARD	VERIFIED	08:32
EXTERNAL STANDARD	0.039	08:33
BLANK TEST	0.000	08:33
EXTERNAL STANDARD	0.039	08:34
BLANK TEST	0.000	08:35
EXTERNAL STANDARD	0.040	08:35
BLANK TEST	0.000	08:36
EXTERNAL STANDARD	0.040	08:36
BLANK TEST	0.000	08:37
EXTERNAL STANDARD	0.039	08:37
BLANK TEST	0.000	08:38

Average = 0.0394  
Std Dev = 0.0005

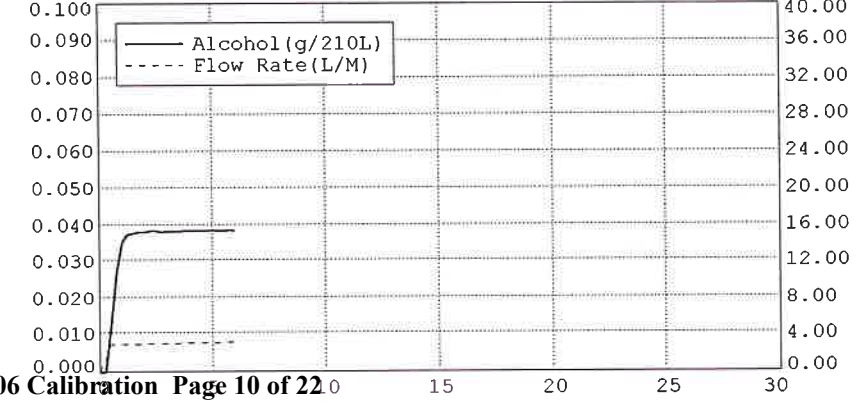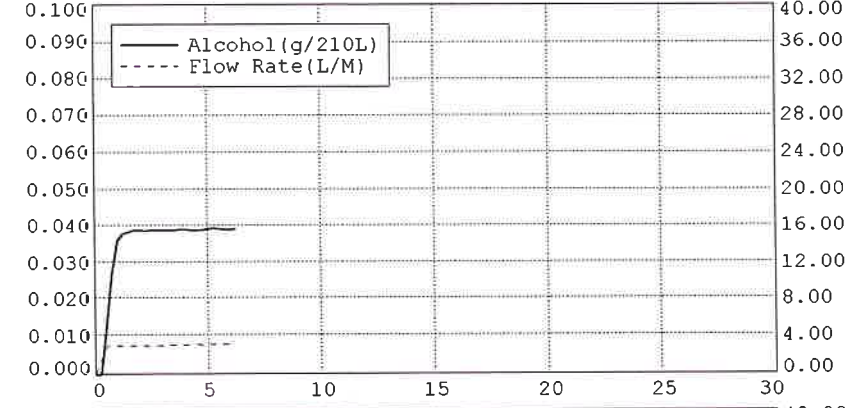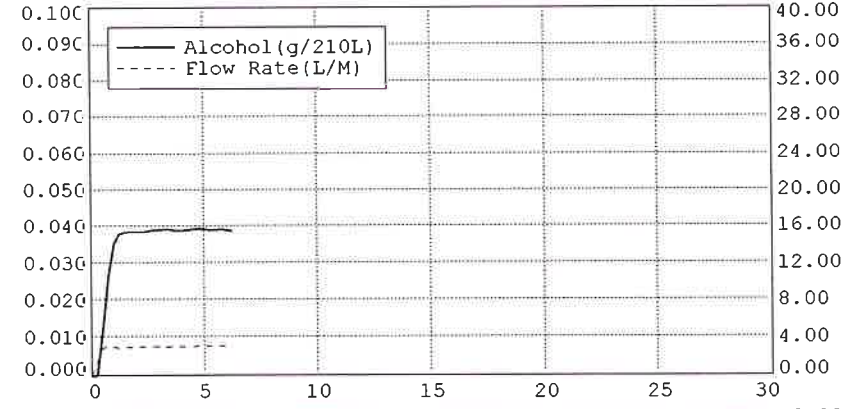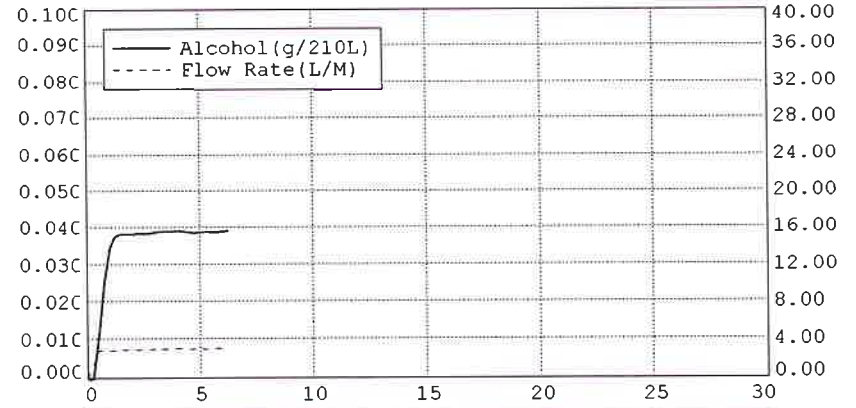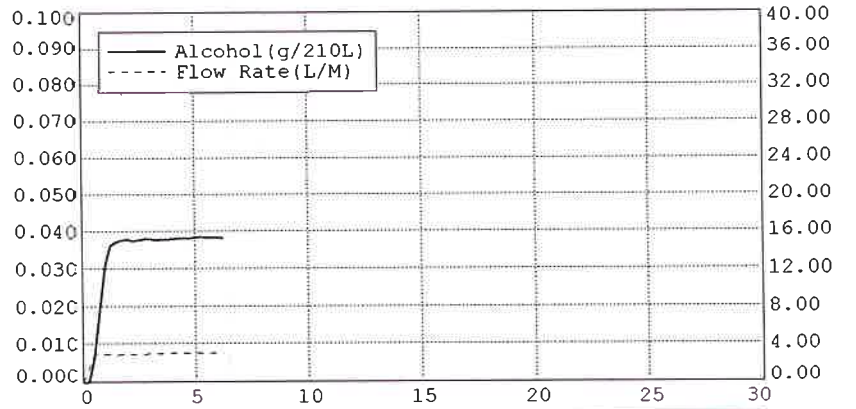

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
DATAMASTER dmt: 100672






Date: 06/06/2024  
Time: 08:41:31

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.27: 0.078  
LOT #: AG310901  
EXPIRATION: 04/19/2025  
TANK PRESSURE: 392 psi

BLANK TEST	0.000	08:42
INTERNAL STANDARD	VERIFIED	08:42
EXTERNAL STANDARD	0.077	08:43
BLANK TEST	0.000	08:44
EXTERNAL STANDARD	0.076	08:44
BLANK TEST	0.000	08:45
EXTERNAL STANDARD	0.078	08:45
BLANK TEST	0.000	08:46
EXTERNAL STANDARD	0.078	08:46
BLANK TEST	0.000	08:47
EXTERNAL STANDARD	0.077	08:47
BLANK TEST	0.000	08:48

Average = 0.0772  
Std Dev = 0.0008

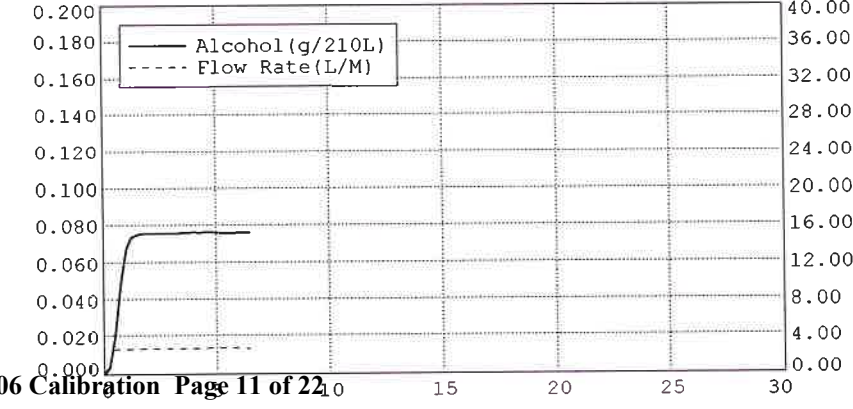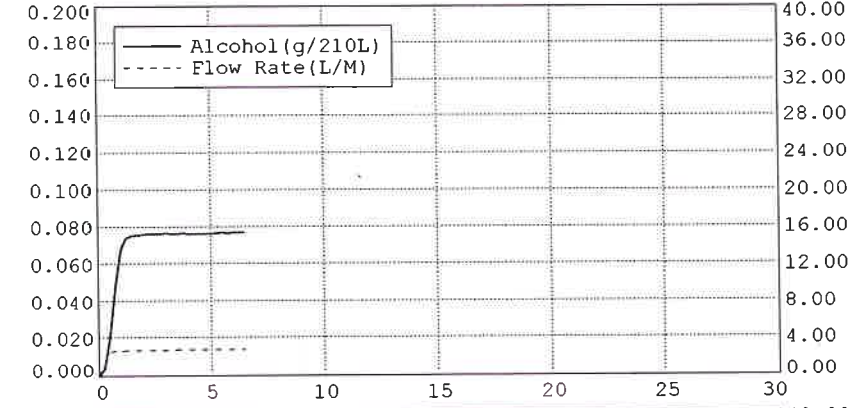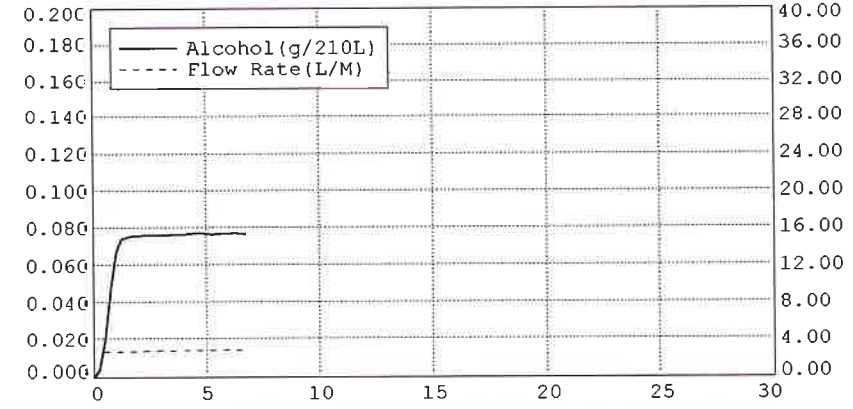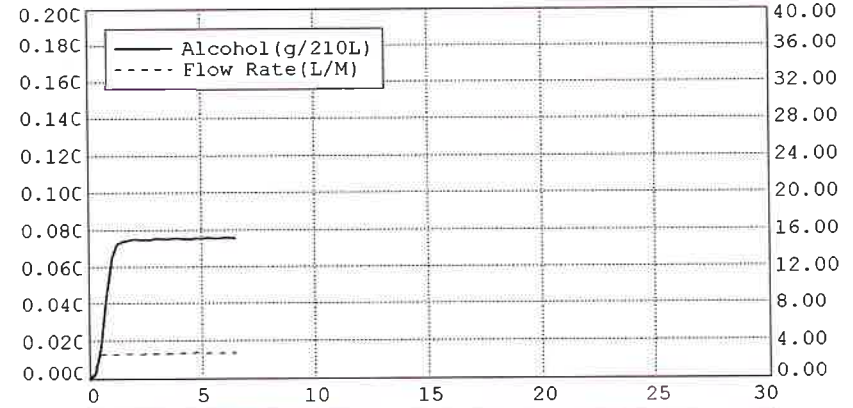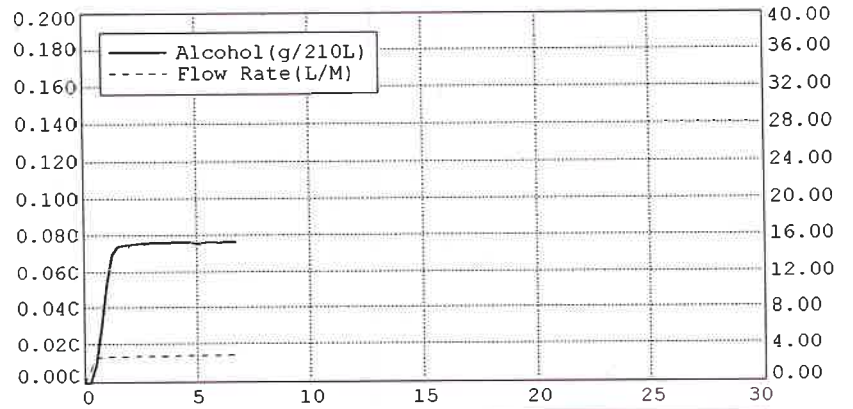



LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100672






Date: 06/06/2024  
 Time: 08:48:54

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.27: 0.098  
 LOT #: AG333401  
 EXPIRATION: 11/30/2025  
 TANK PRESSURE: 1156 psi

BLANK TEST	0.000	08:50
INTERNAL STANDARD	VERIFIED	08:50
EXTERNAL STANDARD	0.099	08:50
BLANK TEST	0.000	08:51
EXTERNAL STANDARD	0.099	08:51
BLANK TEST	0.000	08:52
EXTERNAL STANDARD	0.099	08:52
BLANK TEST	0.000	08:53
EXTERNAL STANDARD	0.099	08:53
BLANK TEST	0.000	08:54
EXTERNAL STANDARD	0.099	08:55
BLANK TEST	0.000	08:55

Average = 0.0990  
 Std Dev = 0.0000

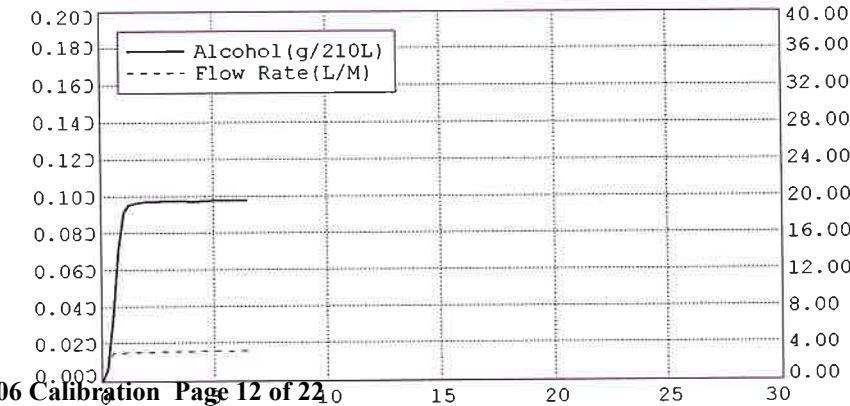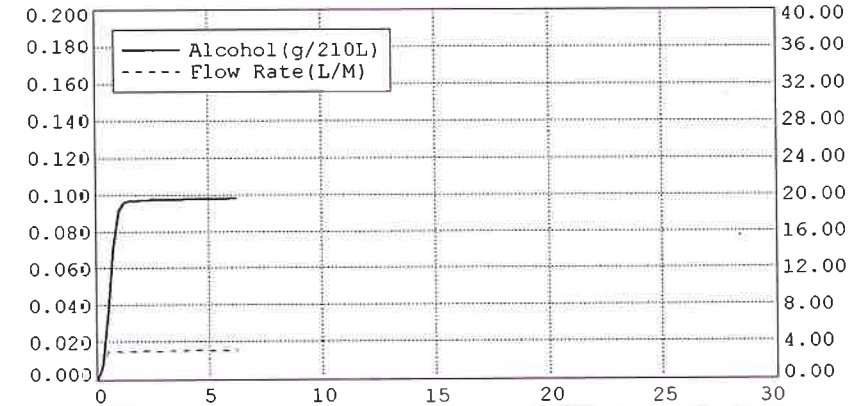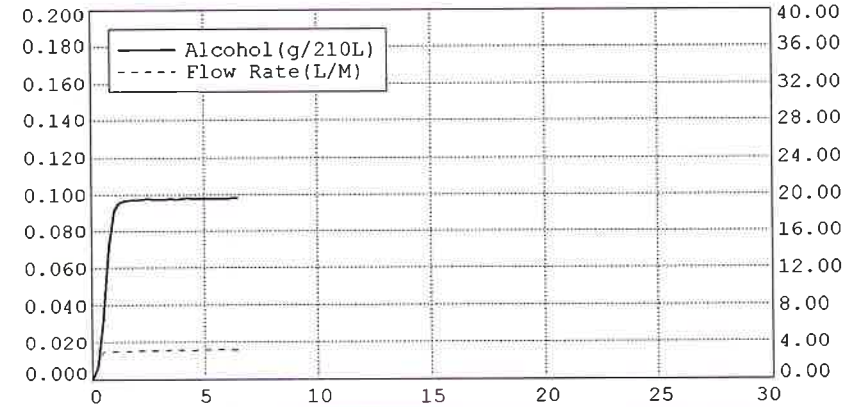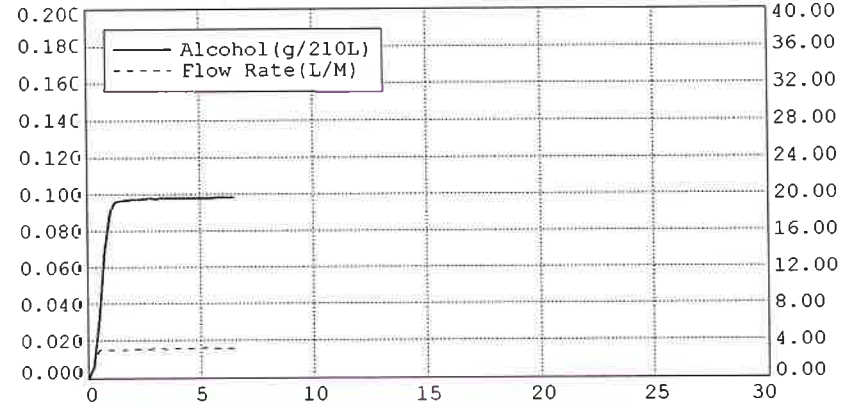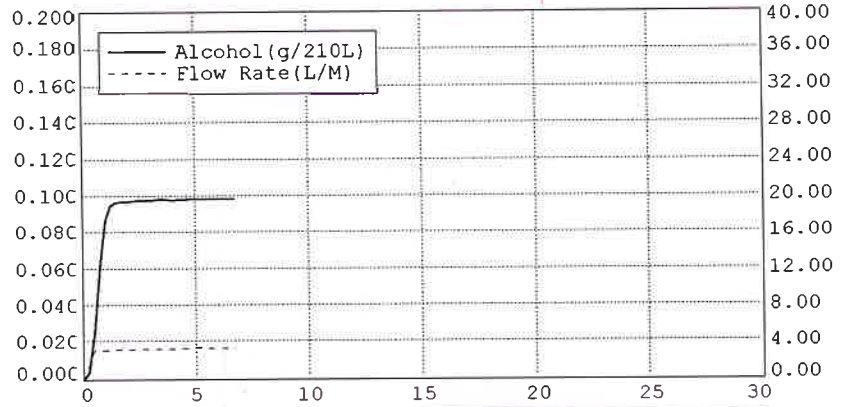

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100672






Date: 06/06/2024  
 Time: 09:18:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.29: 0.147  
 LOT #: AG332004  
 EXPIRATION: 11/16/2025  
 TANK PRESSURE: 648 psi

BLANK TEST	0.000	09:20
INTERNAL STANDARD	VERIFIED	09:20
EXTERNAL STANDARD	0.145	09:20
BLANK TEST	0.000	09:21
EXTERNAL STANDARD	0.145	09:21
BLANK TEST	0.000	09:22
EXTERNAL STANDARD	0.145	09:22
BLANK TEST	0.000	09:23
EXTERNAL STANDARD	0.145	09:23
BLANK TEST	0.000	09:24
EXTERNAL STANDARD	0.146	09:24
BLANK TEST	0.000	09:25

Average = 0.1452  
 Std Dev = 0.0004

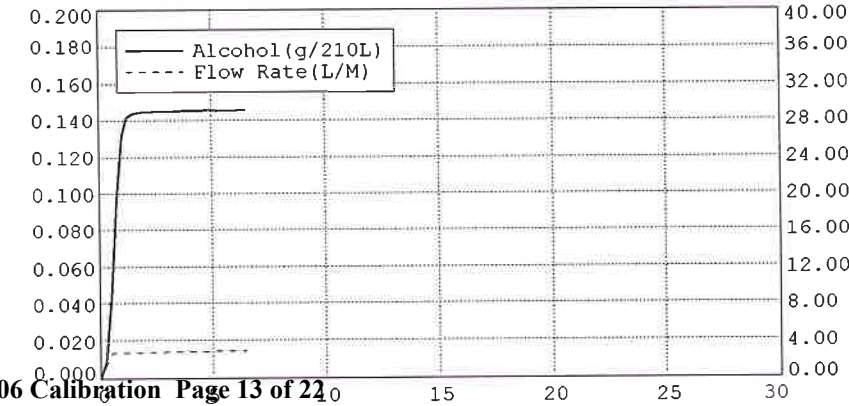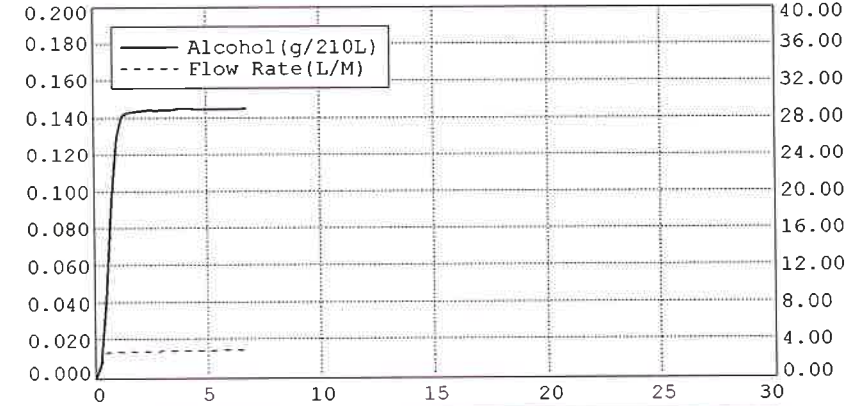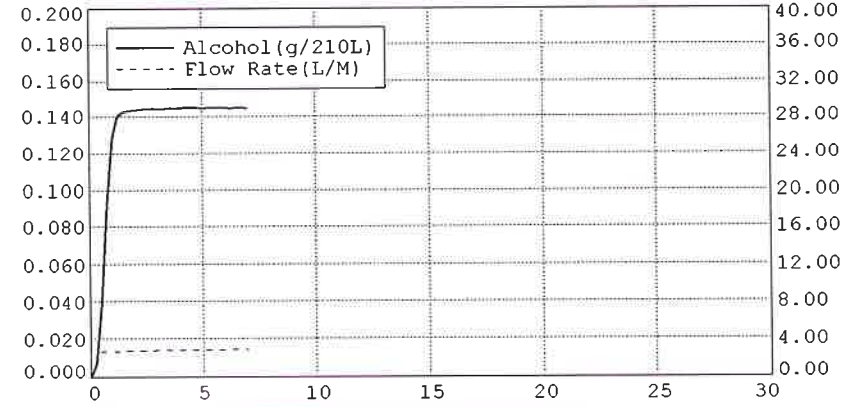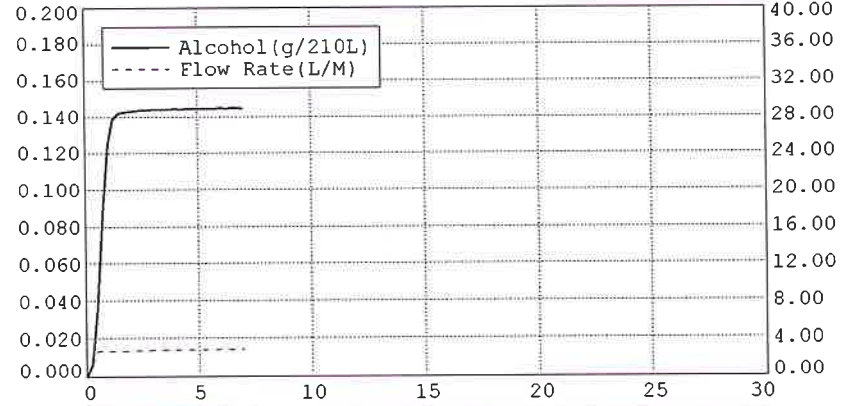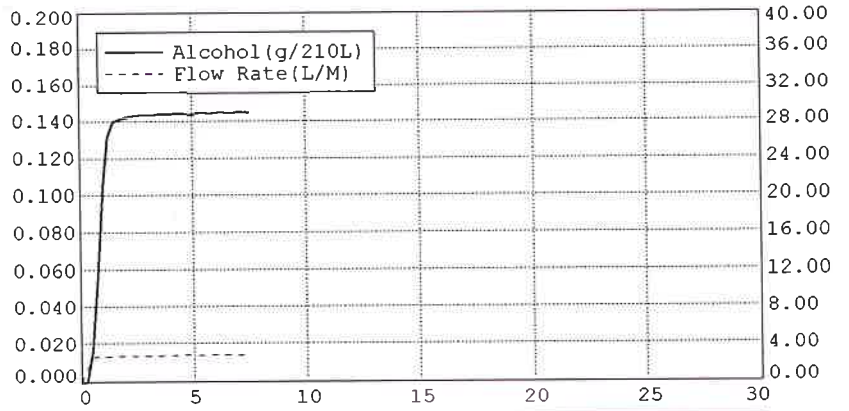

LINEARITY CHECK: Control Test 6






Alaska Department of Public Safety  
DATAMASTER dmt: 100672

Date: 06/06/2024  
Time: 09:26:25

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.300  
TARGET AT 29.29: 0.294  
LOT #: AG327804  
EXPIRATION: 10/05/2025  
TANK PRESSURE: 277 psi

BLANK TEST	0.000	09:27
INTERNAL STANDARD	VERIFIED	09:27
EXTERNAL STANDARD	0.295	09:28
BLANK TEST	0.000	09:29
EXTERNAL STANDARD	0.294	09:29
BLANK TEST	0.000	09:30
EXTERNAL STANDARD	0.295	09:30
BLANK TEST	0.000	09:31
EXTERNAL STANDARD	0.294	09:31
BLANK TEST	0.000	09:32
EXTERNAL STANDARD	0.295	09:32
BLANK TEST	0.000	09:33

Average = 0.2946  
Std Dev = 0.0005

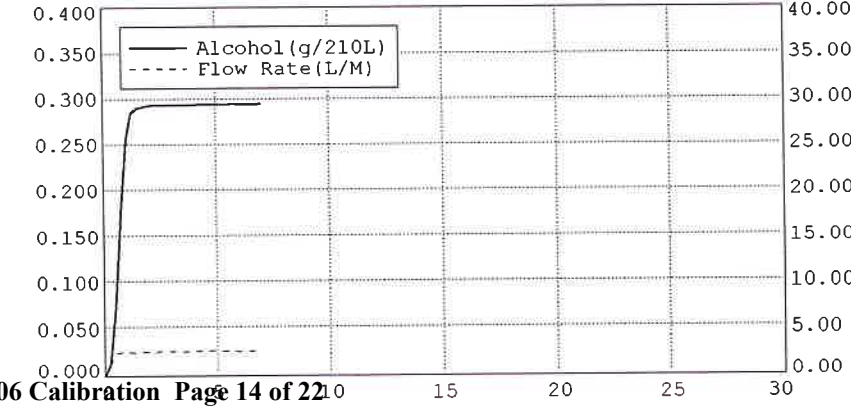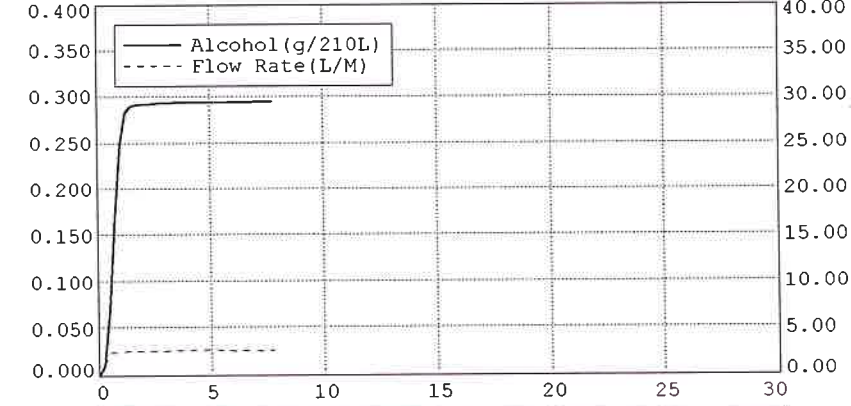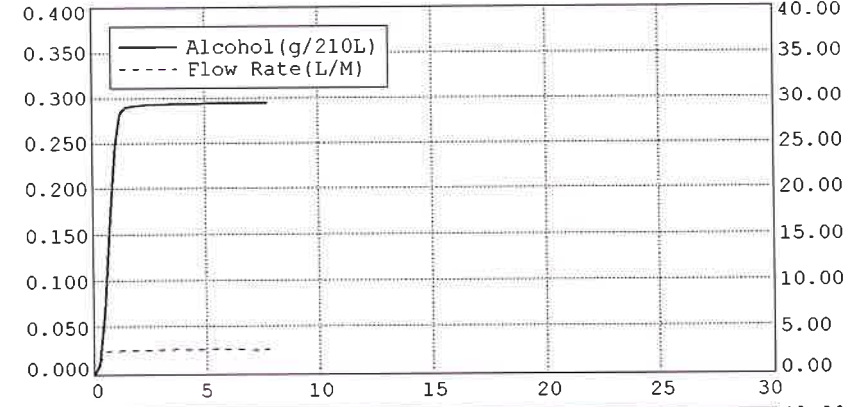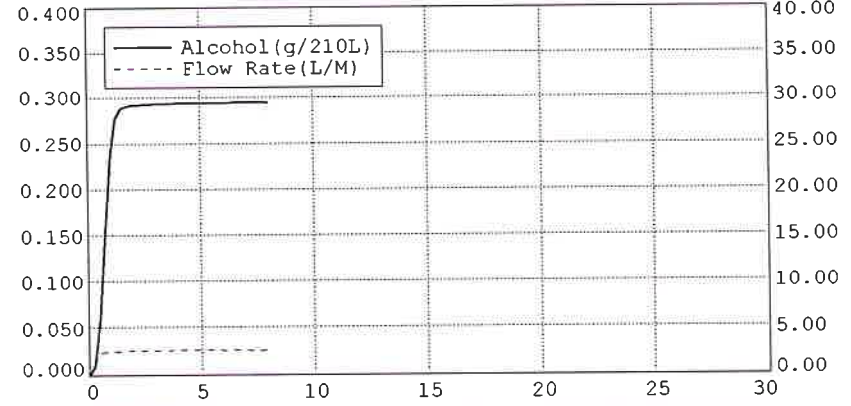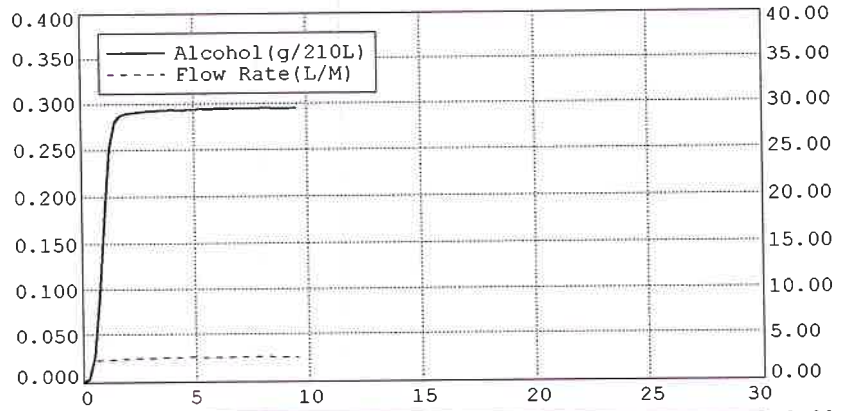



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100672

Date: 06/06/2024  
Time: 09:38:42

SUBJECT NAME:

TEST TEST ~~XXX~~ KS 6/18/24  
LICENSE #: ~~10746~~

OPERATOR NAME:

KAIJA SWISHER  
OPERATOR'S #: 10746

Lgt # AG7310901  
Exp 4/19/25  
KS 6/18/24

DEPT/AGENCY:

INCOMPLETE

CASE/REPORT: XXX

TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.29: 0.078

DIAGNOSTIC CHECK

PASSED 09:39  
BLANK TEST 0.000 09:39  
INTERNAL STANDARD VERIFIED 09:39  
EXTERNAL STANDARD 0.078 09:40  
BLANK TEST 0.000 09:41  
SUBJECT SAMPLE INCOMPLETE 09:43

KS

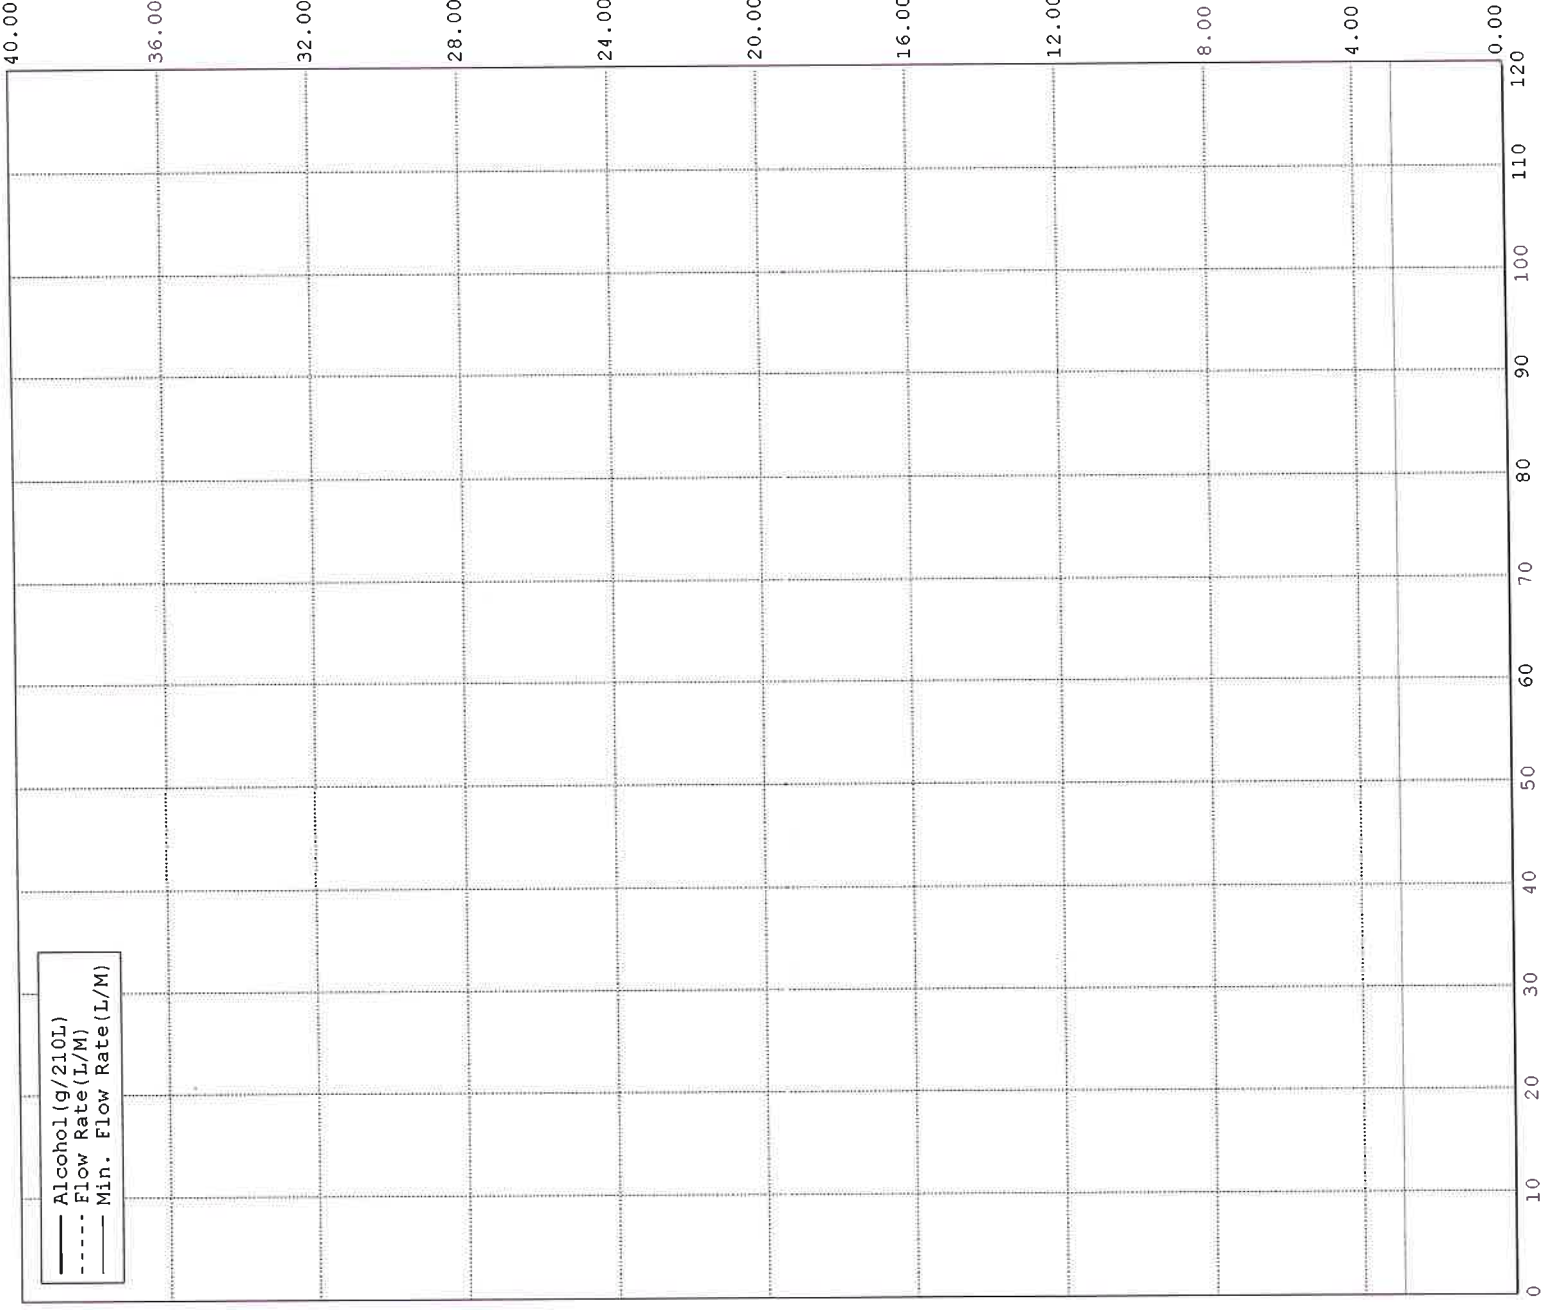

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100672

Date: 06/06/2024  
Time: 09:45:10

SUBJECT NAME:

TEST TEST *xxx* *KS 6/18/24*  
LICENSE #: *10740* *Lot # A6310901*  
*Exp 4/19/25*

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:

MAXIMUM ATTEMPTS EXCEEDED  
CASE/REPORT: *xxx*  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080  
TARGET AT 29.30: 0.078

DIAGNOSTIC CHECK

PASSED 09:46  
BLANK TEST 0.000 09:46  
INTERNAL STANDARD VERIFIED 09:46  
EXTERNAL STANDARD 0.078 09:46  
BLANK TEST 0.000 09:47  
SUBJECT SAMPLE *xxx* 09:47

Maximum Attempts Exceeded

*KS*

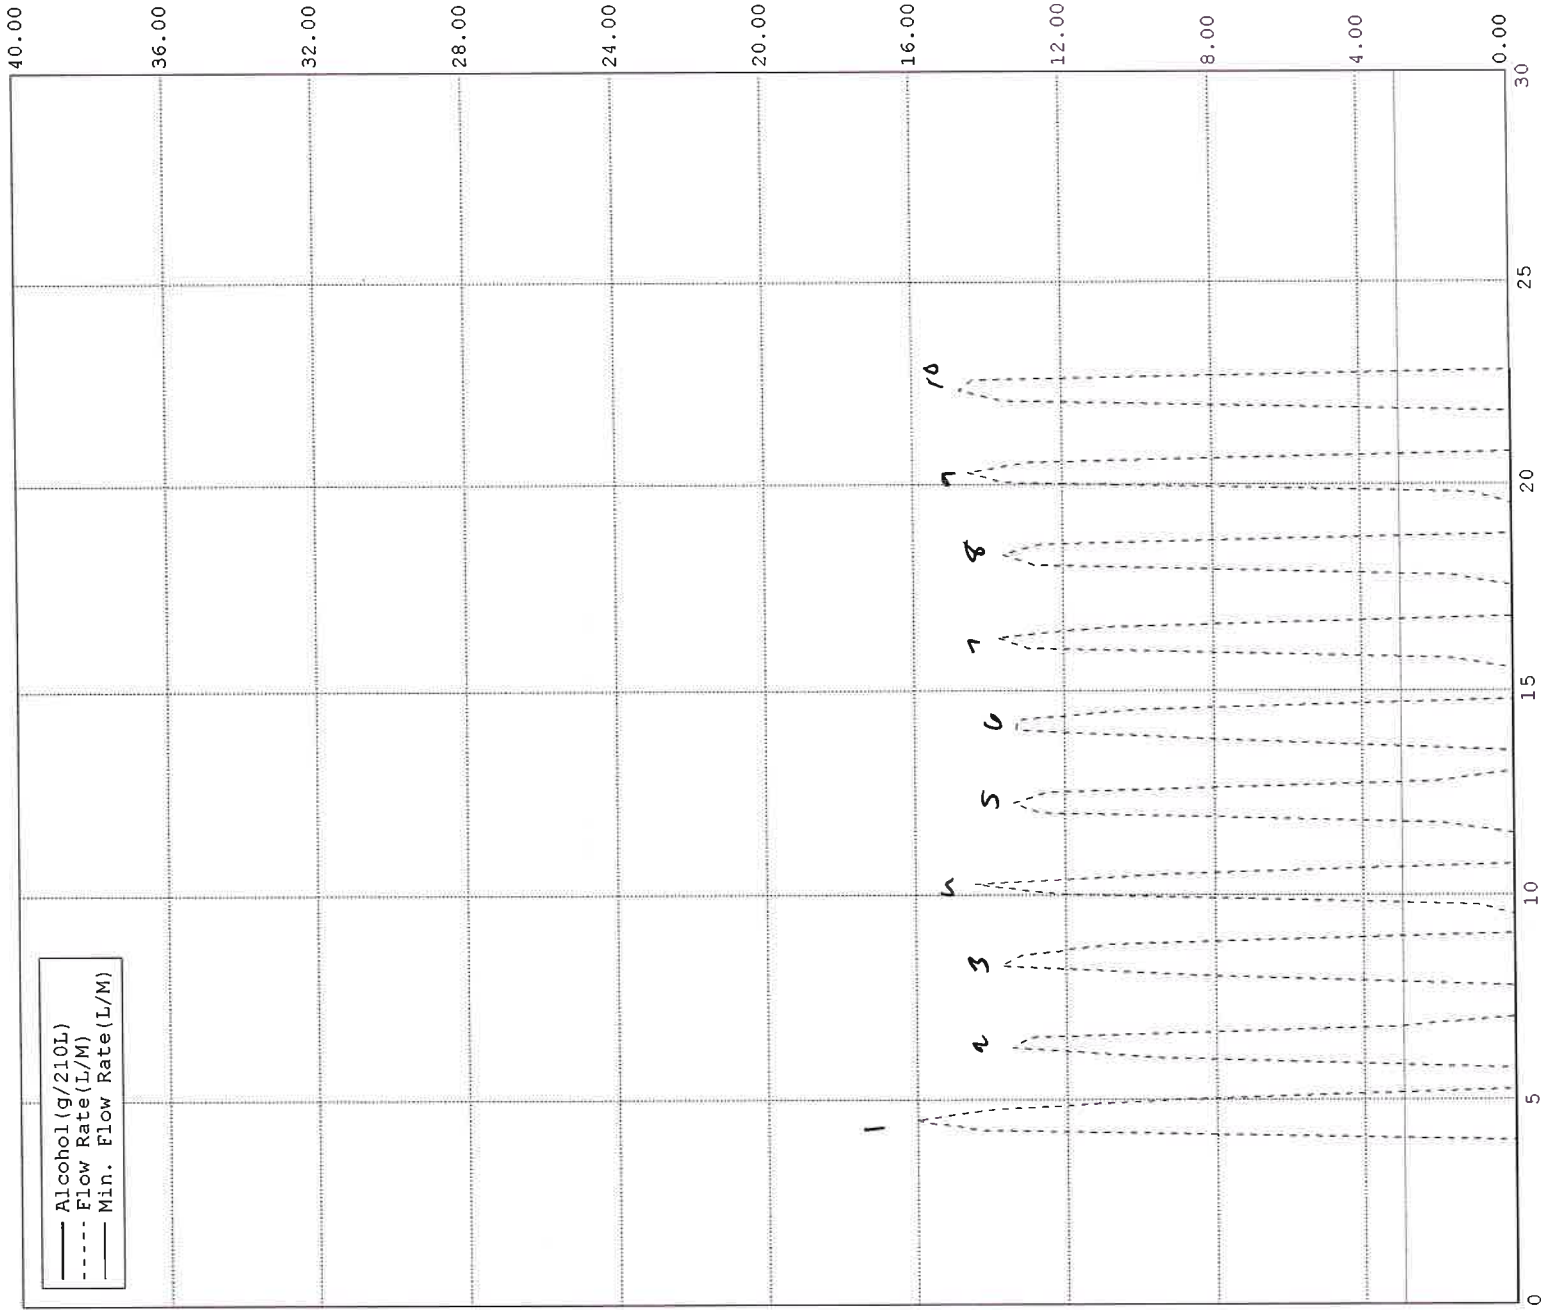



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100672

Date: 06/06/2024  
Time: 10:19:27

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

*Lot # AG316901  
Exp 4/19/25  
KS 6/18/24*

DEPT/AGENCY:  
INVALID

CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.30: 0.078

DIAGNOSTIC CHECK PASSED 10:20  
BLANK TEST 0.000 10:20  
INTERNAL STANDARD VERIFIED 10:20  
EXTERNAL STANDARD 0.077 10:20  
BLANK TEST 0.000 10:21  
SUBJECT SAMPLE INVALID 10:22

*KS*



SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100672  
-----

Date: 06/06/2024  
Time: 10:23:53

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

*Lot # AG310901  
GAP 4/19/25  
KS 6/18/24*

DEPT/AGENCY:  
RFI

CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.31: 0.078

DIAGNOSTIC CHECK	PASSED	10:24
BLANK TEST	0.000	10:24
INTERNAL STANDARD	VERIFIED	10:25
EXTERNAL STANDARD	0.077	10:25

RFI DETECTED

*KS*

SUBJECT TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100672

Date: 06/06/2024  
 Time: 10:04:34

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXX


OPERATOR NAME:  
 KAIJA SWISHER  
 OPERATOR'S #: 10746

DEPT/AGENCY:  
 INTERFERENCE - ACETONE  
 CASE/REPORT: XXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.31: 0.078

DIAGNOSTIC CHECK	PASSED	10:06
BLANK TEST	0.000	10:06
INTERNAL STANDARD	VERIFIED	10:06
Xq = 0.113 (0.63%)		
EXTERNAL STANDARD	0.077	10:06
X[1] = 0.0771 (0.0003) (0.0024)		
BLANK TEST	0.000	10:07
SUBJECT SAMPLE	XXX	10:08
X[1] = 0.1050 (-0.0168) (0.0019)		

Interference Detected

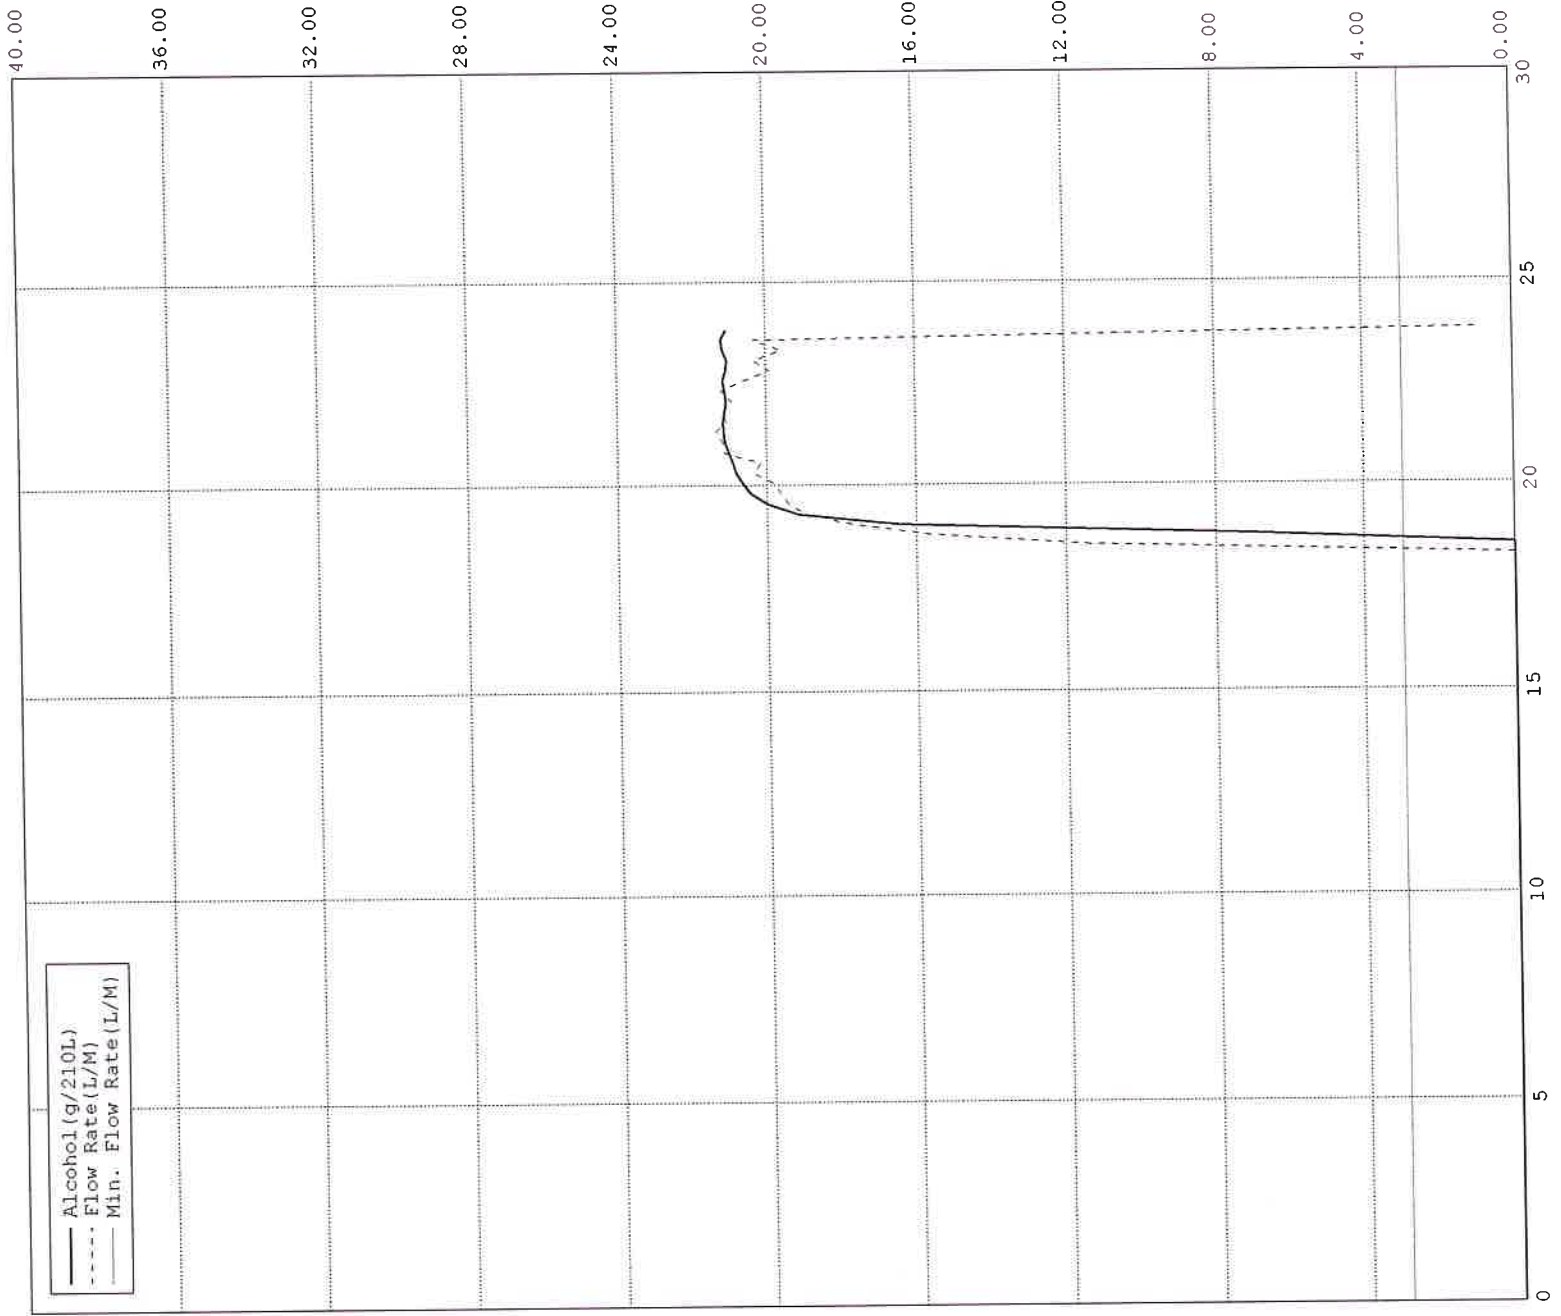

KS

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100672

Date: 06/06/2024  
Time: 10:09:54

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

Lot# A6310901  
Exp 4/19/25  
KS 6/18/24

DEPT/AGENCY:  
INTERFERENCE - IPA  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.31: 0.078

DIAGNOSTIC CHECK	PASSED	10:11
BLANK TEST	0.000	10:11
INTERNAL STANDARD	VERIFIED	10:11
Xq = 0.114 (0.86%)		
EXTERNAL STANDARD	0.077	10:12
X[1] = 0.0770 (-0.0001)	(0.0023)	
BLANK TEST	0.000	10:12
SUBJECT SAMPLE	XXX	10:13
X[1] = 0.1125 (-0.0202)	(0.0015)	

Interference Detected

KS

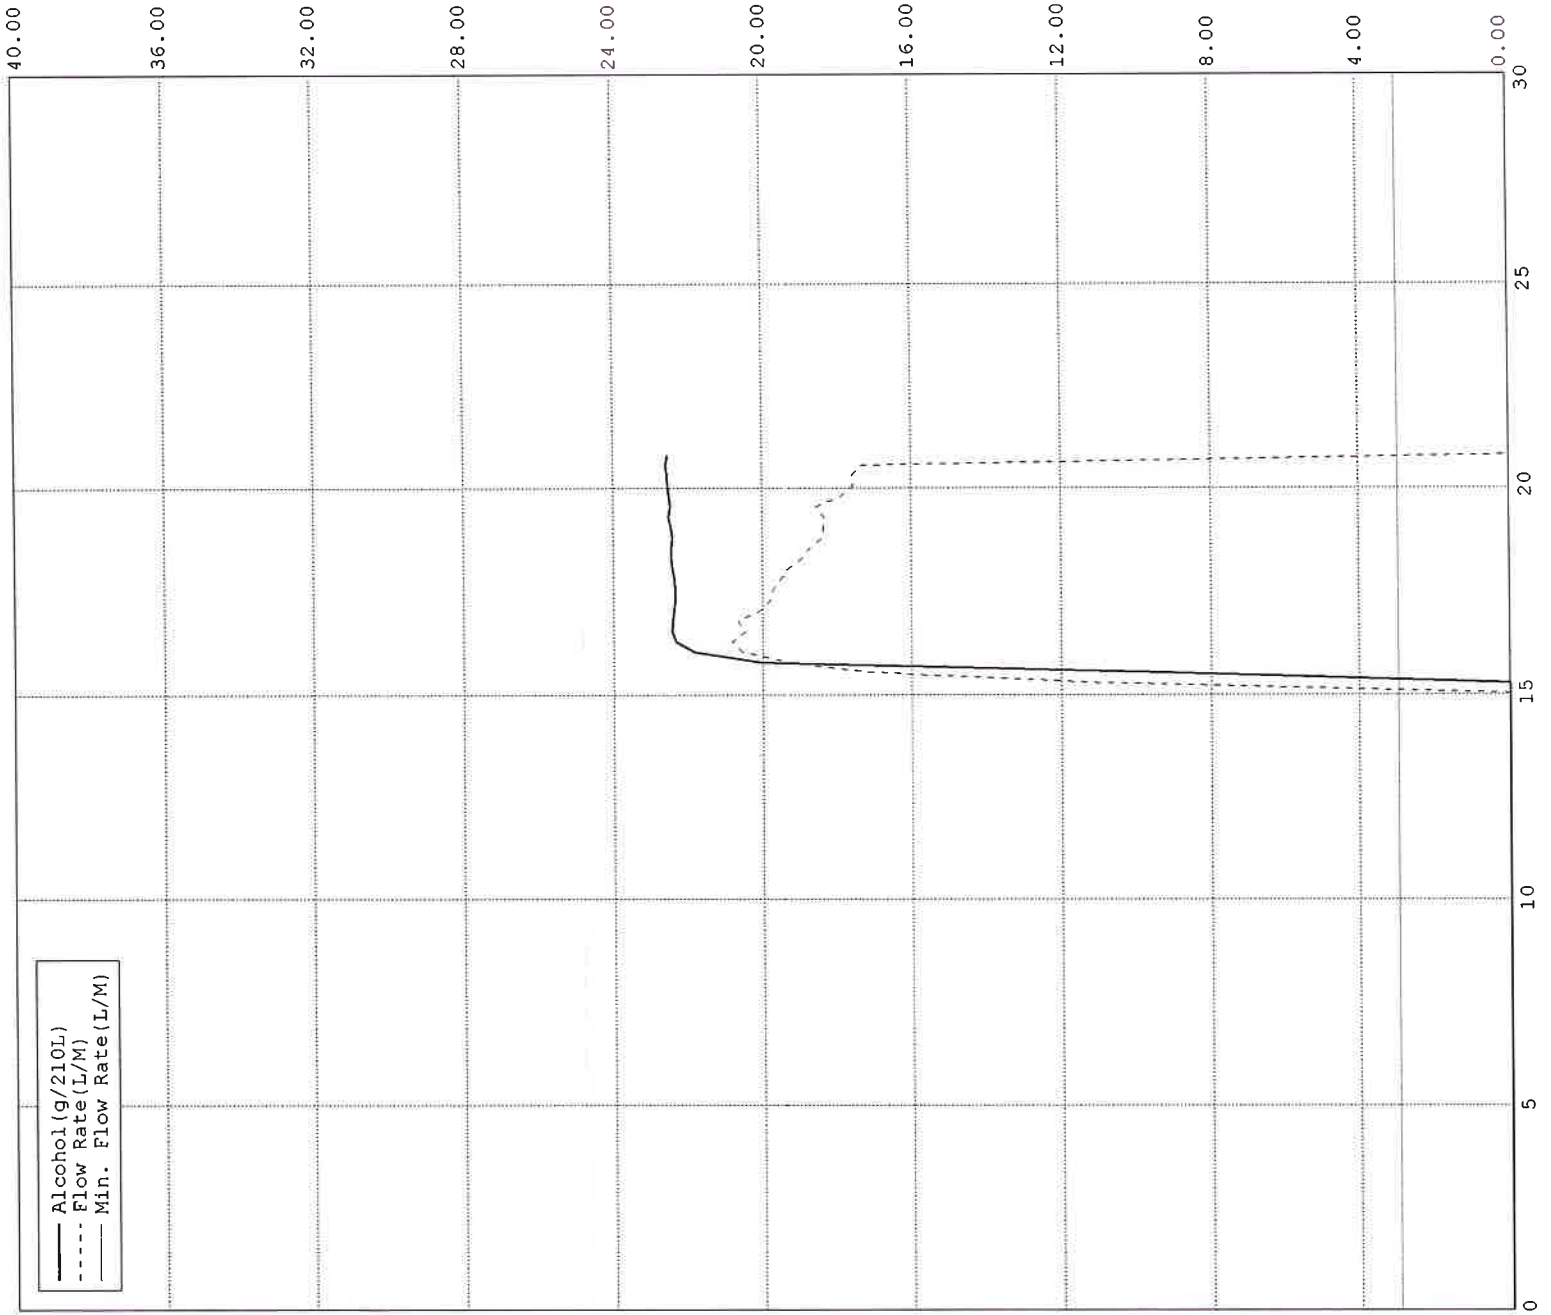

SUBJECT TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100672

Date: 06/06/2024  
 Time: 09:56:48

SUBJECT NAME:

TEST TEST ~~2222~~ KS 6/18/24  
 LICENSE #: ~~10746~~ Lot # AG316901  
 OPERATOR NAME: KAIJA SWISHER Exp 4/19/25  
 OPERATOR'S #: 10746

DEPT/AGENCY:

INTERFERENCE - NEGATIVE  
 CASE/REPORT: XXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.29: 0.078

DIAGNOSTIC CHECK	PASSED	09:58
BLANK TEST	0.000	09:58
INTERNAL STANDARD	VERIFIED	09:58
Xg = 0.114 (0.94%)		
EXTERNAL STANDARD	0.076	09:58
X[1] = 0.0760 (-0.0005) (0.0030)		
BLANK TEST	0.000	09:59
SUBJECT SAMPLE (Vol=1.75L)	0.089	09:59
X[1] = 0.0899 (0.0001) (0.0002)		
BLANK TEST	0.000	10:00
EXTERNAL STANDARD	0.077	10:01
X[1] = 0.0774 (0.0009) (0.0021)		
BLANK TEST	0.000	10:02

Filter 2 average : 0.0002

Filter 3 average : 0.0025

KS 6/6/24 JM  
 06/21/24

KS



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100672

Date: 06/06/2024  
Time: 11:11:04

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
NON DRINKING SUBJECT TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.33: 0.078

DIAGNOSTIC CHECK	PASSED	11:12
BLANK TEST	0.000	11:12
INTERNAL STANDARD	VERIFIED	11:12
EXTERNAL STANDARD	0.078	11:12
BLANK TEST	0.000	11:13
SUBJECT SAMPLE (Vol=1.74L)	0.000	11:14
BLANK TEST	0.000	11:15
EXTERNAL STANDARD	0.078	11:15
BLANK TEST	0.000	11:16

*Lot # AGS16901  
Exp 4/19/25  
KS 6/18/24*

*KS*

